

US00D692564S

(12) **United States Design Patent**
Ninomiya et al.

(10) **Patent No.:** **US D692,564 S**
(45) **Date of Patent:** **** Oct. 29, 2013**

(54) **PROBE CONNECTOR FOR ULTRASOUND
DIAGNOSTIC APPARATUS**

(75) Inventors: **Atsushi Ninomiya**, Tokyo (JP);
Kazuyuki Yanase, Tokyo (JP); **Katsumi
Usami**, Tokyo (JP); **Gen Siina**, Tokyo
(JP); **Tomoyuki Yagi**, Tokyo (JP);
Masaru Yokoyama, Tokyo (JP)

(73) Assignee: **Hitachi Aloka Medical, Ltd.**, Tokyo
(JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/431,917**

(22) Filed: **Sep. 12, 2012**

(30) **Foreign Application Priority Data**

Mar. 15, 2012 (JP) 2012-005868

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/187**

(58) **Field of Classification Search**
USPC D24/107, 129, 138, 141, 158, 164, 165,
D24/167, 170, 186-187, 231; D10/57, 60,
D10/78, 80; 600/407, 461, 459; 378/98.7,
378/98.8, 189

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,688,578 A * 8/1987 Takano et al. 600/459
4,796,632 A * 1/1989 Boyd et al. 600/459
D327,740 S * 7/1992 Arioka et al. D24/186

D547,871 S * 7/2007 Watson et al. D24/186
D564,659 S * 3/2008 Hayashi D24/129
D564,660 S * 3/2008 Hayashi D24/138
D566,284 S * 4/2008 Kitayama et al. D24/186
D585,556 S * 1/2009 Kosaku D24/186
D603,050 S * 10/2009 Chen D24/187
D603,520 S * 11/2009 Ninomiya et al. D24/187
D609,814 S * 2/2010 Banryu D24/187
D629,526 S * 12/2010 Ladwig et al. D24/187
D629,527 S * 12/2010 Crunkilton D24/187
D638,131 S * 5/2011 Buckels et al. D24/187
D684,265 S * 6/2013 Cadera D24/187

* cited by examiner

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Antonelli, Terry, Stout &
Kraus, LLP.

(57) **CLAIM**

We claim the ornamental design for probe connector for
ultrasound diagnosis apparatus, as shown.

DESCRIPTION

FIG. 1 is a front, top and right side perspective view of an
probe connector for ultrasound diagnostic apparatus showing
our new design;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear side elevational view thereof;

FIG. 4 is a left side elevational view thereof;


FIG. 5 is a right side elevational view thereof;

FIG. 6 is a top plan view thereof; and,

FIG. 7 is a bottom plan view thereof.

The broken lines are included for the purpose of illustrating
portions of the probe connector for ultrasound diagnostic
apparatus that forms no part of the claimed design.

1 Claim, 3 Drawing Sheets

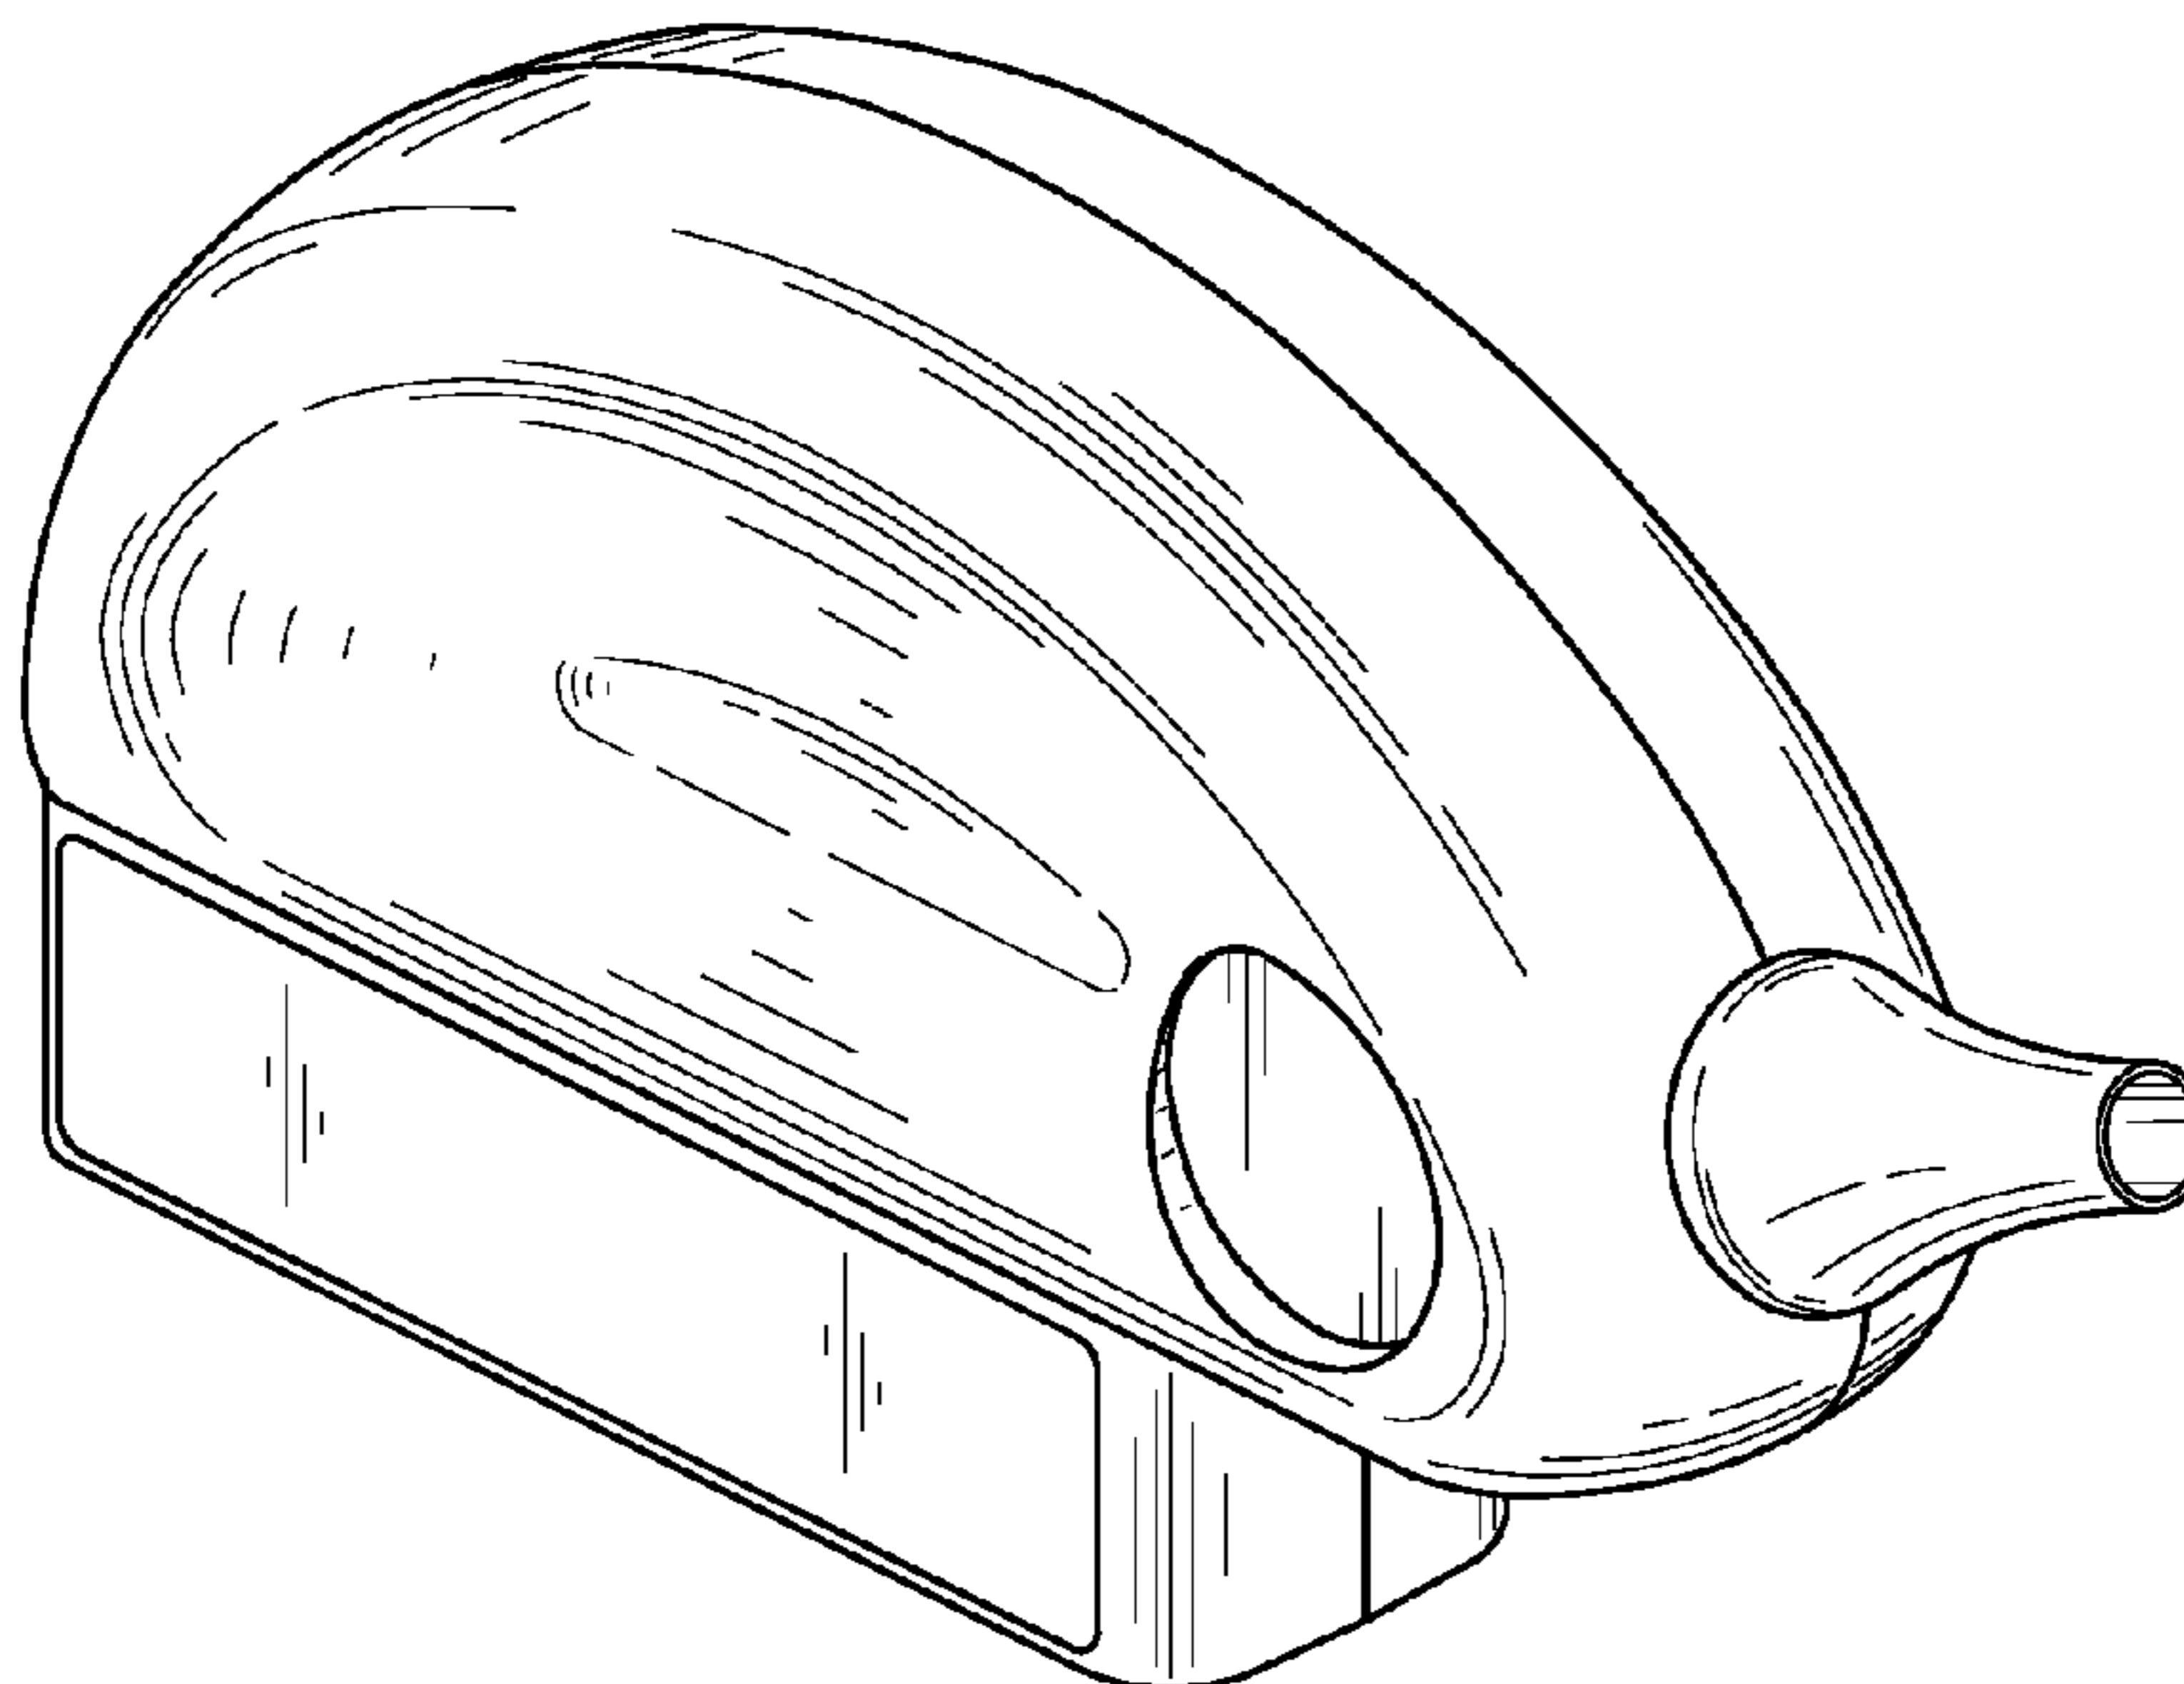

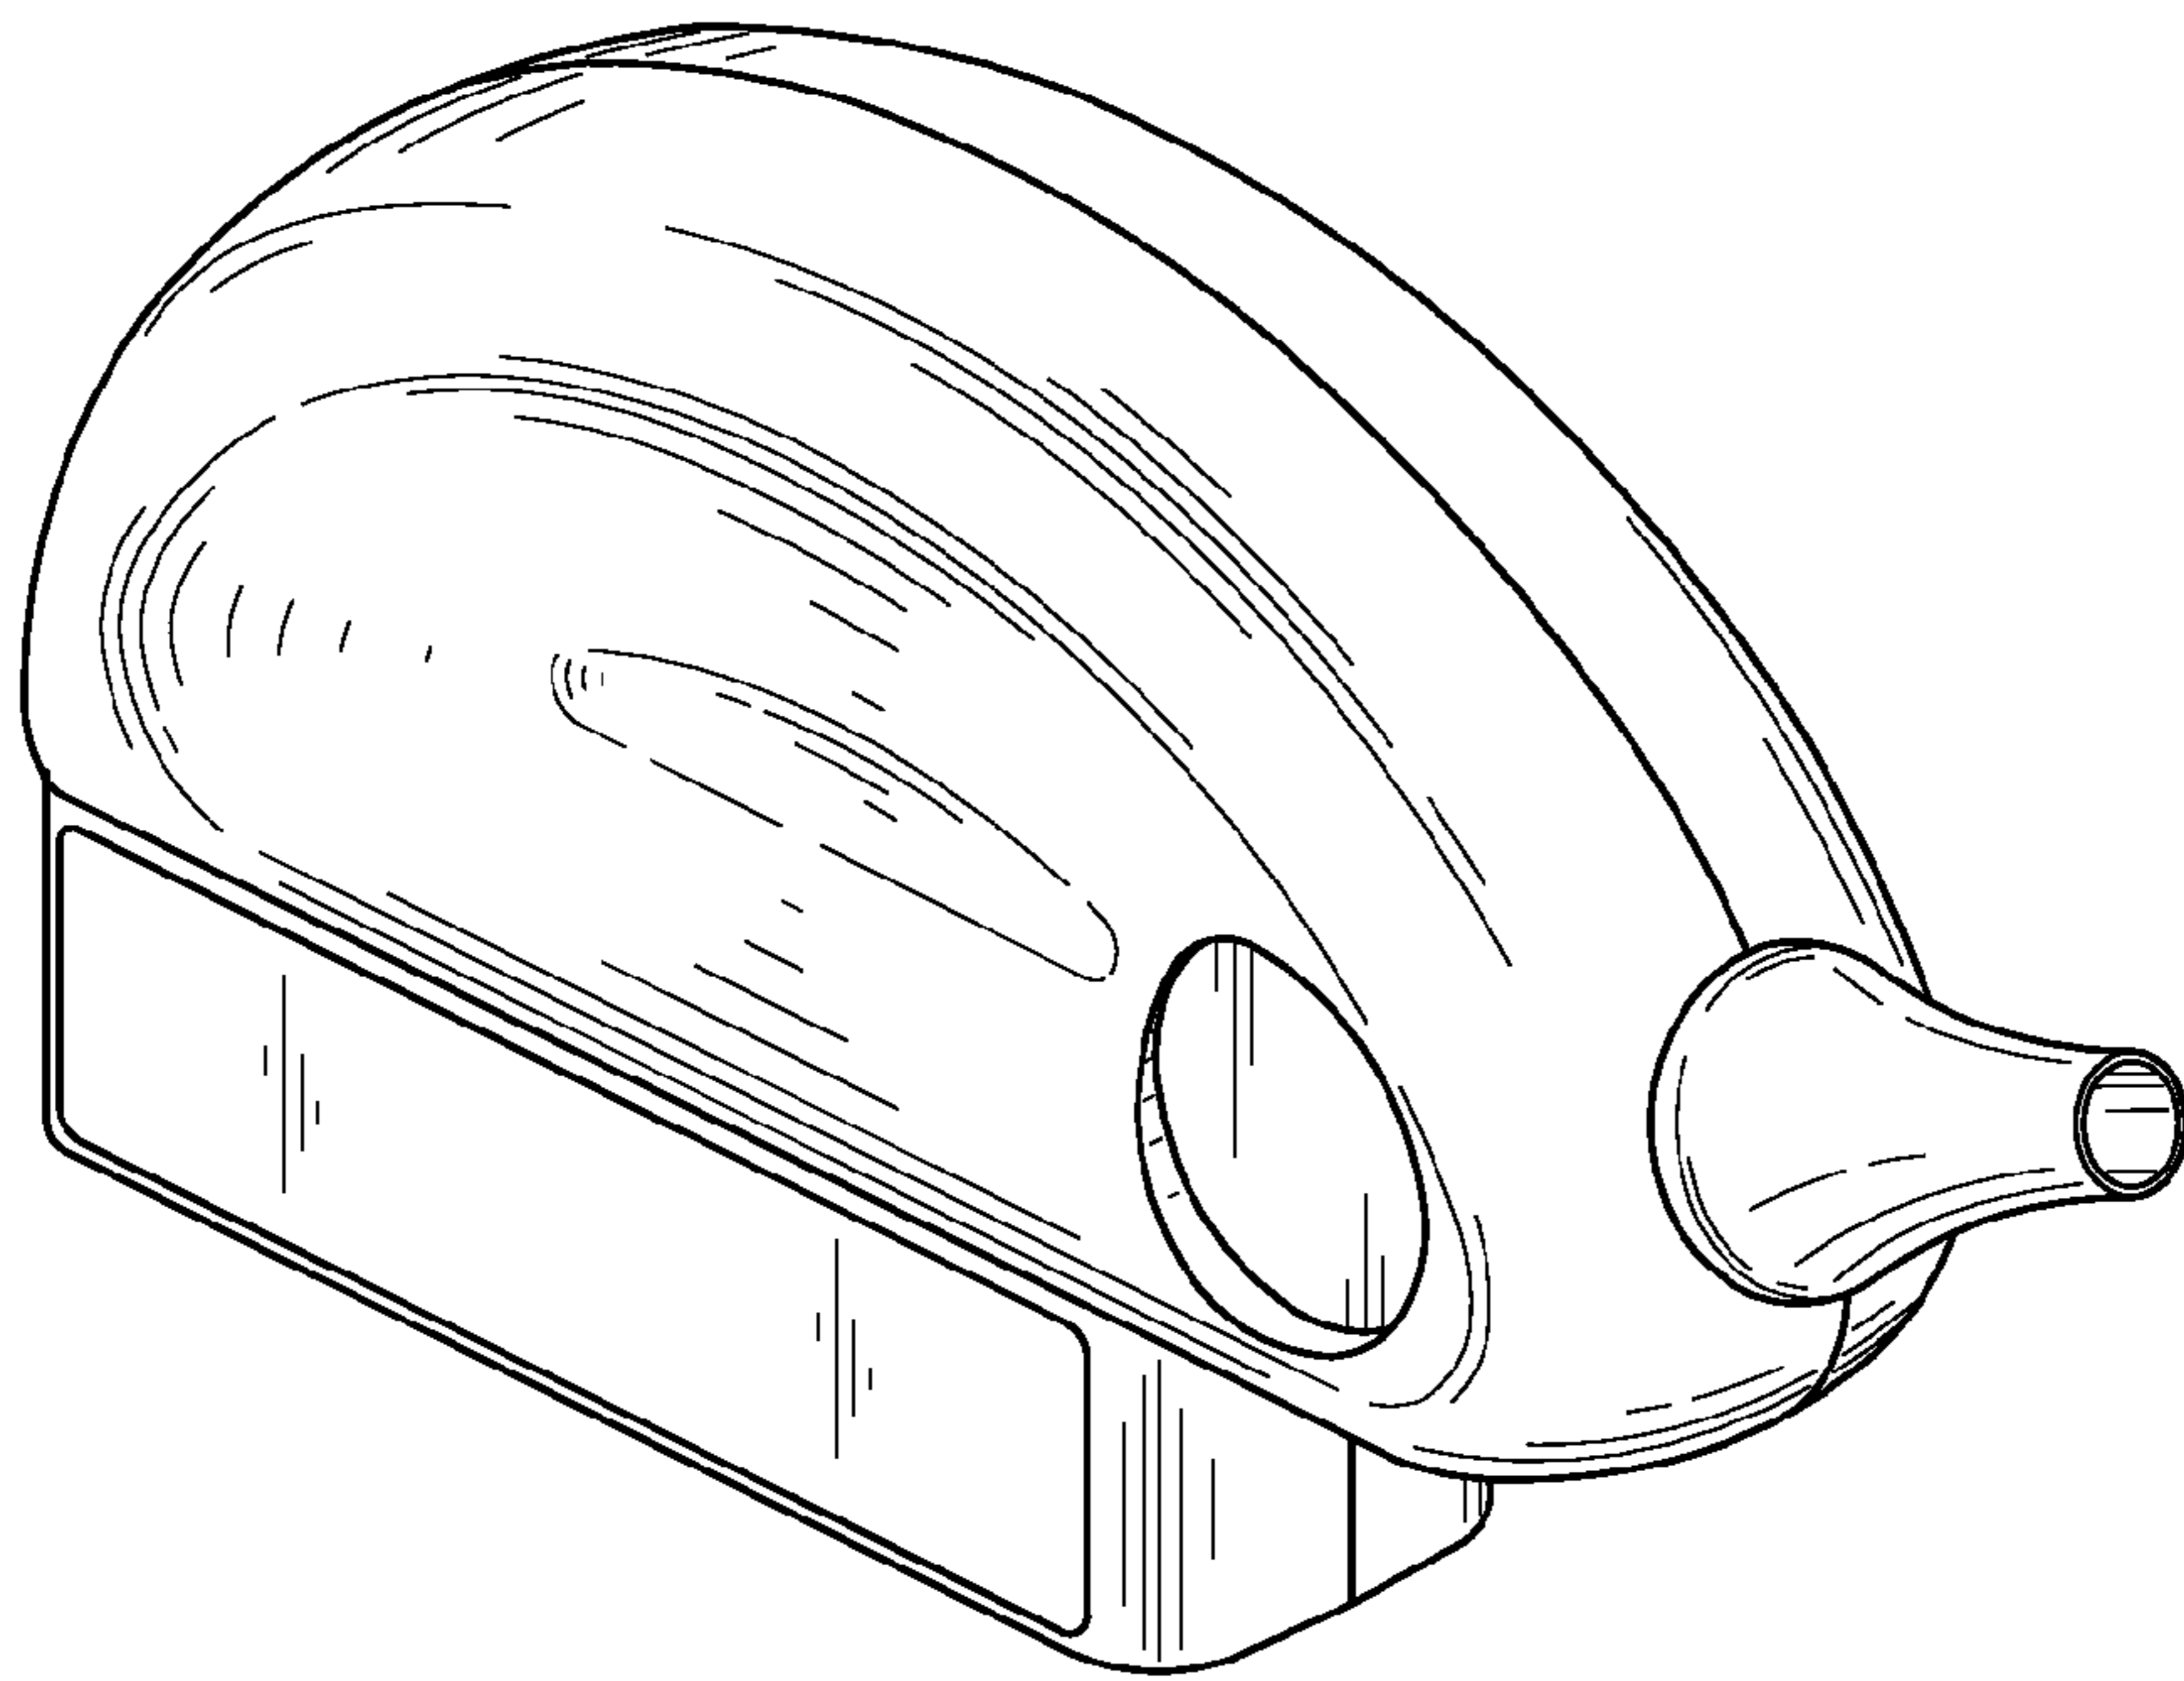


FIG. 1

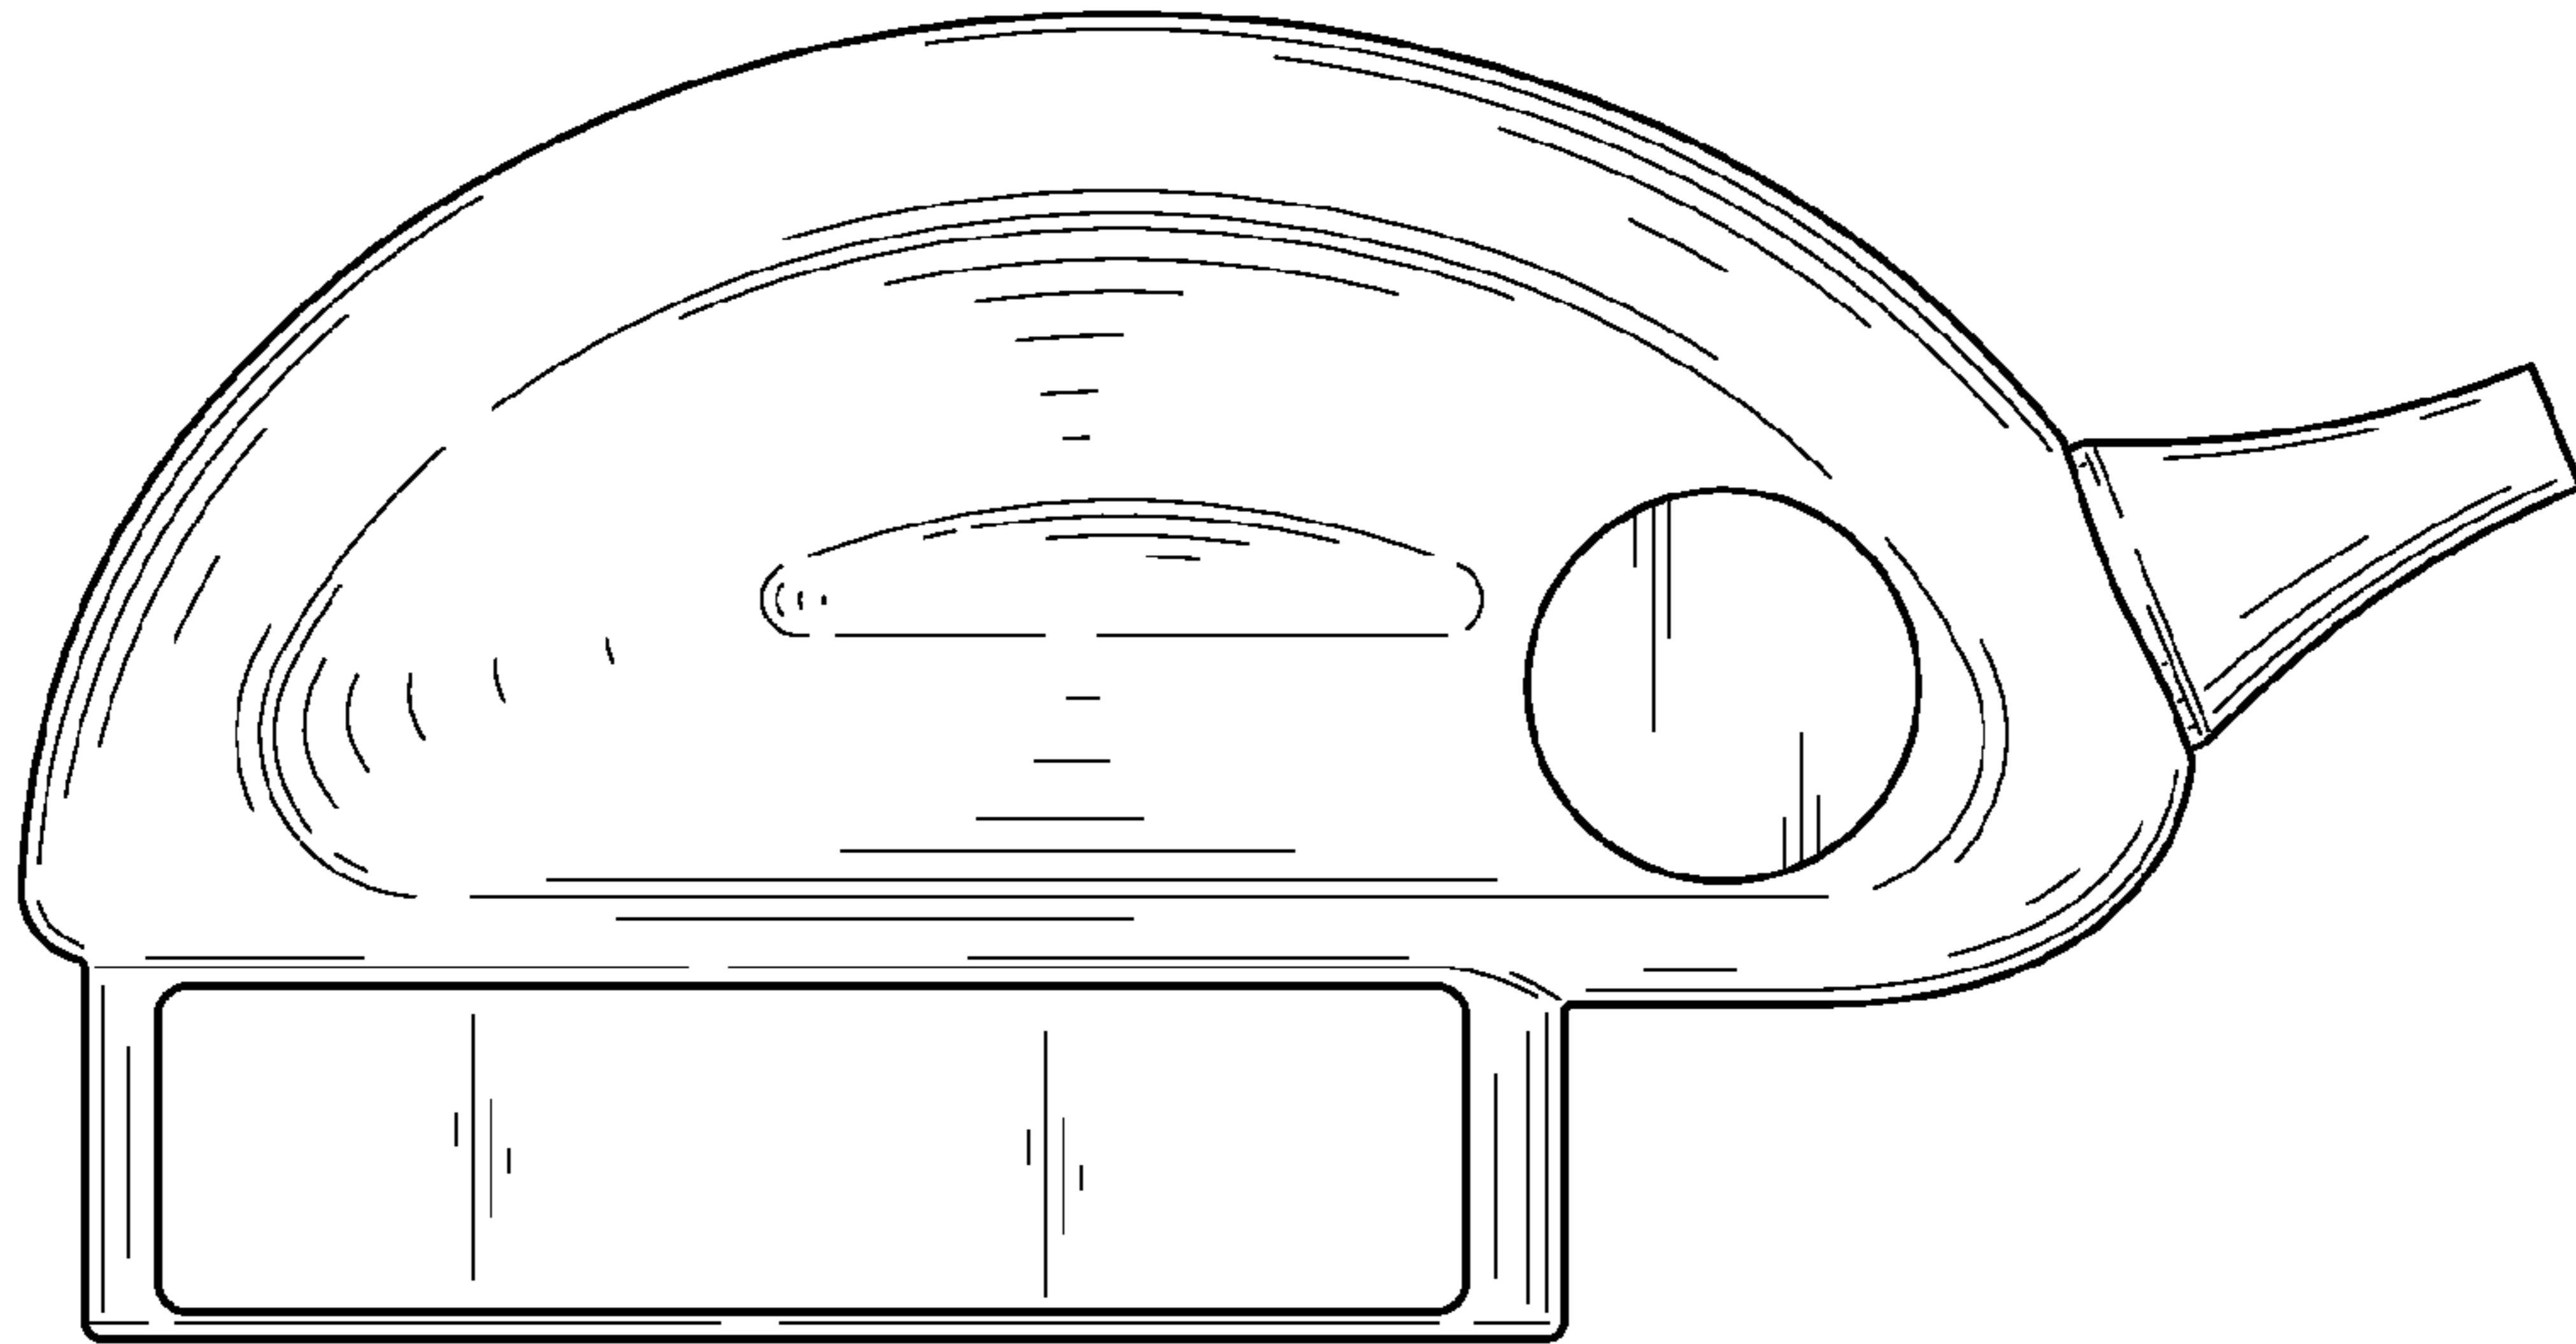


FIG. 2

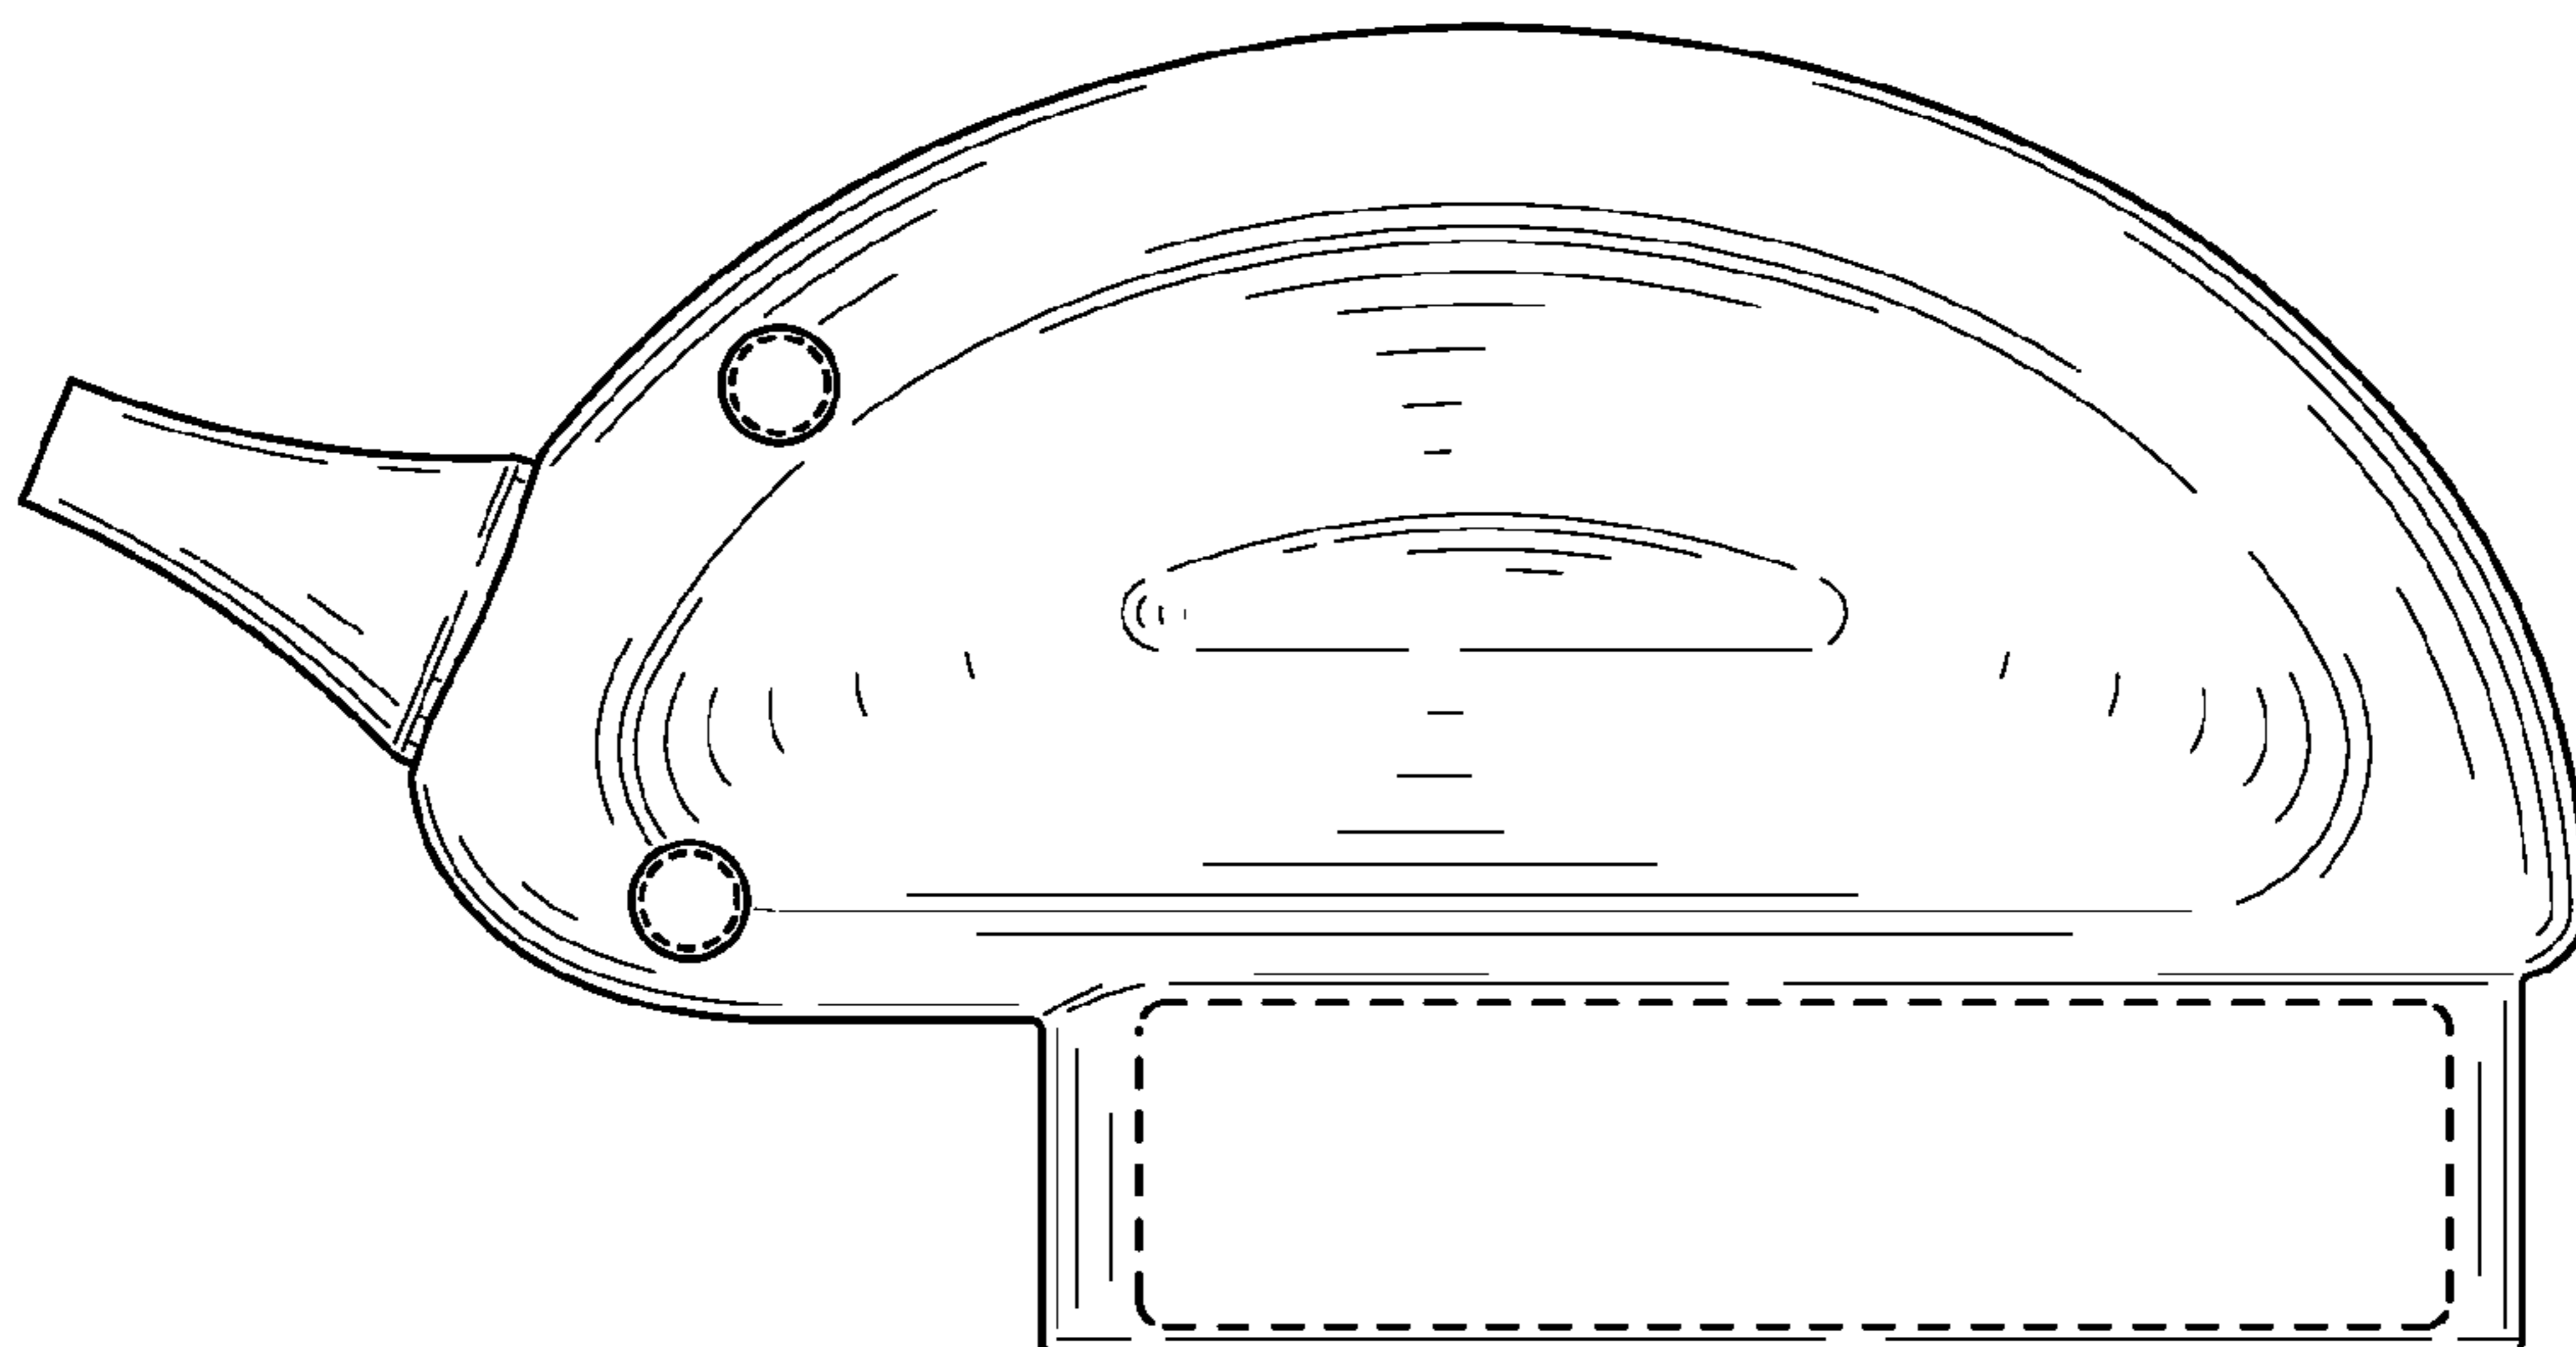


FIG. 3

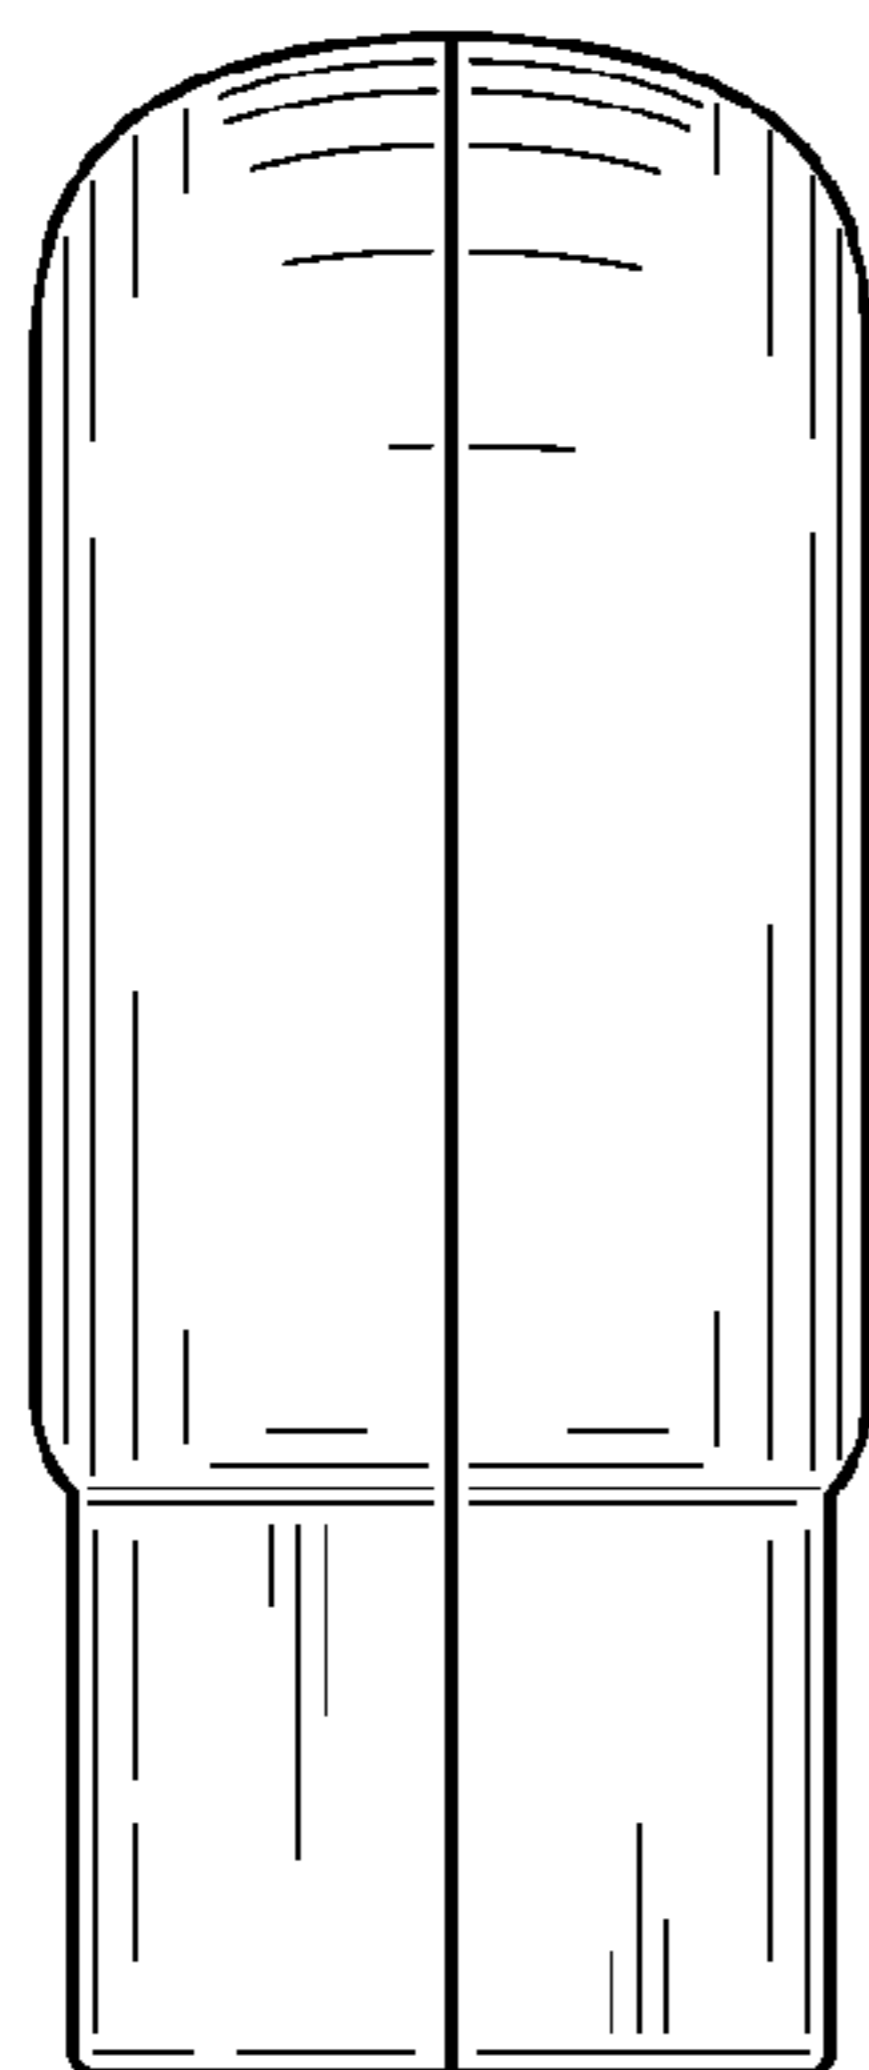


FIG. 4

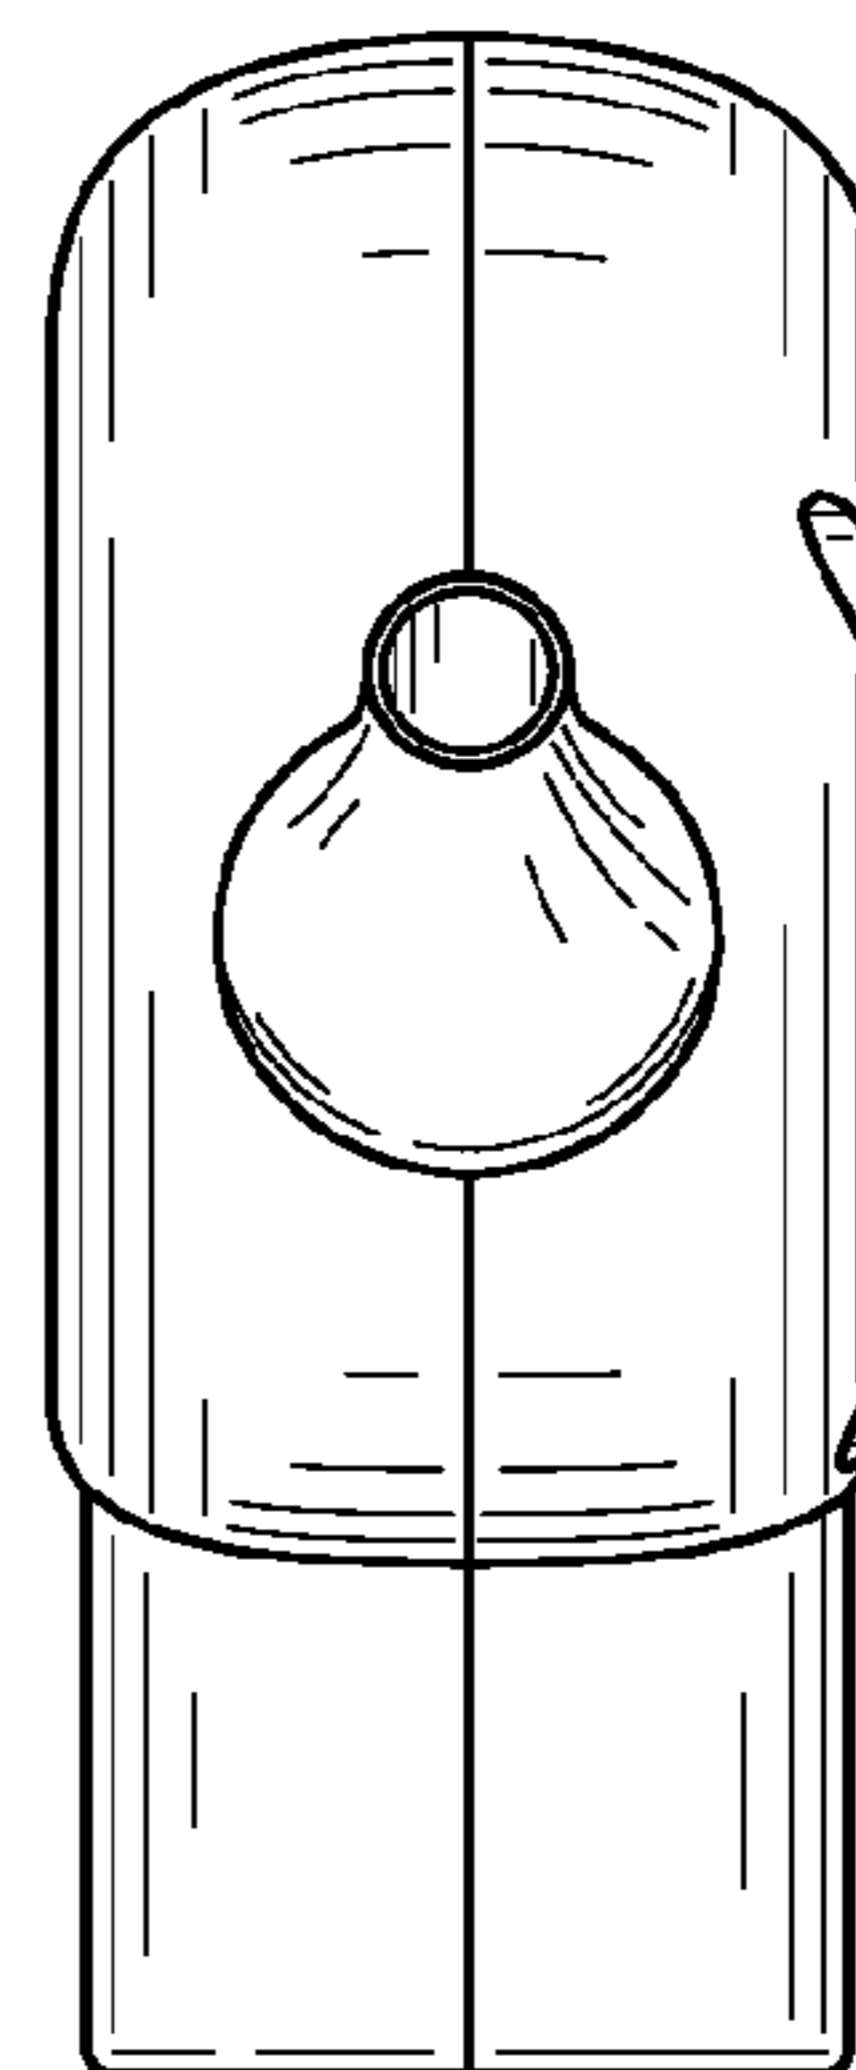


FIG. 5

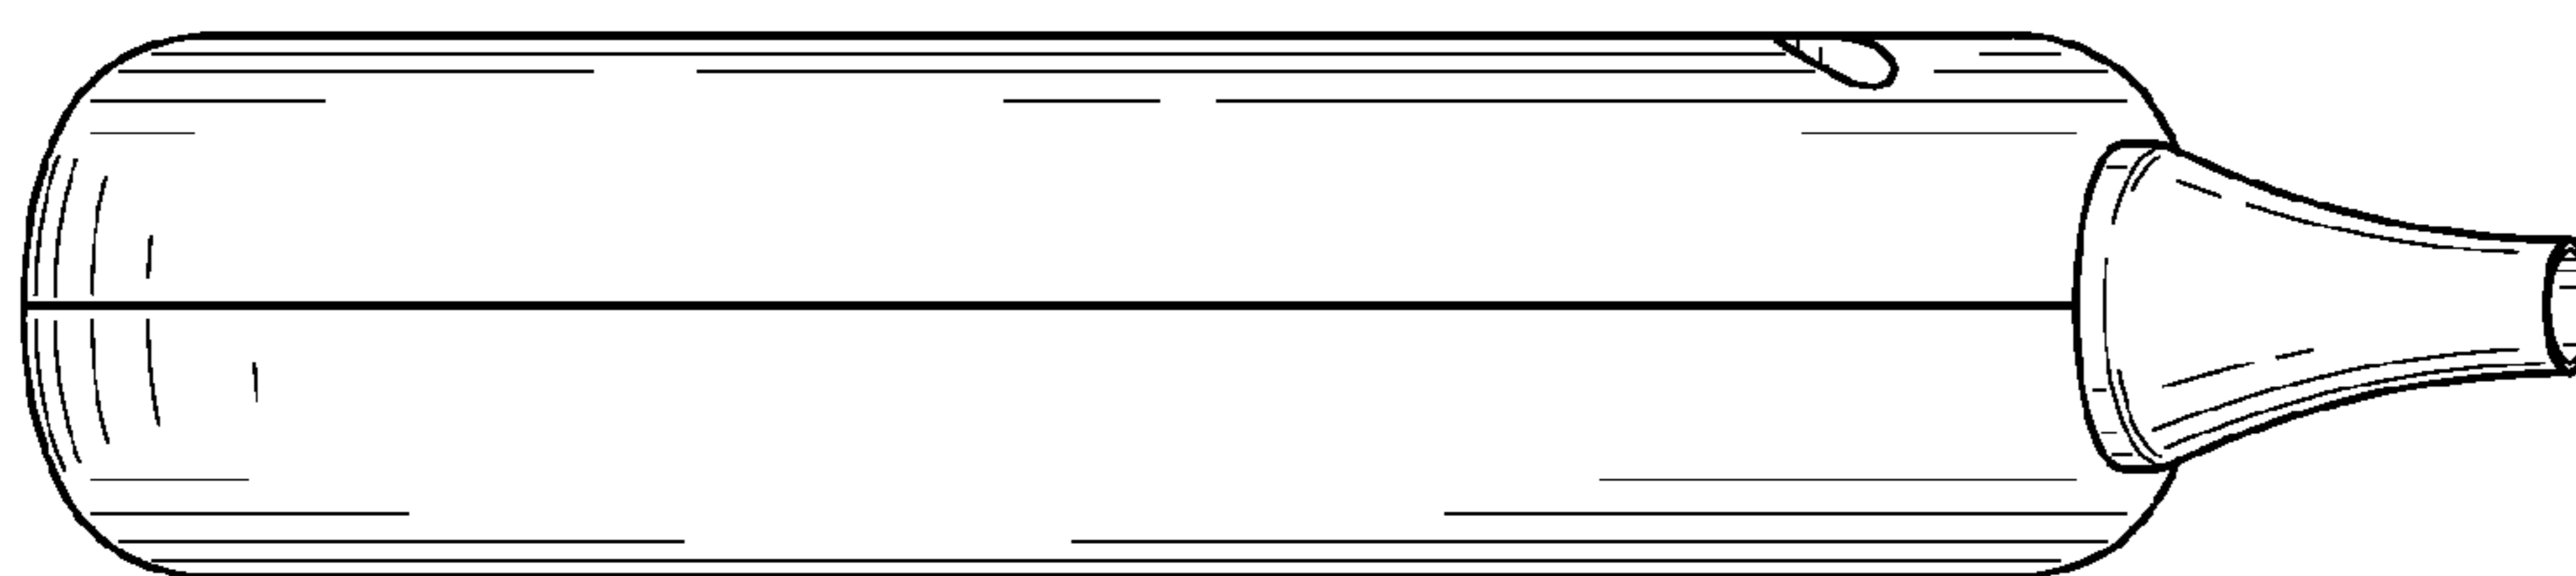


FIG. 6

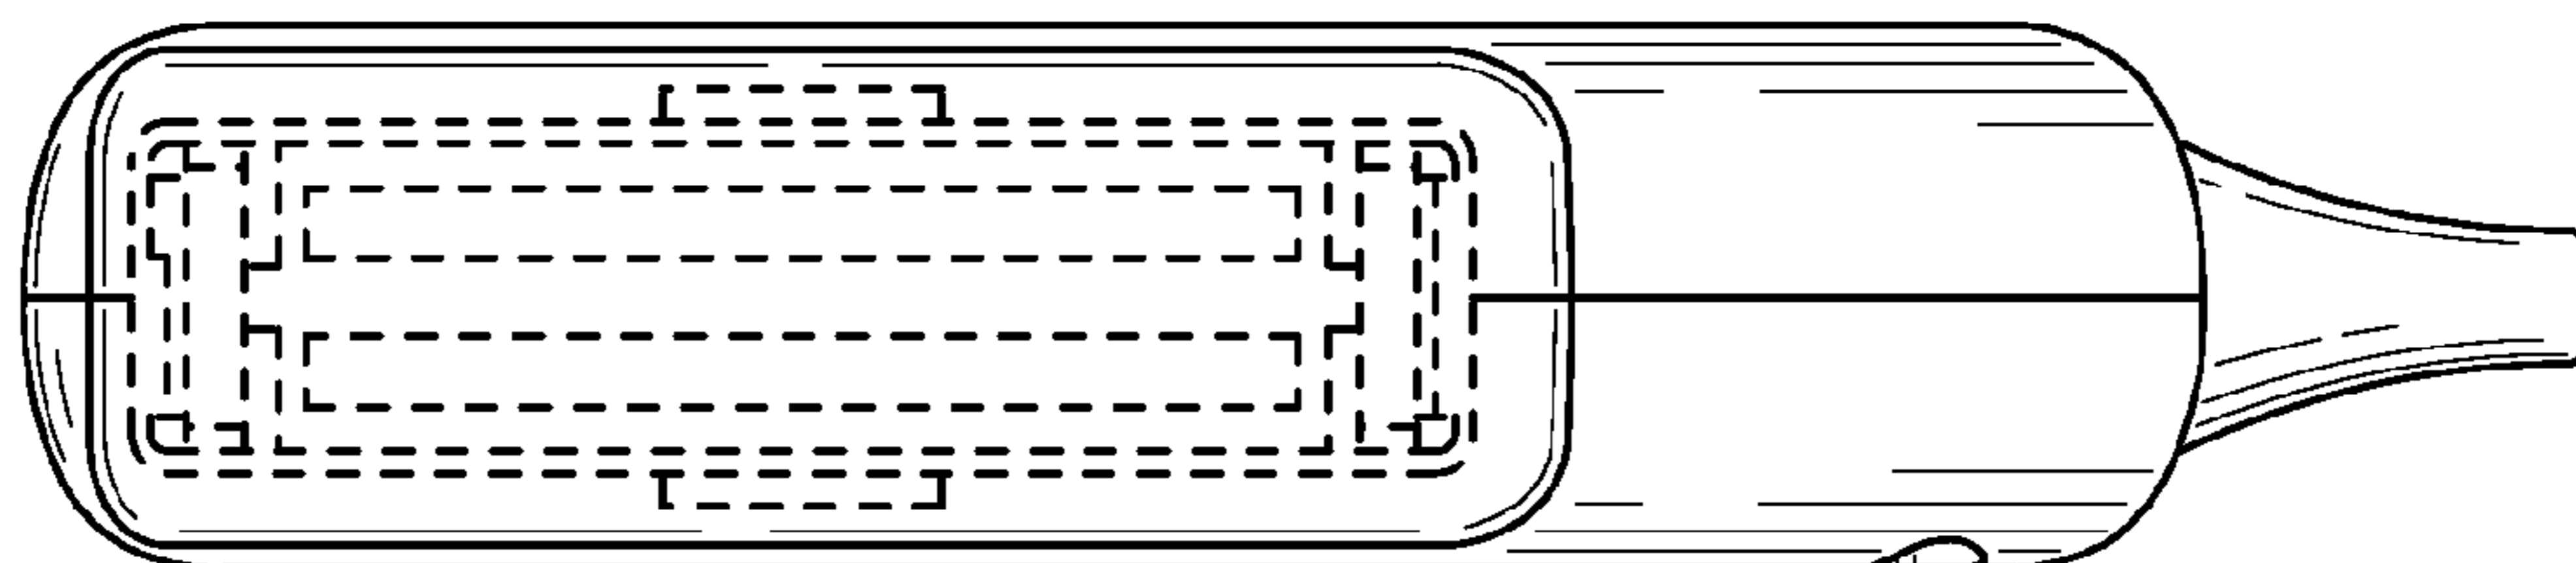


FIG. 7