



US00D694908S

(12) **United States Design Patent**  
**Okihara**

(10) **Patent No.:** **US D694,908 S**  
(45) **Date of Patent:** **\*\* Dec. 3, 2013**

(54) **MEDICAL SYRINGE CONTAINER**

(71) Applicant: **Terumo Kabushiki Kaisha**, Tokyo (JP)

(72) Inventor: **Hitoshi Okihara**, Fujinomiya (JP)

(73) Assignee: **Terumo Kabushiki Kaisha** (JP)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/436,616**

(22) Filed: **Nov. 7, 2012**

(30) **Foreign Application Priority Data**

May 7, 2012 (JP) ..... 2012-010496

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/230**

(58) **Field of Classification Search**  
USPC ..... D24/108, 127–130, 216, 224, 227–232;  
206/446, 443; 211/74, 70.1, 72;  
604/192; 356/246, 244; 422/102, 104,  
422/63–64, 250, 266, 297, 300, 476, 553;  
D19/37

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D265,126 S *	6/1982	Beall	.....	D24/230
D283,162 S *	3/1986	Godsey	.....	D24/226
D284,700 S *	7/1986	Mehra et al.	.....	D24/229
5,047,019 A *	9/1991	Sincock	.....	604/192
5,048,957 A *	9/1991	Berthold et al.	.....	356/246
D323,400 S *	1/1992	Frenkel et al.	.....	D24/230
D325,975 S *	5/1992	Grade et al.	.....	D24/230
D359,126 S *	6/1995	Hovatter	.....	D24/227
5,487,872 A *	1/1996	Hafeman et al.	.....	422/553
D369,415 S *	4/1996	Boulton et al.	.....	D24/224
D414,271 S *	9/1999	Mendoza	.....	D24/224

D420,743 S *	2/2000	Monks	.....	D24/224
D448,854 S *	10/2001	Kuiper et al.	.....	D24/230
D461,554 S *	8/2002	Lafond et al.	.....	D24/230
D466,219 S *	11/2002	Wynschenk et al.	.....	D24/227
D506,833 S *	6/2005	Wescott, III	.....	D24/230
D533,948 S *	12/2006	Schaub et al.	.....	D24/229
D576,208 S *	9/2008	Quercetti	.....	D19/37
D598,128 S *	8/2009	Pihl et al.	.....	D24/227

(Continued)

**FOREIGN PATENT DOCUMENTS**

EP 0 976 453 2/2000

**OTHER PUBLICATIONS**

USD—De-nesting syringes, [http://www.boschpackaging.com/moellerdevicon/eng/pdf/USD\\_300\\_Brochure.pdf](http://www.boschpackaging.com/moellerdevicon/eng/pdf/USD_300_Brochure.pdf) (2 pages).  
Optima Packaging Group GmbH, <http://www.pharmaceutical-int.com/suppliers/optima-packaging-machinery-plc.html> printed on Dec. 25, 2011 (2 pages).

(Continued)

*Primary Examiner* — T. Chase Nelson  
*Assistant Examiner* — Mark Cavanna  
(74) *Attorney, Agent, or Firm* — Banner & Witcoff, Ltd.



(57) **CLAIM**

The ornamental design for the medical syringe container, as shown and described.

**DESCRIPTION**

FIG. 1 is a front perspective view of a medical syringe container showing my new design;  
FIG. 2 is a rear perspective view thereof;  
FIG. 3 is a front view thereof;  
FIG. 4 is a rear view thereof;  
FIG. 5 is a left side view thereof;  
FIG. 6 is a right side view thereof;  
FIG. 7 is a top plan view thereof; and,  
FIG. 8 is a bottom view thereof.  
The broken lines represent the portions of the design that form no part of the claim.

**1 Claim, 6 Drawing Sheets**

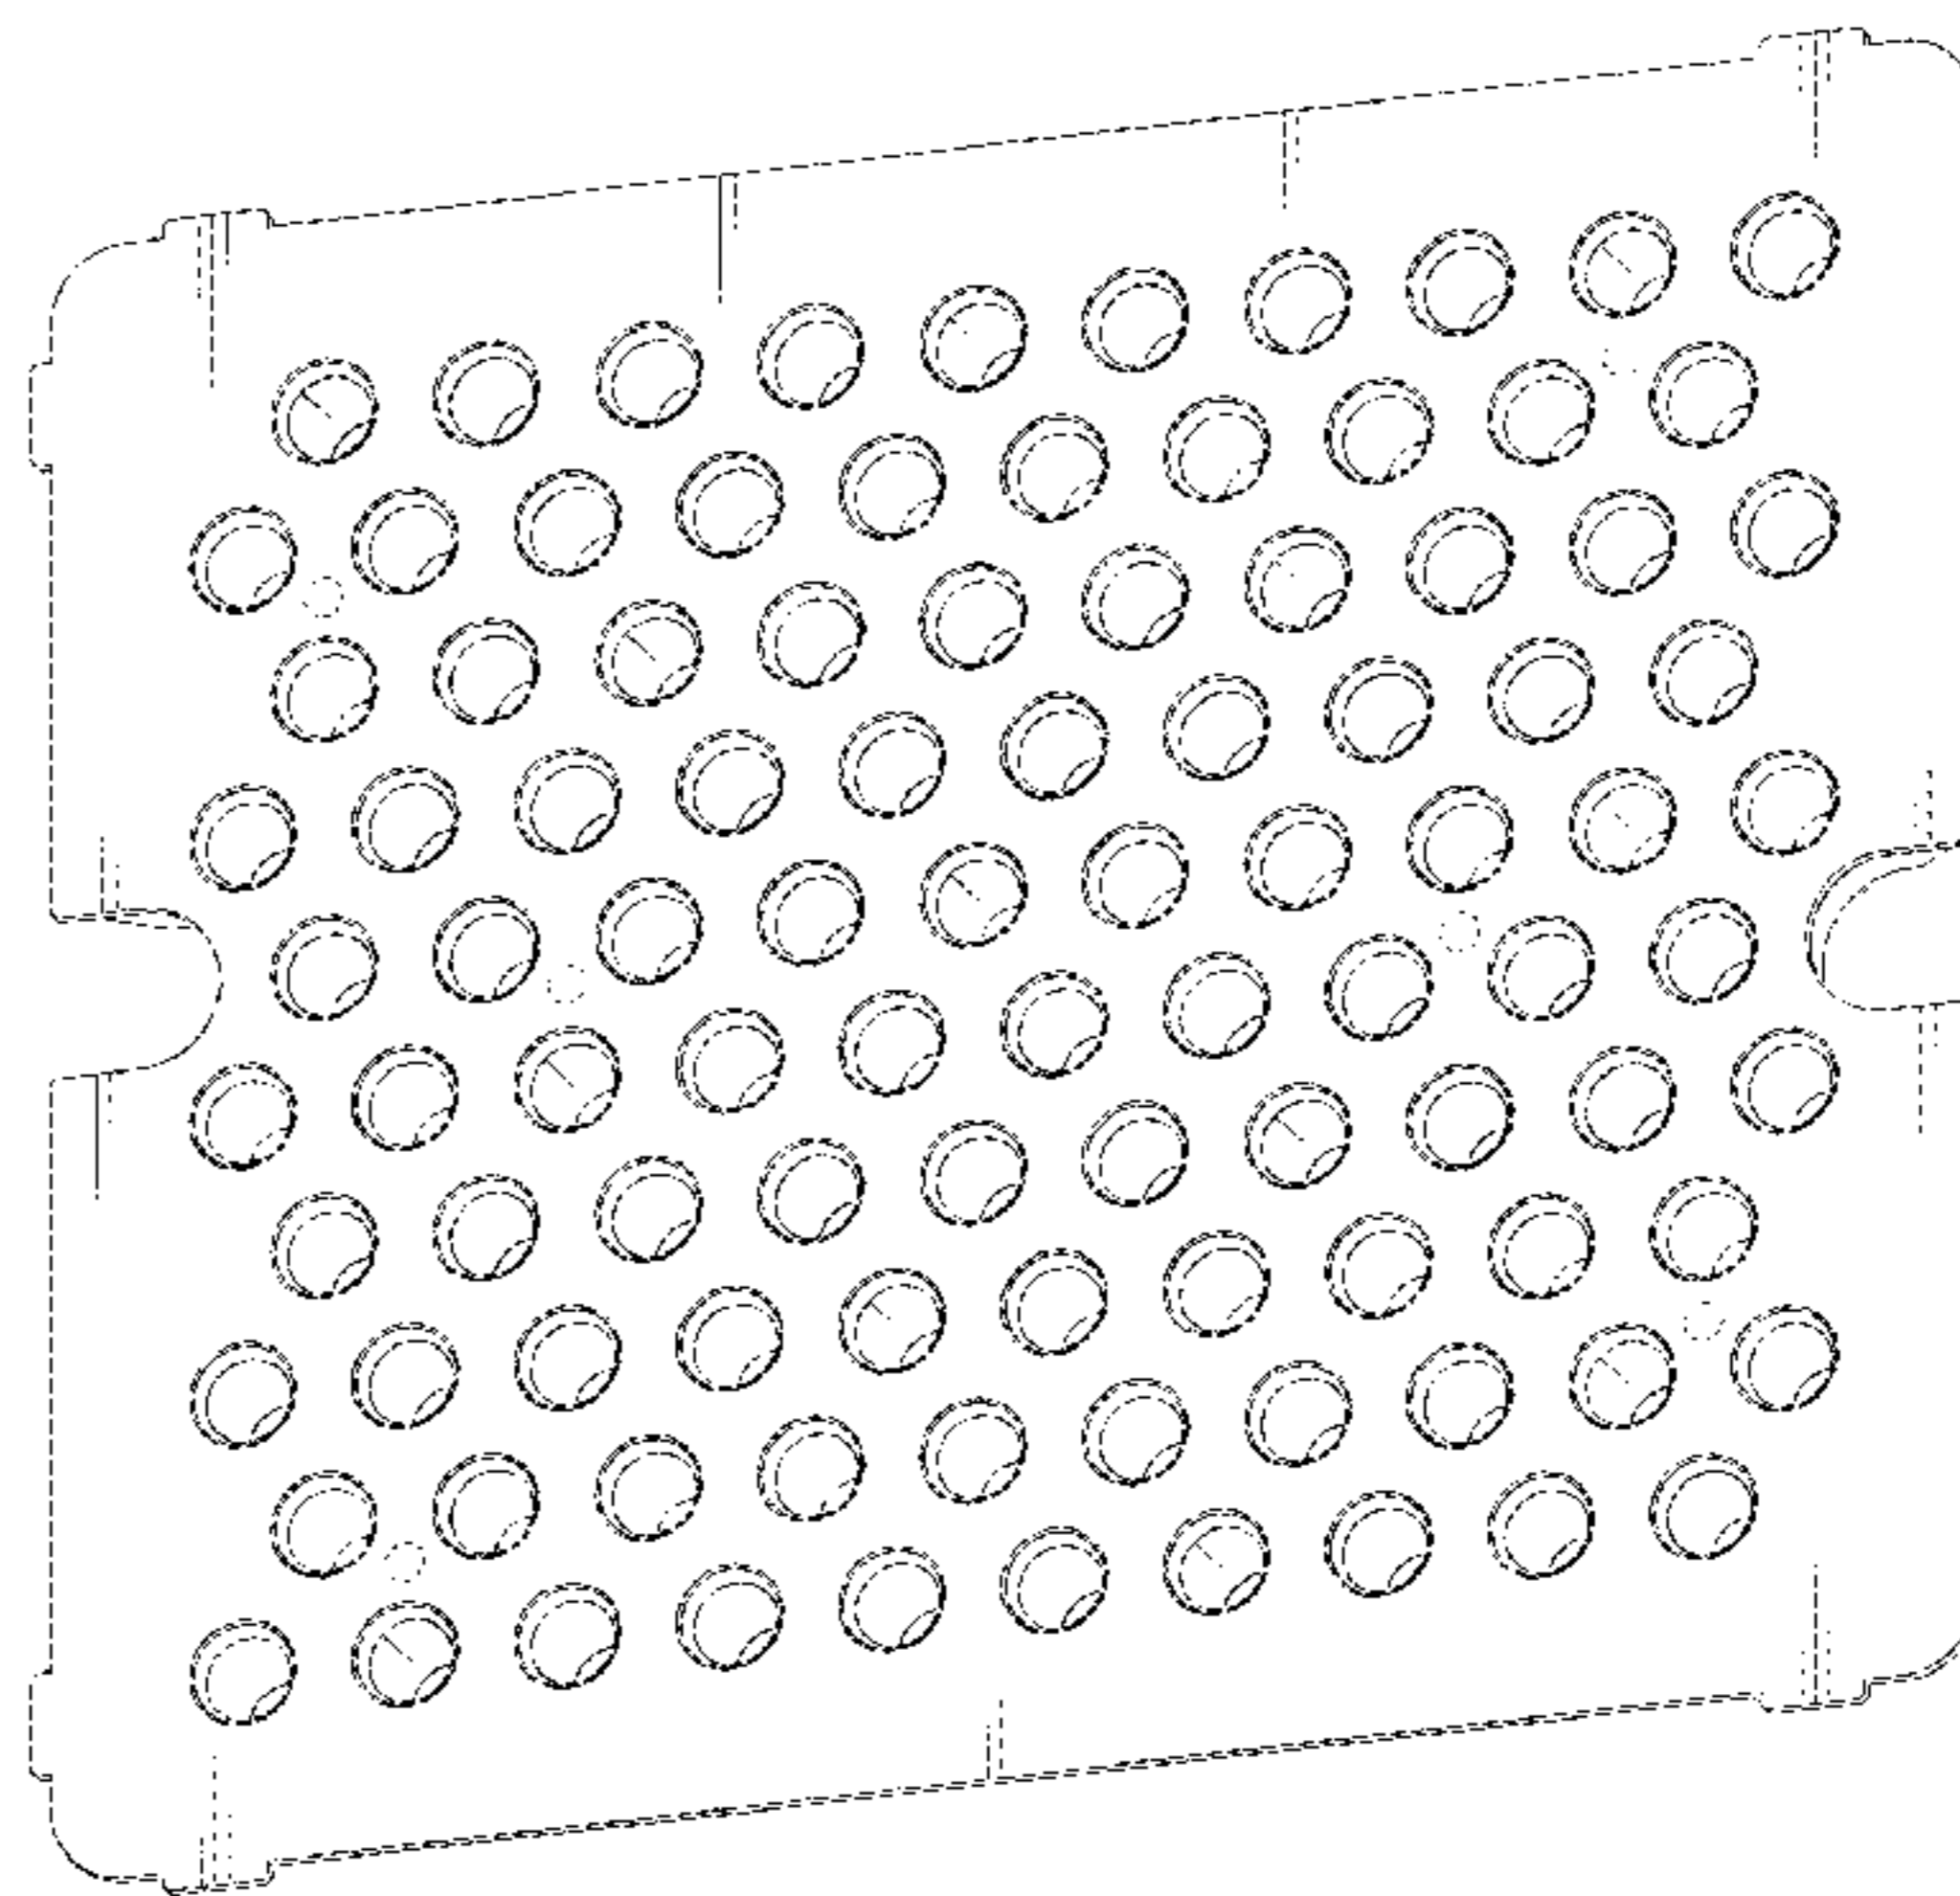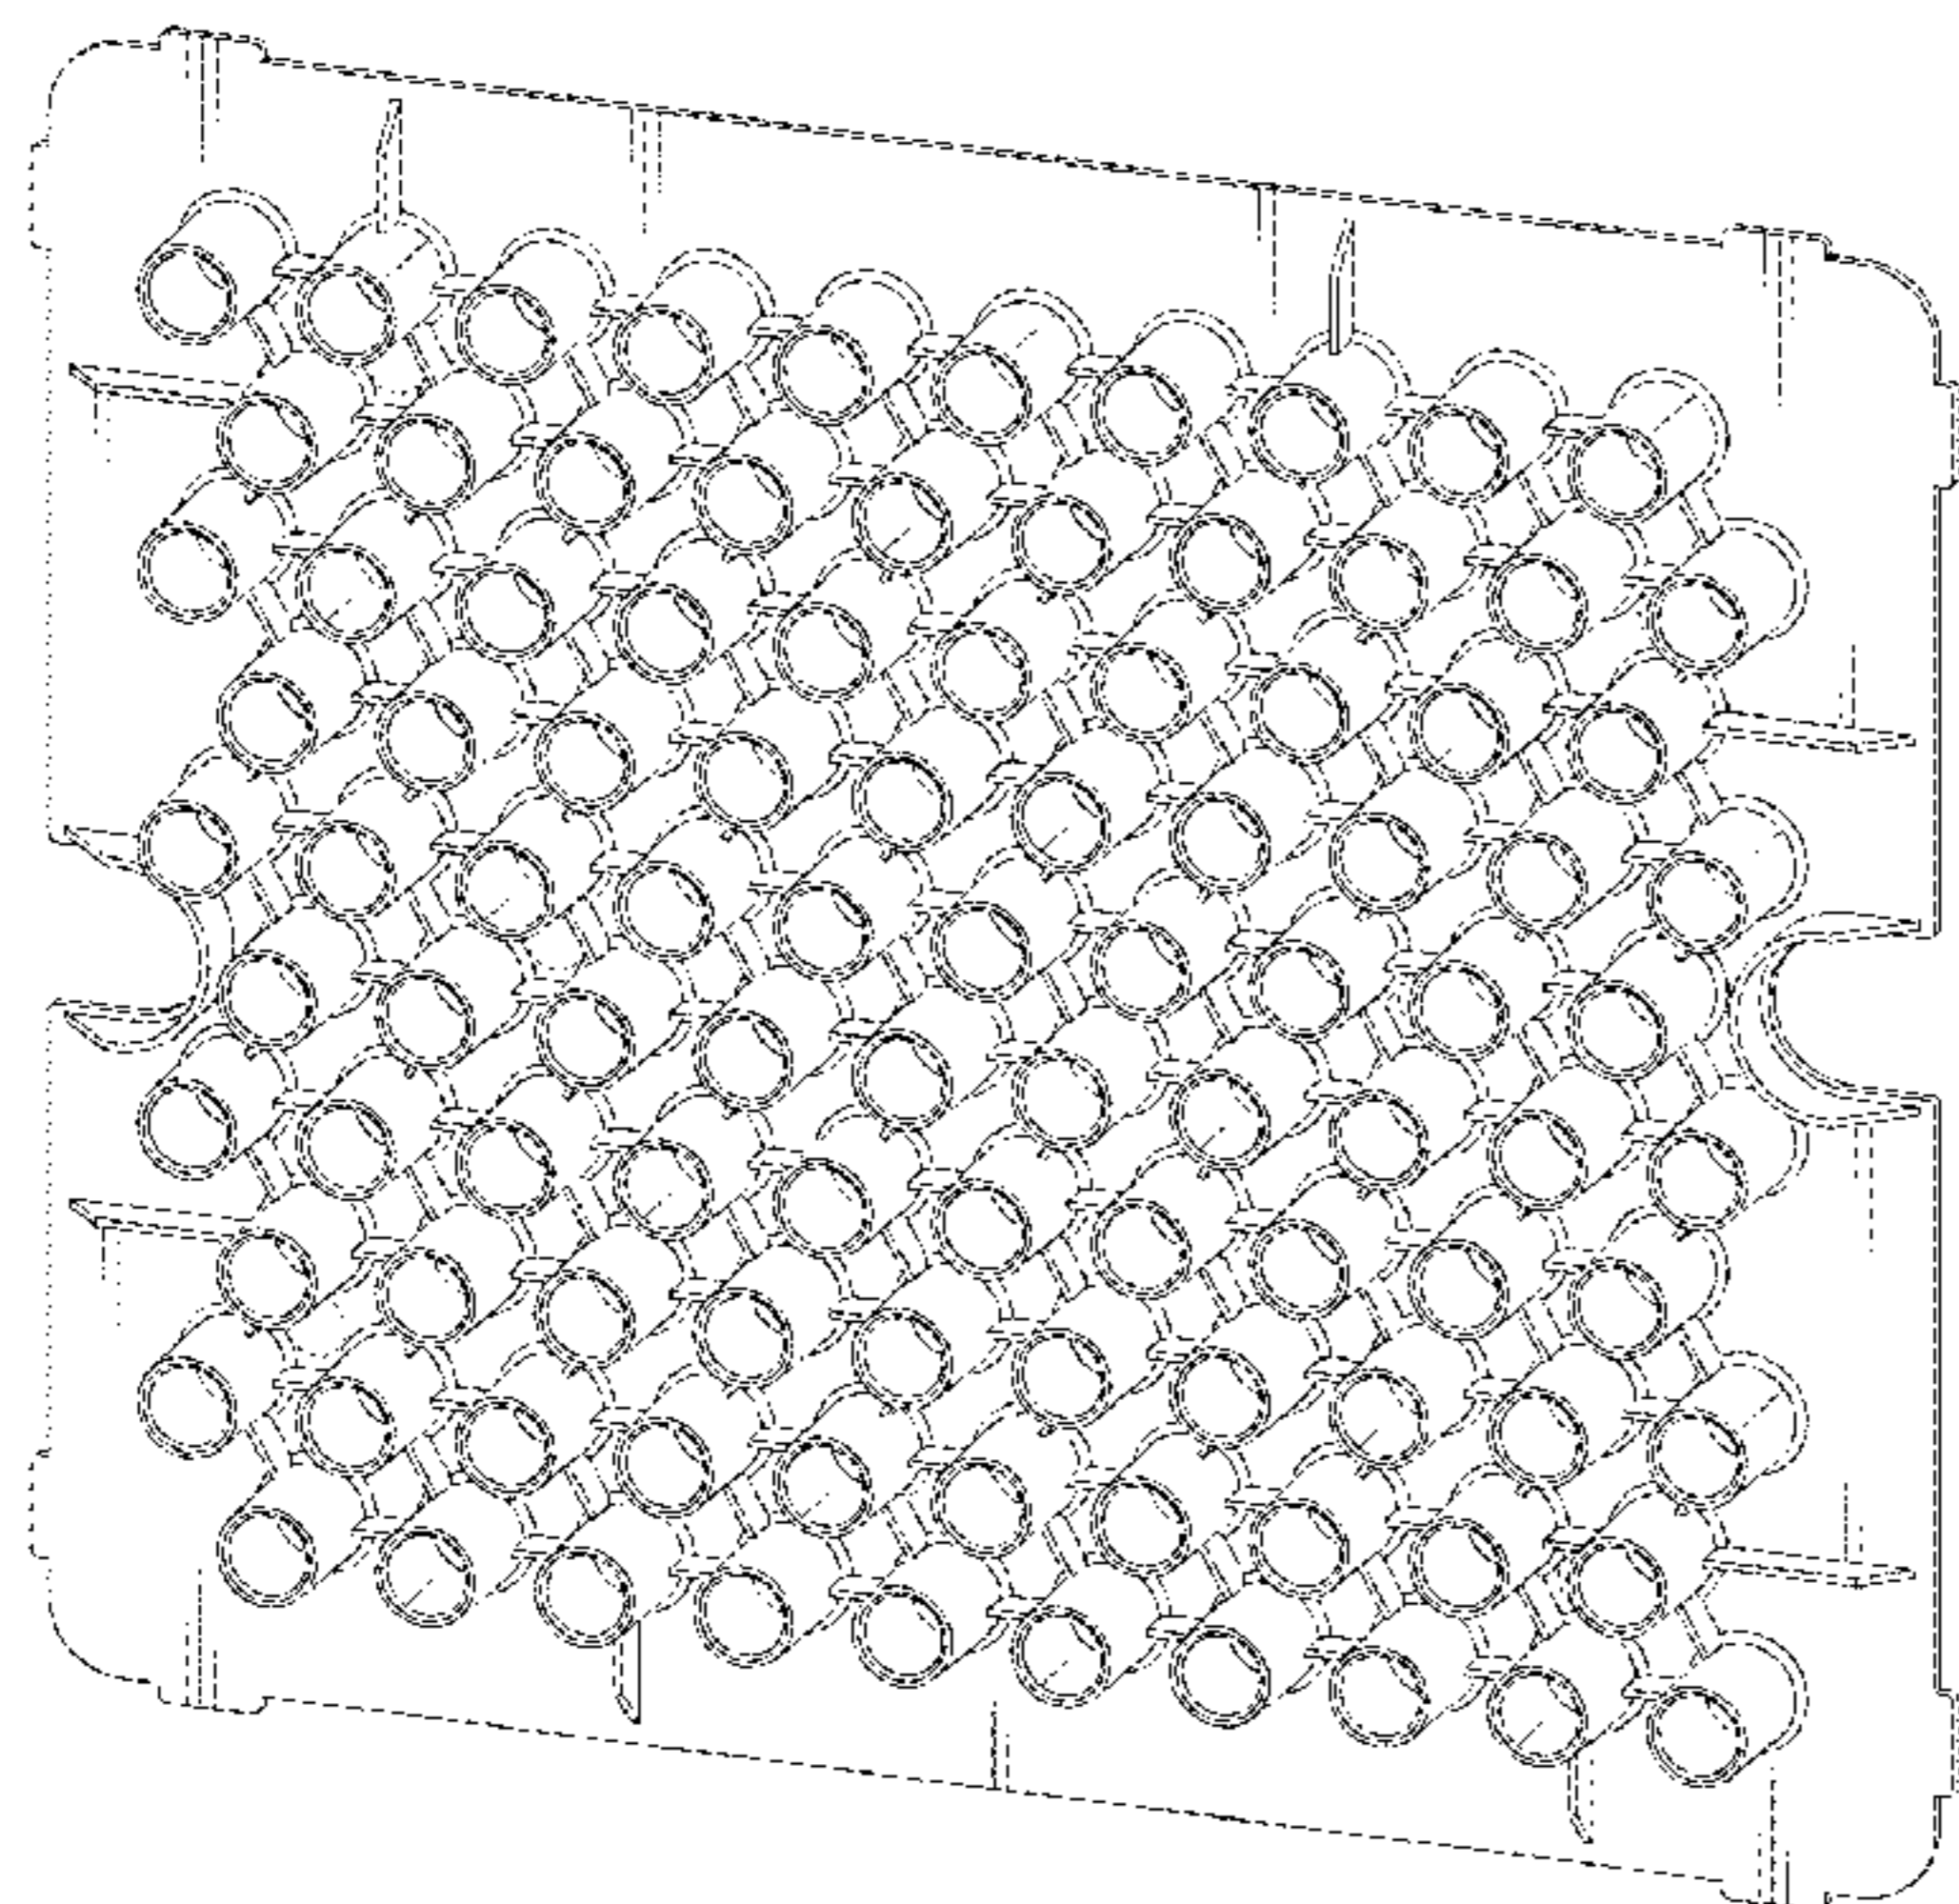

(56)

**References Cited**

U.S. PATENT DOCUMENTS

D601,713 S *	10/2009	Lohn et al. ....	D24/226
D601,714 S *	10/2009	Lohn et al. ....	D24/226
D608,013 S *	1/2010	Coulling et al. ....	D24/224
D620,605 S *	7/2010	Reitze .....	D24/227
D622,860 S *	8/2010	Karpiloff .....	D24/230
D632,404 S *	2/2011	Karpiloff .....	D24/230
D638,138 S *	5/2011	Wong .....	D24/227
D639,447 S *	6/2011	Karpiloff .....	D24/230
D645,156 S *	9/2011	Reitze .....	D24/227
D673,294 S *	12/2012	Motadel .....	D24/227
2011/0192756 A1	8/2011	Hill	

OTHER PUBLICATIONS

Processing Disposable Syringes in Nests, [http://www.bausch-stroebel.com/en/single-use\\_syringes\\_-\\_processing\\_in\\_nest--ene.html](http://www.bausch-stroebel.com/en/single-use_syringes_-_processing_in_nest--ene.html) printed on Dec. 25, 2011 (1 page).  
Gerresheimer Flyer 2008 (1 page).  
BD Hypak Brochure, Listed print date of Nov. 2000 (8 pages).  
Gerresheimer PharmaSystems, Pharmaceutical Systems and Packaging Catalog, BG Form 1200-1-04/05, 31 pages, date unknown, but prior to the filing of this application.  
Schott Pharmaceutical Packaging, Sterile prefillable glass and polymer syringes, Longterm storage and injection system in one, 6 pages, date unknown, but prior to the filing of this application.

\* cited by examiner

Fig. 1

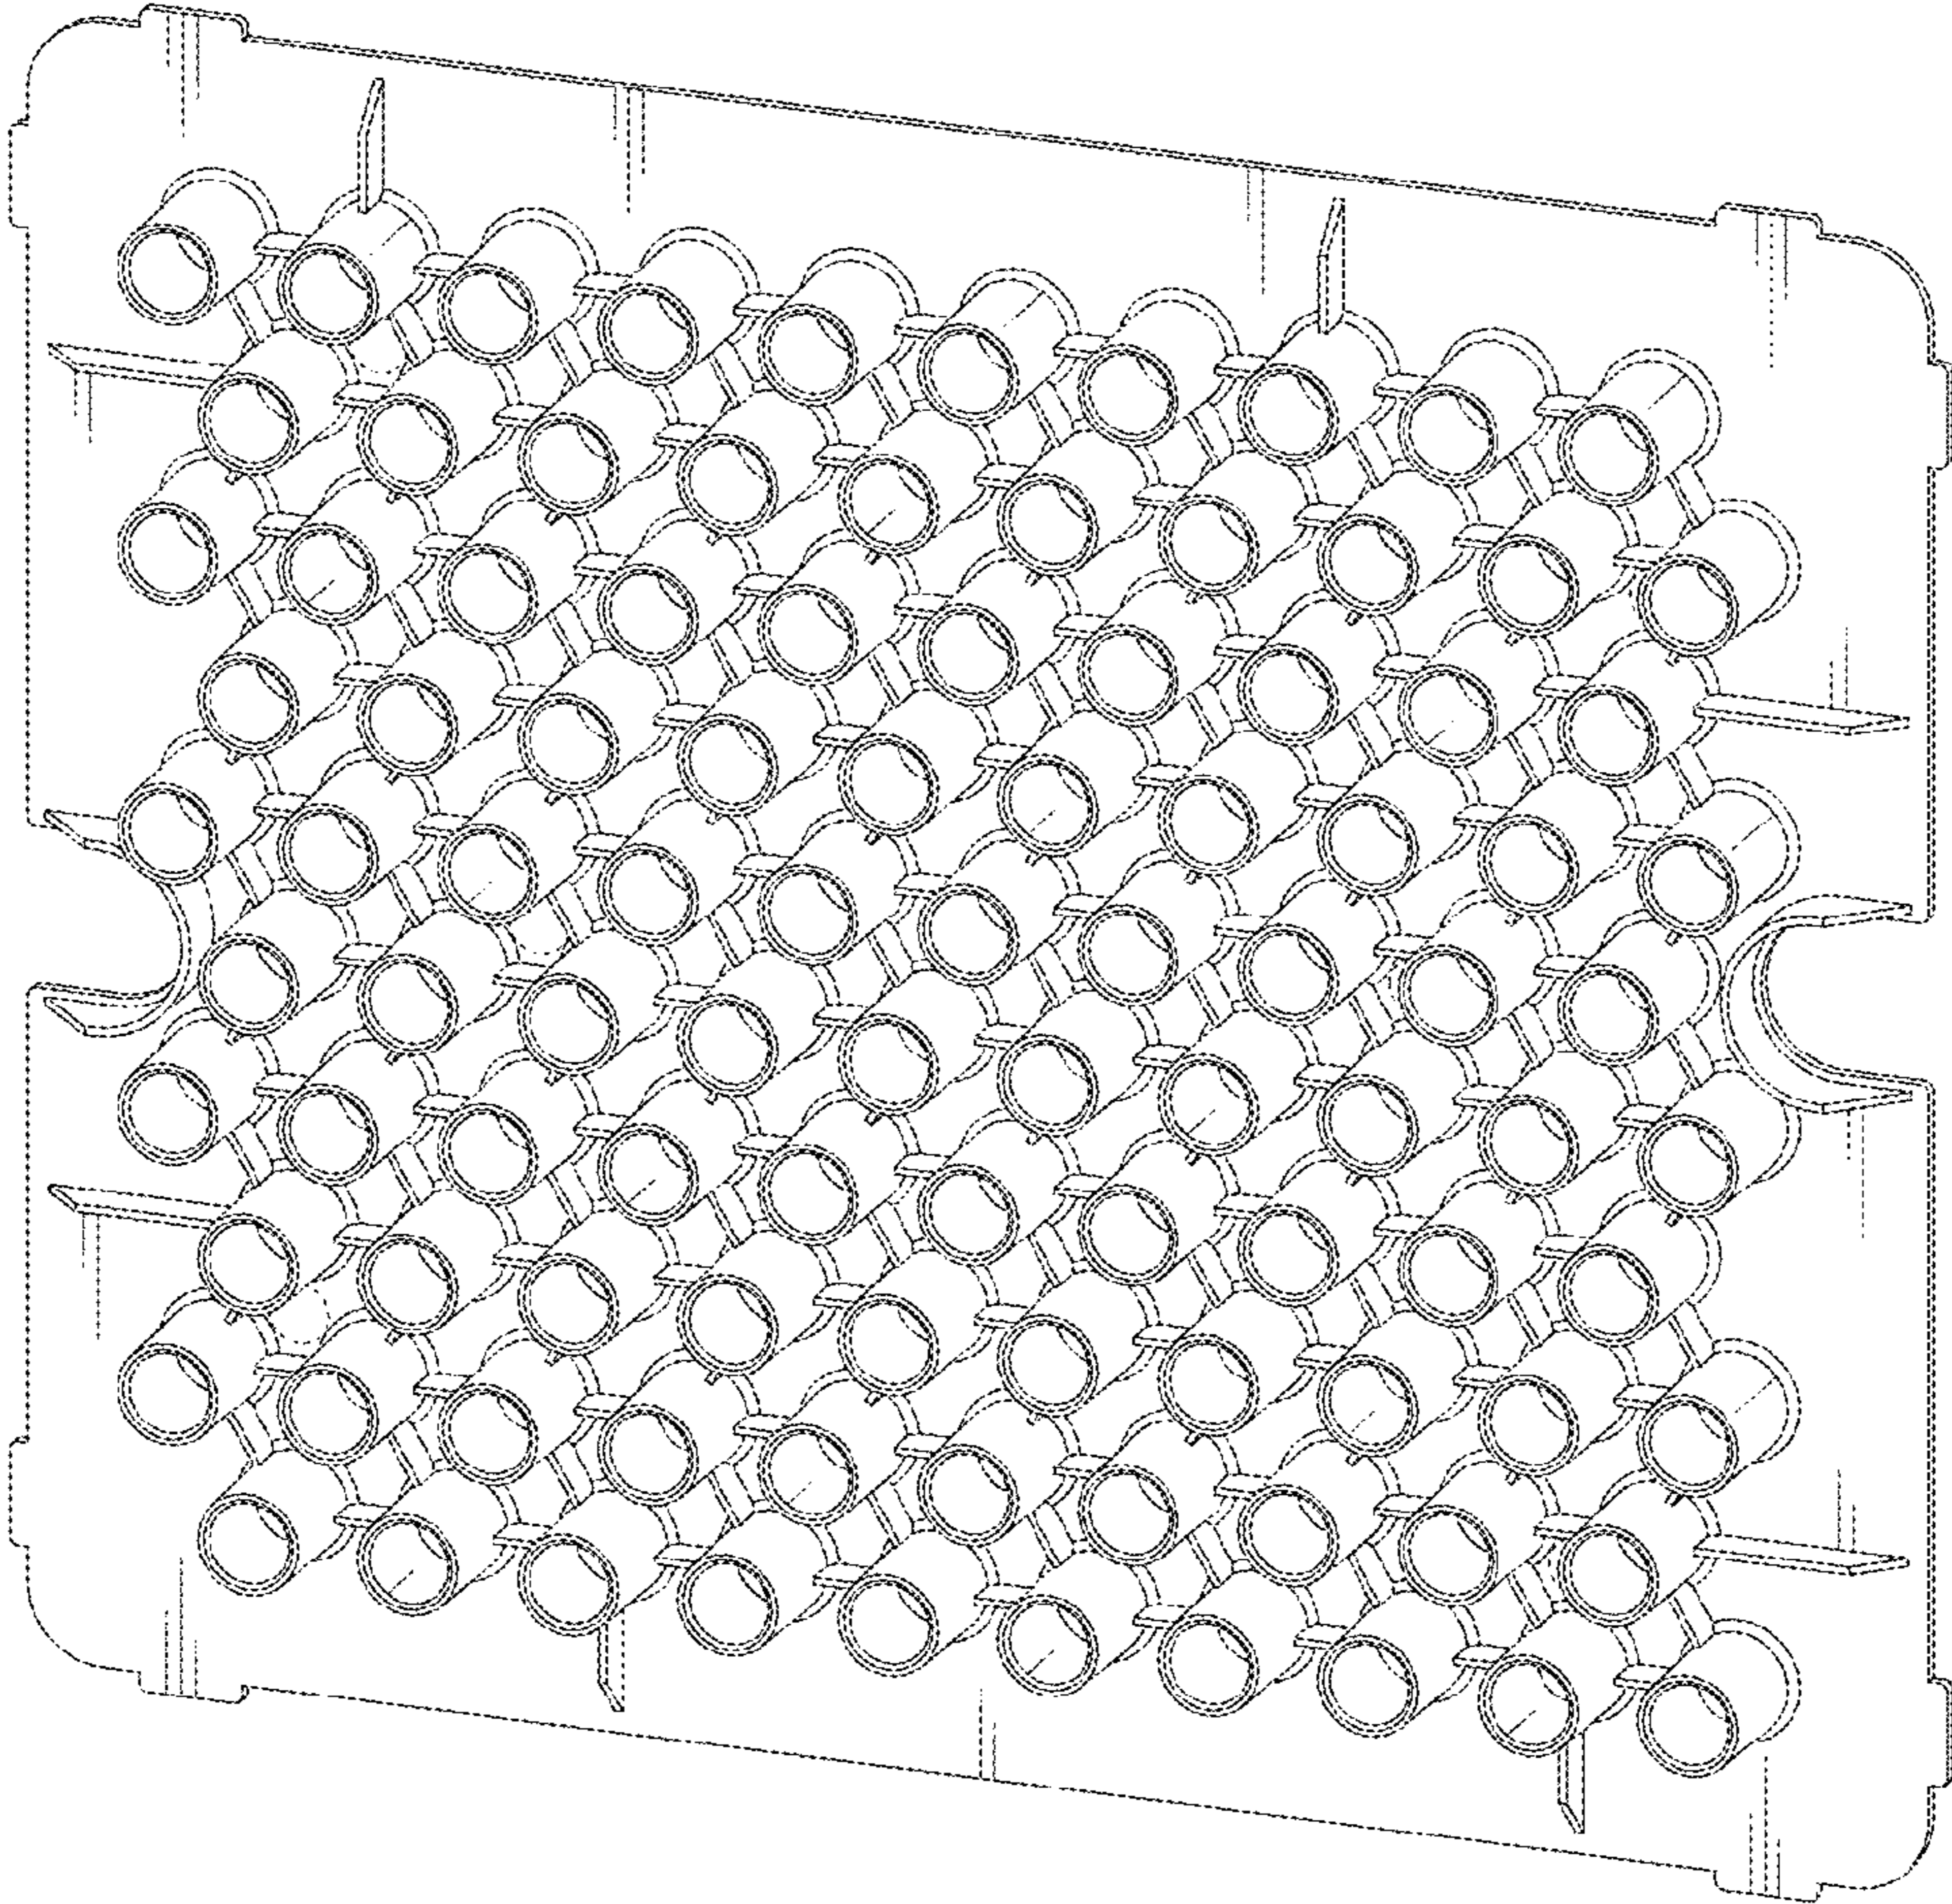


Fig. 2

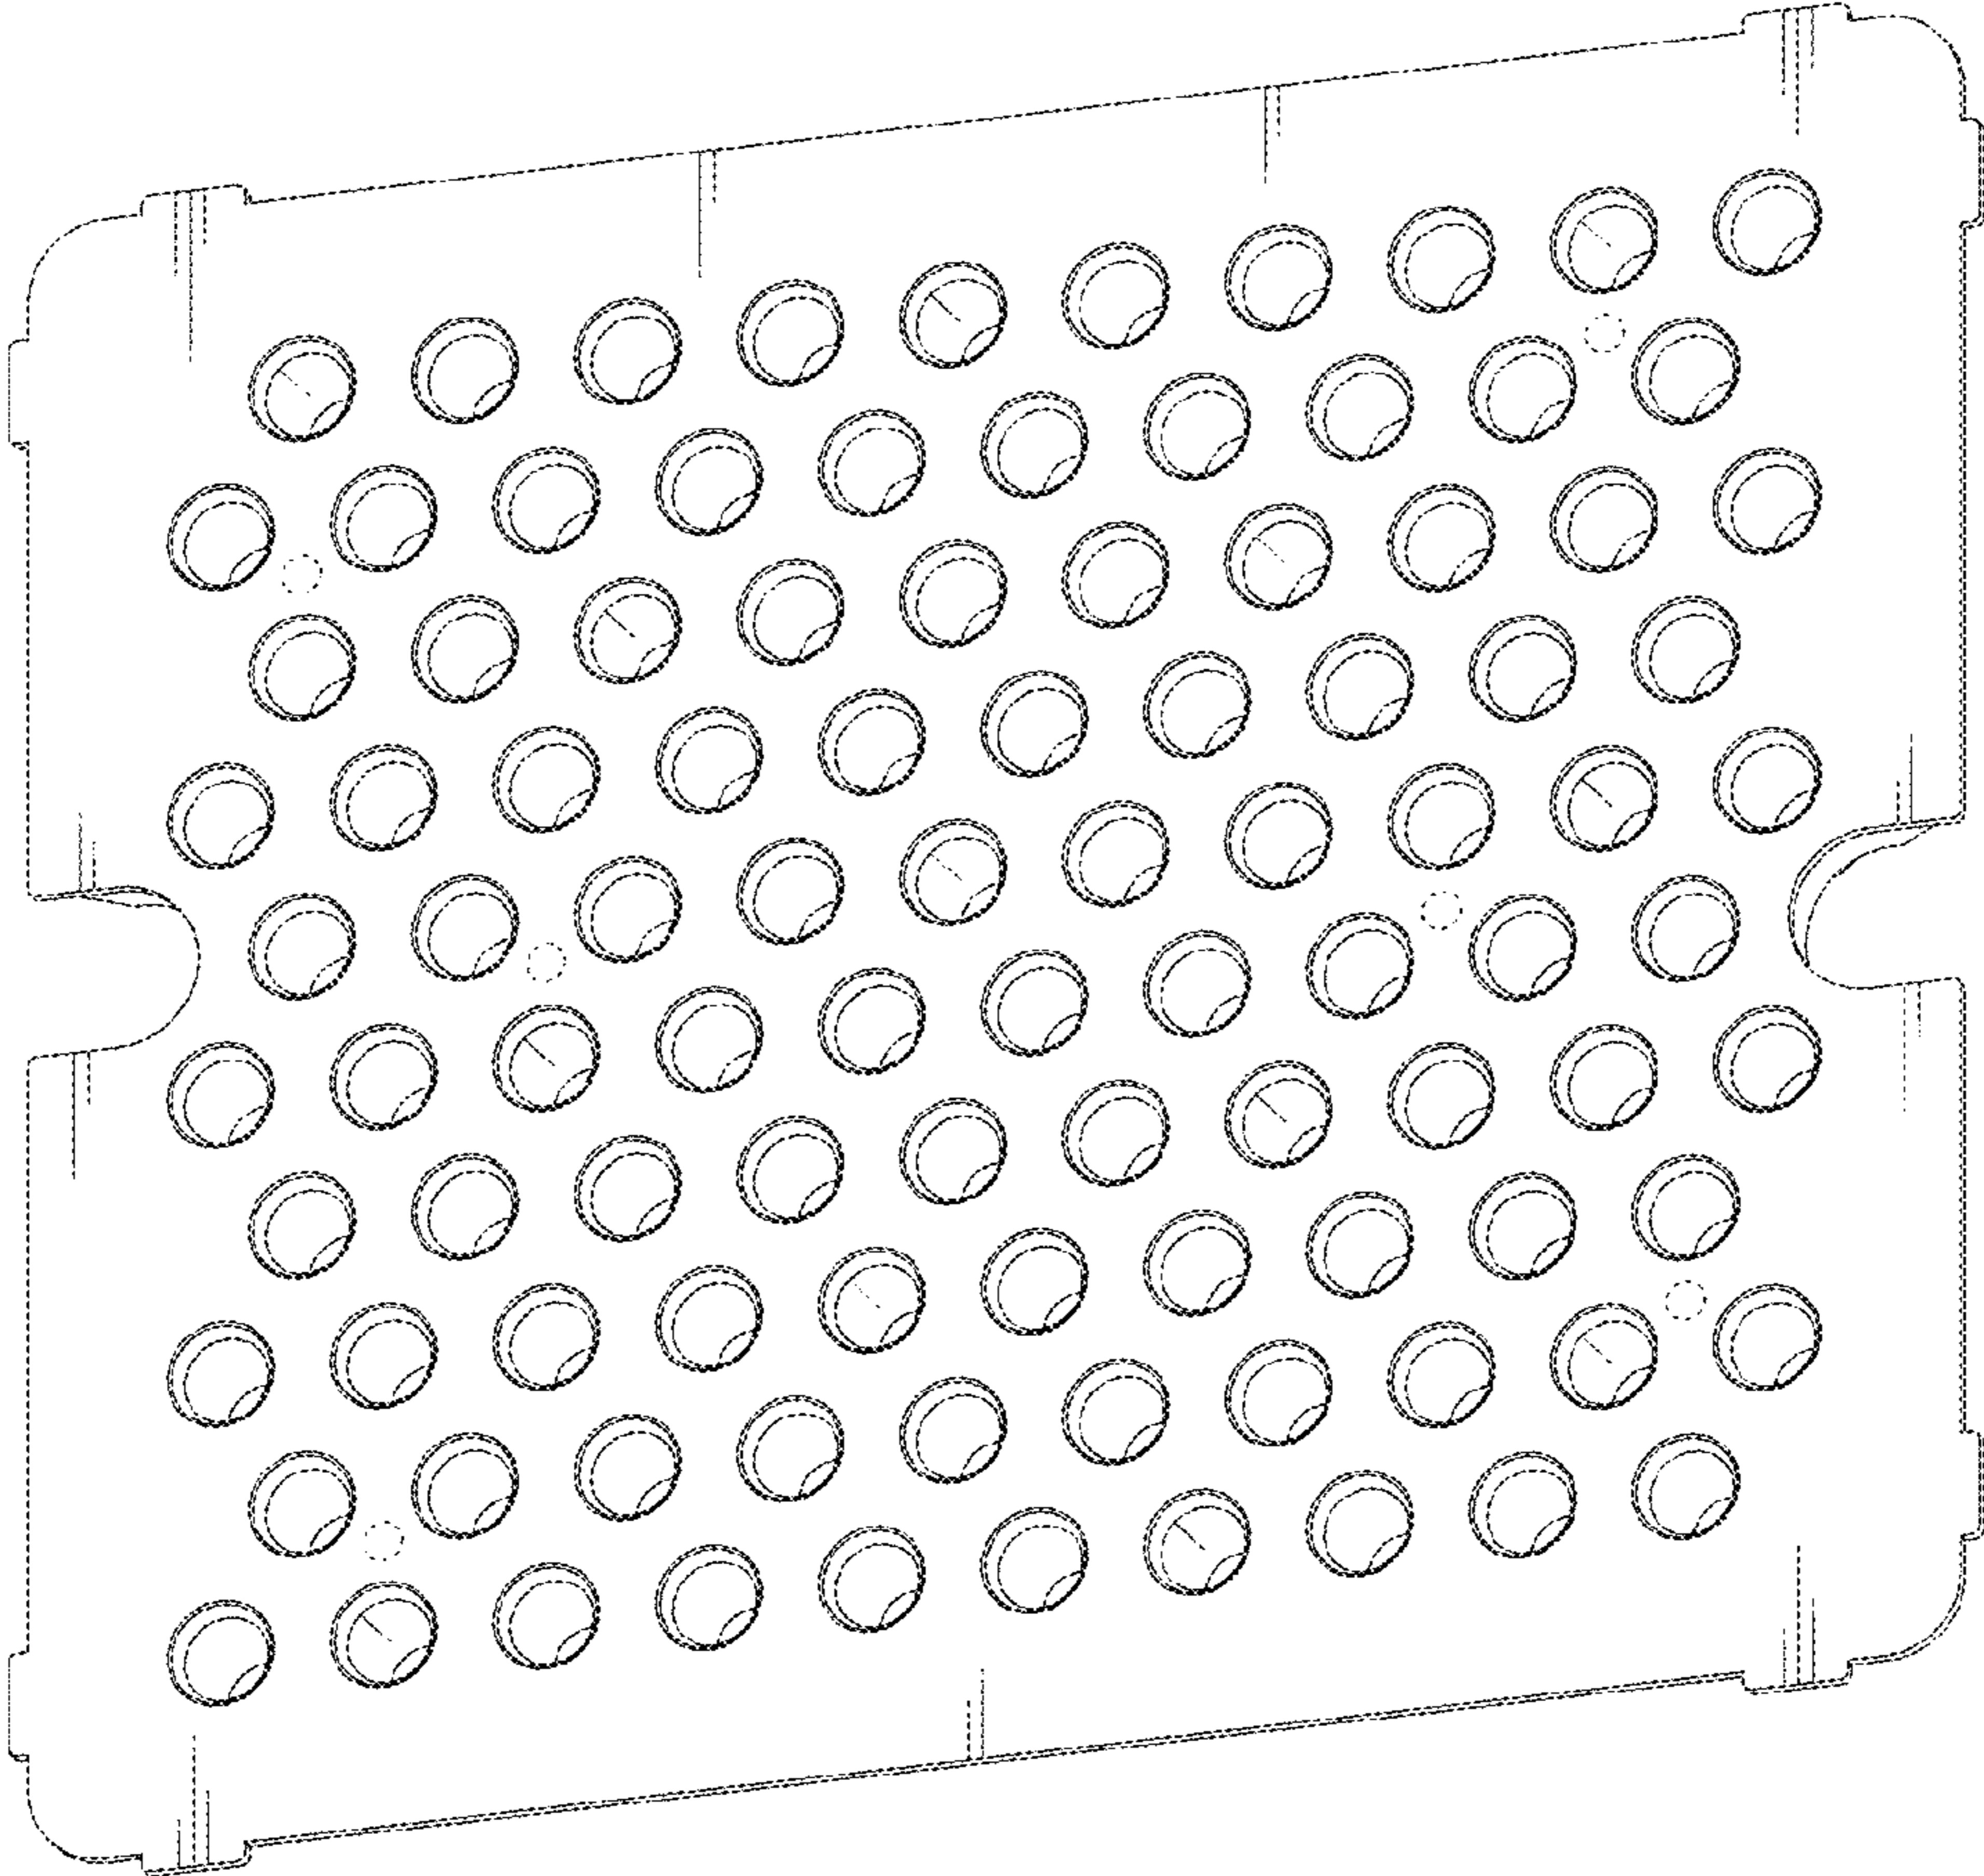


Fig. 3

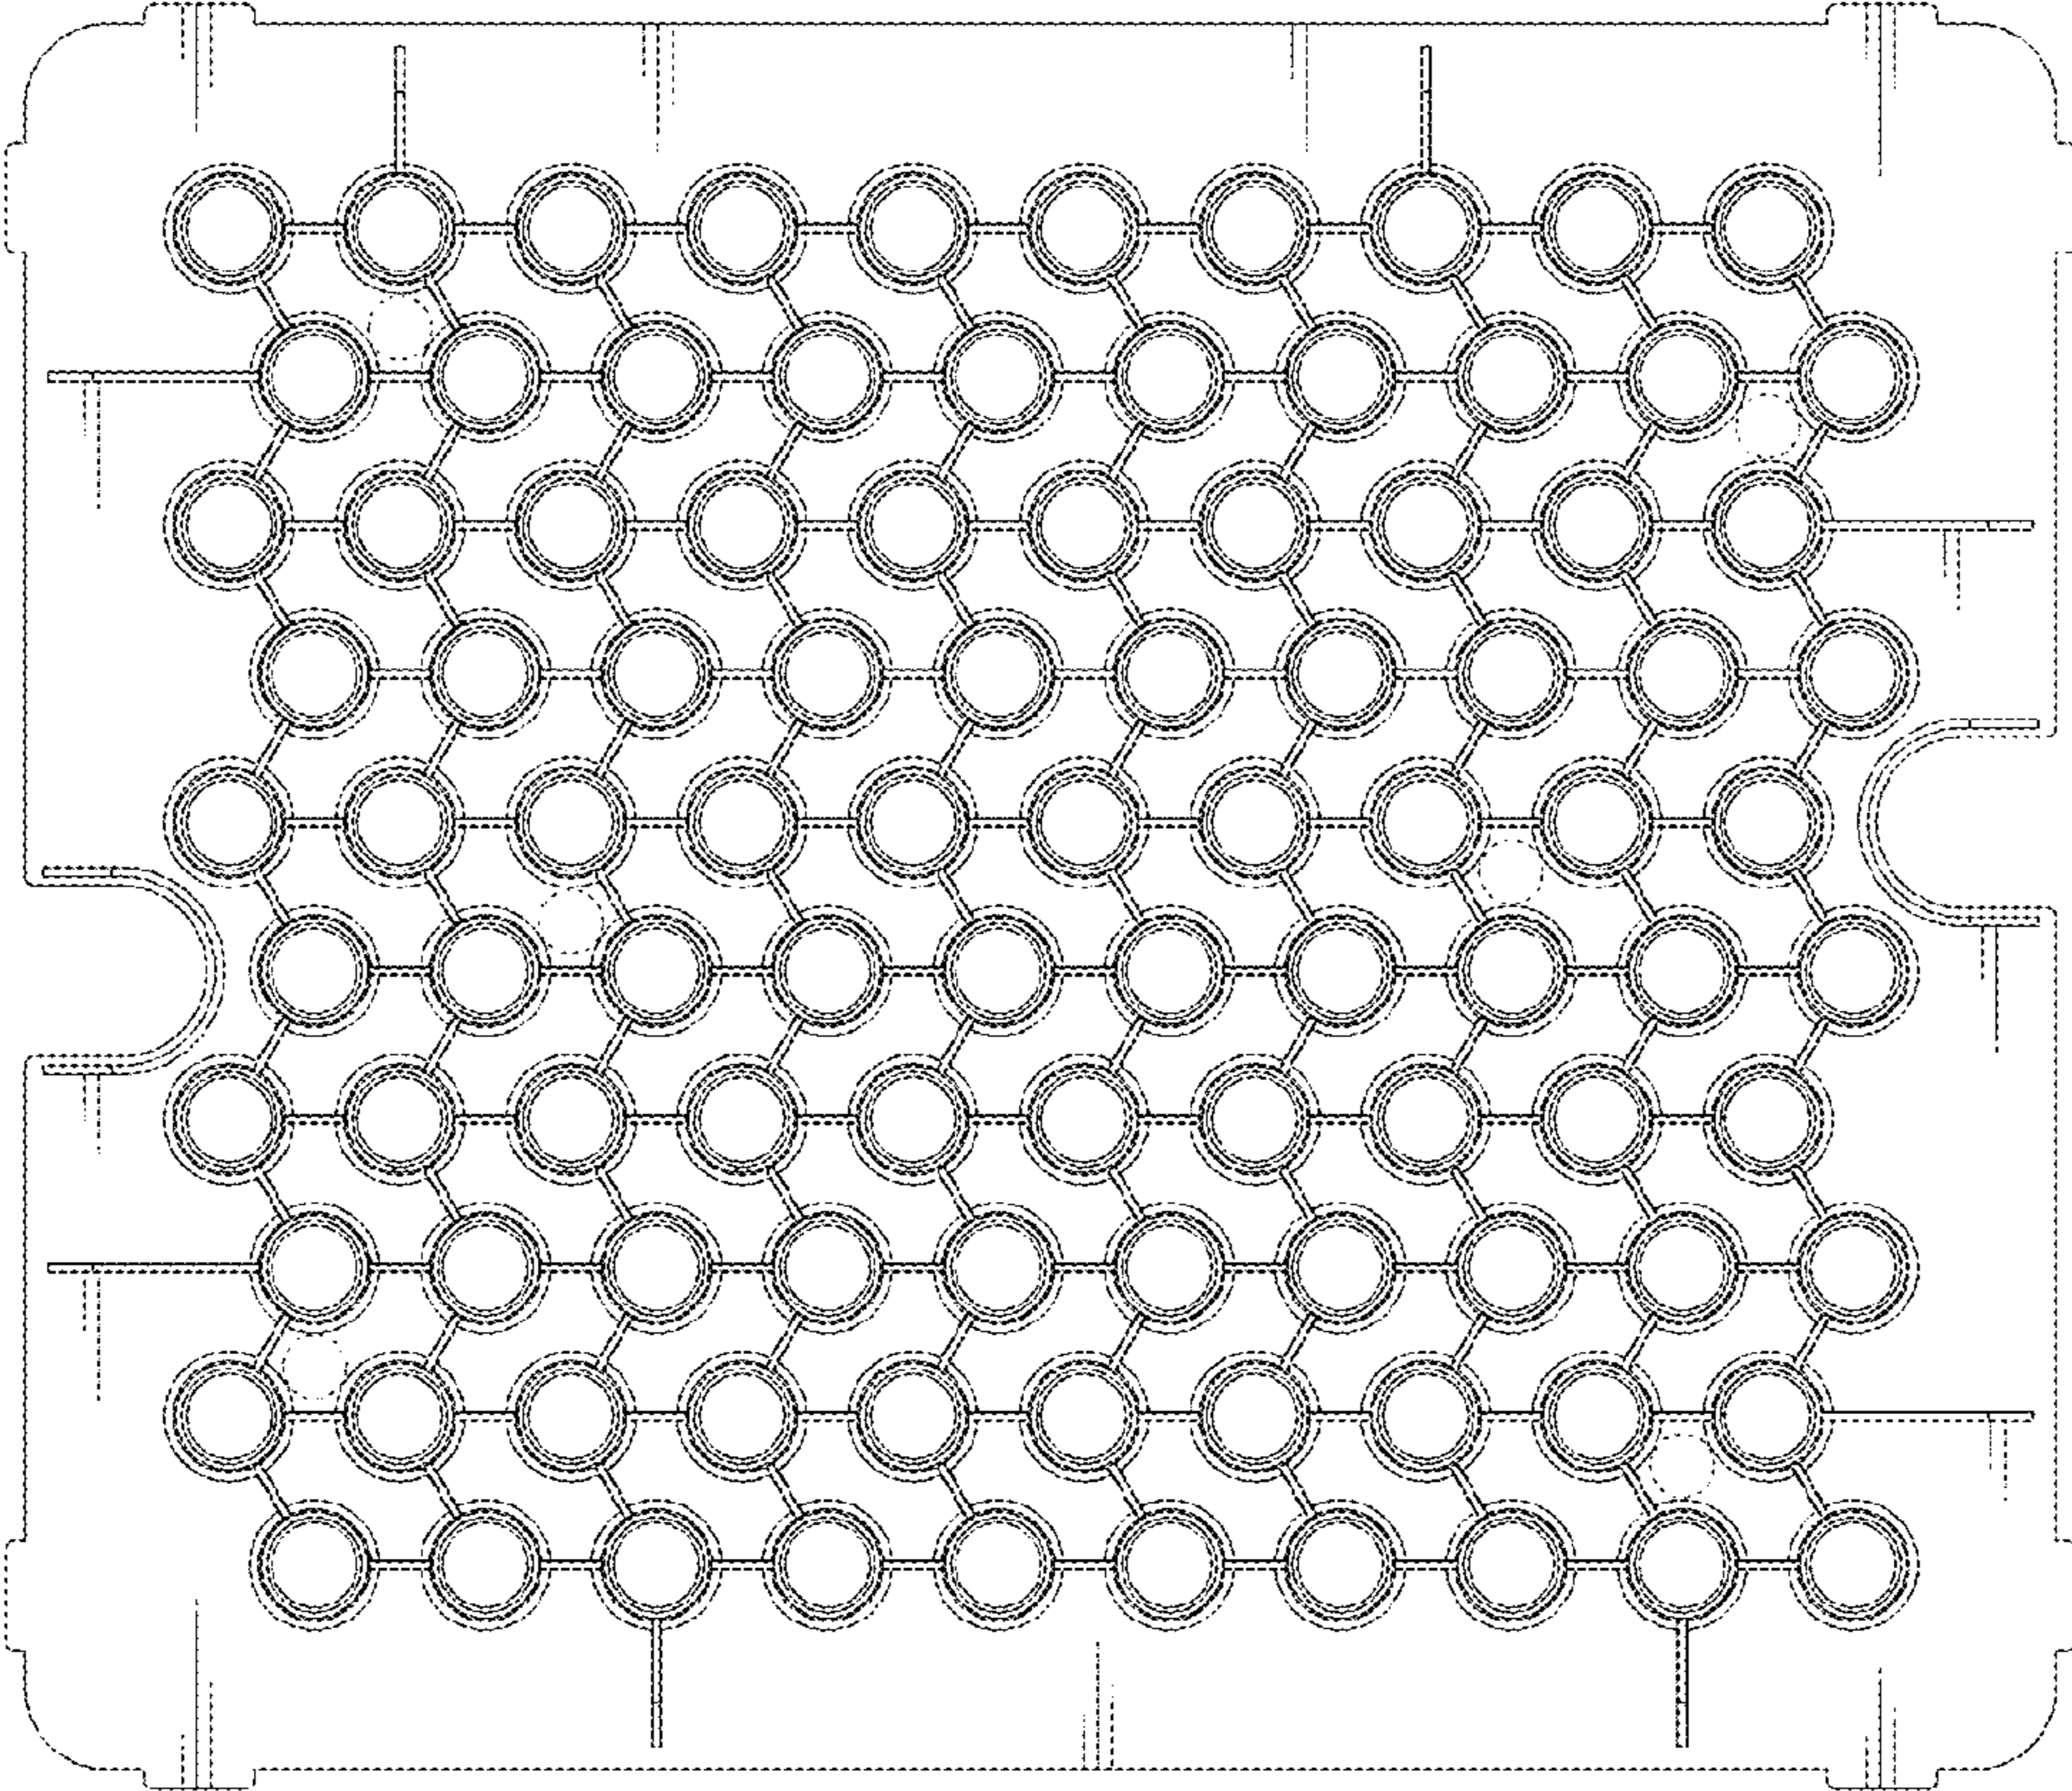


Fig. 4

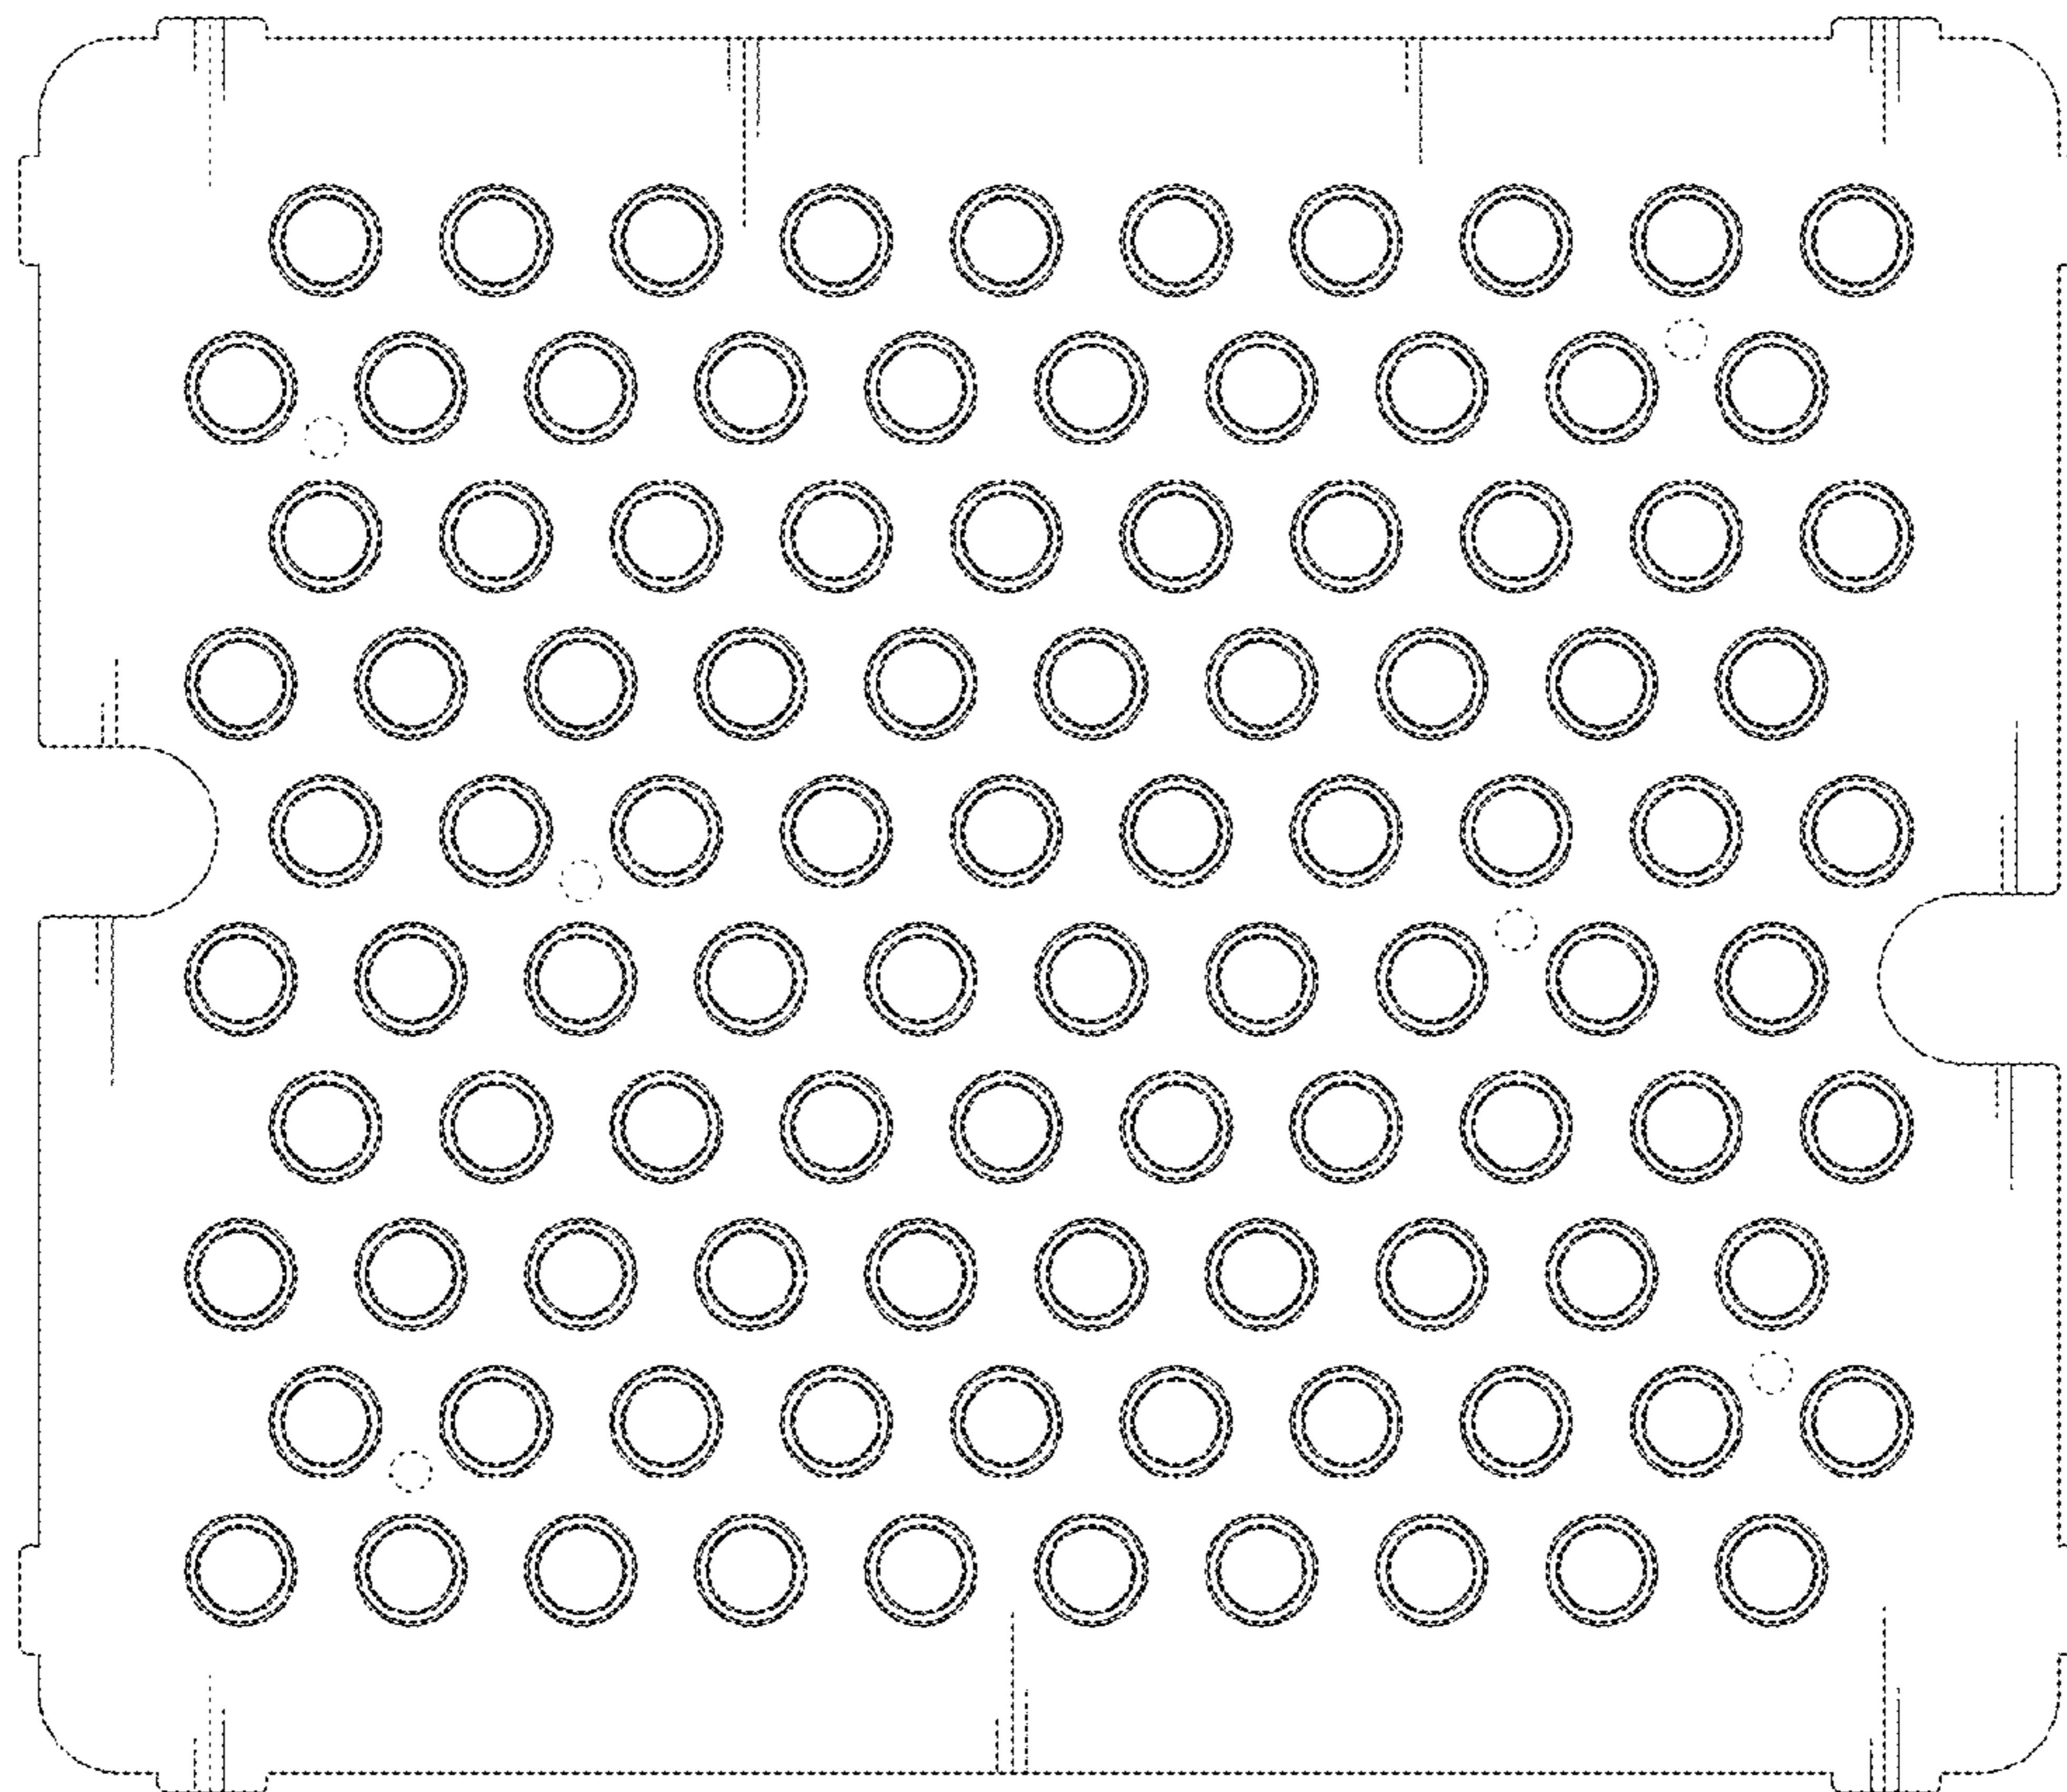


Fig. 5

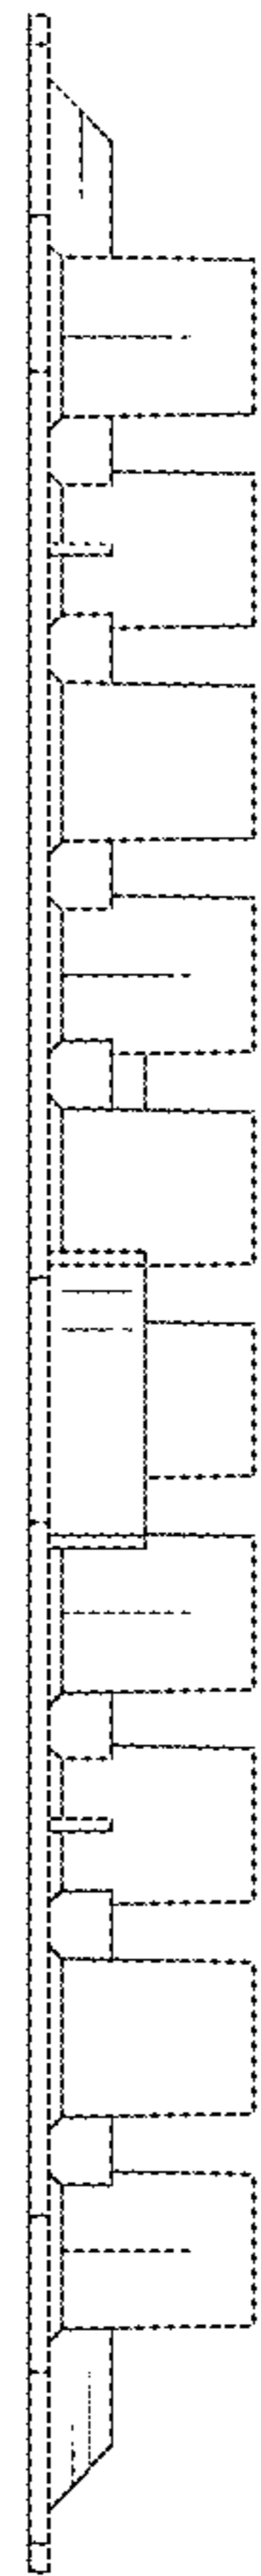


Fig. 6

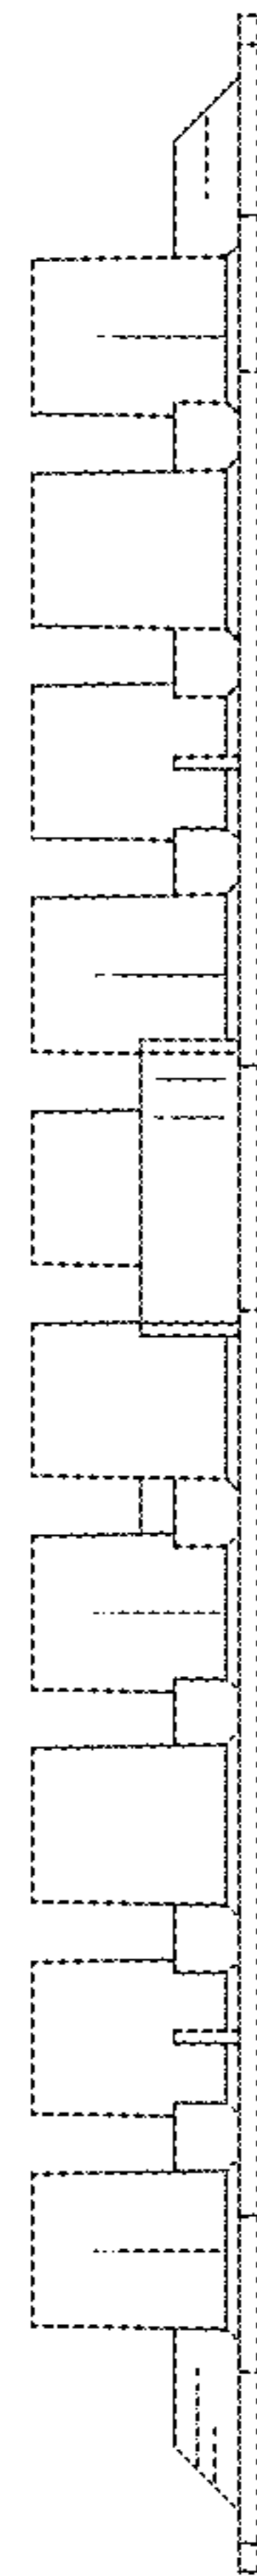


Fig. 7

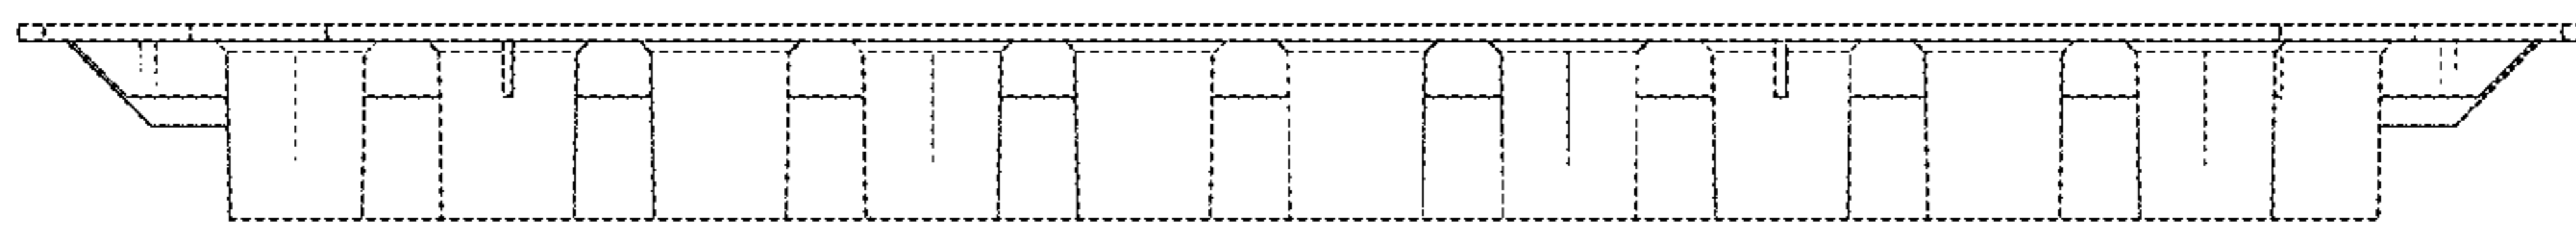


Fig. 8

