



US00D697080S

(12) **United States Design Patent**
Scholz et al.

(10) **Patent No.:** **US D697,080 S**
(45) **Date of Patent:** **** Jan. 7, 2014**

(54) **DISPLAY SCREEN WITH AN ICON**

FOREIGN PATENT DOCUMENTS

(75) Inventors: **Wolfgang Scholz**, Beverly, MA (US);
Stefan P. Nelwan, Rotterdam (NL)

WO 2006033038 A2 3/2006
WO WO 2008064682 6/2008
WO 2009077915 A1 6/2009

(73) Assignee: **Draeger Medical Systems, Inc.**,
Telford, PA (US)

OTHER PUBLICATIONS

(**) Term: **14 Years**

(21) Appl. No.: **29/357,231**

(22) Filed: **Mar. 9, 2010**

Related U.S. Application Data

(63) Continuation of application No.
PCT/US2010/025509, filed on Feb. 26, 2010.

(51) **LOC (10) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/489**

(58) **Field of Classification Search**
USPC D14/485-95; D18/24-33; D19/6, 52;
D20/11; D21/324-33; 715/700-867,
715/973-77; 600/509, 523

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,811,040	A	5/1974	Weinfurt et al.	
3,983,867	A *	10/1976	Case	600/522
6,721,591	B2	4/2004	Wei et al.	
D536,340	S *	2/2007	Jost et al.	D14/485
7,266,408	B2	9/2007	Bojovic et al.	
7,275,218	B2 *	9/2007	Petrella et al.	715/771
7,596,406	B2 *	9/2009	Boese et al.	600/523
7,786,996	B2 *	8/2010	Unger	345/506
8,229,551	B2 *	7/2012	Xue	600/509
2004/0056859	A1 *	3/2004	Ohba et al.	345/426
2009/0275846	A1	11/2009	Costa Ribalta et al.	
2011/0060234	A1 *	3/2011	Zhou et al.	600/509
2012/0083706	A1 *	4/2012	Nelwan et al.	600/523

ACC/AHA 2002 Guideline Update for Management of Patients with Unstable Angina and Non-ST-Segment Elevation Myocardial Infarction, J Am Coll Cardiol 2002; 40:1366-1374.

Anderson et al., "The ST Compass: spatial visualization of ST-segment deviations and estimation of the ST injury vector," ScienceDirect, Journal of Electrocardiology, www.jecgonline.com; vol. 43, Issue 2, pp. 121-131, Mar. 2010.

Bacharova et al., "The Dipolar ElectroCARDioTOpographic (DECARTO) like method for graphic presentation of location and extent of area at risk estimated from ST-segment deviations in patients with acute myocardial infarction," ScienceDirect, Journal of Electrocardiology 42 (2009) 172-180.

(Continued)

Primary Examiner — Melanie H Tung

(74) *Attorney, Agent, or Firm* — Mintz Levin Cohn Ferris Glovsky and Popeo, P.C.

(57) **CLAIM**

The ornamental design for a display screen with an icon, as shown and described.


DESCRIPTION

FIG. 1 is a front view of a display screen with an icon; and, FIG. 2 is a front view of a second embodiment thereof.

The broken line showing in both views forms no part of the claimed design.

Graphic display of electrocardiogram (ECG) data, such ST segment elevation/depression, in form of an icon on a display screen during a medical evaluation or procedure.

1 Claim, 2 Drawing Sheets

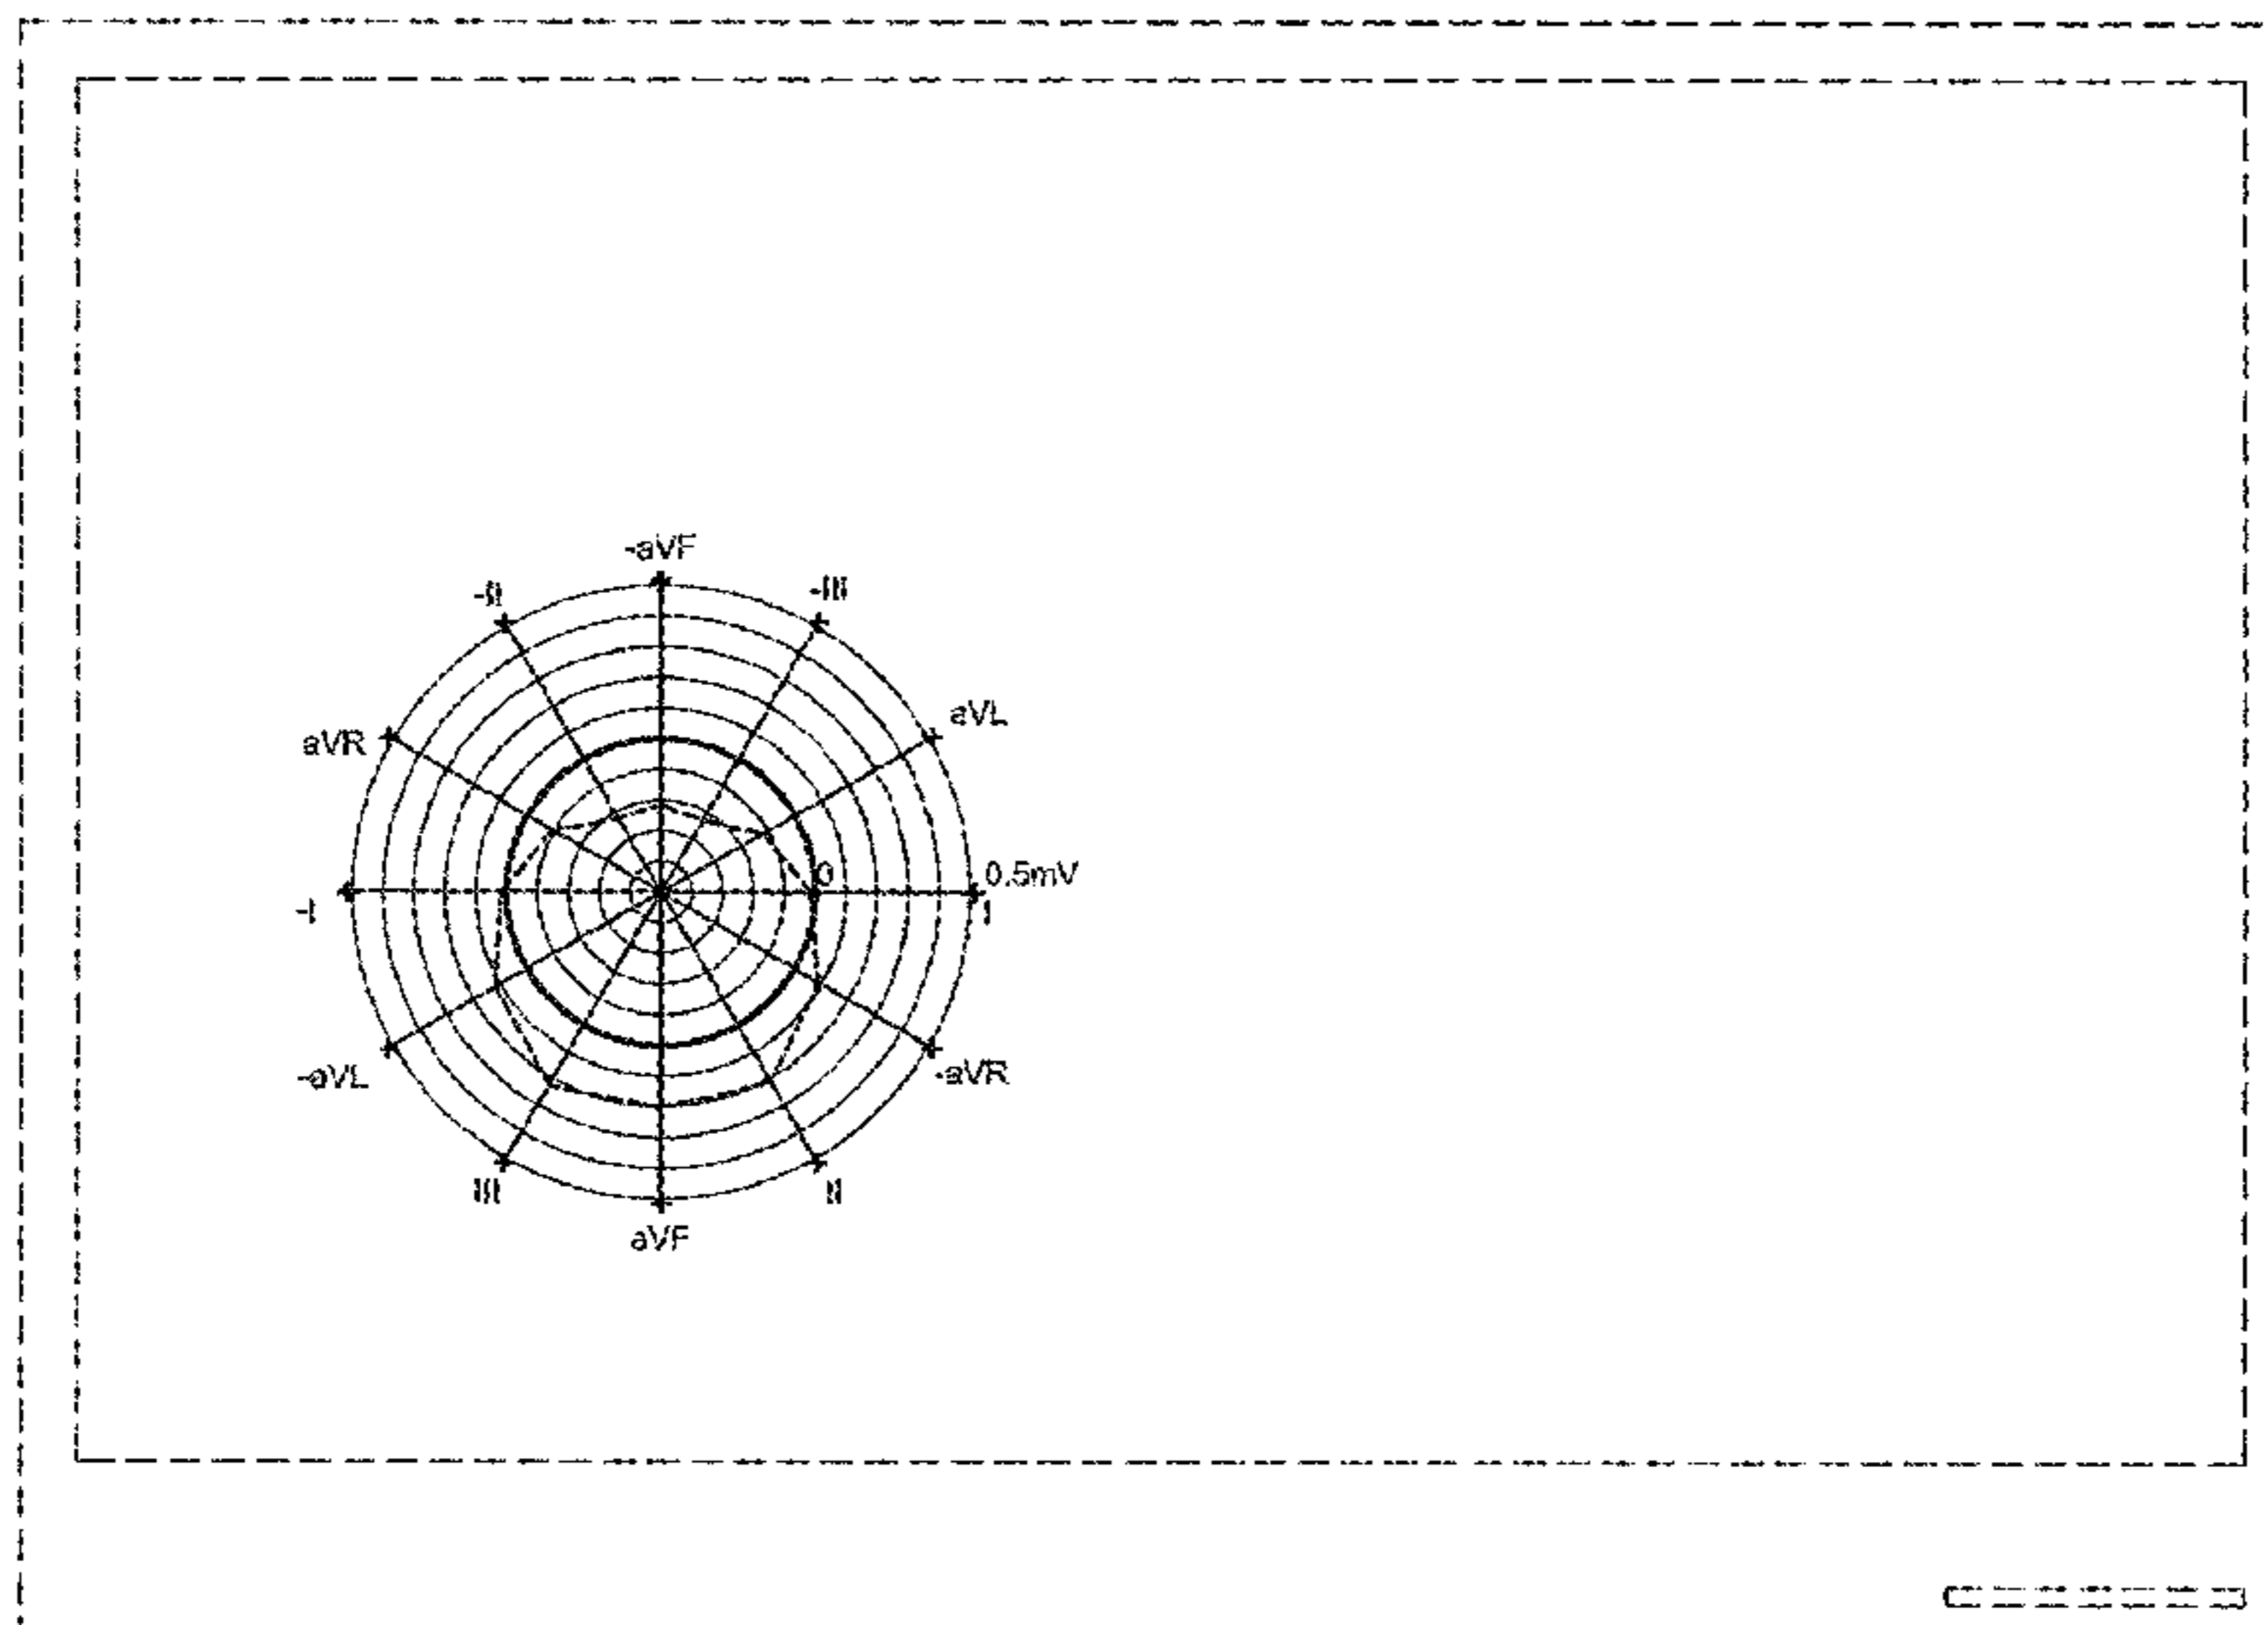

(56)

References Cited

OTHER PUBLICATIONS

Drew et al., "Comparison of a New Reduced Lead Set ECG With the Standard ECG for Diagnosing Cardiac Arrhythmias and Myocardial Ischemia," *Journal of Electrocardiology* vol. 35 Supplement 2002.
Horacek, et al., "On designing and testing transformations for derivation of standard 12-lead/18-lead electrocardiograms and vectorcardiograms from reduced sets of predictor leads," *ScienceDirect, Journal of Electrocardiology* 41 (2008) 220-229.

Pahlm-Webb, et al., "A New Method for Using the Direction of ST-Segment Deviation to Localize the Site of Acute Coronary Occlusion: The 24-View Standard Electrocardiogram," *Am J Med.* 2002; 113: 75-78.

Van Herpen, et al., "Are Additional Right Precordial and Left Posterior ECG Leads Useful for the Diagnosis of Right Ventricular Infarct and Posterior Infarct?" *Journal of Electrocardiology* vol. 32 Supplement 1999.

* cited by examiner

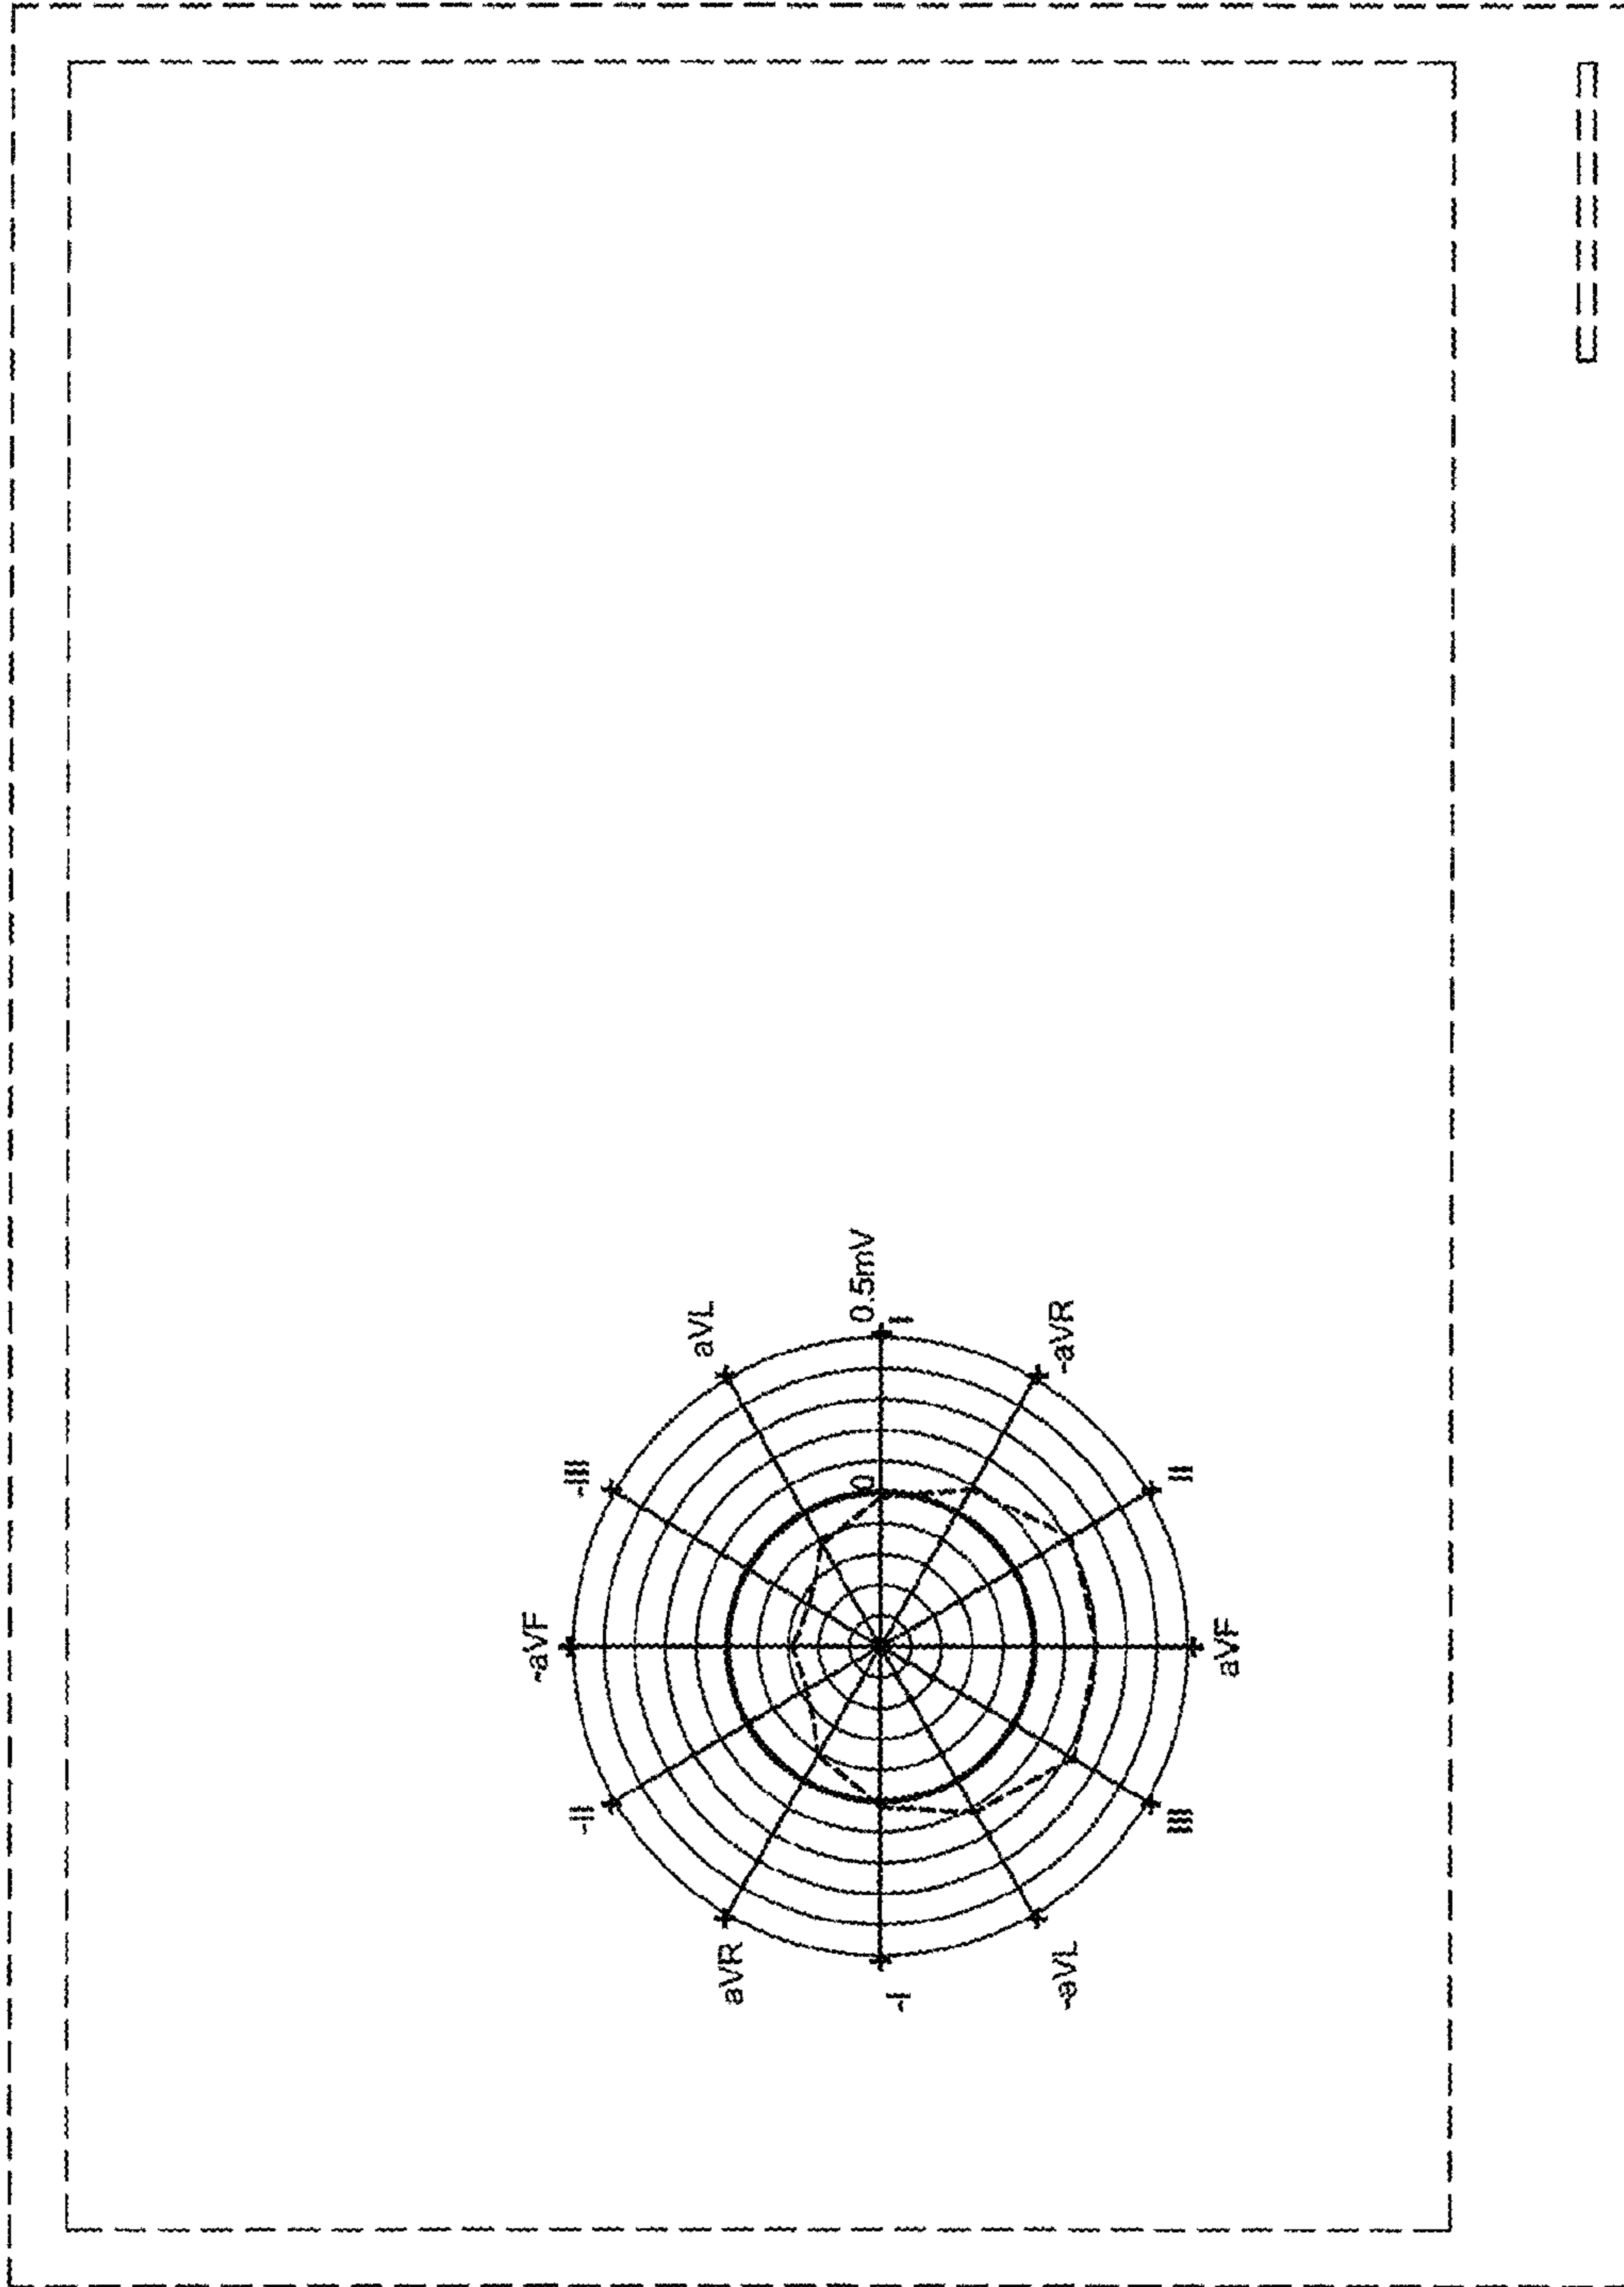


Figure 1

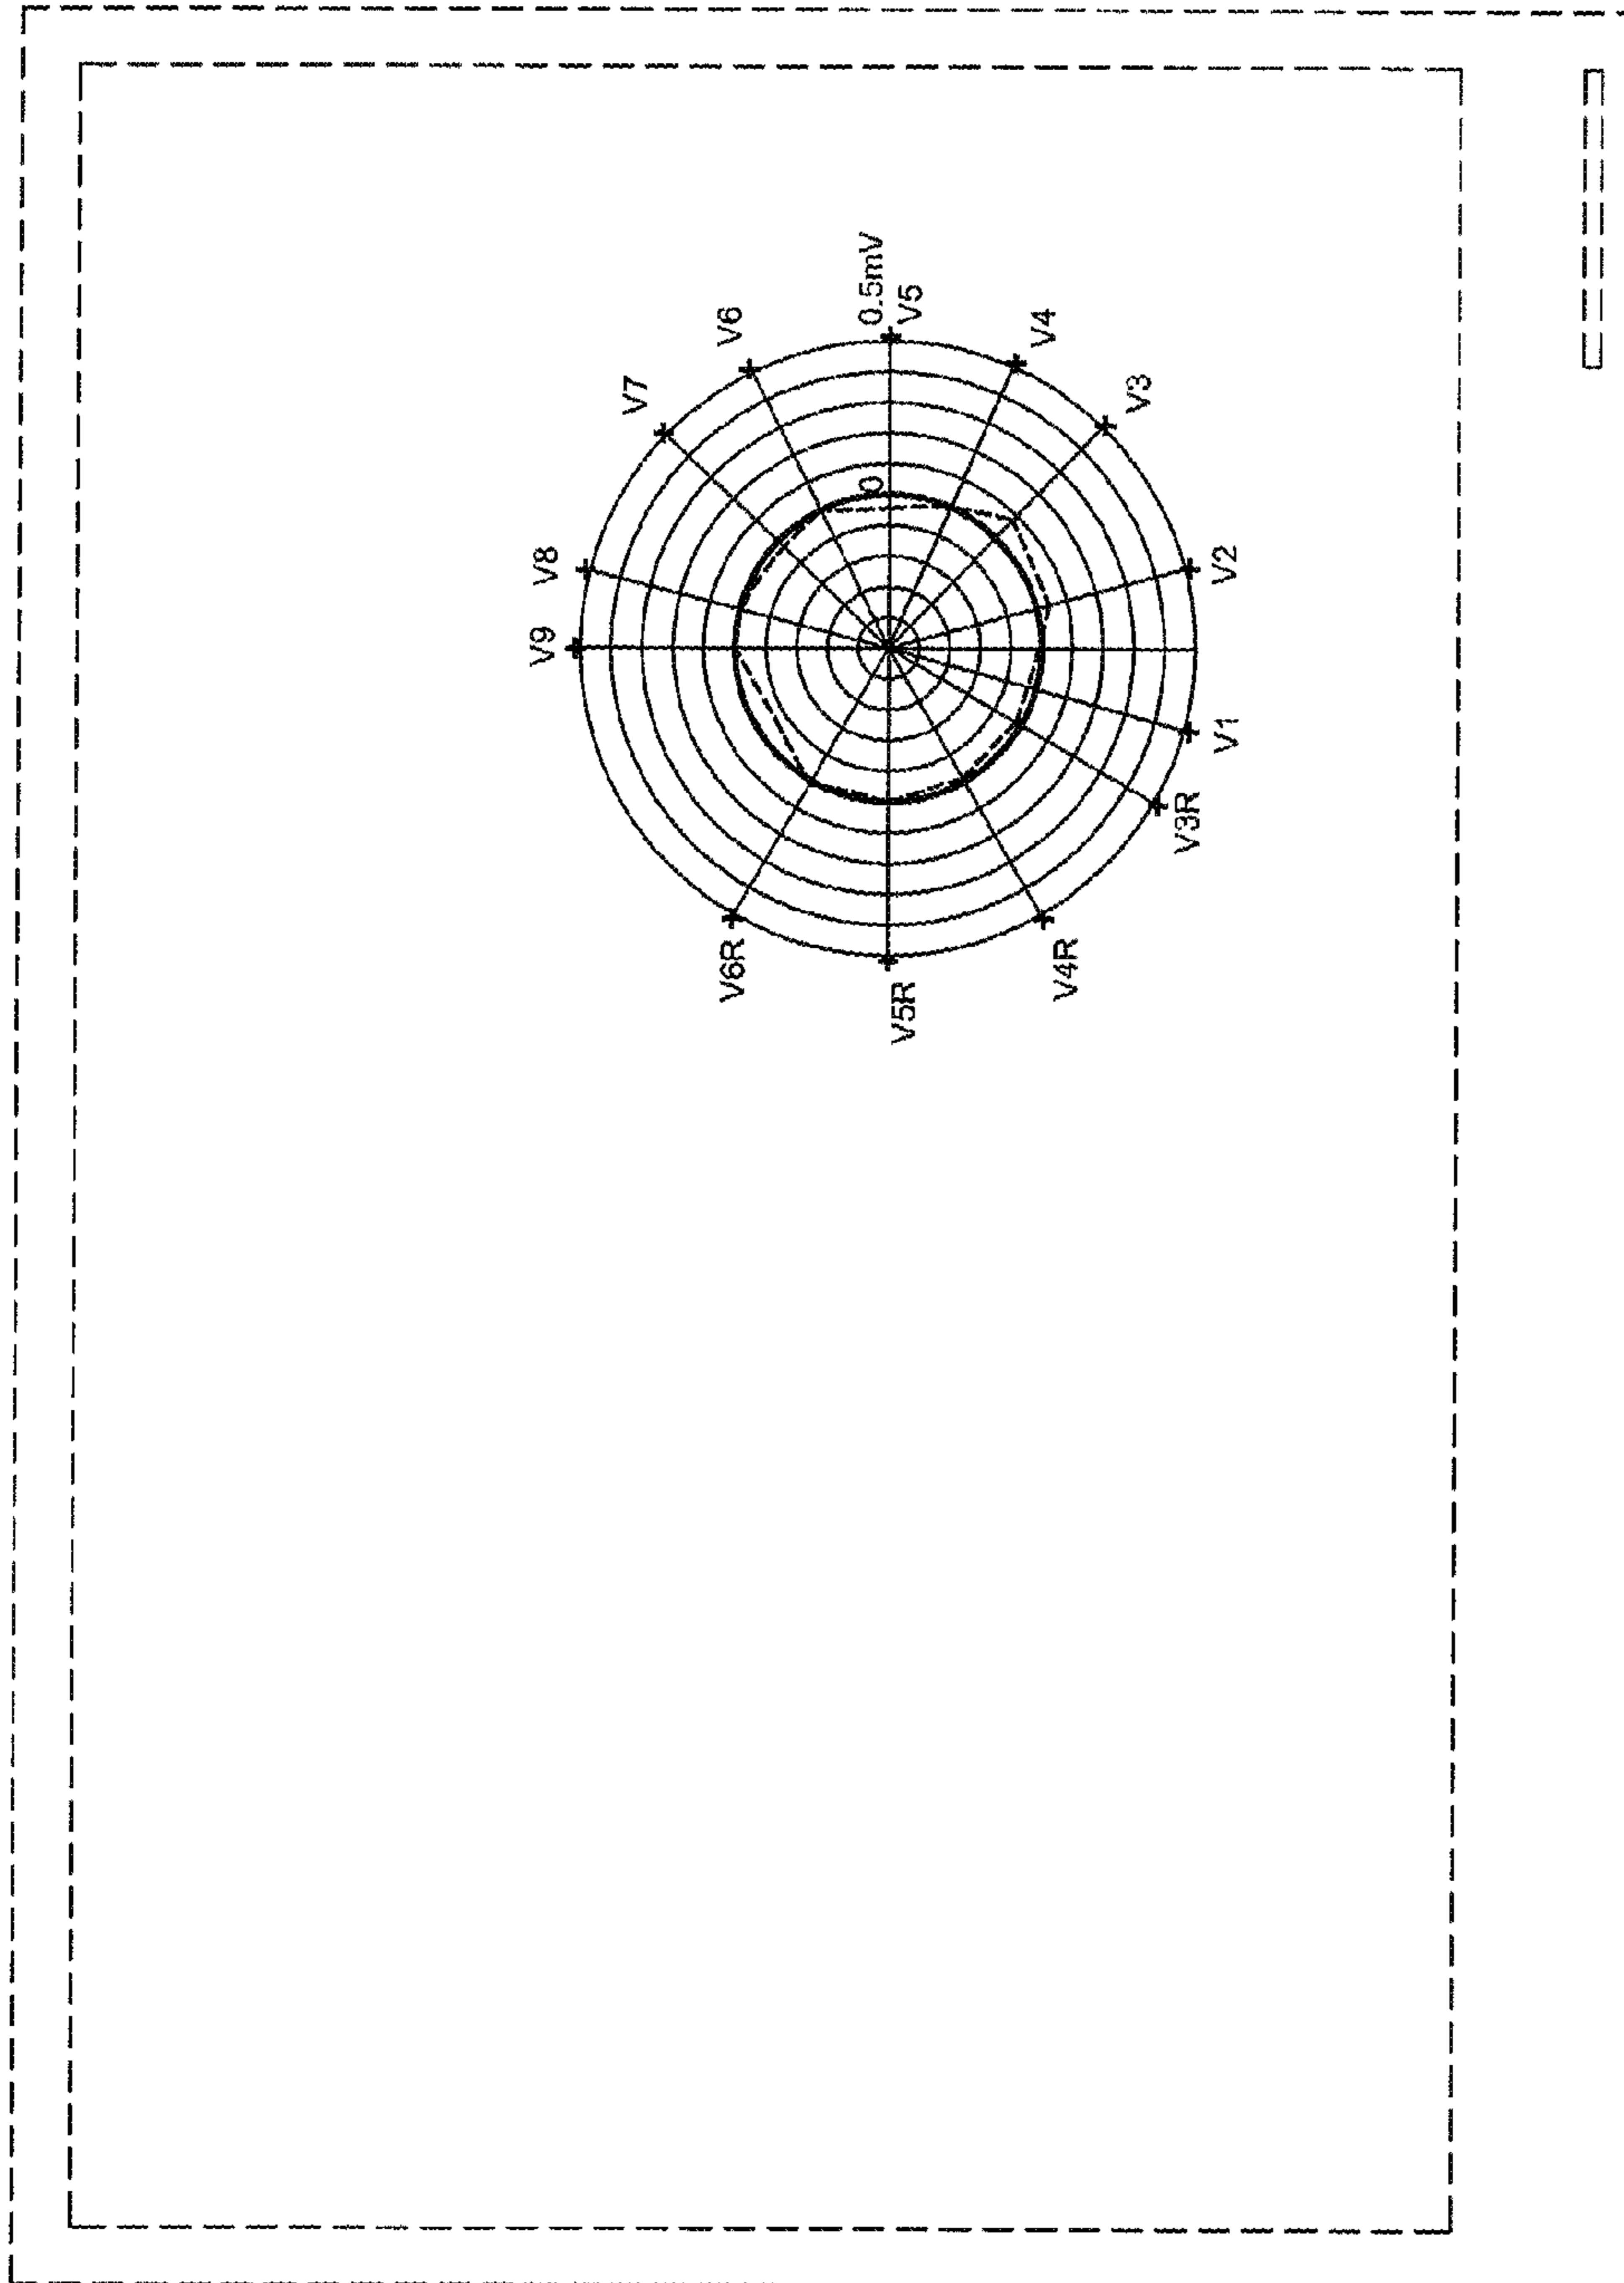


Figure 2