



US00D697617S

(12) **United States Design Patent**
Sanders

(10) **Patent No.:** **US D697,617 S**
(45) **Date of Patent:** **** Jan. 14, 2014**

(54) **MEDICAL INJECTOR**

(71) Applicant: **David Sanders**, Warwick (GB)

(72) Inventor: **David Sanders**, Warwick (GB)

(73) Assignee: **Sanofi-Aventis Deutschland GmbH**,
Frankfurt (DE)

(**) Term: **14 Years**

(21) Appl. No.: **29/455,552**

(22) Filed: **May 22, 2013**

Related U.S. Application Data

(62) Division of application No. 29/365,403, filed on Jul. 8,
2010, now Pat. No. Des. 685,464.

(30) **Foreign Application Priority Data**

Jan. 11, 2010 (EM) 001188411

(51) **LOC (10) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/113**

(58) **Field of Classification Search**

USPC D24/112-114, 133, 186, 104, 130, 127;
606/181, 185; 604/232, 187, 158,
604/164.08, 192, 263, 163, 181, 184, 198,
604/227, 207

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,398,544 A 4/1946 Lockhart
4,637,403 A 1/1987 Garcia et al.

(Continued)

FOREIGN PATENT DOCUMENTS

DE 101-06368.7 2/2001
JP 1 178 092 6/2003

(Continued)

OTHER PUBLICATIONS

Yorkshire Diabetes for Patients, Optiset Pen, available at http://www.yorkshirediabetes.com/downloads/UK_Lantus_Optiset_PIL.pdf.

(Continued)

Primary Examiner — David Muller

(74) *Attorney, Agent, or Firm* — Finnegan, Henderson,
Farabow, Garrett and Dunner, LLP

(57) **CLAIM**

The ornamental design for a medical injector, as shown and
described.

DESCRIPTION

The file of this patent contains at least one photograph
executed in color. Copies of this patent with color photo-
graphs will be provided by the Office upon request and pay-
ment of the necessary fee.

FIG. 1 is a front elevation view of a first embodiment of a
medical injector showing my new design;

FIG. 2 is a right side view thereof;

FIG. 3 is a rear view thereof;

FIG. 4 is a left side view thereof;

FIG. 5 is a perspective view thereof;

FIG. 6 is a top plan view thereof;

FIG. 7 is a bottom view thereof;

FIG. 8 is a front elevation view of the second embodiment of
a medical injector showing my new design;

FIG. 9 is a right side view thereof;

FIG. 10 is a rear view thereof;

FIG. 11 is a left side view thereof;

FIG. 12 is a perspective view thereof;

FIG. 13 is a top plan view thereof;

FIG. 14 is a bottom view thereof;

FIG. 15 is a front elevation view of the third embodiment of a
medical injector showing my new design;

FIG. 16 is a right side view thereof;

FIG. 17 is a rear view thereof;


FIG. 18 is a left side view thereof;

FIG. 19 is a perspective view thereof;

FIG. 20 is a top plan view thereof; and,

FIG. 21 is a bottom view thereof.

1 Claim, 12 Drawing Sheets
(12 of 12 Drawing Sheet(s) Filed in Color)

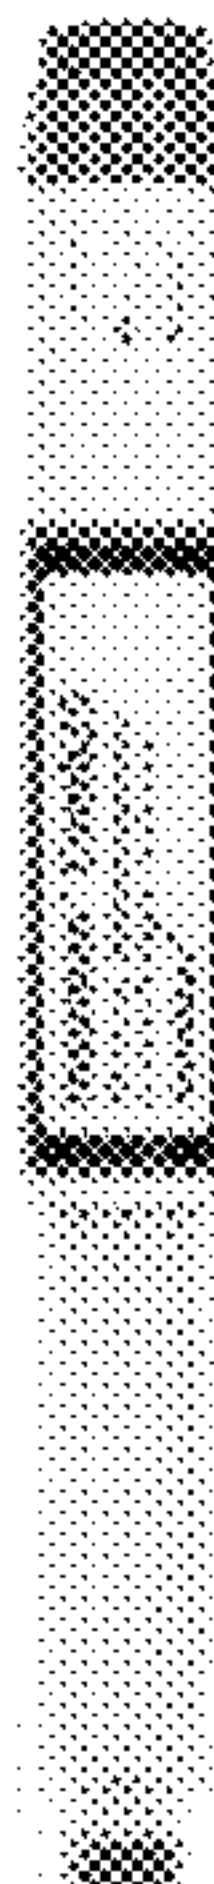

(56)

References Cited**U.S. PATENT DOCUMENTS**

D289,424	S	4/1987	Huang	
4,936,833	A	6/1990	Sams	
5,104,380	A	4/1992	Holman et al.	
5,226,895	A	7/1993	Harris	
5,279,586	A	1/1994	Balkwill	
5,295,976	A	3/1994	Harris	
5,334,144	A	8/1994	Alchas et al.	
D368,961	S	4/1996	Himbert et al.	
5,599,314	A	2/1997	Neill	
D414,201	S	9/1999	Larson et al.	
6,001,082	A	12/1999	Dair et al.	
6,001,089	A	12/1999	Burroughs et al.	
D426,299	S	6/2000	Bydlon et al.	
D426,572	S	6/2000	Salemme et al.	
6,086,567	A	7/2000	Kirchhofer et al.	
6,110,149	A	8/2000	Klitgaard et al.	
6,193,698	B1	2/2001	Kirchhofer et al.	
D462,760	S	9/2002	Ahlgrim et al.	
6,454,746	B1	9/2002	Bydlon et al.	
D479,599	S *	9/2003	Bainton	D24/114
D479,600	S *	9/2003	Bainton	D24/114
D479,602	S	9/2003	Bainton	
D479,603	S *	9/2003	Tyce	D24/114
D479,747	S	9/2003	Bainton	
D479,748	S	9/2003	Tyce	
6,613,023	B2	9/2003	Kirchhofer et al.	
D482,122	S	11/2003	Cohn et al.	
D482,724	S	11/2003	Nishida	
6,699,224	B2	3/2004	Kirchhofer et al.	
D492,027	S	6/2004	Tyce et al.	
D492,405	S	6/2004	Bainton	
D499,485	S	12/2004	Tyce	
6,827,708	B2	12/2004	Kirchhofer	
D501,253	S	1/2005	Bainton	
D503,477	S	3/2005	Hawley et al.	
D503,797	S	4/2005	Tyce	
D505,490	S	5/2005	Tyce	
D506,005	S	6/2005	Hawley et al.	
6,932,794	B2	8/2005	Giambattista et al.	
D516,719	S	3/2006	Turchi et al.	
D518,175	S	3/2006	Hardin et al.	
7,018,364	B2	3/2006	Giambattista et al.	
D520,636	S	5/2006	Hawley et al.	
7,169,133	B2	1/2007	Broennimann et al.	
D540,465	S	4/2007	Bainton	
D546,447	S	7/2007	White	
D548,835	S	8/2007	Galbraith	
D550,363	S	9/2007	Hannant et al.	
D551,341	S	9/2007	Galbraith	
D553,681	S	10/2007	Cetera	
7,316,670	B2	1/2008	Graf et al.	
D567,938	S *	4/2008	Shinohara	D24/114
D567,939	S	4/2008	Mattigka	
7,377,913	B2	5/2008	Gurtner	
7,396,347	B2	7/2008	Hjertman et al.	
7,407,492	B2	8/2008	Gurtner	
D580,052	S	11/2008	White	
D580,069	S	11/2008	Lee	
D599,009	S	8/2009	Tyee	
D599,010	S	8/2009	Tyee	
D600,794	S	9/2009	Tyee	
D600,795	S	9/2009	Tyee	

7,621,891	B2	11/2009	Wyrick	
D610,251	S *	2/2010	Tyce	D24/113
D610,252	S *	2/2010	Tyce	D24/113
D618,789	S *	6/2010	Sanders et al.	D24/113
D619,244	S *	7/2010	Van der Stappen	D24/113
D619,702	S *	7/2010	Galbraith	D24/114
D622,374	S *	8/2010	Julian et al.	D24/113
D624,238	S *	9/2010	Turner	D24/133
D626,216	S *	10/2010	Tyce	D24/114
D627,061	S *	11/2010	Van der Stappen	D24/113
D641,077	S	7/2011	Sanders et al.	
D651,305	S	12/2011	Hawley et al.	
D652,136	S	1/2012	Hawley et al.	
2004/0236284	A1	11/2004	Hoste et al.	
2005/0187523	A1	8/2005	Giambattista et al.	
2005/0222540	A1	10/2005	Kirchhofer et al.	
2005/0251103	A1	11/2005	Steffen et al.	
2006/0229570	A1	10/2006	Lovell et al.	
2007/0106227	A1	5/2007	Burren et al.	
2007/0123829	A1	5/2007	Atterbury et al.	
2007/0129687	A1	6/2007	Marshall et al.	
2007/0167921	A1	7/2007	Burren et al.	
2007/0233015	A1	10/2007	Saiki	
2008/0071226	A1	3/2008	Moser et al.	
2009/0124981	A1	5/2009	Evans	

FOREIGN PATENT DOCUMENTS

JP	D1197948	2/2004
JP	D1203775	4/2004
TW	D104991	9/1991
TW	579273	5/1992
TW	D122771	4/1996
TW	D122772	4/1996
TW	D122774	4/1996
TW	D124492	8/1996
WO	WO 2005/102421 A1	11/2005

OTHER PUBLICATIONS

Lantus Optiset, vol. 23, No. 8, Sep. 2004, available at www.doyfarma.com/doyfarma.

Optiset injector with packaging, as shown in publication "Offarm," title of the article, "Actualidad Profesional Mostrador," shown on p. 52 (of The publication), p. 8 of the reference (upper left-hand corner). Dated Sep. 3, 2004.

OptiSet information brochure as found on www.diabetesplein.nl (link indicated by arrow on p. 3), untranslated, brochure dated Aug. 24, 2007 (see p. 20).

Informational brochure on OptiSet injector, dated Oct. 16, 2007 (see p. 9), at the following link: www.insulin.se/insulinse/Insulinpennor/OptiSet/.

SoloSTAR disposable pen injector by DCA Design International for Sanofi Aventis GmbH, as shown on www.effectedesign.org.uk, dated 10-022-2009 (3 pages).

DCA brochure for SoloSTAR disposable pen injector for insulin, as found on www.effectedesign.org.uk, as indicated at arrow on Item "U" above, dated Jun. 2, 2009 (10 pages). Reference to date of product launch (2007) on p. 2, last paragraph.

Article on www.diabeteshealth.com about FDA approval of Lantus SoloStar disposable insulin pen, with a picture of the product, dated May 4, 2007 (5 pages).

* cited by examiner

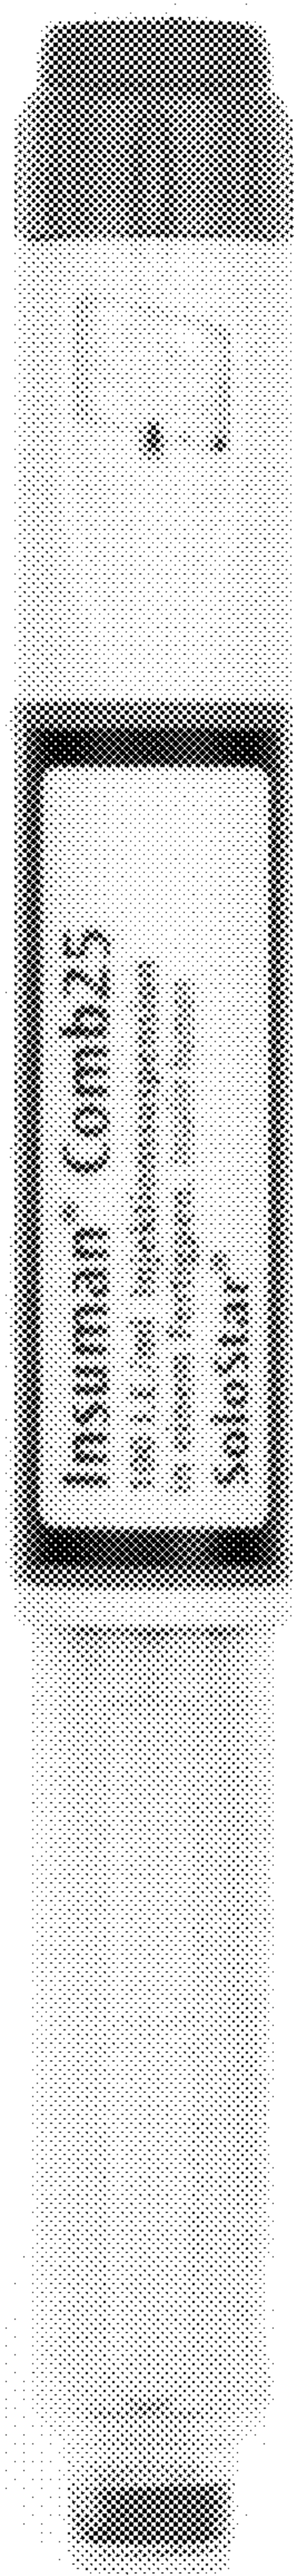


FIG. 1

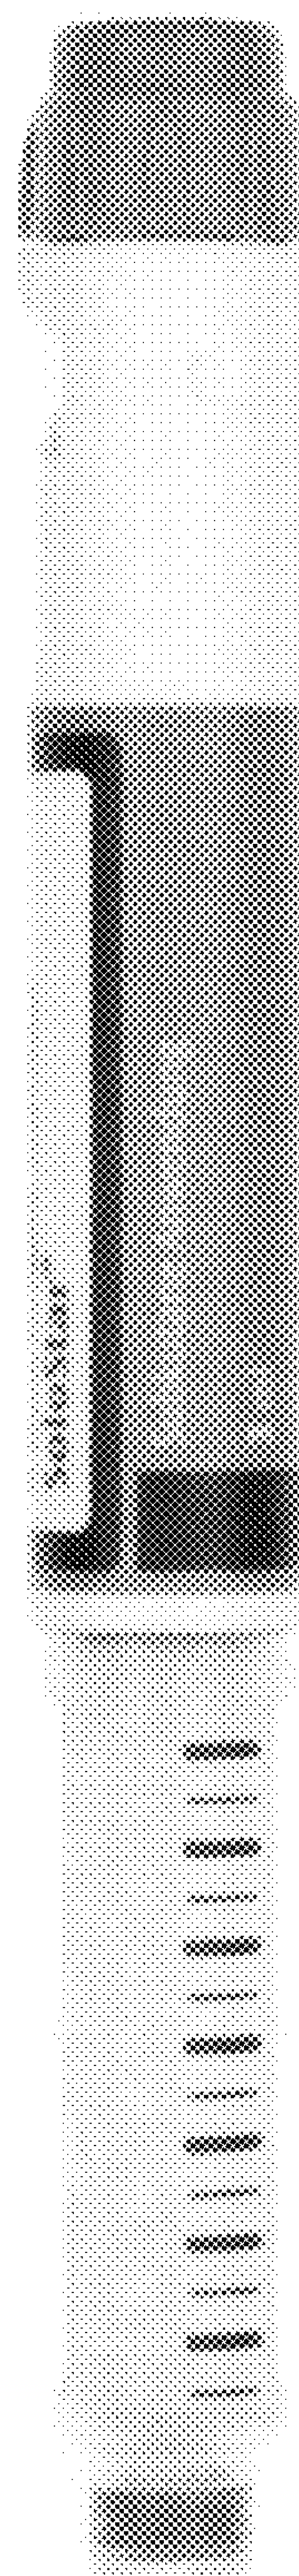


FIG. 2

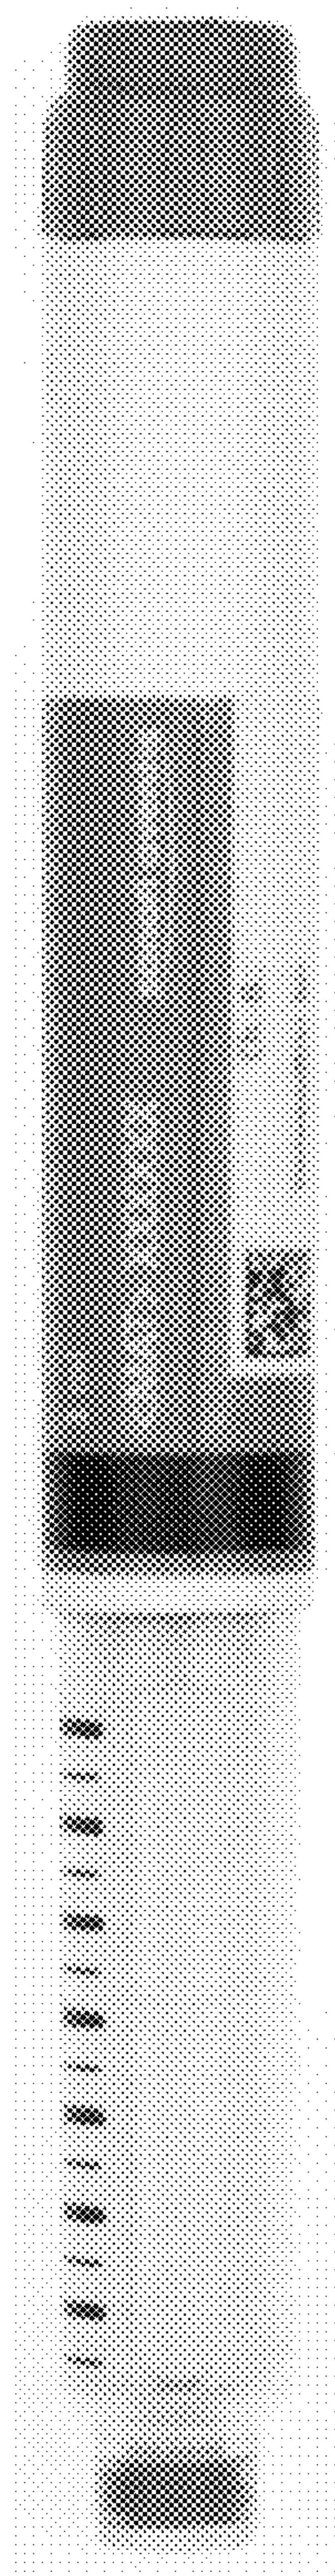


FIG. 3

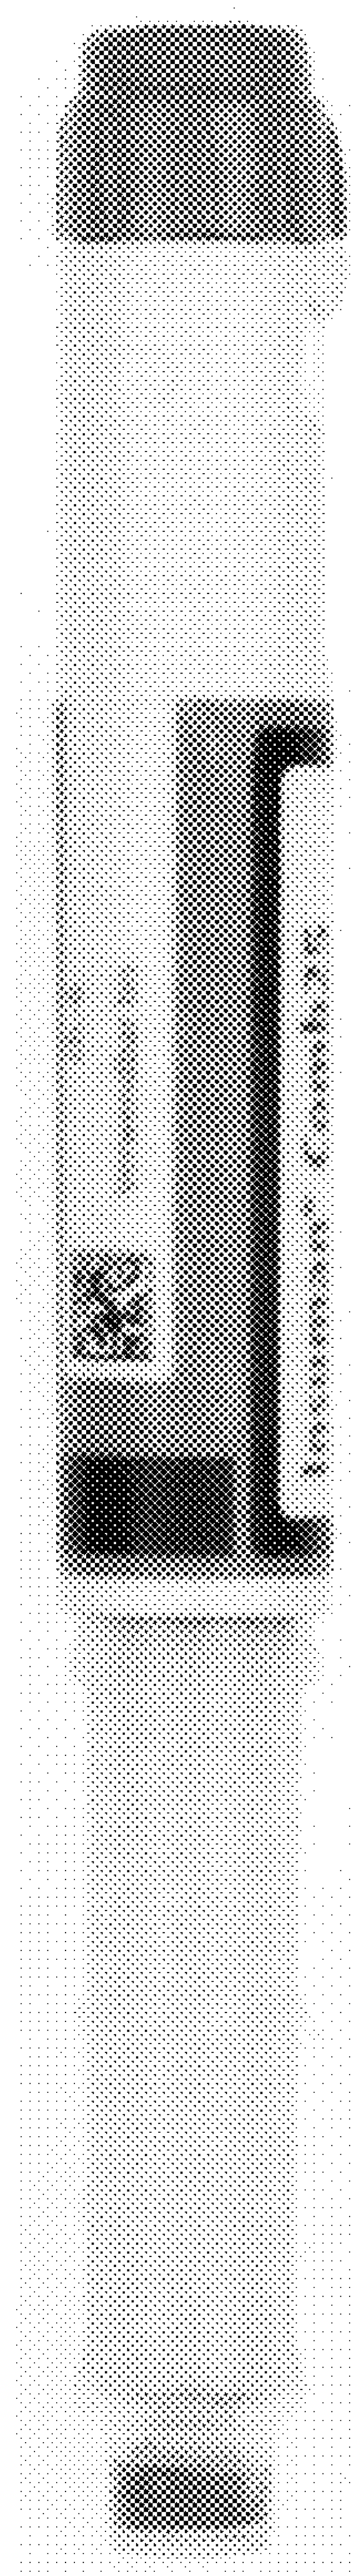


FIG. 4



FIG. 5

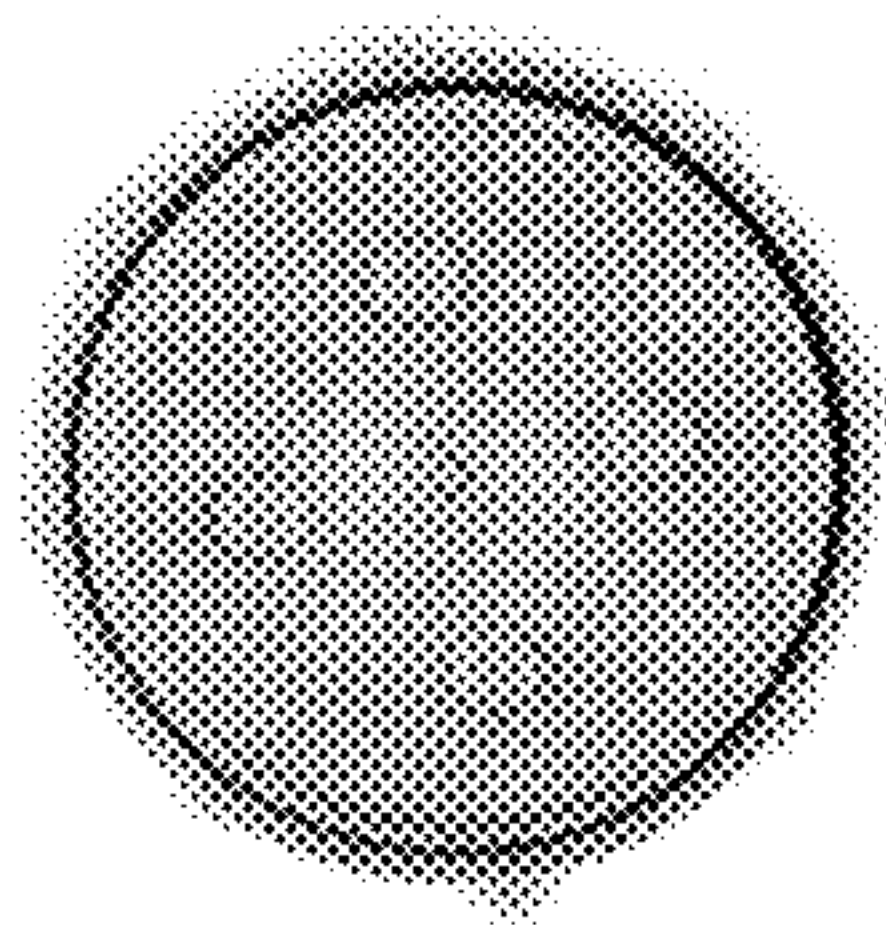


FIG. 6

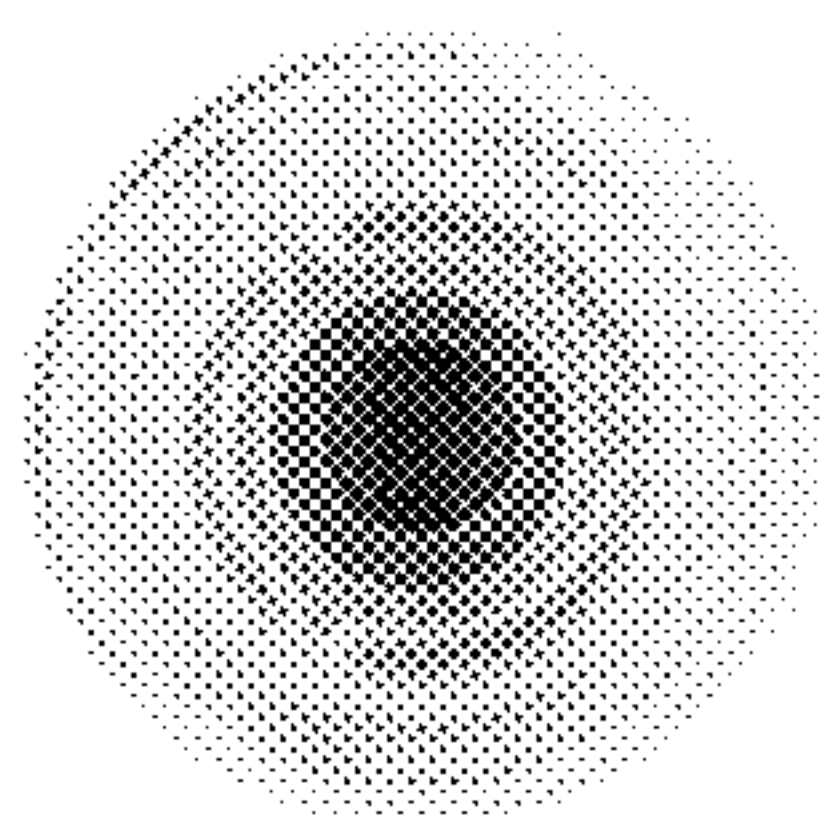


FIG. 7

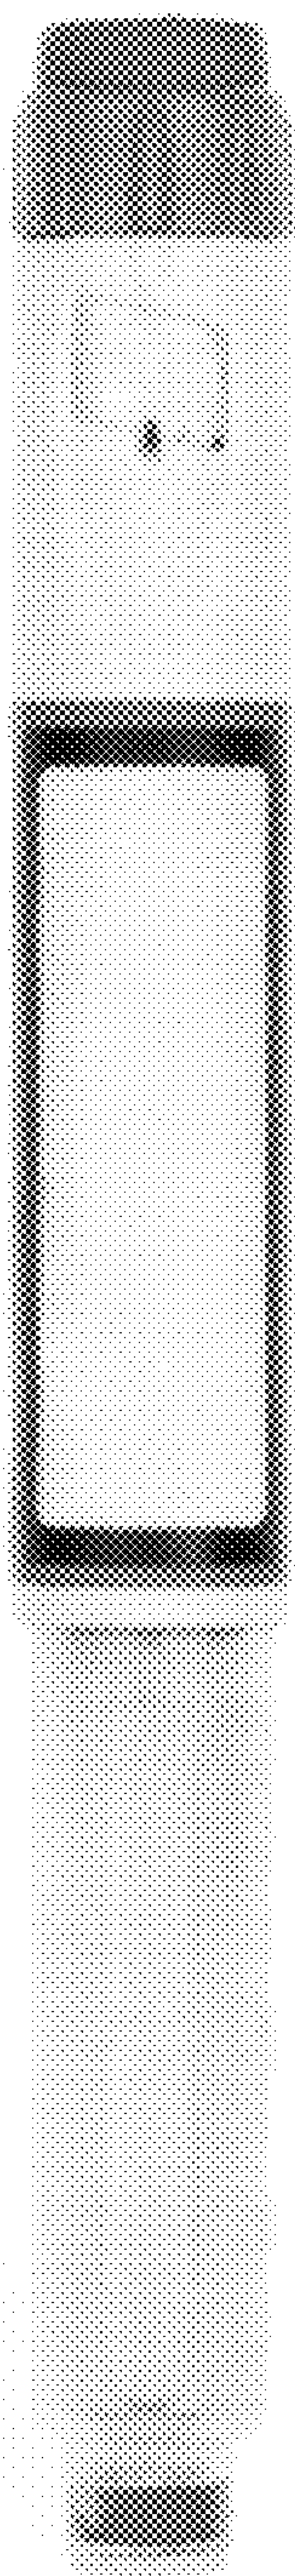


FIG. 8

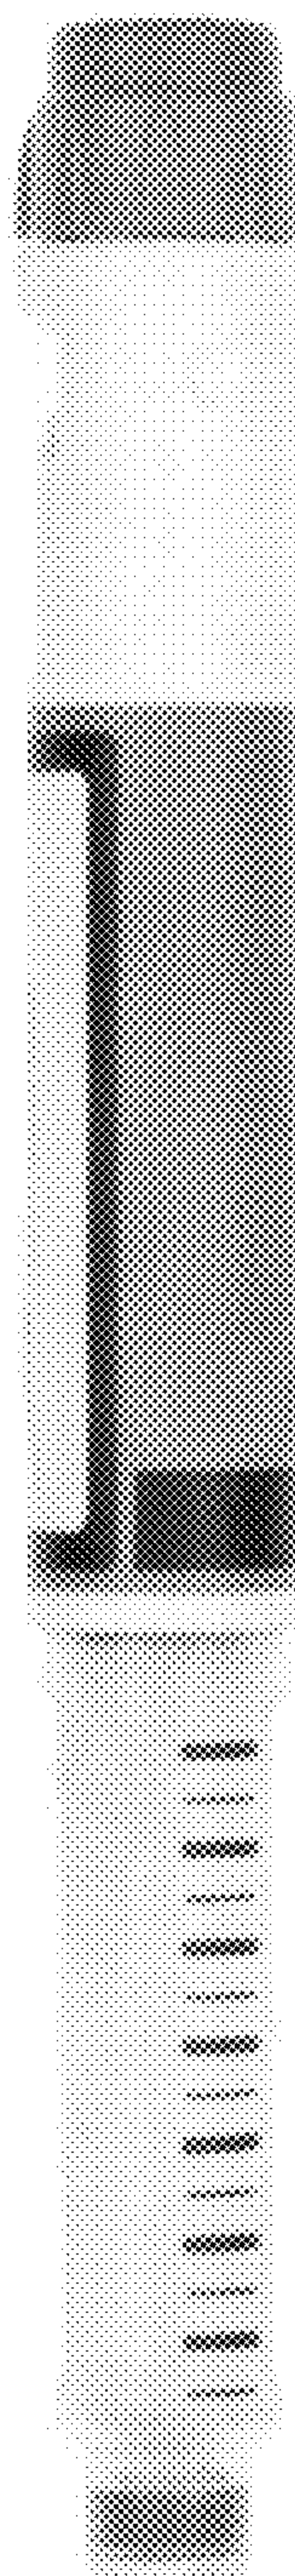


FIG. 9

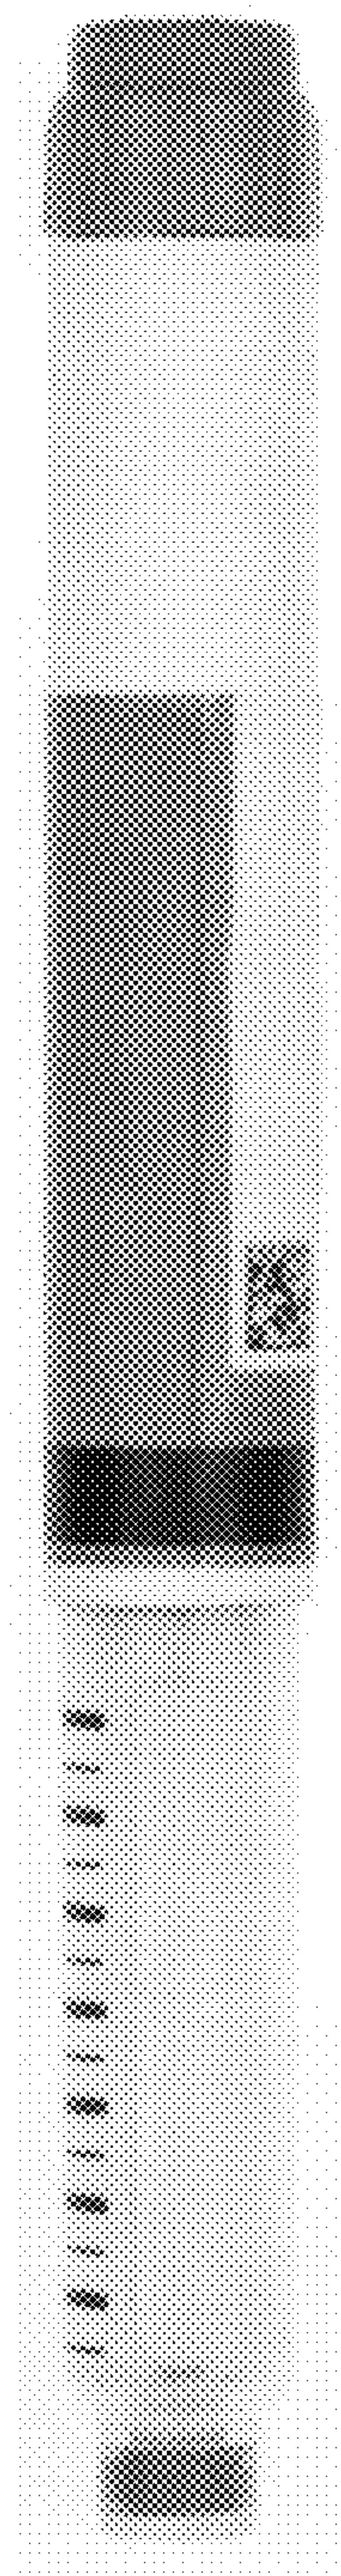


FIG. 10

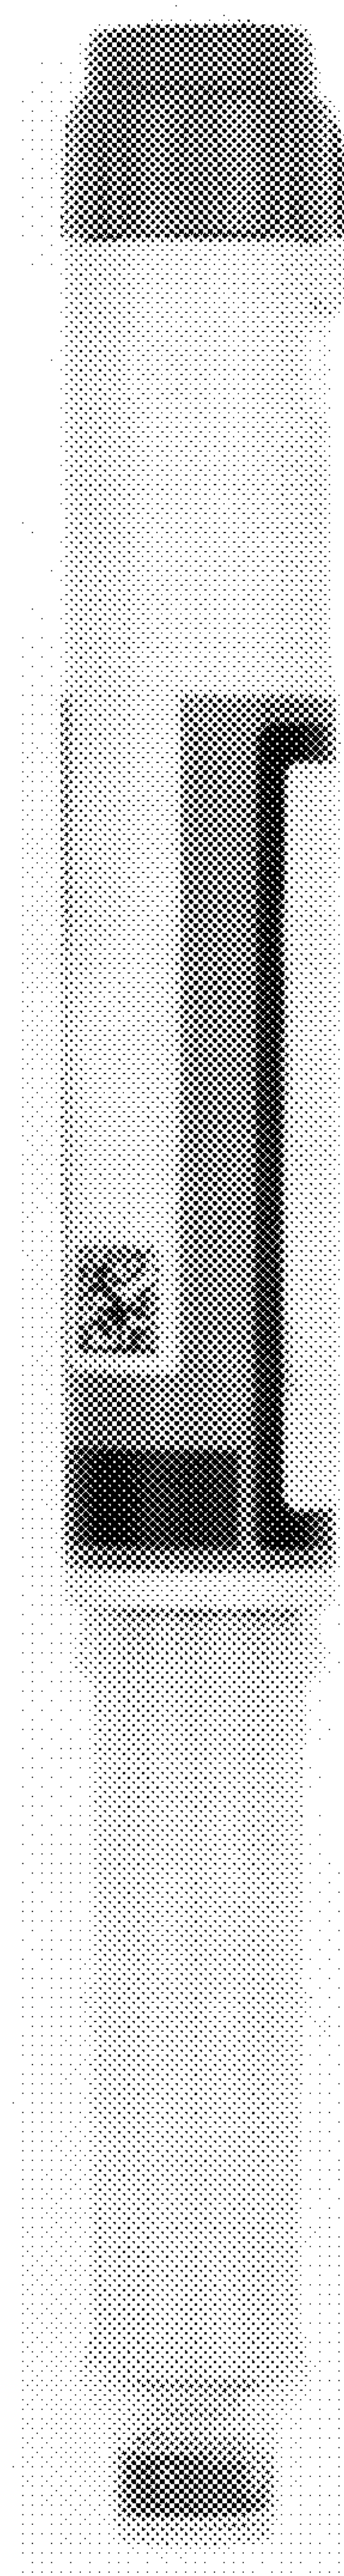


FIG. 11



FIG. 12

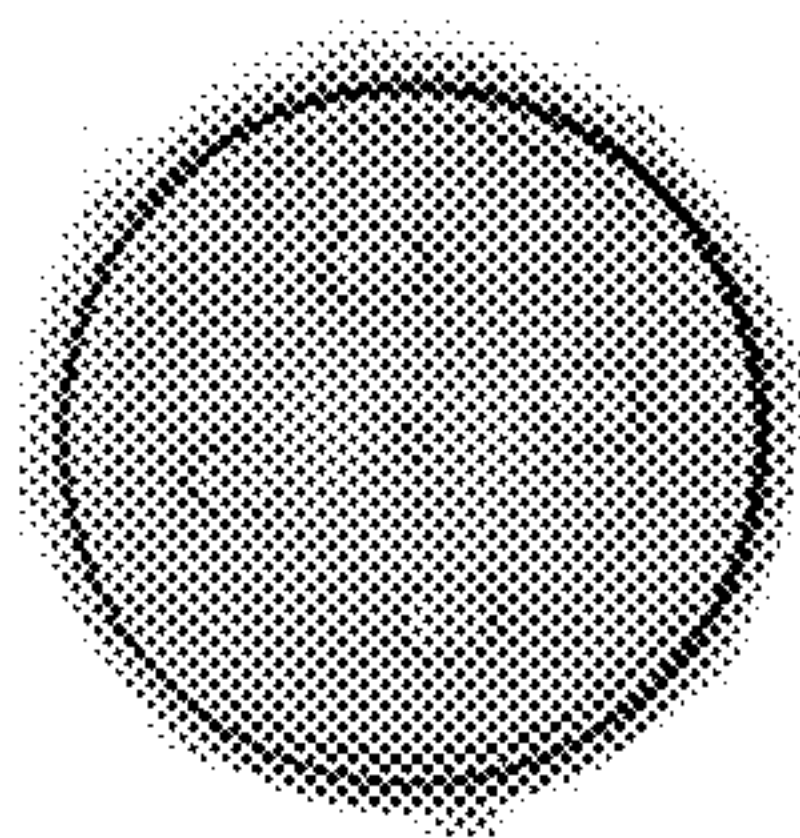


FIG. 13

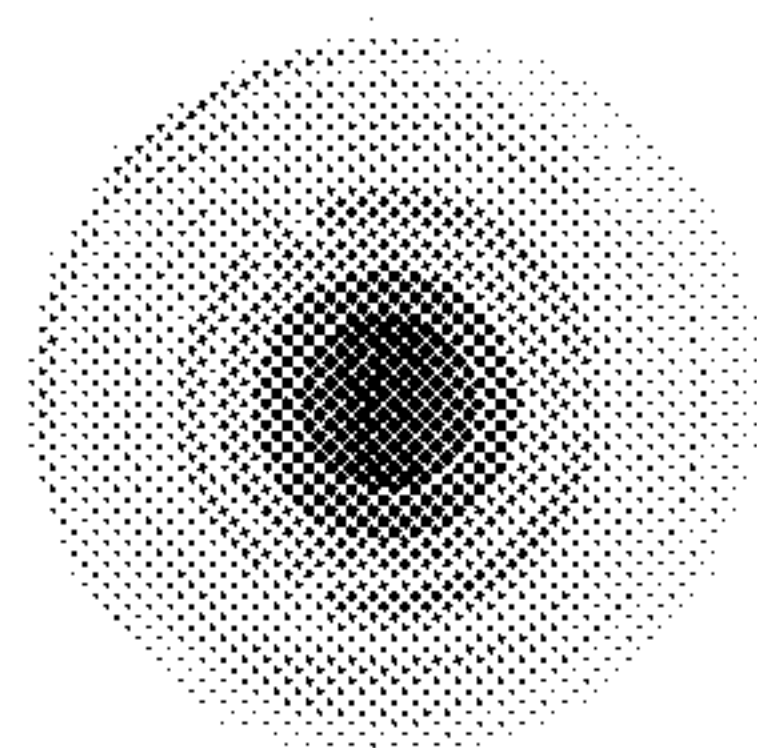


FIG. 14

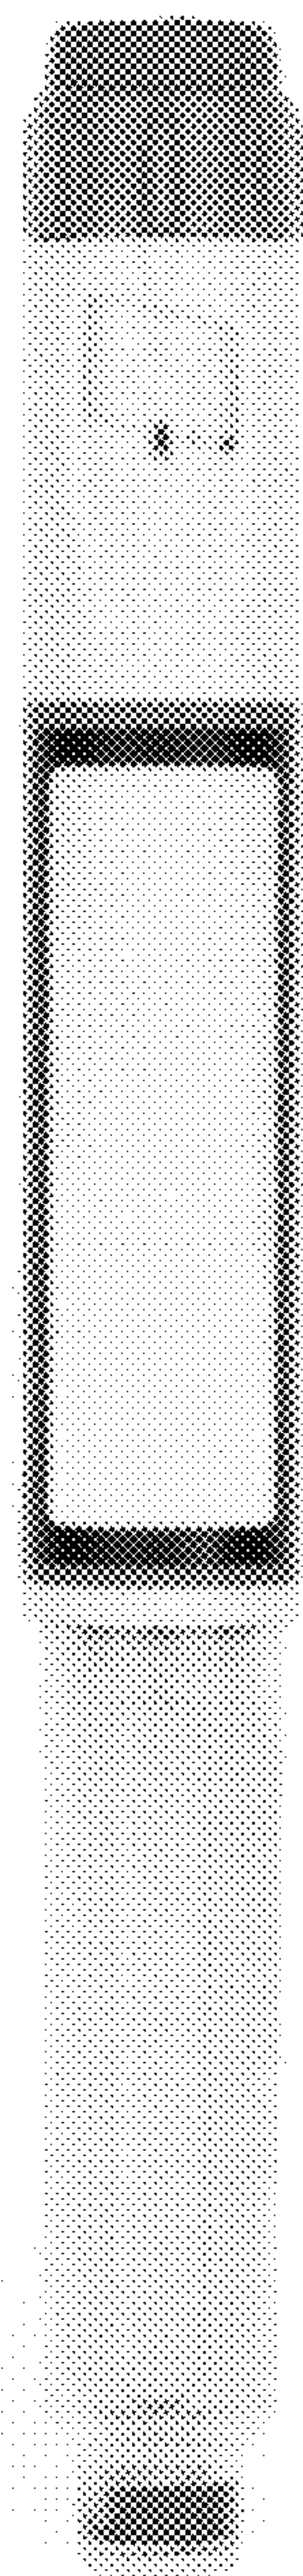


FIG. 15

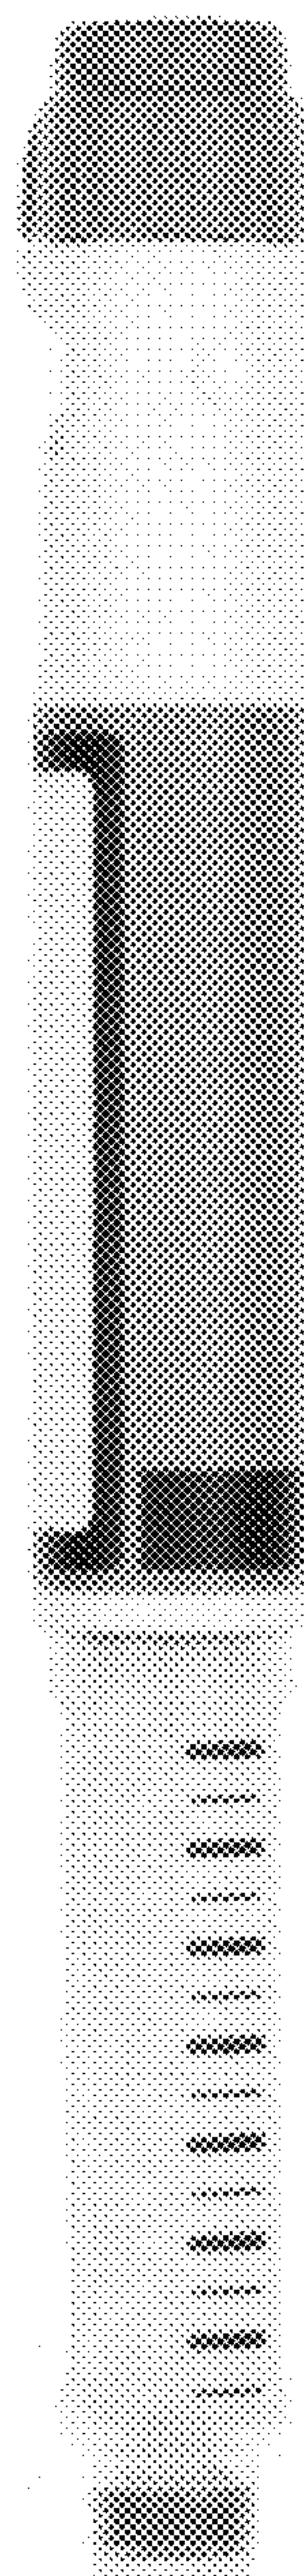


FIG. 16

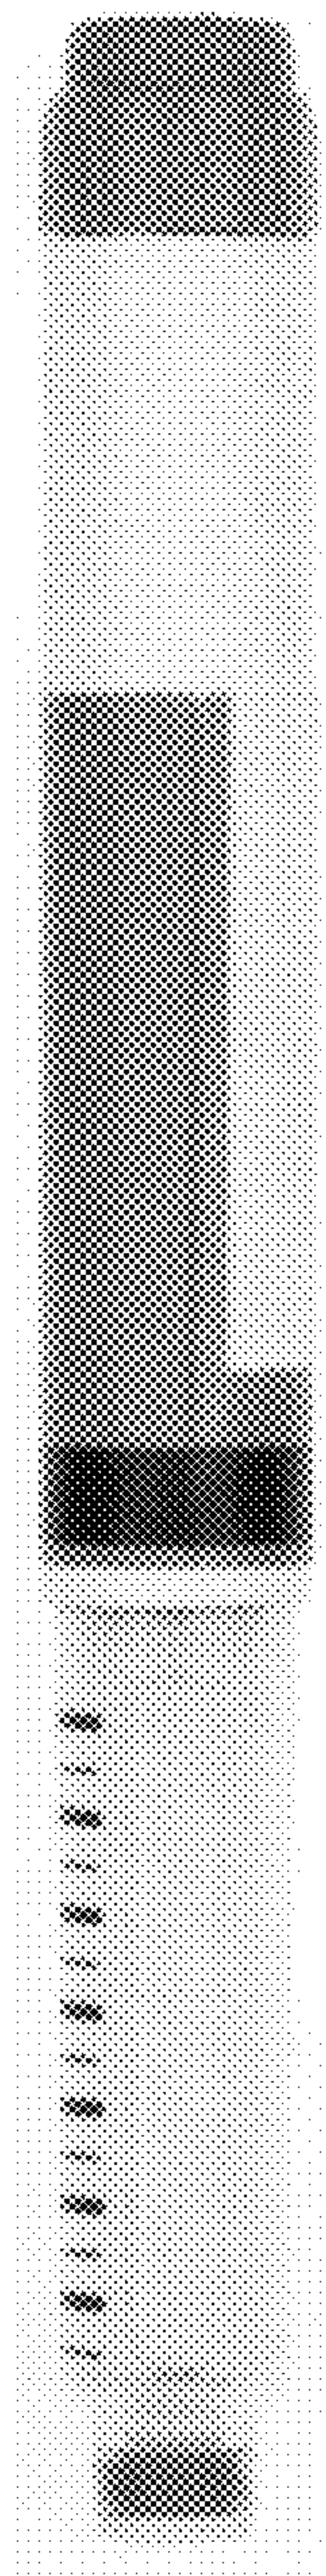


FIG. 17

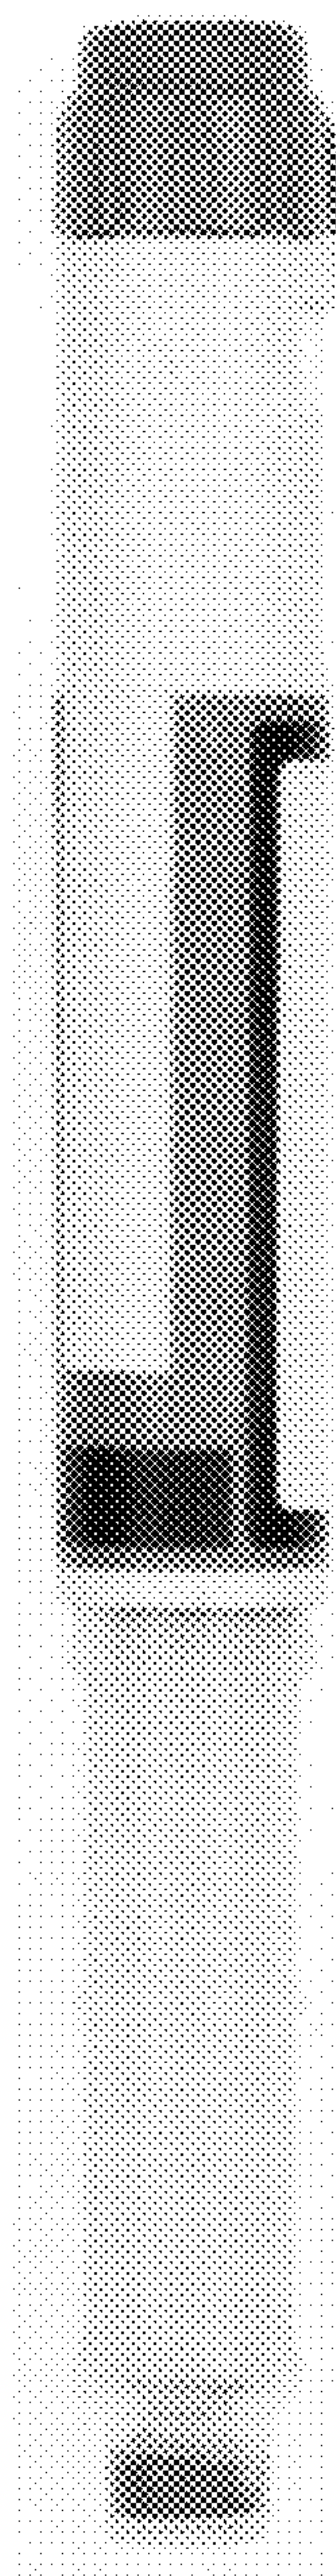


FIG. 18



FIG 19

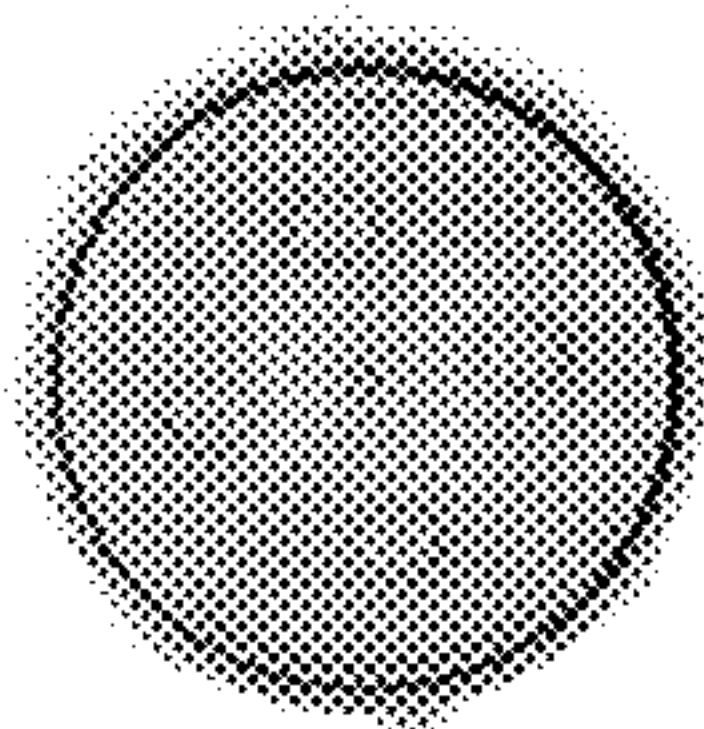


FIG. 20

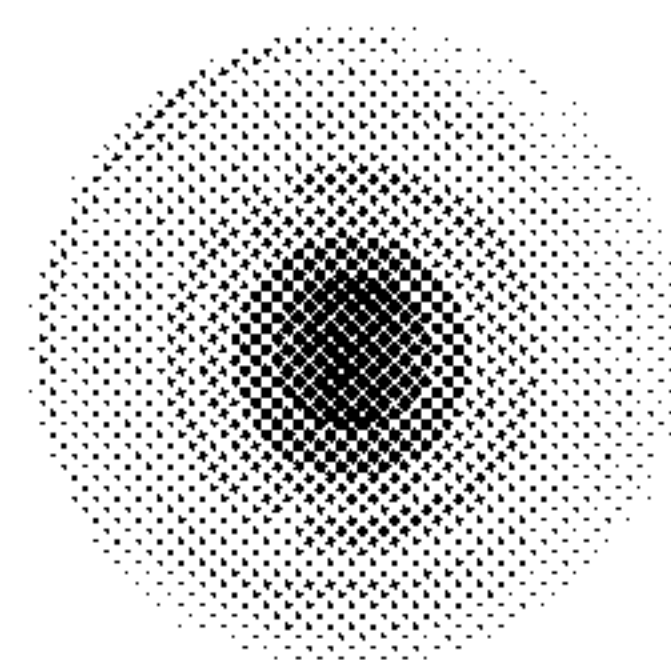


FIG. 21