

US00D697621S

(12) **United States Design Patent**
Chung et al.

(10) **Patent No.:** **US D697,621 S**
(45) **Date of Patent:** **** Jan. 14, 2014**

(54) **ULTRASONIC DIAGNOSTIC EQUIPMENT**

(71) Applicant: **Samsung Electronics Co., Ltd.**,
Suwon-si (KR)

(72) Inventors: **Yeon-Moo Chung**, Seoul (KR); **Jun-Pil Moon**, Seoul (KR)

(73) Assignee: **Samsung Electronics Co., Ltd.** (KR)

(**) Term: **14 Years**

(21) Appl. No.: **29/437,927**

(22) Filed: **Nov. 21, 2012**

(30) **Foreign Application Priority Data**

Jun. 26, 2012 (KR) 30-2012-0031070

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/158**

(58) **Field of Classification Search**

USPC D24/158–161, 185, 186; 606/32–34;
600/1–3, 104, 437, 443, 459; 312/209,
312/223.1, 223.2, 249.12; 248/47.34, 282.1
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D387,168 S * 12/1997 Edelman et al. D24/186
D472,635 S * 4/2003 Stringer et al. D24/160
D559,390 S * 1/2008 Diener et al. D24/186

D626,238 S * 10/2010 Zinnanti D24/185
D626,239 S * 10/2010 Lia et al. D24/185
D628,299 S * 11/2010 Held D24/185
D631,970 S * 2/2011 Held D24/185
D648,855 S * 11/2011 Smith et al. D24/158
D652,936 S * 1/2012 Ross et al. D24/185
D657,470 S * 4/2012 Schon et al. D24/186
2010/0004535 A1 * 1/2010 Song et al. 600/437
2012/0289828 A1 * 11/2012 Jensen et al. 600/437

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Cantor Colburn LLP

(57) **CLAIM**

The ornamental design for an ultrasonic diagnostic equipment, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an ultrasonic diagnostic equipment showing our new design;
FIG. 2 is a front view thereof;
FIG. 3 is a rear view thereof;
FIG. 4 is a left side view thereof;
FIG. 5 is a right side view thereof;
FIG. 6 is a top plan view thereof;
FIG. 7 is a bottom plan view thereof; and,
FIG. 8 is an enlarged fragmental perspective view thereof.
The broken lines in the drawing views are included for the purpose of illustrating portions of the ultrasonic diagnostic equipment that form no part of the claimed design.

1 Claim, 8 Drawing Sheets

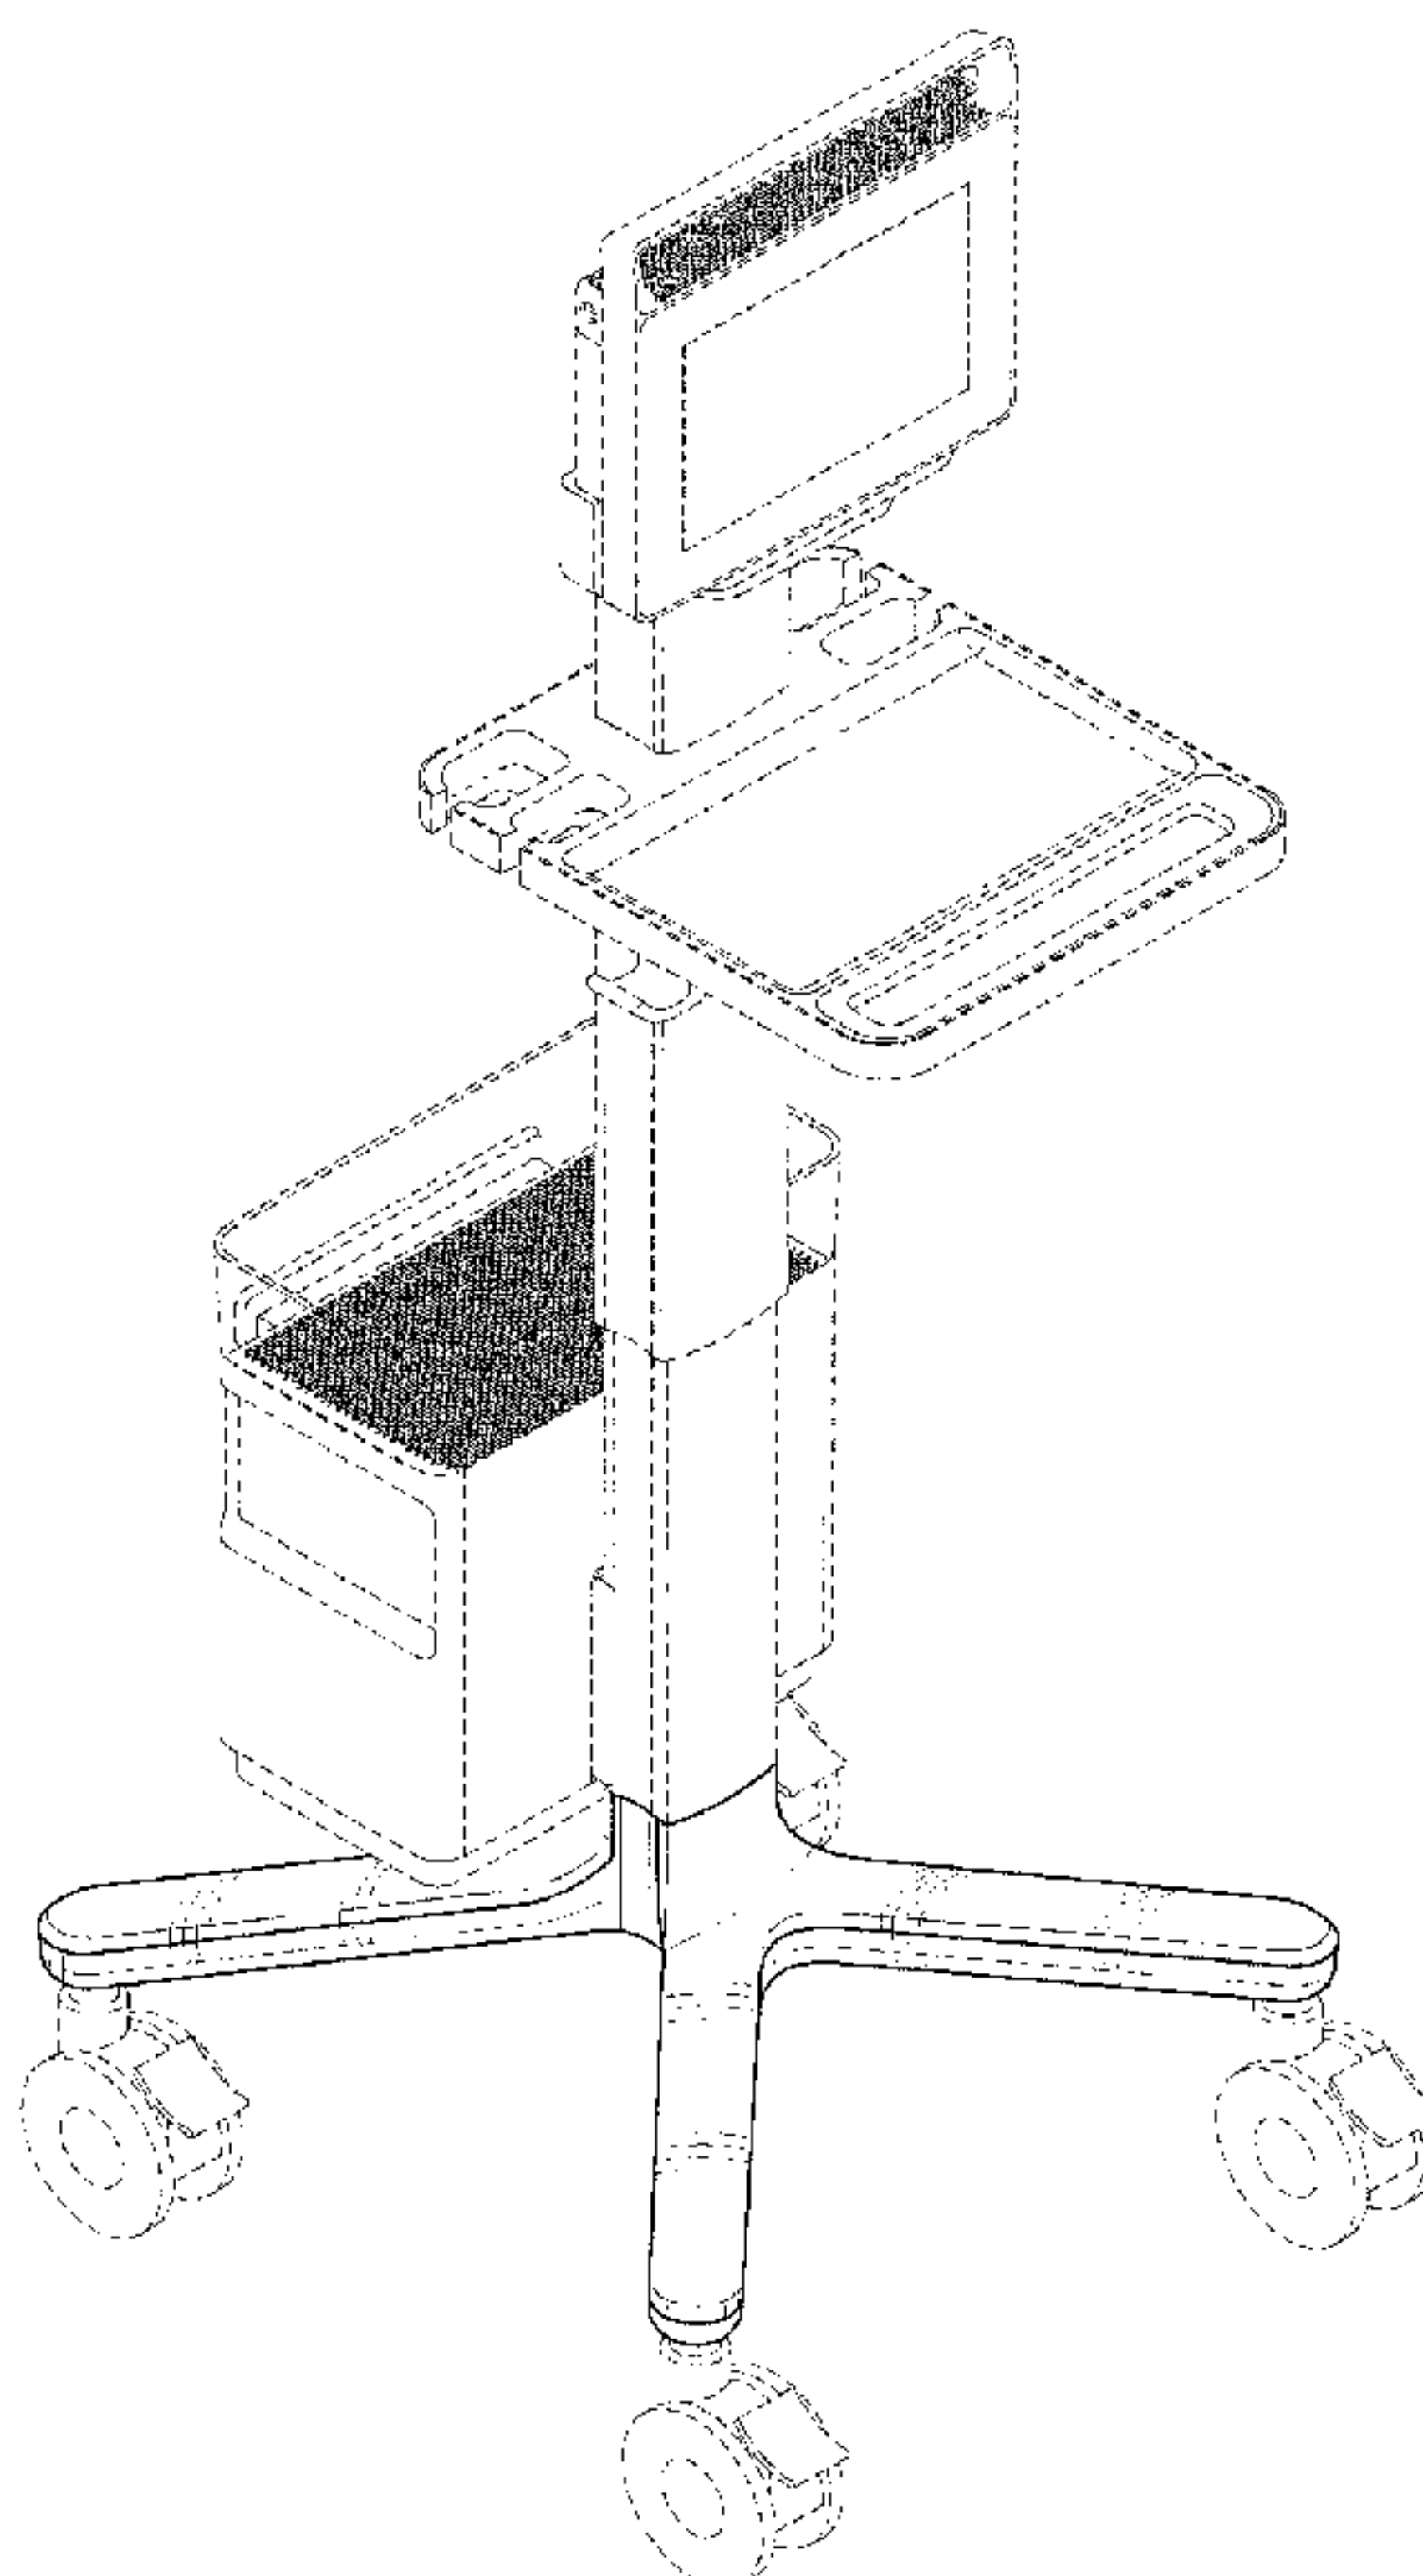


FIG. 1

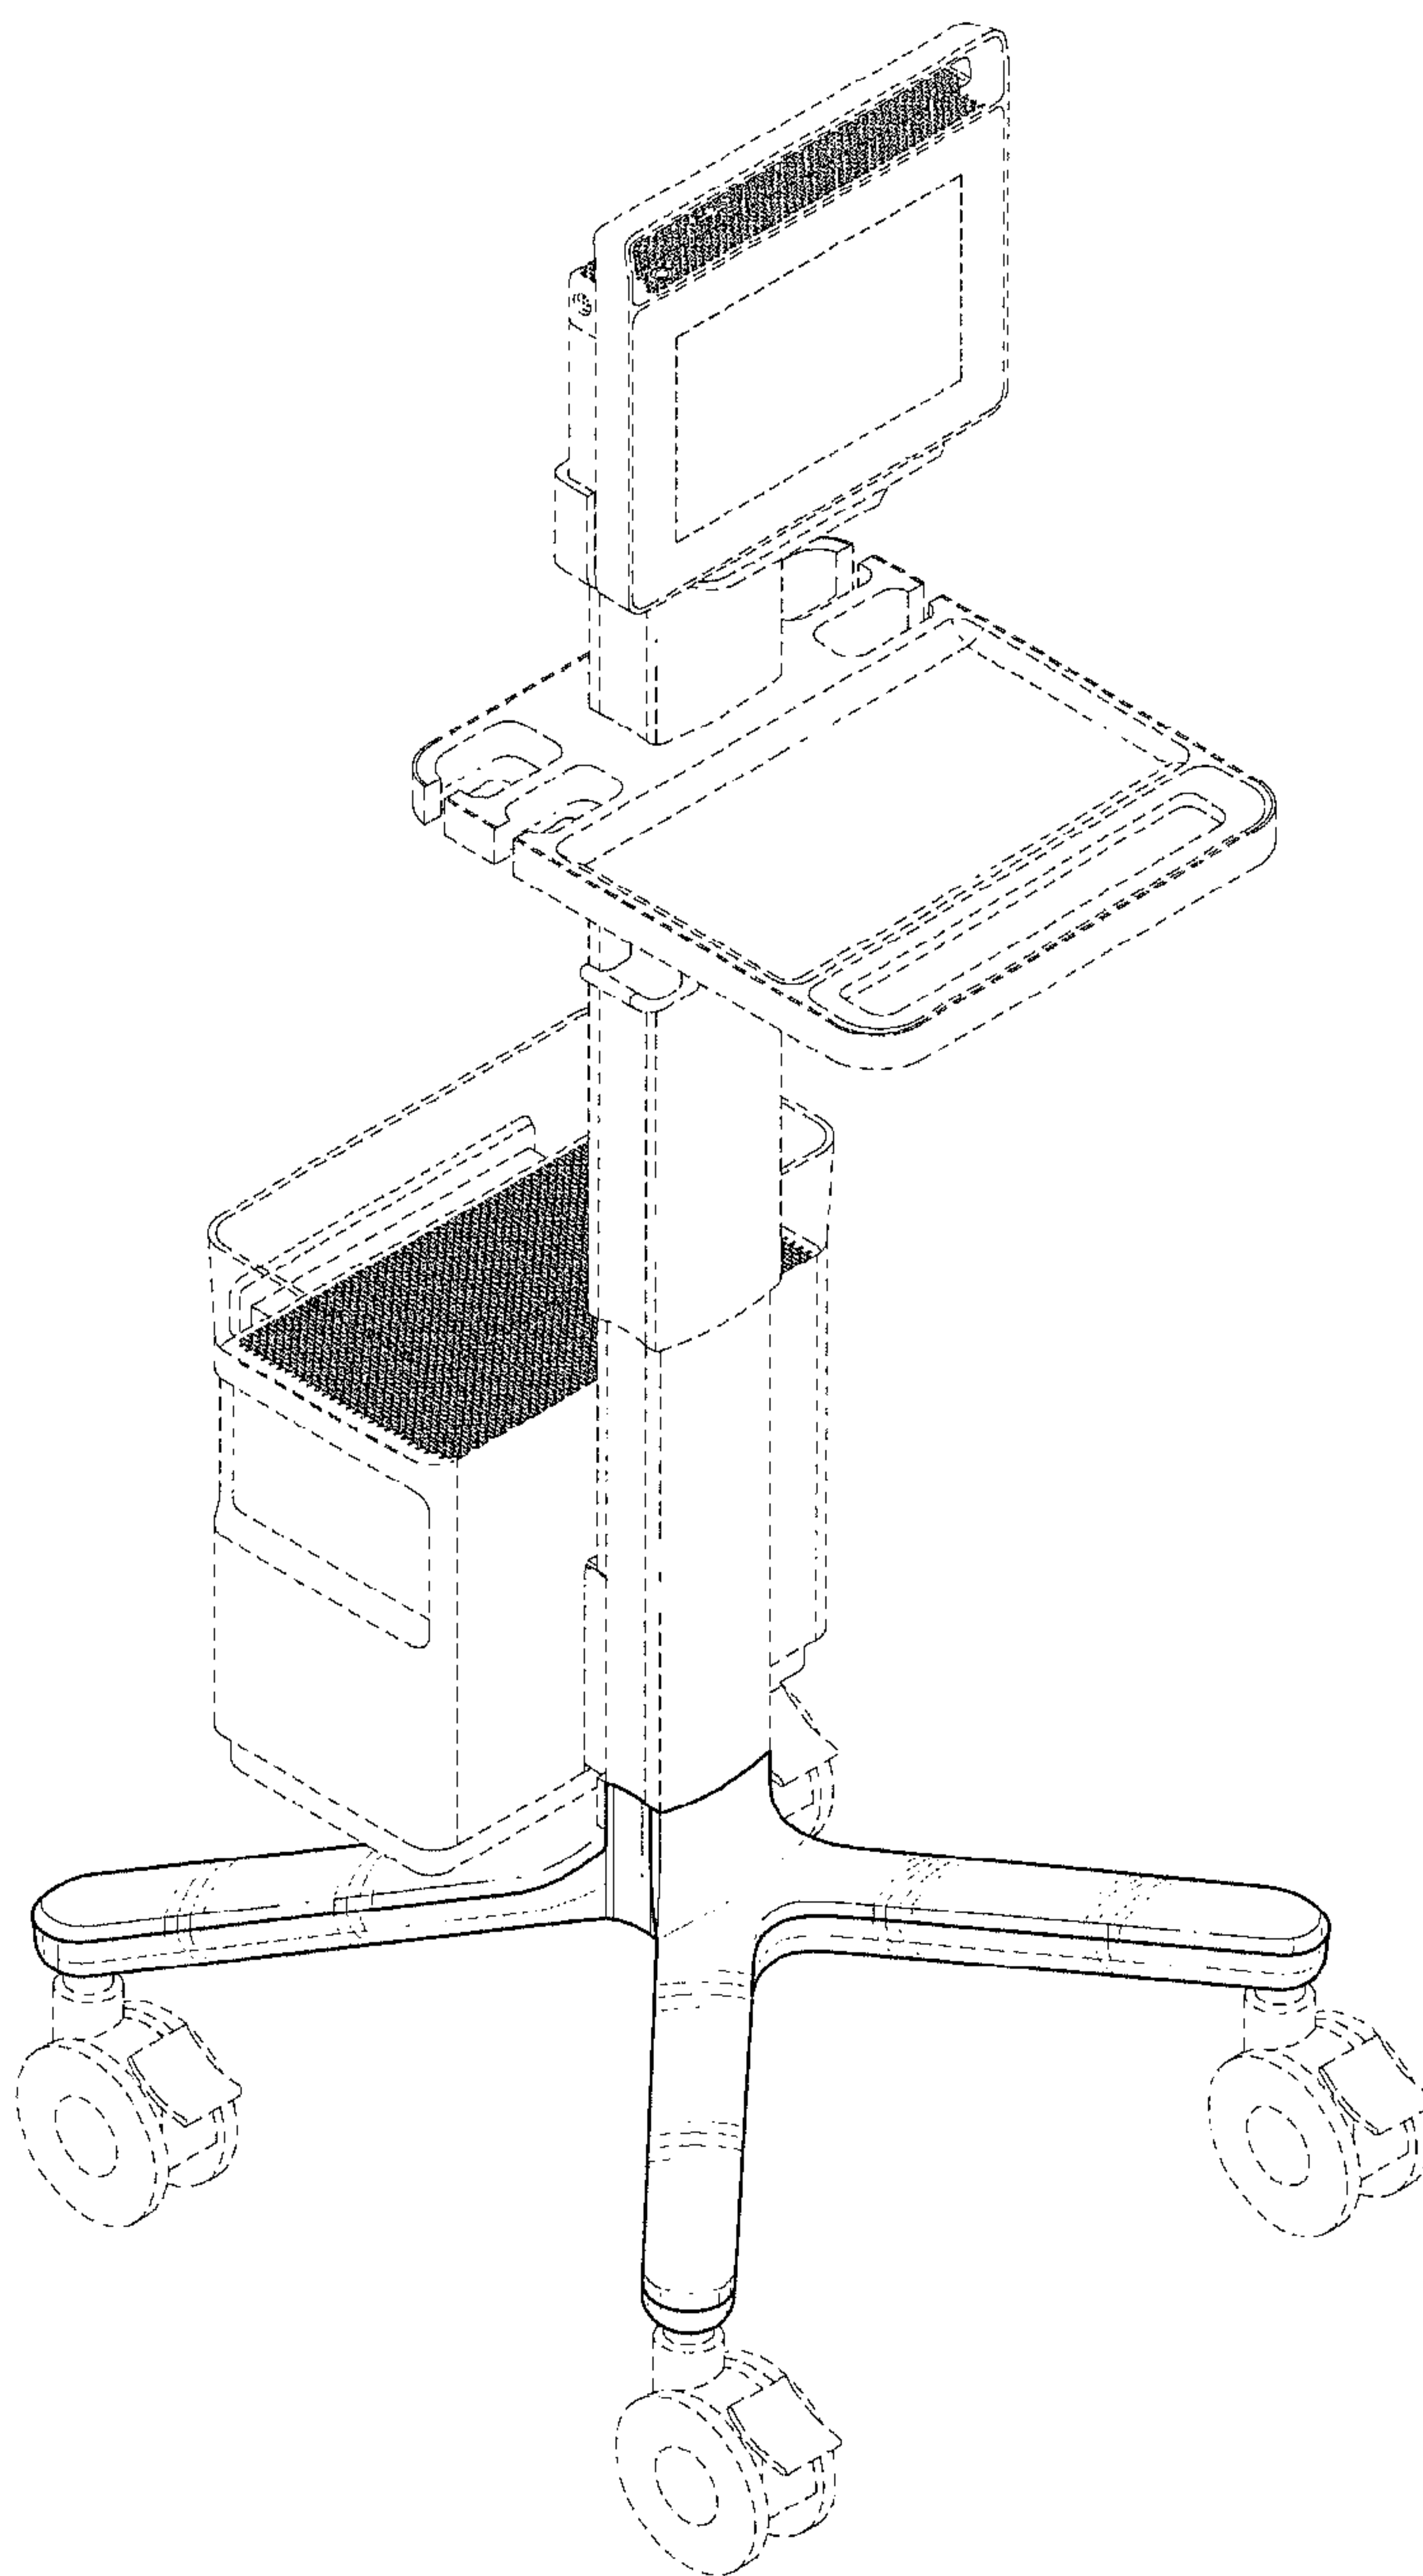


FIG.2

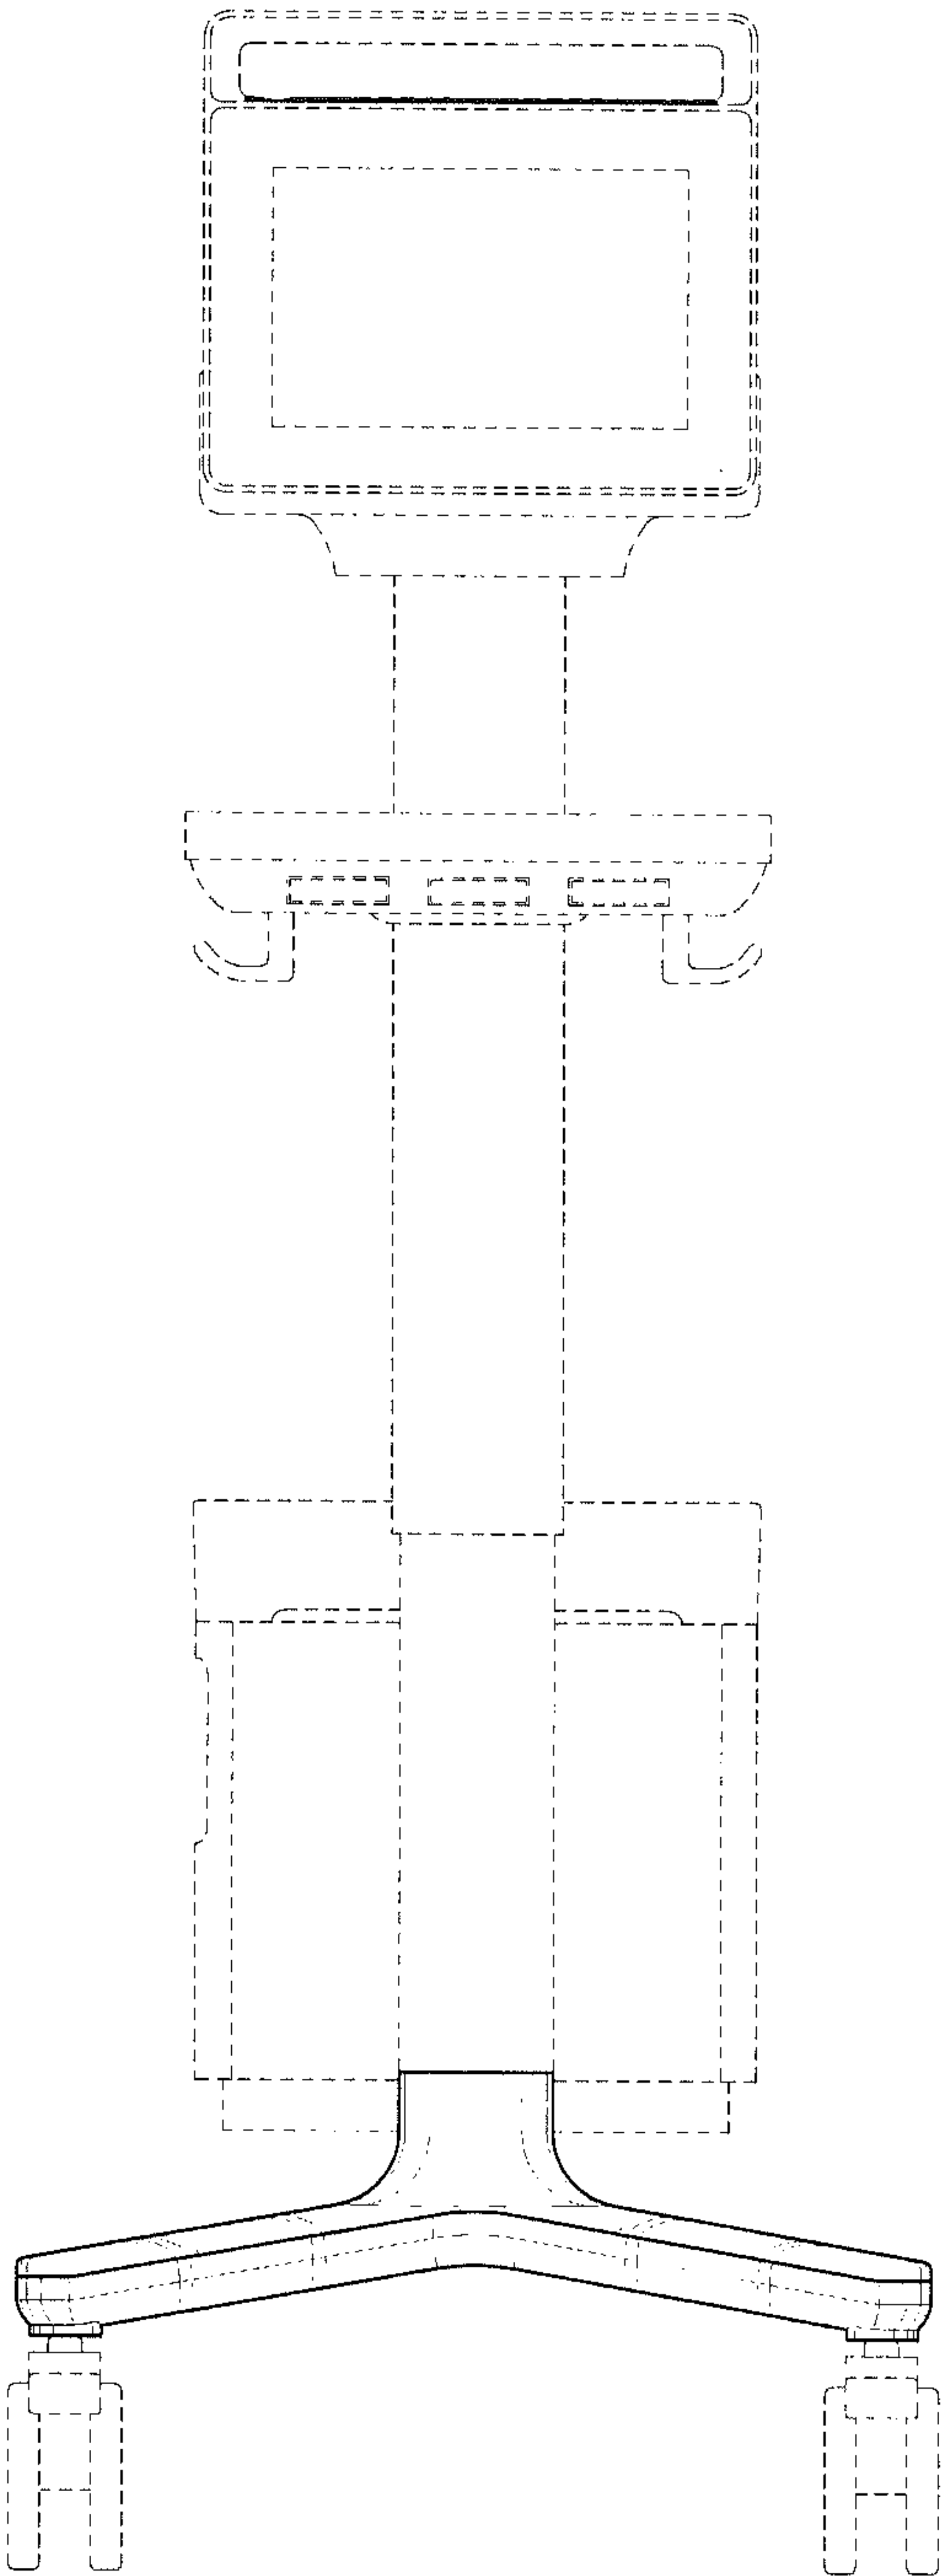


FIG. 3

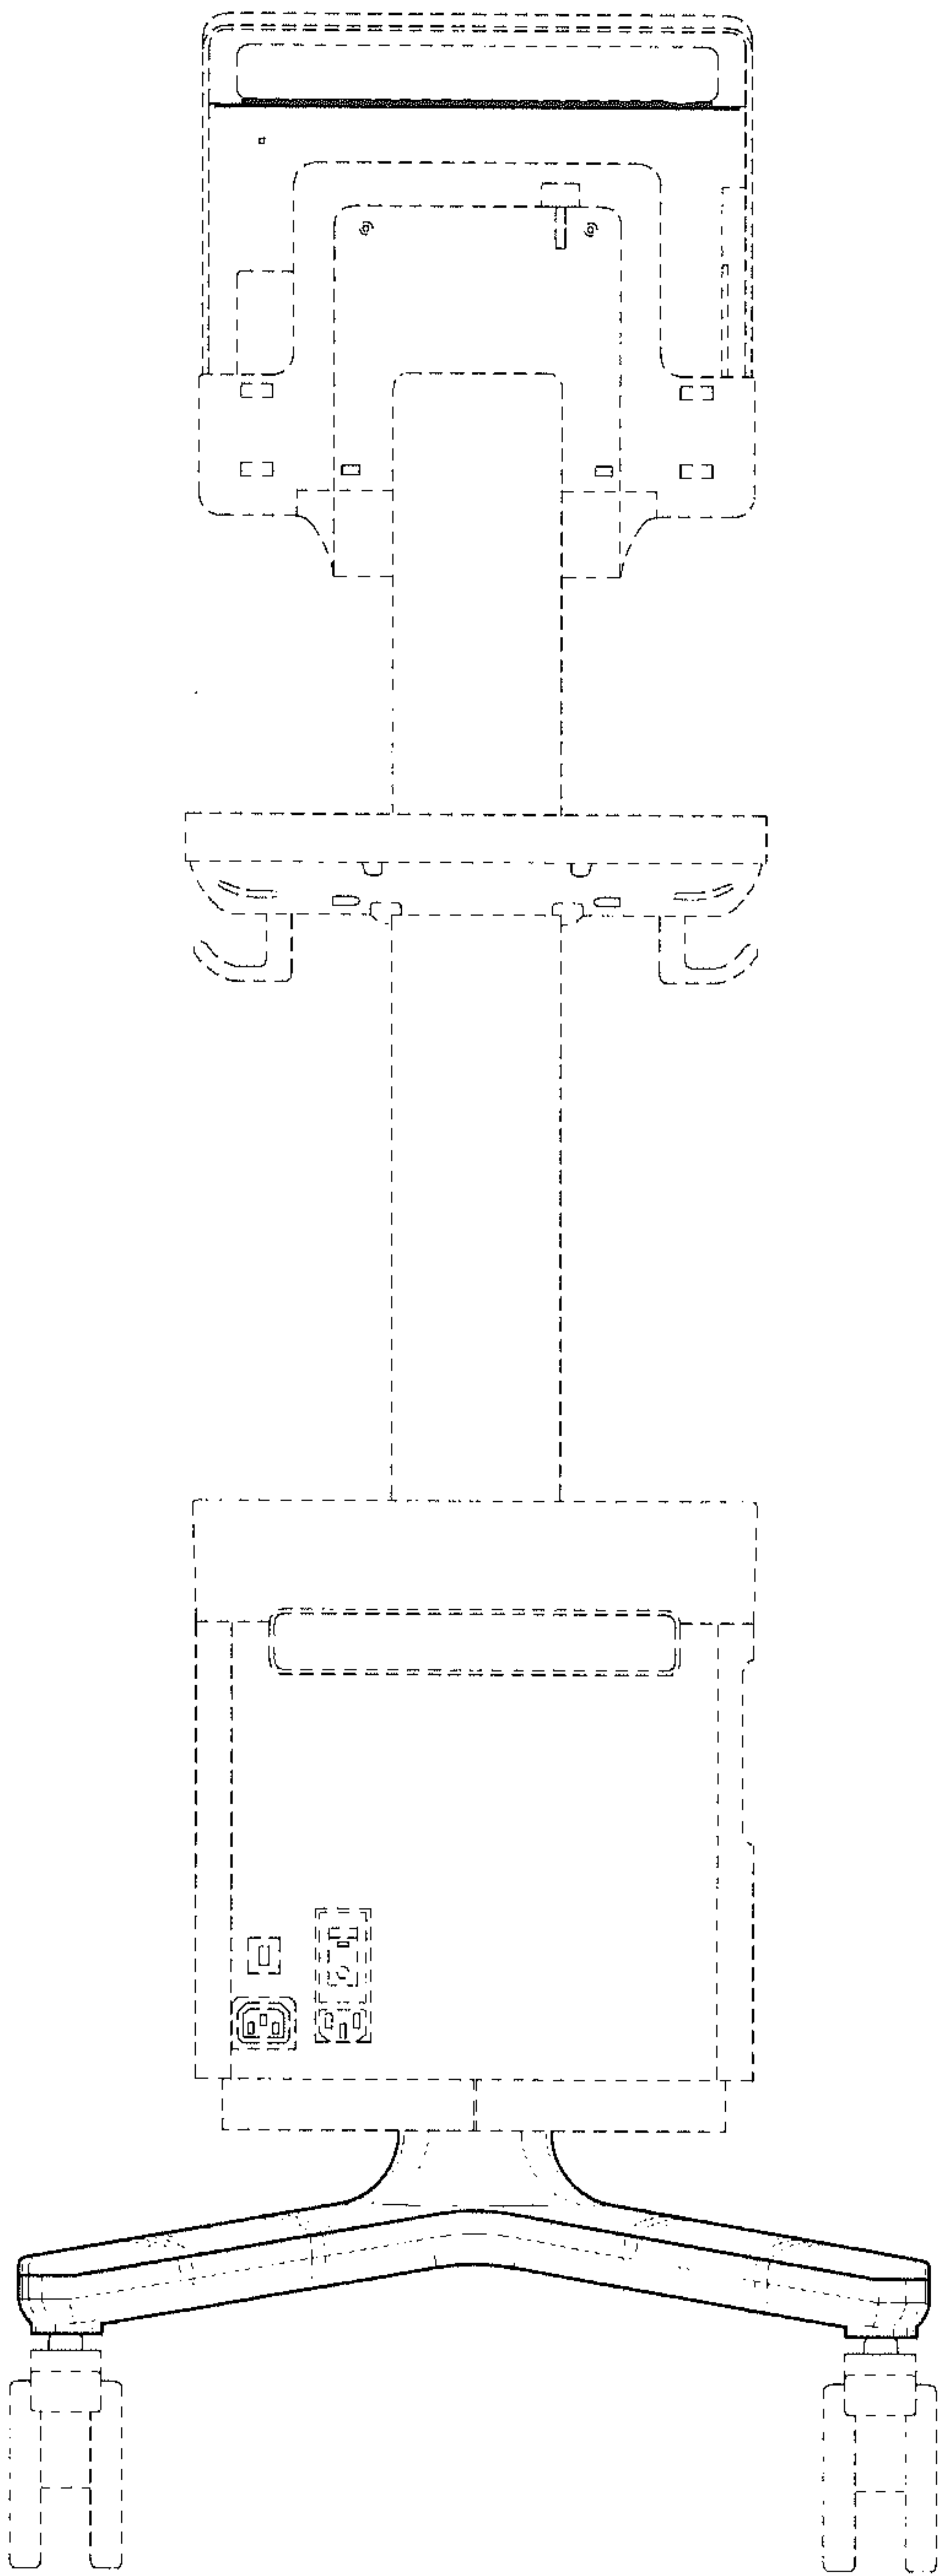


FIG. 4

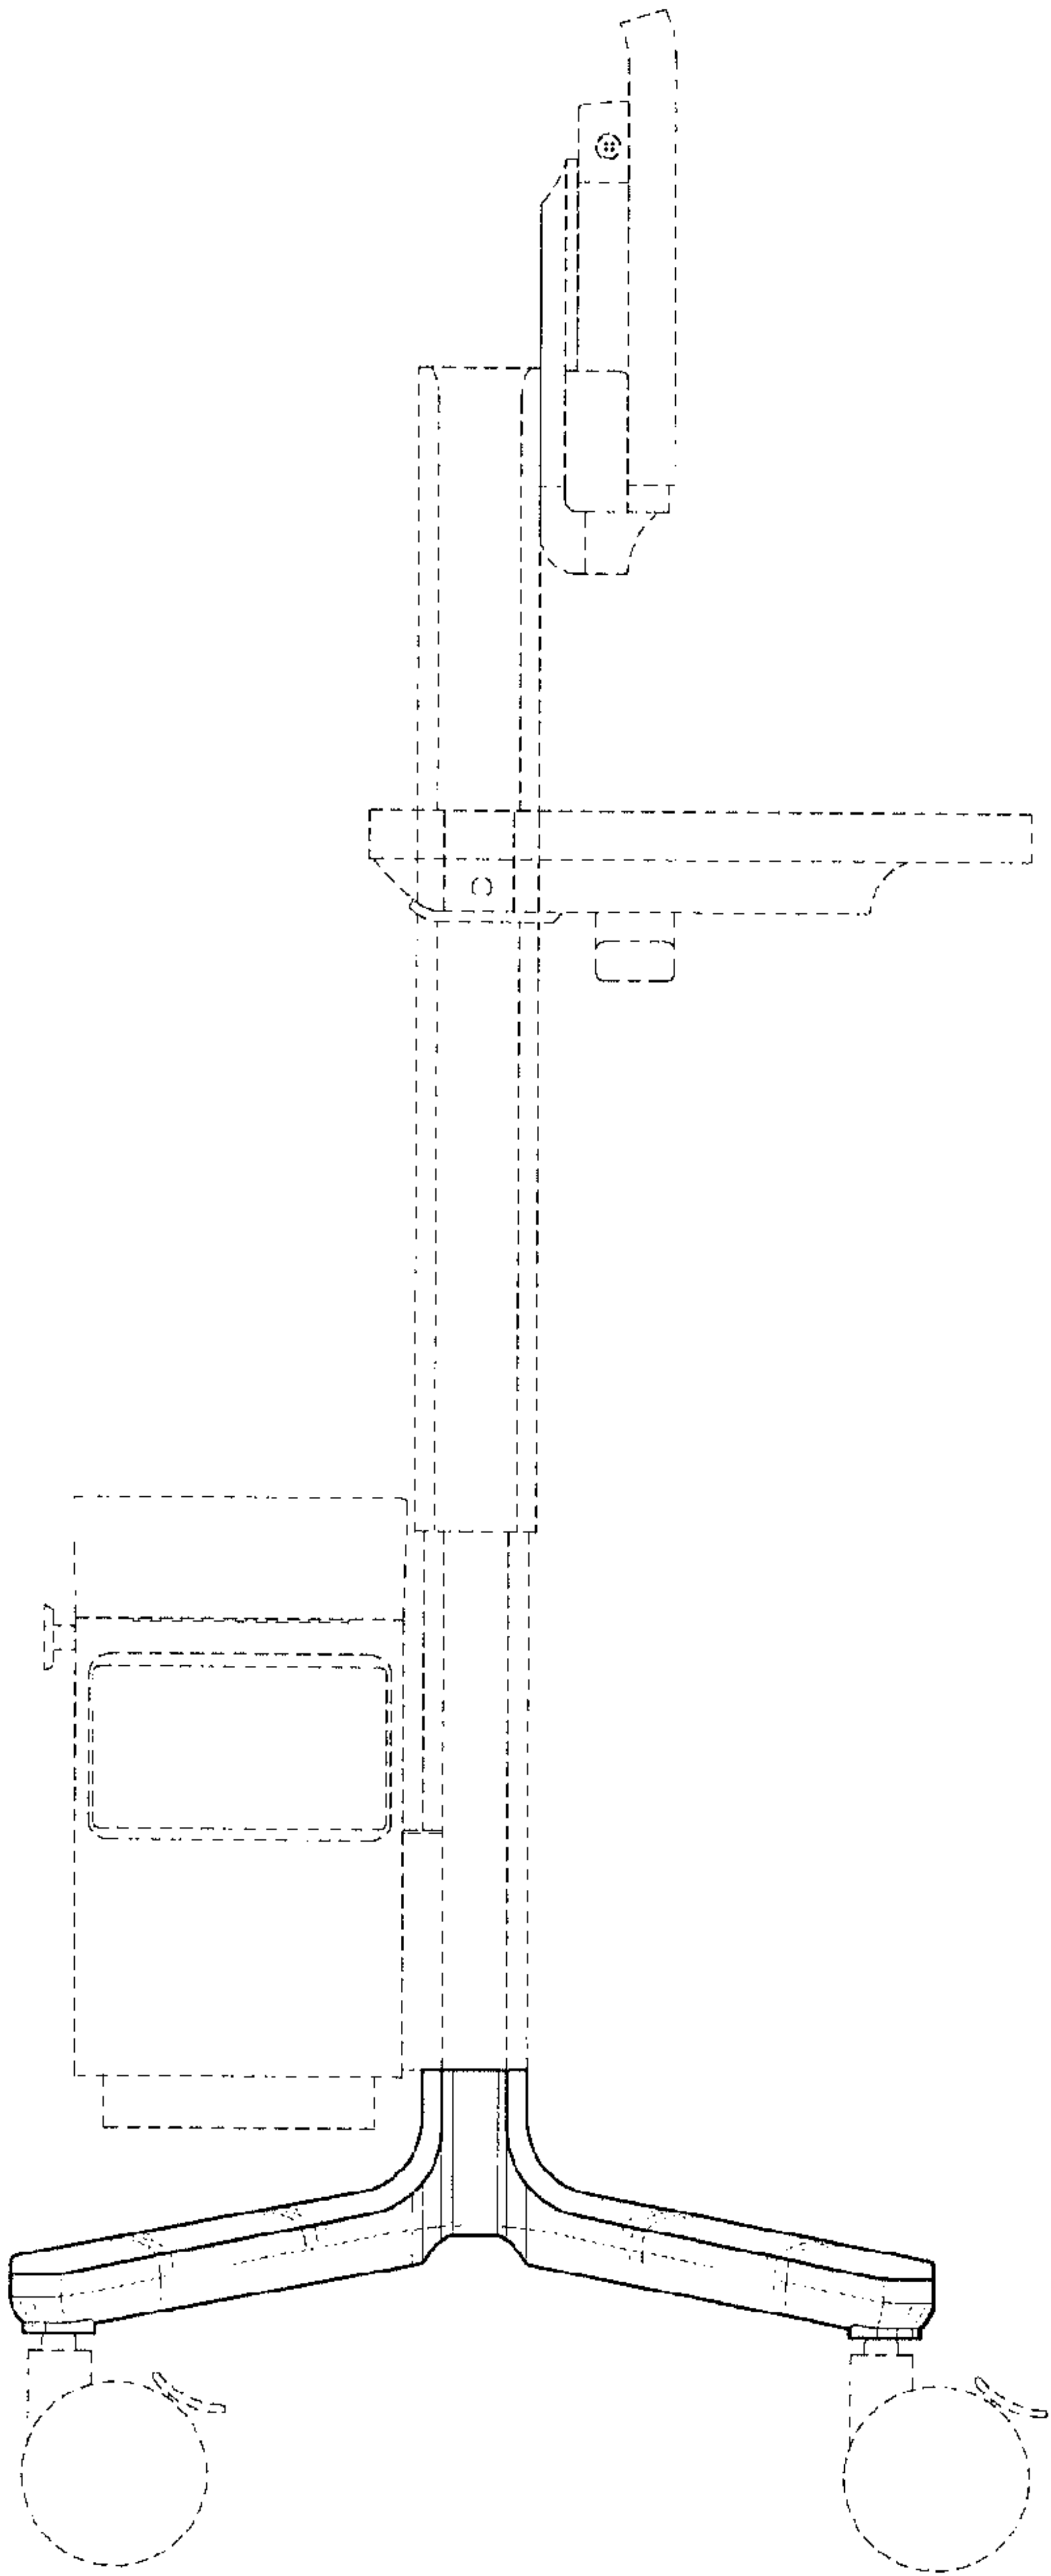


FIG.5

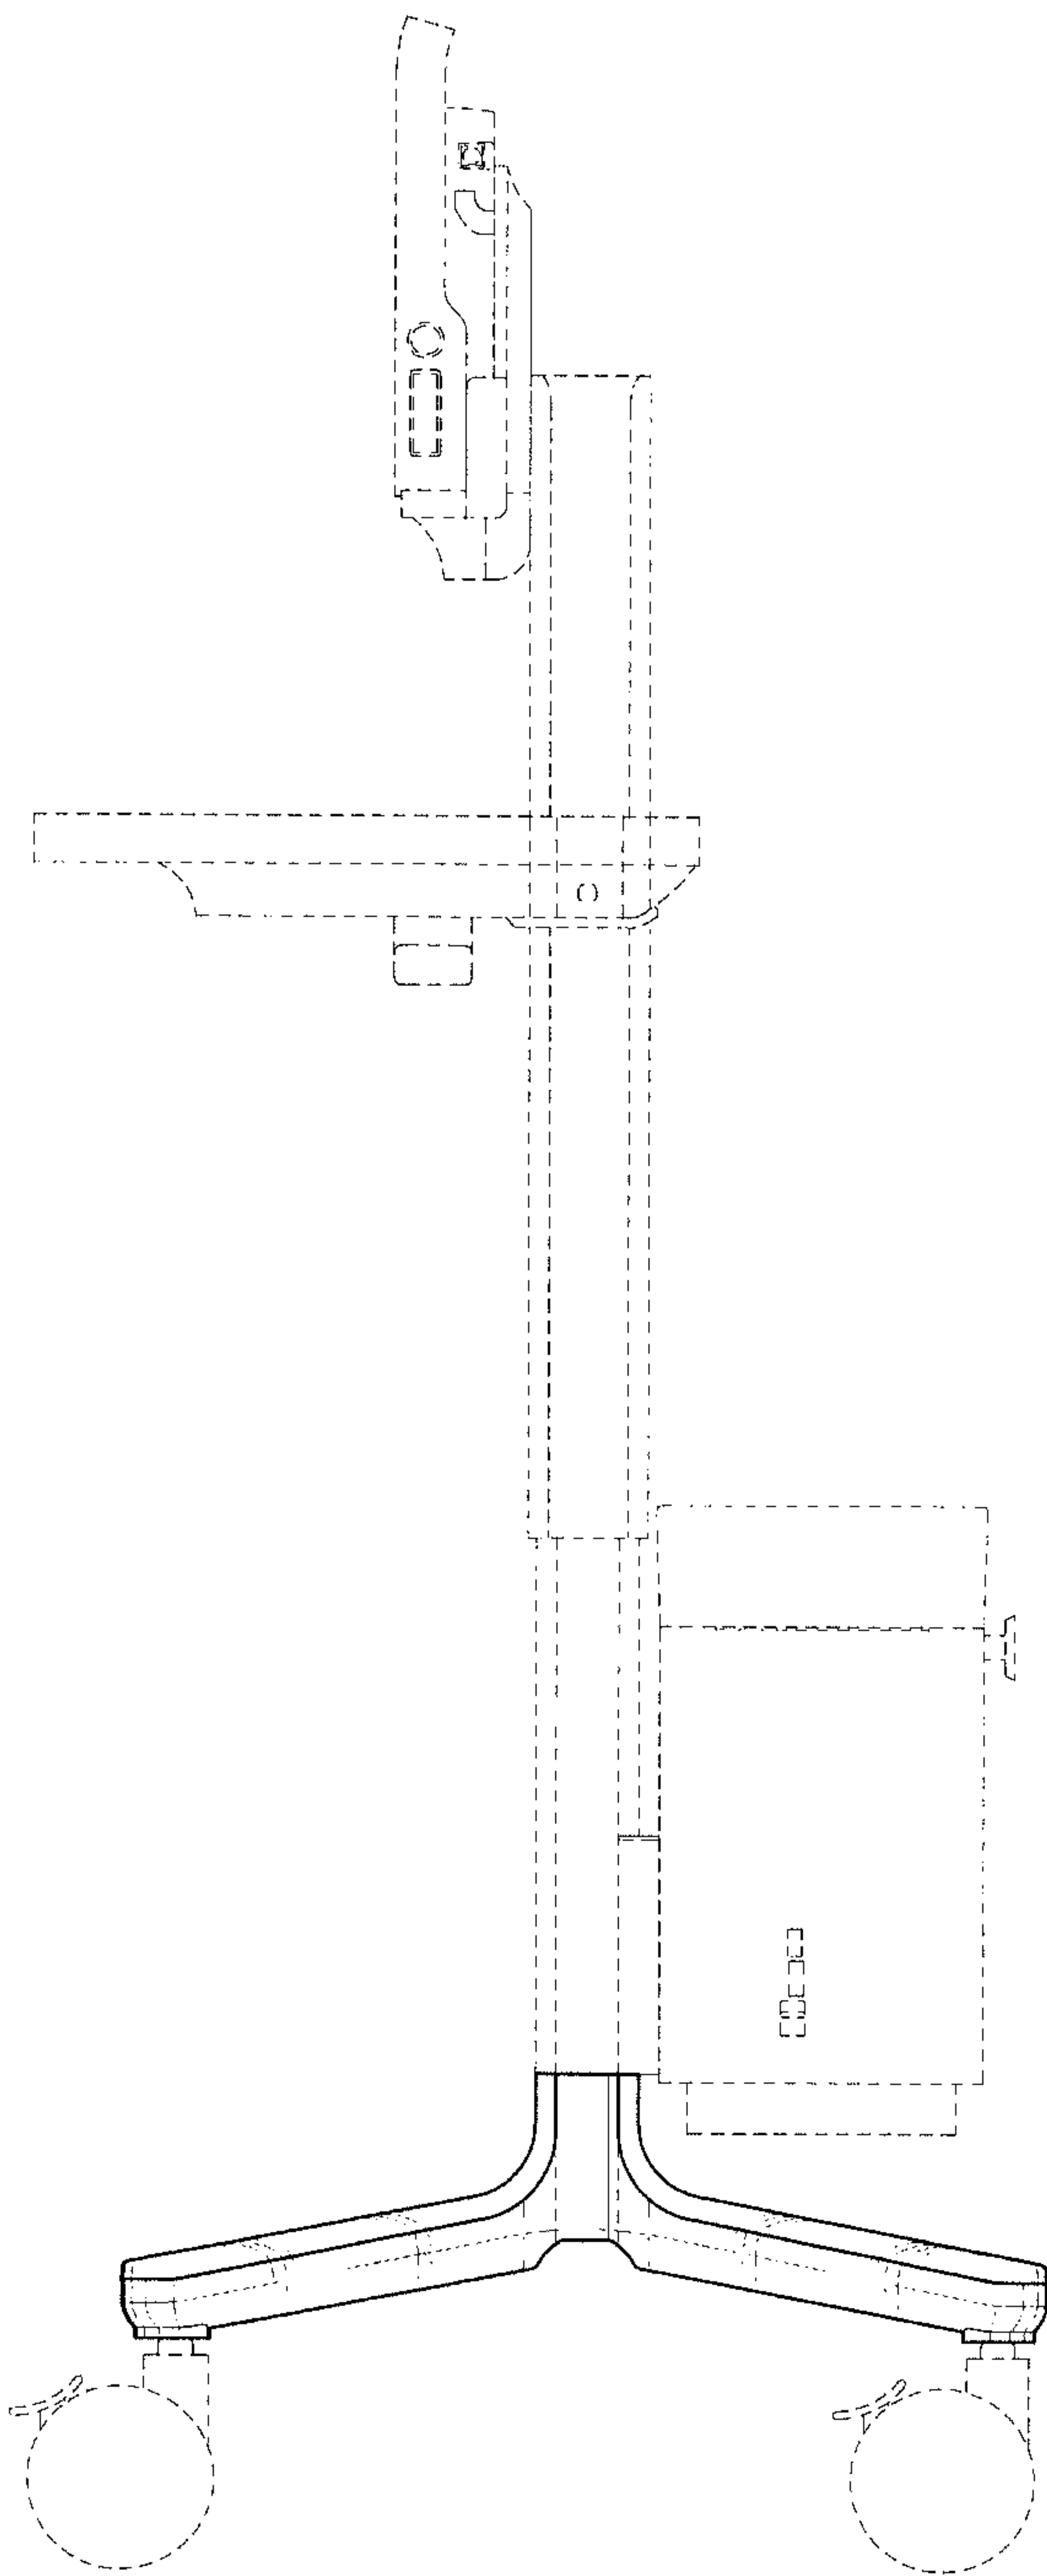


FIG.6

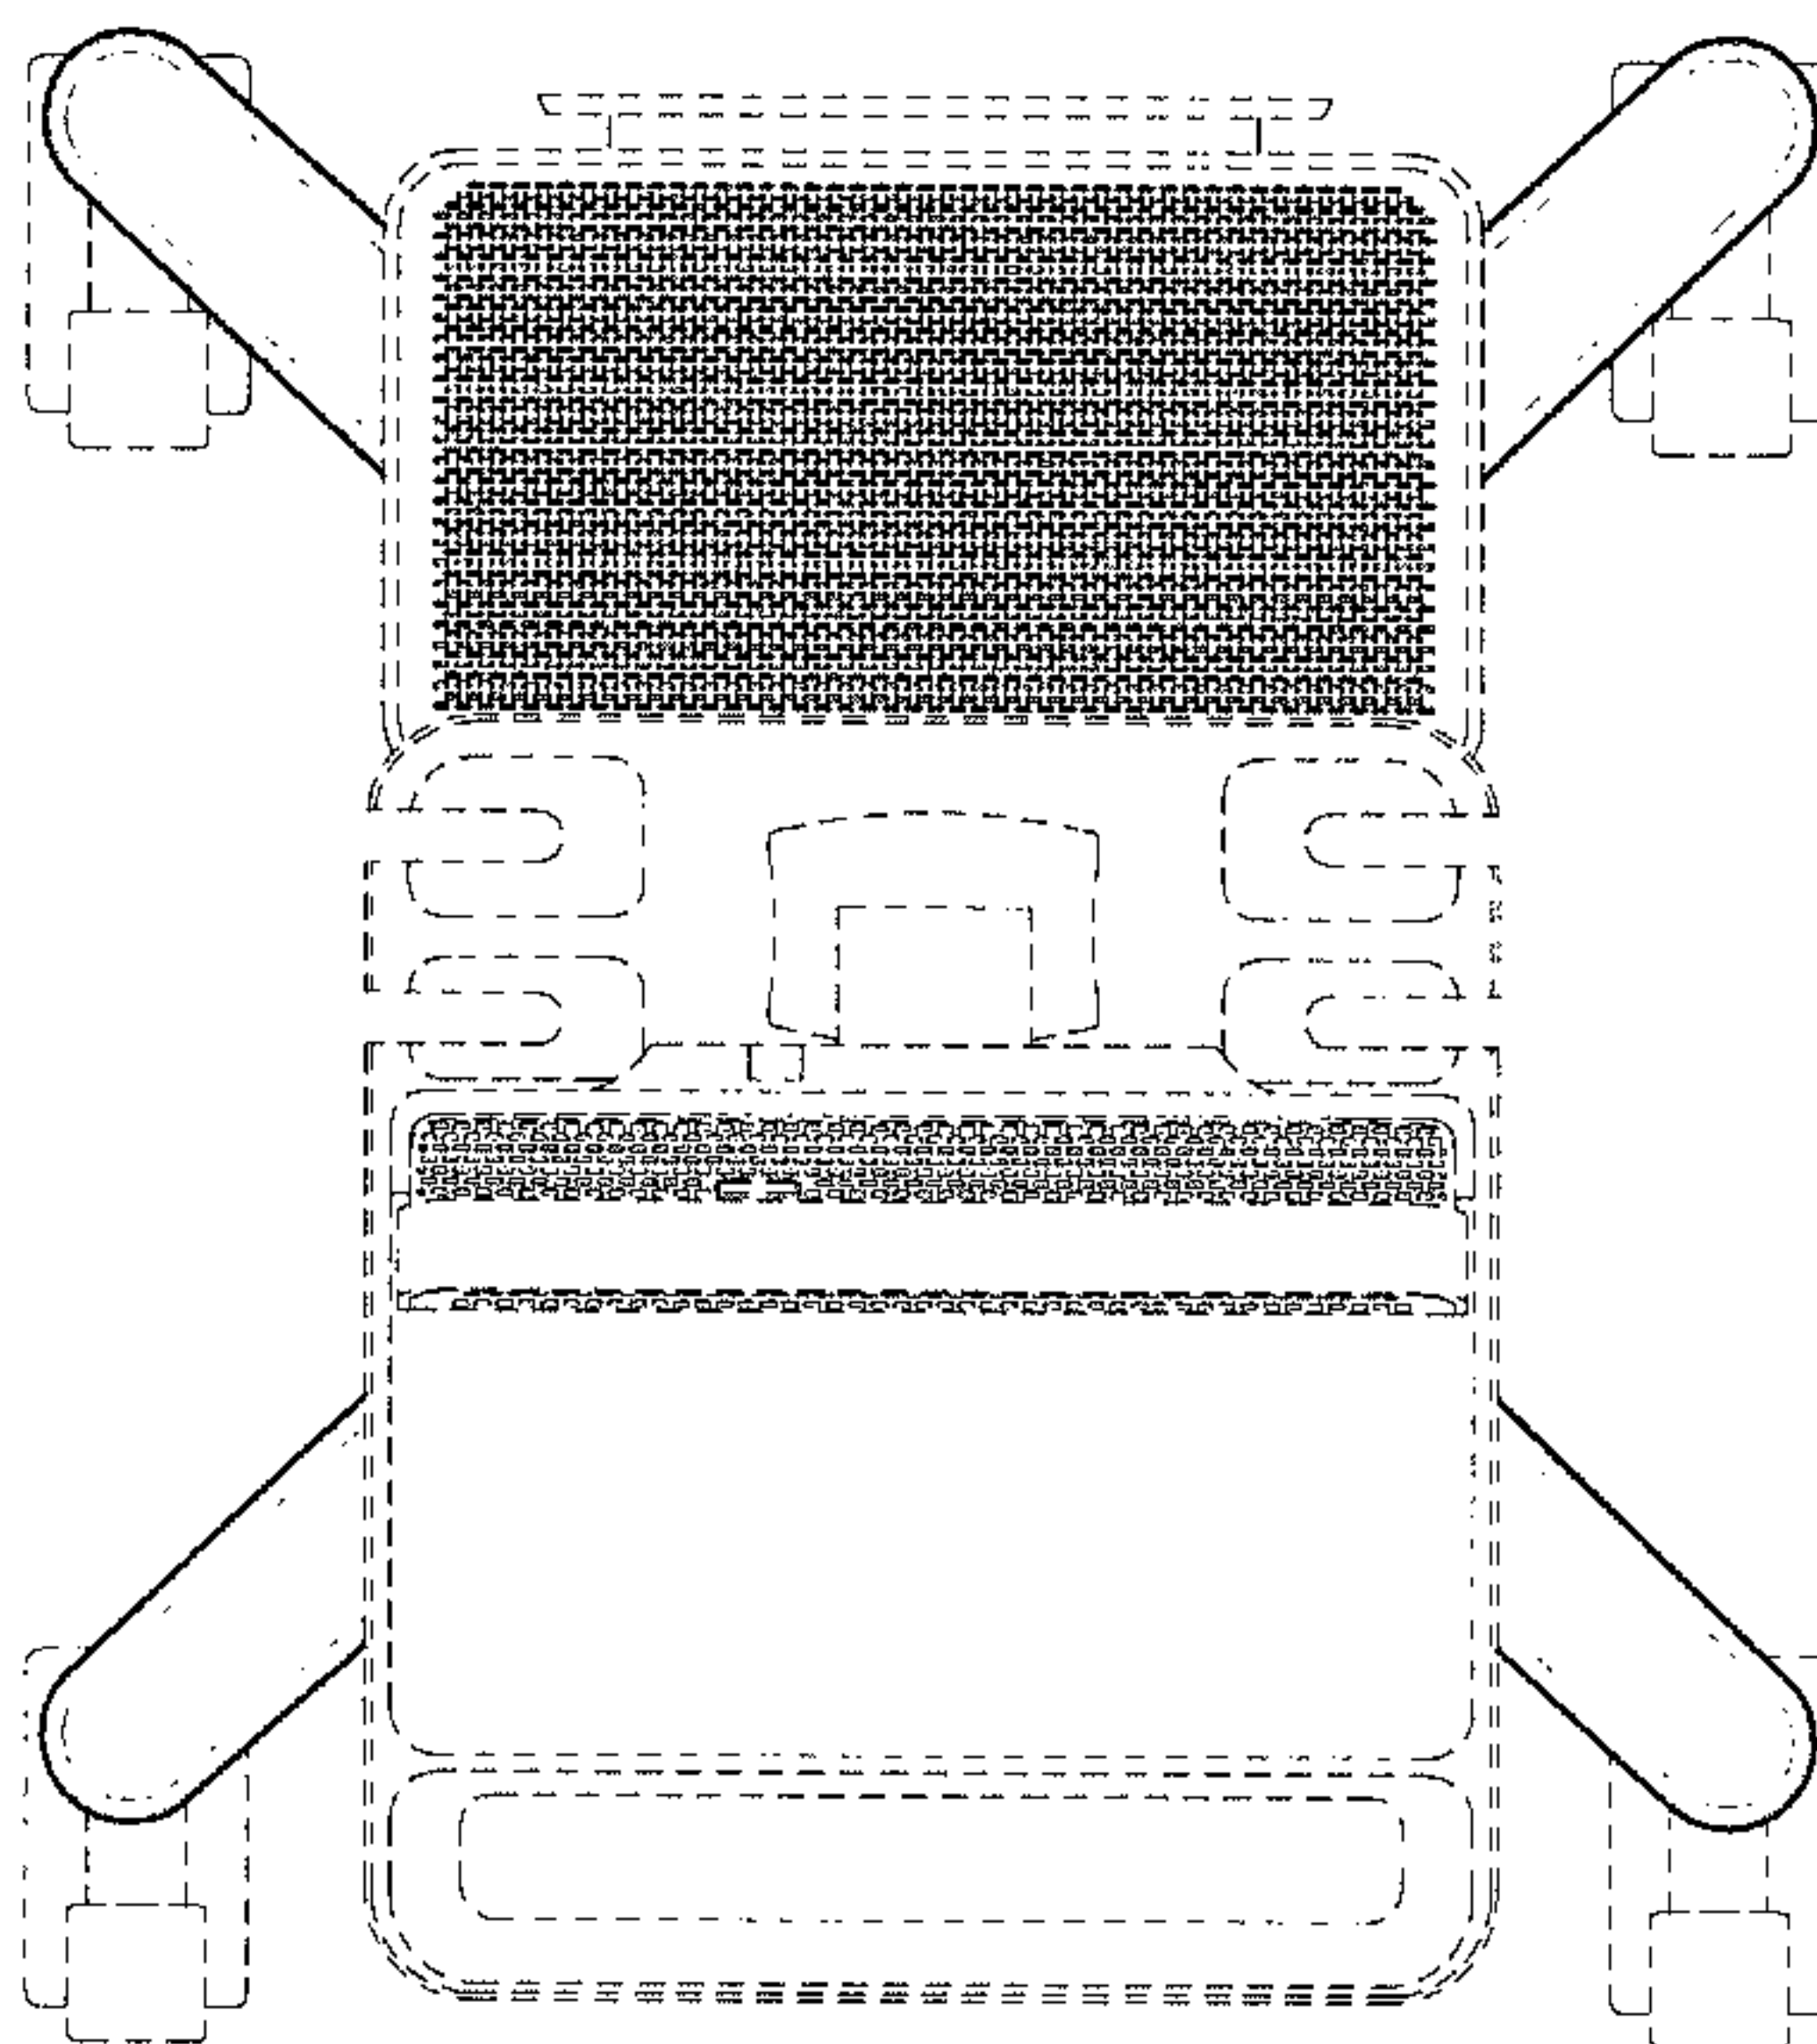


FIG. 7


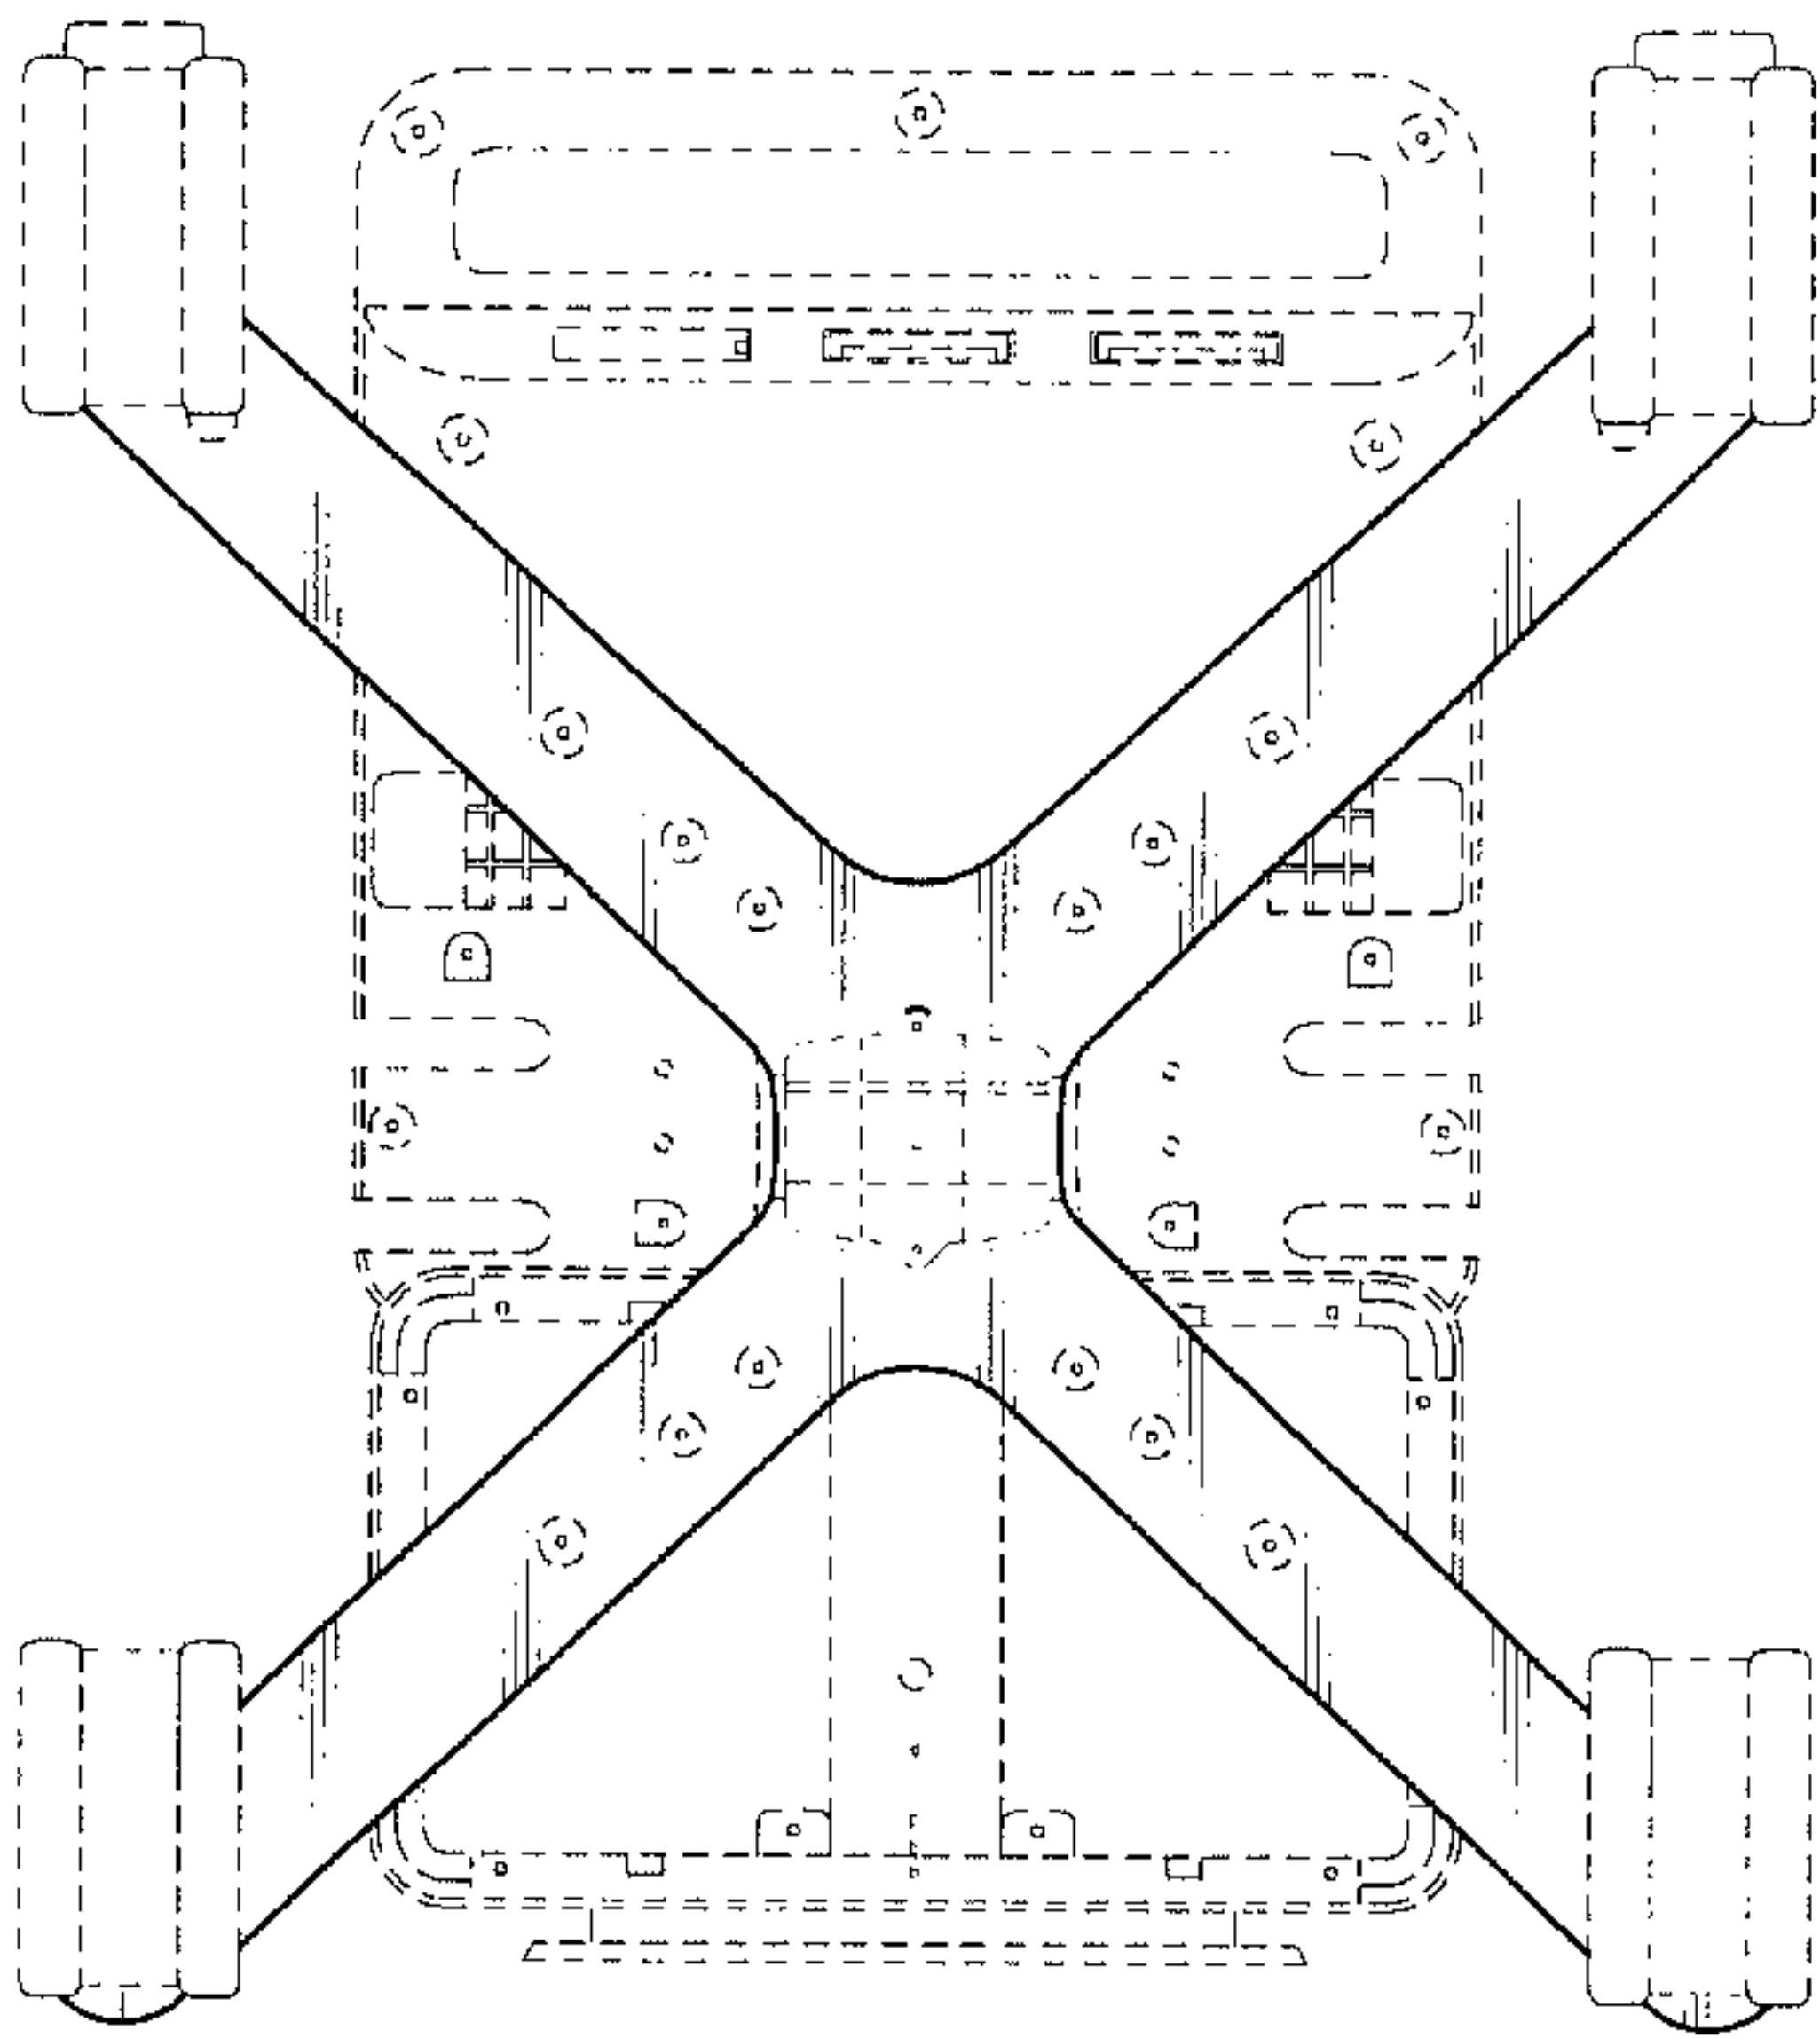


FIG. 8

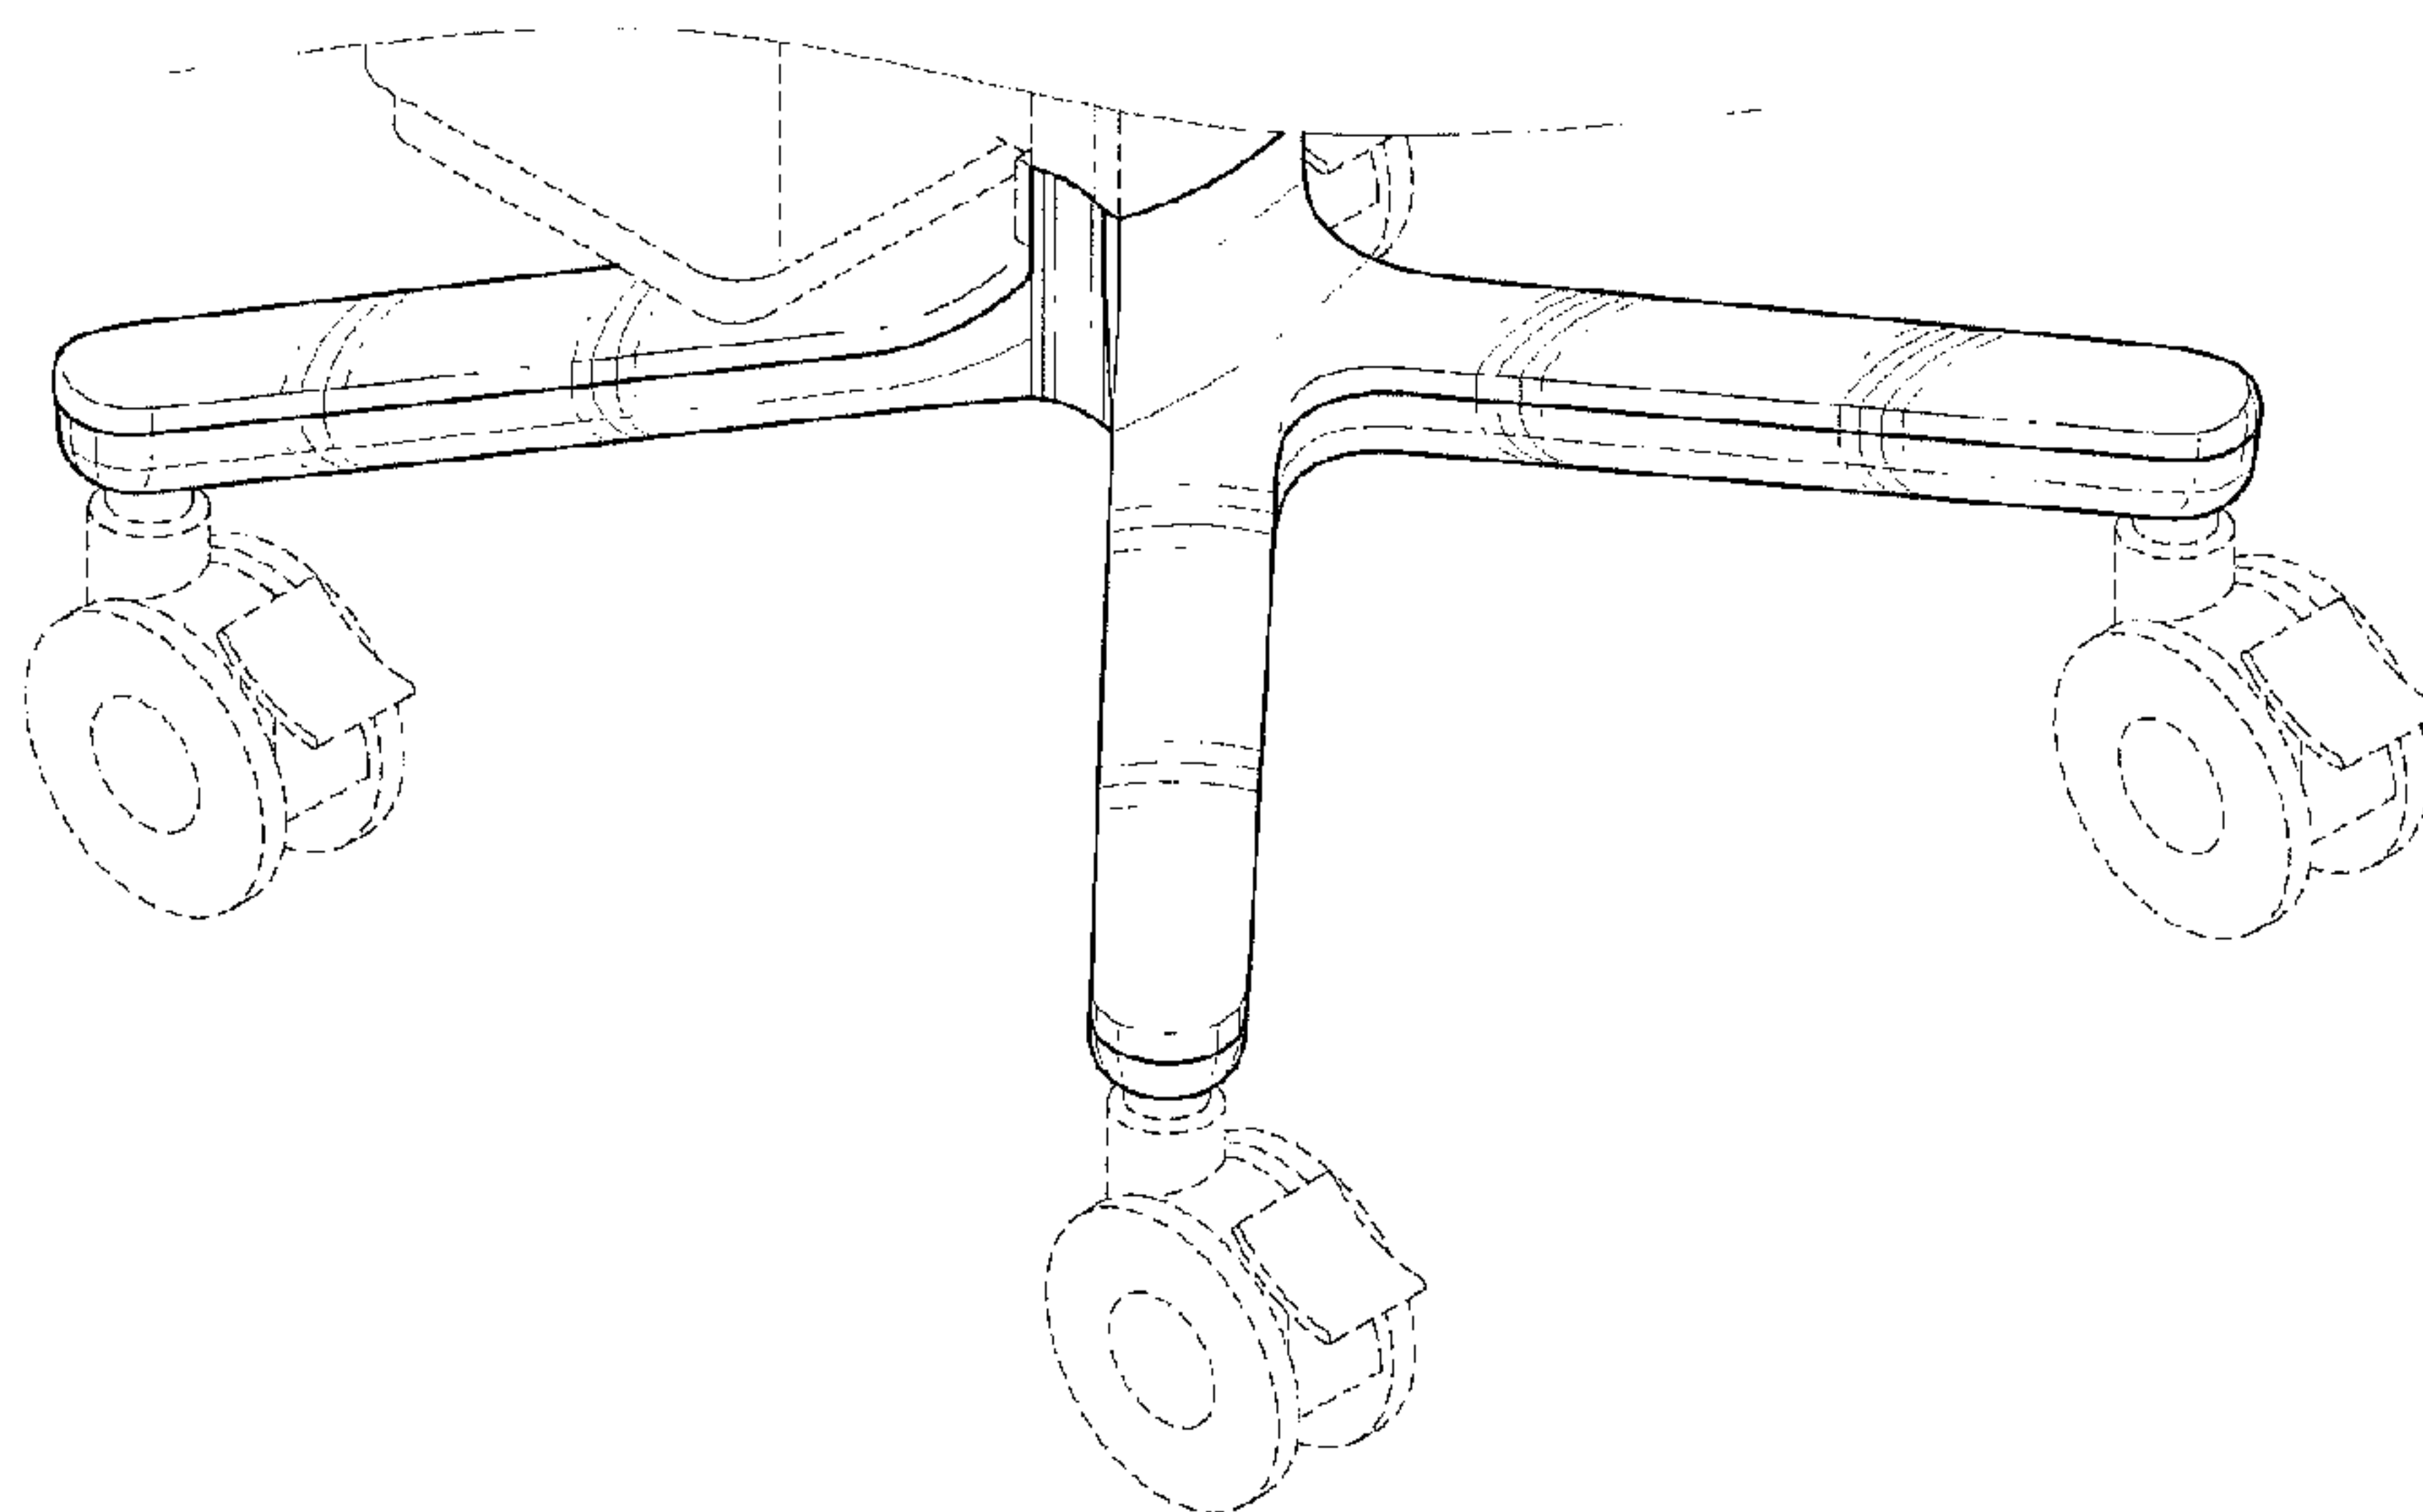

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : D697,621 S
APPLICATION NO. : 29/437927
DATED : January 14, 2014
INVENTOR(S) : Yeon-Moo Chung et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the Title Page Item (62) "Related U.S. Application Data" insert therefor -- Continuation of Application No. 29/431,369 filed on September 6, 2012. --.

Signed and Sealed this
Seventeenth Day of February, 2015



Michelle K. Lee
Deputy Director of the United States Patent and Trademark Office