



US00D700327S

(12) **United States Design Patent**  
**Darian**

(10) **Patent No.:** **US D700,327 S**  
(45) **Date of Patent:** **\*\* Feb. 25, 2014**

(54) **ULTRASONIC OSTEOTOME TIP**

(75) Inventor: **Alexander L. Darian**, Brightwaters, NY (US)

(73) Assignee: **Misonix, Inc.**, Farmingdale, NY (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/403,580**

(22) Filed: **Oct. 7, 2011**

(51) **LOC (10) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/146**

(58) **Field of Classification Search**  
USPC ..... D24/144, 146-147, 170; D8/20, 26, 98;  
606/1, 39, 45, 53, 83-85, 86 R, 79, 167,  
606/169-171  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,261,922	A *	11/1993	Hood	.....	606/167
5,318,570	A *	6/1994	Hood et al.	.....	D24/144
5,935,142	A *	8/1999	Hood	.....	606/169
6,254,622	B1 *	7/2001	Hood	.....	606/169
6,423,082	B1 *	7/2002	Houser et al.	.....	606/169
6,443,969	B1 *	9/2002	Novak et al.	.....	606/169
7,217,270	B2 *	5/2007	Clement et al.	.....	606/45

D667,117	S *	9/2012	Darian et al.	.....	D24/144
2005/0234484	A1 *	10/2005	Houser et al.	.....	606/167
2005/0273127	A1 *	12/2005	Novak et al.	.....	606/169
2010/0057118	A1 *	3/2010	Dietz et al.	.....	606/169
2010/0089405	A1 *	4/2010	Johnson et al.	.....	128/207.29
2013/0090660	A1 *	4/2013	Darian	.....	606/84

\* cited by examiner

*Primary Examiner* — Wan Laymon

(74) *Attorney, Agent, or Firm* — R. Neil Sudol; Coleman Sudol Sapone, P.C.


(57) **CLAIM**

The ornamental design for the ultrasonic osteotome tip, as shown and described.

**DESCRIPTION**

FIG. 1 is a top, front, and left side perspective view of an ultrasonic osteotome tip, showing my new design; FIG. 2 is a left-side elevational view thereof, the right side elevation being a mirror image; FIG. 3 is a bottom plan view thereof; FIG. 4 is a top plan view thereof; FIG. 5 is a front elevational view thereof; and, FIG. 6 is a rear elevational view thereof. The broken lines in FIG. 6 are included for the purpose of illustrating portions of the ultrasonic osteotome tip that form no part of the claimed design.

**1 Claim, 1 Drawing Sheet**

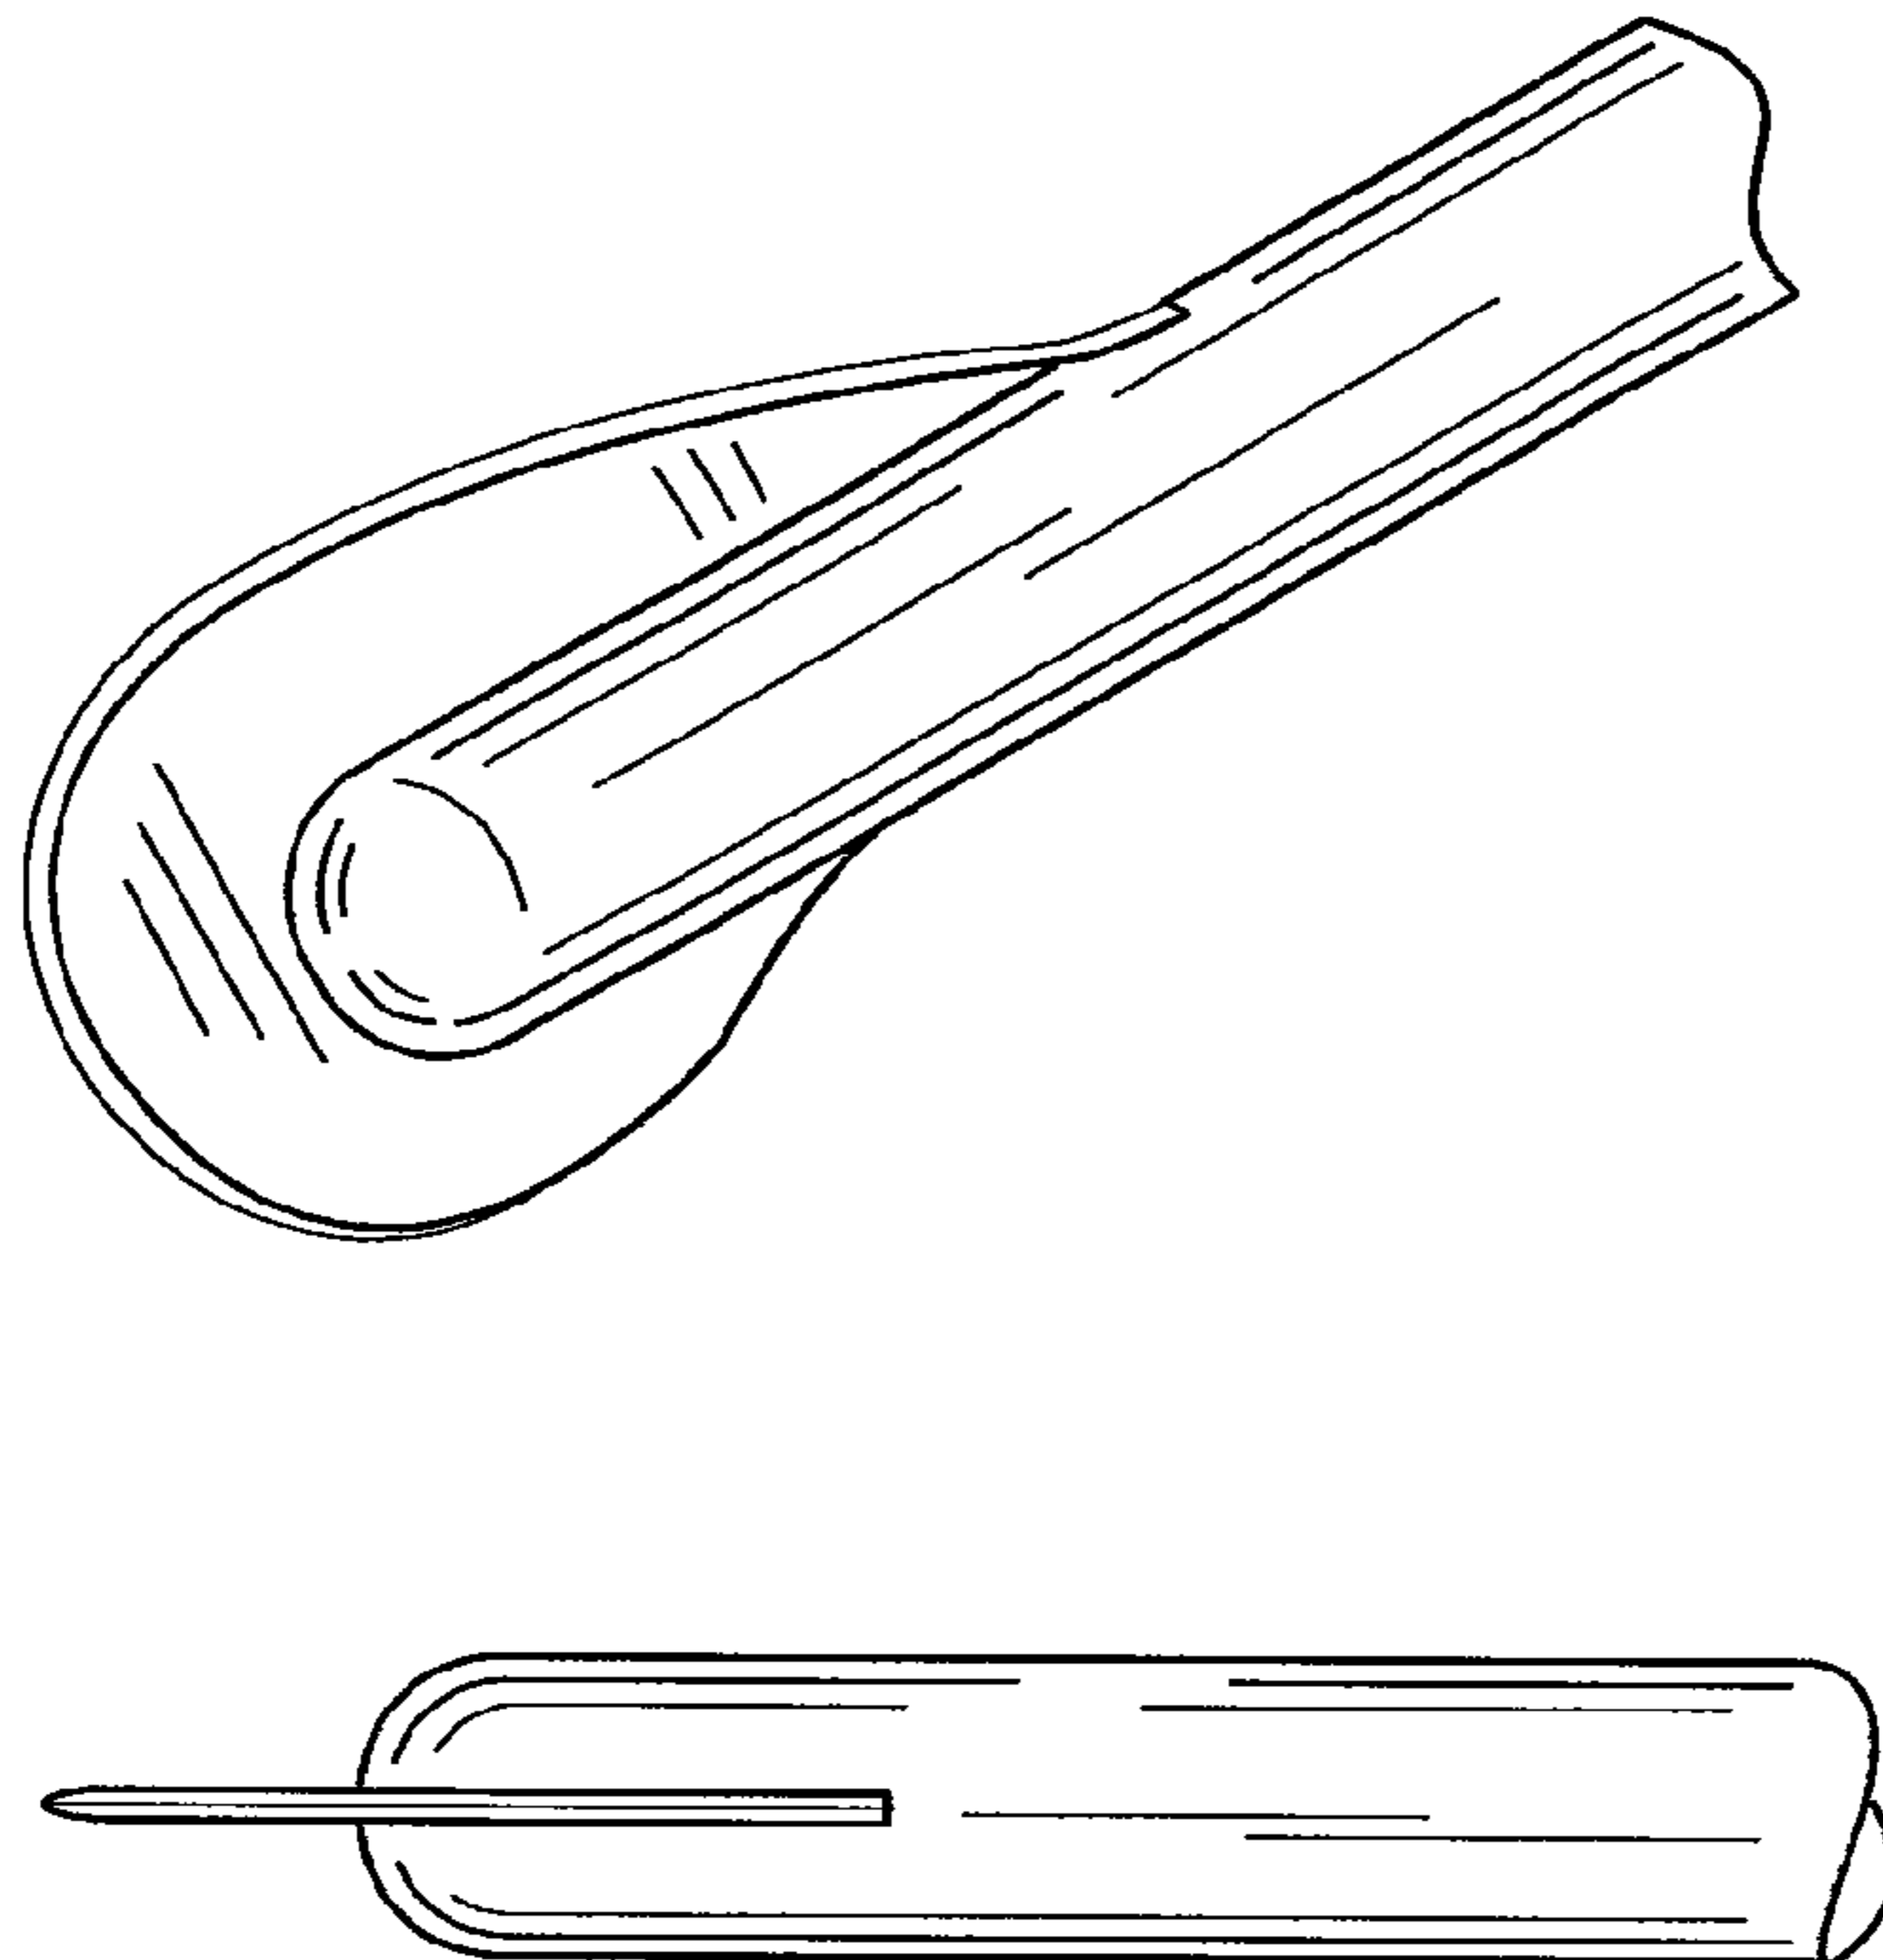

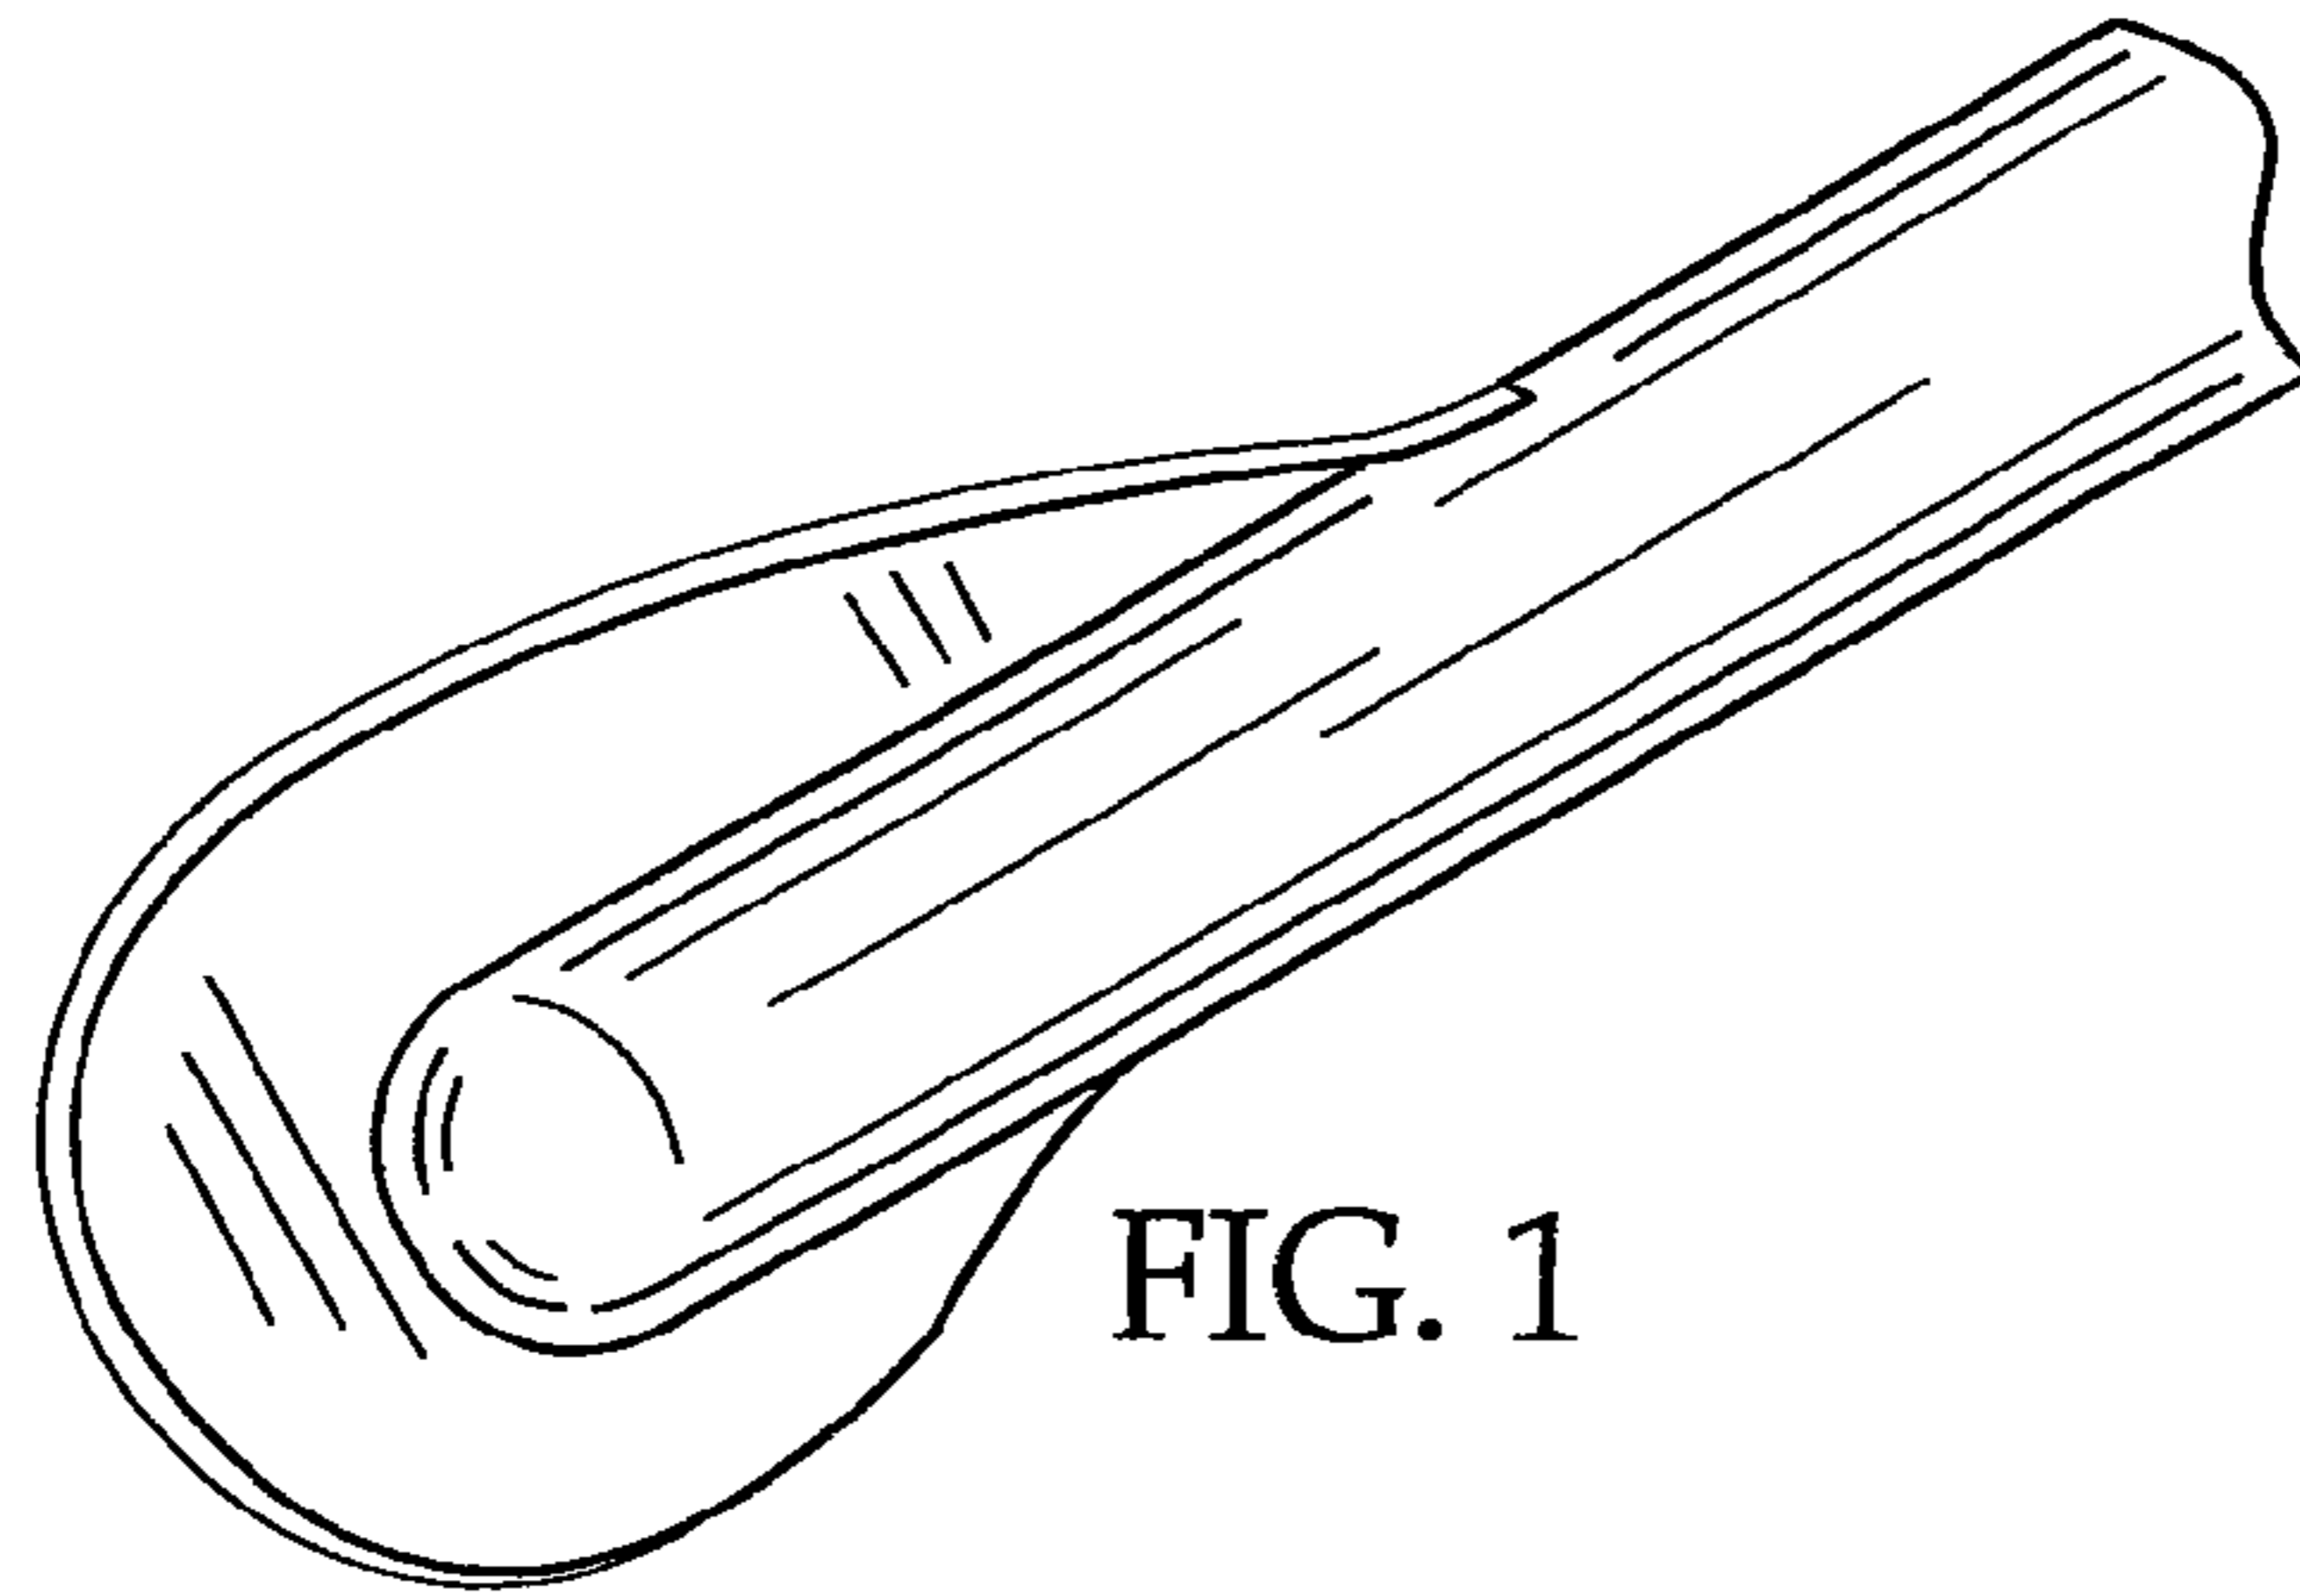


FIG. 1

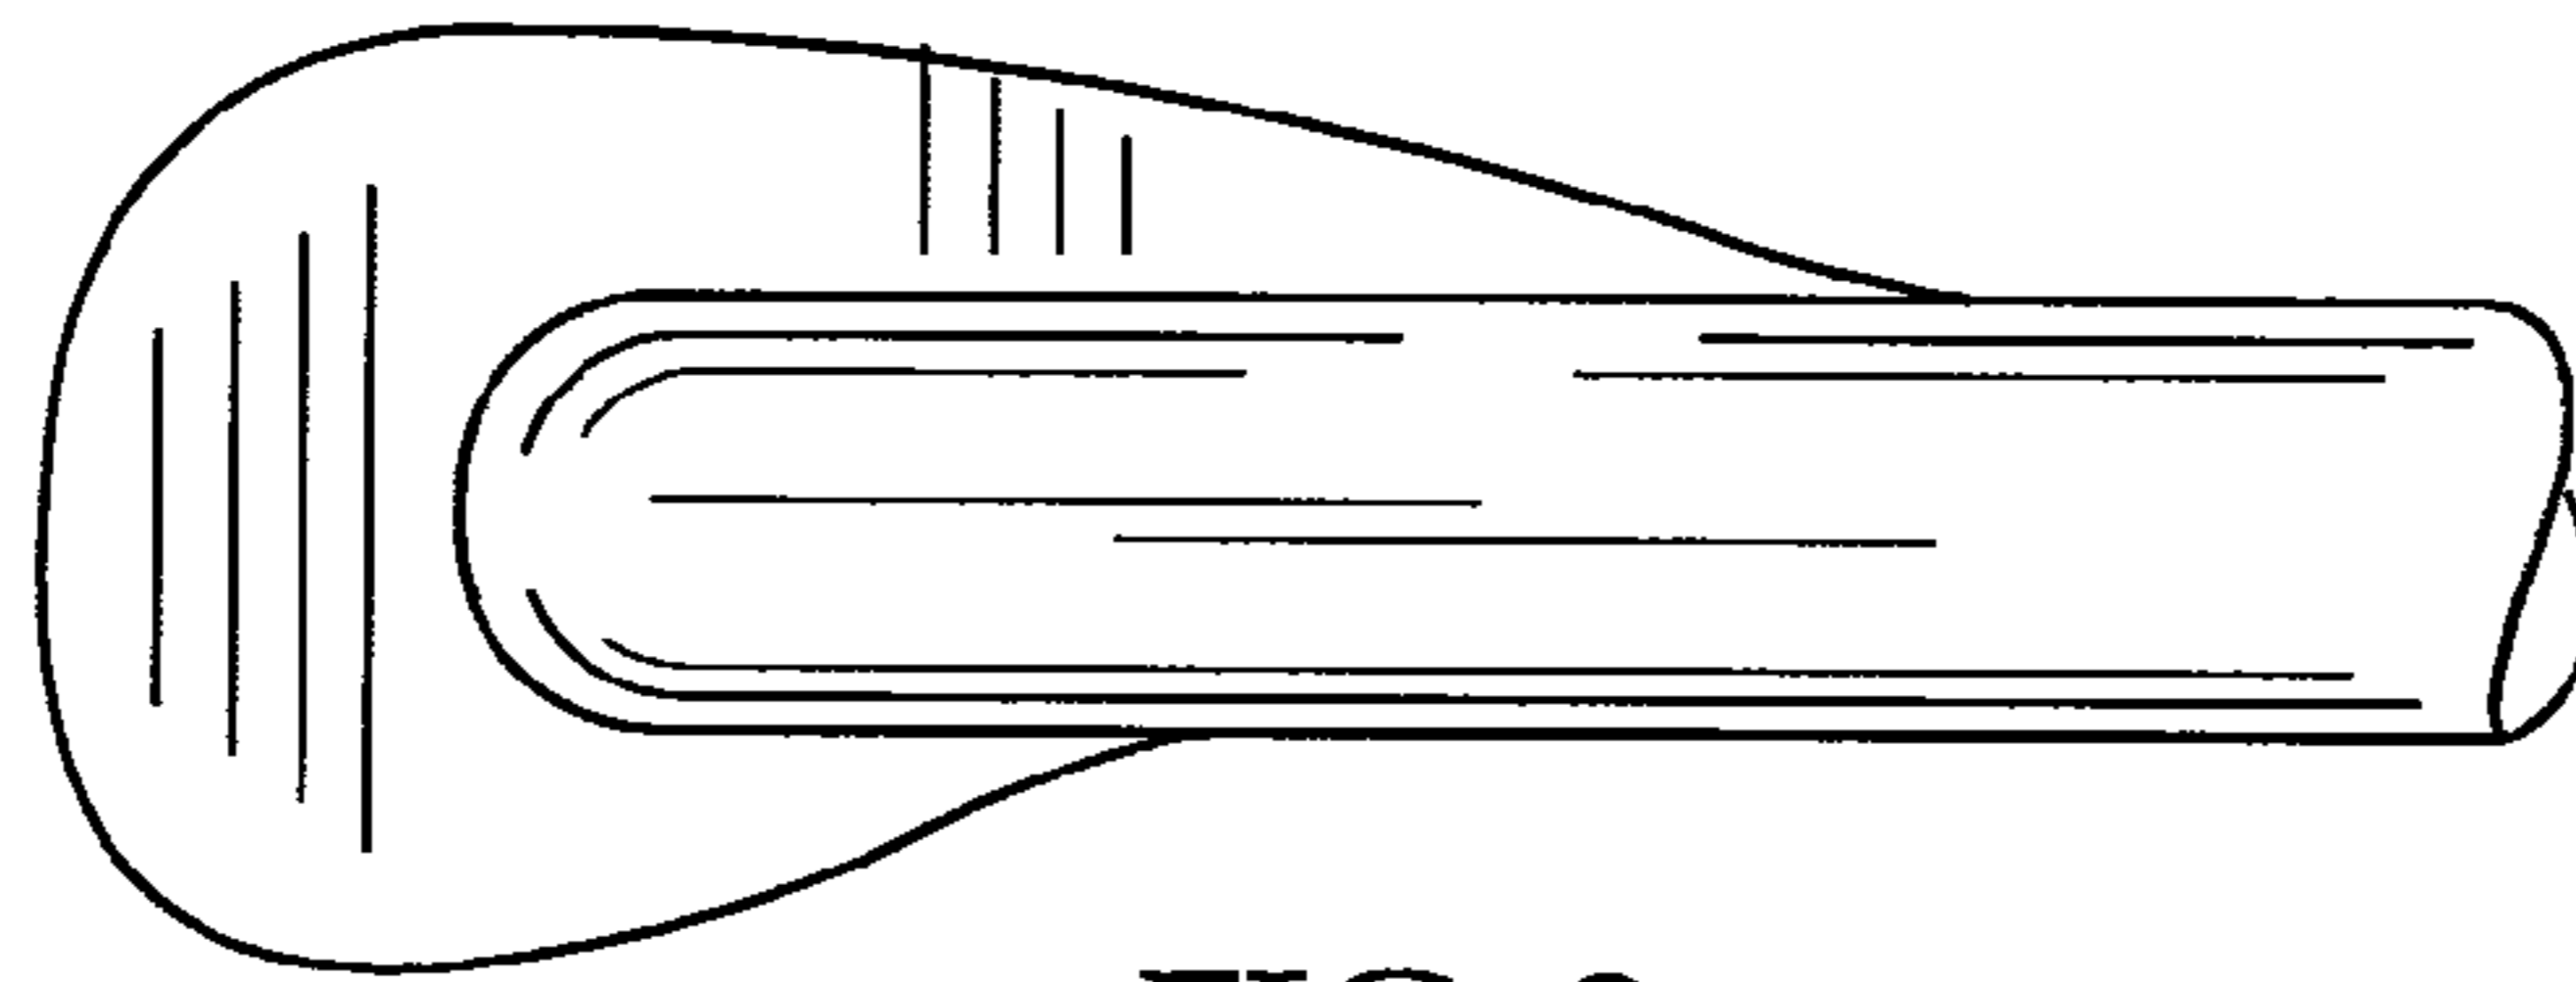


FIG. 2

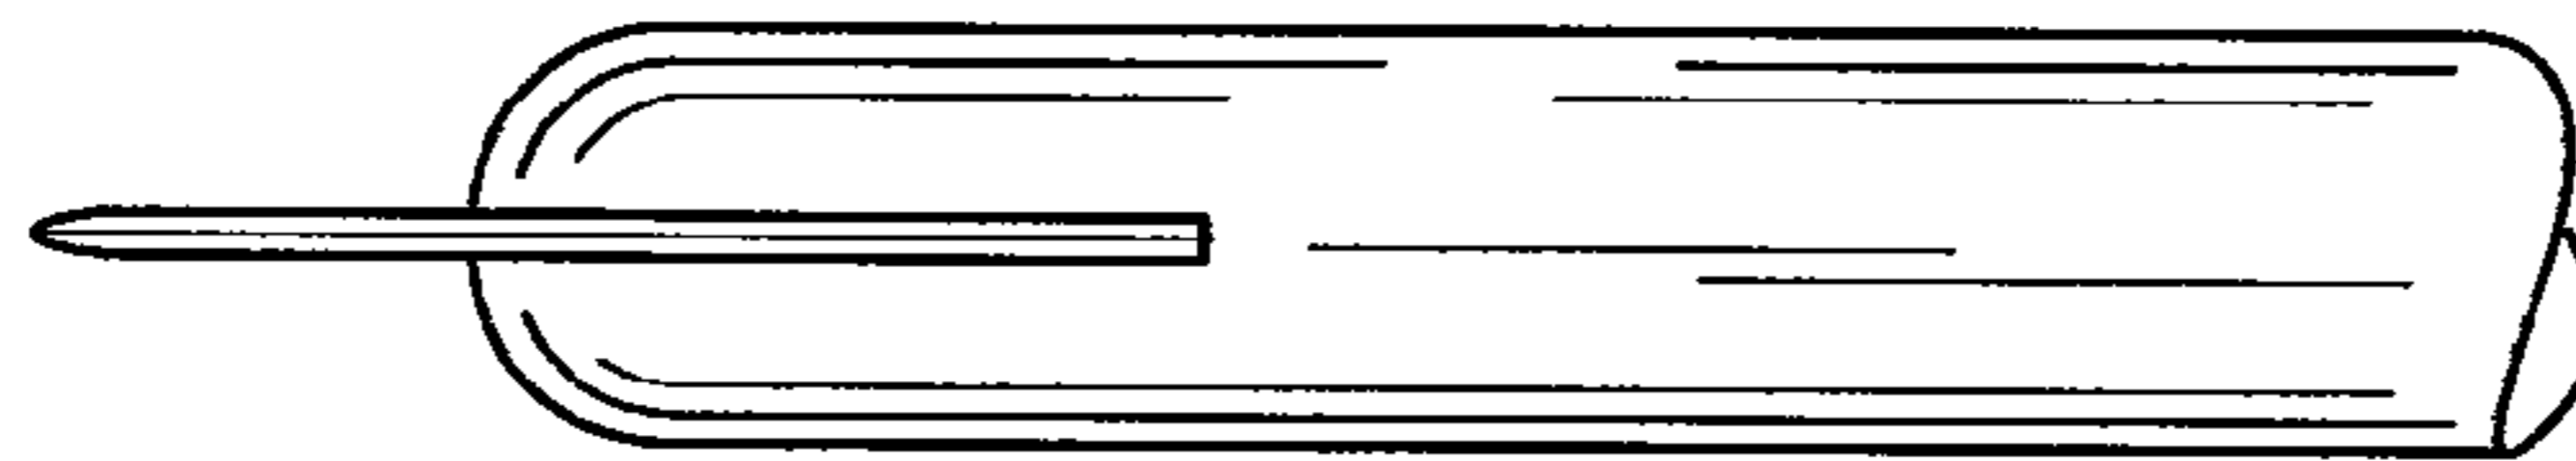


FIG. 3

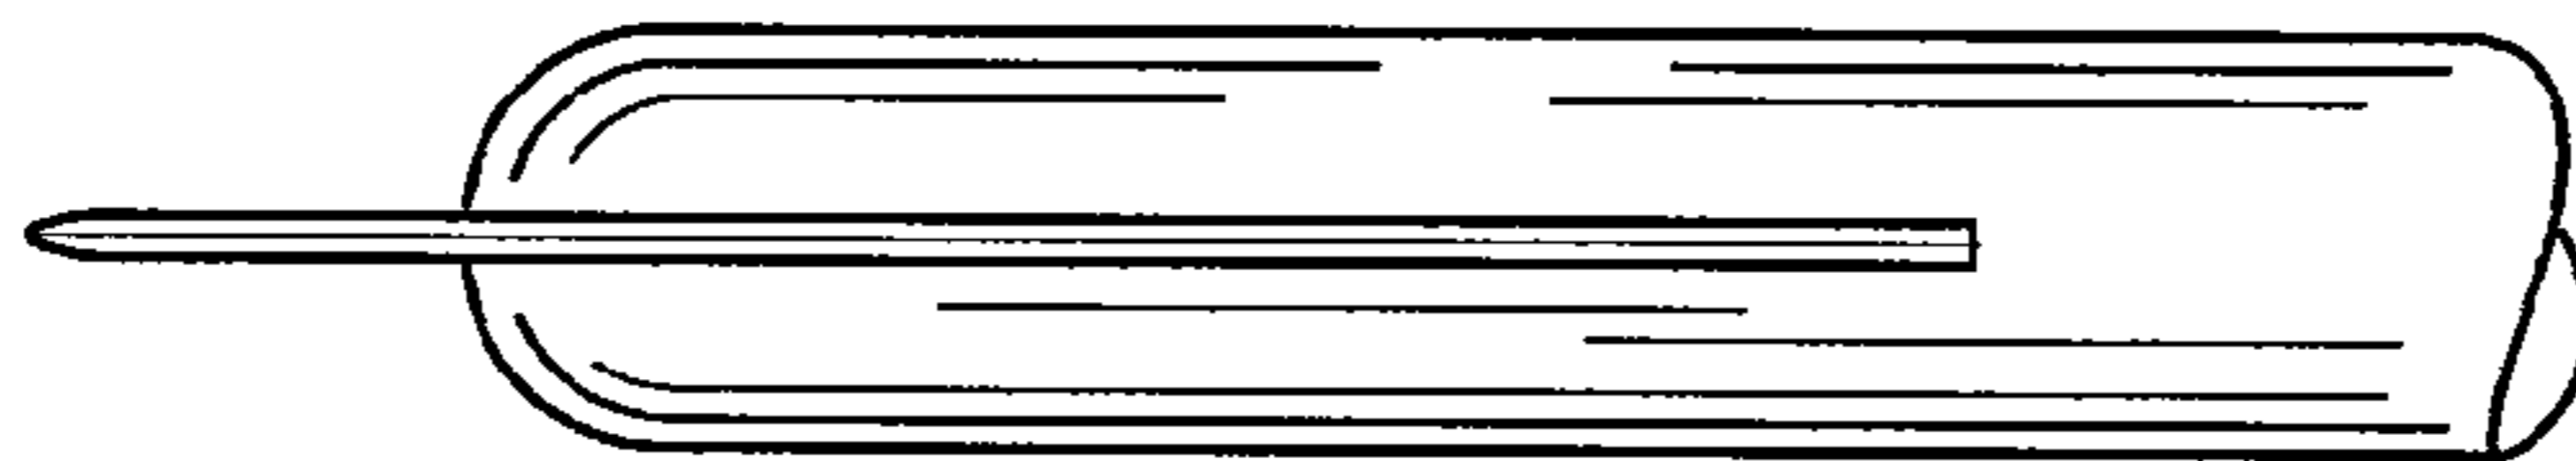


FIG. 4

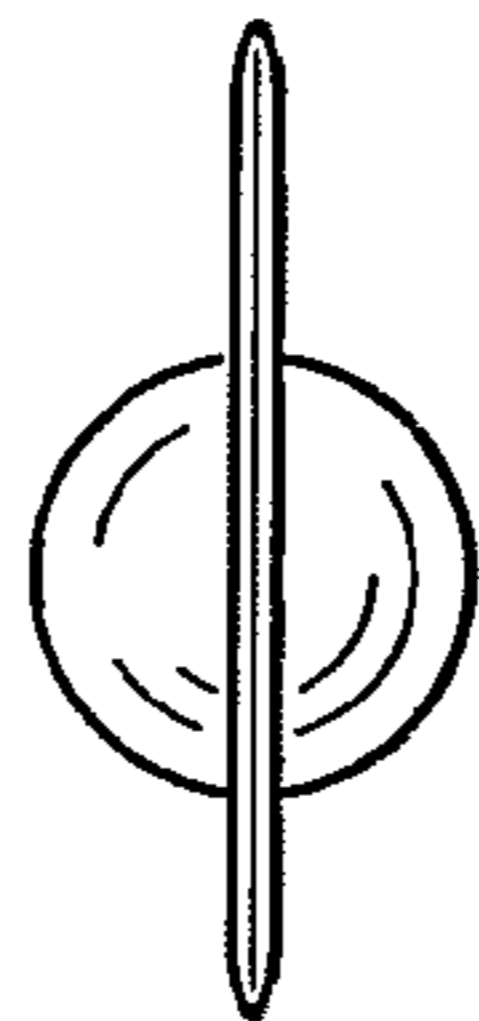


FIG. 5

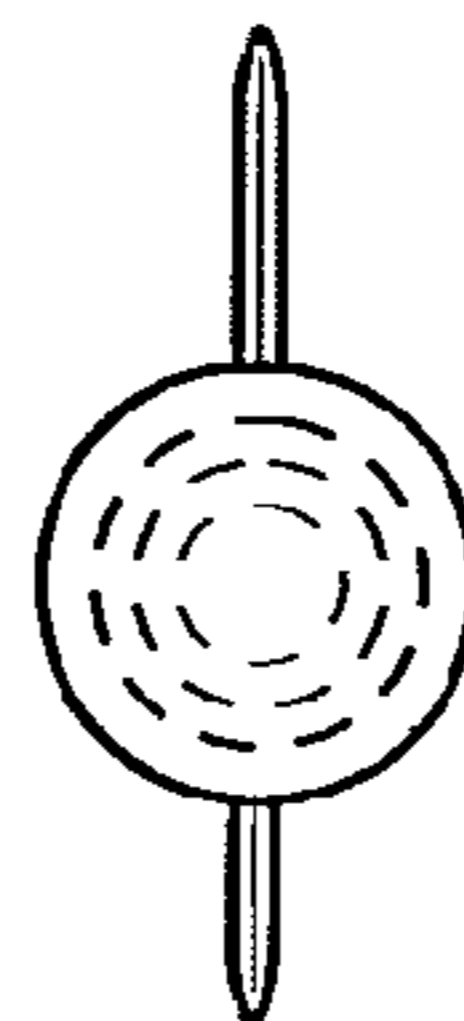


FIG. 6