

US00D702352S

(12) **United States Design Patent**
Yokoyama et al.

(10) **Patent No.:** **US D702,352 S**
(45) **Date of Patent:** **** Apr. 8, 2014**

(54) **MAGNETIC RESONANCE IMAGING APPARATUS**

(56) **References Cited**

U.S. PATENT DOCUMENTS

(71) Applicant: **Hitachi Medical Corporation**, Tokyo (JP)
(72) Inventors: **Masaru Yokoyama**, Tokyo (JP); **Atsushi Ninomiya**, Tokyo (JP); **Shin Hoshino**, Tokyo (JP); **Satoshi Yamashita**, Tokyo (JP); **Takeshi Yatsuo**, Tokyo (JP)

D564,096	S	*	3/2008	Banryu		D24/158
D625,416	S	*	10/2010	Kasai et al.		D24/158
D659,248	S	*	5/2012	Ramos		D24/159
D678,527	S	*	3/2013	Boninger		D24/158
D681,207	S	*	4/2013	Ninomiya et al.		D24/158
D681,815	S	*	5/2013	Ninomiya et al.		D24/158

* cited by examiner

(73) Assignee: **Hitachi Medical Corporation**, Tokyo (JP)

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Antonelli, Terry, Stout & Kraus, LLP.

(**) Term: **14 Years**

(57) **CLAIM**

(21) Appl. No.: **29/454,730**

We claim the ornamental design for a magnetic resonance imaging apparatus, as shown.

(22) Filed: **May 14, 2013**

DESCRIPTION

(30) **Foreign Application Priority Data**

Nov. 16, 2012 (JP) 2012-027984

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/158**

(58) **Field of Classification Search**
USPC D24/158-161, 185, 186; 378/4, 15, 17, 378/20, 21, 23-27, 62, 68, 146, 195-198, 378/57; 600/410, 421, 422

See application file for complete search history.

FIG. 1 is a front, top and right side perspective view of a magnetic resonance imaging apparatus showing our new design;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear side elevational view thereof;


FIG. 4 is a left side elevational view thereof;

FIG. 5 is a right side elevational view thereof;

FIG. 6 is a top plan view thereof; and,

FIG. 7 is a bottom plan view thereof.

1 Claim, 7 Drawing Sheets

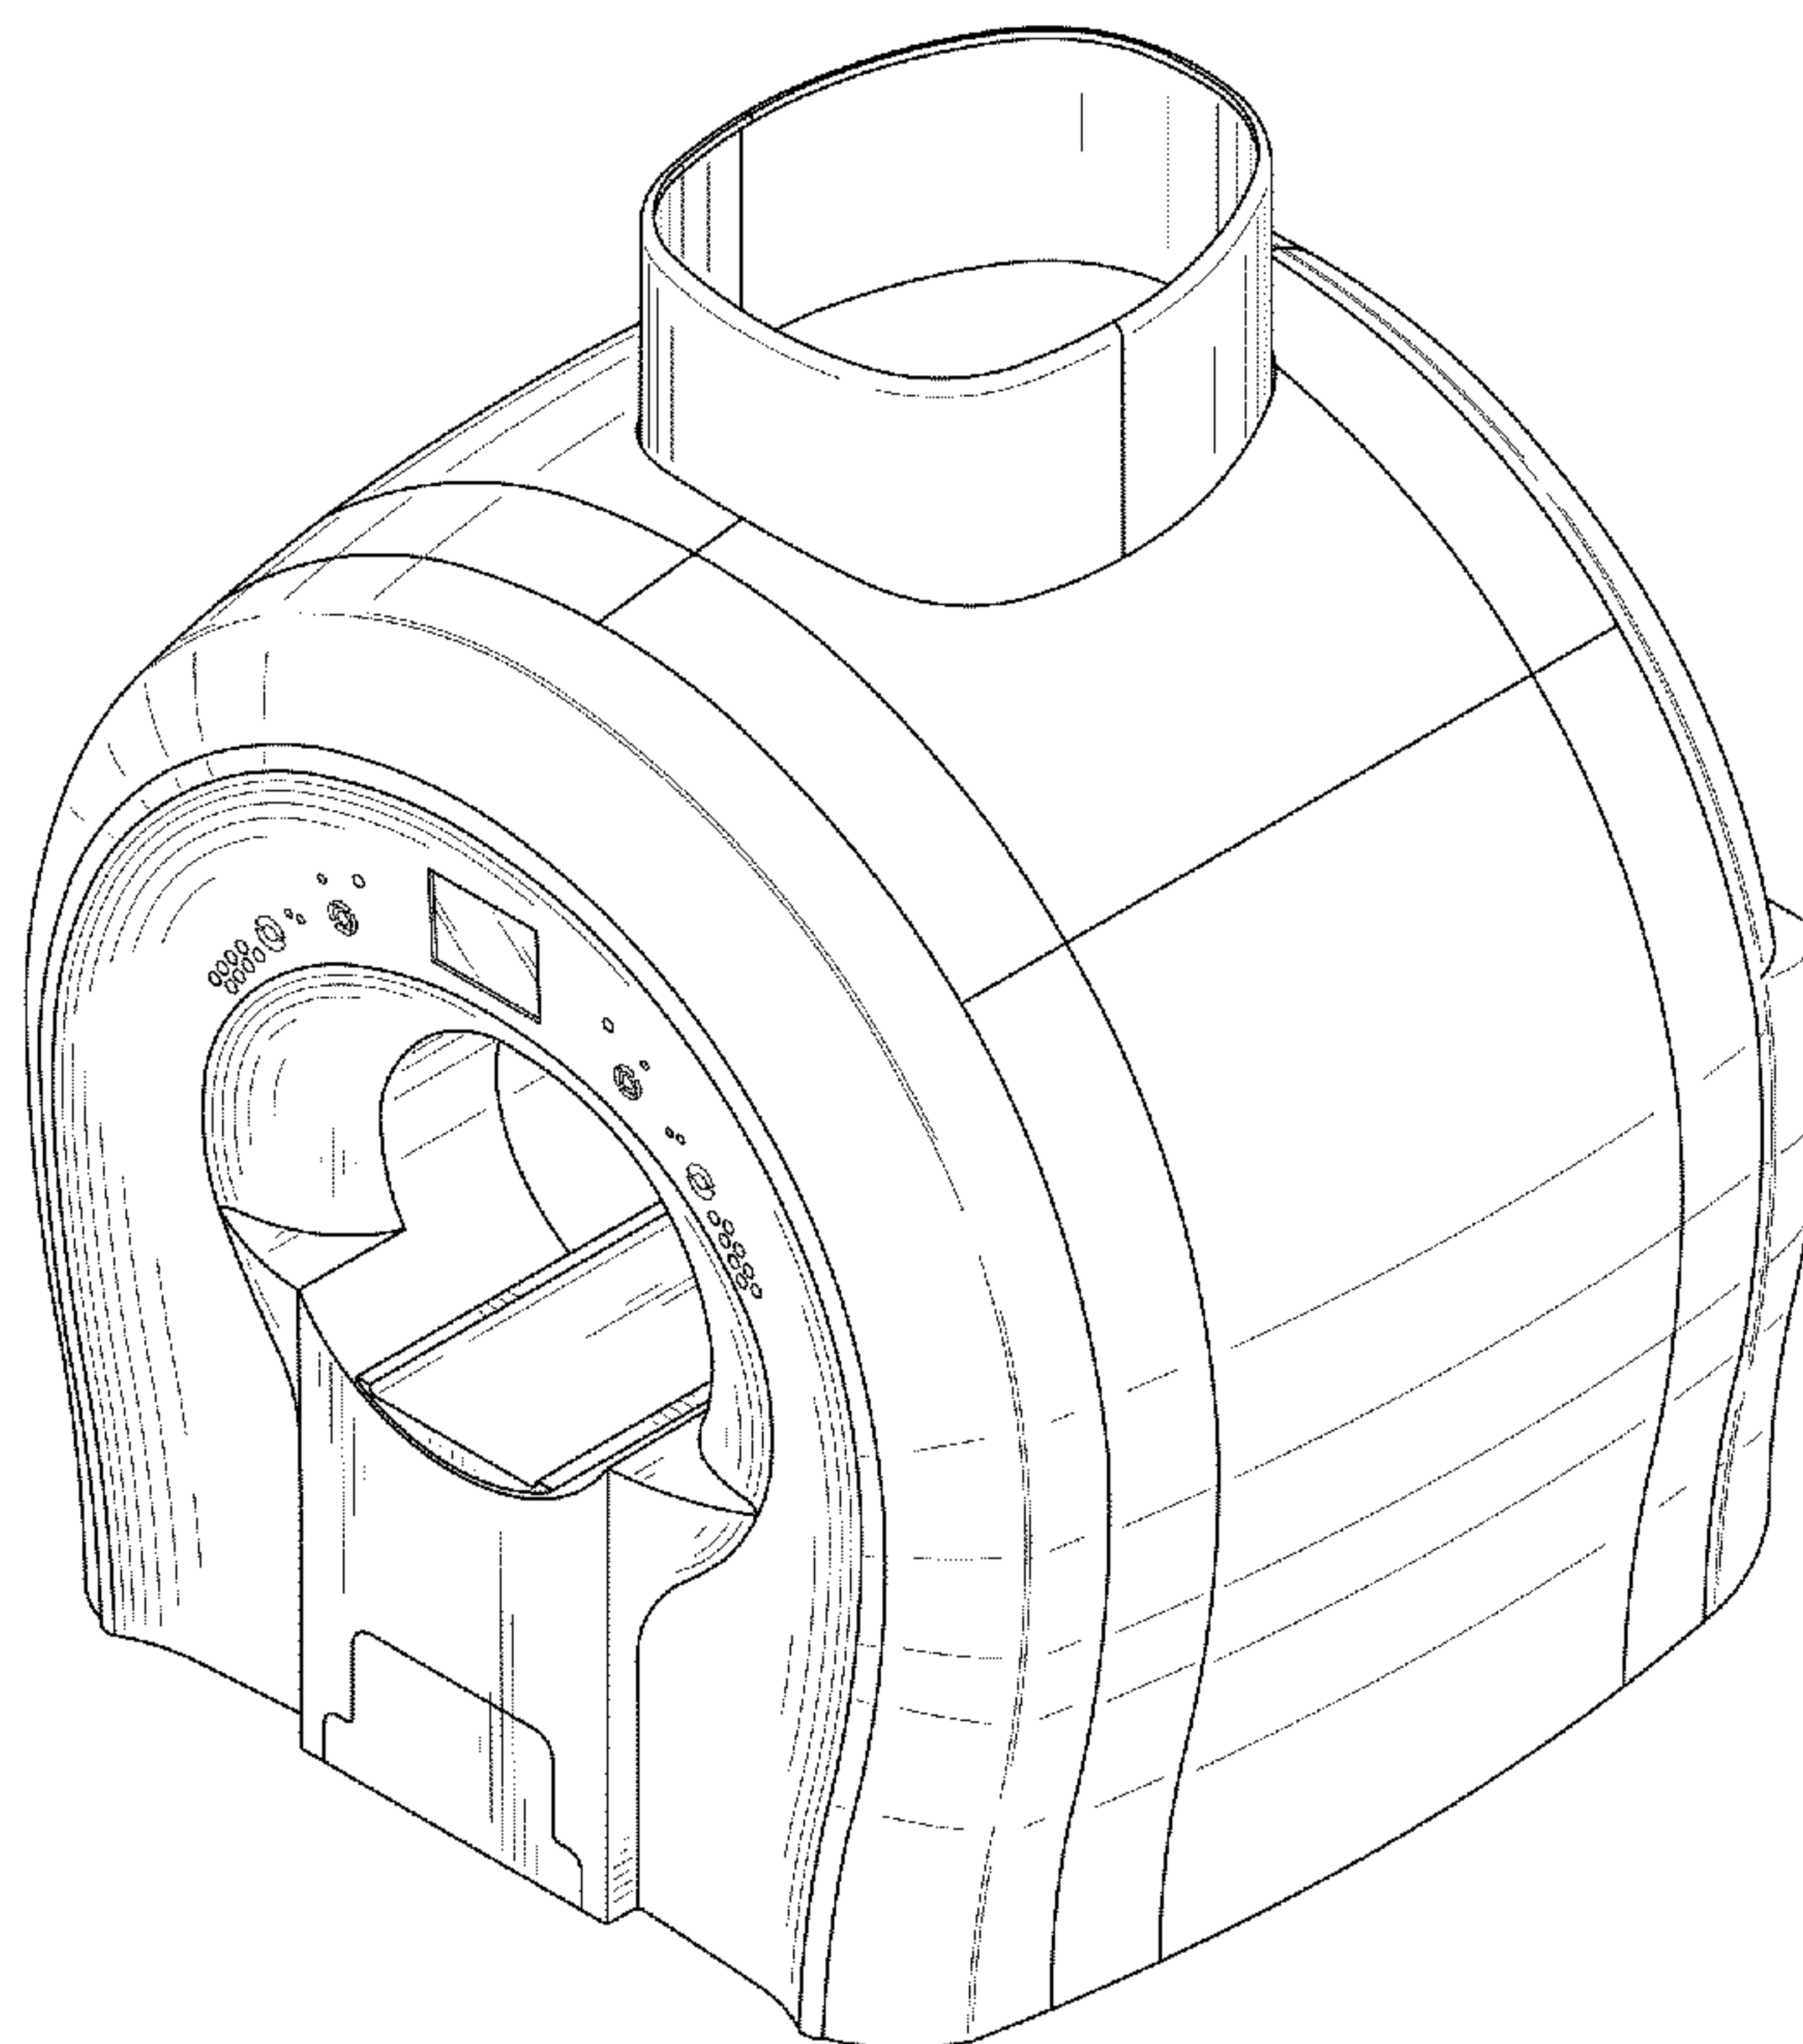

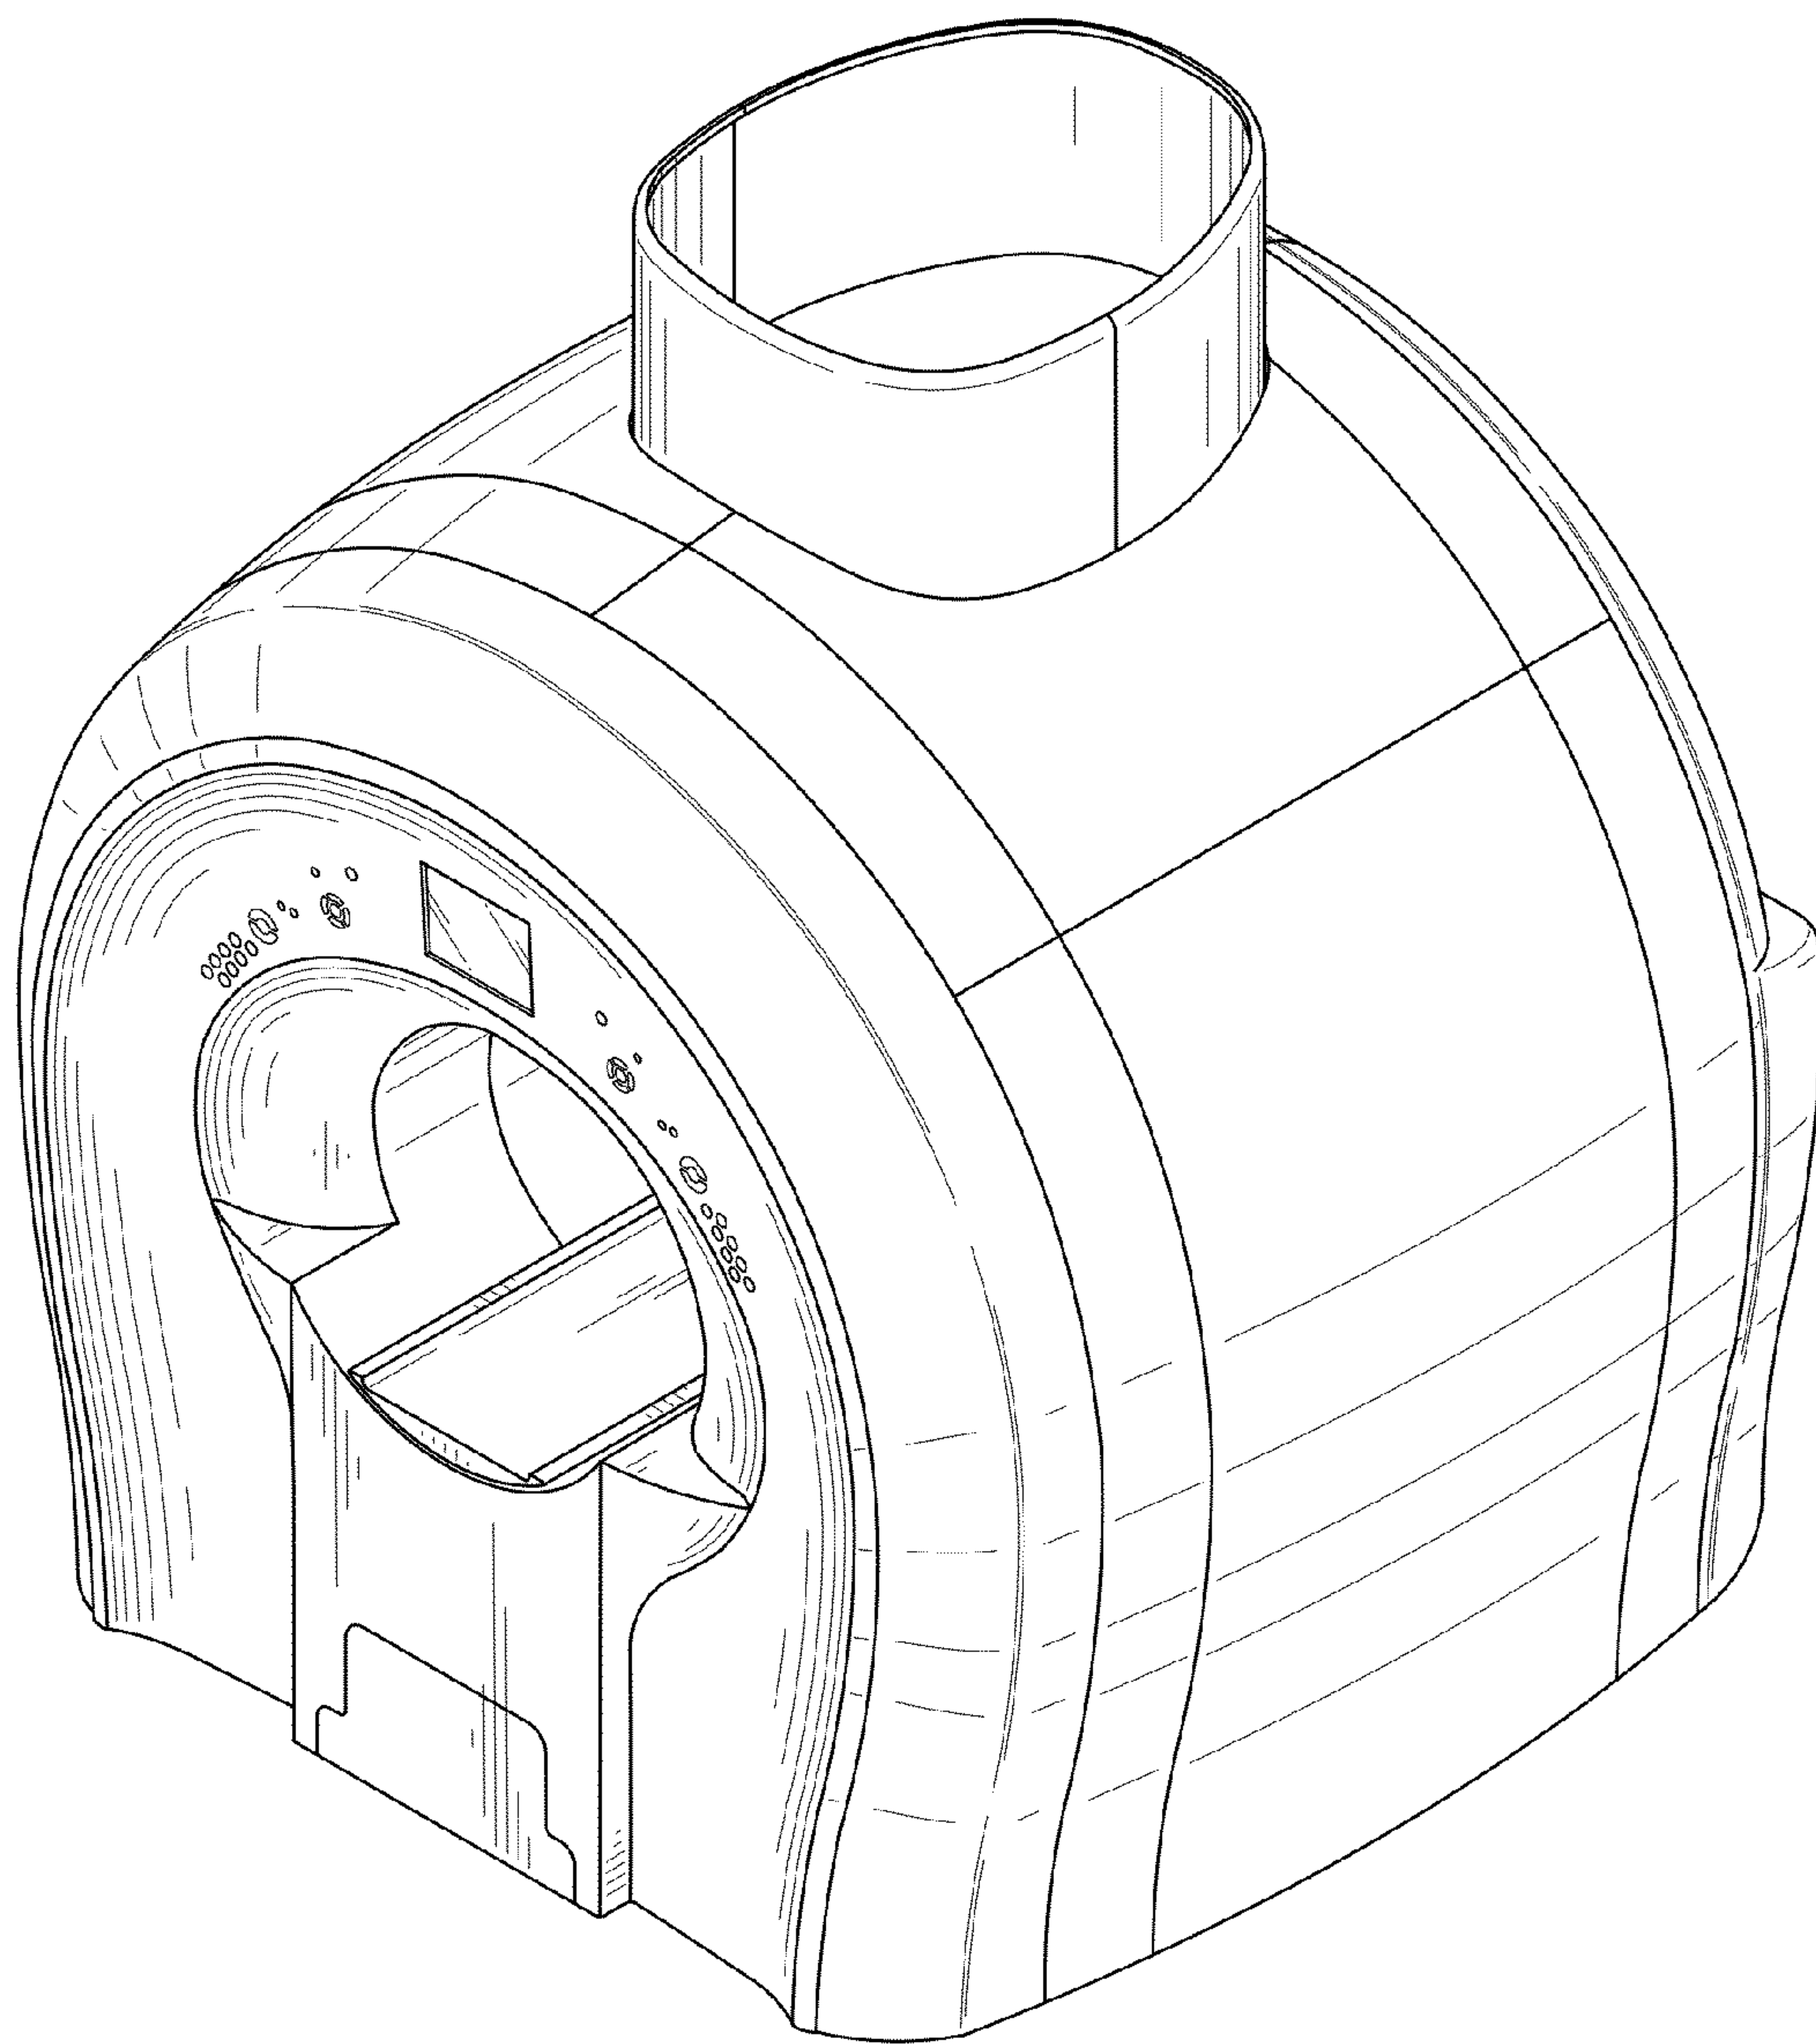


FIG. 1

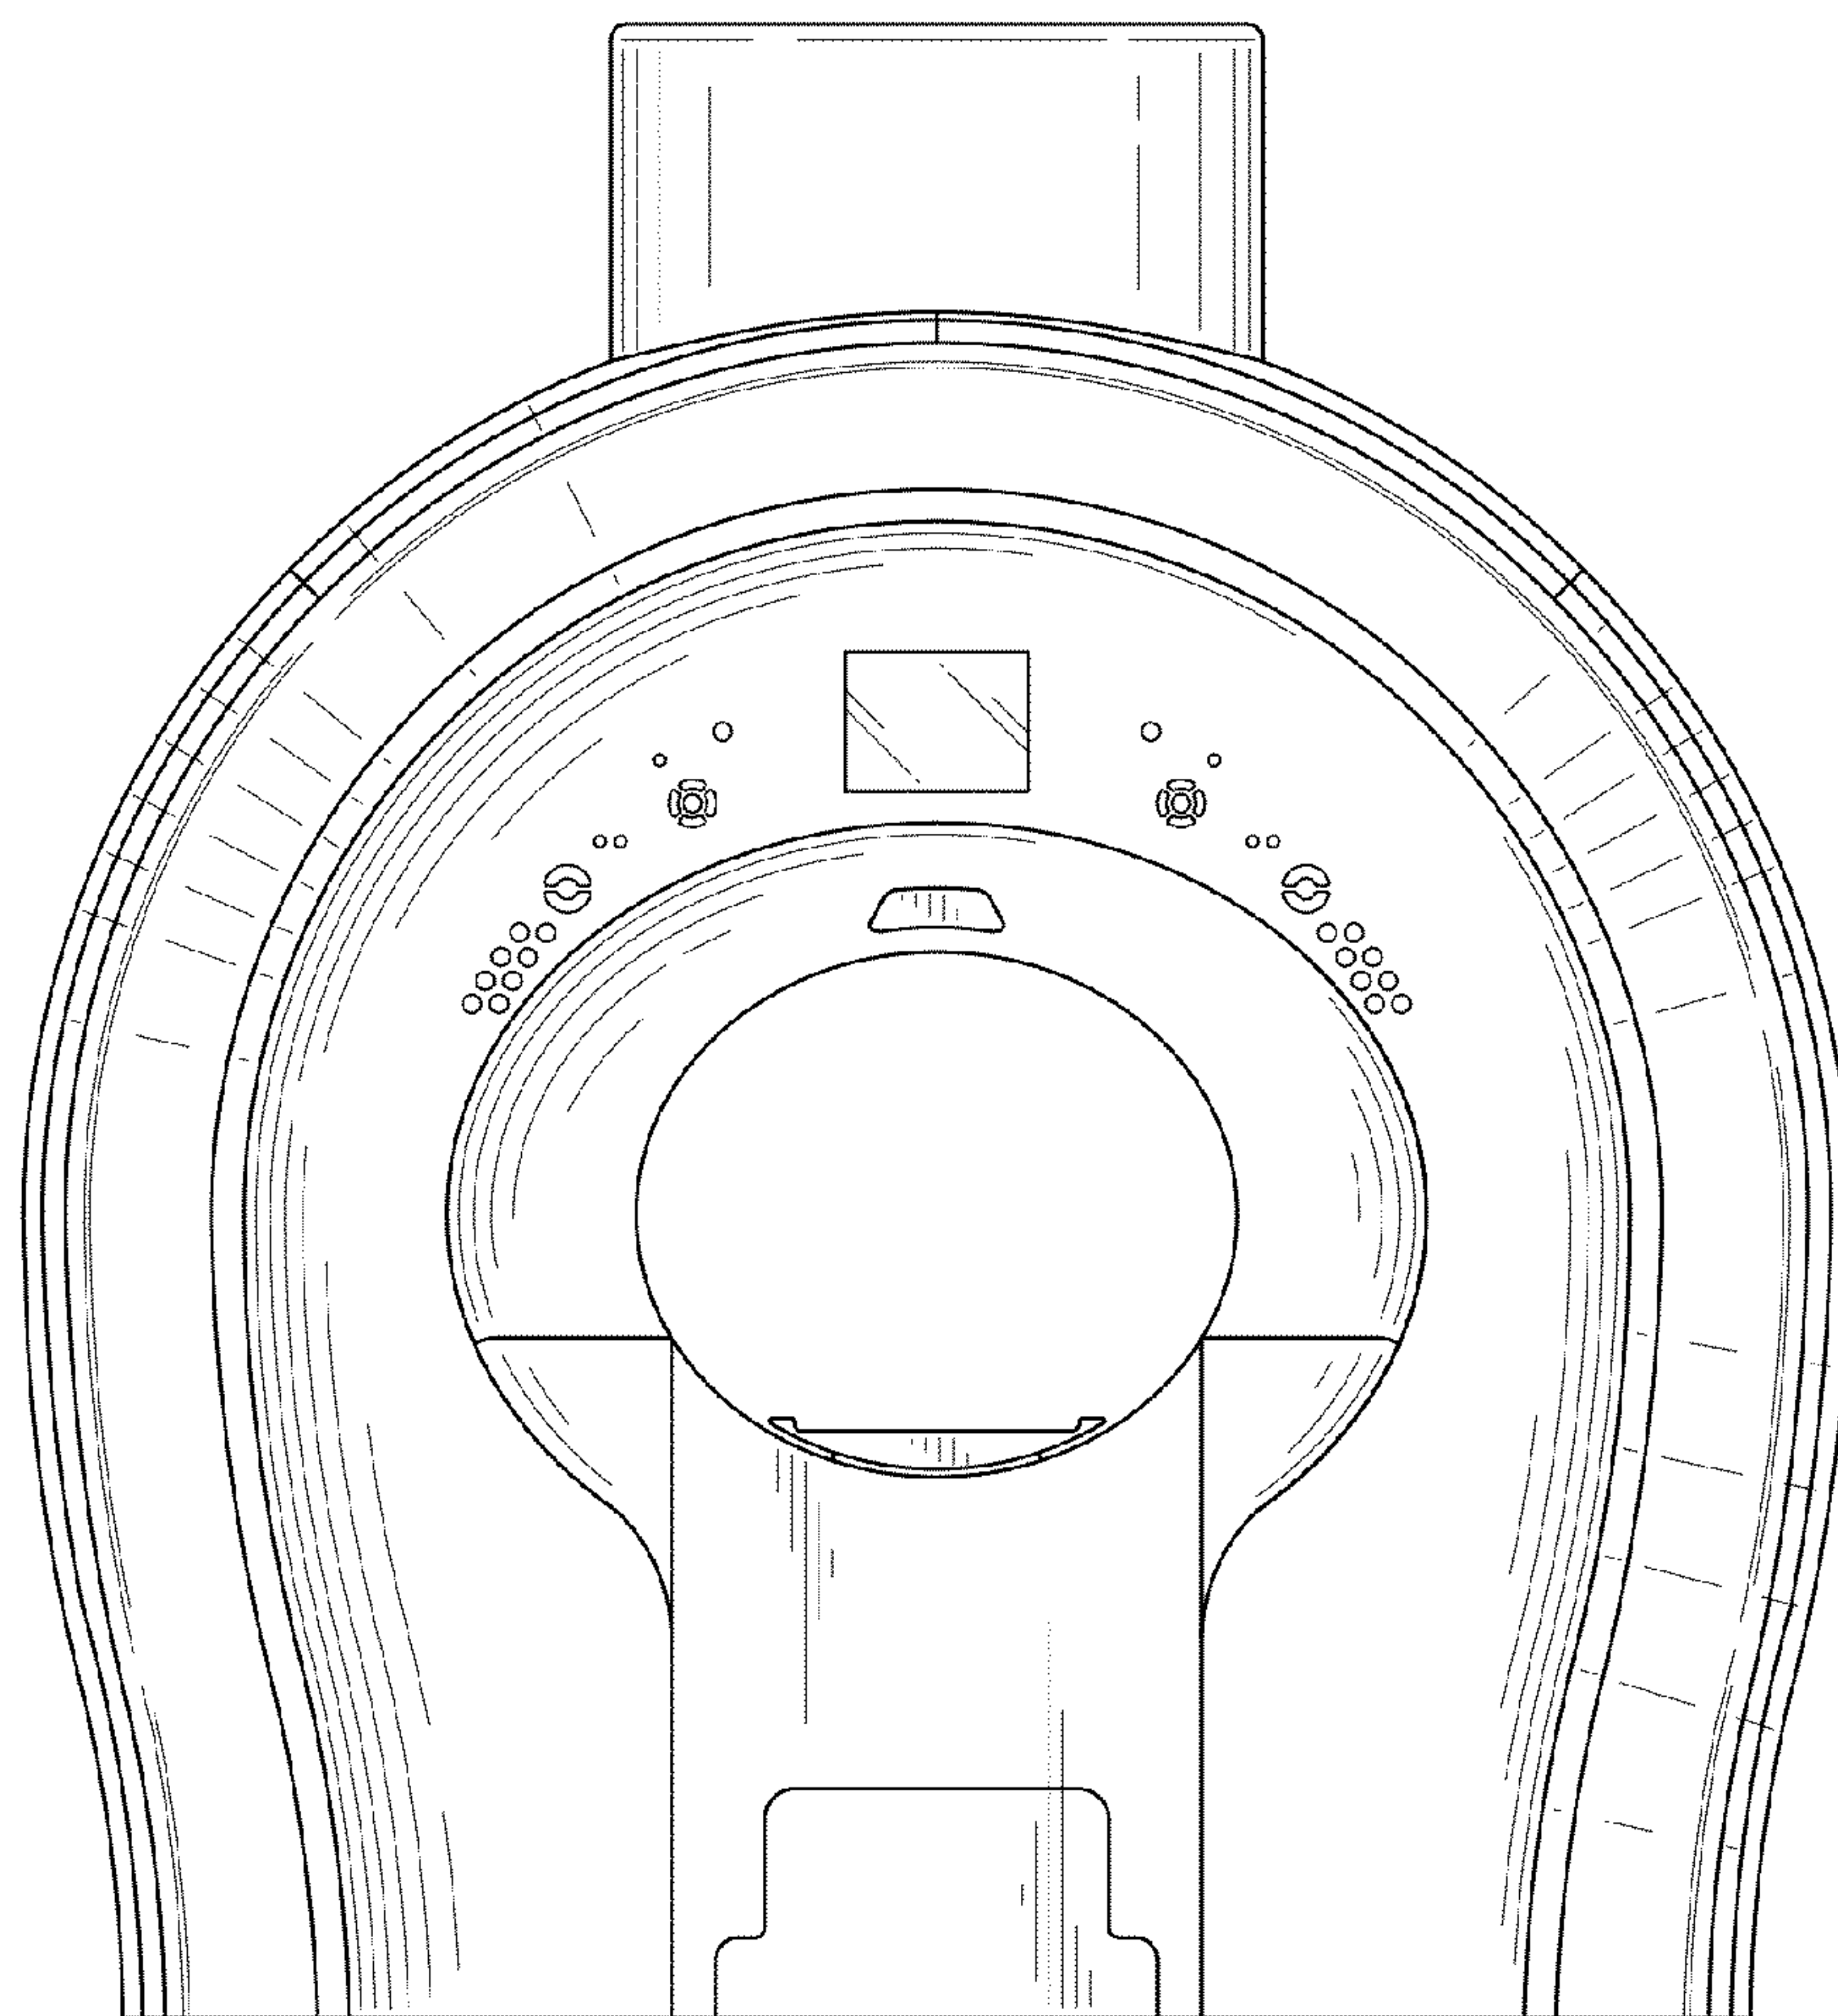


FIG. 2

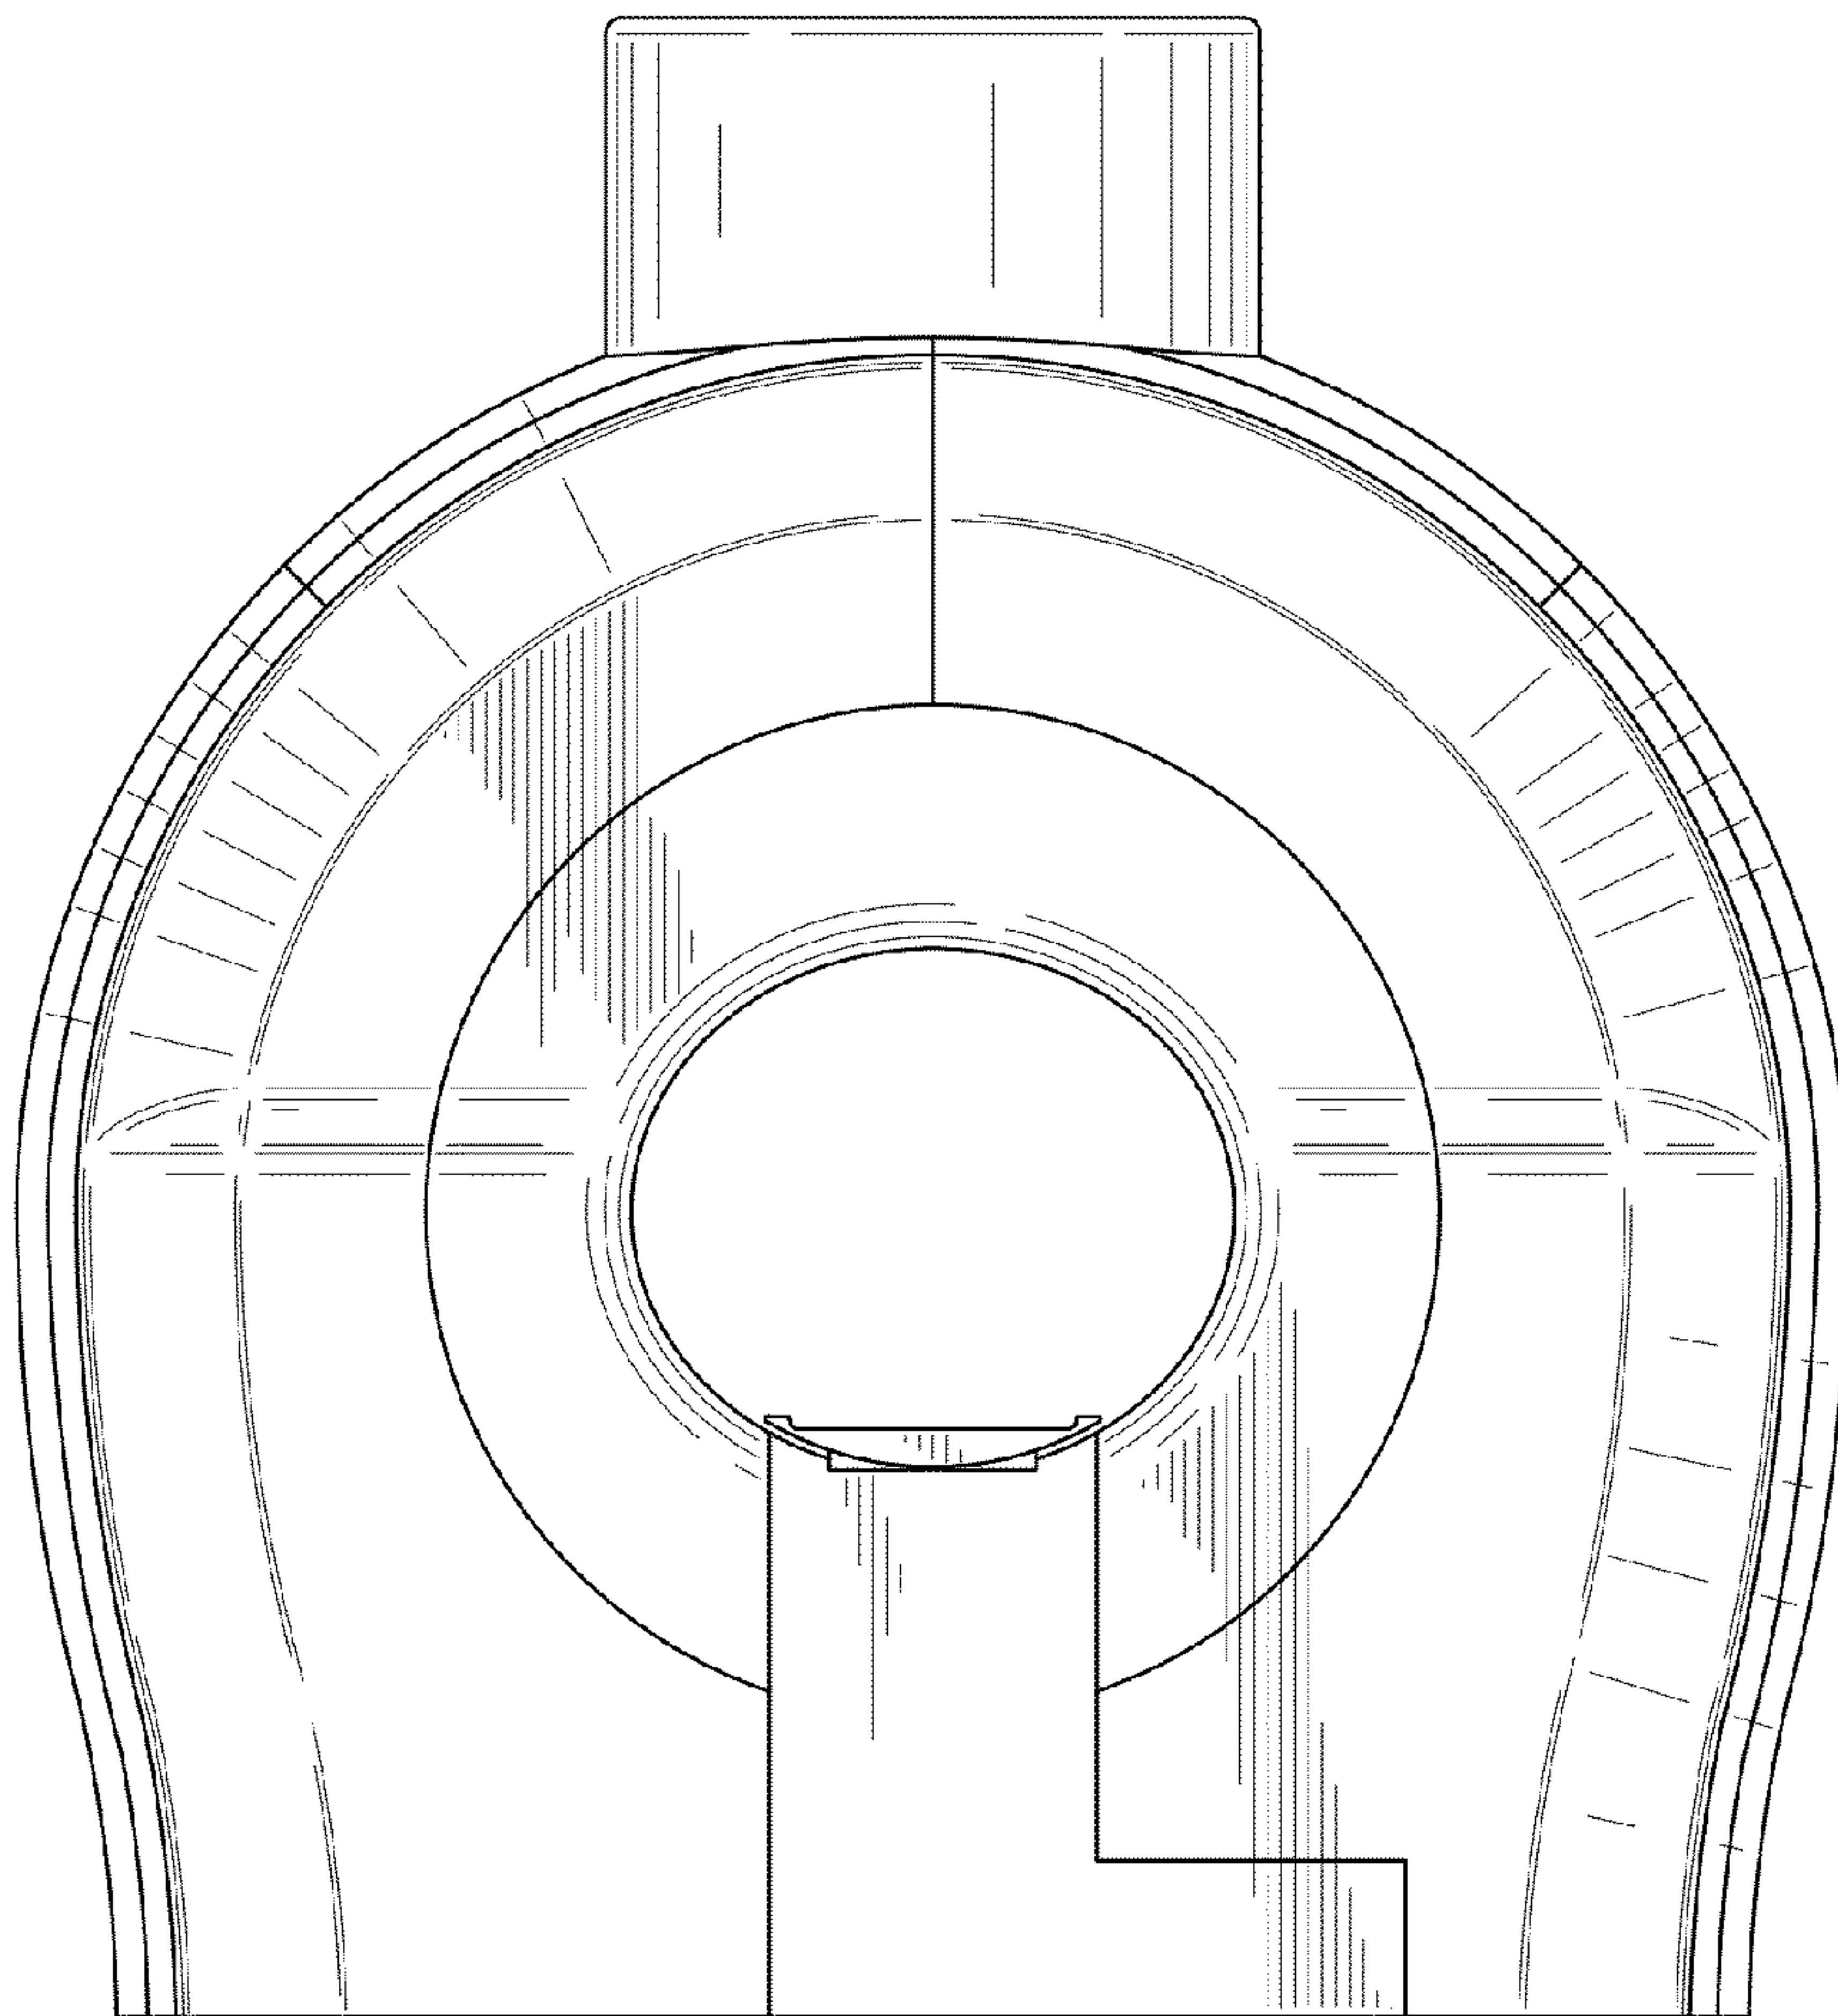


FIG. 3

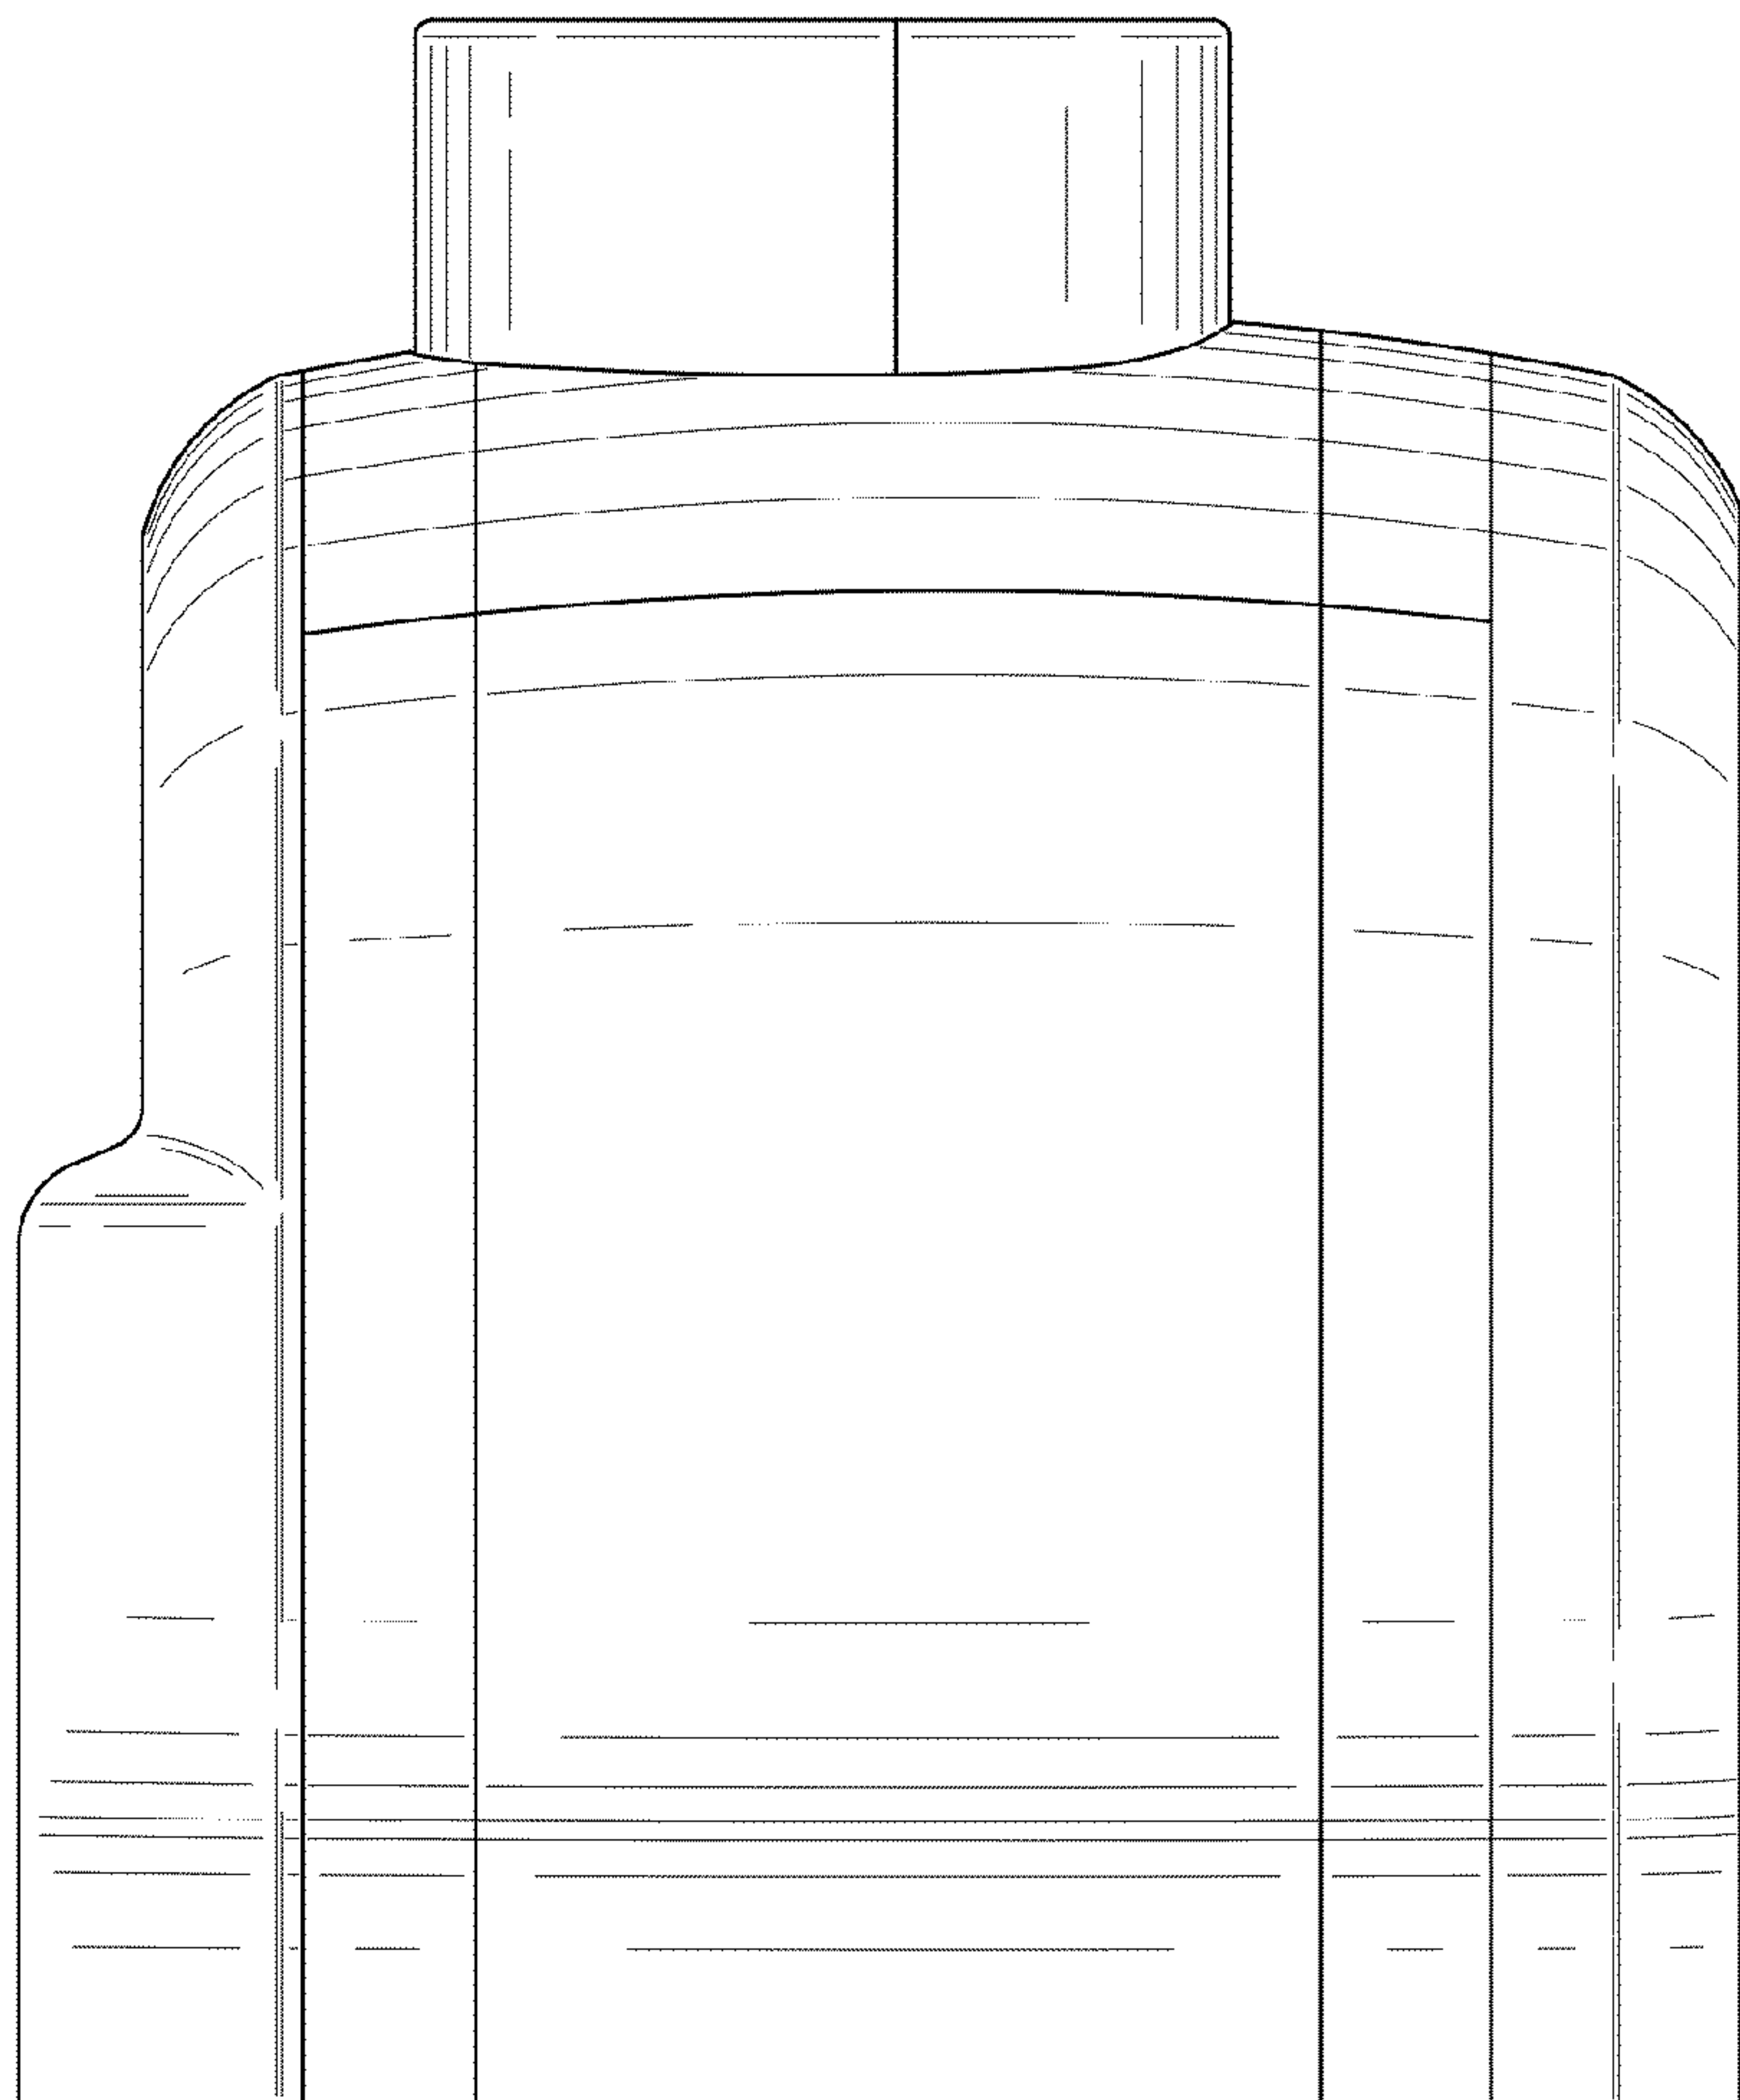


FIG. 4

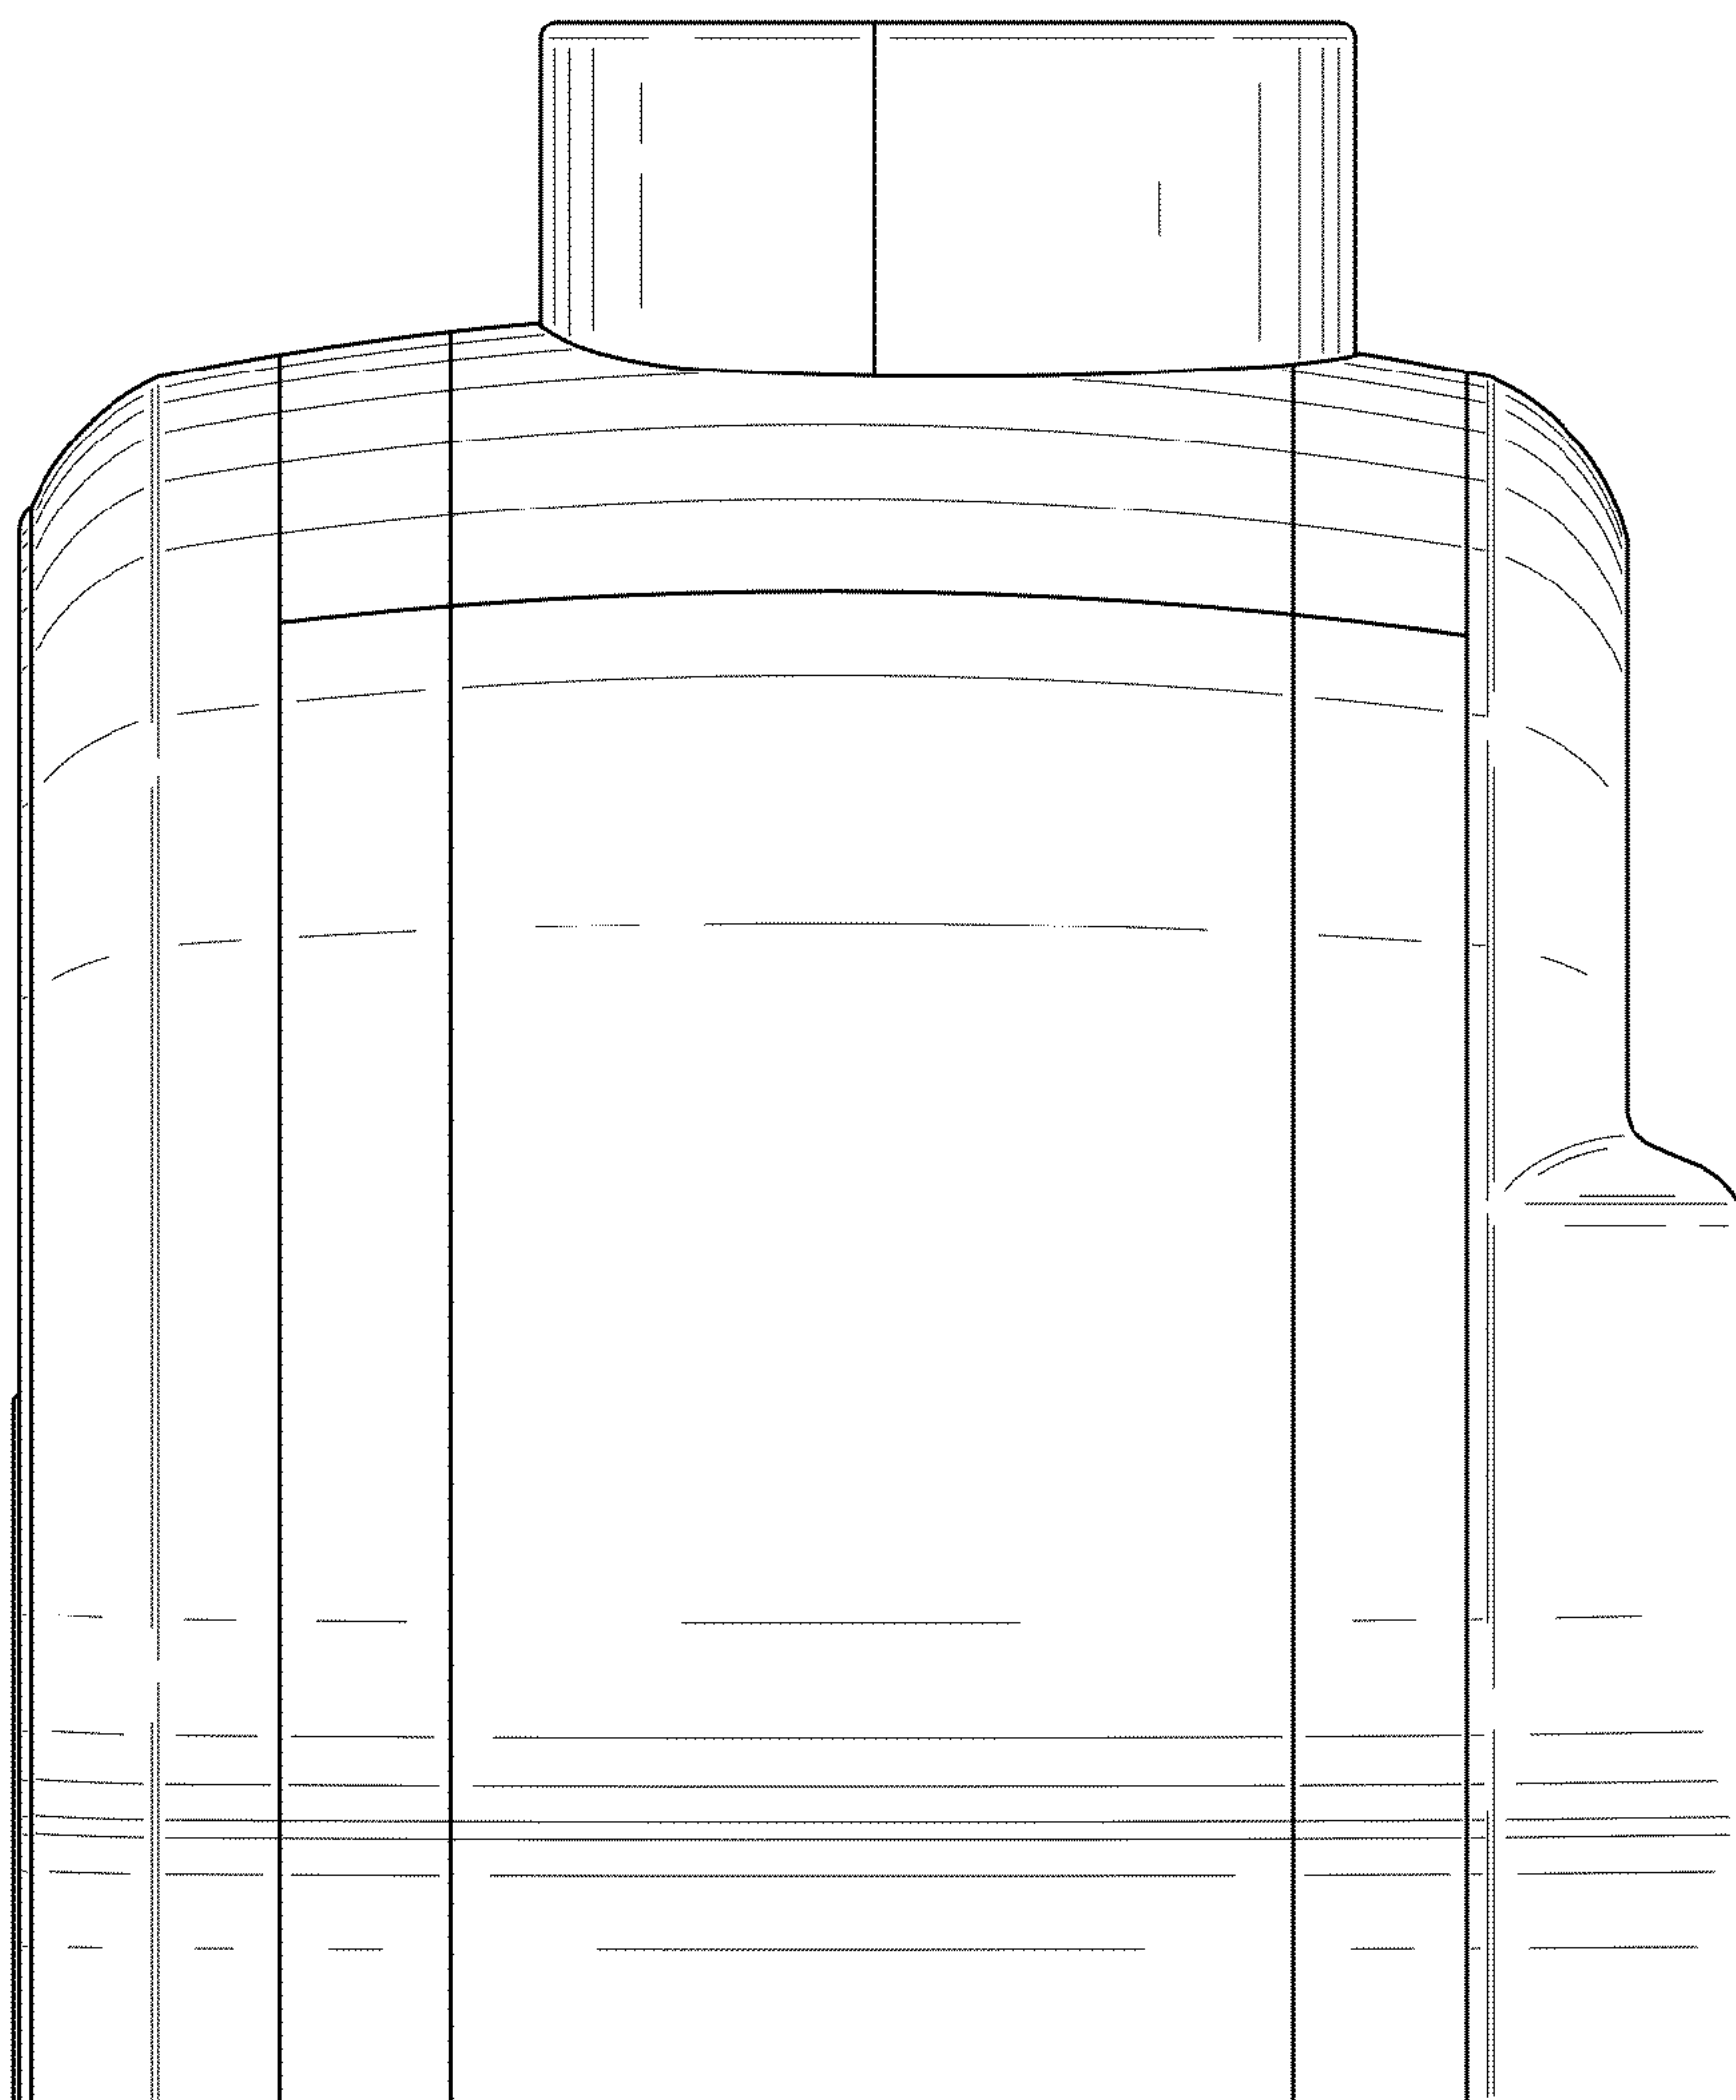


FIG. 5

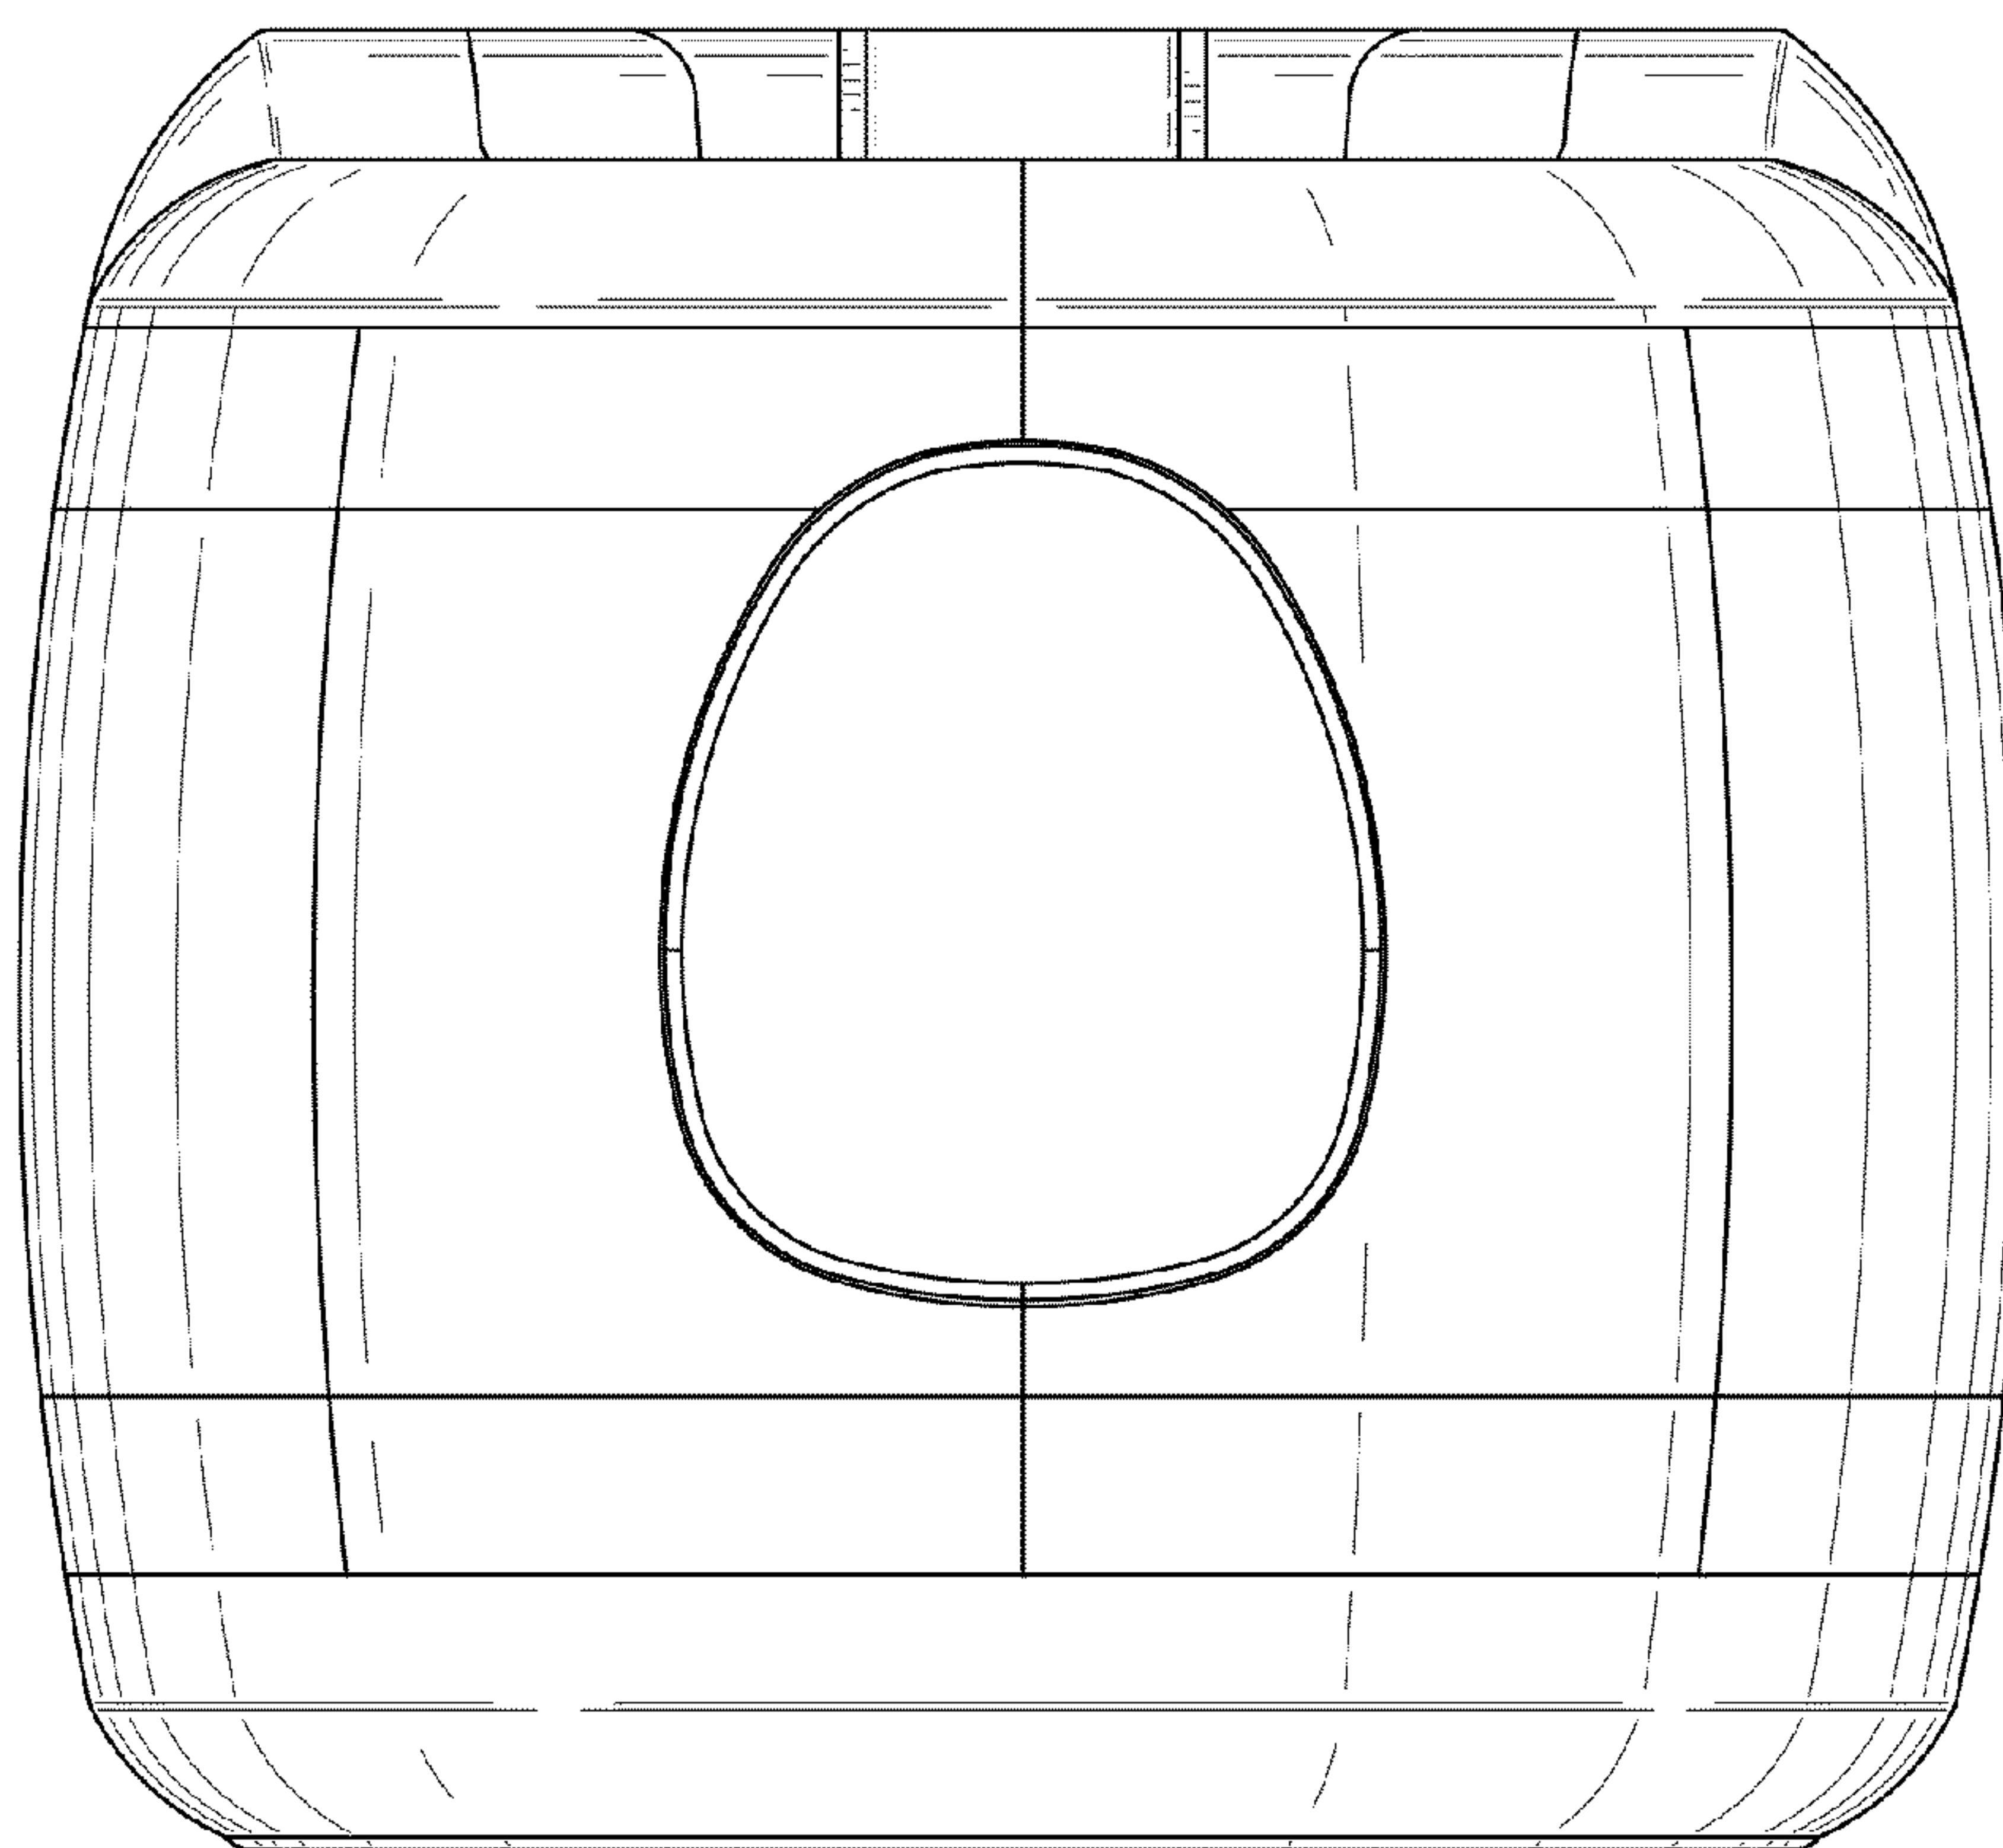


FIG. 6

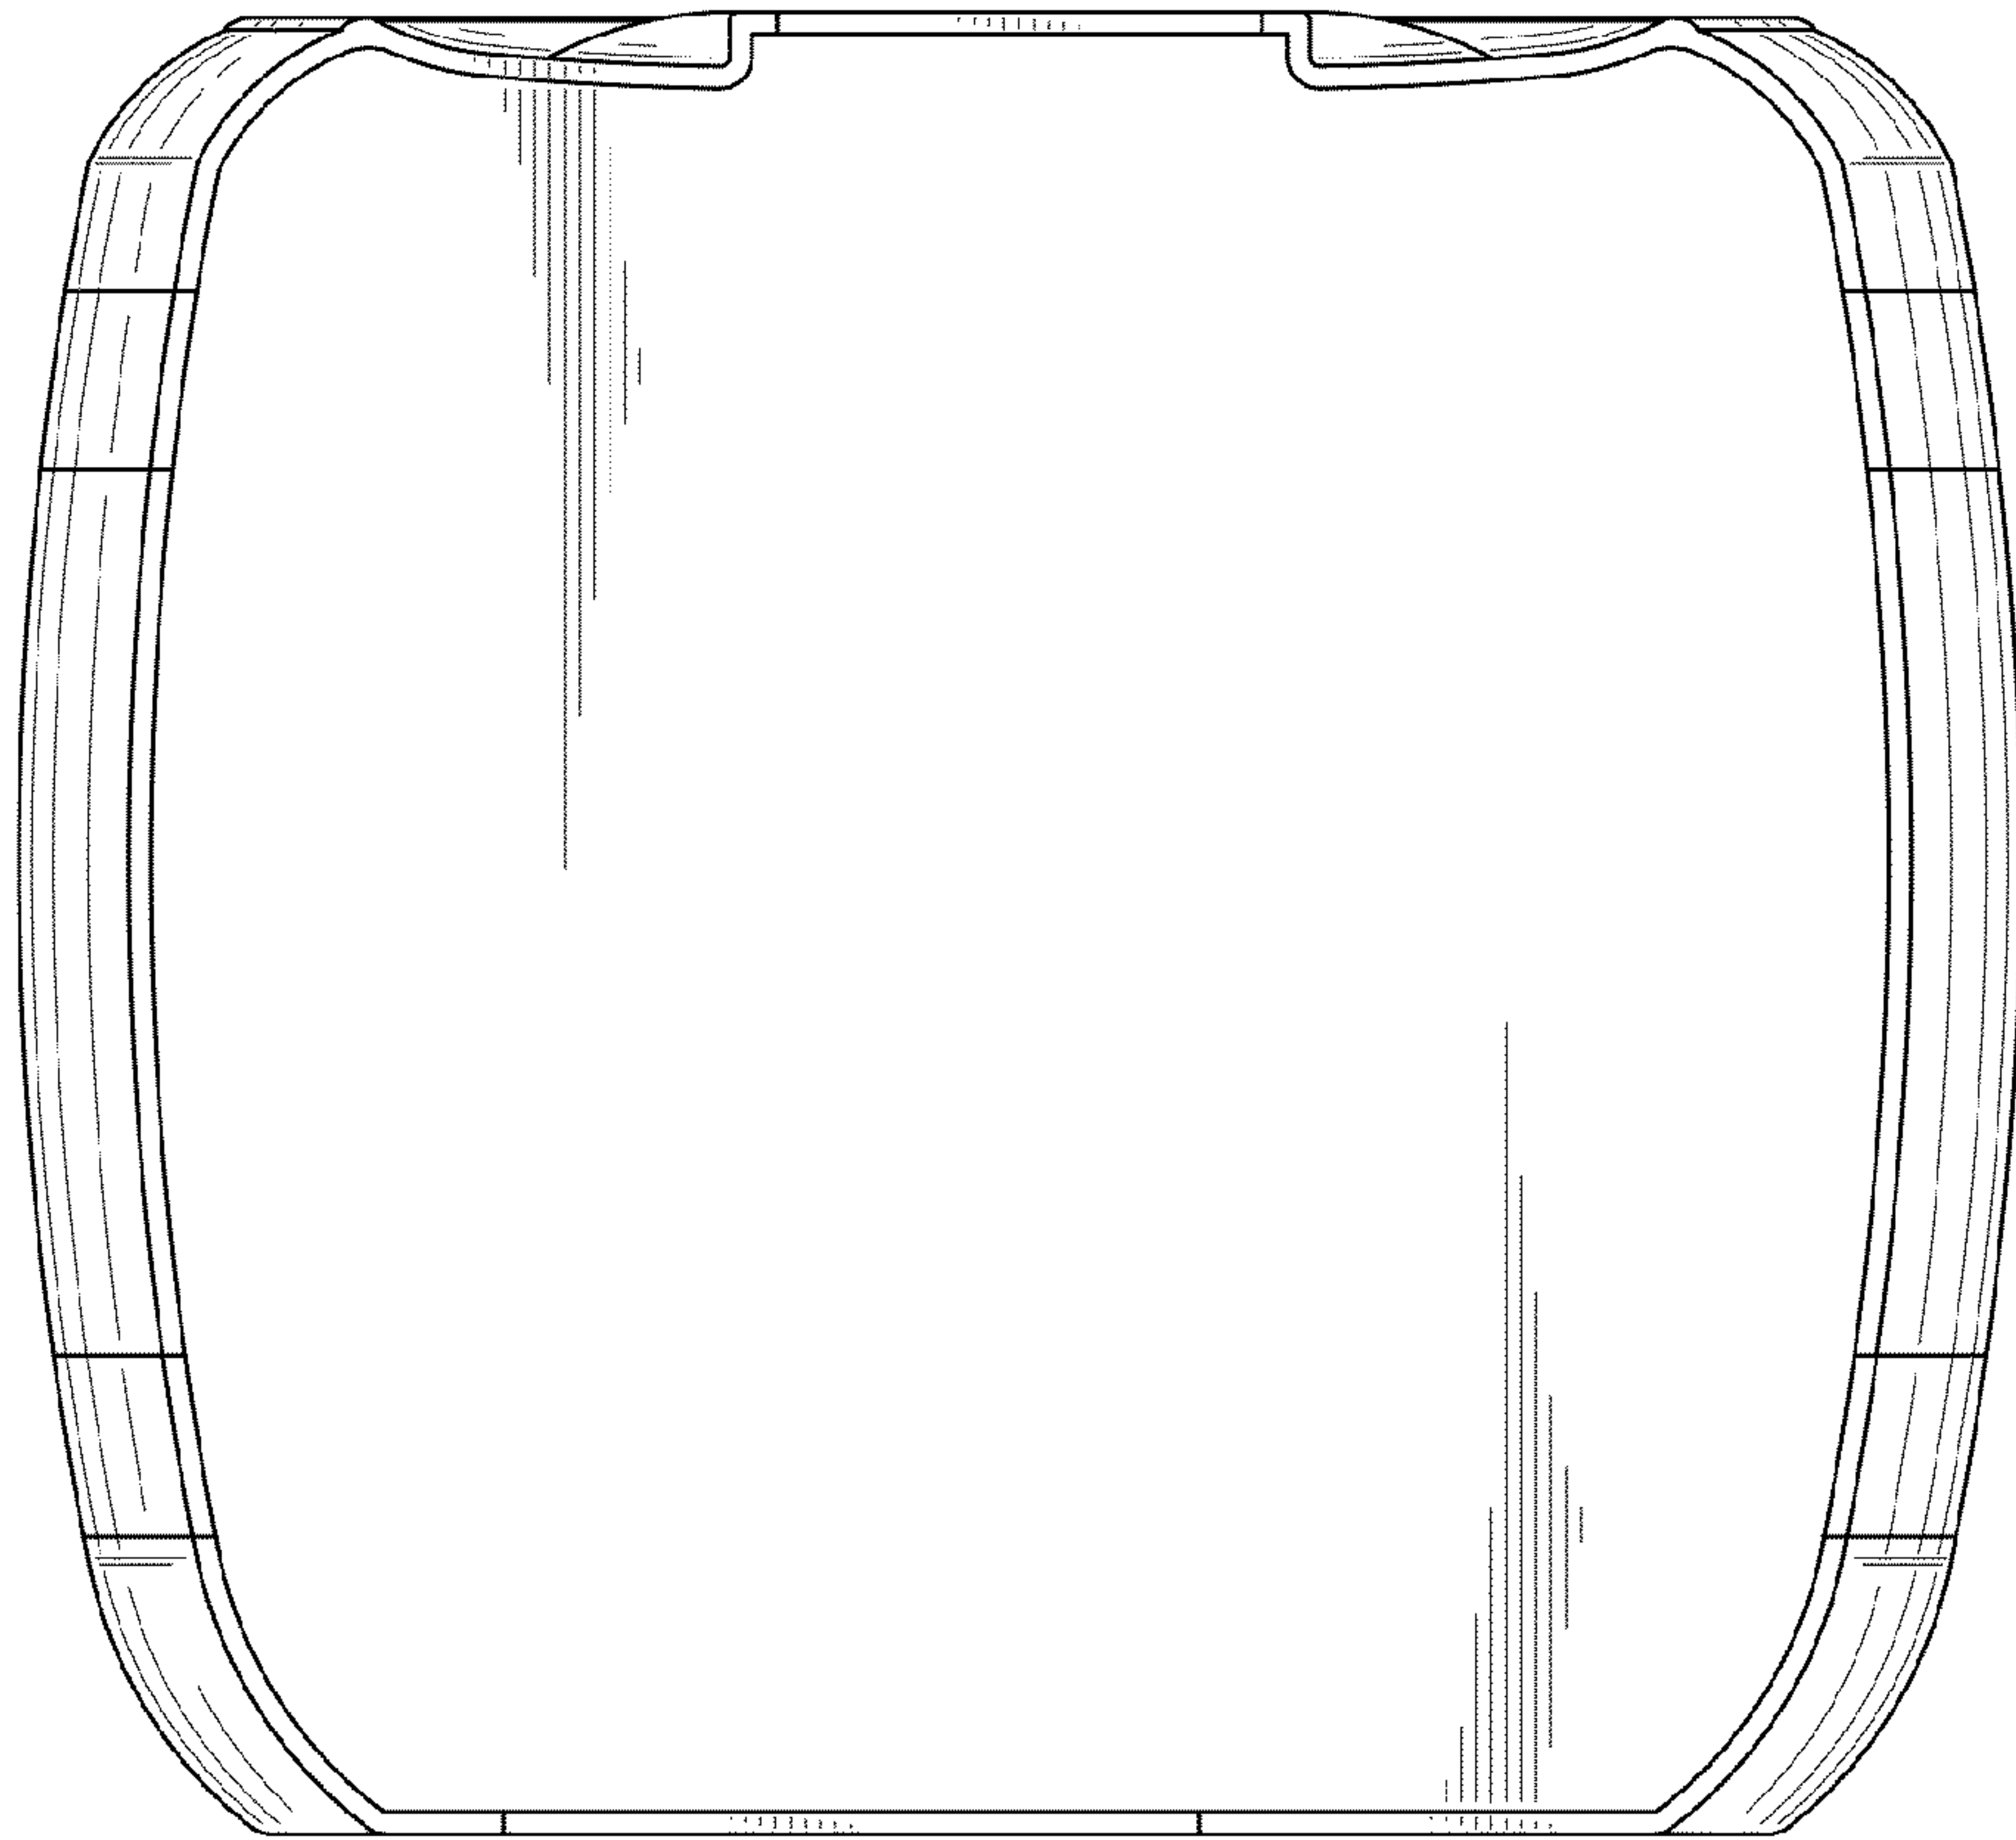


FIG. 7