



US00D702842S

(12) **United States Design Patent**  
**Hyde et al.**

(10) **Patent No.:** **US D702,842 S**

(45) **Date of Patent:** **\*\* Apr. 15, 2014**

(54) **PORTABLE MEDICAL UNIT**

(75) Inventors: **Aidan Hyde**, Manhattan, NY (US);  
**Nicholas E. Barker**, Laguna Beach, CA  
(US)

(73) Assignee: **MAQUET Cardiovascular LLC**,  
Wayne, NJ (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/389,514**

(22) Filed: **Apr. 12, 2011**

(51) **LOC (10) Cl.** ..... **24-00**

(52) **U.S. Cl.**  
USPC ..... **D24/185**

(58) **Field of Classification Search**  
USPC ..... D24/143, 170, 164, 171, 172, 185, 234,  
D24/221, 190, 186, 183, 188, 150; 606/54,  
606/56, 57, 59  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D387,168 S *	12/1997	Edelman et al. ....	D24/186
D467,001 S *	12/2002	Buczek et al. ....	D24/172
D477,082 S *	7/2003	Bromley ..... D24/170	
6,616,598 B2	9/2003	Kaushansky et al.	
D486,915 S	2/2004	Warschewske et al.	
D497,462 S	10/2004	Ryan	
D512,508 S	12/2005	Mesaros	
D557,421 S	12/2007	Fleck et al.	
D559,390 S	1/2008	Diener et al.	
D603,048 S	10/2009	Fleck et al.	
D606,202 S	12/2009	Banryu	
D610,770 S	2/2010	Rossini et al.	
D611,610 S *	3/2010	Fleck et al. ....	D24/185
D612,561 S	3/2010	Hunter et al.	
D612,941 S *	3/2010	Youngquist et al. ....	D24/172
D619,264 S	7/2010	Livengood	
D620,121 S	7/2010	Moscovita	
D626,236 S *	10/2010	Ninomiya et al. ....	D24/185

D630,752 S *	1/2011	Suzuki .....	D24/158
D639,948 S	6/2011	Personnelli	
D642,763 S	8/2011	Liang	
D643,535 S *	8/2011	Ross et al. ....	D24/164

(Continued)

**OTHER PUBLICATIONS**

Product Brochure—CS300 IABP—Product Features—2009 Publication—Maquet Cardiovascular LLC. U.S.A.

(Continued)

*Primary Examiner* — Robert M Spear

*Assistant Examiner* — Rhea Shields


(57) **CLAIM**

The ornamental design for a portable medical unit, as shown and described.

**DESCRIPTION**

FIG. 1 is a front perspective view of a portable medical unit showing my new design;  
 FIG. 2 is a rear perspective view thereof;  
 FIG. 3 is a front view thereof;  
 FIG. 4 is a top view thereof;  
 FIG. 5 is a left side view thereof;  
 FIG. 6 is a right side view thereof;  
 FIG. 7 is a rear view thereof;  
 FIG. 8 is a bottom view thereof;  
 FIG. 9 is a detail view taken about the oval shaped border labelled "FIG. 9" in FIG. 3;  
 FIG. 10 is a detail view taken about the oval shaped border labelled "FIG. 10" in FIG. 4;  
 FIG. 11 is a detail view taken about the oval shaped border labelled "FIG. 11" in FIG. 7; and,  
 FIG. 12 is a detail view taken about the oval shaped border labelled "FIG. 12" in FIG. 7.  
 The broken lines in the figures are for illustrative purposes only and form no part of the claimed design.

**1 Claim, 12 Drawing Sheets**

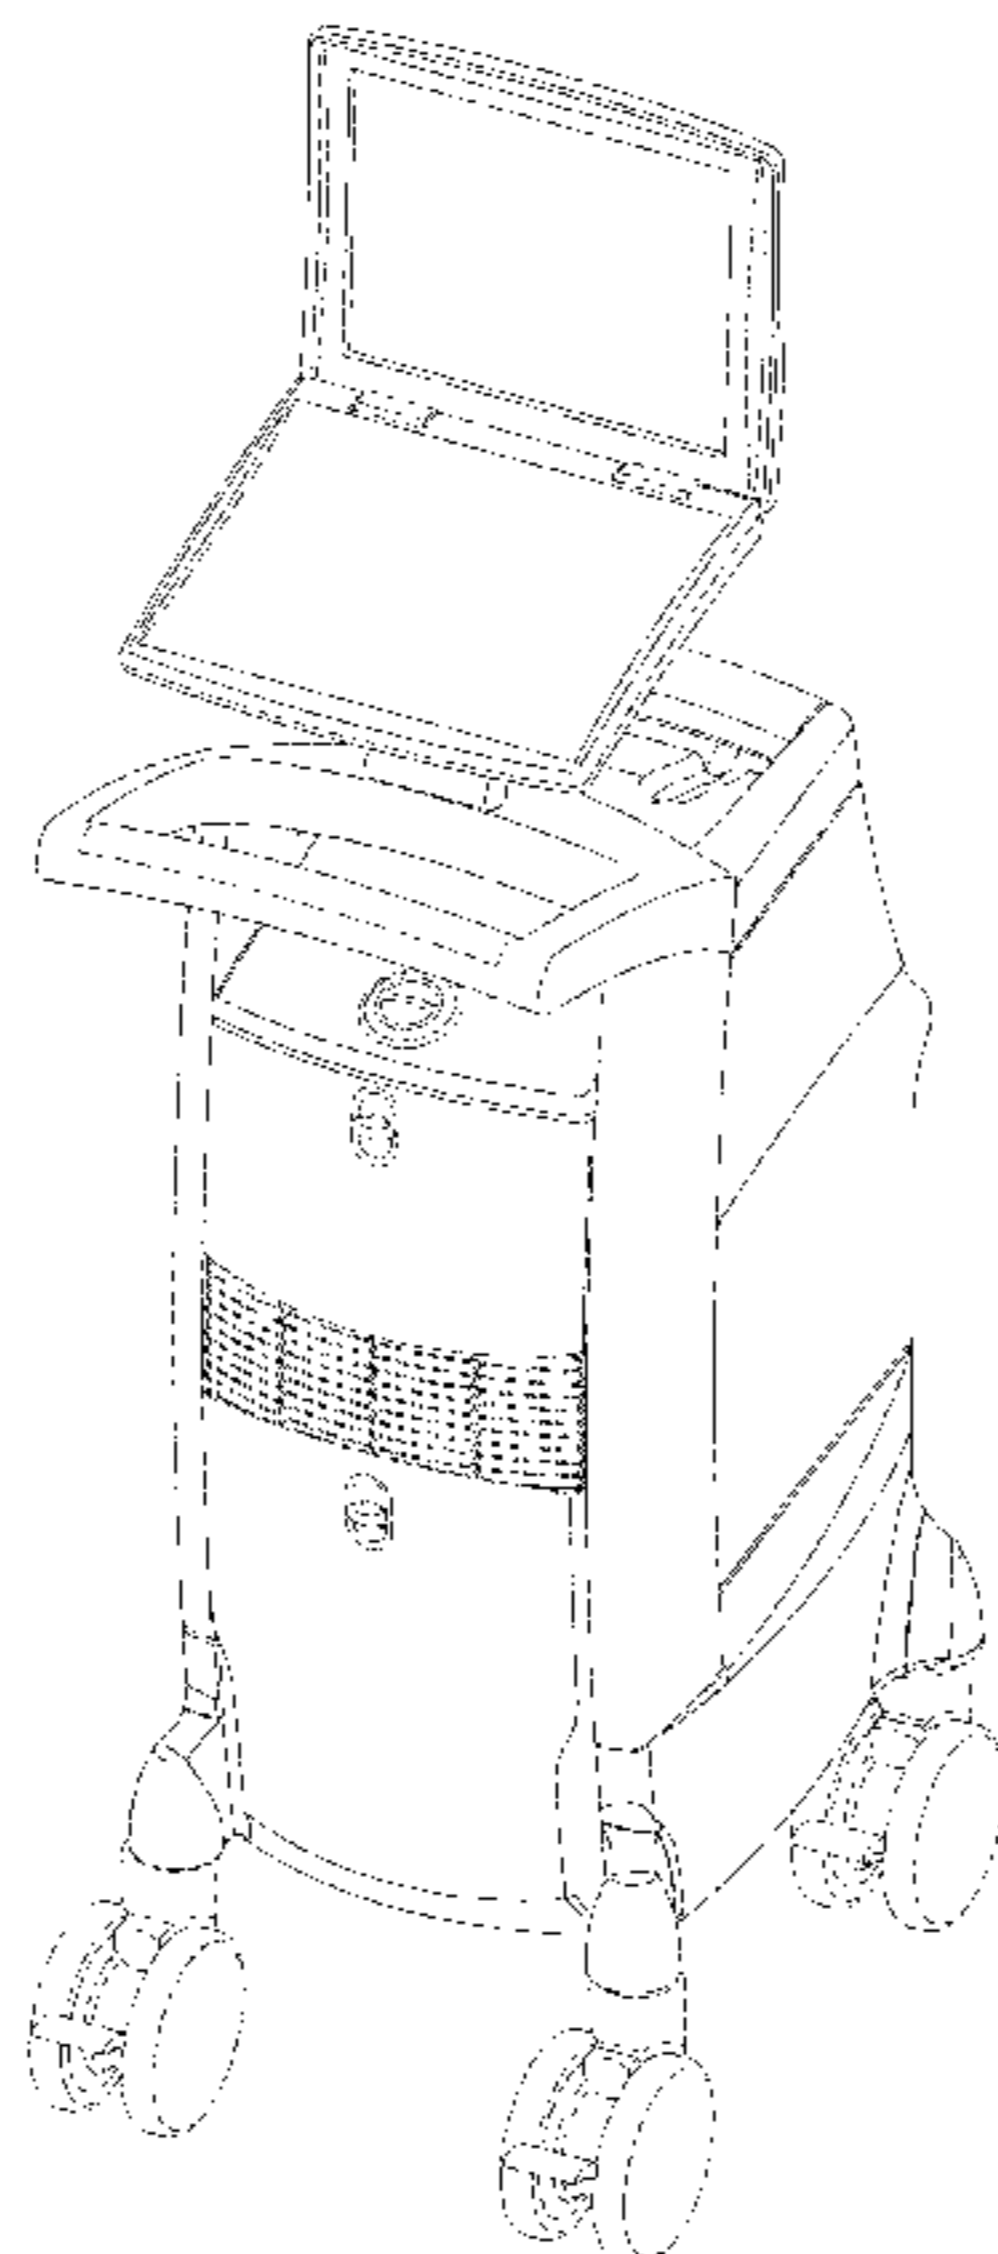

(56)

**References Cited**

U.S. PATENT DOCUMENTS

D650,482 S	*	12/2011	Kim et al.	.....	D24/158
D652,520 S		1/2012	Sabaris Vilas		
D652,521 S		1/2012	Ross et al.		
D652,936 S		1/2012	Ross et al.		
D662,208 S	*	6/2012	Otoha et al.	.....	D24/185
D672,046 S	*	12/2012	Fuster	.....	D24/200
2003/0055309 A1		3/2003	Kaushansky et al.		

OTHER PUBLICATIONS

Product Brochure—CS100 IABP—Intelligent Counterpulsation—2010 Publication—Maquet Cardiovascular LLC. U.S.A.  
 Operators Guide—The CS100/CS100i Abbreviated Operator’s Guide—2009 Publication—Maquet Cardiovascular LLC. U.S.A.  
 Operators Guide—Datascope Abbreviated Operator’s Guide for the System 97 Intra-Aortic Balloon Pump—Published prior to 2009—Datascope Corp. U.S.A.  
 Brochure—Sensation and CS300 IABP System Smaller Meets Faster—Published in 2009—Maquet Cardiovascular LLC. U.S.A.

Brochure—CS300 IABP Product Features—Published in 2009—Maquet Cardiovascular LLC. U.S.A.  
 Brochure—CS100—Intelligent Counterpulsation—Published prior to 2009—Datascope Corp. U.S.A.  
 Brochure—Datascope System 97—Published Prior to 2009—Datascope Corp. U.S.A.  
 Abbreviated Operation and Troubleshooting Guide—Arrow AutoCat2 Wave IAB Abbreviated Operation and Troubleshooting Guide—2005—Arrow International, Inc.  
 Troubleshooting Brochure—Troubleshooting Beyond the Basics—Arrow Intra-Aortic Balloon Pump—1999—Arrow International, Inc.  
 Educational Material—AutoCAT2 Series Intra-Aortic Balloon Pump—Timing, Triggering, and Troubleshooting—2005—Arrow International, Inc. U.S.A.  
 Brochure—Changing Disposable Helium Tank—2005—Arrow International, Inc. U.S.A.  
 Educational Materials—ACAT1 Plus Intra-Aortic Balloon Pump—Timing, Triggering, and Troubleshooting—2005—Arrow International, Inc. U.S.A.  
 Brochure/Flyer—Feature Comparison—Arrow AutoCAT2 Series—2006—Arrow International, Inc. U.S.A.

\* cited by examiner

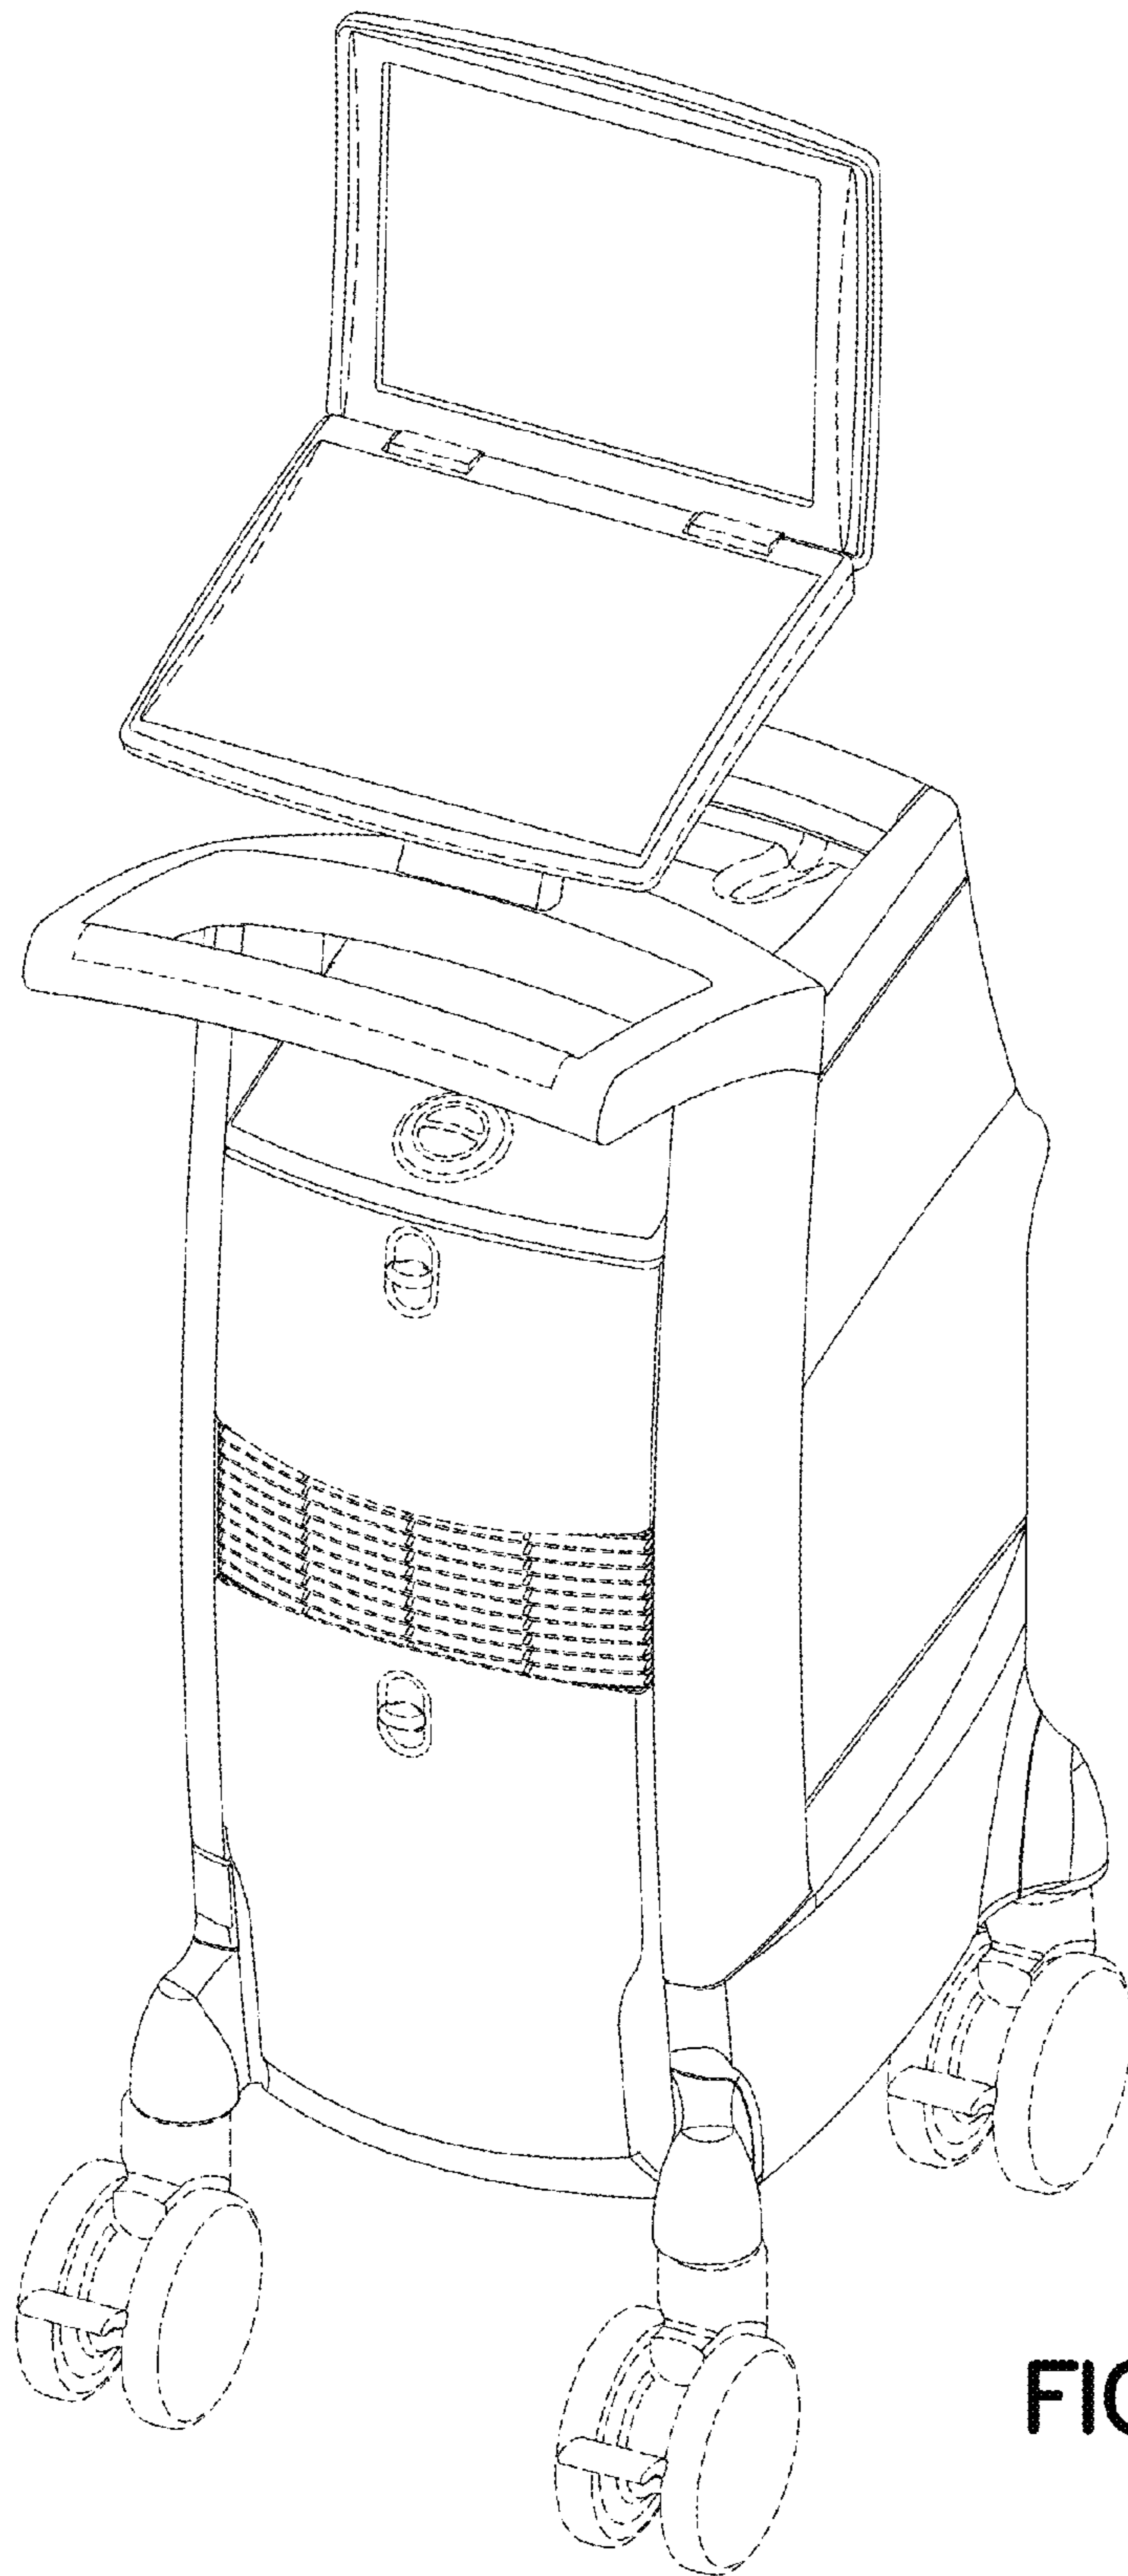


FIG. 1

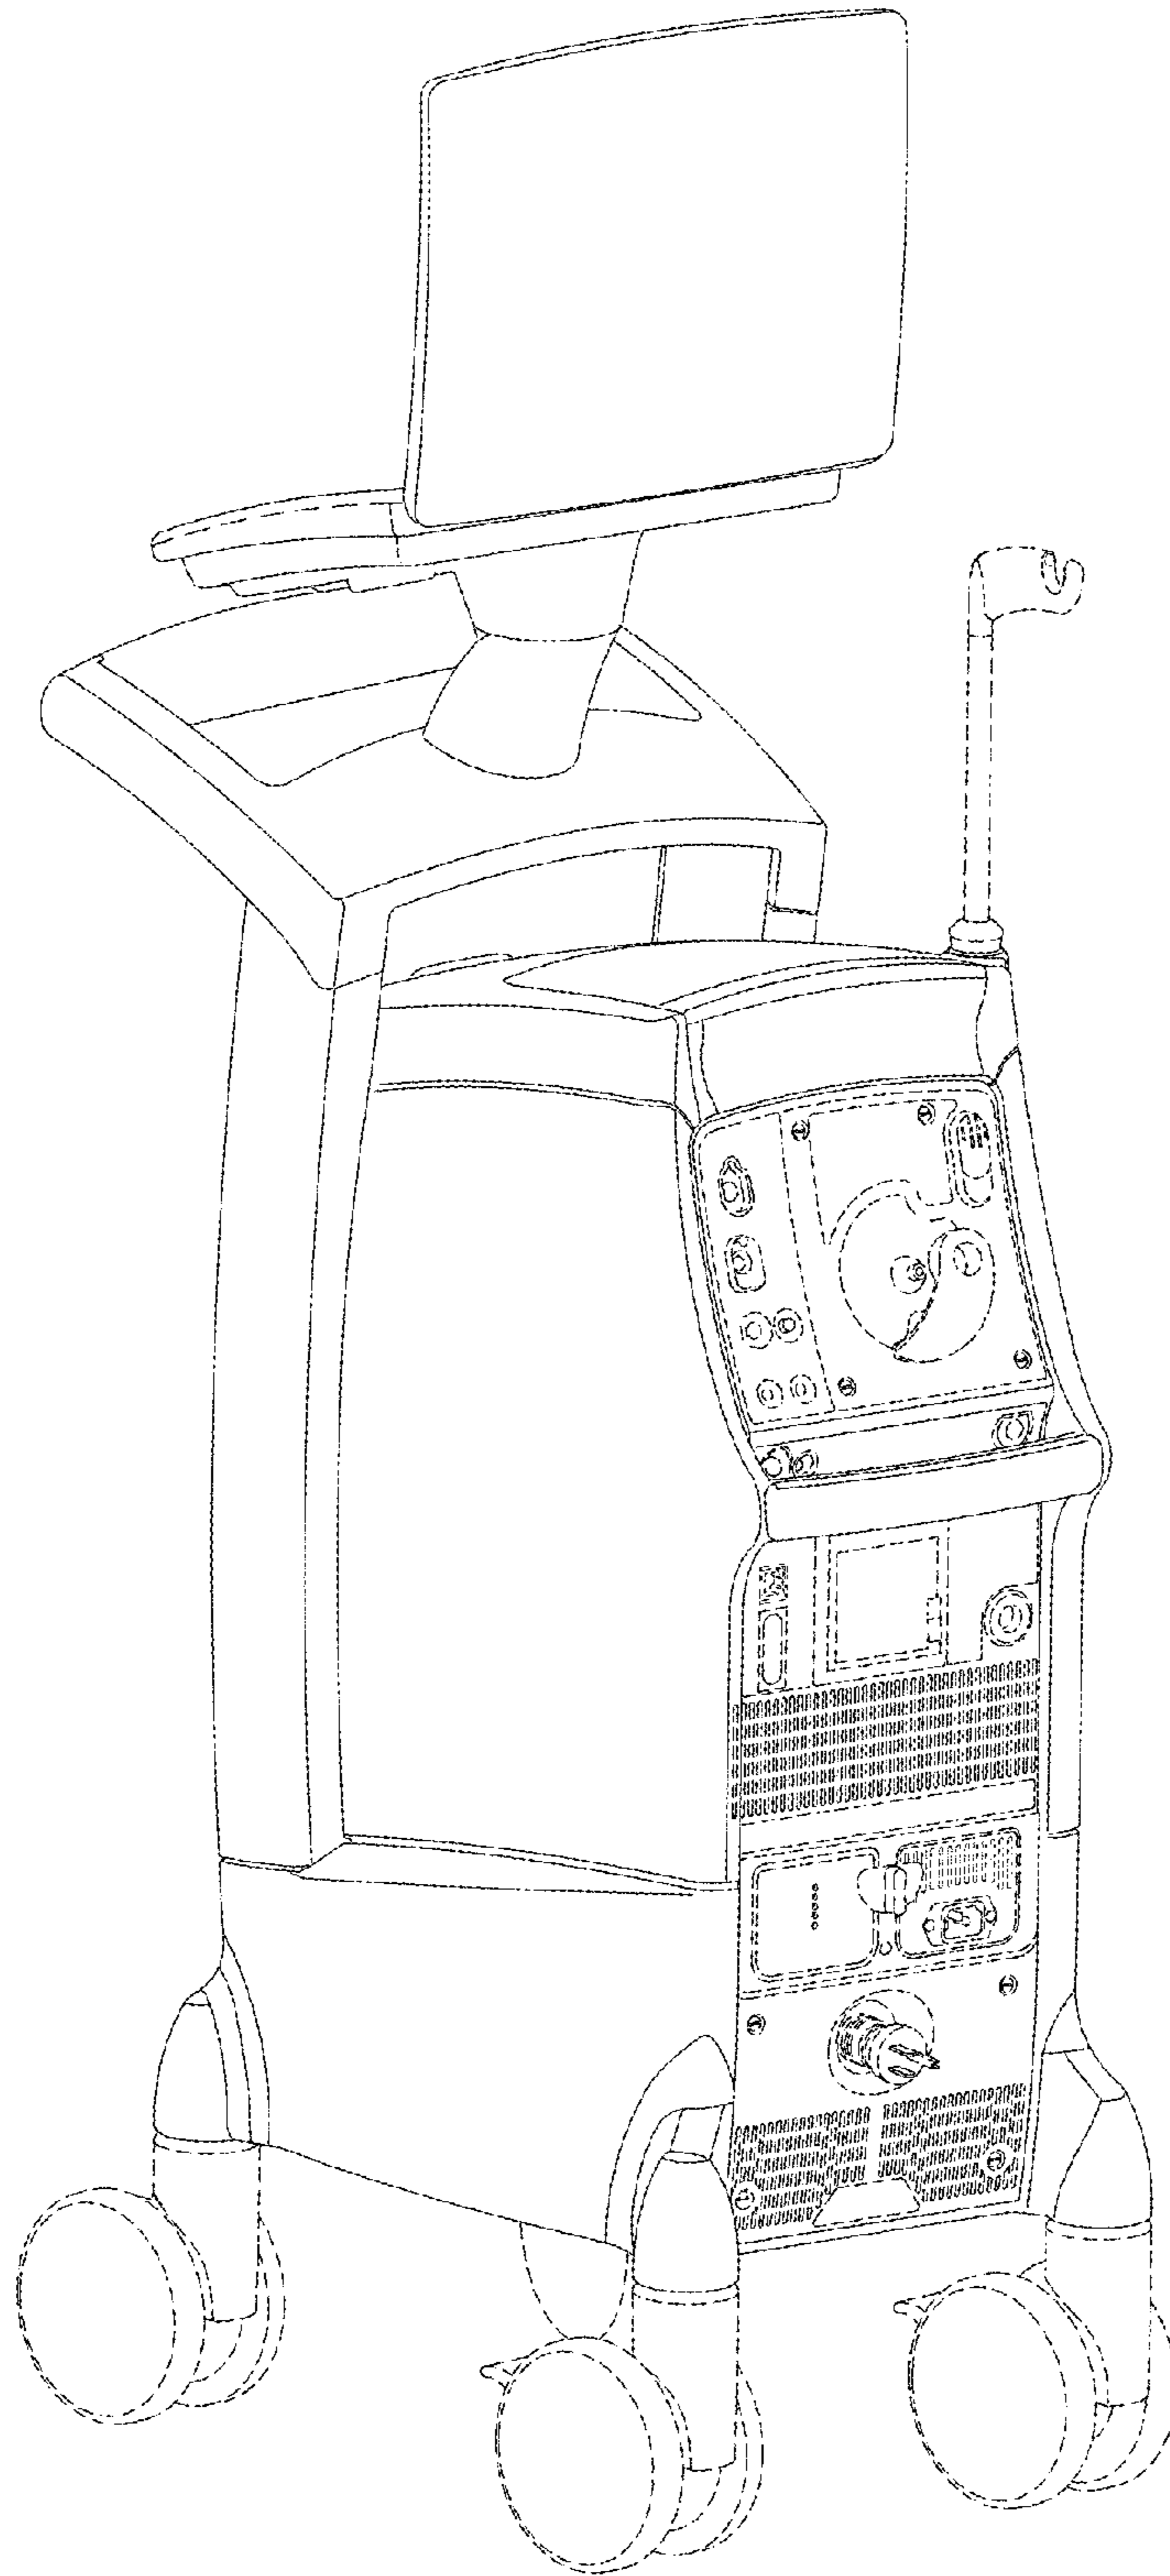


FIG.2

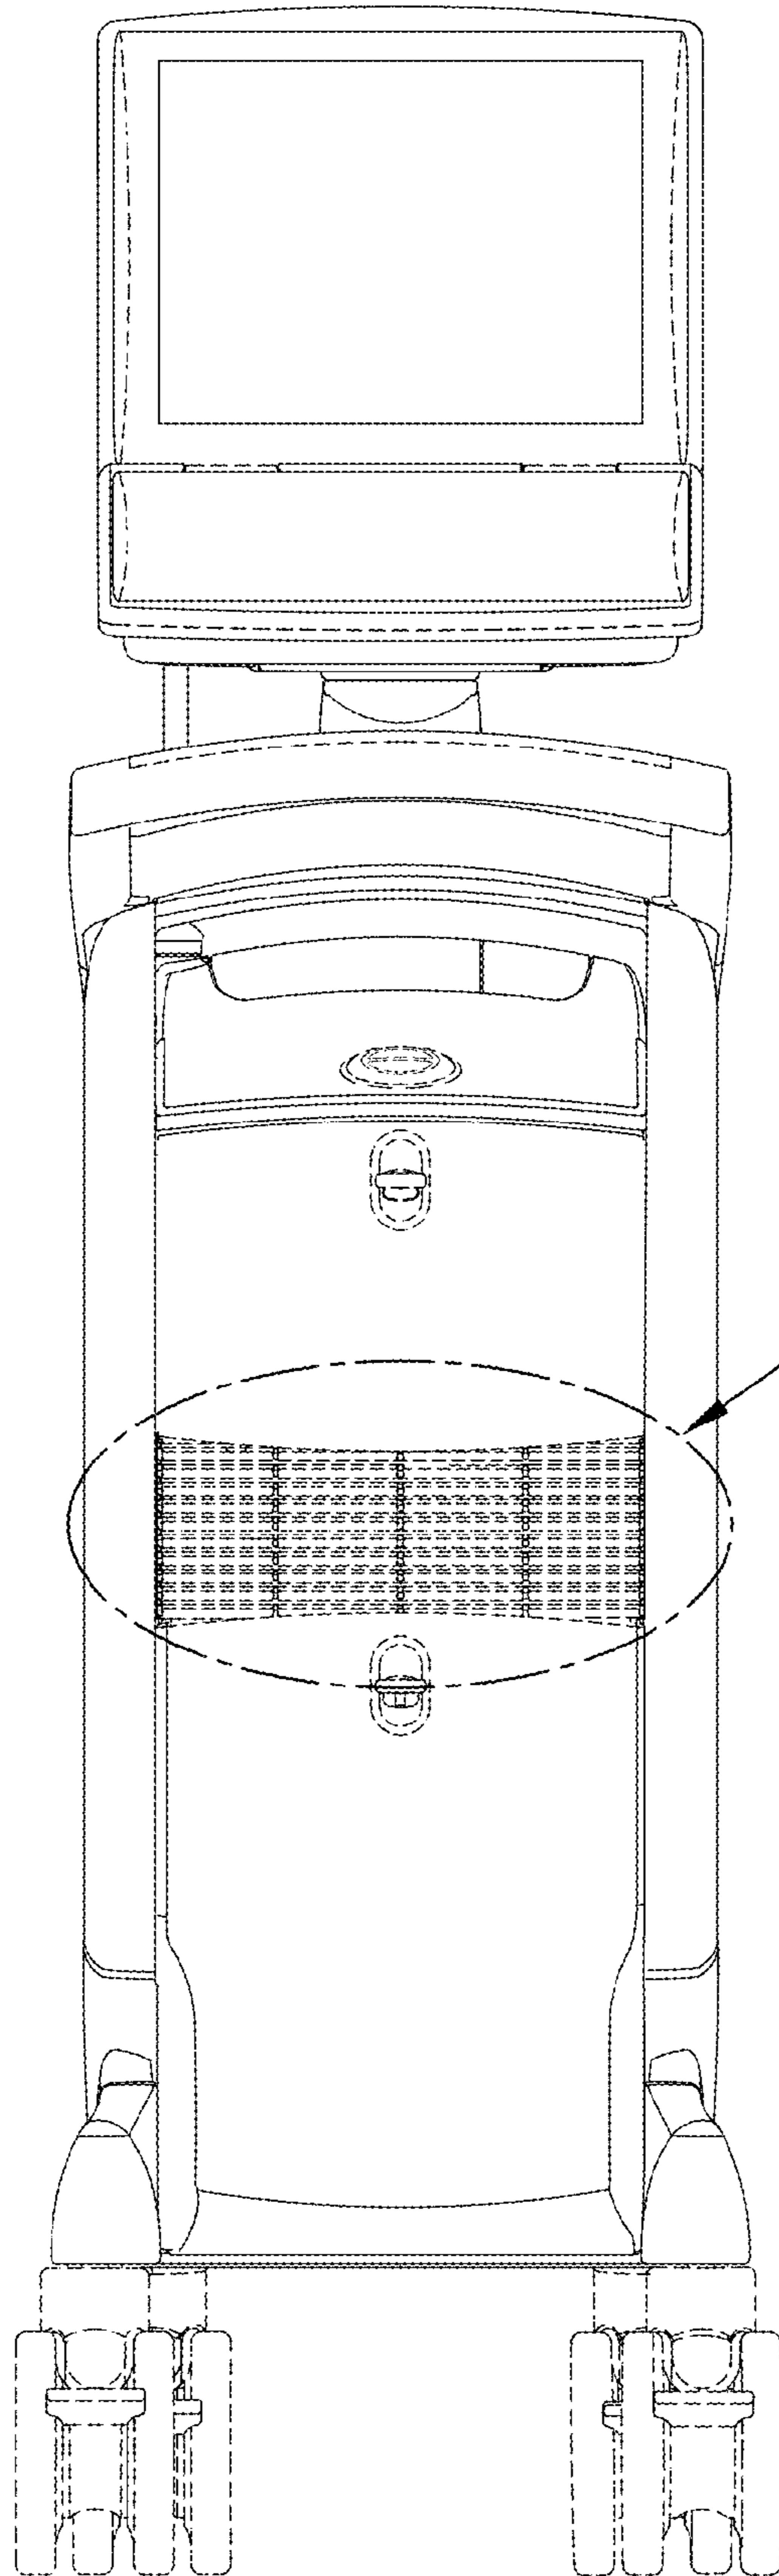


FIG.9

FIG.3

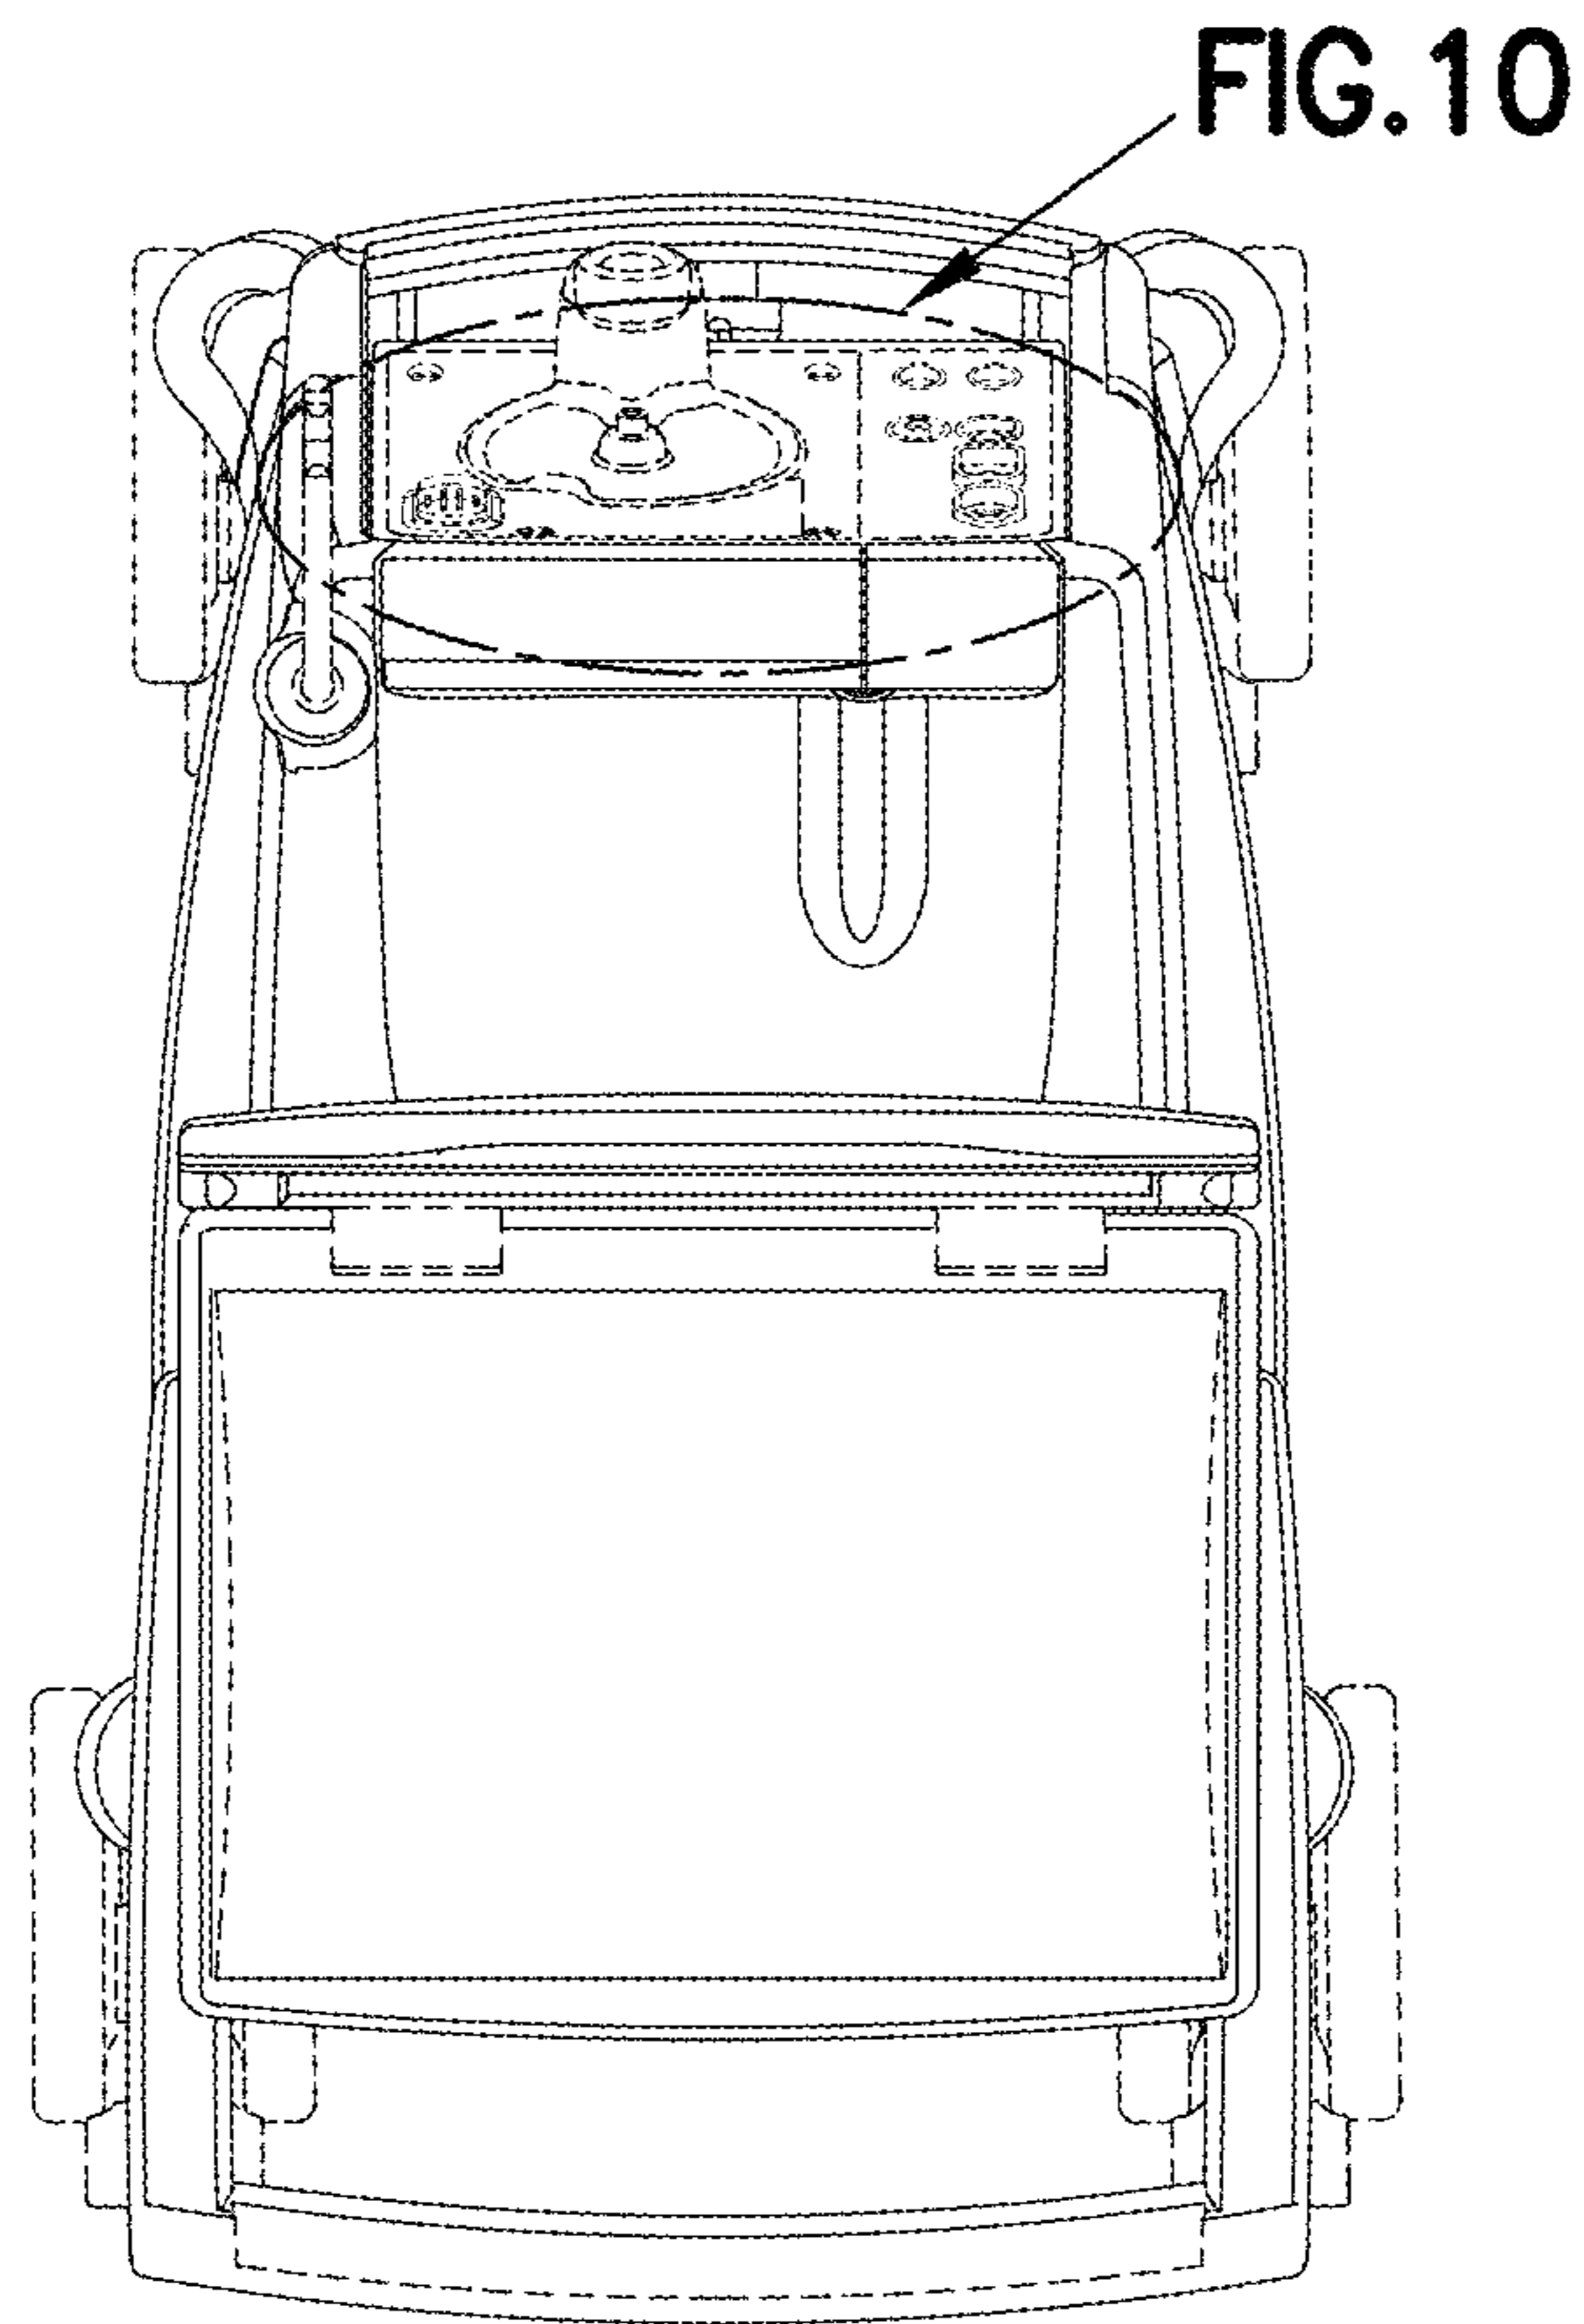


FIG.4

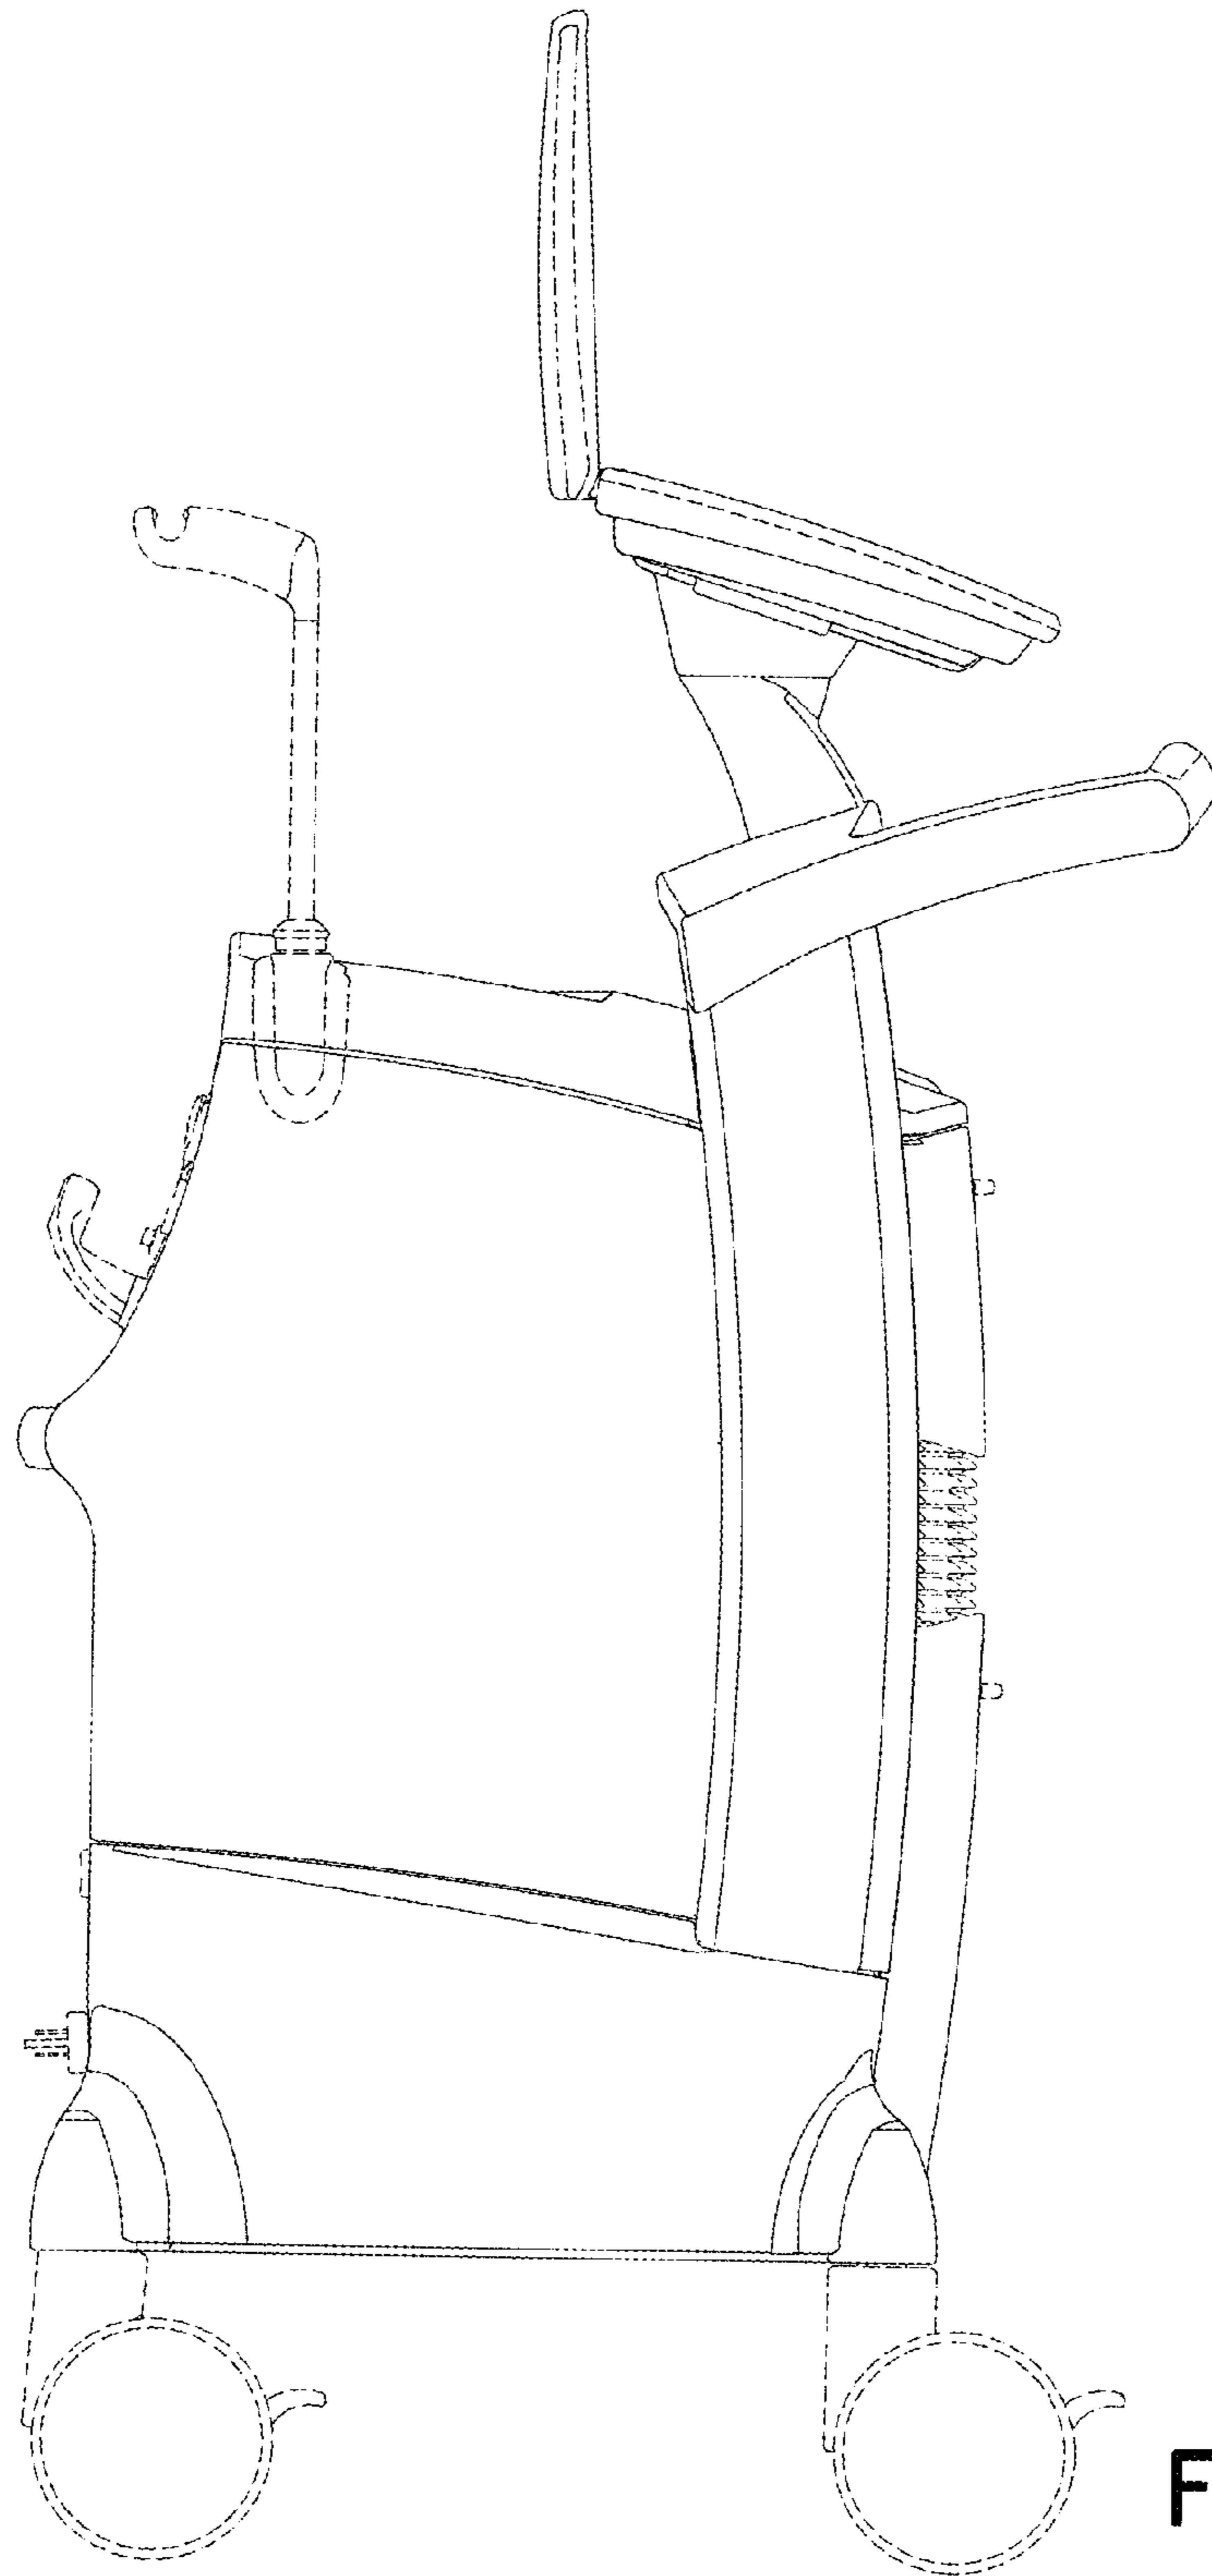


FIG. 5

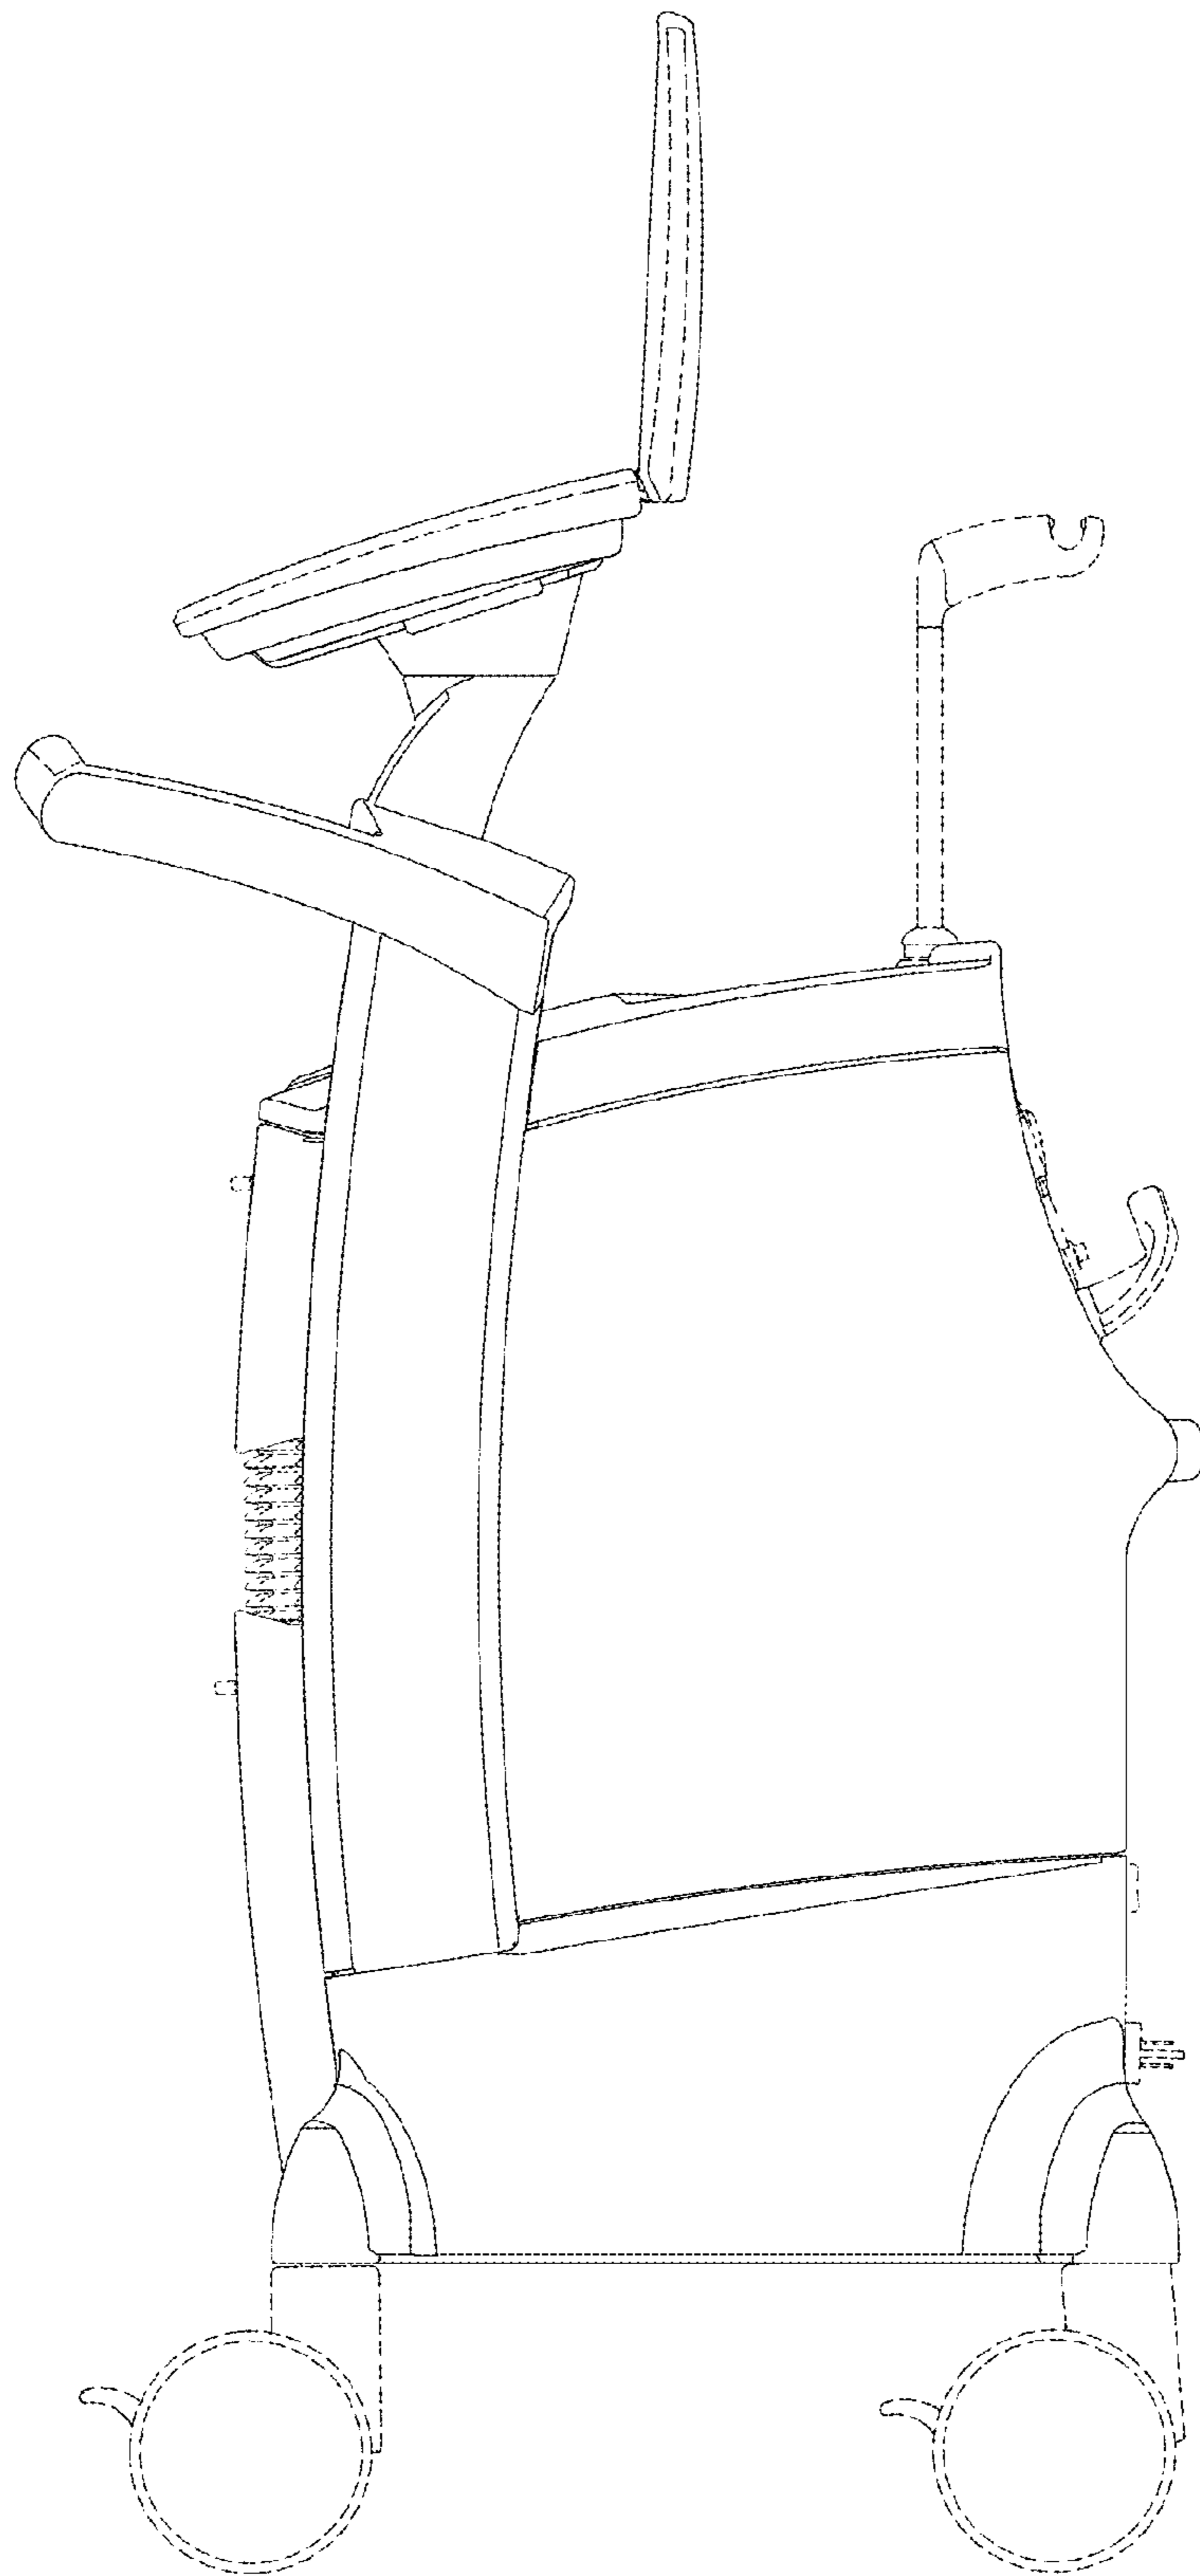


FIG. 6



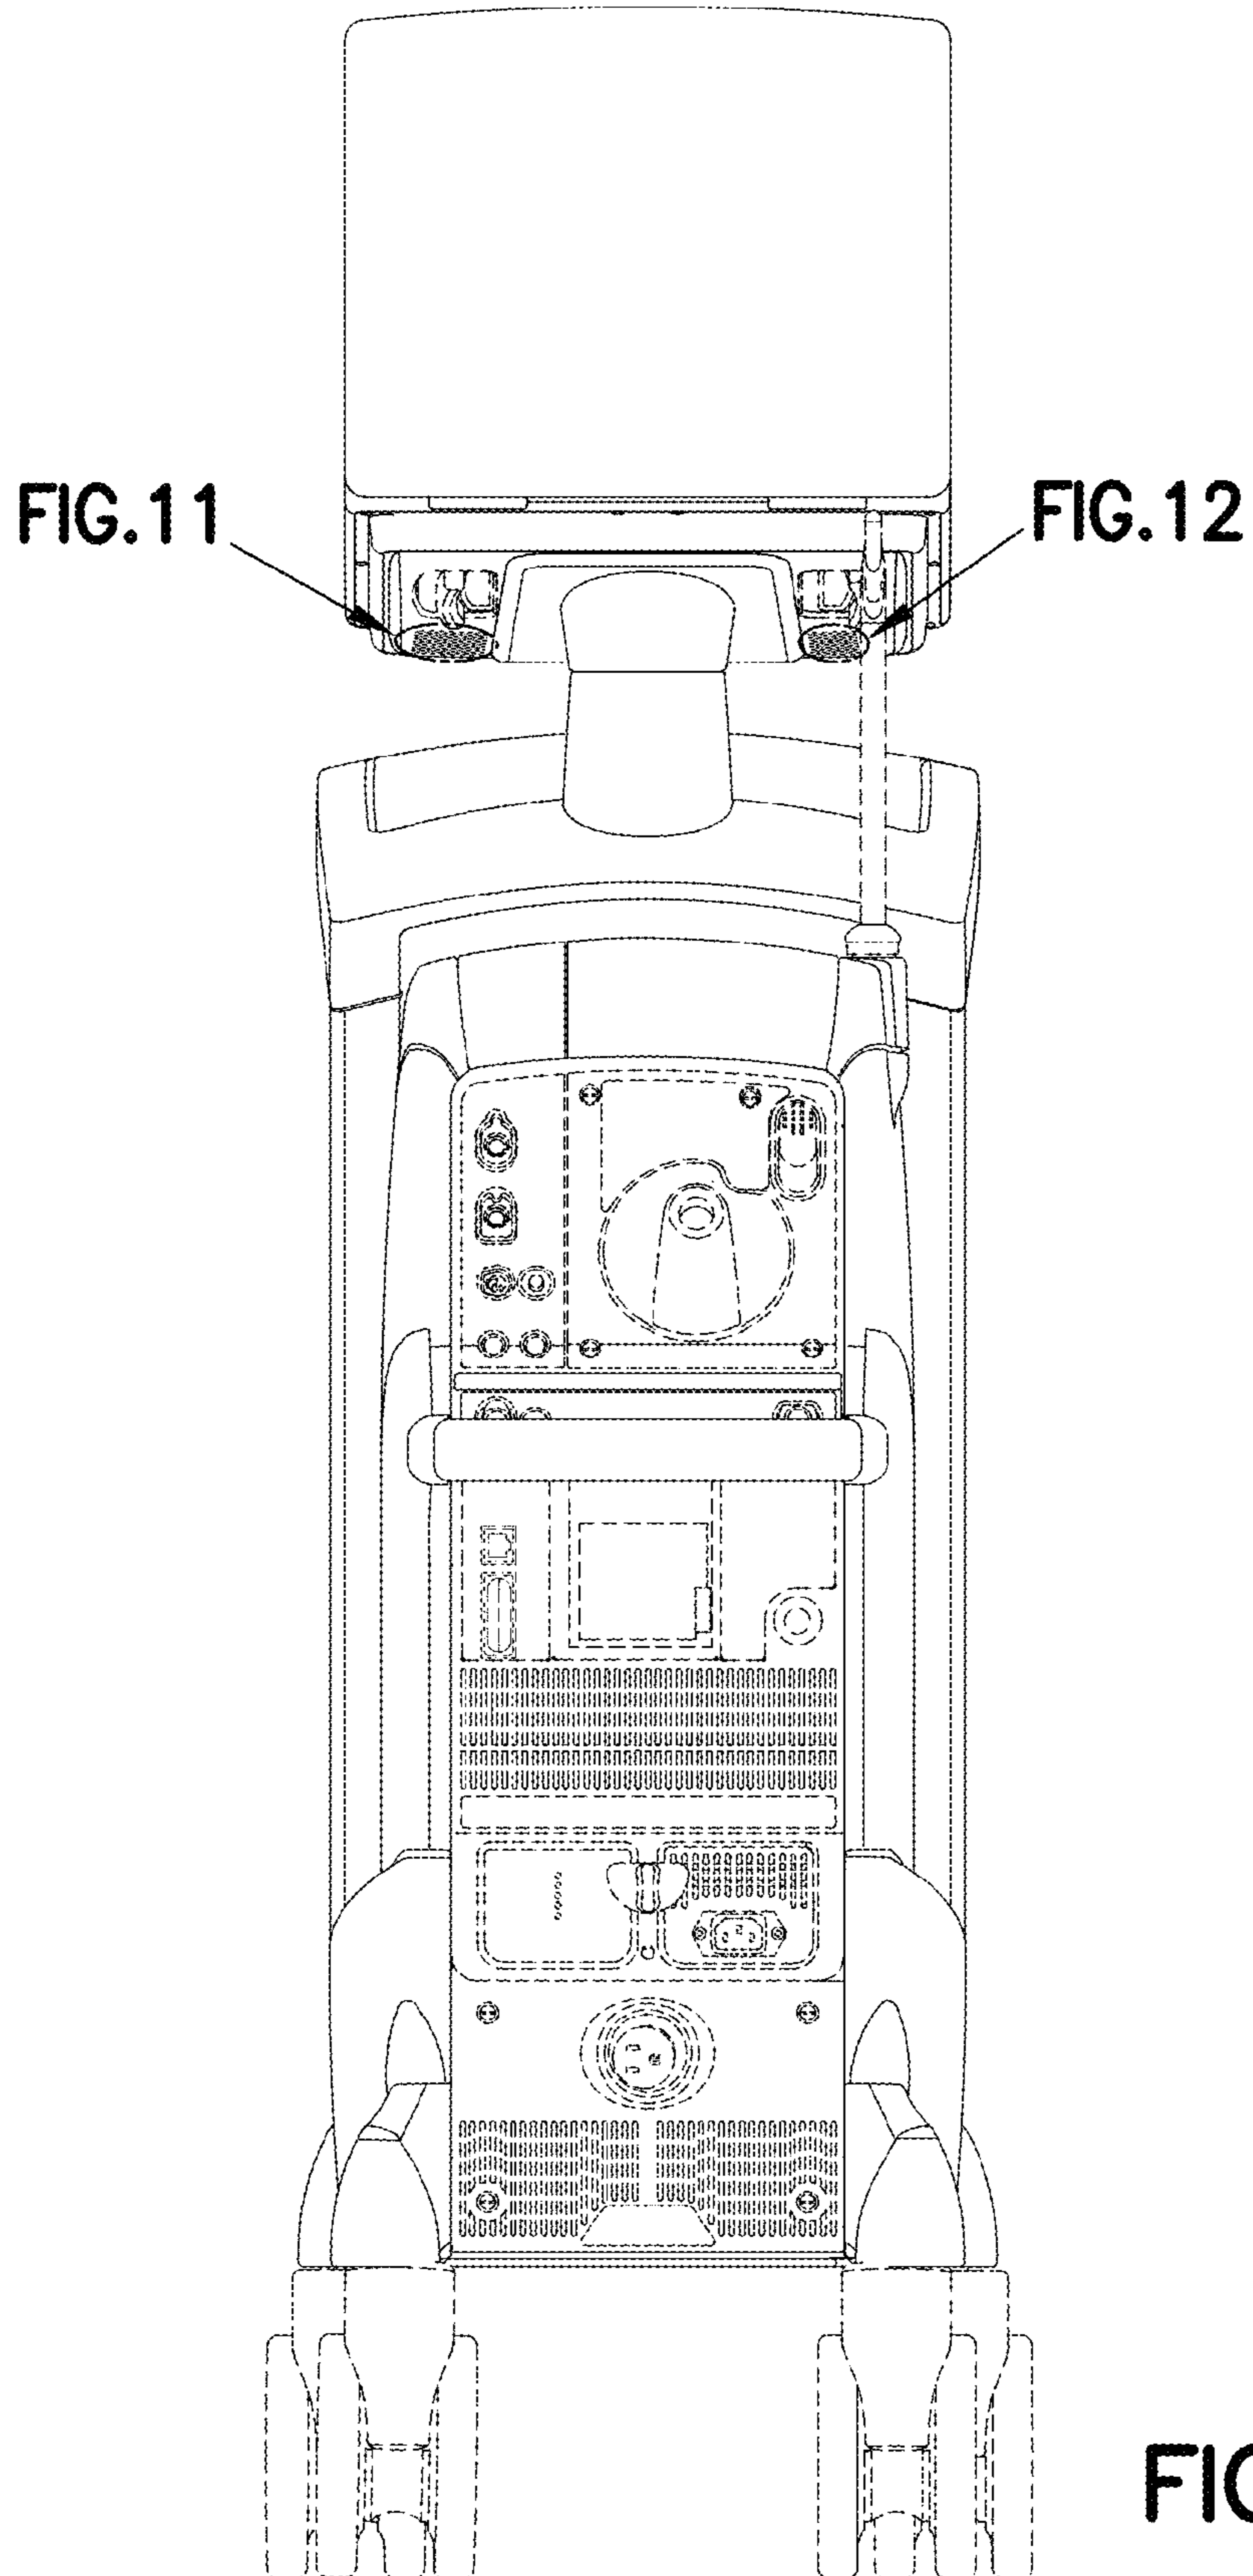


FIG.7

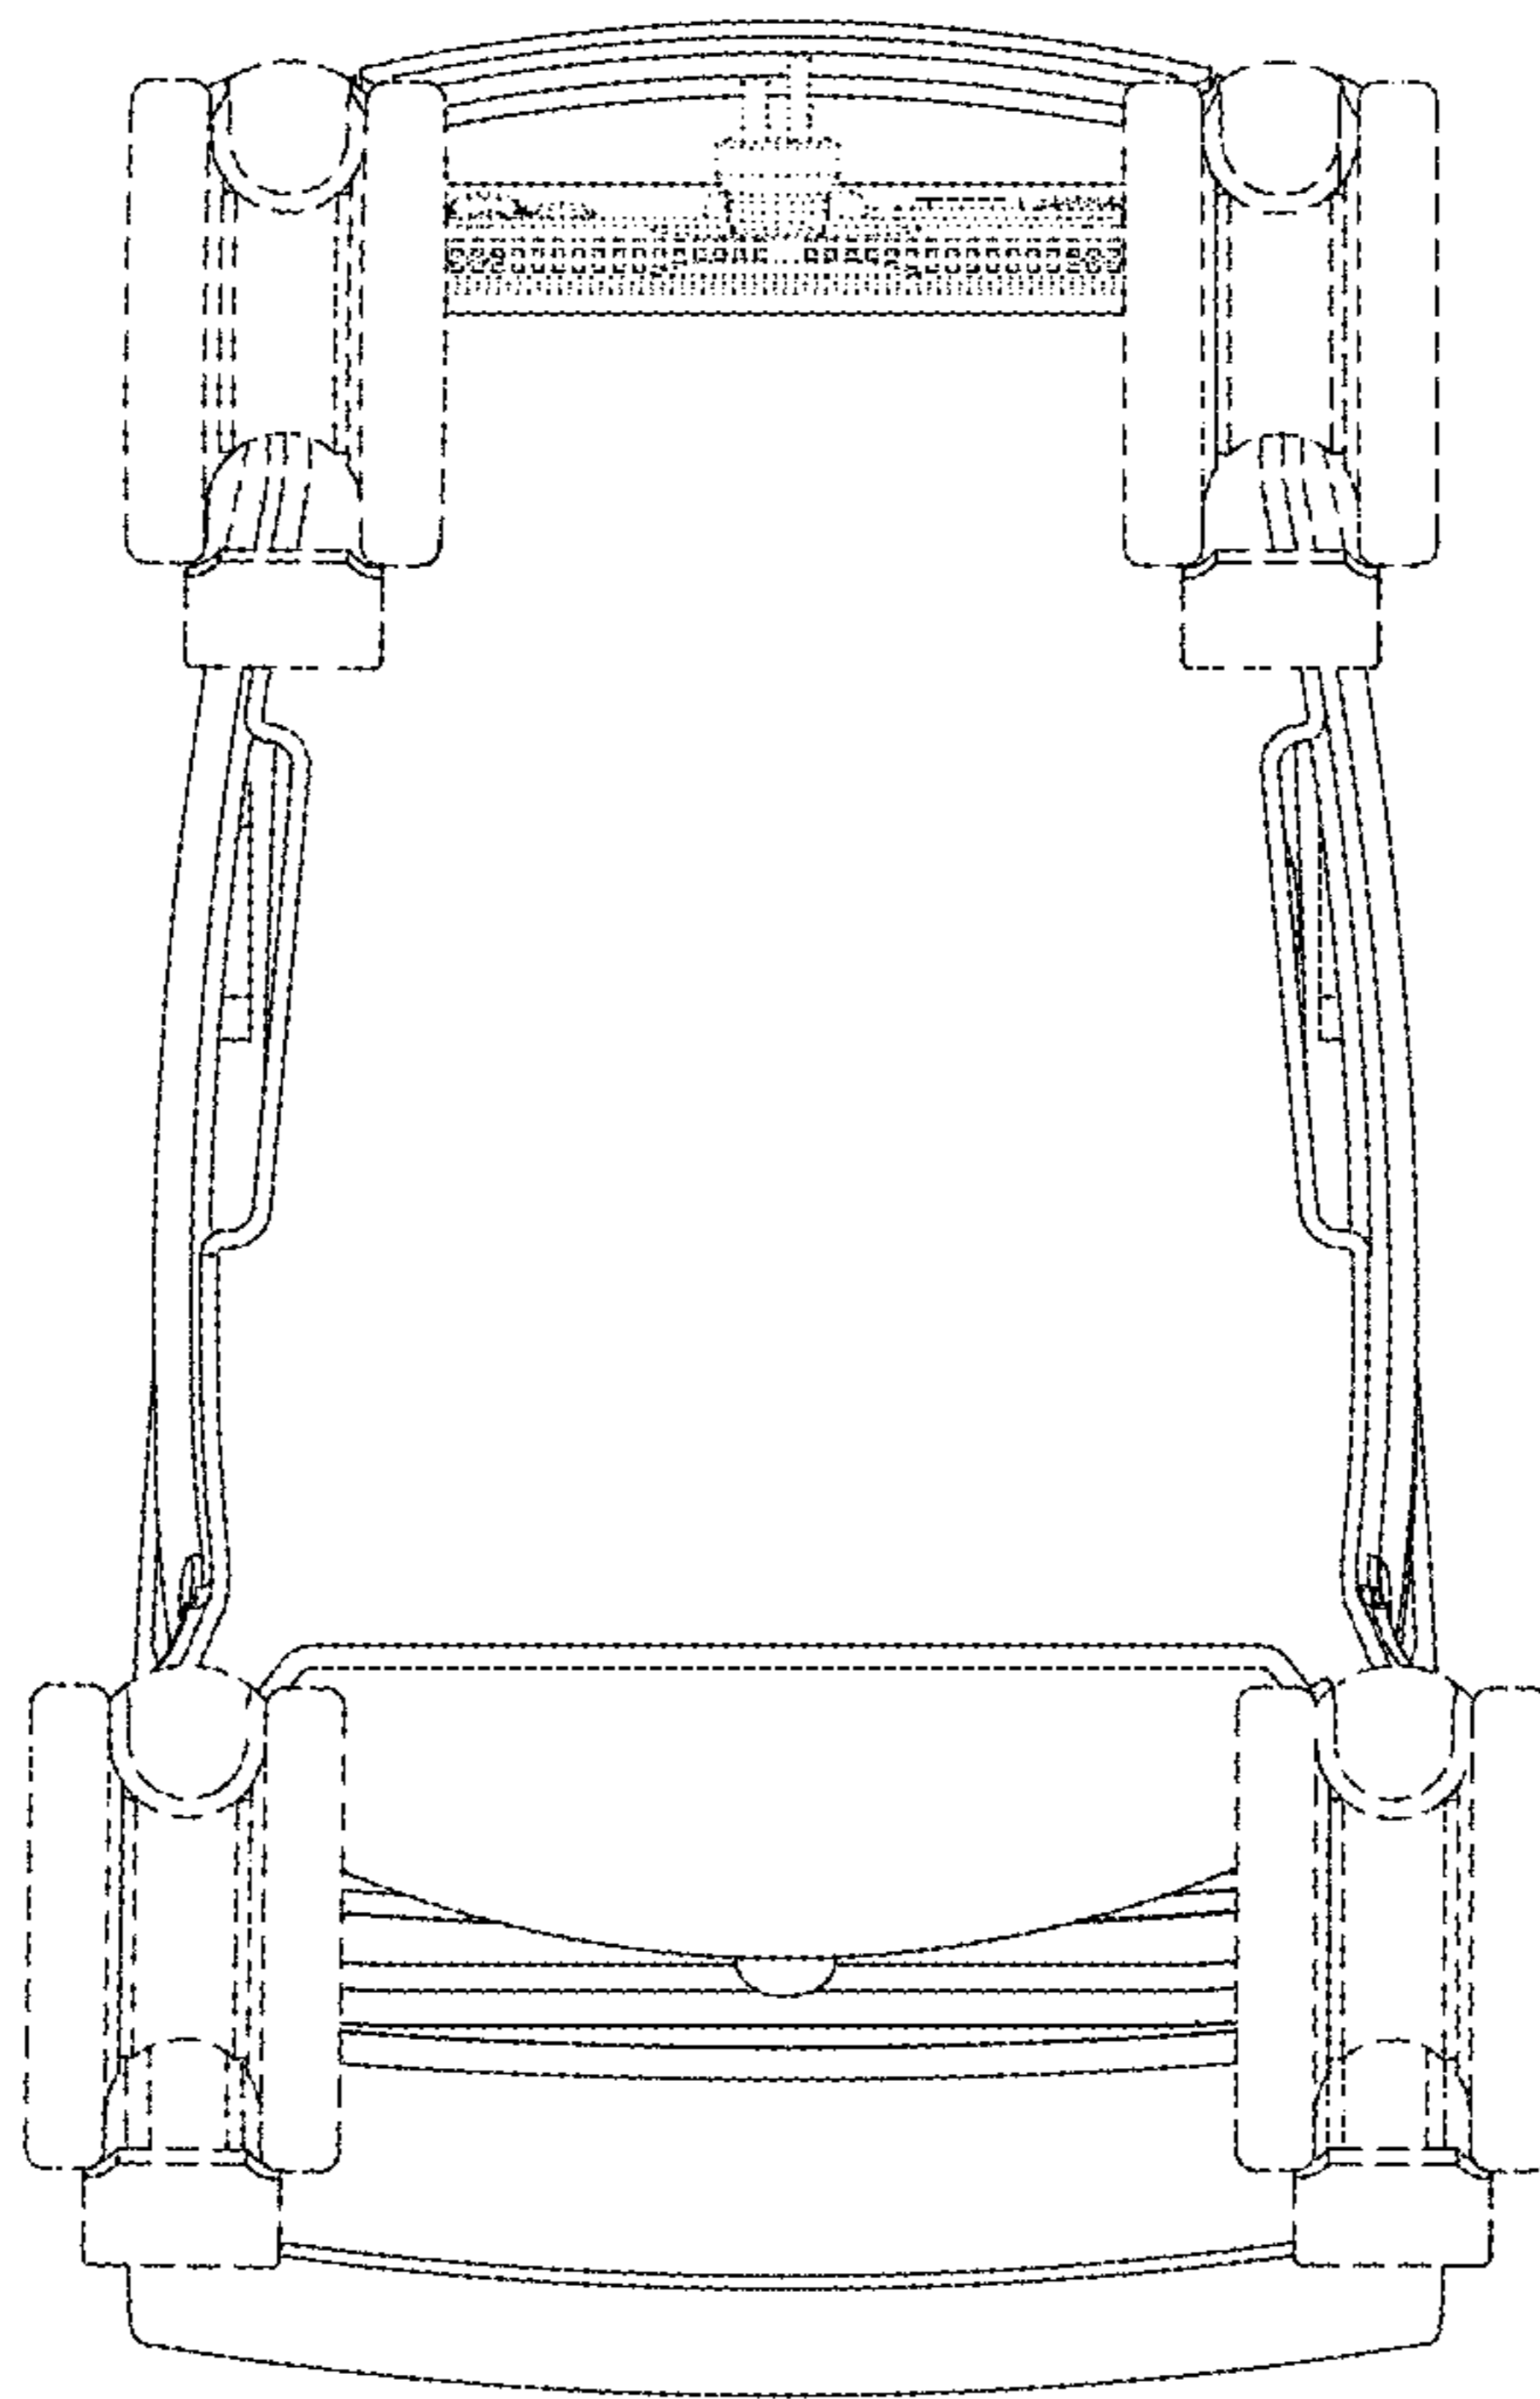


FIG.8

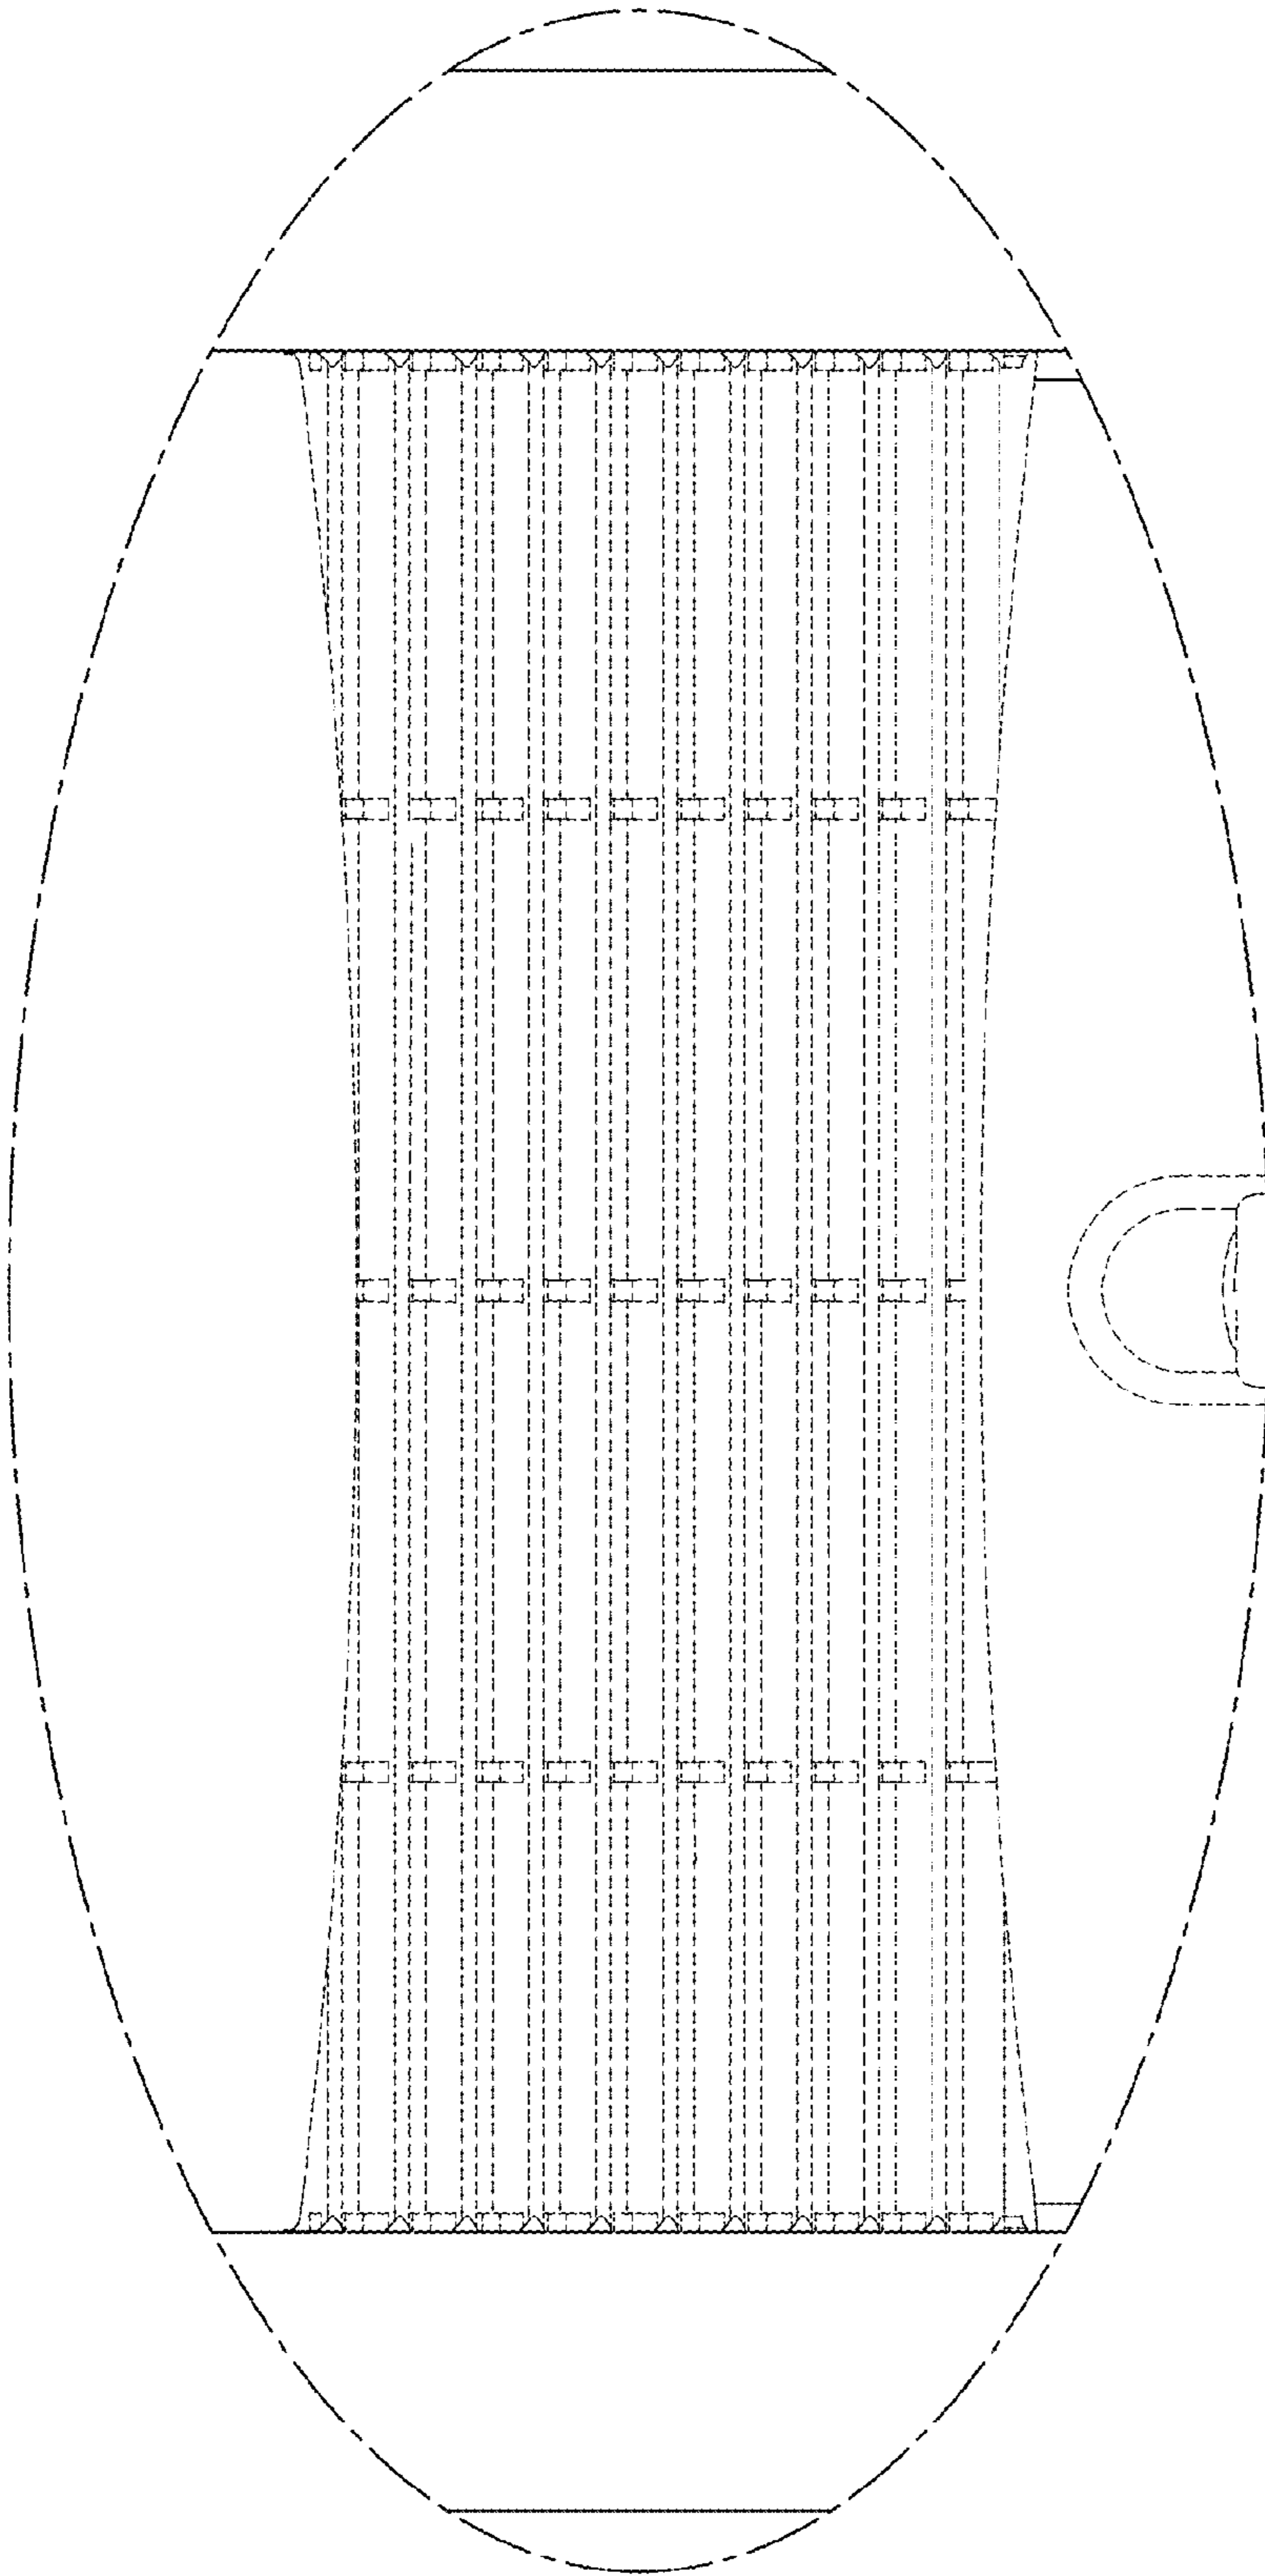


FIG.9

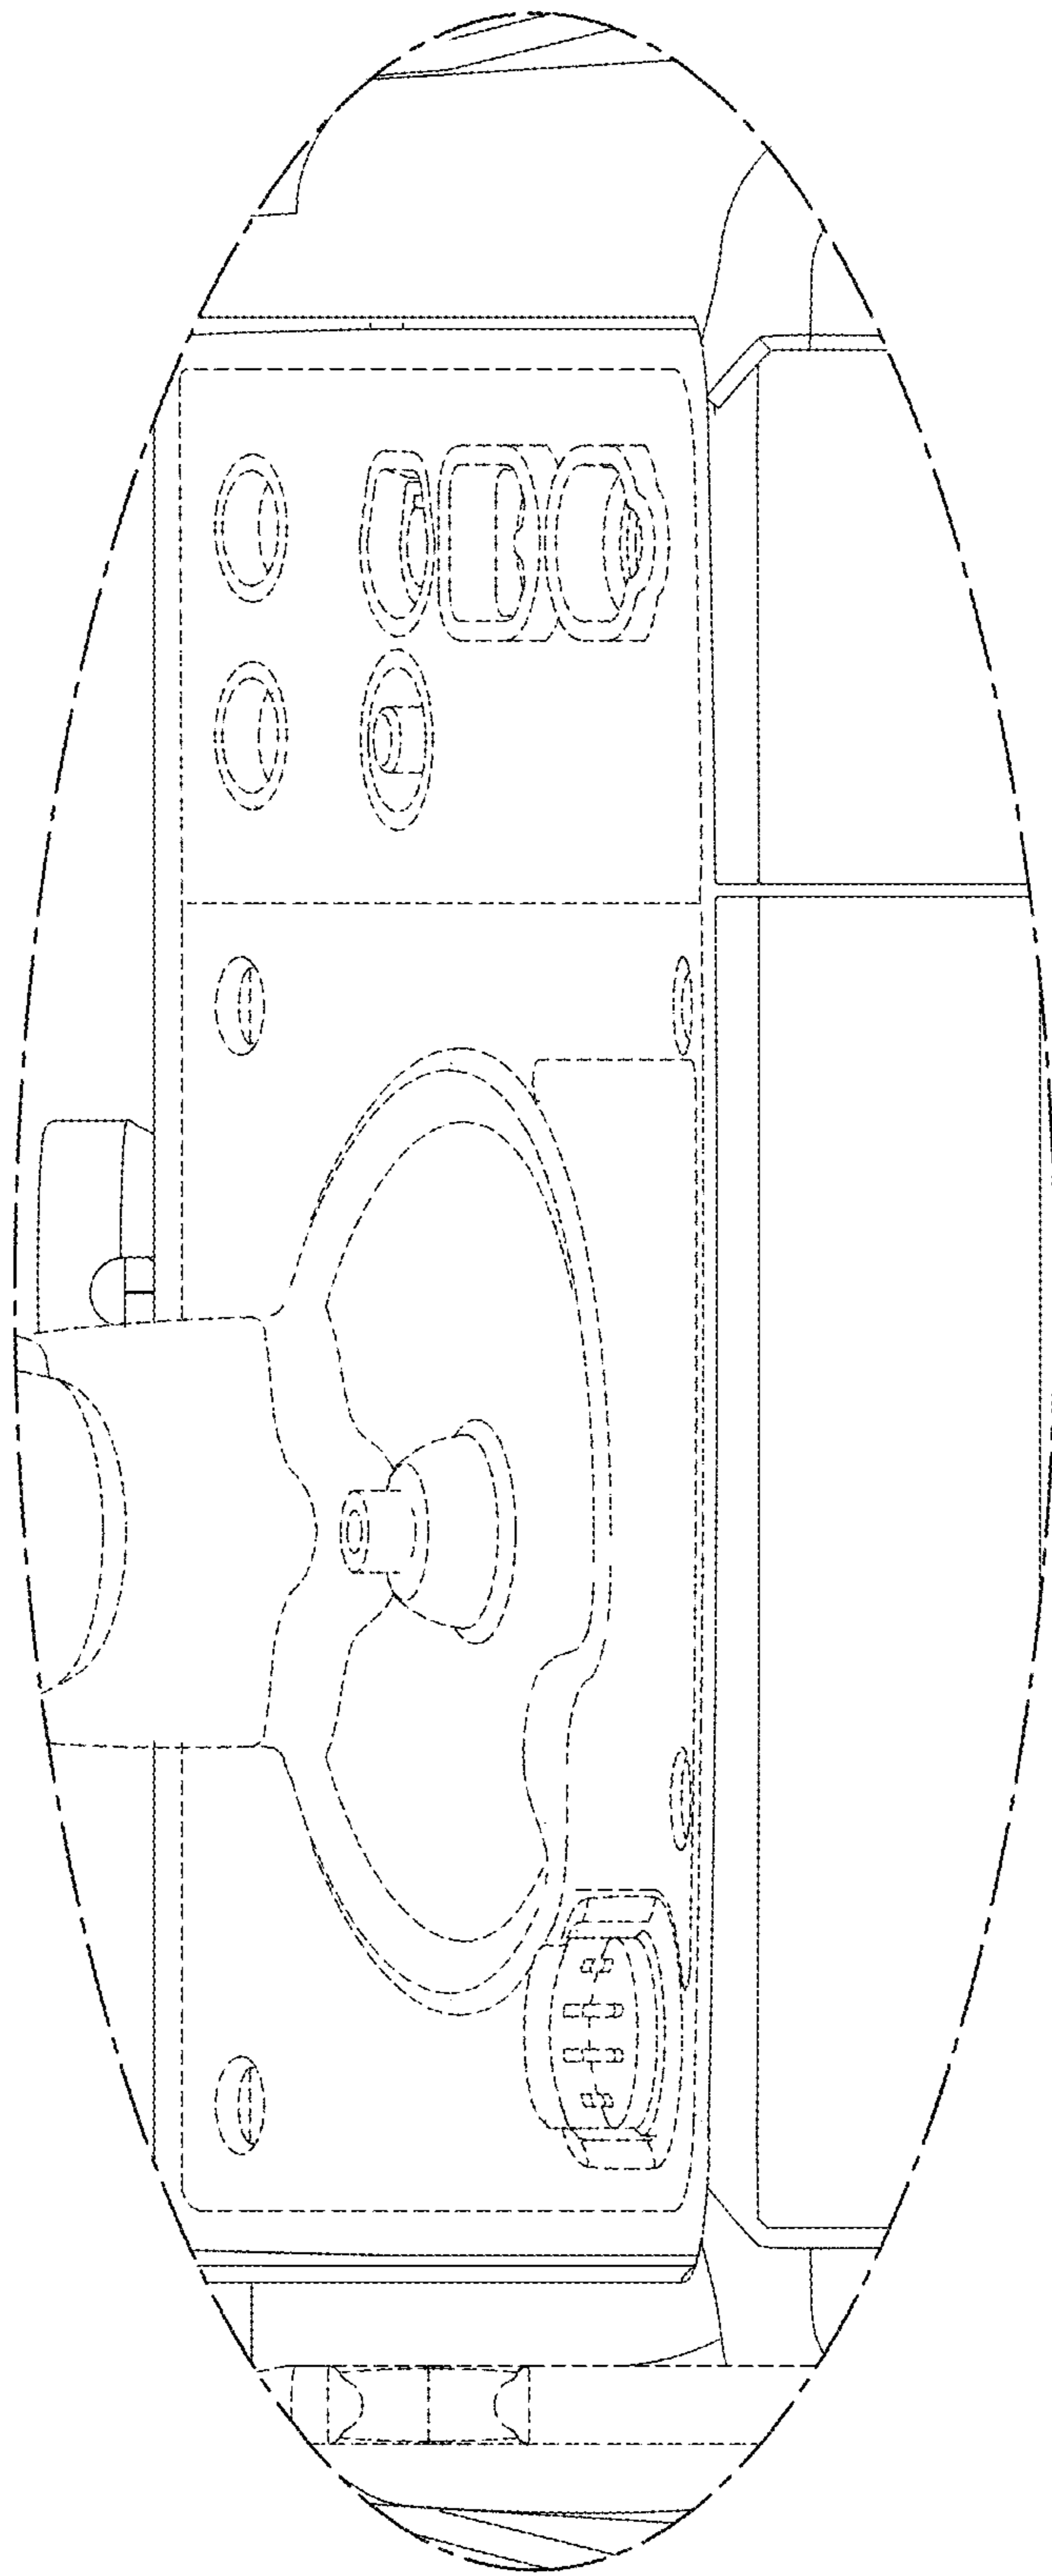


FIG.10

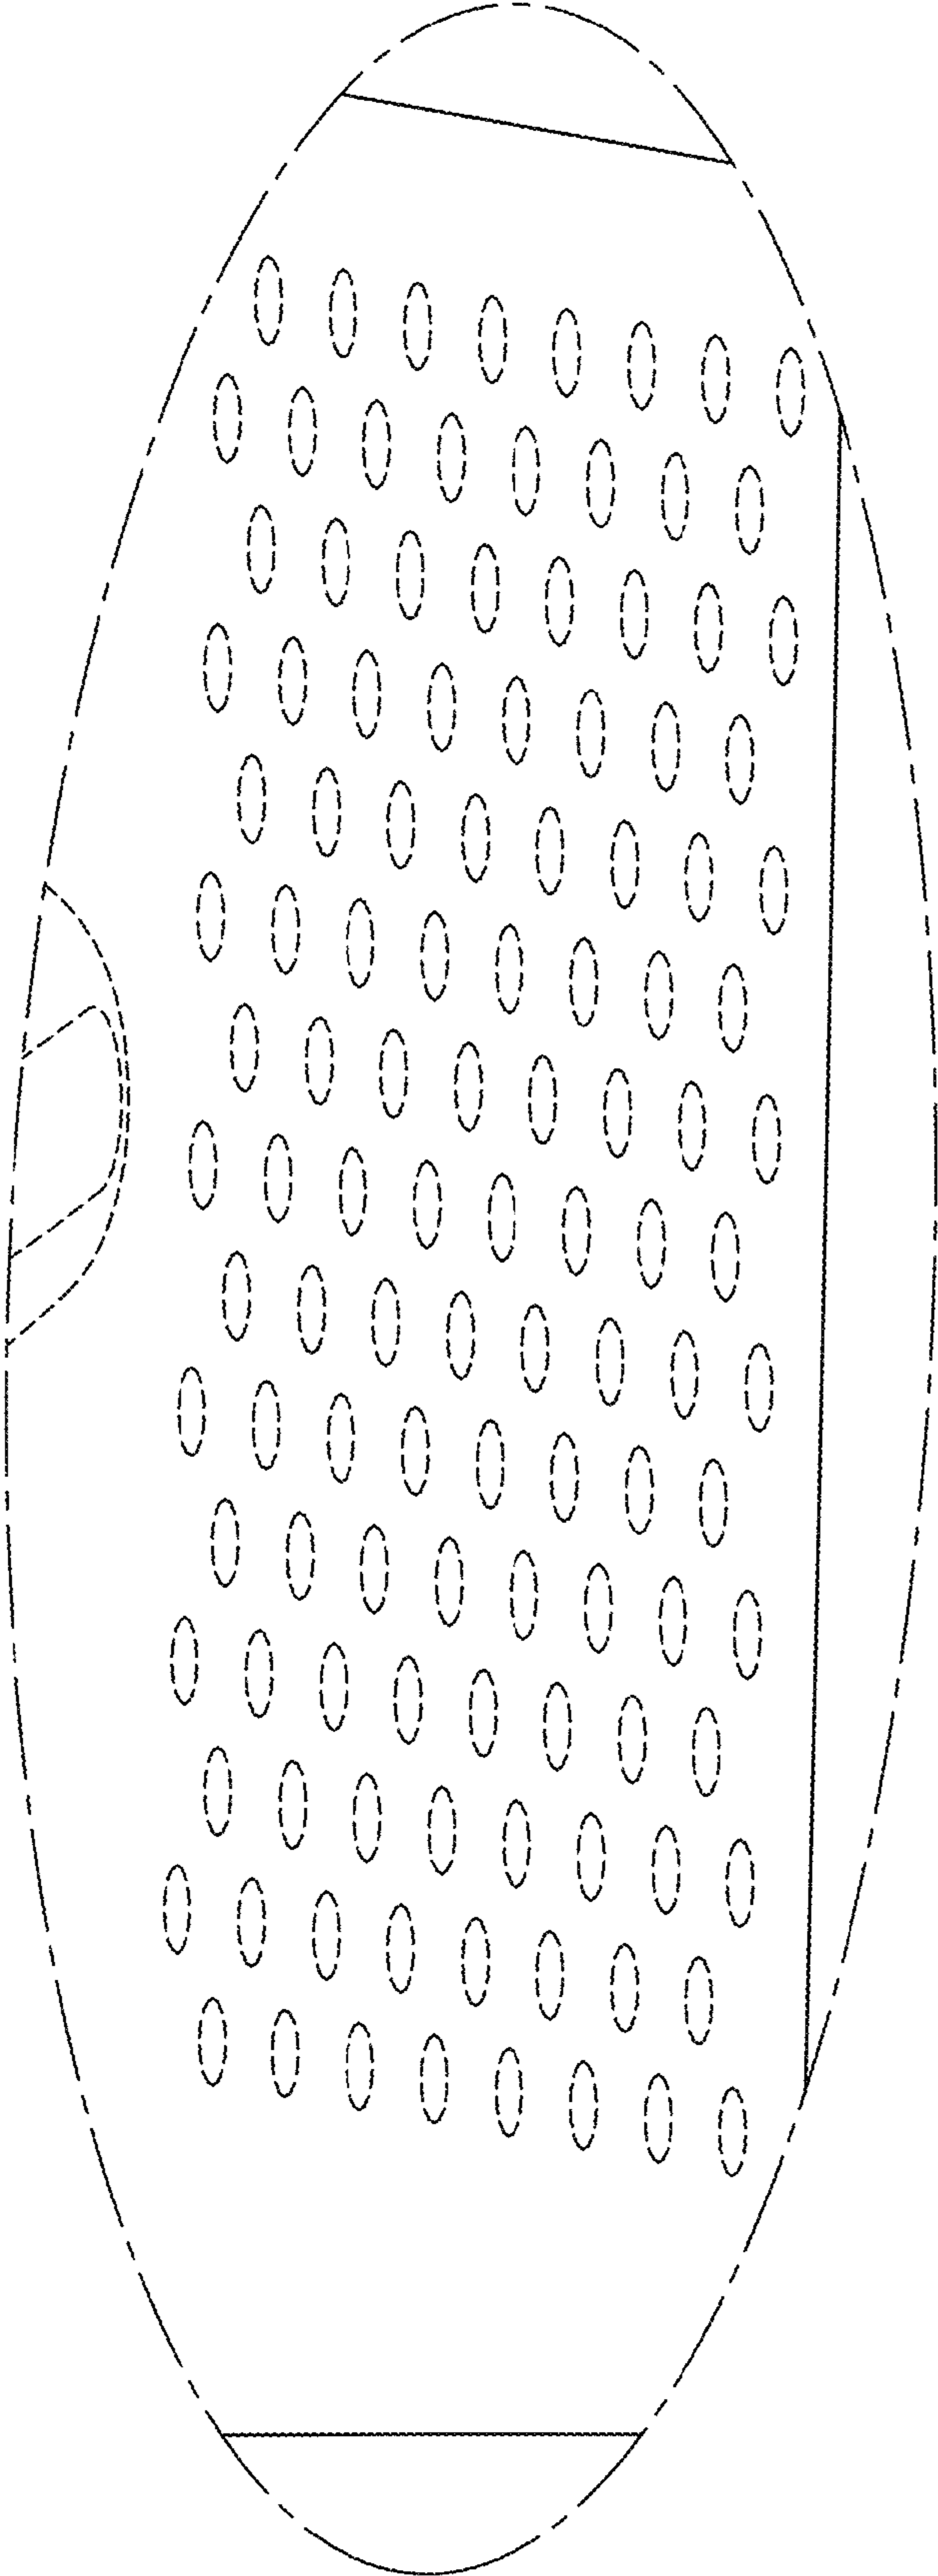


FIG.11

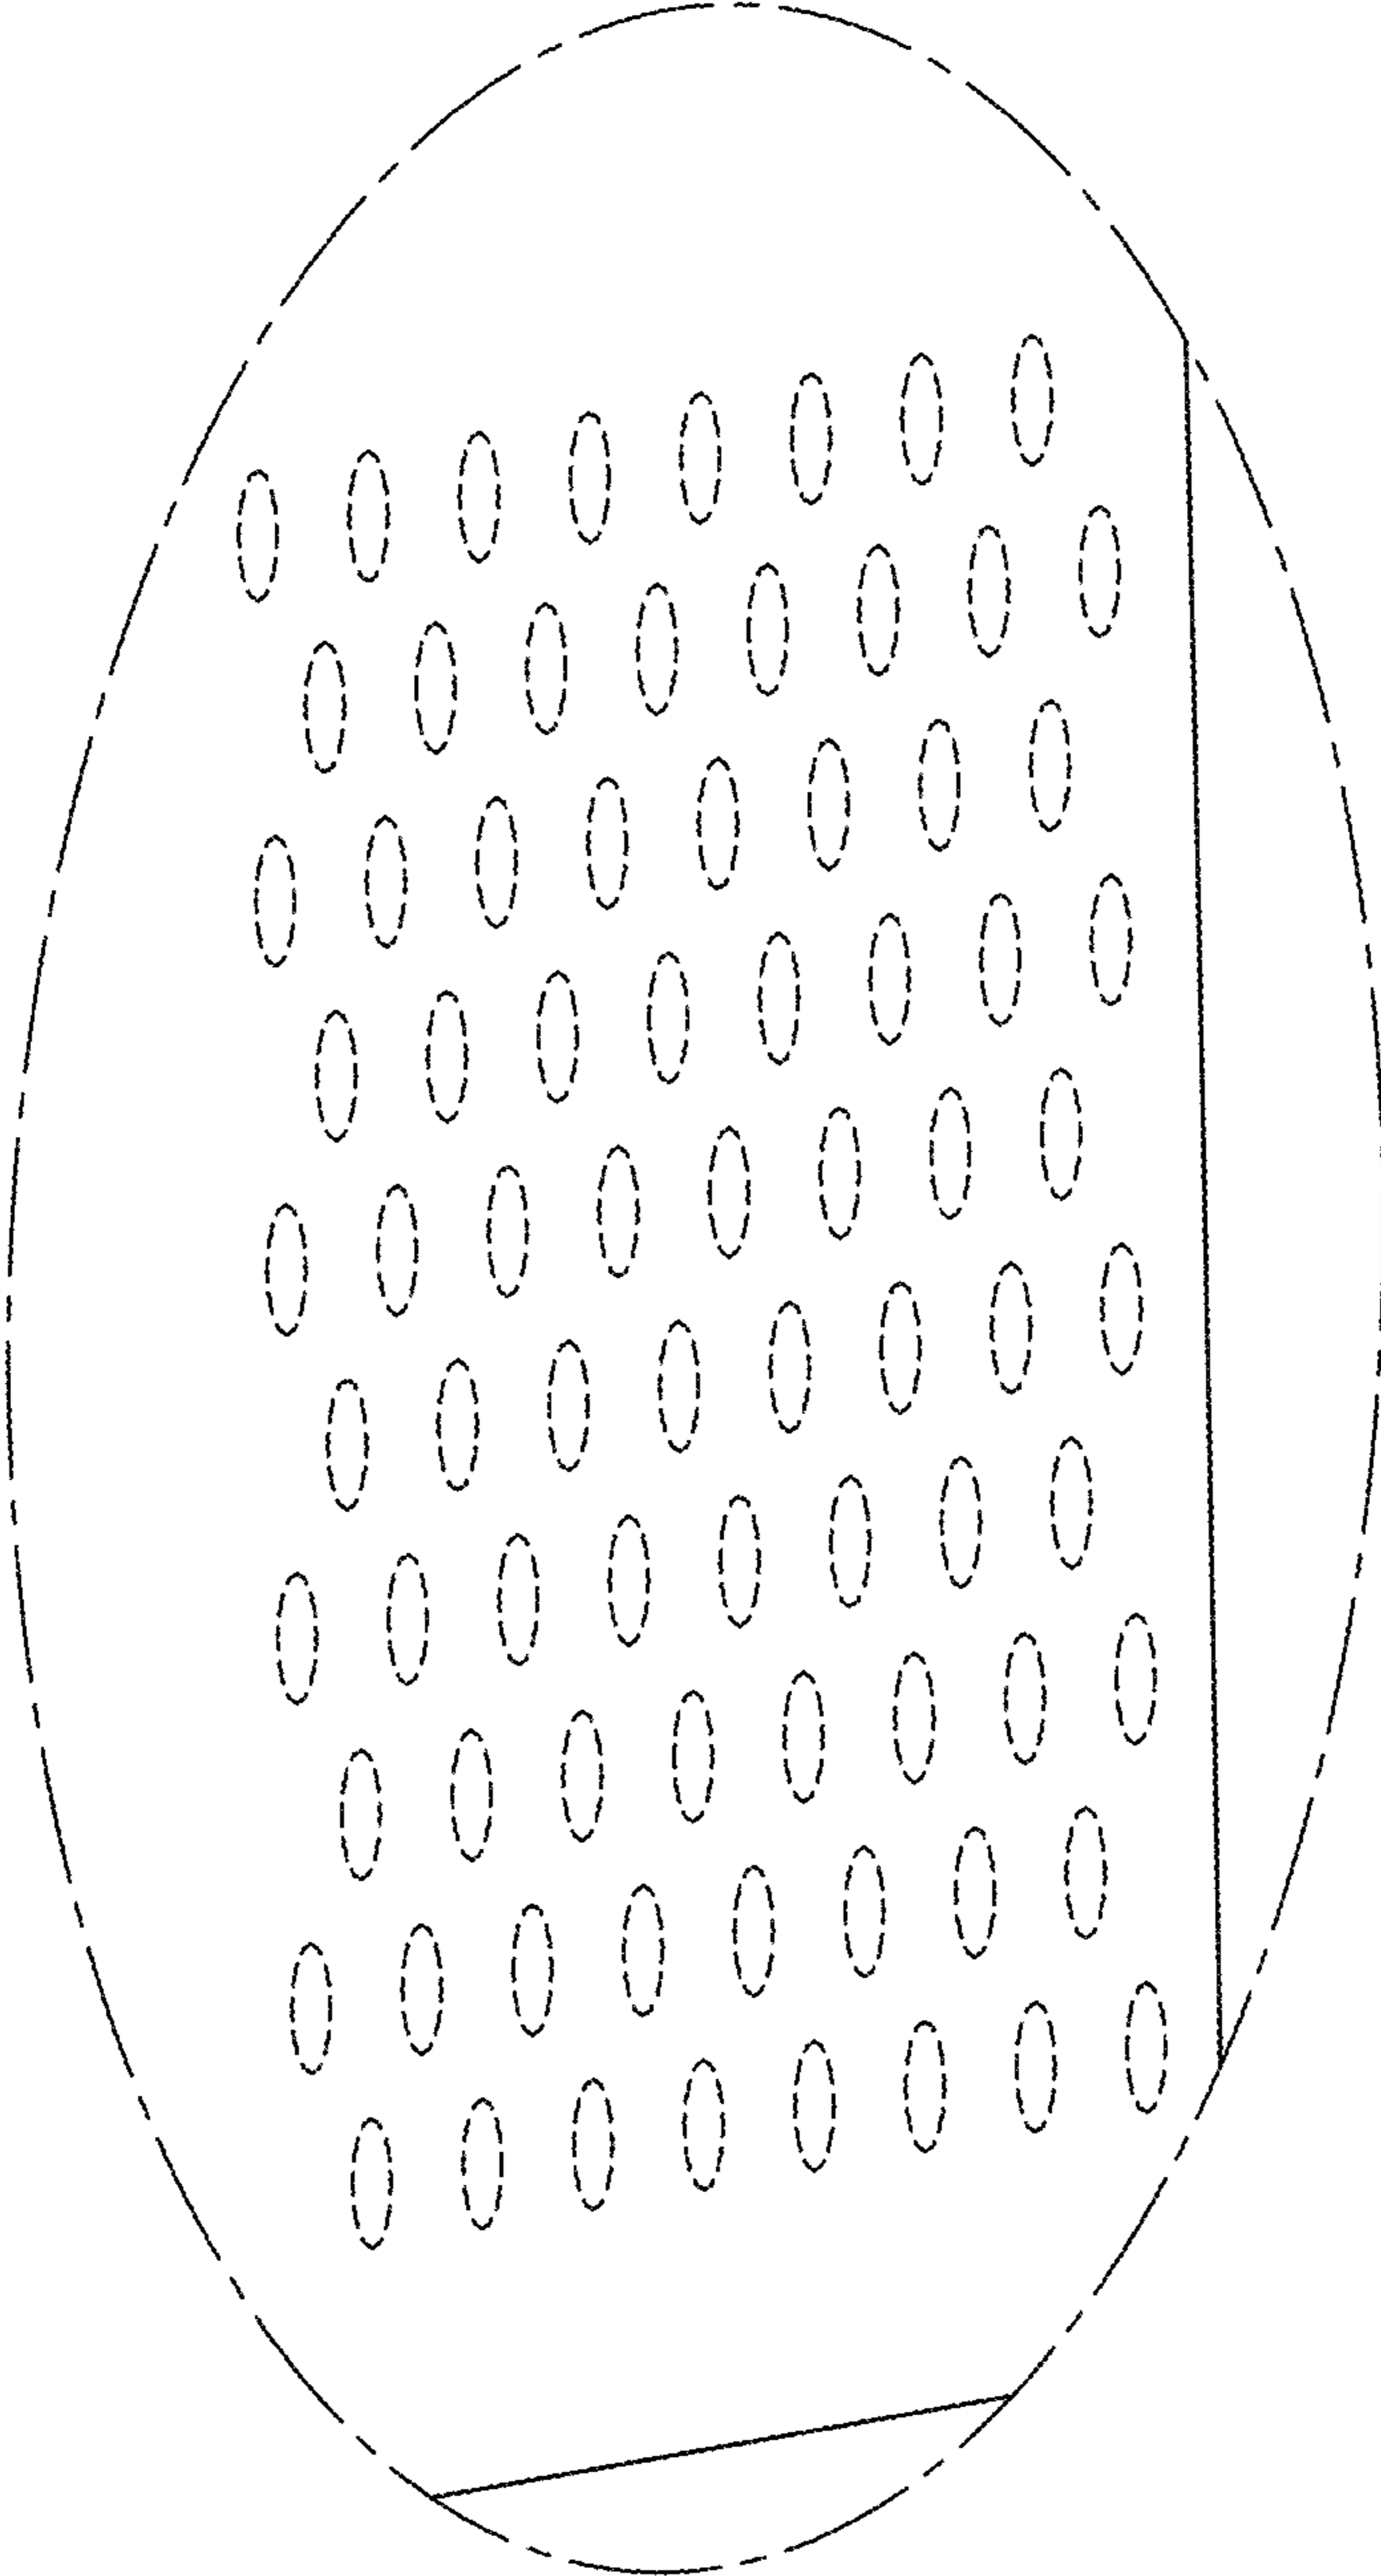


FIG.12