



US00D703332S

(12) **United States Design Patent**  
**Saeki**

(10) **Patent No.:** **US D703,332 S**

(45) **Date of Patent:** **\*\* Apr. 22, 2014**

(54) **ULTRASONIC PROBE**

(71) Applicant: **Nihon Dempa Kogyo Co., Ltd.**, Tokyo (JP)

(72) Inventor: **Isao Saeki**, Saitama (JP)

(73) Assignee: **Nihon Dempa Kogyo Co., Ltd.**, Tokyo (JP)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/464,691**

(22) Filed: **Aug. 20, 2013**

(30) **Foreign Application Priority Data**

Mar. 28, 2013 (JP) ..... 2013-006942

(51) **LOC (10) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/187**

(58) **Field of Classification Search**  
USPC ..... D24/138, 141, 158, 164, 165, 167, 170,  
D24/186-187, 133, 144; D10/57, 60, 78,  
D10/80; 600/407, 461, 446, 439; 378/98.7,  
378/98.8, 189  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D389,919 S \* 1/1998 Ninomiya et al. .... D24/186  
D390,959 S \* 2/1998 Mesaros et al. .... D24/186  
D392,044 S \* 3/1998 Mesaros et al. .... D24/186

5,897,503 A \* 4/1999 Lyon et al. .... 600/459  
6,436,050 B2 \* 8/2002 Garrison et al. .... 600/459  
D544,606 S 6/2007 Hasegawa et al.  
D545,433 S \* 6/2007 Messerly et al. .... D24/158  
D546,460 S 7/2007 Hasegawa  
D598,108 S 8/2009 Hasegawa  
D619,266 S \* 7/2010 Sakai ..... D24/186  
D639,434 S \* 6/2011 Wodecki et al. .... D24/160  
D681,824 S \* 5/2013 Shinohara et al. .... D24/186  
D681,825 S \* 5/2013 Shinohara et al. .... D24/186  
D681,828 S \* 5/2013 Shinohara et al. .... D24/186  
D682,433 S \* 5/2013 Shinohara et al. .... D24/186  
D688,376 S \* 8/2013 Bartlett ..... D24/187

\* cited by examiner

*Primary Examiner* — T. Chase Nelson

*Assistant Examiner* — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Edwards Wildman Palmer LLP; Scott D. Wofsy



(57) **CLAIM**

The ornamental design for an ultrasonic probe, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of the ultrasonic probe as viewed from above;  
FIG. 2 is a perspective view of the ultrasonic probe as viewed from below;  
FIG. 3 is a front elevation view of the ultrasonic probe;  
FIG. 4 is a left side elevation view of the ultrasonic probe;  
FIG. 5 is a right side elevation view of the ultrasonic probe;  
FIG. 6 is a top plan view of the ultrasonic probe; and,  
FIG. 7 is a bottom plan view of the ultrasonic probe.

**1 Claim, 4 Drawing Sheets**

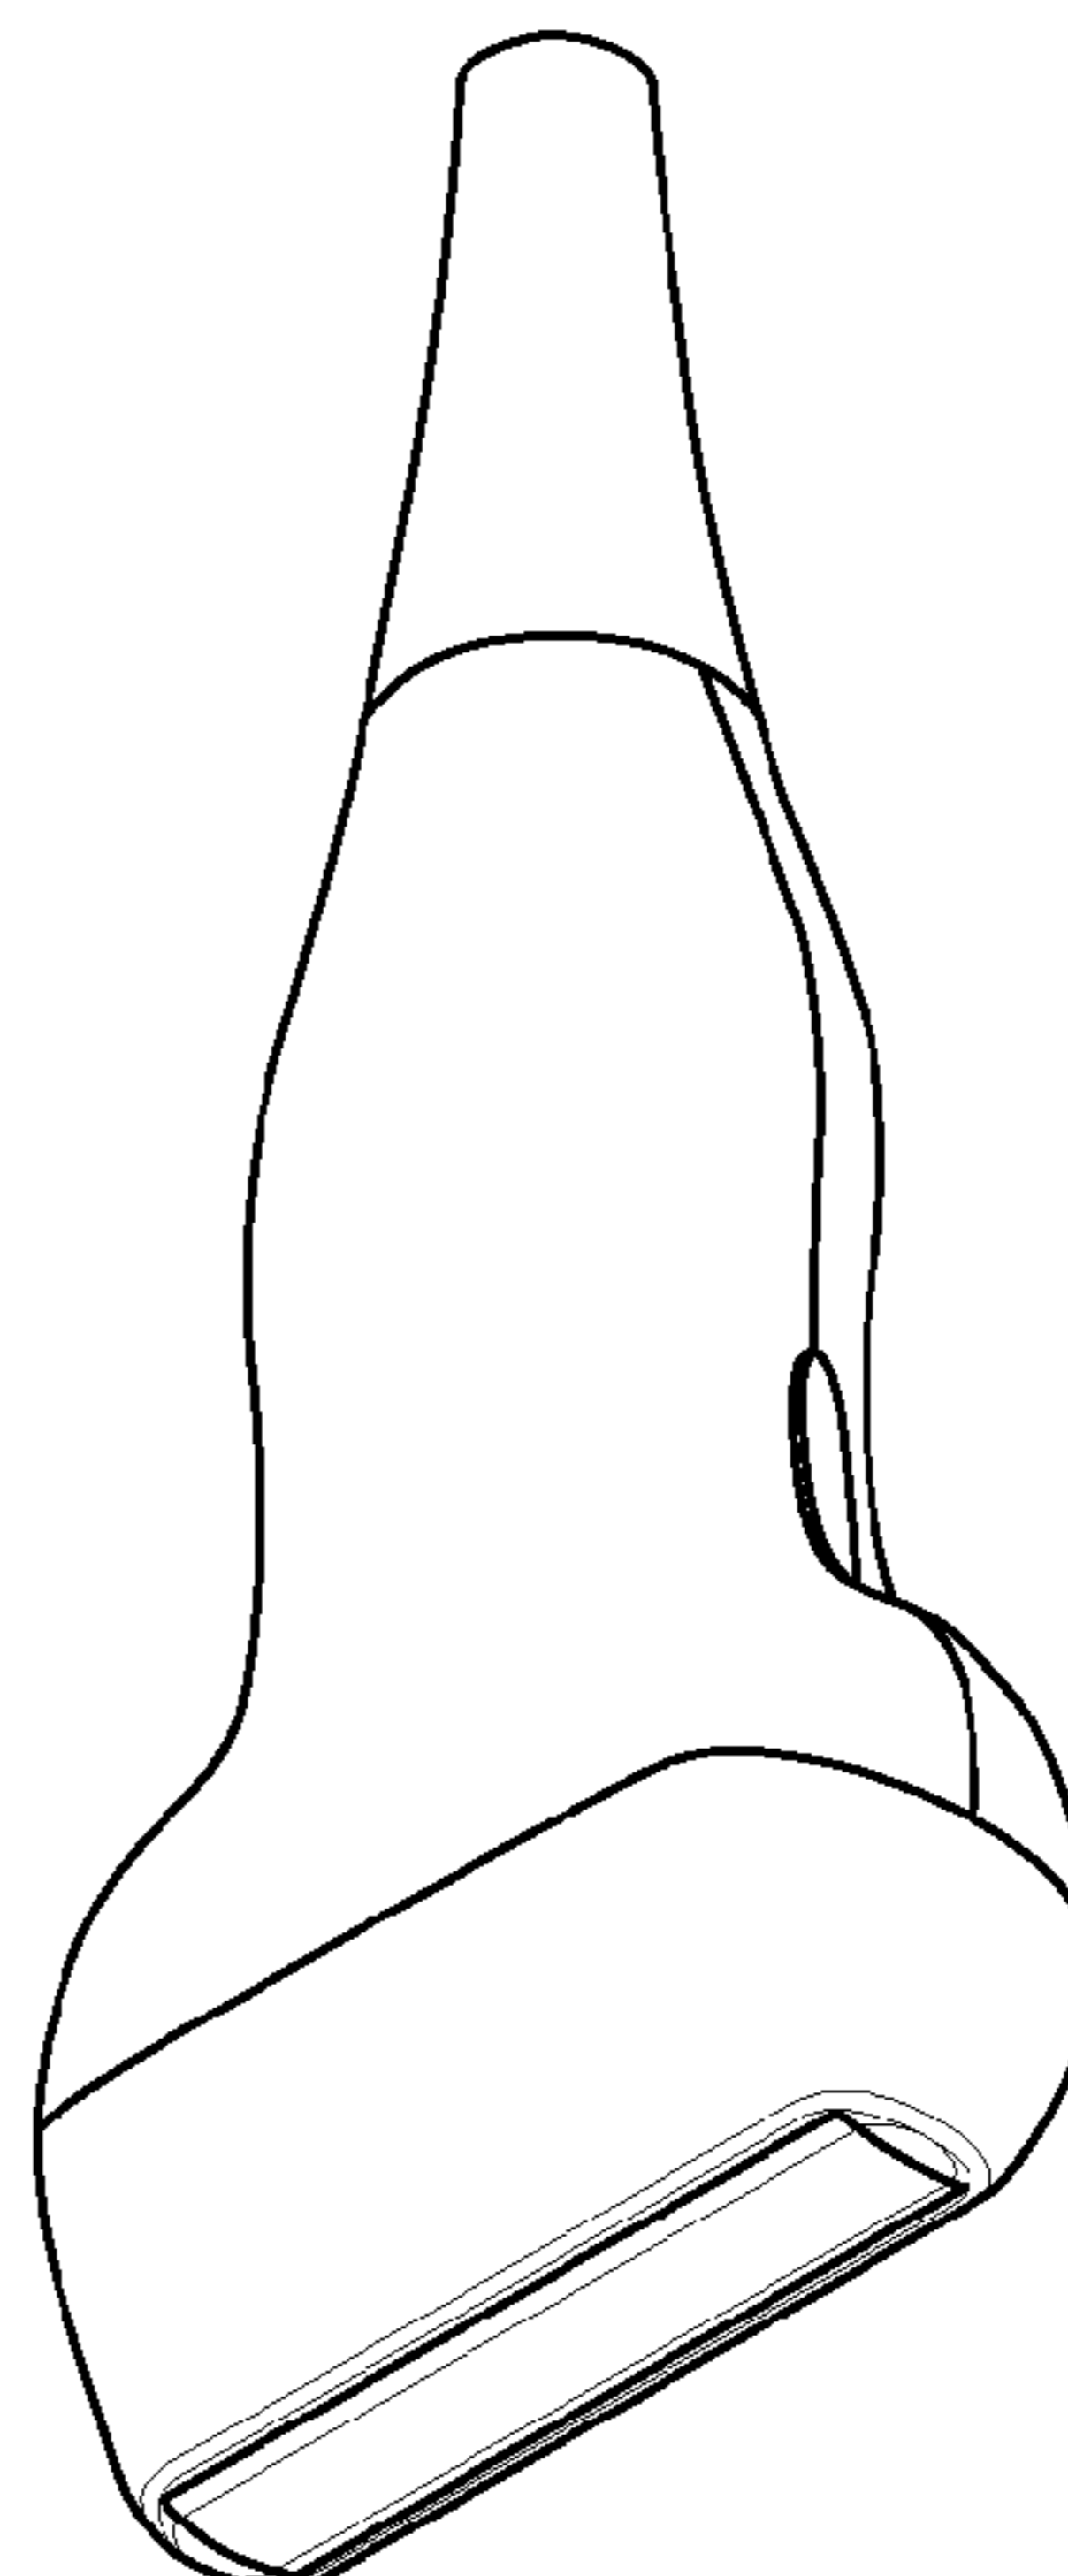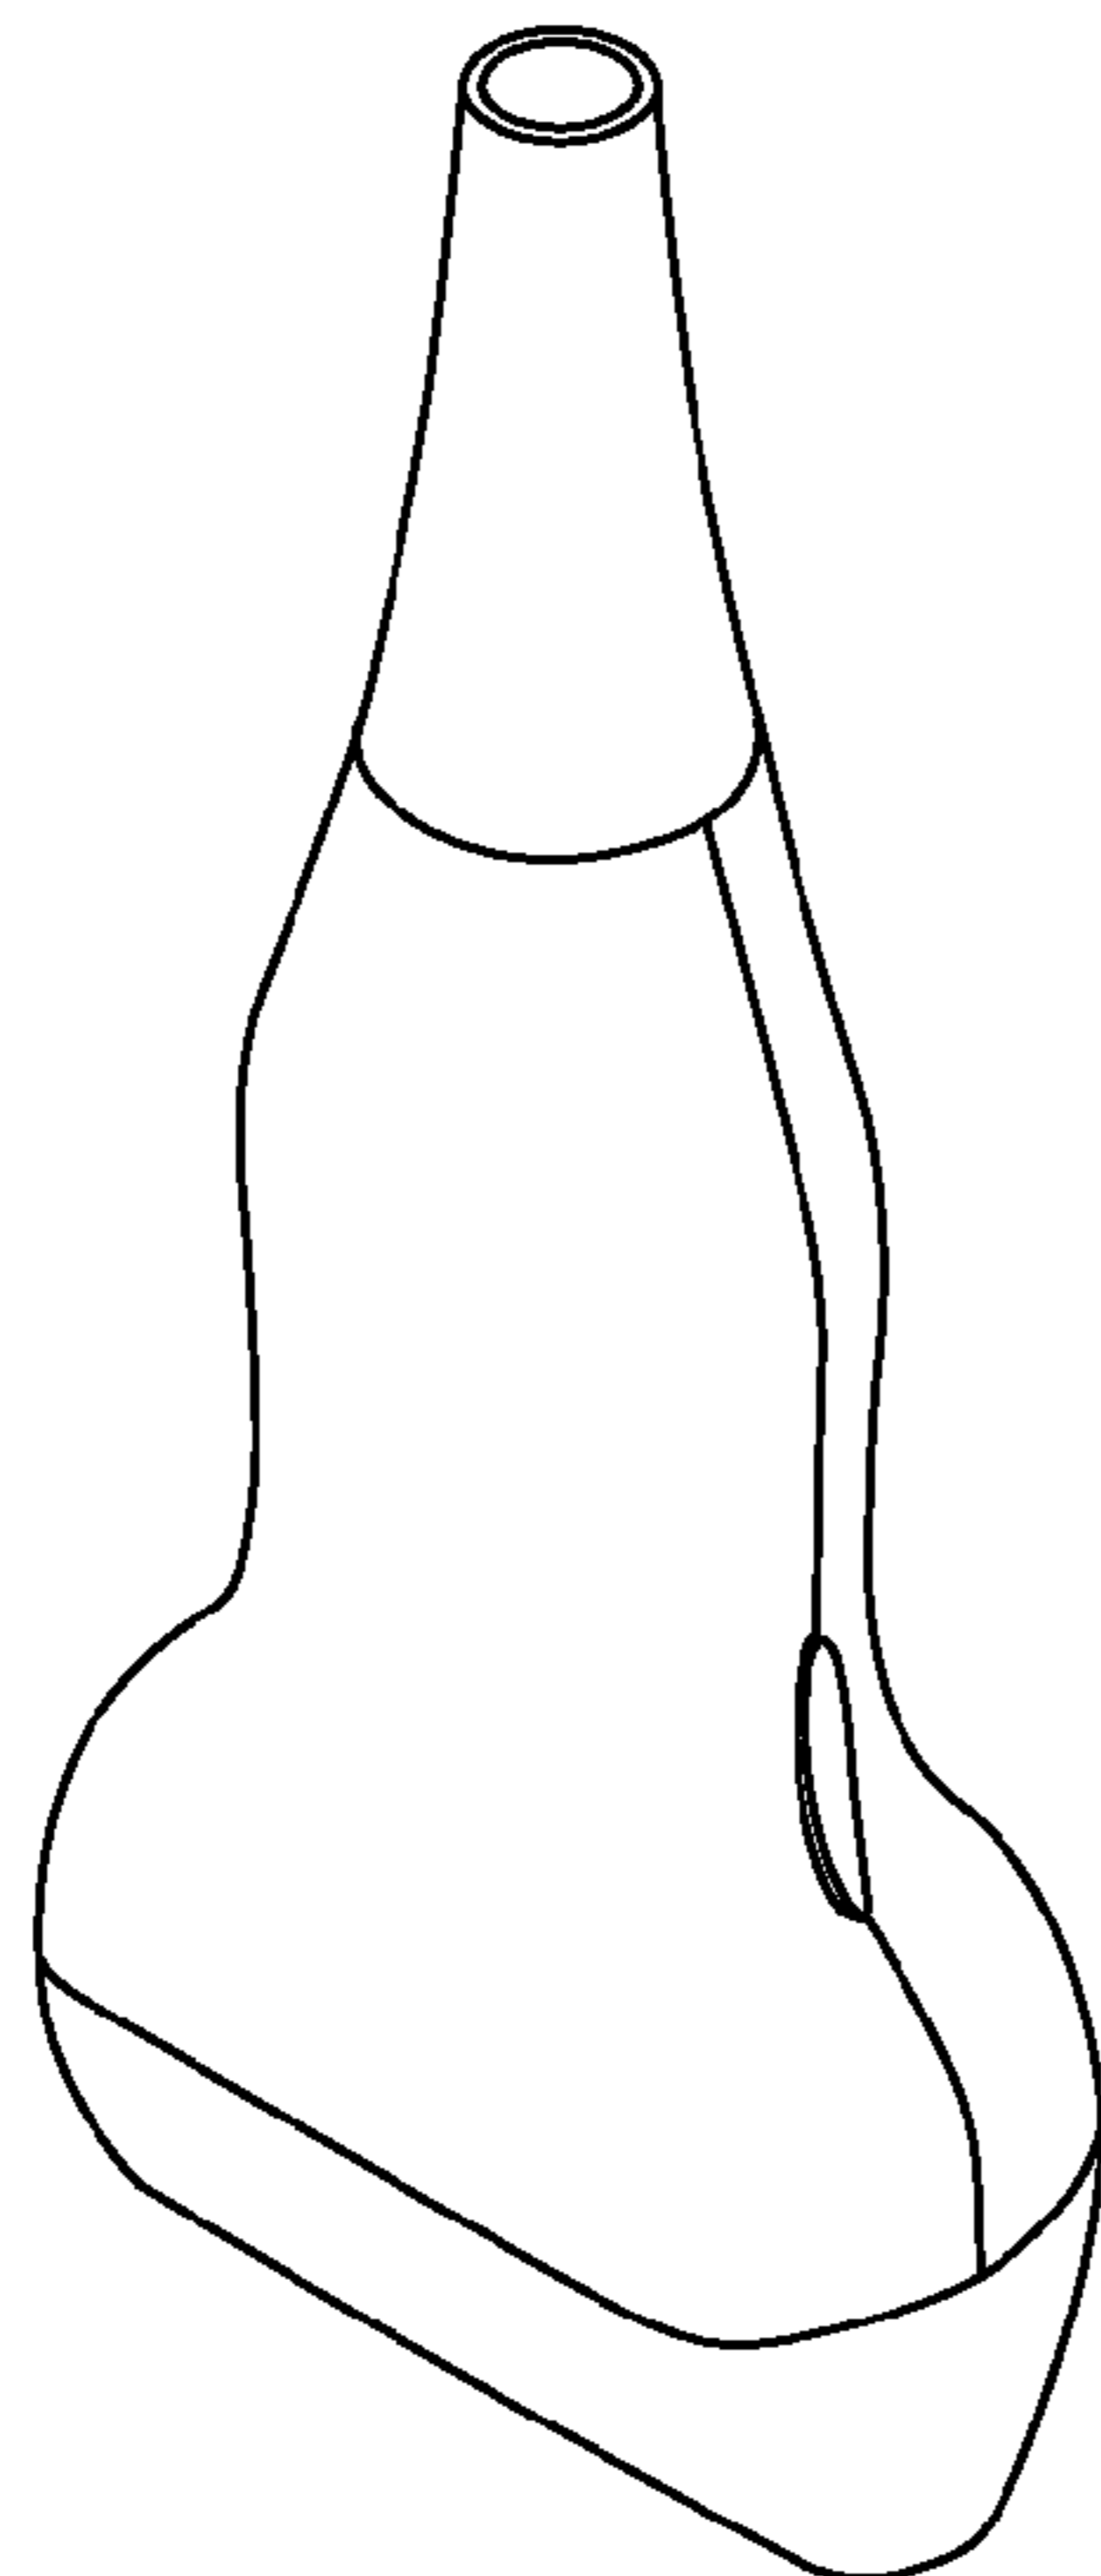

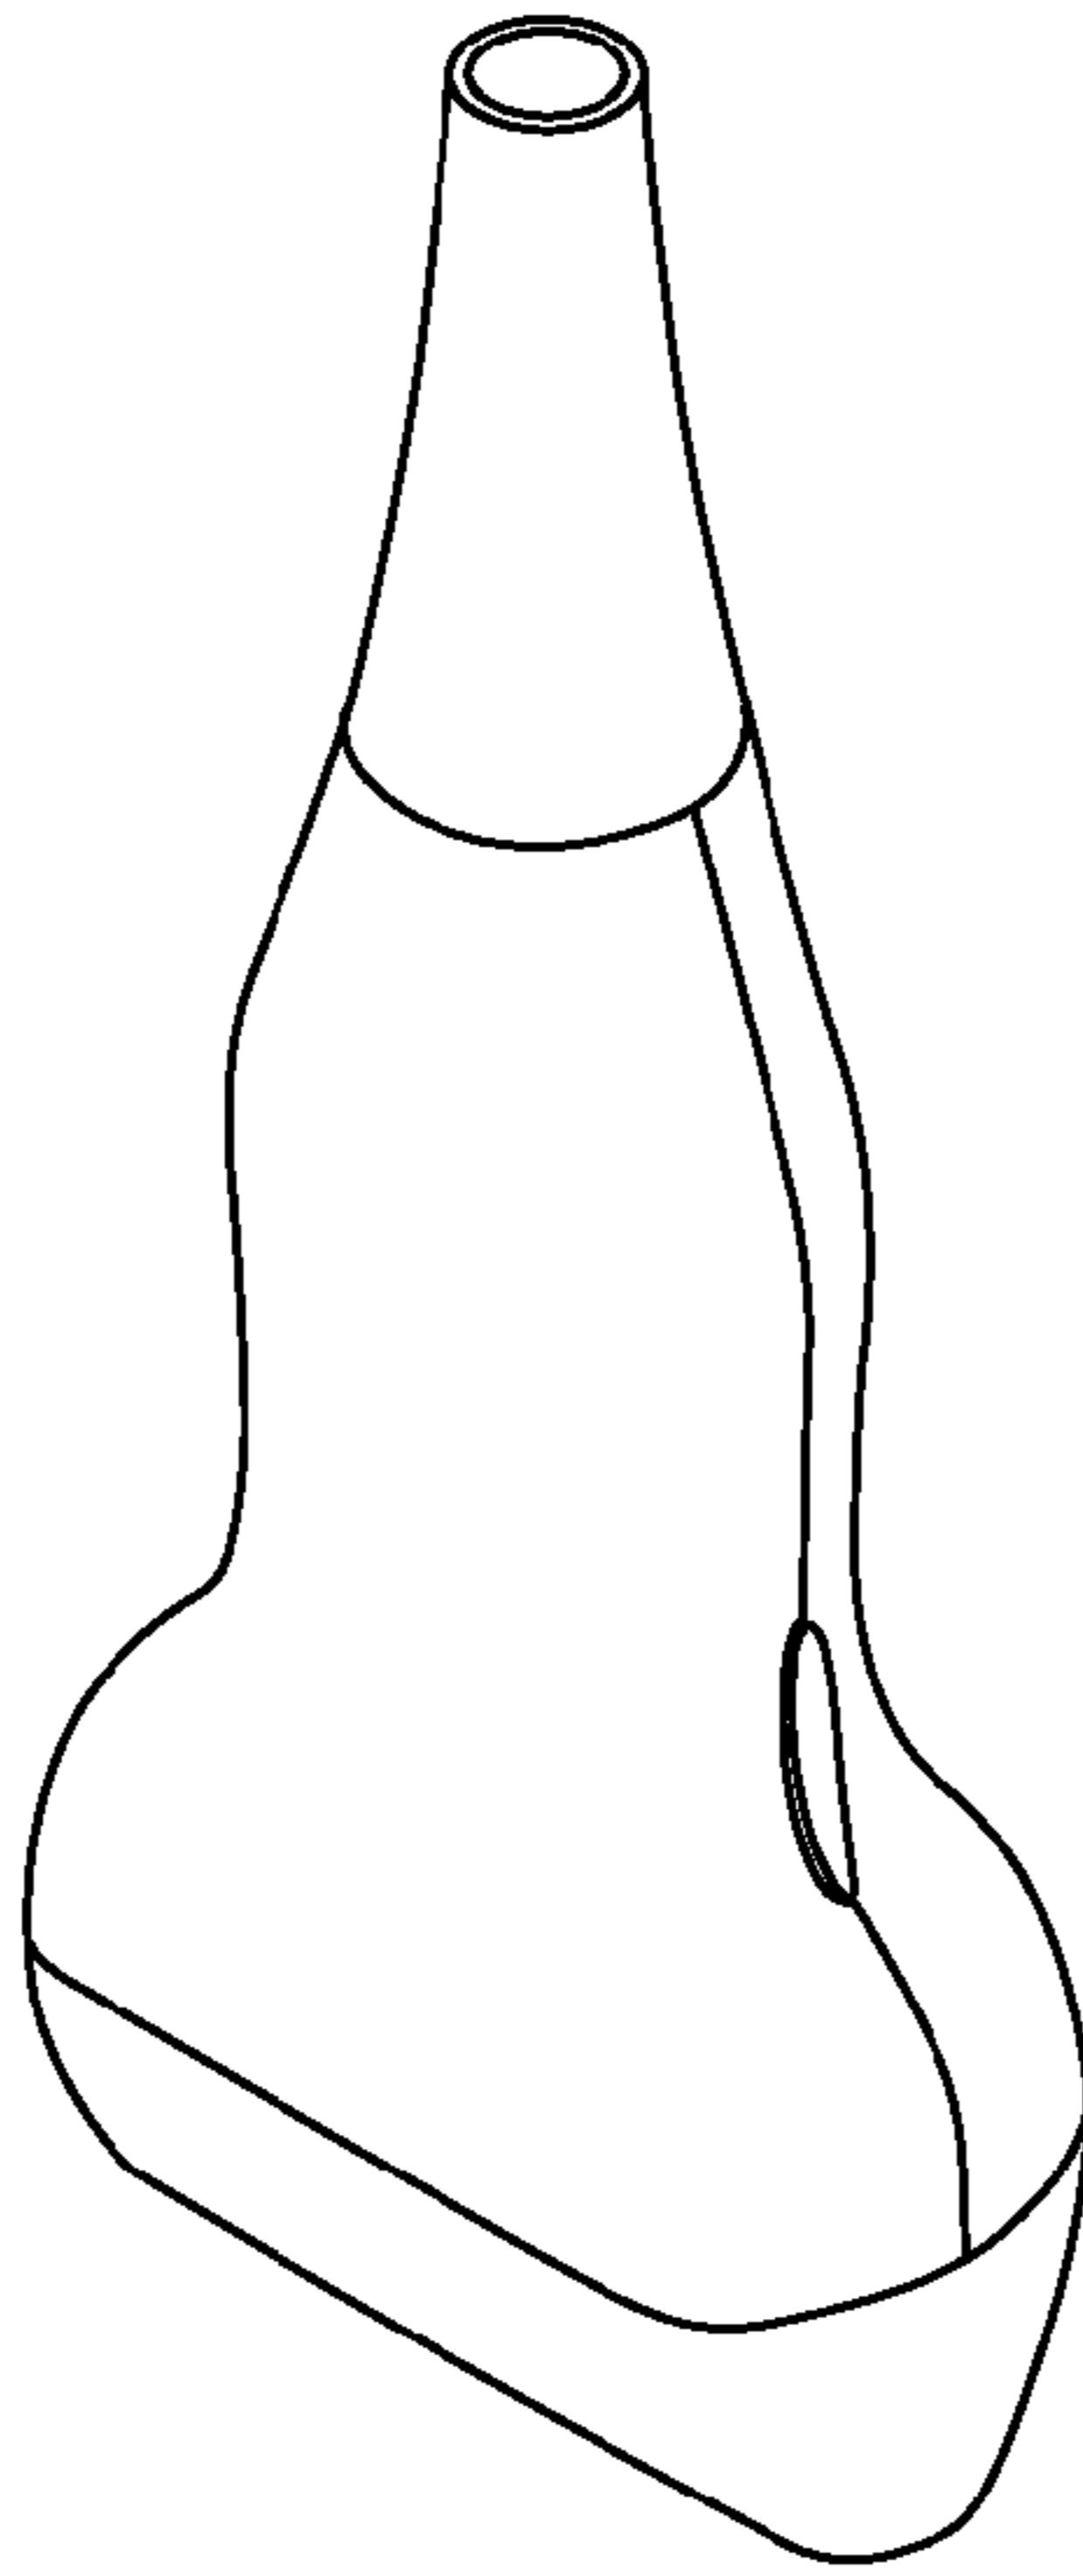


FIG. 1

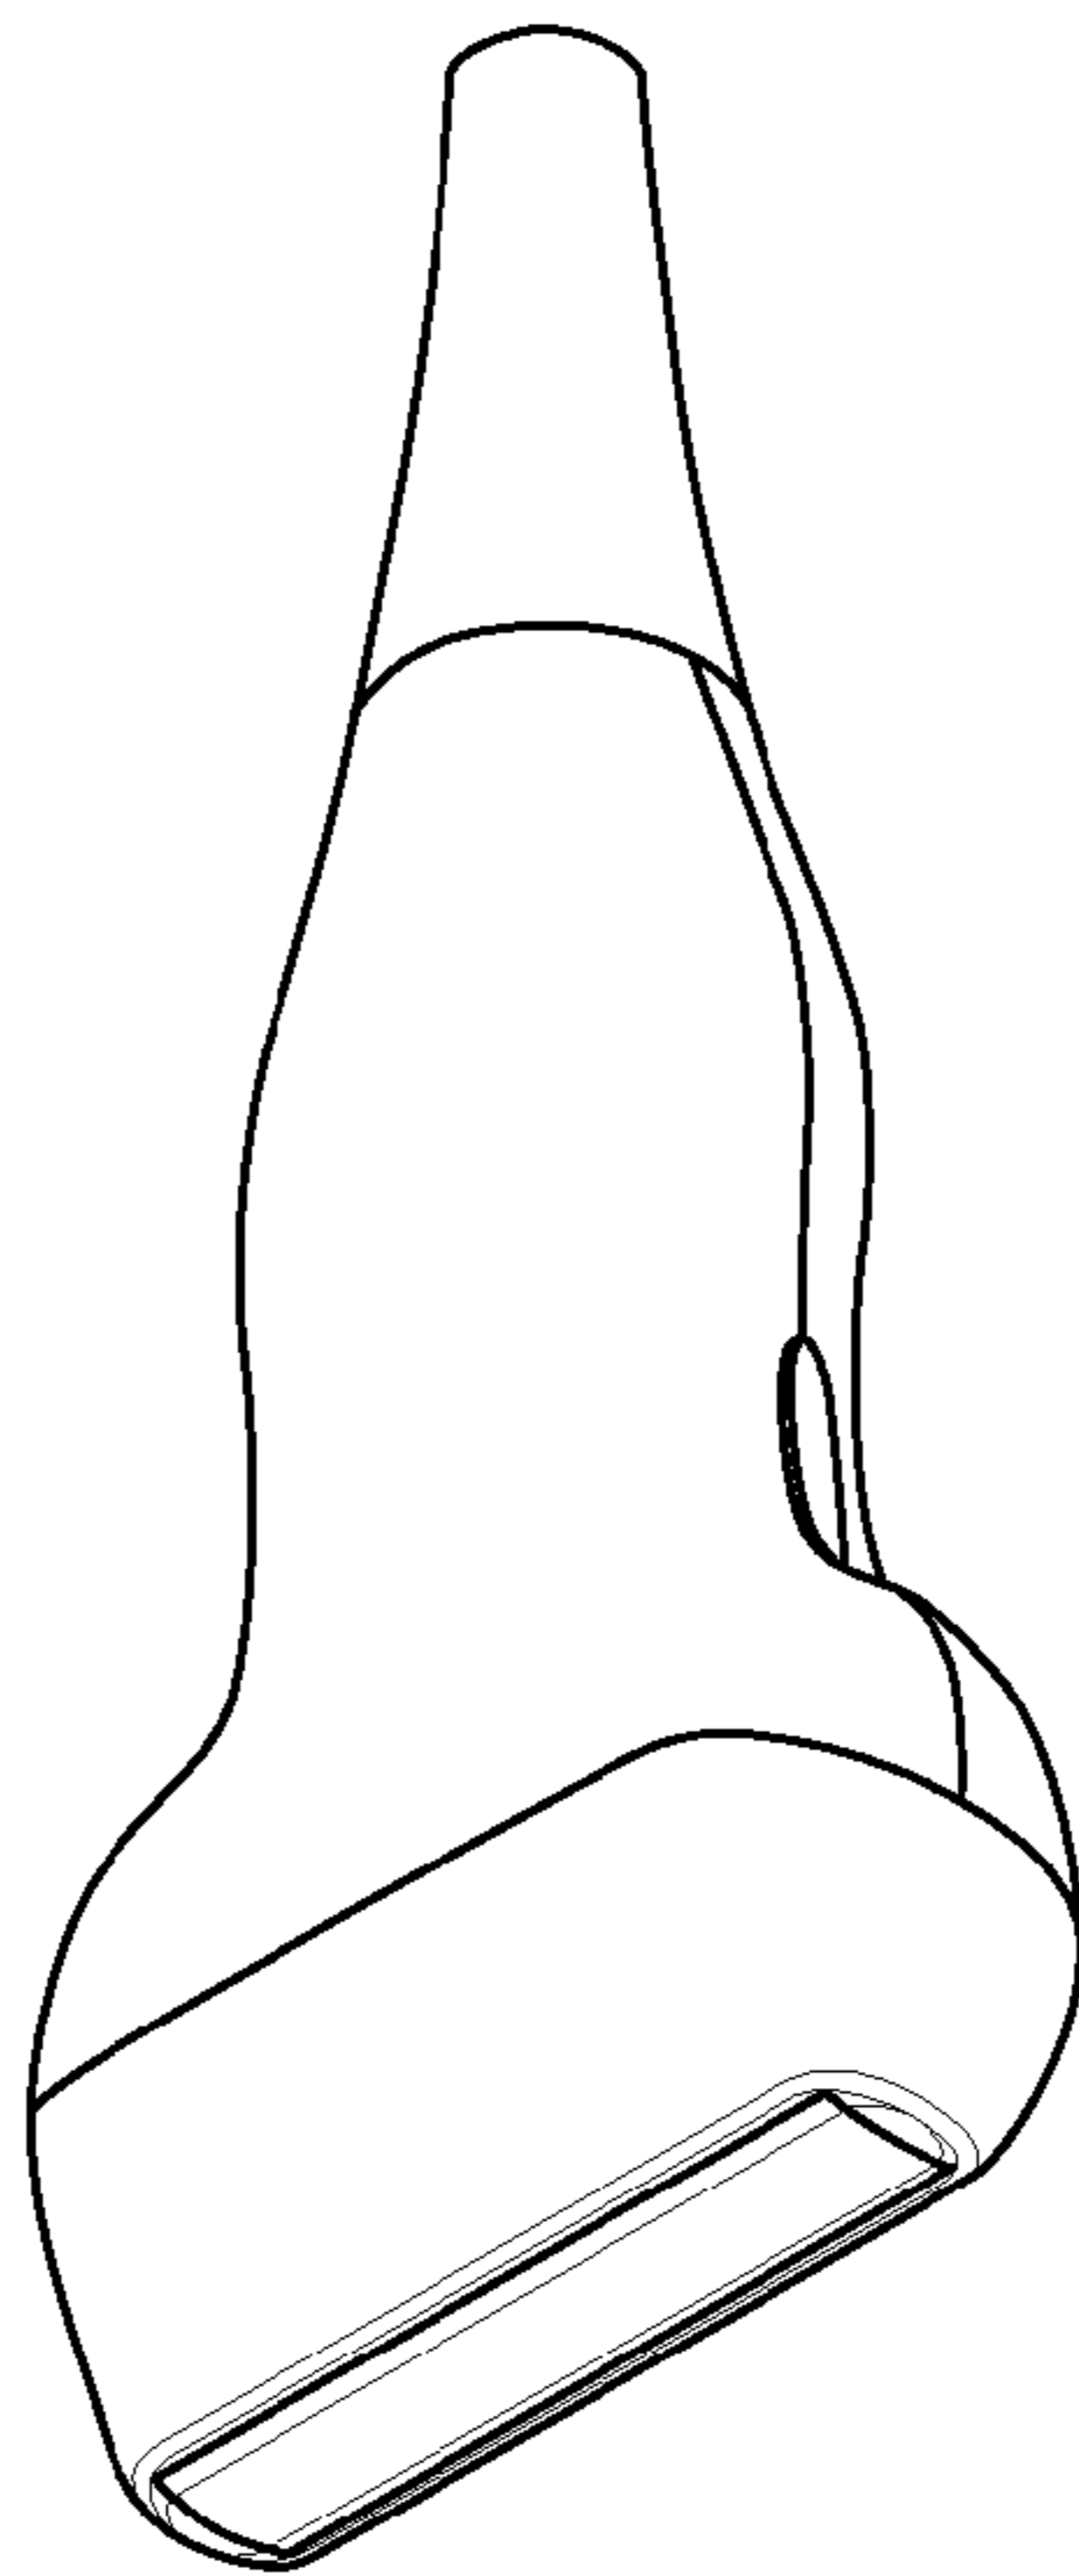


FIG. 2

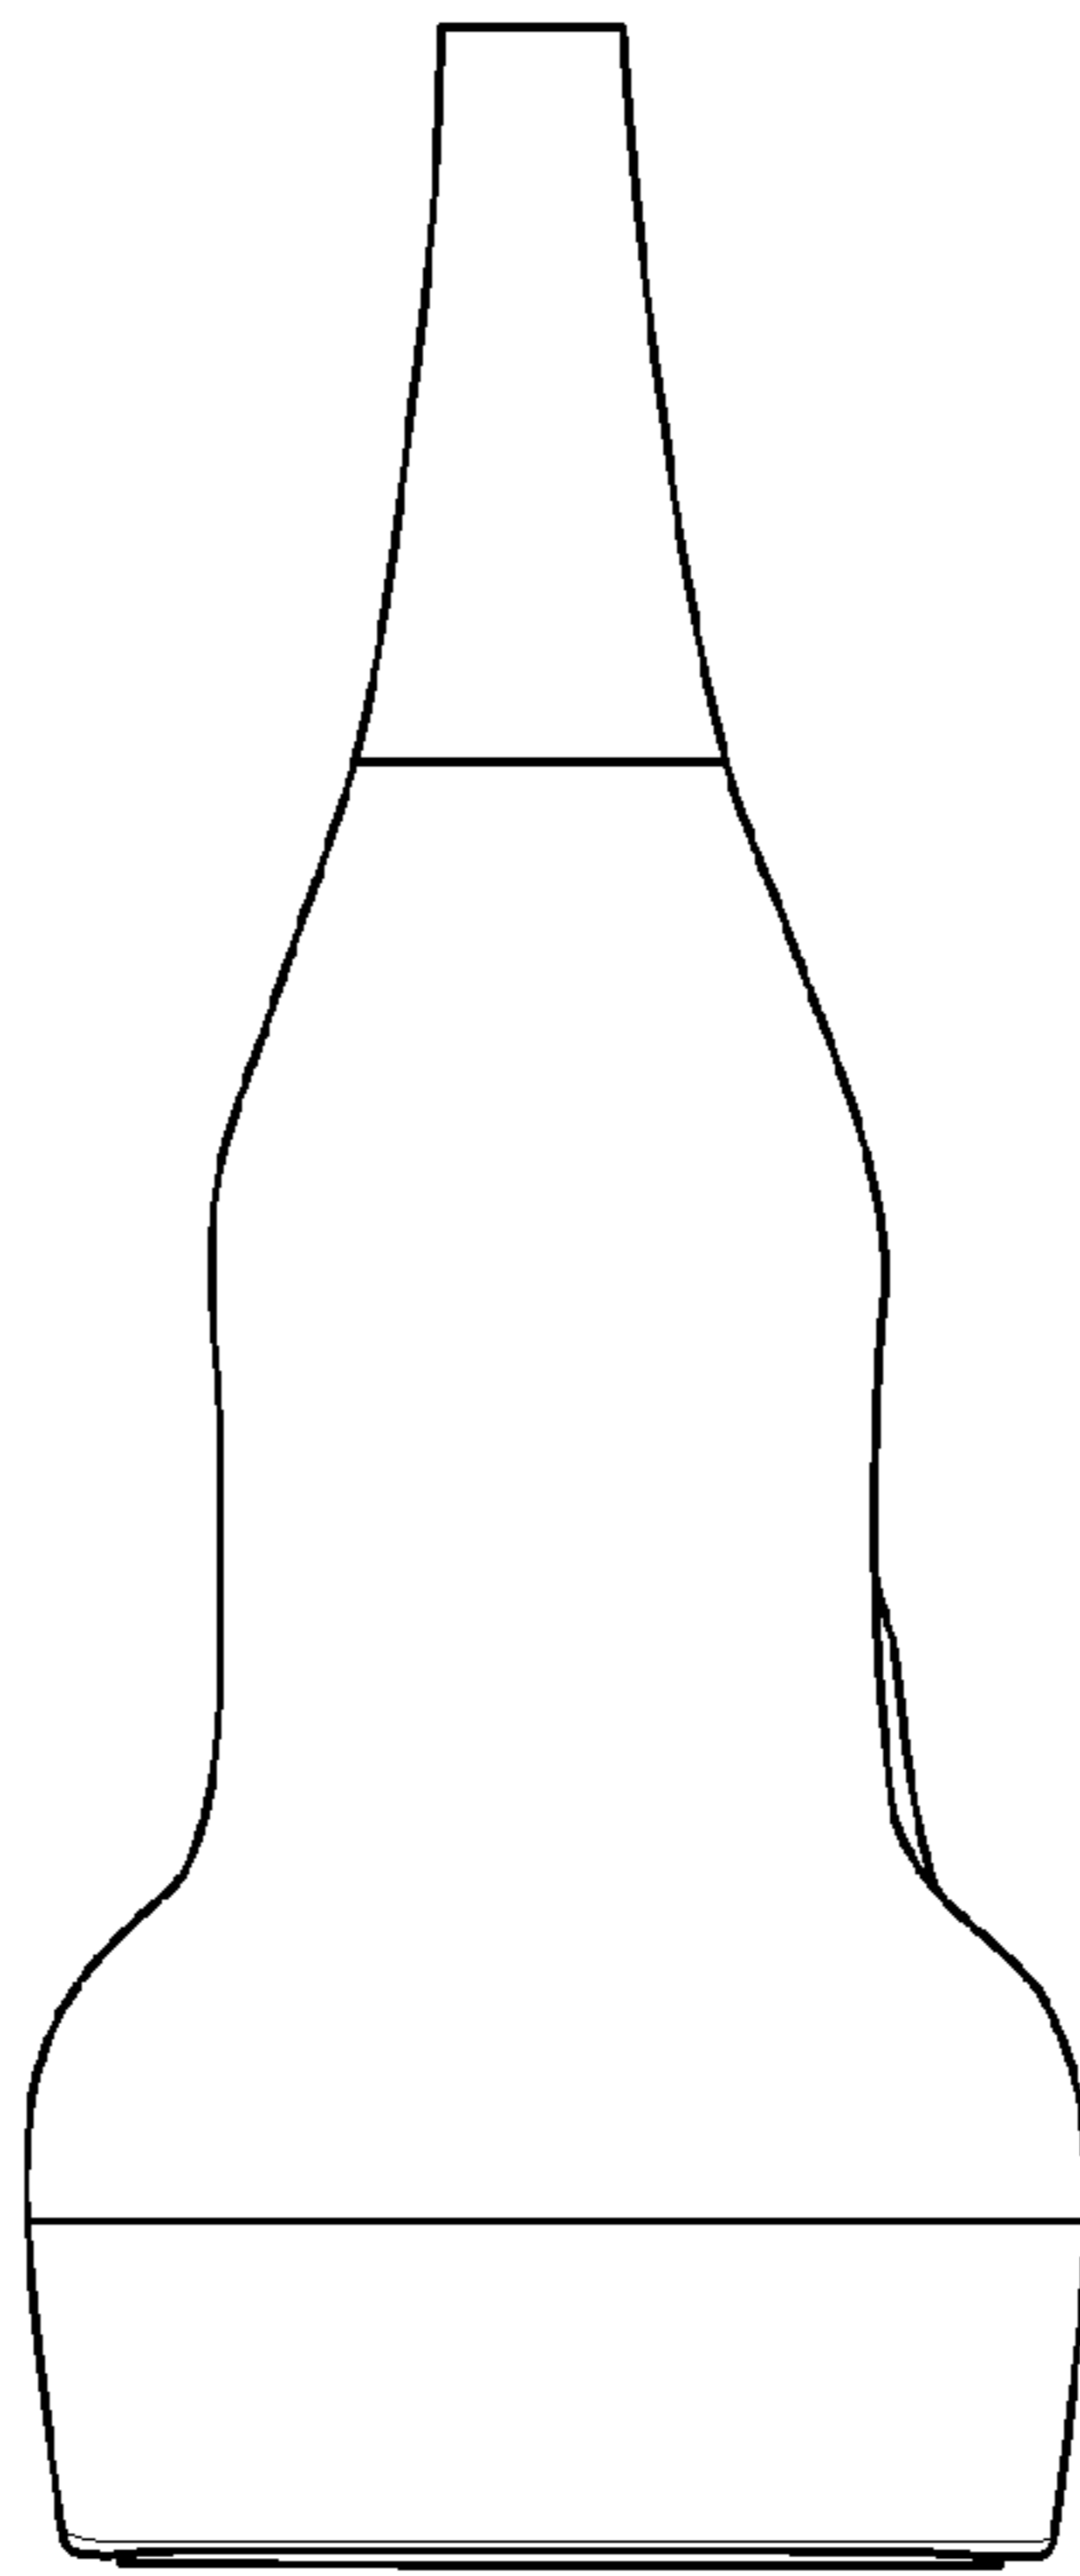


FIG.3

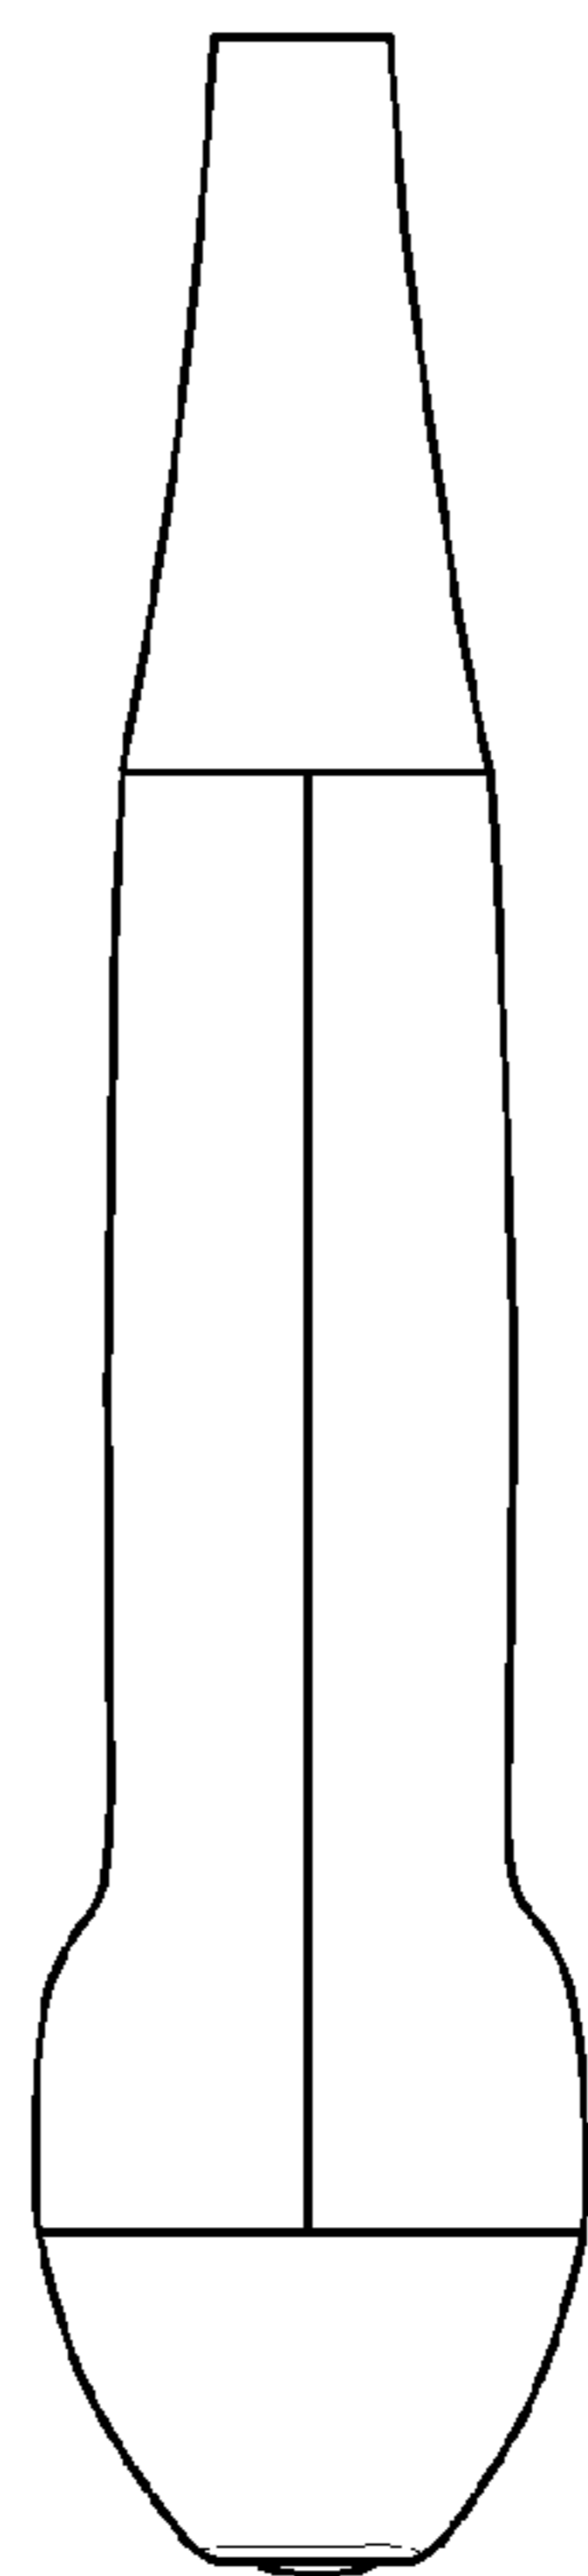


FIG.4

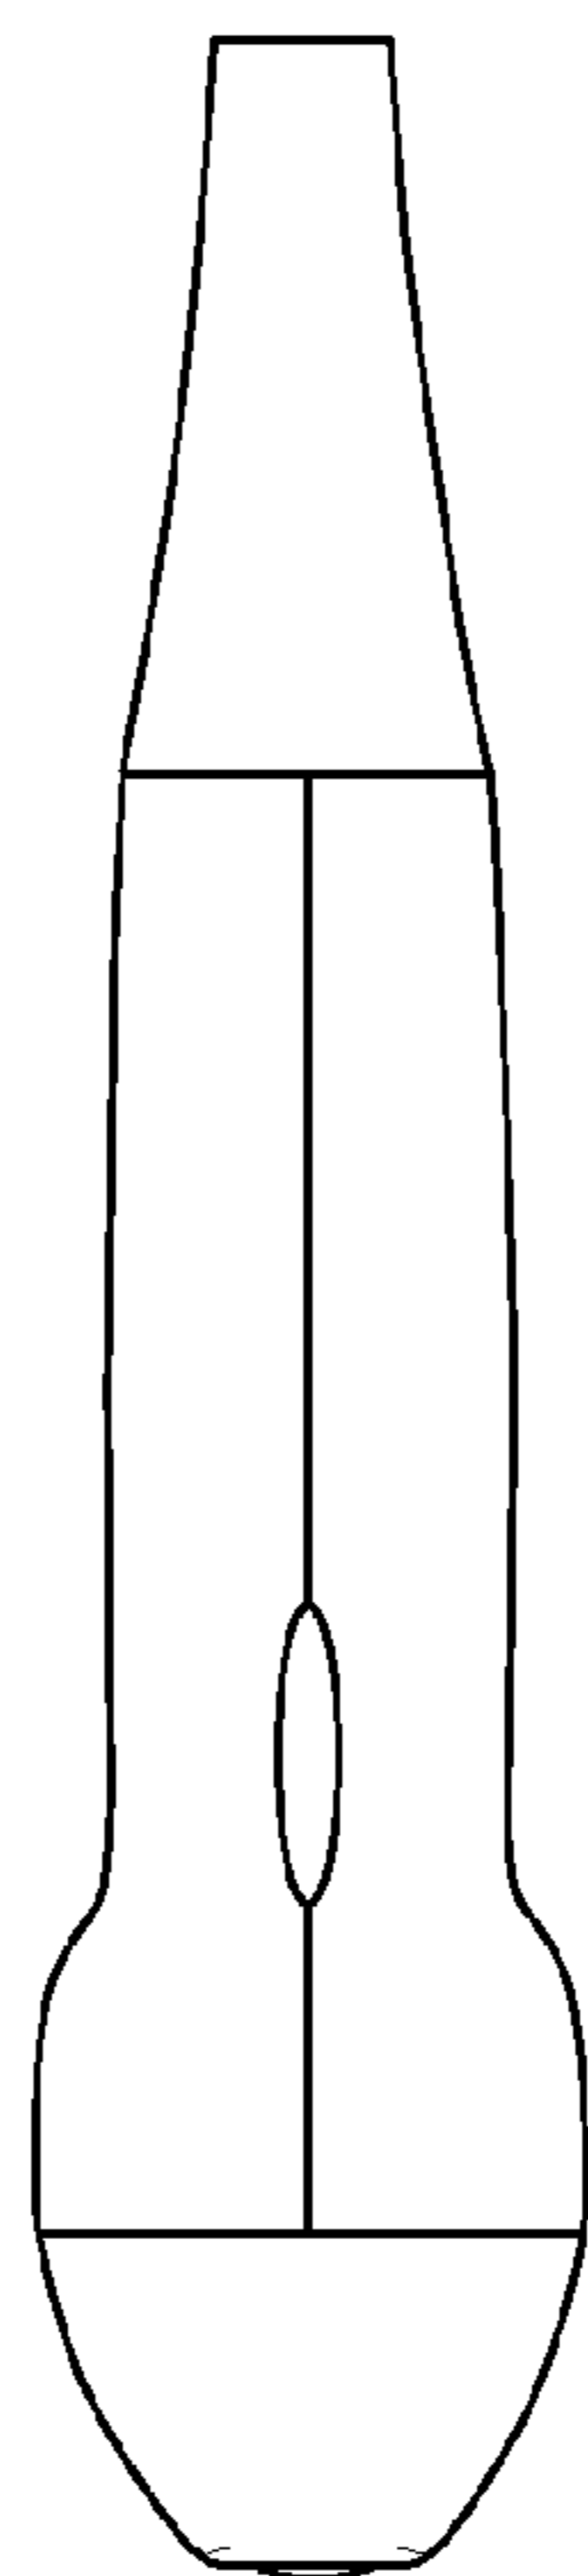


FIG.5

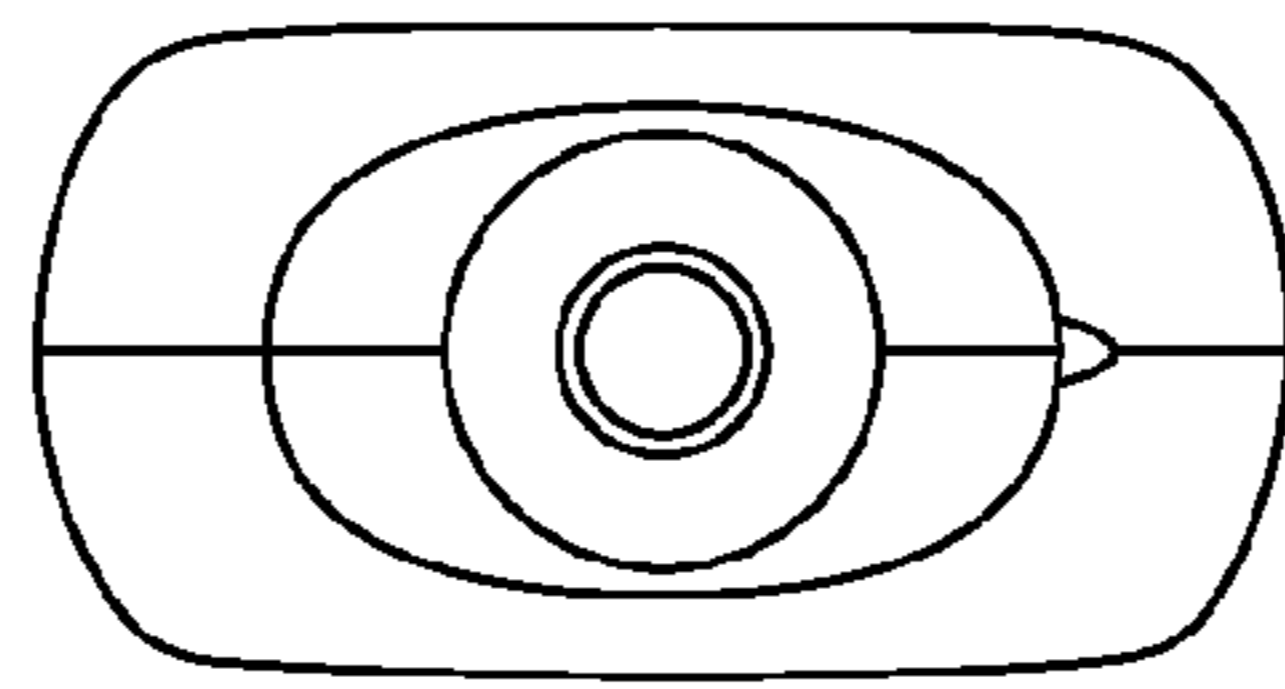


FIG. 6

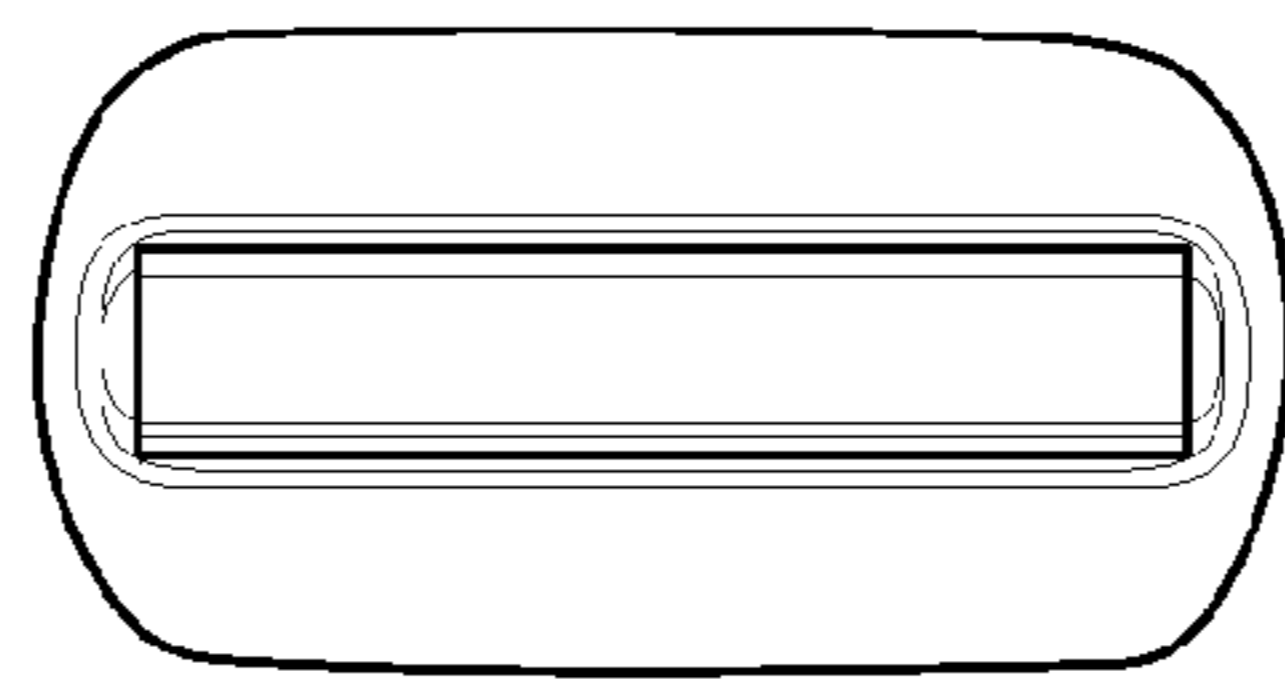


FIG. 7