



US00D703332S

(12) **United States Design Patent**
Saeki

(10) **Patent No.:** **US D703,332 S**
(45) **Date of Patent:** **** Apr. 22, 2014**

(54) **ULTRASONIC PROBE**

(71) Applicant: **Nihon Dempa Kogyo Co., Ltd.**, Tokyo (JP)

(72) Inventor: **Isao Saeki**, Saitama (JP)

(73) Assignee: **Nihon Dempa Kogyo Co., Ltd.**, Tokyo (JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/464,691**

(22) Filed: **Aug. 20, 2013**

(30) **Foreign Application Priority Data**

Mar. 28, 2013 (JP) 2013-006942

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/187**

(58) **Field of Classification Search**

USPC D24/138, 141, 158, 164, 165, 167, 170,
D24/186-187, 133, 144; D10/57, 60, 78,
D10/80; 600/407, 461, 446, 439; 378/98.7,
378/98.8, 189

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D389,919 S * 1/1998 Ninomiya et al. D24/186
D390,959 S * 2/1998 Mesaros et al. D24/186
D392,044 S * 3/1998 Mesaros et al. D24/186

5,897,503 A * 4/1999 Lyon et al. 600/459
6,436,050 B2 * 8/2002 Garrison et al. 600/459
D544,606 S 6/2007 Hasegawa et al.
D545,433 S * 6/2007 Messerly et al. D24/158
D546,460 S 7/2007 Hasegawa
D598,108 S 8/2009 Hasegawa
D619,266 S * 7/2010 Sakai D24/186
D639,434 S * 6/2011 Wodecki et al. D24/160
D681,824 S * 5/2013 Shinohara et al. D24/186
D681,825 S * 5/2013 Shinohara et al. D24/186
D681,828 S * 5/2013 Shinohara et al. D24/186
D682,433 S * 5/2013 Shinohara et al. D24/186
D688,376 S * 8/2013 Bartlett D24/187

* cited by examiner

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Edwards Wildman Palmer LLP; Scott D. Wofsy

(57) **CLAIM**

The ornamental design for an ultrasonic probe, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the ultrasonic probe as viewed from above;

FIG. 2 is a perspective view of the ultrasonic probe as viewed from below;

FIG. 3 is a front elevation view of the ultrasonic probe;



FIG. 4 is a left side elevation view of the ultrasonic probe;

FIG. 5 is a right side elevation view of the ultrasonic probe;

FIG. 6 is a top plan view of the ultrasonic probe; and,

FIG. 7 is a bottom plan view of the ultrasonic probe.

1 Claim, 4 Drawing Sheets

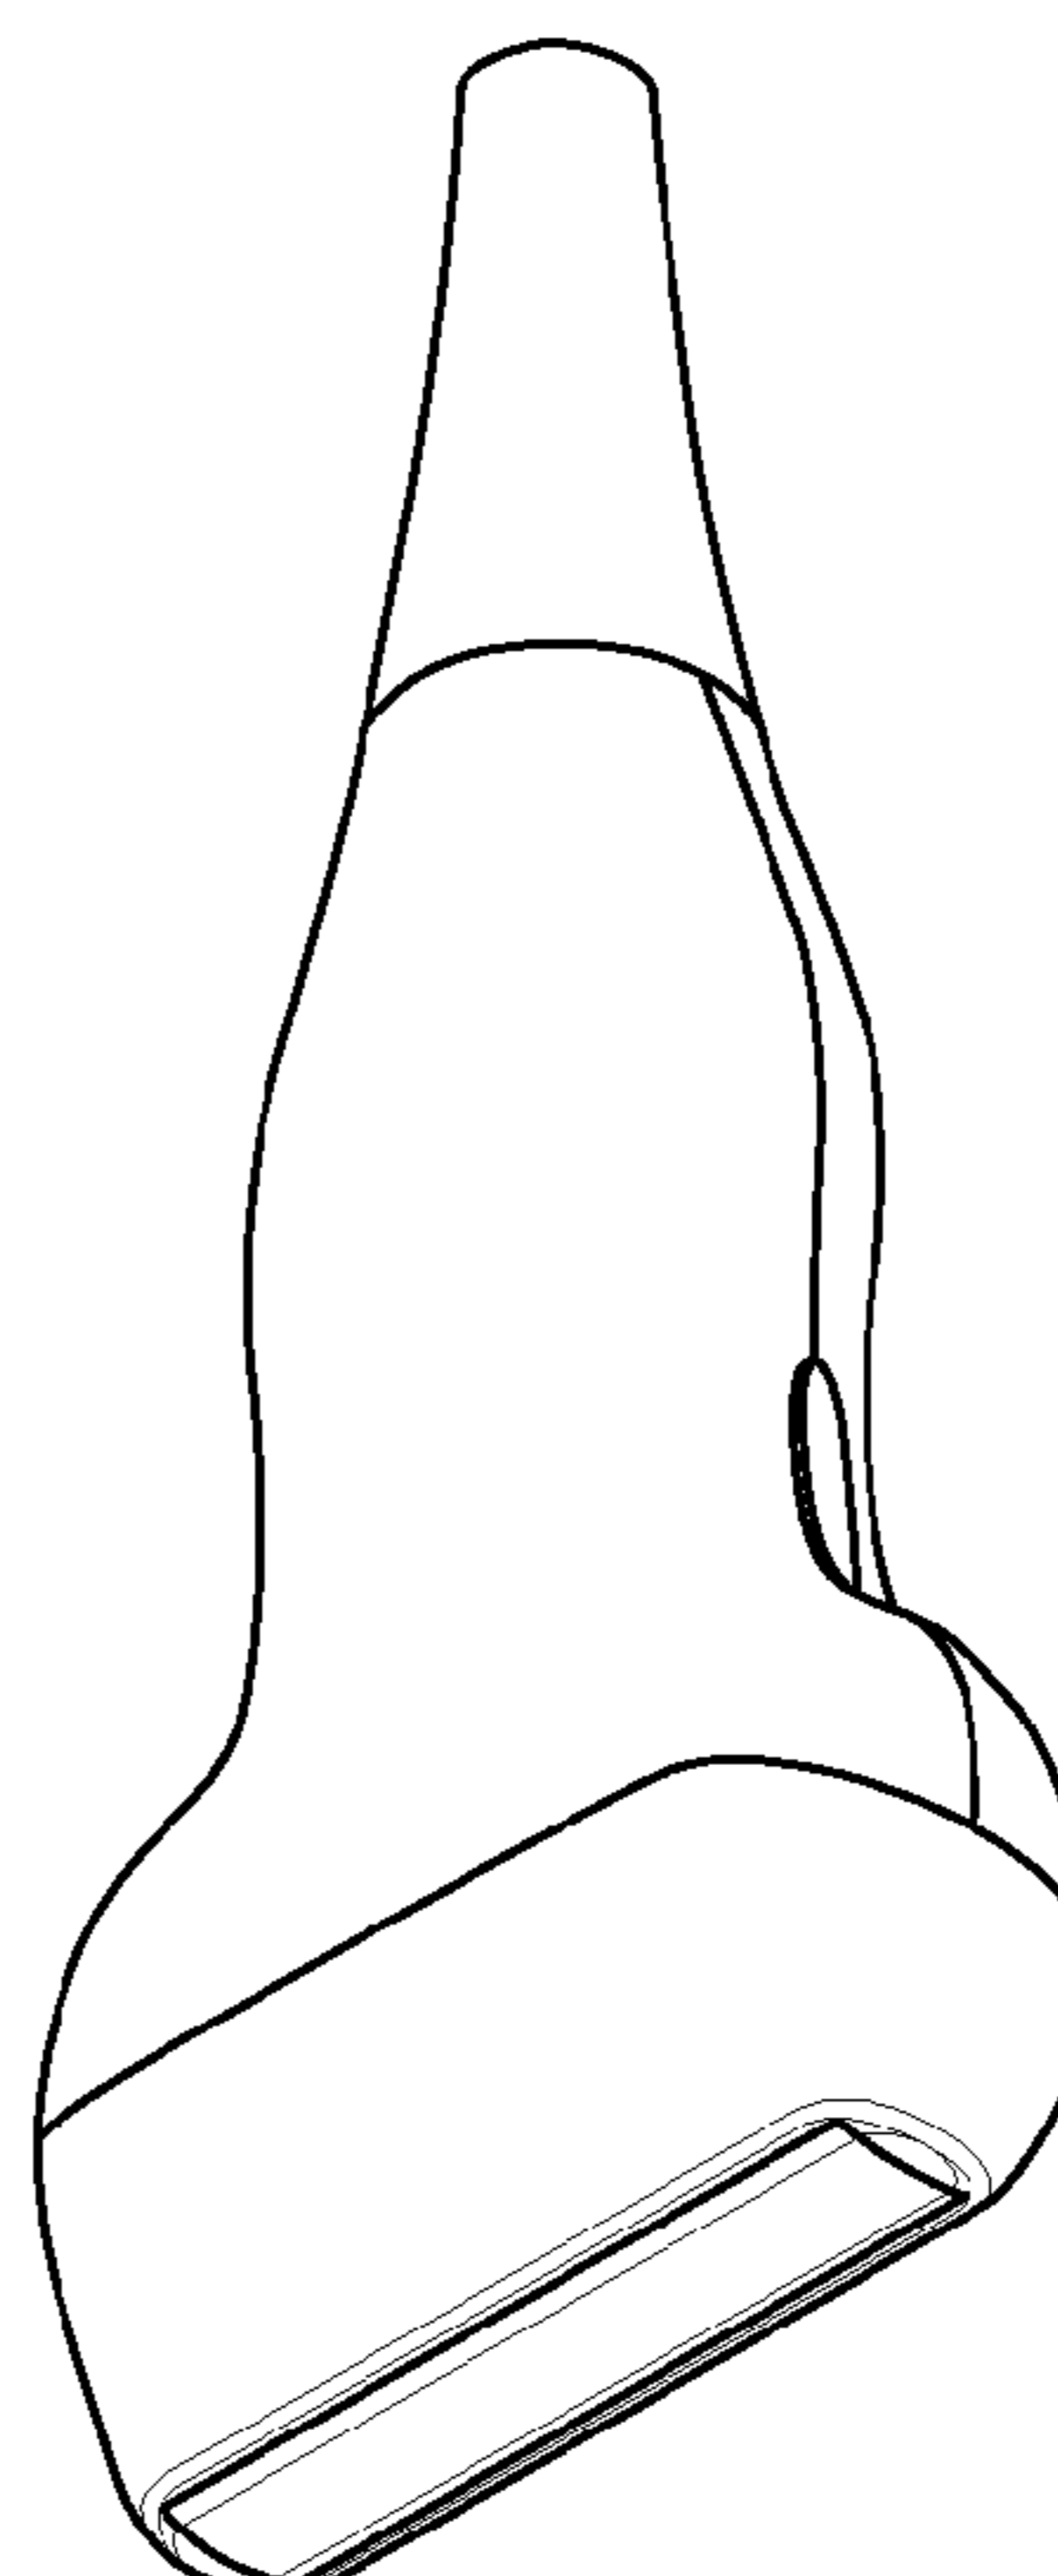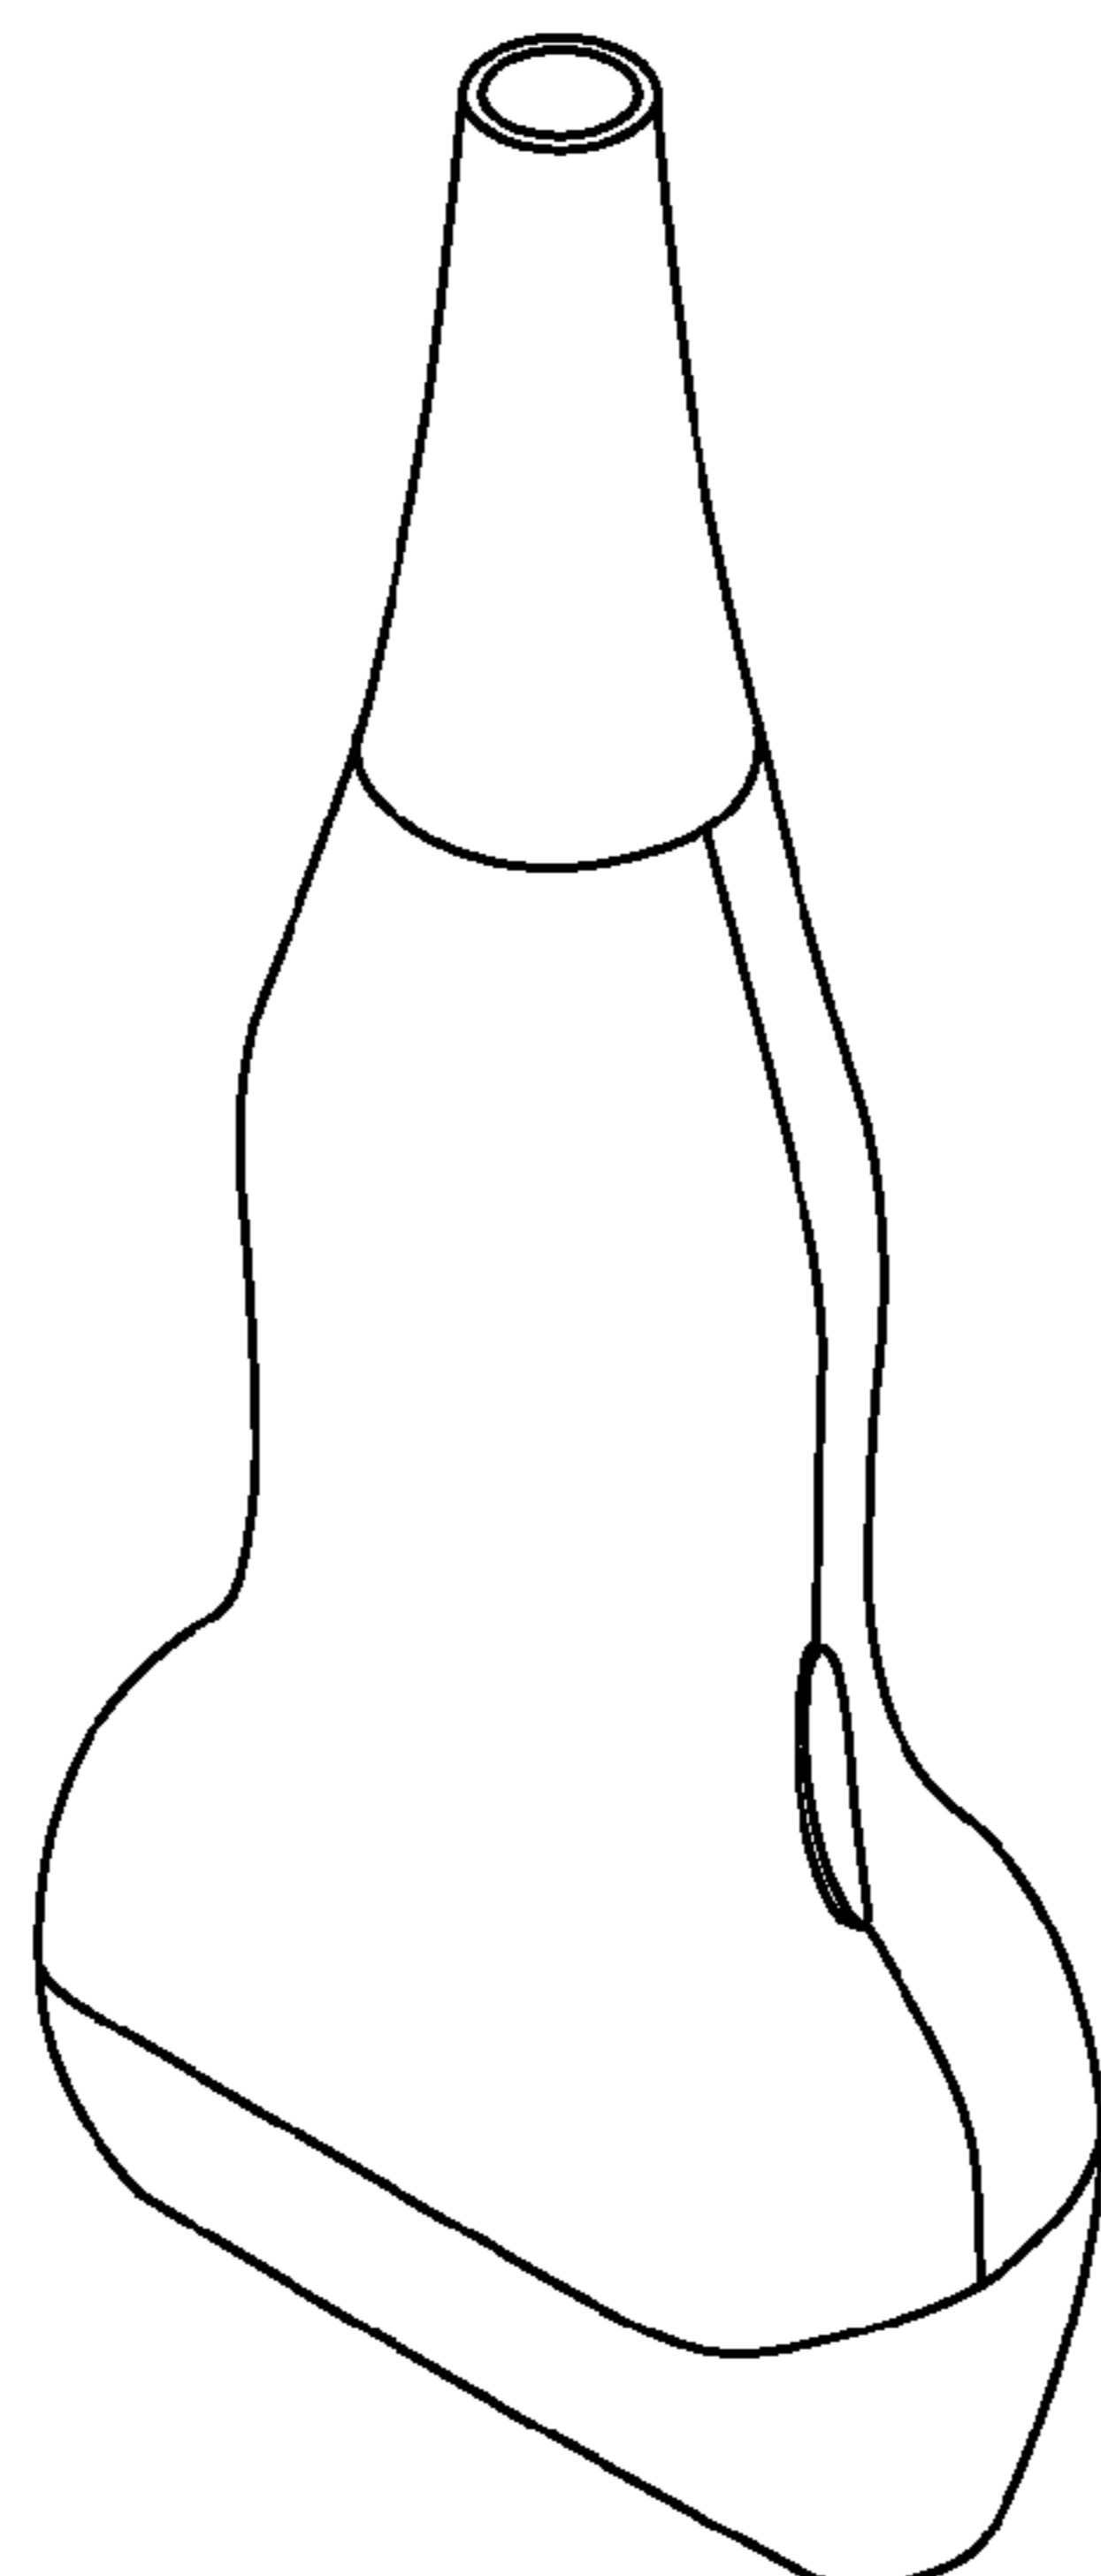

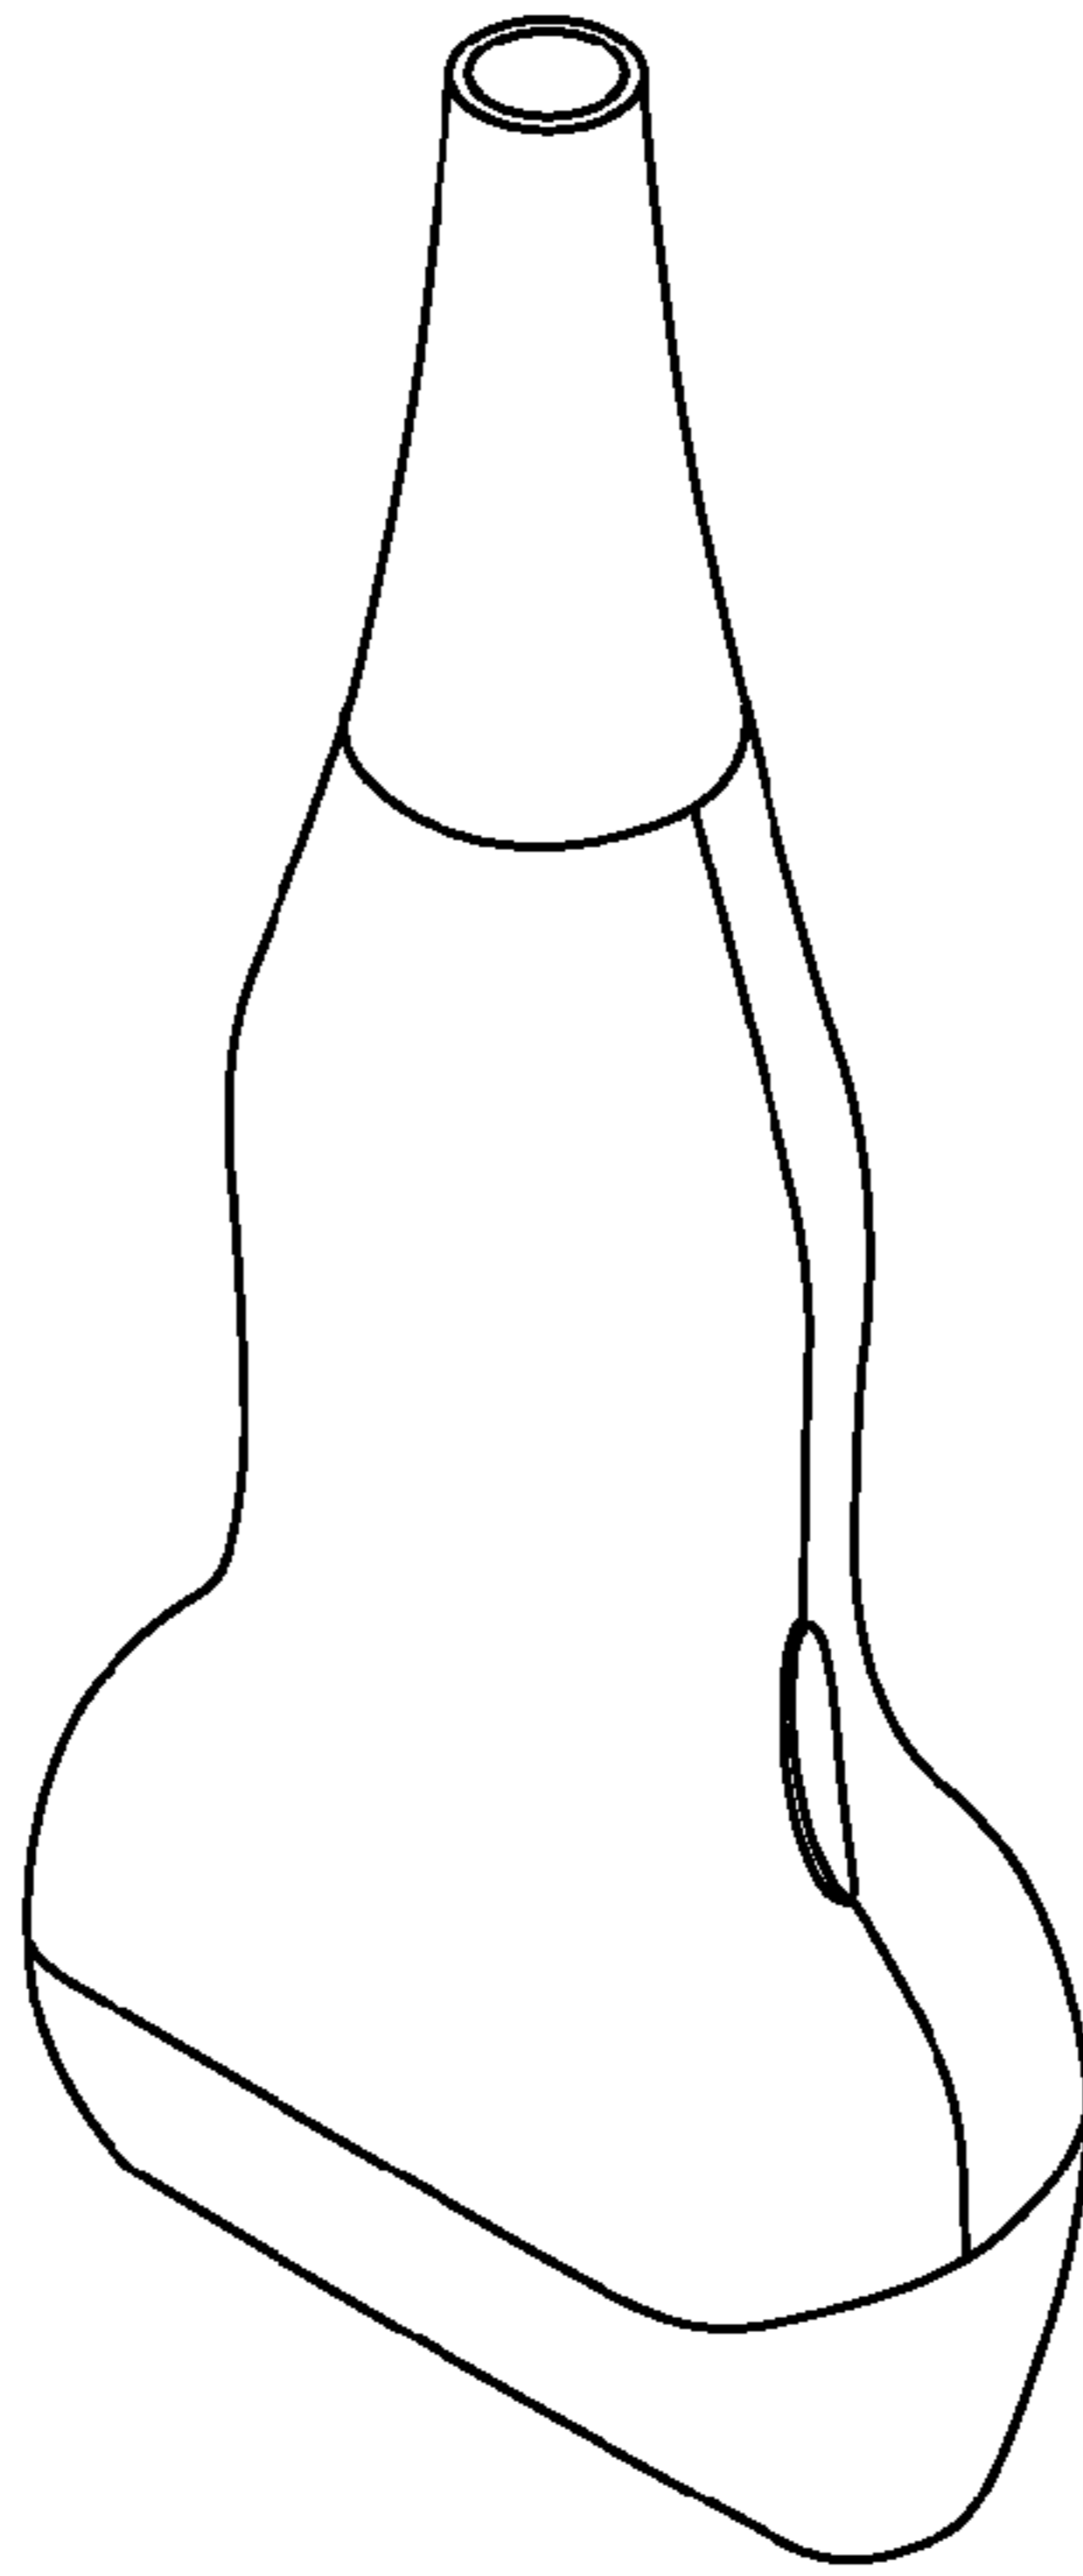


FIG. 1

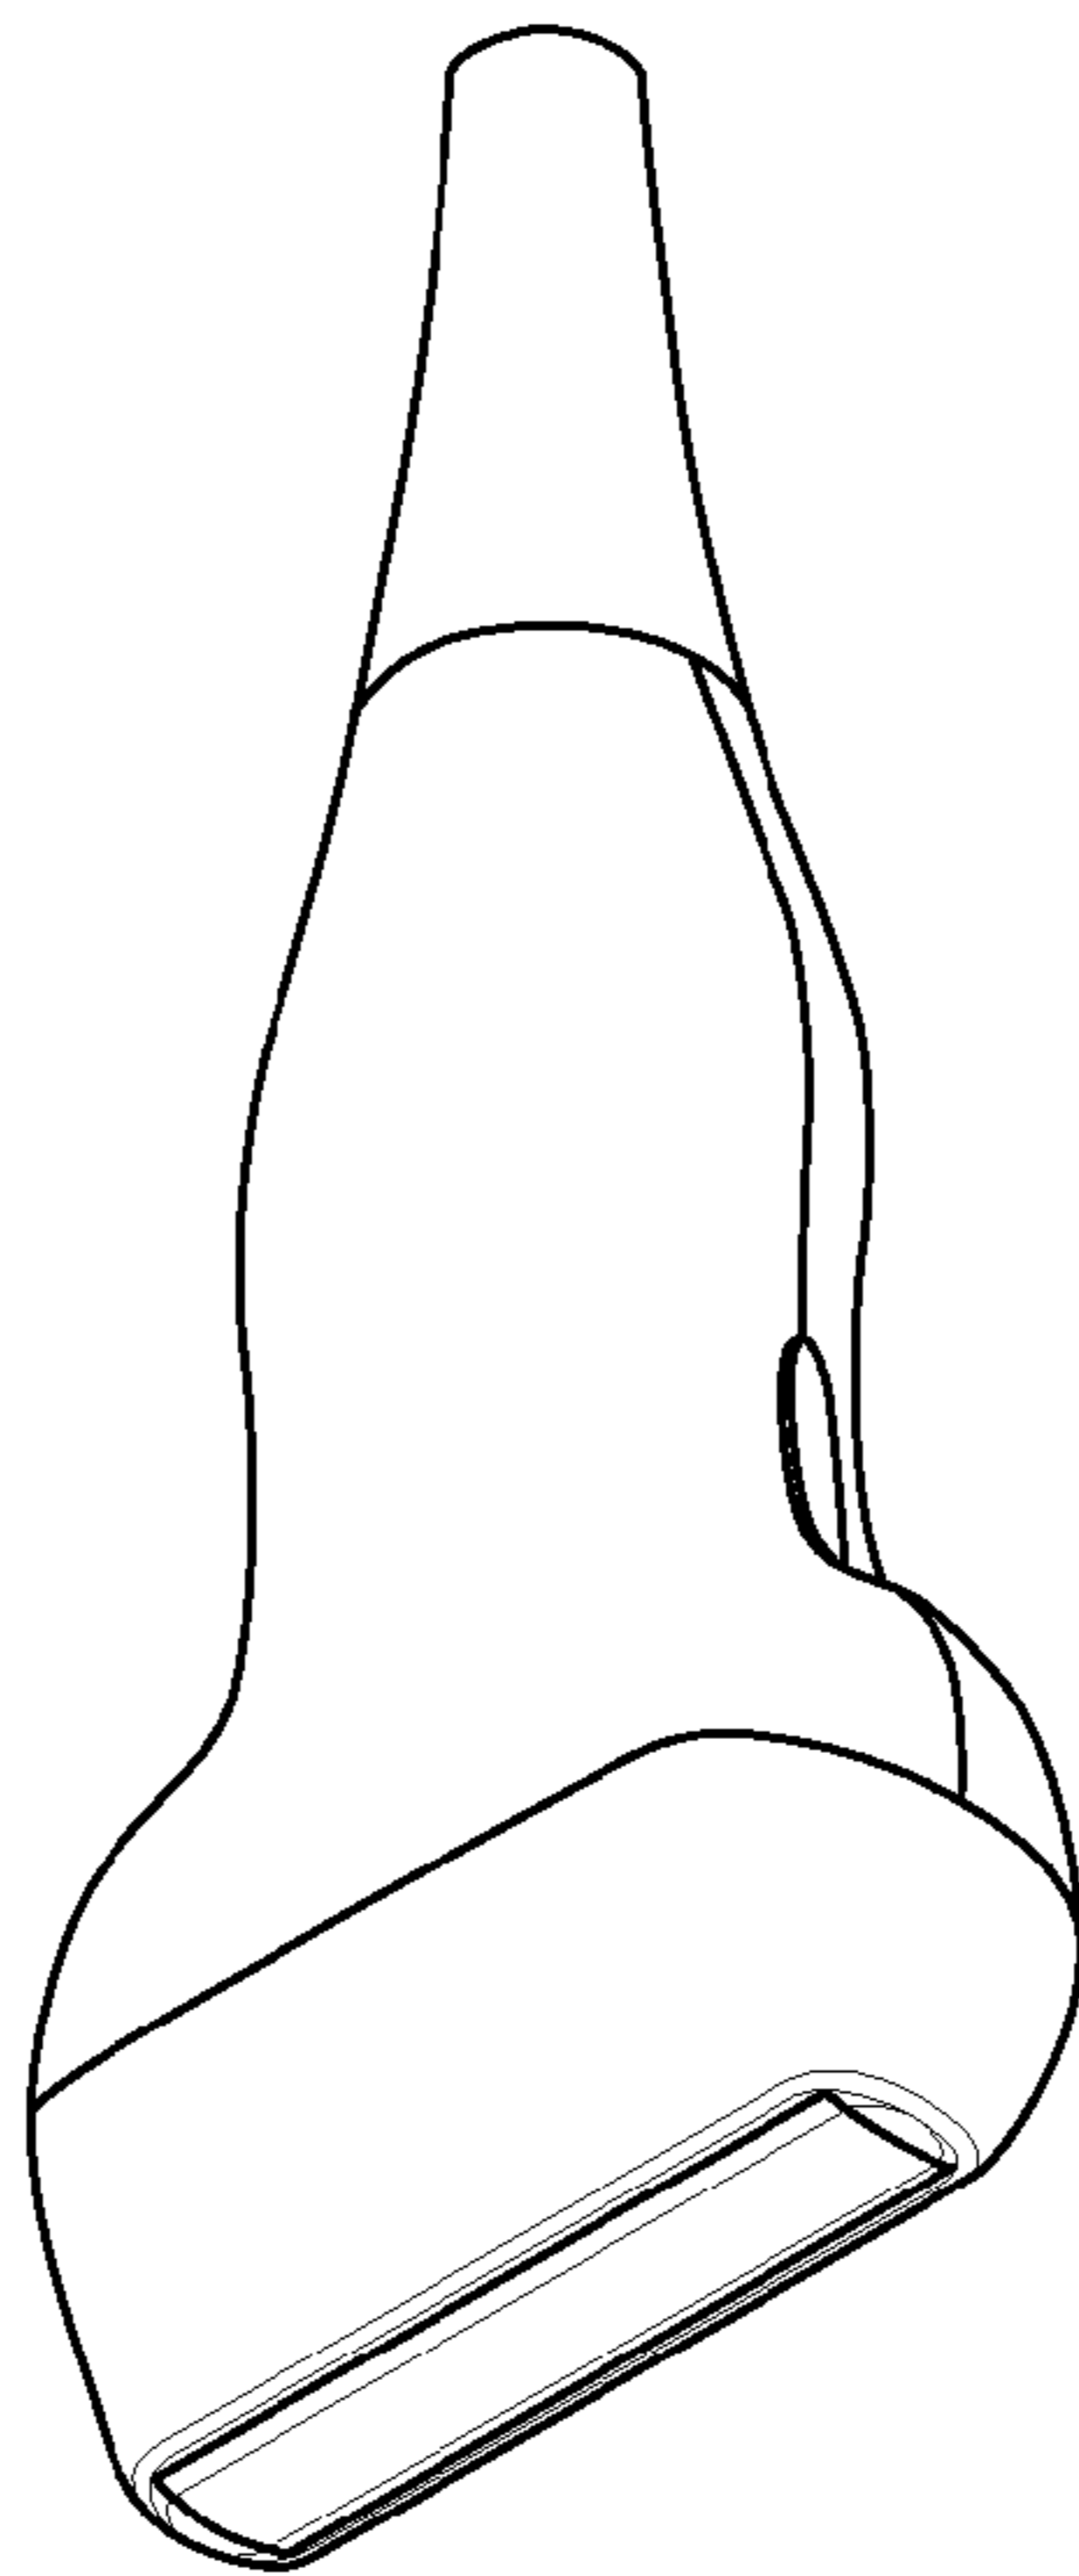


FIG. 2

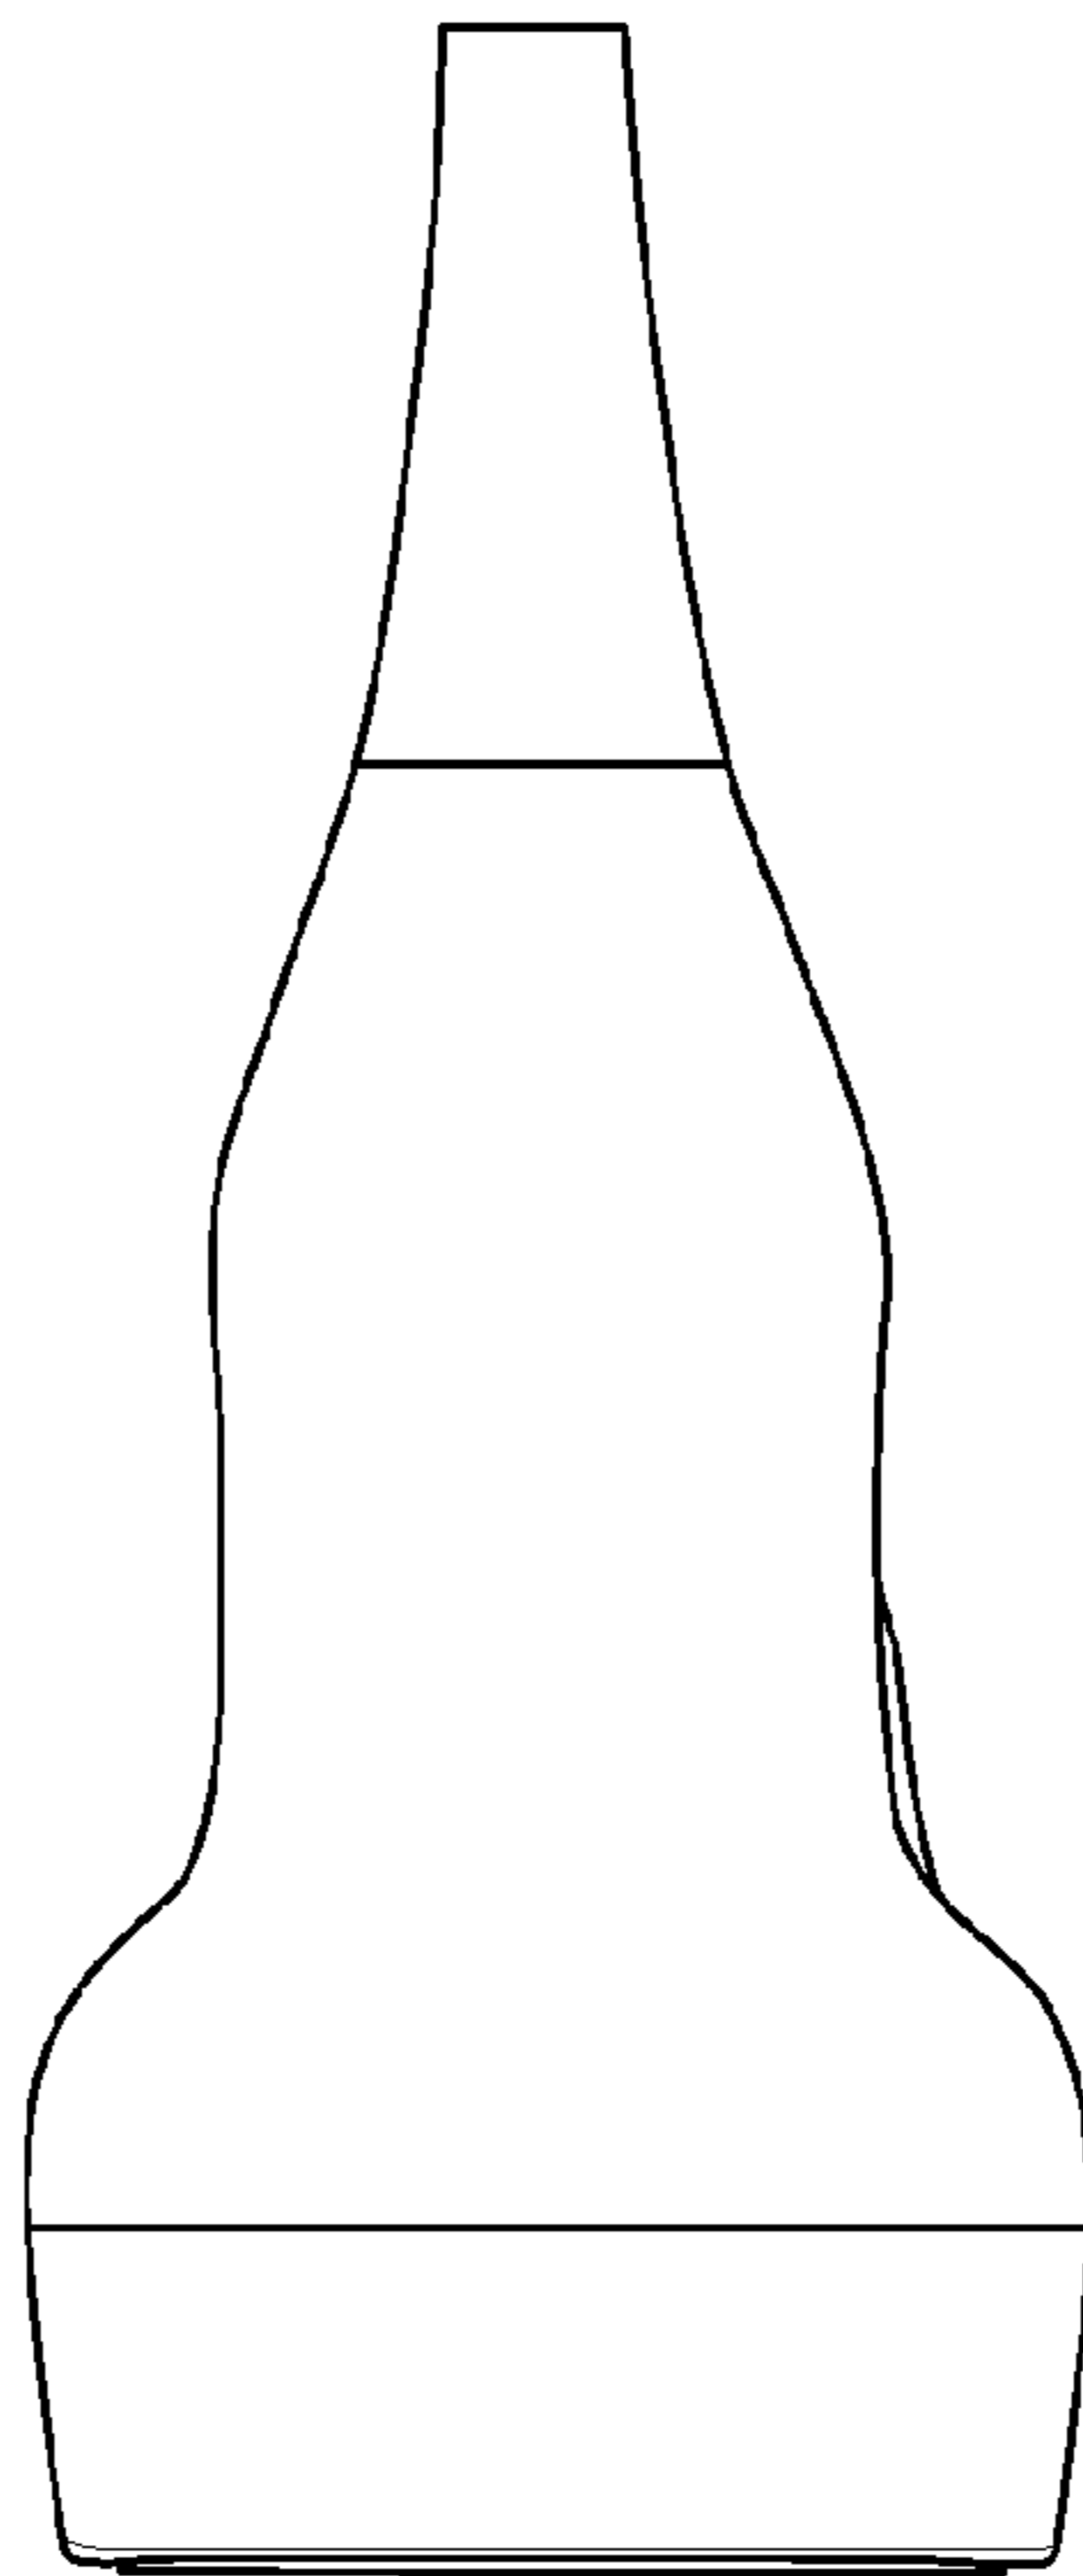


FIG. 3

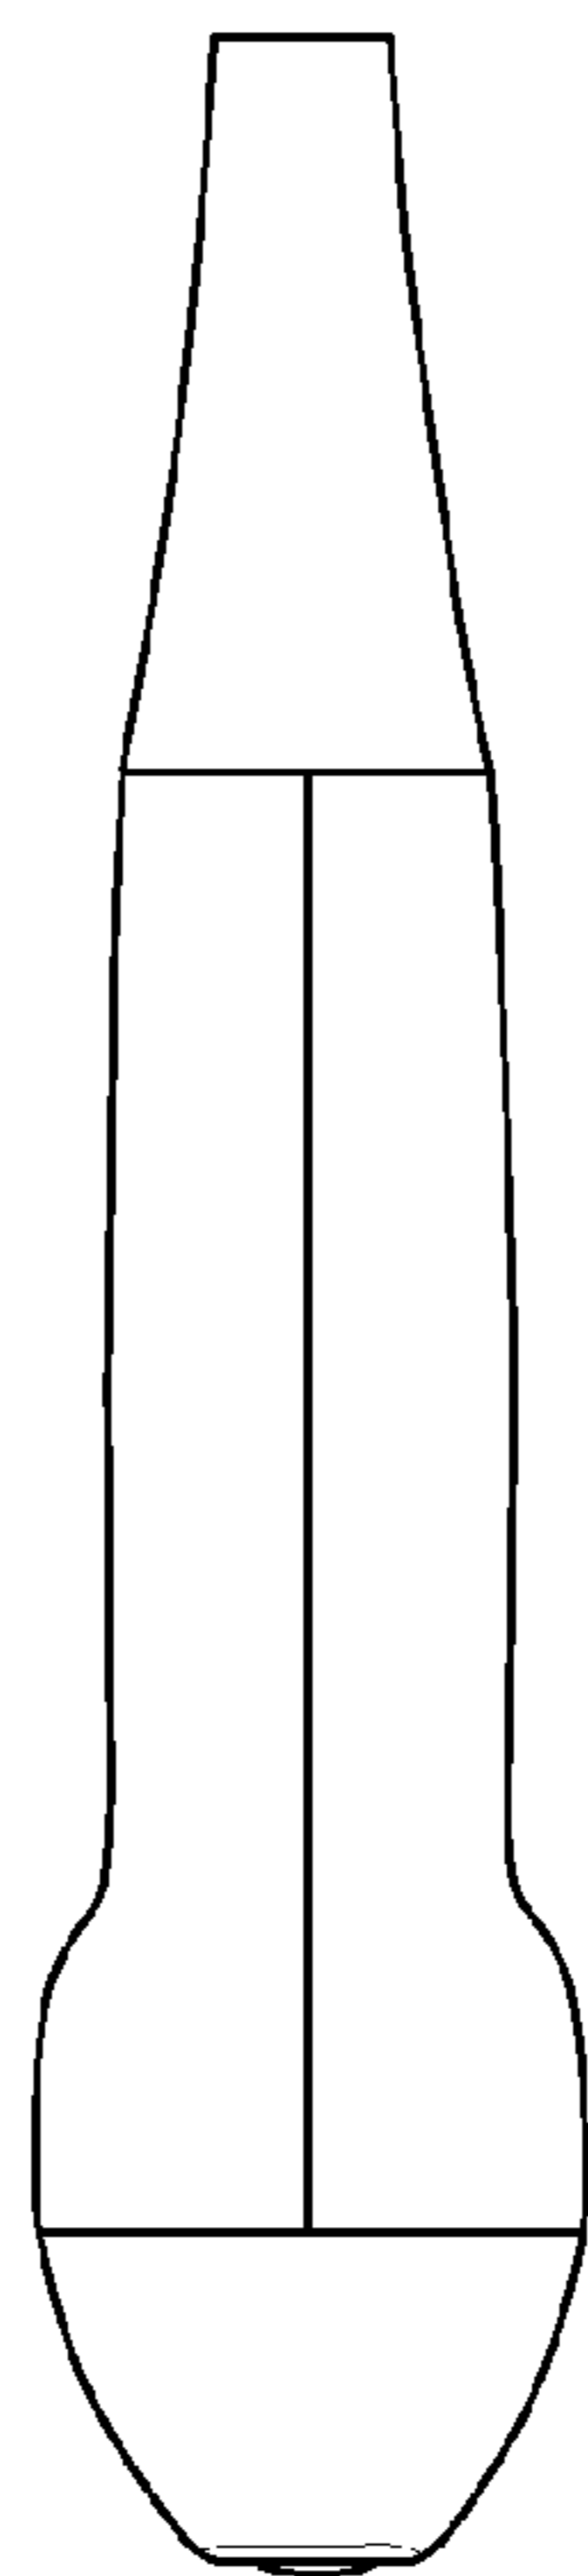


FIG.4

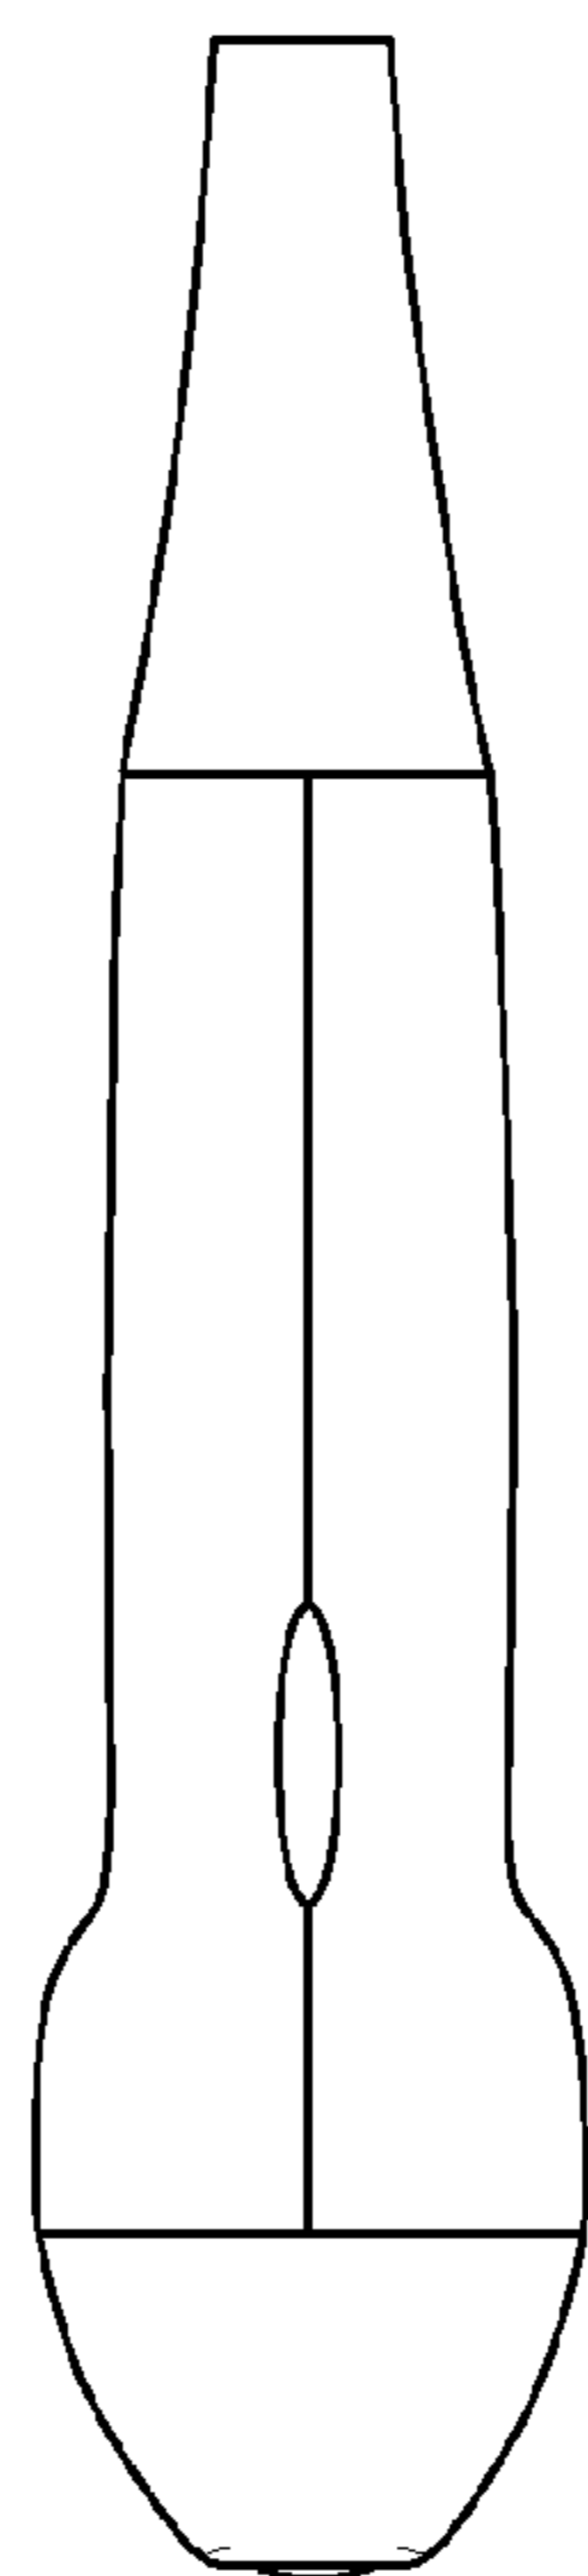


FIG.5

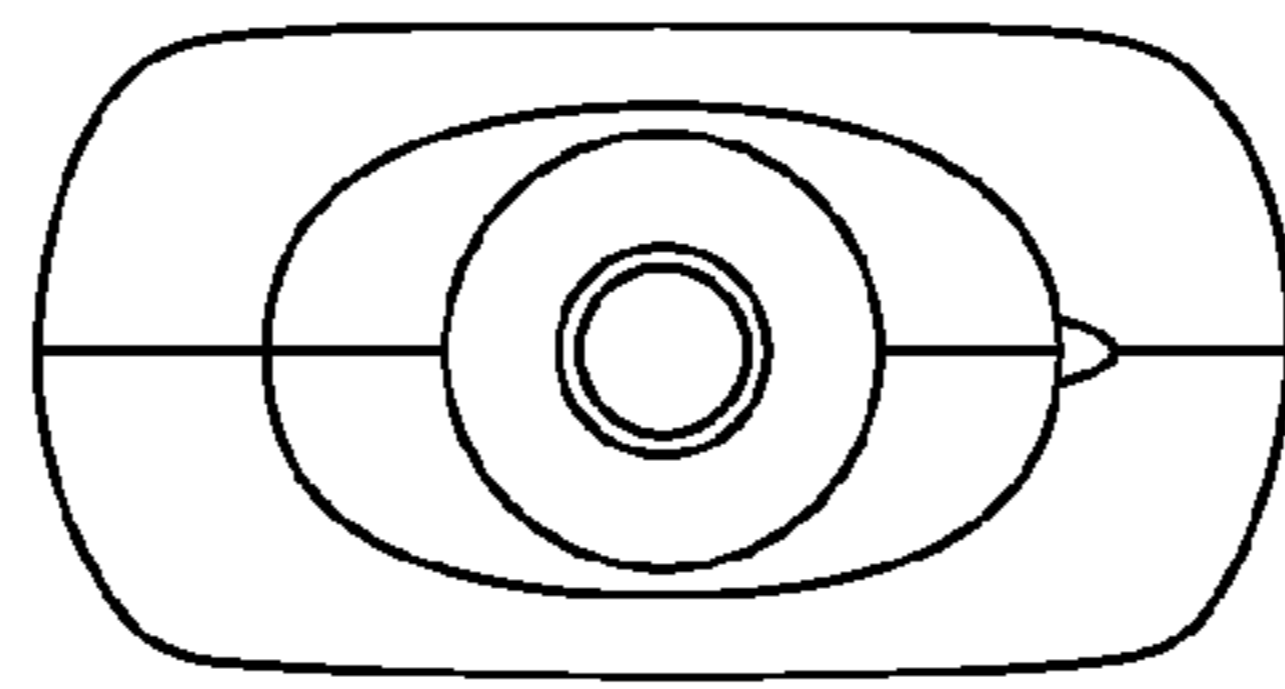


FIG. 6

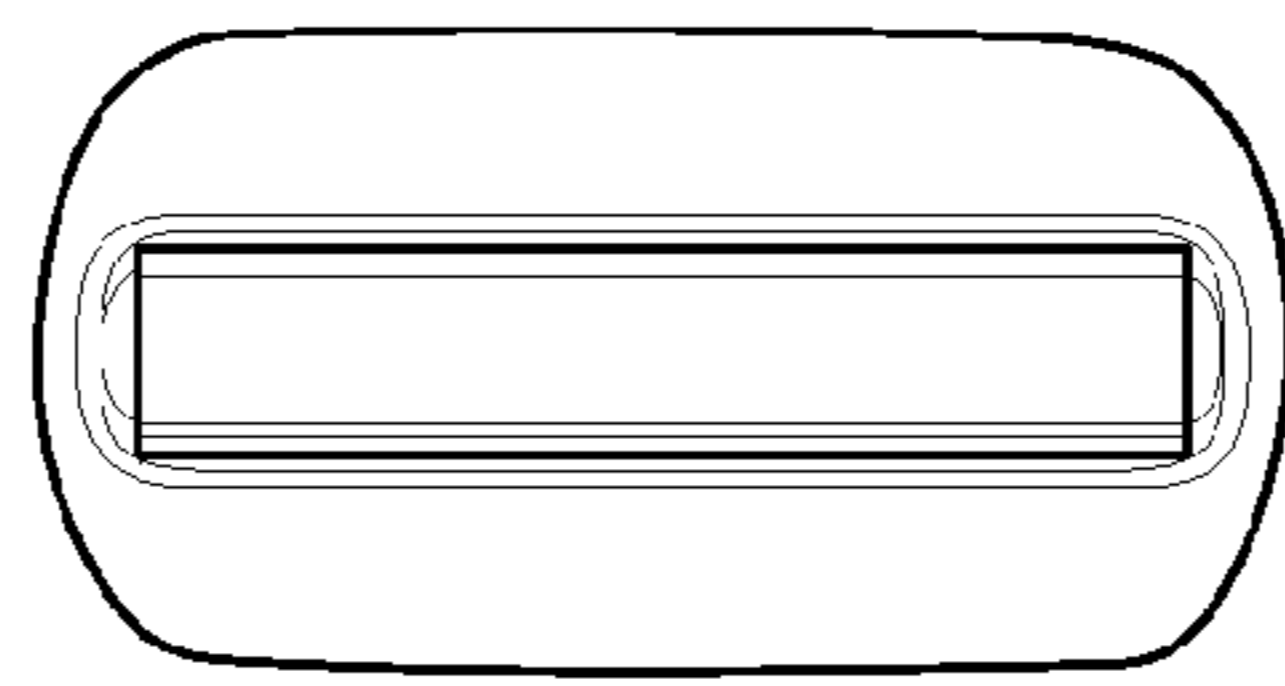


FIG. 7