



US00D705432S

(12) **United States Design Patent**
Lura et al.

(10) **Patent No.:** **US D705,432 S**
(45) **Date of Patent:** **** May 20, 2014**

(54) **PORTABLE DIALYSIS CABINET**

DESCRIPTION

(71) Applicant: **Medtronic, Inc.**, Minneapolis, MN (US)

(72) Inventors: **David B. Lura**, Maple Grove, MN (US);
Martin T Gerber, Maple Grove, MN
(US); **Bryant J. Pudil**, Plymouth, MN
(US); **Thomas E. Meyer**, Stillwater, MN
(US); **Brian Mullins**, Minneapolis, MN
(US)

(73) Assignee: **Medtronic, Inc.**, Minneapolis, MN (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/446,277**

(22) Filed: **Feb. 21, 2013**

(51) **LOC (10) Cl.** **24-00**

(52) **U.S. Cl.**
USPC **D24/185**

(58) **Field of Classification Search**

USPC D24/185, 186, 144, 160, 167-169, 172,
D24/200, 158, 164; D34/12, 14; 312/22,
312/109, 209, 223.1, 286, 249.8, 249.12;
248/282.1; 600/437, 443, 459

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D86,687 S * 4/1932 Prouty D24/185
D101,605 S * 10/1936 Anderson D24/200

(Continued)

Primary Examiner — Robert M Spear

Assistant Examiner — Rhea Shields

(74) *Attorney, Agent, or Firm* — Hahn & Voight PLLC;
Roger C. Hahn

(57) **CLAIM**

We claim the ornamental design for a portable dialysis cabinet, as shown and described.

FIG. 1 is a perspective view of a portable dialysis cabinet according to one embodiment;

FIG. 2 is a front view of the portable dialysis cabinet referenced in FIG. 1;

FIG. 3 is a rear view of the portable dialysis cabinet referenced in FIG. 1;

FIG. 4 is a left side view of the portable dialysis cabinet referenced in FIG. 1;

FIG. 5 is a right side view of the portable dialysis cabinet referenced in FIG. 1;

FIG. 6 is a top view of the portable dialysis cabinet referenced in FIG. 1;

FIG. 7 is a bottom view of the portable dialysis cabinet referenced in FIG. 1;

FIG. 8 is a perspective view of a portable dialysis cabinet according to another embodiment;

FIG. 9 is a front view of the portable dialysis cabinet referenced in FIG. 8;

FIG. 10 is a rear view of the portable dialysis cabinet referenced in FIG. 8;

FIG. 11 is a left side view of the portable dialysis cabinet referenced in FIG. 8;

FIG. 12 is a right side view of the portable dialysis cabinet referenced in FIG. 8;

FIG. 13 is a top view of the portable dialysis cabinet referenced in FIG. 8;

FIG. 14 is a bottom view of the portable dialysis cabinet referenced in FIG. 8;

FIG. 15 is a perspective view of a portable dialysis cabinet according to yet another embodiment;

FIG. 16 is a front view of the portable dialysis cabinet referenced in FIG. 15;

FIG. 17 is a rear view of the portable dialysis cabinet referenced in FIG. 15;

FIG. 18 is a left side view of the portable dialysis cabinet referenced in FIG. 15;


FIG. 19 is a right side view of the portable dialysis cabinet referenced in FIG. 15;

FIG. 20 is a top view of the portable dialysis cabinet referenced in FIG. 15; and,

FIG. 21 is a bottom view of the portable dialysis cabinet referenced in FIG. 15.

The broken lines in the drawings illustrate unclaimed environment only and form no part of the claimed design.

1 Claim, 21 Drawing Sheets

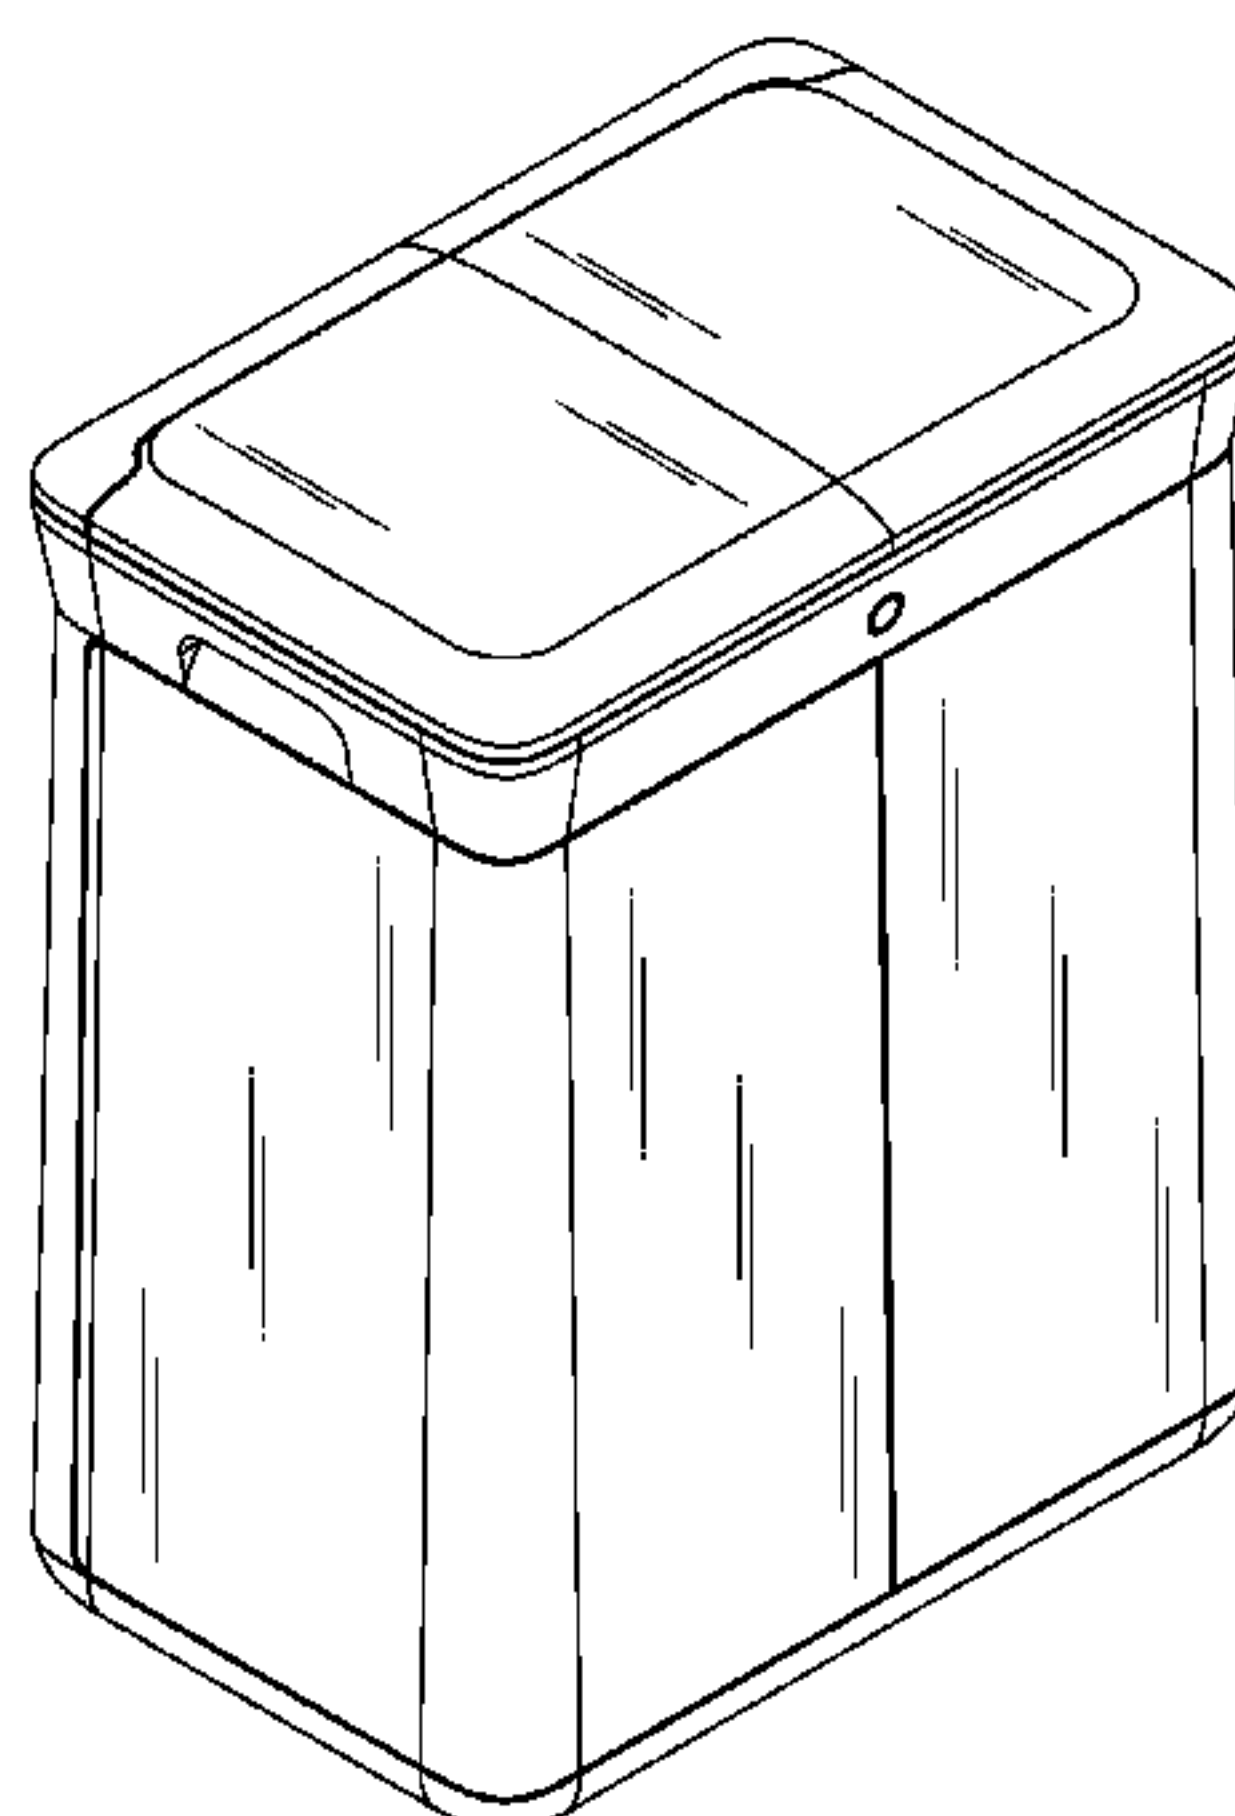

(56)

References Cited

U.S. PATENT DOCUMENTS

D263,573 S * 3/1982 Ingledew D34/14
D273,717 S * 5/1984 McCombs D24/164
D319,308 S * 8/1991 Royse et al. D24/185
5,113,546 A * 5/1992 Parent 15/315
D332,855 S * 1/1993 Royse et al. D34/19
5,465,841 A * 11/1995 Wilson et al. 206/366
D415,328 S * 10/1999 Uehara et al. D34/19
D598,109 S 8/2009 Collins et al.
D609,350 S 2/2010 Hickey et al.

D613,411 S 4/2010 Collins et al.
D629,906 S 12/2010 Hickey et al.
D631,548 S 1/2011 McGill et al.
D637,293 S 5/2011 Hickey et al.
D639,930 S 6/2011 Collins et al.
D646,392 S 10/2011 Collins et al.
D650,063 S 12/2011 Collins et al.
D663,844 S 7/2012 McGill et al.
D664,255 S 7/2012 Hickey et al.
D664,660 S 7/2012 Hickey et al.
D675,727 S 2/2013 Collins et al.
2007/0138922 A1 * 6/2007 Frederick et al. 312/109

* cited by examiner

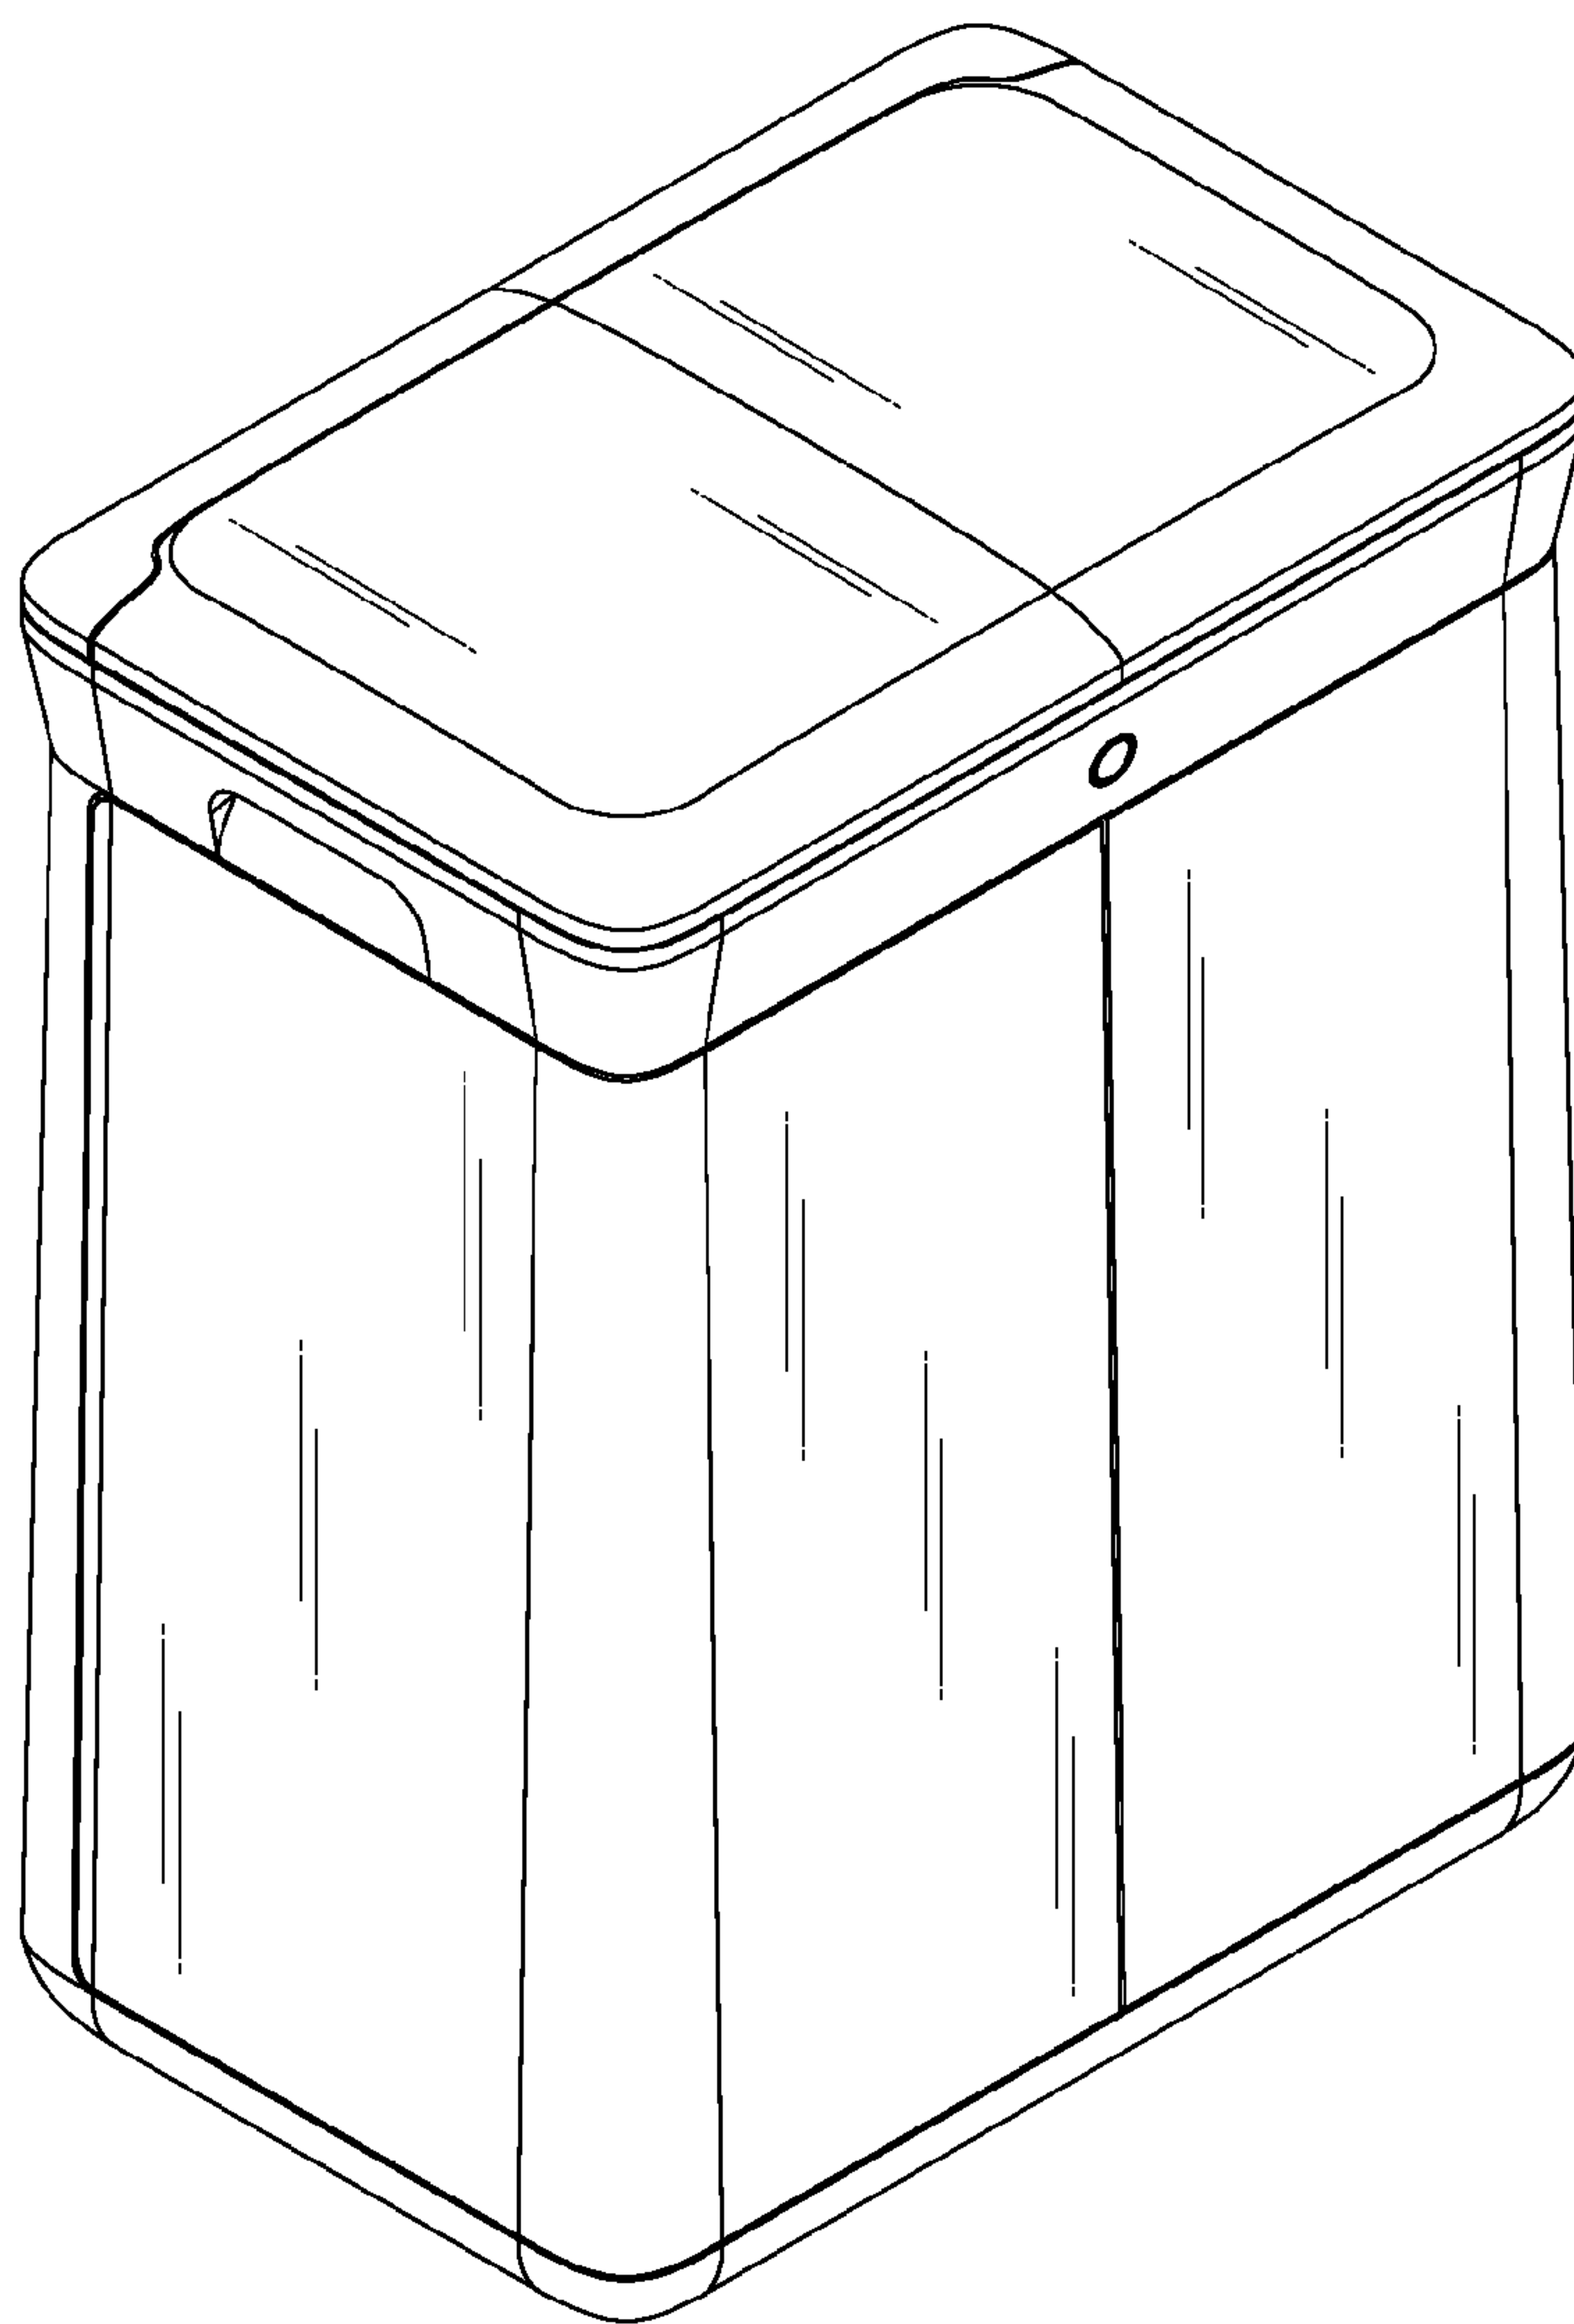


FIG. 1

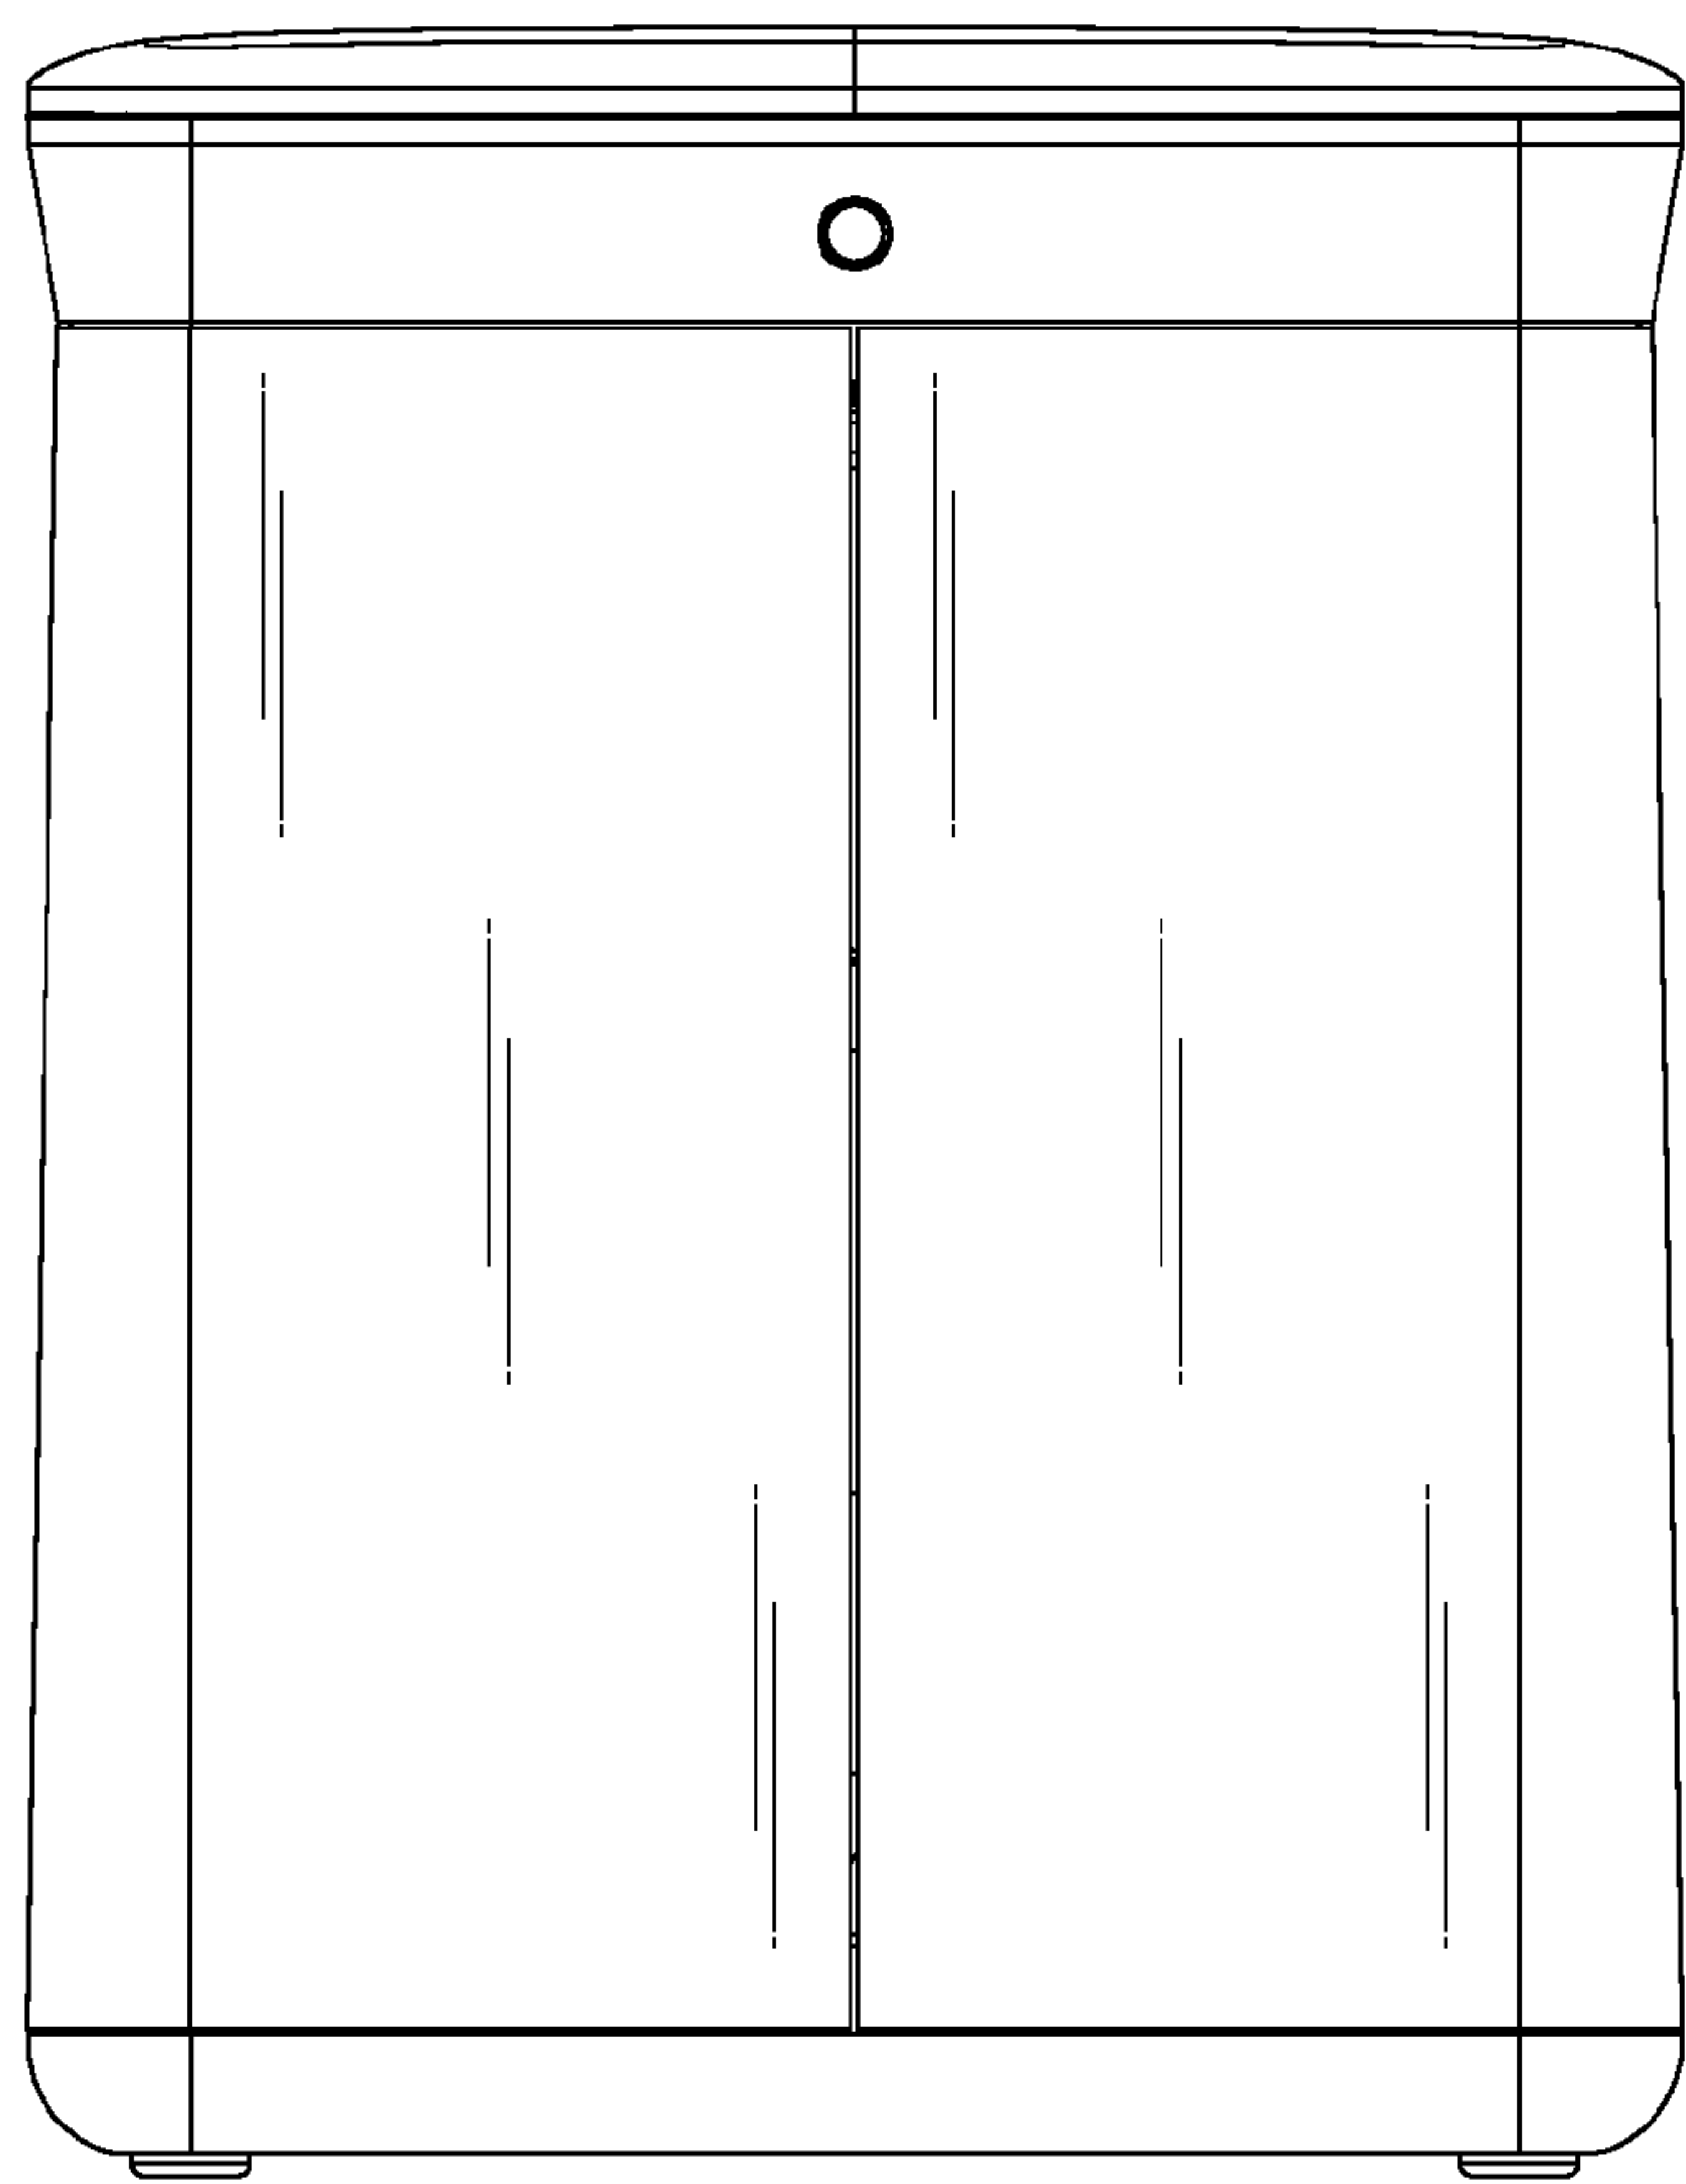


FIG. 2

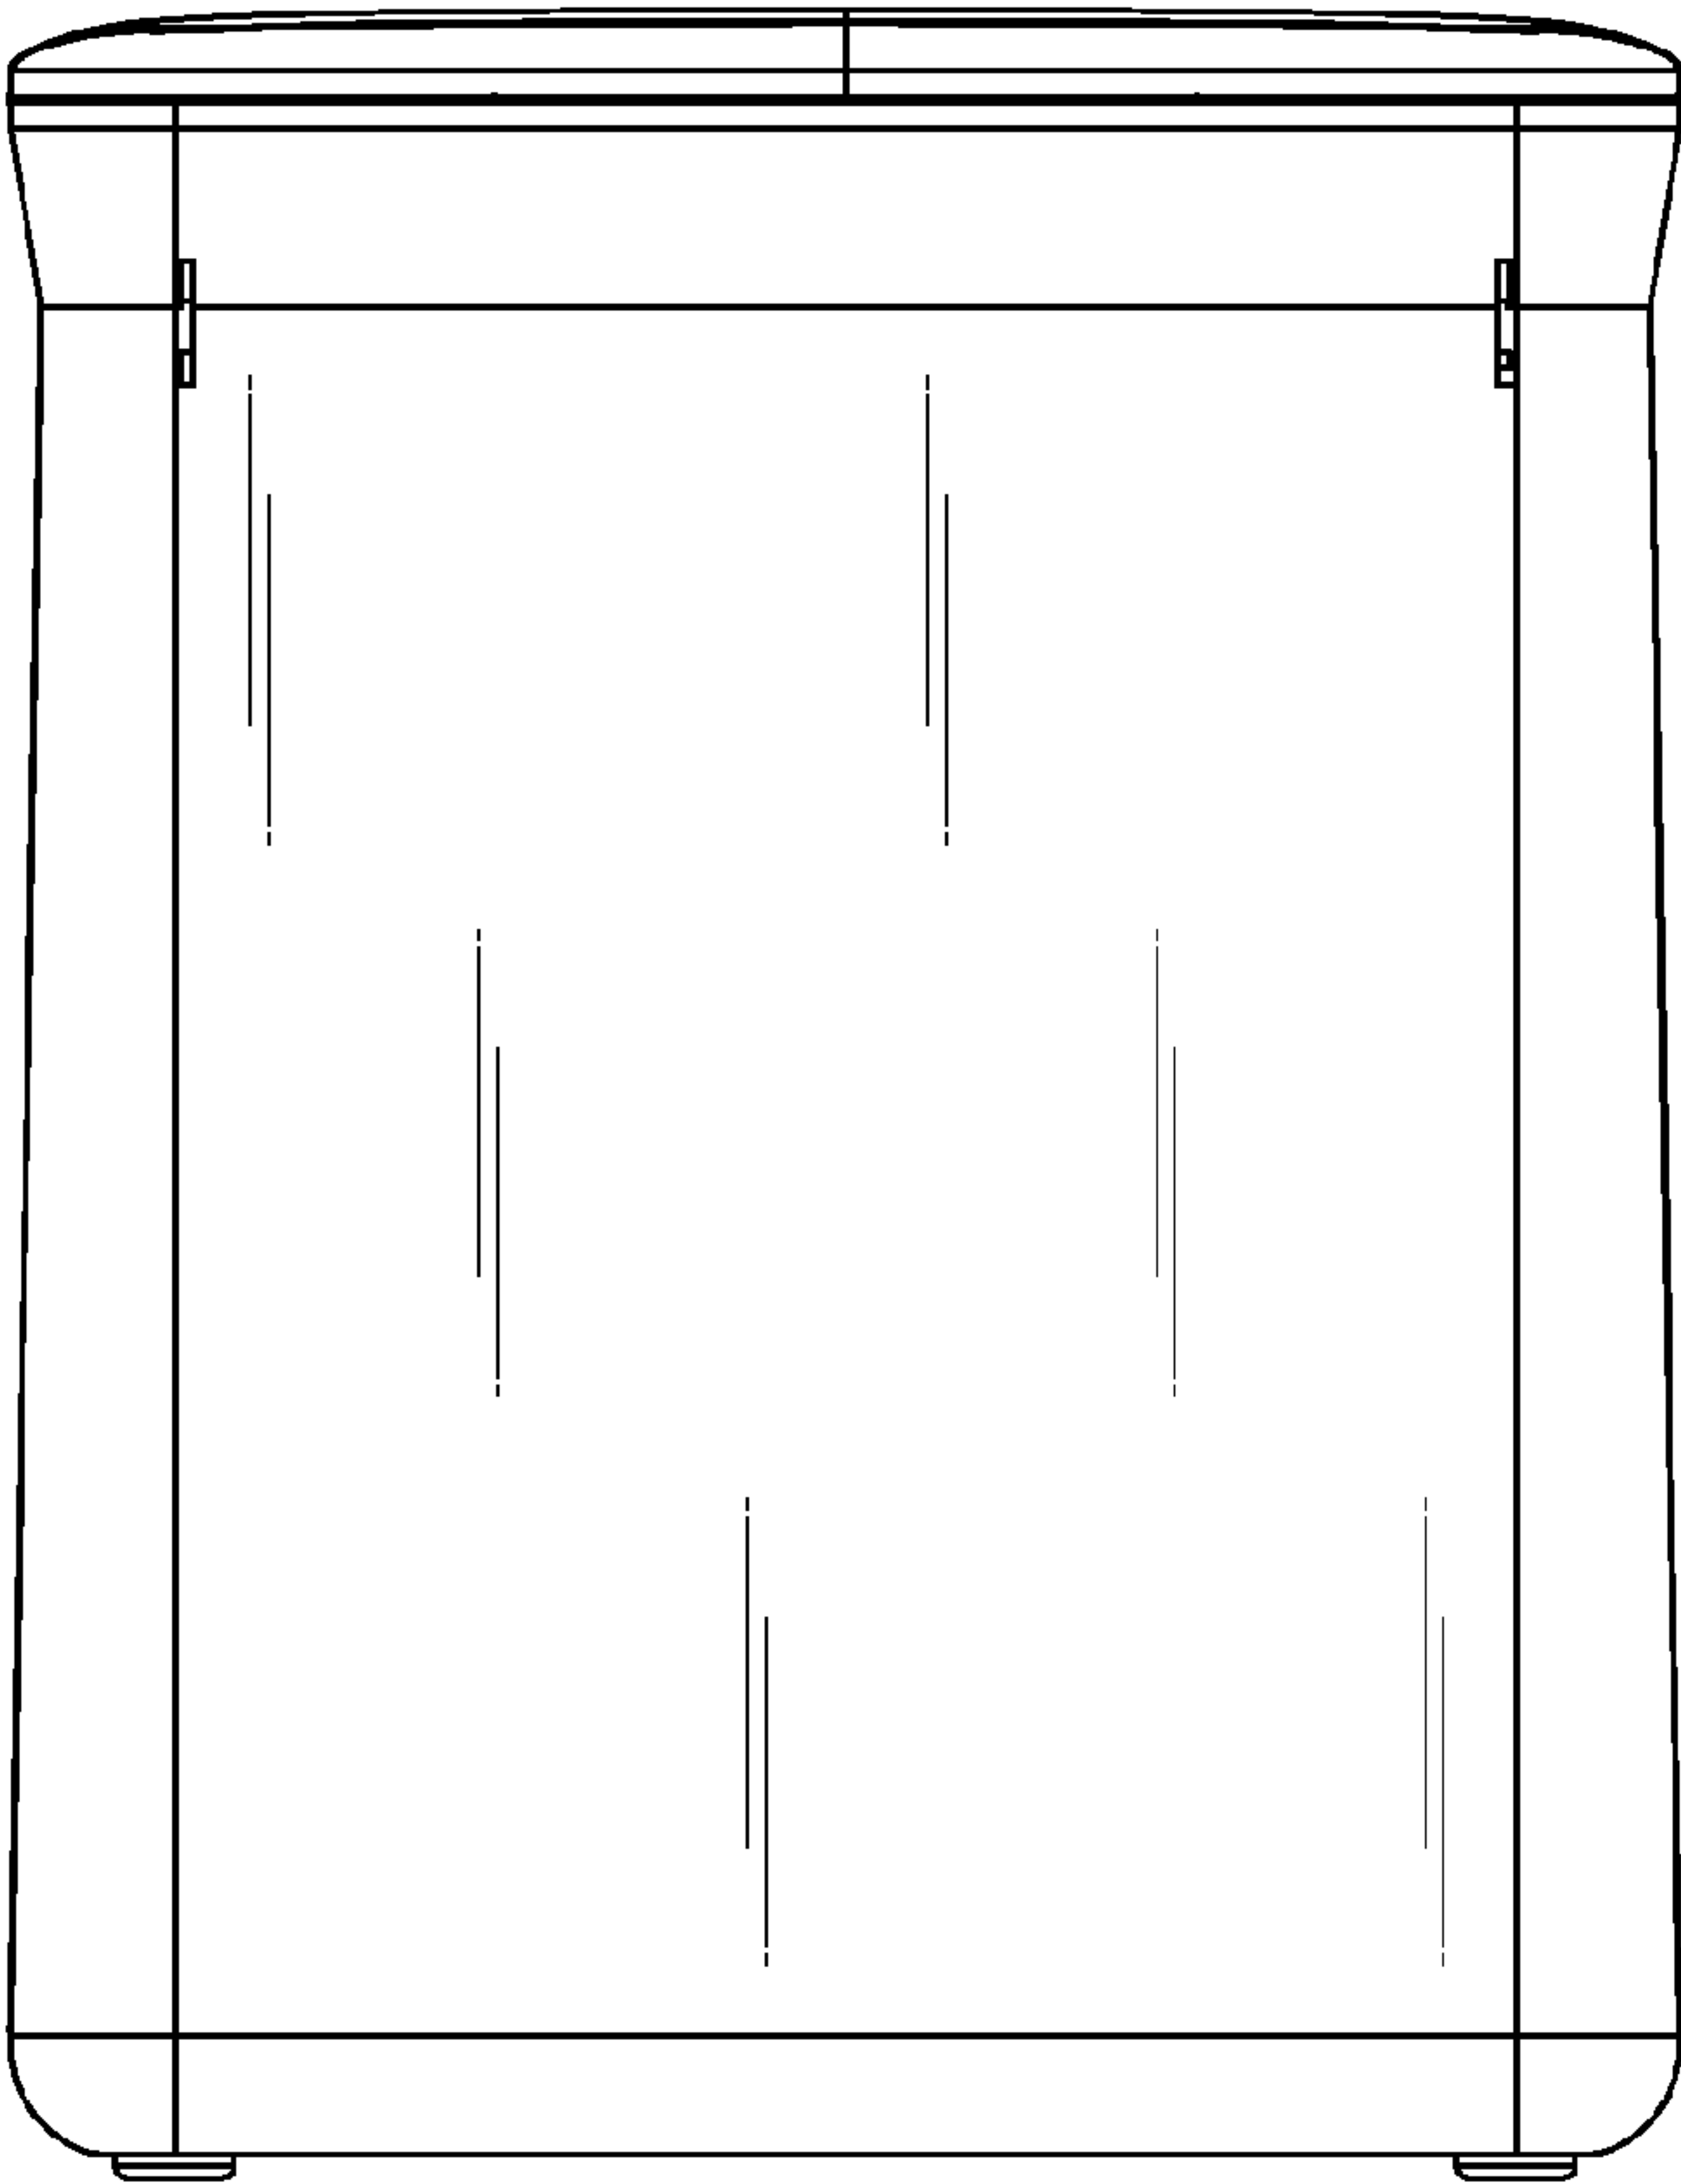


FIG. 3

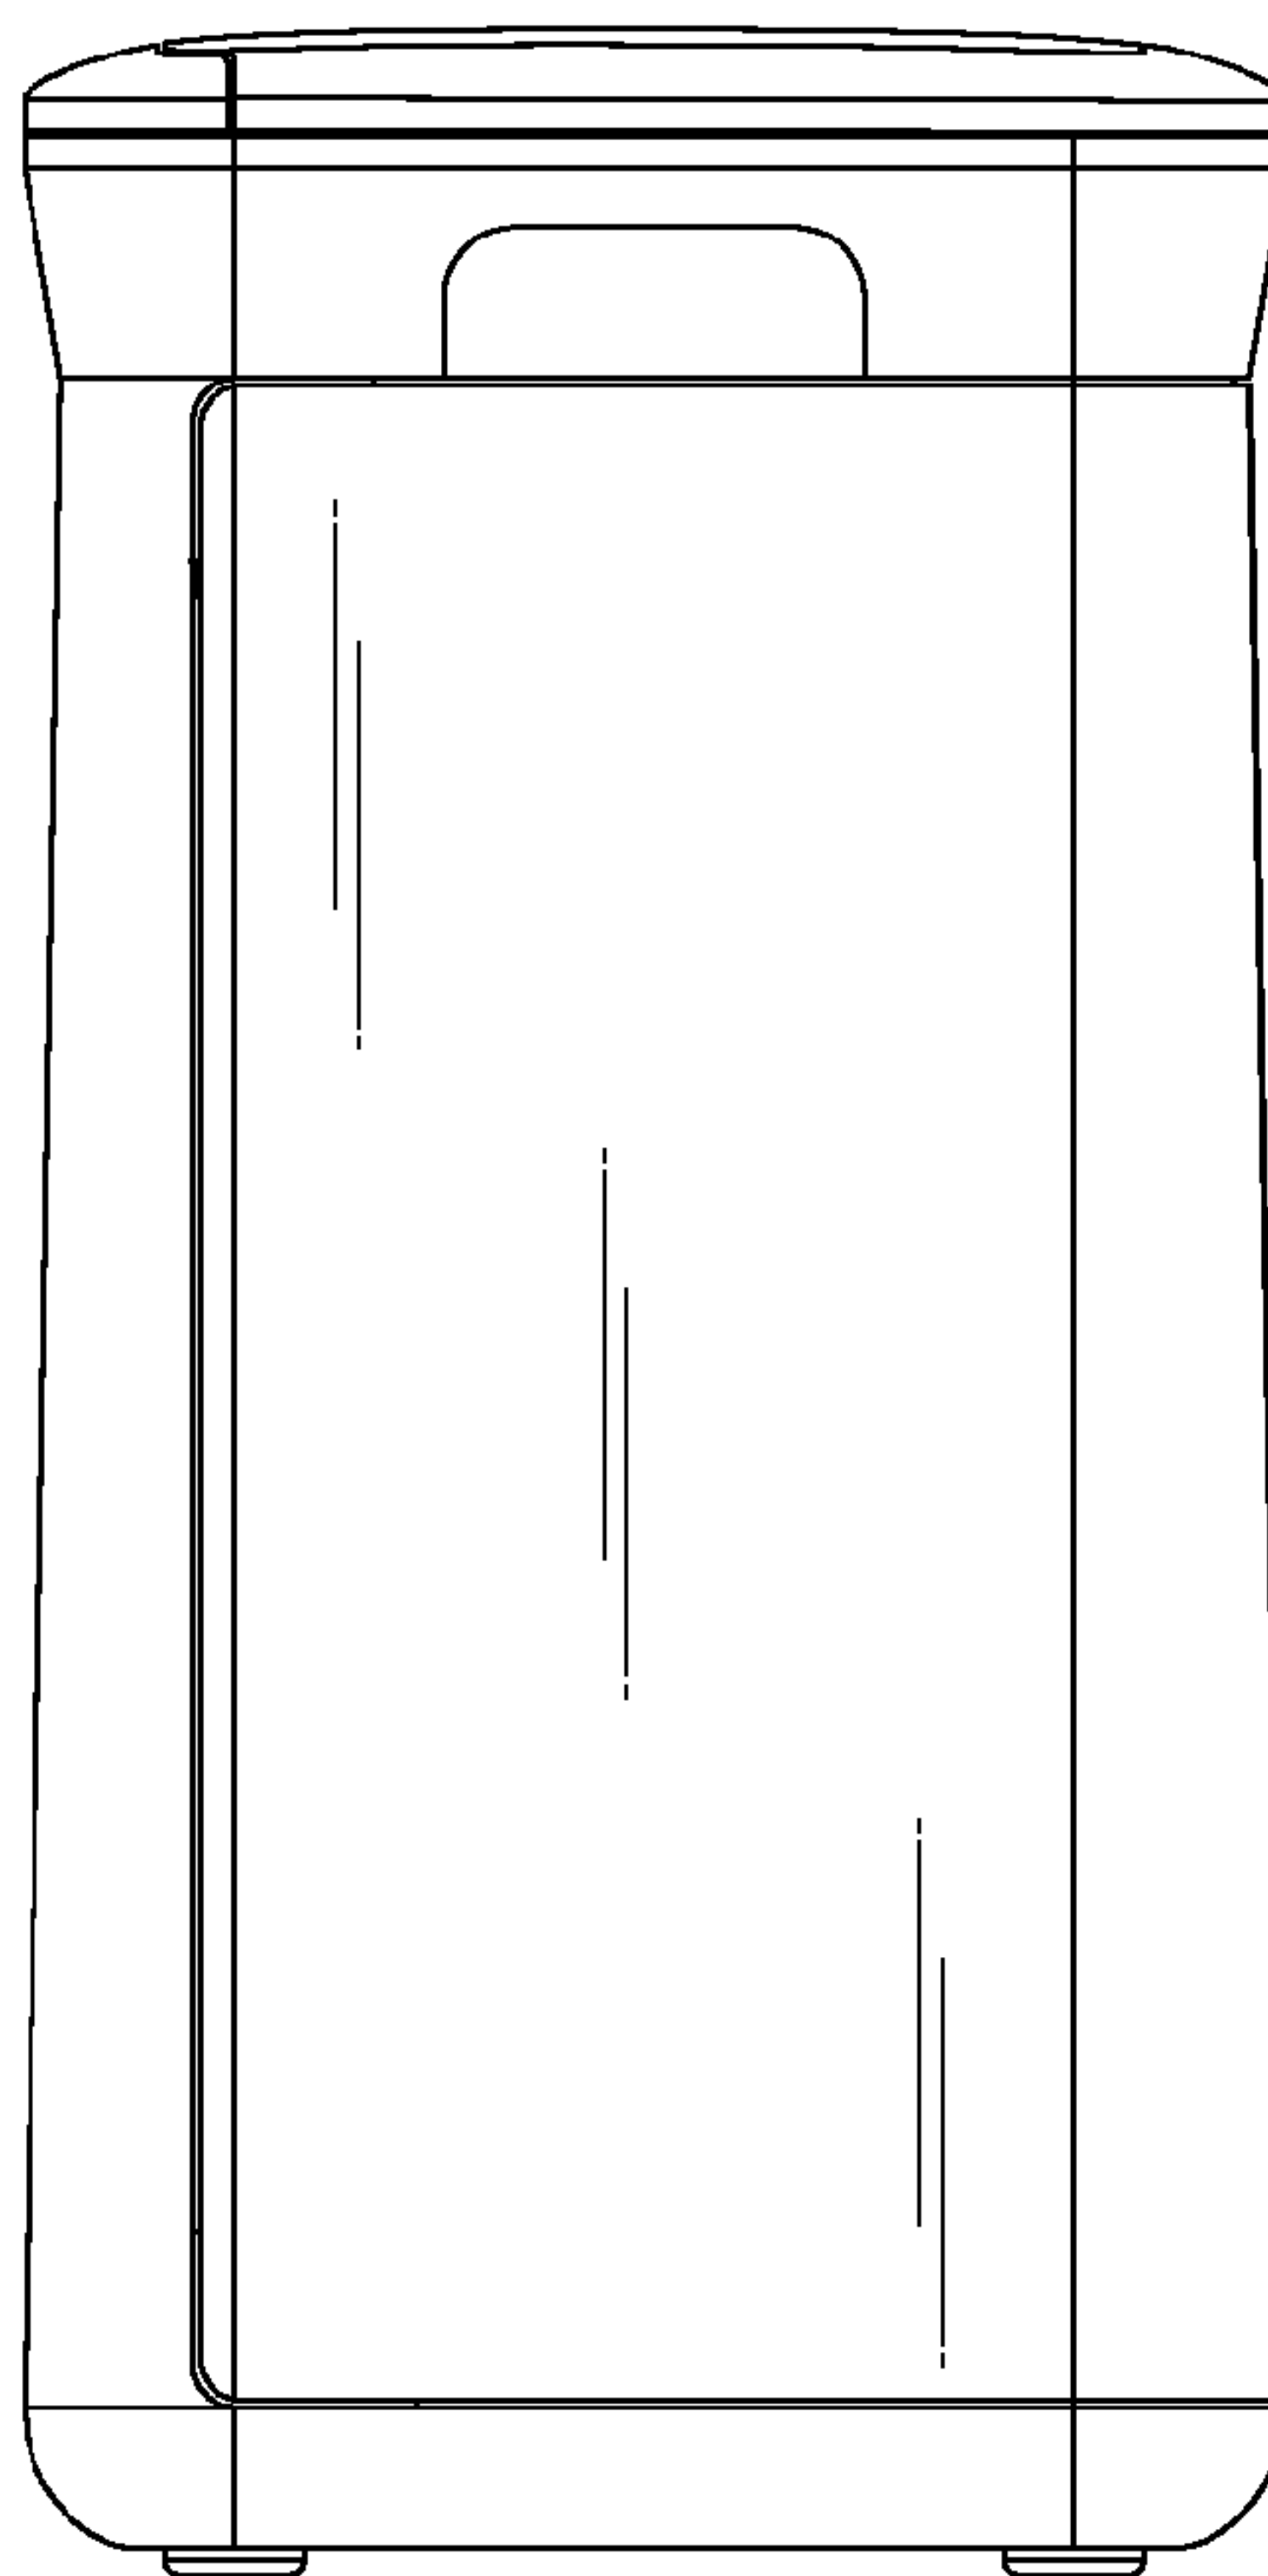


FIG. 4

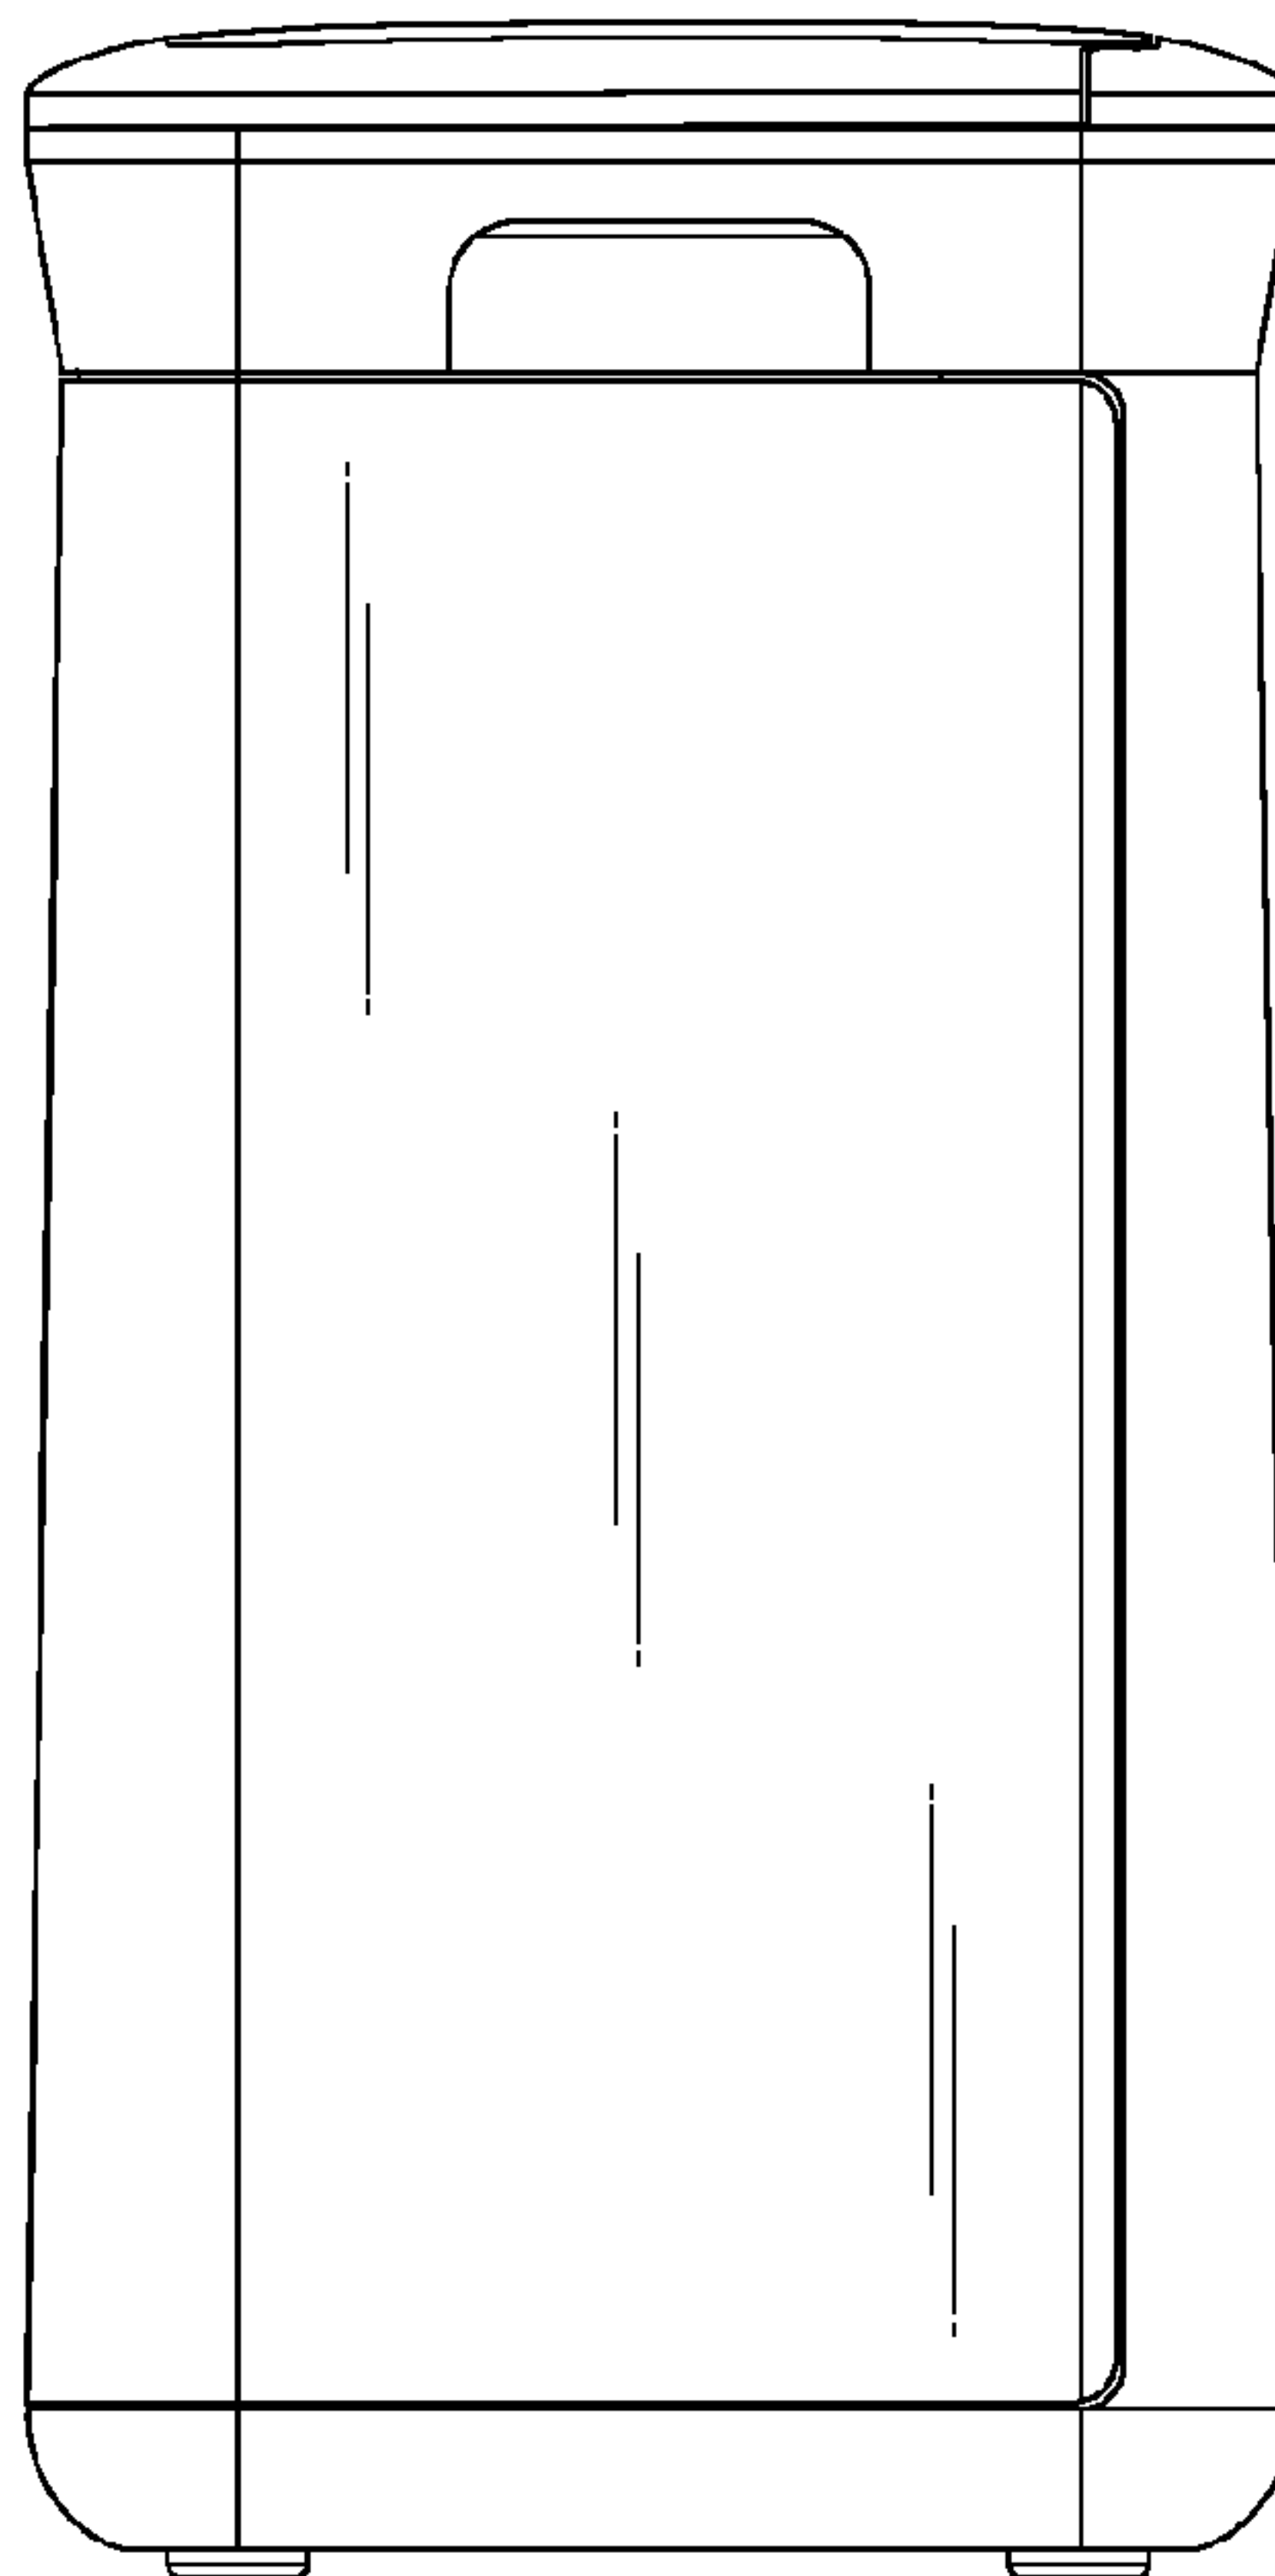


FIG. 5

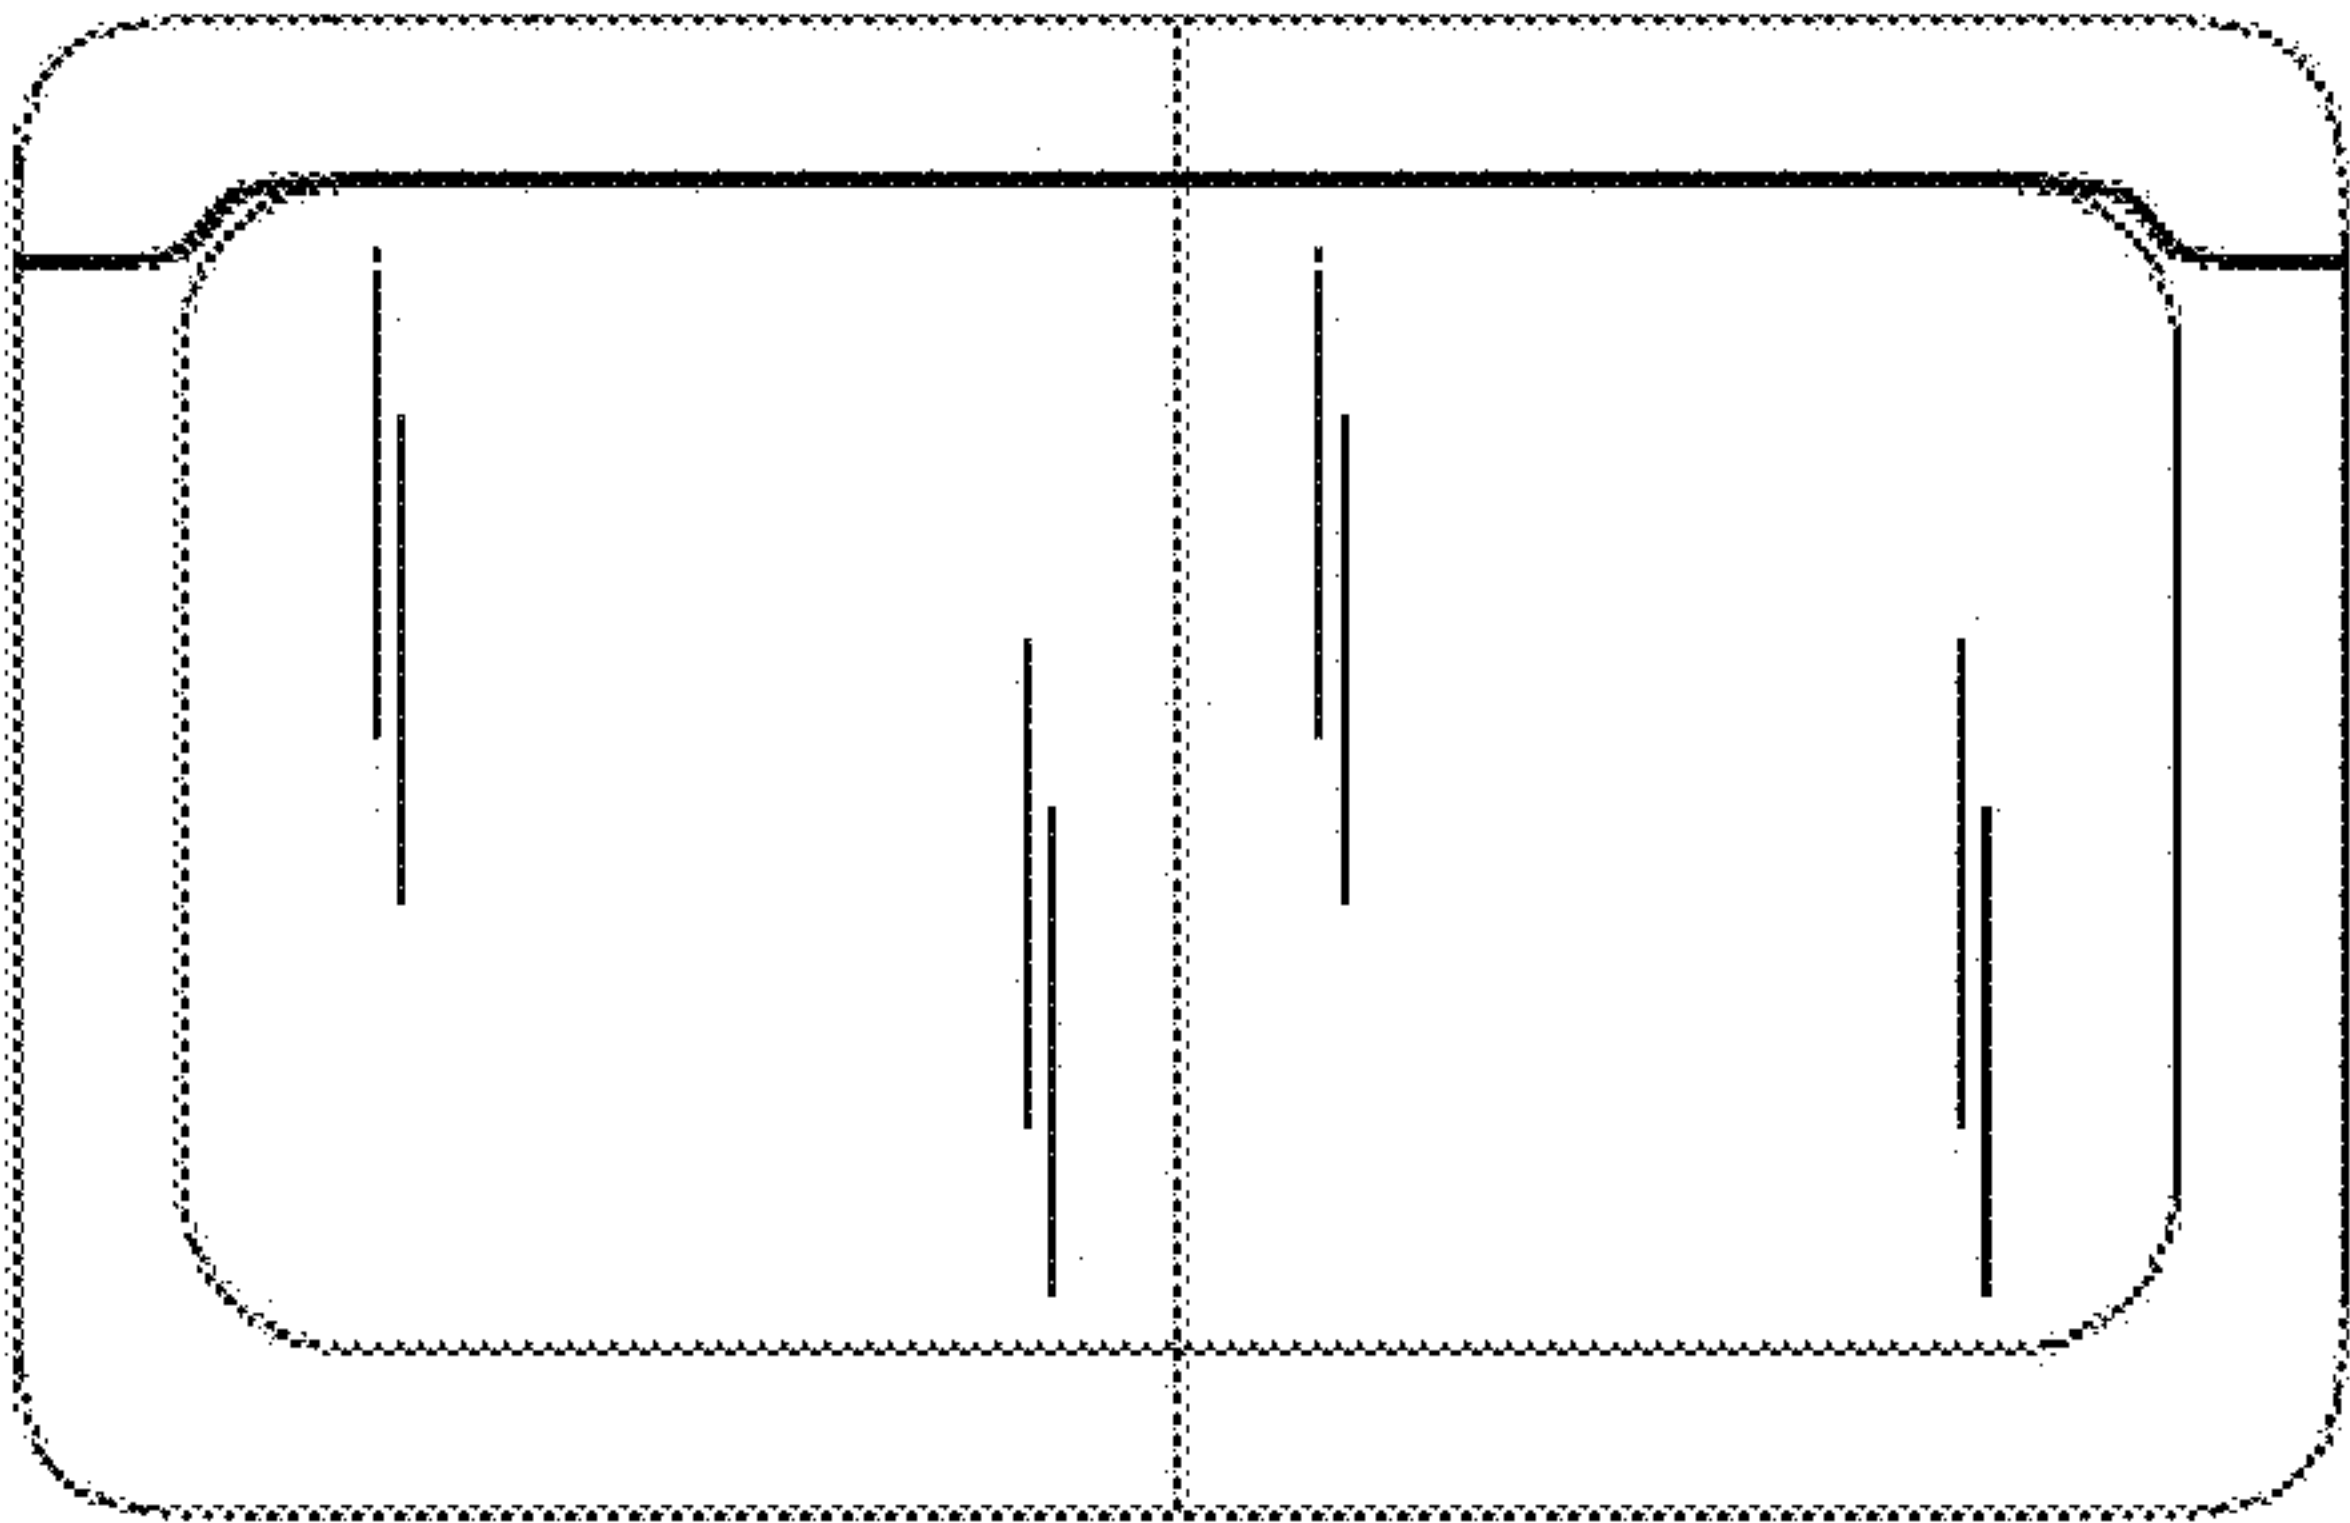


FIG. 6

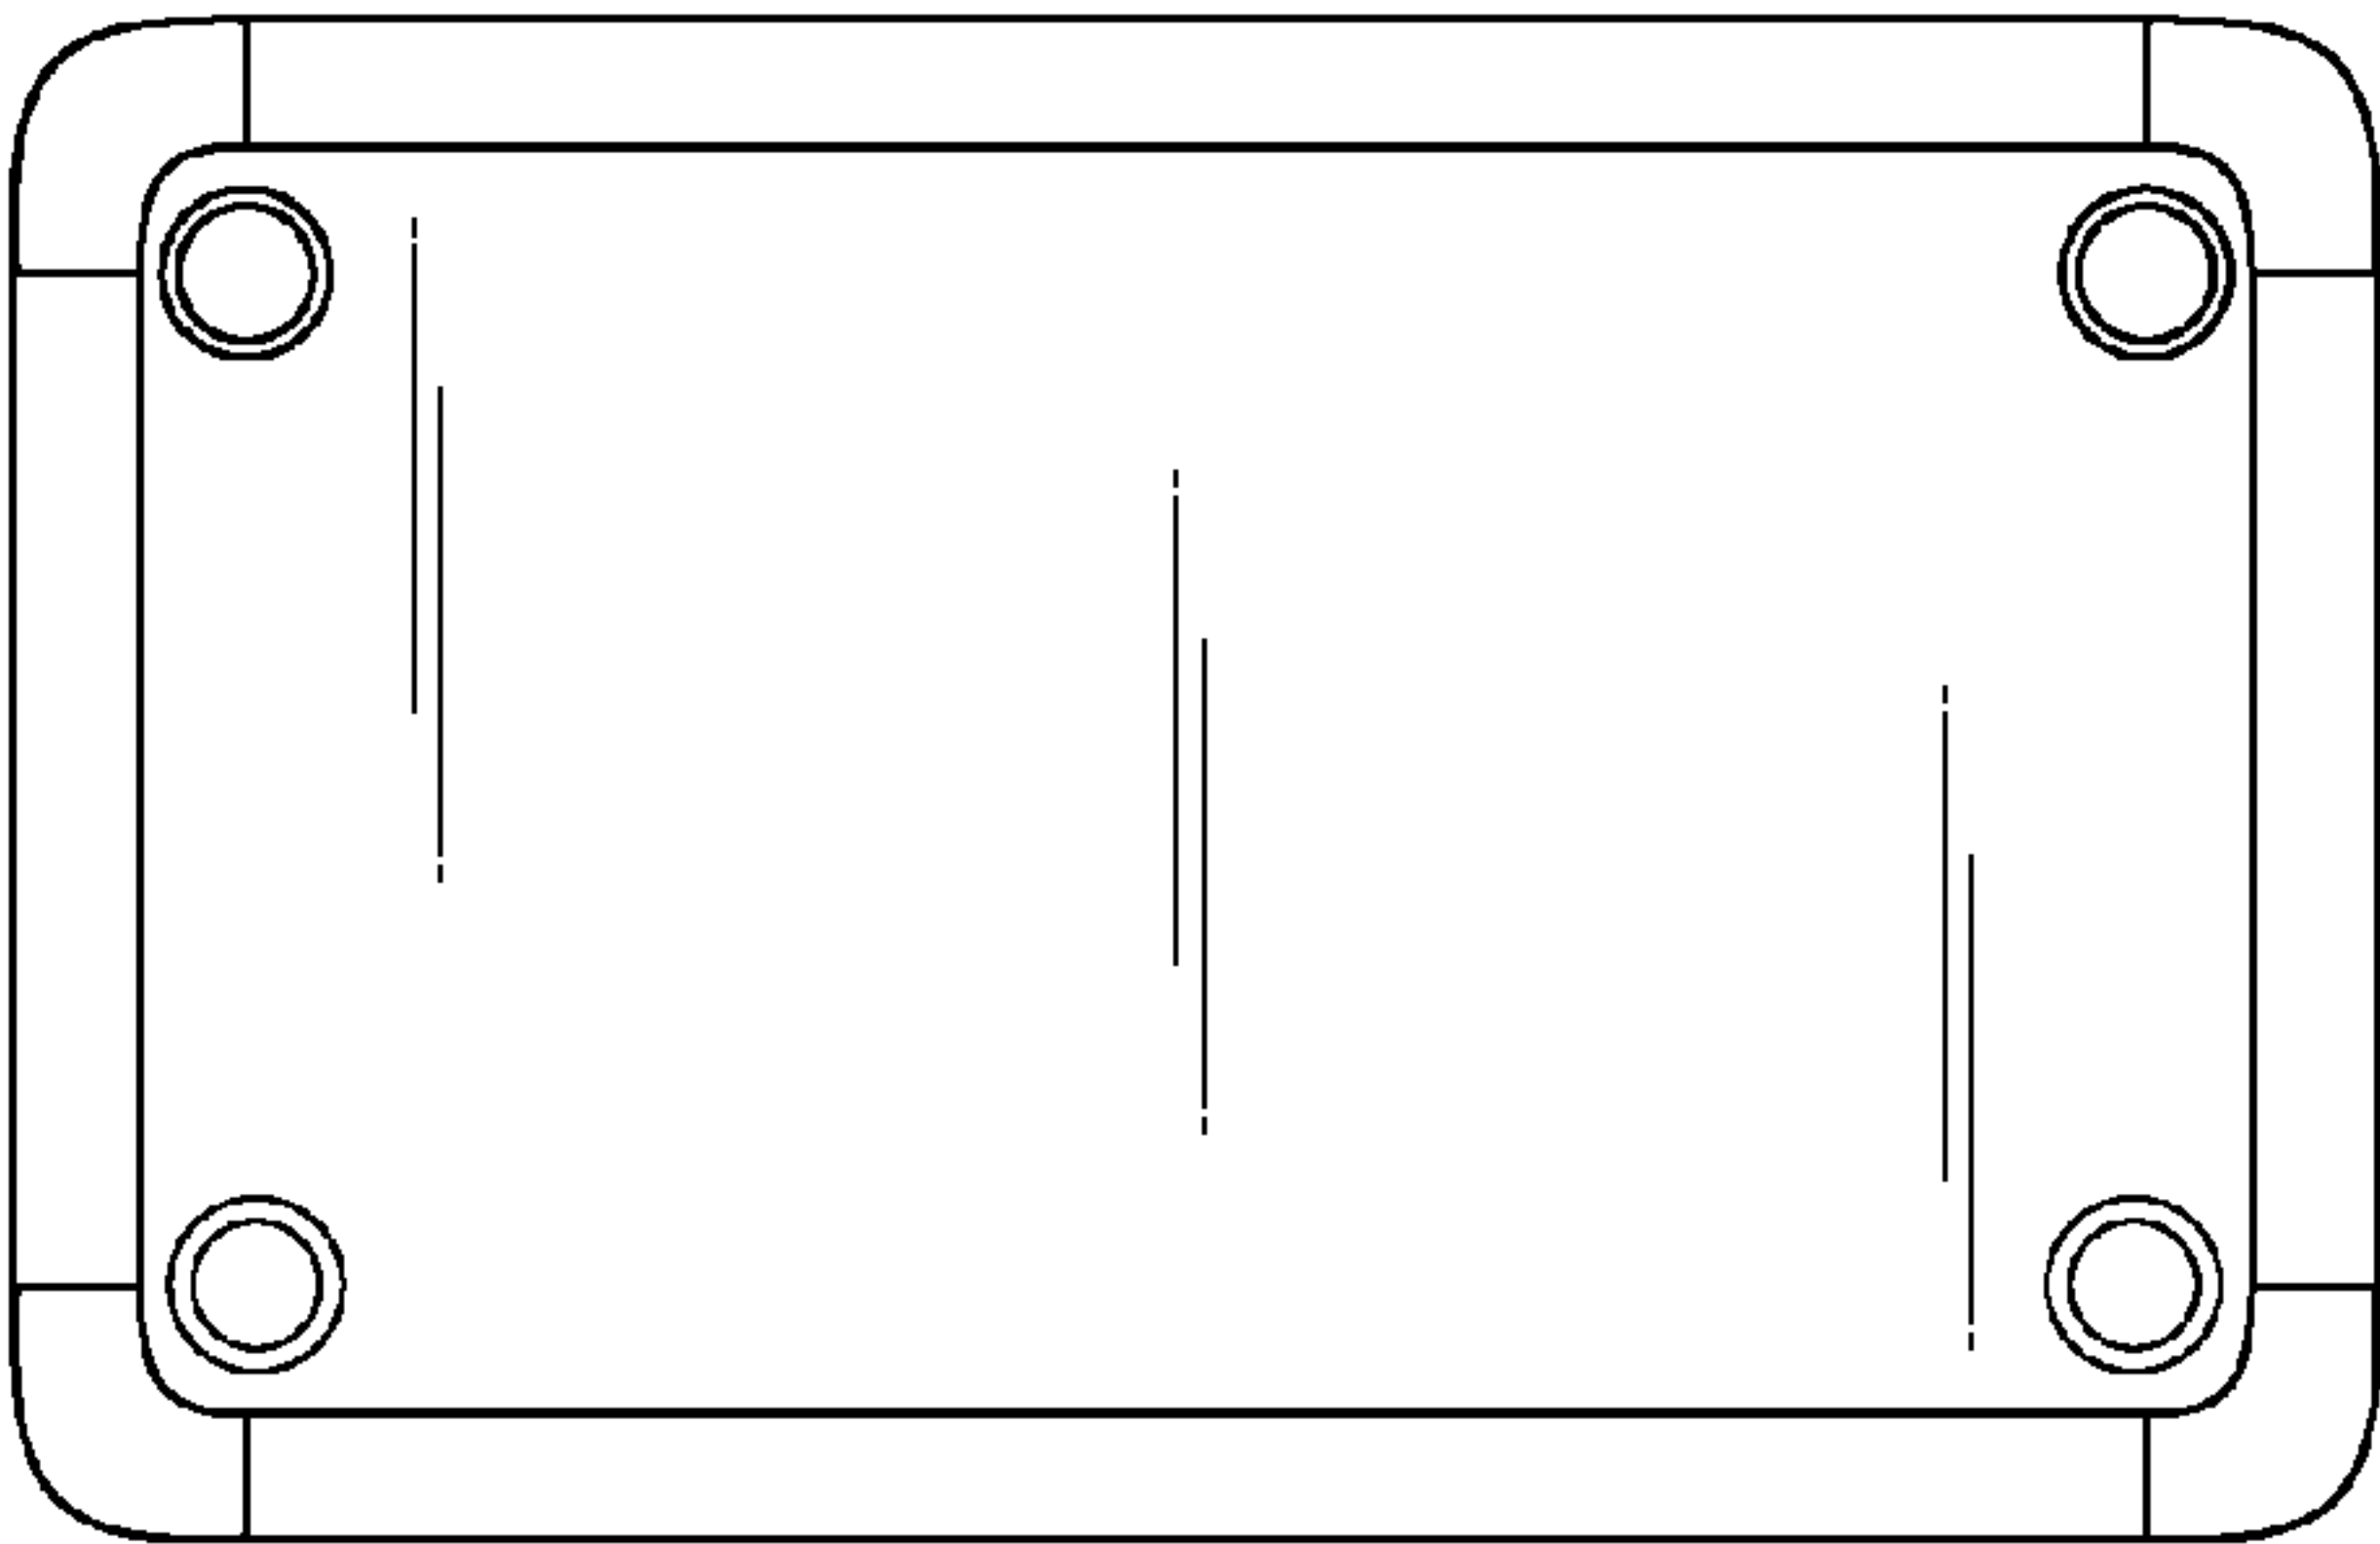


FIG. 7

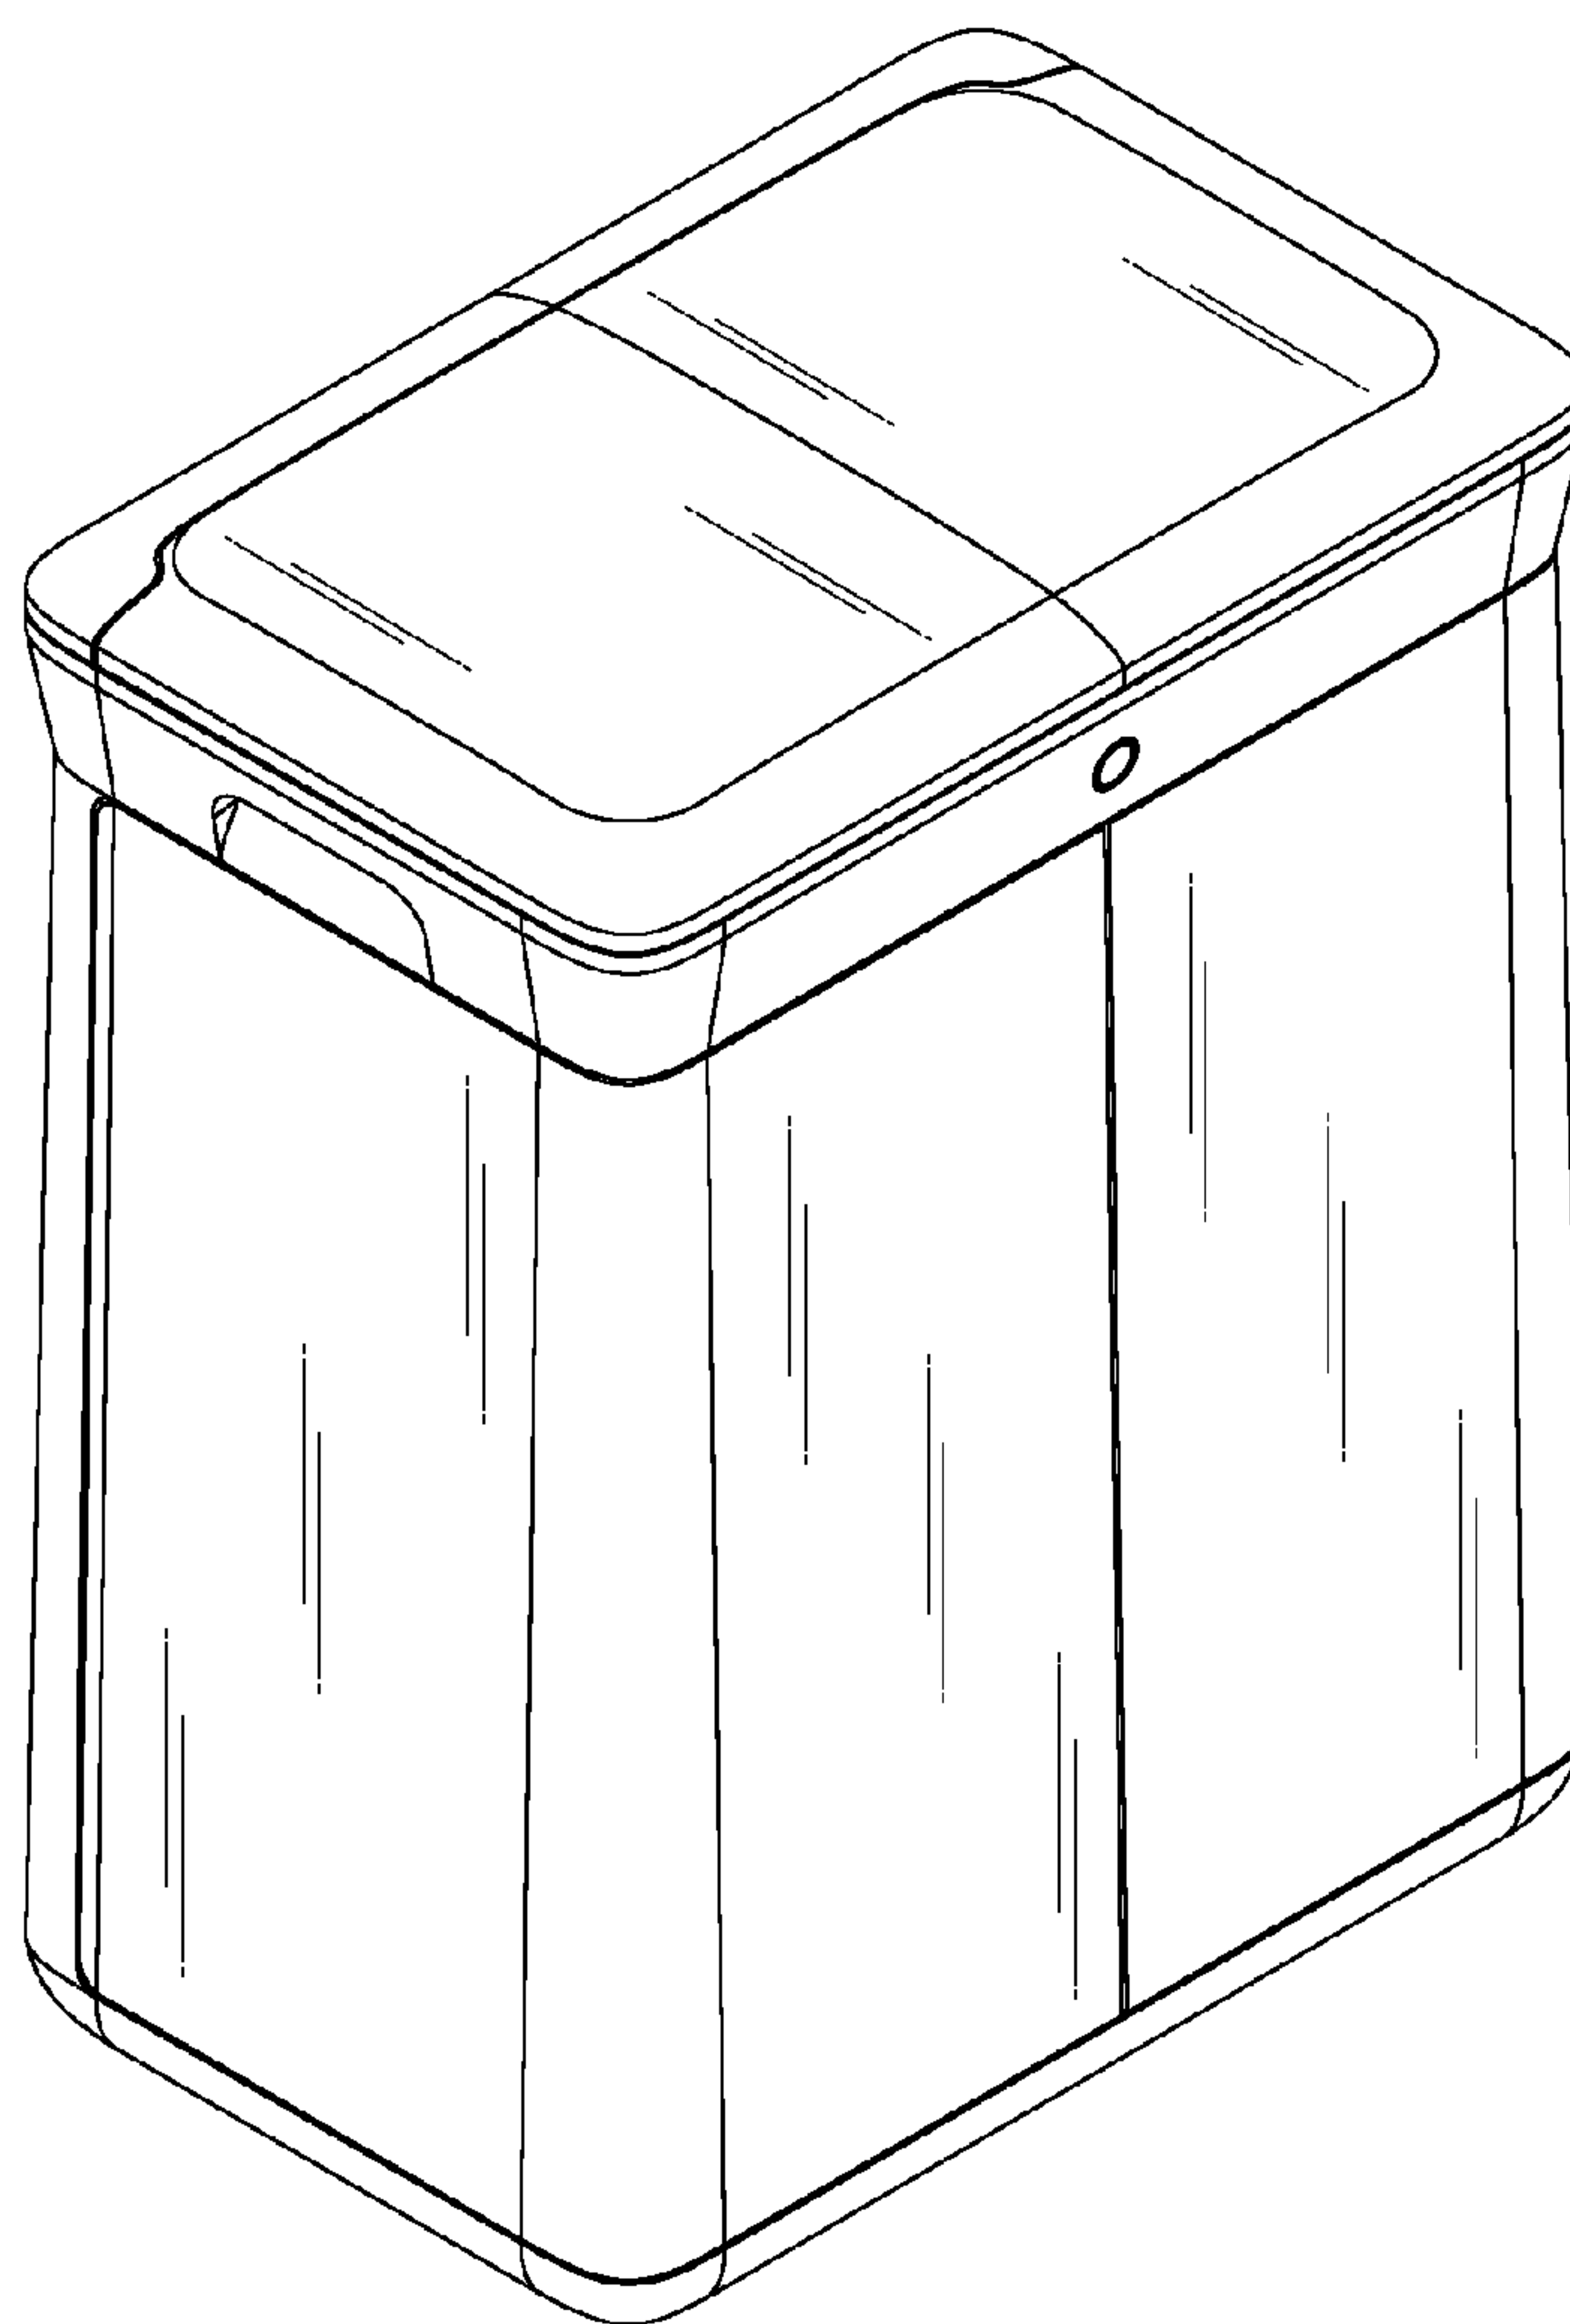


FIG. 8

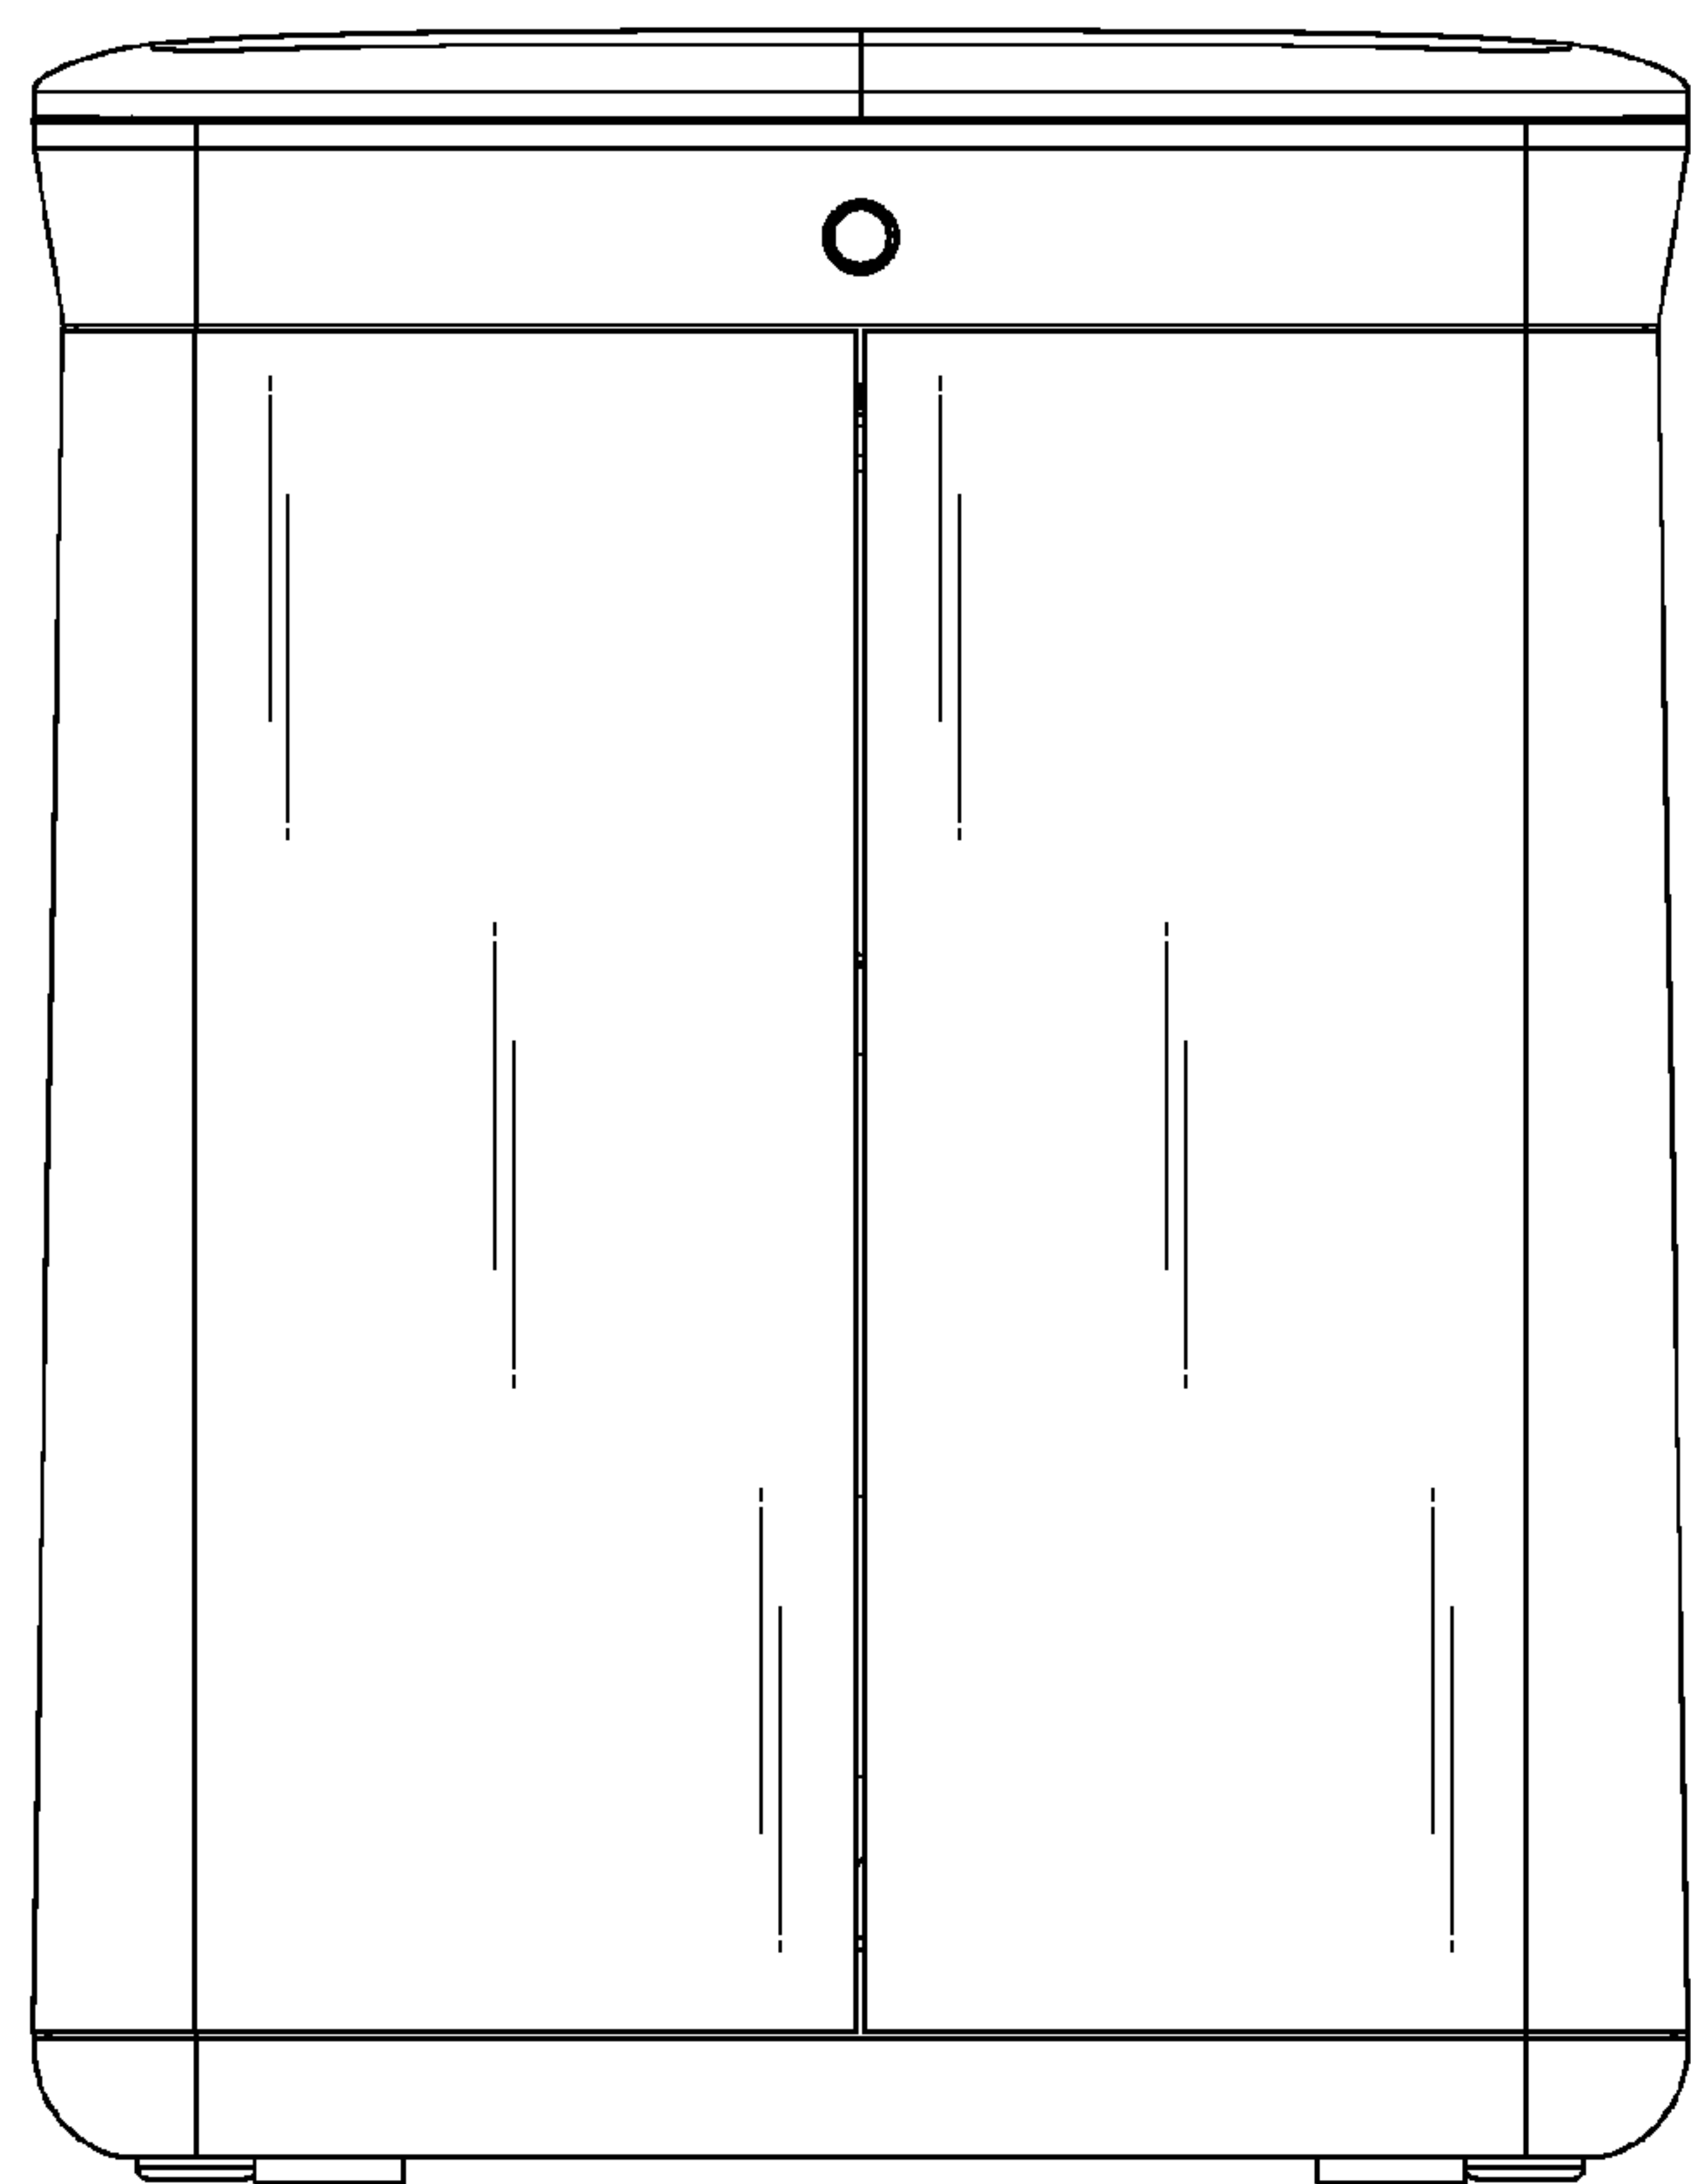


FIG. 9

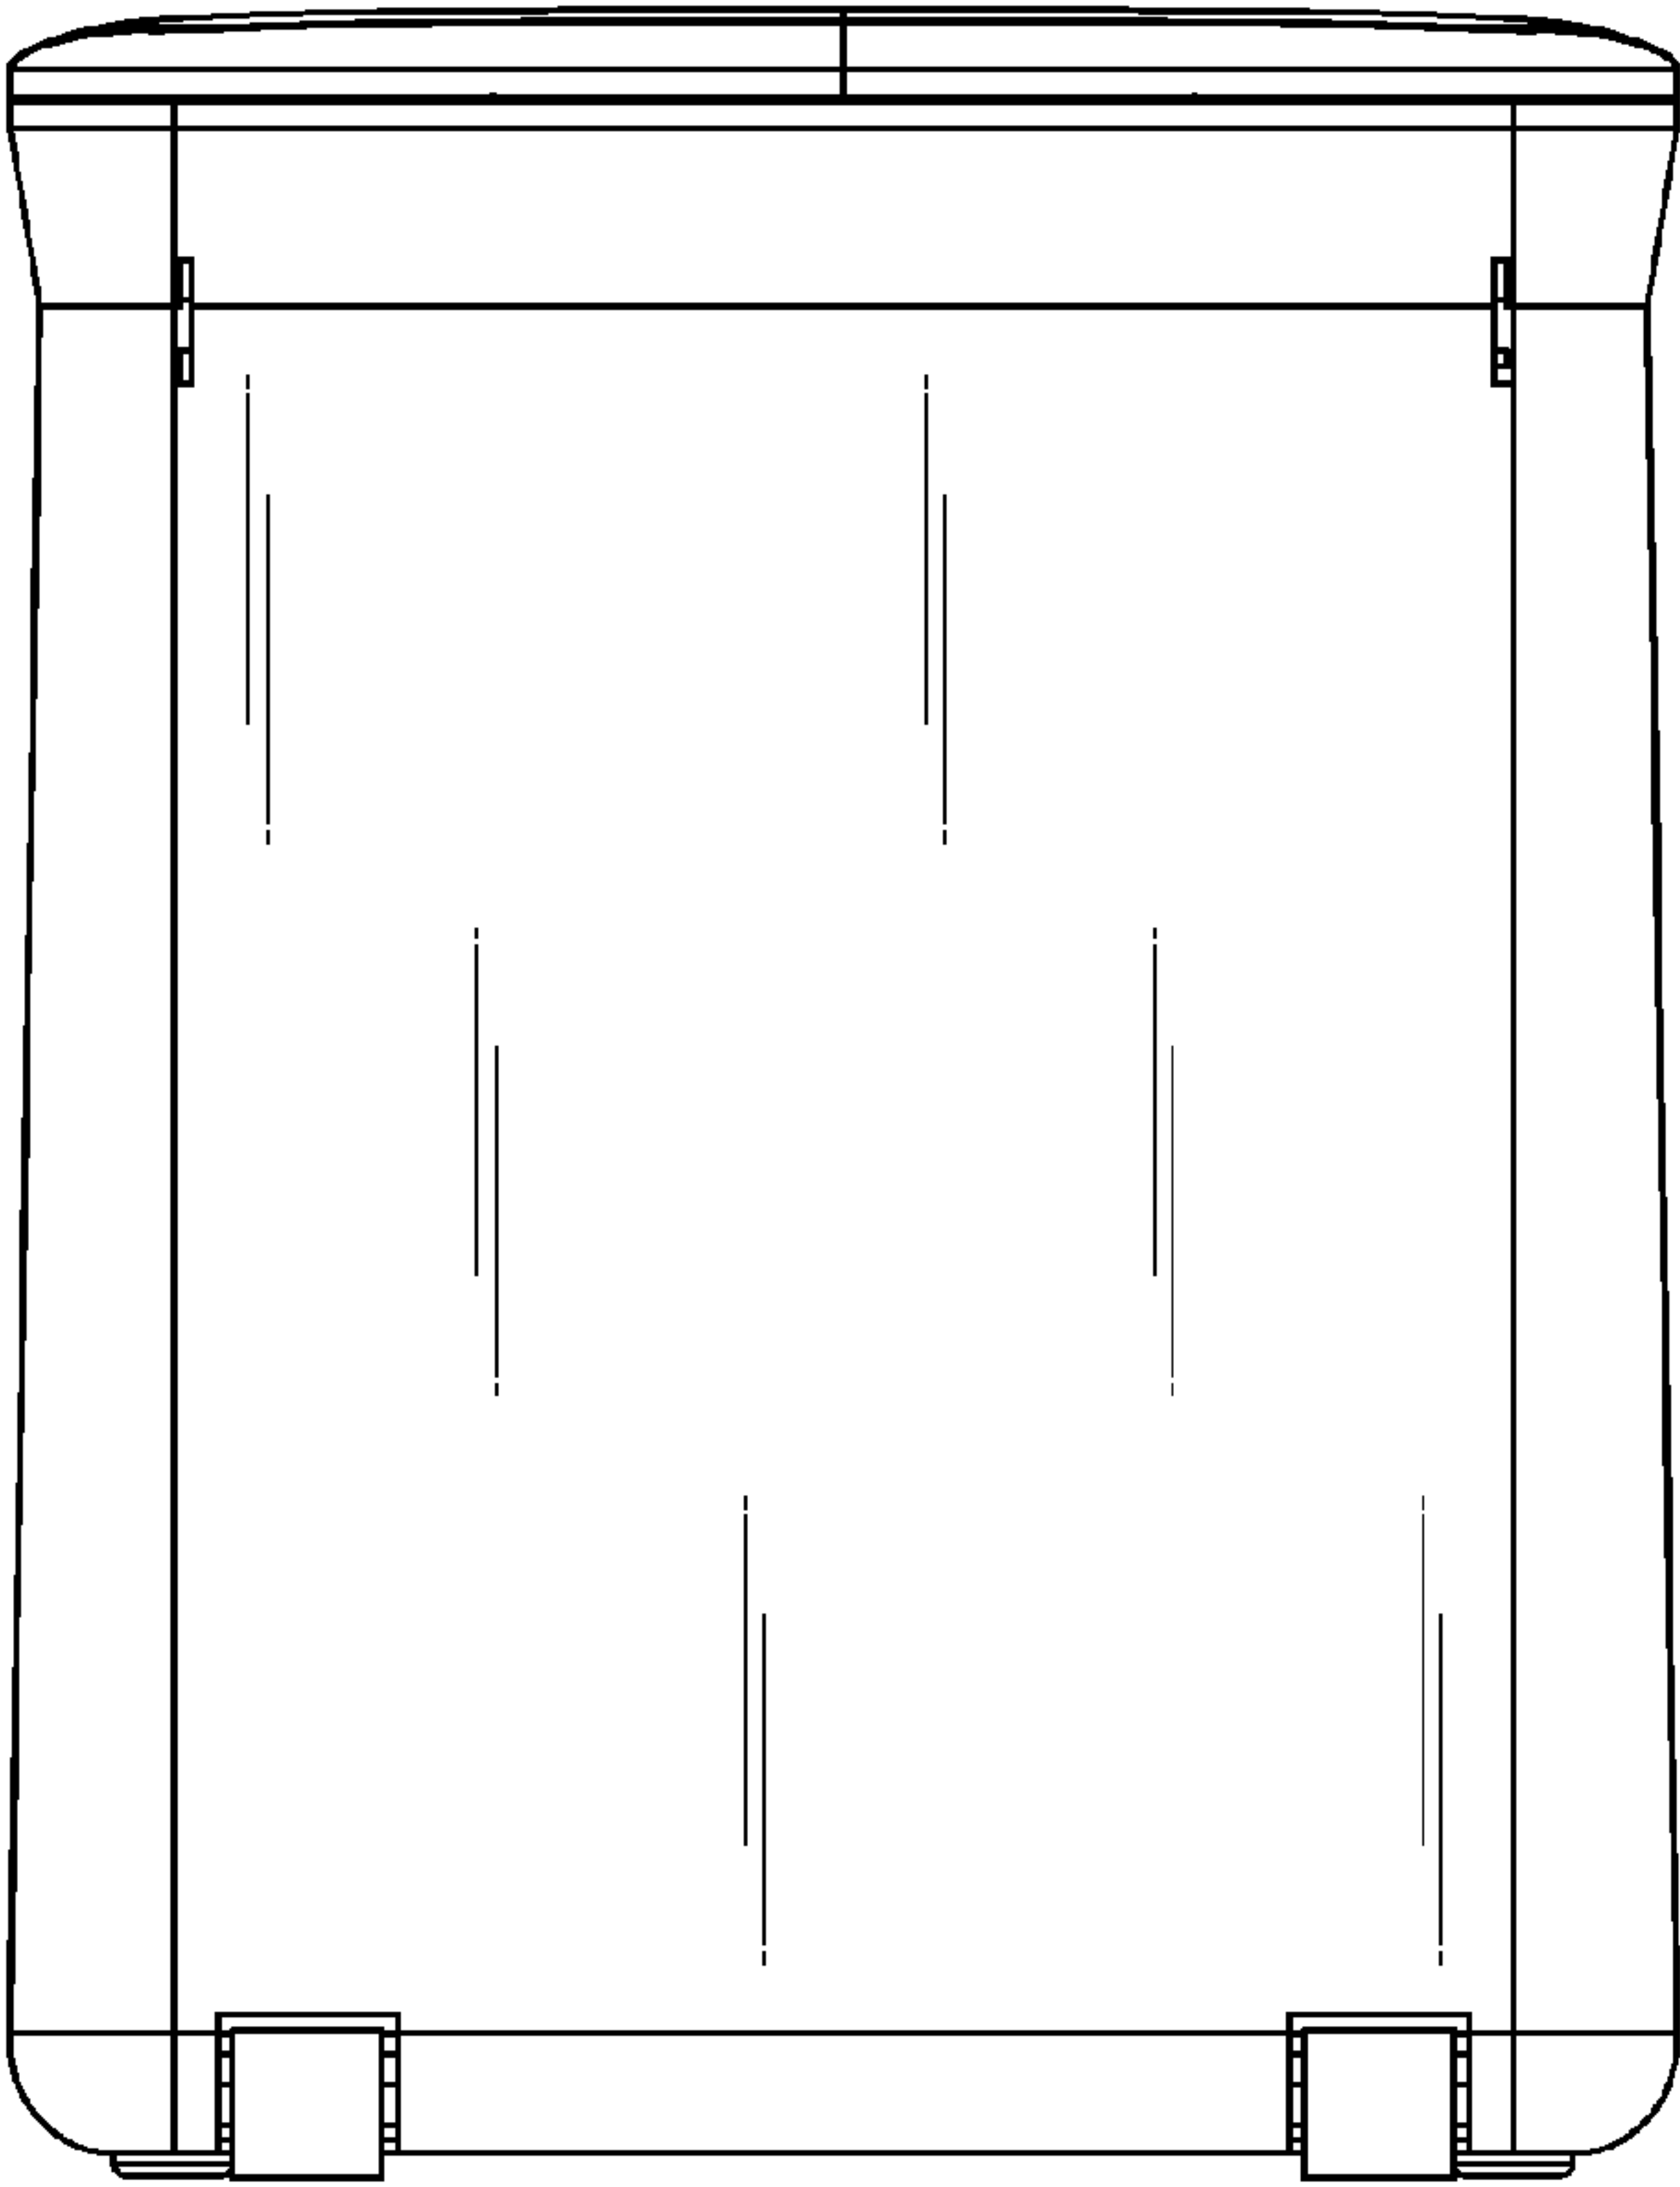


FIG. 10

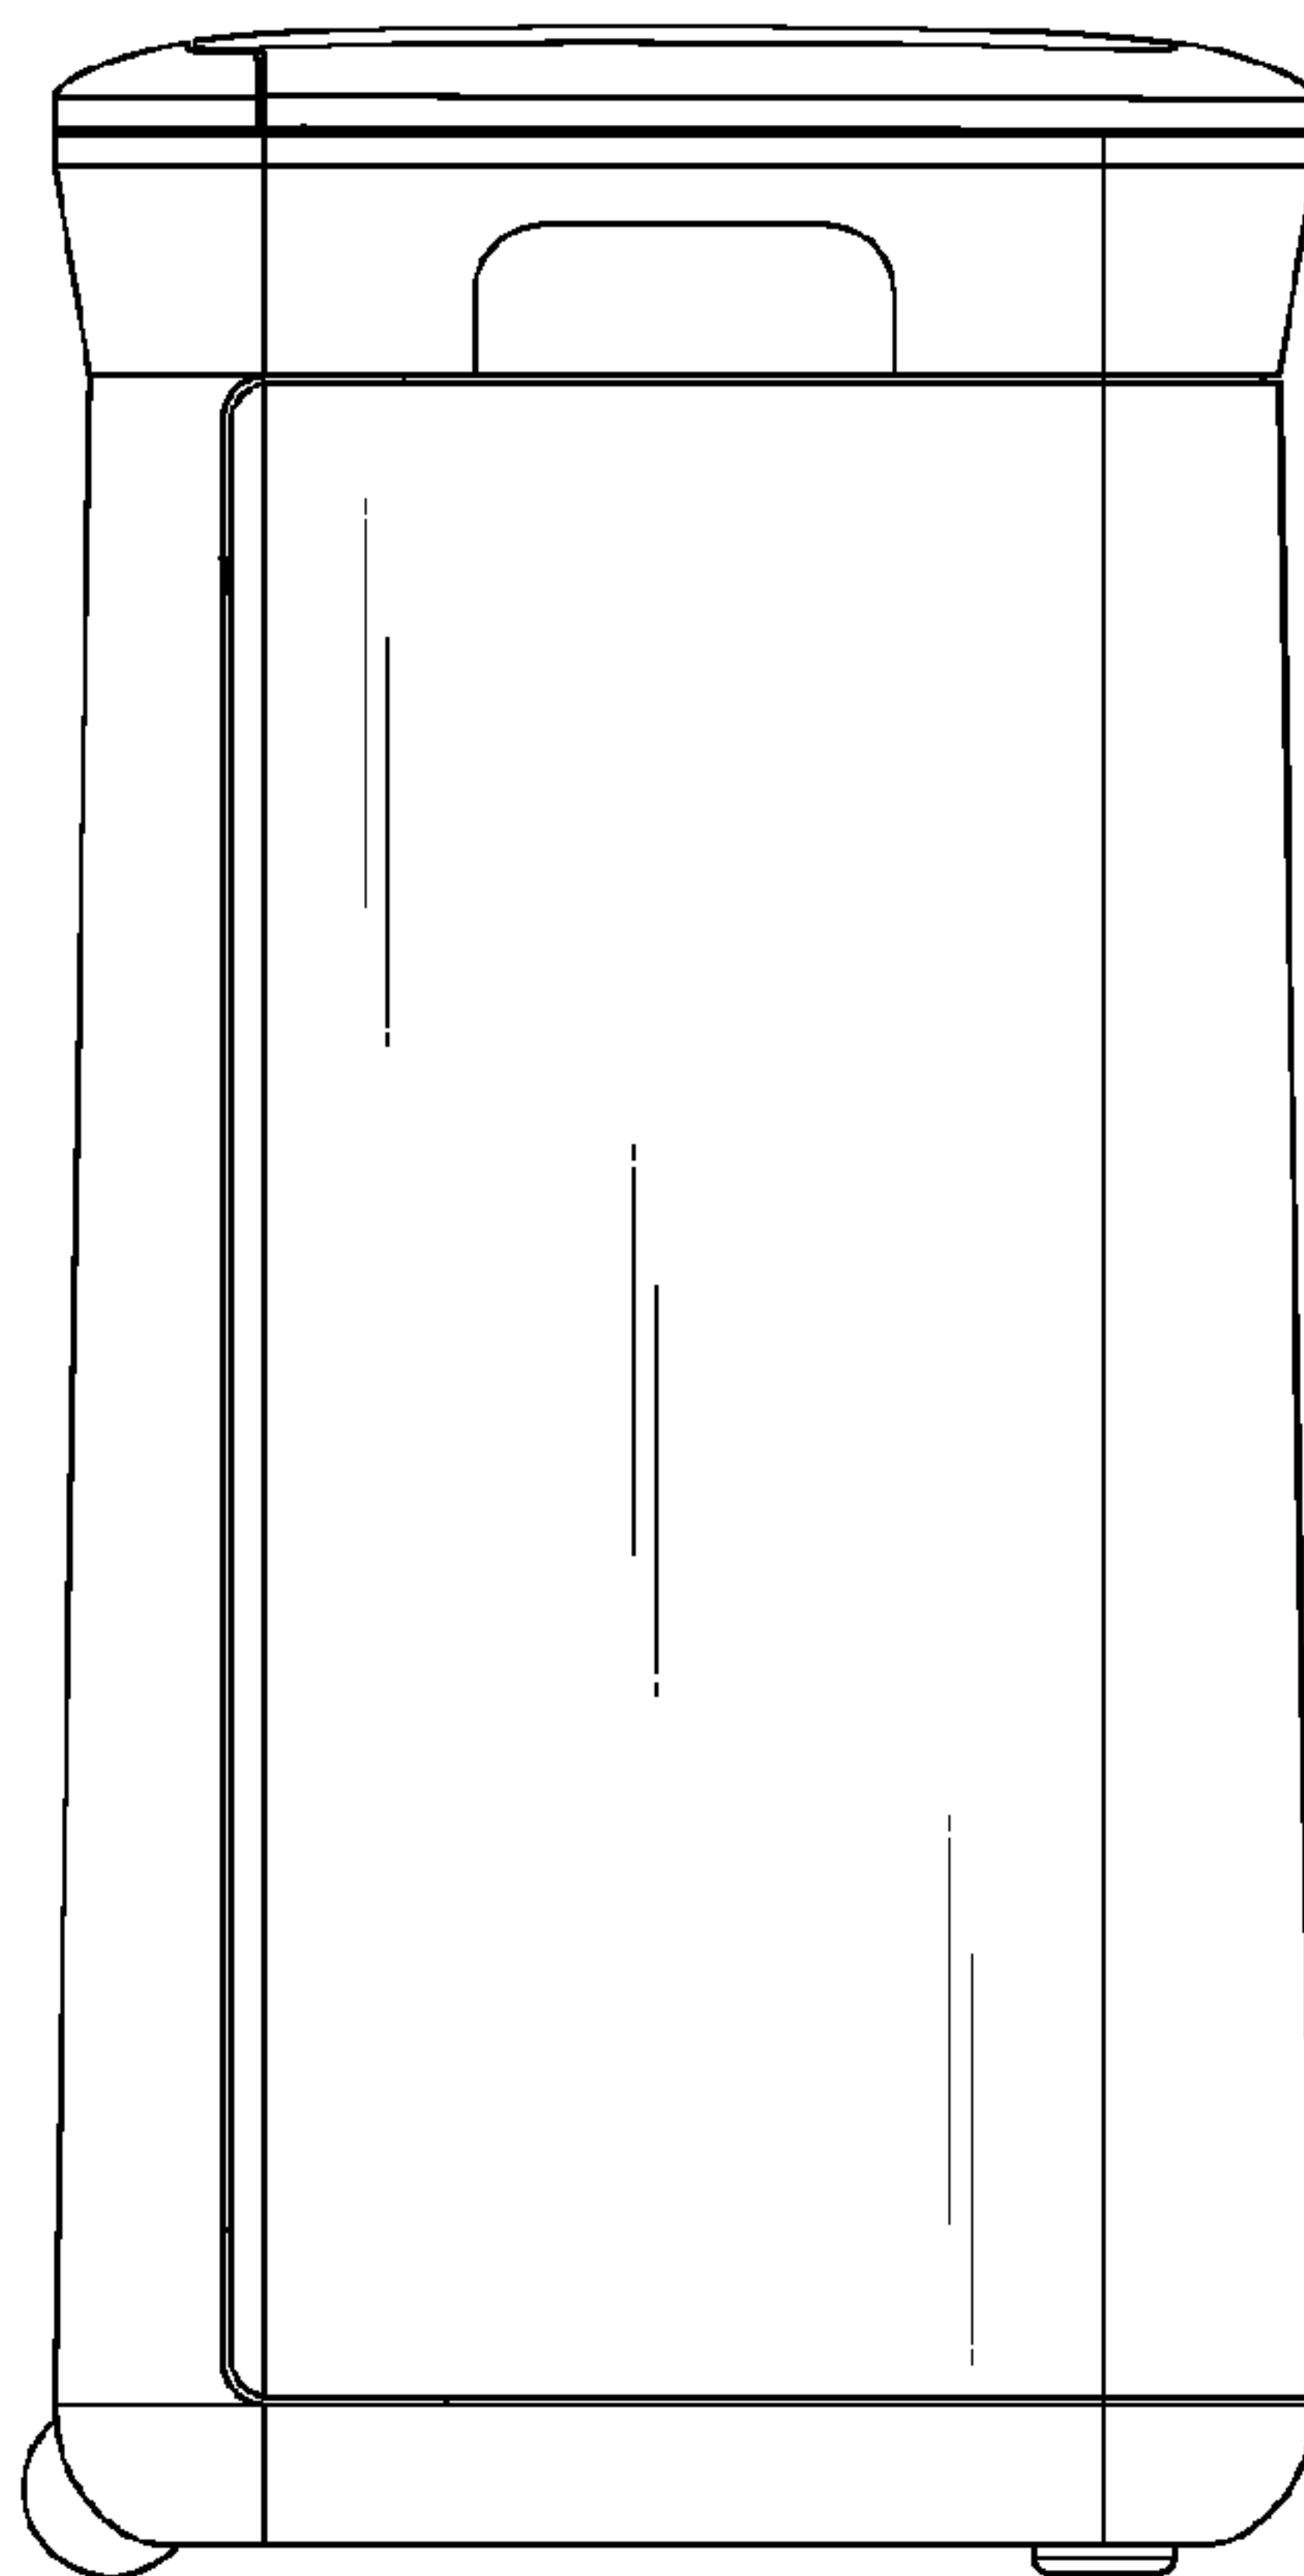


FIG. 11

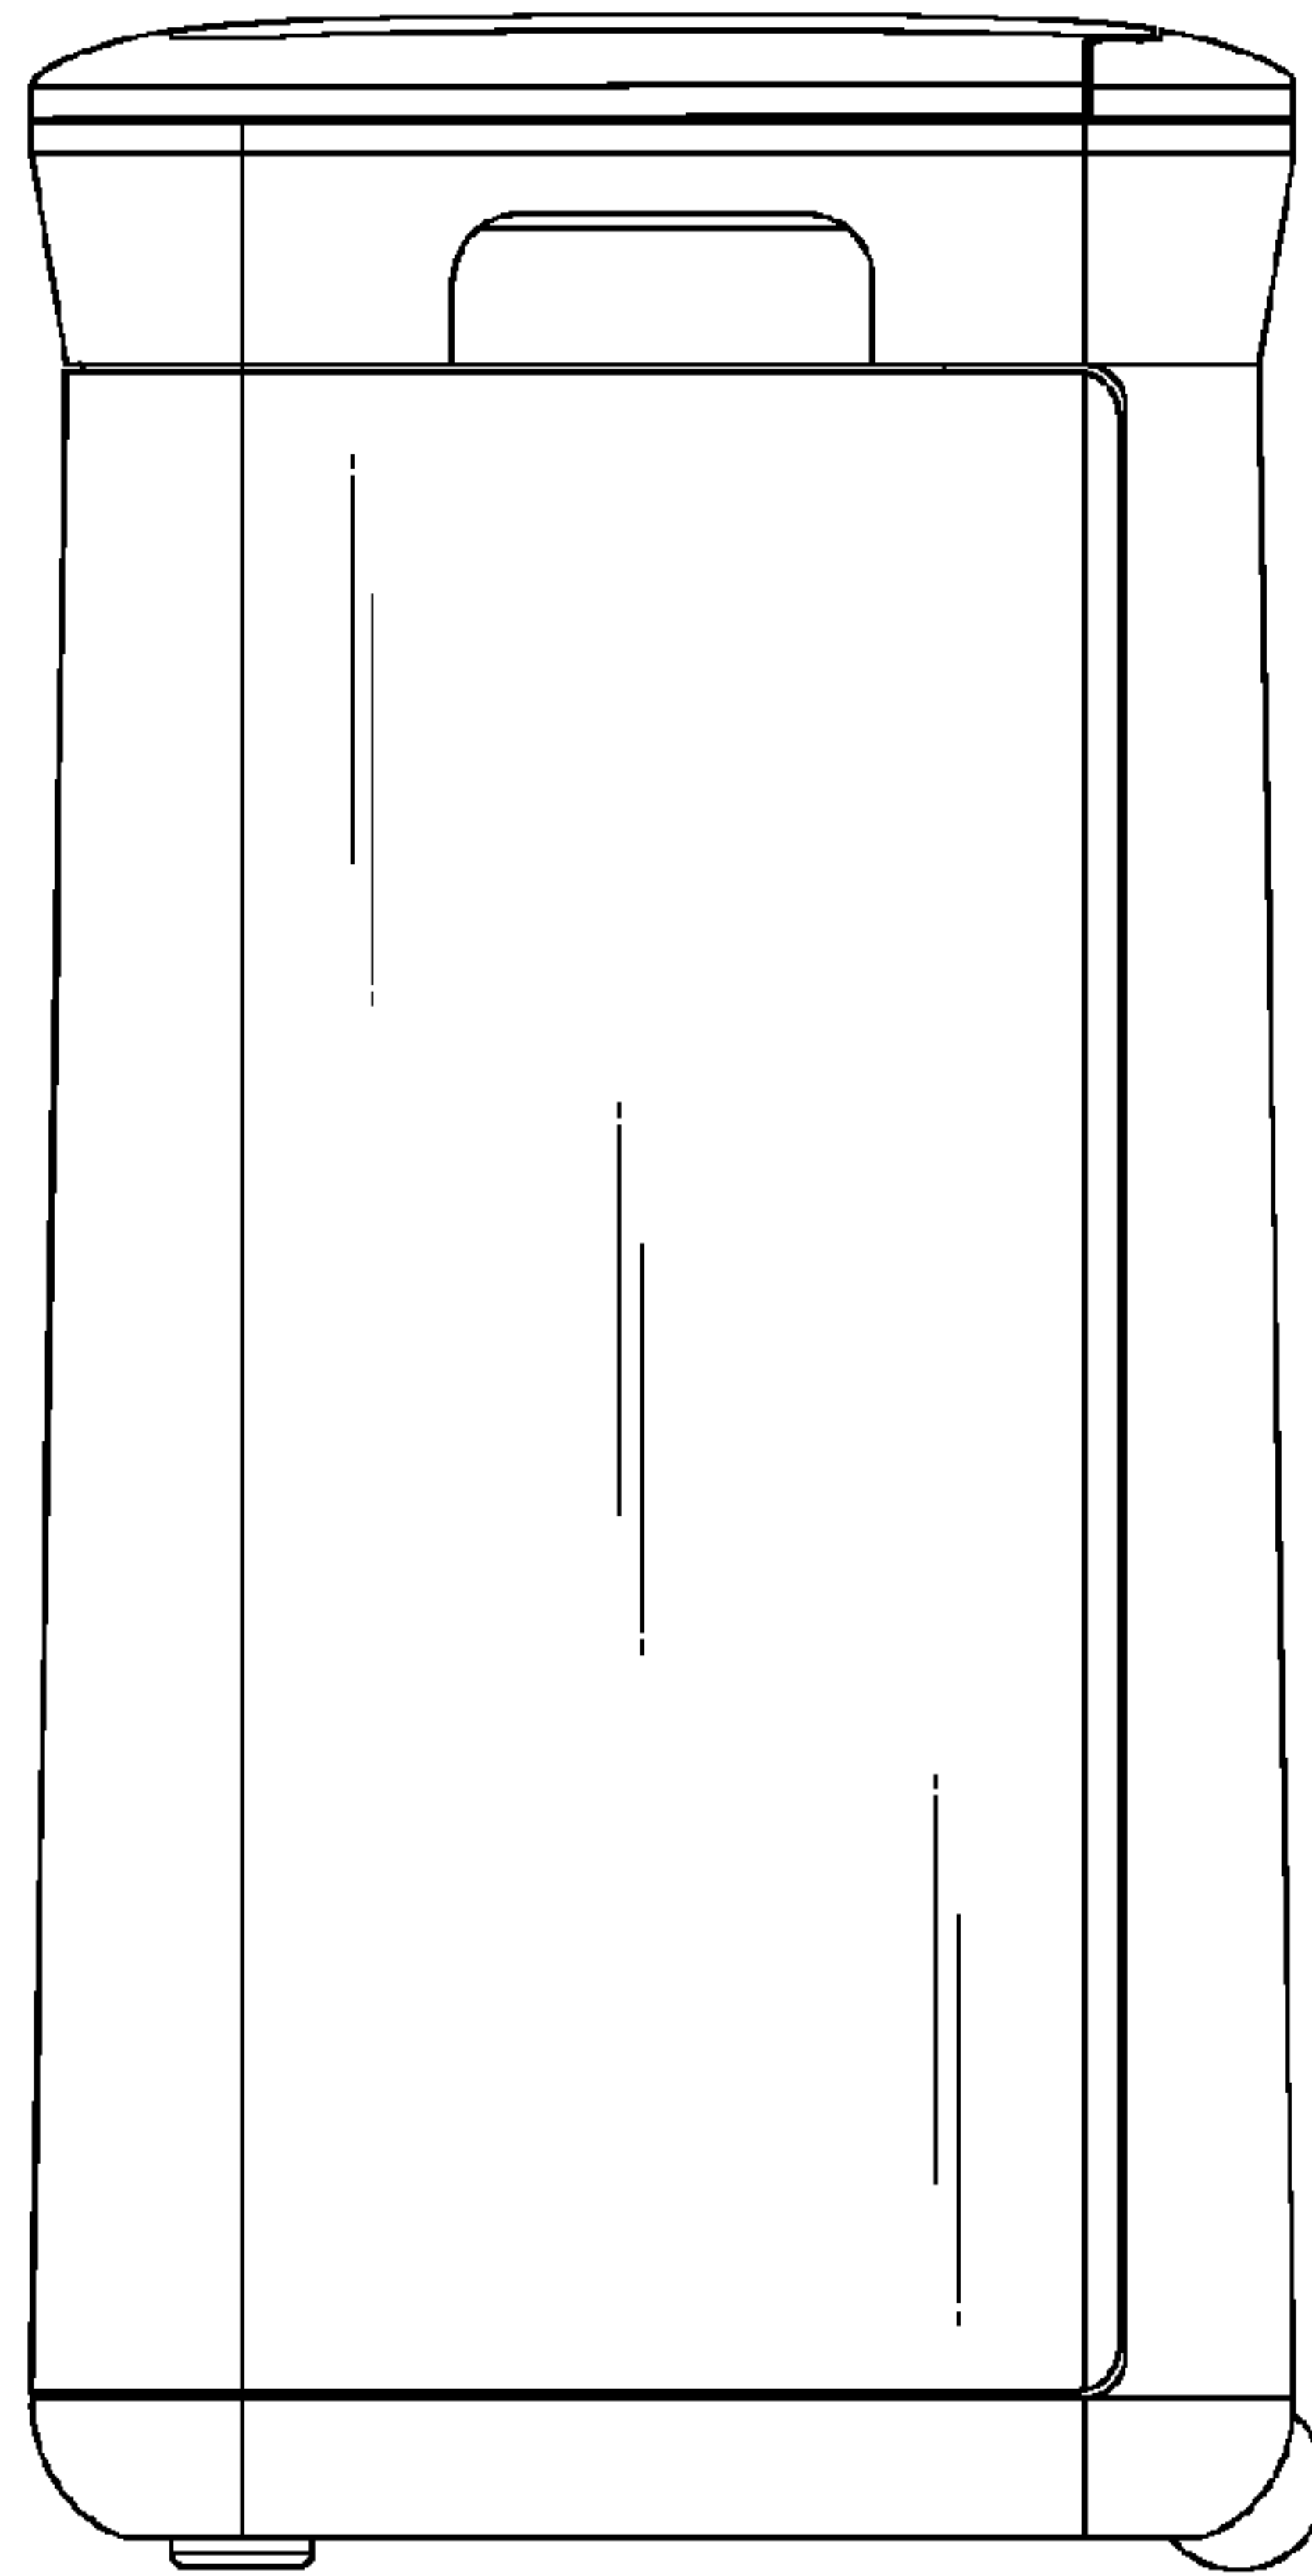


FIG. 12

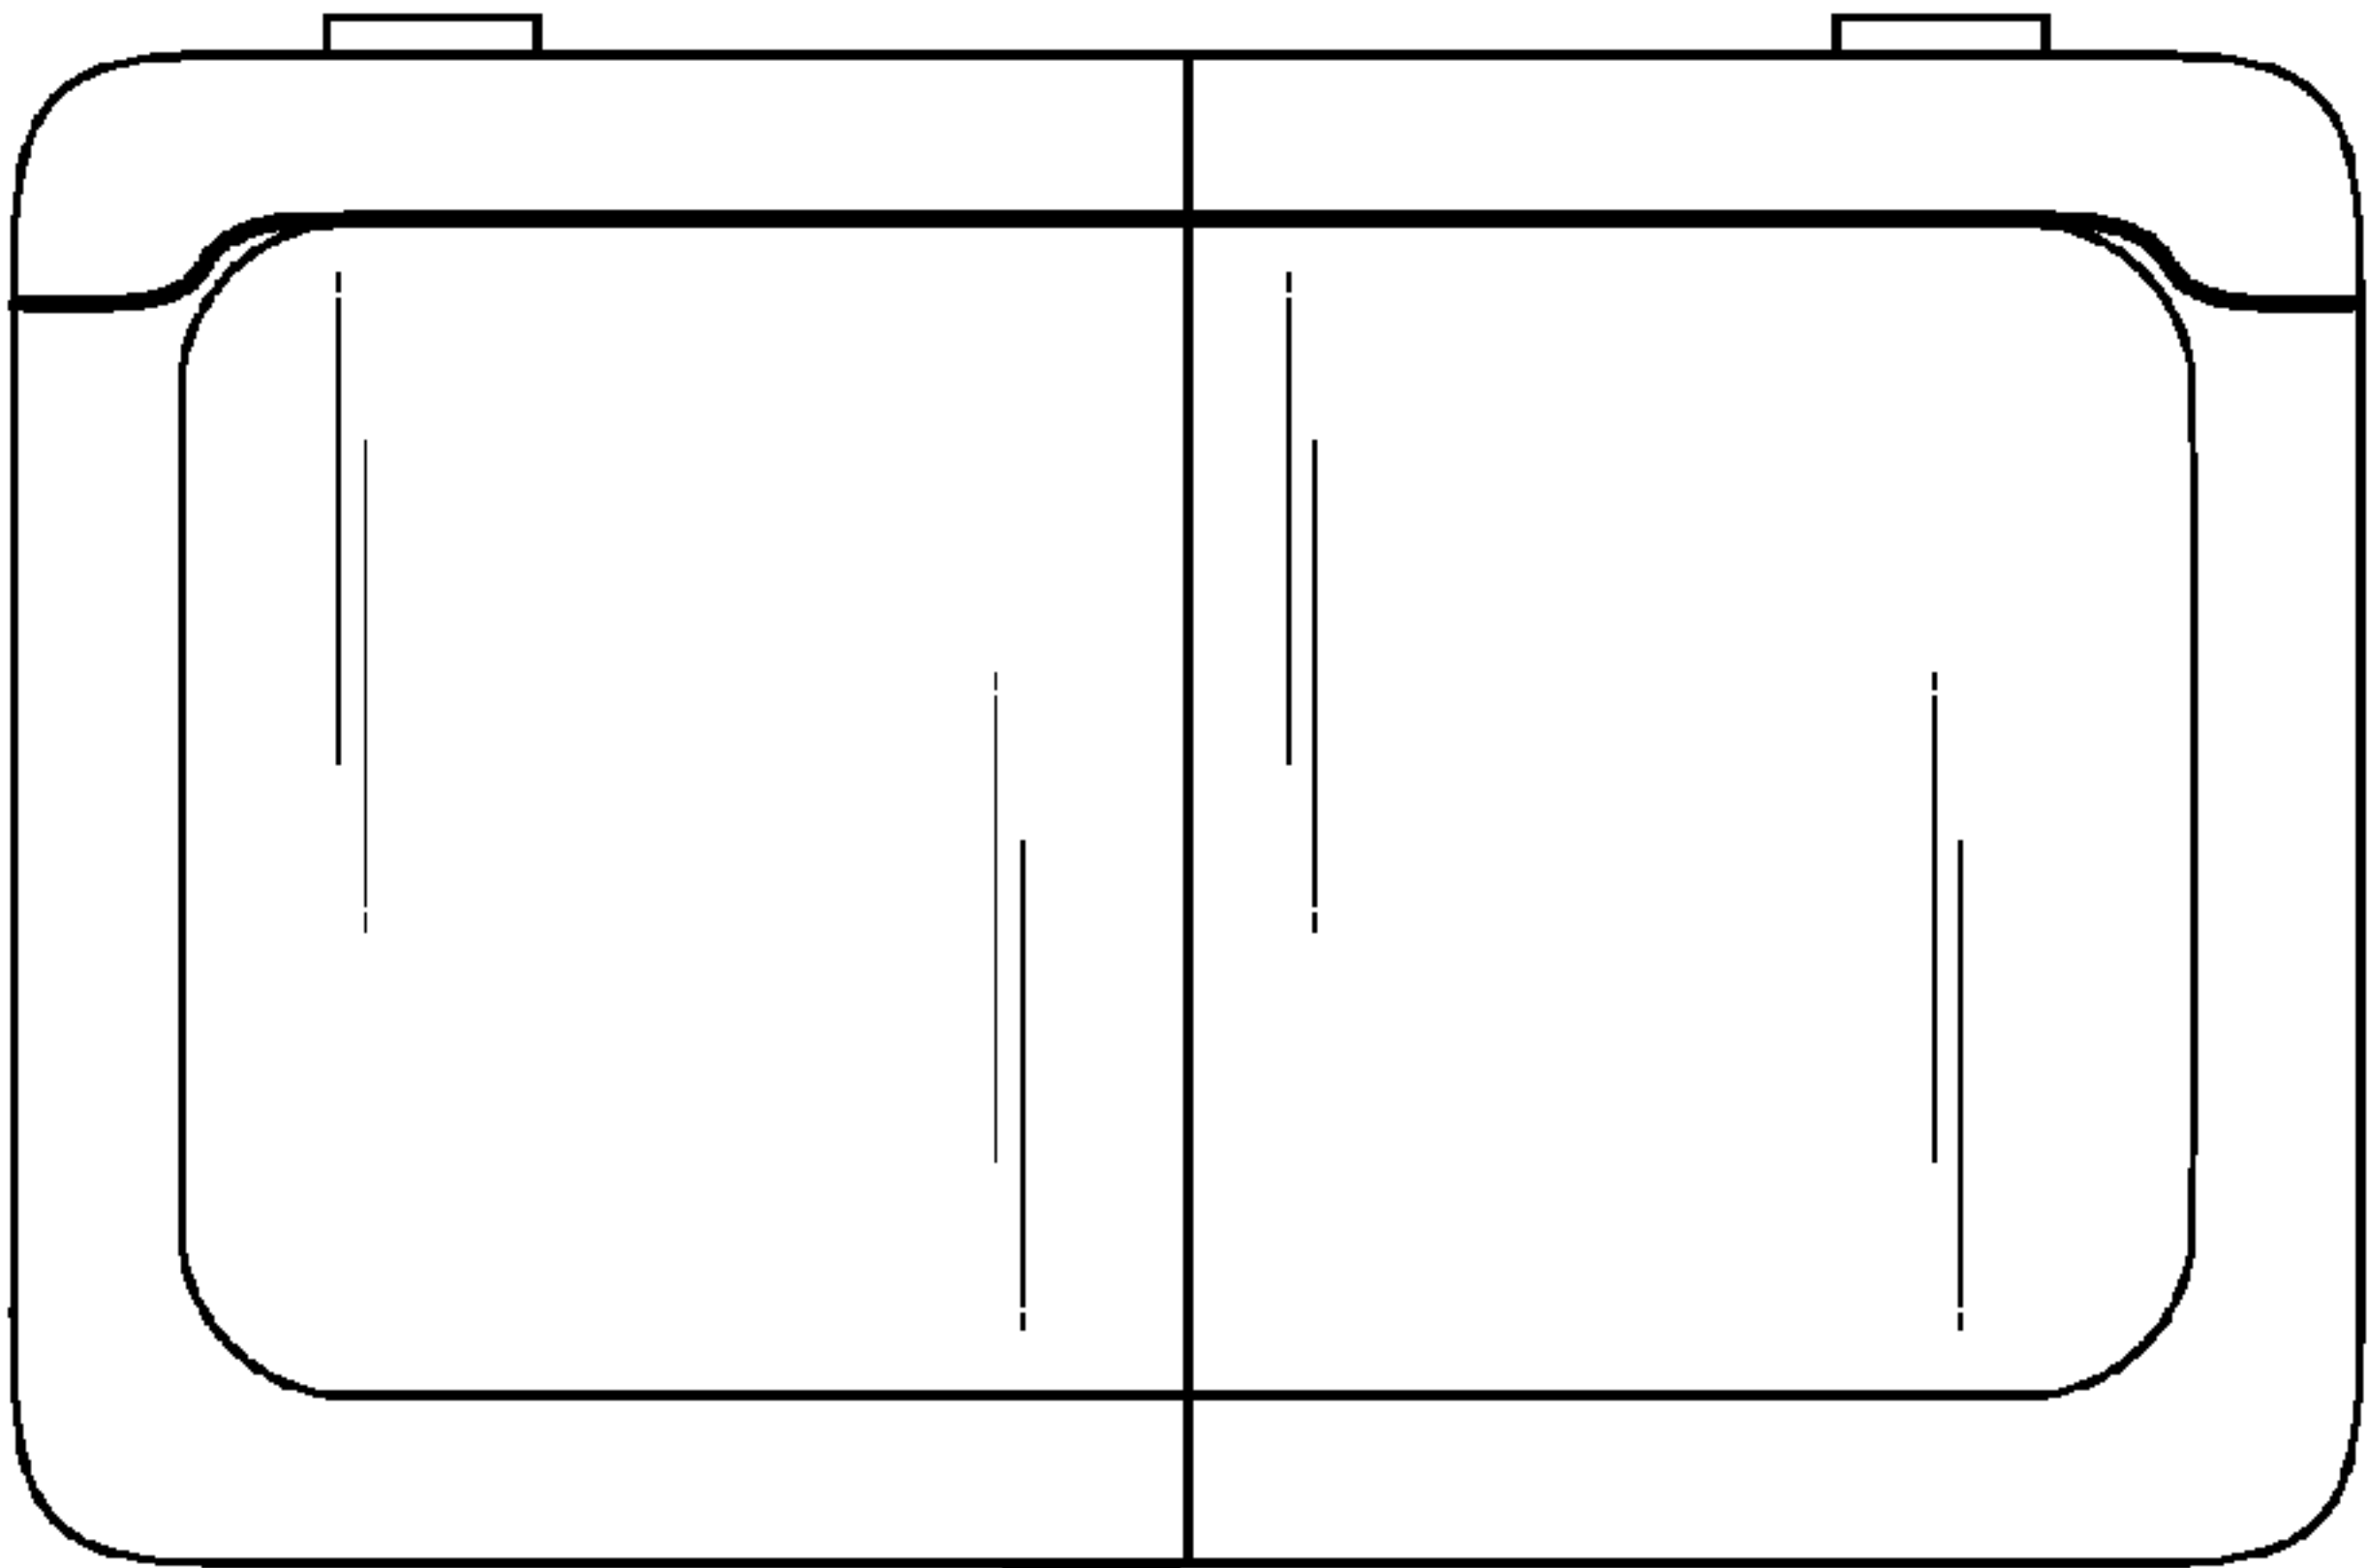


FIG. 13

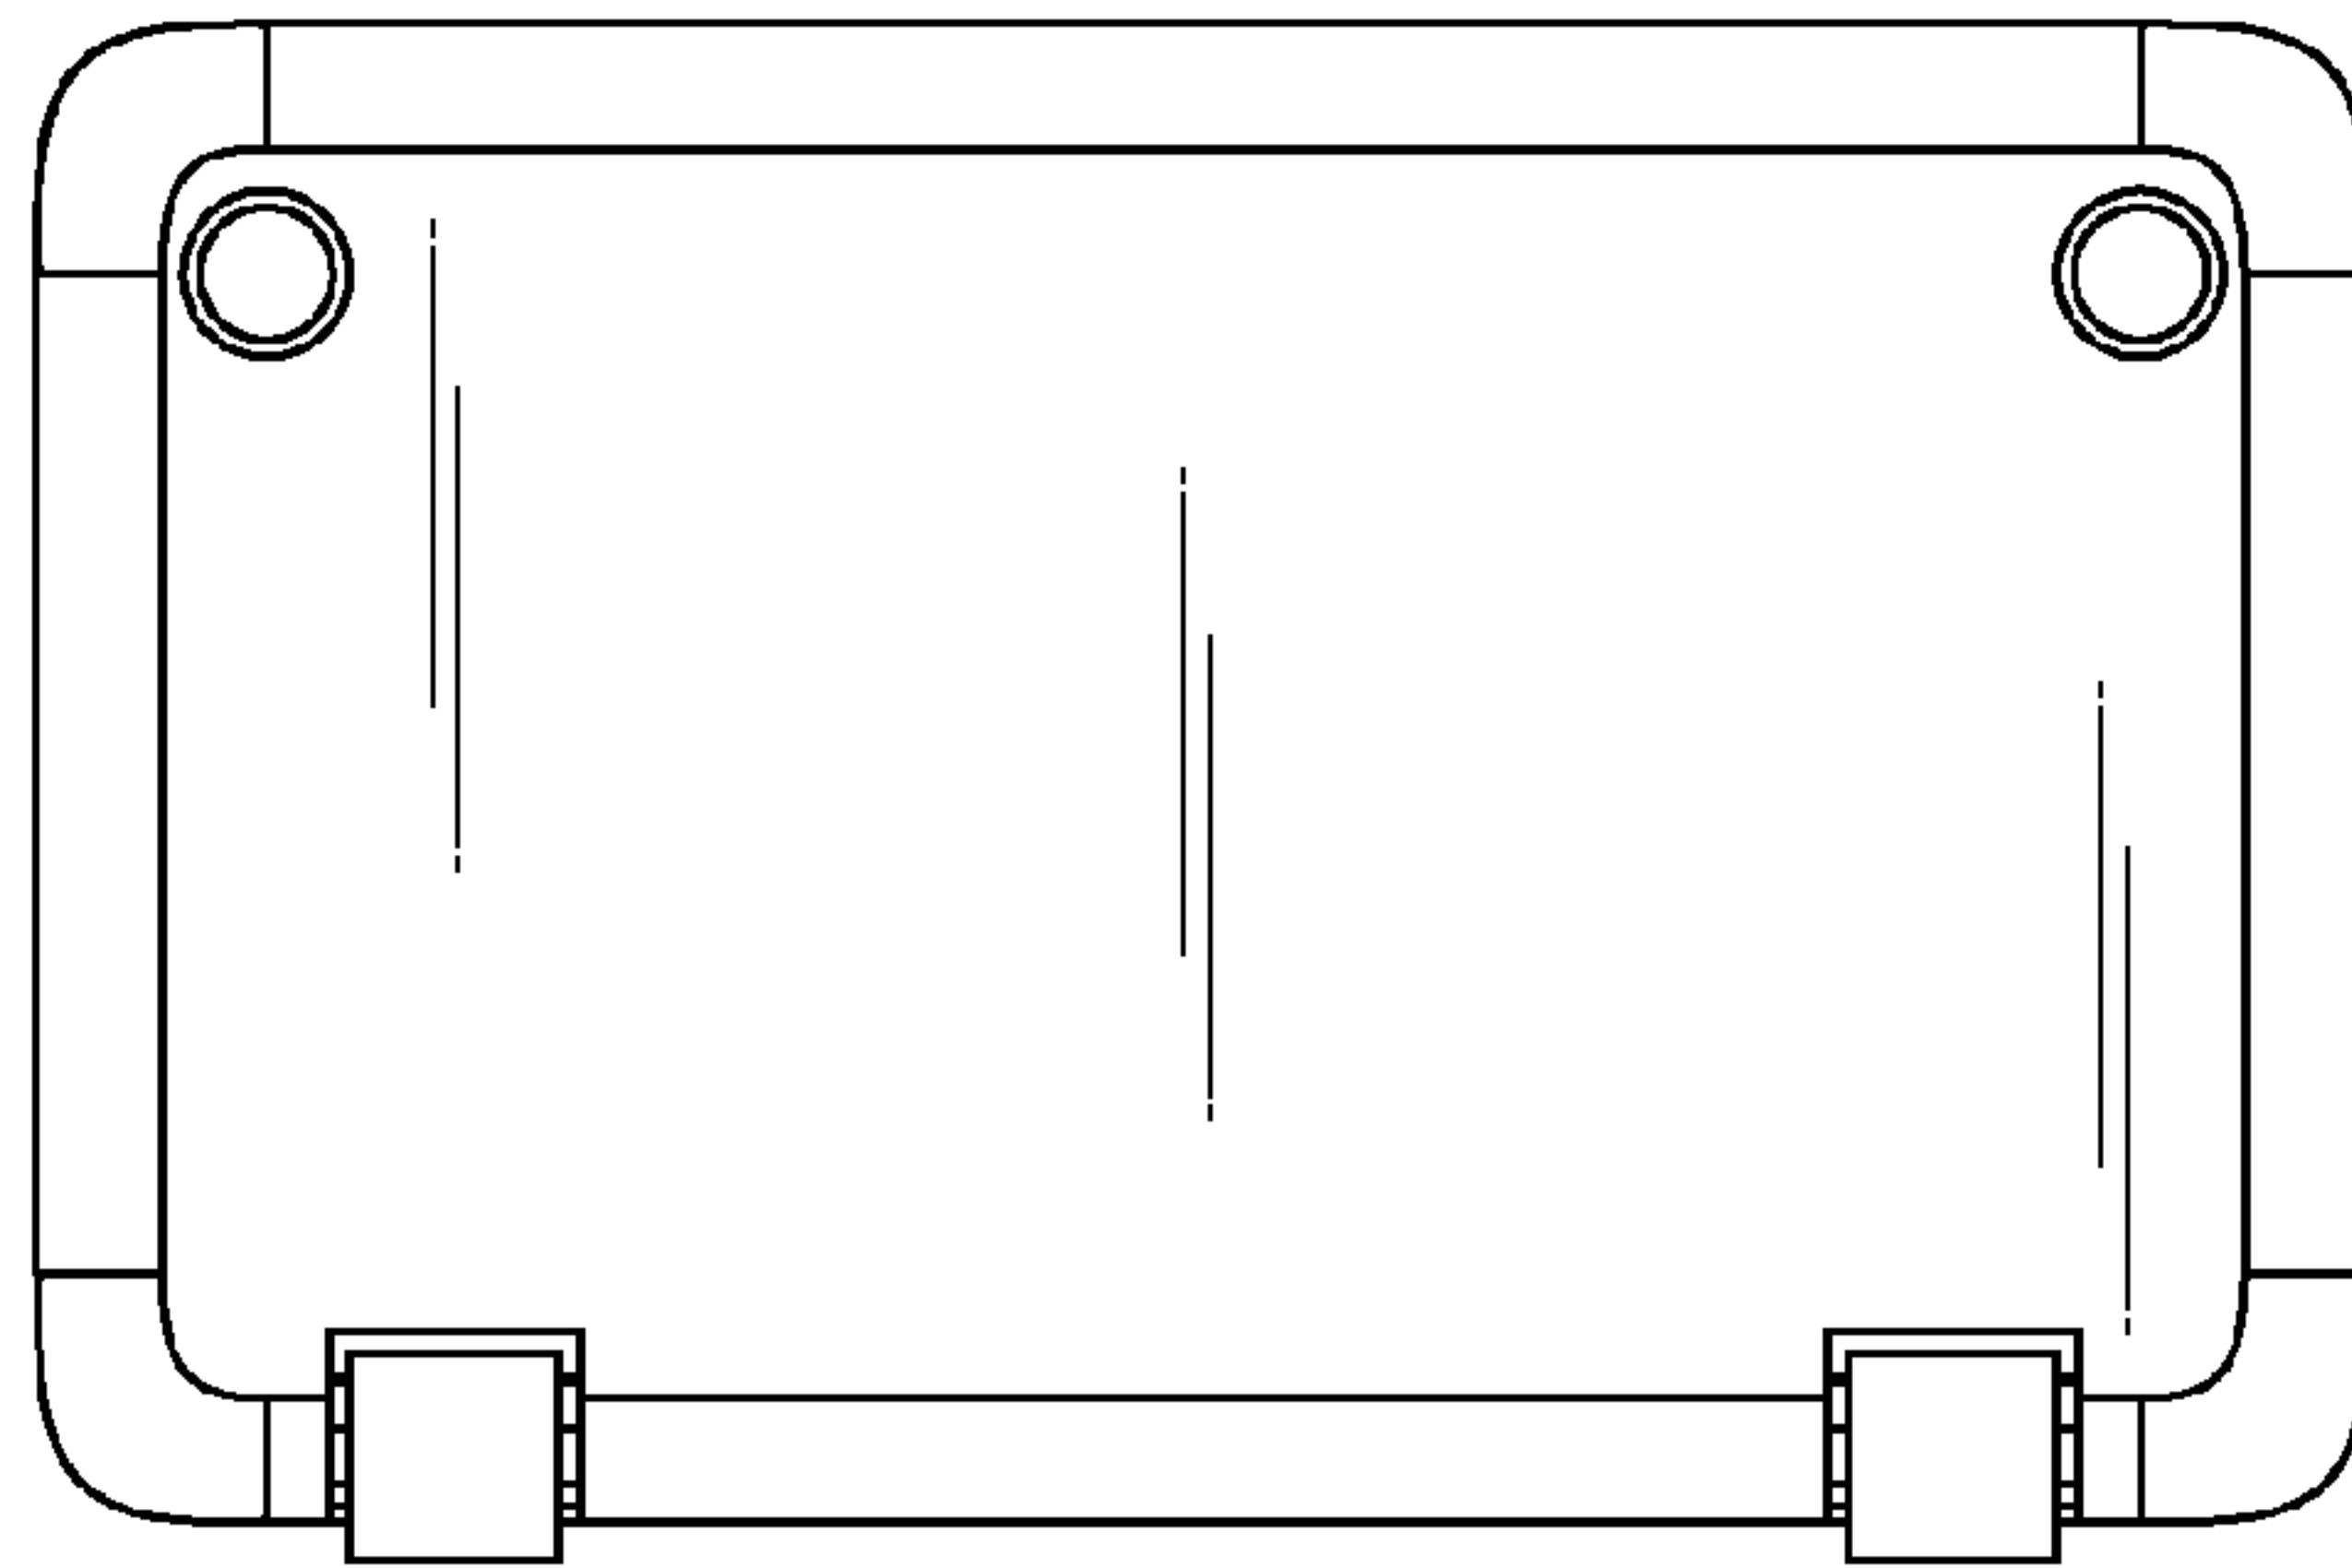


FIG. 14

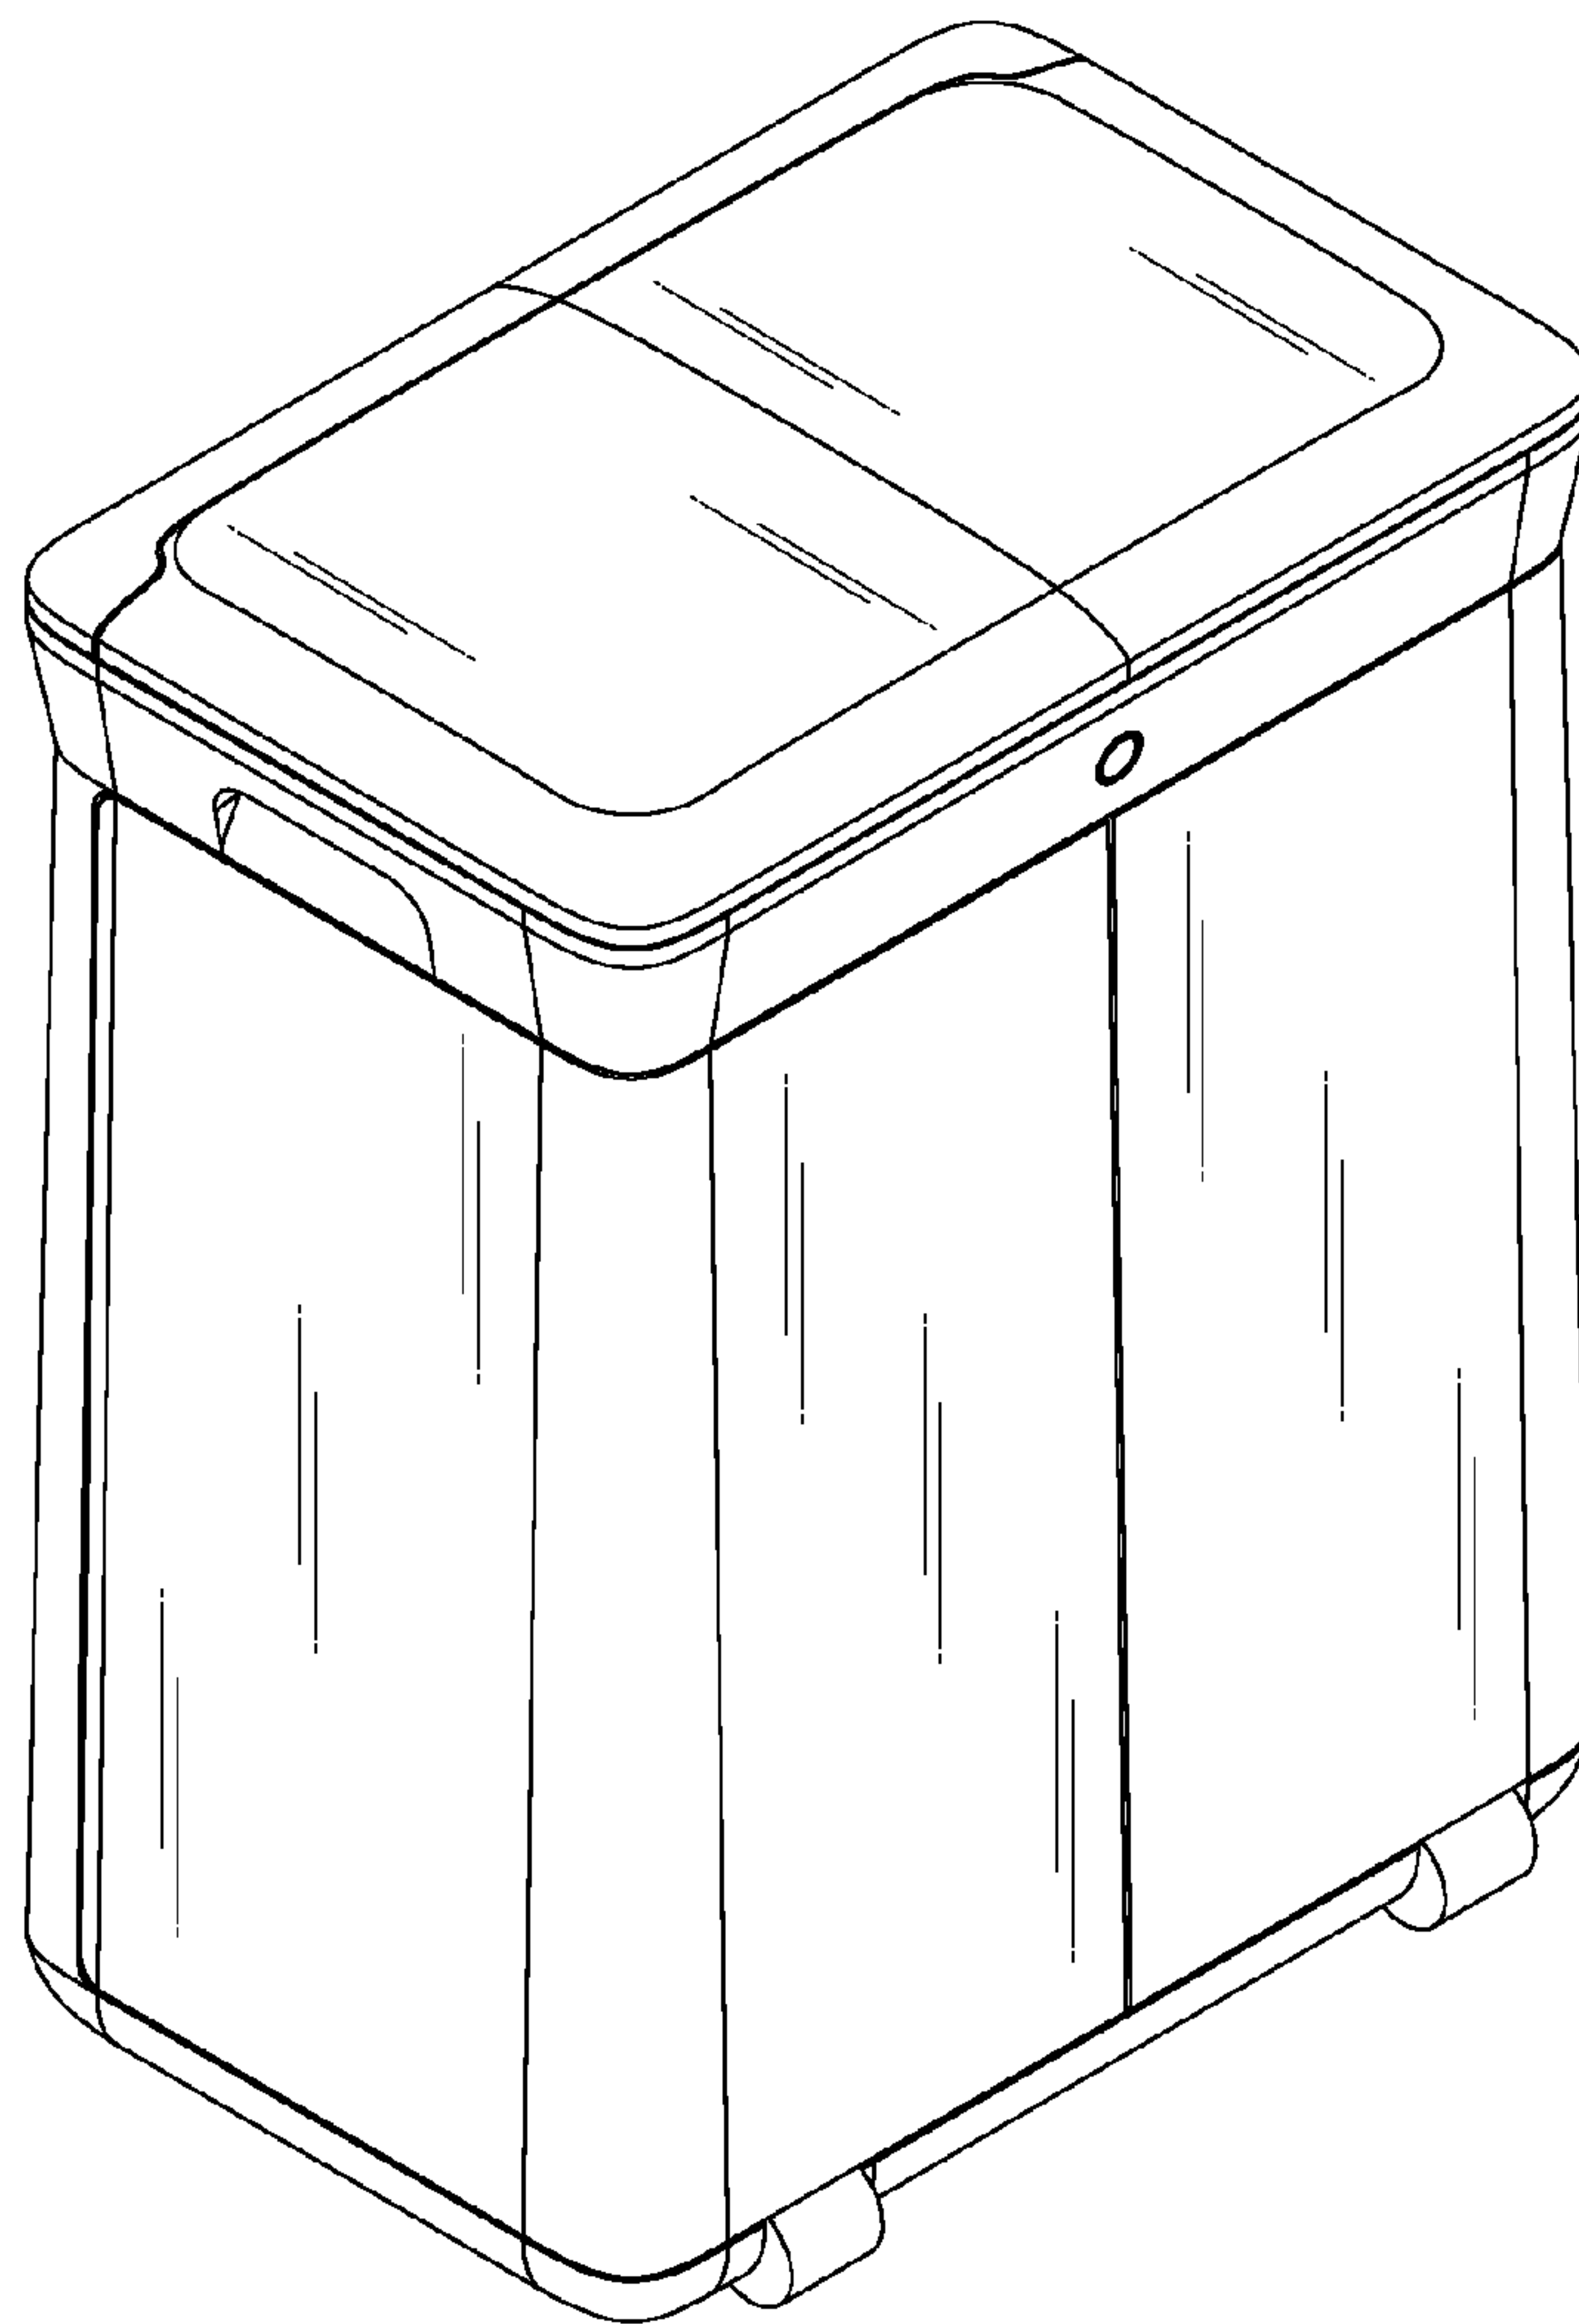


FIG. 15

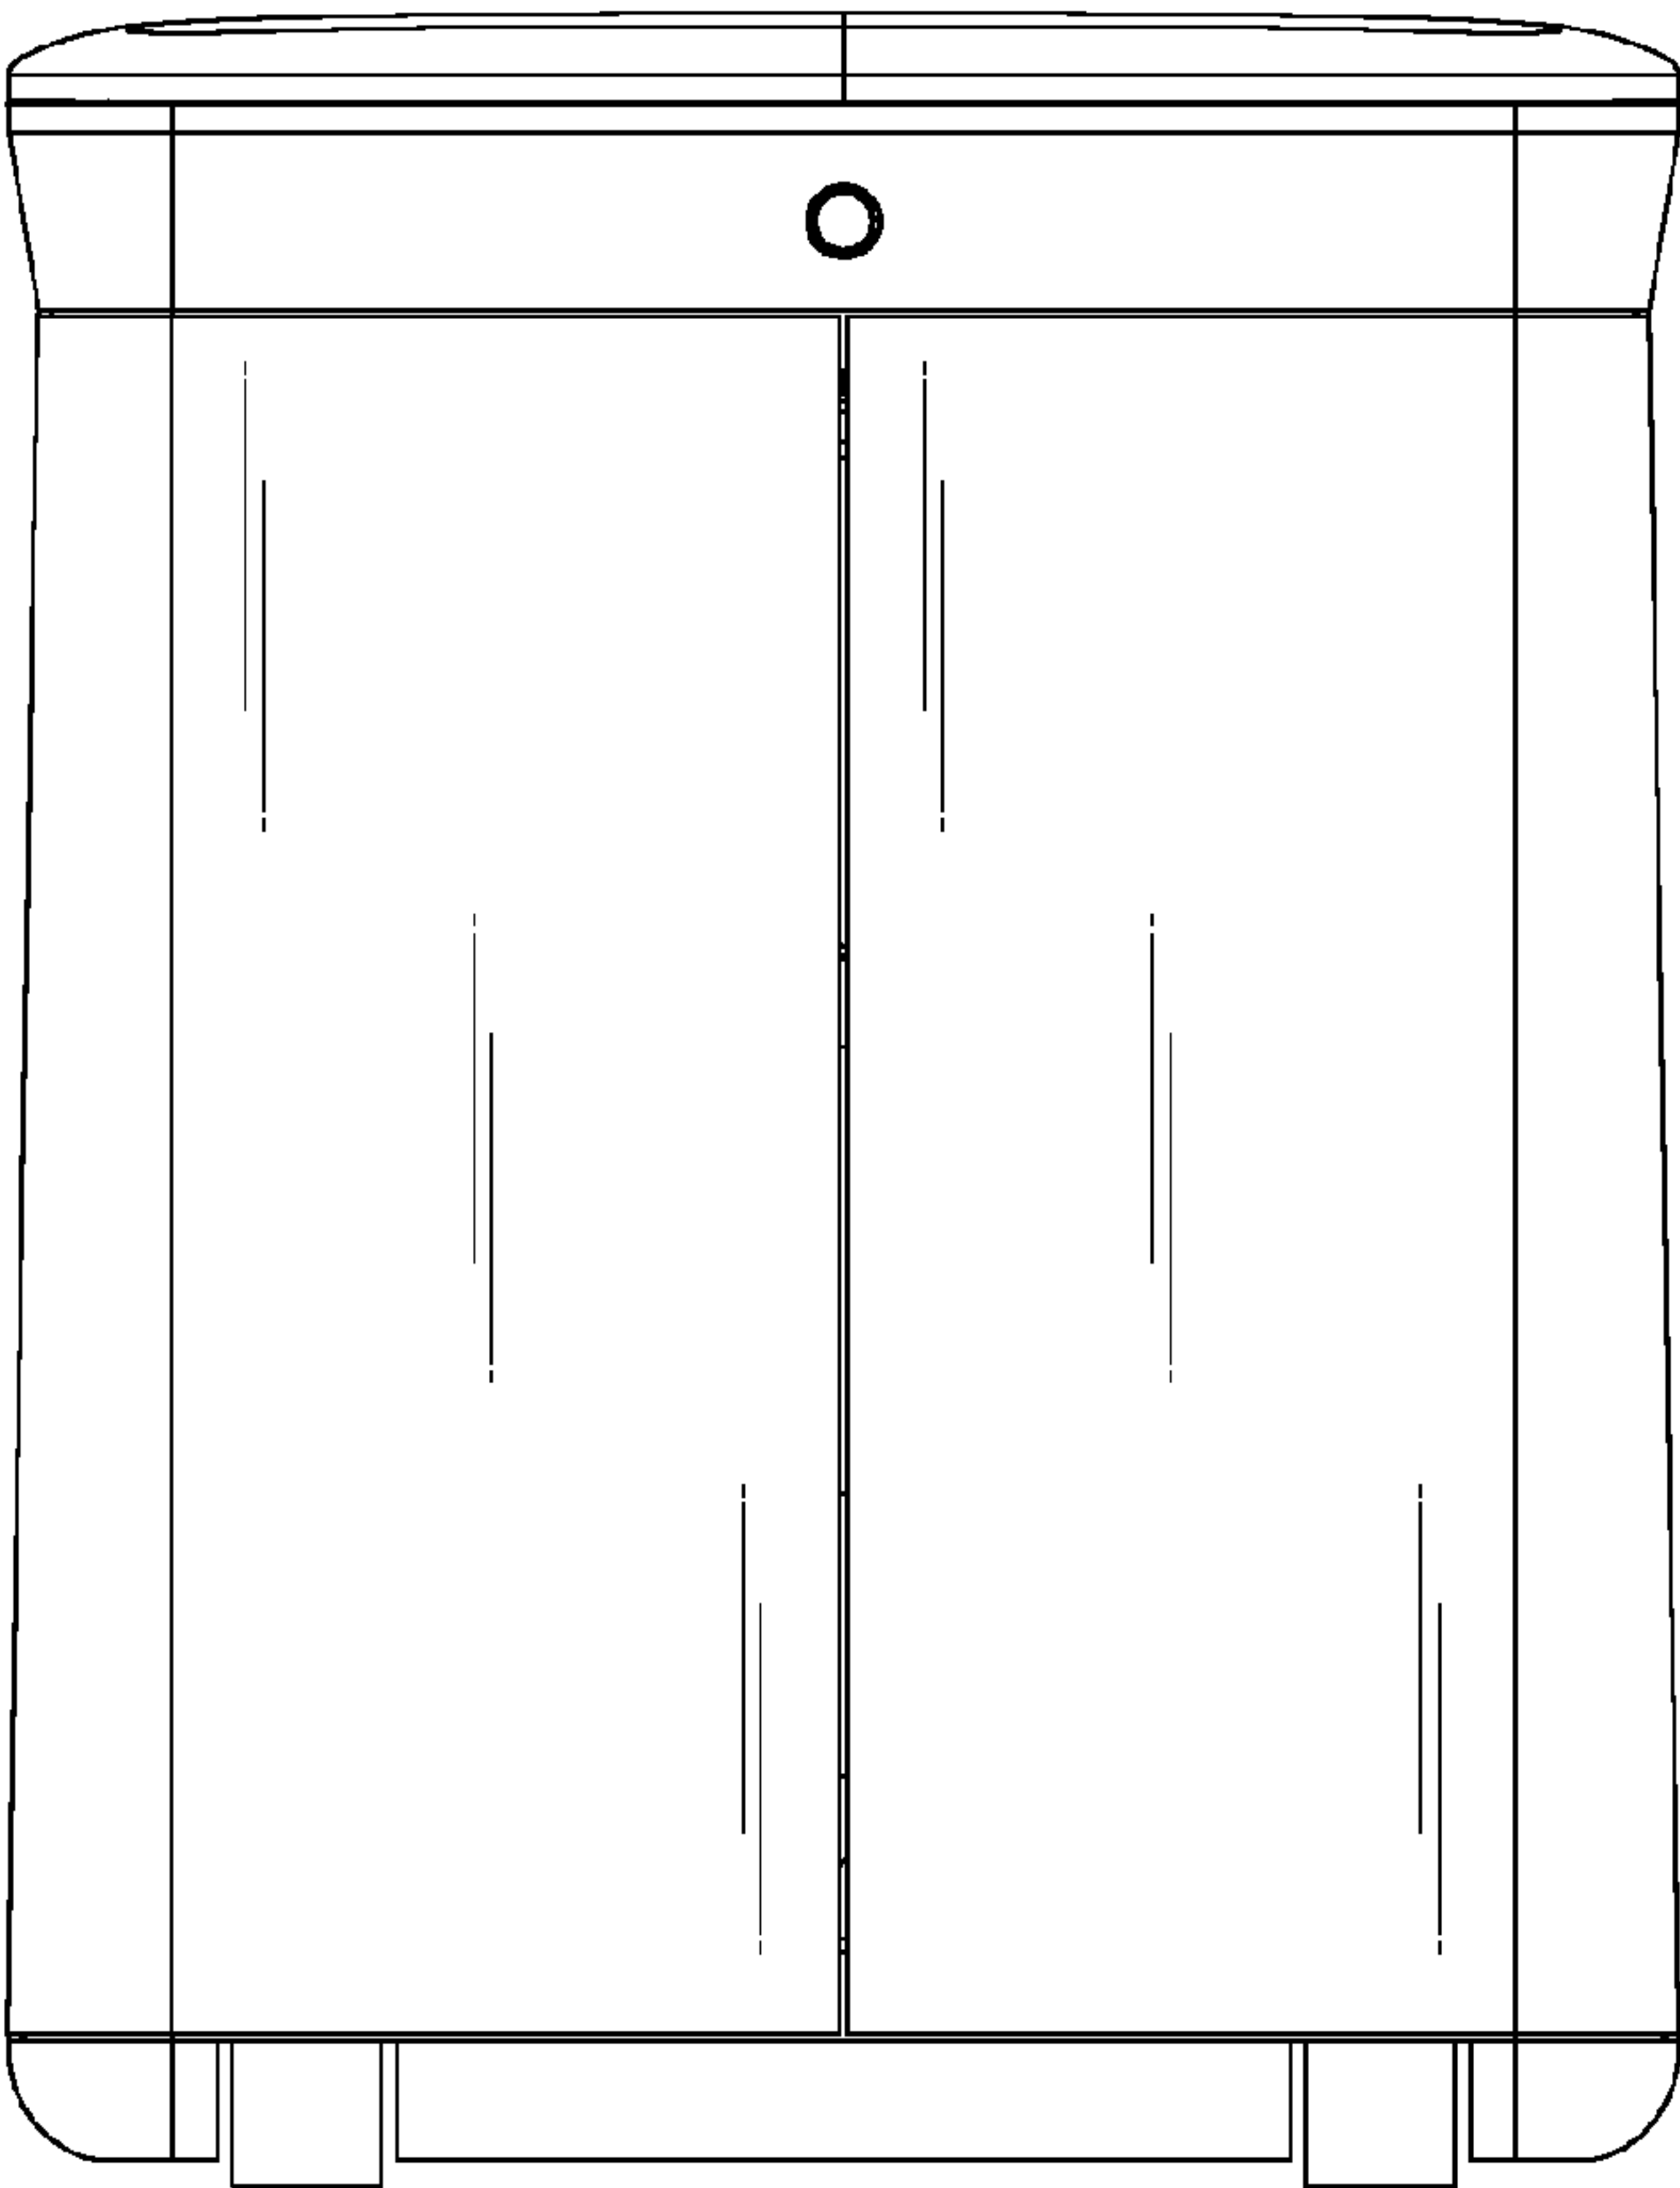


FIG. 16

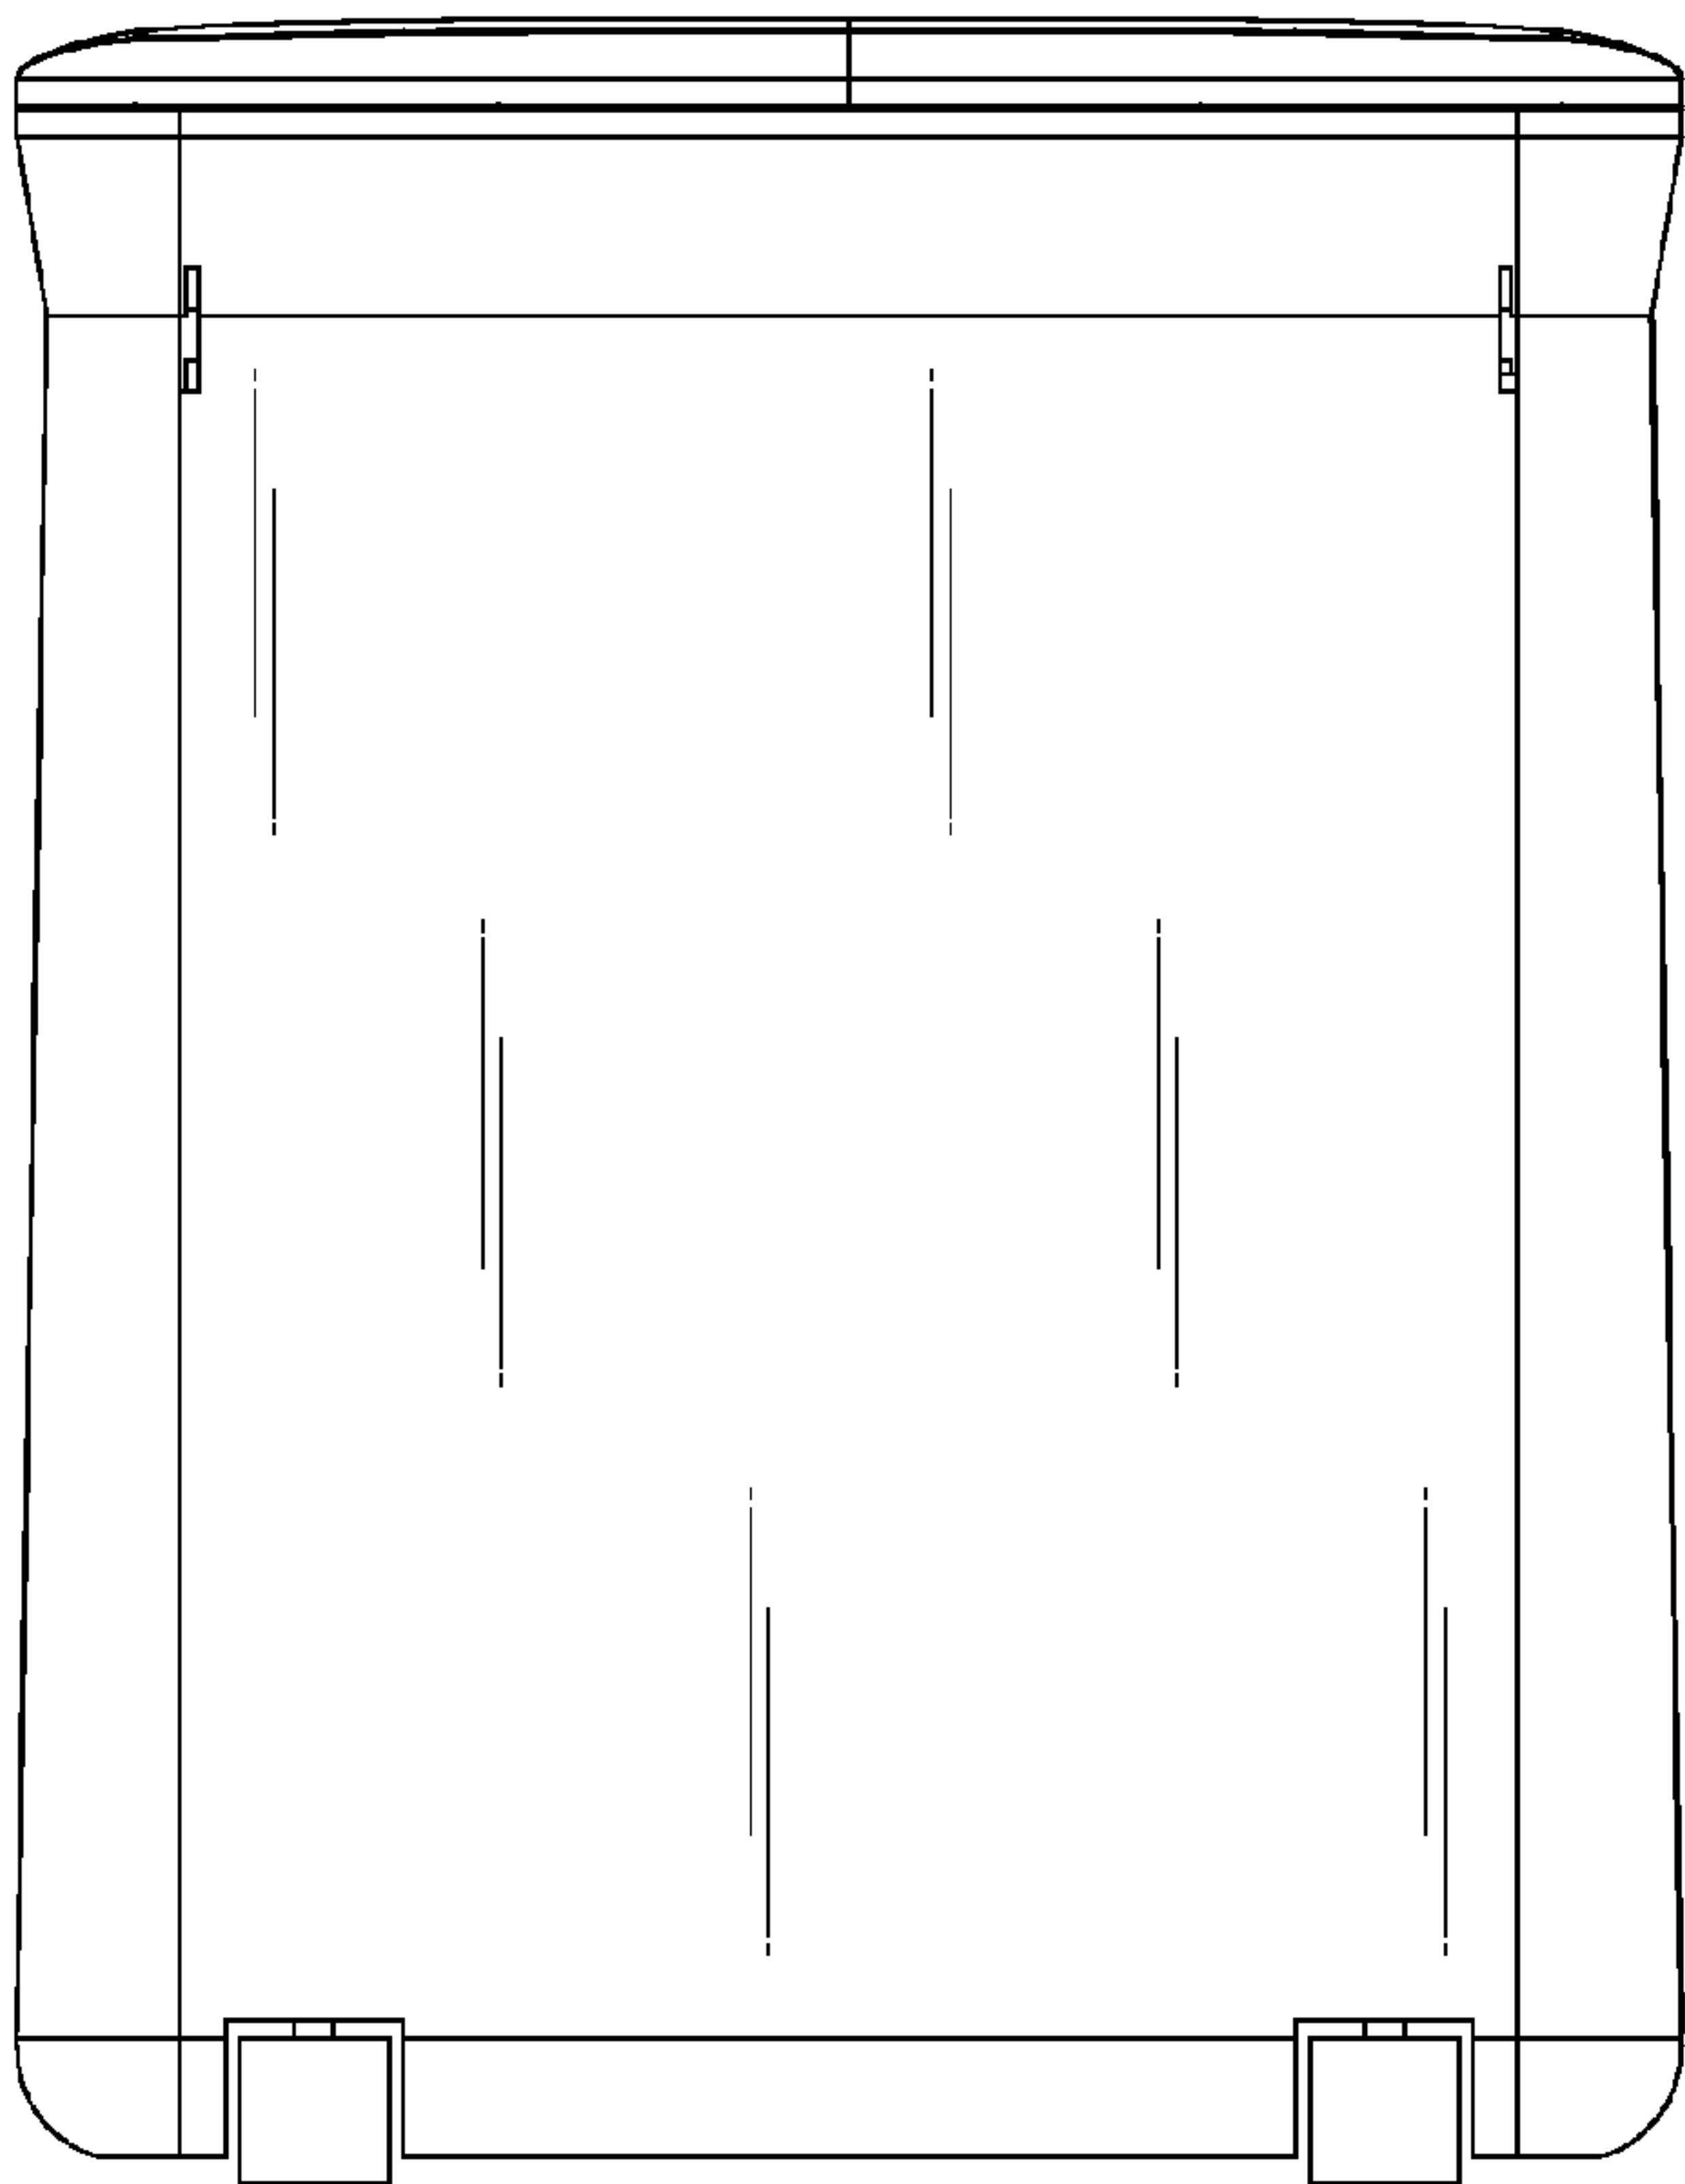


FIG. 17

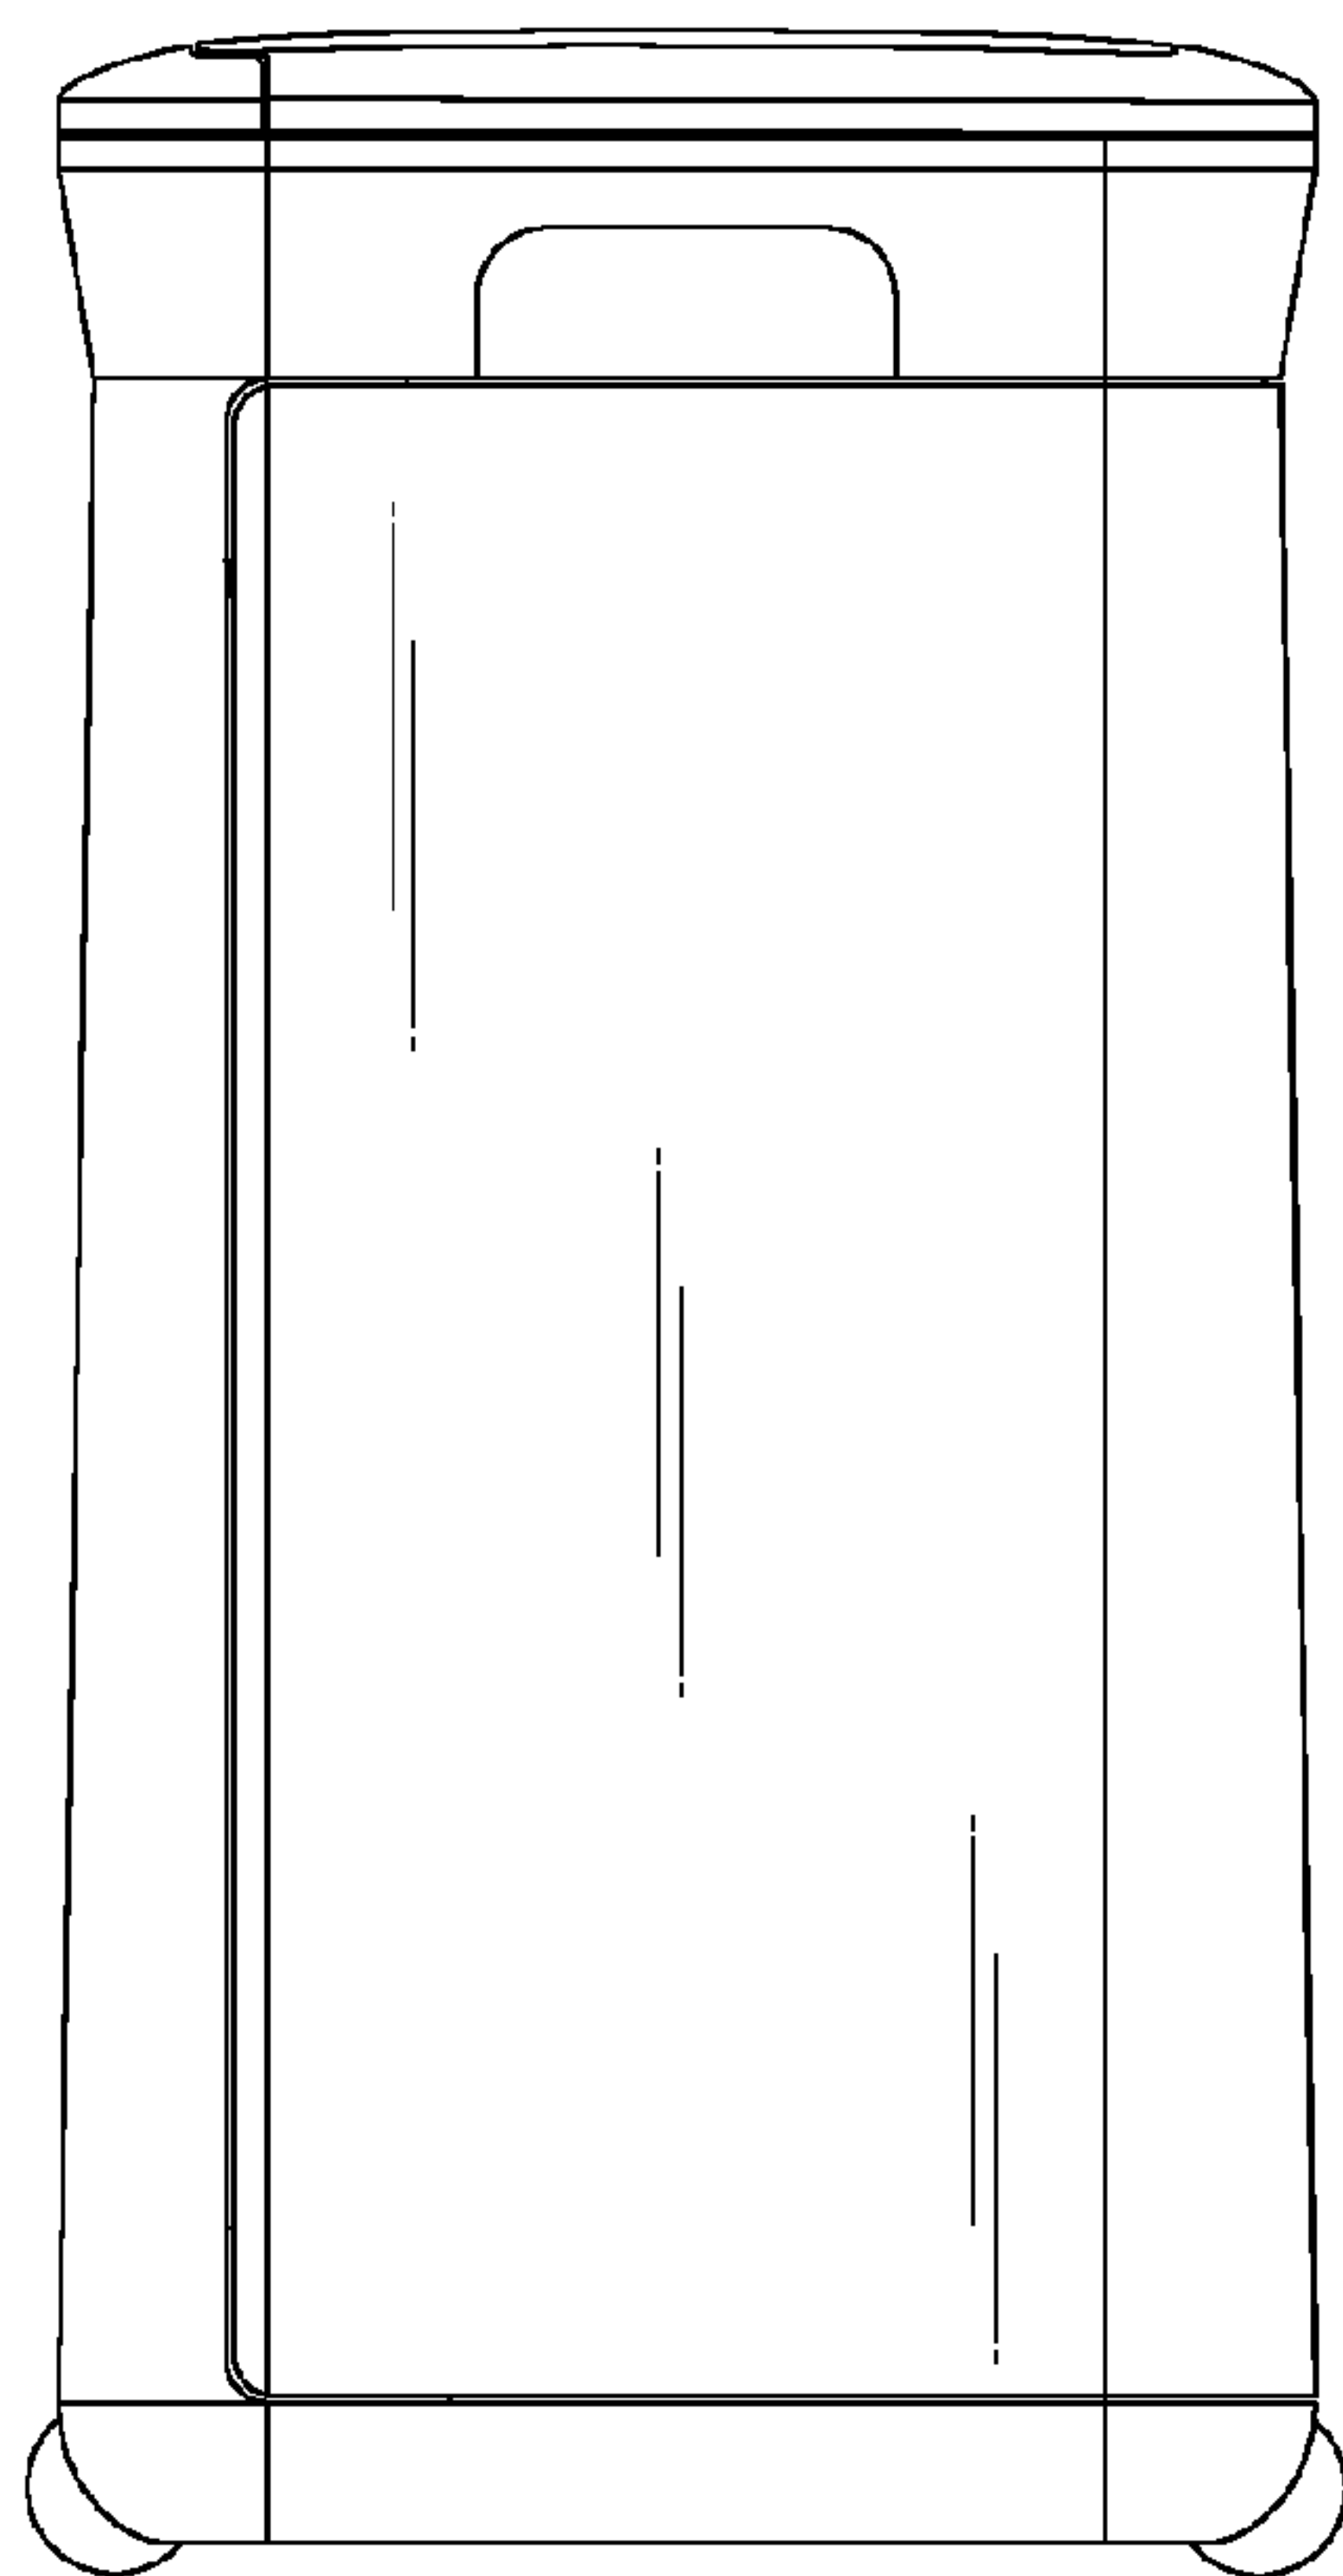


FIG. 18

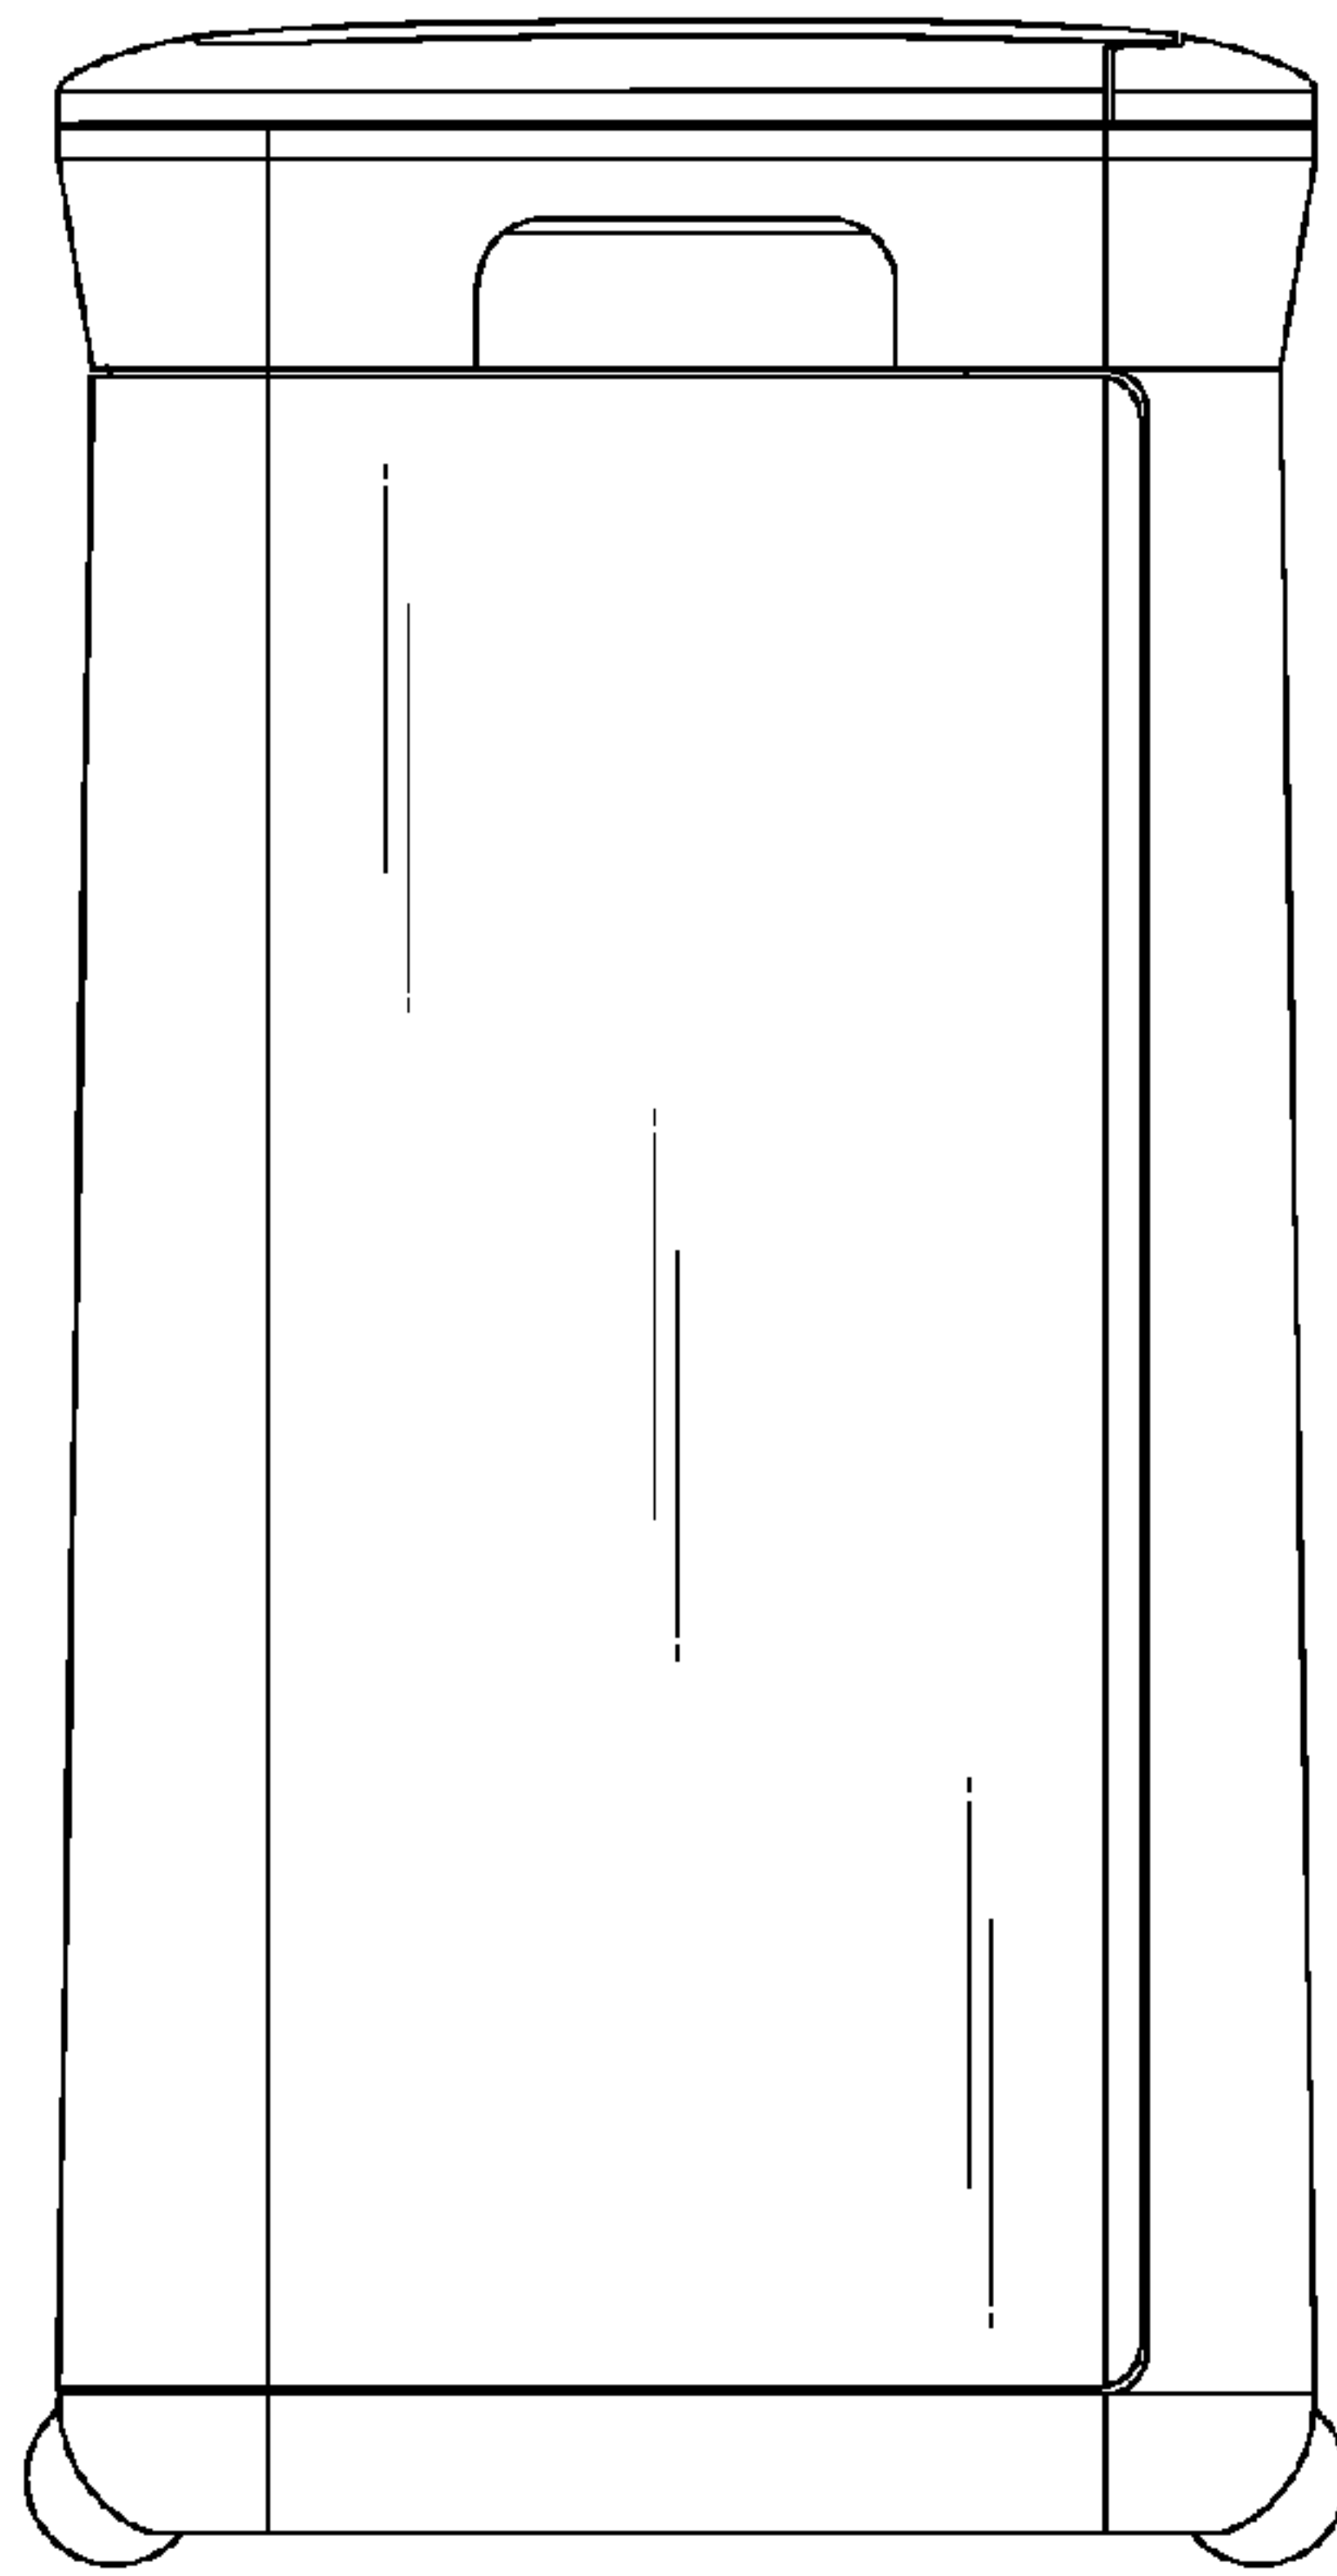


FIG. 19

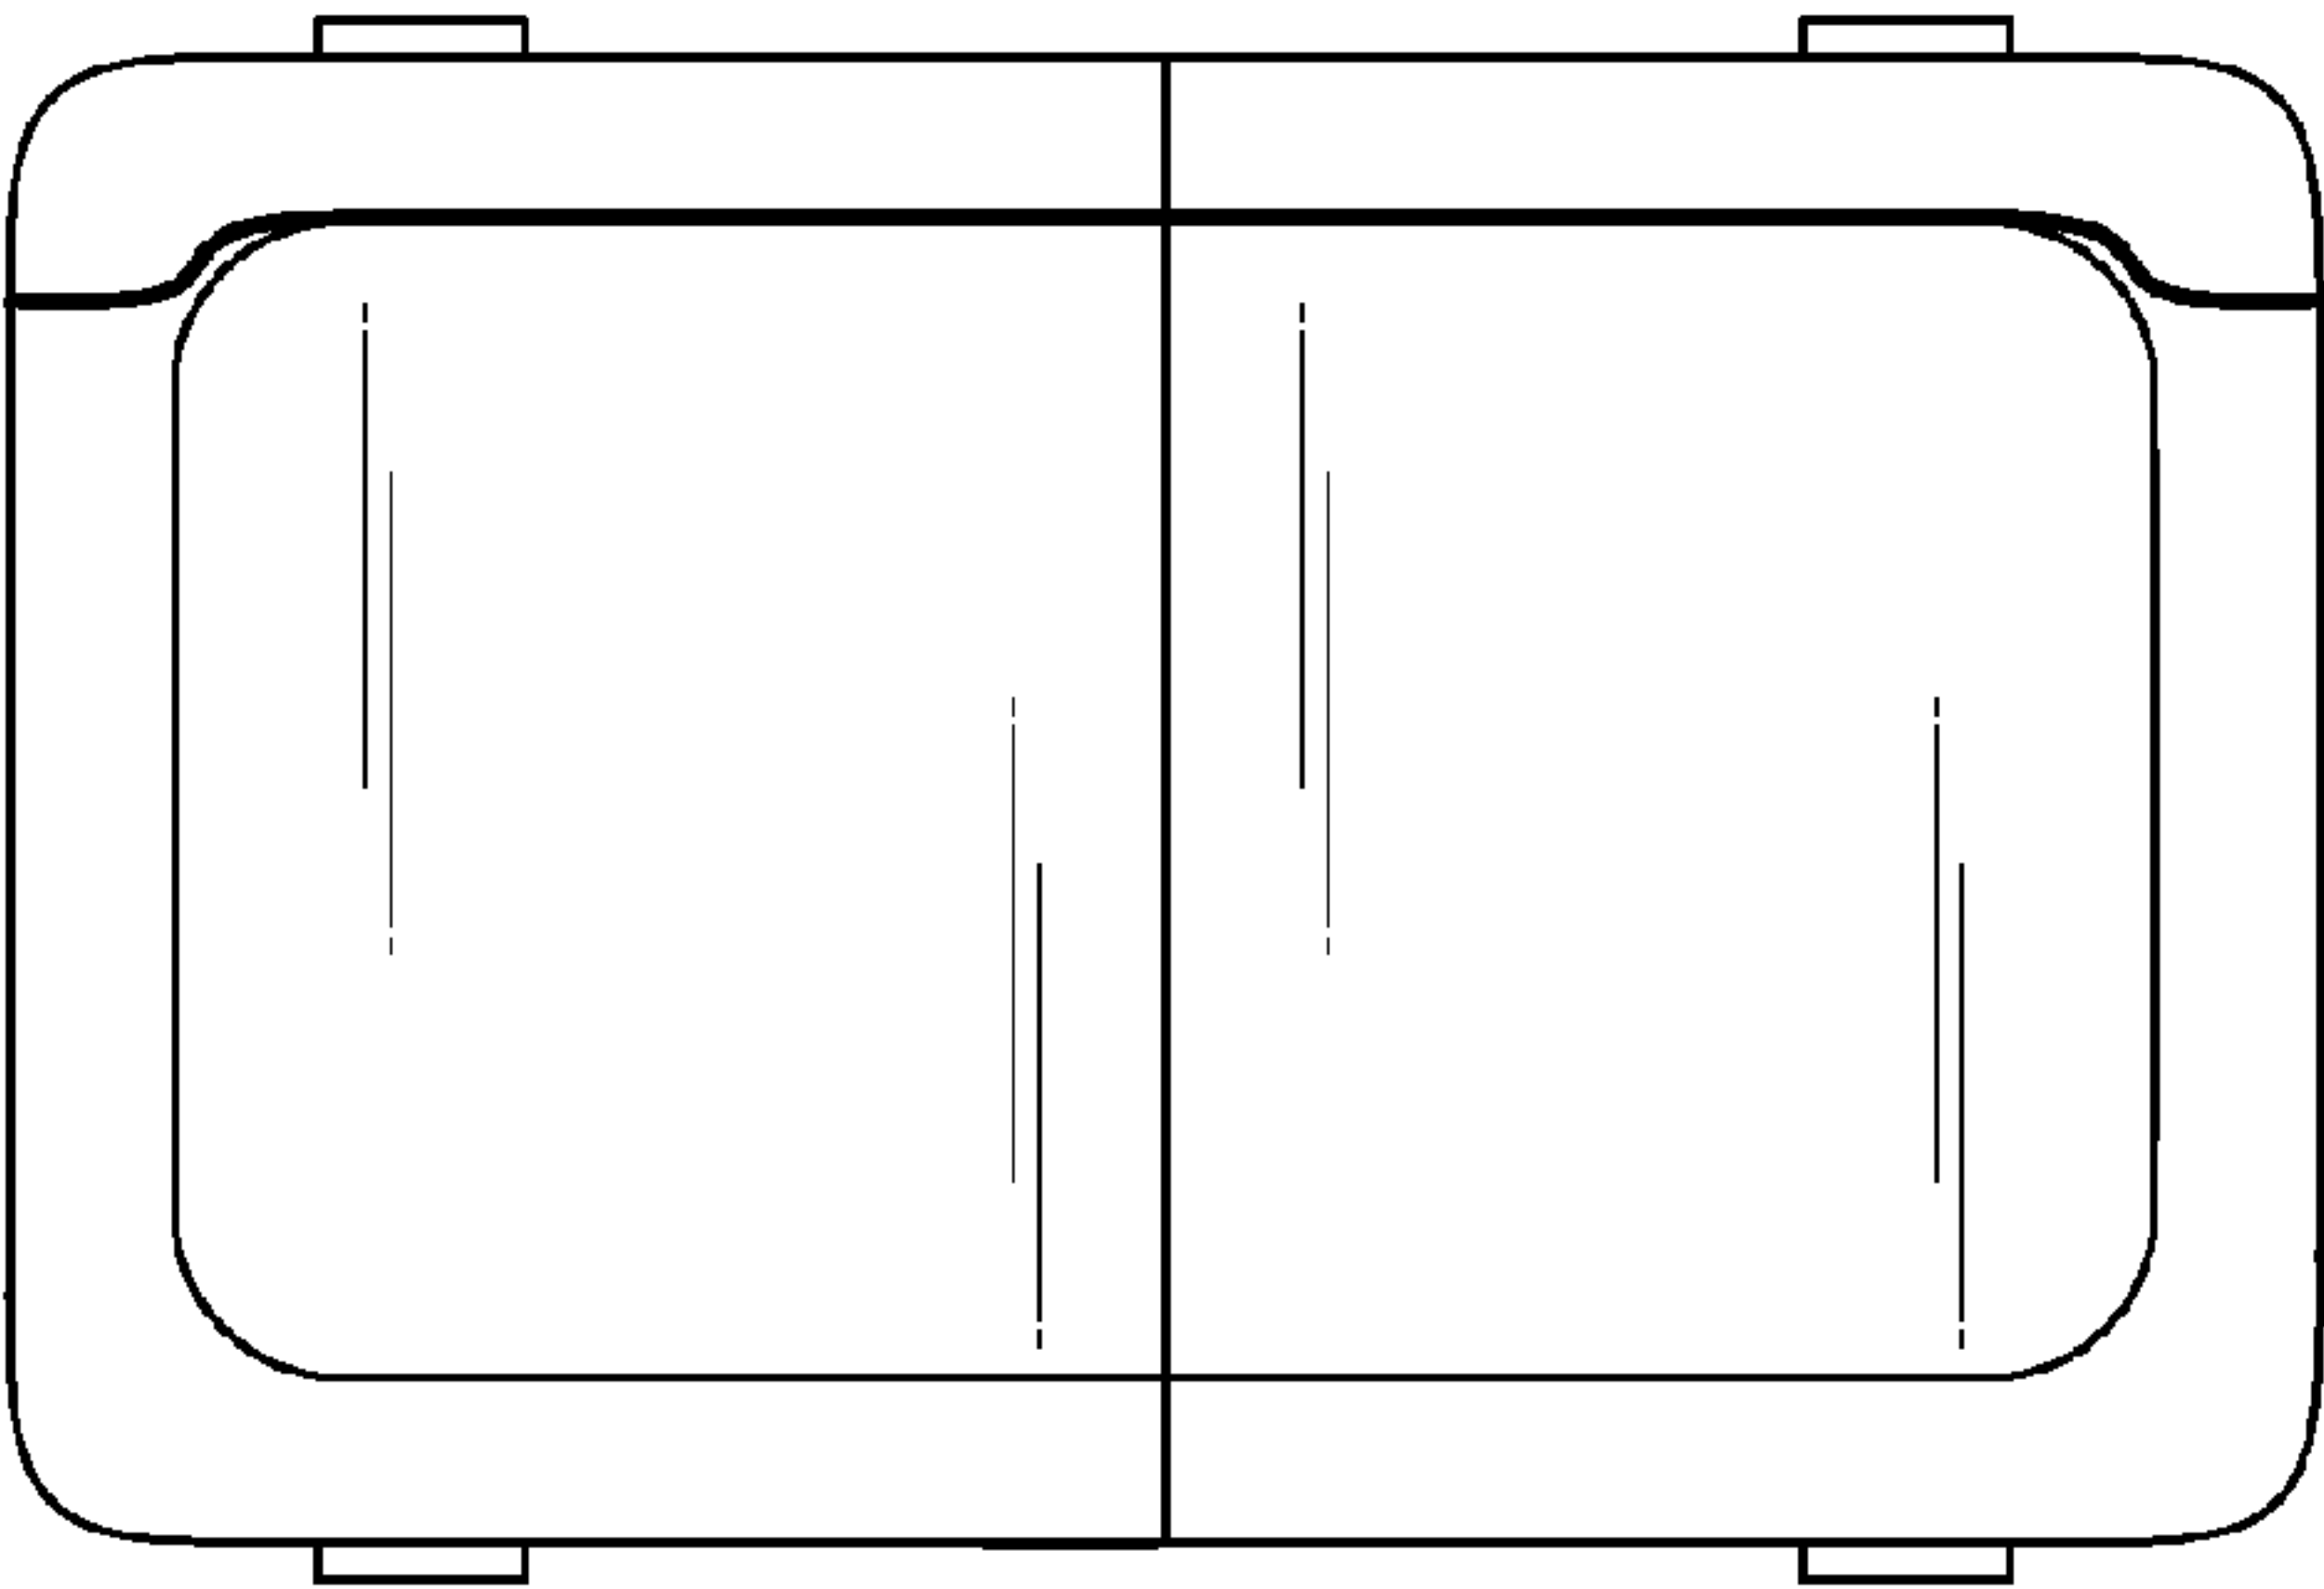


FIG. 20

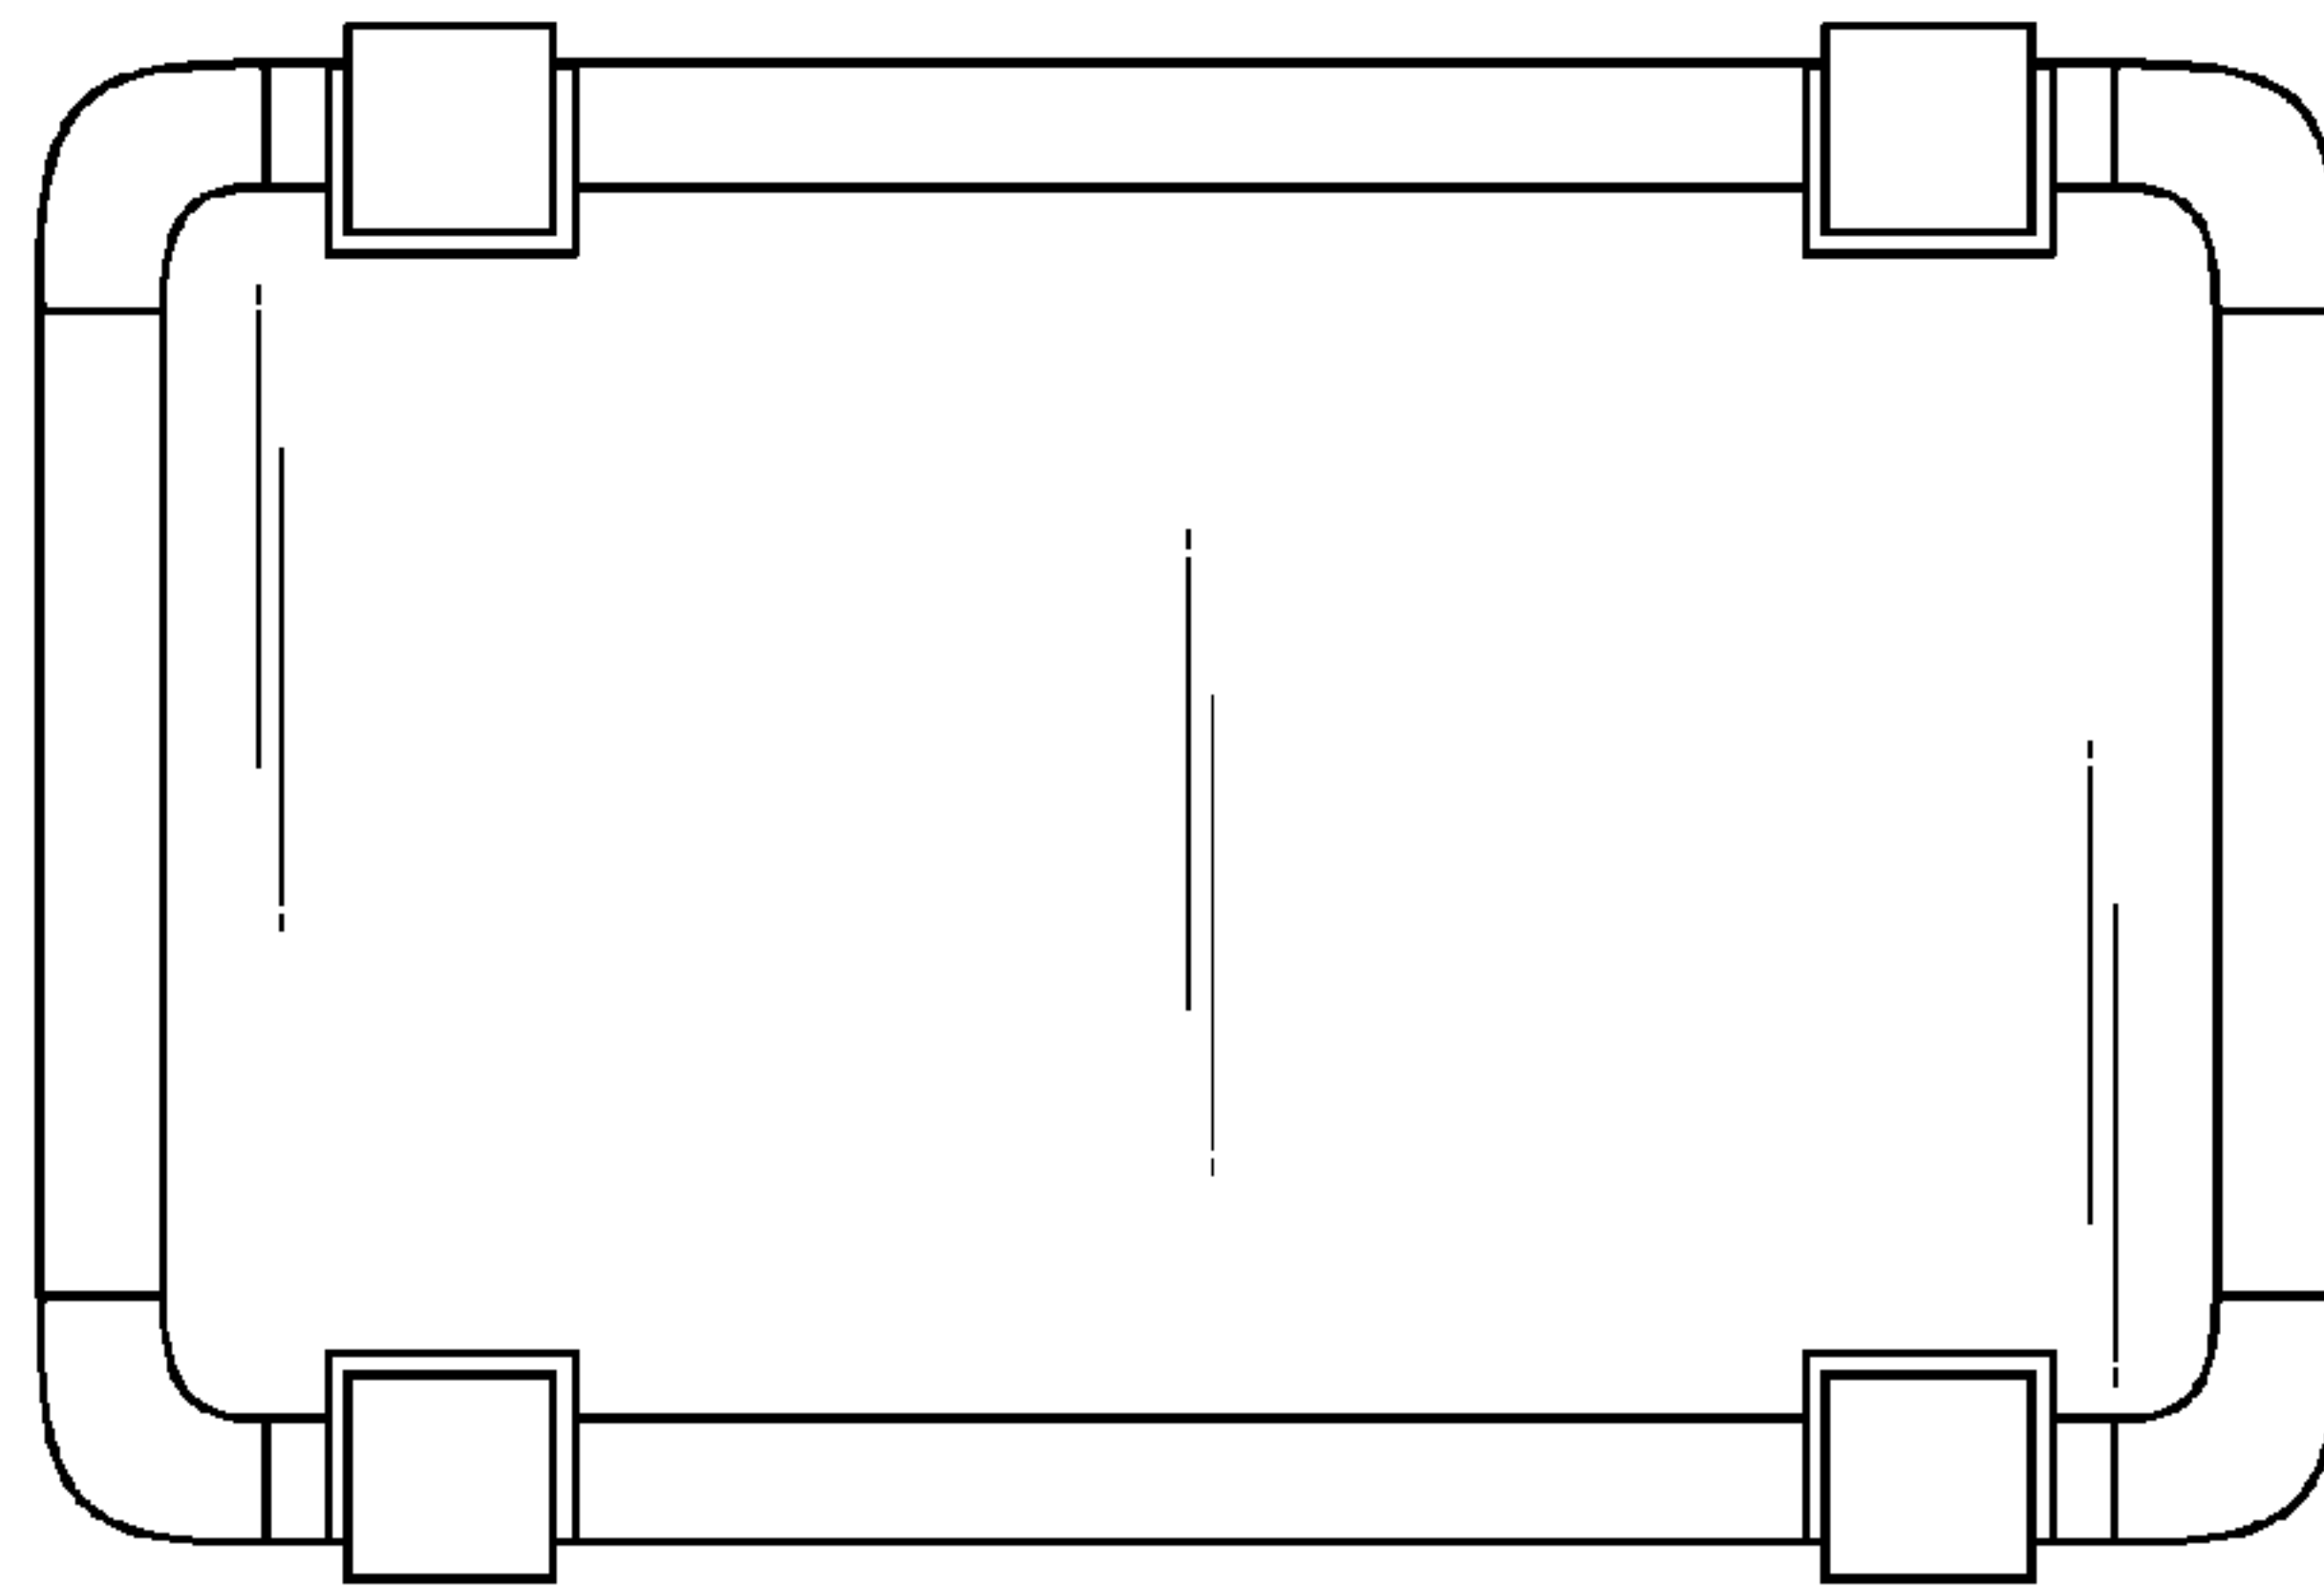


FIG. 21