



US00D705942S

(12) **United States Design Patent**
Hahr et al.

(10) **Patent No.:** **US D705,942 S**

(45) **Date of Patent:** **** May 27, 2014**

(54) **STIMULATION DEVICE**

(71) Applicant: **Senses Toys Intellectual Property Management UG**, Bielefeld (DE)

(72) Inventors: **Meike Hahr**, Hamburg (DE); **Heiko Tullney**, Hamburg (DE); **Till Muhl**, Hamburg (DE); **Thomas Milewski**, Halstenbek (DE)

(**) Term: **14 Years**

(21) Appl. No.: **29/447,962**

(22) Filed: **Mar. 8, 2013**

(30) **Foreign Application Priority Data**

Sep. 10, 2012 (EM) 001342935-0066

(51) **LOC (10) Cl.** **28-03**

(52) **U.S. Cl.**
USPC **D24/215**

(58) **Field of Classification Search**
USPC D24/200, 211, 212, 213, 214, 215;
601/114, 120, 121, 124, 125, 130, 131,
601/134, 135, 136, 137
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D652,526 S * 1/2012 Peddicord D24/215
D670,398 S * 11/2012 Peddicord D24/215

D670,399 S * 11/2012 Peddicord D24/215
8,308,667 B2 * 11/2012 Lee 601/46
D681,220 S * 4/2013 Chen D24/215
2011/0034837 A1 * 2/2011 Lee 601/46
2011/0105837 A1 * 5/2011 Lee 600/38

* cited by examiner

Primary Examiner — Sandra Snapp


(57) **CLAIM**

The ornamental design for a stimulation device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view taken at a first angle from the top, rear and right side of a stimulation device showing the design, the opposite side being a mirror image thereof;
FIG. 2 is a perspective view taken at a second angle from the top, rear and right side of the stimulation device of FIG. 1, the opposite side being a mirror image thereof;
FIG. 3 is a perspective view taken from the top, rear and left side of the stimulation device of FIG. 1, the opposite side view being a mirror image thereof;
FIG. 4 is a left side elevation view of the stimulation device of FIG. 1, the opposite side being a mirror image thereof;
FIG. 5 is a top plan view of the stimulation device of FIG. 1; and,
FIG. 6 is a front elevation view of the stimulation device of FIG. 1.

1 Claim, 6 Drawing Sheets

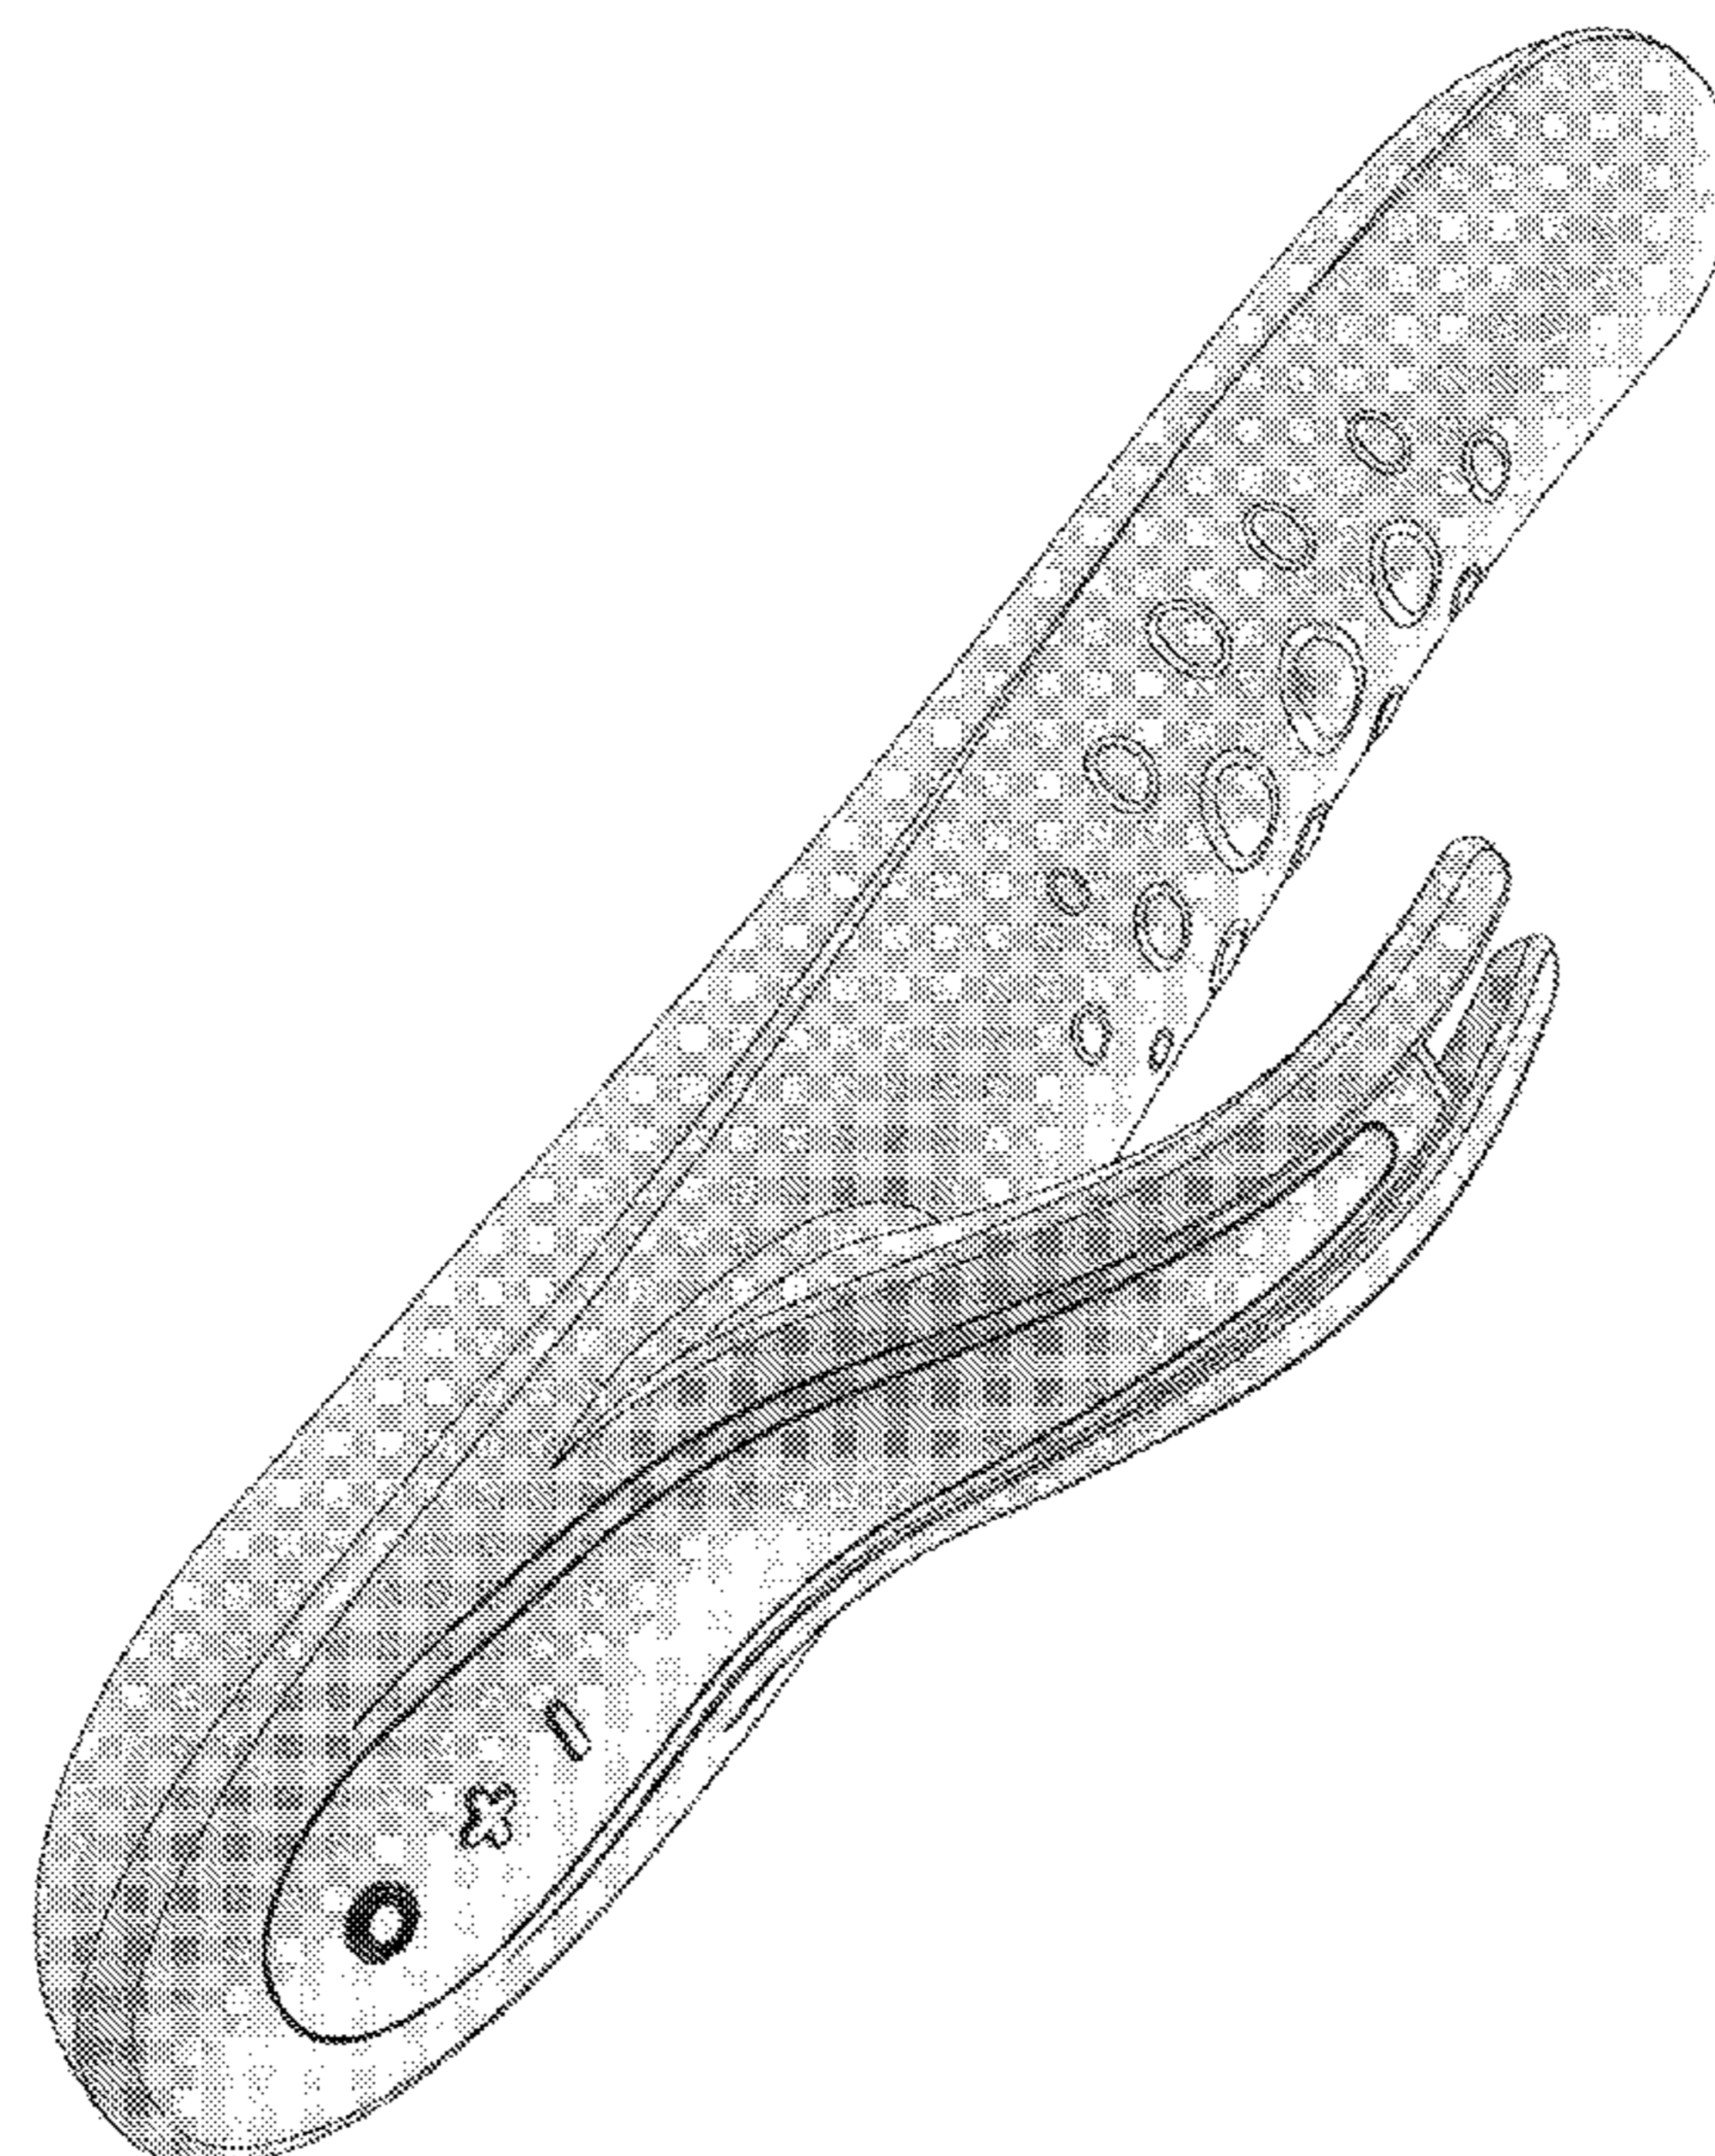

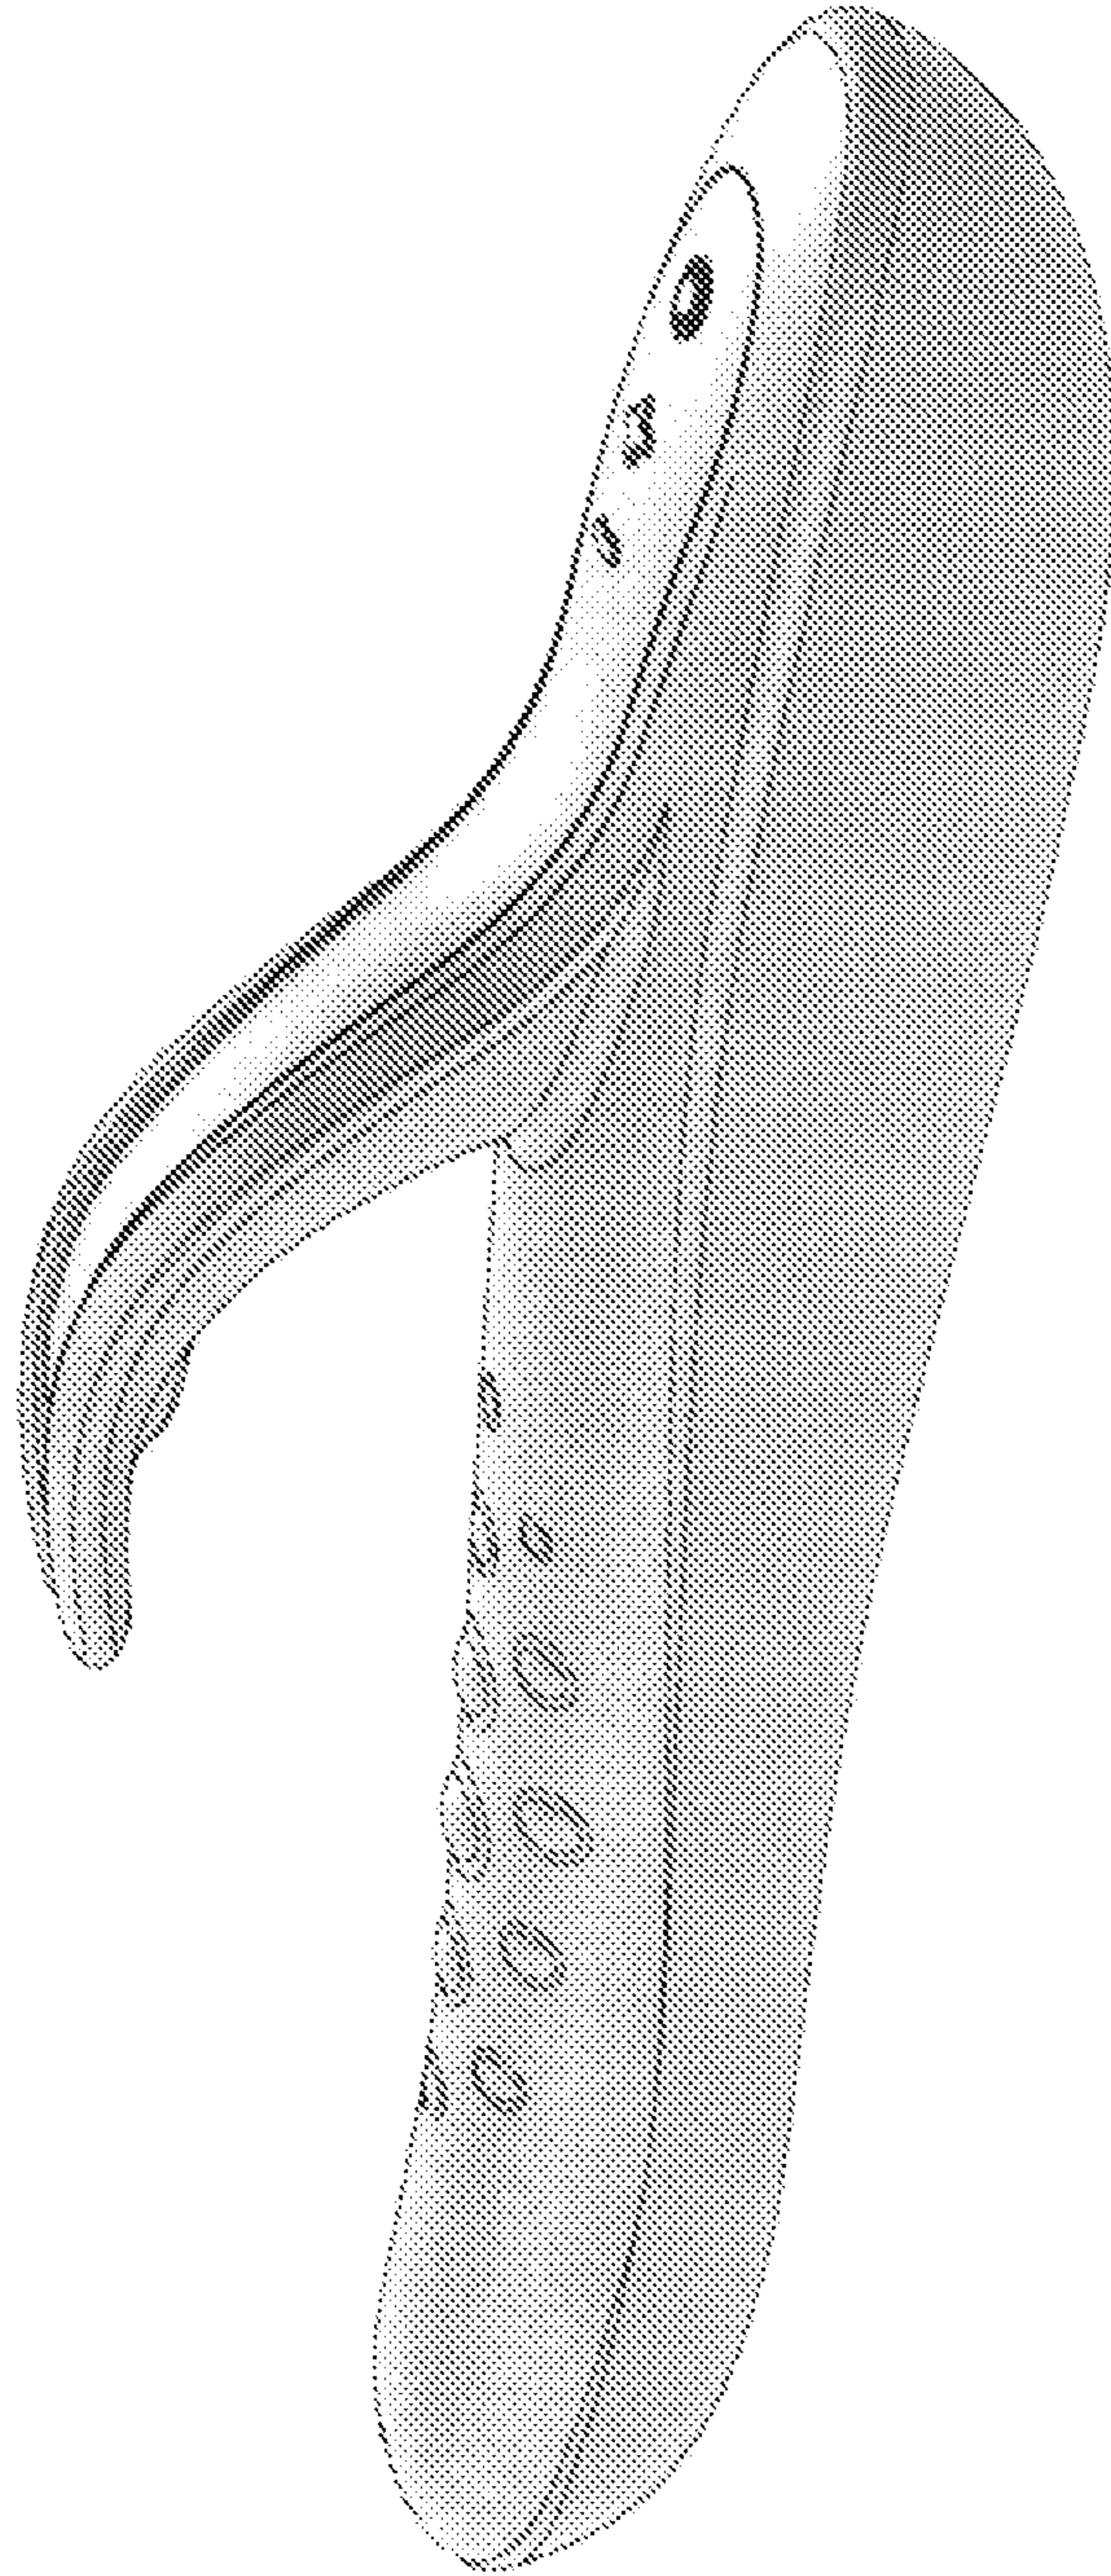


FIG. 1

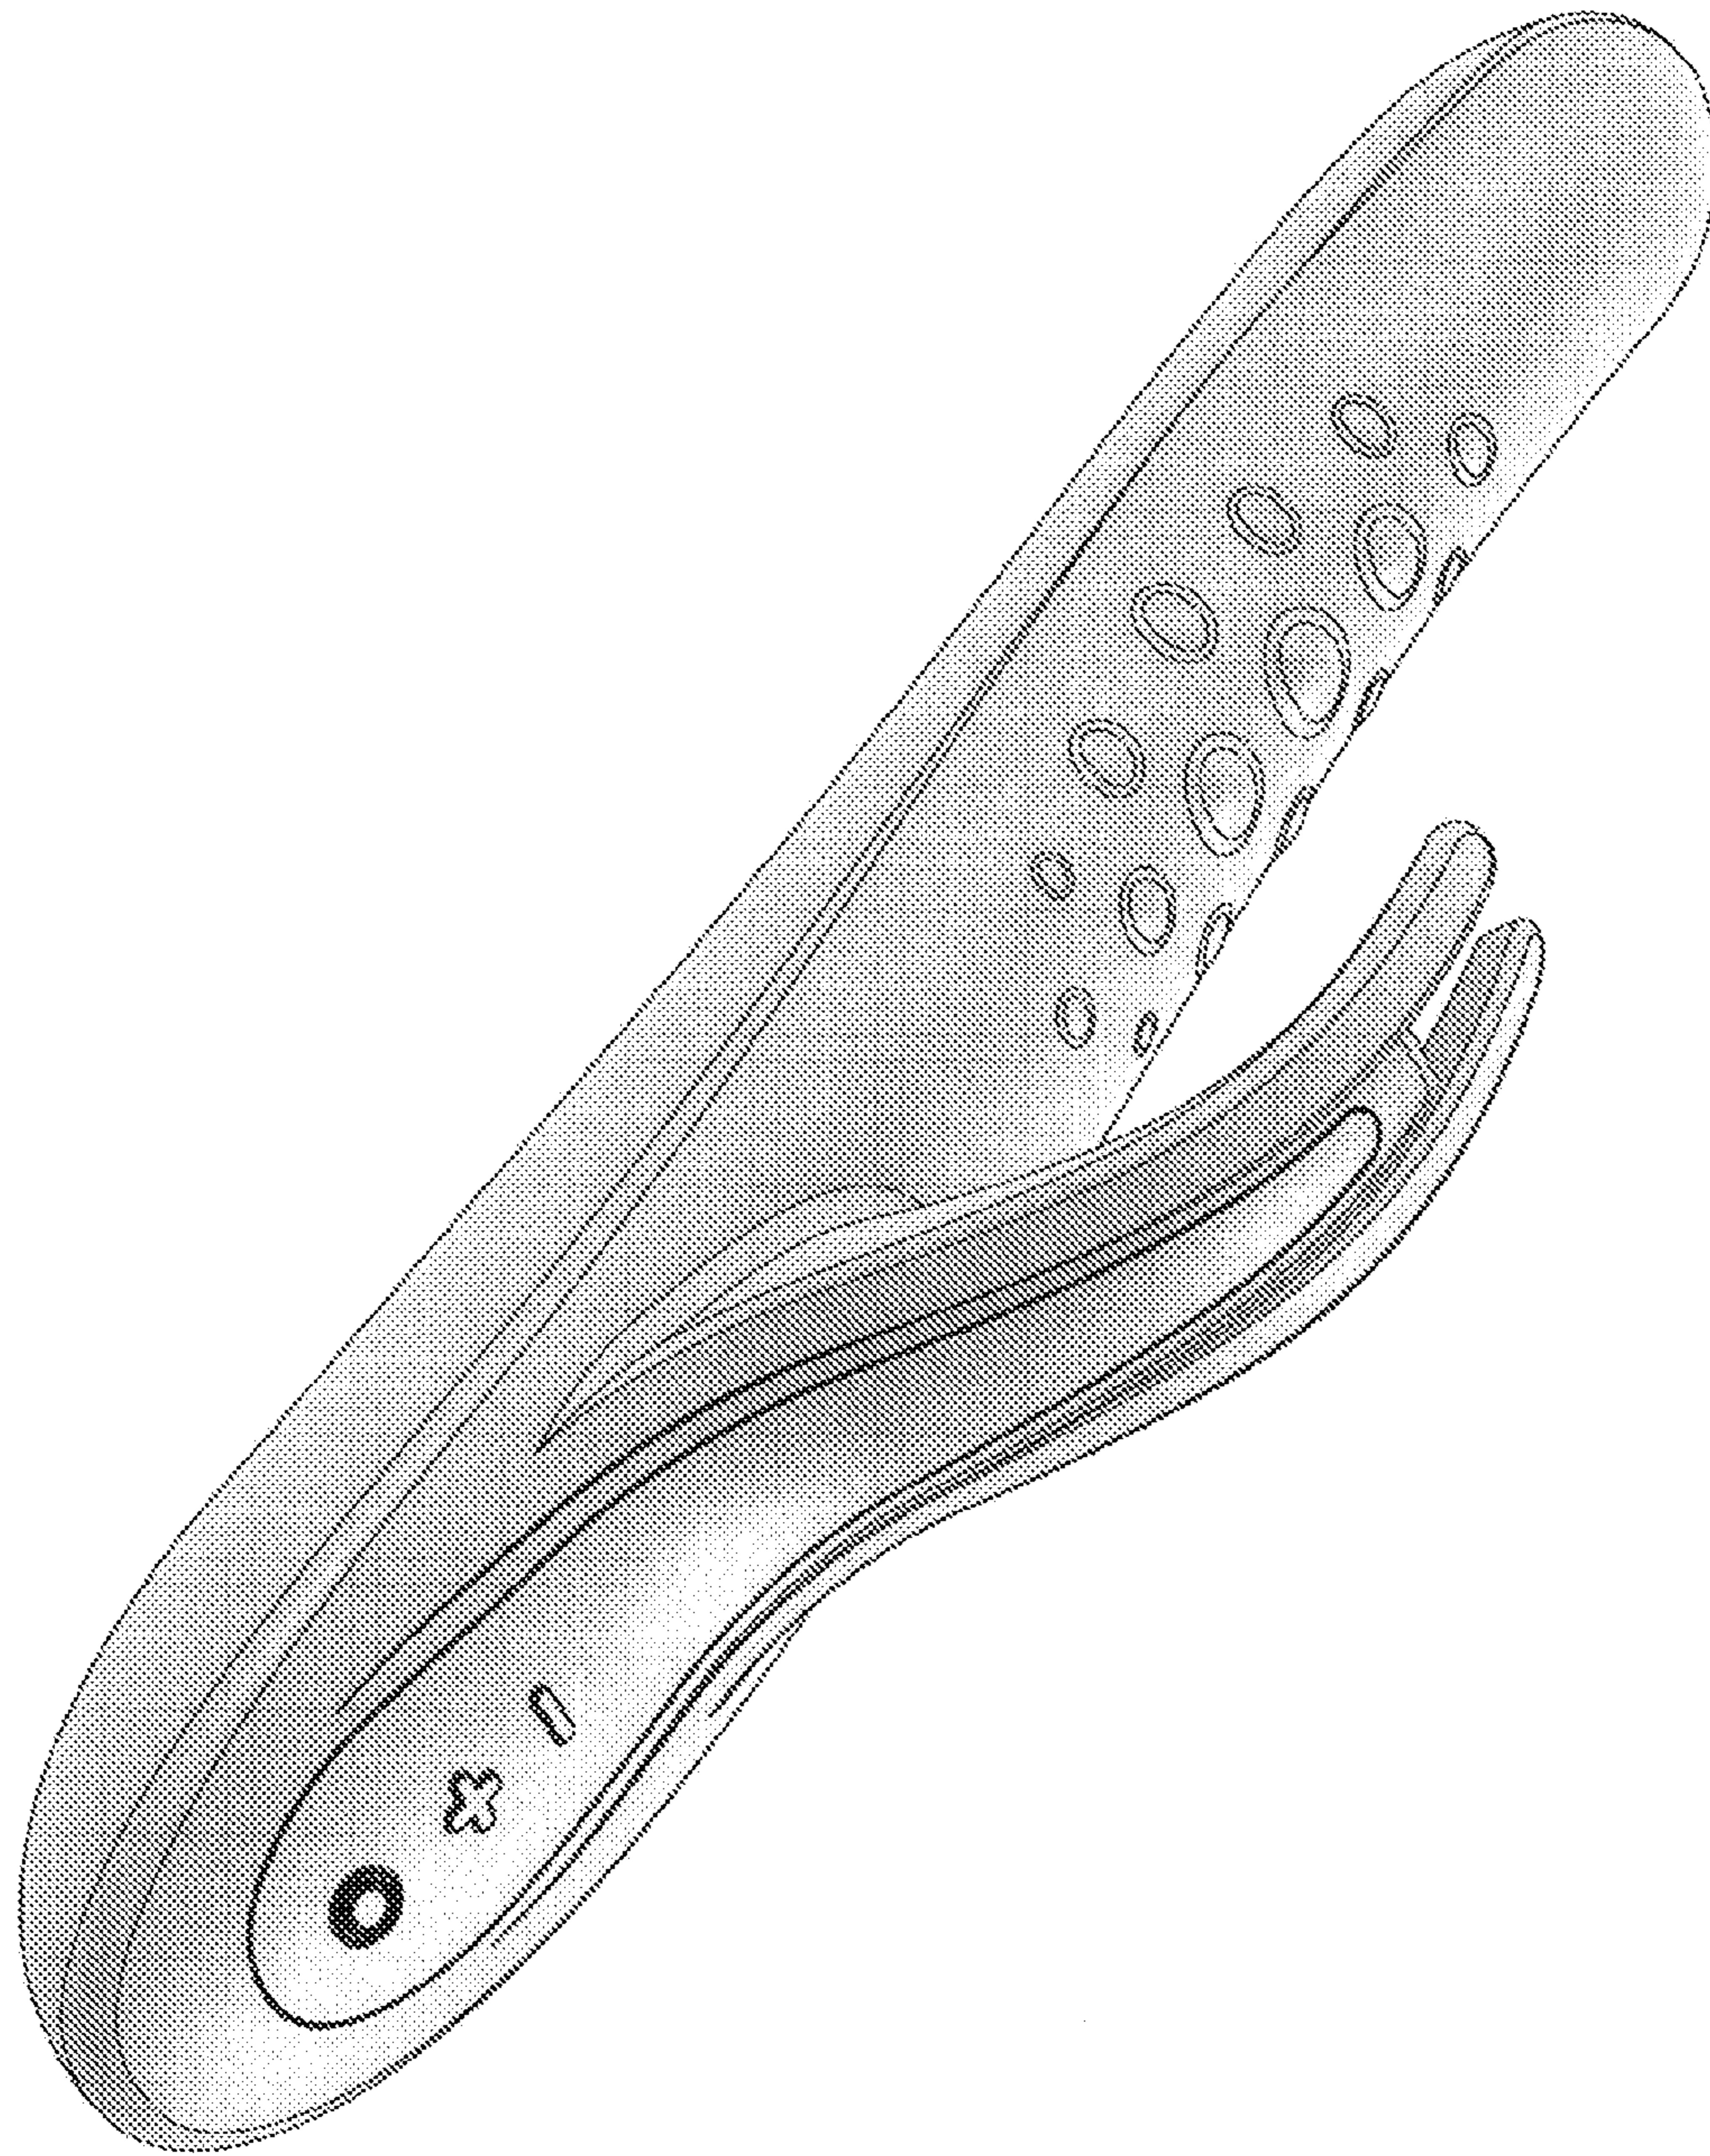


FIG. 2

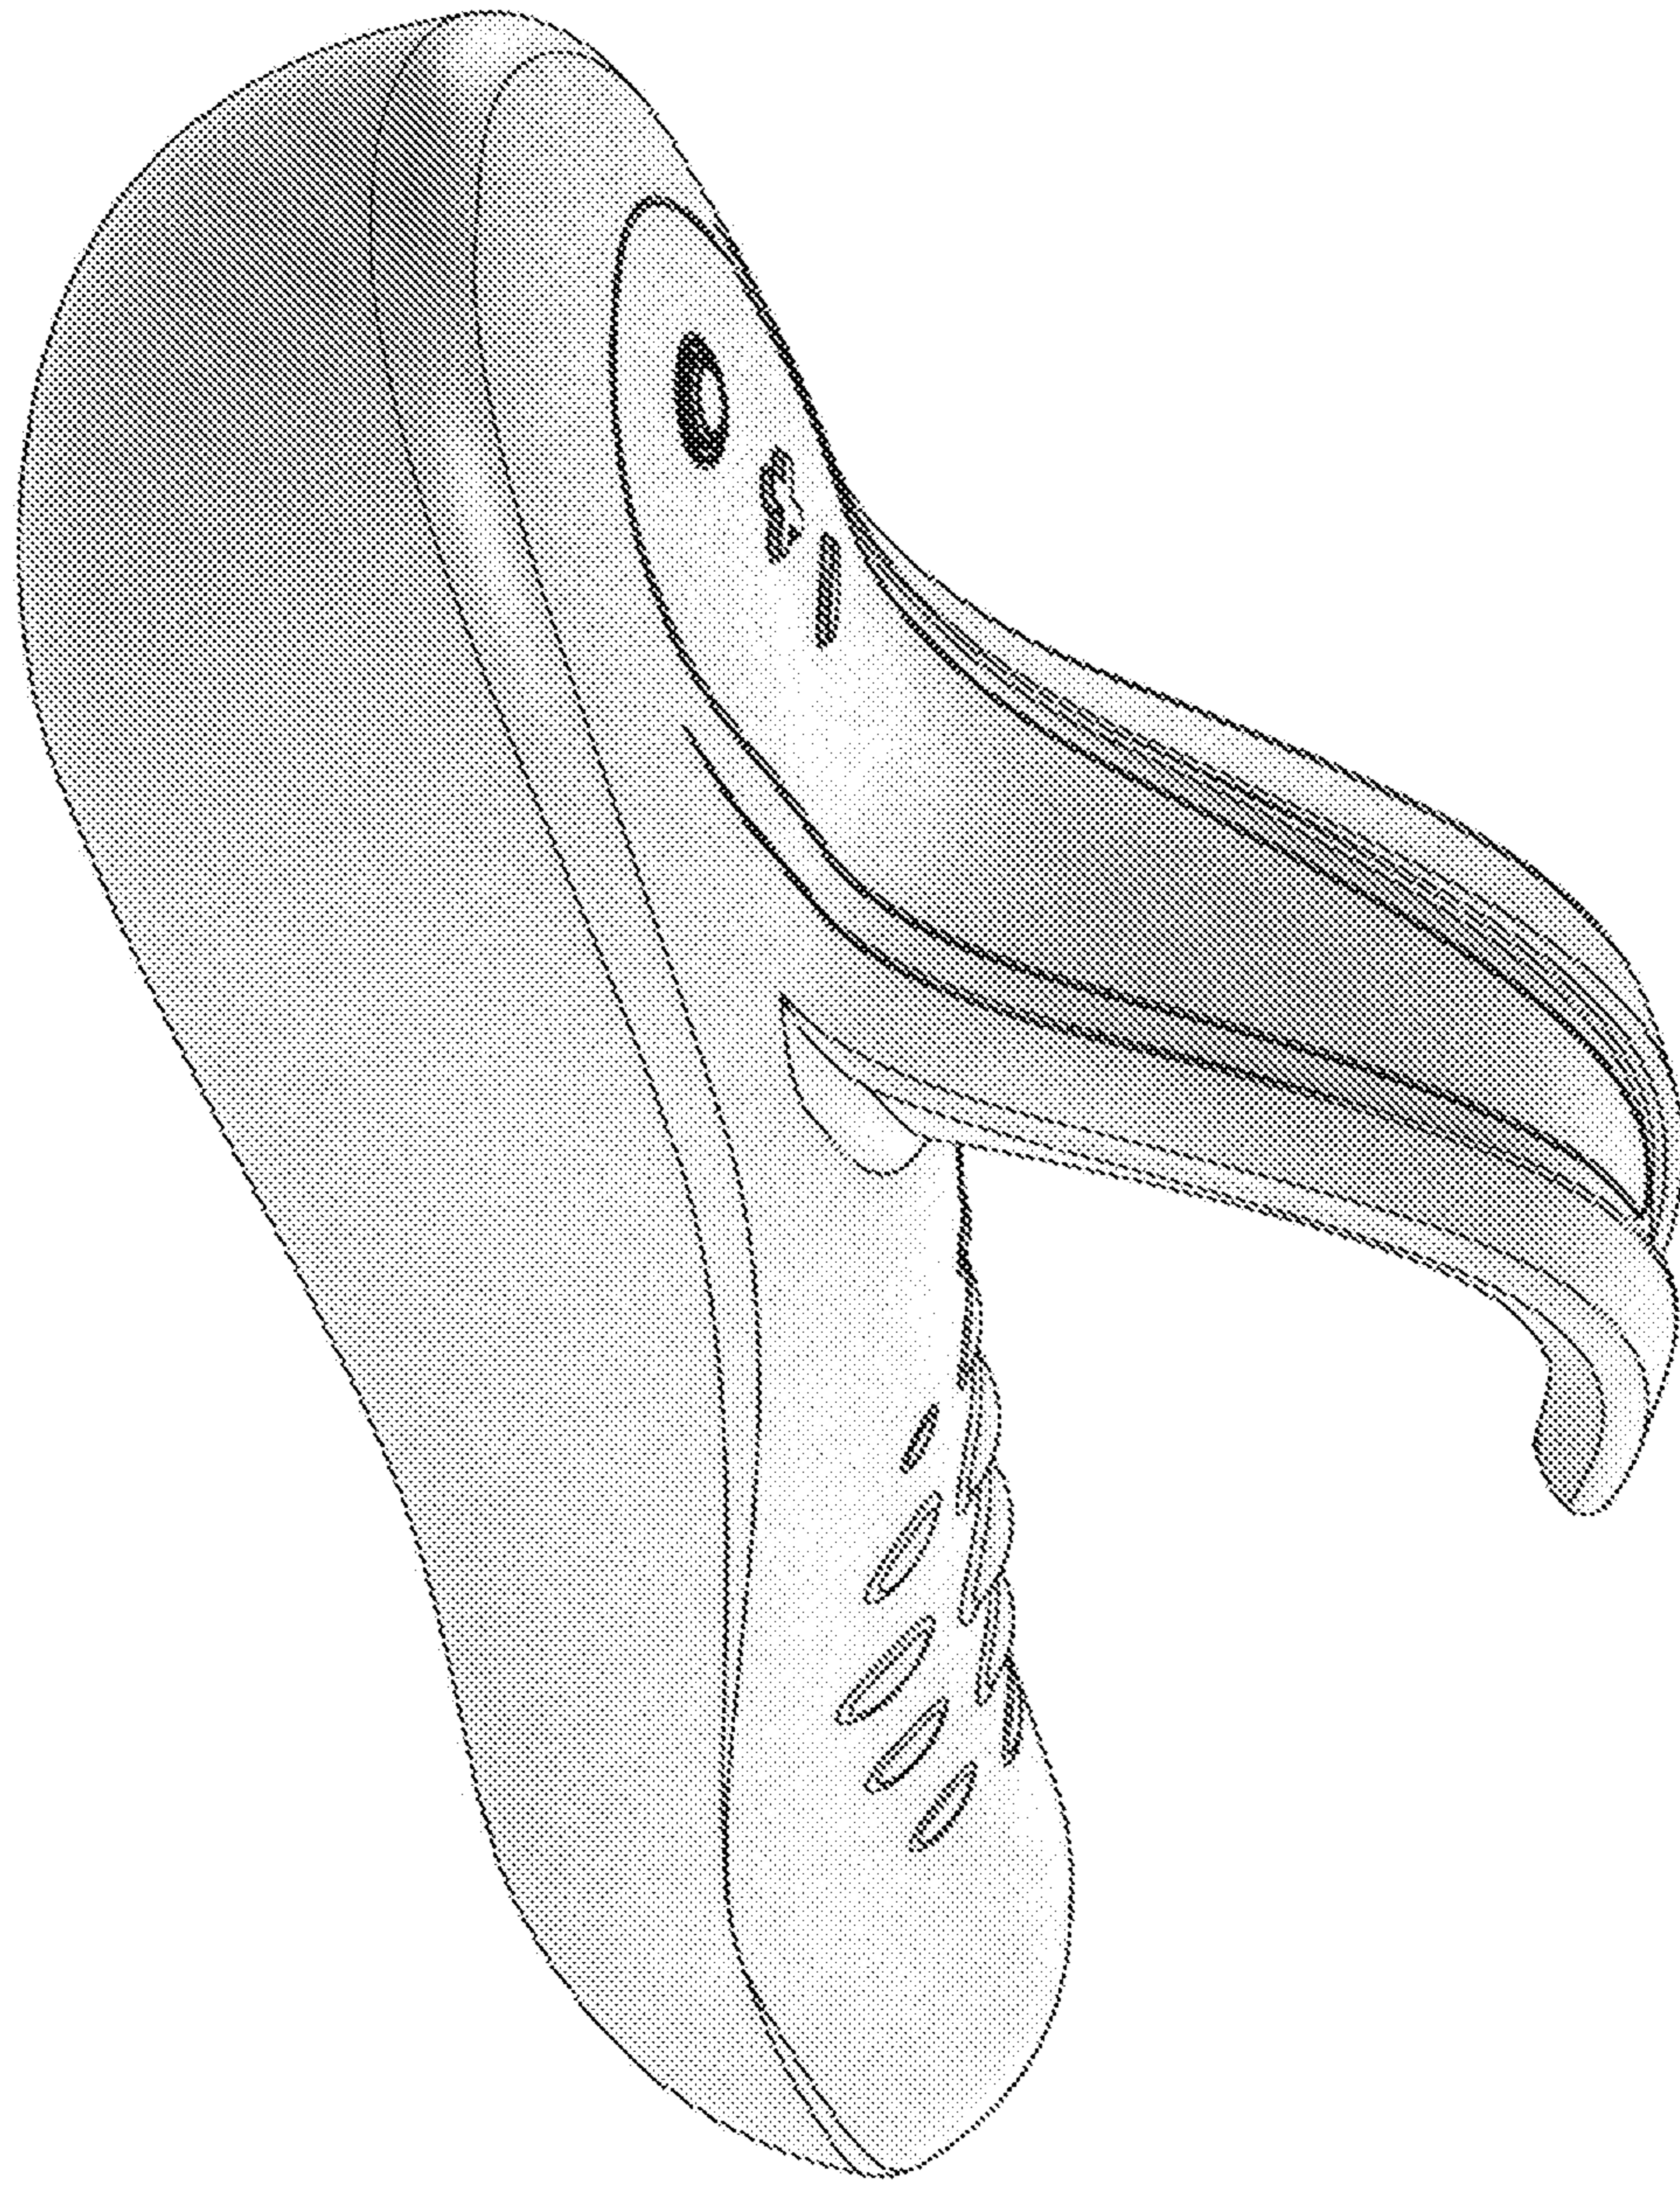


FIG. 3

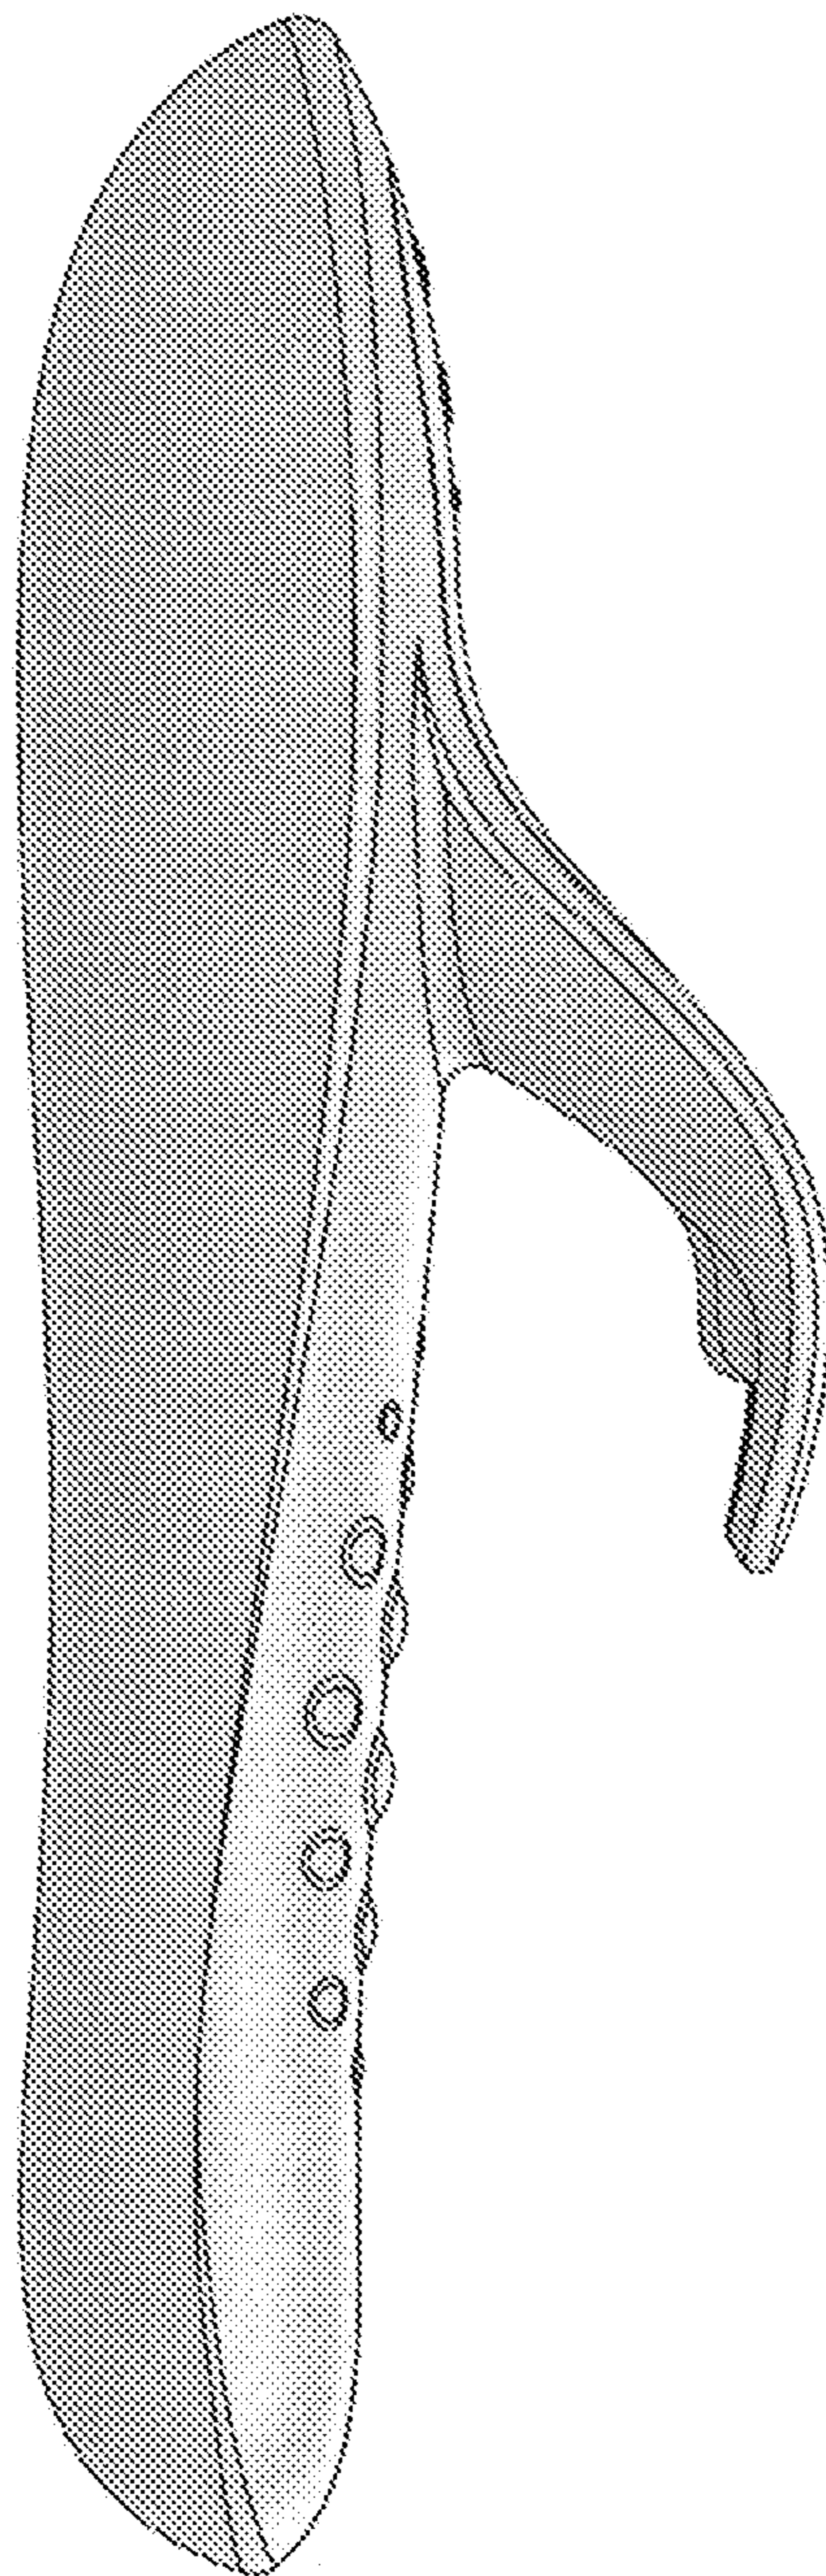


FIG. 4

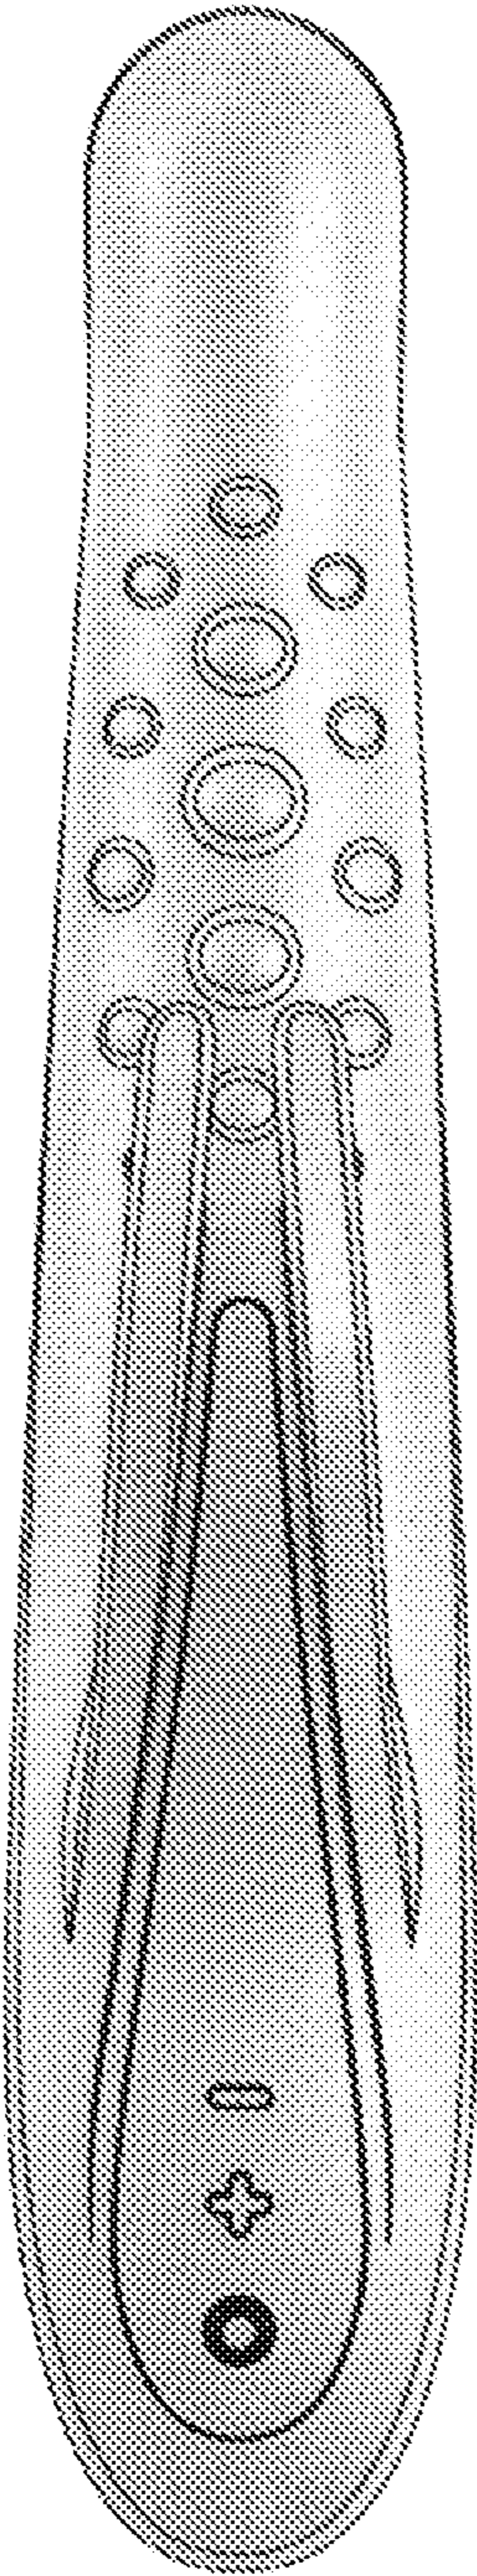


FIG. 5

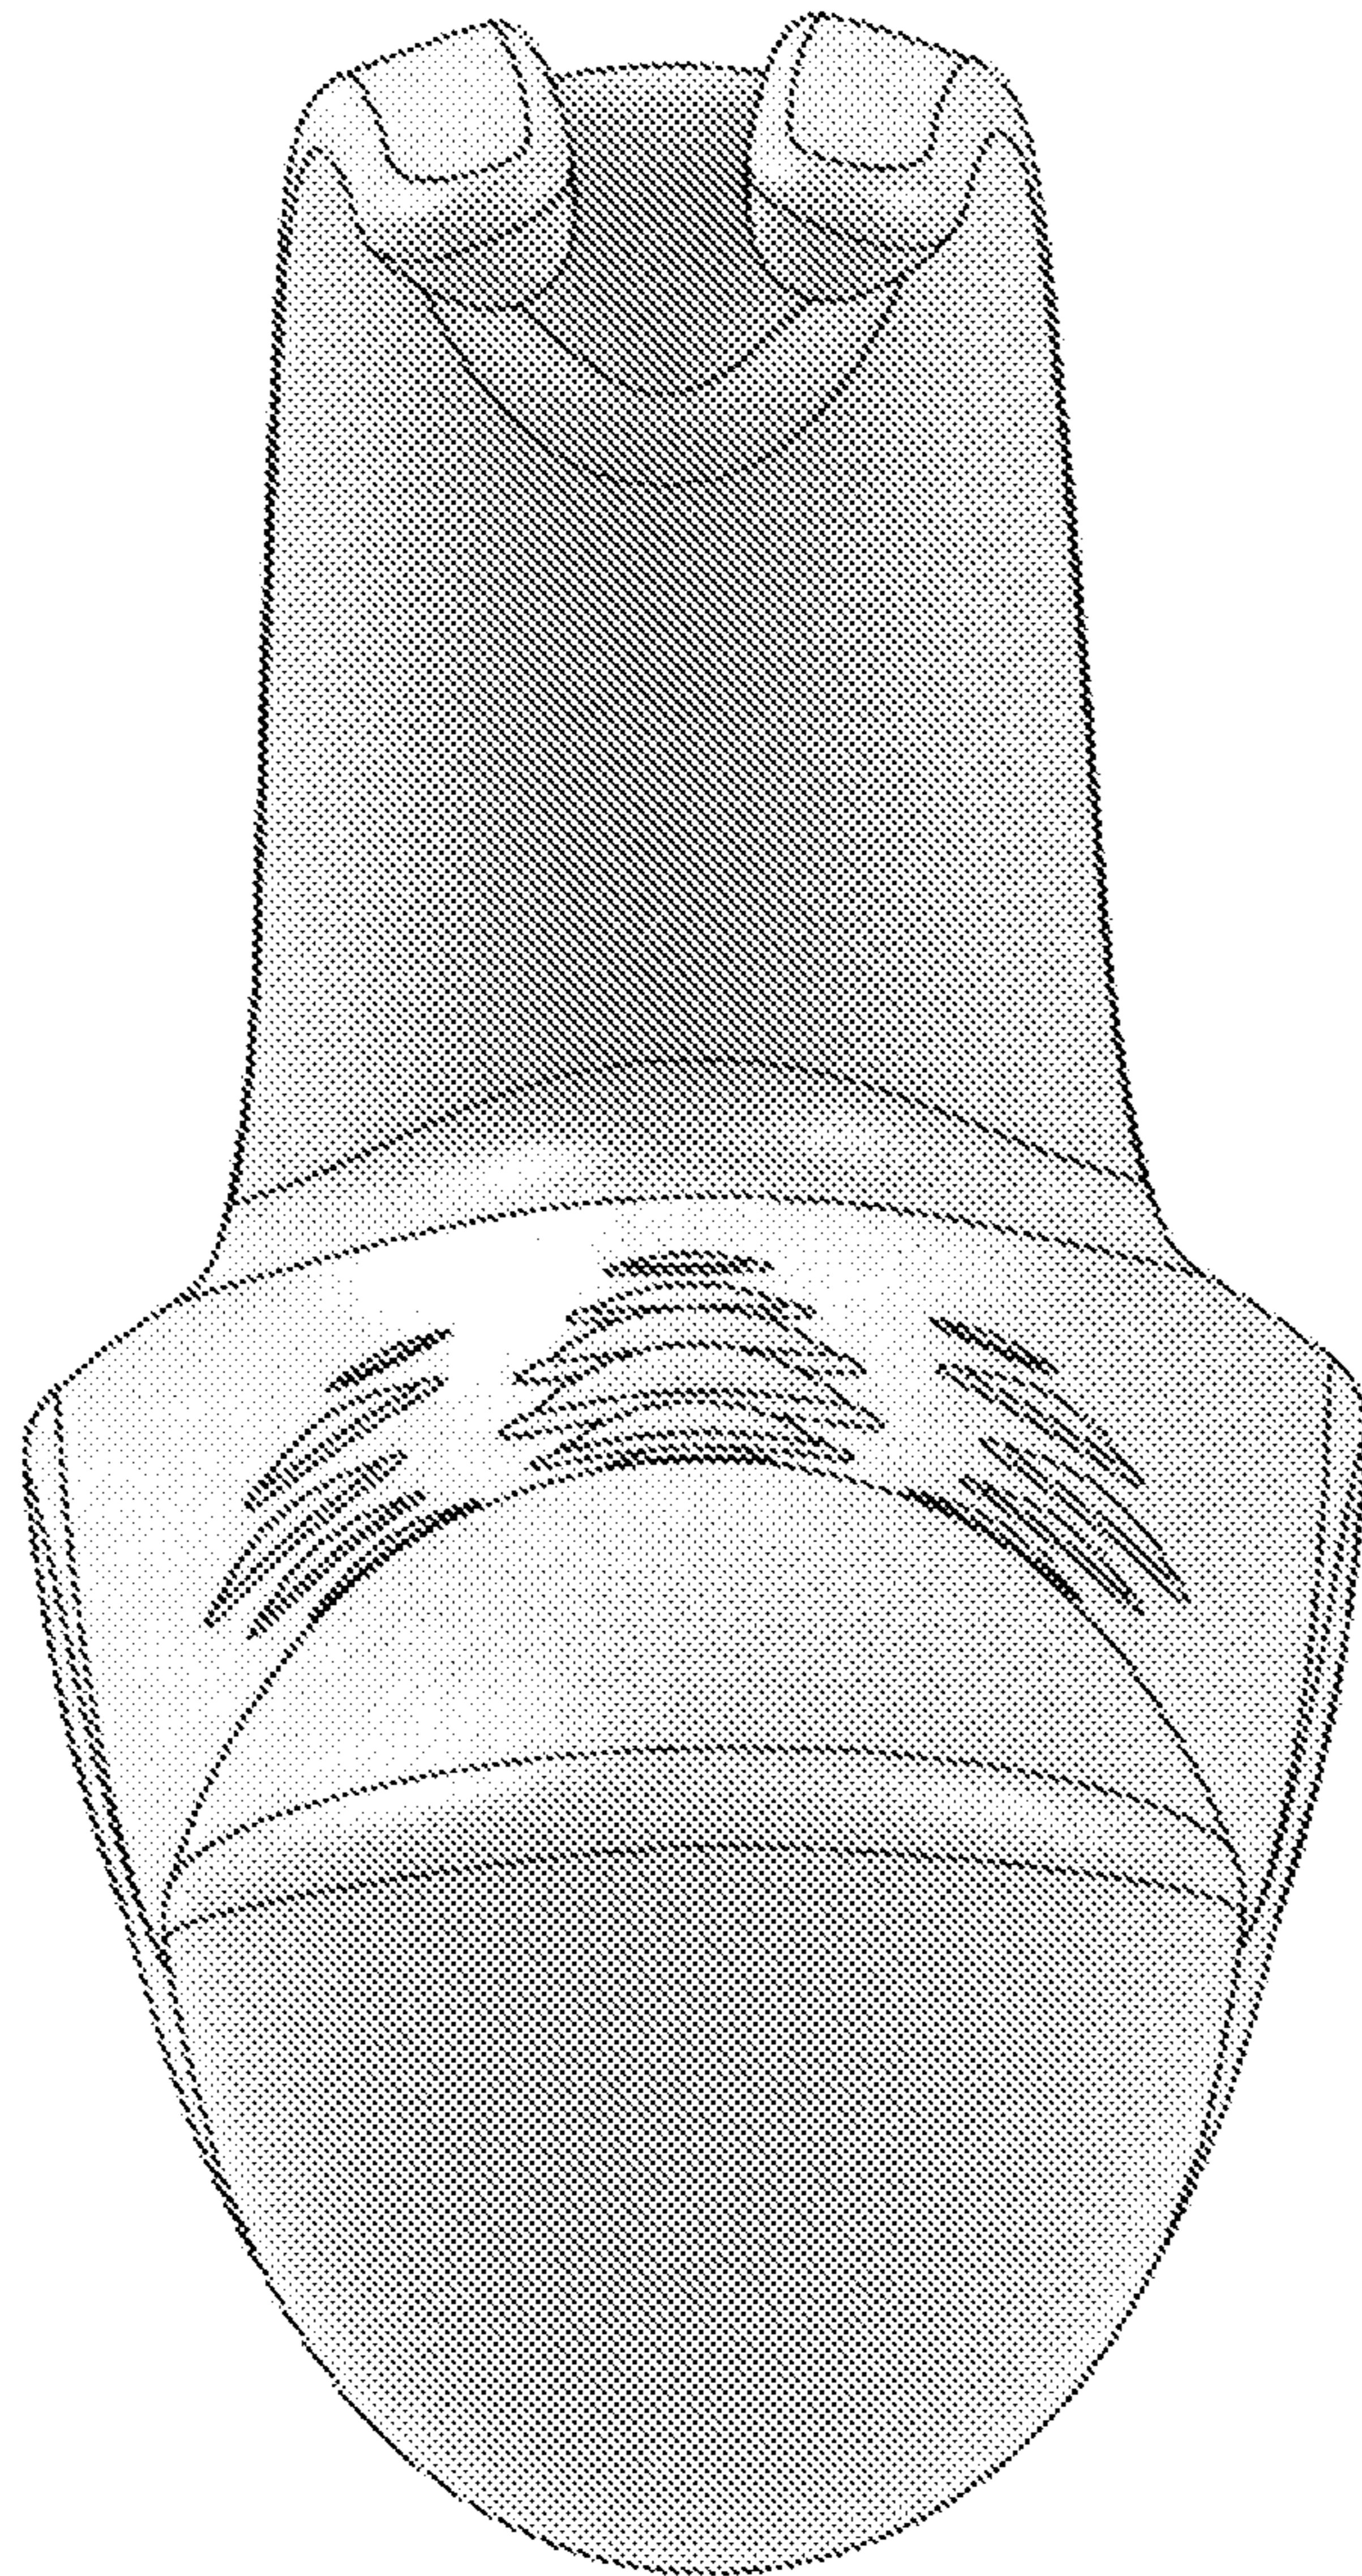


FIG. 6