



US00D706438S

(12) **United States Design Patent**  
**Hahr et al.**

(10) **Patent No.:** **US D706,438 S**  
(45) **Date of Patent:** **\*\* Jun. 3, 2014**

(54) **STIMULATION DEVICE**  
(71) Applicant: **Senses Toys Intellectual Property Management UG**, Bielefeld (DE)  
(72) Inventors: **Meike Hahr**, Hamburg (DE); **Heiko Tullney**, Hamburg (DE); **Till Muhl**, Hamburg (DE); **Thomas Milewski**, Halstenbek (DE)  
(73) Assignee: **Ovo Joint Venture LLC**, Pembroke Park, FL (US)

D564,666 S \* 3/2008 Klearman ..... D24/215  
D566,289 S \* 4/2008 Tasker et al. .... D24/215  
D581,544 S \* 11/2008 Adams ..... D24/215  
D637,302 S \* 5/2011 Post ..... D24/215  
D643,129 S \* 8/2011 Talbot et al. .... D24/215  
D694,897 S \* 12/2013 Small ..... D24/215

\* cited by examiner

*Primary Examiner* — Sandra Snapp

(74) *Attorney, Agent, or Firm* — Merek, Blackmon & Voorhees, LLC

(\*\*) Term: **14 Years**

(57) **CLAIM**

The ornamental design for a stimulation device, as shown and described.

(21) Appl. No.: **29/447,965**

**DESCRIPTION**

(22) Filed: **Mar. 8, 2013**

(30) **Foreign Application Priority Data**

Sep. 10, 2012 (EM) ..... 001342935-0075

(51) **LOC (10) Cl.** ..... **28-03**

(52) **U.S. Cl.**  
USPC ..... **D24/215**

(58) **Field of Classification Search**  
USPC ..... D24/200, 211, 212, 213, 214, 215;  
601/114, 120, 121, 124, 125, 130, 131,  
601/134, 135, 136, 137  
See application file for complete search history.


FIG. 1 is a front elevation of a first embodiment of a stimulation device showing the design;  
FIG. 2 is a top plan view of the stimulation device of FIG. 1;  
FIG. 3 is a right side elevation of the stimulation device of FIG. 1;  
FIG. 4 is a perspective view taken from the front and right side of the stimulation device of FIG. 1;  
FIG. 5 is a perspective view taken from the top, front and left side of the stimulation device of FIG. 1;  
FIG. 6 is a front elevation of a second embodiment of a stimulation device showing the design; and,  
FIG. 7 is a perspective view taken from the top, front and left side of the body of the stimulation device of FIG. 6.  
The right side elevation of the stimulation device of FIG. 6 is identical to FIG. 3.  
A perspective view taken from the front and right side of the stimulation device of FIG. 6 at an angle corresponding to the angle of the perspective view of FIG. 4 is identical to FIG. 4.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D521,151 S \* 5/2006 Dodd et al. .... D24/189  
D523,958 S \* 6/2006 Fang ..... D24/143  
D552,748 S \* 10/2007 Gromosaik et al. .... D24/215  
D552,749 S \* 10/2007 Gromosaik et al. .... D24/215  
D557,806 S \* 12/2007 Gromosaik et al. .... D24/143

**1 Claim, 7 Drawing Sheets**

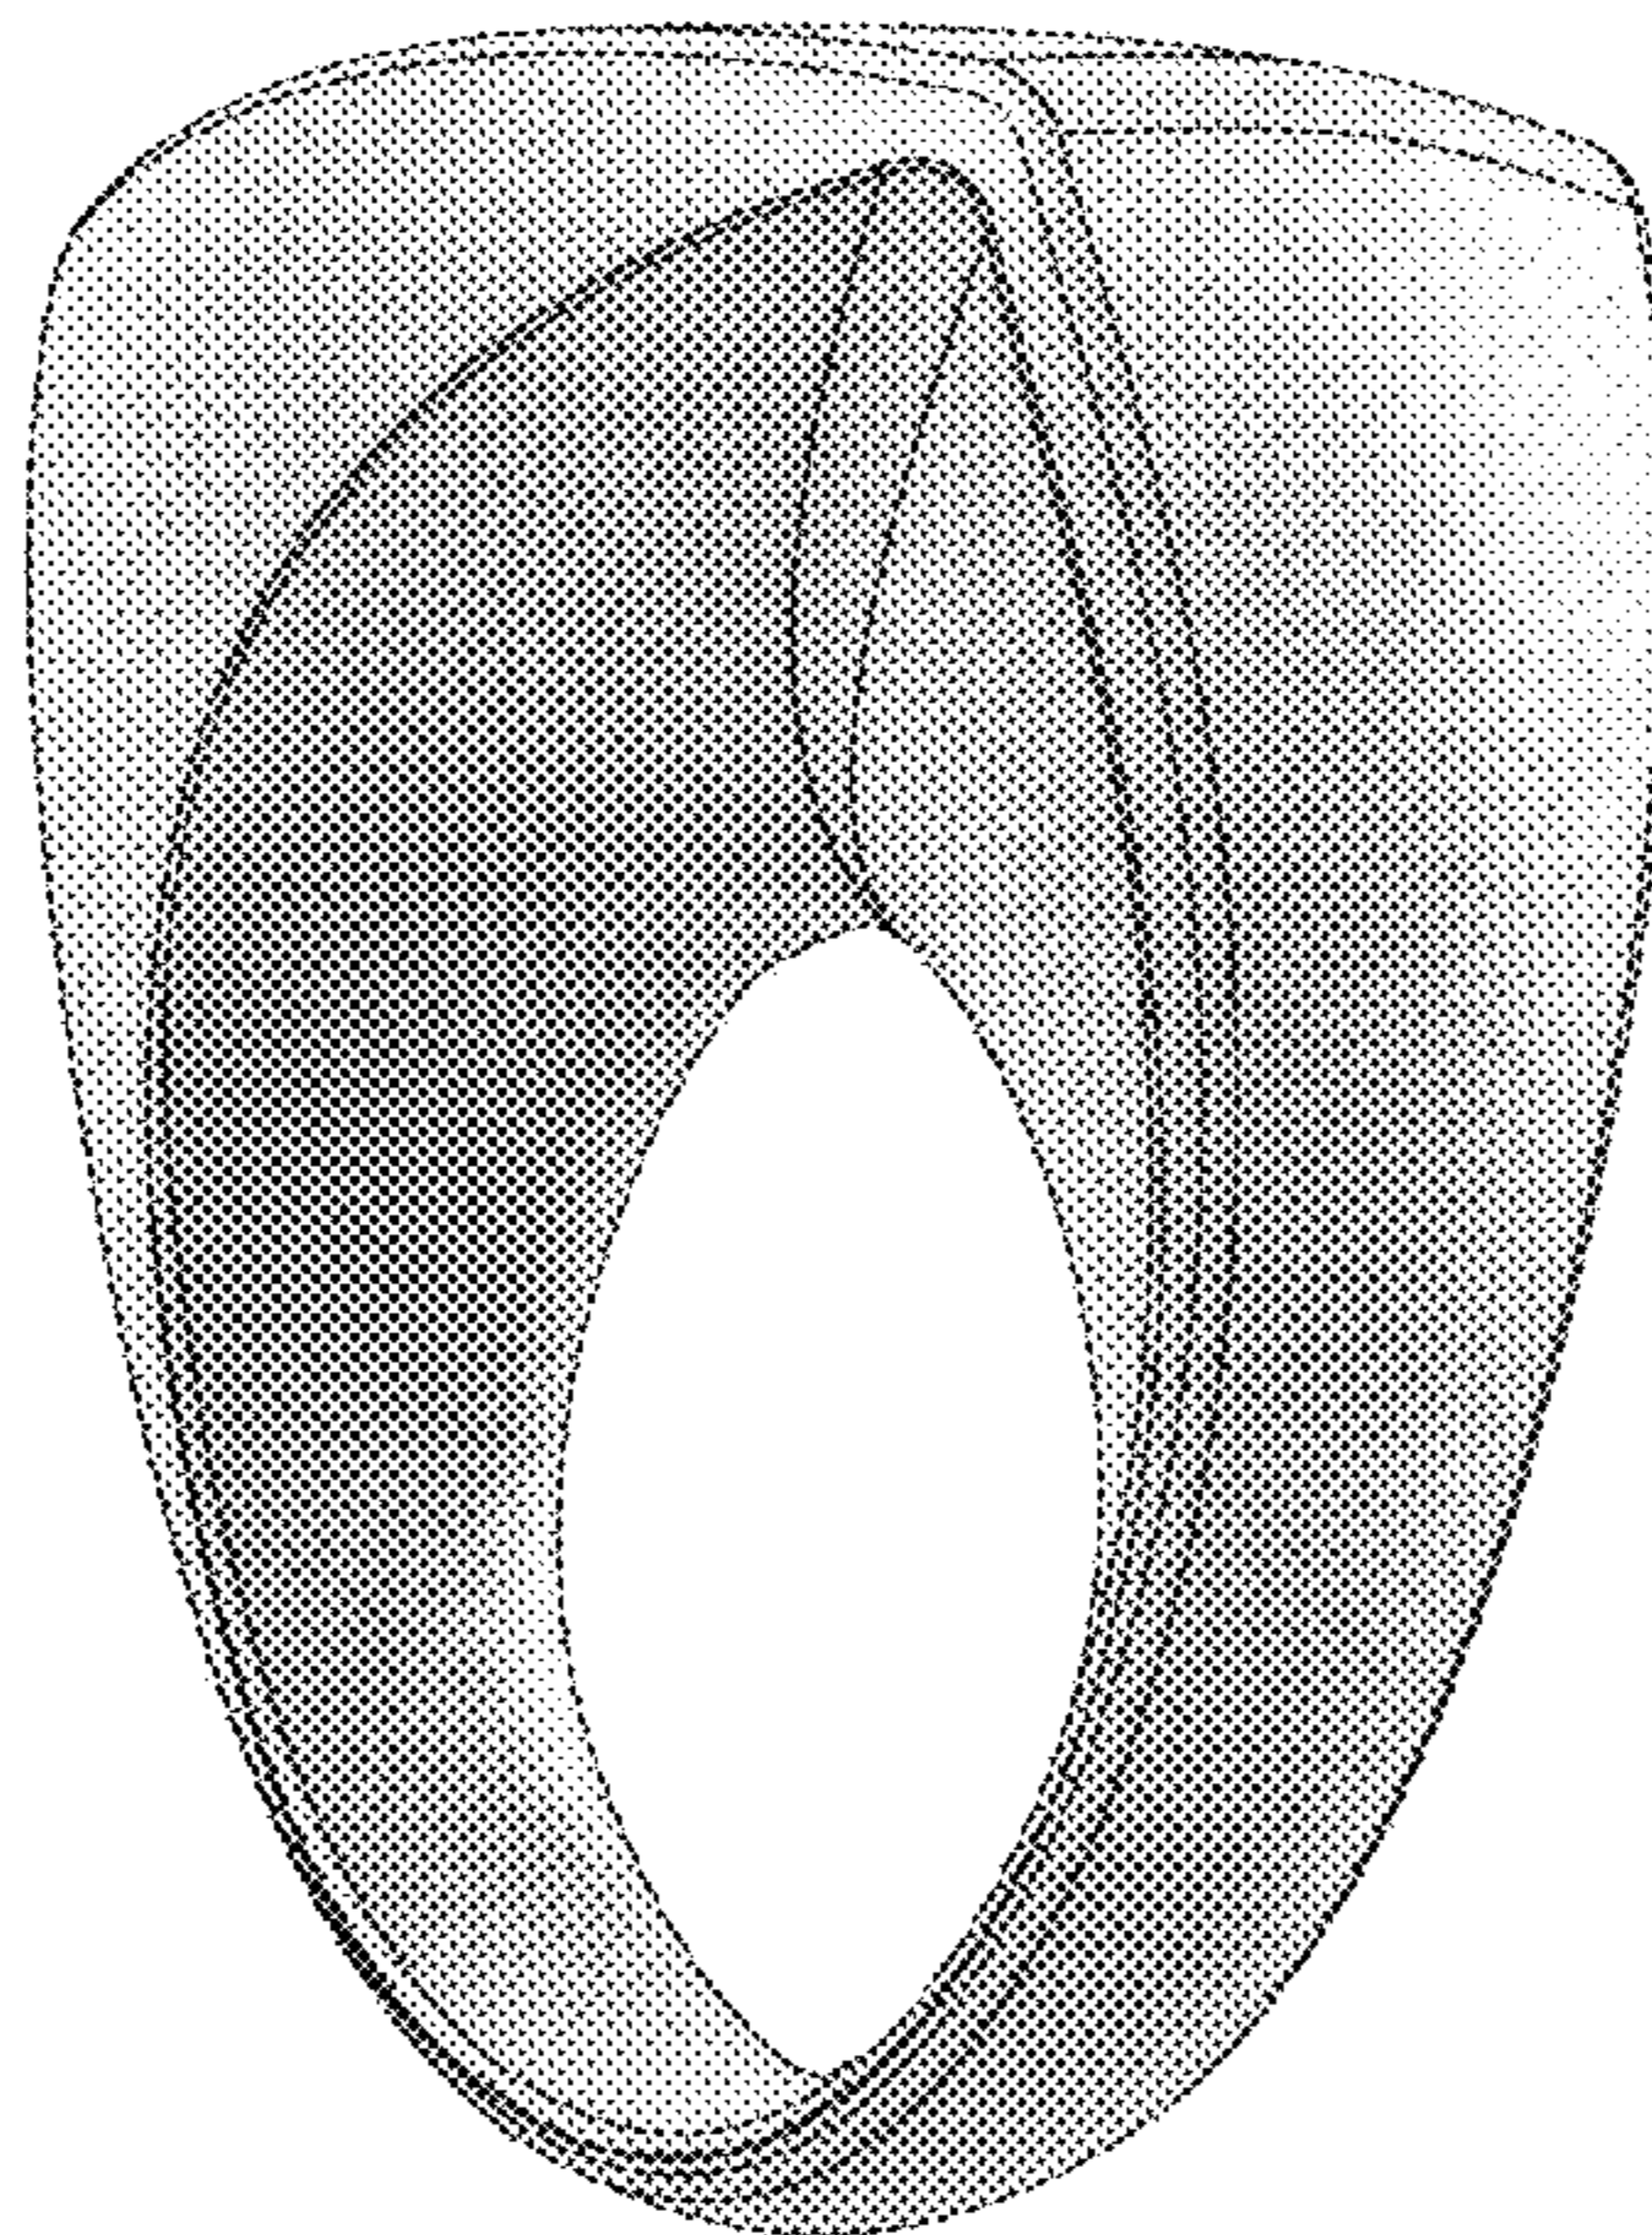

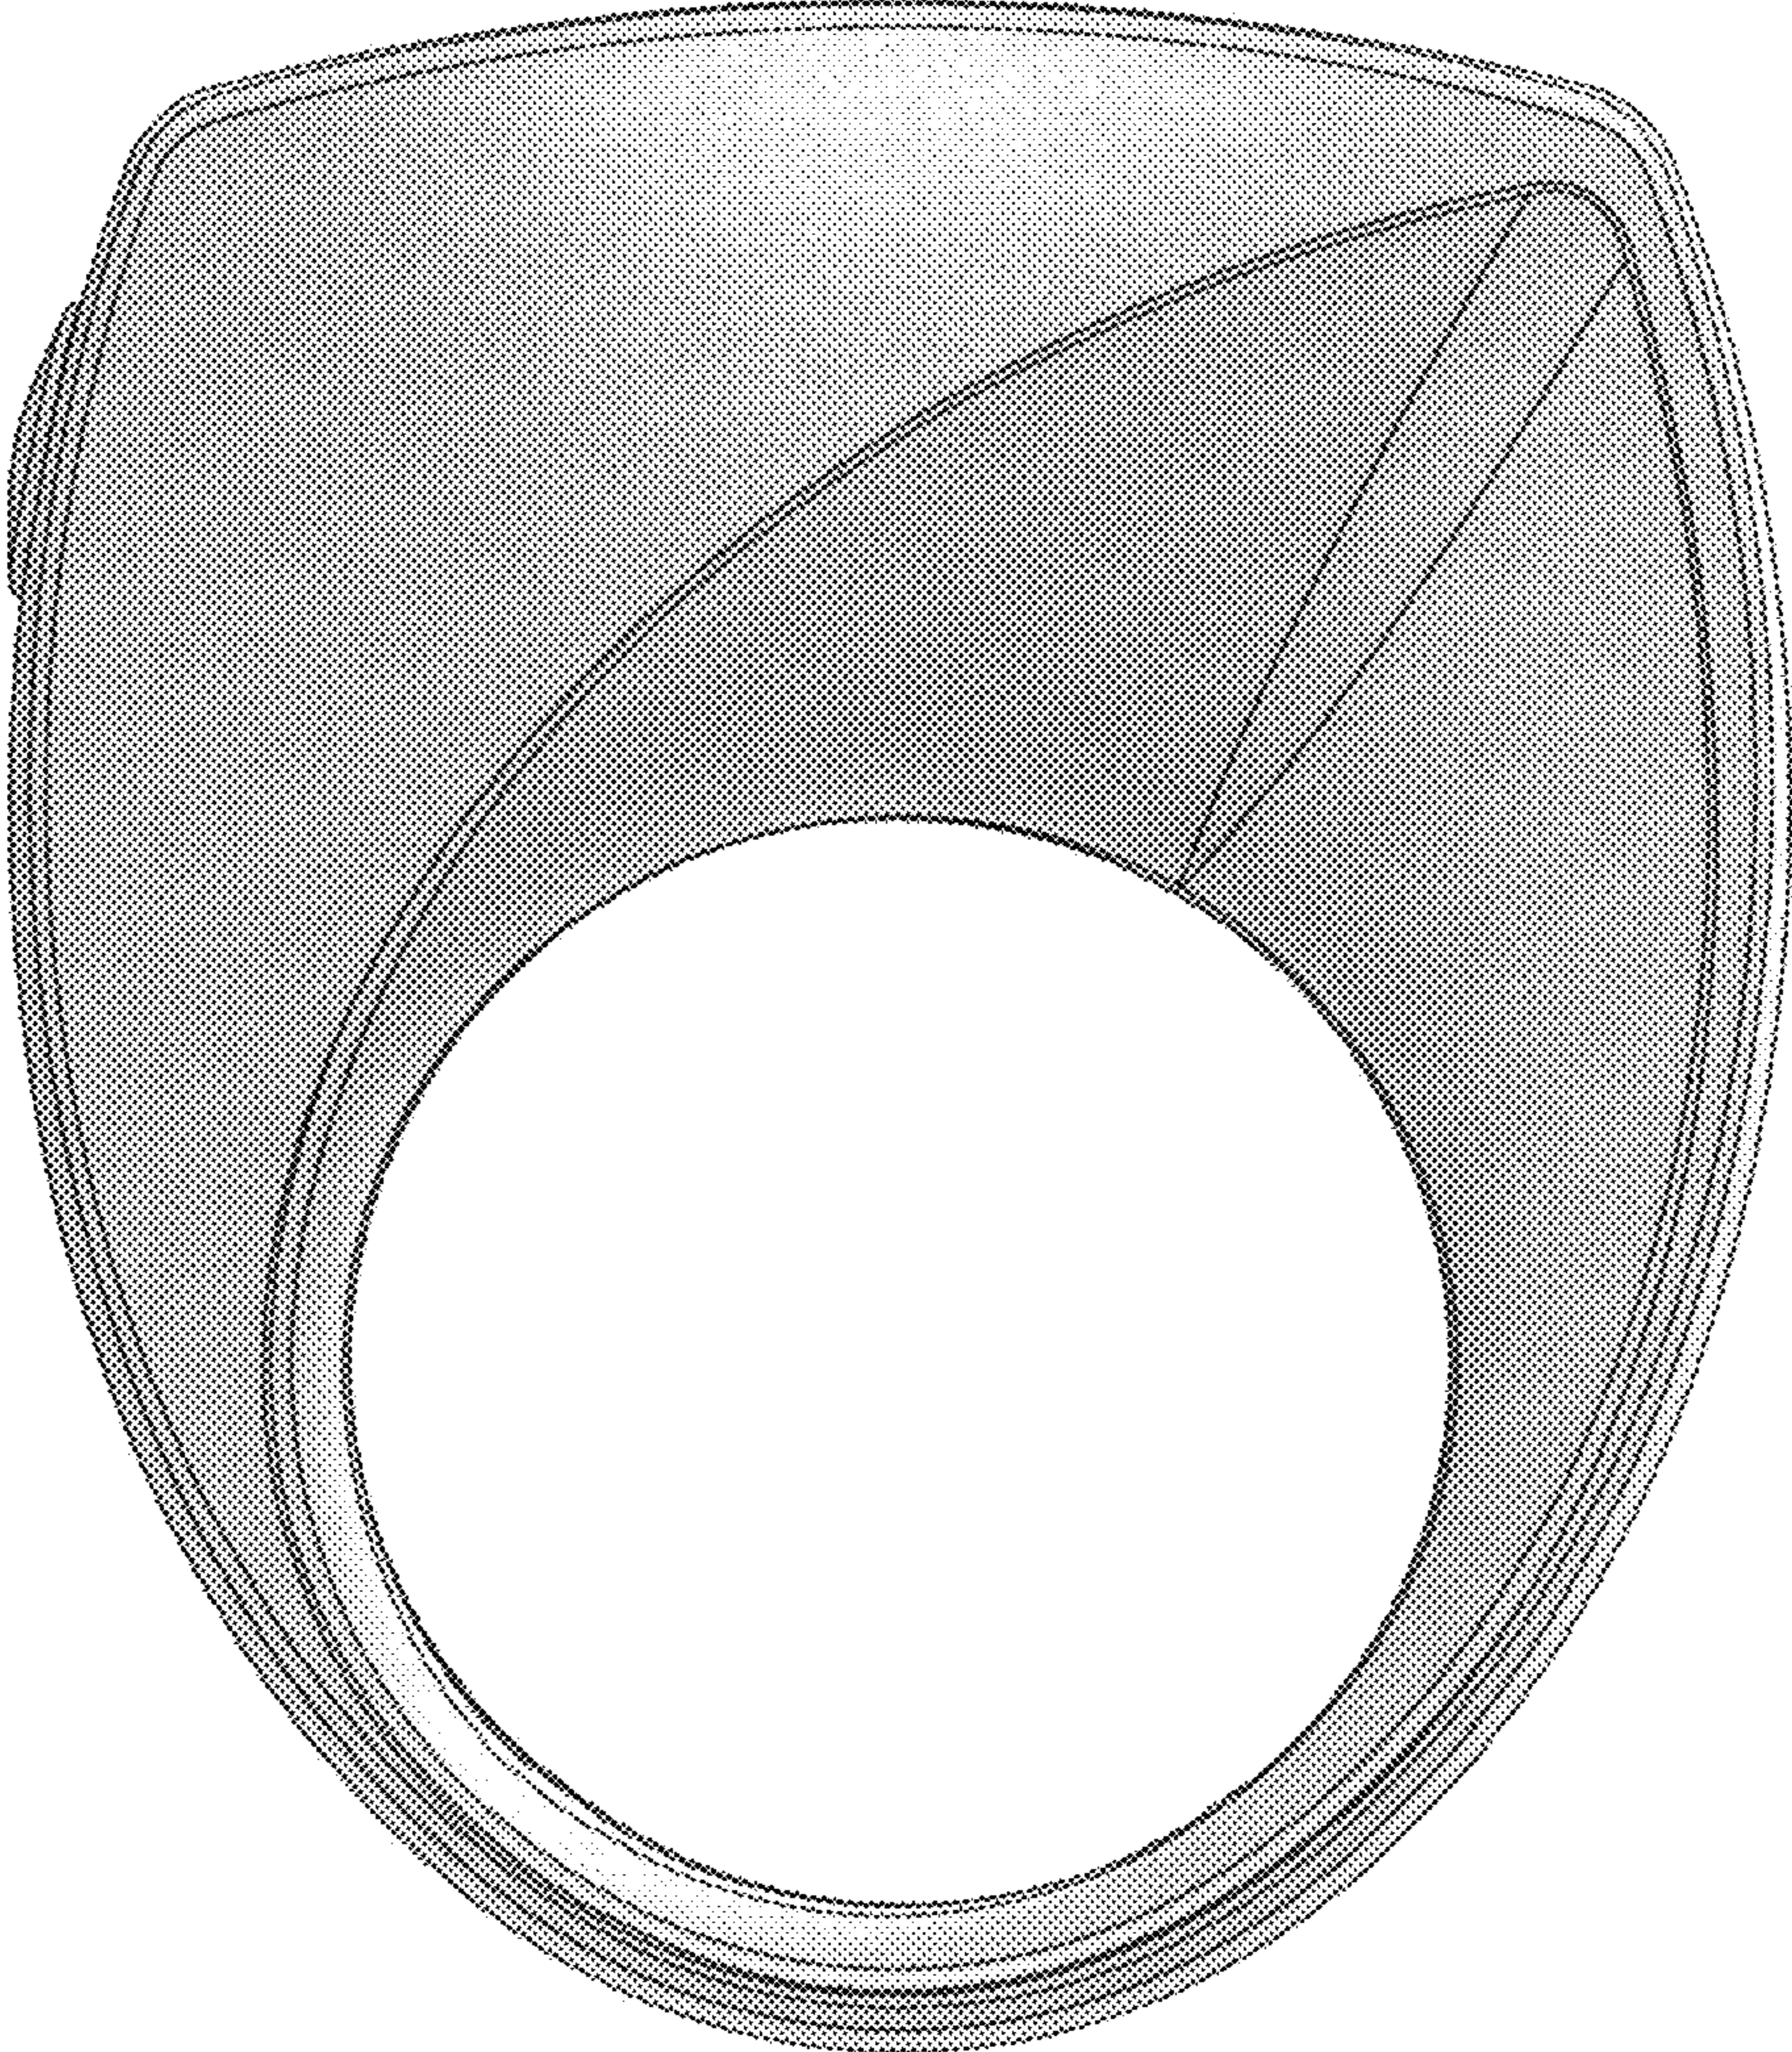


FIG. 1

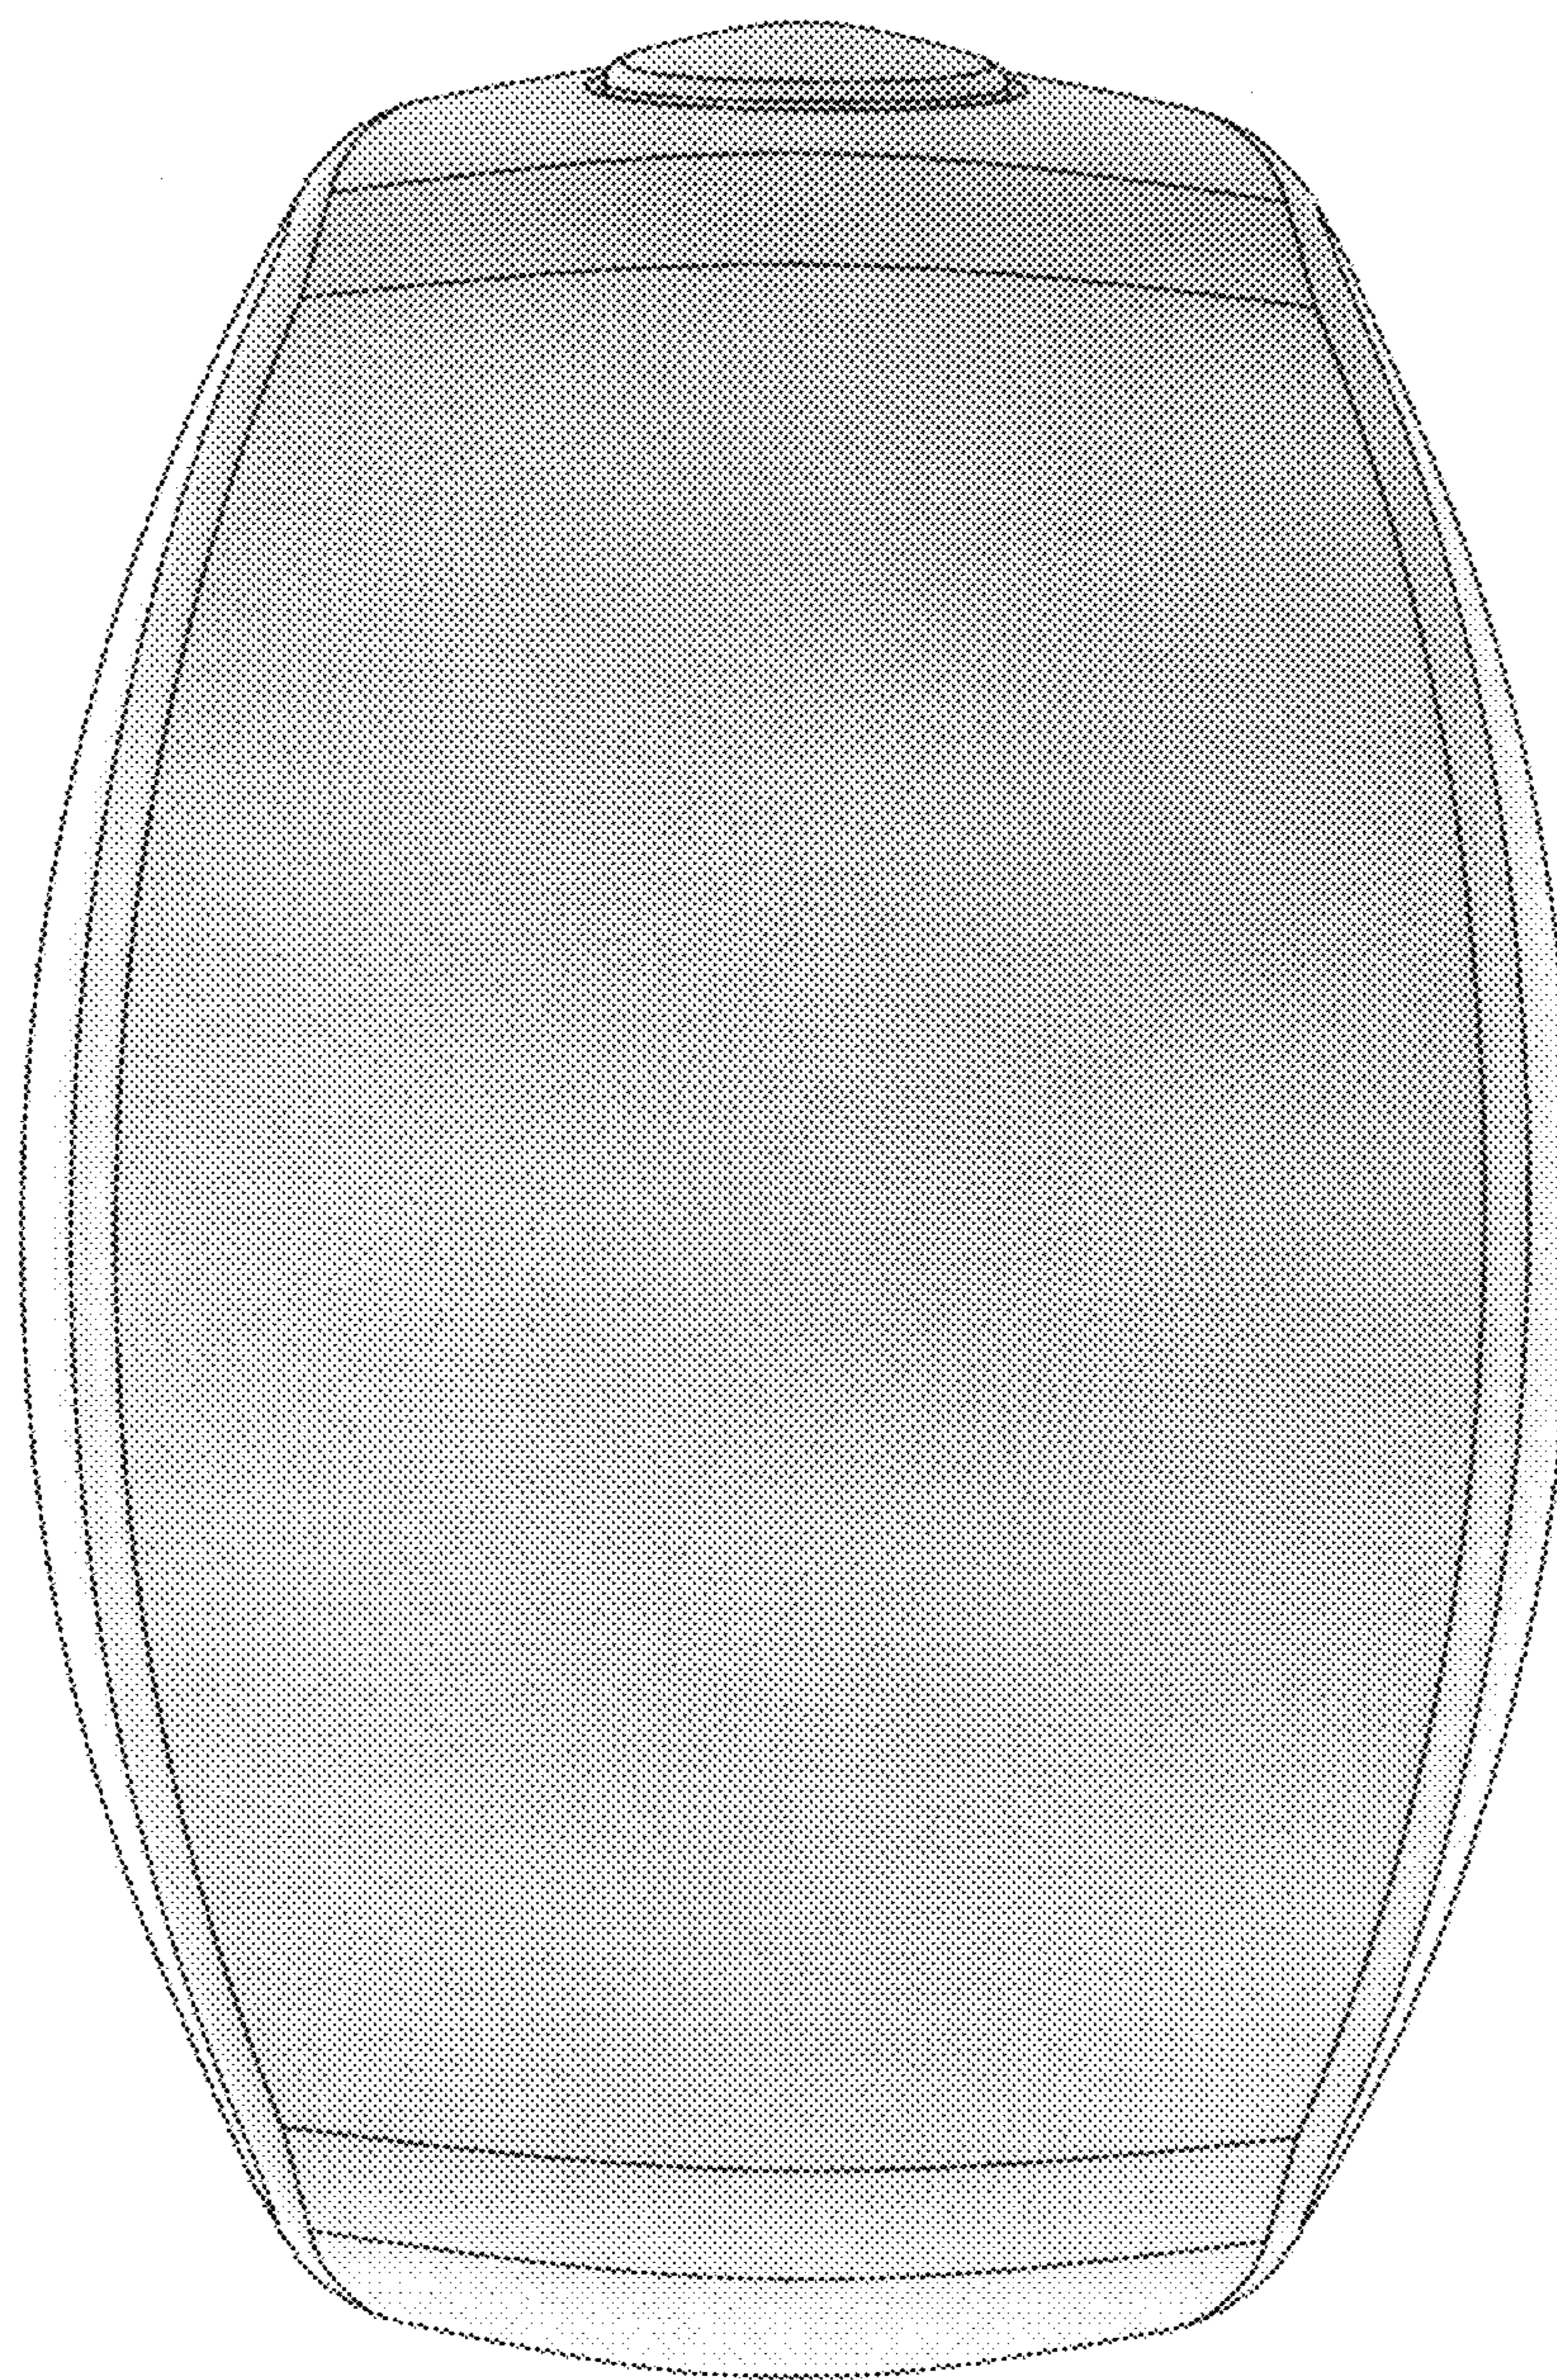


FIG. 2

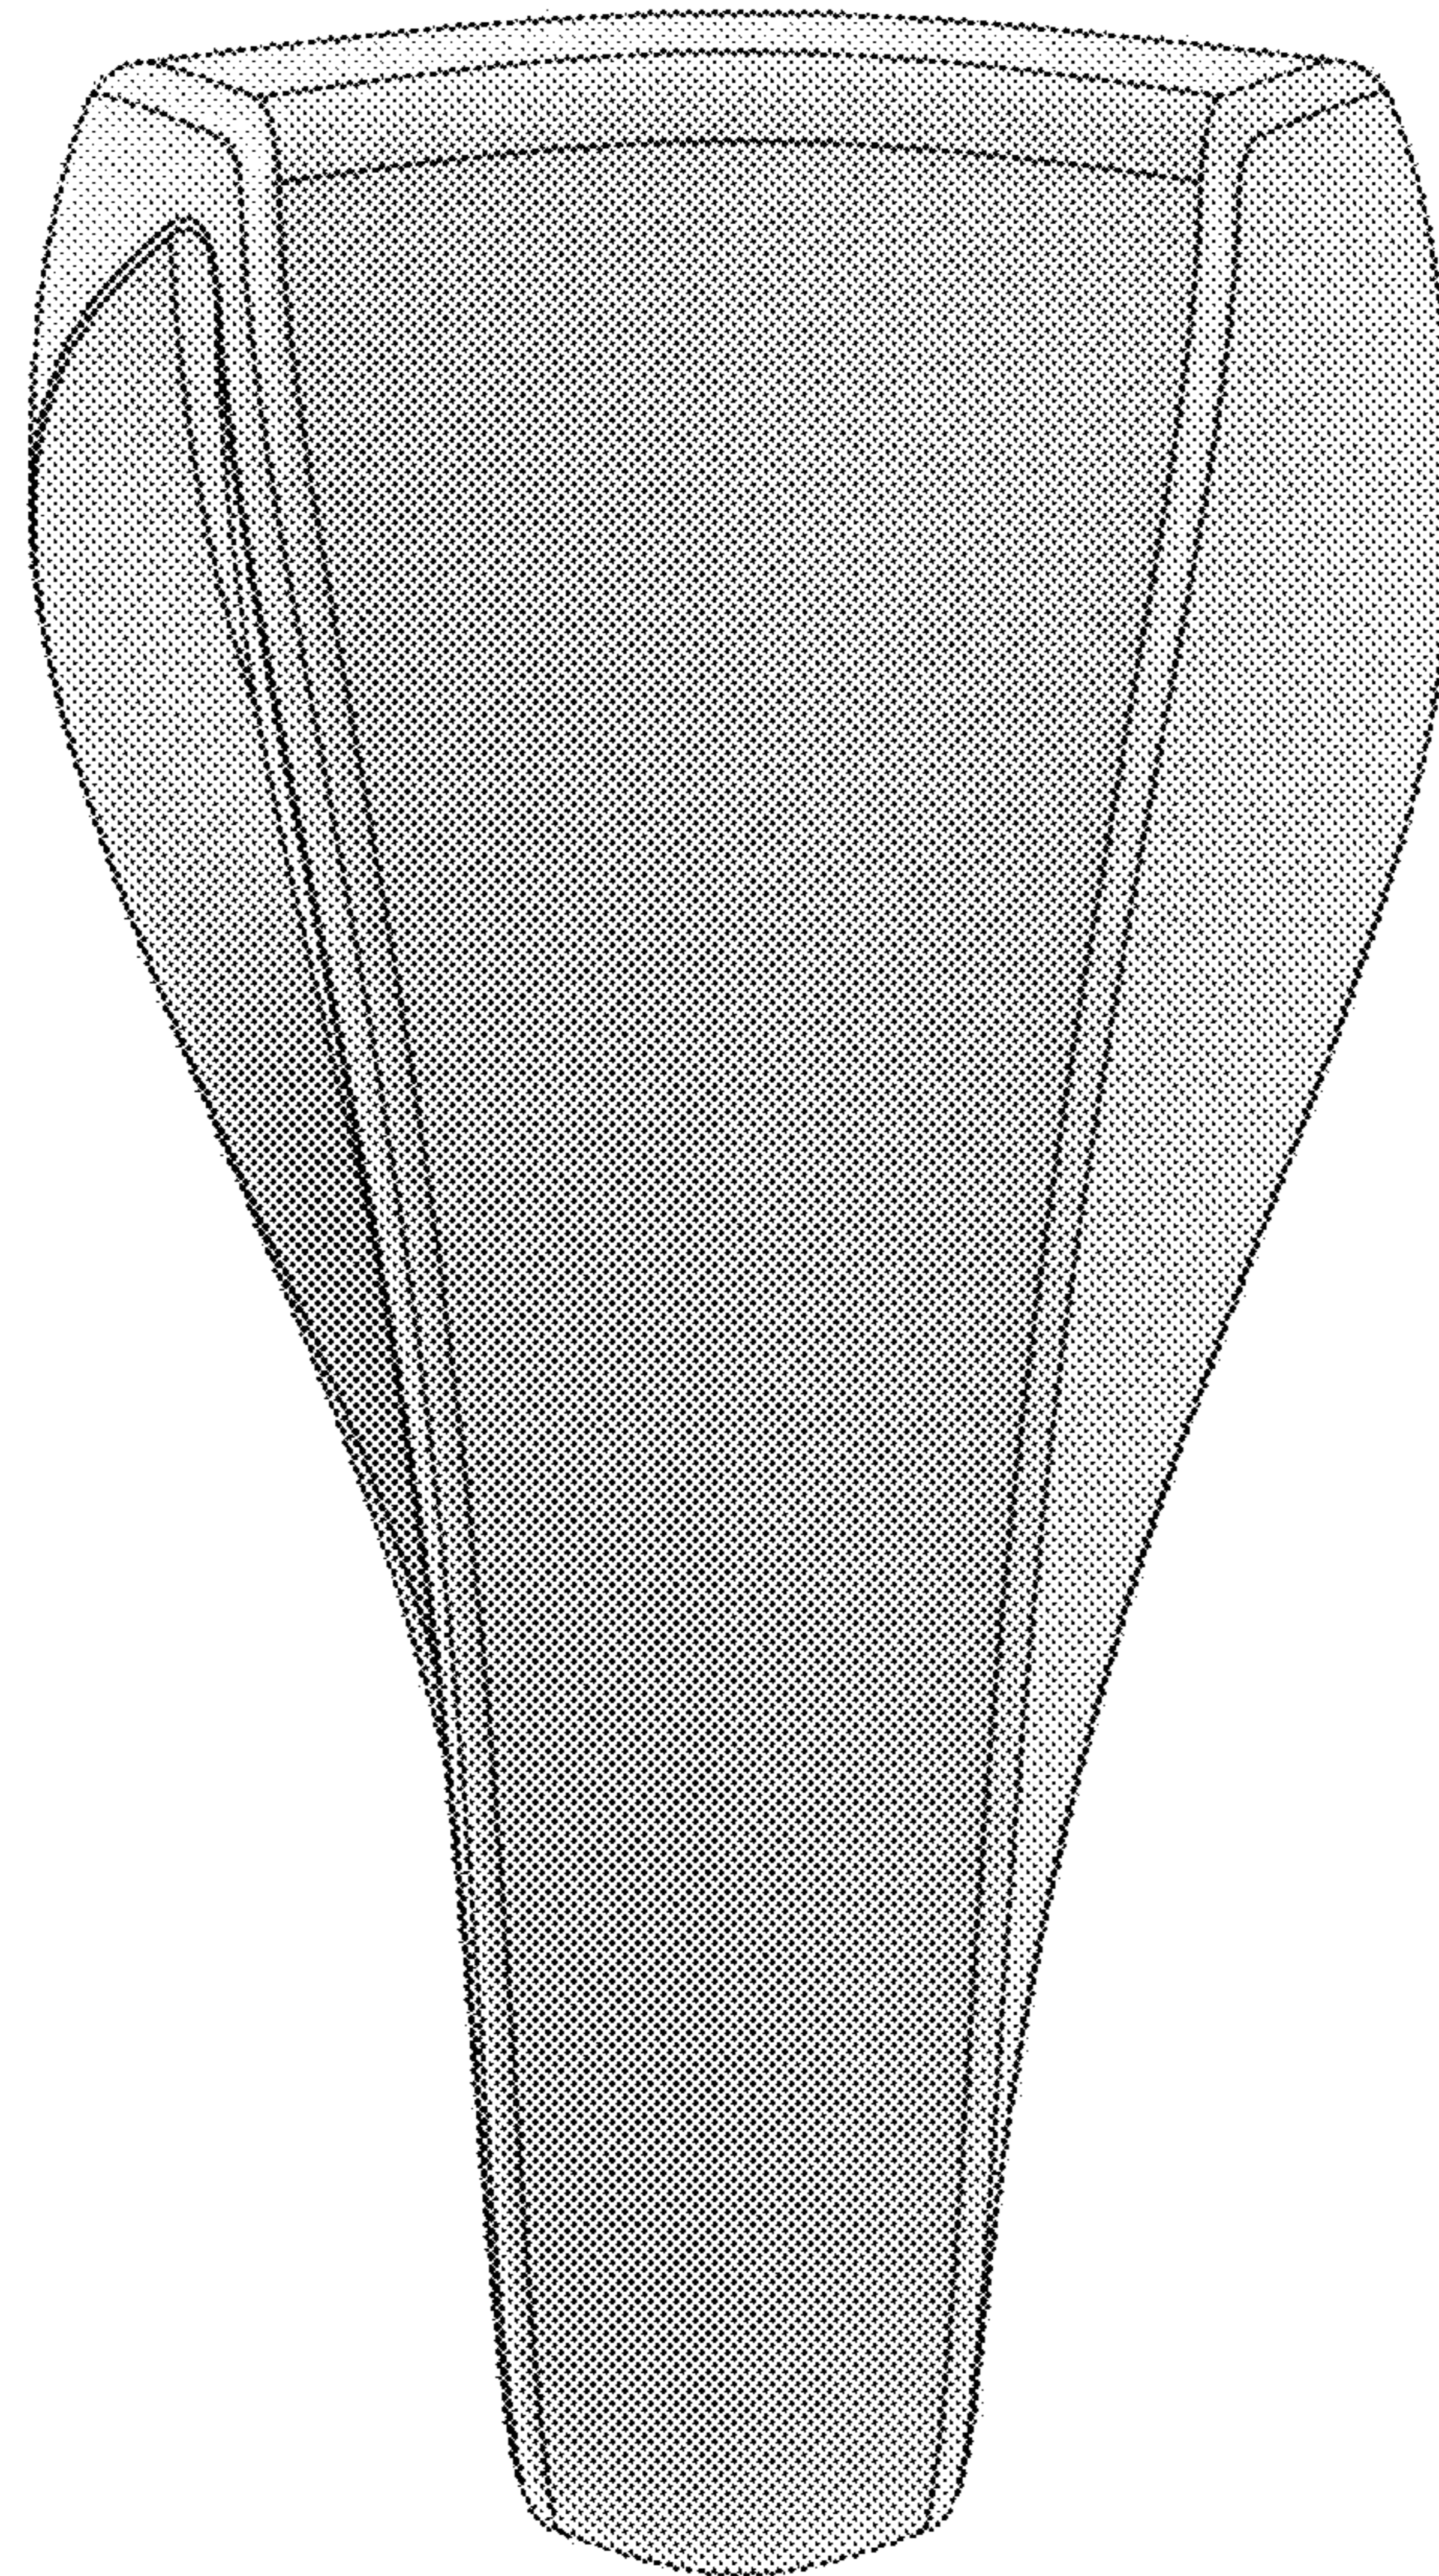


FIG. 3

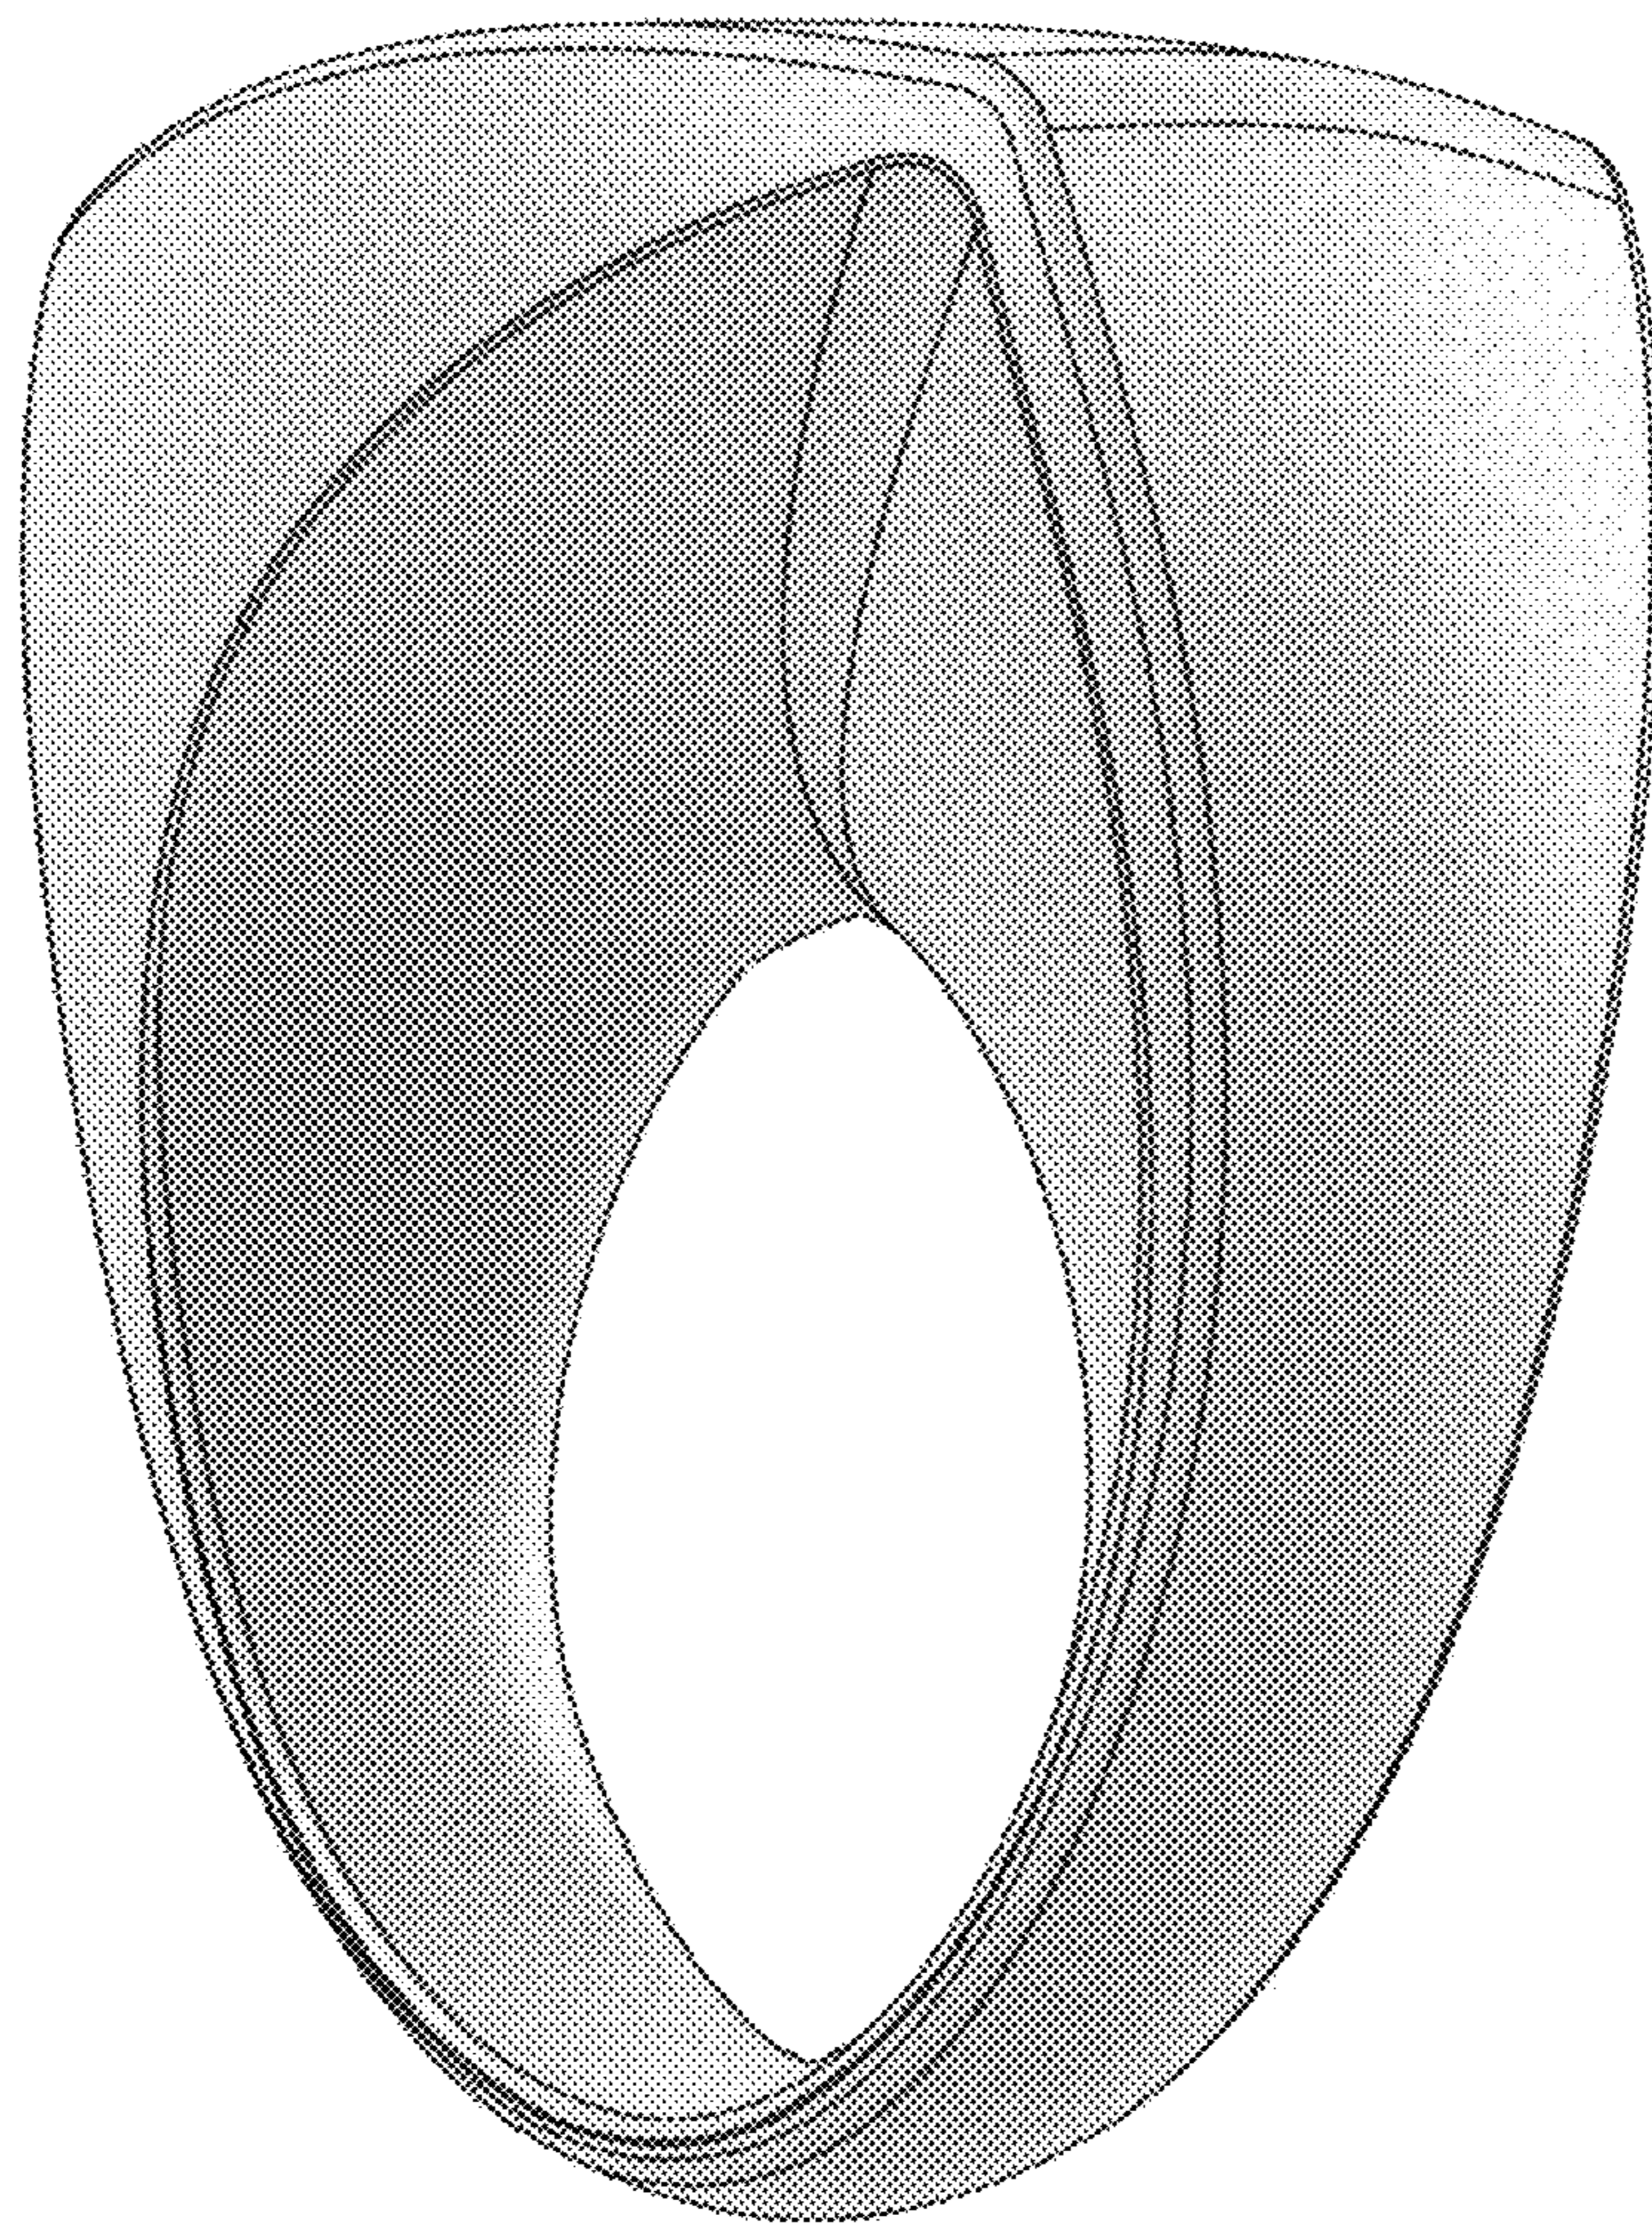


FIG. 4

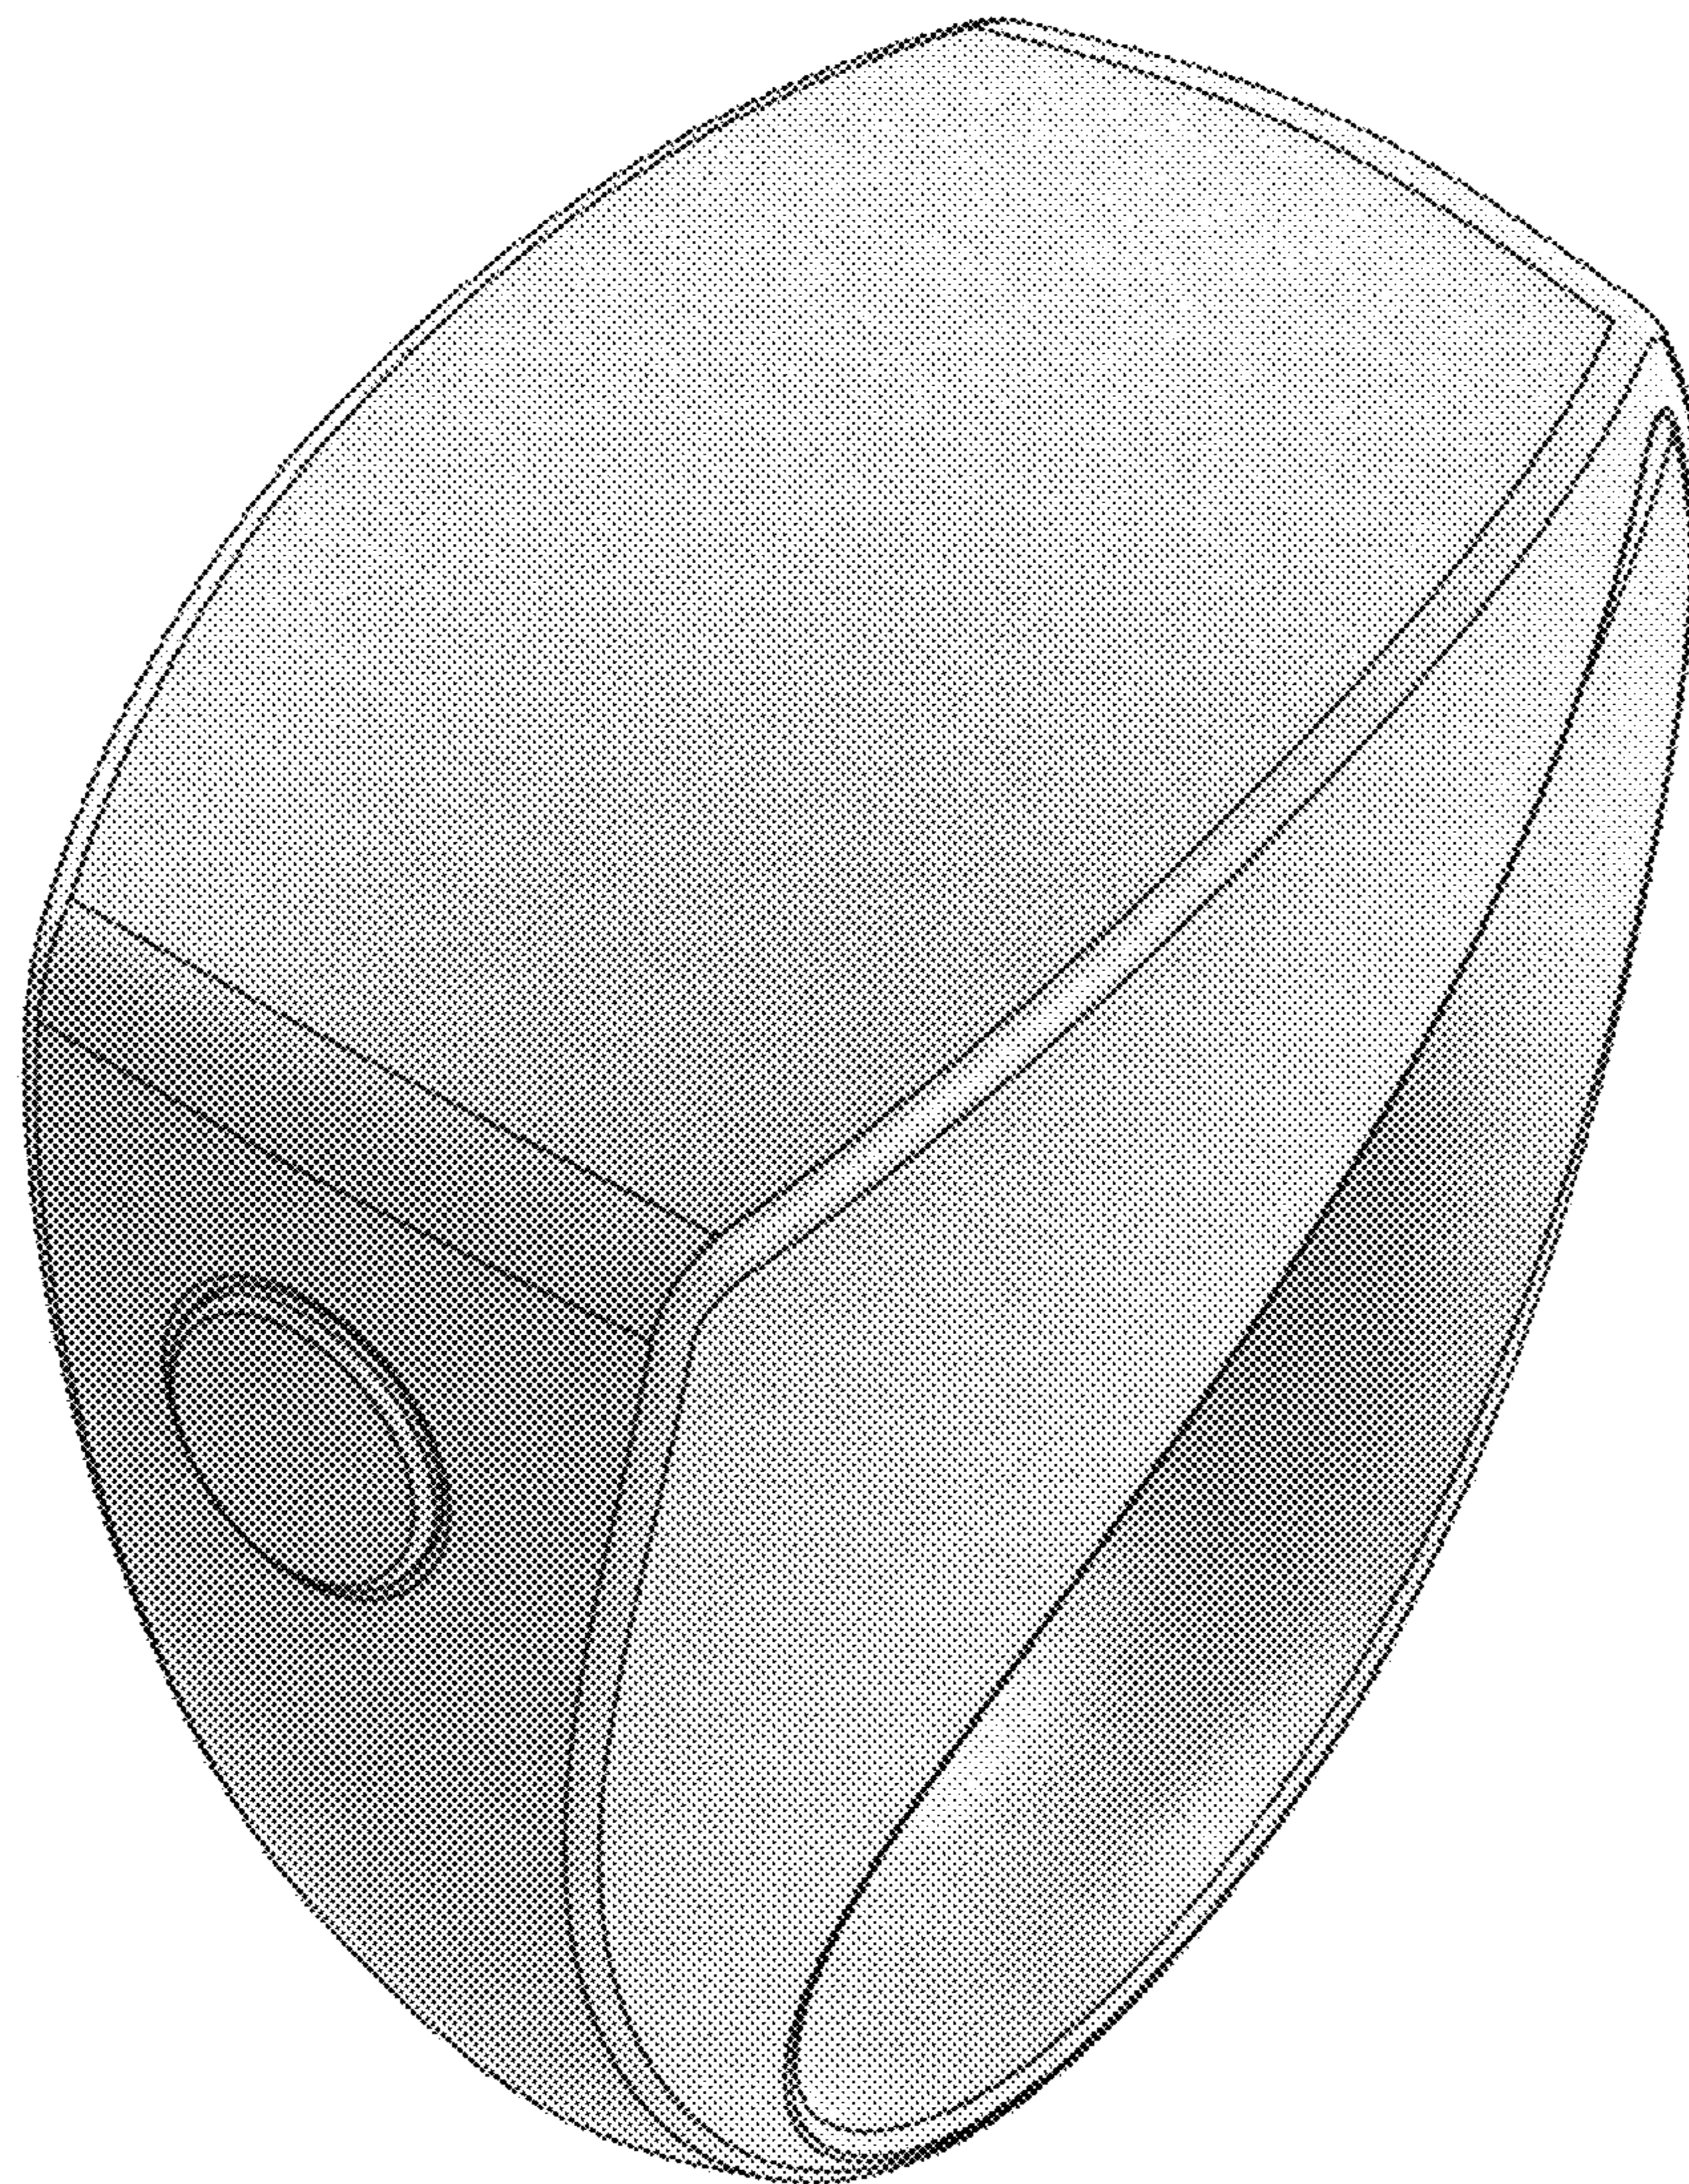


FIG. 5

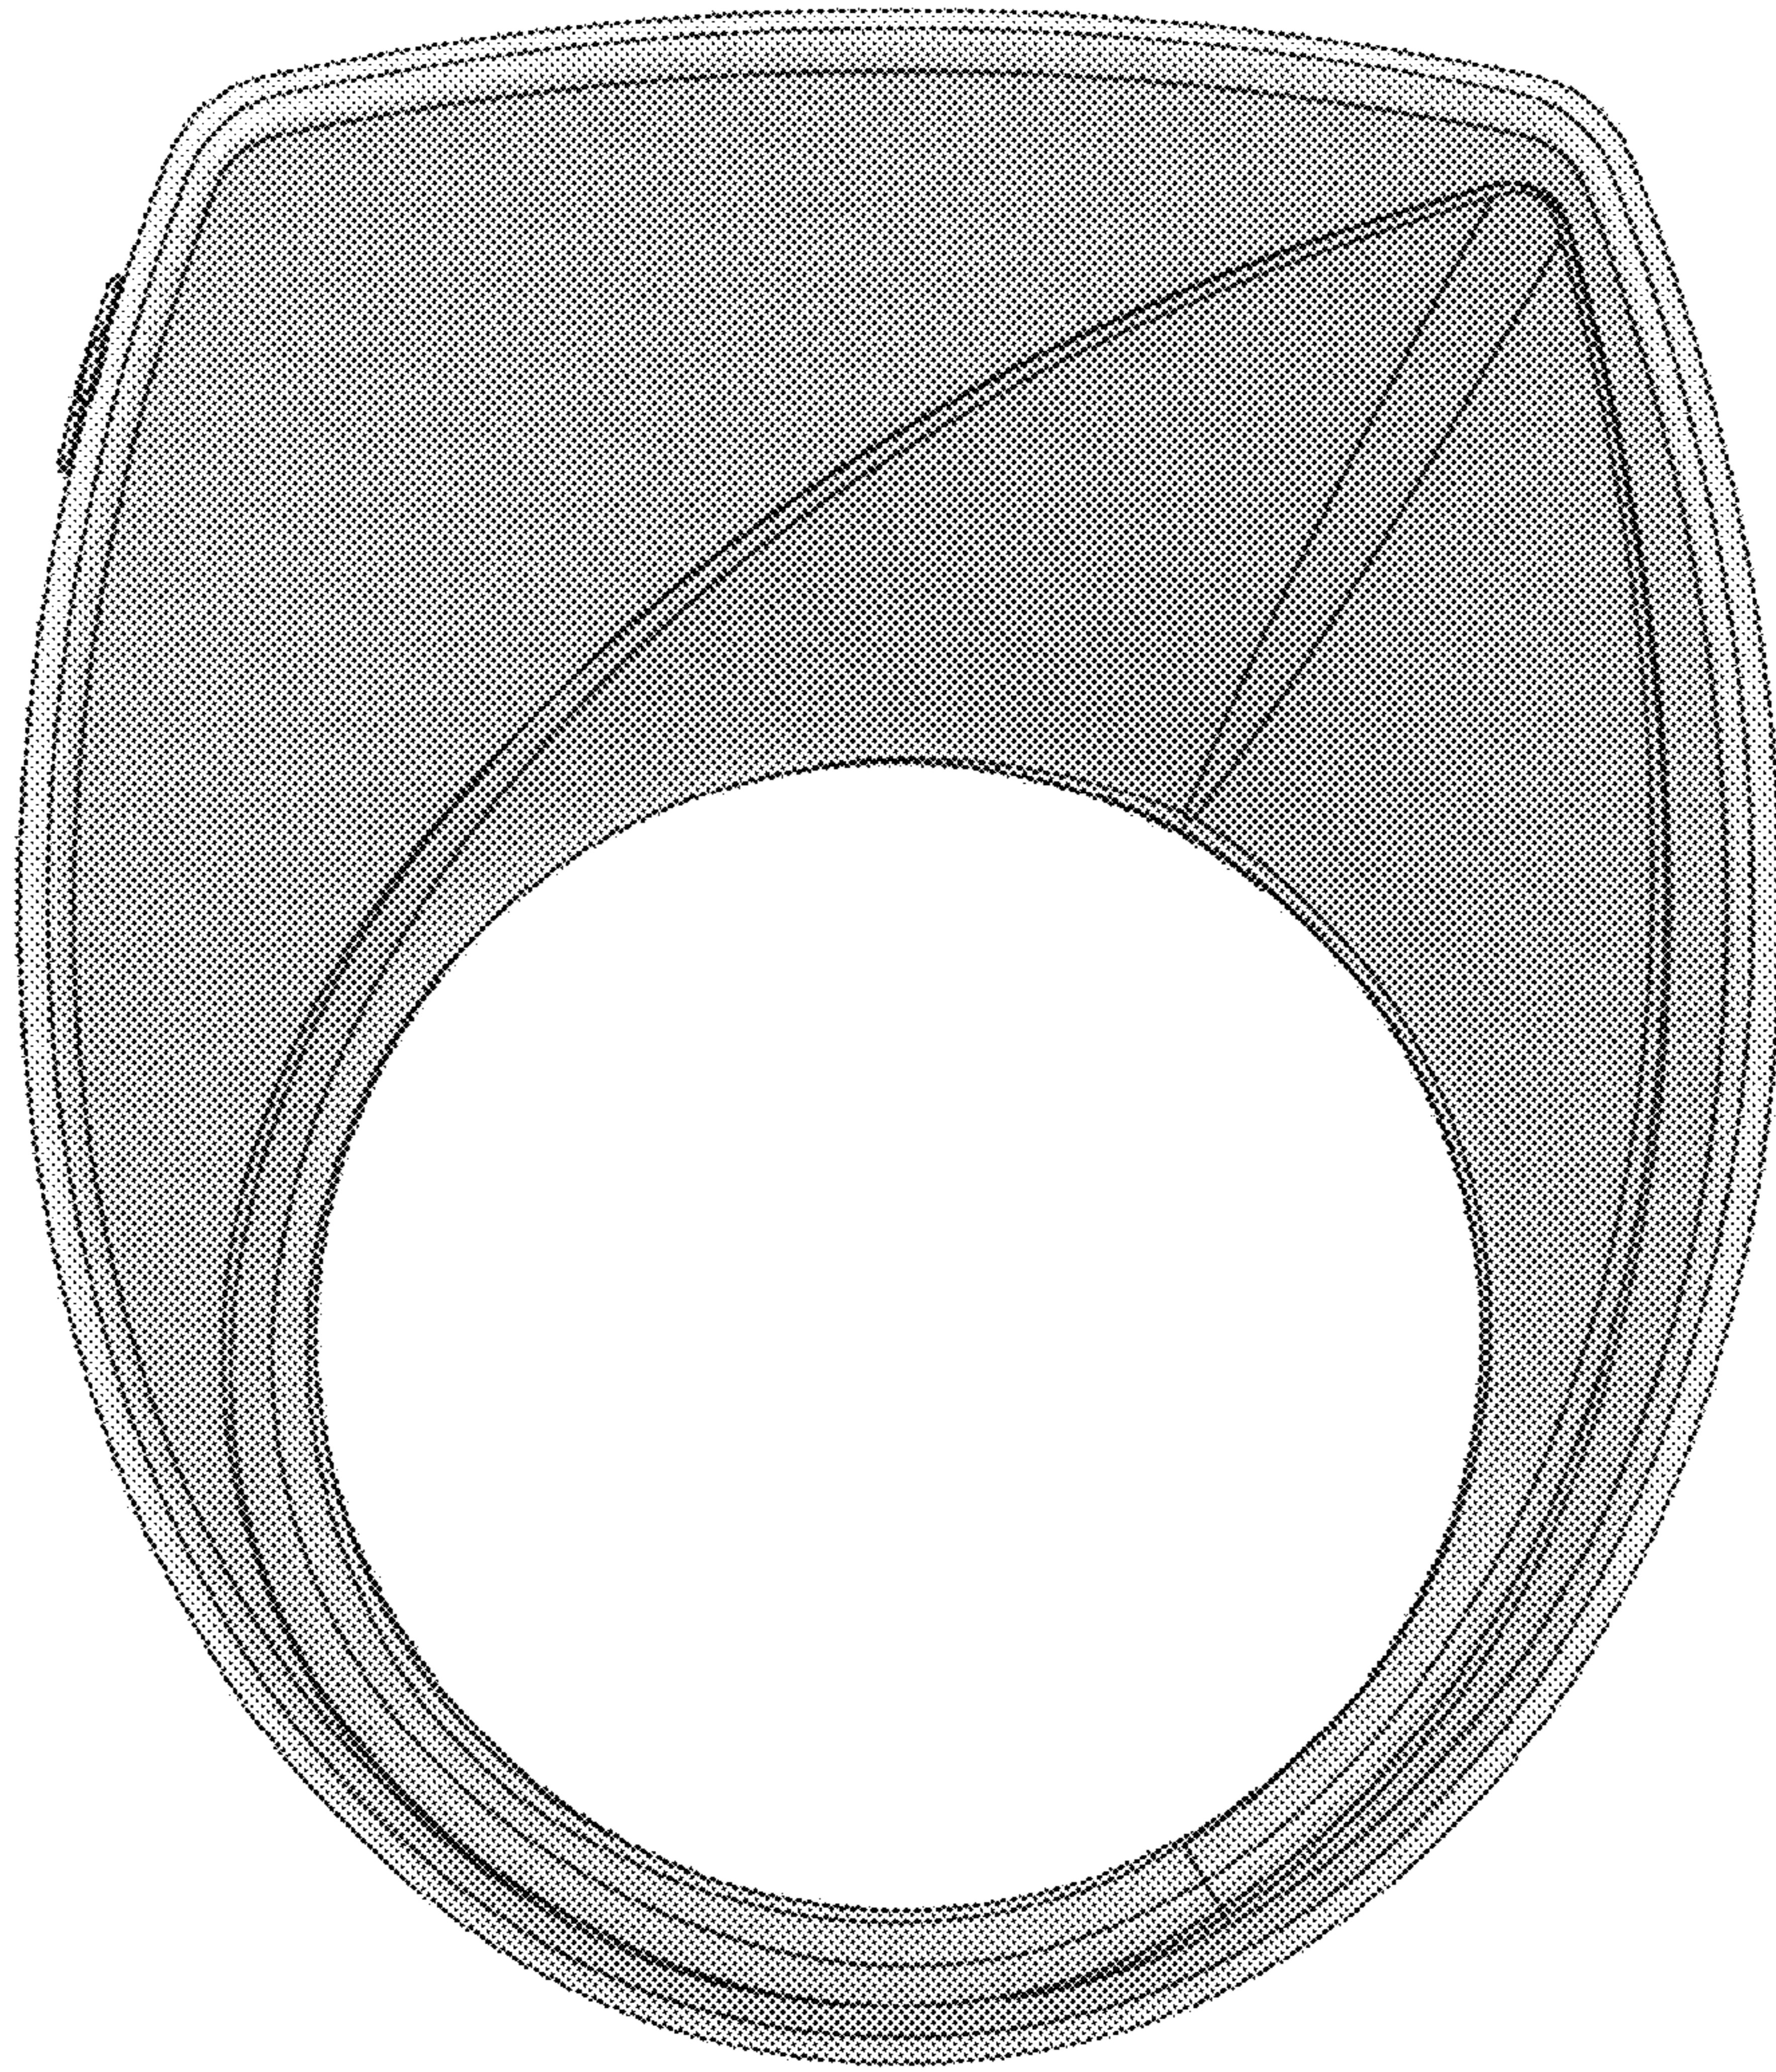


FIG. 6

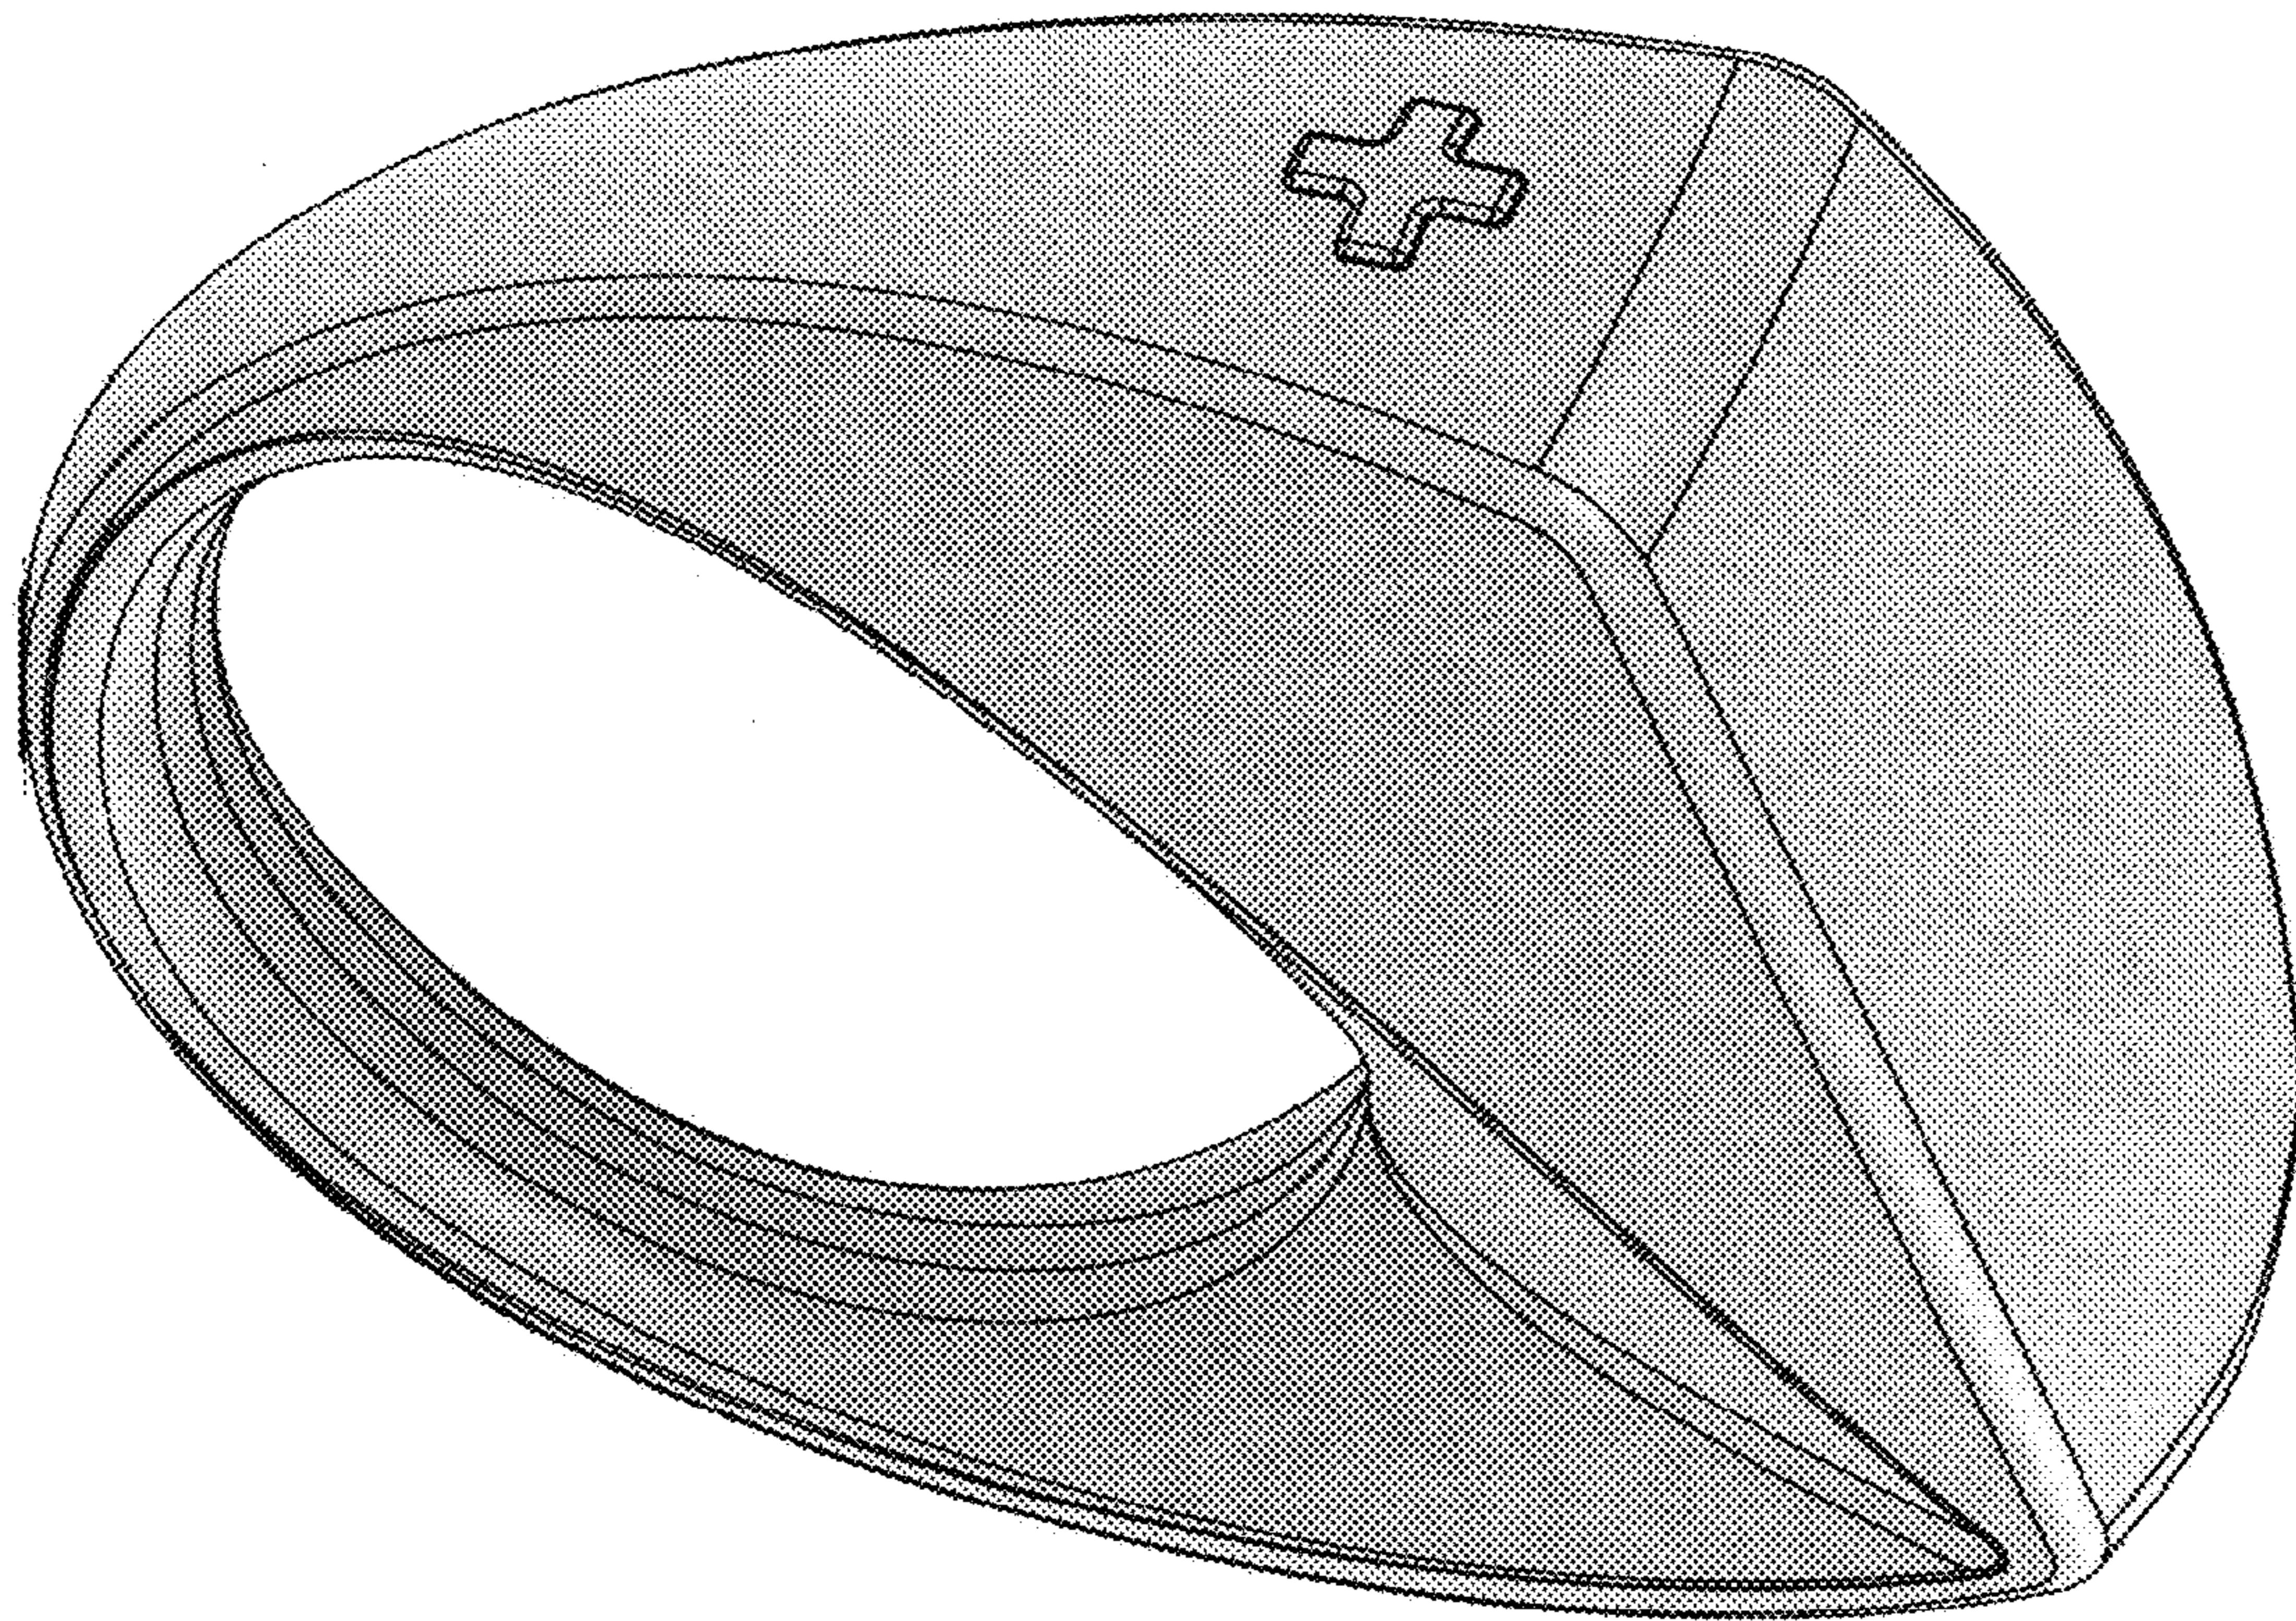


FIG. 7