



US00D706439S

(12) **United States Design Patent**  
**Hahr et al.**

(10) **Patent No.:** **US D706,439 S**  
(45) **Date of Patent:** **\*\* Jun. 3, 2014**

(54) **STIMULATION DEVICE**

D653,349 S \* 1/2012 Chong et al. .... D24/215

(71) Applicant: **Senses Toys Intellectual Property Management UG**, Bielefeld (DE)

\* cited by examiner

(72) Inventors: **Meike Hahr**, Hamburg (DE); **Heiko Tullney**, Hamburg (DE); **Till Muhl**, Hamburg (DE); **Thomas Milewski**, Halstenbek (DE)

*Primary Examiner* — Sandra Snapp

(74) *Attorney, Agent, or Firm* — Merek, Blackmon & Voorhees, LLC

(73) Assignee: **Ovo Joint Venture LLC**, Pembroke Park, FL (US)

(57) **CLAIM**

The ornamental design for a stimulation device, as shown and described.

(\*\*) Term: **14 Years**

**DESCRIPTION**

(21) Appl. No.: **29/447,966**

FIG. 1 is a perspective view taken from the front and left side of a stimulation device showing the design, the opposite side being a mirror image thereof;

(22) Filed: **Mar. 8, 2013**

FIG. 2 is rear elevation view of the stimulation device of FIG. 1;

(30) **Foreign Application Priority Data**

Sep. 10, 2012 (EM) ..... 001342935-0076

FIG. 3 is a left side elevation view of the stimulation device of FIG. 1, the right side elevation view being a mirror image thereof;

(51) **LOC (10) Cl.** ..... **28-03**

FIG. 4 is a perspective view taken from the front and top of the stimulation device of FIG. 1;

(52) **U.S. Cl.**  
USPC ..... **D24/215**

FIG. 5 is a front elevation view of the stimulation device of FIG. 1; and,

(58) **Field of Classification Search**  
USPC ..... D24/200, 211, 212, 213, 214, 215;  
601/114, 120, 121, 124, 125, 130, 131,  
601/134, 135, 136, 137

FIG. 6 is a perspective view taken from the rear and left side of the stimulation device of FIG. 1, the opposite side being a mirror image thereof.

See application file for complete search history.

A perspective view taken from the front and right side of the stimulation device of FIG. 1 at an angle corresponding to the angle of the perspective view of FIG. 1 is a mirror image of FIG. 1.

(56) **References Cited**


**U.S. PATENT DOCUMENTS**

D212,145 S *	8/1968	Madl	.....	D24/214
D291,341 S *	8/1987	Keating et al.	.....	D21/684
D350,397 S *	9/1994	Bruno et al.	.....	D24/214
D581,542 S *	11/2008	Ferber et al.	.....	D24/215
D612,552 S *	3/2010	Matz	.....	D30/160
D648,861 S *	11/2011	Chong et al.	.....	D24/215
D652,943 S *	1/2012	Chong et al.	.....	D24/215

The right side elevation of the stimulation device of FIG. 1 is a mirror image of the left side elevation shown in FIG. 3.

A perspective view taken from the rear and right side of the stimulation device of FIG. 1 at an angle corresponding to the angle of the perspective view of FIG. 6 is a mirror image of FIG. 6.

**1 Claim, 6 Drawing Sheets**

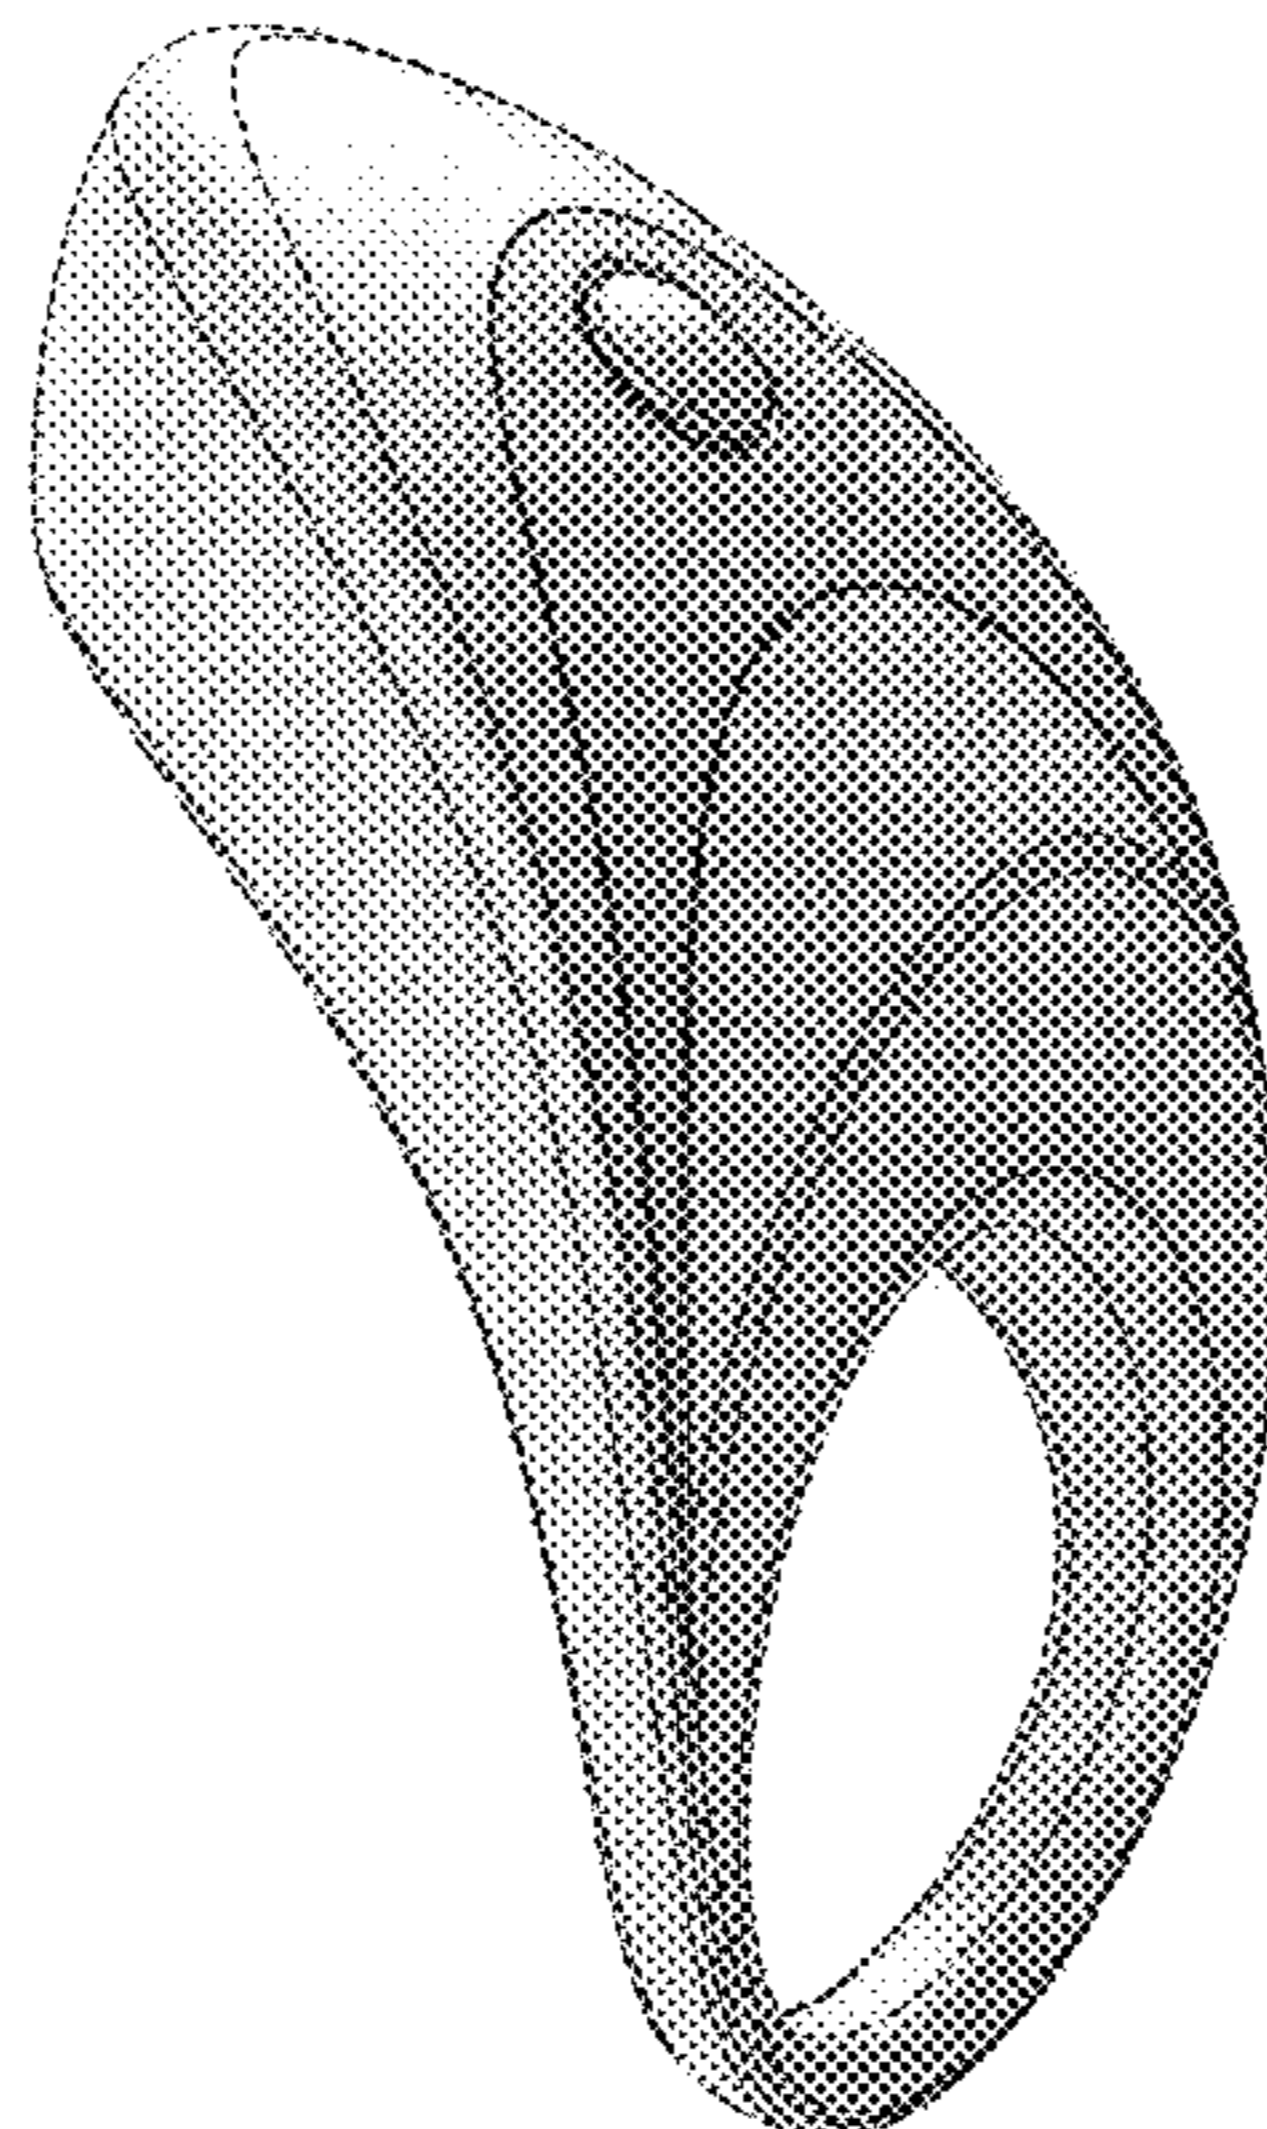

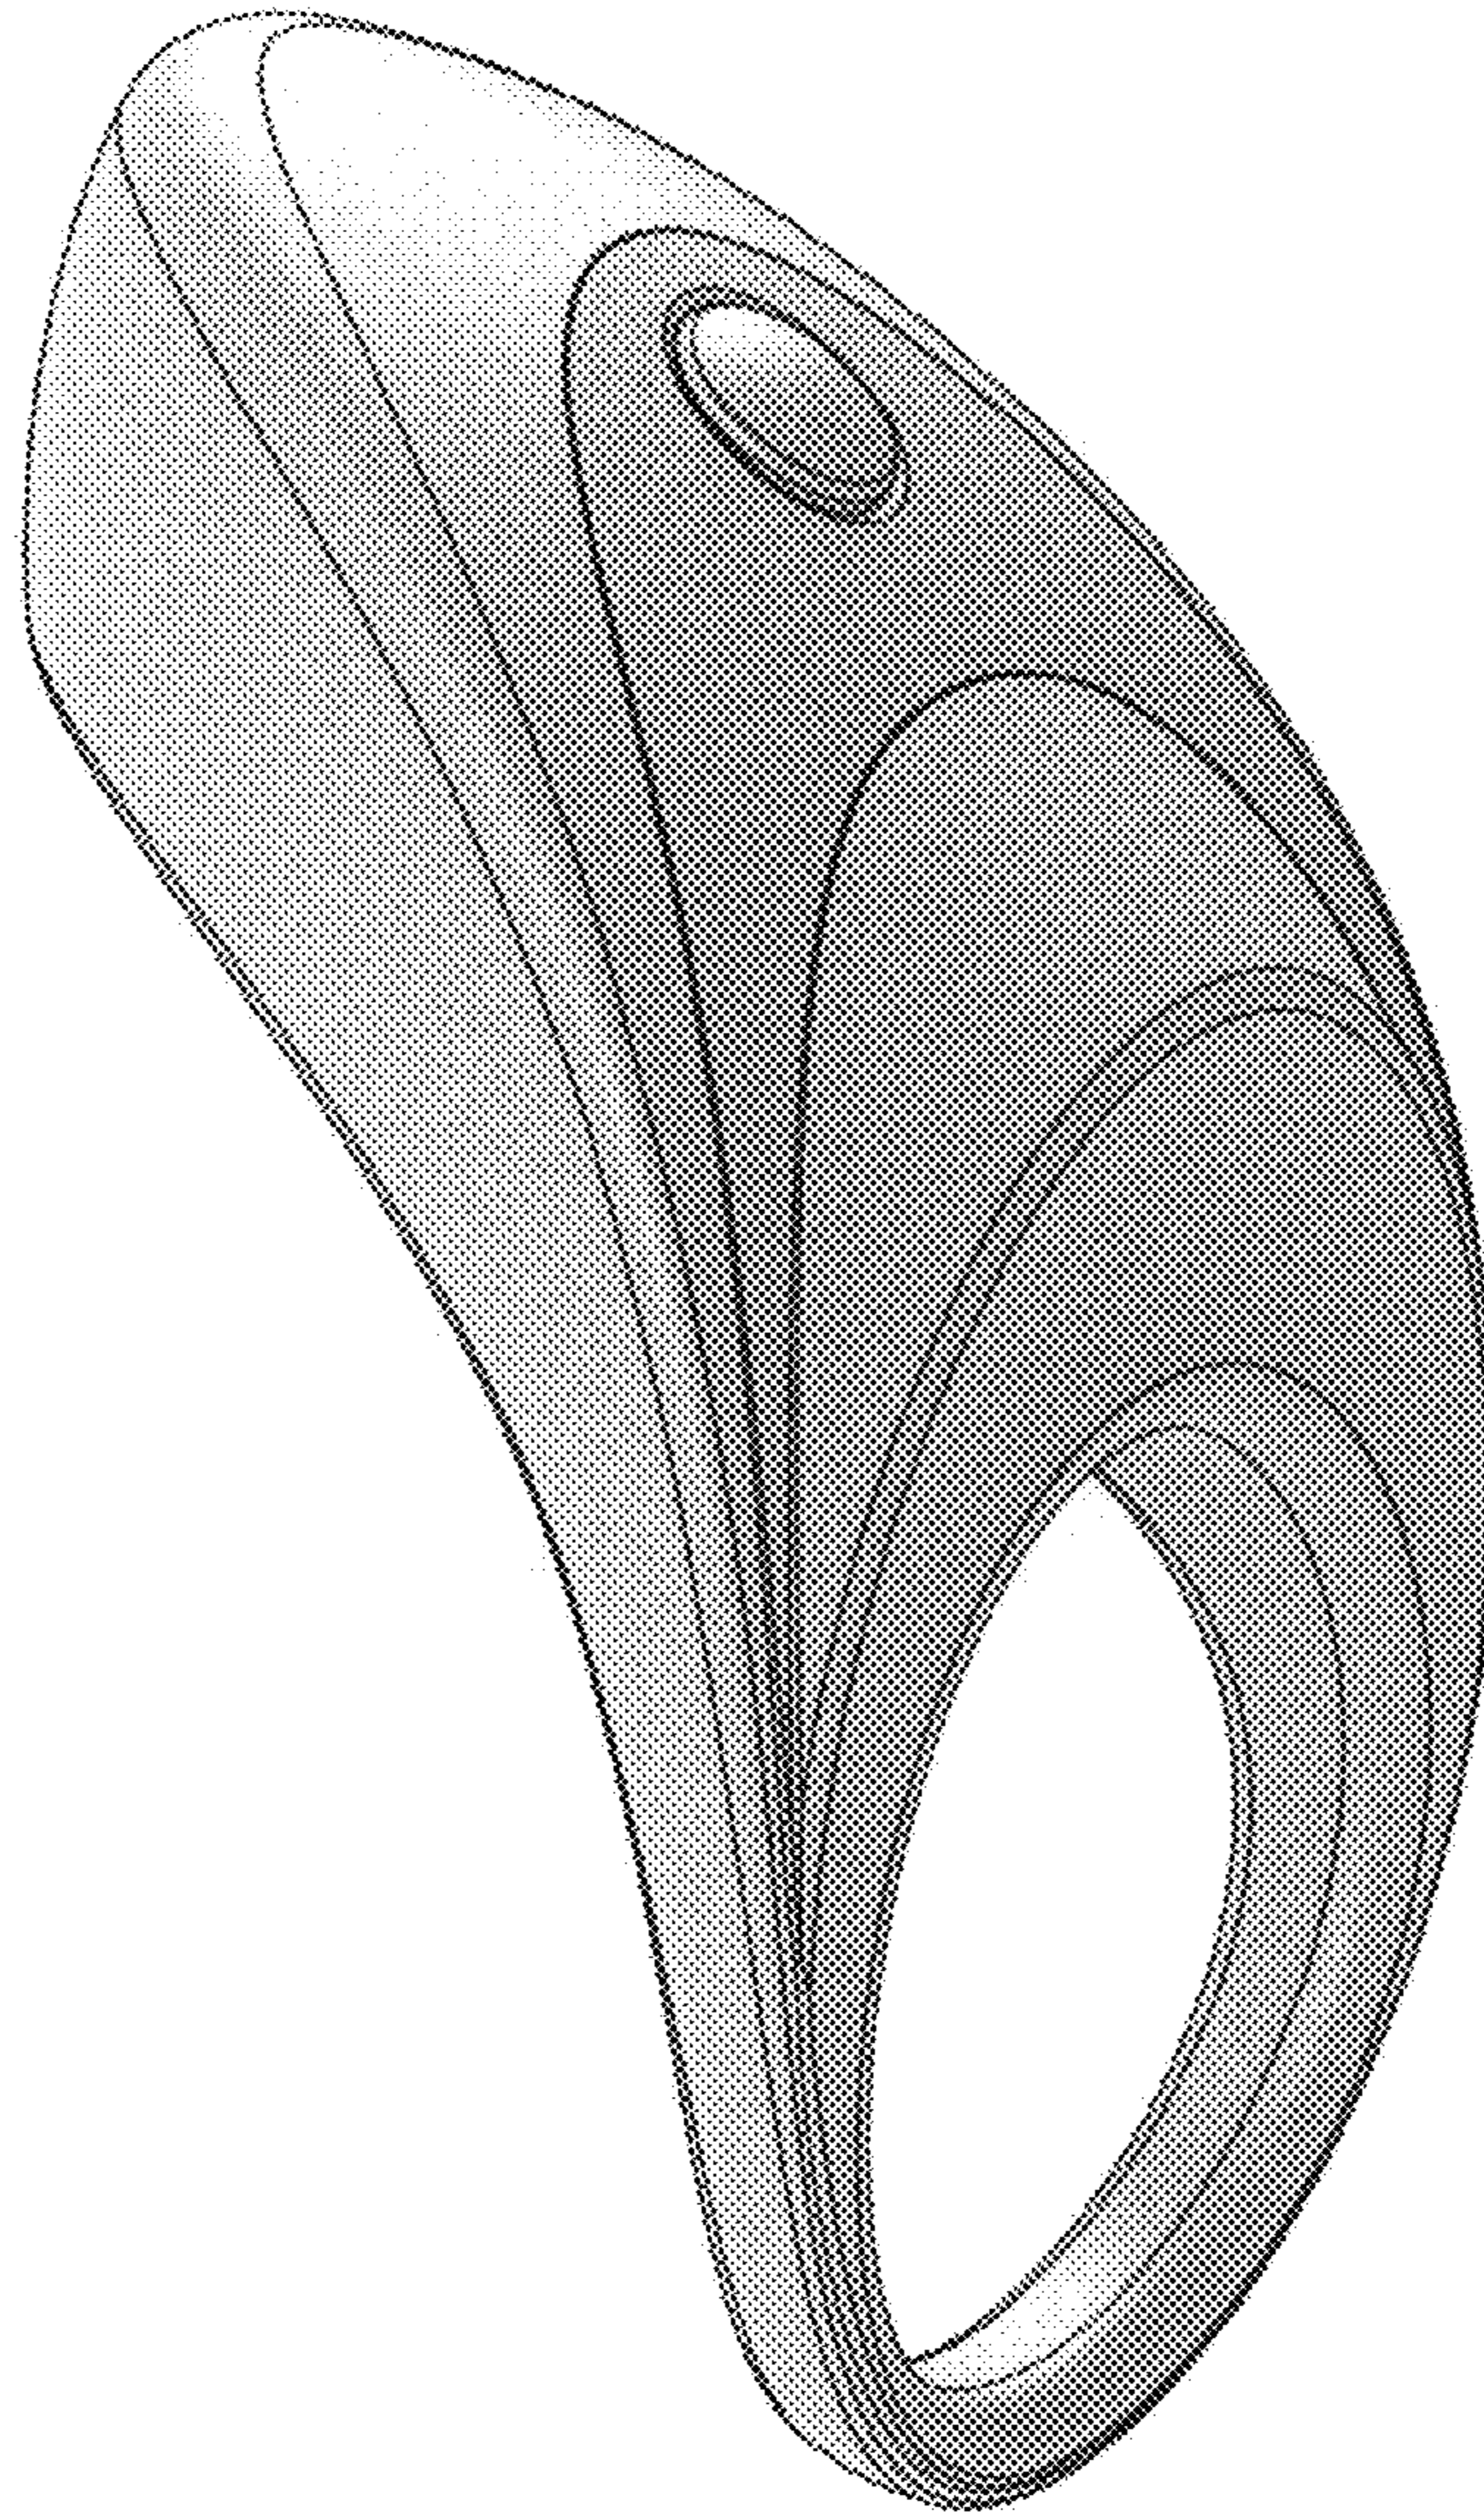


FIG. 1

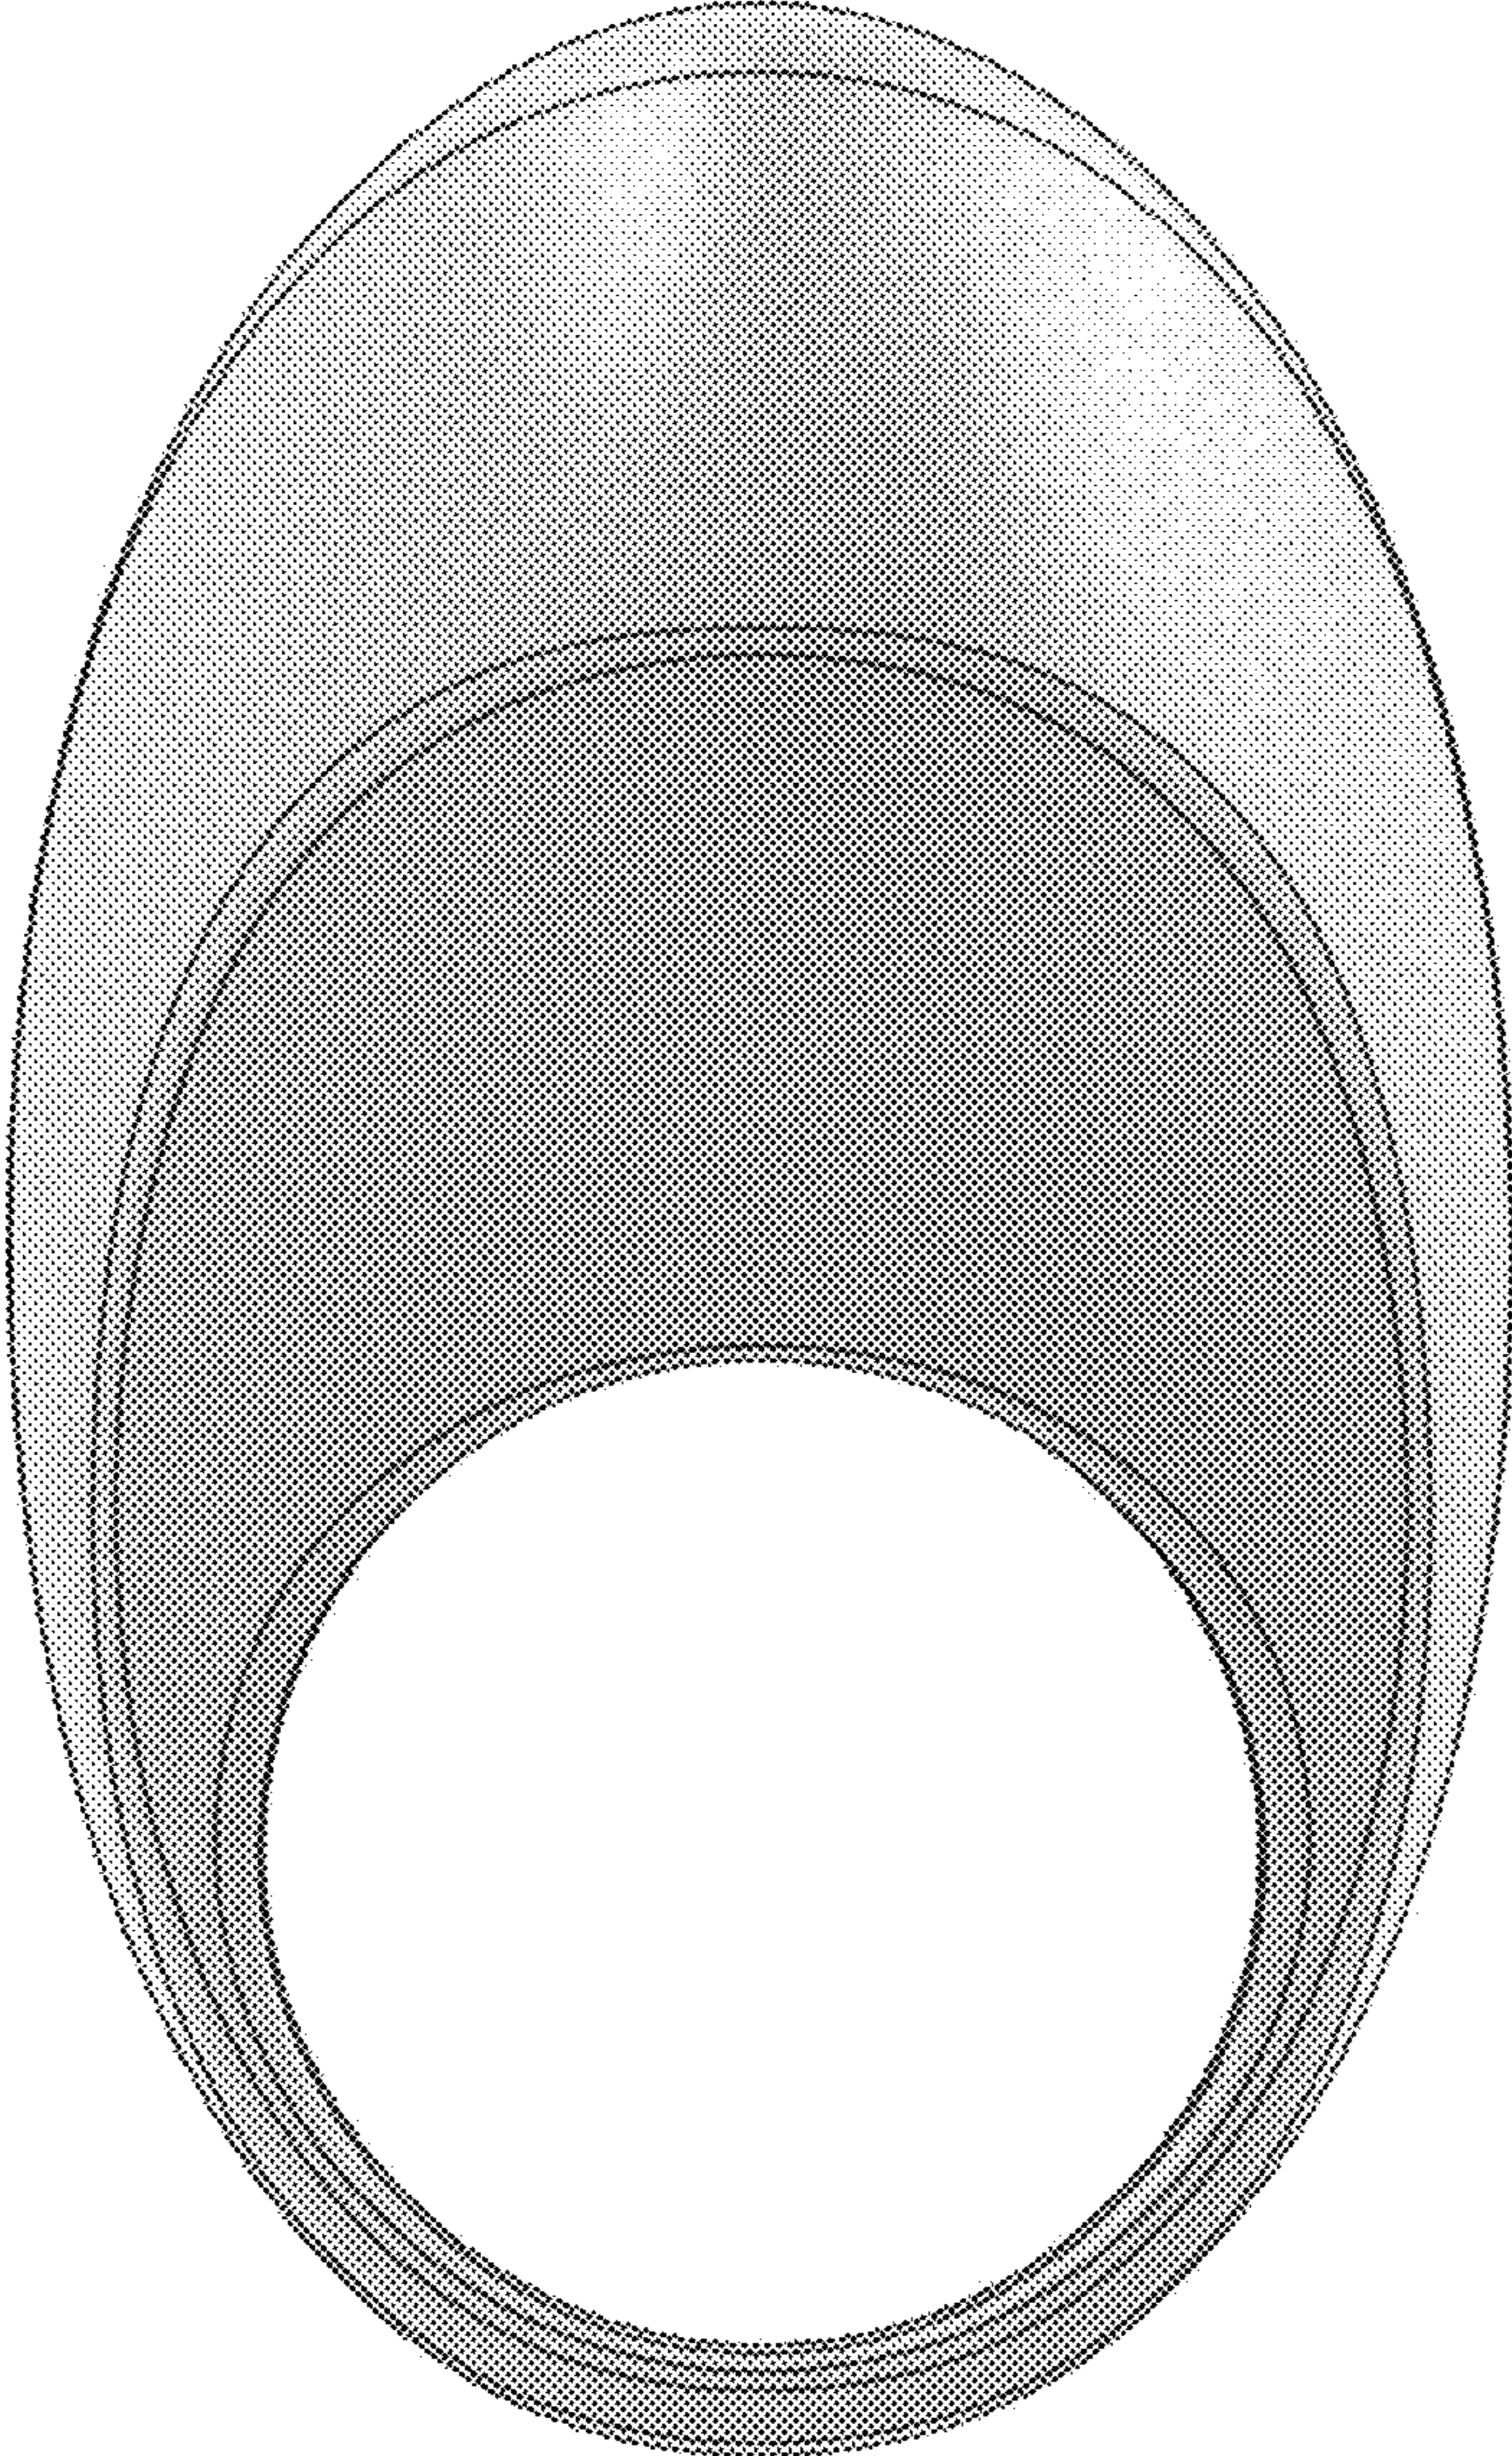


FIG. 2

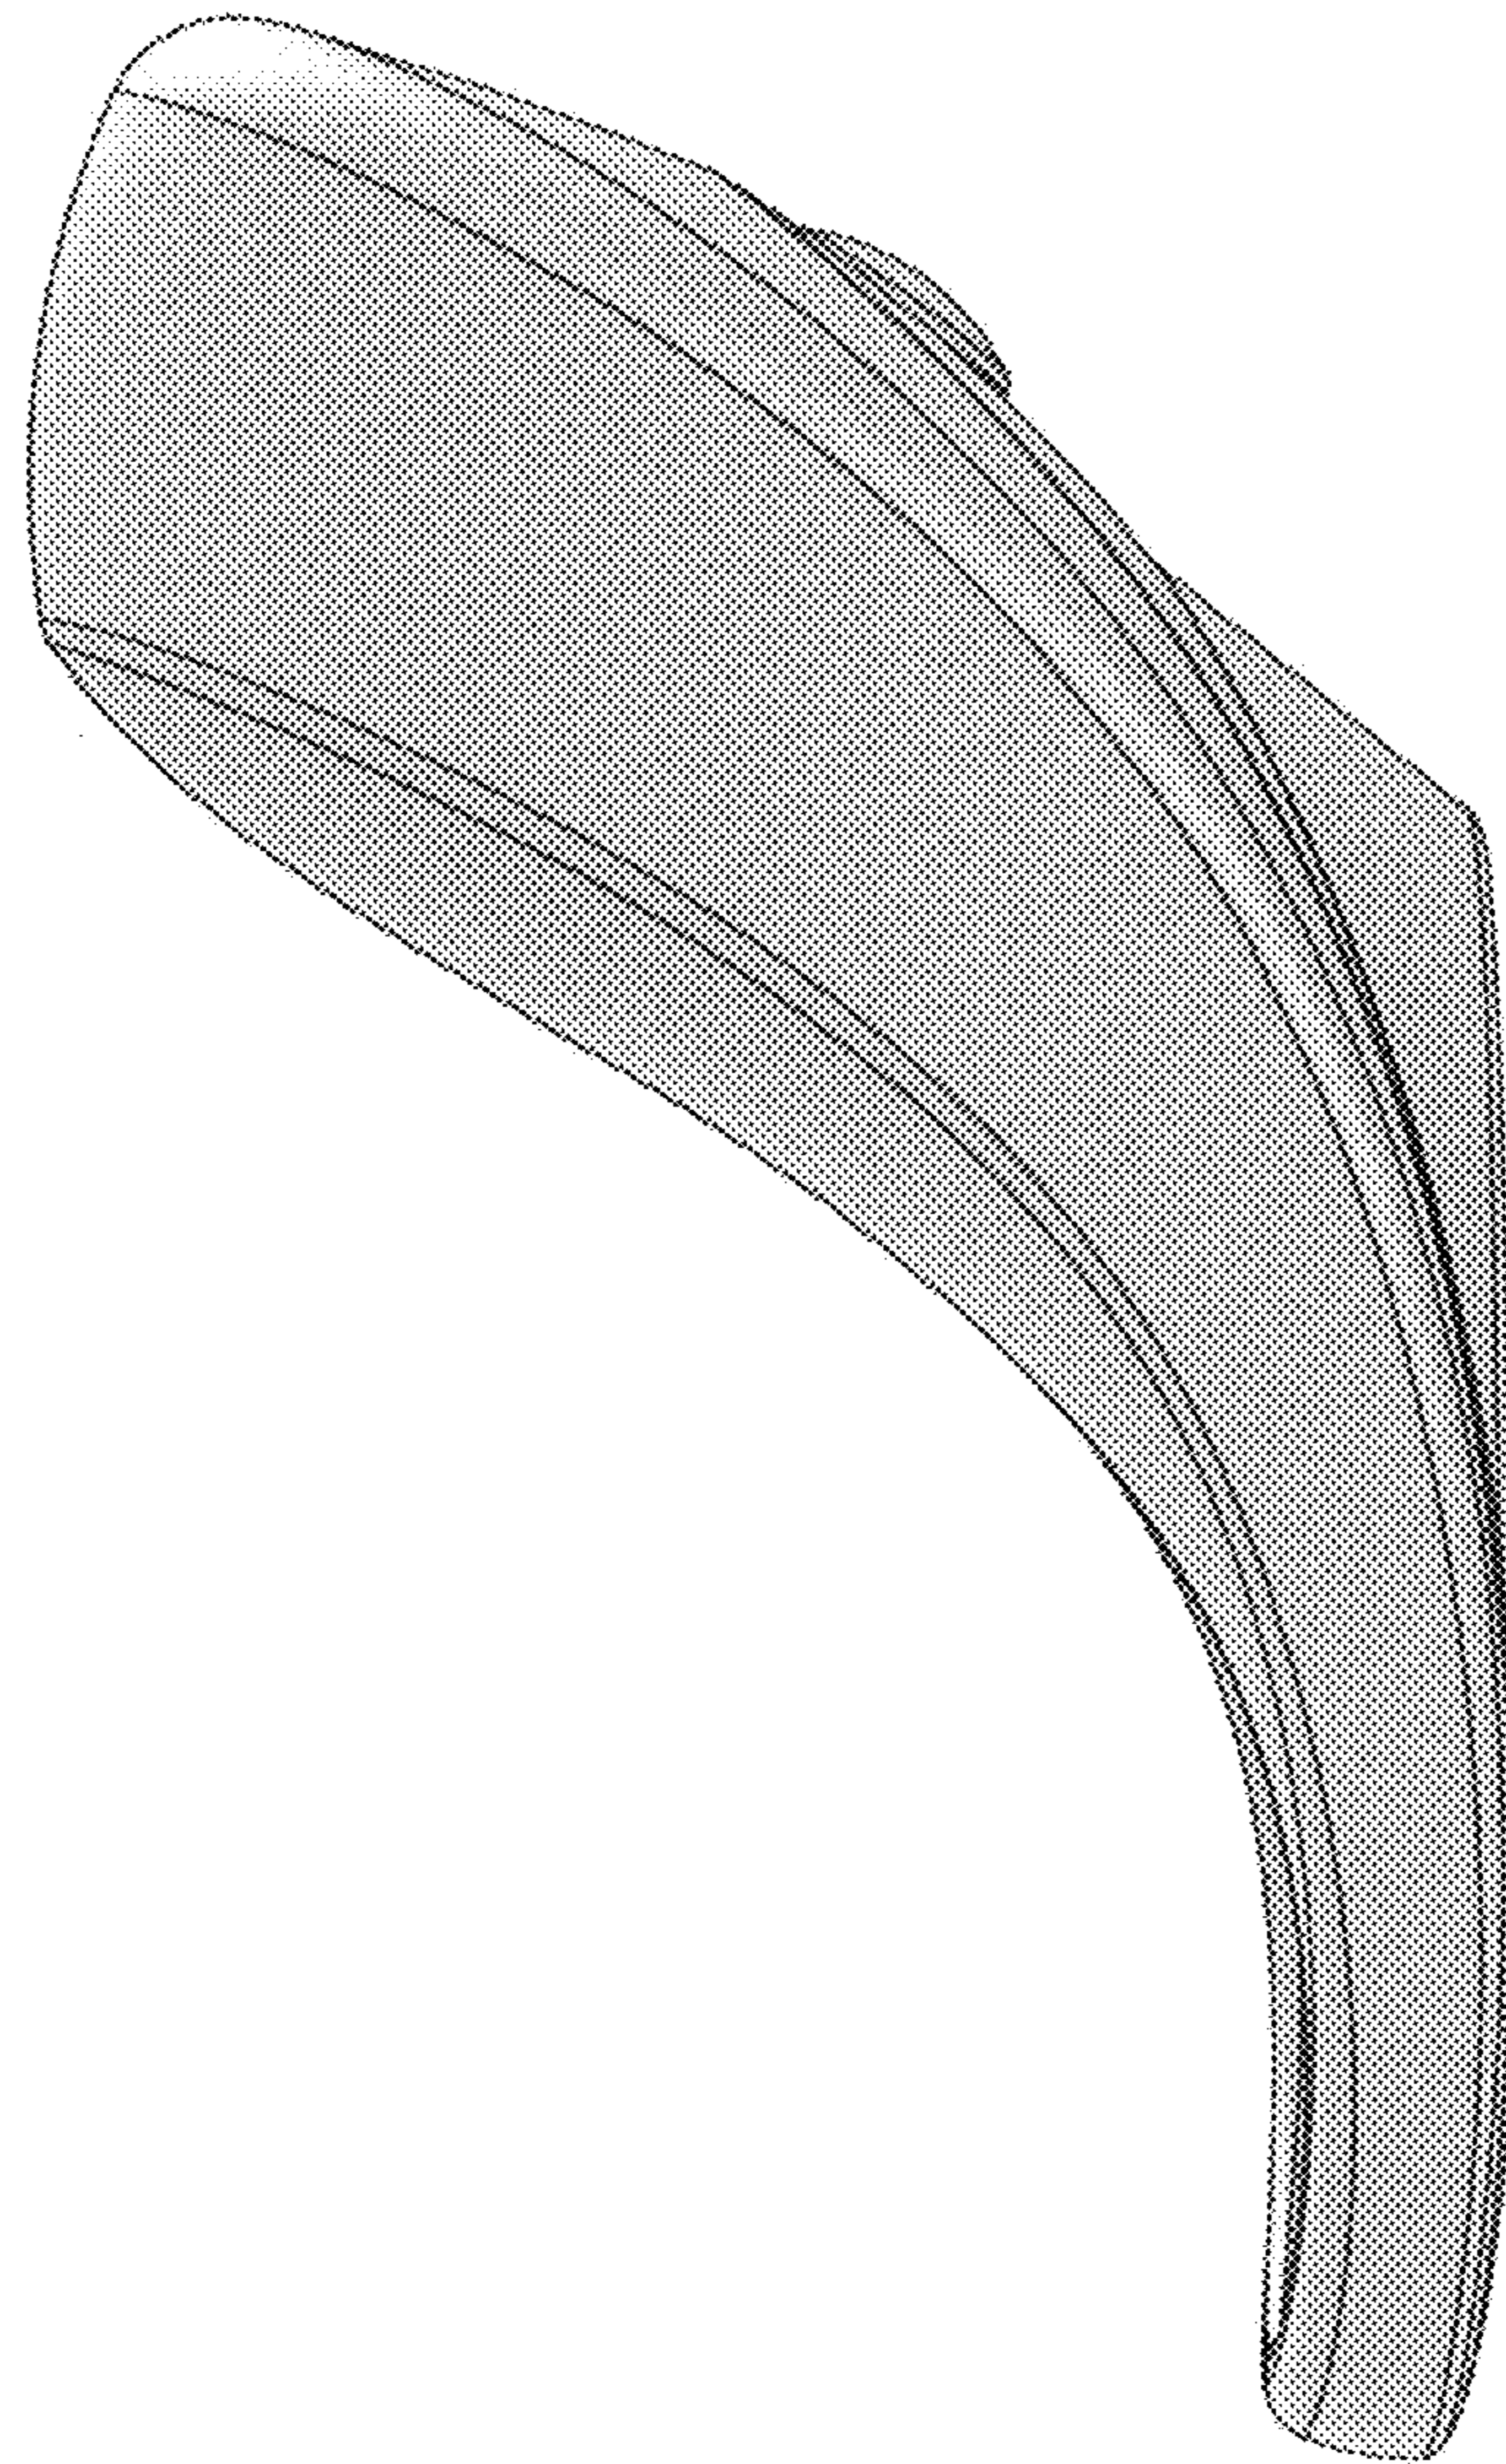


FIG. 3

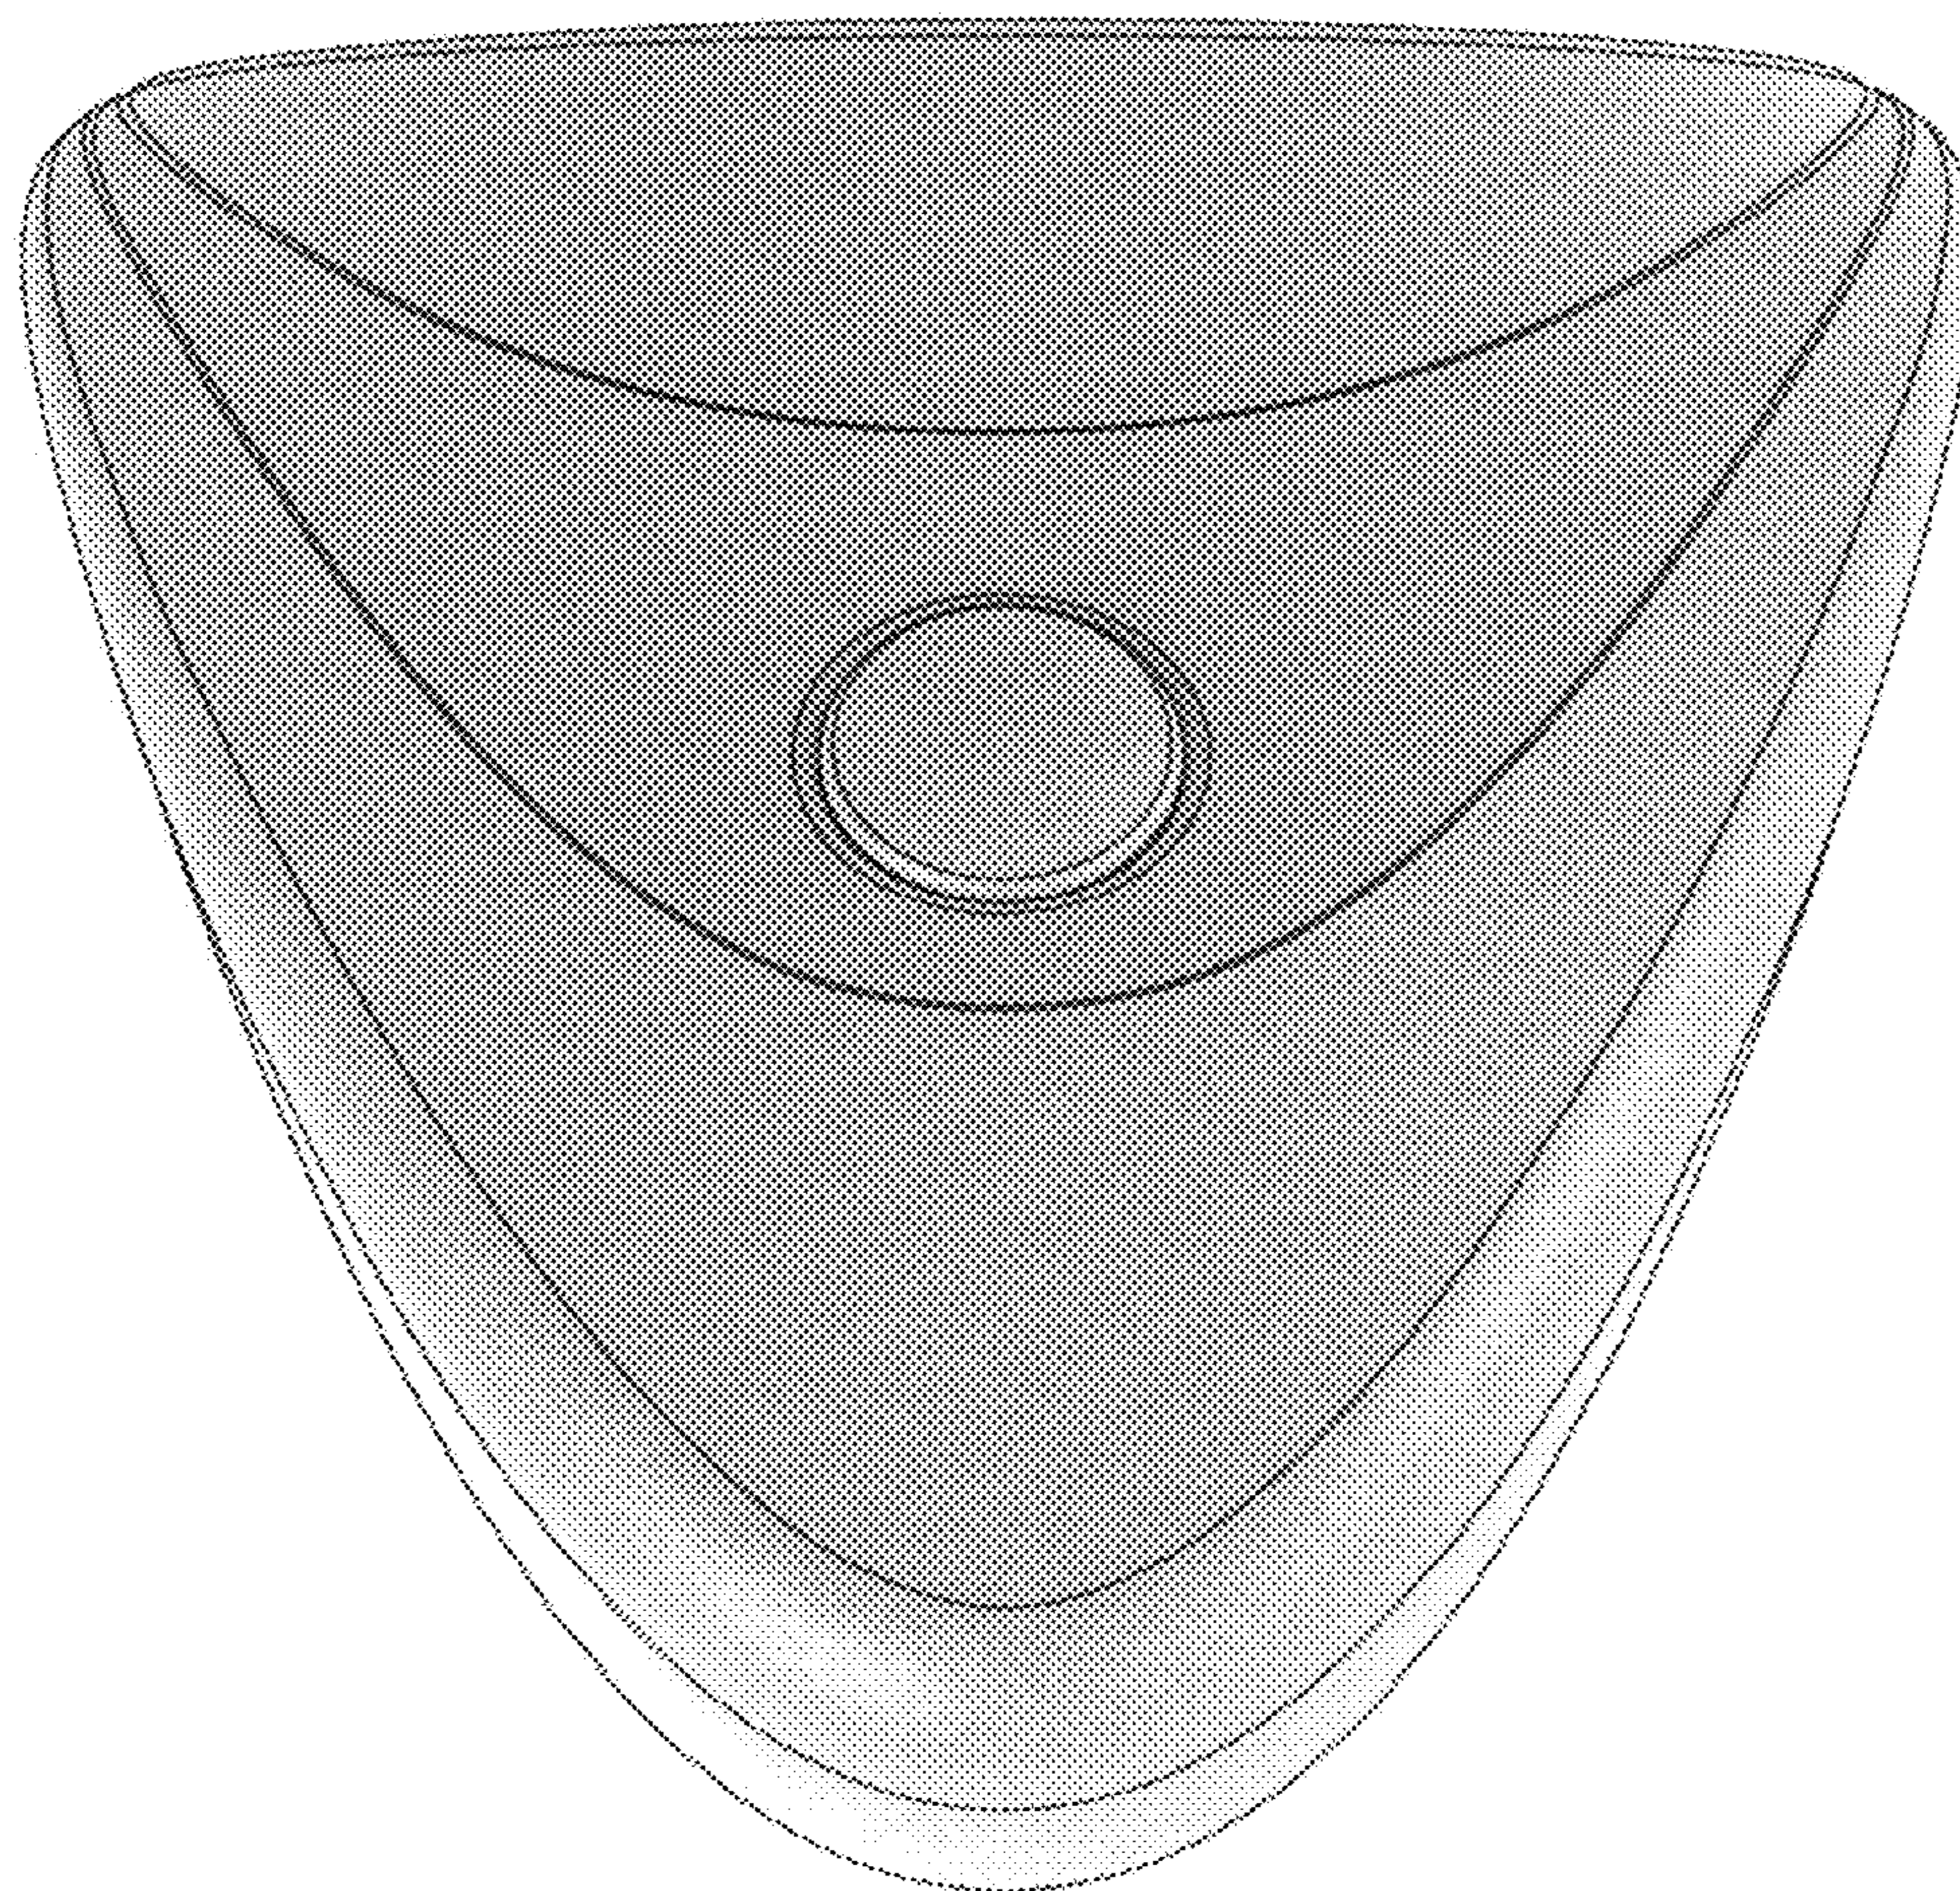


FIG. 4

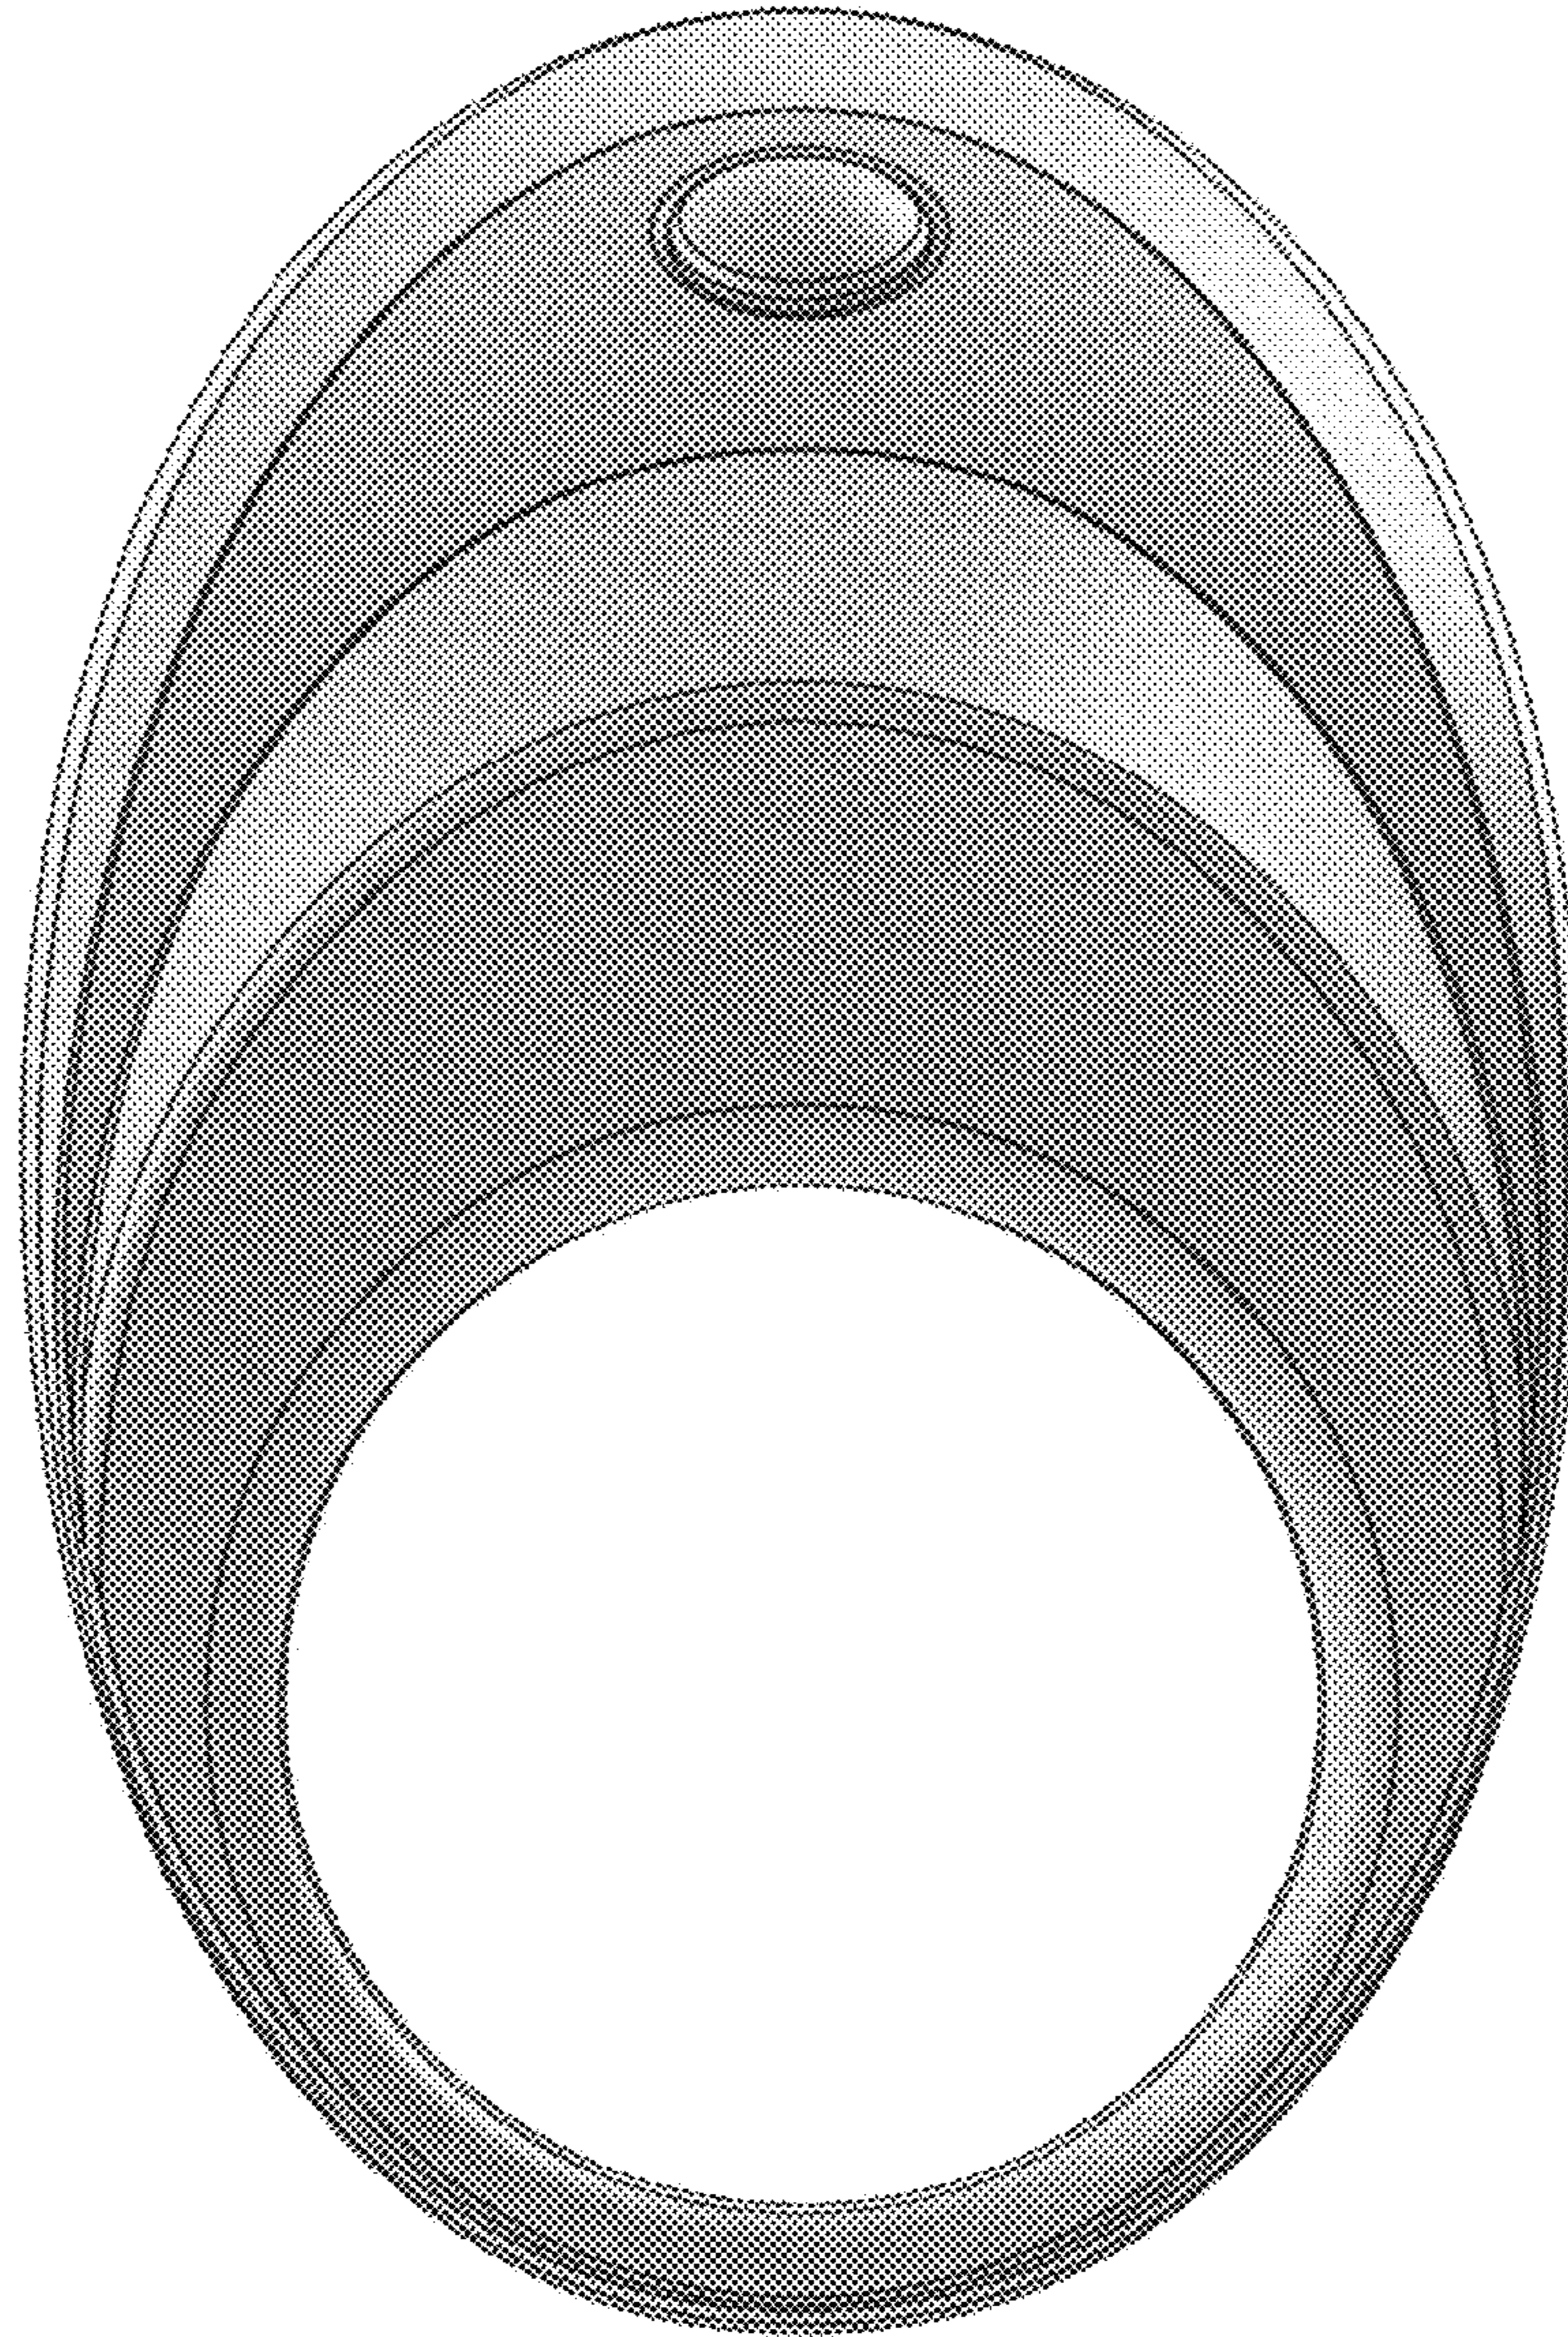


FIG. 5

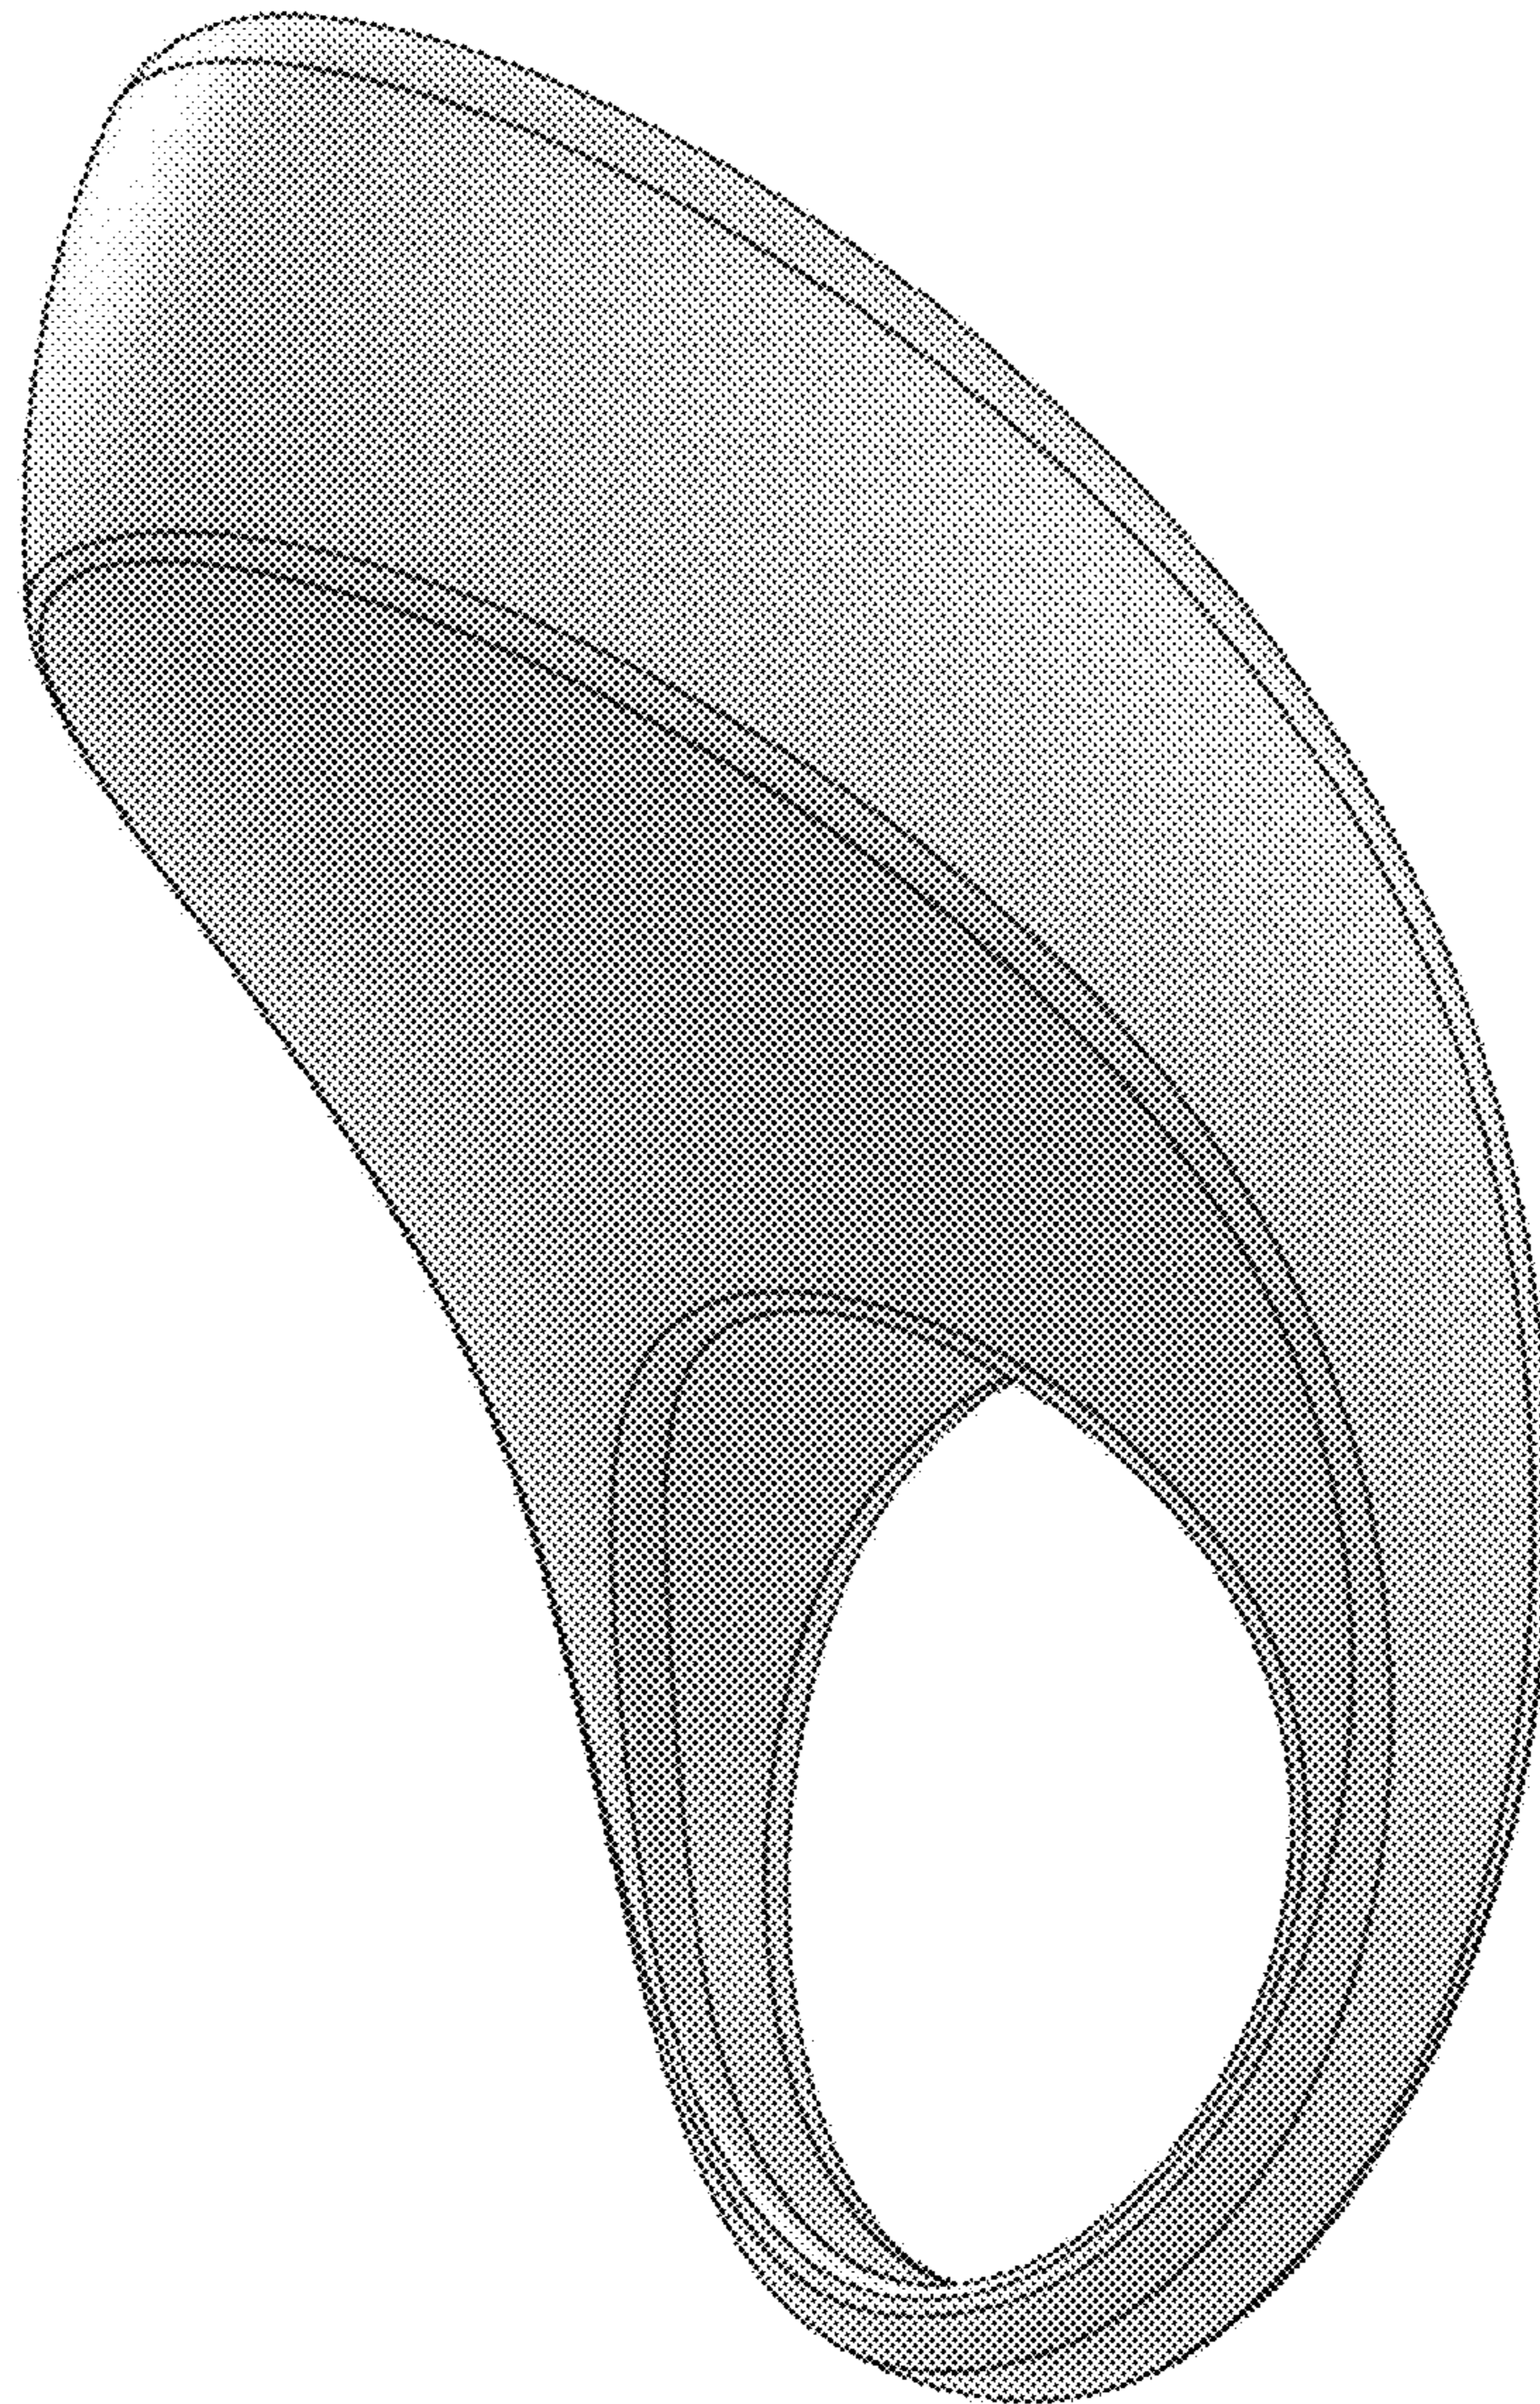


FIG. 6