

US00D706441S

(12) **United States Design Patent**
Hahr et al.

(10) **Patent No.:** **US D706,441 S**
(45) **Date of Patent:** **** Jun. 3, 2014**

(54) **STIMULATION DEVICE**

(71) Applicant: **Senses Toys Intellectual Property Management UG**, Bielefeld (DE)

(72) Inventors: **Meike Hahr**, Hamburg (DE); **Heiko Tullney**, Hamburg (DE); **Till Muhl**, Hamburg (DE); **Thomas Milewski**, Halstenbek (DE)

(73) Assignee: **Ovo Joint Venture LLC**, Pembroke Park, FL (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/447,971**

(22) Filed: **Mar. 8, 2013**

(30) **Foreign Application Priority Data**

Sep. 10, 2012 (EM) 001342935-0117

(51) **LOC (10) Cl.** **28-03**

(52) **U.S. Cl.**
USPC **D24/215**

(58) **Field of Classification Search**
USPC D24/200, 211, 212, 213, 214, 215;
601/114, 120, 121, 124, 125, 130, 131,
601/134, 135, 136, 137
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D30,230 S * 2/1899 Barnet D24/214
D447,811 S * 9/2001 Yiu D24/215

D454,959 S * 3/2002 Harris et al. D24/215
D620,601 S * 7/2010 TerMeer D24/215
D637,309 S * 5/2011 Park D24/215
D643,128 S * 8/2011 Mohamed et al. D24/215
D648,862 S * 11/2011 Yen D24/215
D668,346 S * 10/2012 Zeng et al. D24/215
D673,687 S * 1/2013 Zeng et al. D24/215
D675,745 S * 2/2013 Nan D24/215
D675,746 S * 2/2013 Nan D24/215
D681,225 S * 4/2013 Chen D24/215
D681,842 S * 5/2013 Chang D24/215
D685,105 S * 6/2013 Marshall D24/215
D688,382 S * 8/2013 Marshall D24/215
D693,017 S * 11/2013 Tai D24/215
D693,933 S * 11/2013 Tai D24/215
D694,417 S * 11/2013 Tai D24/215

* cited by examiner

Primary Examiner — Sandra Snapp

(74) *Attorney, Agent, or Firm* — Merek, Blackmon & Voorhees, LLC


(57) **CLAIM**

The ornamental design for a stimulation device, as shown and described.

DESCRIPTION

FIG. 1 is a top plan view of a stimulation device showing the design;
FIG. 2 is a perspective view taken from the top and right side of the stimulation device of FIG. 1, the opposite side being a mirror image thereof; and,
FIG. 3 is a right side elevation view of the stimulation device of FIG. 1, the left side elevation view being a mirror image thereof.

1 Claim, 3 Drawing Sheets

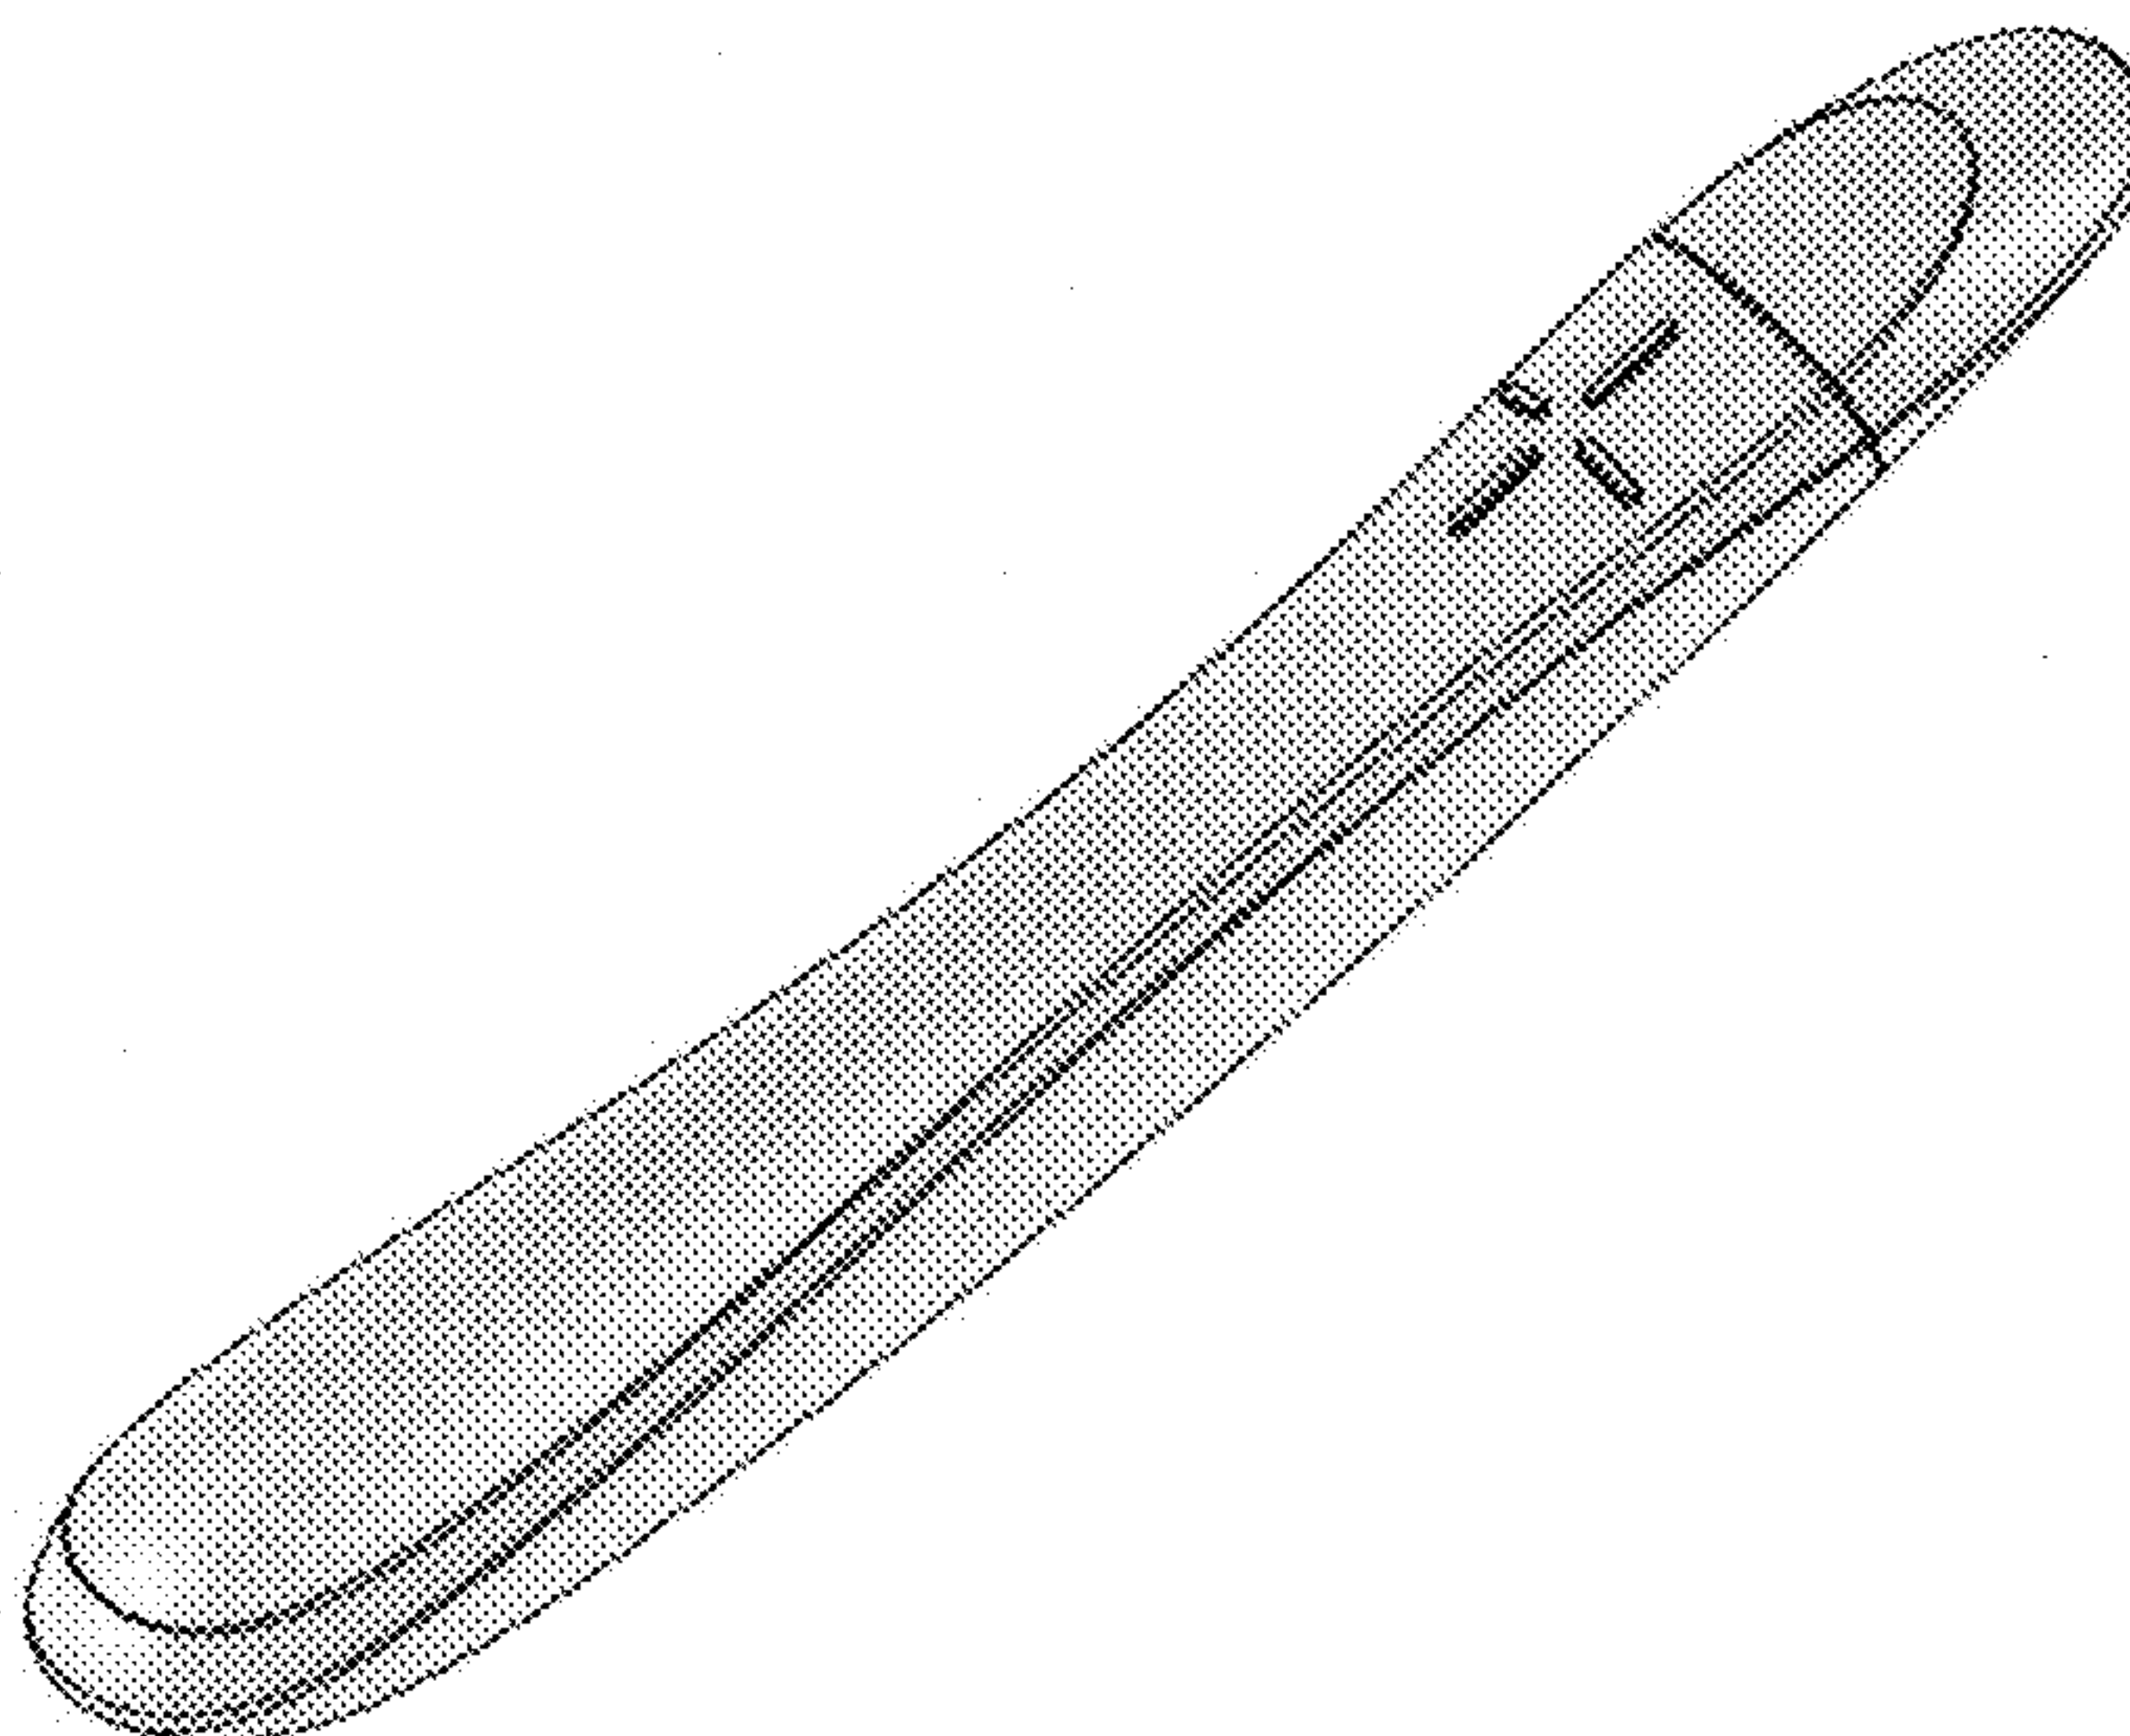

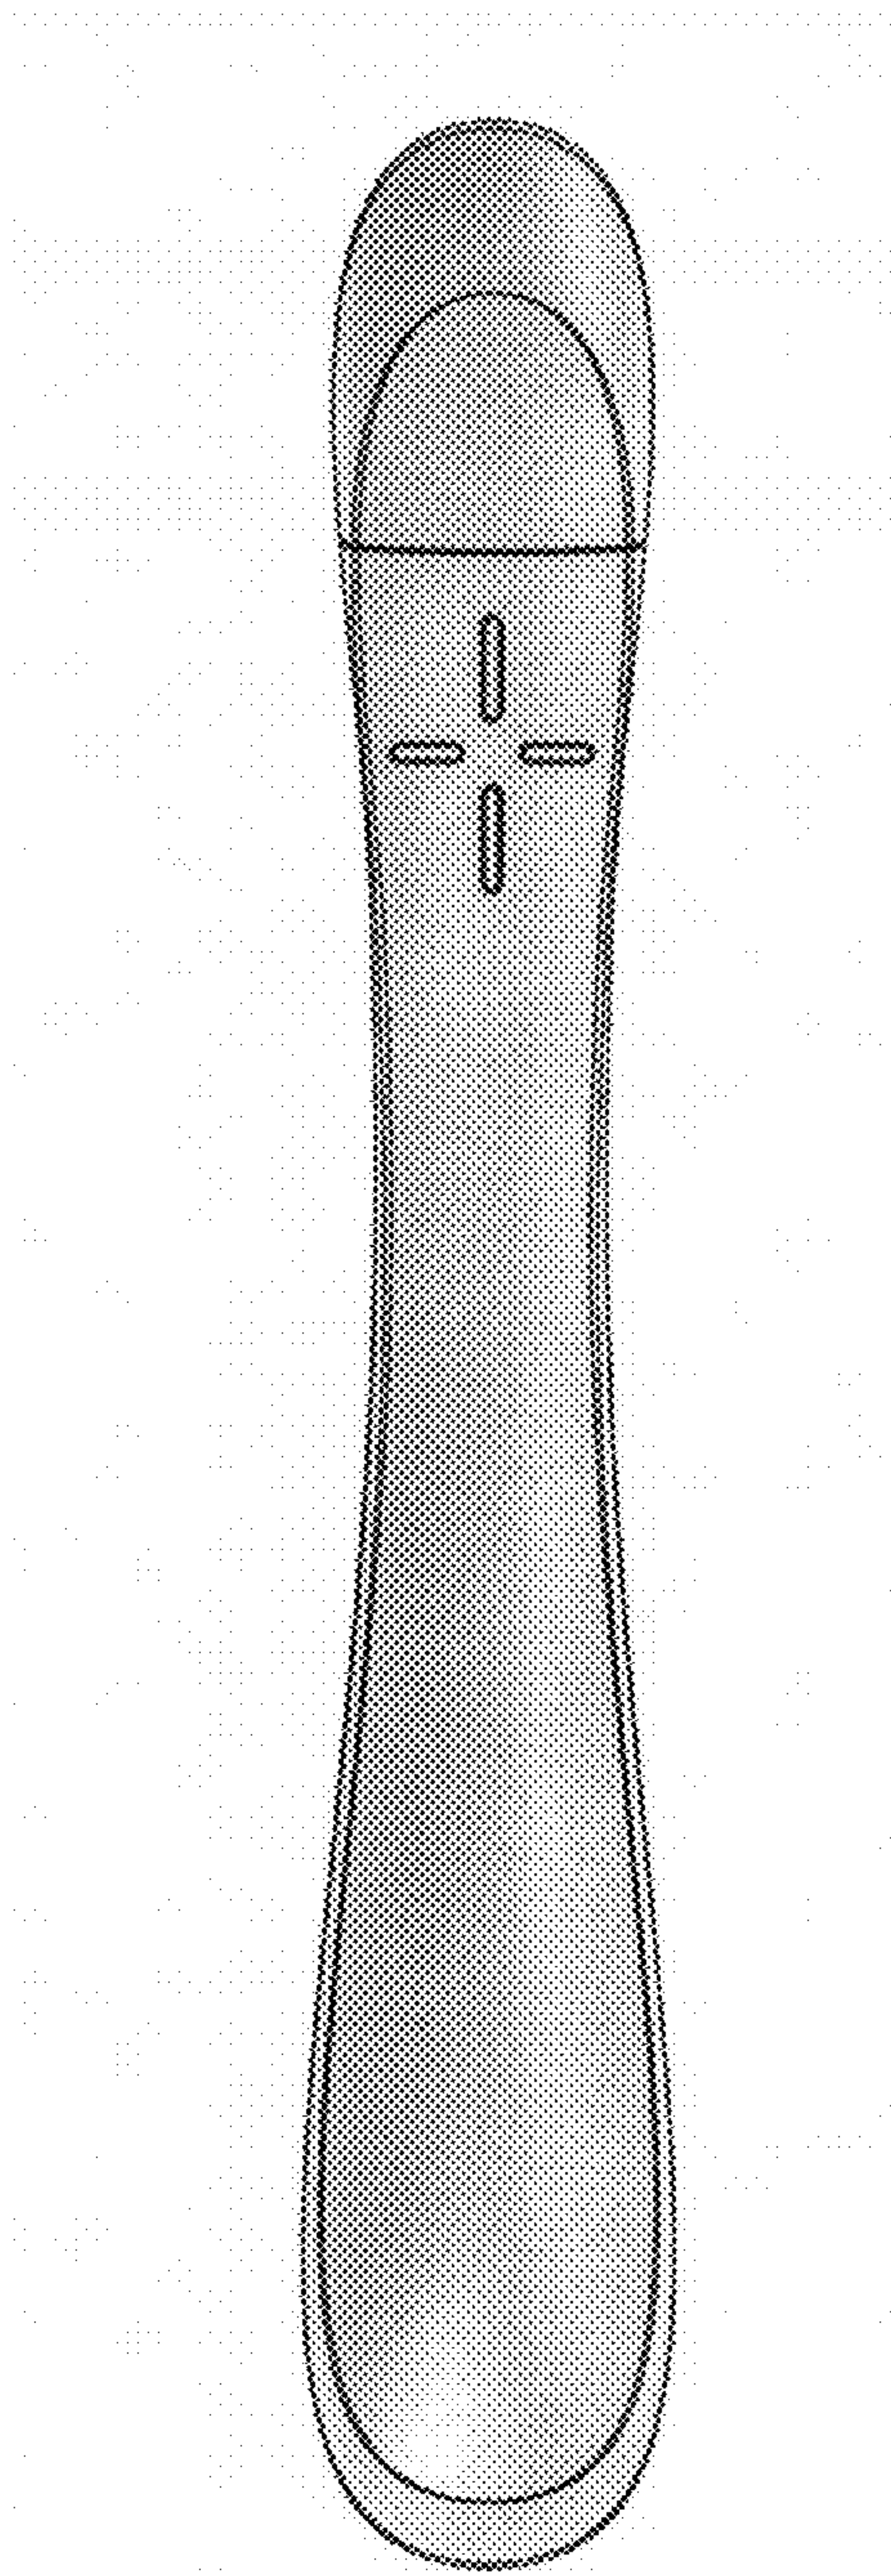


FIG. 1

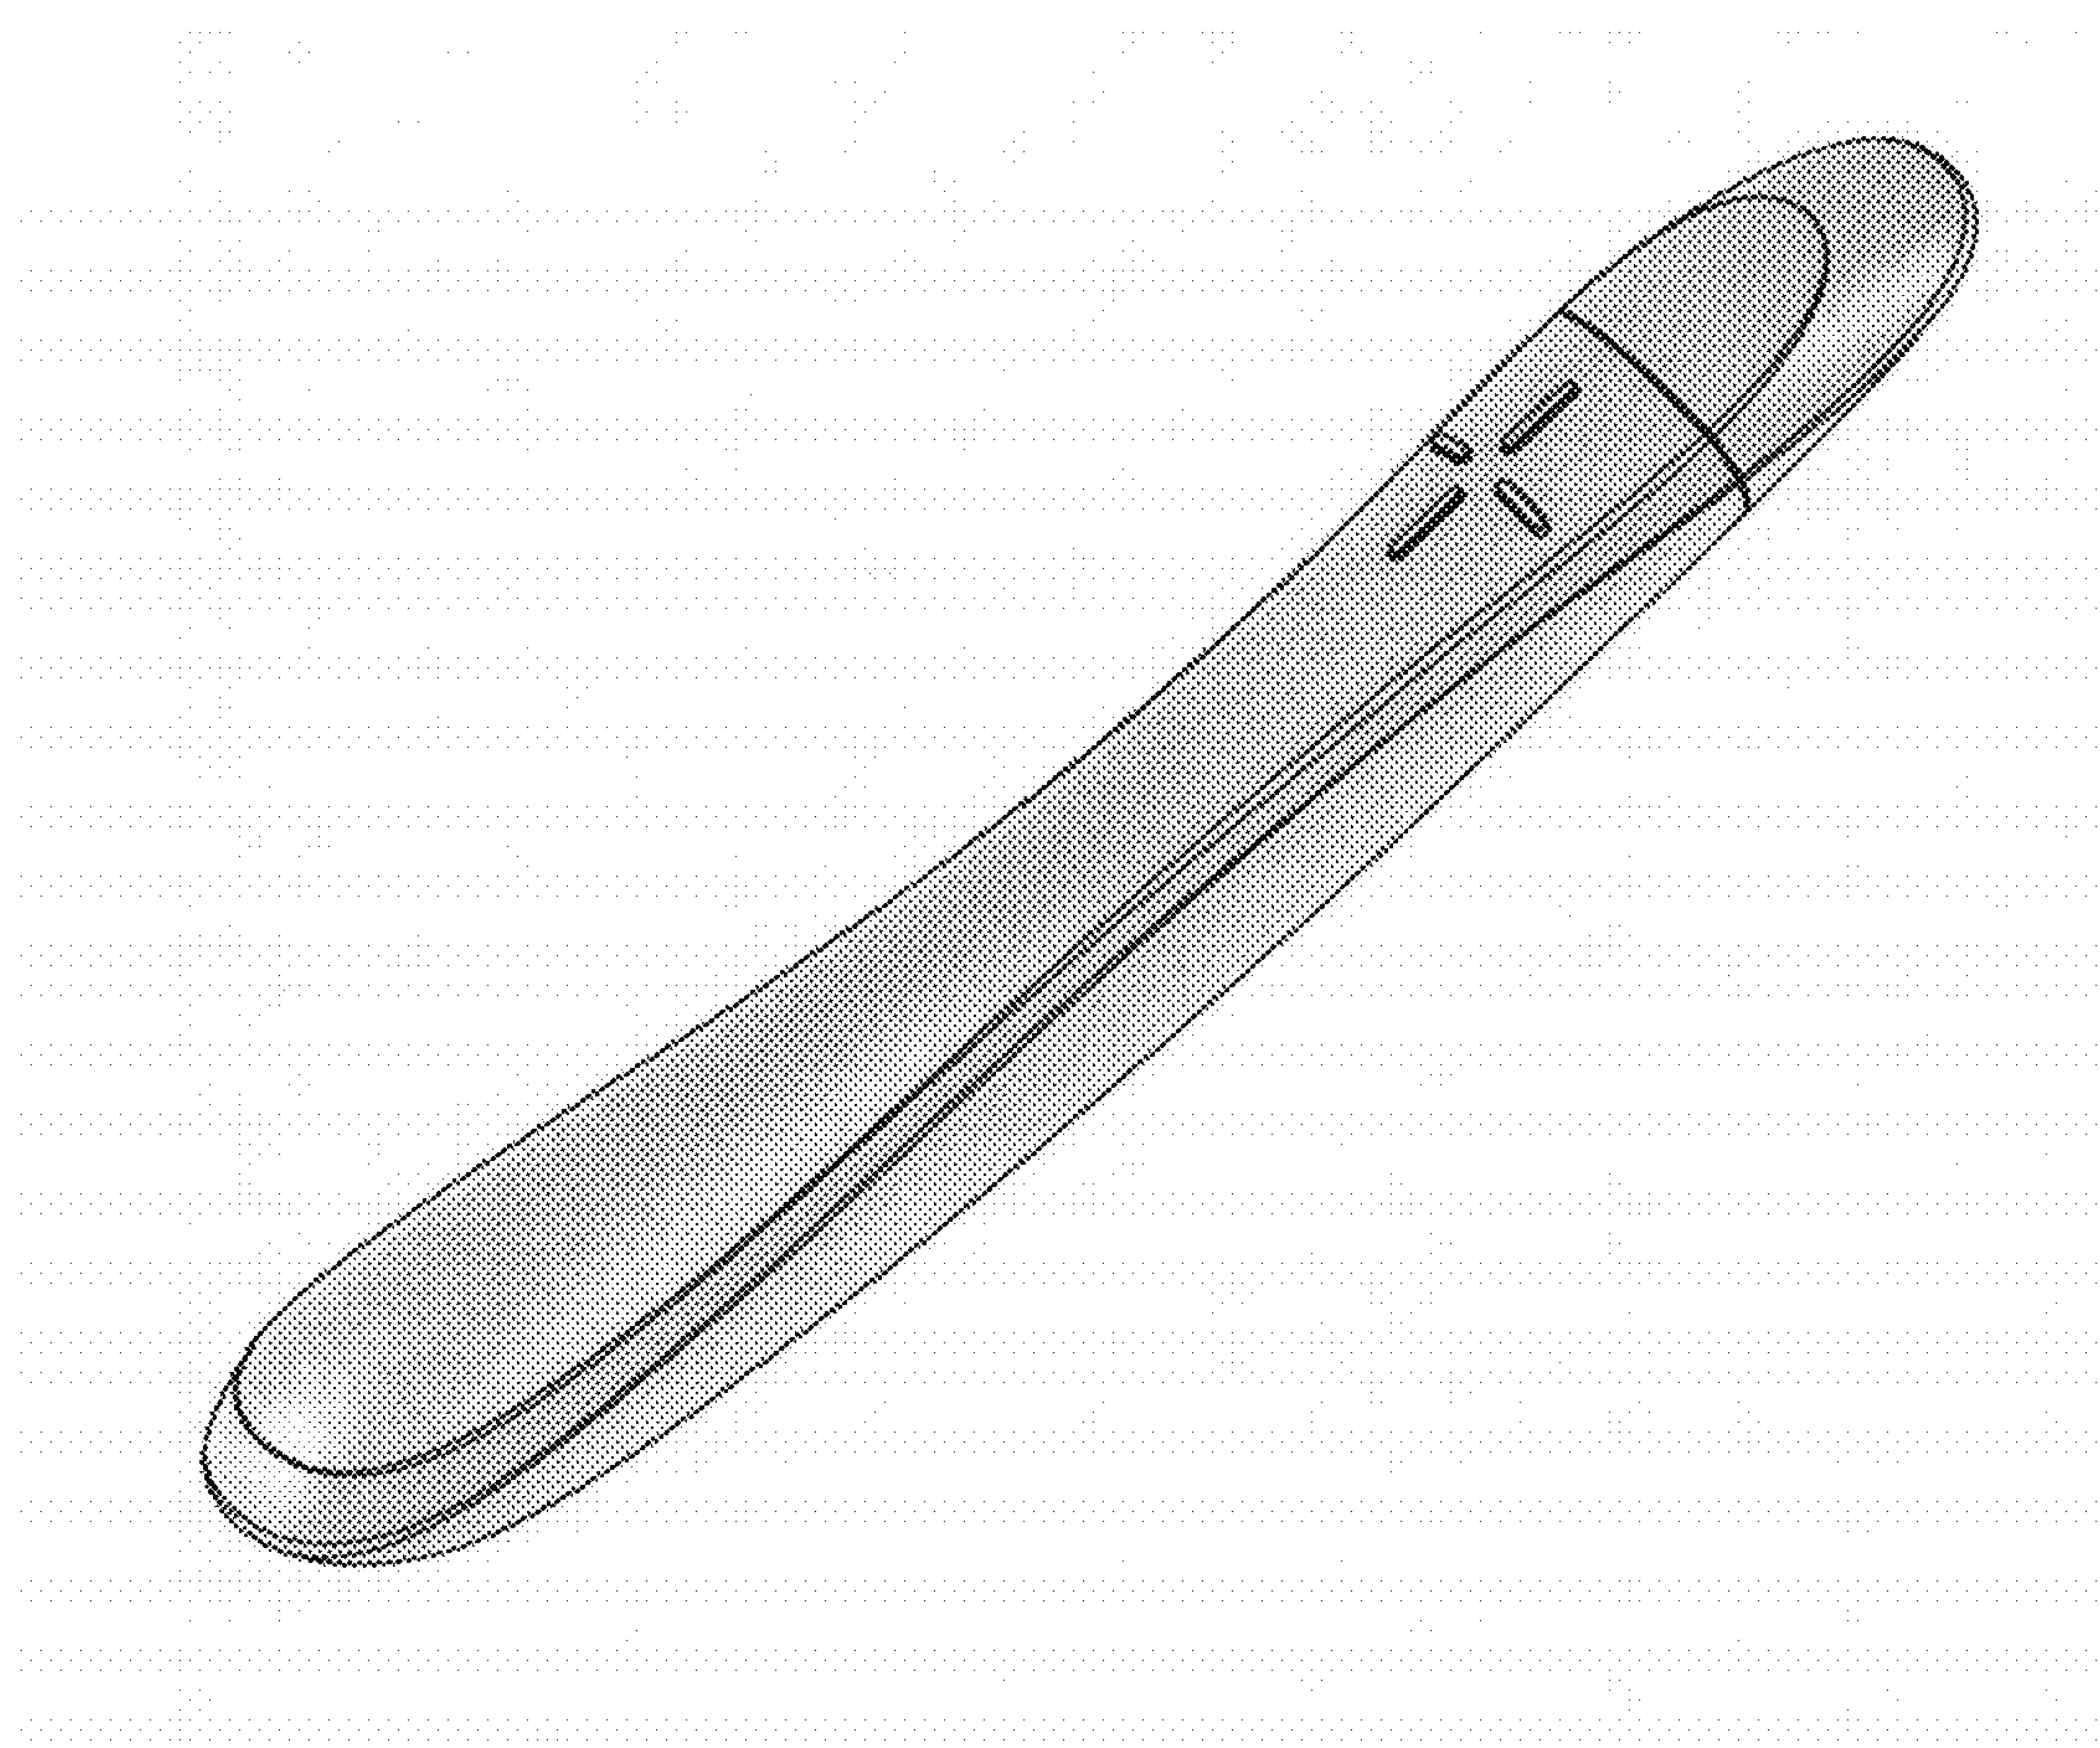


FIG. 2

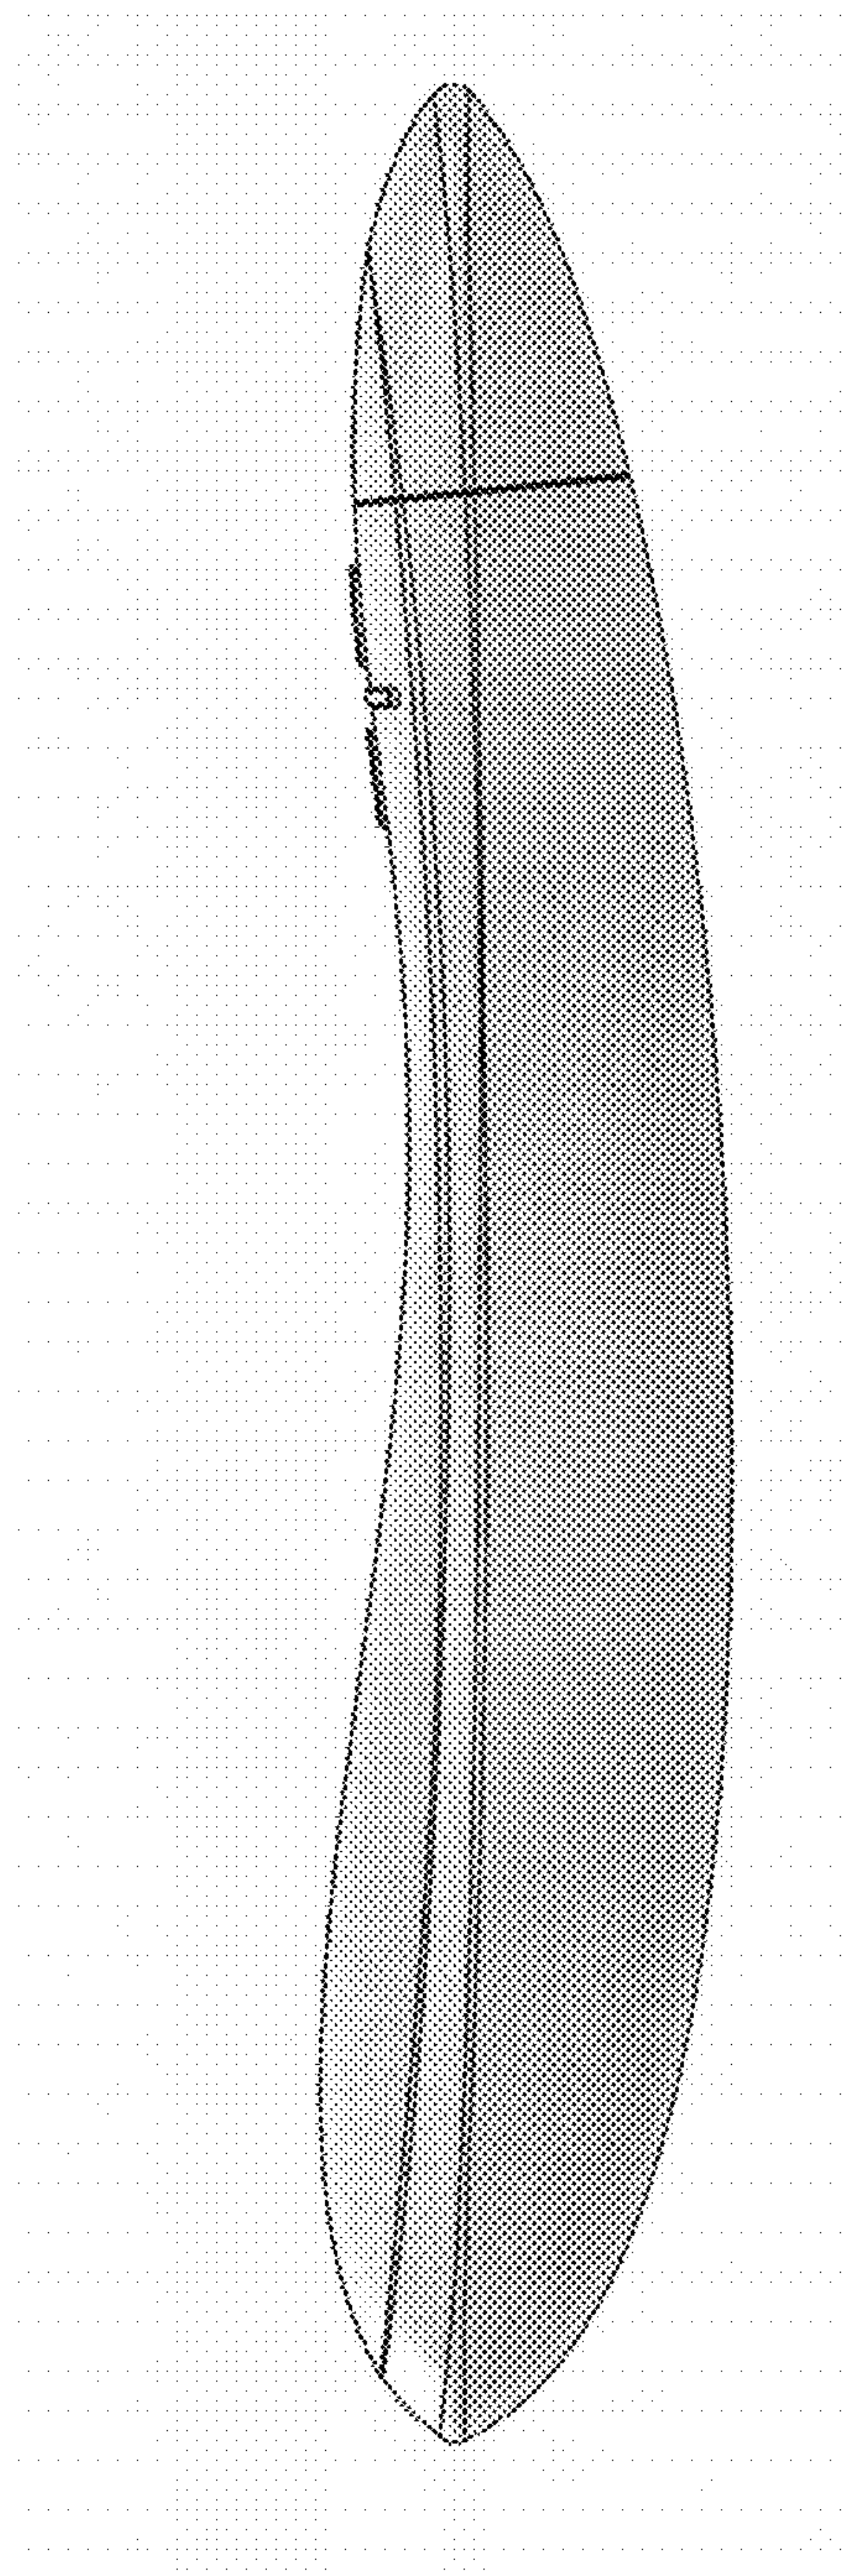


FIG. 3