



US00D706443S

(12) **United States Design Patent**  
**Hahr et al.**(10) **Patent No.:** **US D706,443 S**  
(45) **Date of Patent:** **\*\* Jun. 3, 2014**(54) **STIMULATION DEVICE**

(71) Applicant: **Senses Toys Intellectual Property Management UG**, Bielefeld (DE)

(72) Inventors: **Meike Hahr**, Hamburg (DE); **Heiko Tullney**, Hamburg (DE); **Till Muhl**, Hamburg (DE); **Thomas Milewski**, Halstenbek (DE)

(73) Assignee: **Ovo Joint Venture LLC**, Pembroke Park, FL (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/448,007**

(22) Filed: **Mar. 8, 2013**

(30) **Foreign Application Priority Data**

Sep. 10, 2012 (EM) ..... 001342935-0055

(51) **LOC (10) Cl.** ..... **28-03**  
(52) **U.S. Cl.** ..... **D24/215**

(58) **Field of Classification Search**  
USPC ..... D24/200, 211, 212, 213, 214, 215;  
601/114, 120, 121, 124, 125, 130, 131,  
601/134, 135, 136, 137

See application file for complete search history.

(56) **References Cited**

## U.S. PATENT DOCUMENTS

D350,397 S \* 9/1994 Bruno et al. ..... D24/214  
D648,861 S \* 11/2011 Chong et al. ..... D24/215  
D652,943 S \* 1/2012 Chong et al. ..... D24/215

D653,349 S \* 1/2012 Chong et al. ..... D24/215

\* cited by examiner

Primary Examiner — Sandra Snapp

(74) Attorney, Agent, or Firm — Merek, Blackmon &amp; Voorhees, LLC

(57) **CLAIM**

The ornamental design for a stimulation device, as shown and described.

**DESCRIPTION**

FIG. 1 is a top plan view of a stimulation device showing the design;

FIG. 2 is a perspective view taken from the bottom, rear and left side of the stimulation device of FIG. 1, the opposite side being a mirror image thereof;

FIG. 3 is a right side elevation view of the stimulation device of FIG. 1, the left side elevation view being a mirror image thereof;

FIG. 4 is a rear elevation view of the stimulation device of FIG. 1; and,


FIG. 5 is a perspective view taken from the top and left side of the stimulation device of FIG. 1, the opposite side being a mirror image thereof.


A perspective view taken from the bottom, rear and right side of the stimulation device of FIG. 1 at an angle corresponding to the angle of the perspective view of FIG. 2 is a mirror image of FIG. 2.

The left side elevation of the stimulation device of FIG. 1 is a mirror image of the right side elevation shown in FIG. 3, except for the ridges on the top.


A perspective view taken from the top and right side of the stimulation device of FIG. 1 at an angle corresponding to the angle of the perspective view of FIG. 5 is a mirror image of FIG. 5, except for the ridges on the top.

**1 Claim, 5 Drawing Sheets**

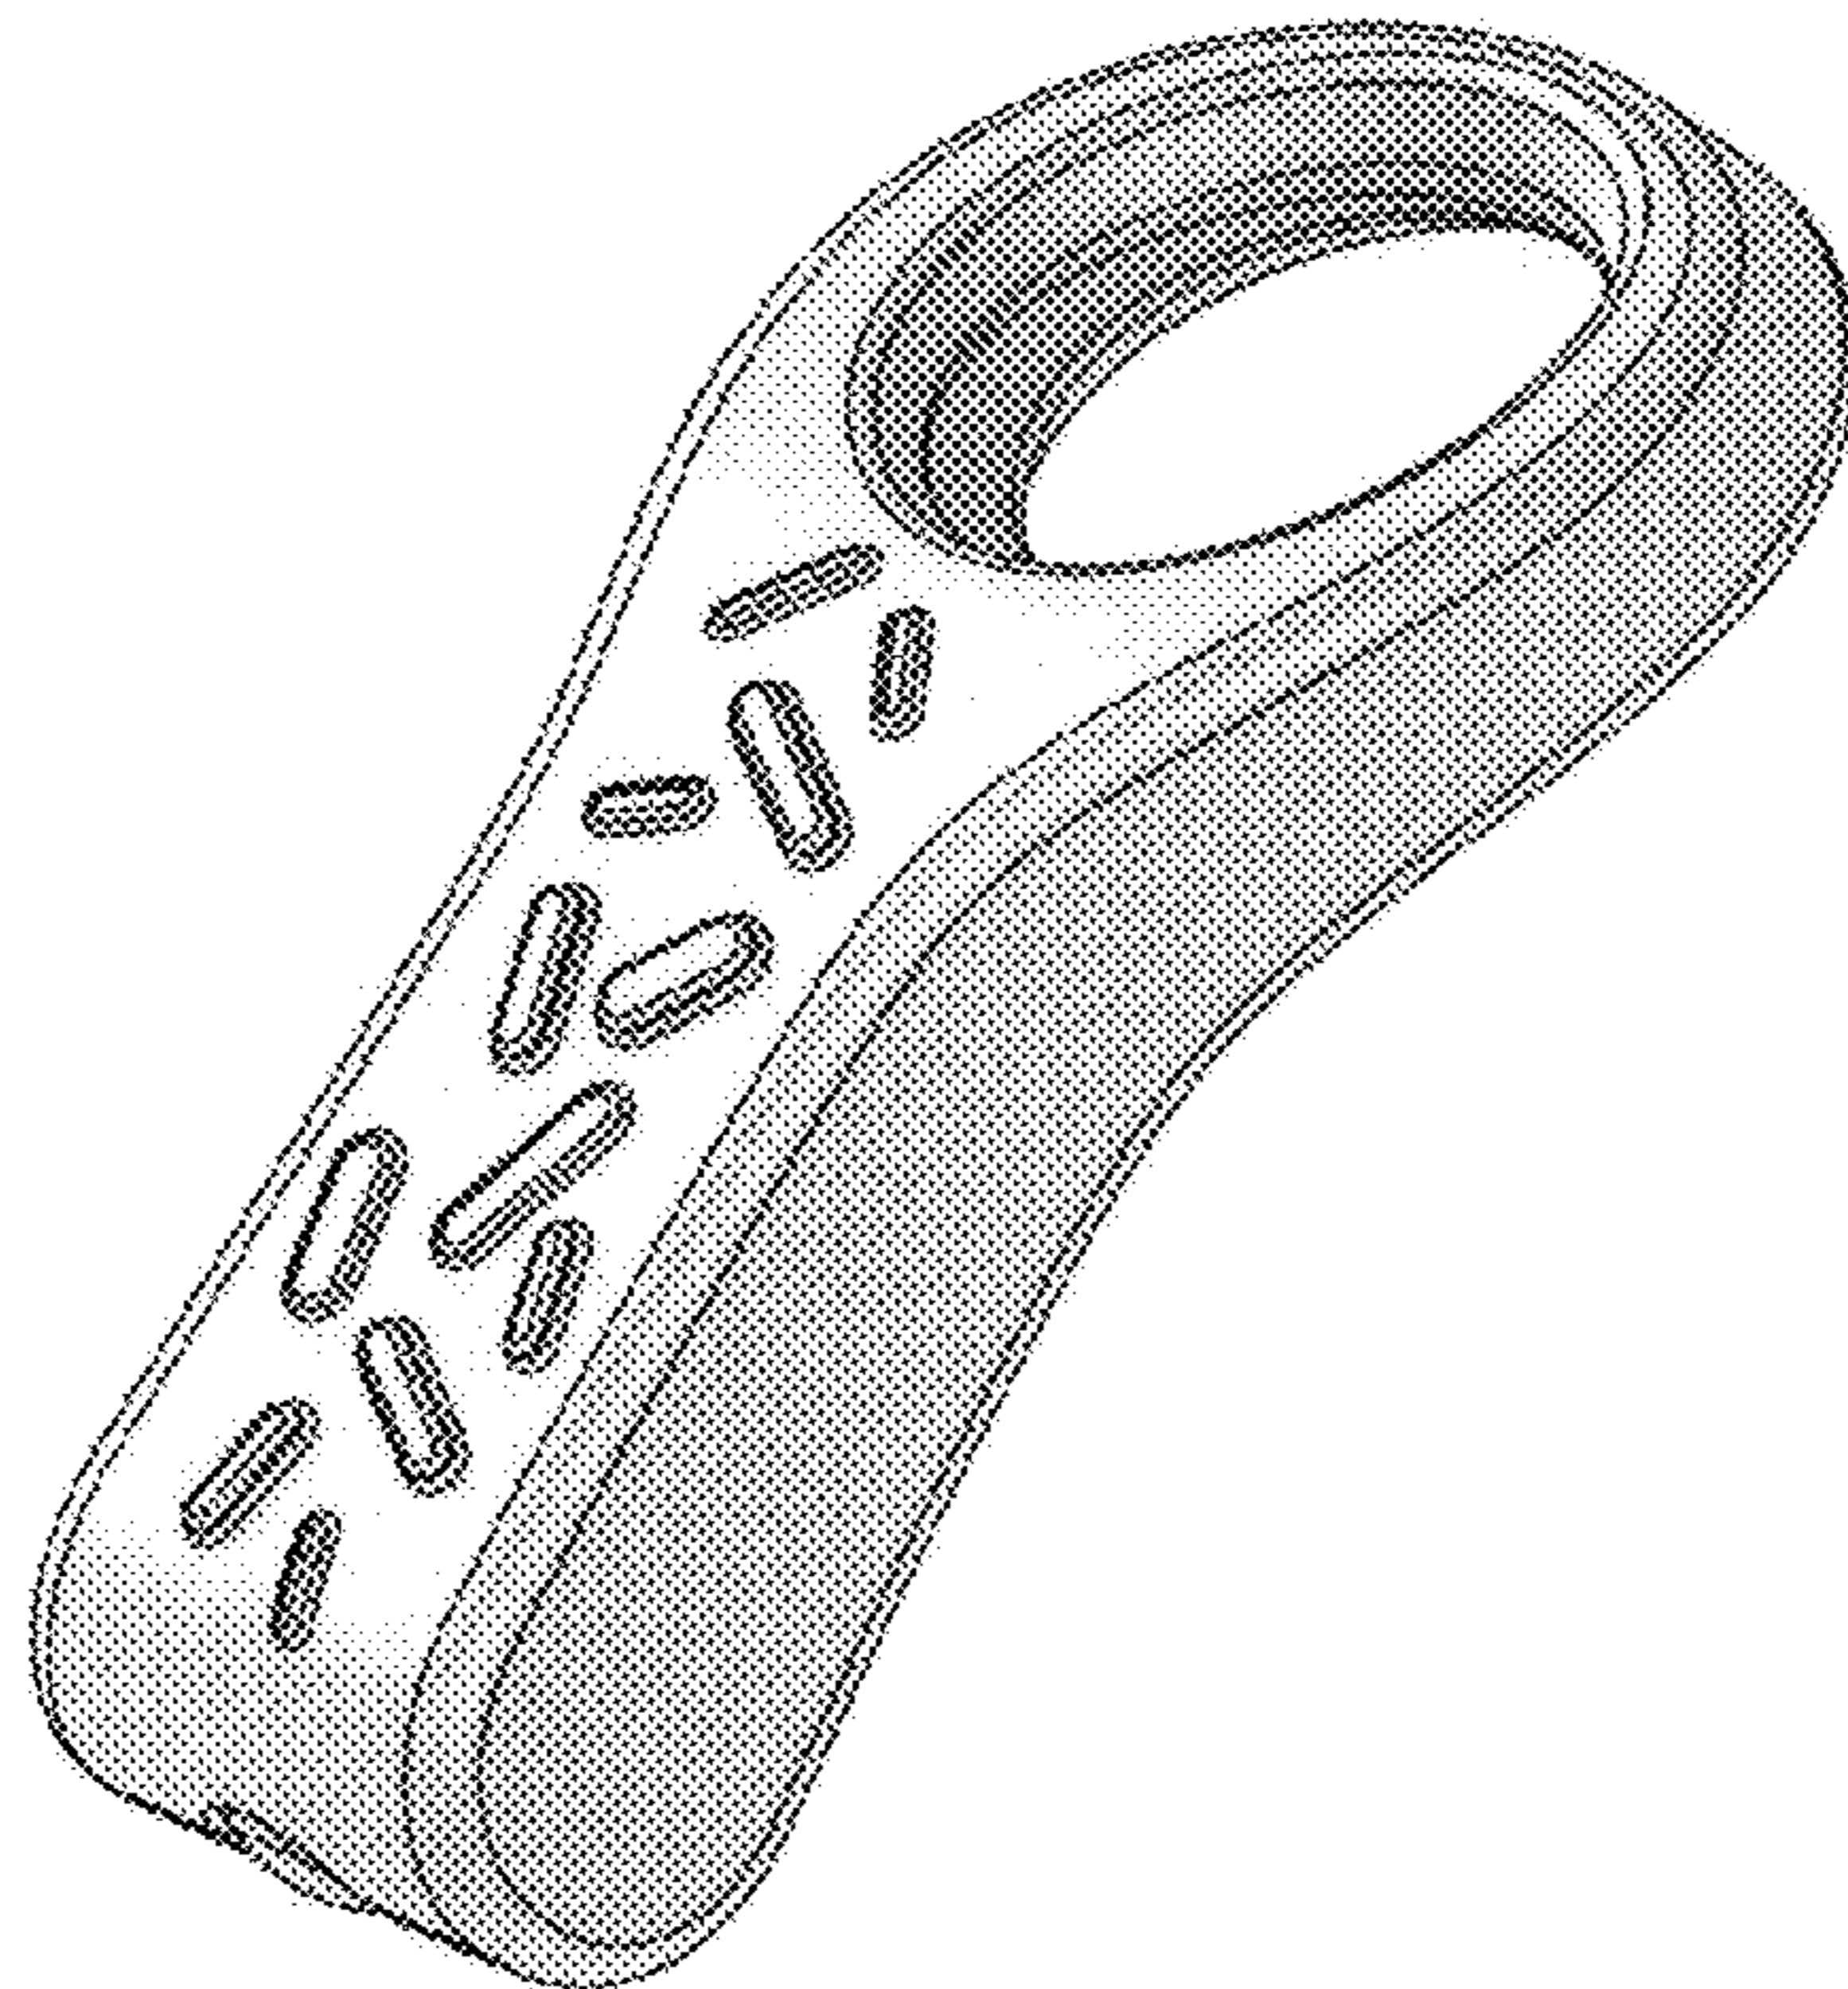


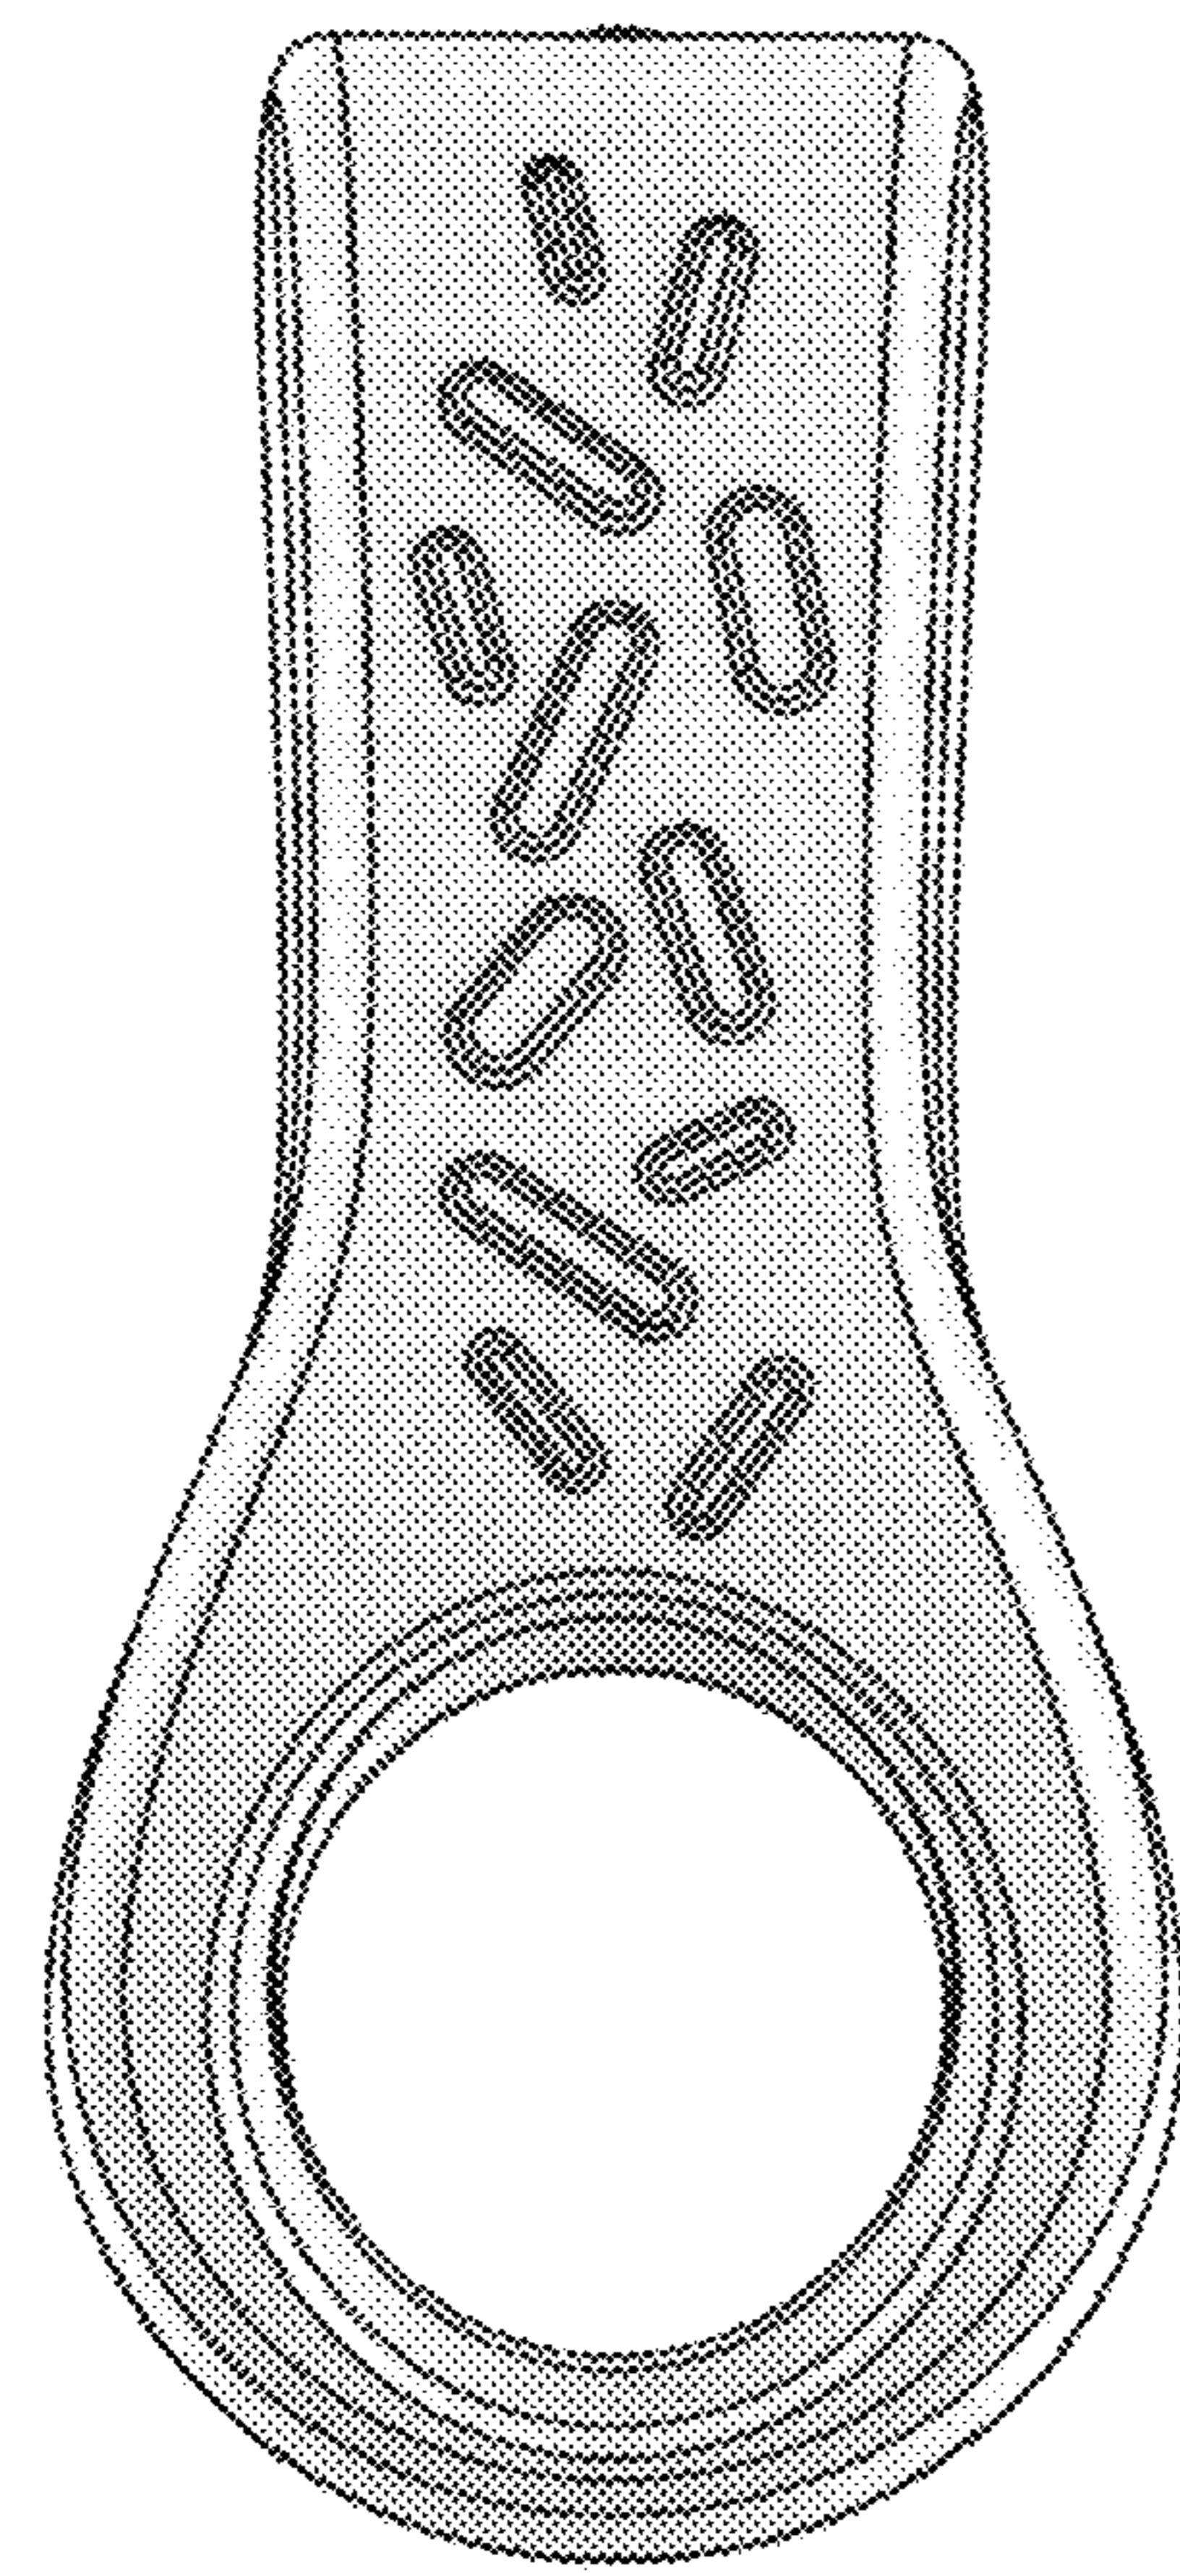


**FIG. 1**

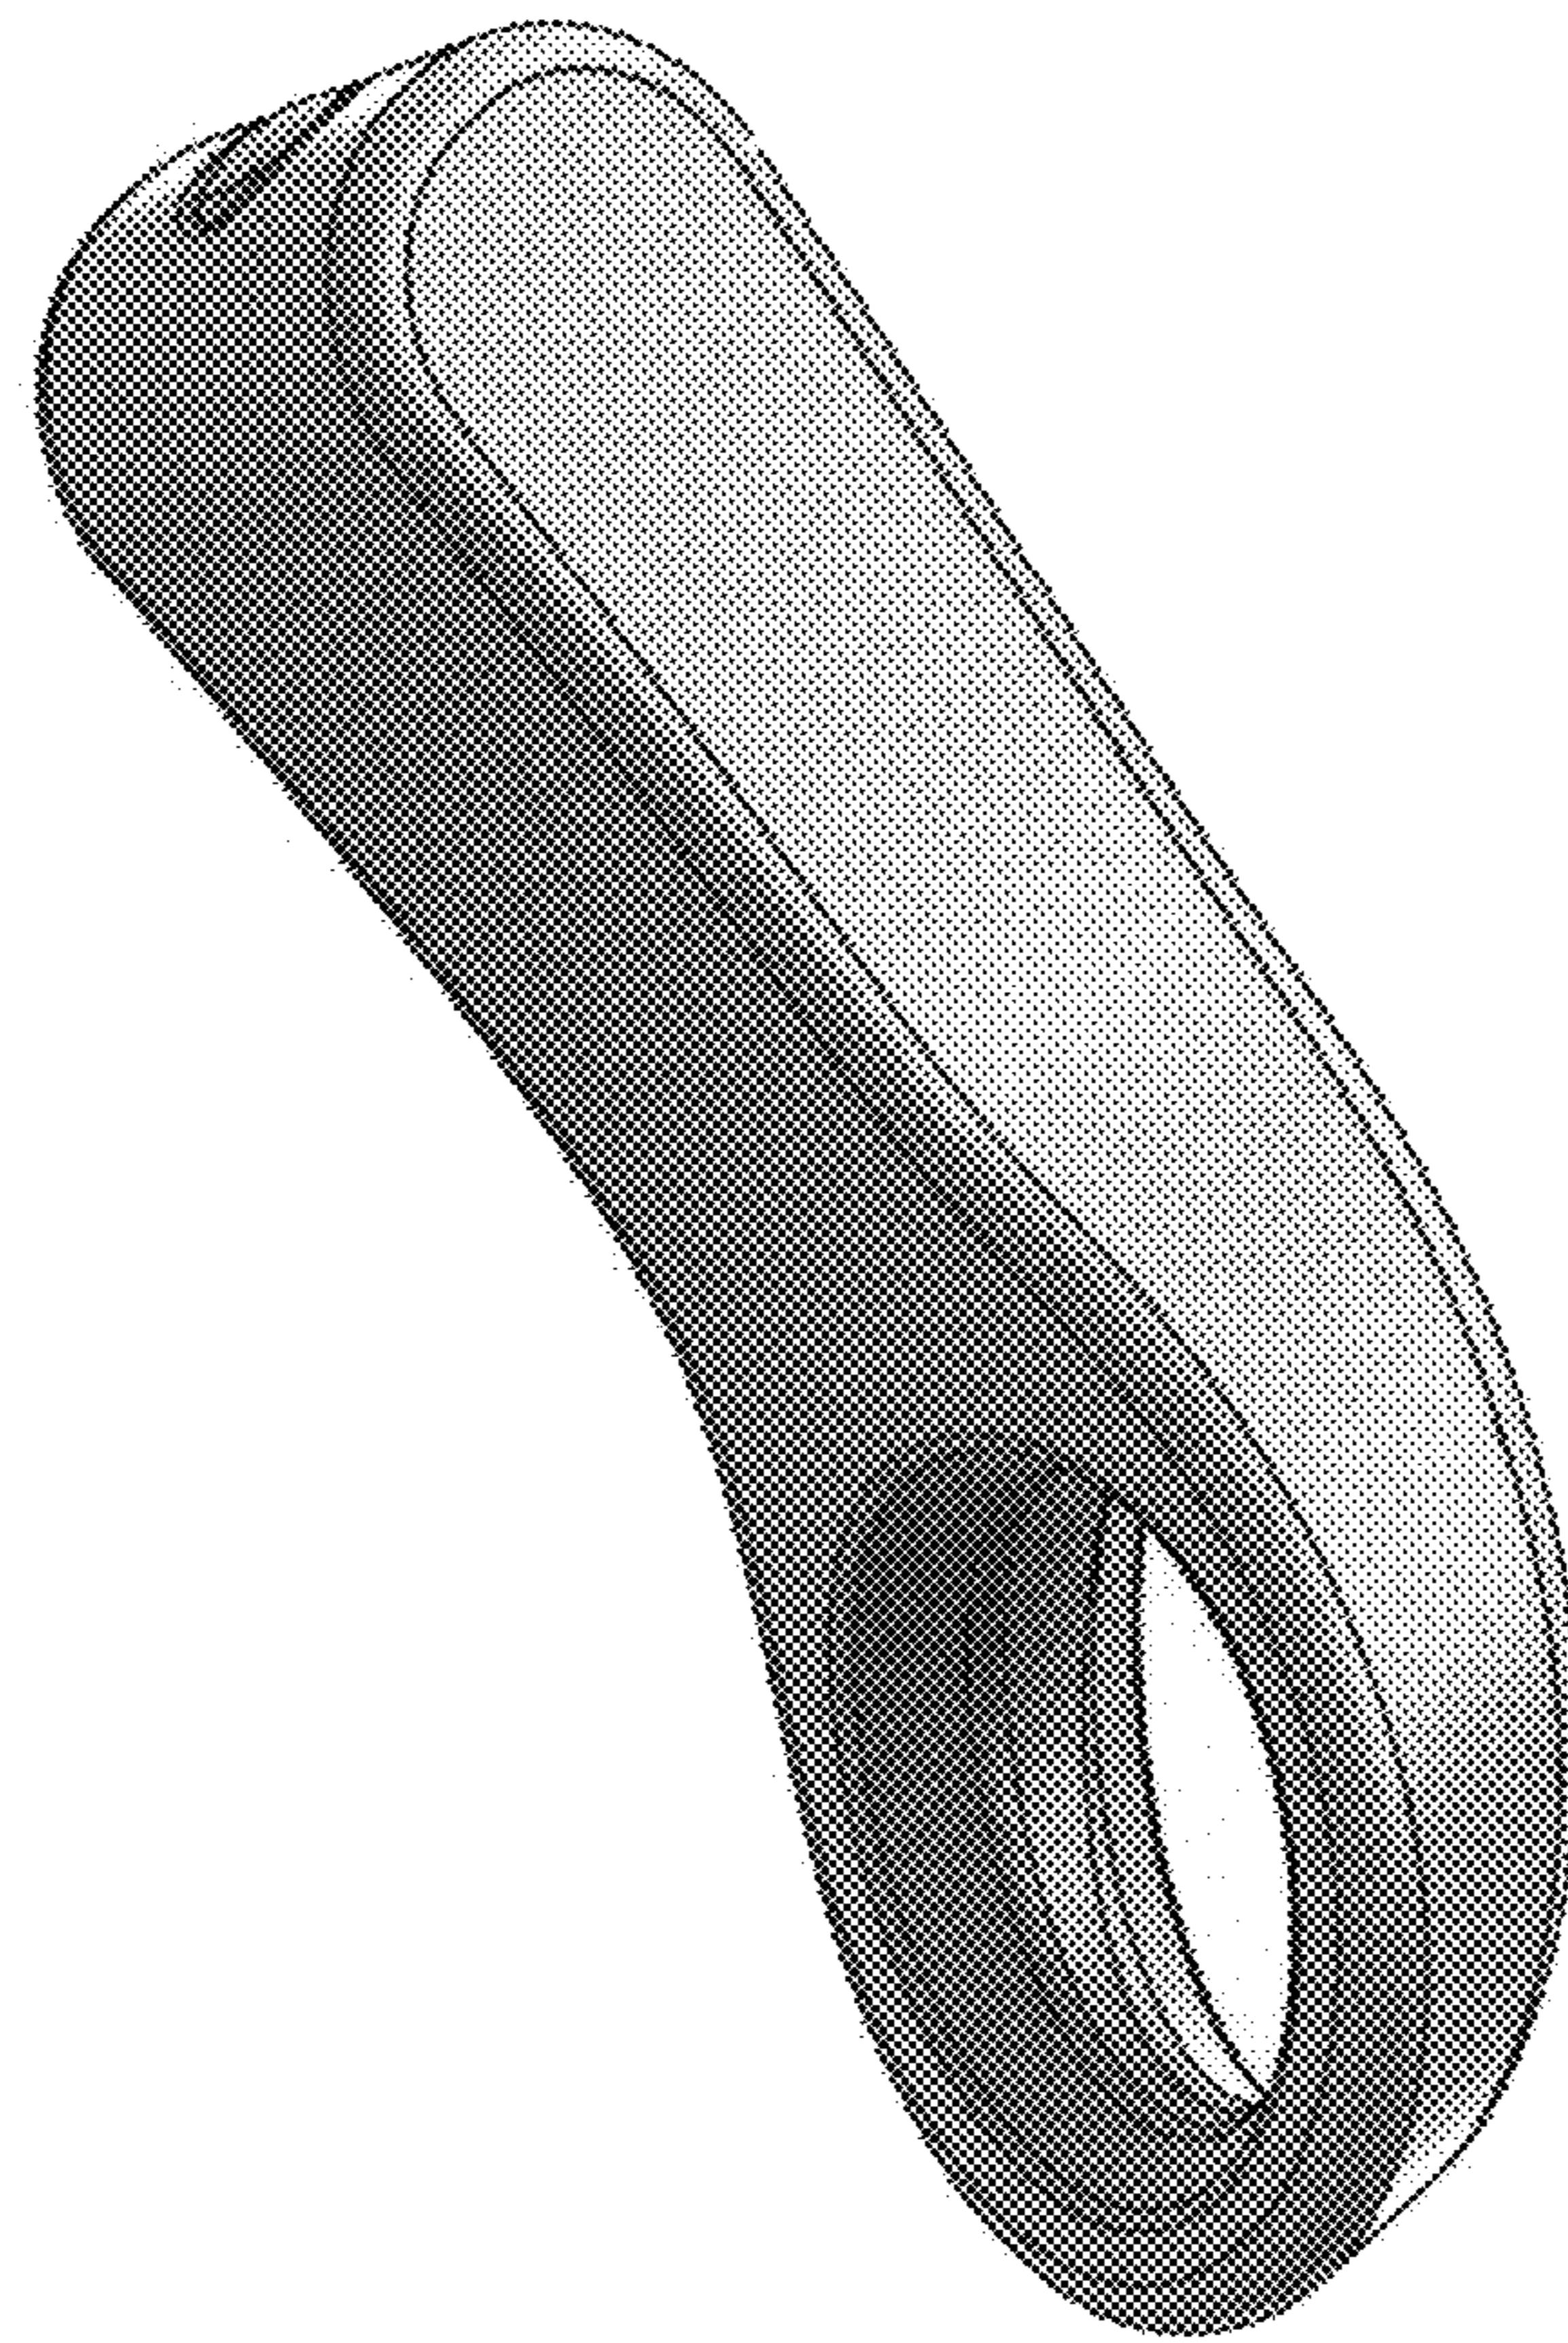

**FIG. 2**

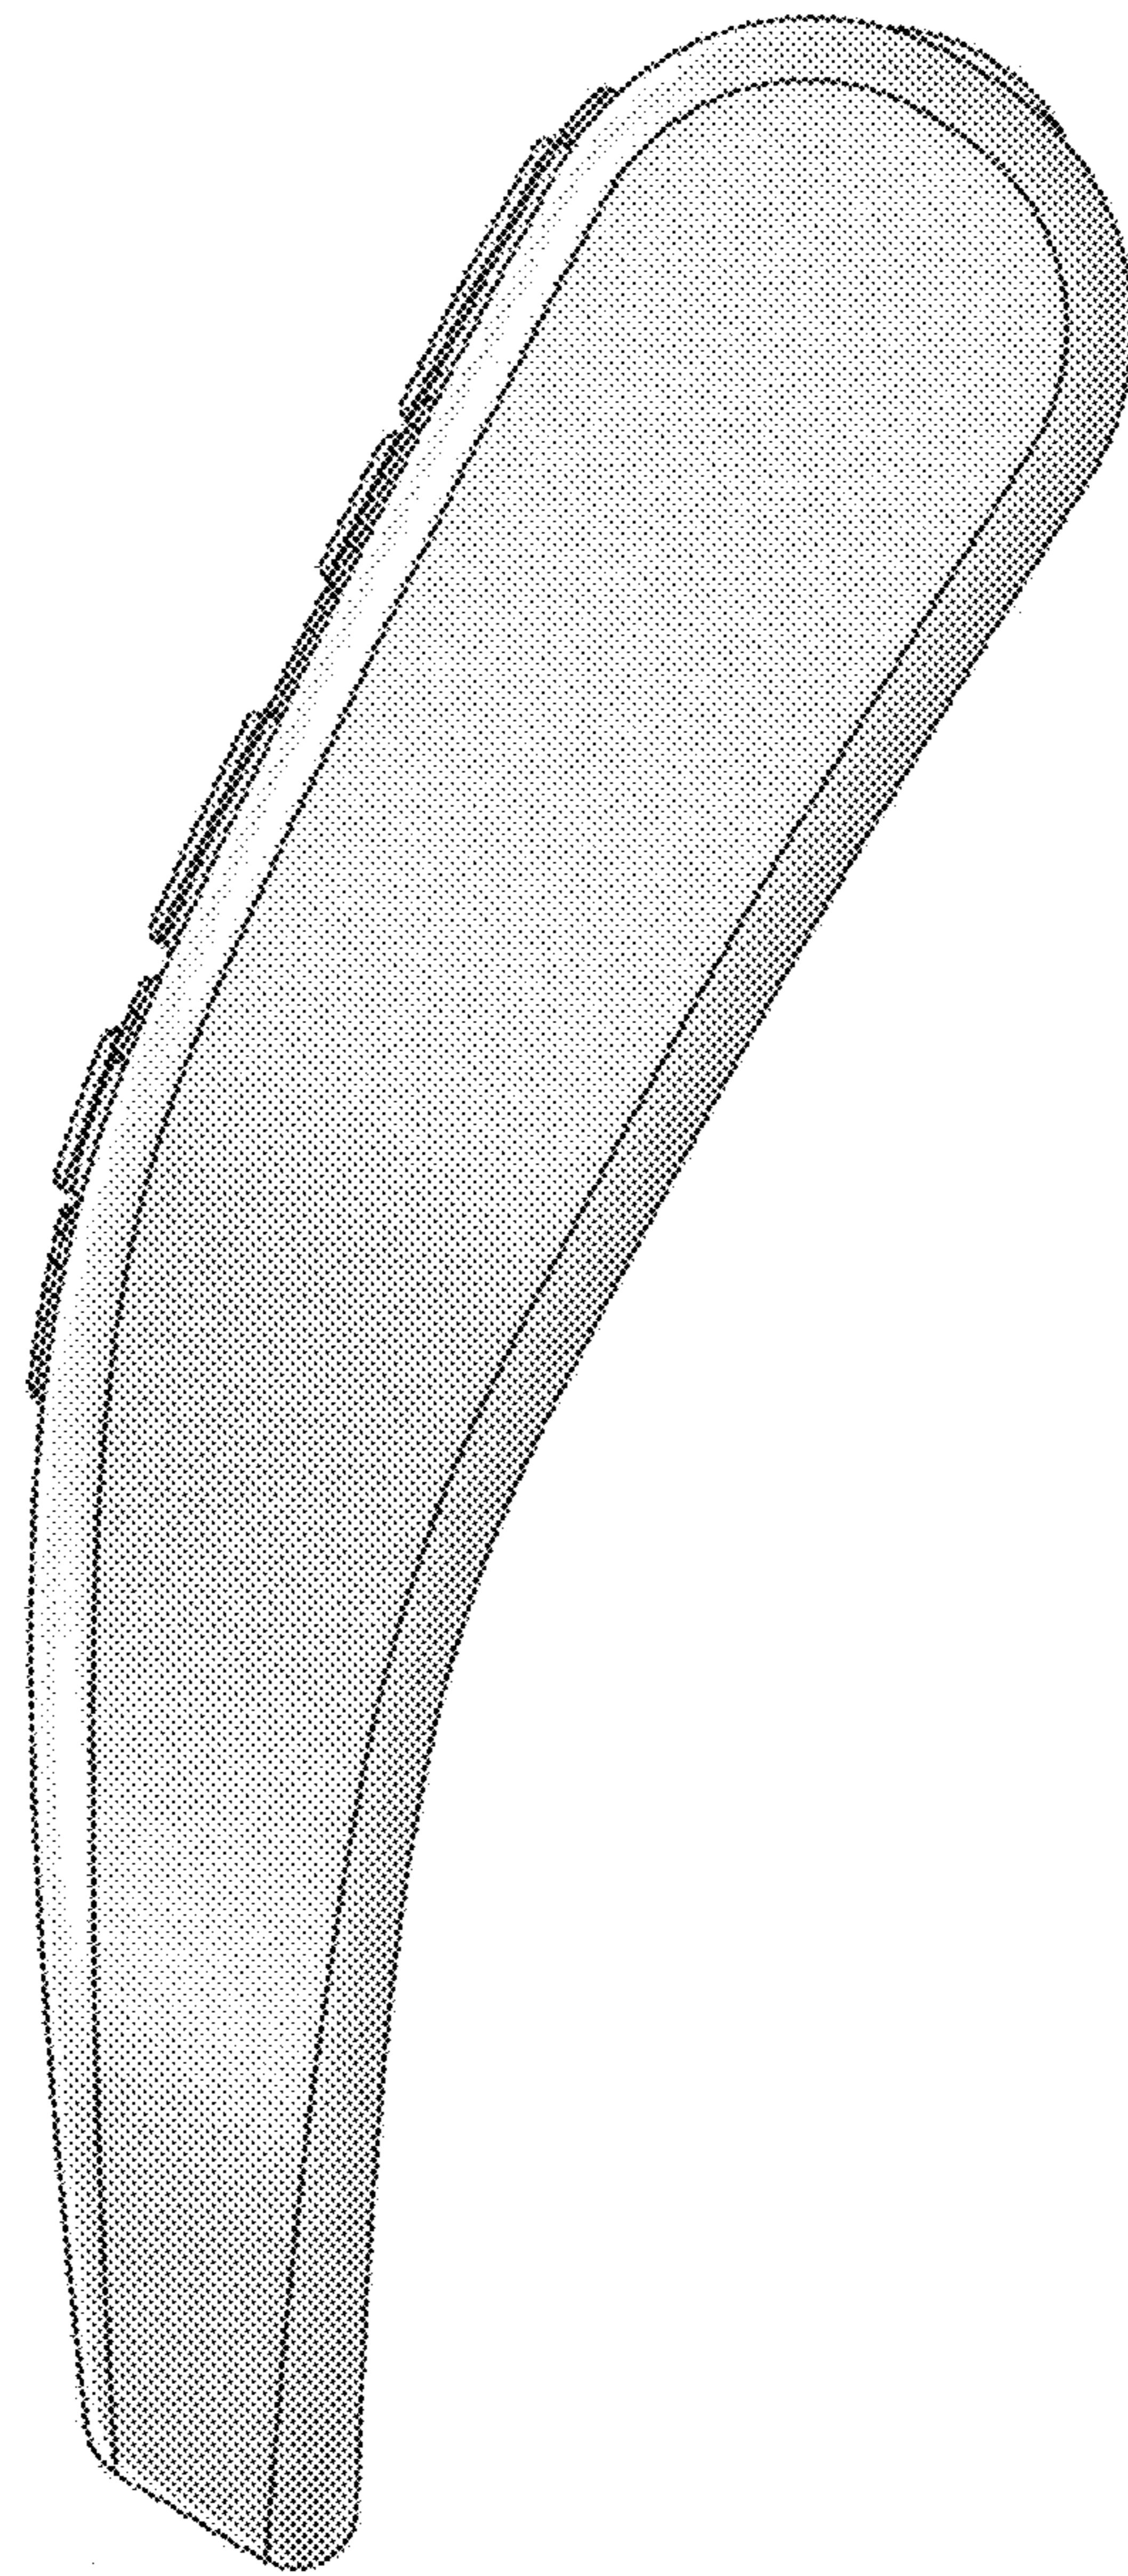

**FIG. 3**

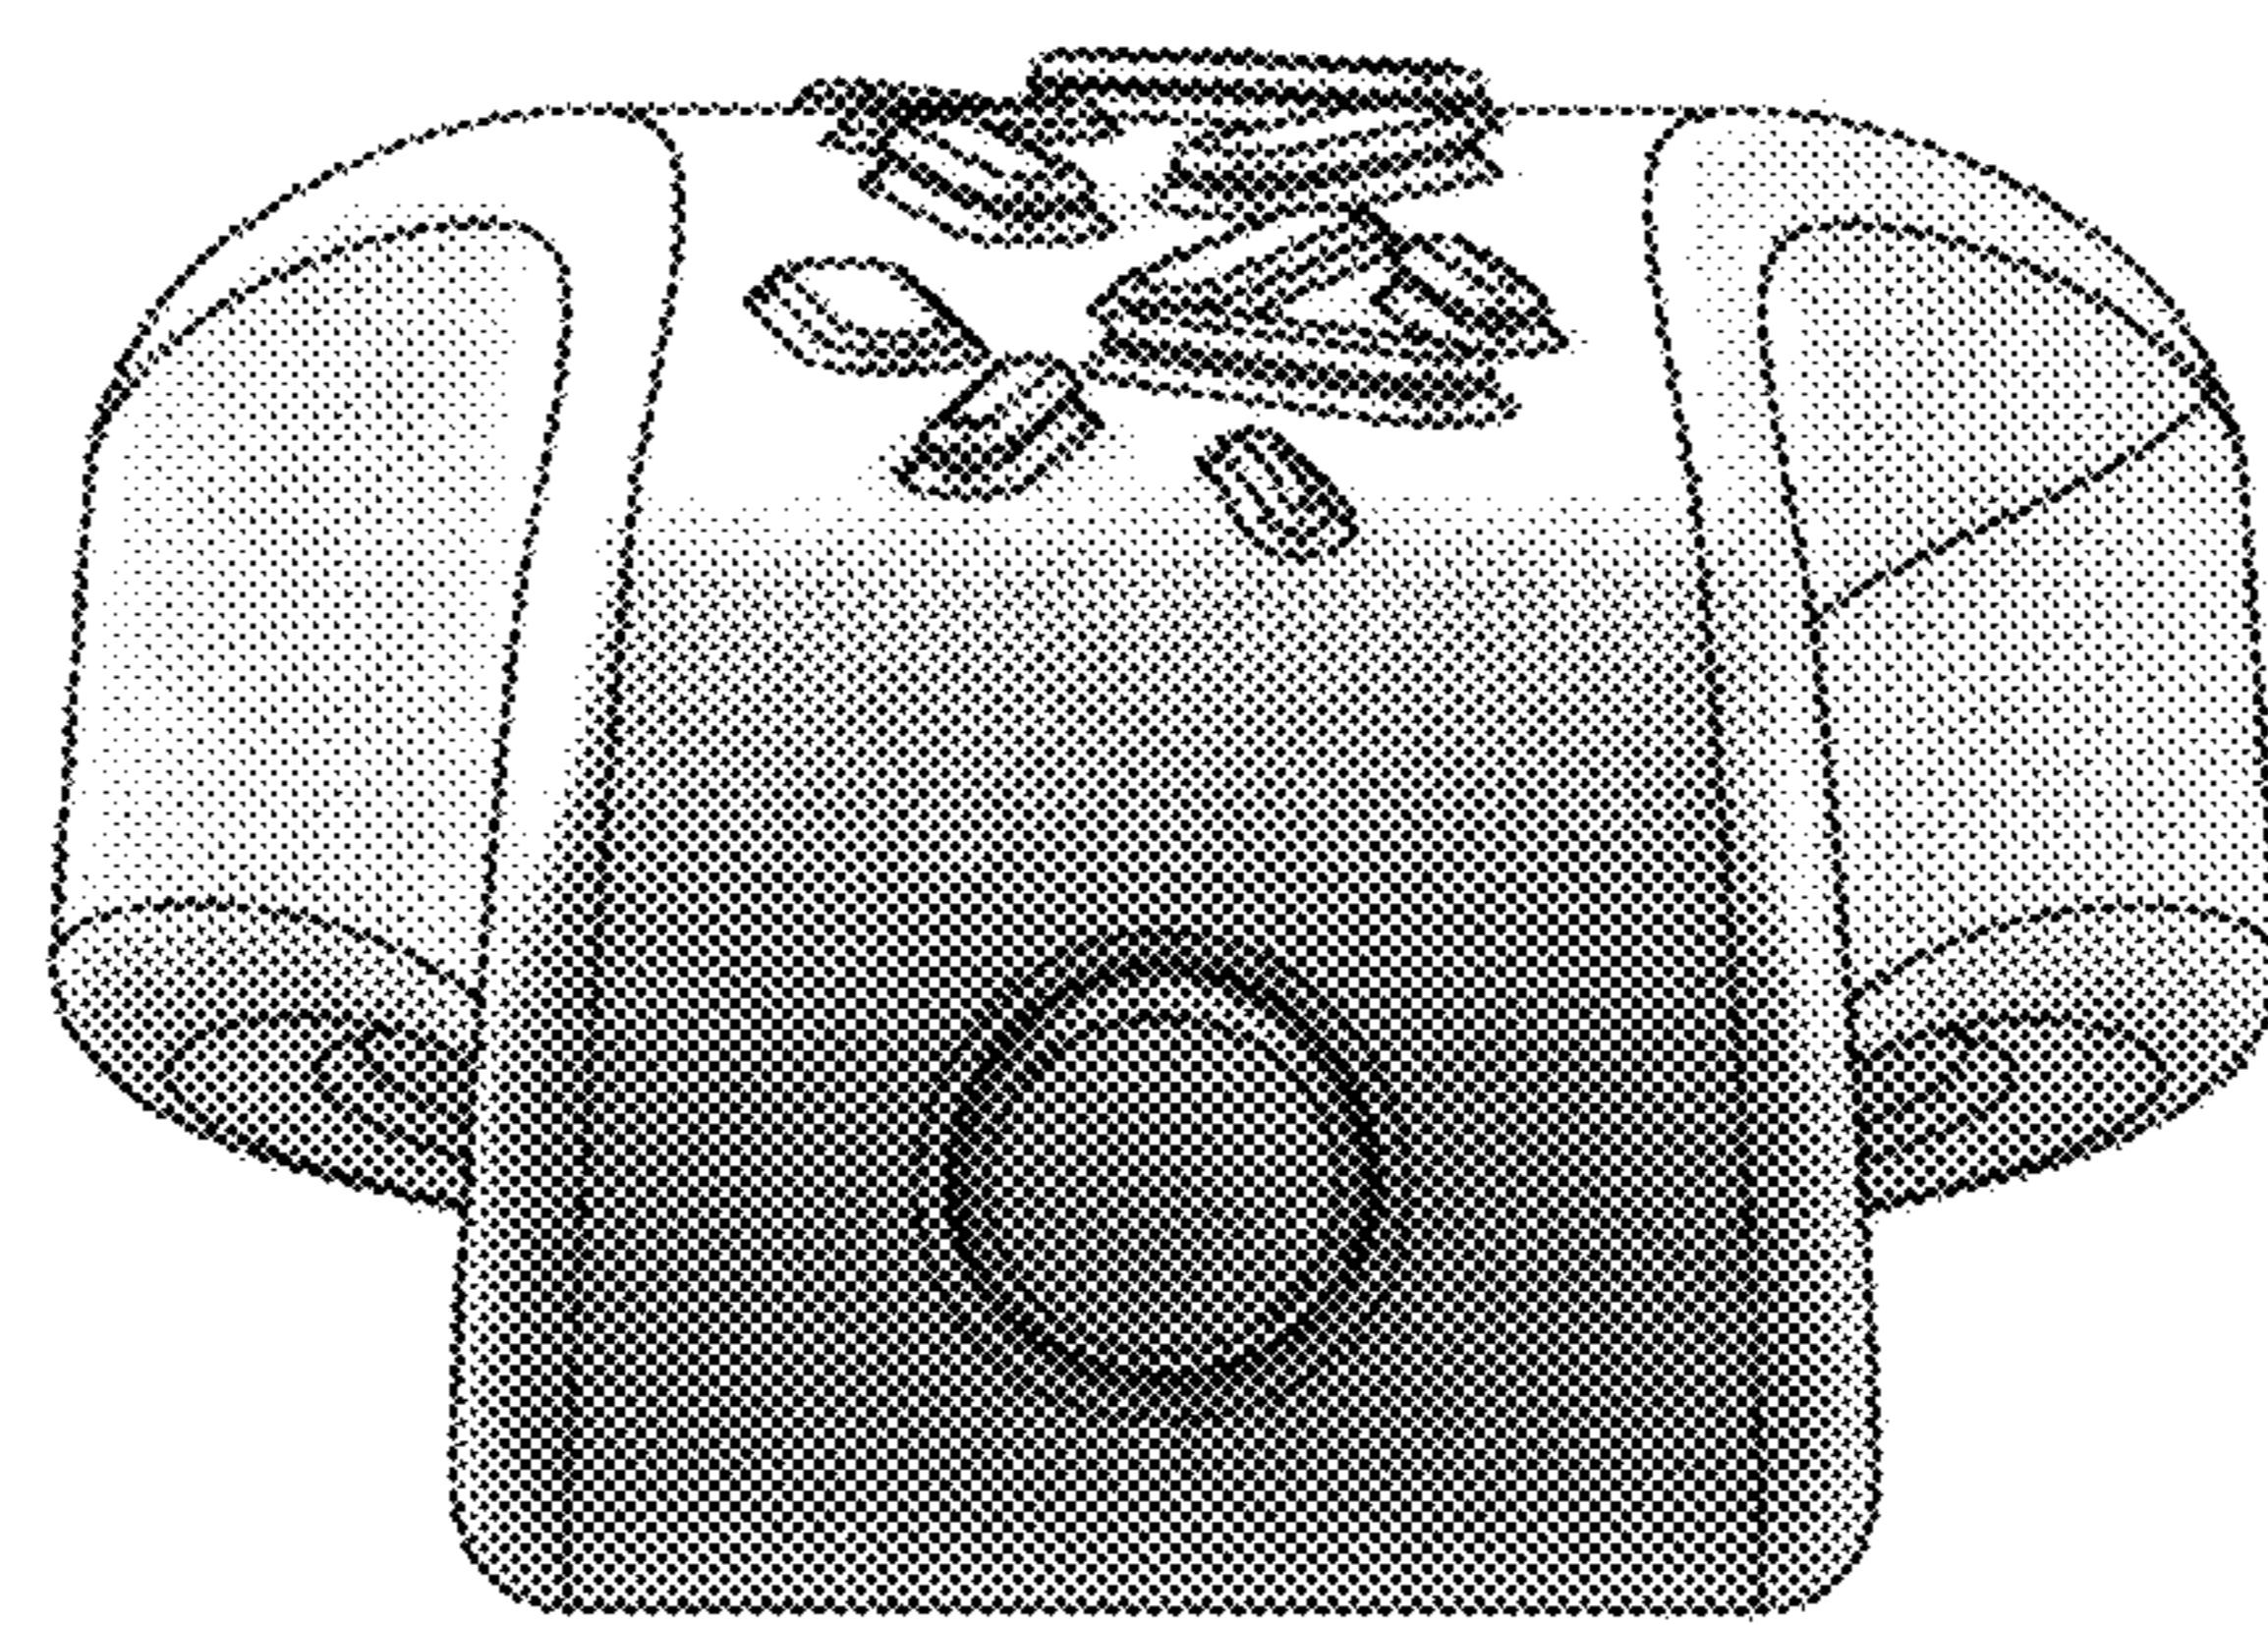

**FIG. 4**



**FIG. 5**