



US00D706443S

(12) **United States Design Patent**  
**Hahr et al.**

(10) **Patent No.:** **US D706,443 S**  
(45) **Date of Patent:** **\*\* Jun. 3, 2014**

- (54) **STIMULATION DEVICE**
- (71) Applicant: **Senses Toys Intellectual Property Management UG**, Bielefeld (DE)
- (72) Inventors: **Meike Hahr**, Hamburg (DE); **Heiko Tullney**, Hamburg (DE); **Till Muhl**, Hamburg (DE); **Thomas Milewski**, Halstenbek (DE)
- (73) Assignee: **Ovo Joint Venture LLC**, Pembroke Park, FL (US)

- (\*\*) Term: **14 Years**
- (21) Appl. No.: **29/448,007**
- (22) Filed: **Mar. 8, 2013**

- (30) **Foreign Application Priority Data**  
Sep. 10, 2012 (EM) ..... 001342935-0055
- (51) **LOC (10) Cl.** ..... **28-03**
- (52) **U.S. Cl.**  
USPC ..... **D24/215**
- (58) **Field of Classification Search**  
USPC ..... D24/200, 211, 212, 213, 214, 215;  
601/114, 120, 121, 124, 125, 130, 131,  
601/134, 135, 136, 137  
See application file for complete search history.

- (56) **References Cited**  
U.S. PATENT DOCUMENTS  
D350,397 S \* 9/1994 Bruno et al. .... D24/214  
D648,861 S \* 11/2011 Chong et al. .... D24/215  
D652,943 S \* 1/2012 Chong et al. .... D24/215


D653,349 S \* 1/2012 Chong et al. .... D24/215  
\* cited by examiner  
*Primary Examiner* — Sandra Snapp  
(74) *Attorney, Agent, or Firm* — Merek, Blackmon & Voorhees, LLC

(57) **CLAIM**  
The ornamental design for a stimulation device, as shown and described.

**DESCRIPTION**

FIG. 1 is a top plan view of a stimulation device showing the design;  
FIG. 2 is a perspective view taken from the bottom, rear and left side of the stimulation device of FIG. 1, the opposite side being a mirror image thereof;  
FIG. 3 is a right side elevation view of the stimulation device of FIG. 1, the left side elevation view being a mirror image thereof;  
FIG. 4 is a rear elevation view of the stimulation device of FIG. 1; and,  
FIG. 5 is a perspective view taken from the top and left side of the stimulation device of FIG. 1, the opposite side being a mirror image thereof.  
A perspective view taken from the bottom, rear and right side of the stimulation device of FIG. 1 at an angle corresponding to the angle of the perspective view of FIG. 2 is a mirror image of FIG. 2.  
The left side elevation of the stimulation device of FIG. 1 is a mirror image of the right side elevation shown in FIG. 3, except for the ridges on the top.  
A perspective view taken from the top and right side of the stimulation device of FIG. 1 at an angle corresponding to the angle of the perspective view of FIG. 5 is a mirror image of FIG. 5, except for the ridges on the top.

**1 Claim, 5 Drawing Sheets**

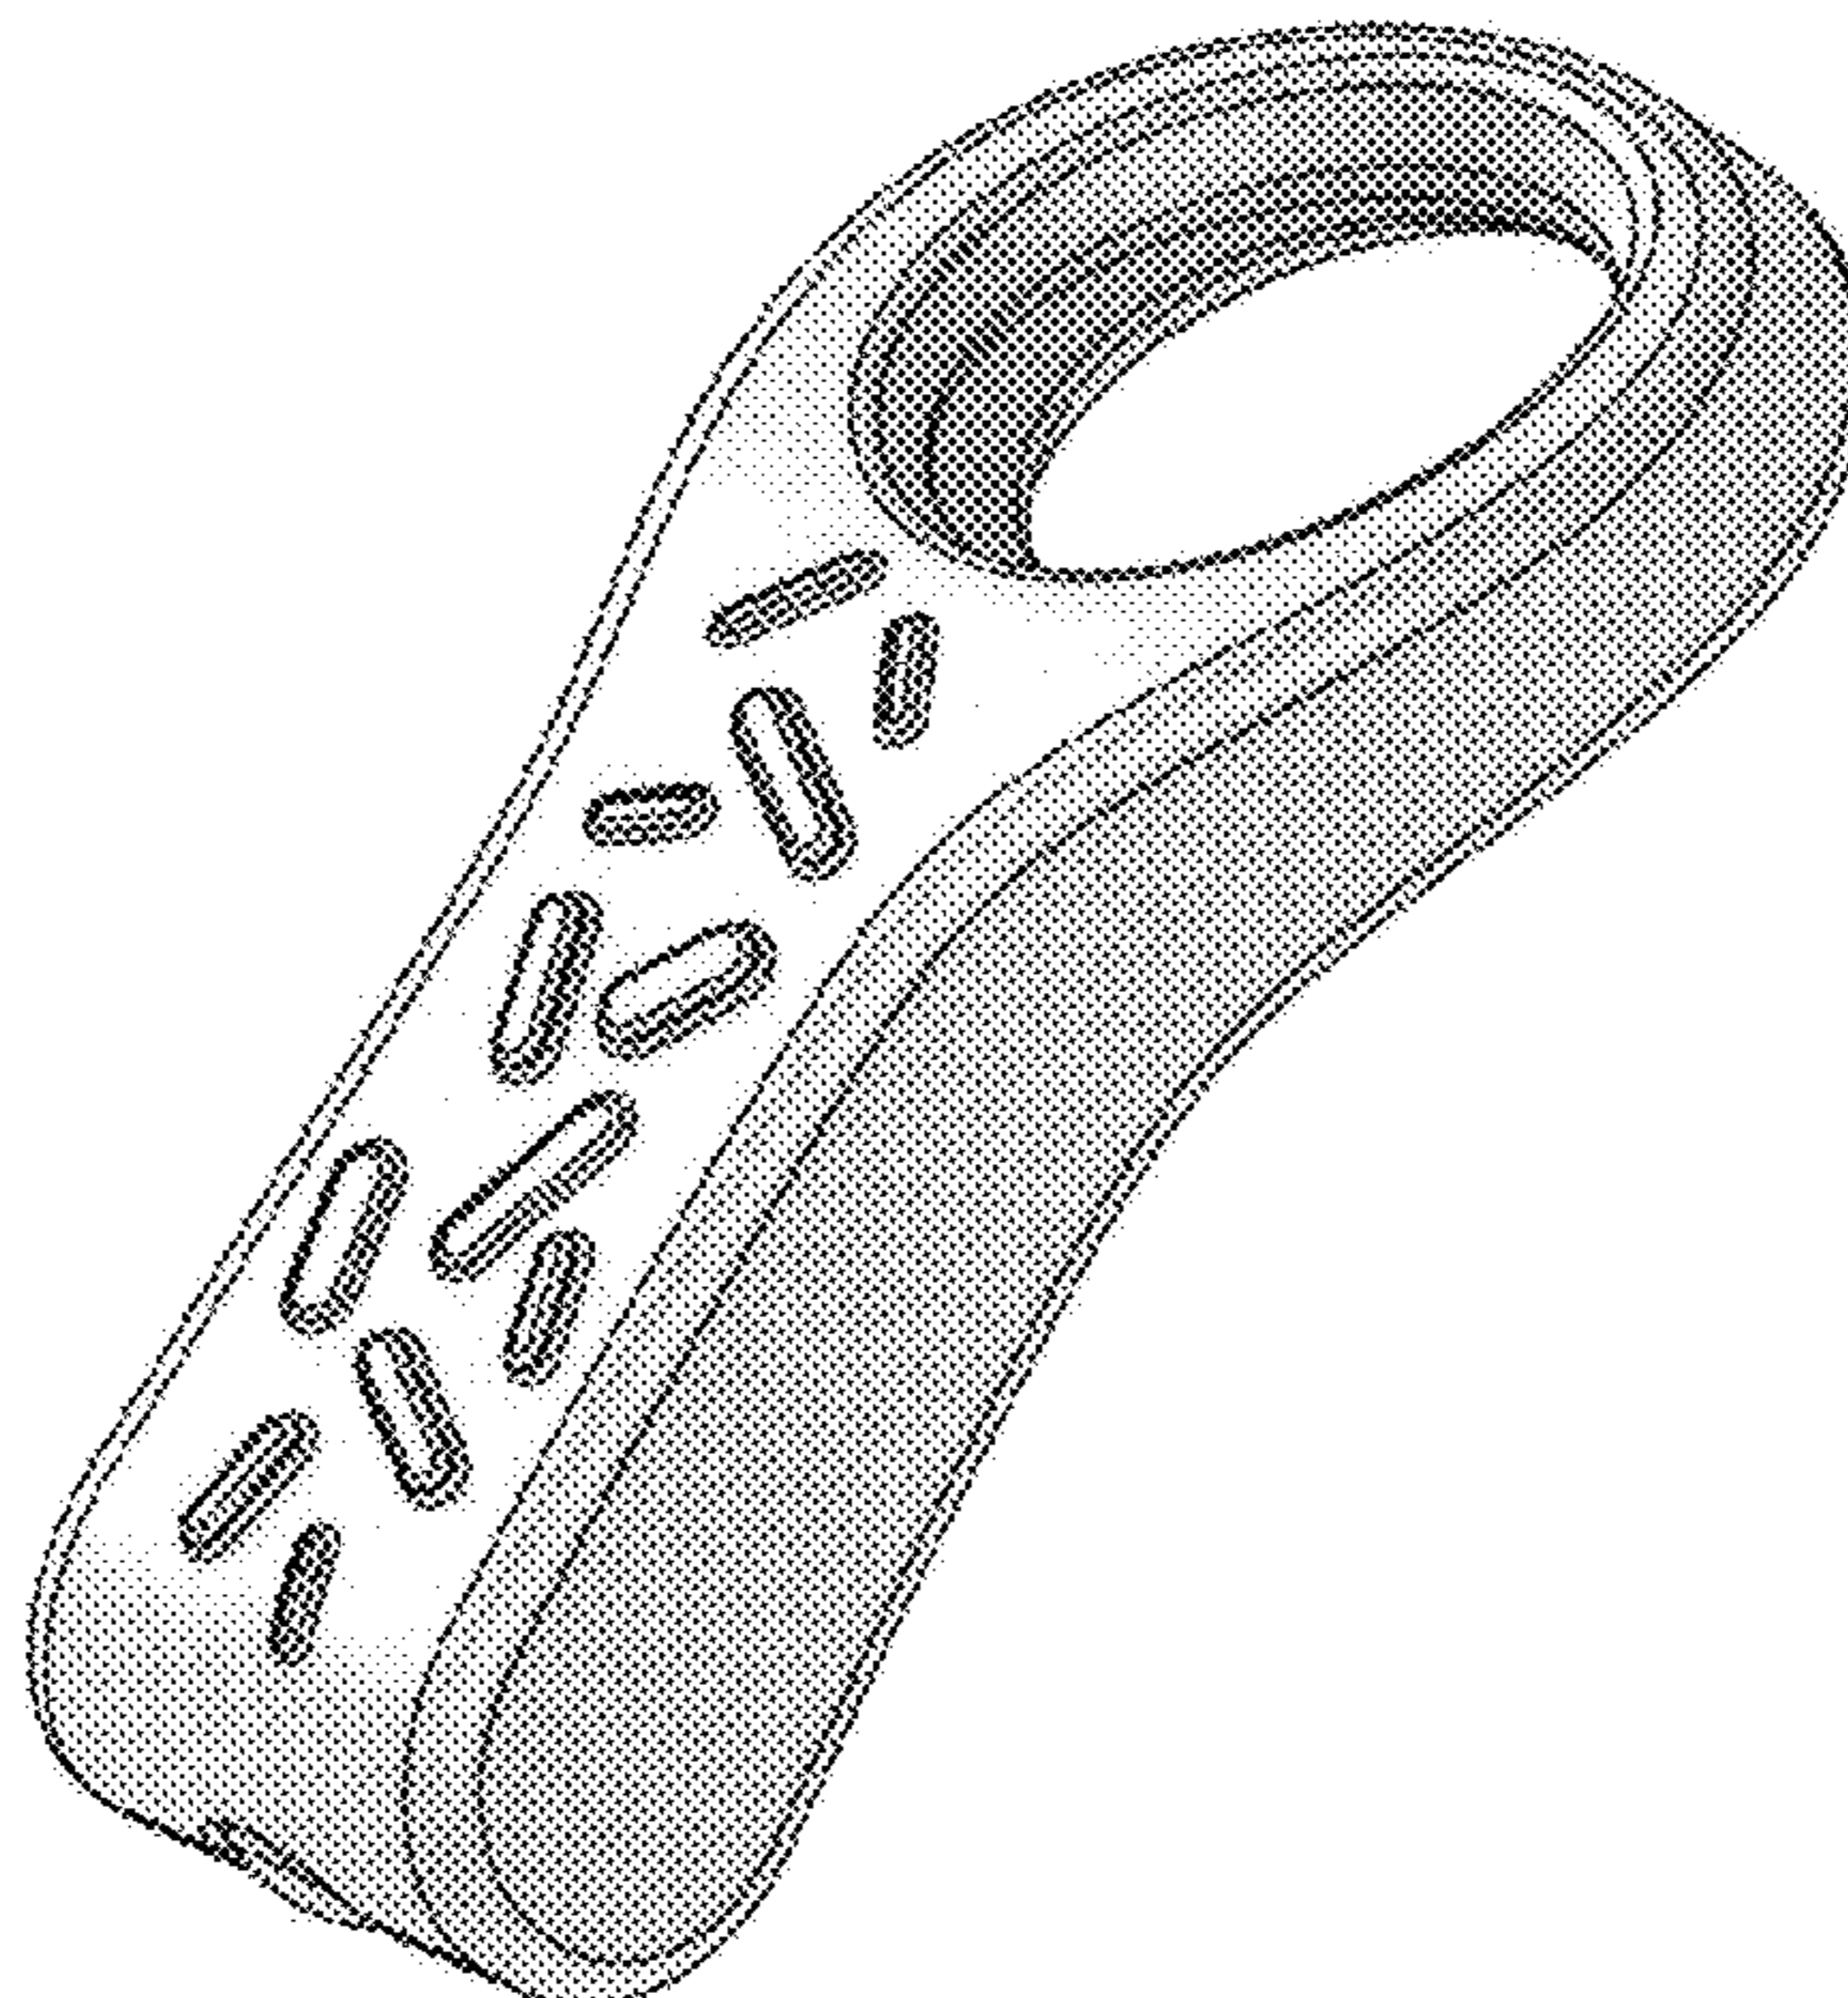

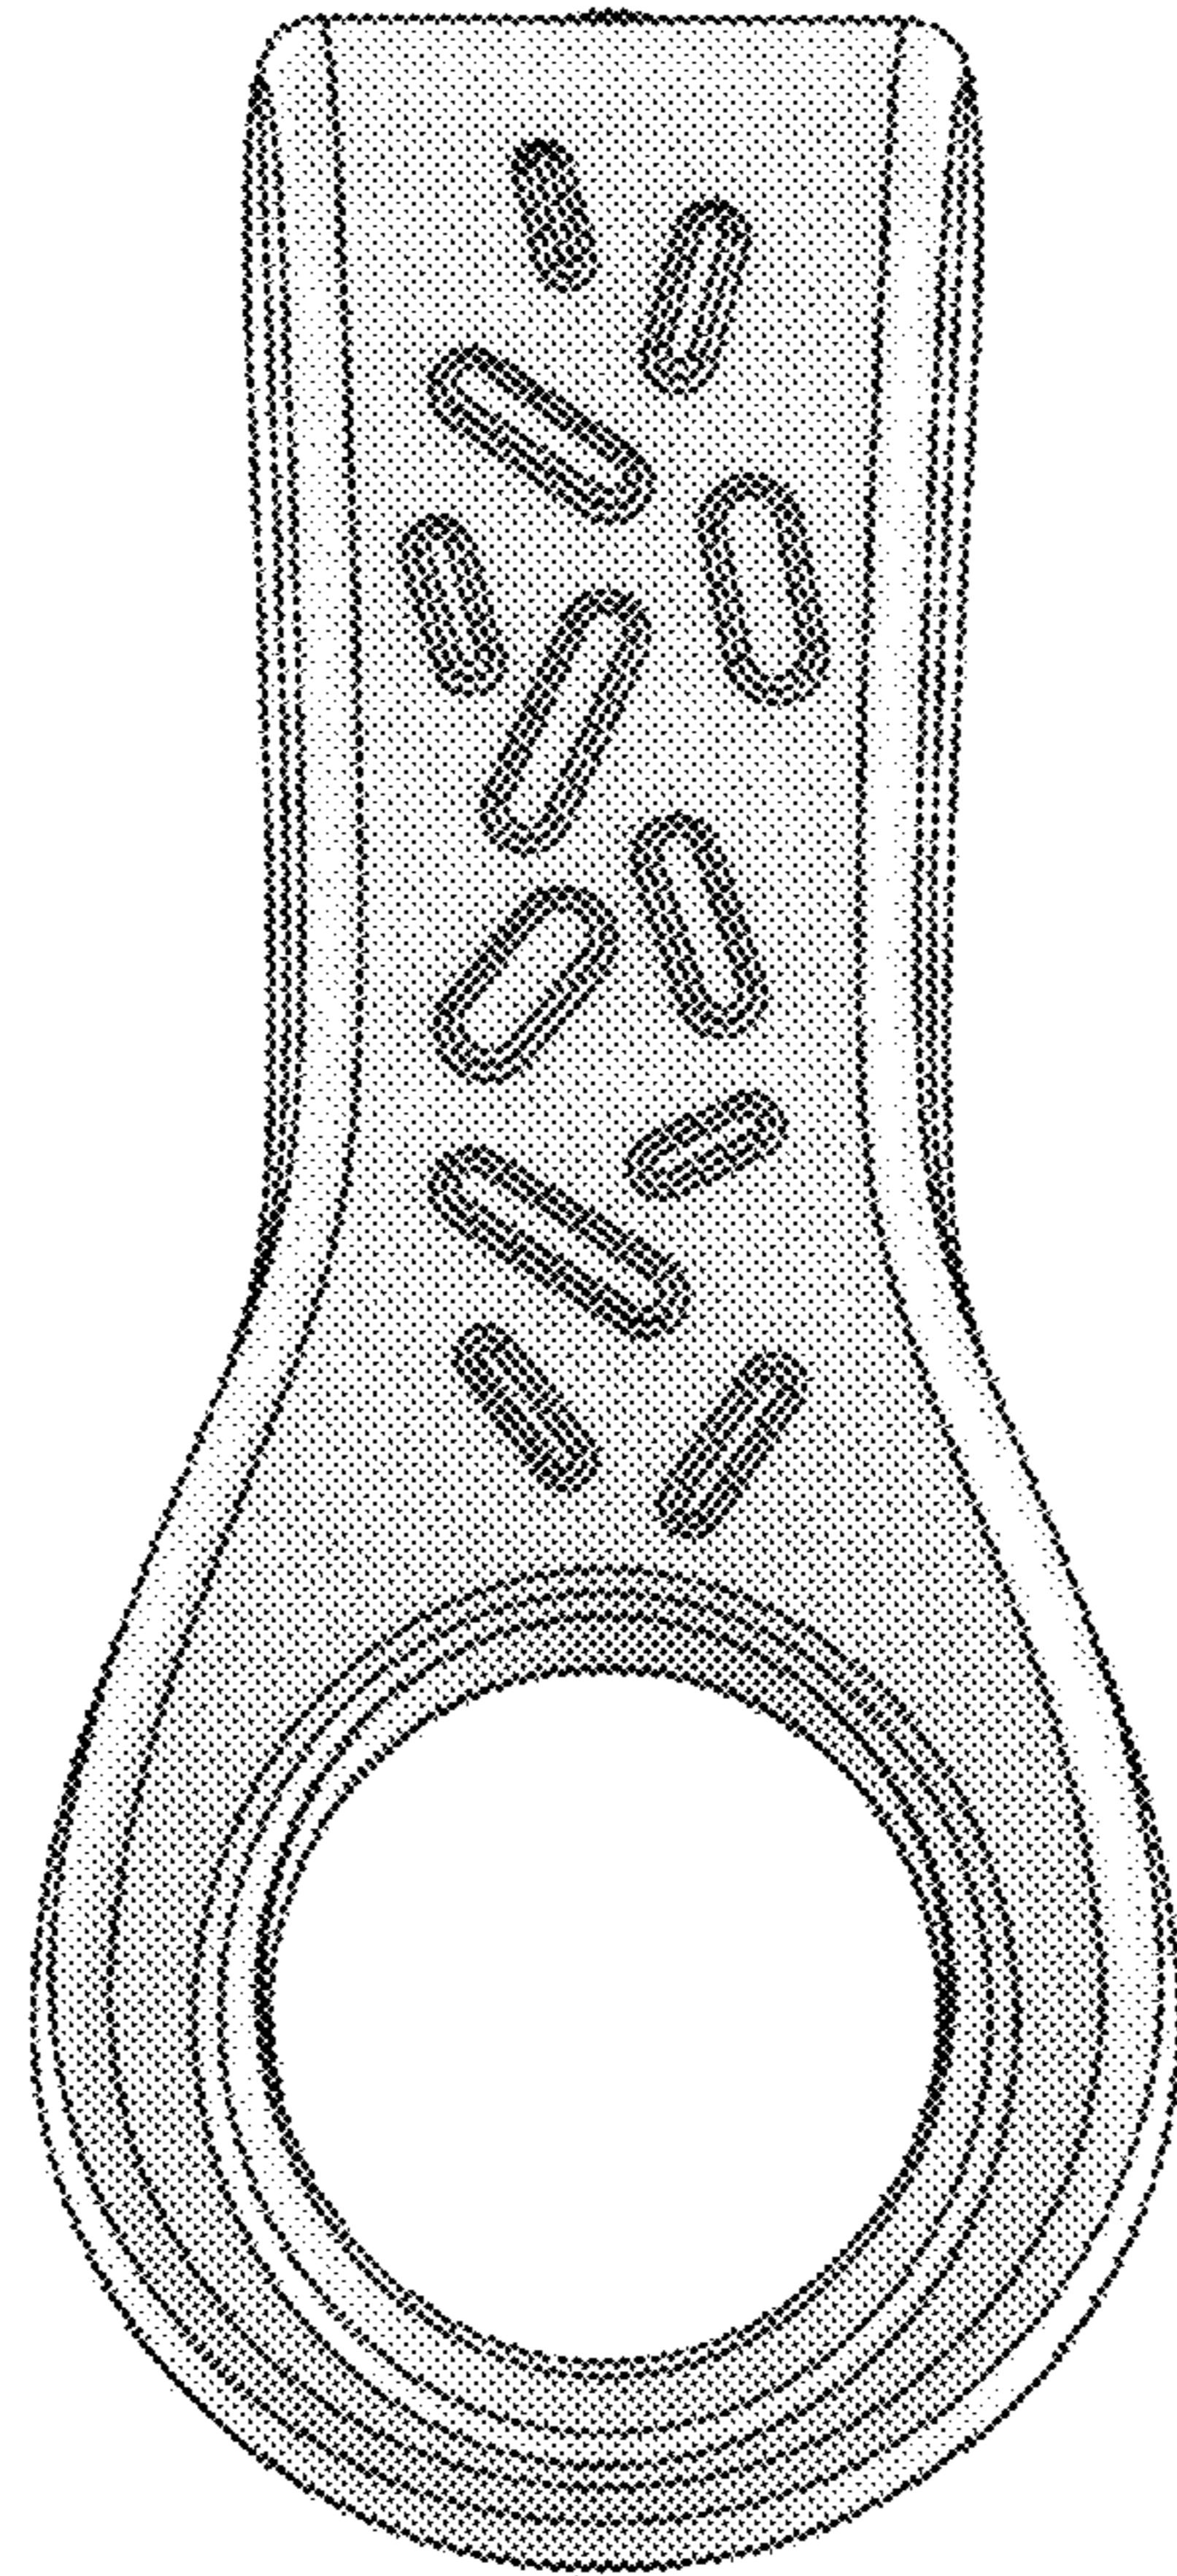


FIG. 1

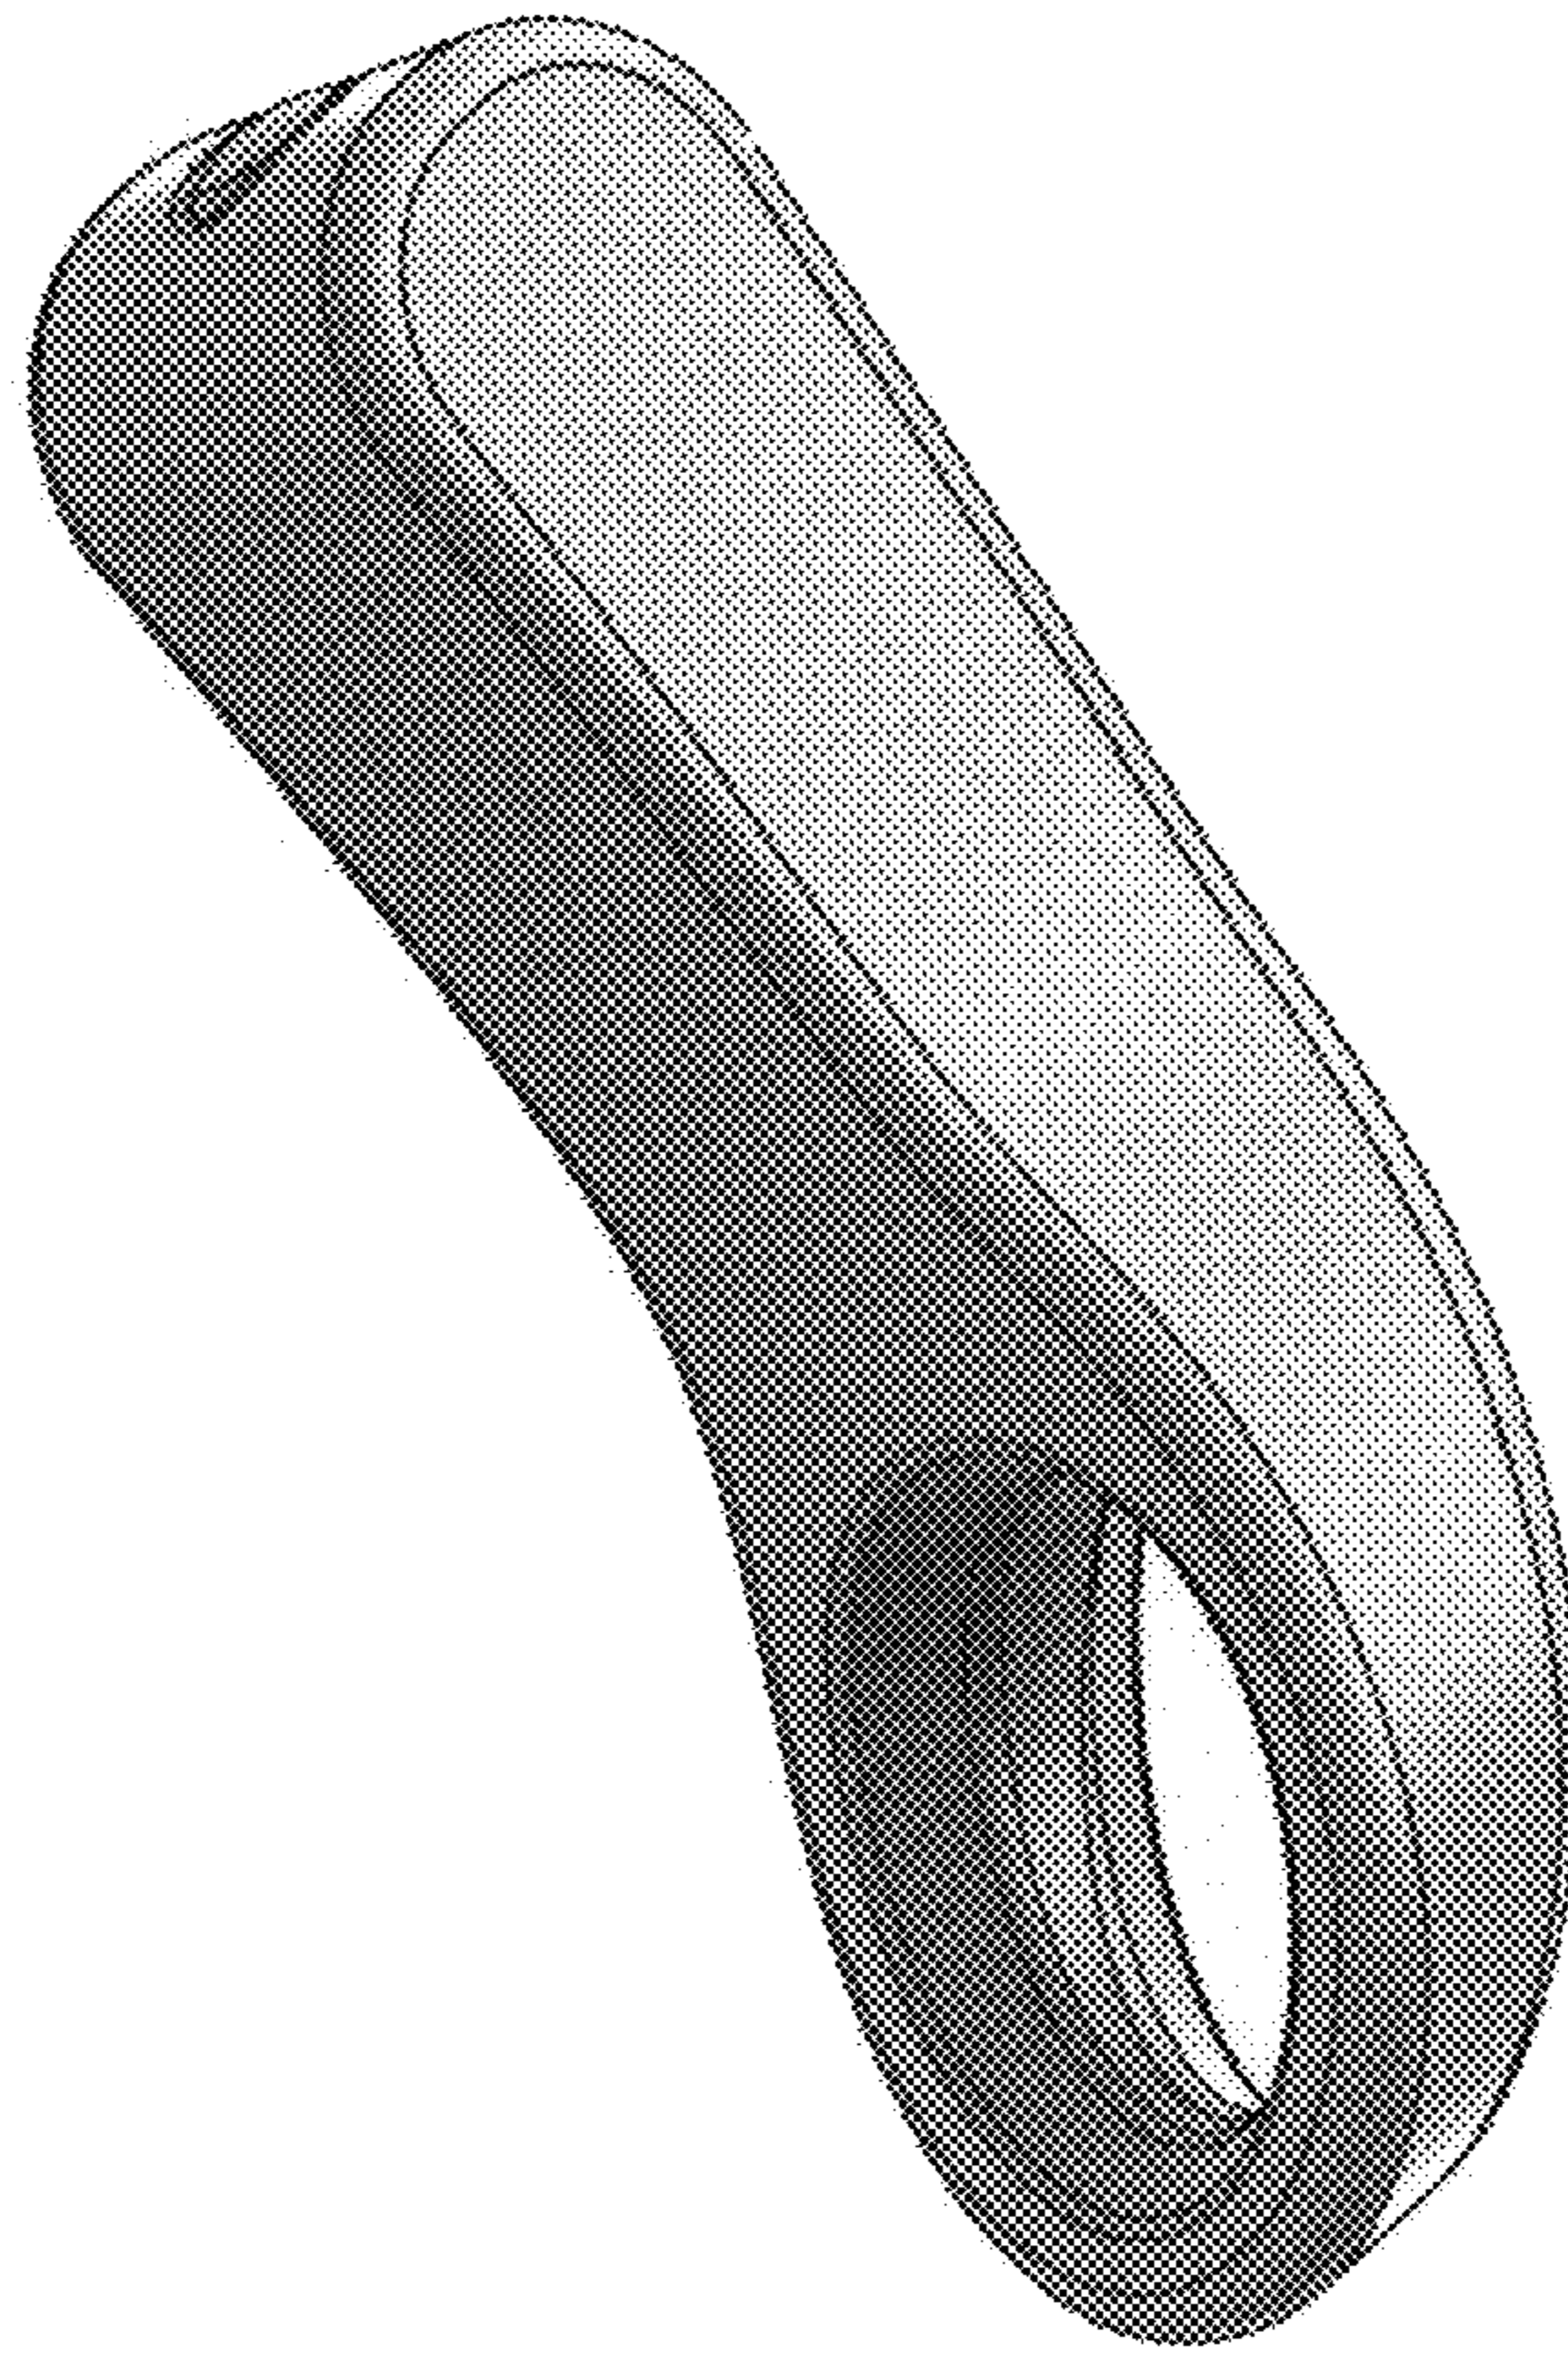


FIG. 2

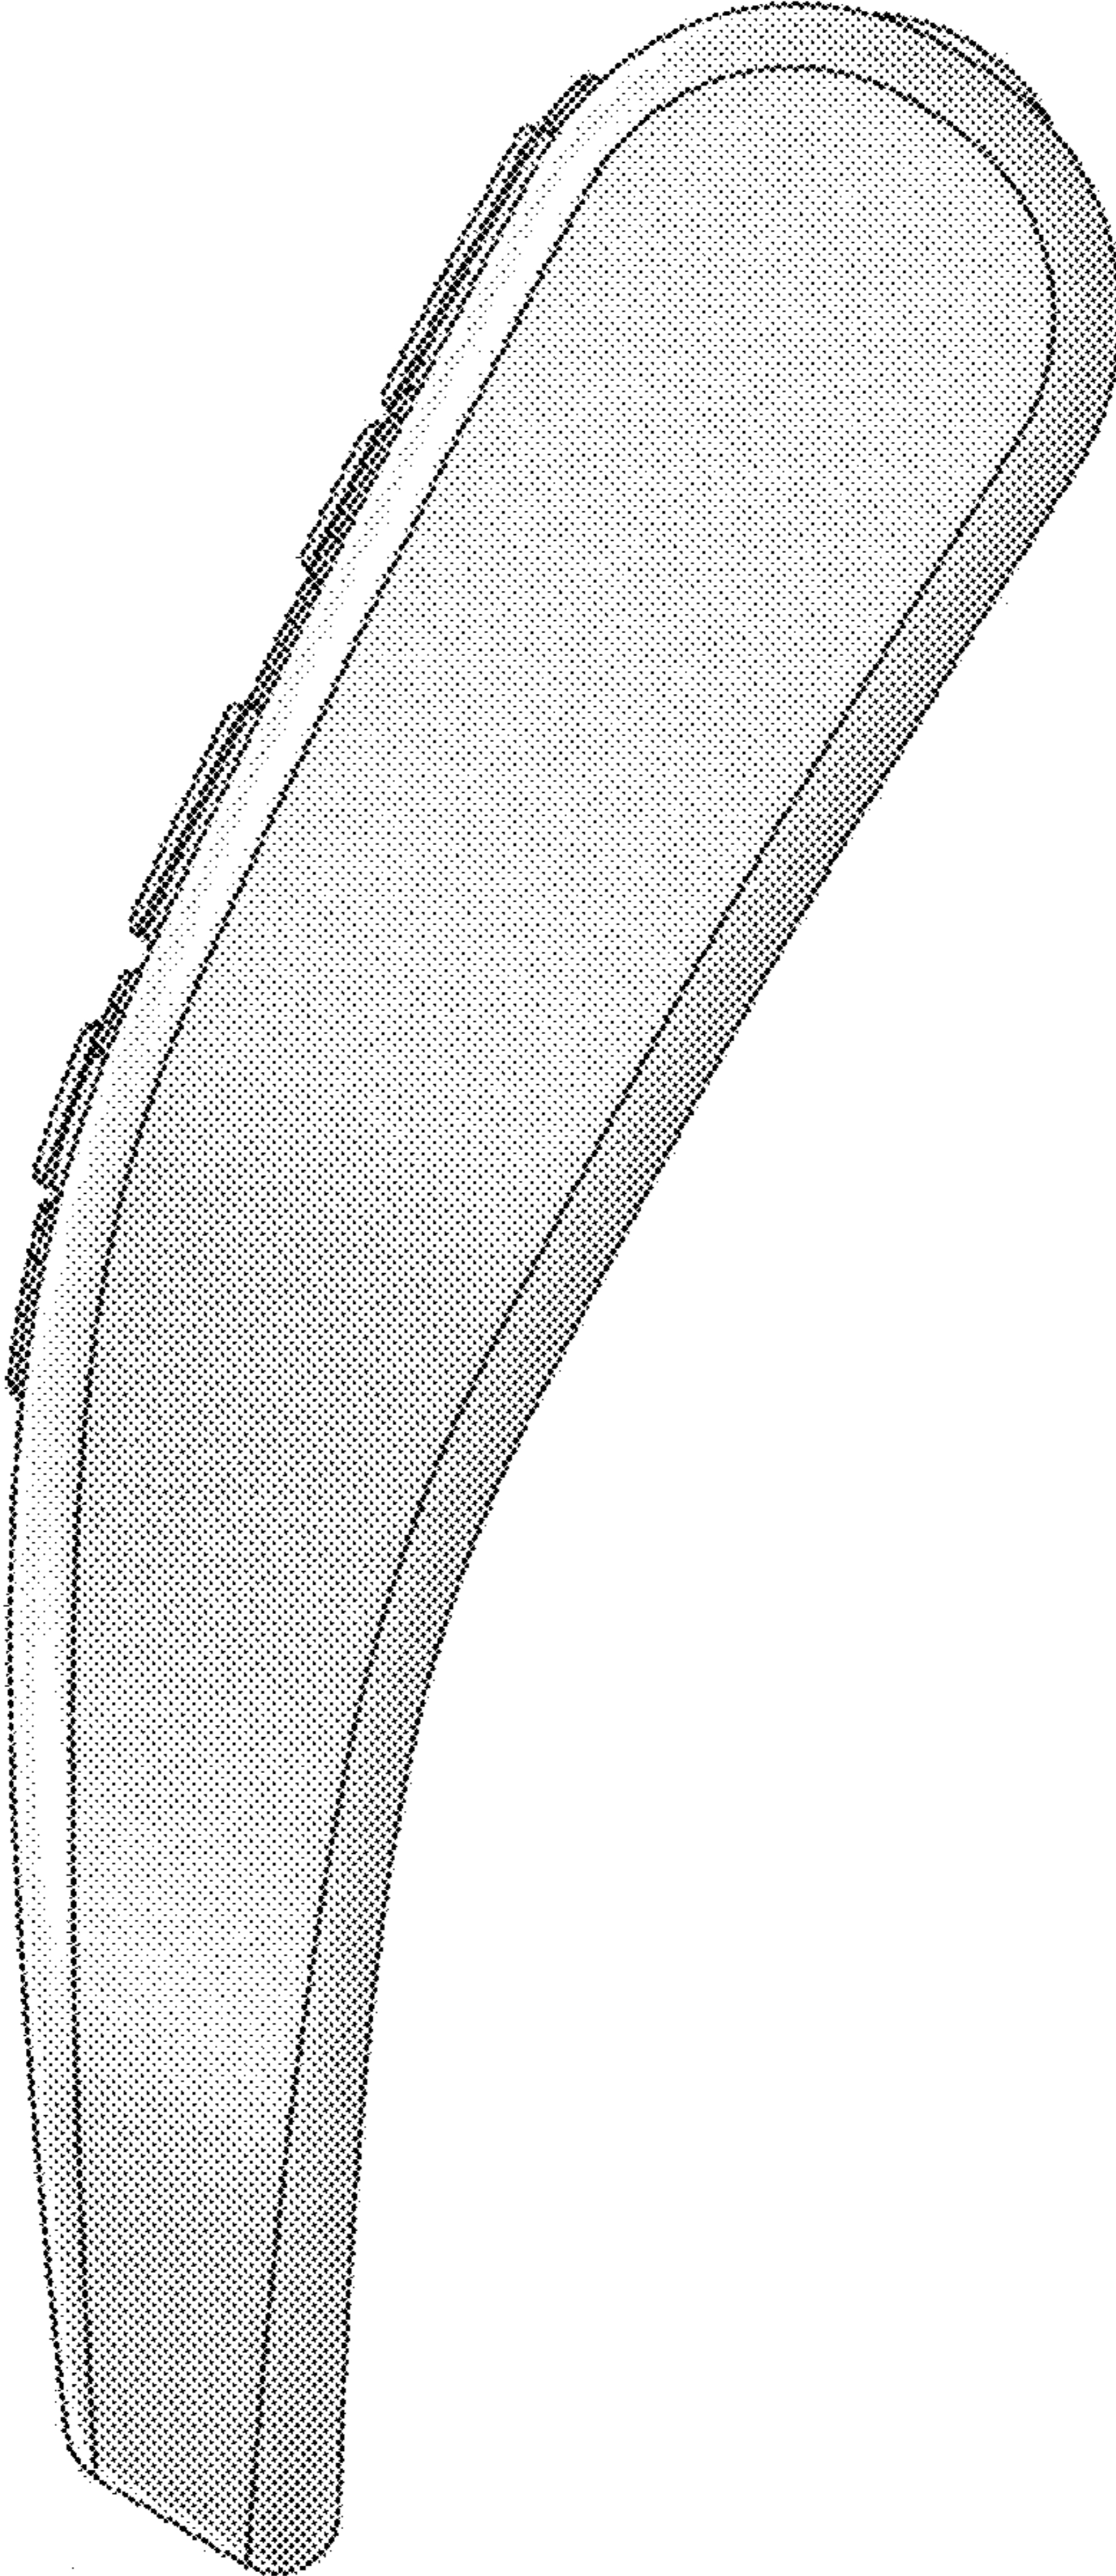


FIG. 3

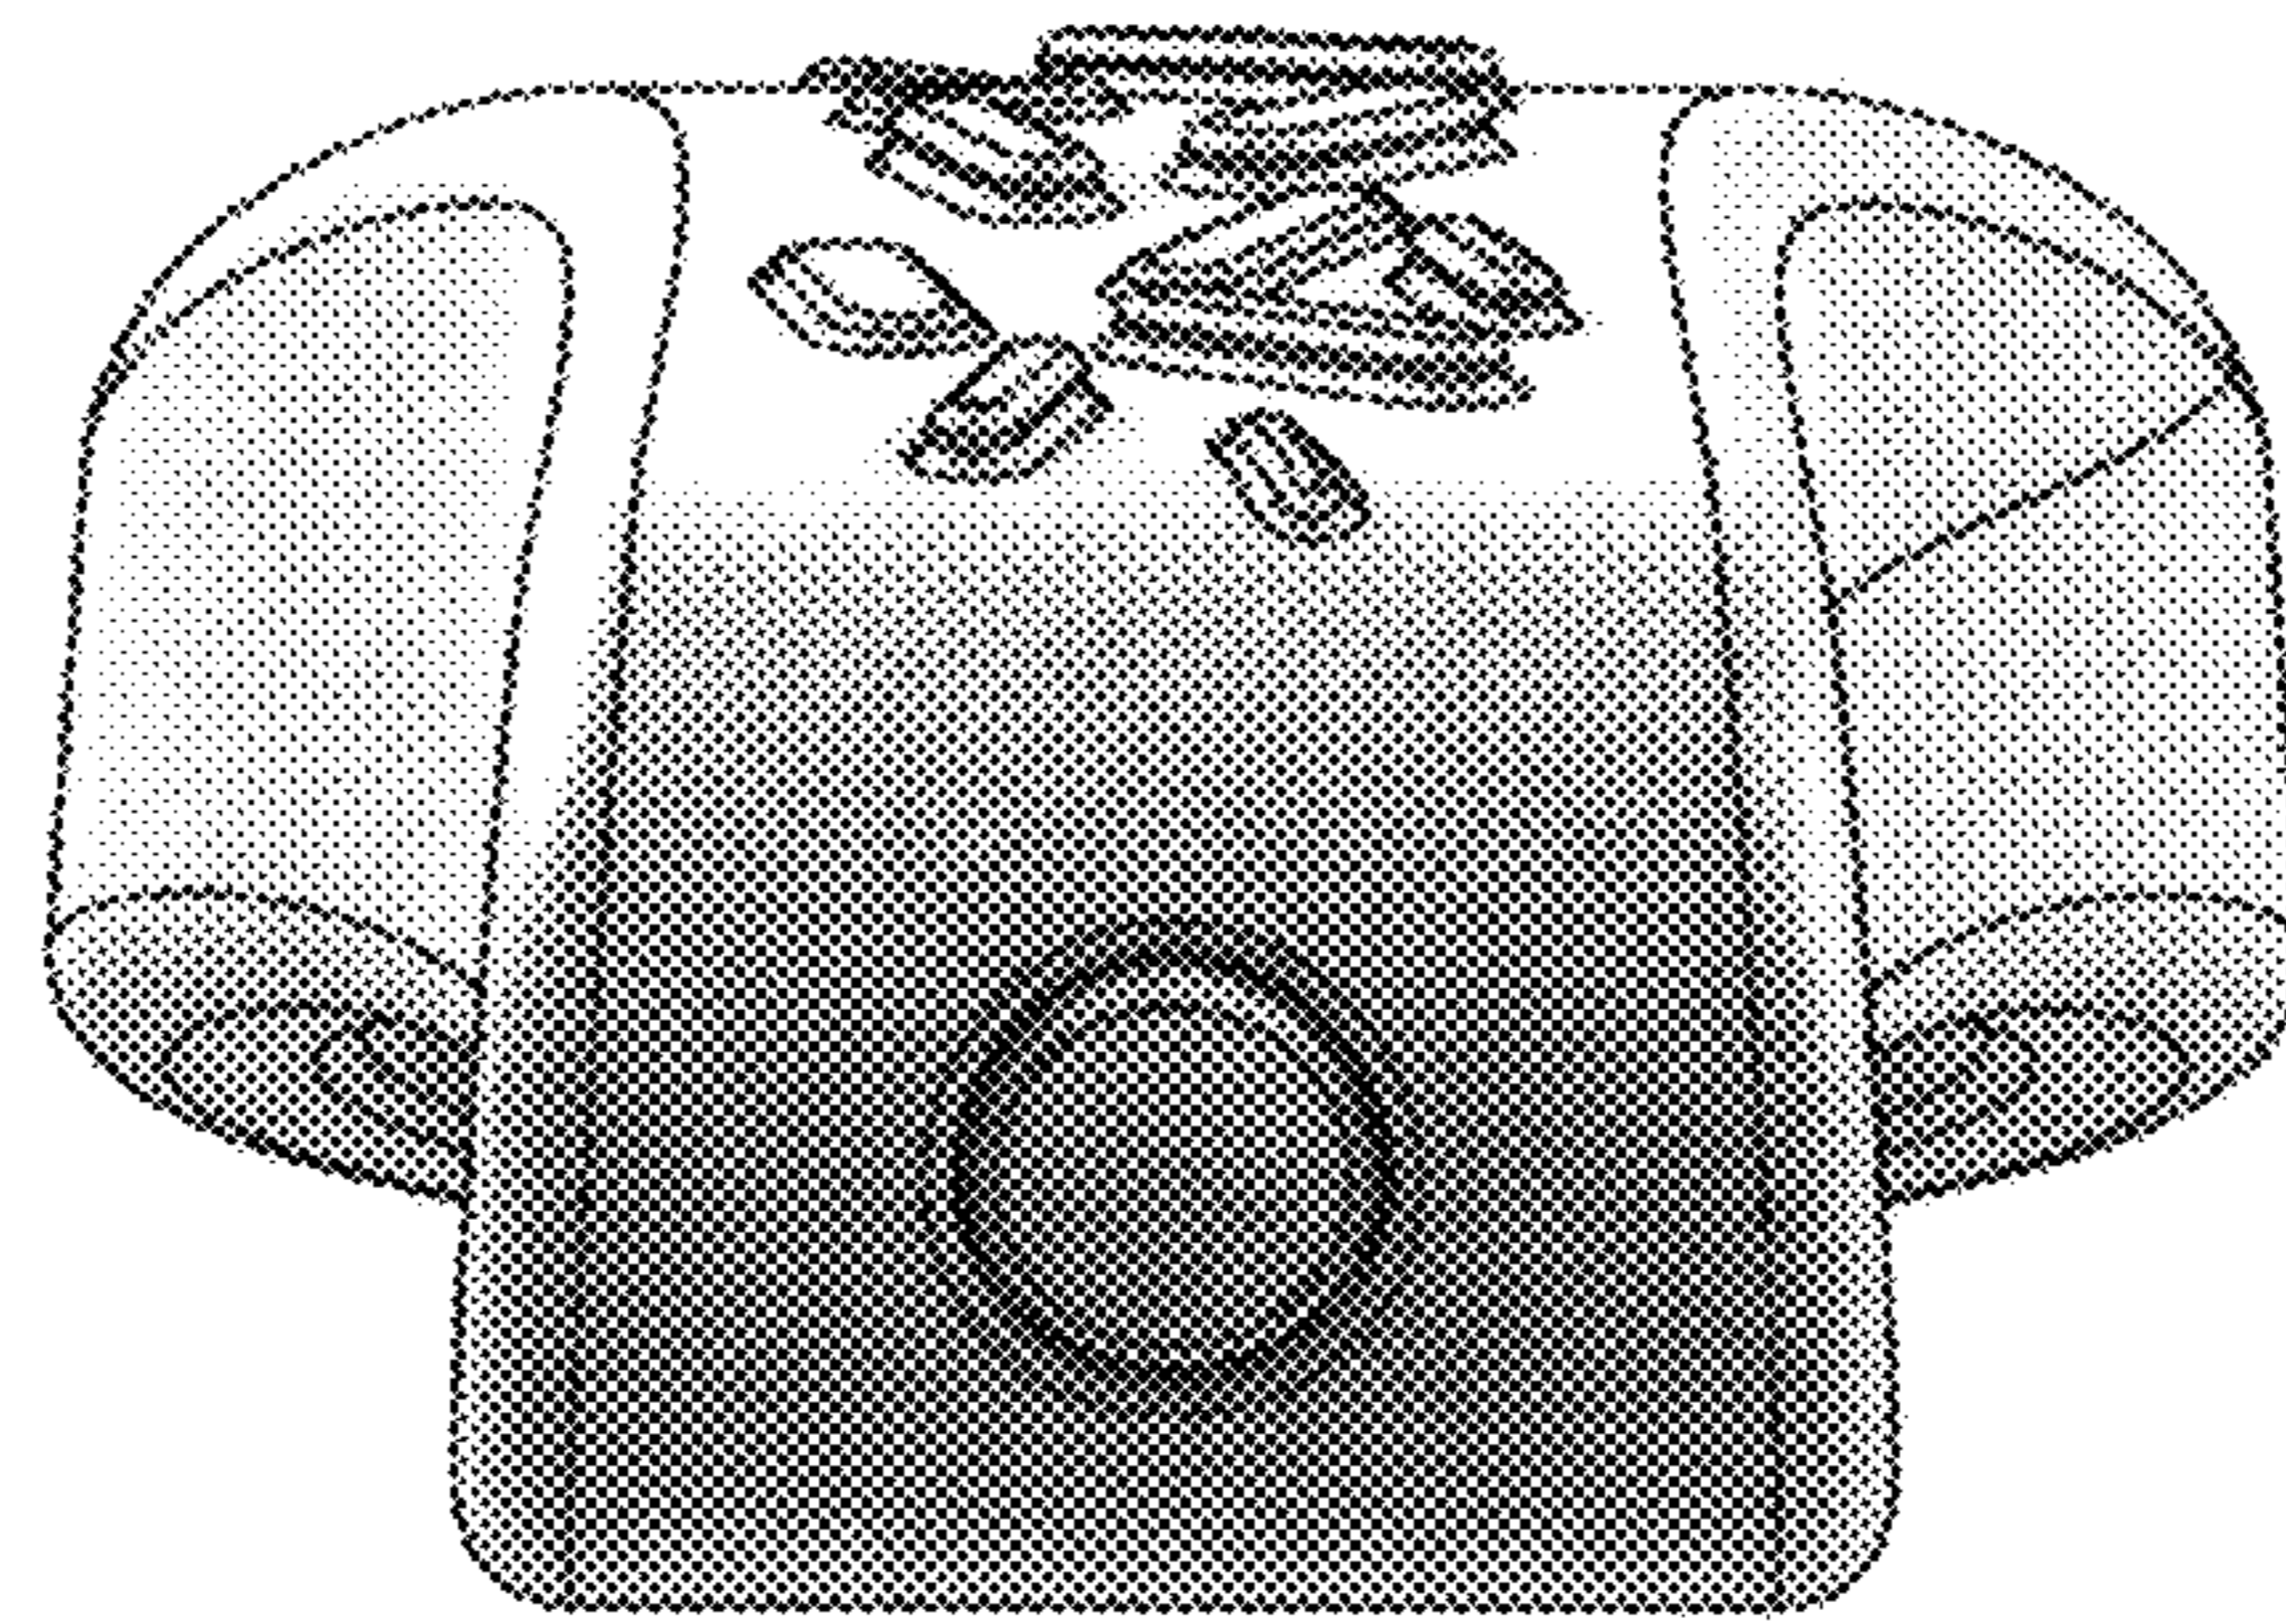


FIG. 4



FIG. 5