



US00D707844S

(12) **United States Design Patent**  
**Hilbey**

(10) **Patent No.:** **US D707,844 S**  
(45) **Date of Patent:** **\*\* Jun. 24, 2014**

(54) **DEVICE FOR MICROBIOLOGICAL ANALYSIS**

(71) Applicant: **AES Chemunex Société Anonyme à conseil d'administration**, Combourg (FR)

(72) Inventor: **Serge Hilbey**, Nantes (FR)

(73) Assignee: **bioMérieux**, Marcy l'Etoile (FR)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/453,201**

(22) Filed: **Apr. 26, 2013**

(51) **LOC (10) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/216**

(58) **Field of Classification Search**  
USPC ..... D24/216, 217, 219, 223, 231, 232, 233, D24/107, 169, 186; D10/81; 422/500, 547, 422/62-65, 67; 435/287.1, 287.3; 436/43, 436/45, 47

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D508,999	S	*	8/2005	Fanning et al.	.....	D24/216
D535,403	S	*	1/2007	Isozaki et al.	.....	D24/232
D588,276	S	*	3/2009	Isozaki et al.	.....	D24/232
D653,764	S	*	2/2012	Macemon et al.	.....	D24/216
D676,976	S	*	2/2013	Walsh et al.	.....	D24/216
D687,963	S	*	8/2013	Perpect	.....	D24/216

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Winstead PC


(57) **CLAIM**

The ornamental design for a device for microbiological analysis, as shown and described.

**DESCRIPTION**

FIG. 1 is a front perspective view of a device for microbiological analysis in accordance with the design; FIG. 2 is a front view thereof; FIG. 3 is a back view thereof; FIG. 4 is a left side view thereof; FIG. 5 is a top plan view thereof; and, FIG. 6 is a rear perspective view thereof. Any broken lines present in the drawings are for illustrative purposes only and form no part of the design to be patented.

**1 Claim, 6 Drawing Sheets**

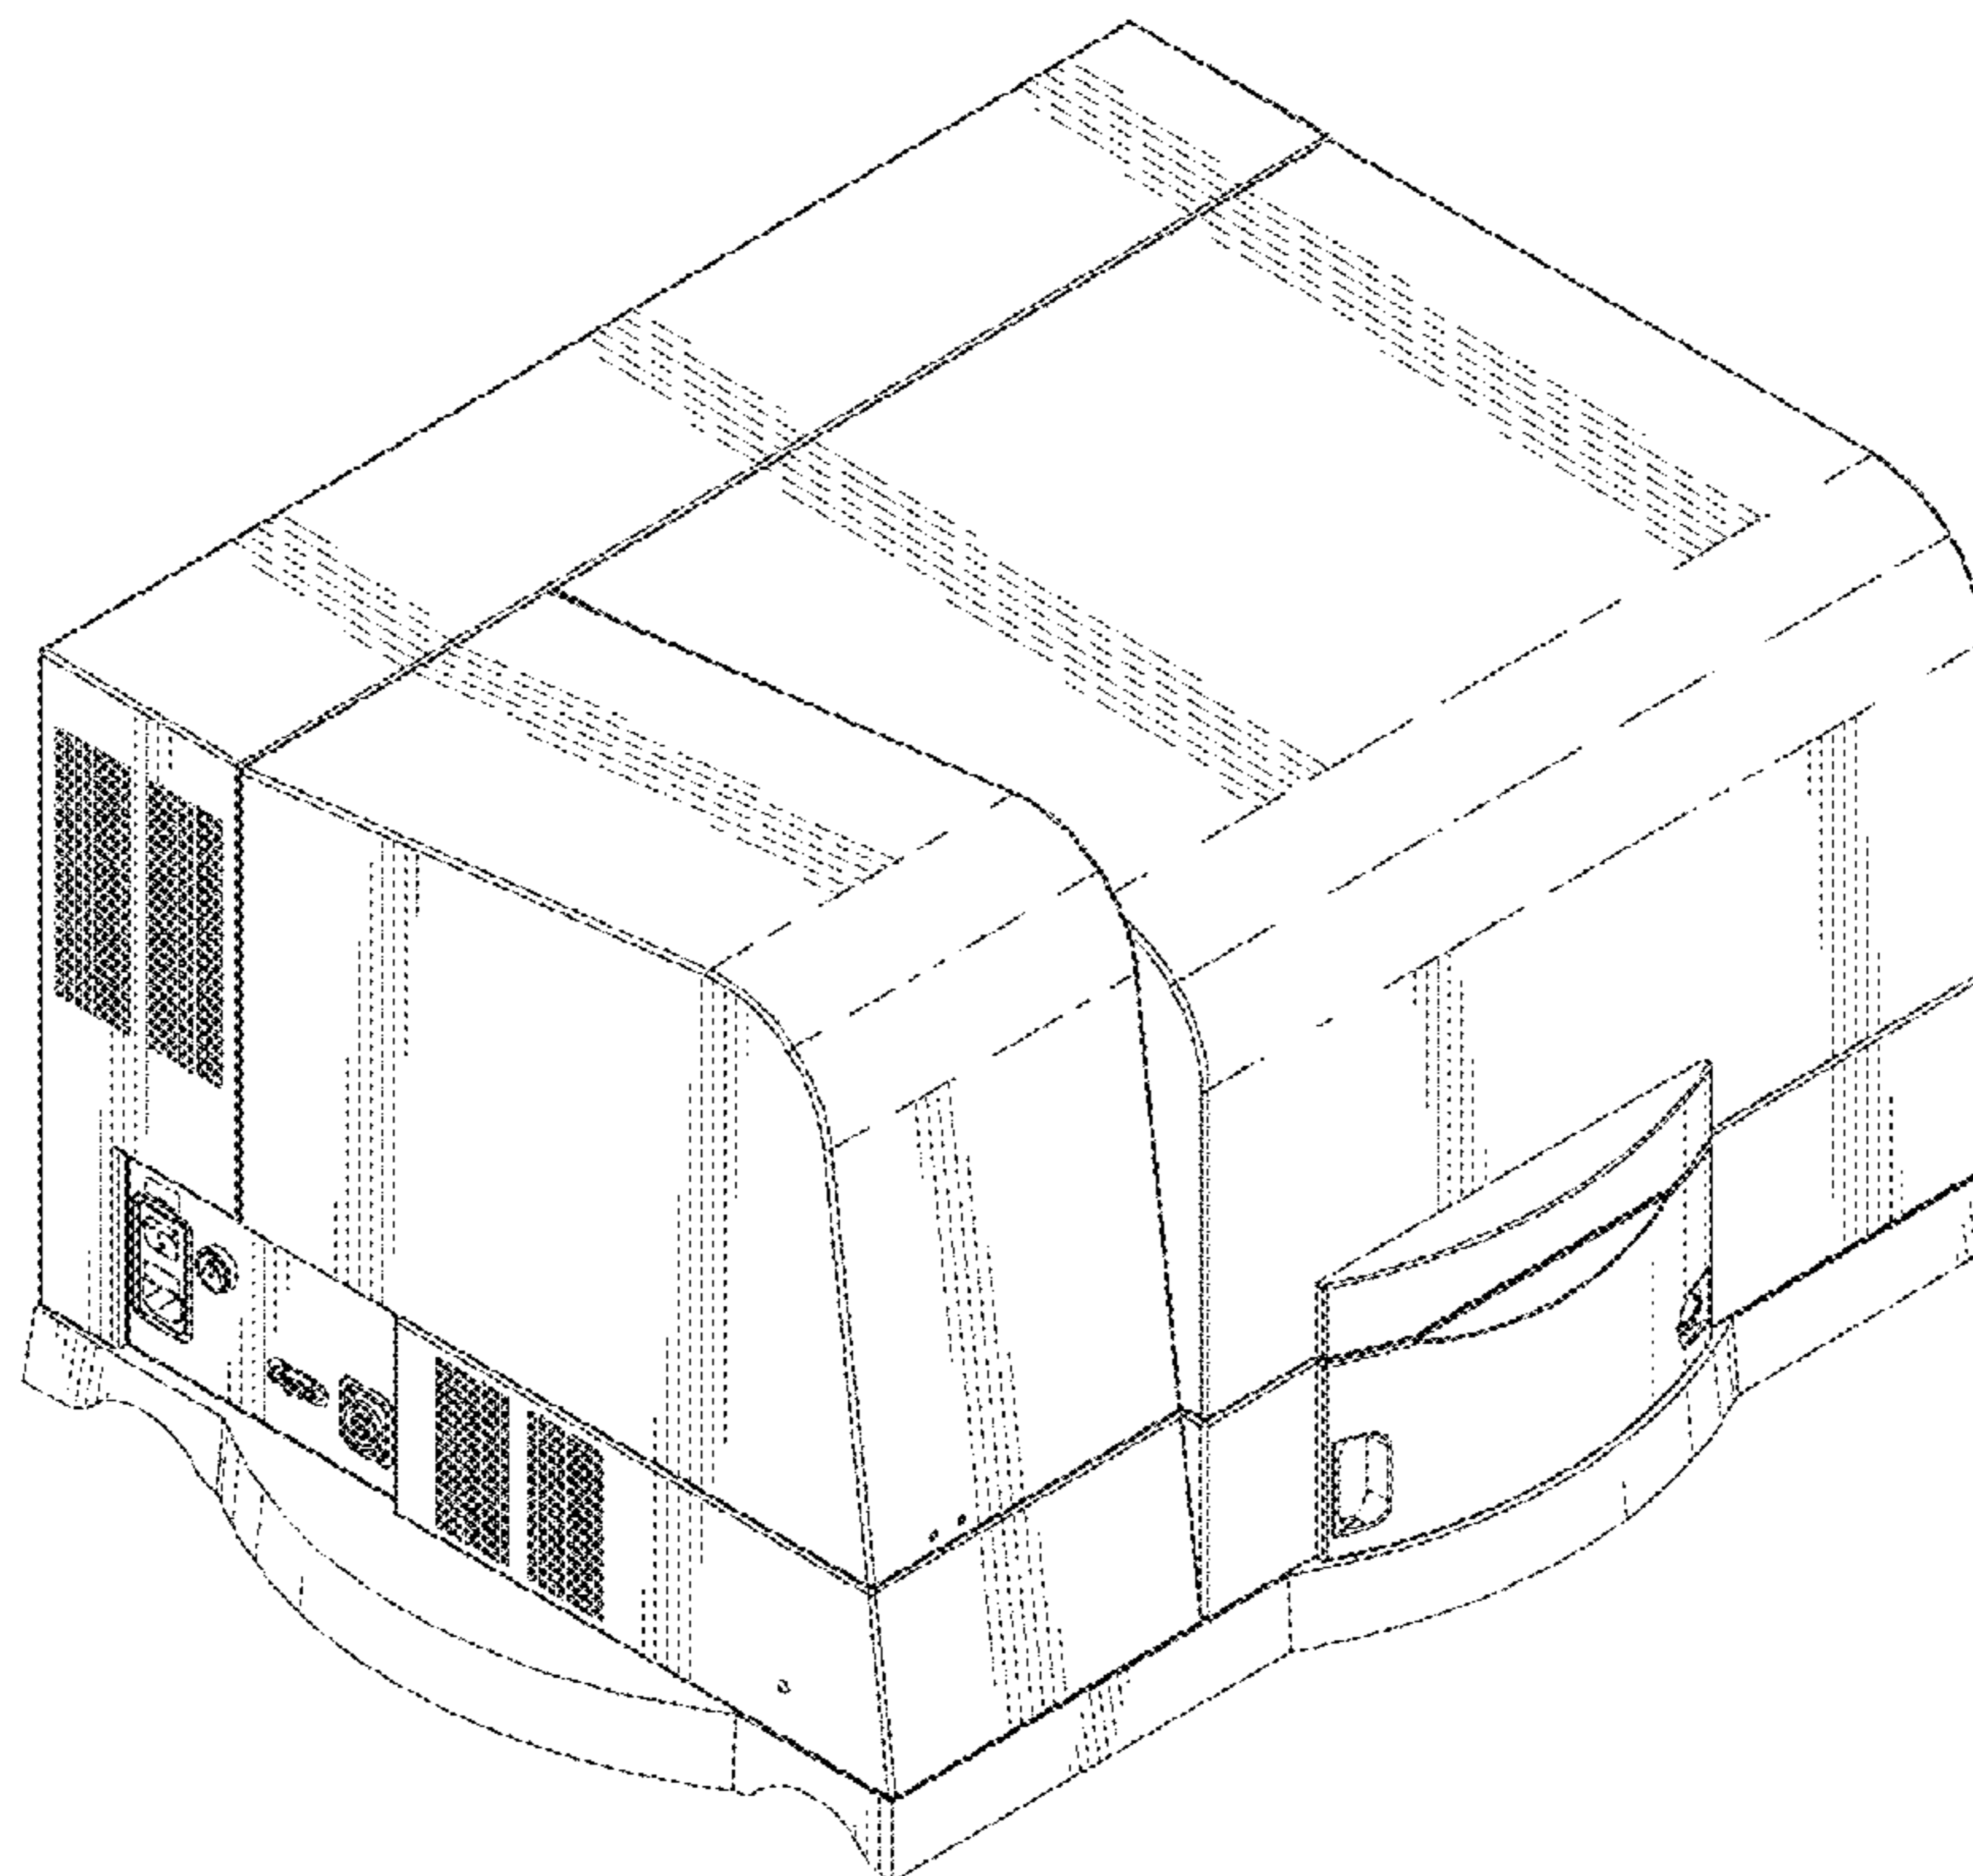

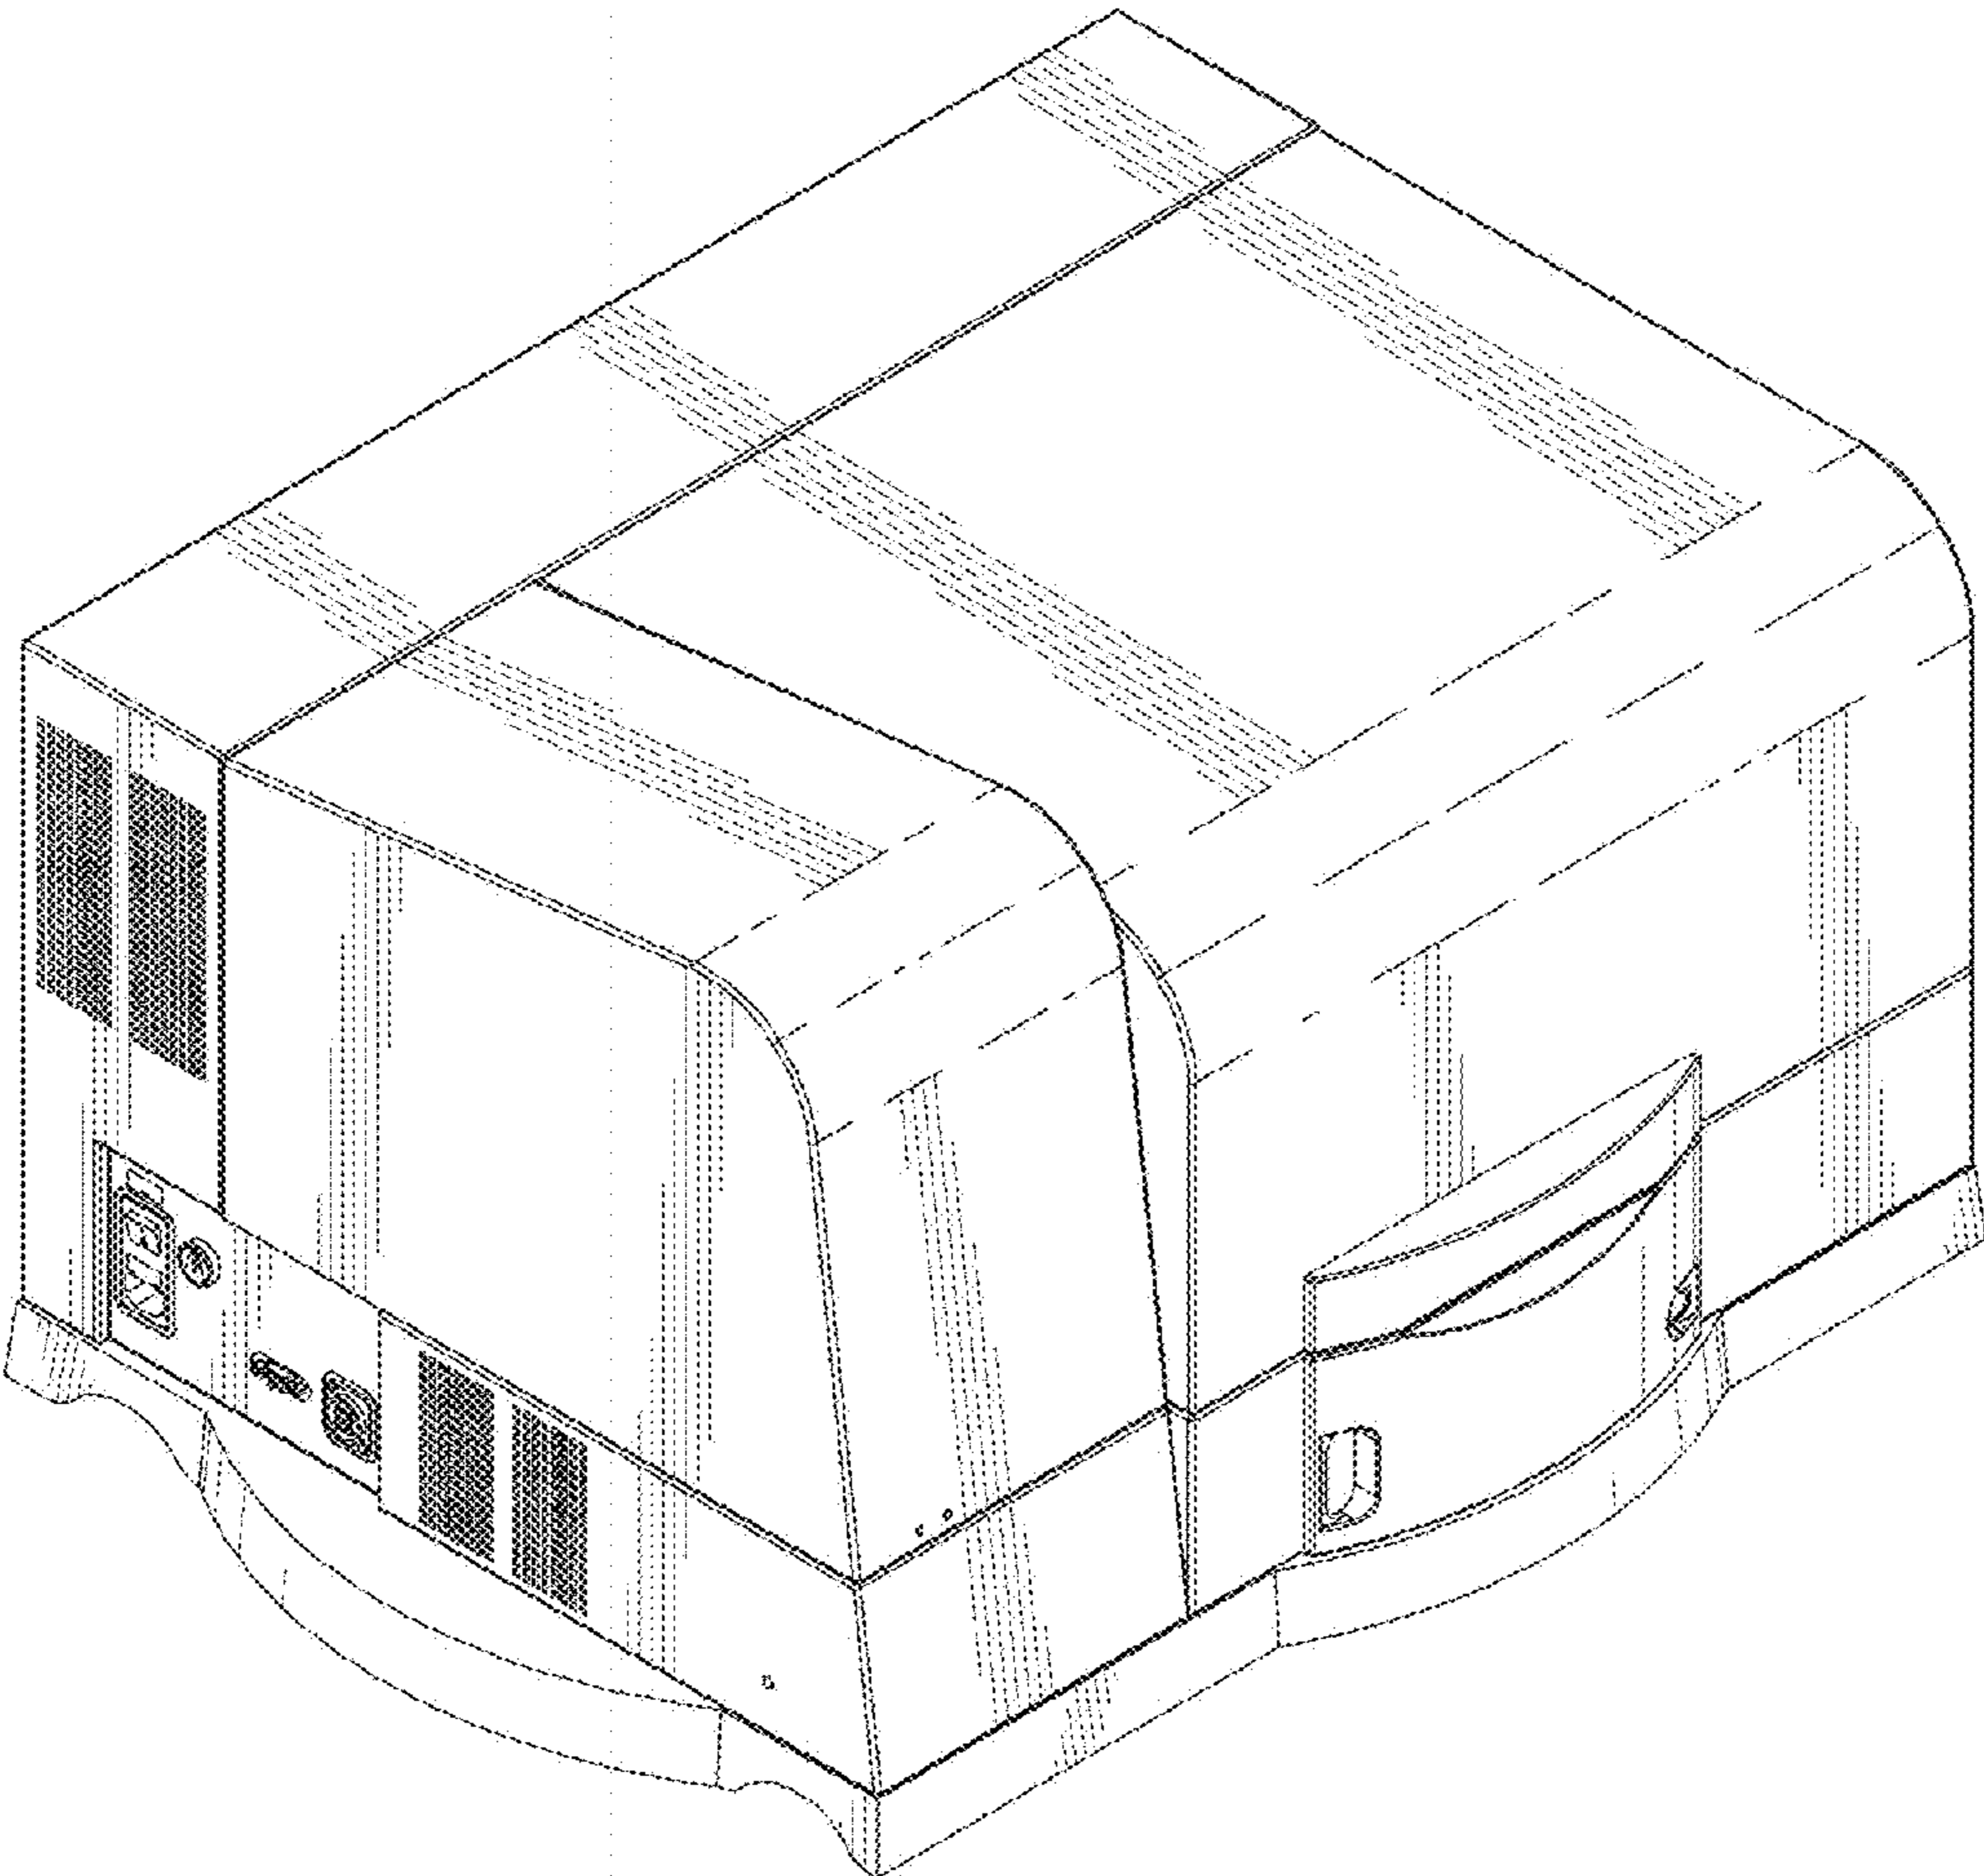


Figure 1

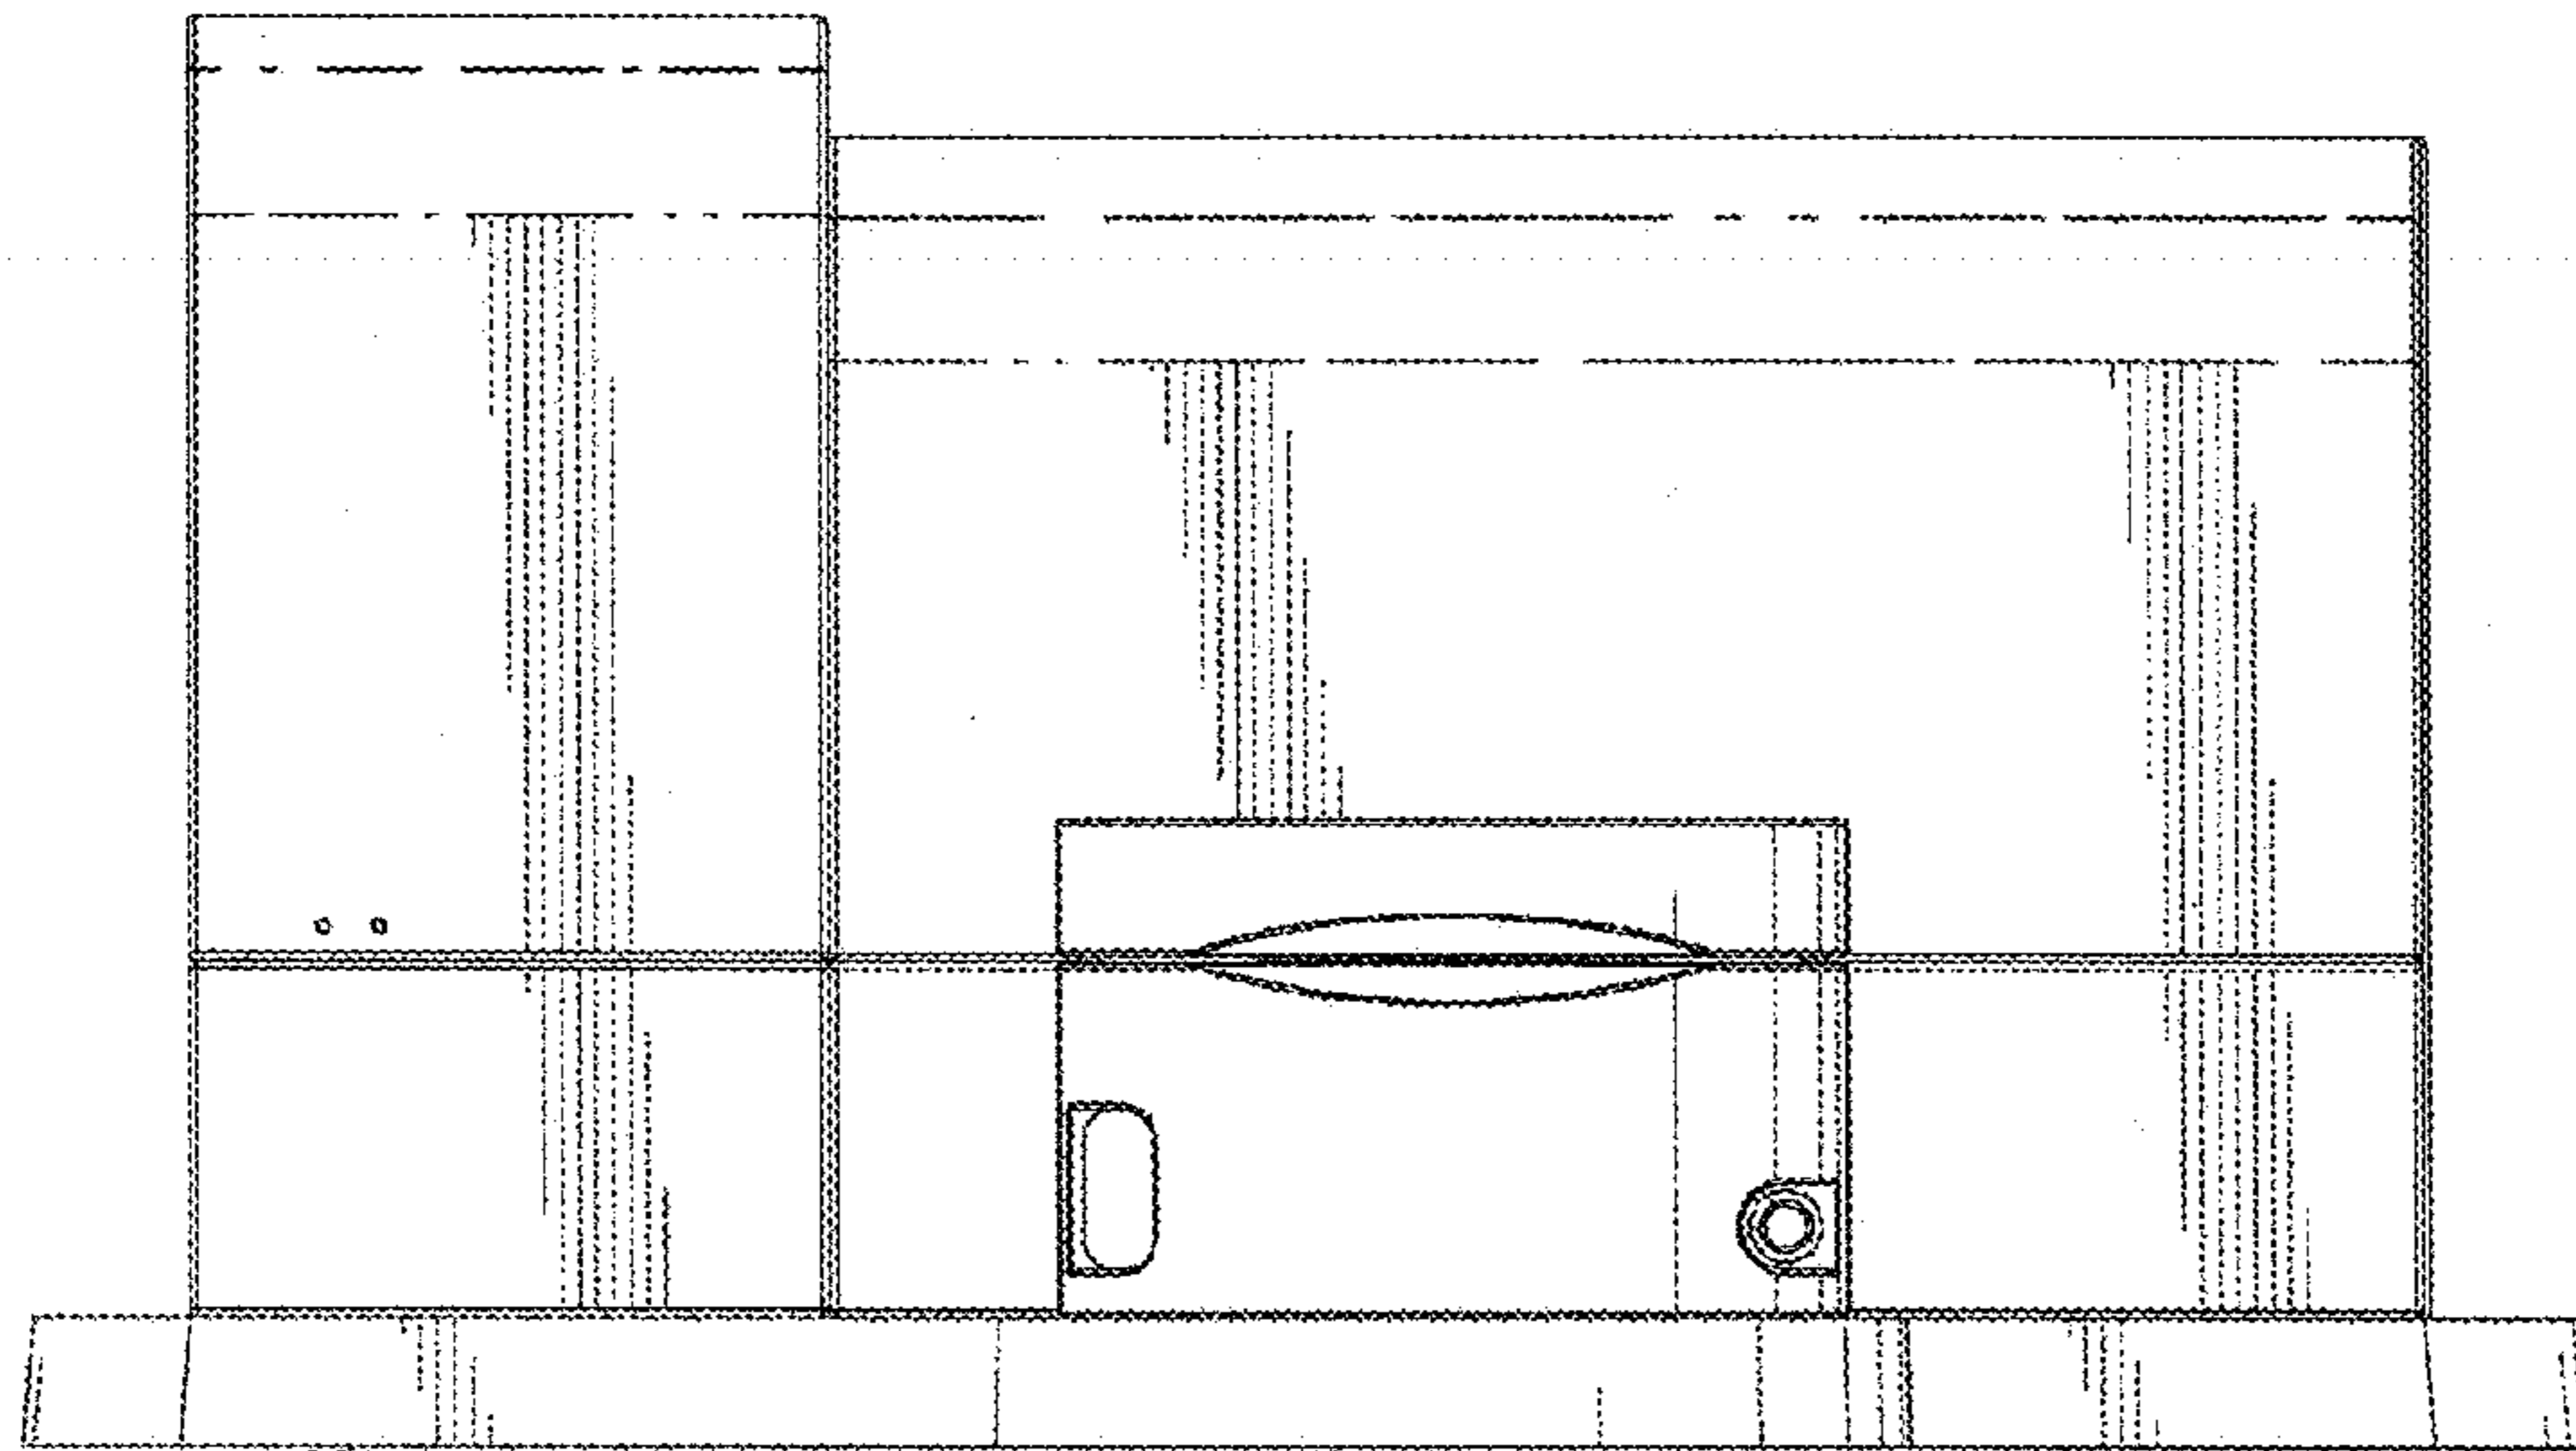


Figure 2

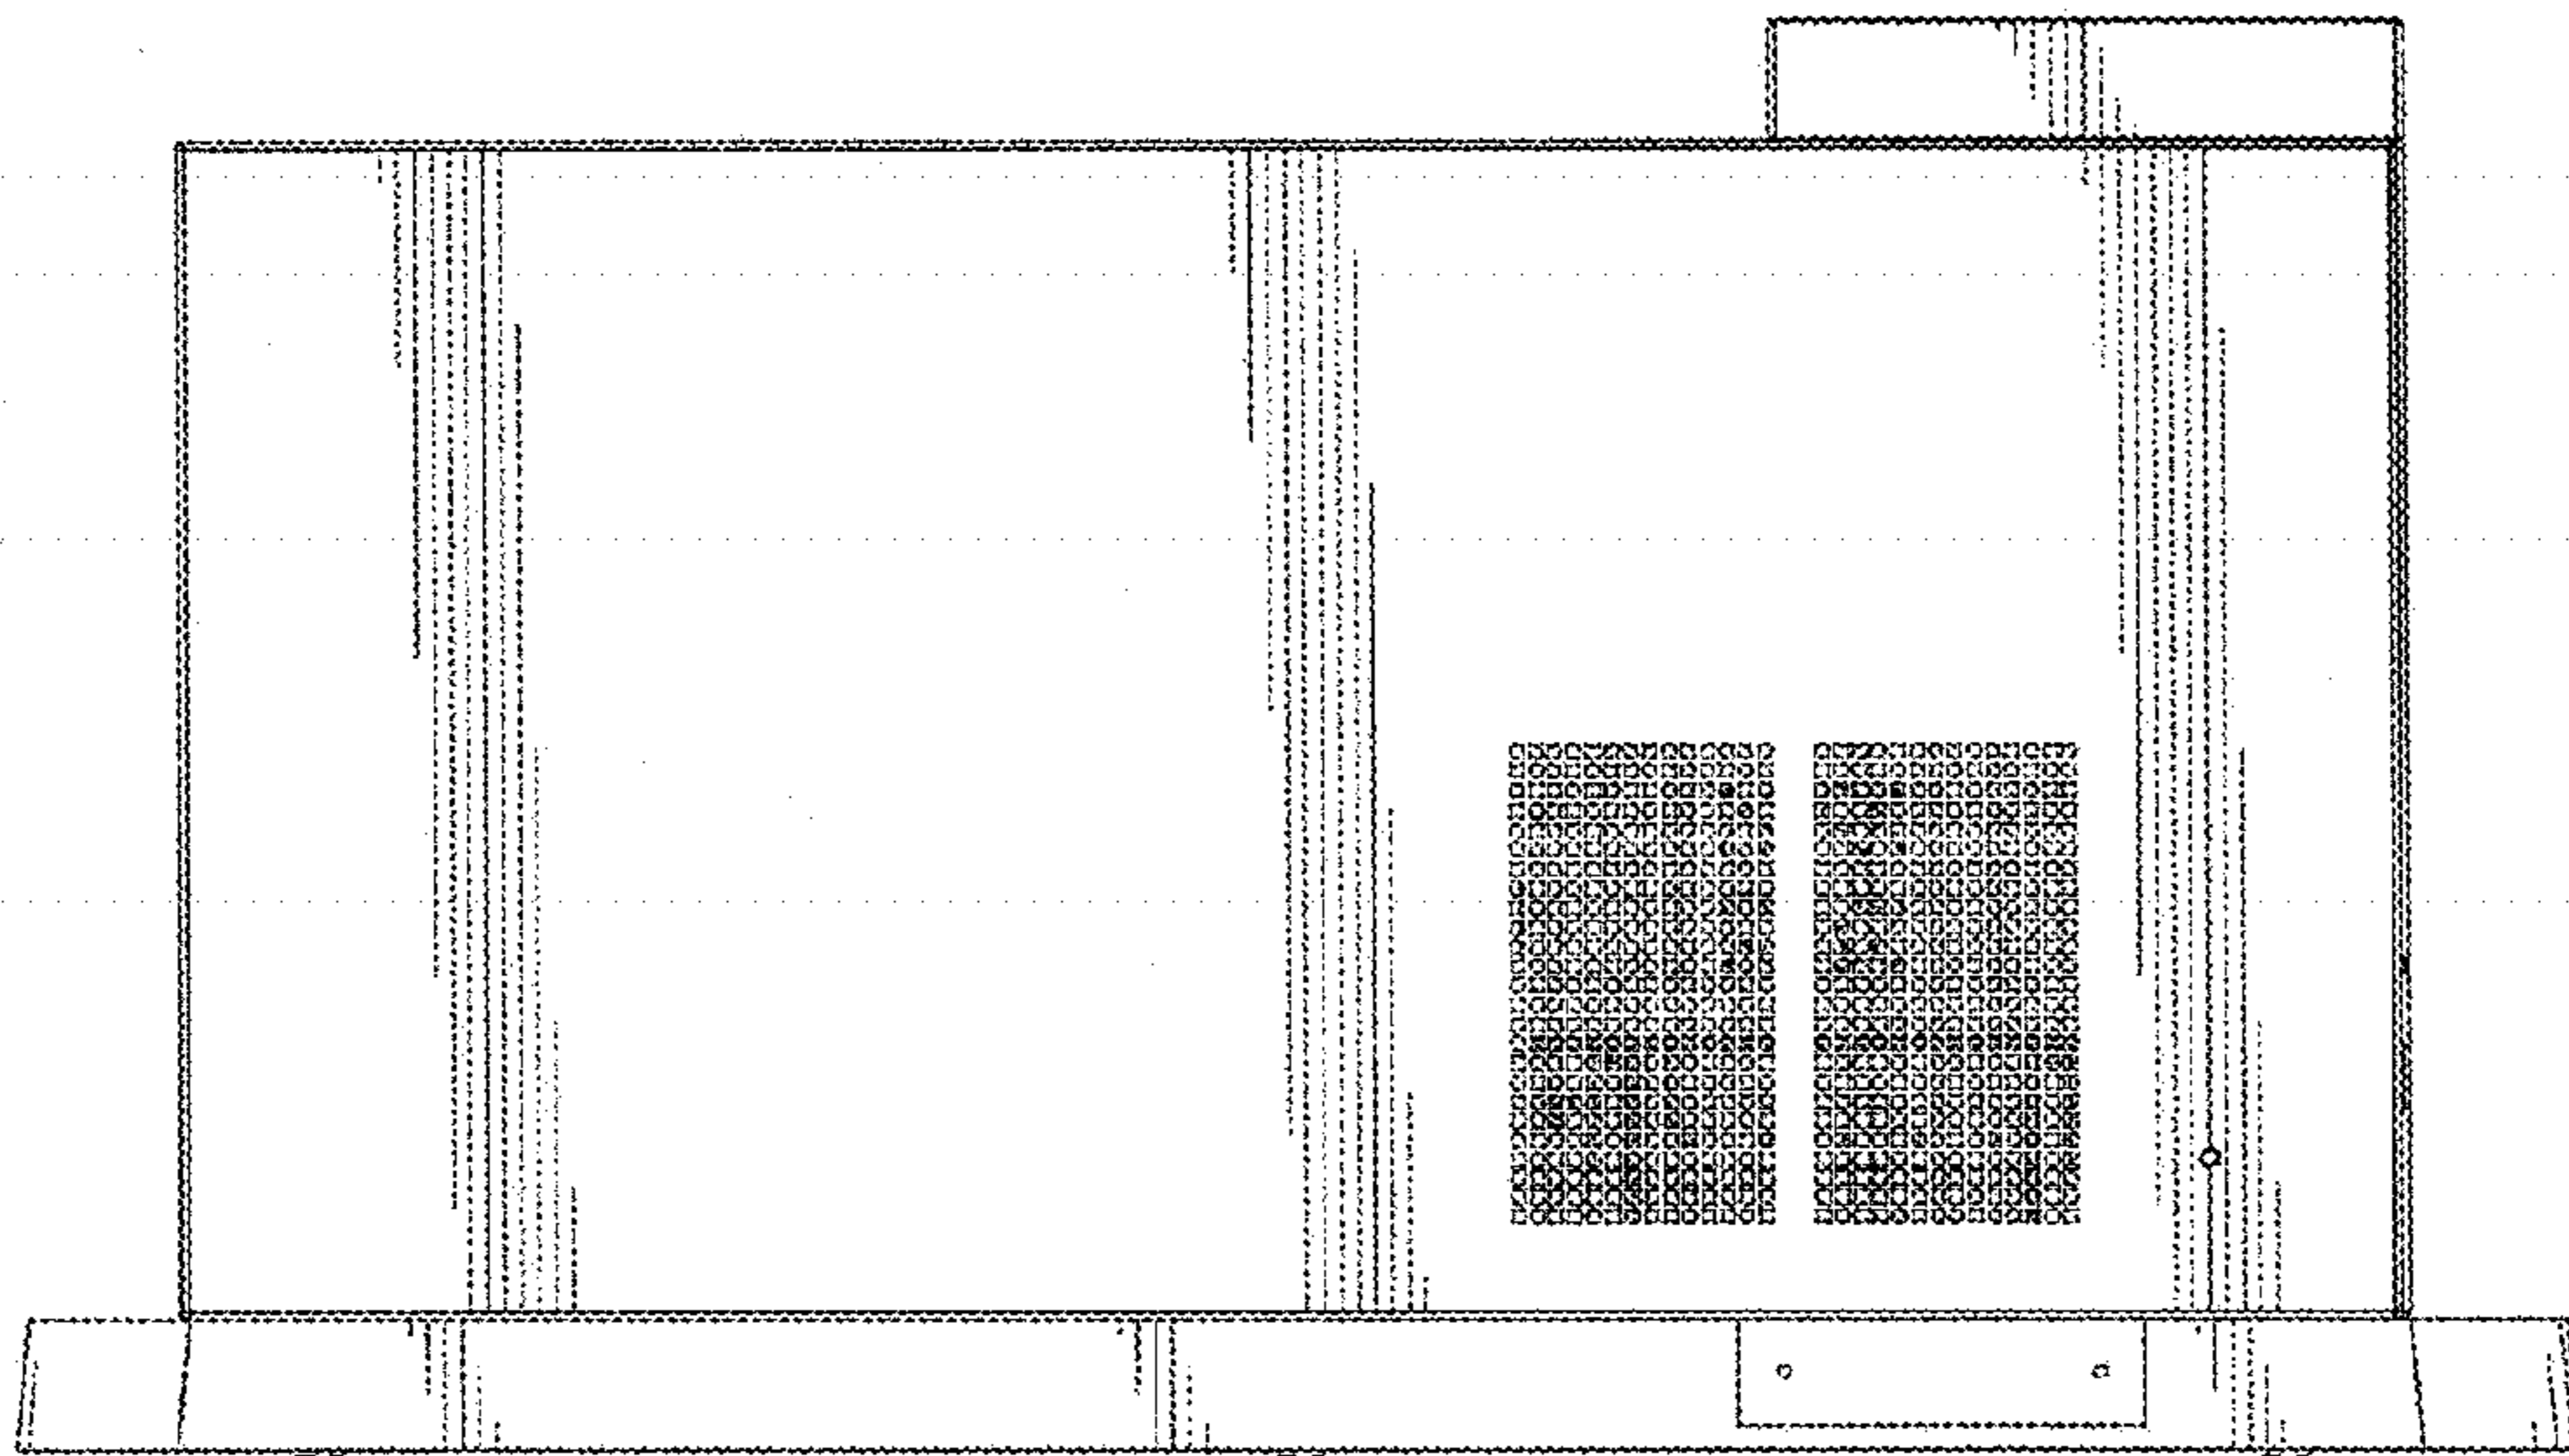


Figure 3

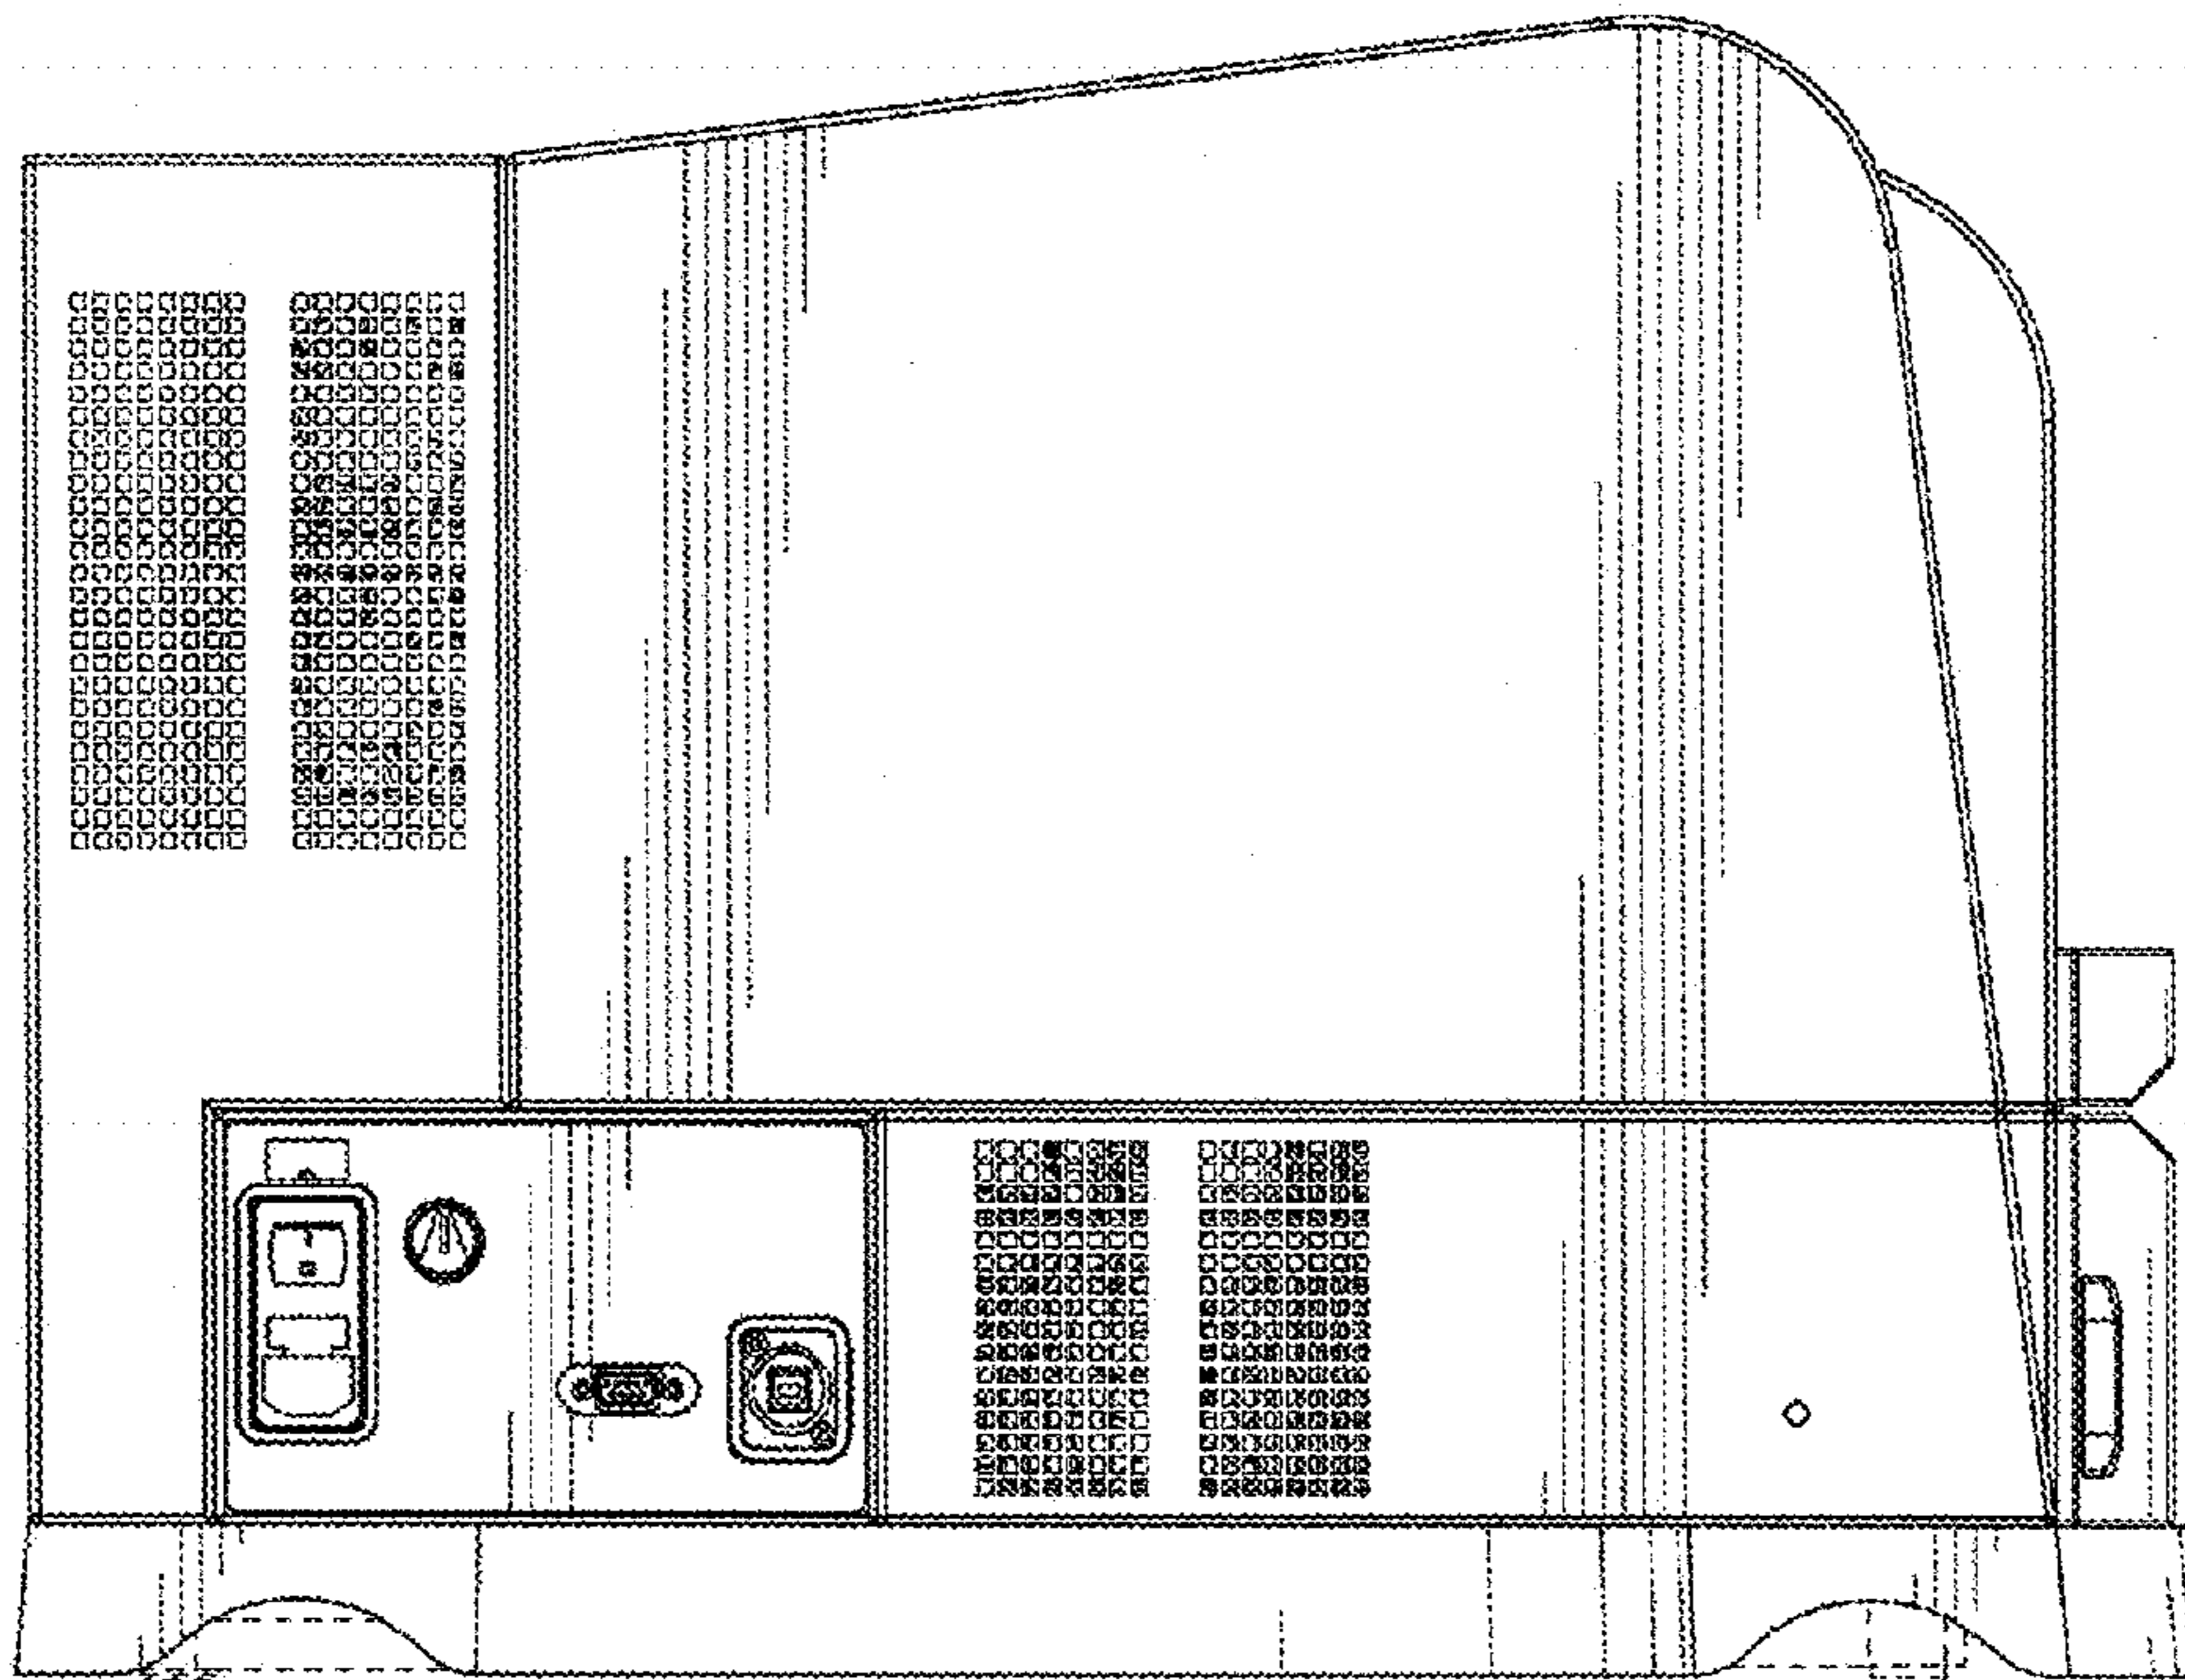


Figure 4

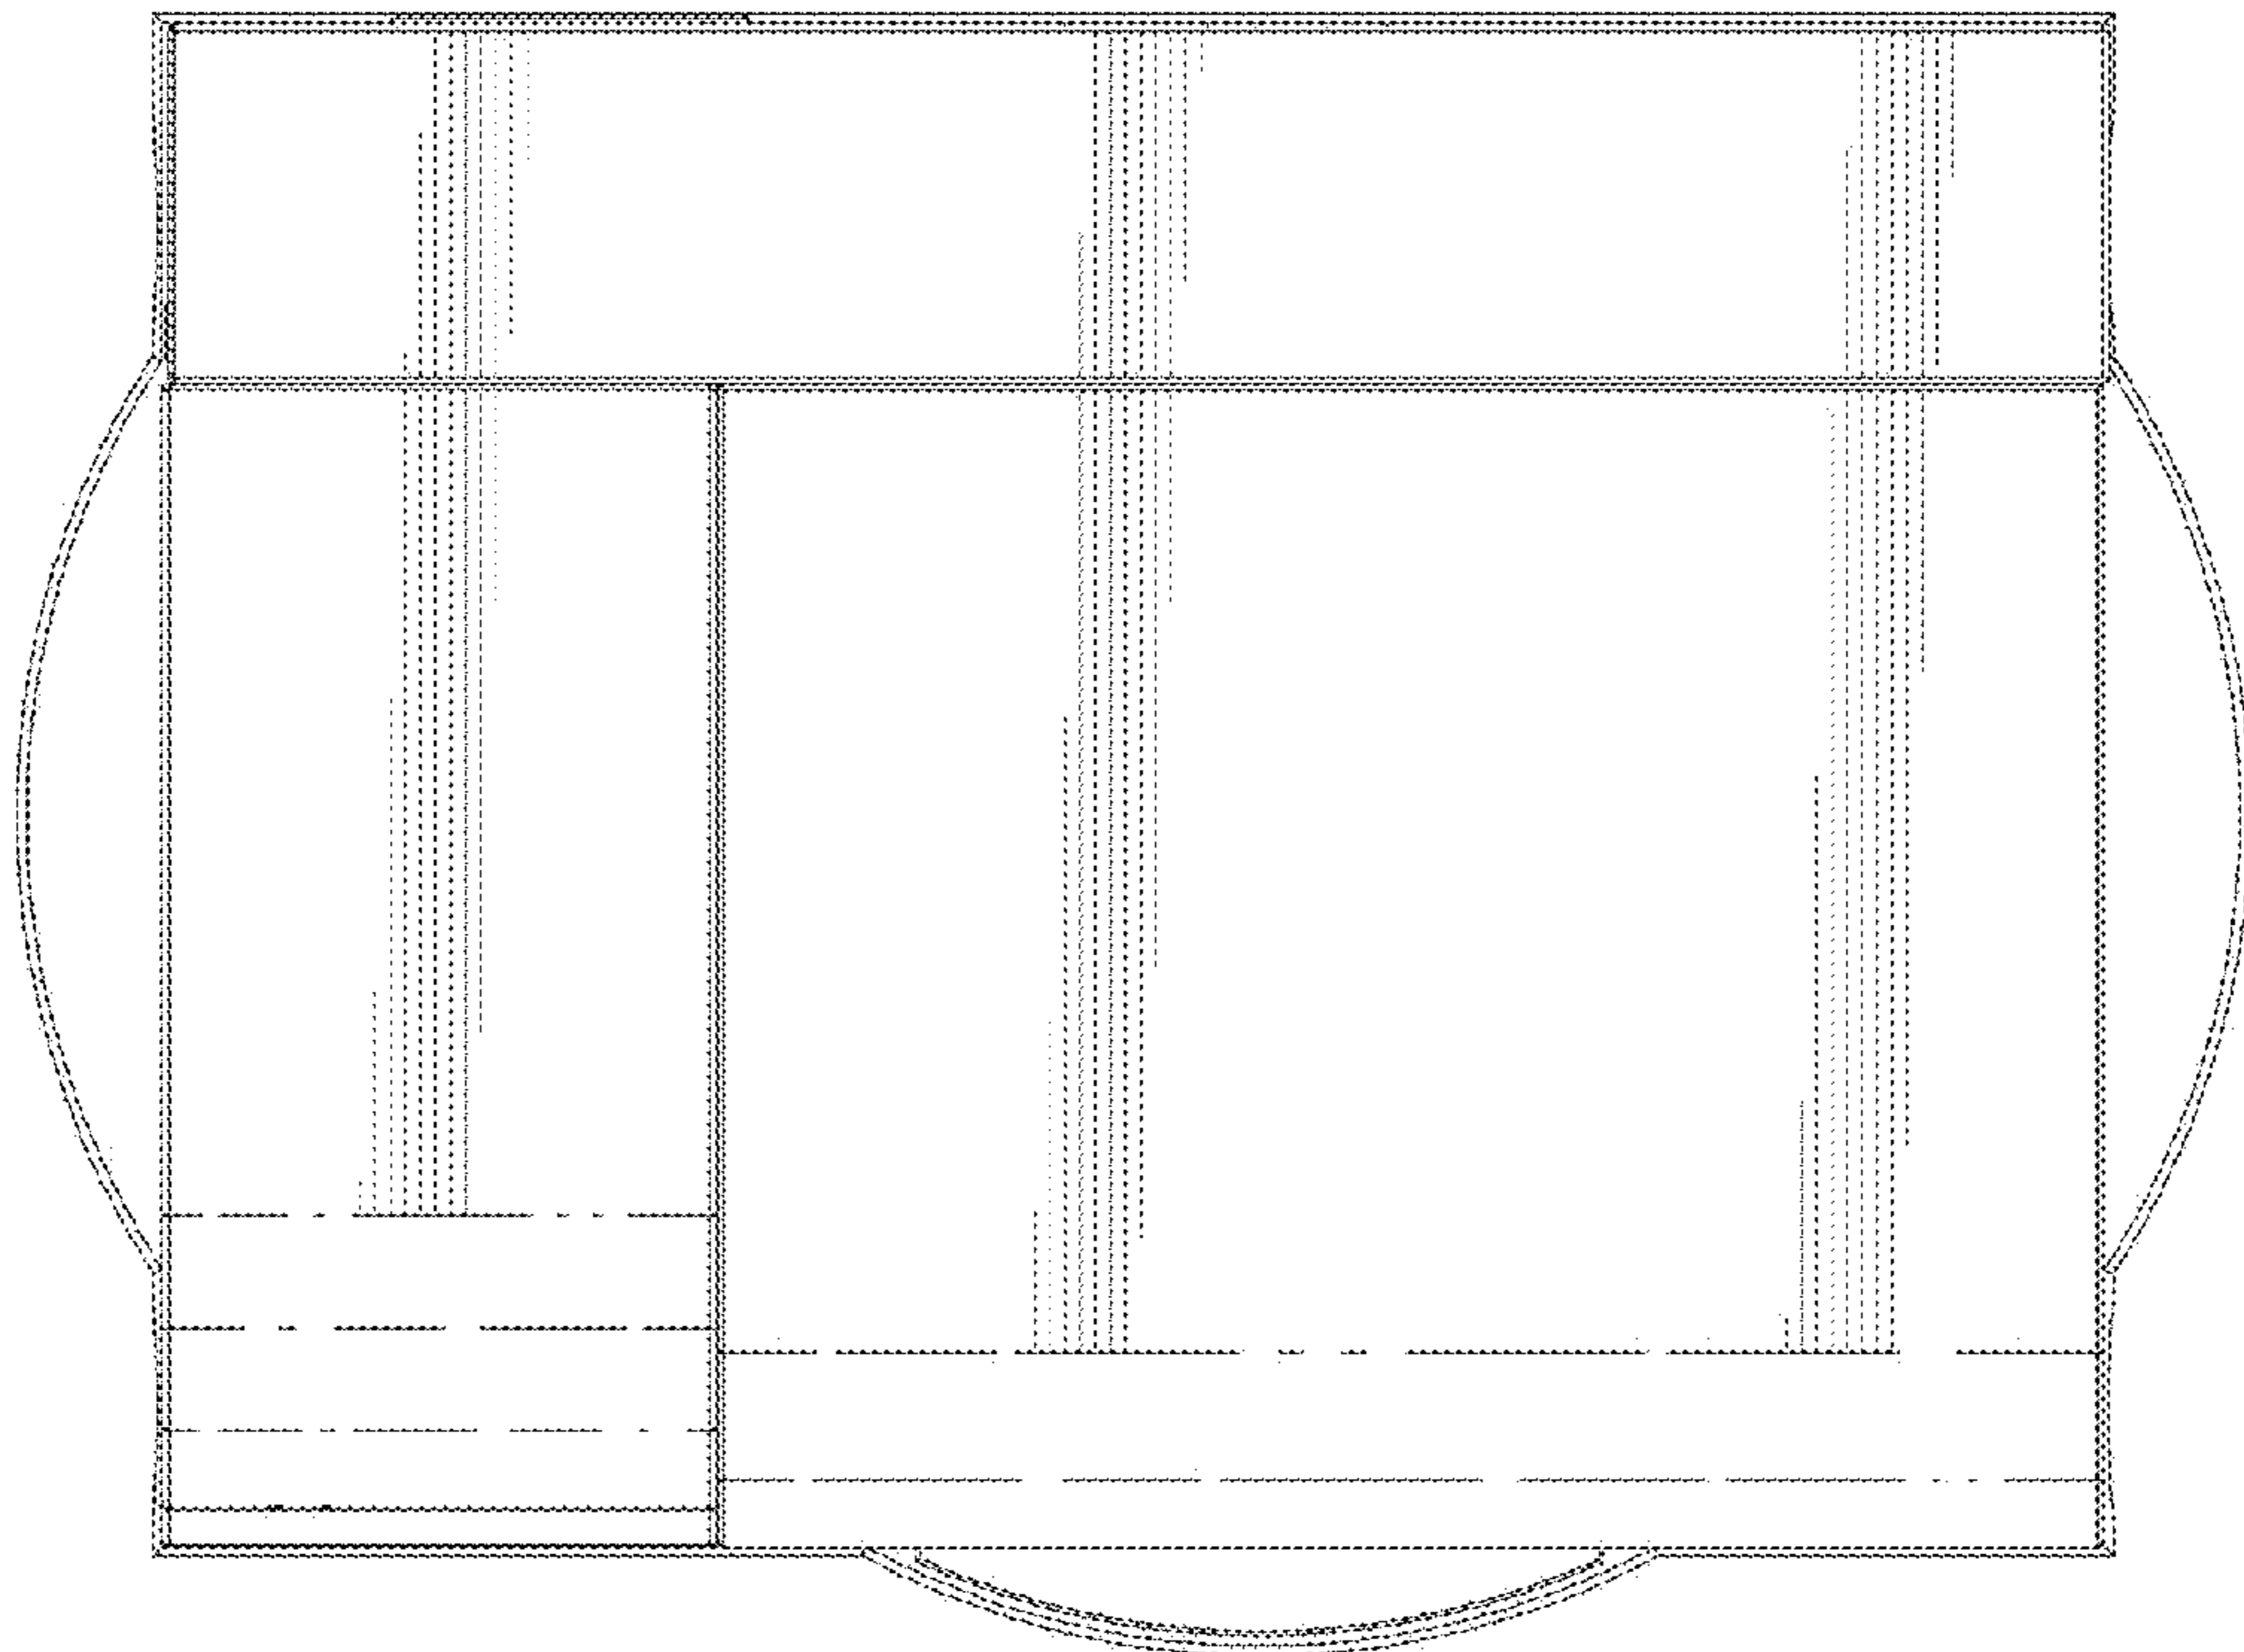


Figure 5

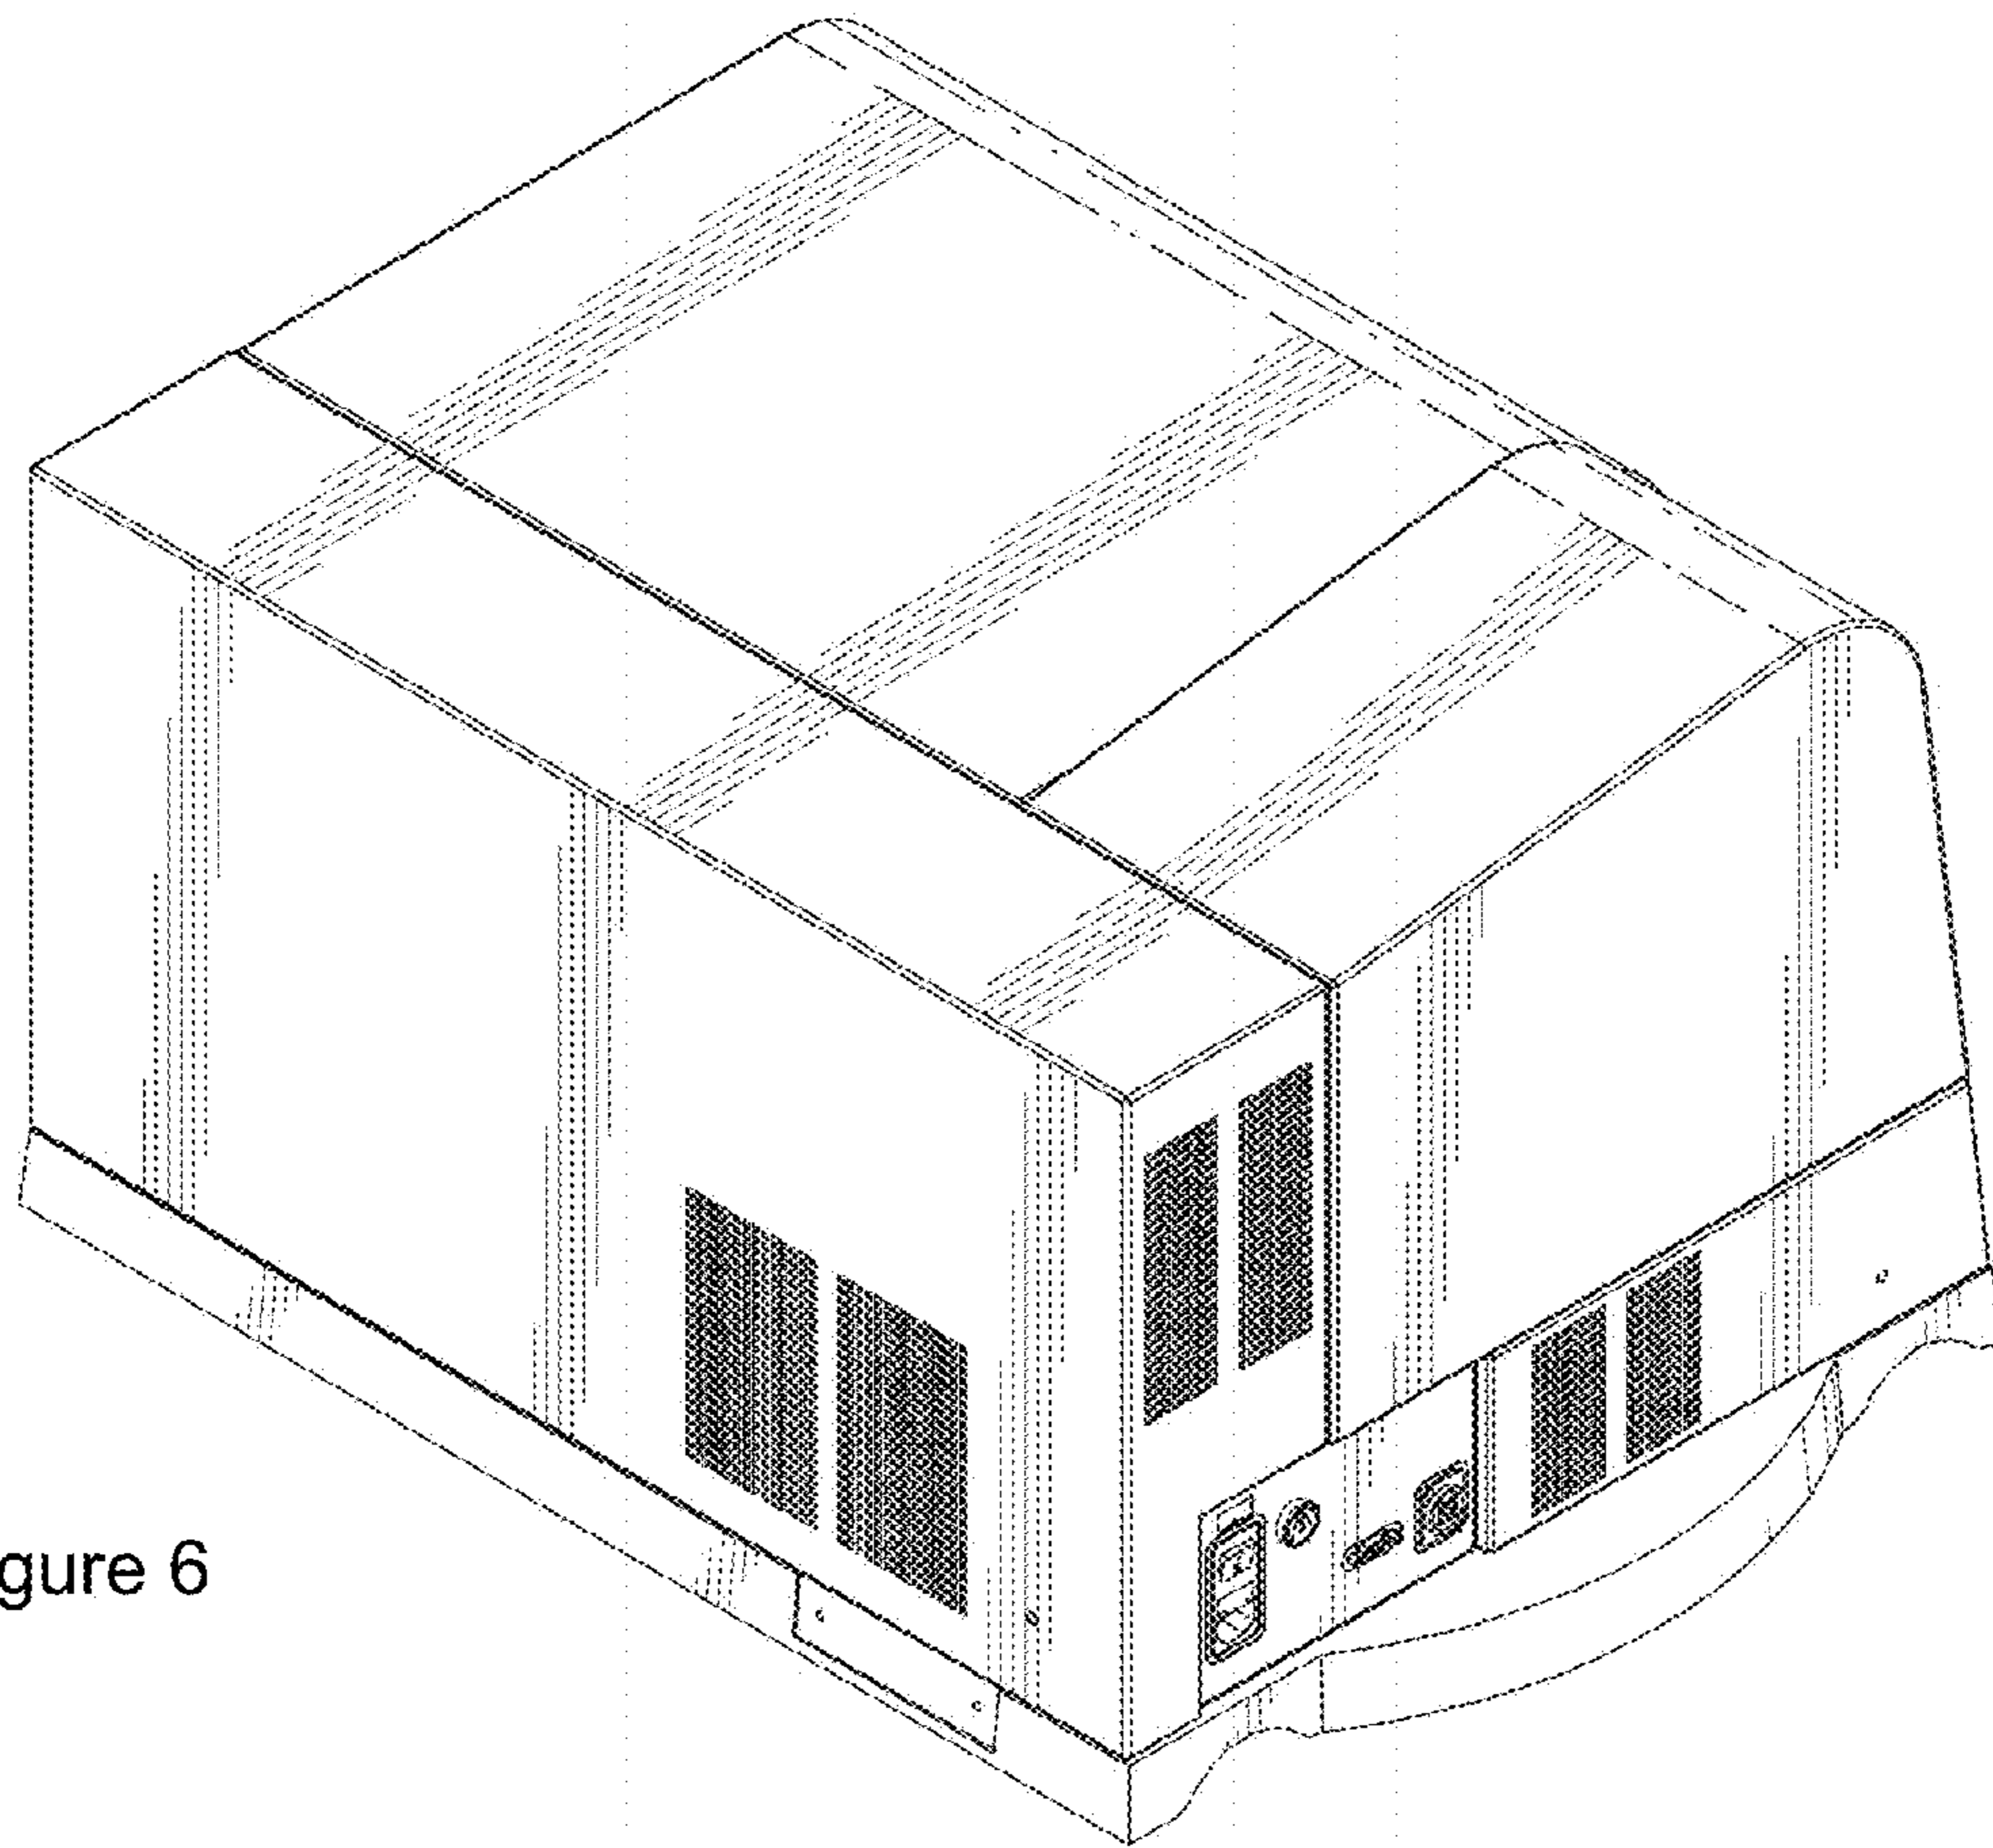


Figure 6