



US00D707848S

(12) **United States Design Patent**  
**Shigeno et al.**

(10) **Patent No.:** **US D707,848 S**  
(45) **Date of Patent:** **\*\* Jun. 24, 2014**

(54) **TRAY FOR VITAL SIGNS MONITOR**

(75) Inventors: **Takashi Shigeno**, Kawasaki (JP);  
**Kazuya Andachi**, Tokyo (JP);  
**Yoshikazu Inami**, Akashi (JP); **Ayumu Okada**, Aichi (JP); **Tomonori Inoue**,  
Kyoto (JP); **Yoshihisa Miwa**, Kusatsu  
(JP)

(73) Assignee: **Omron Healthcare Co., Ltd.**, Kyoto  
(JP)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/399,250**

(22) Filed: **Aug. 11, 2011**

(30) **Foreign Application Priority Data**

Feb. 15, 2011 (JP) ..... 2011-003116

(51) **LOC (10) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/229**

(58) **Field of Classification Search**  
USPC ..... D24/123, 176, 216, 218, 224, 226-232;  
422/99, 102, 104, 297, 300, 559;  
433/77; D3/304, 307, 308, 313-315;  
D7/500, 550.1, 543, 602, 554.3, 361,  
D7/354, 587; 206/438; 211/74; D6/406.1,  
D6/406.3, 406.4

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D202,013 S \* 8/1965 Hamilton ..... D24/229  
D209,641 S \* 12/1967 Golberg ..... D24/230  
D213,933 S \* 4/1969 Folkman ..... D24/230  
D213,934 S \* 4/1969 Folkman ..... D24/229

D218,077 S \* 7/1970 Gabriel ..... D24/229  
D237,317 S \* 10/1975 Nowaskowski et al. .... D24/229  
D248,871 S \* 8/1978 Forsman et al. .... D24/230  
D249,362 S \* 9/1978 Forsman et al. .... D24/230  
D325,526 S \* 4/1992 Deguchi et al. .... D9/415  
D343,687 S \* 1/1994 Houghton et al. .... D24/227  
D402,767 S \* 12/1998 Davis et al. .... D24/229  
D437,941 S \* 2/2001 Frattini ..... D24/229  
D442,697 S \* 5/2001 Hajianpour ..... D24/229  
D450,391 S \* 11/2001 Hunt et al. .... D24/227  
D471,640 S \* 3/2003 McMichael et al. .... D24/229  
D471,641 S \* 3/2003 McMichael et al. .... D24/229  
D480,816 S \* 10/2003 McMichael et al. .... D24/229  
D489,973 S \* 5/2004 Root et al. .... D9/415  
D495,807 S \* 9/2004 Agbodoe et al. .... D24/229  
D565,743 S \* 4/2008 Phillips et al. .... D24/229  
D618,821 S \* 6/2010 Larsen ..... D24/227  
D631,558 S \* 1/2011 Harmston et al. .... D24/229  
D646,796 S \* 10/2011 Walter ..... D24/227  
D650,912 S \* 12/2011 Tomes et al. .... D24/227

\* cited by examiner

*Primary Examiner* — T. Chase Nelson

*Assistant Examiner* — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Capitol City TechLaw

(57) **CLAIM**

The ornamental design for a tray for vital signs monitor, as shown.

**DESCRIPTION**

FIG. 1 is a front perspective view of a tray for vital signs monitor showing our new design;  
FIG. 2 is a rear perspective view thereof;  
FIG. 3 is a front view thereof;  
FIG. 4 is a rear view thereof;  
FIG. 5 is a top view thereof;  
FIG. 6 is a bottom view thereof;  
FIG. 7 is a right side view thereof; and,  
FIG. 8 is a left side view thereof.

**1 Claim, 8 Drawing Sheets**

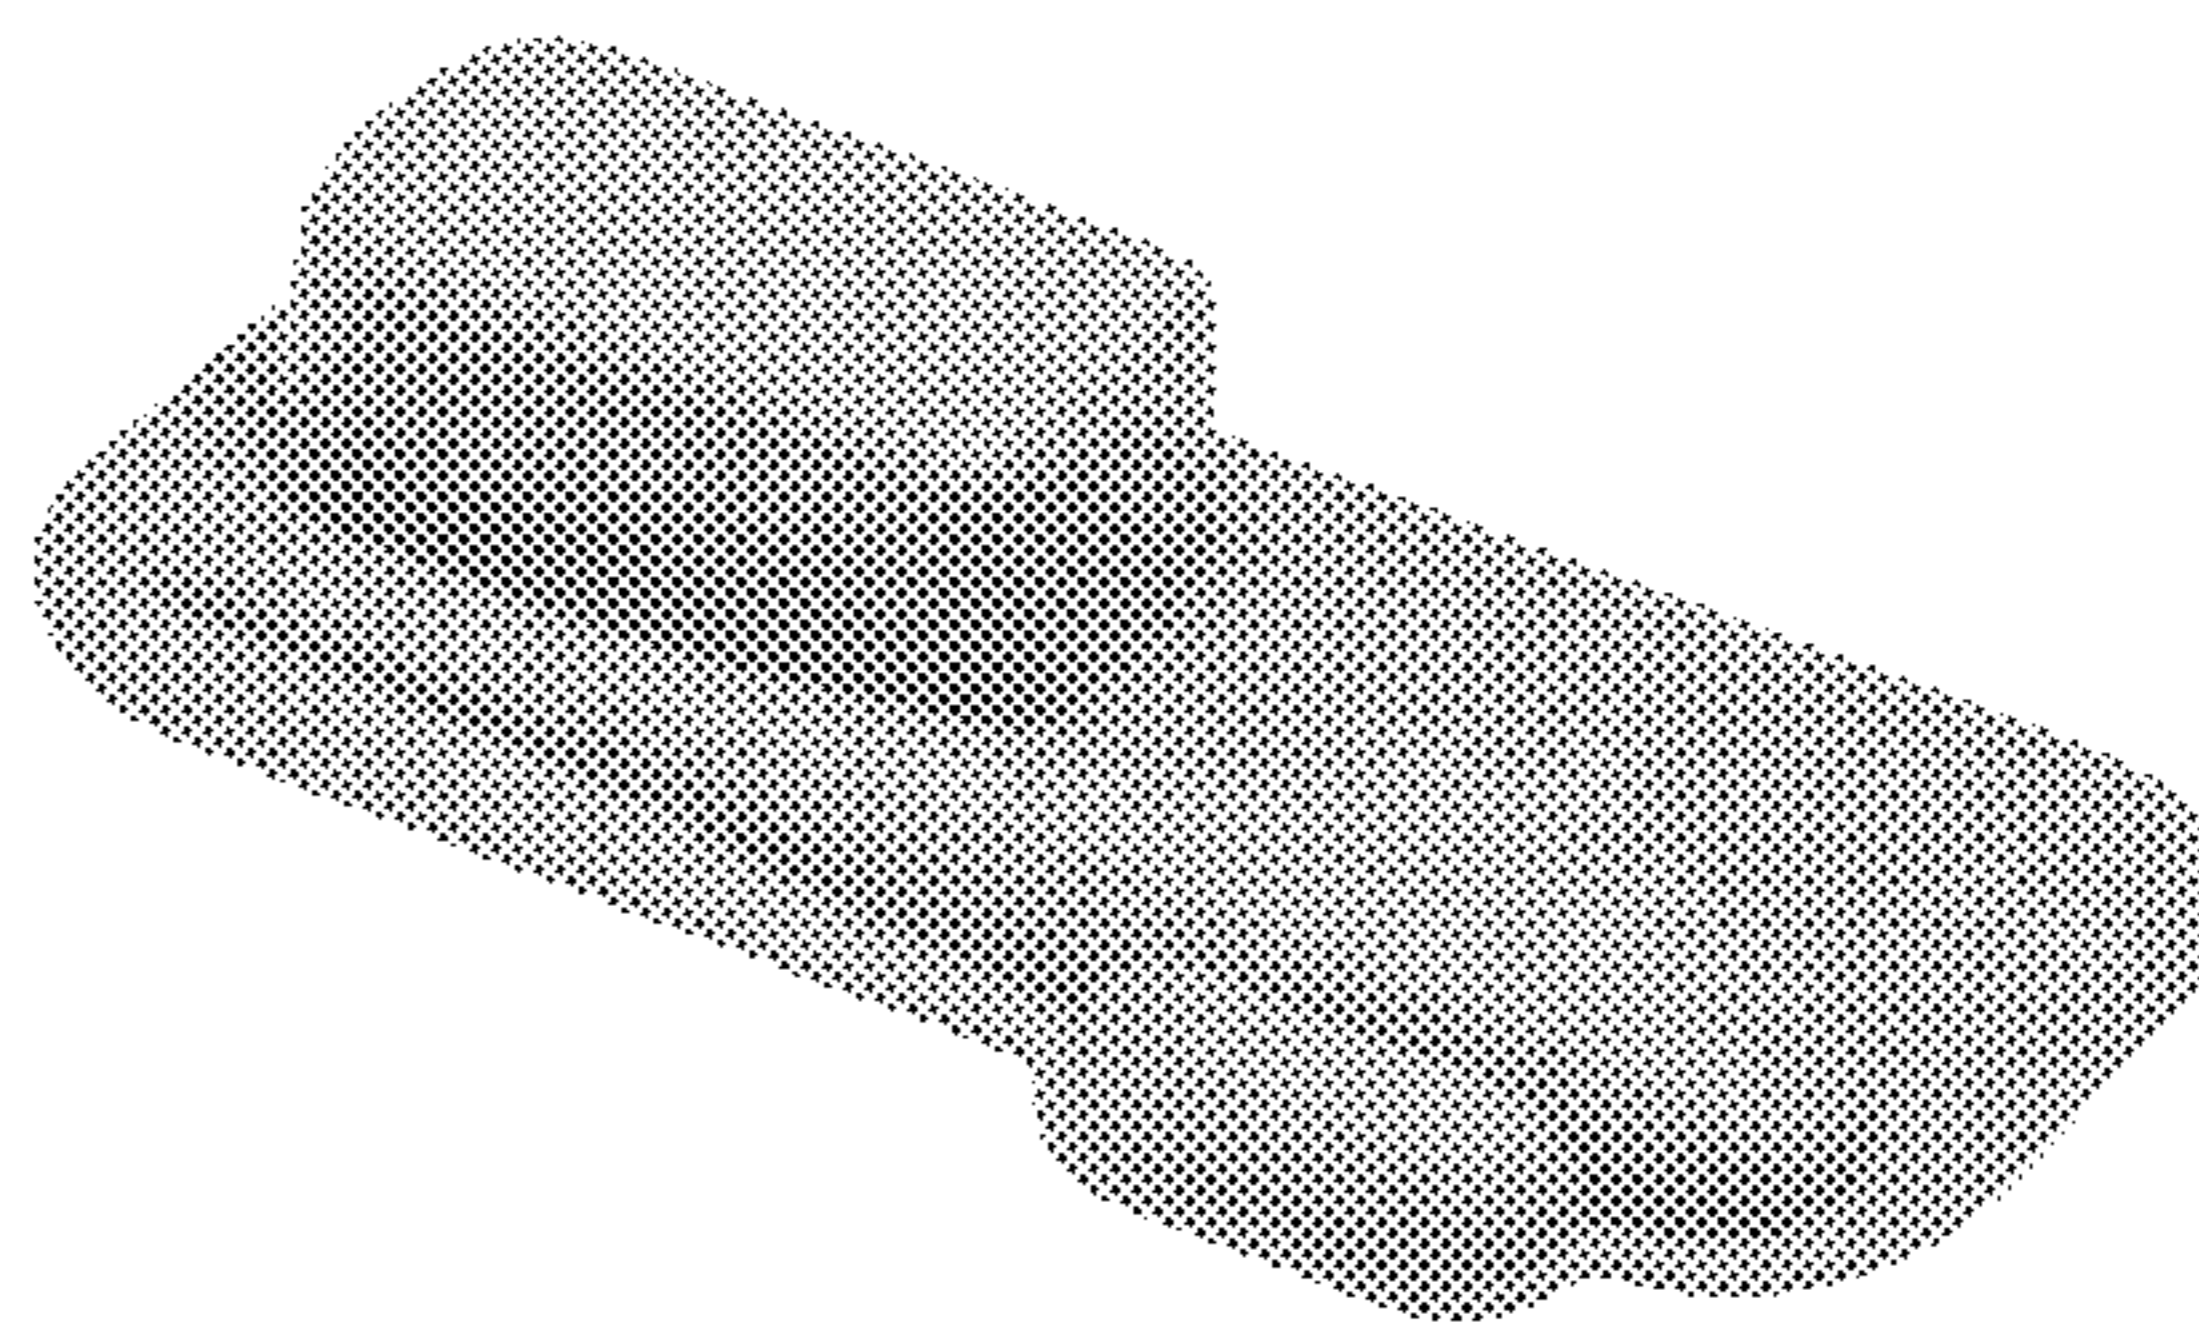
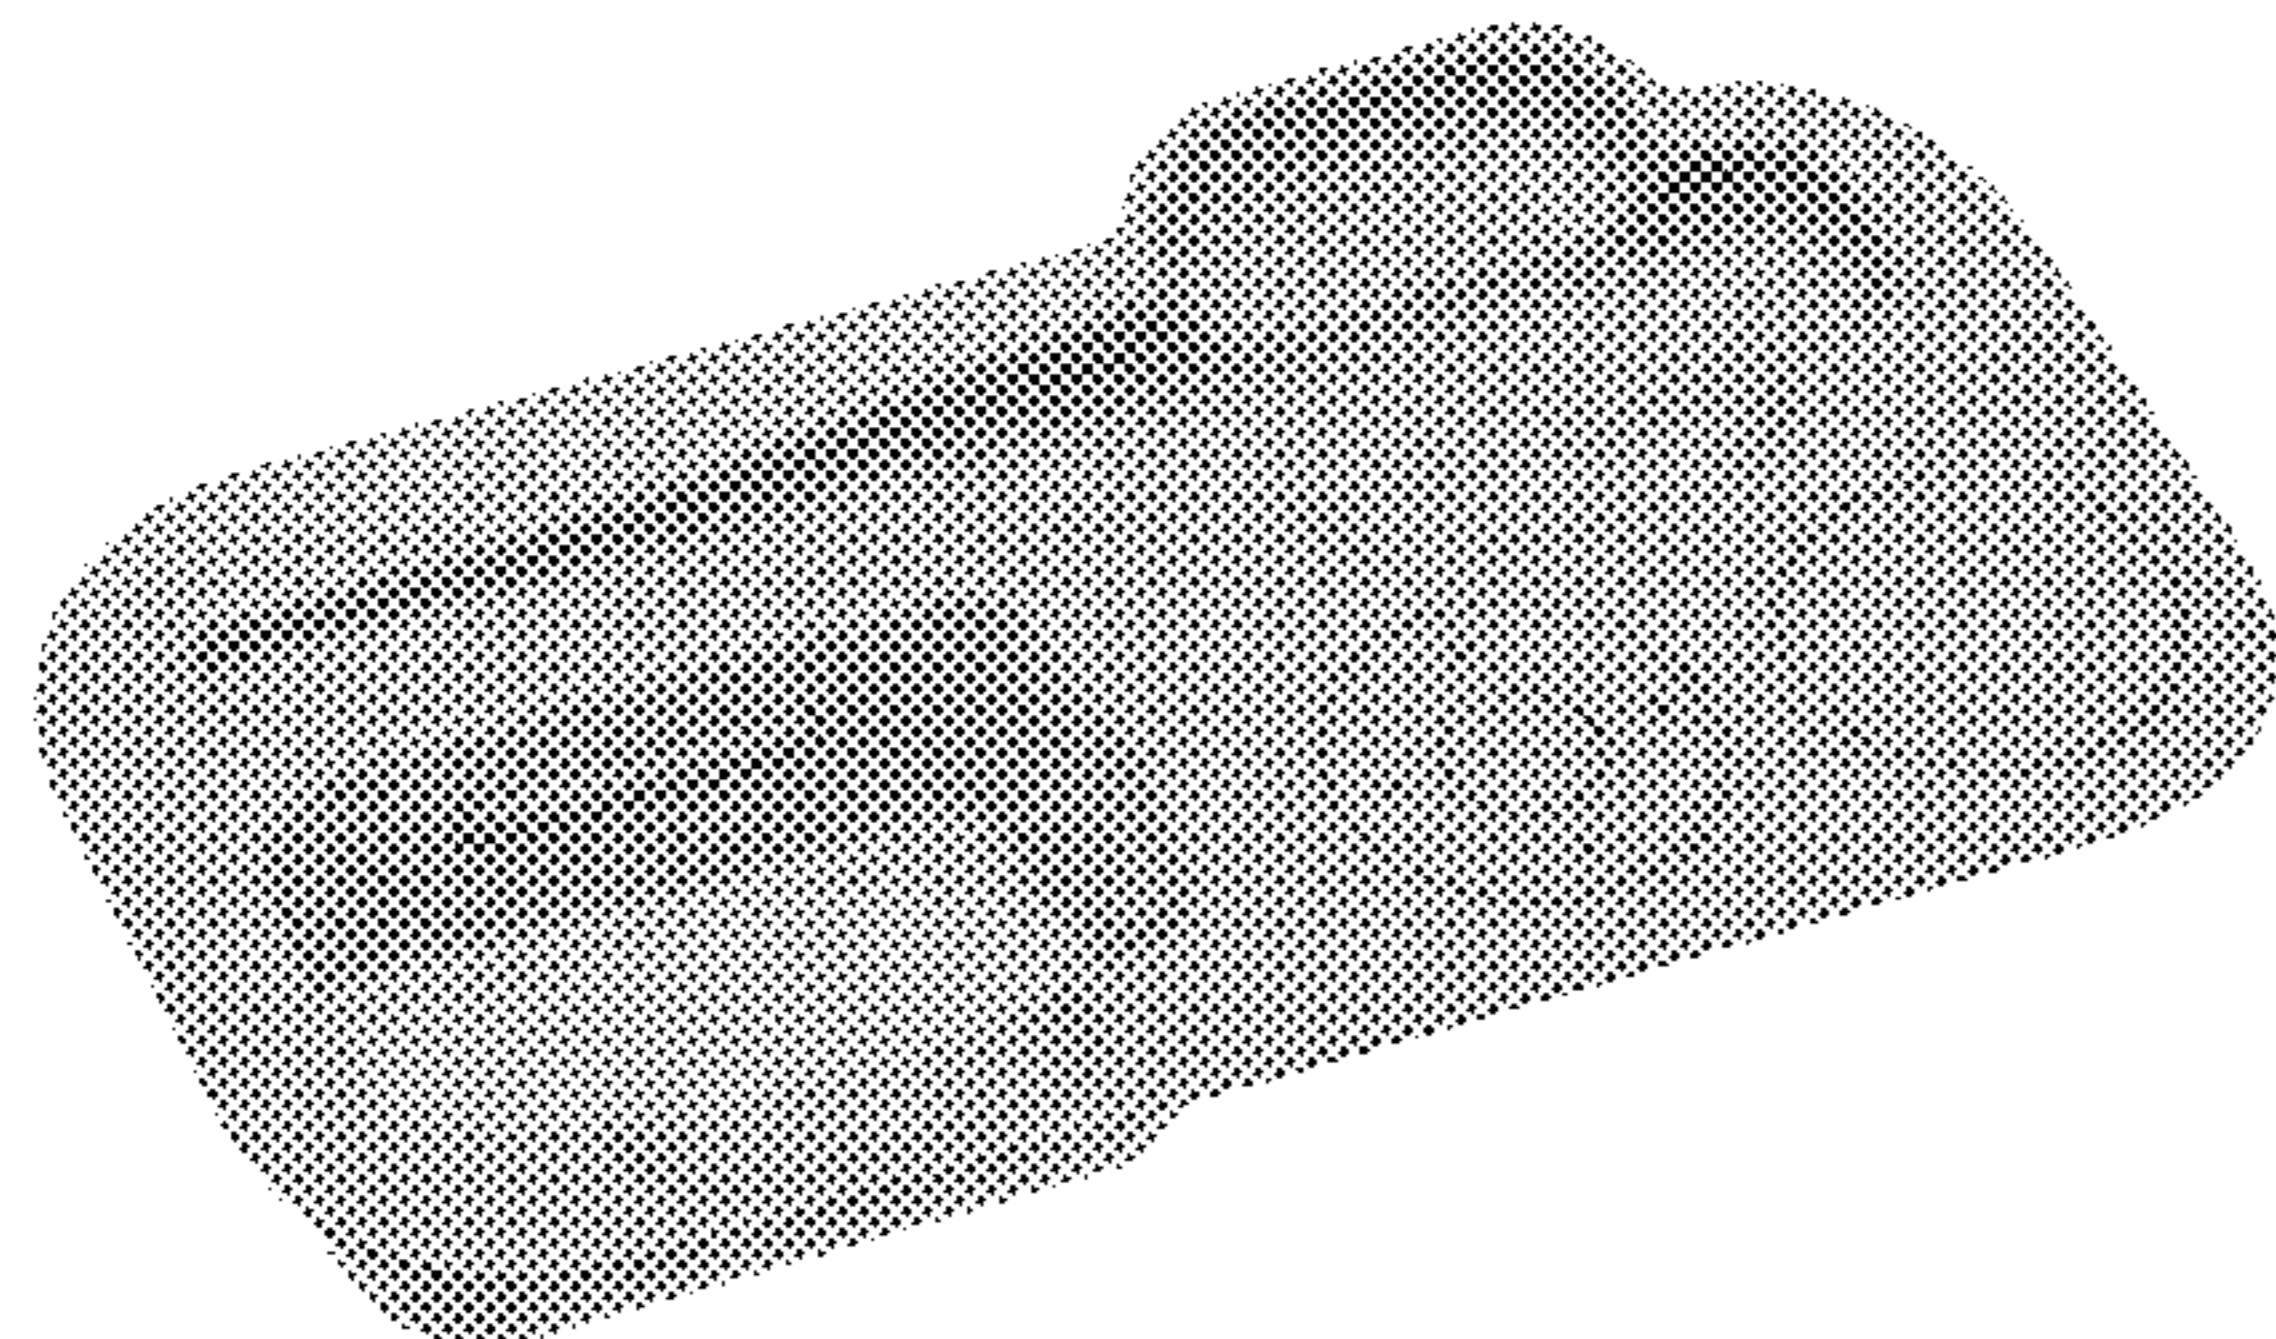


FIG.1

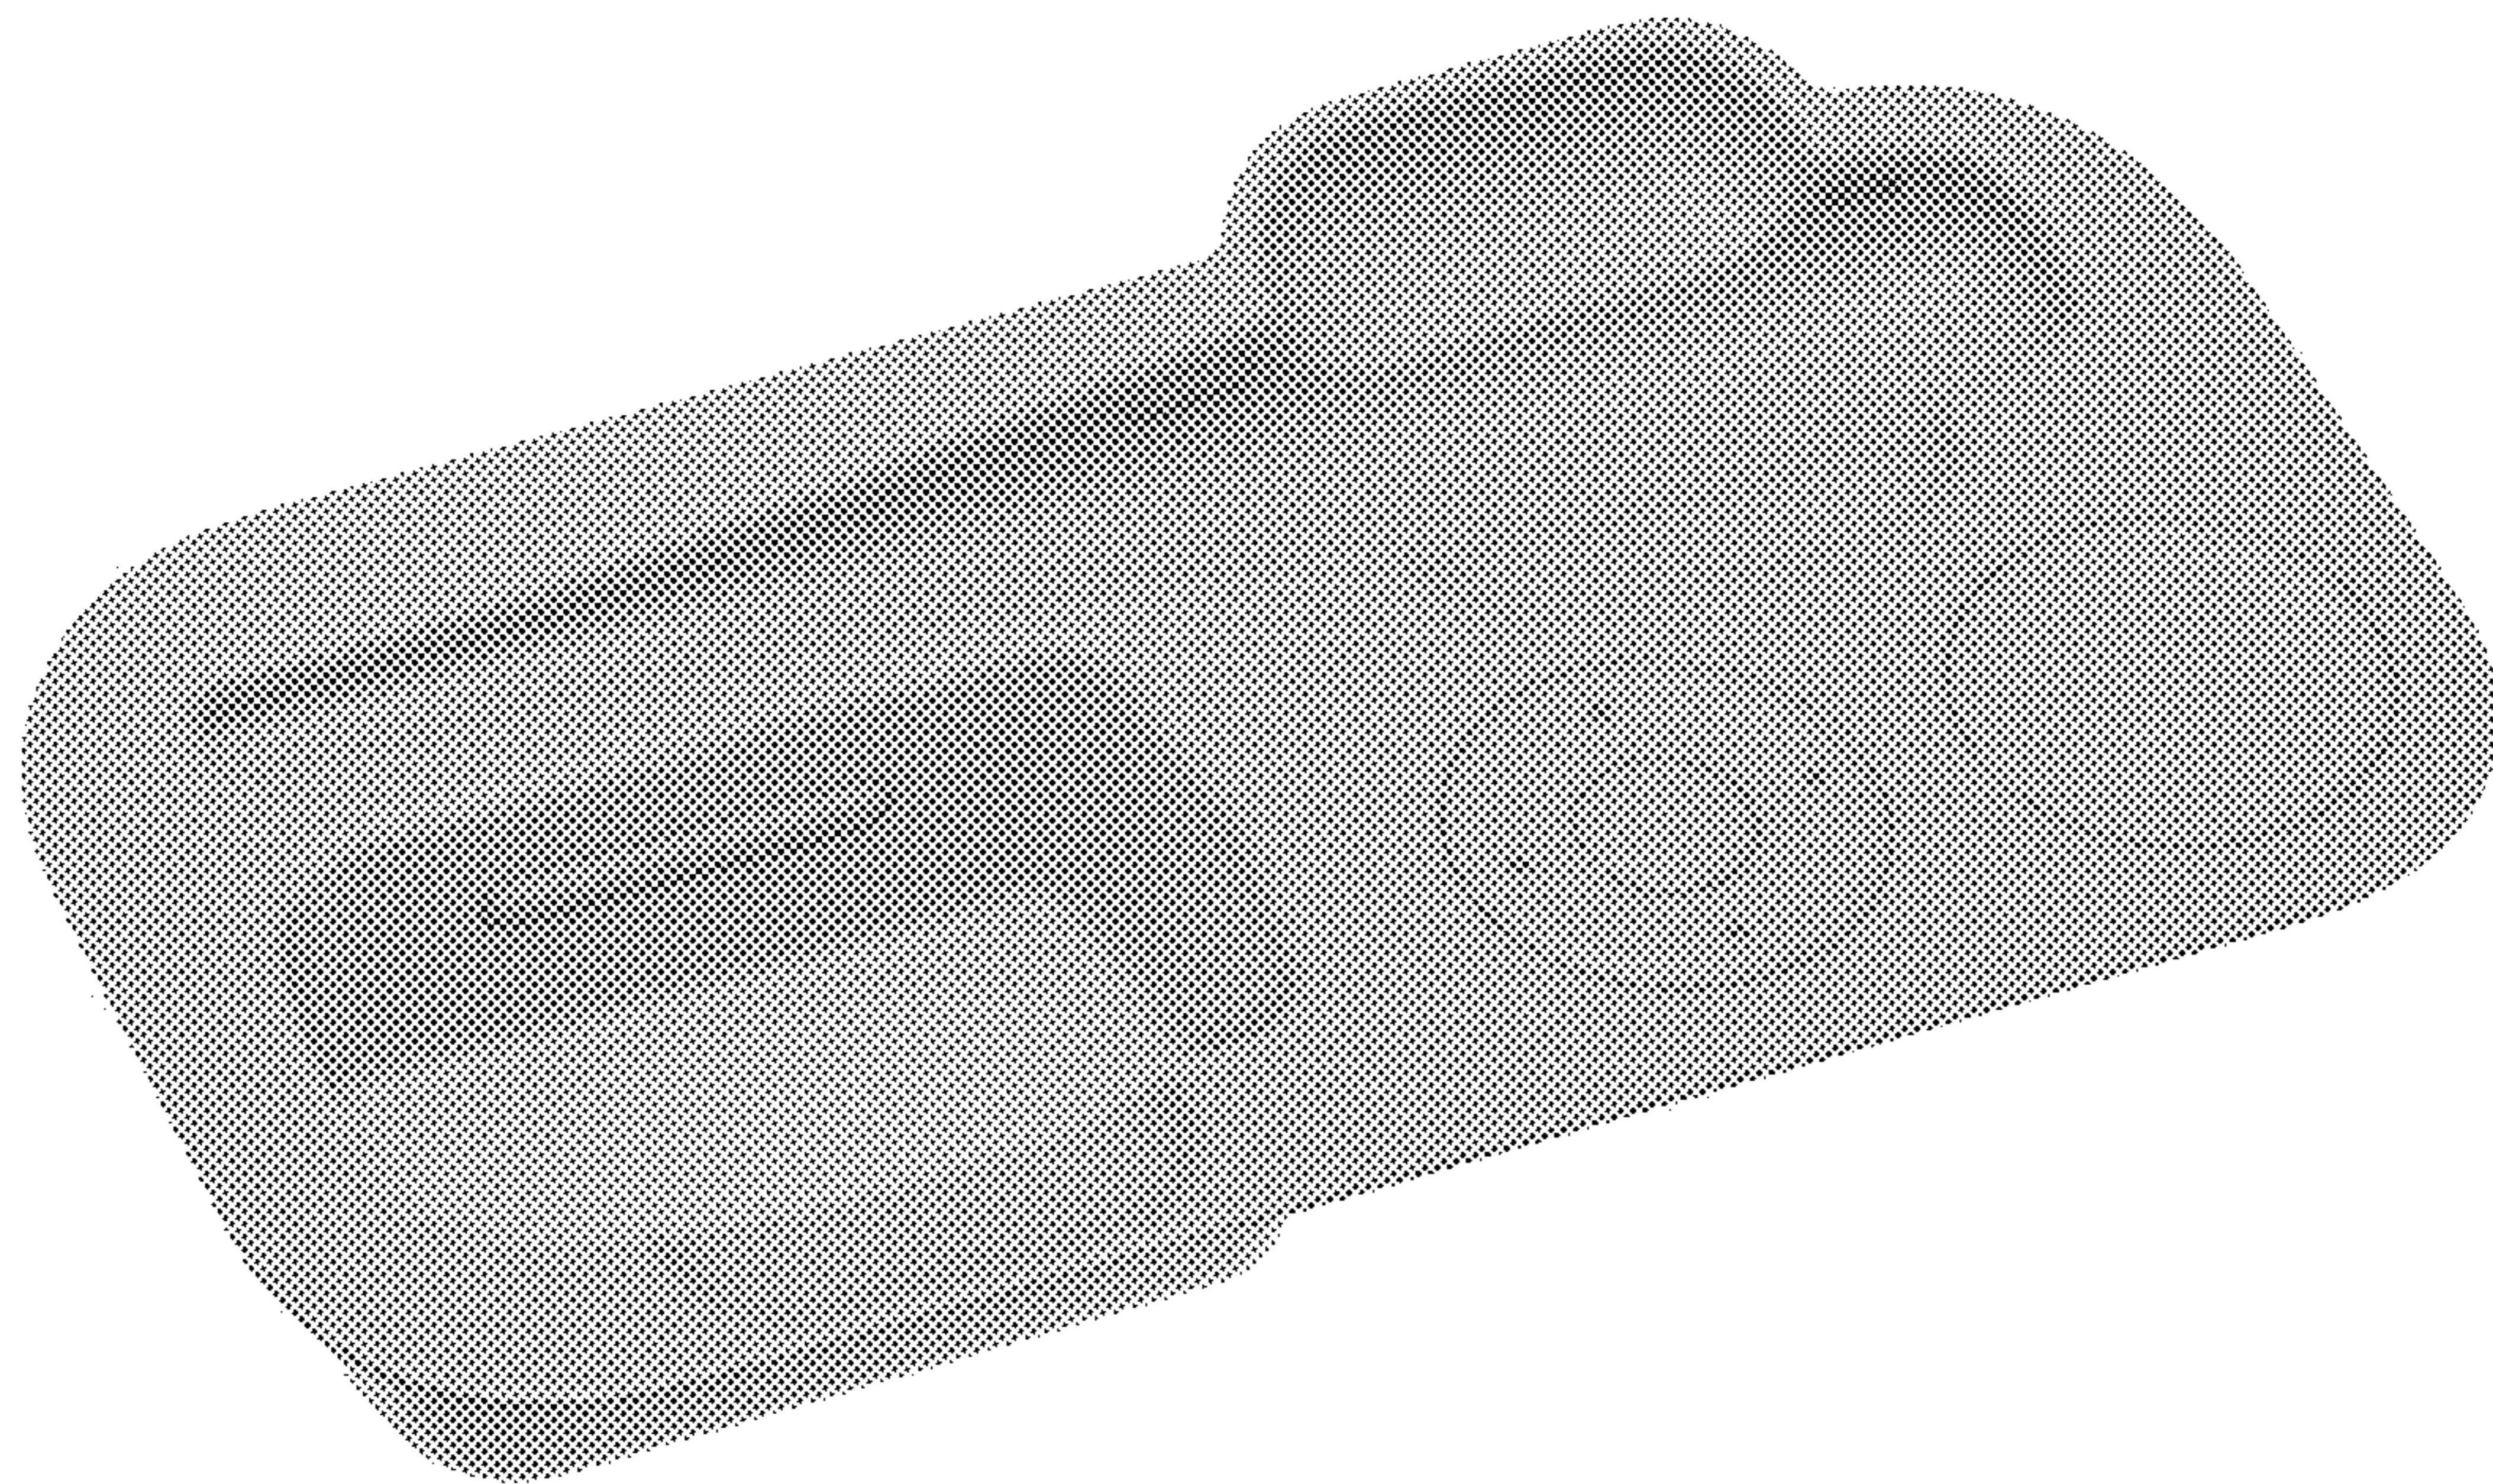


FIG.2

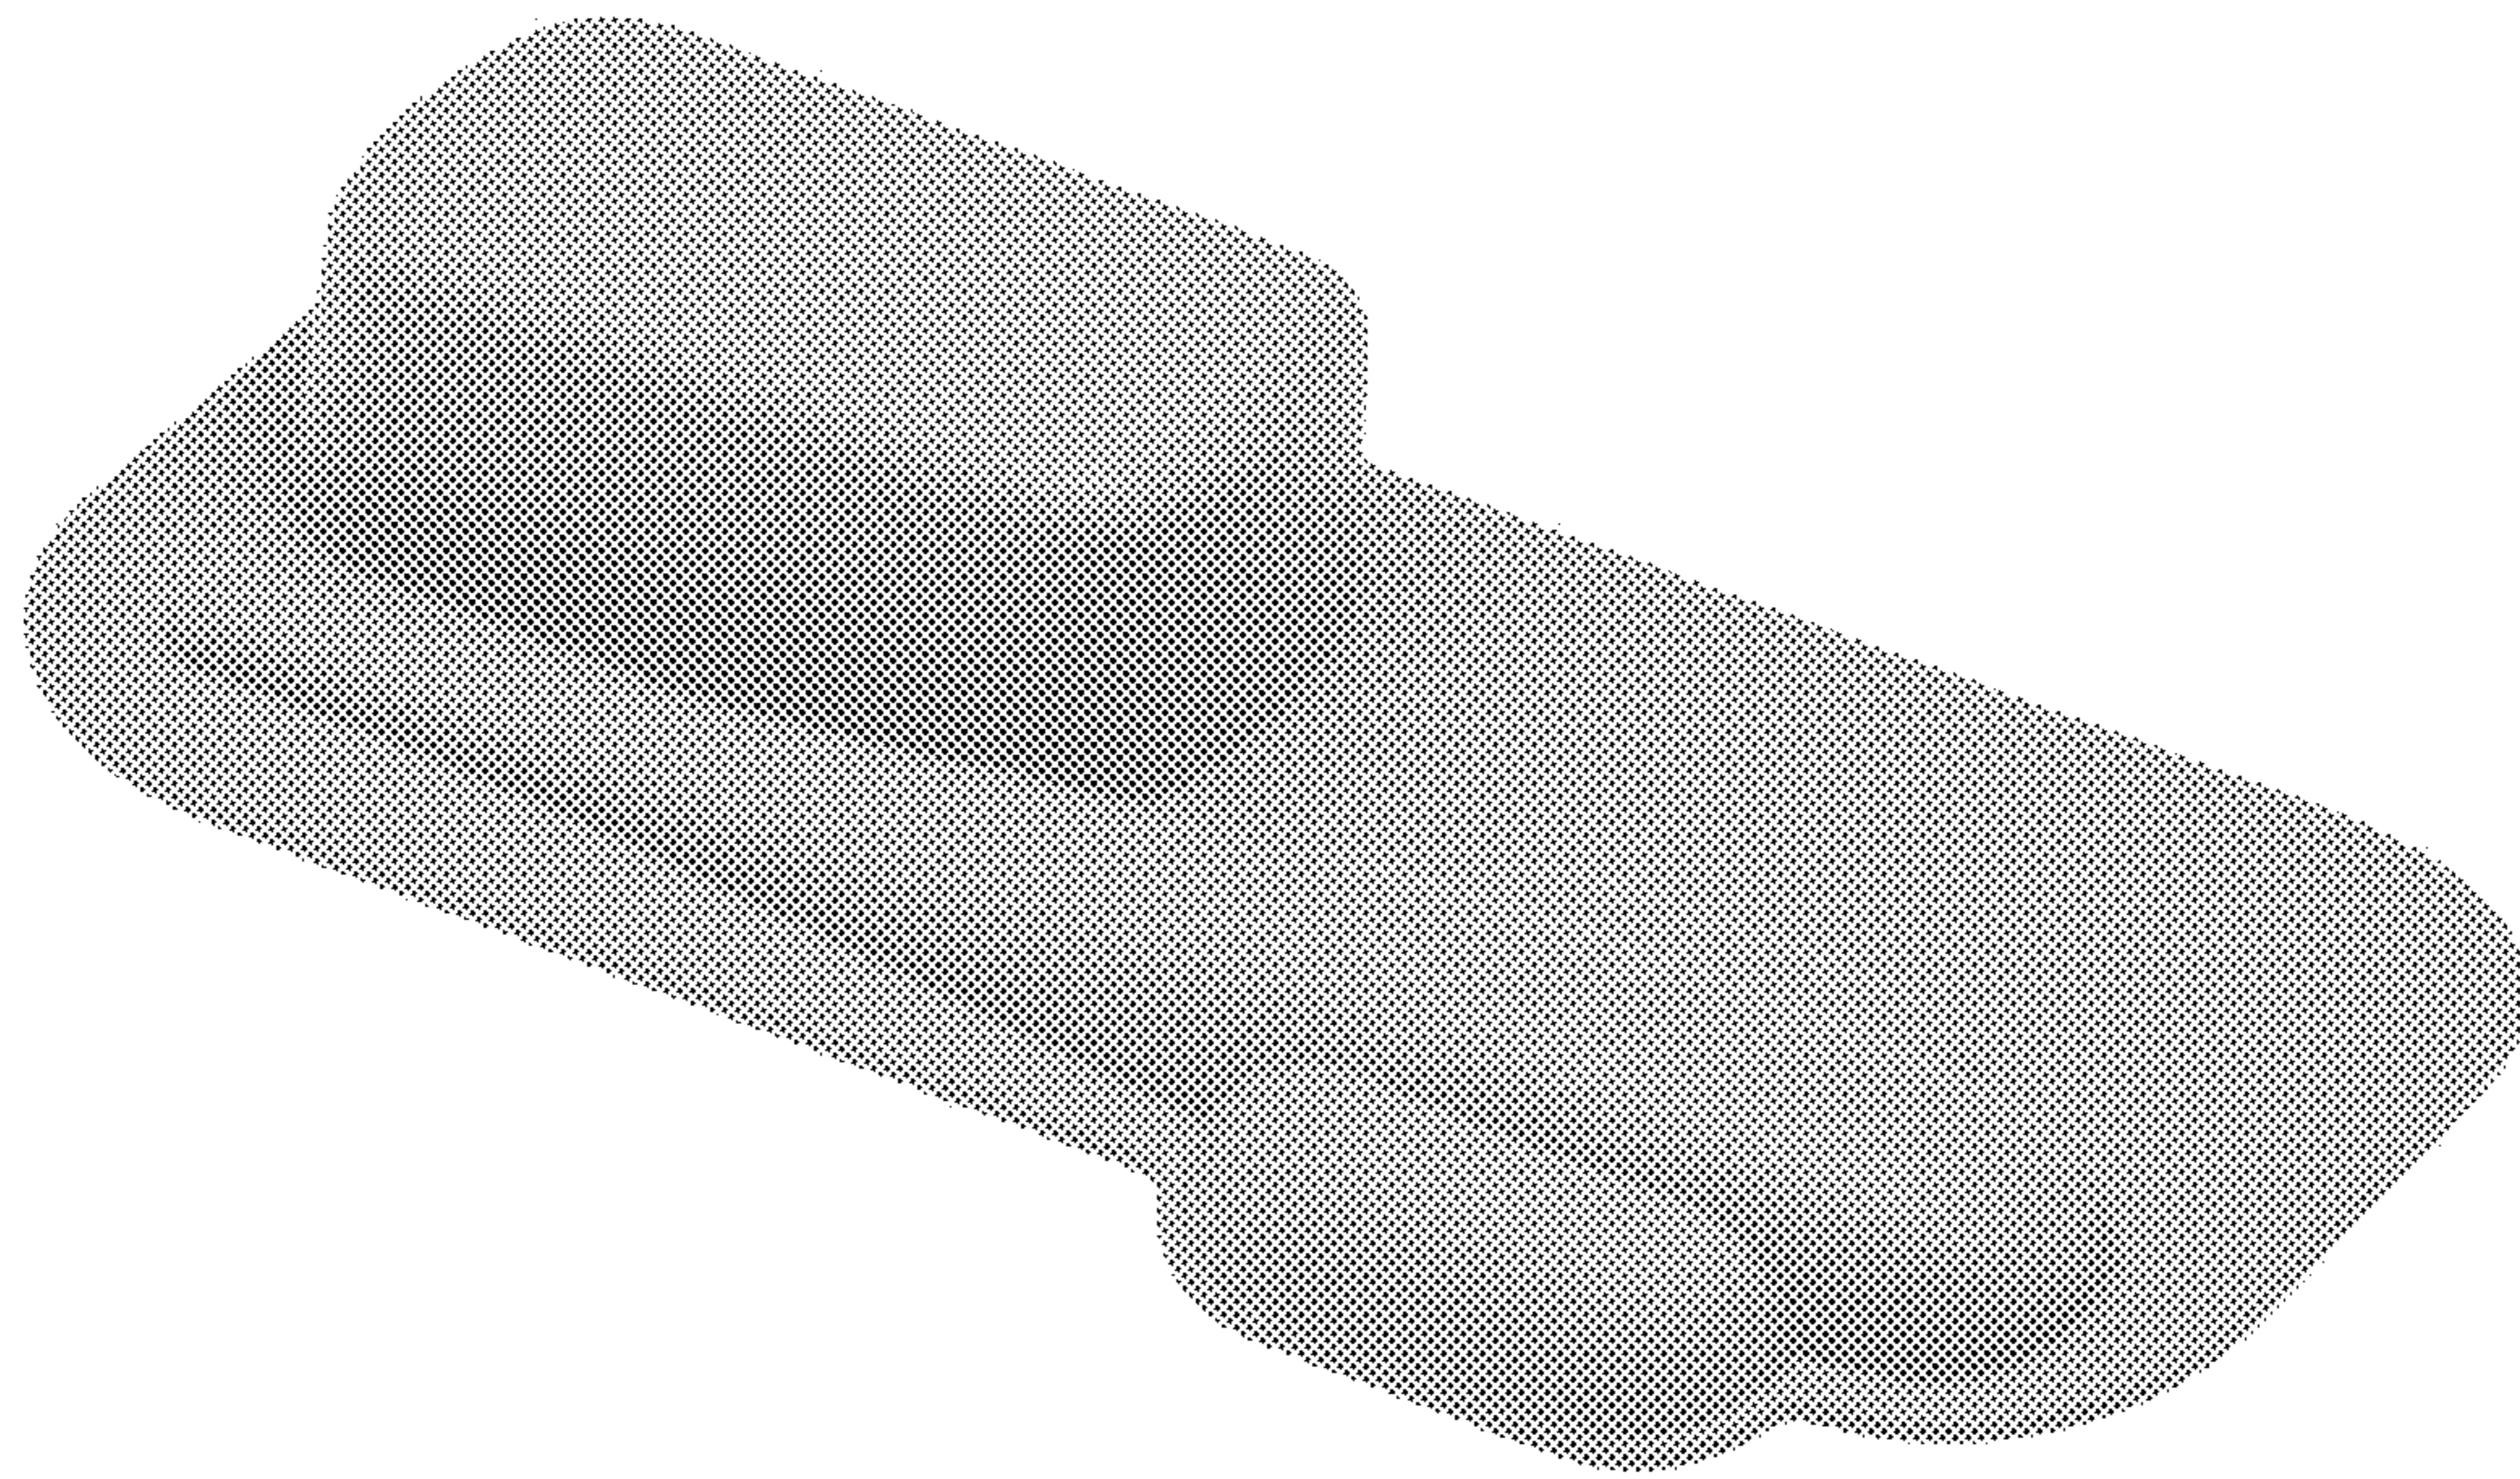


FIG.3

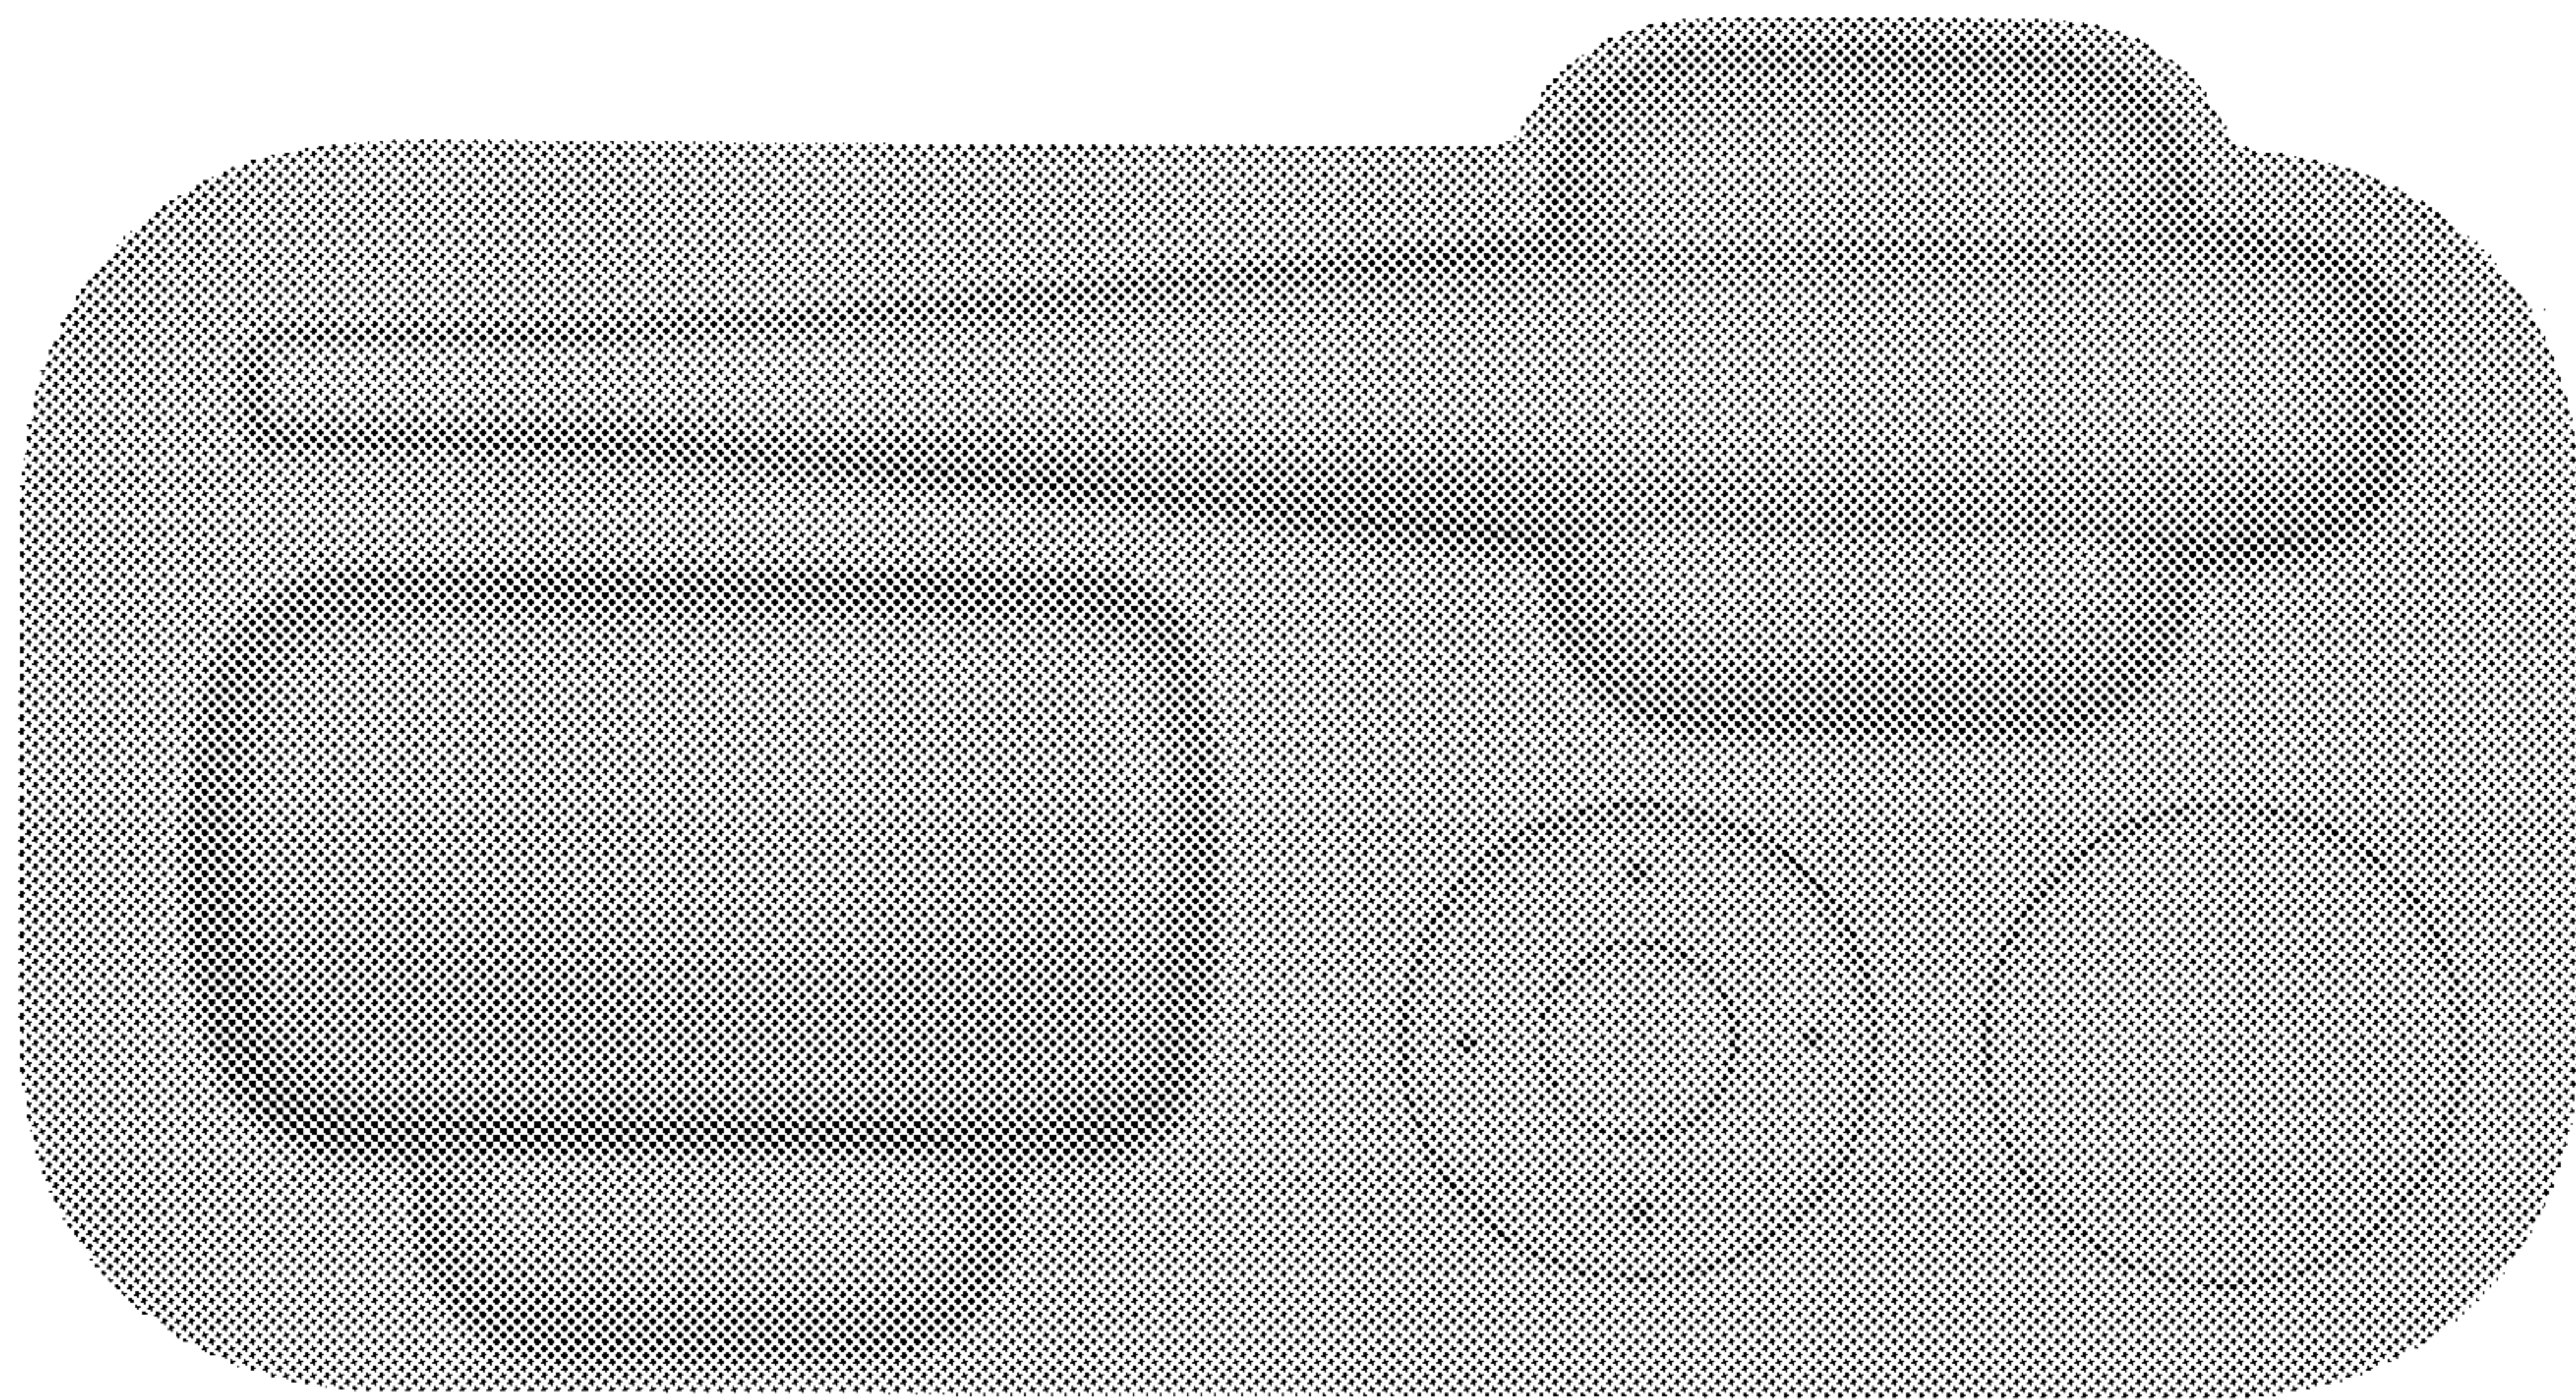


FIG.4

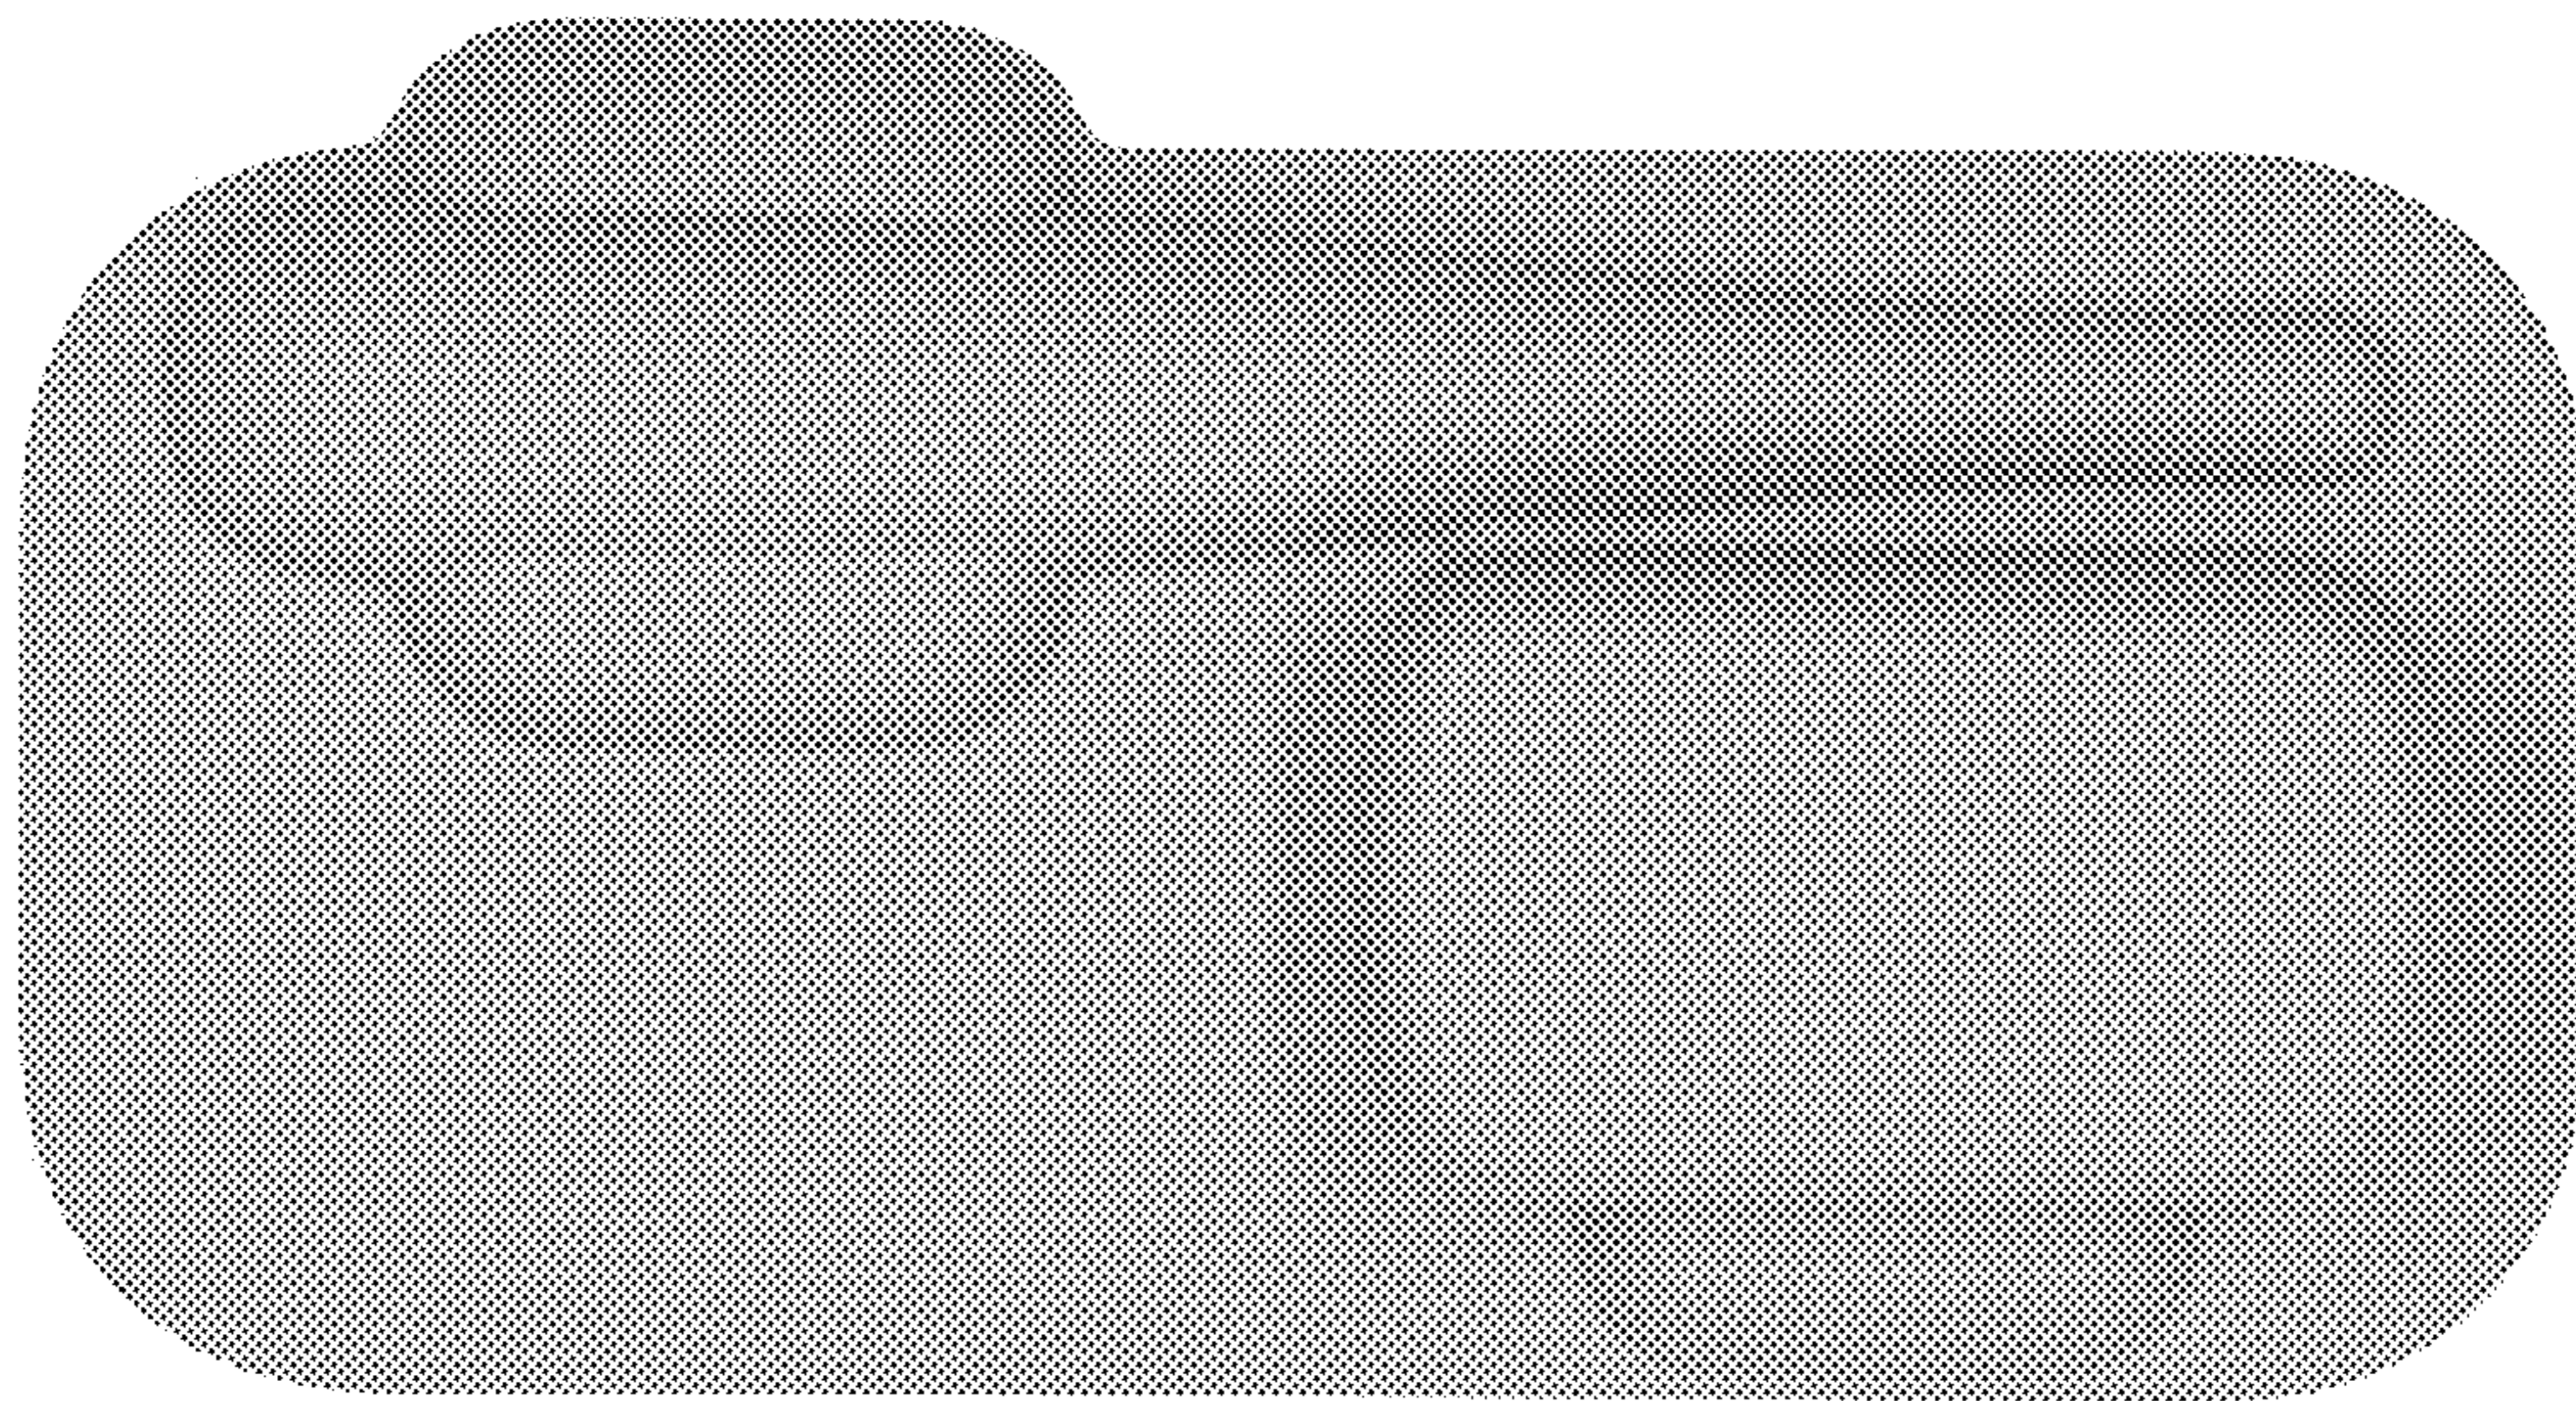


FIG.5

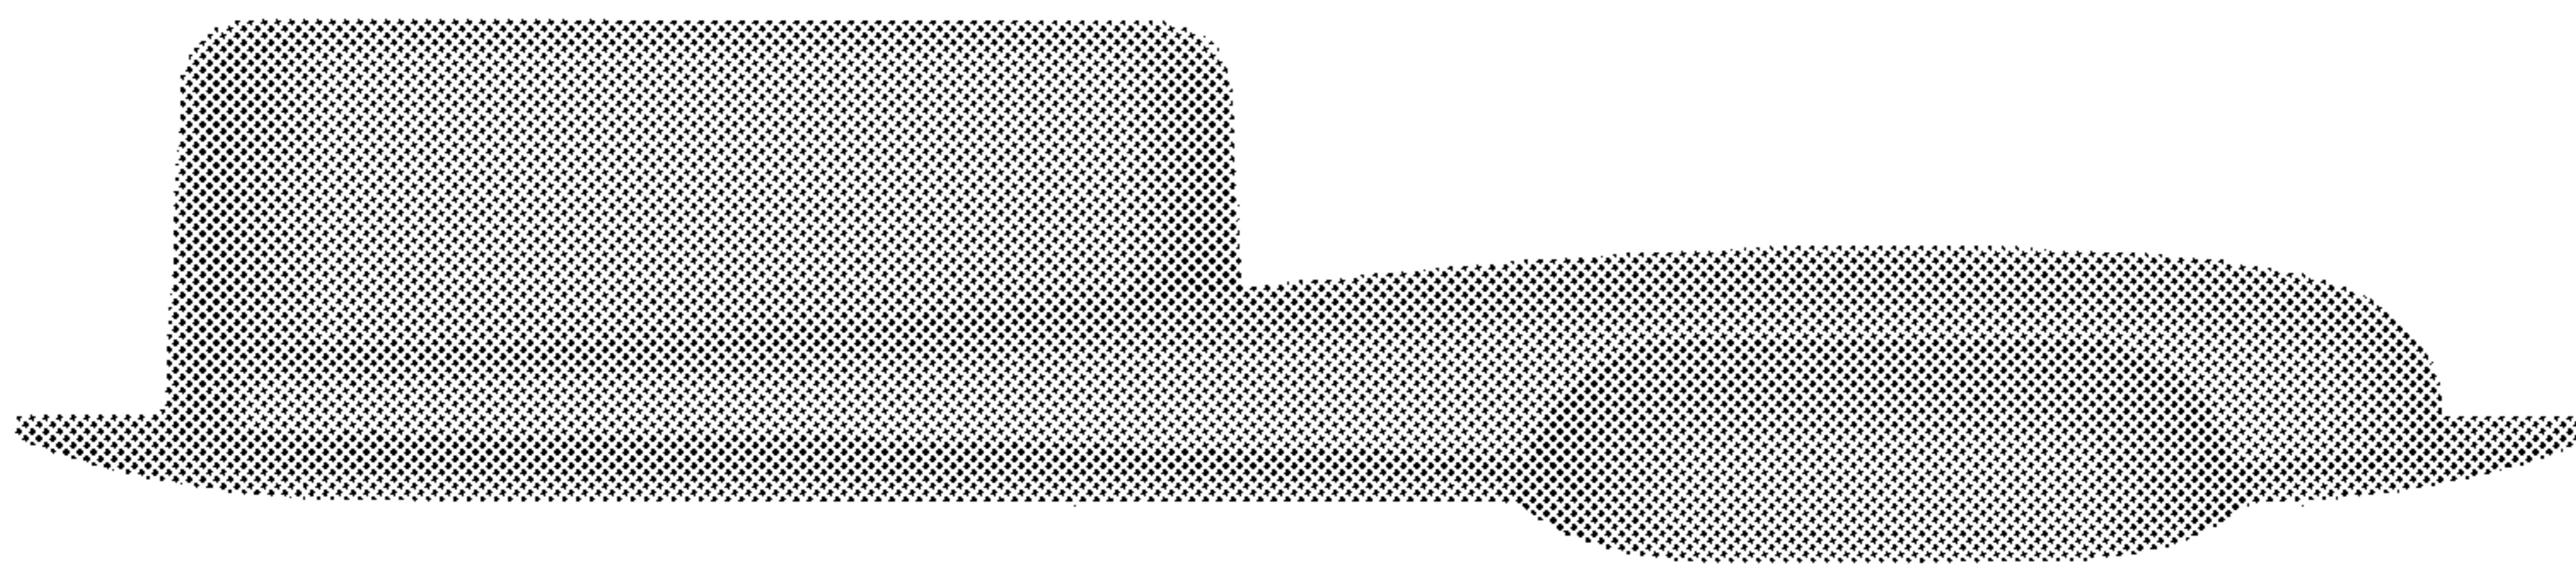


FIG.6

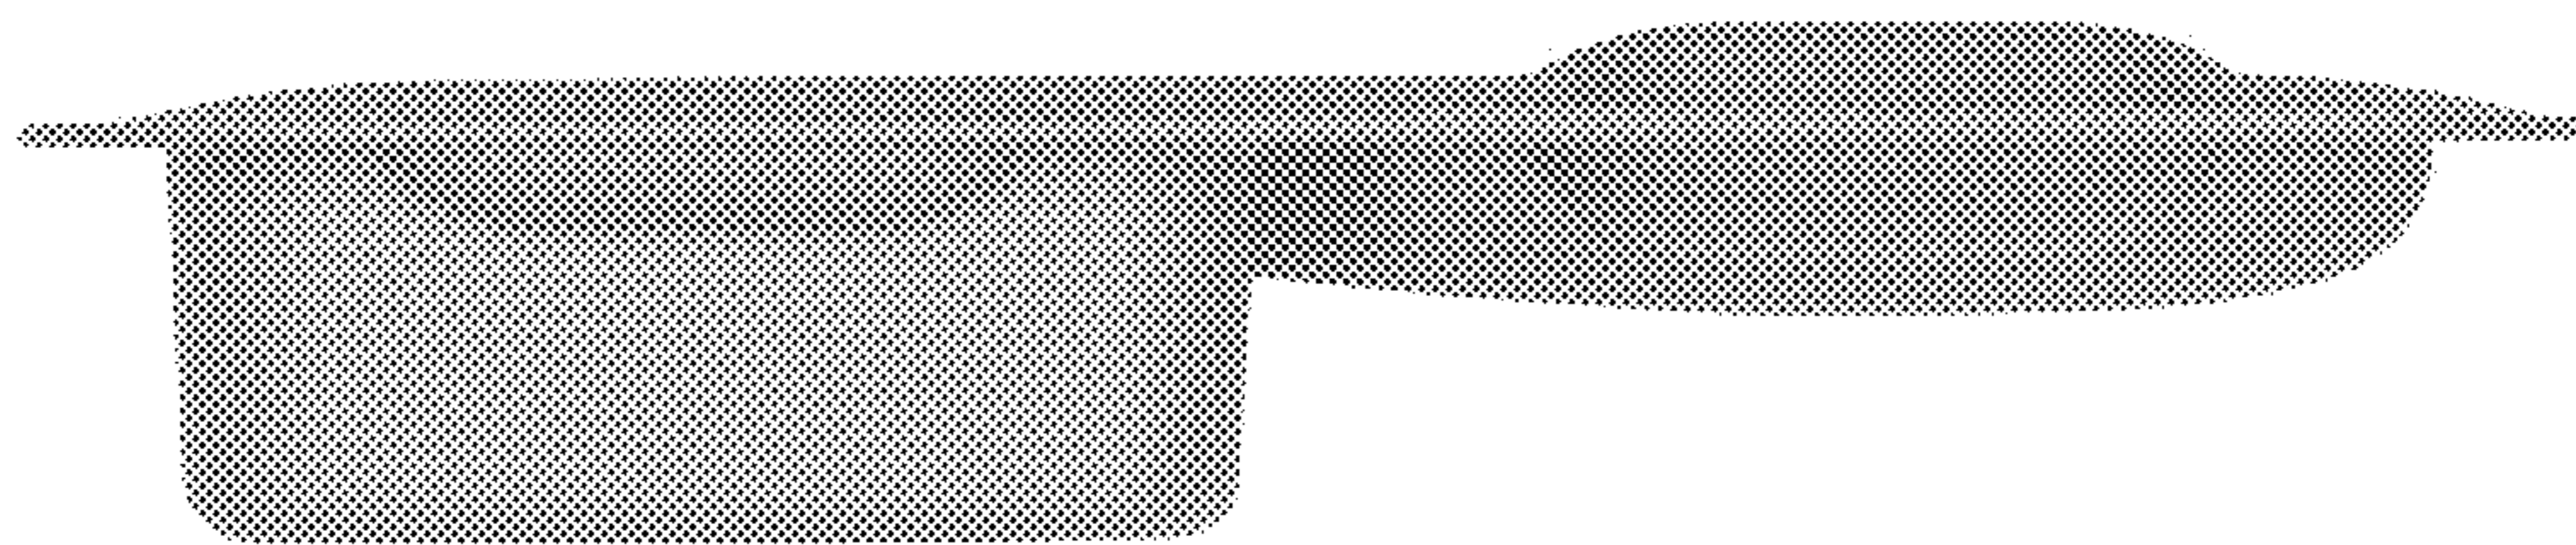


FIG.7

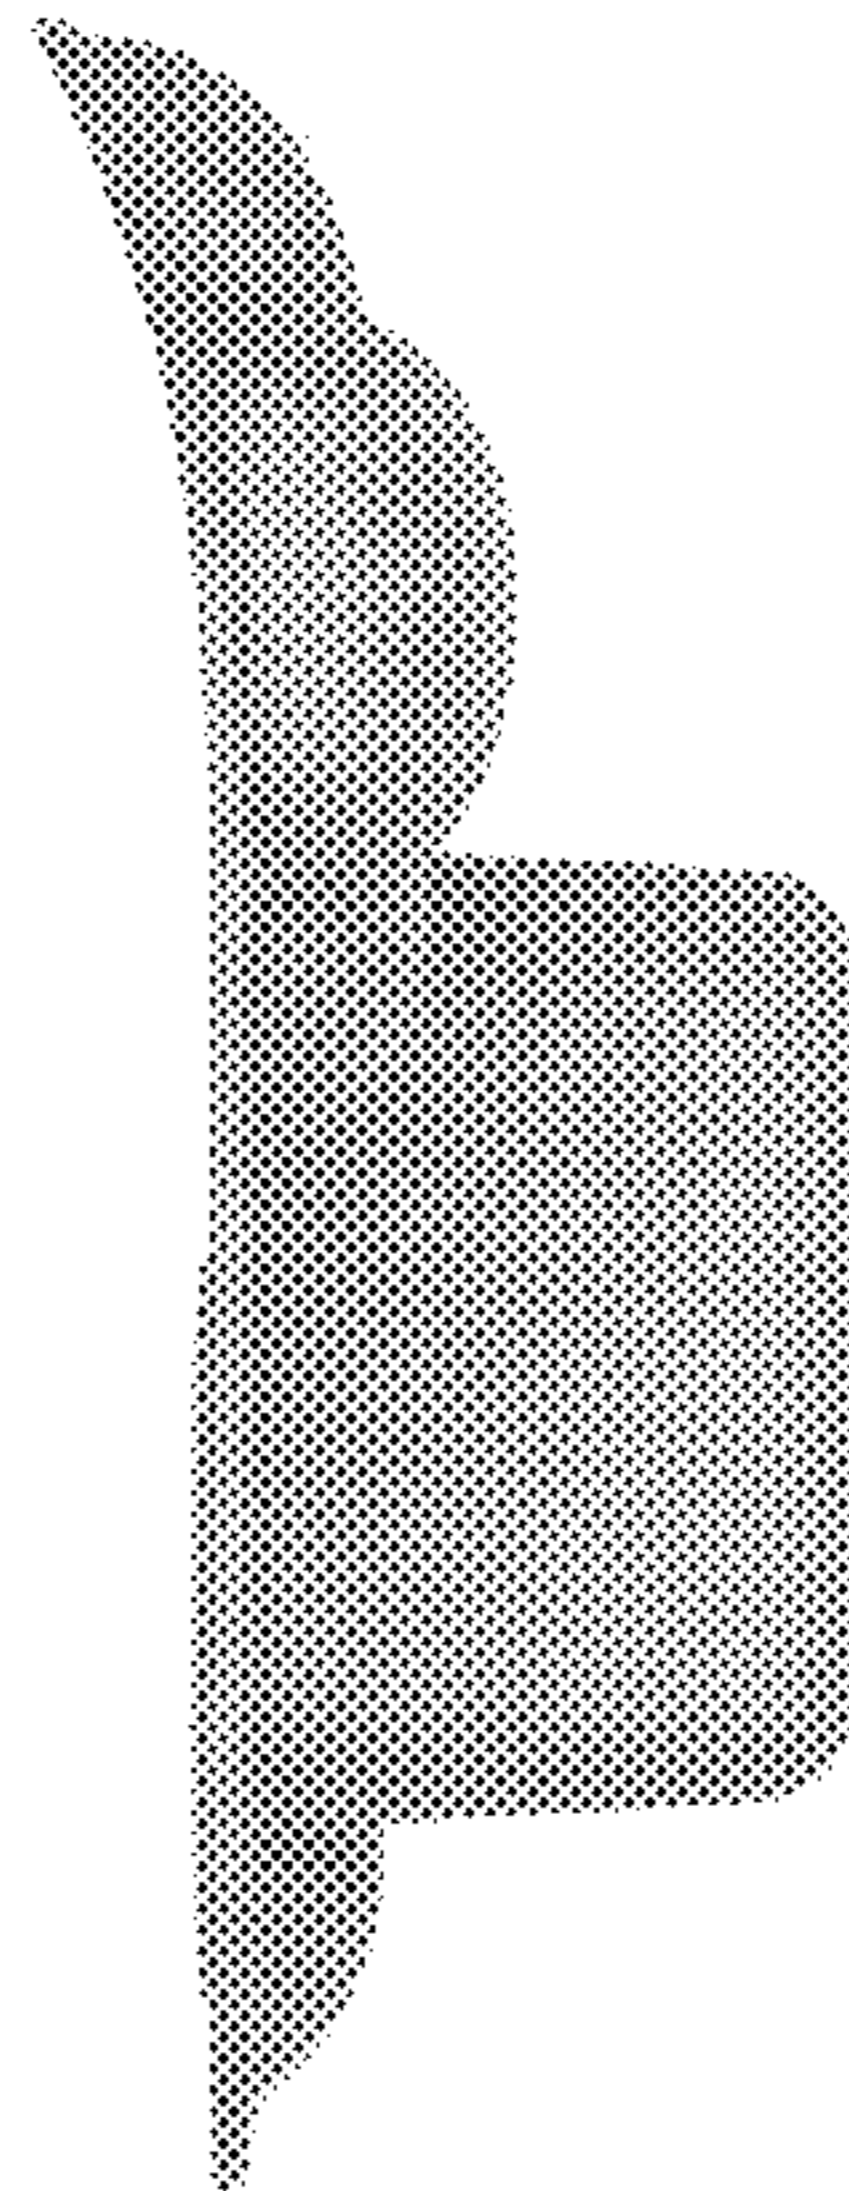




FIG.8

