



US00D709048S

(12) **United States Design Patent**  
**Ganske et al.**

(10) **Patent No.:** **US D709,048 S**  
(45) **Date of Patent:** **\*\* Jul. 15, 2014**

(54) **CONTROLLER FOR REMOTE ISCHEMIC  
CONDITIONING**

(75) Inventors: **Rocky Eugene Ganske**, Ontario (CA);  
**Lahav Gil**, Toronto (CA); **Adam  
Shepperdley**, Toronto (CA); **Son  
Chung**, Toronto (CA)

(73) Assignee: **CellAegis Devices Inc.**, Toronto (CA)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/429,684**

(22) Filed: **Aug. 15, 2012**

**Related U.S. Application Data**

(63) Continuation of application No. 13/088,243, filed on  
Apr. 15, 2011.

(51) **LOC (10) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D14/169**

(58) **Field of Classification Search**  
USPC ..... D24/143, 165–169, 186, 189, 200;  
606/201, 202, 203; 601/84, 149–151;  
602/53; D13/158, 162, 168, 171  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

3,552,383	A	1/1971	Krueger et al.
4,106,002	A	8/1978	Hogue, Jr.
4,206,764	A	6/1980	Williams
4,321,929	A	3/1982	Lemelson et al.
4,664,651	A	5/1987	Weinshenker et al.
4,690,151	A	9/1987	Utsunomiya et al.
4,967,758	A	11/1990	Masciarotte
5,072,736	A	12/1991	Ogawa et al.
5,135,003	A	8/1992	Souma
5,201,758	A	4/1993	Glover

5,267,565	A	12/1993	Beard et al.
D374,931	S *	10/1996	Cesaroni et al. .... D24/169
5,569,304	A	10/1996	Ulrich
5,571,075	A	11/1996	Bullard et al.
5,634,467	A	6/1997	Nevo
5,643,315	A	7/1997	Daneshvar
5,651,369	A	7/1997	Tomita
D420,449	S *	2/2000	Schifrin et al. .... D24/189
6,152,881	A	11/2000	Raines et al.
6,210,423	B1	4/2001	Kim
6,245,023	B1	6/2001	Clemmons
6,251,080	B1	6/2001	Henkin et al.

(Continued)

**FOREIGN PATENT DOCUMENTS**

EP	1016379	5/2000
GB	1323365	7/1973

(Continued)

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Wolf, Greenfield & Sacks,  
P.C.


(57) **CLAIM**

The ornamental design for a controller for remote ischemic conditioning, as shown and described.

**DESCRIPTION**

FIG. 1 is a top perspective view of the controller for remote ischemic conditioning;  
FIG. 2 is a bottom perspective view thereof;  
FIG. 3 is a top plan view thereof;  
FIG. 4 bottom plan view thereof  
FIG. 5 is a left side elevational view thereof;  
FIG. 6 is a rear elevational view thereof; and,  
FIG. 7 is a front elevational view thereof.  
The broken lines in the drawing views illustrate unclaimed portions of the controller for remote ischemic conditioning and form no part of the claimed design.

**1 Claim, 3 Drawing Sheets**

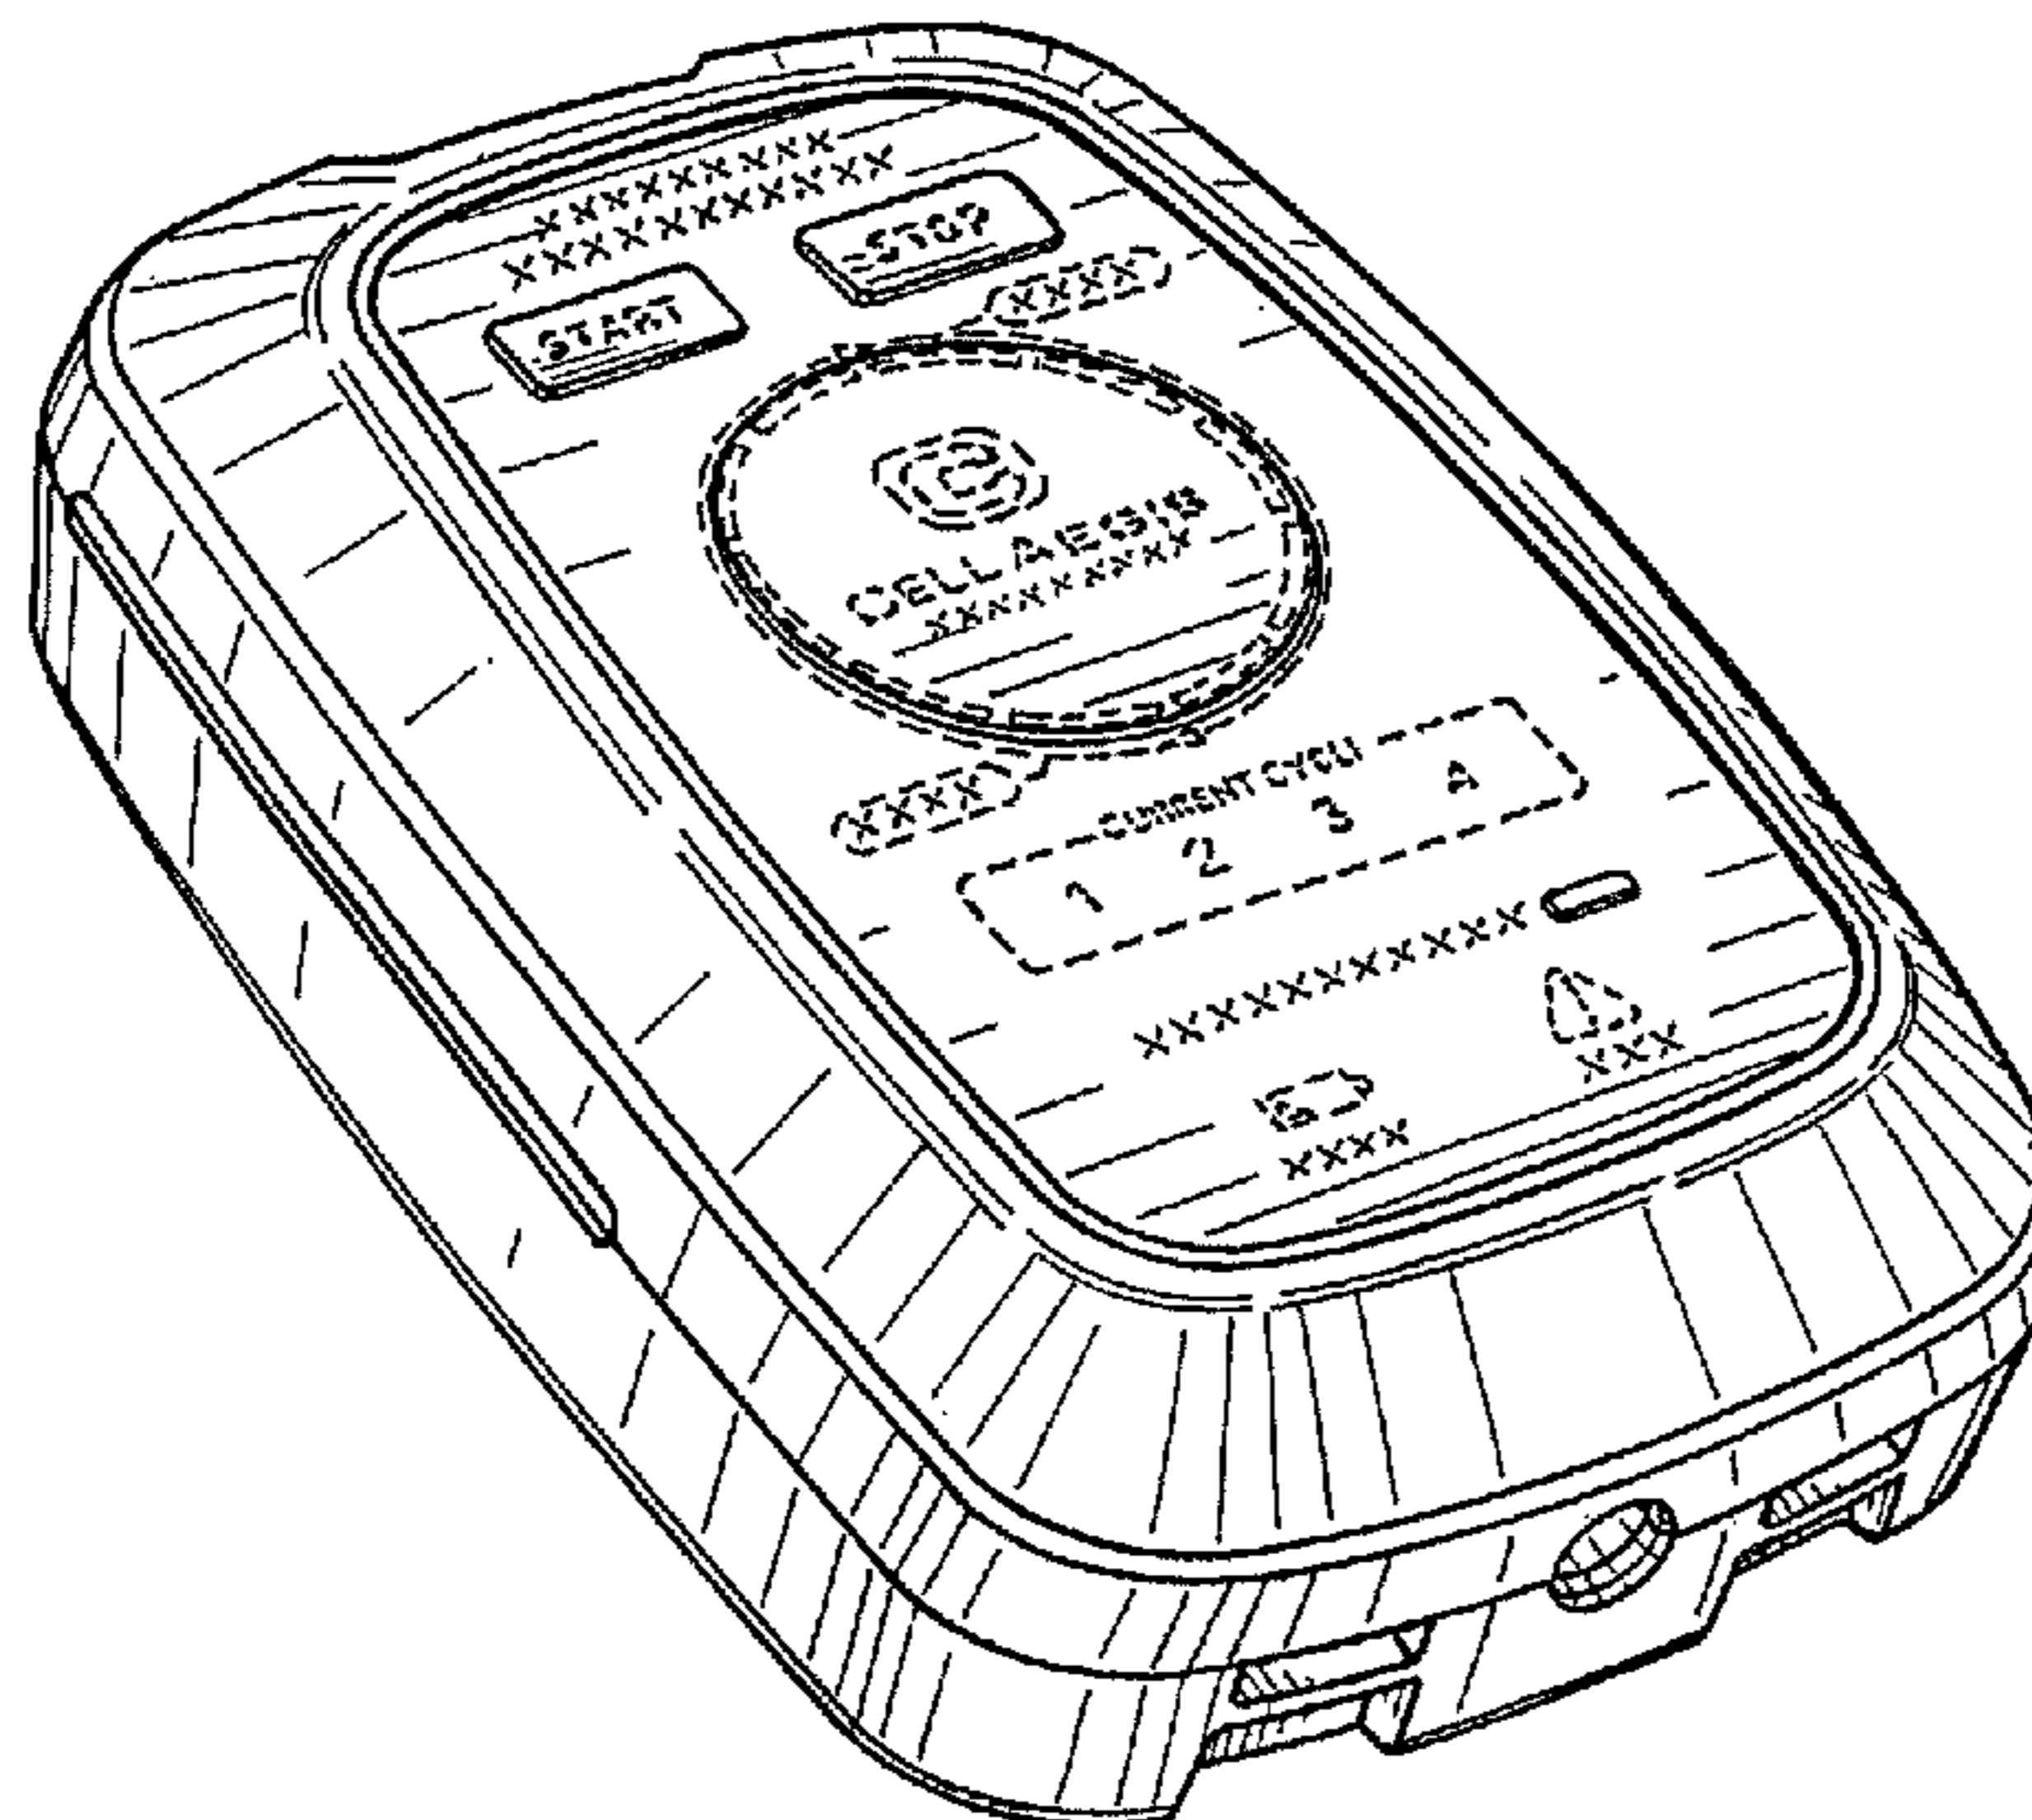

(56)

References Cited

U.S. PATENT DOCUMENTS


D462,450 S \* 9/2002 Robinette ..... D24/200  
 6,485,429 B2 11/2002 Forstner  
 6,550,482 B1 4/2003 Burbank et al.  
 D476,421 S \* 6/2003 Heston ..... D24/169  
 6,626,840 B2 9/2003 Drzewiecki et al.  
 6,702,720 B2 3/2004 Dardik  
 6,719,704 B2 4/2004 Narimatsu et al.  
 6,858,012 B2 2/2005 Burns et al.  
 6,962,599 B2 11/2005 Hui  
 7,004,907 B2 2/2006 Banet et al.  
 D517,695 S \* 3/2006 Gillis et al. .... D24/169  
 7,018,335 B2 3/2006 Kario et al.  
 7,048,702 B2 5/2006 Hui  
 7,111,346 B2 9/2006 Inman et al.  
 7,166,077 B2 1/2007 Millay et al.  
 7,228,576 B2 6/2007 Inman et al.  
 7,314,478 B2 1/2008 Hui  
 7,338,410 B2 3/2008 Dardik et al.  
 7,374,540 B2 5/2008 Schnall et al.  
 7,390,303 B2 6/2008 Dafni  
 7,404,221 B2 7/2008 Sackner  
 7,427,268 B2 9/2008 Millay et al.  
 7,485,131 B2 2/2009 Hovanes et al.  
 7,689,286 B2 3/2010 Pastore et al.  
 7,717,855 B2 5/2010 Caldarone et al.  
 7,885,710 B2 2/2011 Sih et al.  
 D642,281 S \* 7/2011 Bachinski ..... D24/200  
 8,114,026 B2 2/2012 Leschinsky  
 8,246,548 B2 8/2012 Naghavi  
 D672,727 S \* 12/2012 McCullar et al. .... D13/168  
 D701,610 S \* 3/2014 Thomas et al. .... D24/200  
 2001/0029389 A1 10/2001 Kim et al.  
 2003/0013974 A1 1/2003 Natarajan et al.  
 2003/0065270 A1 4/2003 Raines et al.  
 2003/0176795 A1 9/2003 Harris et al.  
 2003/0216651 A1 11/2003 Burns et al.  
 2003/0233118 A1 12/2003 Hui  
 2004/0044290 A1 3/2004 Ward et al.  
 2004/0064076 A1 4/2004 Bilgi et al.  
 2004/0102818 A1 5/2004 Hakky et al.  
 2004/0241634 A1 12/2004 Millis et al.  
 2004/0255956 A1 12/2004 Vinten-Johansen  
 2005/0004476 A1 1/2005 Payvar et al.  
 2005/0070405 A1 3/2005 Egger  
 2005/0159640 A1 7/2005 Barbut et al.  
 2005/0171444 A1 8/2005 Ono et al.

2005/0177078 A1 8/2005 Loeb et al.  
 2006/0052712 A1 3/2006 Poliac et al.  
 2006/0052713 A1 3/2006 Poliac et al.  
 2006/0052714 A1 3/2006 Poliac et al.  
 2006/0058717 A1 3/2006 Hui et al.  
 2006/0100639 A1 5/2006 Levin et al.  
 2006/0142663 A1 6/2006 Sawanoi et al.  
 2007/0005106 A1 1/2007 Adducci  
 2007/0055188 A1\* 3/2007 Avni et al. .... 601/151  
 2007/0135836 A1 6/2007 McEwen et al.  
 2007/0150005 A1 6/2007 Sih et al.  
 2007/0247304 A1 10/2007 Bonnefin et al.  
 2008/0139949 A1 6/2008 Caldarone et al.  
 2008/0222769 A1 9/2008 Natanson et al.  
 2009/0036785 A1 2/2009 Danielsson  
 2009/0124912 A1 5/2009 McEwen et al.  
 2009/0137884 A1 5/2009 Naghavi et al.  
 2009/0287069 A1 11/2009 Naghavi et al.  
 2009/0318818 A1\* 12/2009 Whitaker et al. .... 600/495  
 2009/0324748 A1 12/2009 Dobson  
 2010/0081941 A1 4/2010 Naghavi et al.  
 2010/0081977 A1 4/2010 Vess  
 2010/0105993 A1 4/2010 Naghavi et al.  
 2010/0160799 A1 6/2010 Caldarone et al.  
 2010/0185220 A1 7/2010 Naghavi et al.  
 2010/0186752 A1 7/2010 Rixson  
 2010/0268130 A1 10/2010 Khan  
 2010/0292619 A1 11/2010 Redington et al.  
 2010/0305607 A1 12/2010 Caldarone et al.  
 2010/0322467 A1 12/2010 Reed et al.  
 2010/0324429 A1 12/2010 Leschinsky  
 2010/0328142 A1 12/2010 Zoughi et al.  
 2011/0077566 A1 3/2011 Ganapathy  
 2011/0190807 A1 8/2011 Redington et al.  
 2011/0238107 A1 9/2011 Raheman  
 2011/0240043 A1 10/2011 Redington  
 2011/0251635 A1 10/2011 Caldarone  
 2012/0130419 A1 5/2012 Leschinsky  
 2012/0209153 A1\* 8/2012 Farrow et al. .... 601/18  
 2012/0265240 A1 10/2012 Ganske


FOREIGN PATENT DOCUMENTS

JP 2001221 1/1990  
 WO WO 91/18571 12/1991  
 WO WO 2006/024871 3/2006  
 WO WO 2007/085828 8/2007

\* cited by examiner

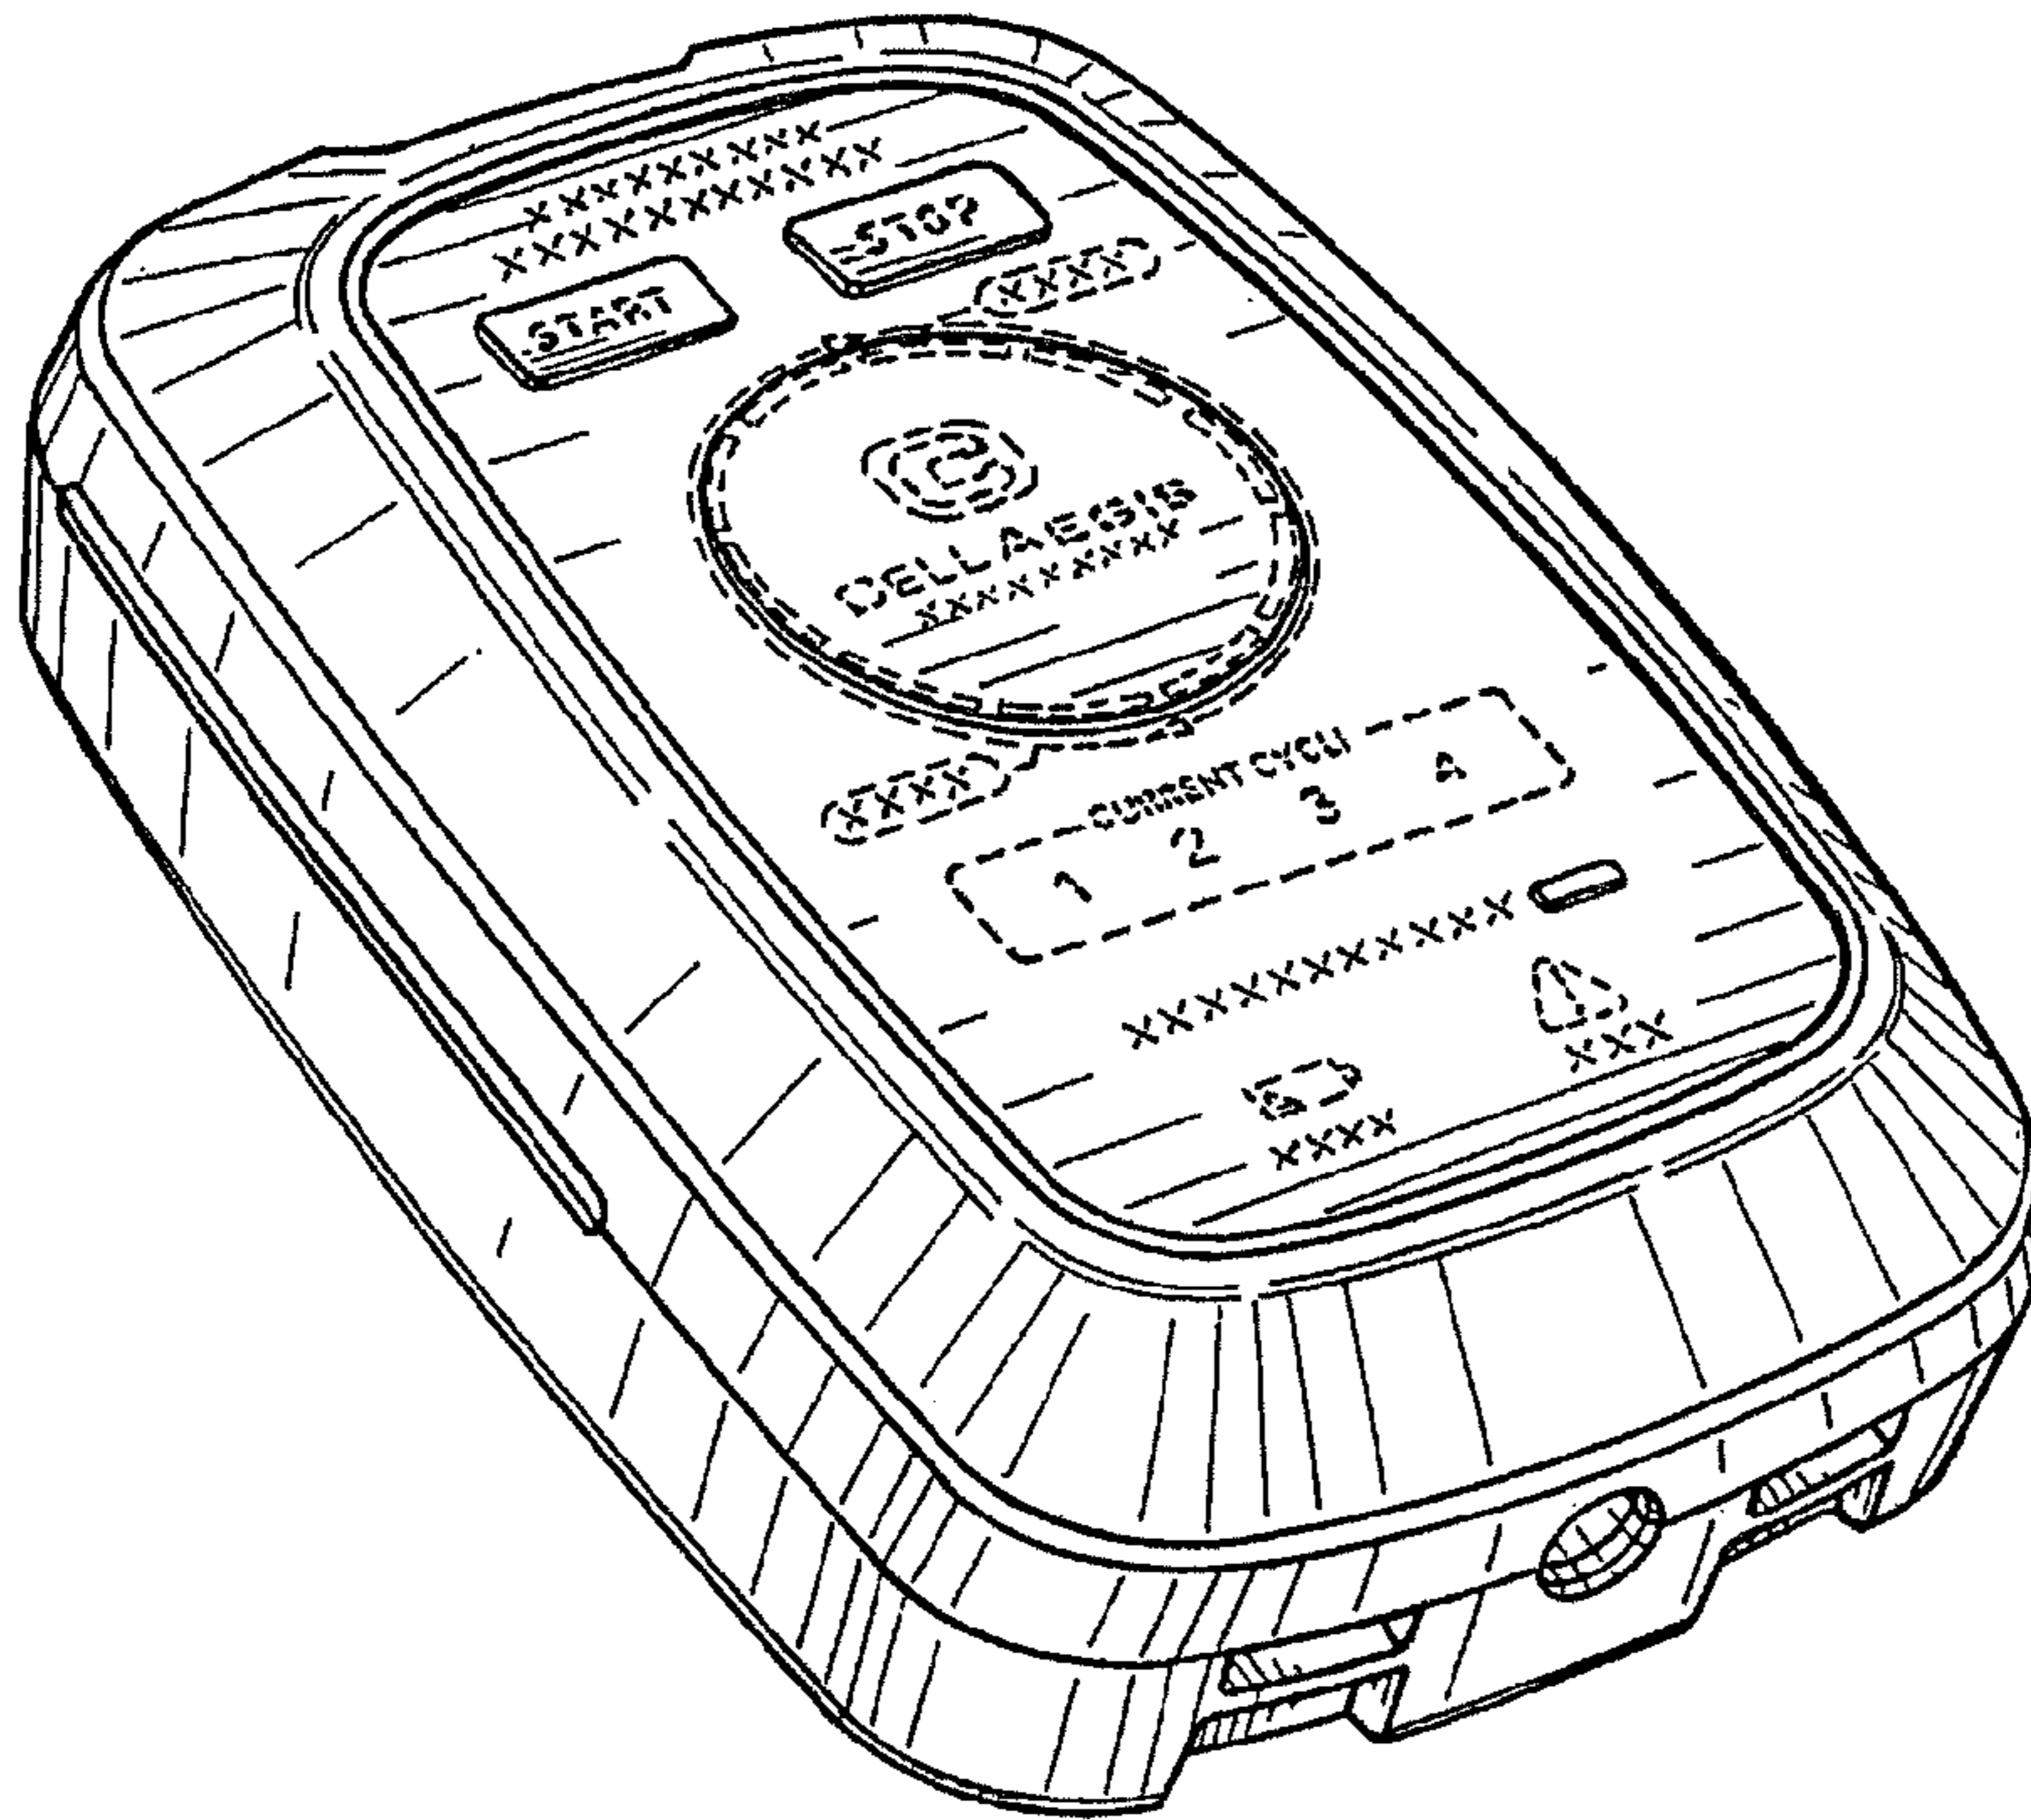

*Fig. 1*

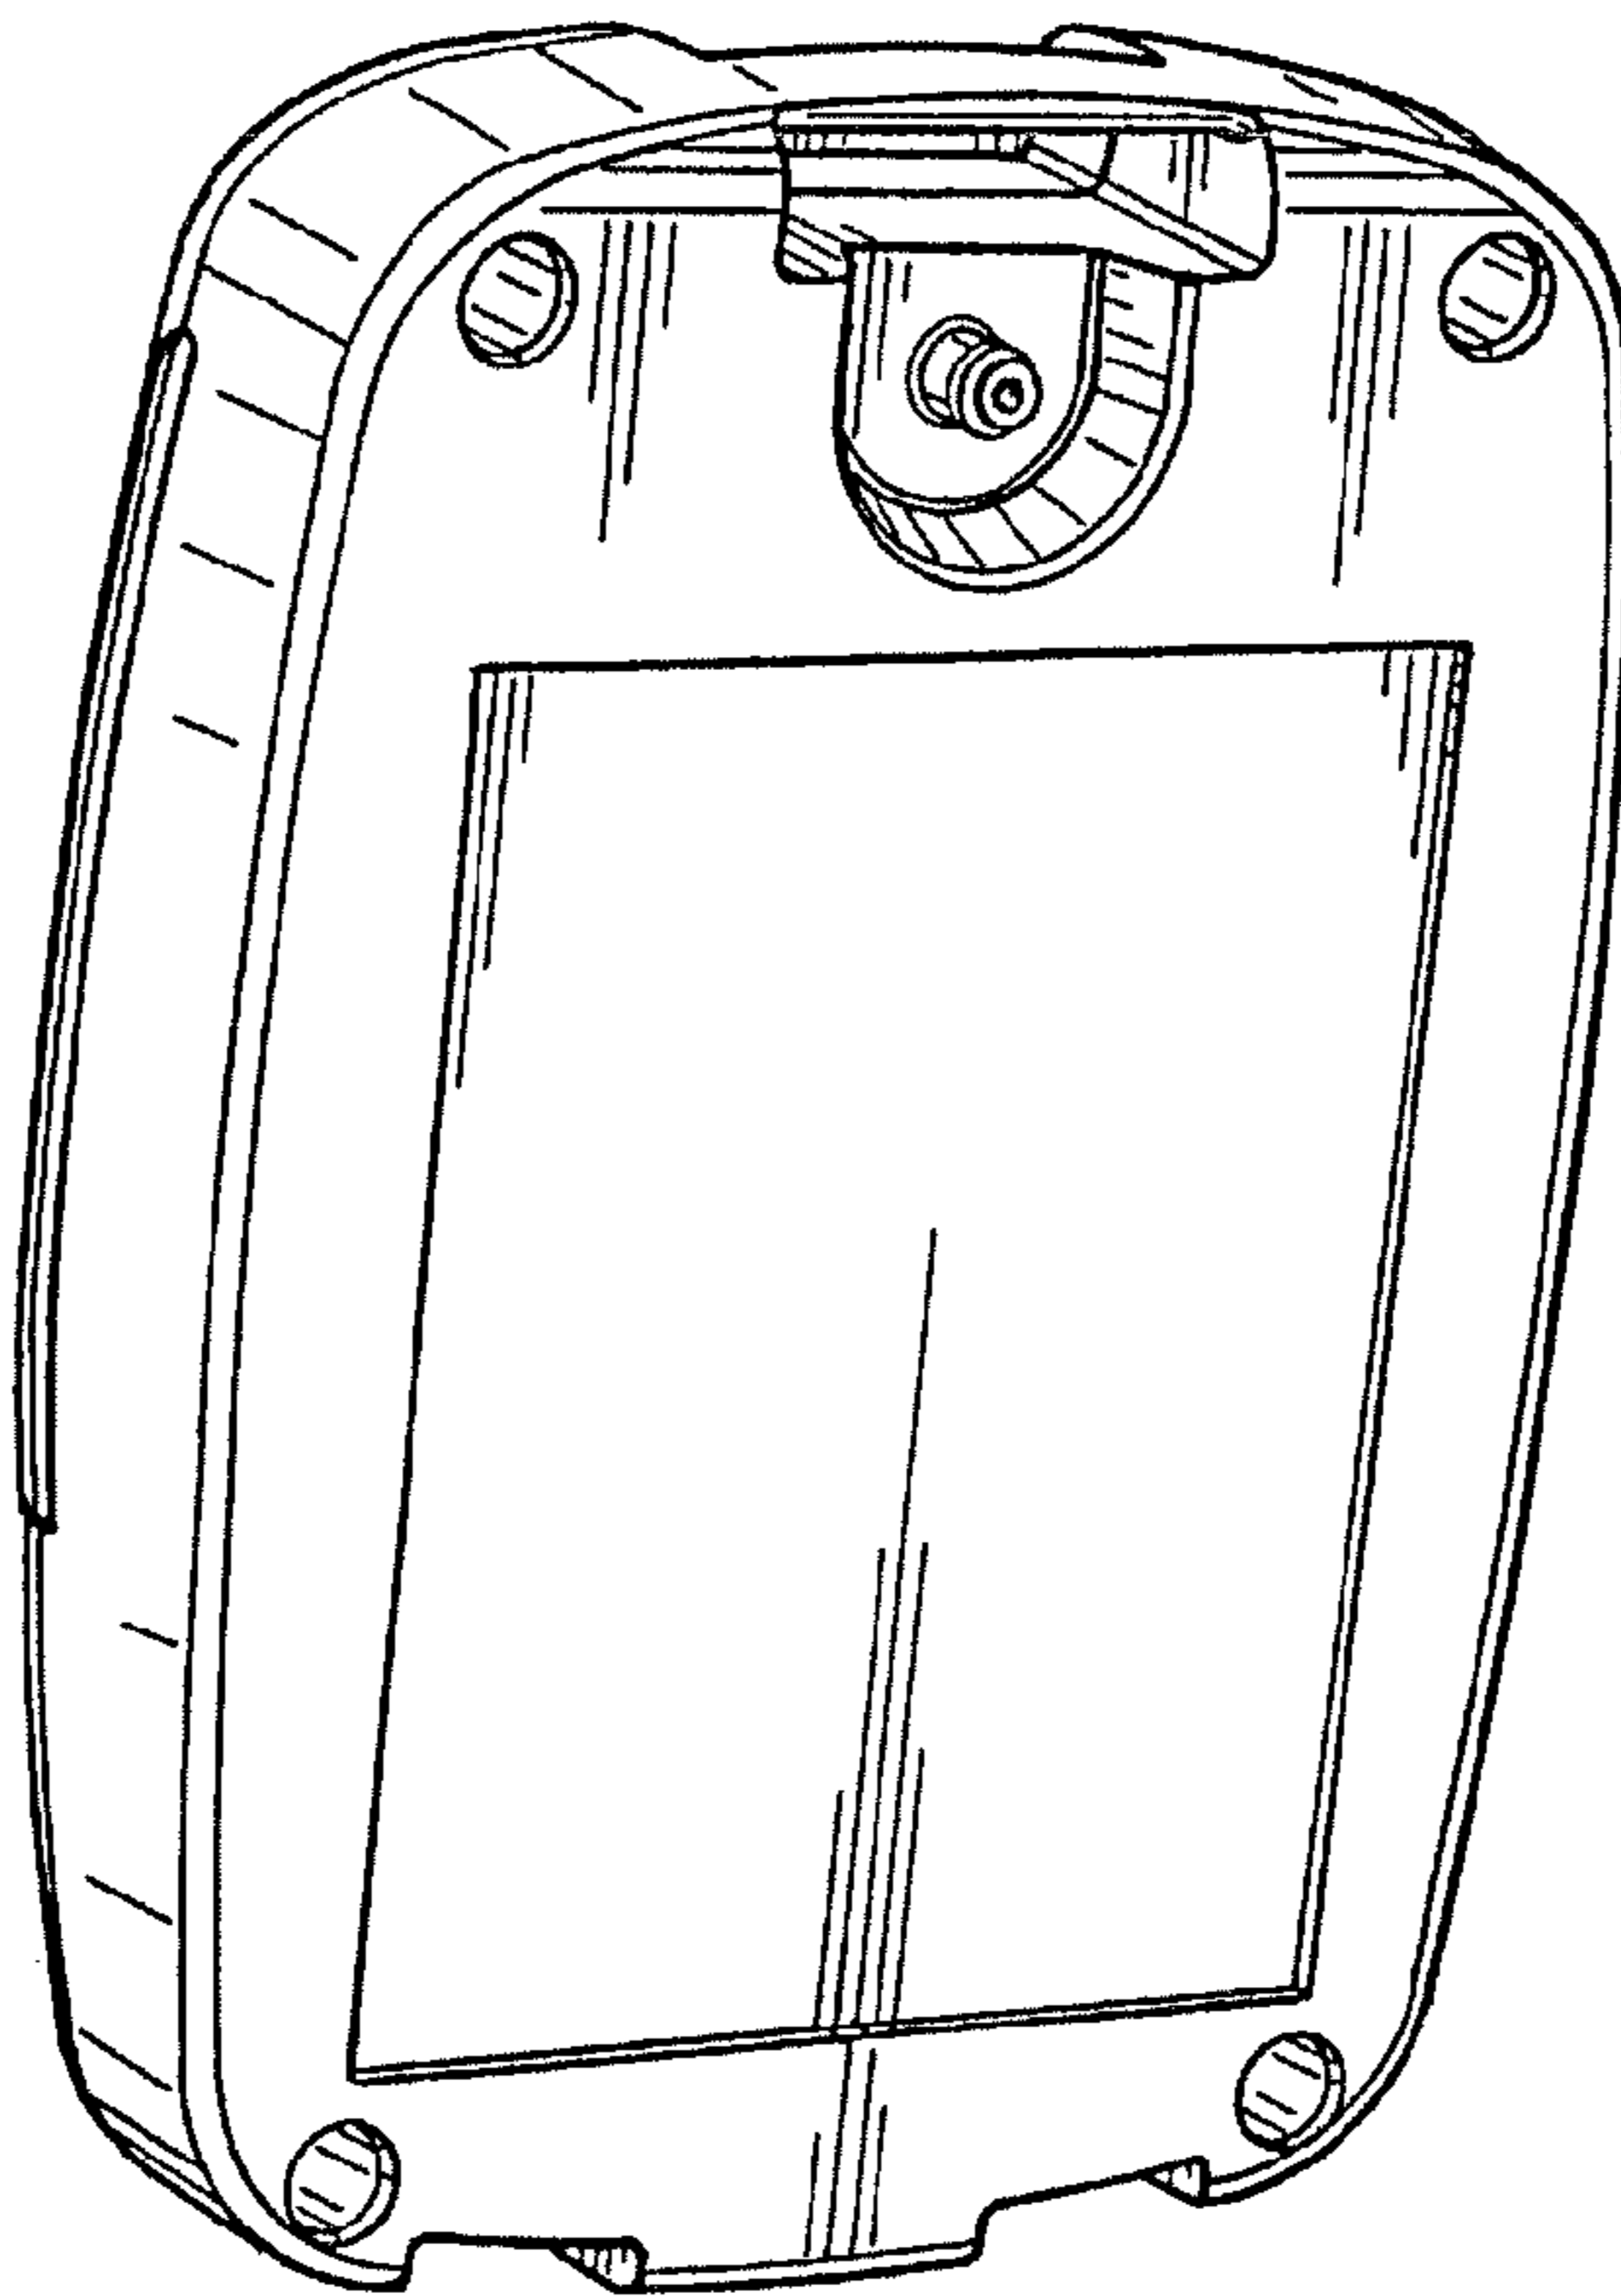

*Fig. 2*

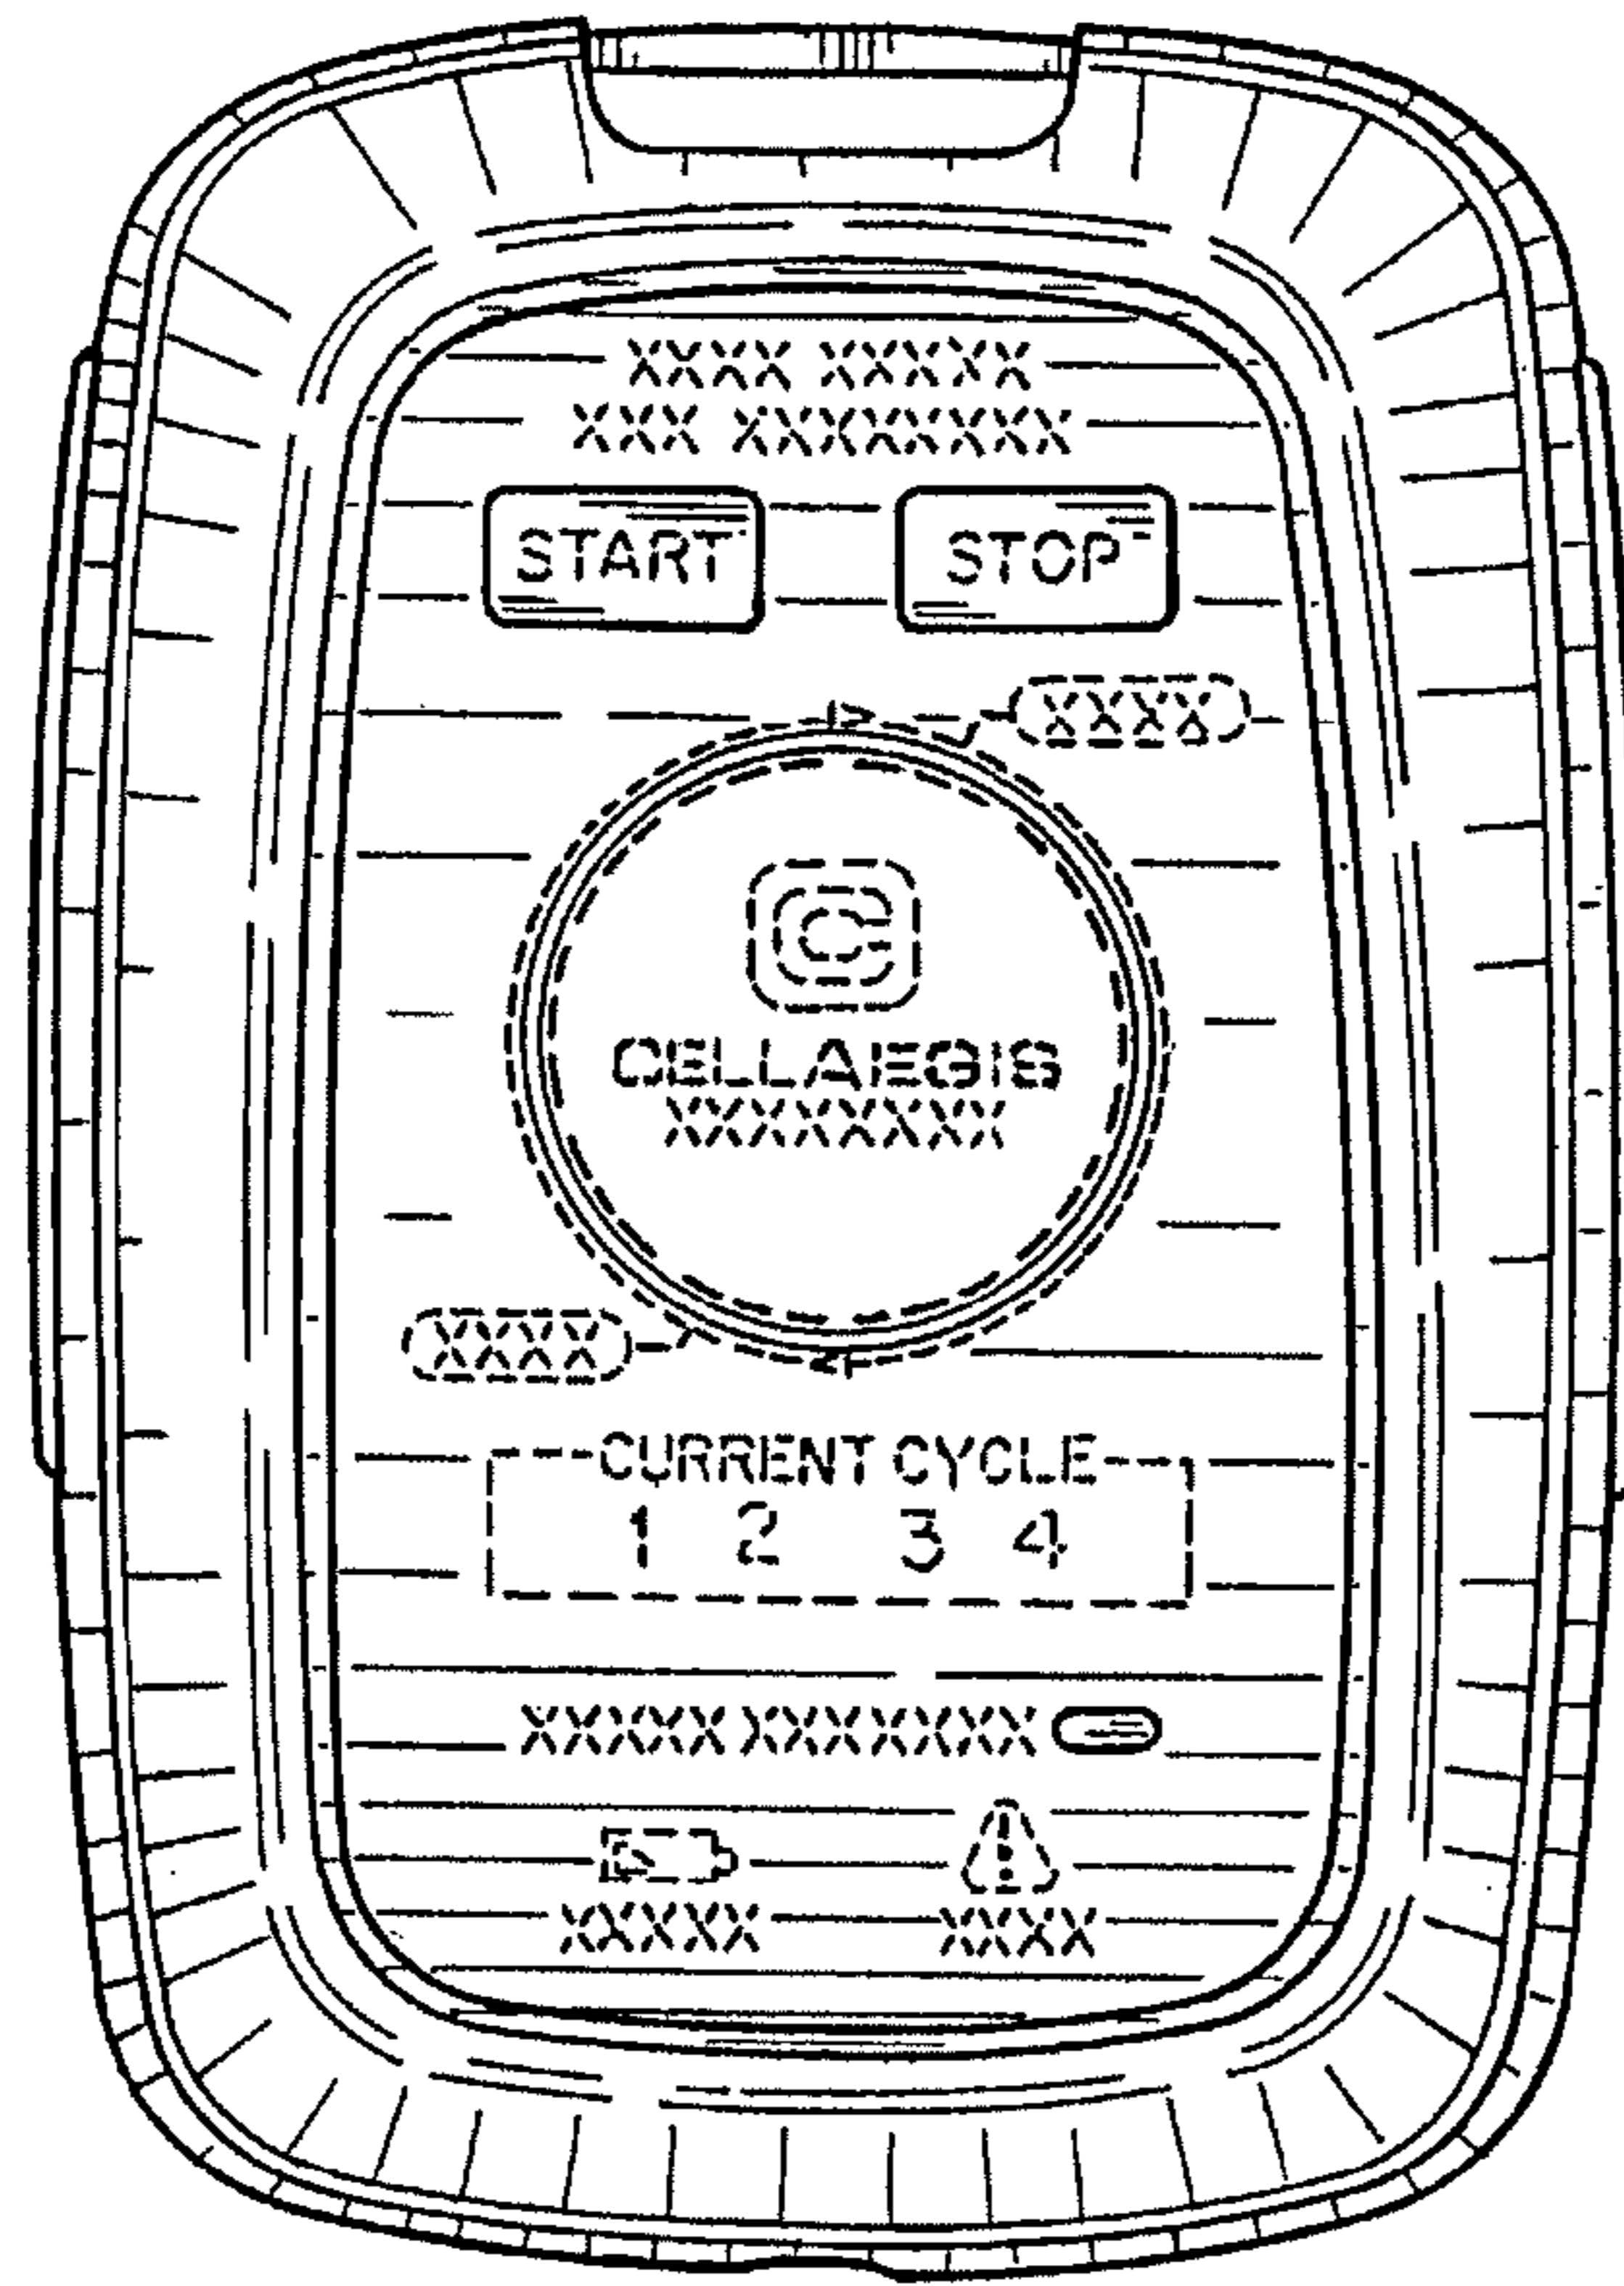


Fig. 3



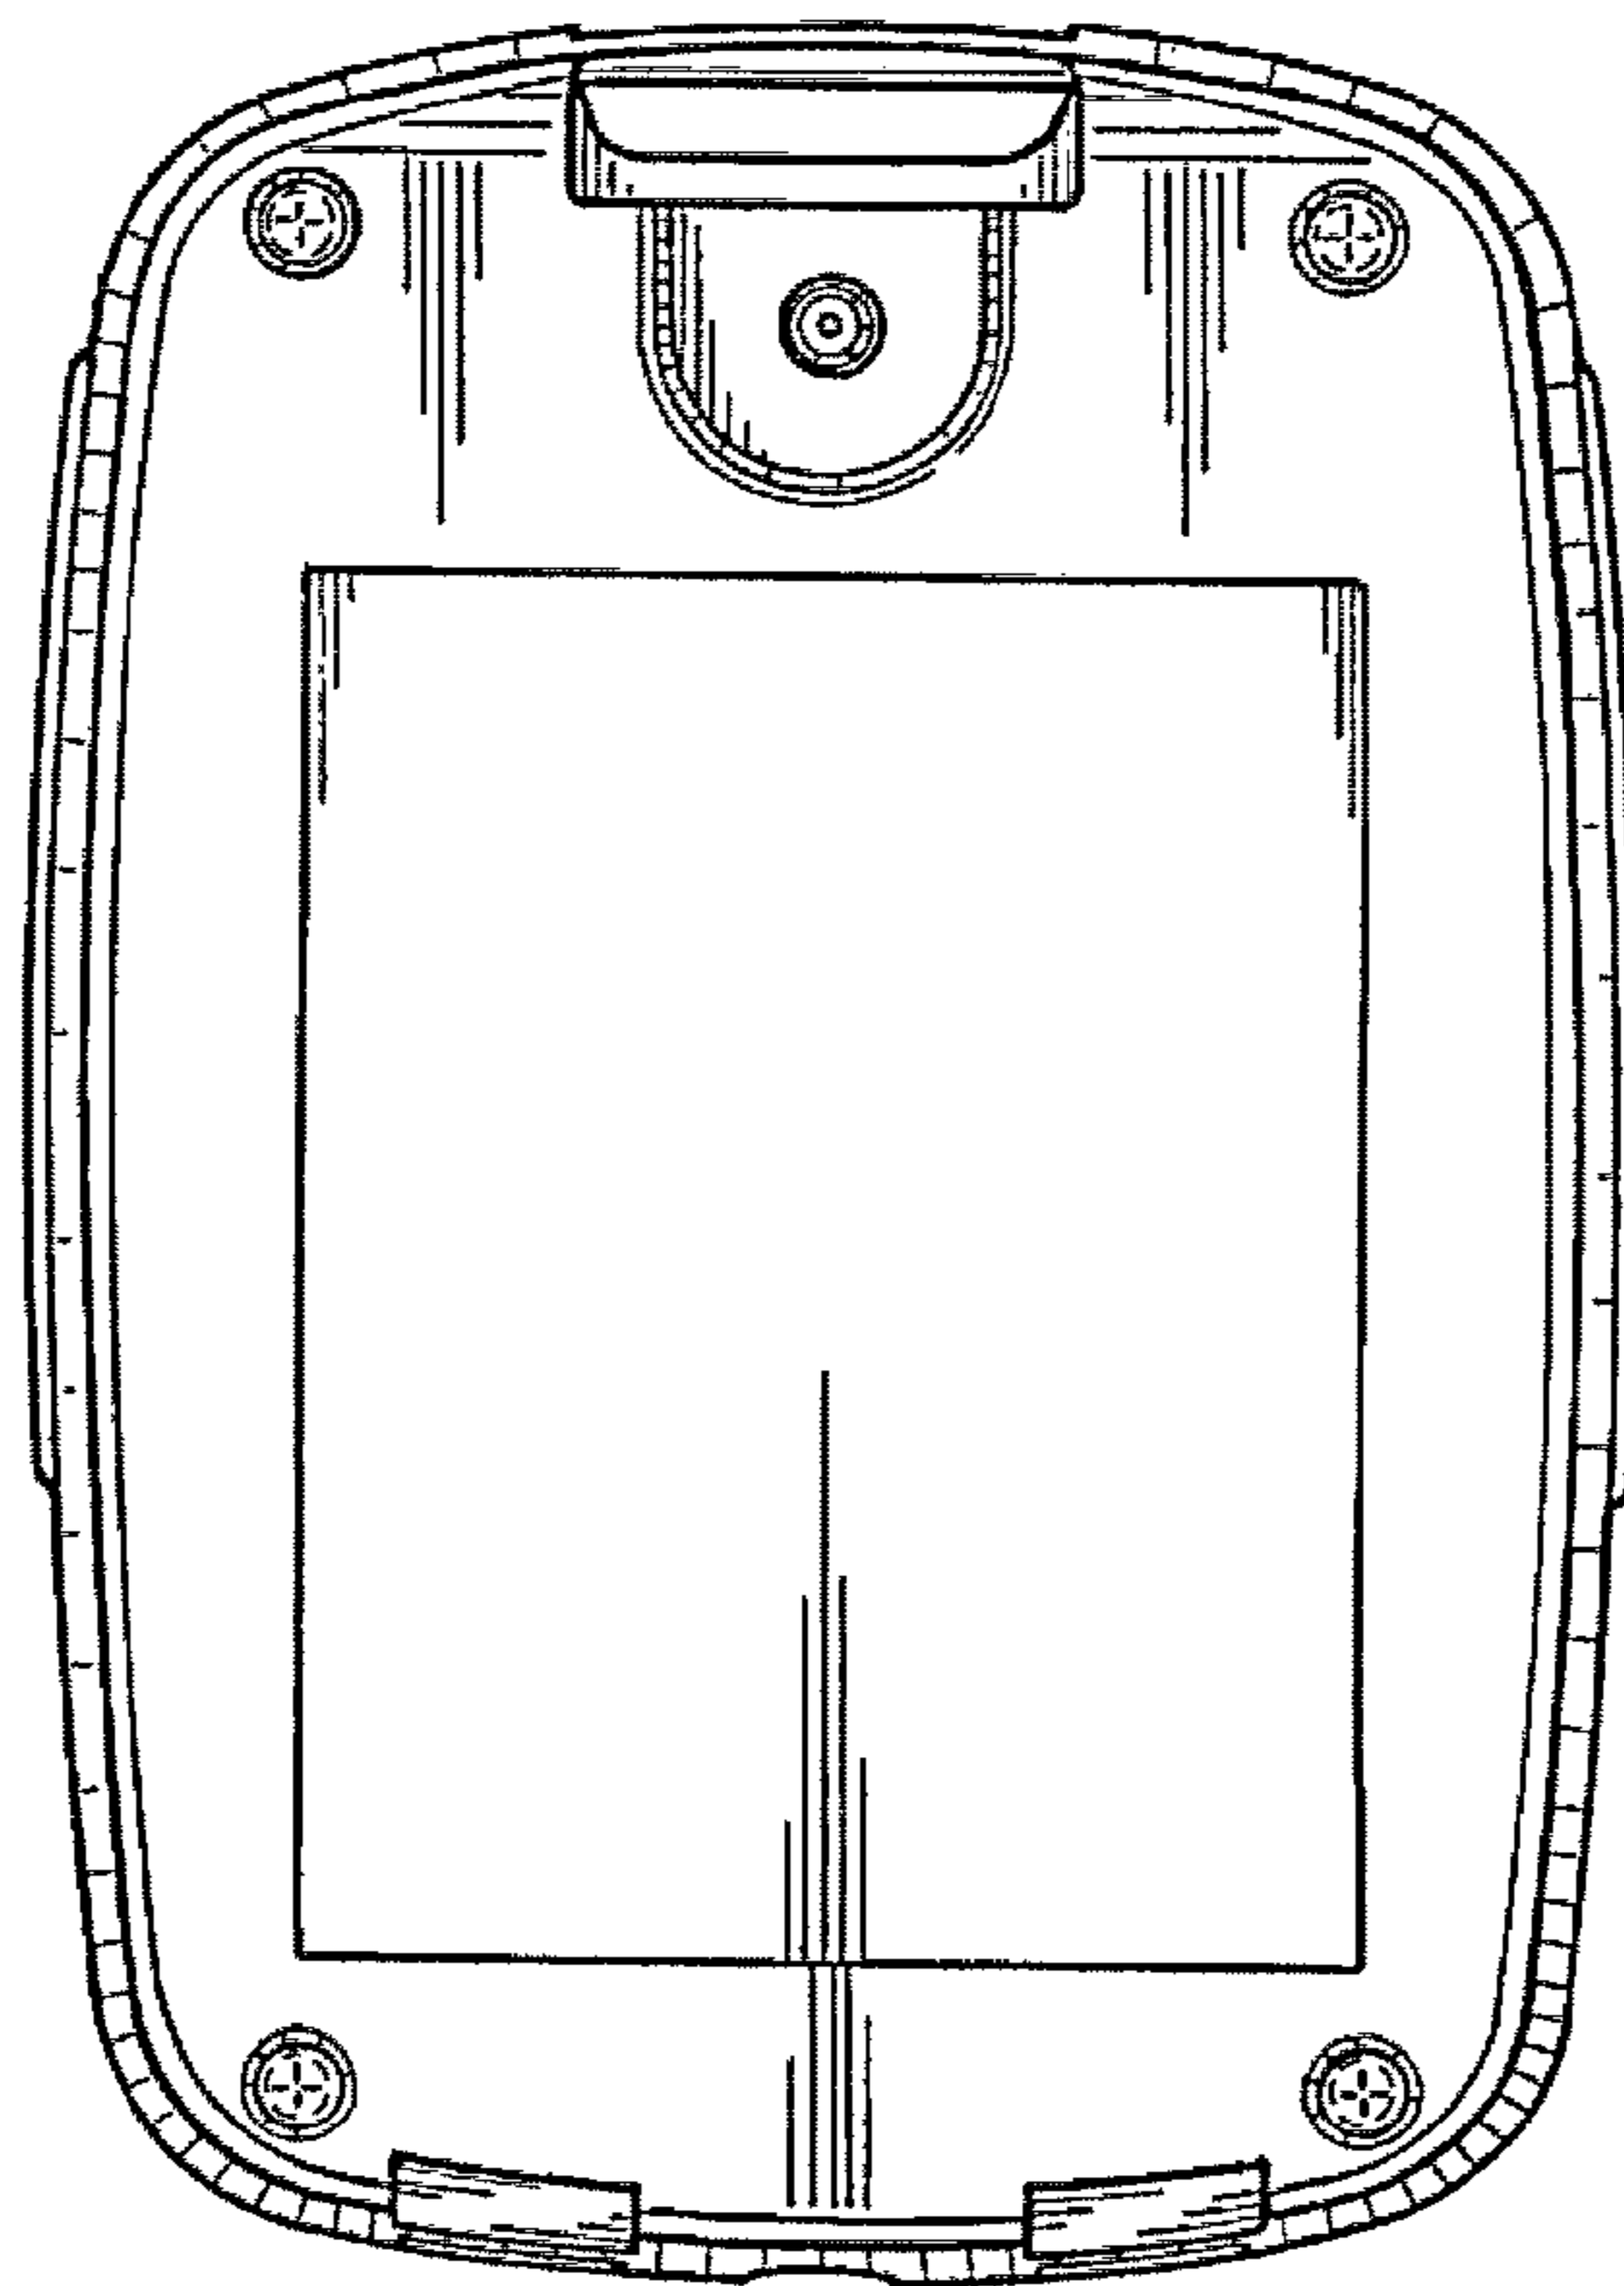



Fig. 4

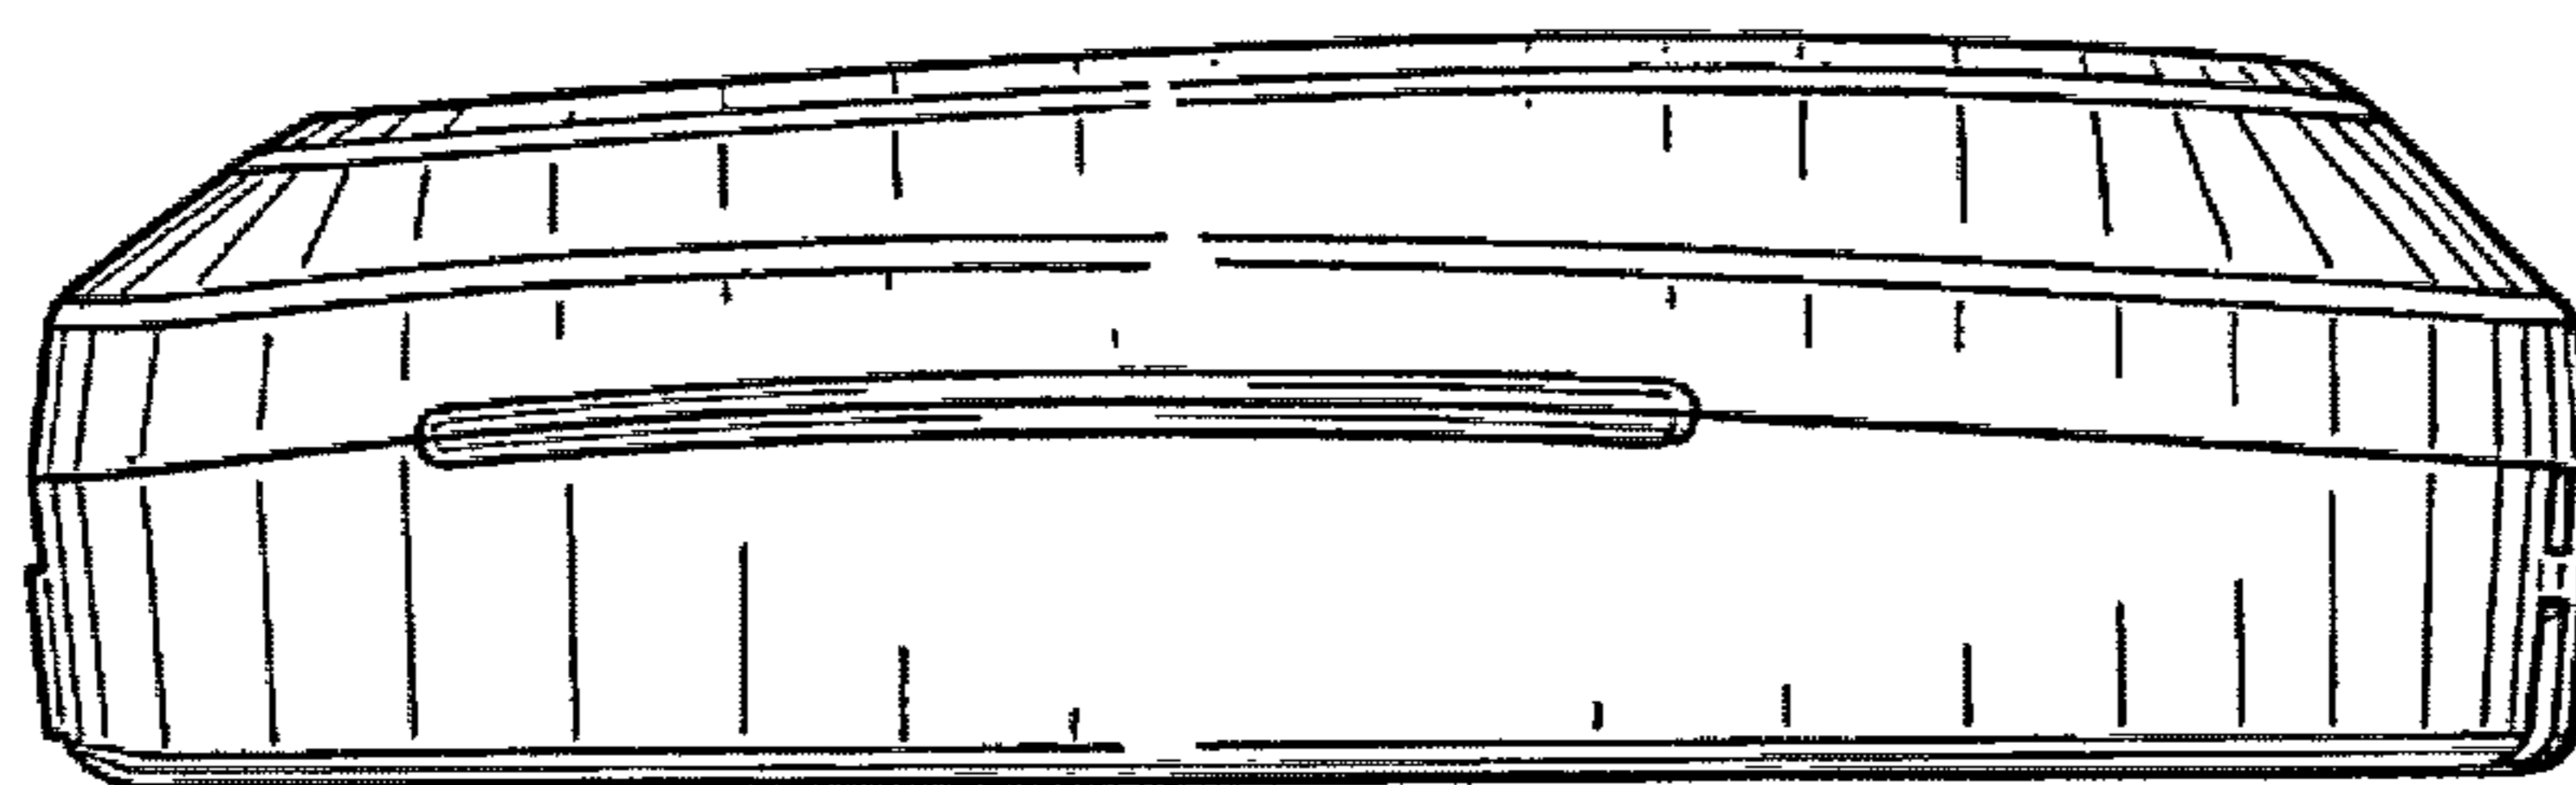

*Fig. 5*

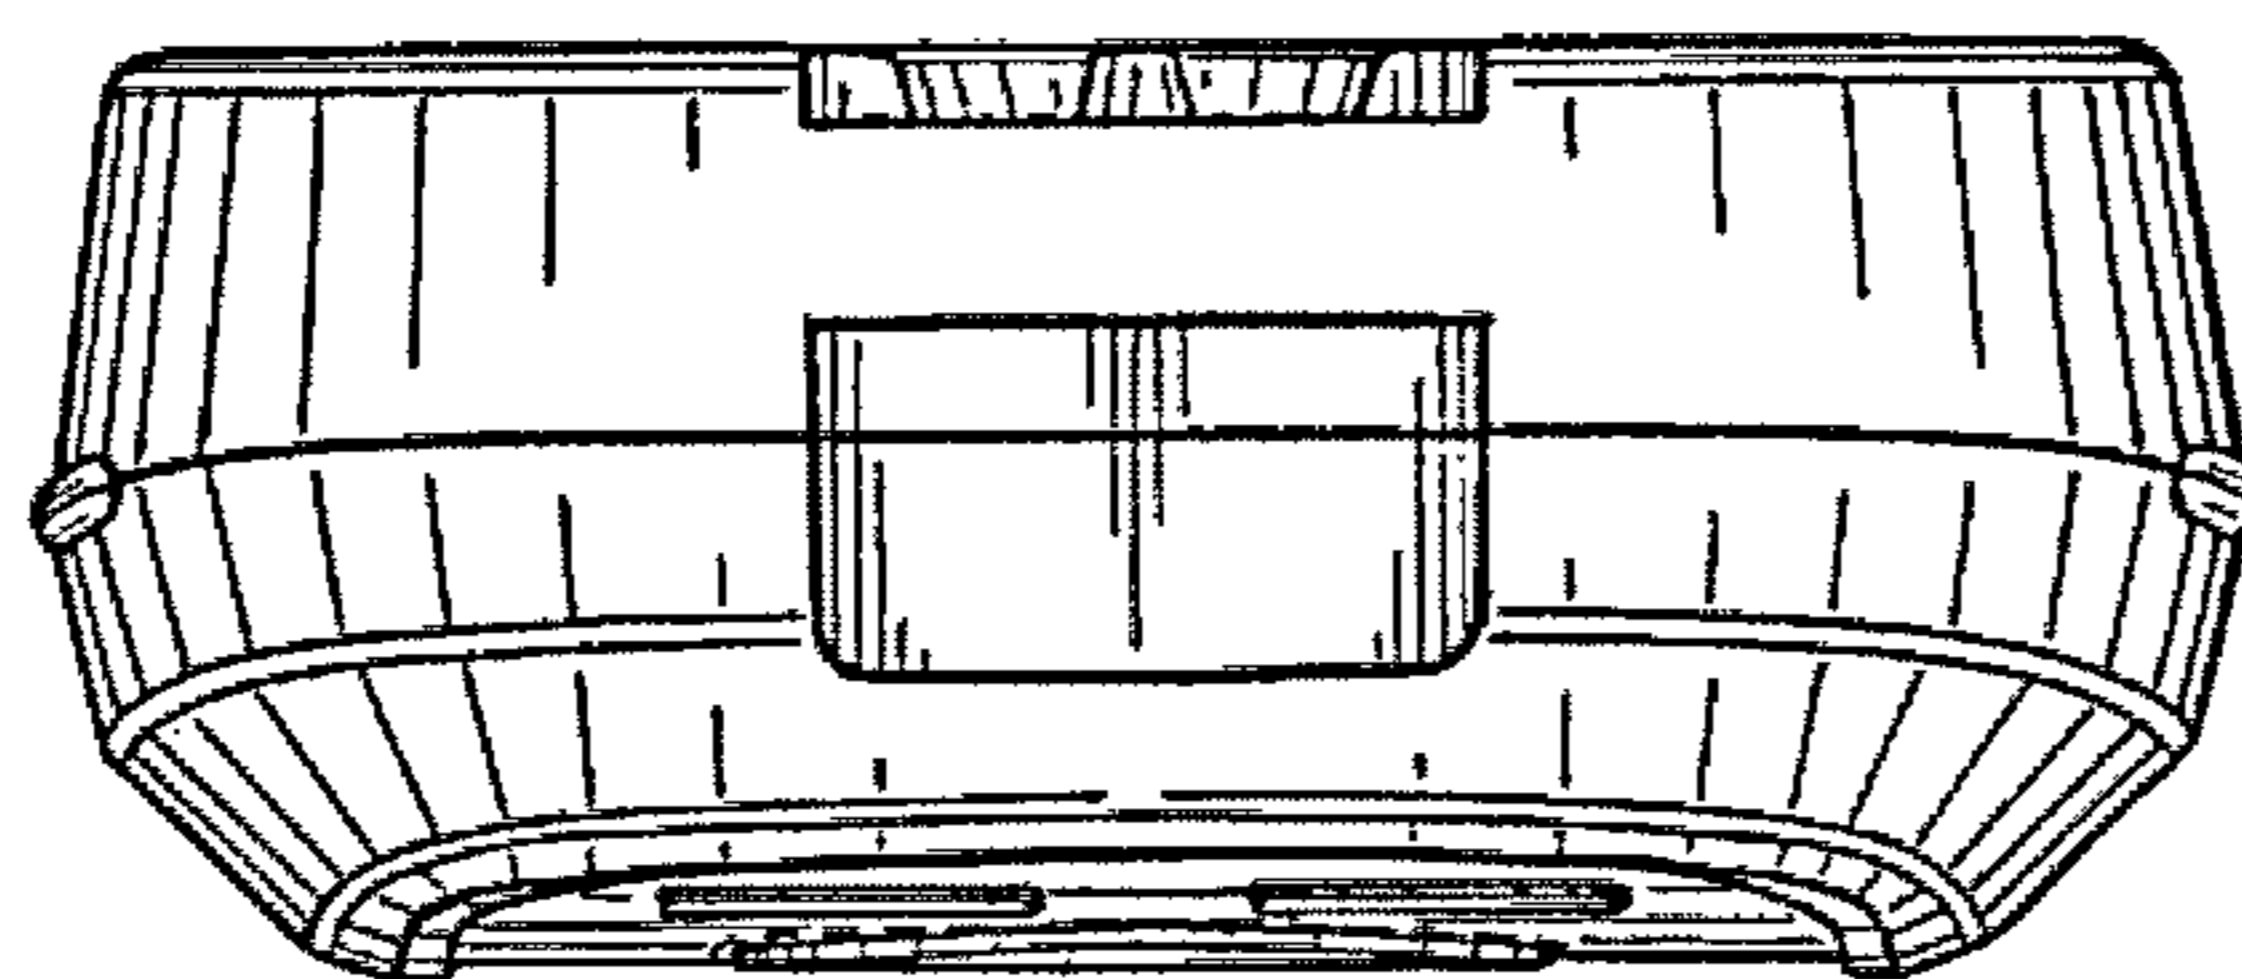

*Fig. 6*

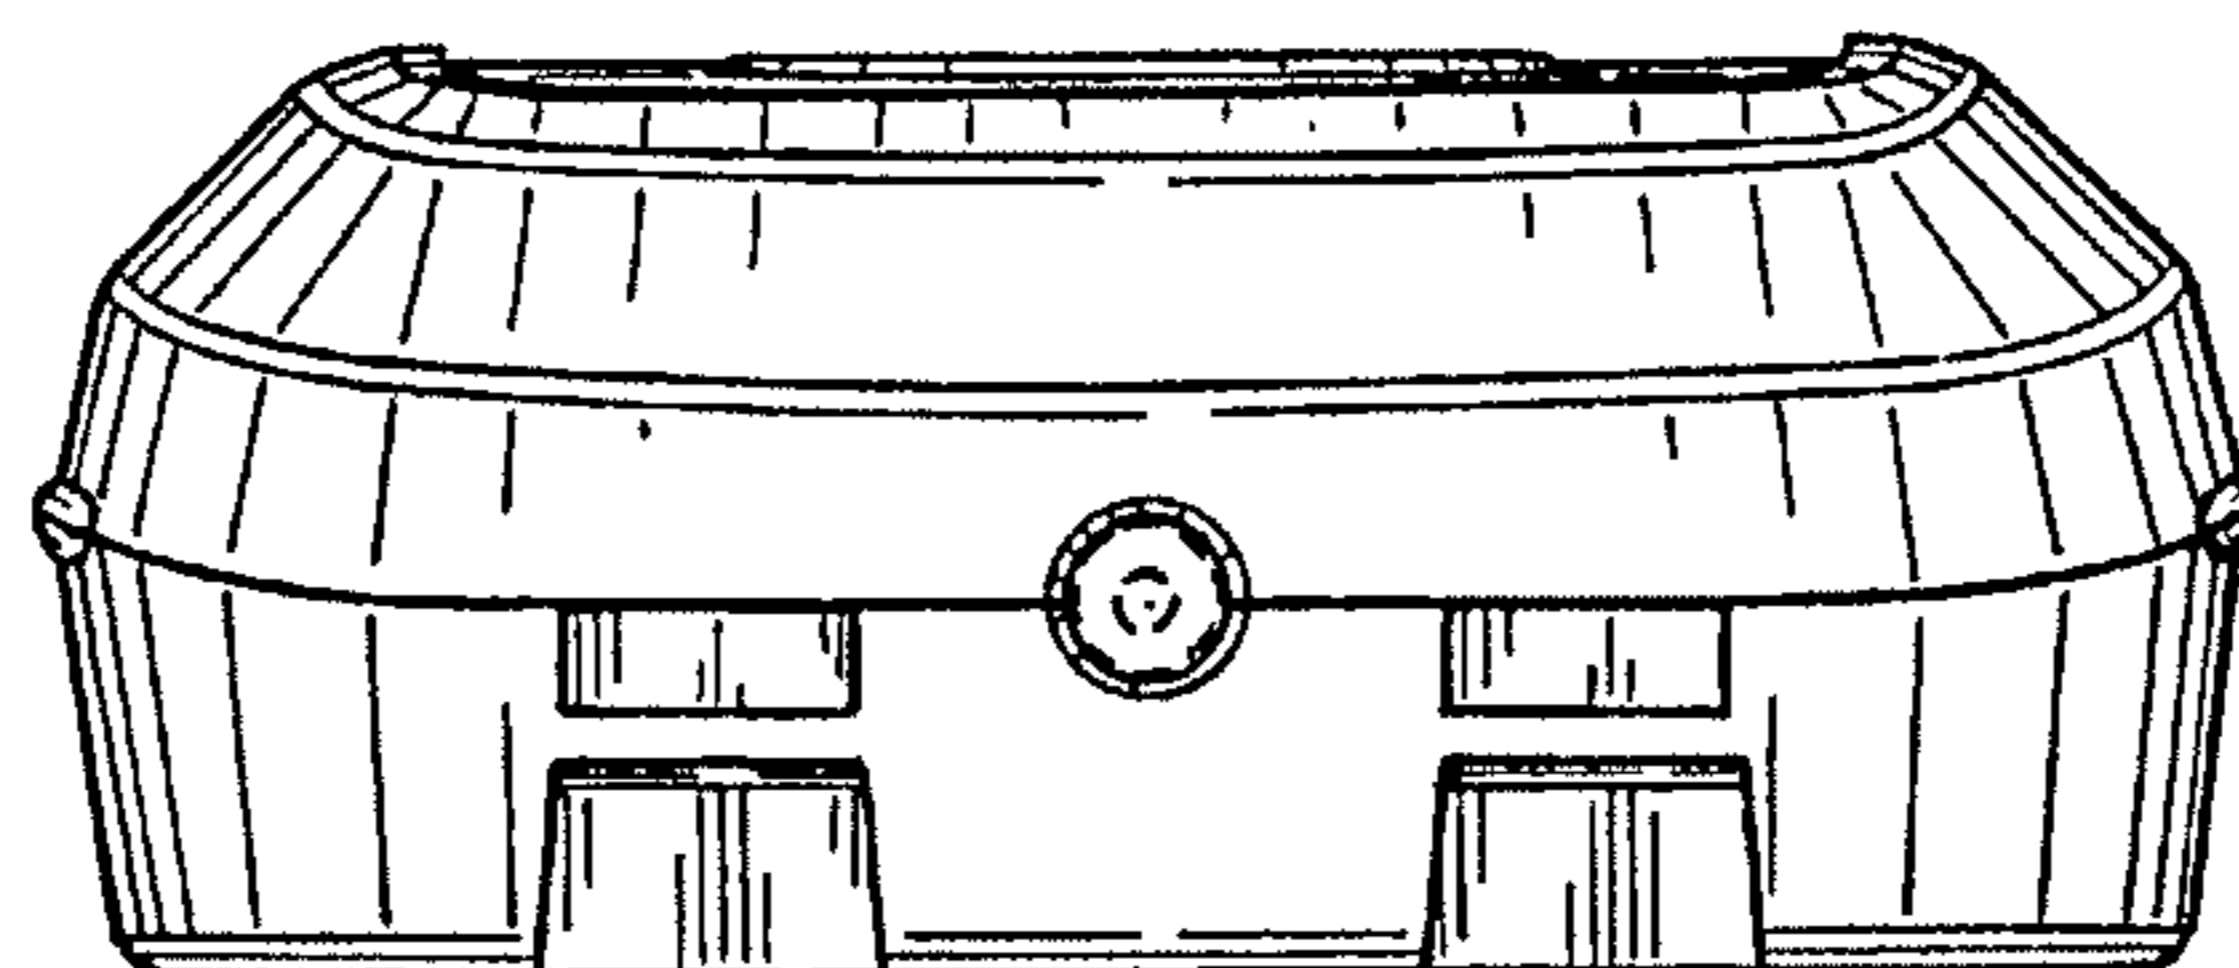

*Fig. 7*