



US00D709188S

(12) **United States Design Patent**  
**Guala**

(10) **Patent No.:** **US D709,188 S**

(45) **Date of Patent:** **\*\* Jul. 15, 2014**

(54) **SPIKE FOR INFUSION / TRANSFUSION  
MEDICAL DEVICES**

(75) Inventor: **Gianni Guala**, Turin (IT)

(73) Assignee: **Industrie Borla S.p.A.**, Moncalieri  
(Turin) (IT)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/394,656**

(22) Filed: **Jun. 20, 2011**

(30) **Foreign Application Priority Data**

Dec. 22, 2010 (EP) ..... 001797531-0001  
Dec. 22, 2010 (EP) ..... 001797531-0002  
Dec. 22, 2010 (EP) ..... 001797531-0003  
Dec. 22, 2010 (EP) ..... 001797531-0004  
Dec. 22, 2010 (EP) ..... 001797531-0005

(51) **LOC (10) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/130**

(58) **Field of Classification Search**  
USPC ..... D24/127-131, 112-114, 133, 186;  
606/181, 185; 604/264, 272, 115, 232,  
604/187, 158, 164.08, 192, 263, 163, 181,  
604/184, 1, 98, 227; 600/101, 139, 143;  
128/200.24, 207.14, 207.15

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,317,445 A \* 3/1982 Robinson ..... 604/168.01  
D469,871 S \* 2/2003 Sand ..... D24/133  
D614,296 S \* 4/2010 Young ..... D24/130  
D615,648 S \* 5/2010 Burke ..... D24/130  
7,744,567 B2 \* 6/2010 Glowacki et al. .... 604/164.08  
D619,251 S \* 7/2010 Justiniano-Garcia  
et al. .... D24/133  
D620,107 S \* 7/2010 Bartlett et al. .... D24/112  
D620,591 S \* 7/2010 Young ..... D24/130  
D625,003 S \* 10/2010 Stephens ..... D24/129  
D625,004 S \* 10/2010 McGrady et al. .... D24/129  
D653,338 S \* 1/2012 Mangeshikar ..... D24/133  
D663,832 S \* 7/2012 Essinger et al. .... D24/112  
D668,336 S \* 10/2012 Yanagawa ..... D24/130

\* cited by examiner

*Primary Examiner* — David Muller

(74) *Attorney, Agent, or Firm* — Heslin Rothenberg Farley  
& Mesiti P.C.; Victor A. Cardona

(57) **CLAIM**


The design for the spike for infusion/transfusion medical  
devices, as shown and described.


**DESCRIPTION**

FIG. 1 is a top perspective view of a spike for infusion/  
transfusion medical devices comprising the new design;  
FIG. 2 is a side perspective view thereof;  
FIG. 3 is top view thereof;  
FIG. 4 is a right side view thereof;  
FIG. 5 is front end view thereof; and,  
FIG. 6 is a rear end thereof.


The broken lines in the figures are for illustration purposes  
only and form no part of the claimed invention.

**1 Claim, 6 Drawing Sheets**

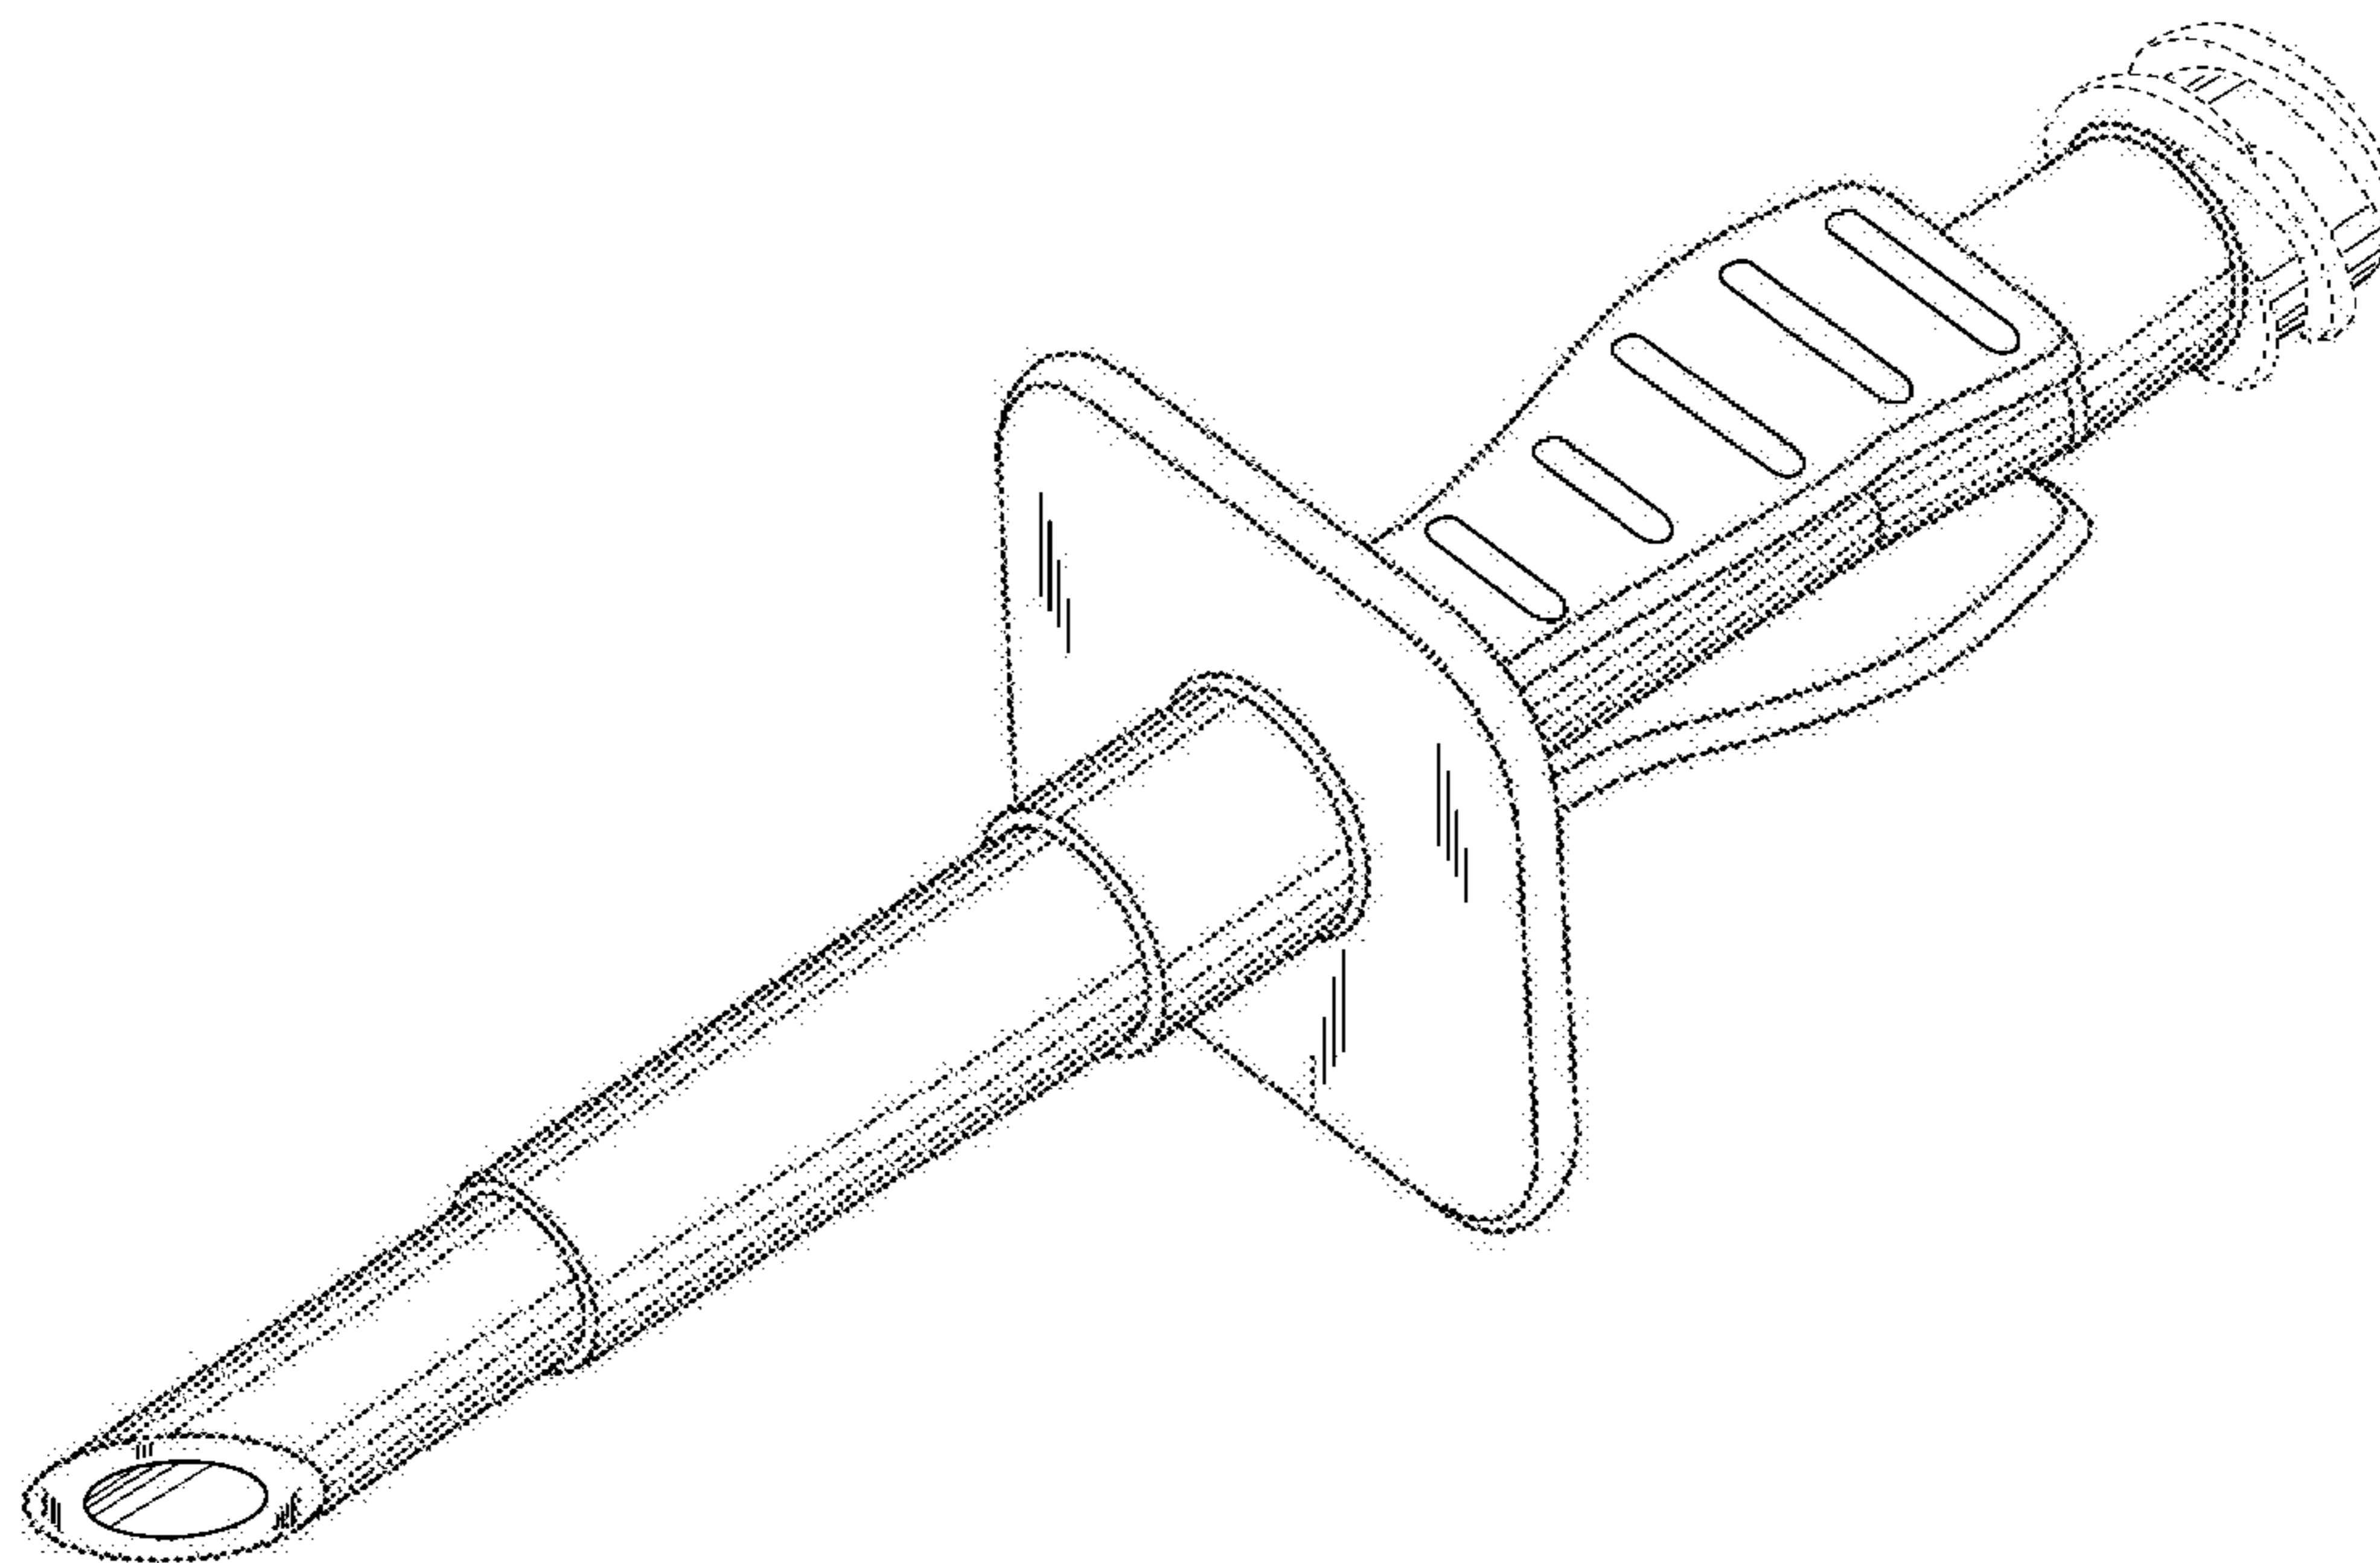

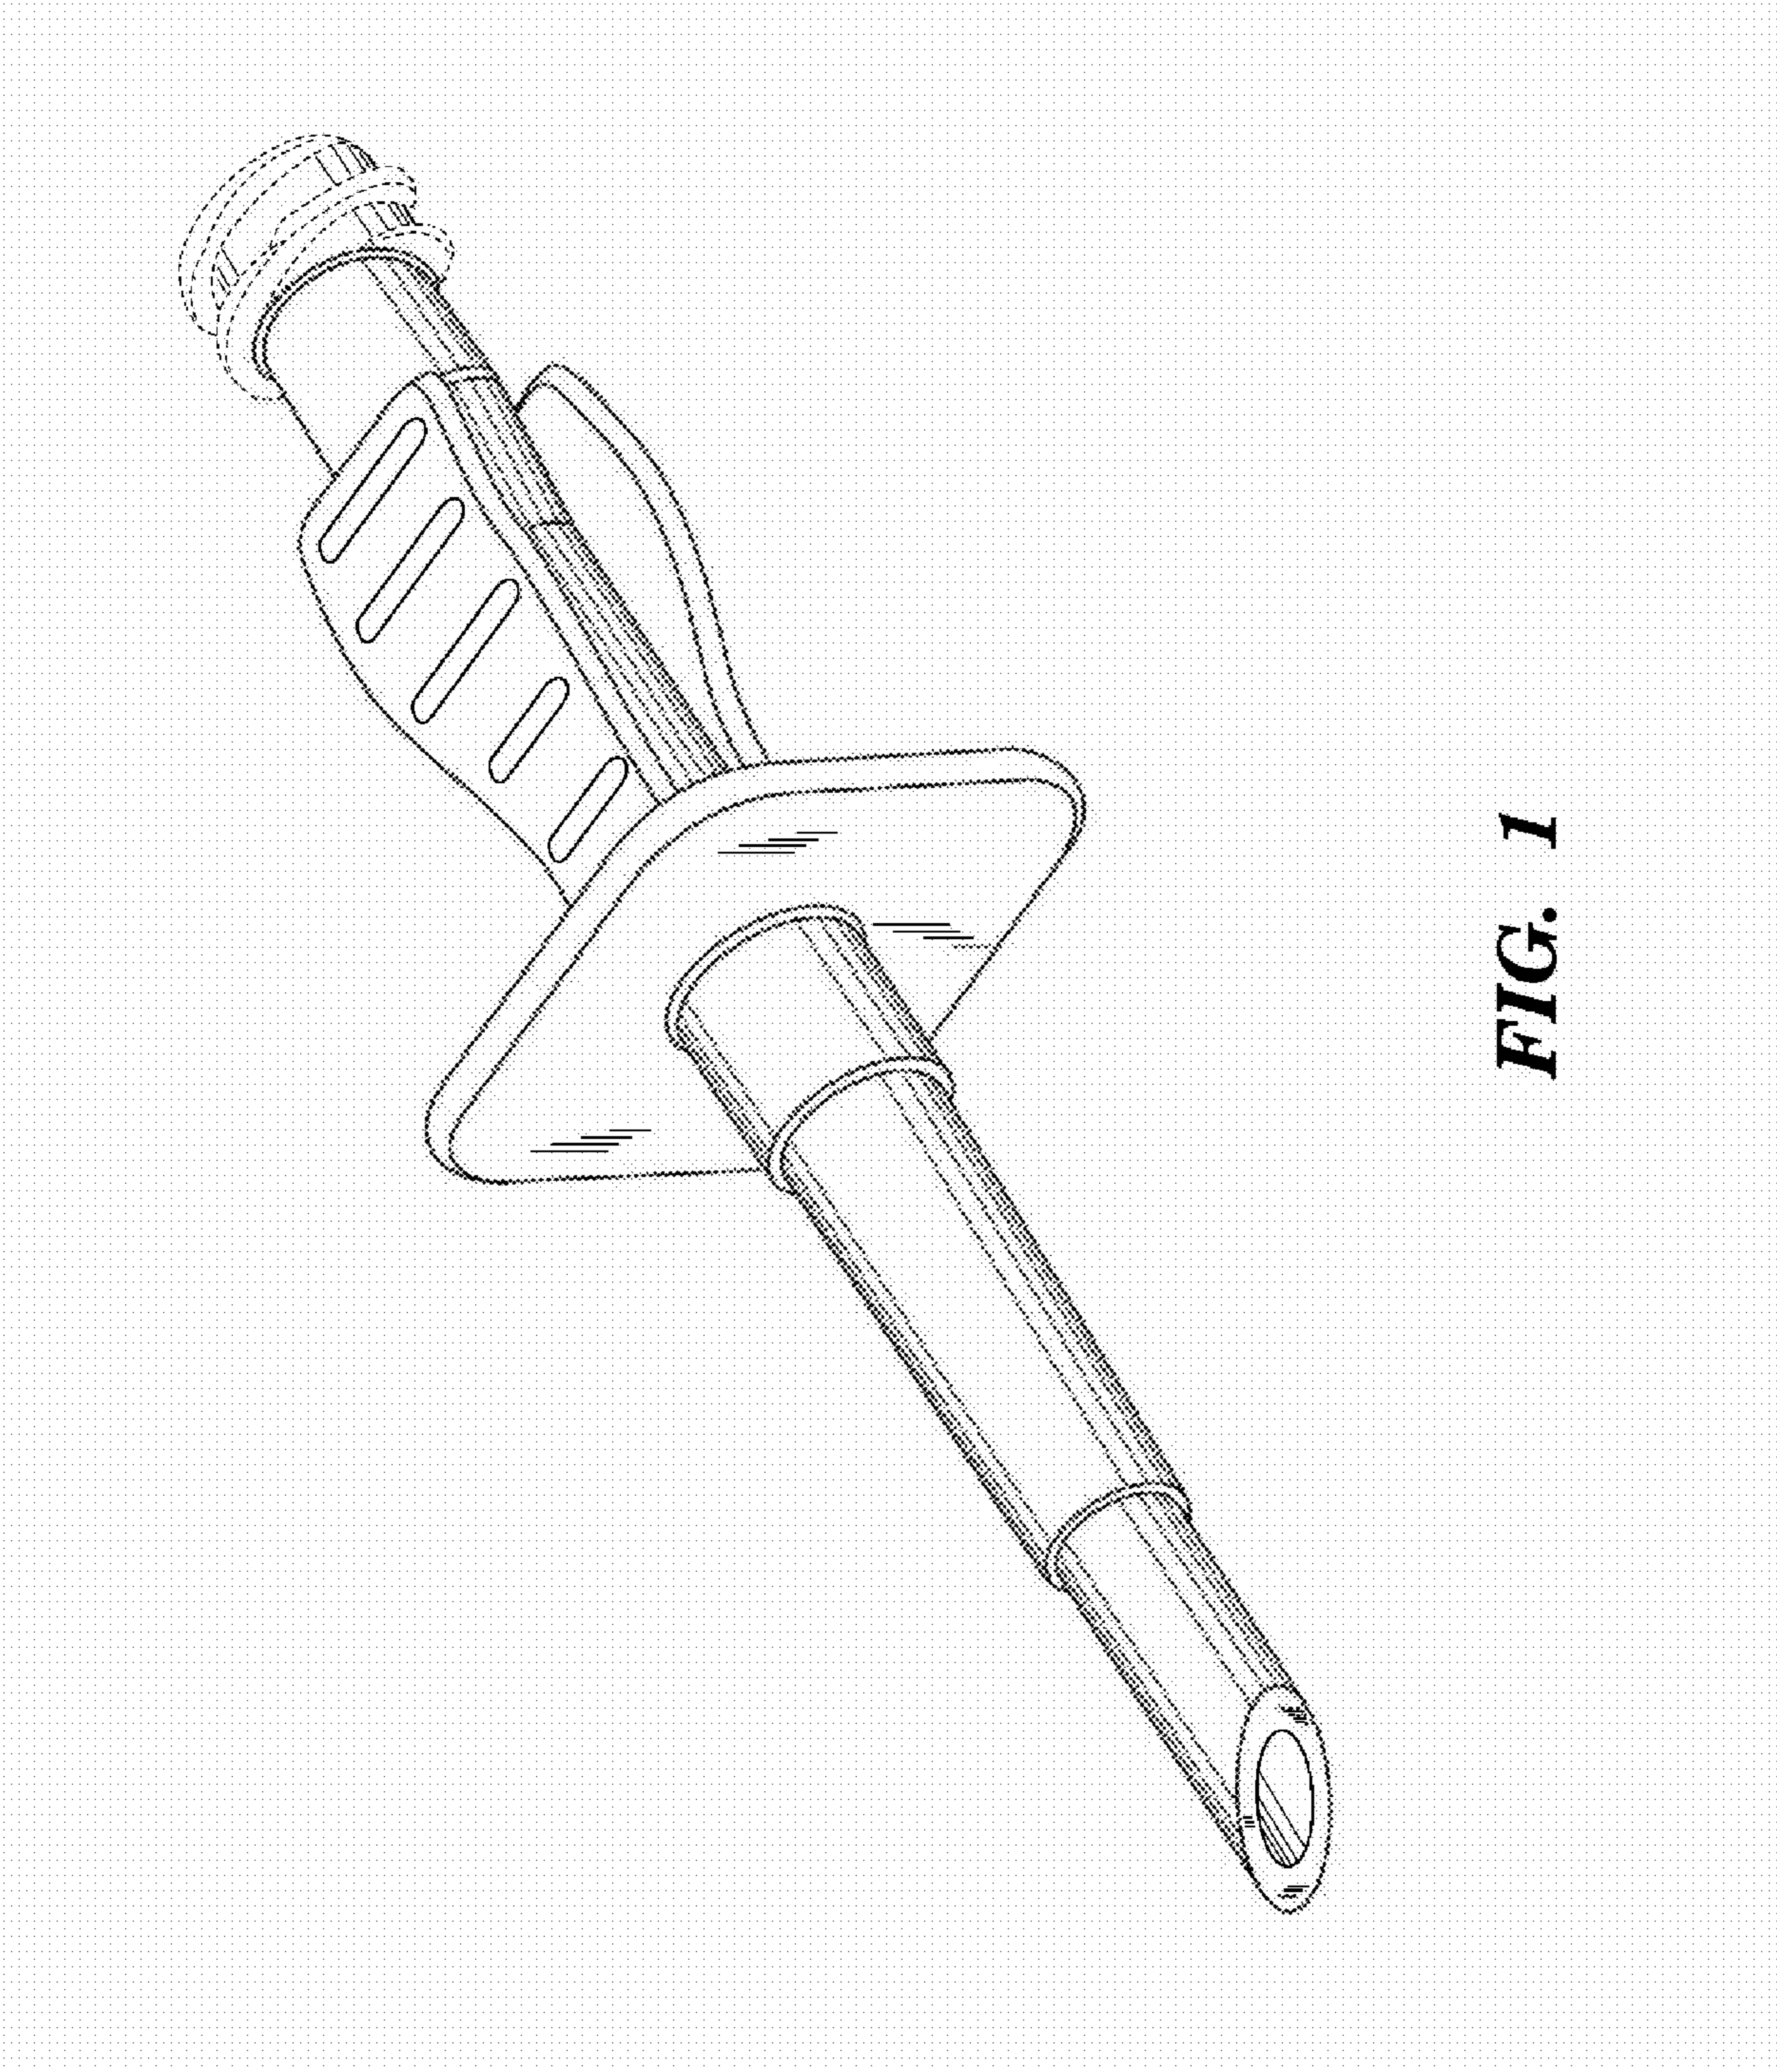


**FIG. 1**

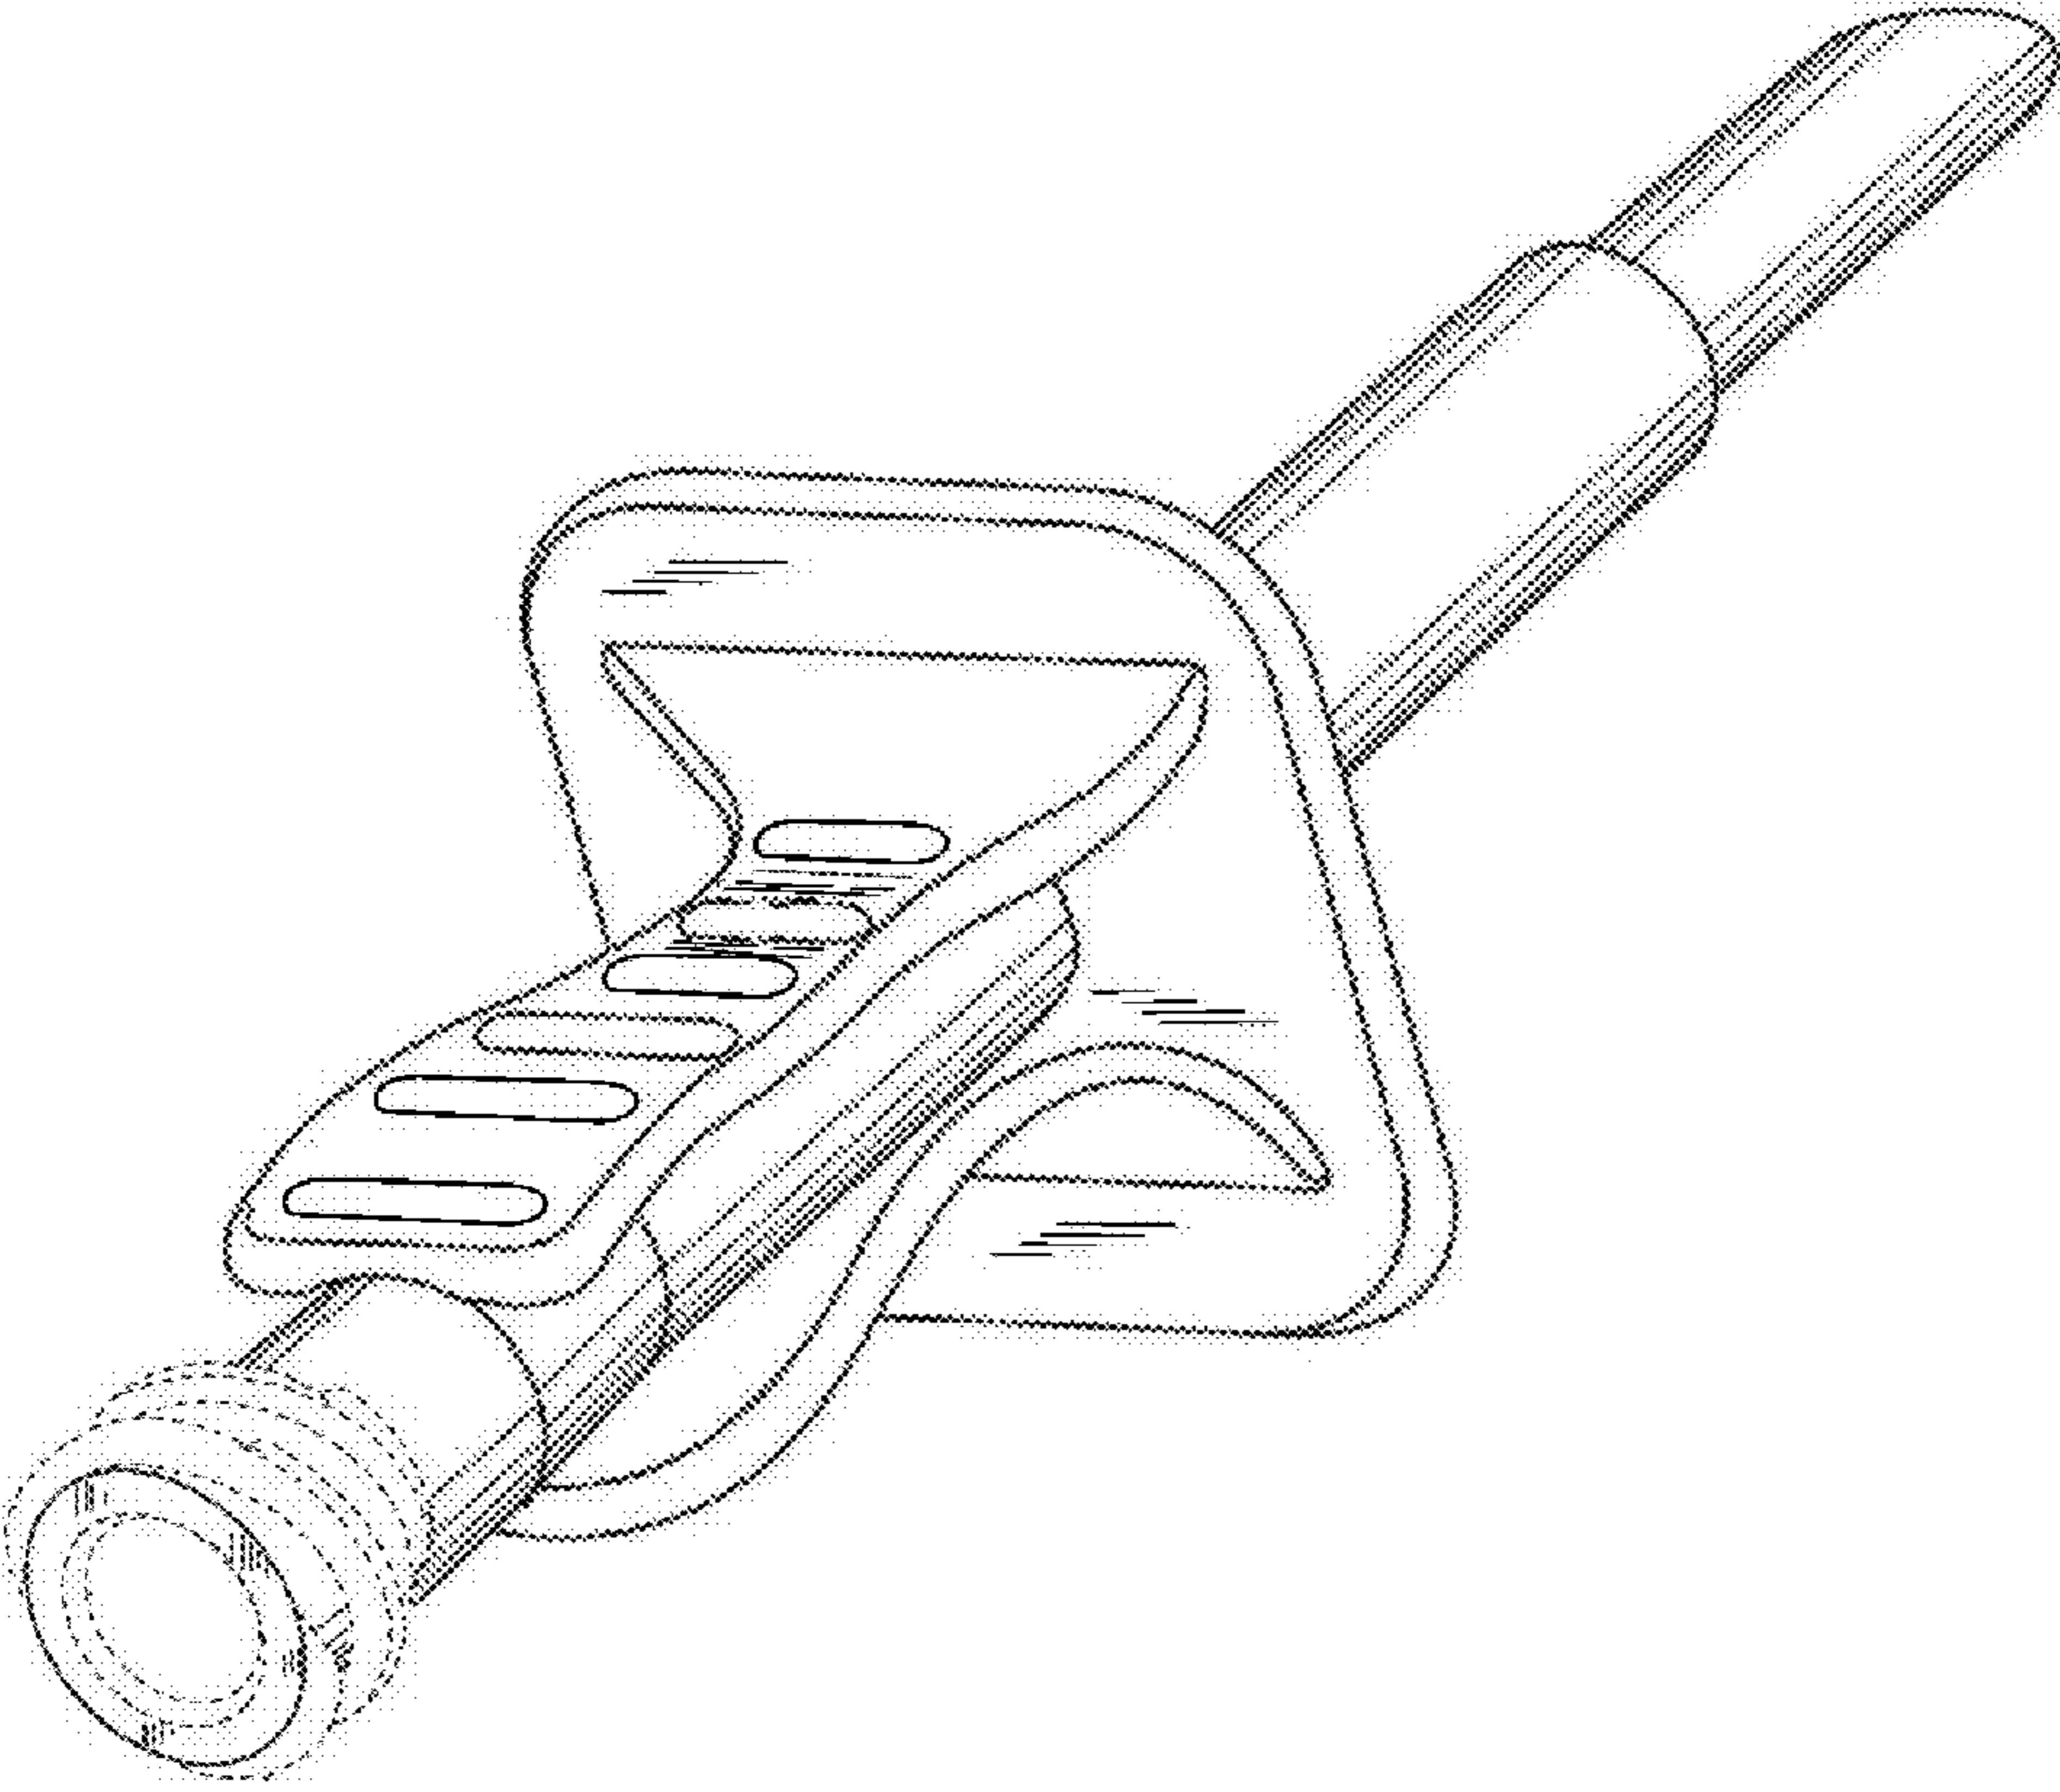


**FIG. 2**




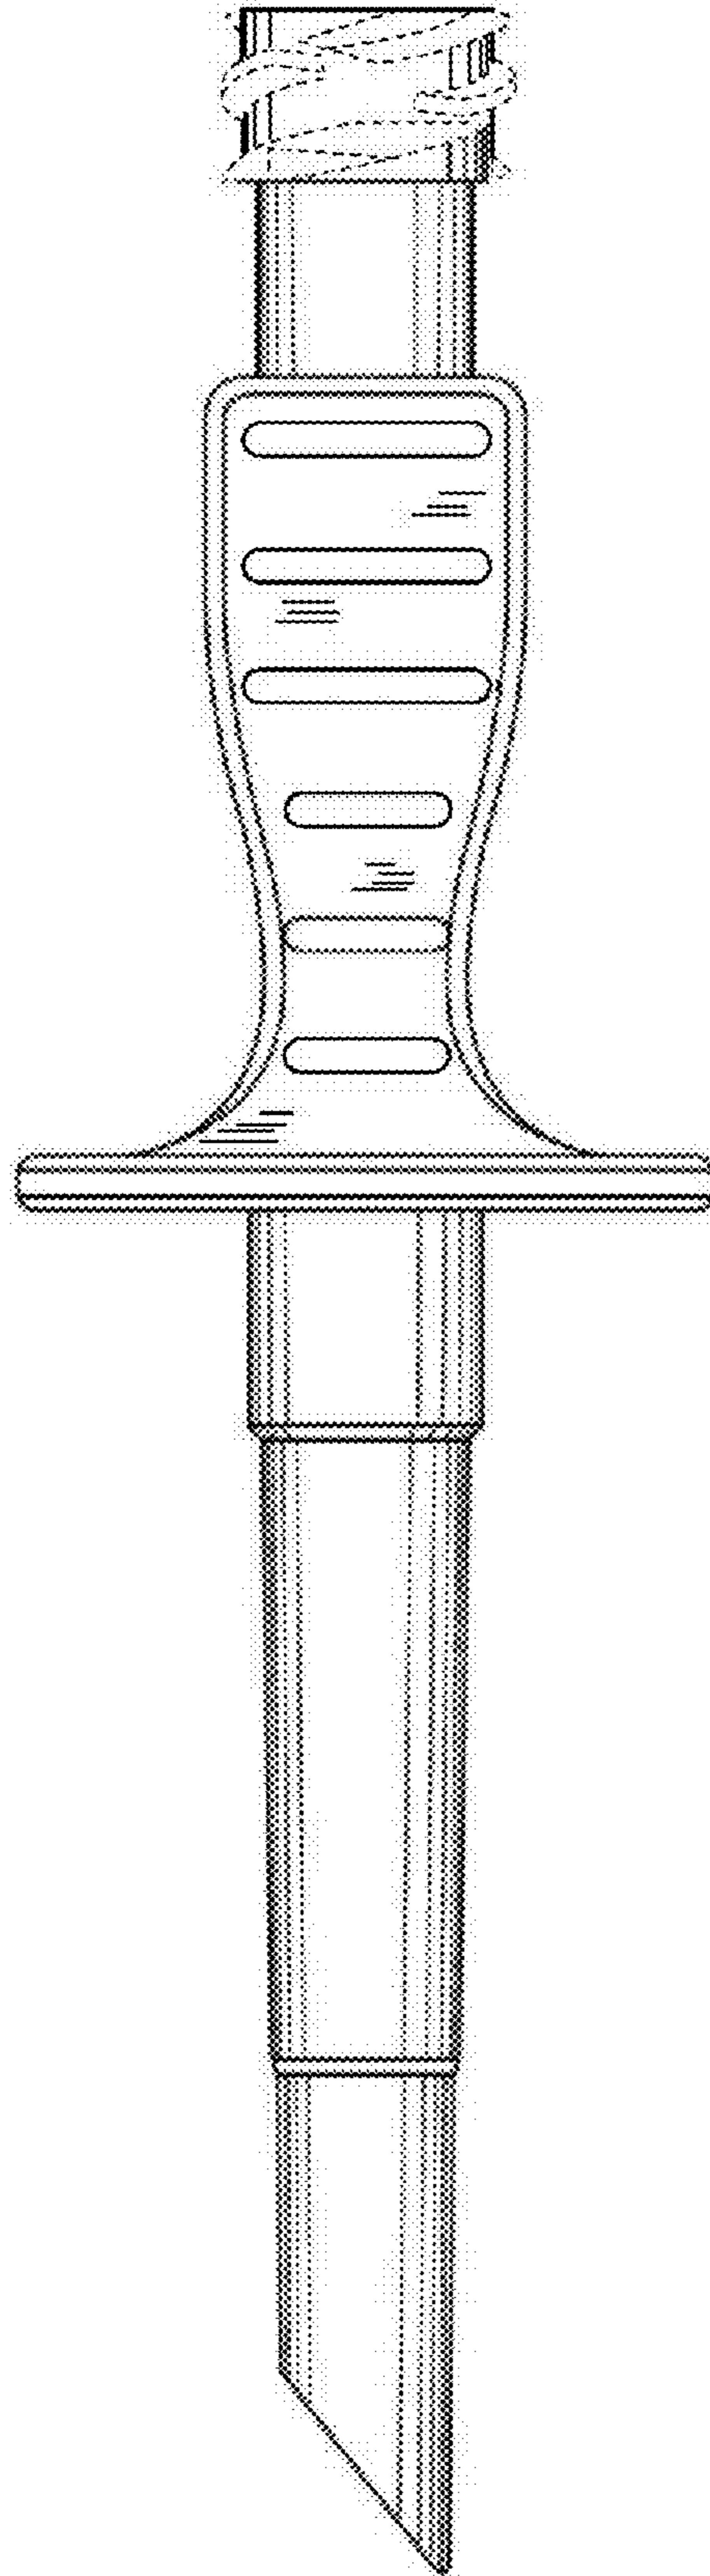


**FIG. 3**

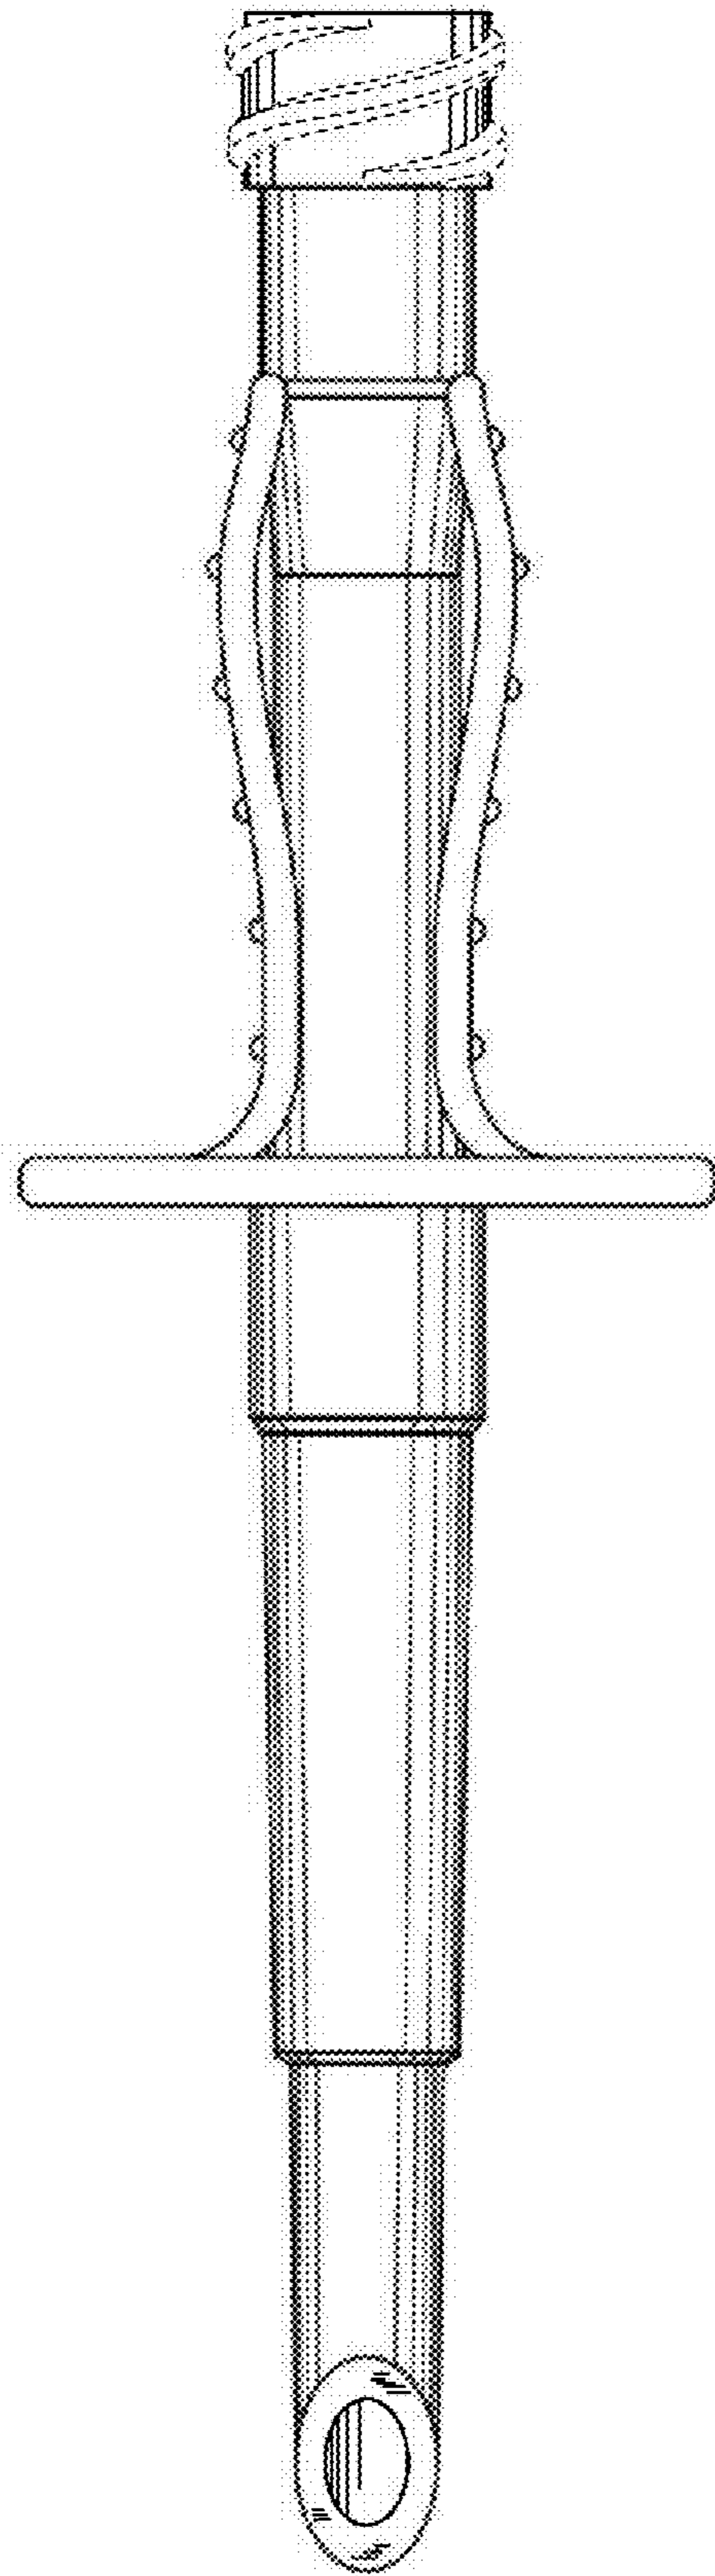

**FIG. 4**

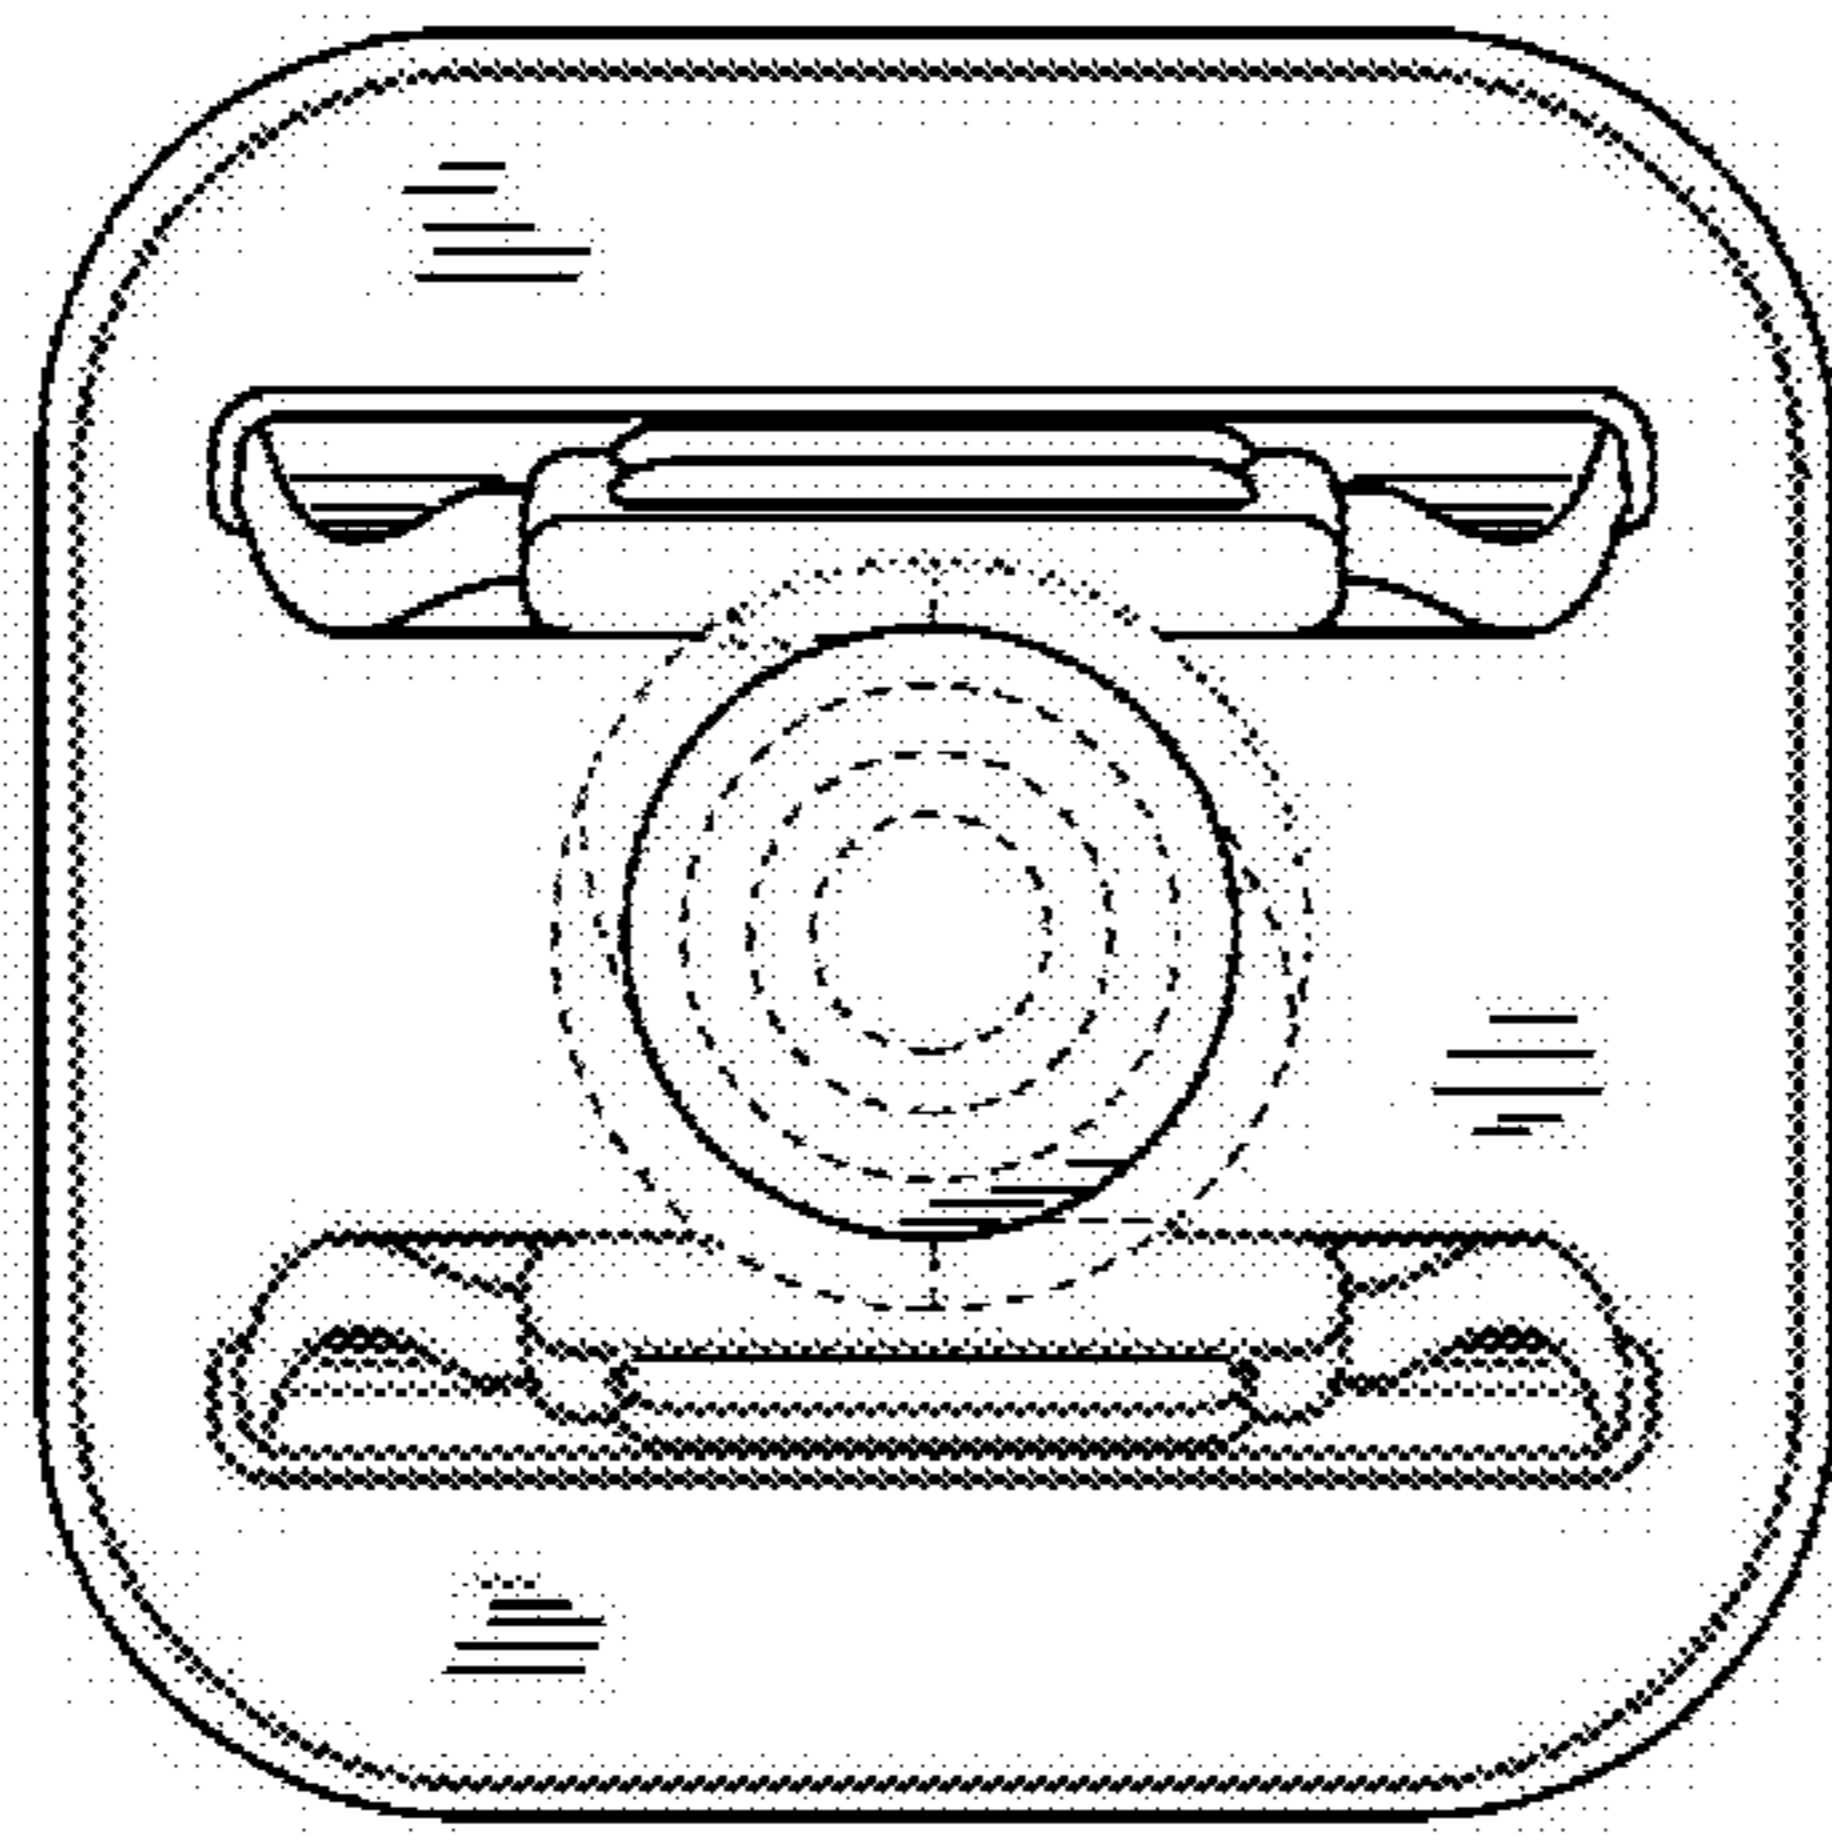

**FIG. 5**

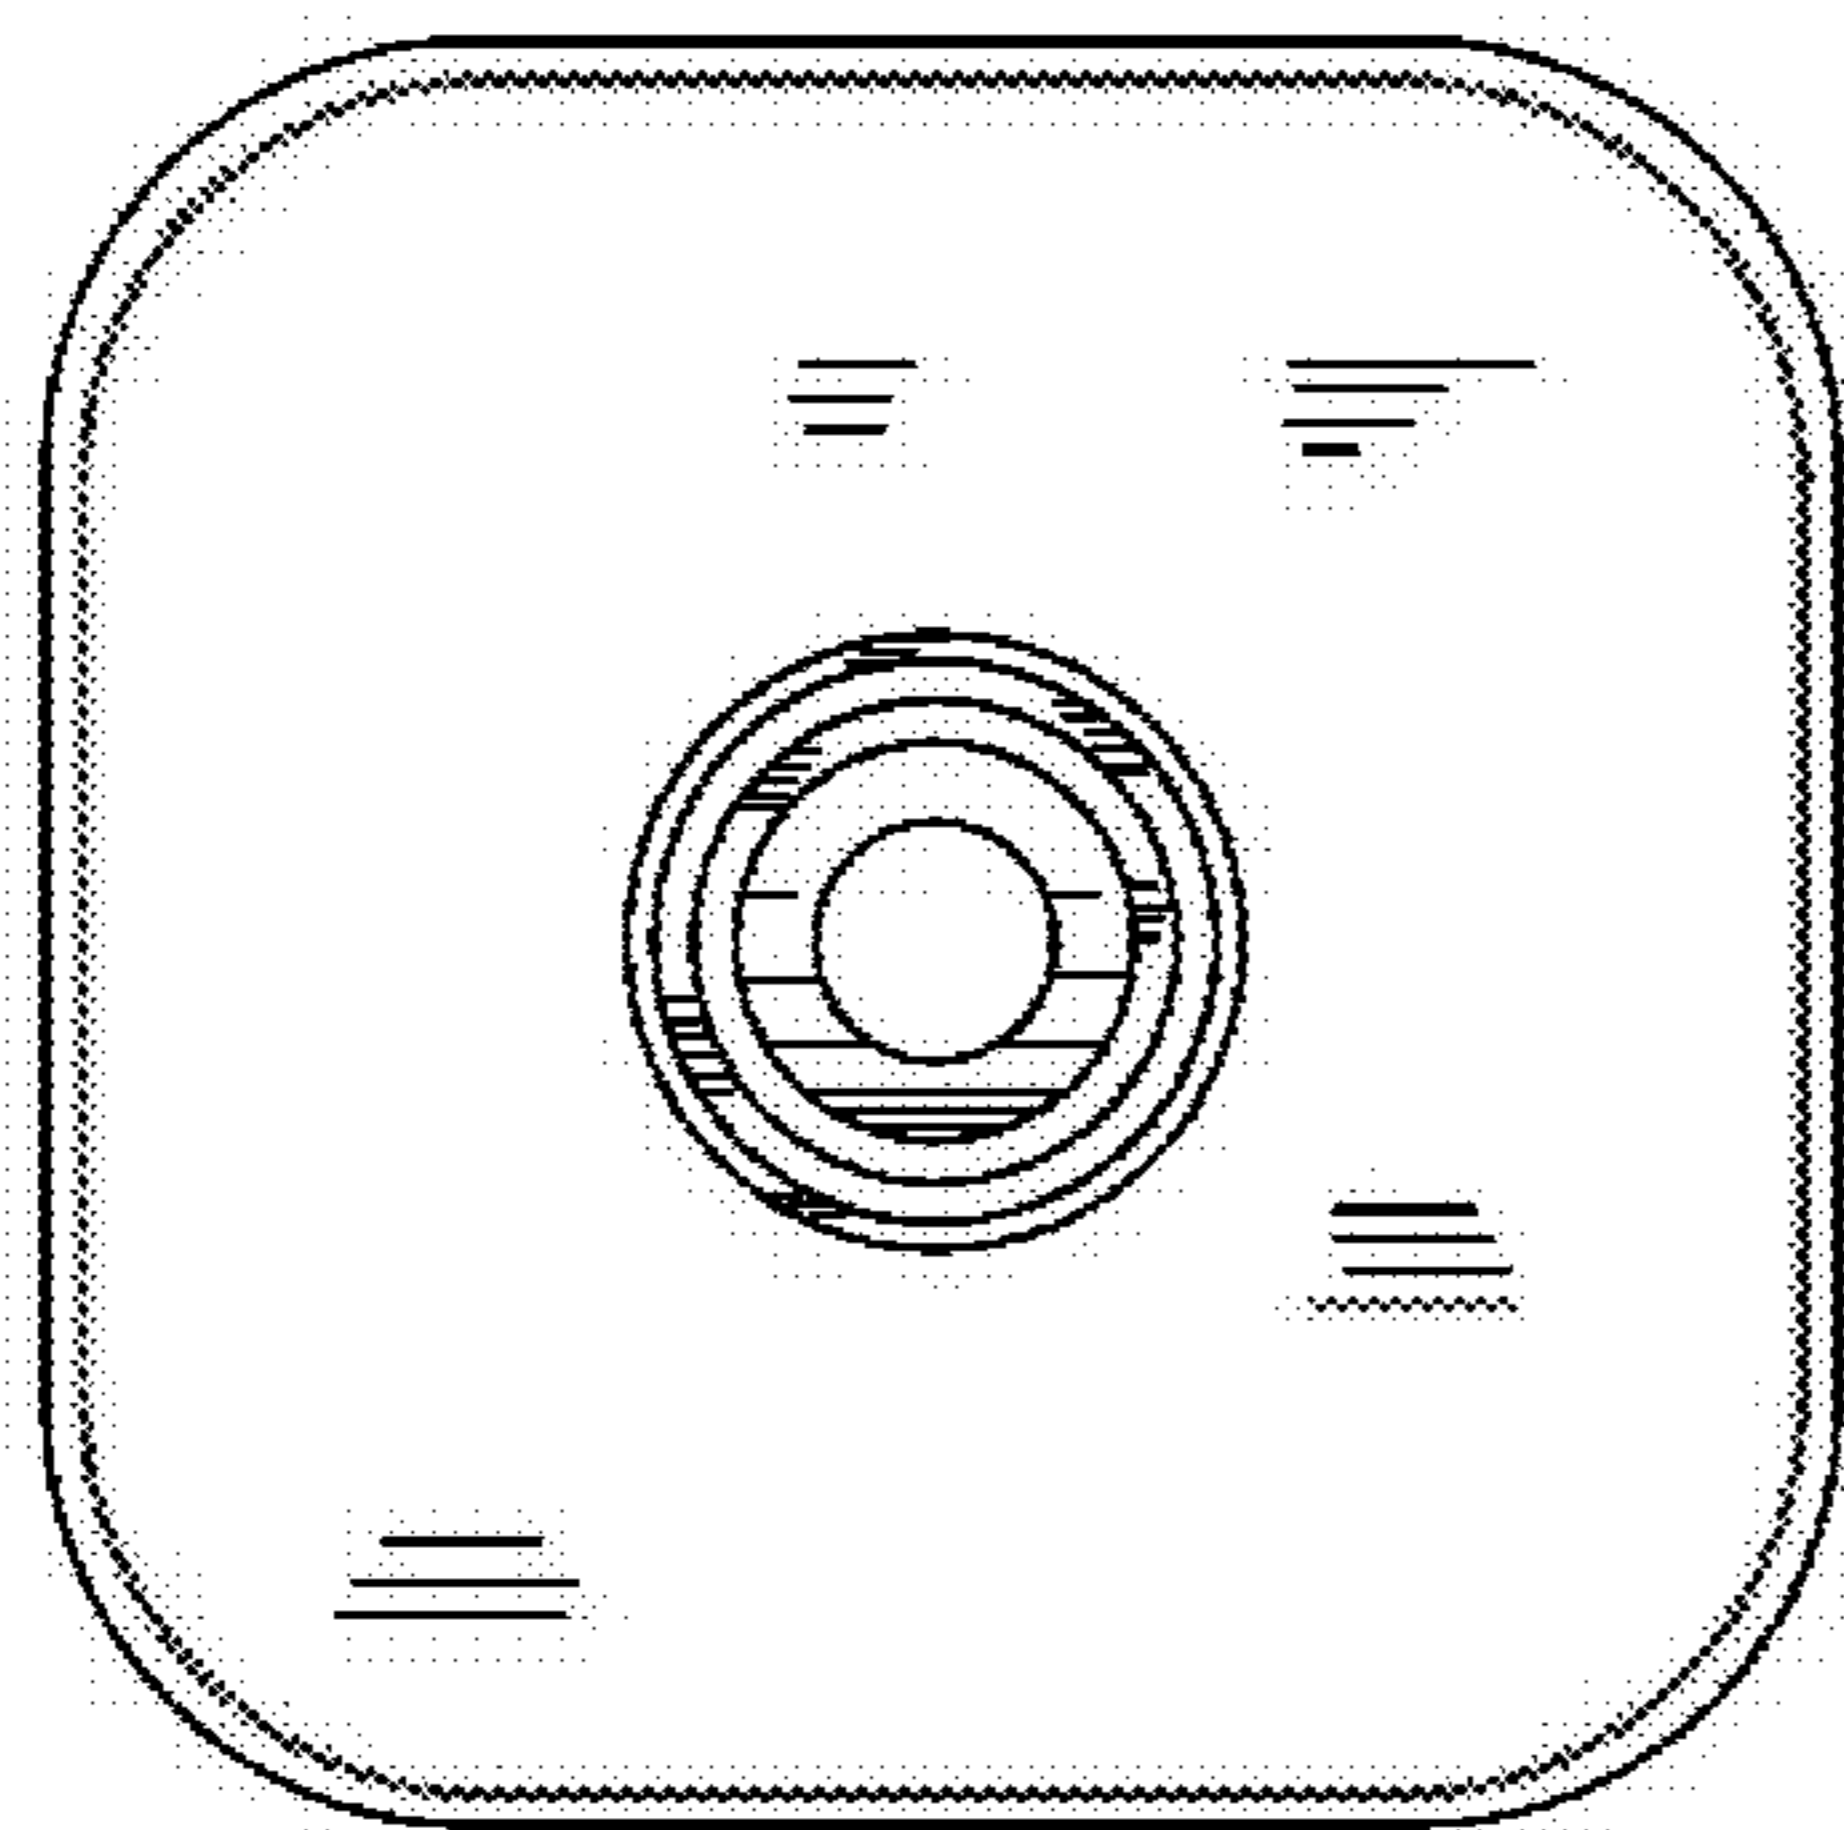

**FIG. 6**