



US00D709901S

(12) **United States Design Patent**
Landis et al.

(10) **Patent No.:** **US D709,901 S**
(45) **Date of Patent:** **** Jul. 29, 2014**

(54) **DISPLAY SCREEN WITH COMPUTER ICON FOR BLOOD GLUCOSE MONITORING**

(75) Inventors: **Jeremy Landis**, New York City, NY (US); **Salve Retuta Pascual**, Washington, DC (US)

(73) Assignee: **Lifescan, Inc.**, Milipitas, CA (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/393,126**

(22) Filed: **May 31, 2011**

(51) **LOC (10) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/486**

(58) **Field of Classification Search**
USPC D14/485-495; 715/710, 706, 772, 716; D9/434
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | |
|-----------|------|--------|----------------|-------------|
| 6,437,804 | B1 * | 8/2002 | Ibe et al. | 715/736 |
| D502,184 | S * | 2/2005 | Glezer et al. | D14/486 |
| 7,020,847 | B1 * | 3/2006 | Holzheuer | 715/855 |
| D594,911 | S * | 6/2009 | Hall et al. | D21/385 |
| D598,923 | S * | 8/2009 | Chen et al. | D14/485 |
| 7,689,585 | B2 * | 3/2010 | Zeng et al. | 707/999.104 |
| D618,695 | S * | 6/2010 | Bennett et al. | D14/485 |

| | | | | |
|--------------|------|---------|------------------|---------|
| D638,024 | S * | 5/2011 | Wall et al. | D14/486 |
| D654,084 | S * | 2/2012 | Joseph | D14/485 |
| D656,946 | S * | 4/2012 | Judy et al. | D14/486 |
| D658,204 | S * | 4/2012 | Jones | D14/492 |
| D667,022 | S * | 9/2012 | LoBosco et al. | D14/486 |
| D674,404 | S * | 1/2013 | Pearcy et al. | D14/486 |
| 2009/0276724 | A1 * | 11/2009 | Rosenthal et al. | 715/771 |
| 2010/0105999 | A1 * | 4/2010 | Dixon et al. | 600/347 |
| 2011/0053121 | A1 * | 3/2011 | Heaton | 434/127 |

* cited by examiner

Primary Examiner — Kevin Rudzinski


(57) **CLAIM**

We claim the ornamental design for a display screen with computer icon for blood glucose monitoring, as shown and described.

DESCRIPTION

The patent file contains at least one drawing executed in color. Copies of this patent with a color drawing will be provided by the Office upon request and payment of the necessary fee. FIG. 1 illustrates a front view of a display screen with computer icon for blood glucose monitoring showing our new design; FIG. 2 illustrates a second embodiment thereof; FIG. 3 illustrates a third embodiment thereof; and, FIG. 4 illustrates a fourth embodiment thereof. The features shown in broken lines in various Figures are for illustrating reference or environmental structure and form no part of the claimed design.

1 Claim, 4 Drawing Sheets
(4 of 4 Drawing Sheet(s) Filed in Color)

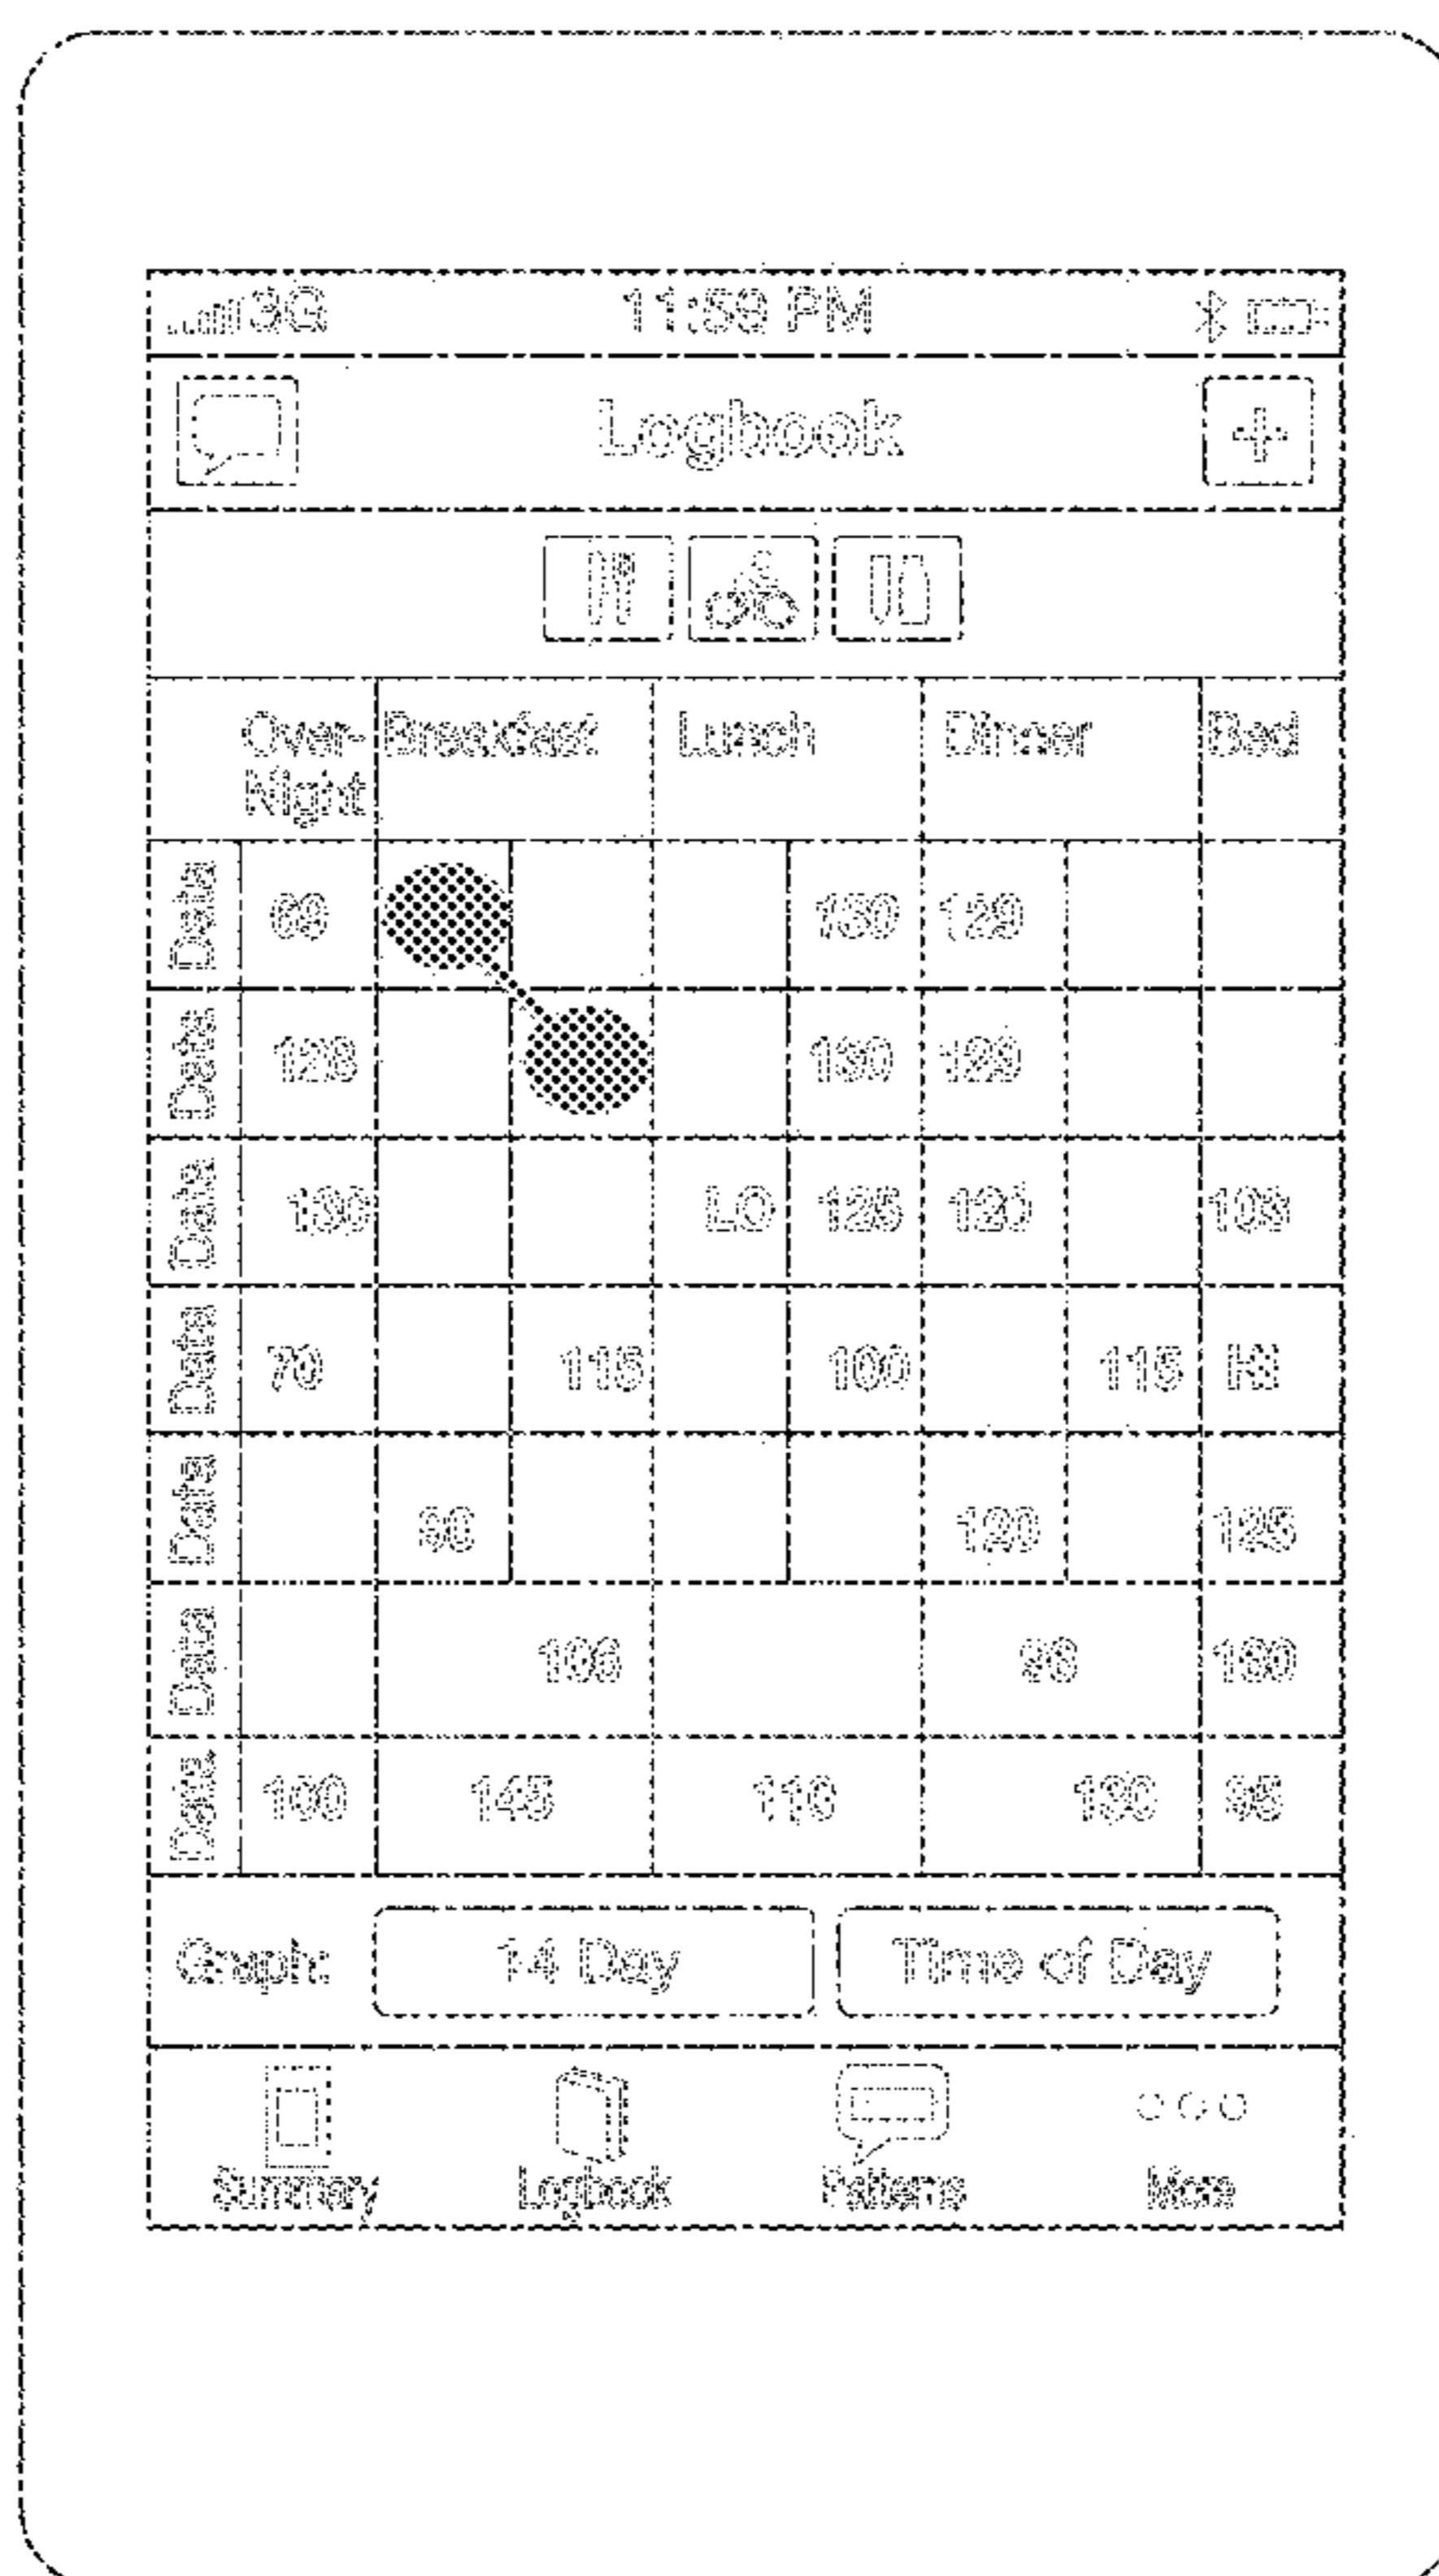

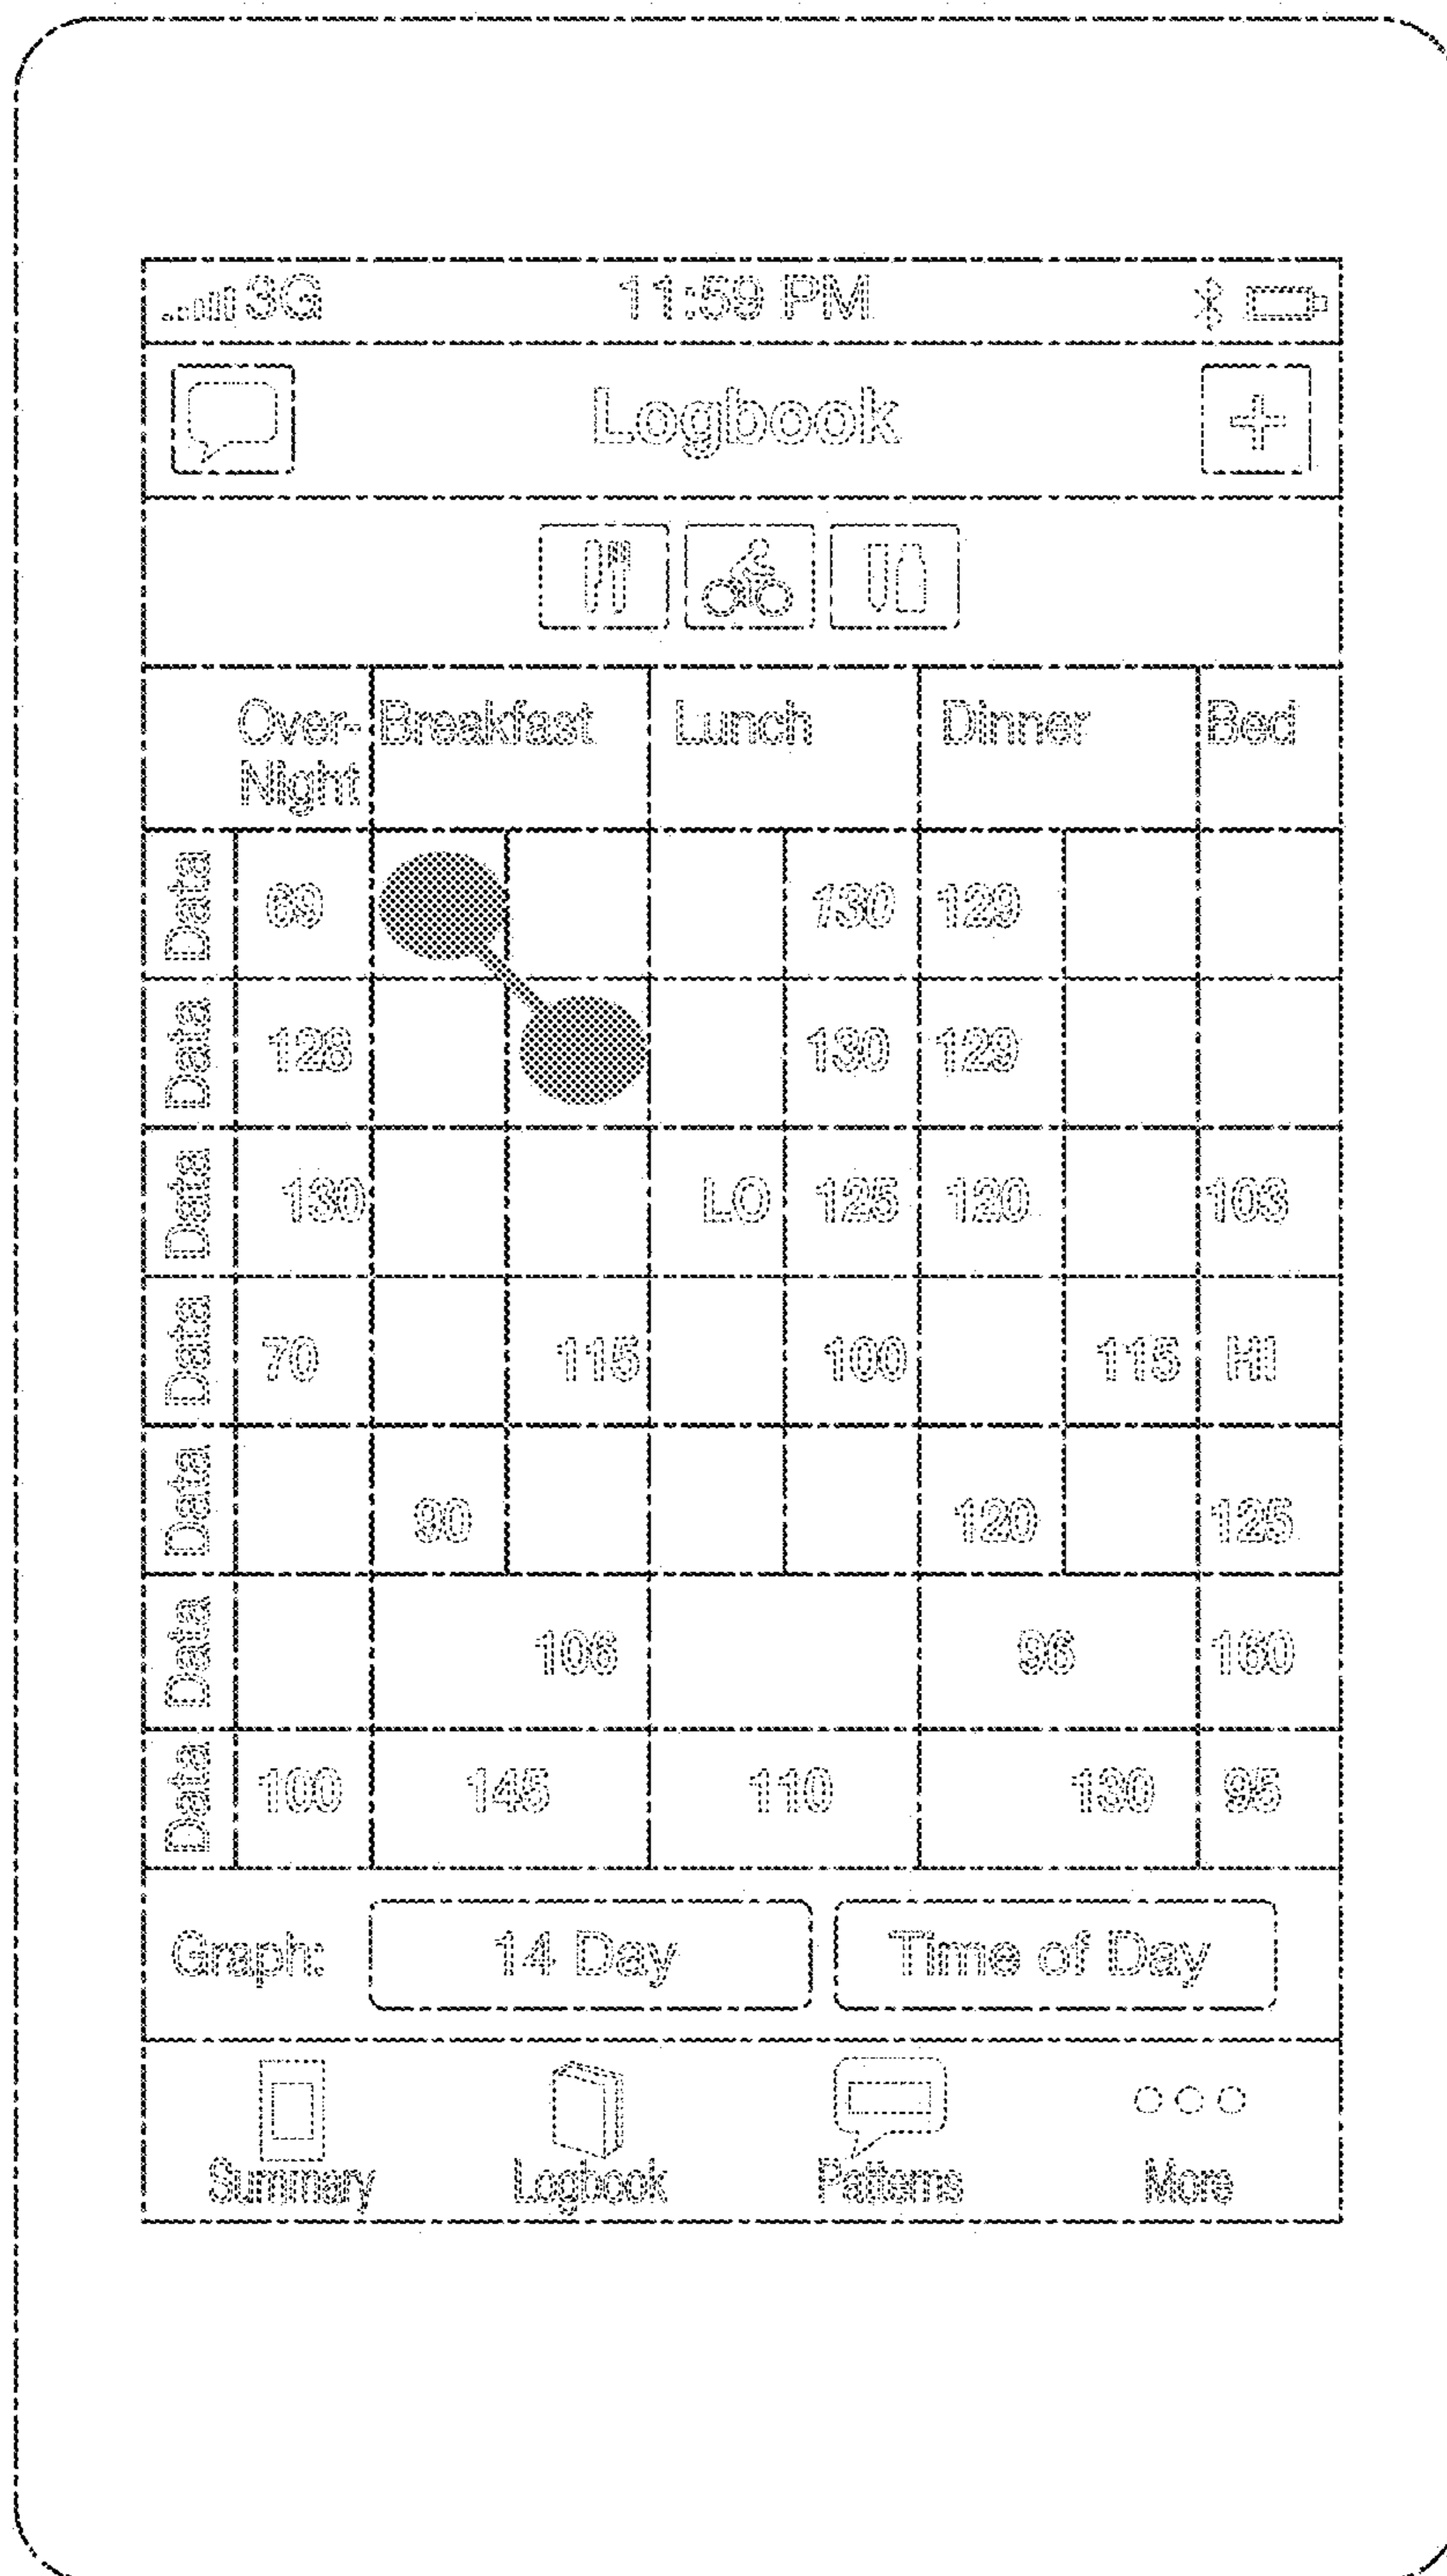


FIG. 1

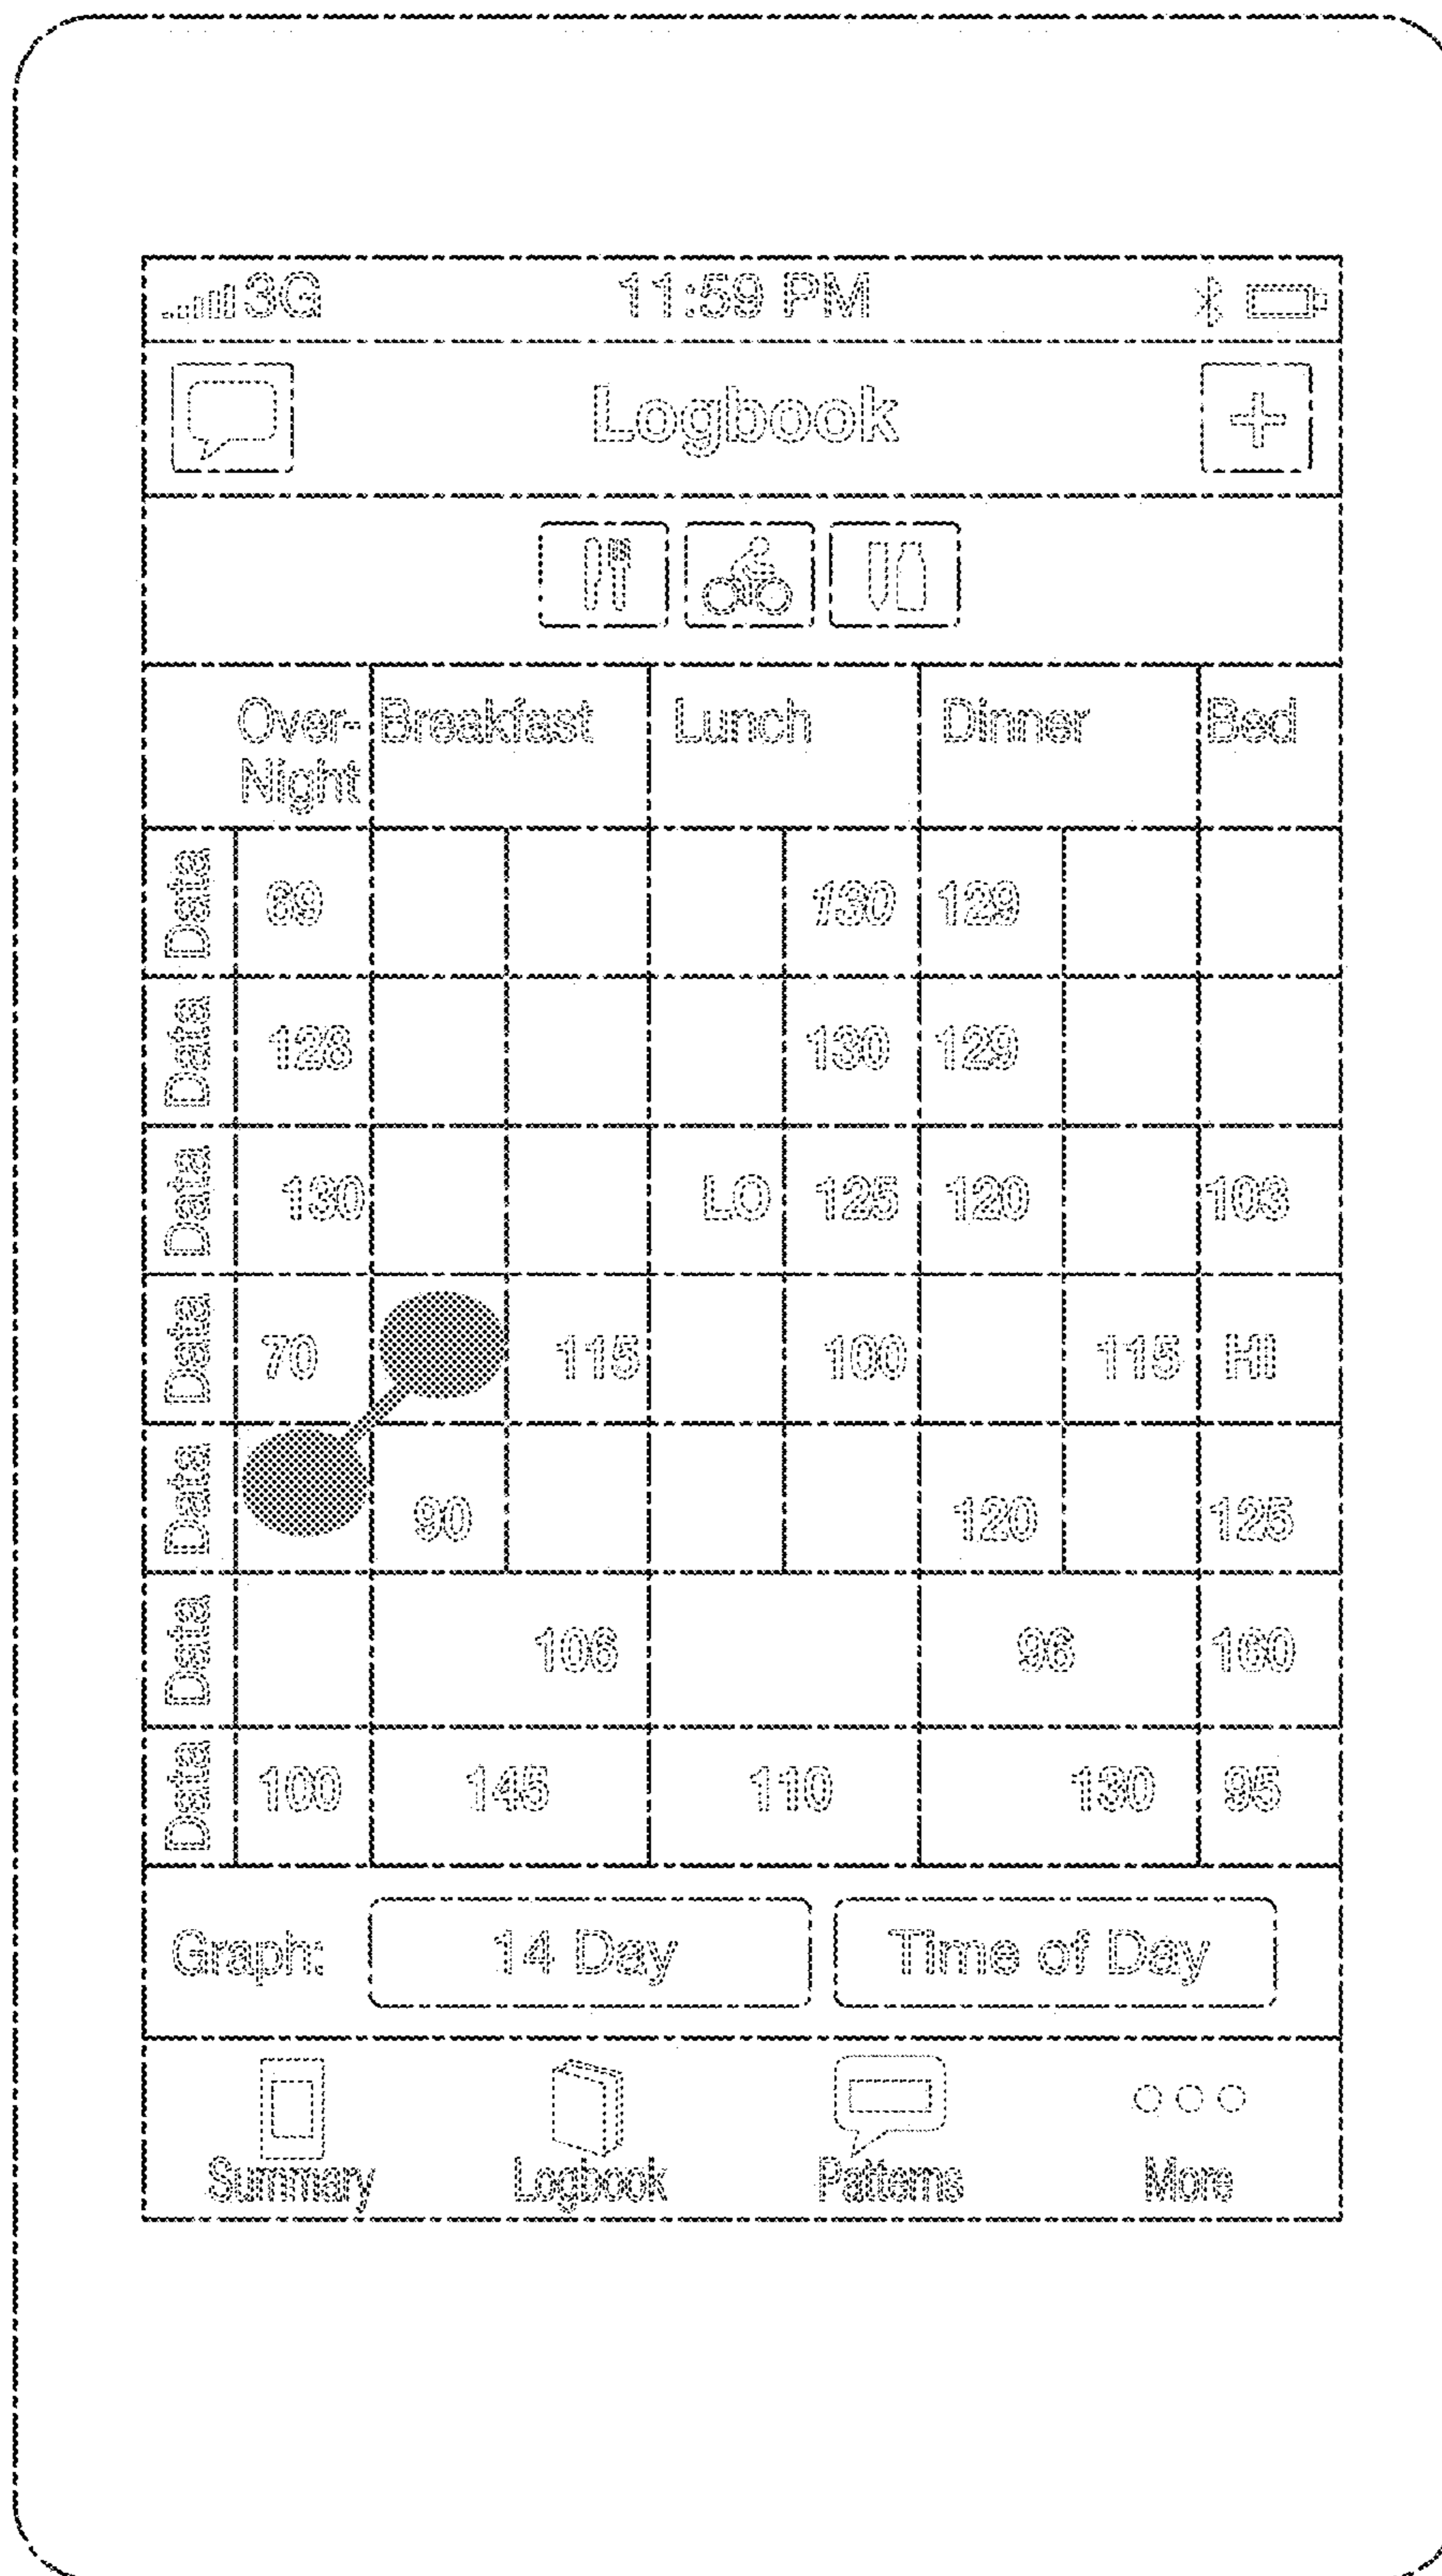


FIG. 2

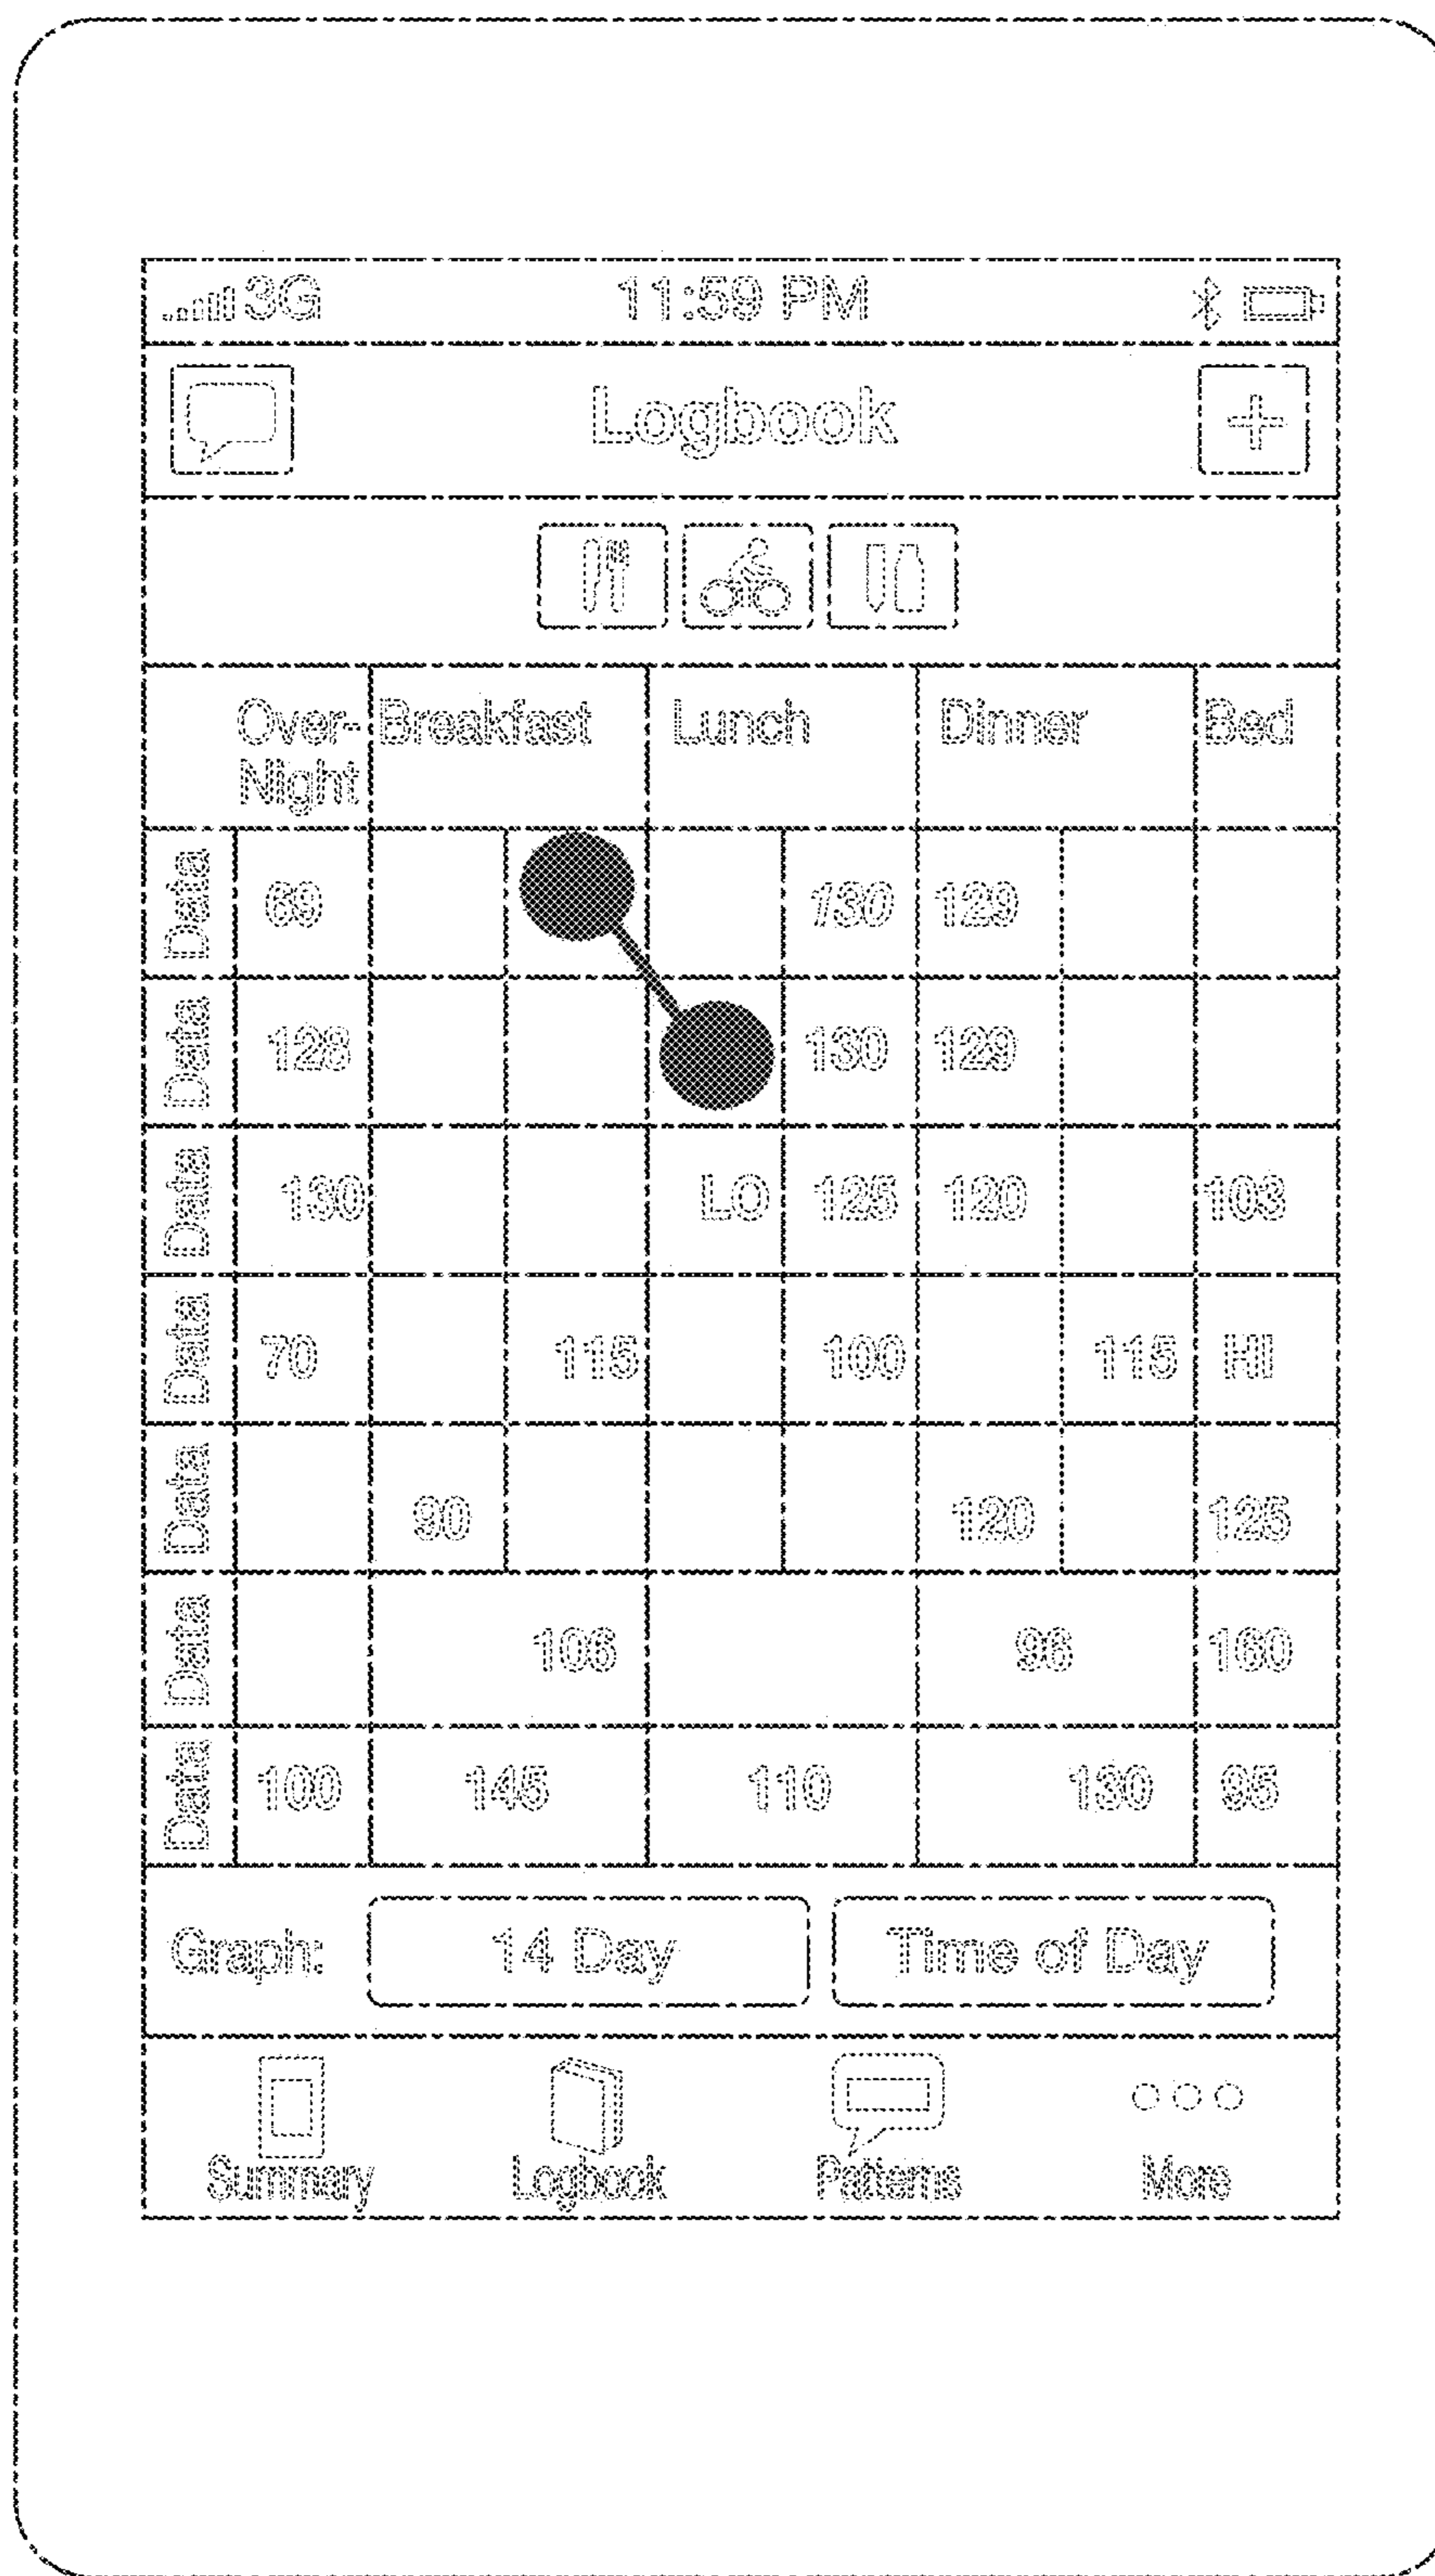


FIG. 3

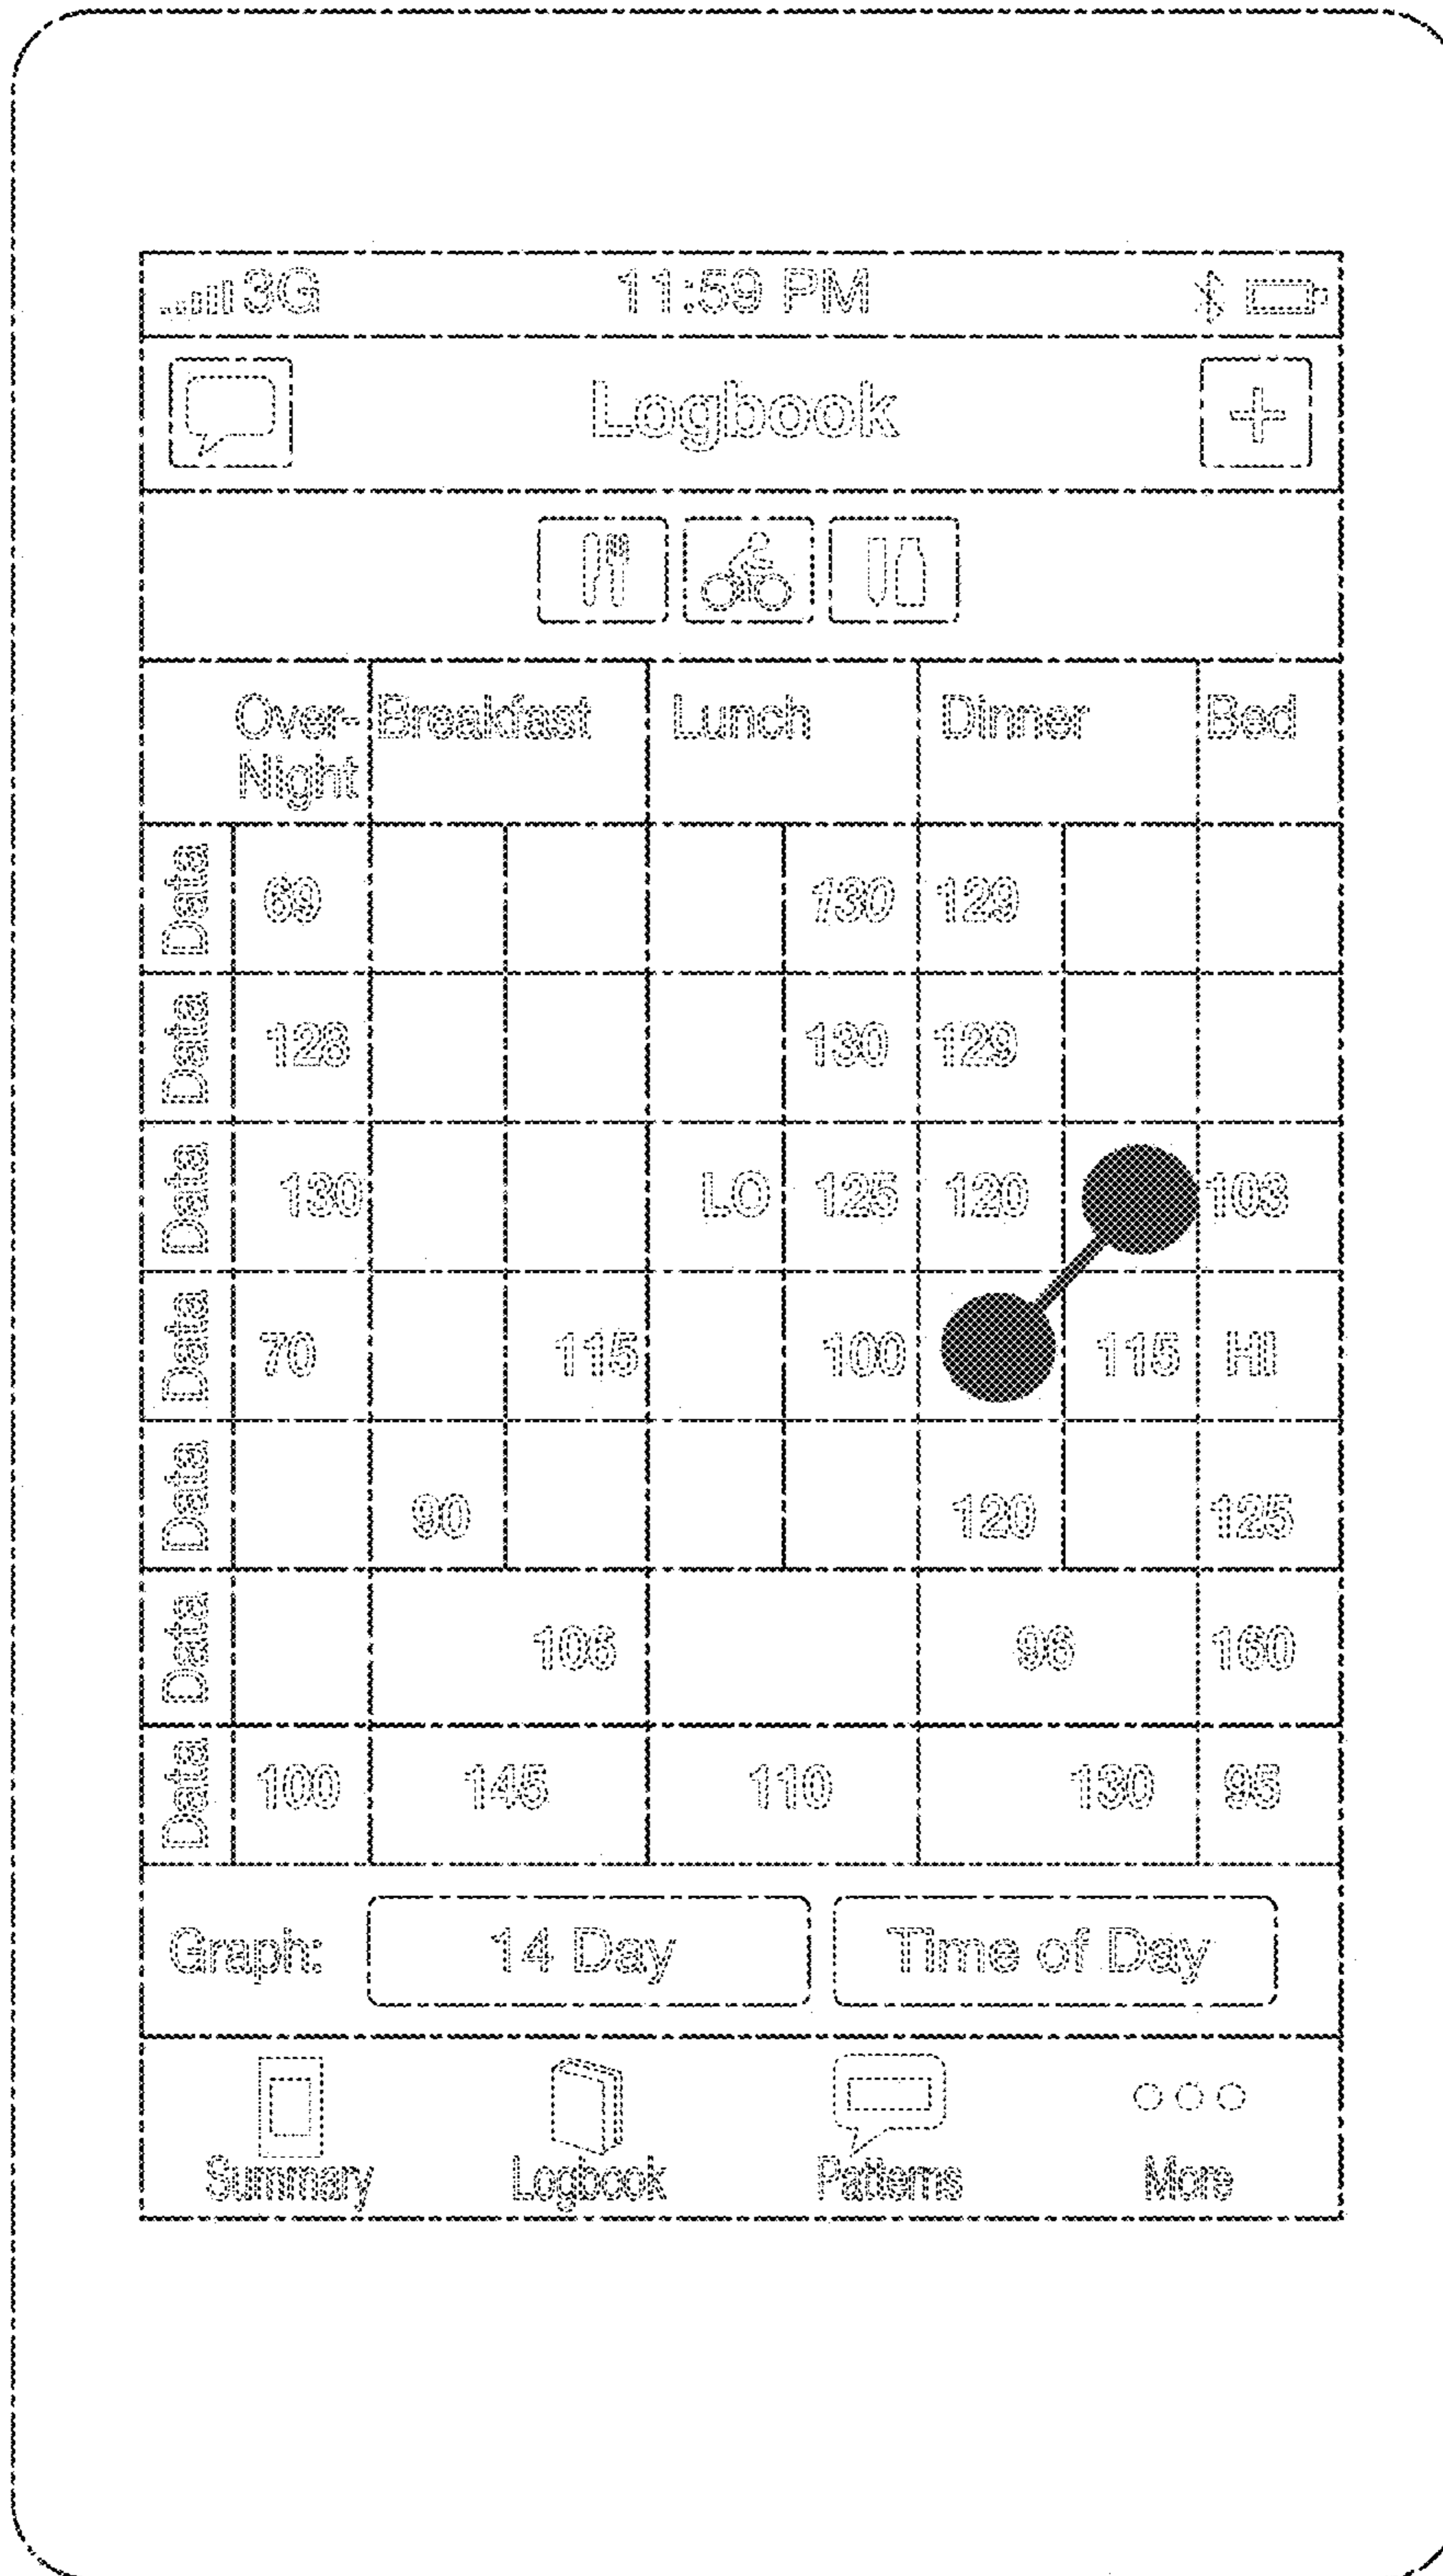


FIG. 4

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : D709,901 S
APPLICATION NO. : 29/393126
DATED : July 29, 2014
INVENTOR(S) : Jeremy Landis et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the title page, above DESCRIPTION, enter the following information:

-- Cross-Reference to Related Applications

This application claims the benefits under 35 U.S.C. § 120 as a continuation application of U.S. Patent Application Serial No. 13/192,348, filed July 27, 2011, which claims the benefit of prior U.S. Provisional Patent Application Serial No. 61/415,598 filed November 19, 2010, all of the disclosures of the prior applications are incorporated herein by reference in their entireties. --

Signed and Sealed this
Twenty-first Day of July, 2015



Michelle K. Lee
Director of the United States Patent and Trademark Office