



US00D710501S

(12) **United States Design Patent**
Hayman et al.

(10) **Patent No.:** **US D710,501 S**
(45) **Date of Patent:** **** *Aug. 5, 2014**

(54) **RECEPTOR HOLDING DEVICE**

(71) Applicant: **Zuma Dental, LLC**, Los Angeles, CA
(US)

(72) Inventors: **Robert Hayman**, Los Angeles, CA
(US); **Ekram Khan**, League City, TX
(US); **Michael Paloian**, Cold Spring
Harbor, NY (US); **Anthony Orchard**,
Wantagh, NY (US)

(73) Assignee: **Zuma Dental, LLC**, Los Angeles, CA
(US)

(*) Notice: This patent is subject to a terminal dis-
claimer.

(**) Term: **14 Years**

(21) Appl. No.: **29/449,990**

(22) Filed: **Mar. 15, 2013**

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/161**

(58) **Field of Classification Search**
USPC D24/158–161, 185, 186, 152, 176, 177;
D8/394, 396; 378/38–40, 169–170,
378/177, 180, 191, 205
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D246,798 S * 12/1977 Jermyn D24/161
4,484,342 A * 11/1984 Allison et al. 378/168
D283,157 S * 3/1986 Maldonado et al. D24/161

5,289,522 A * 2/1994 Kanbar et al. 378/170
D370,732 S * 6/1996 Smith D24/176
5,652,779 A * 7/1997 Levy et al. 378/170
D406,892 S * 3/1999 Warren D24/161
6,592,256 B2 * 7/2003 Da Rold et al. 378/168
D537,943 S * 3/2007 Schmulenson D24/158
7,871,199 B2 * 1/2011 Szommer 378/170
8,016,483 B2 * 9/2011 Steward, Jr. 378/170
8,573,844 B2 * 11/2013 Steward et al. 378/170
2006/0245549 A1 * 11/2006 Calderwood et al. 378/191
2010/0027756 A1 * 2/2010 Hof 378/170
2011/0299663 A1 * 12/2011 Steward, Jr. 378/170

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Quan & Associates; Nancy
N. Quan; Christopher N. Quan

(57) **CLAIM**


The ornamental design for a receptor holding device, as
shown and described.

DESCRIPTION

FIG. 1 is a back and side perspective view of receptor holding
device embodying our new design;
FIG. 2 is a front and side perspective view thereof;
FIG. 3 is front view thereof;
FIG. 4 is a back view thereof;
FIG. 5 is a top view thereof;
FIG. 6 is a right side view thereof;
FIG. 7 is a bottom view; and,
FIG. 8 is a left side view thereof.

The break lines in the drawing views indicate that a specific
length of the receptor holding device forms no part of the
claimed design.

1 Claim, 2 Drawing Sheets

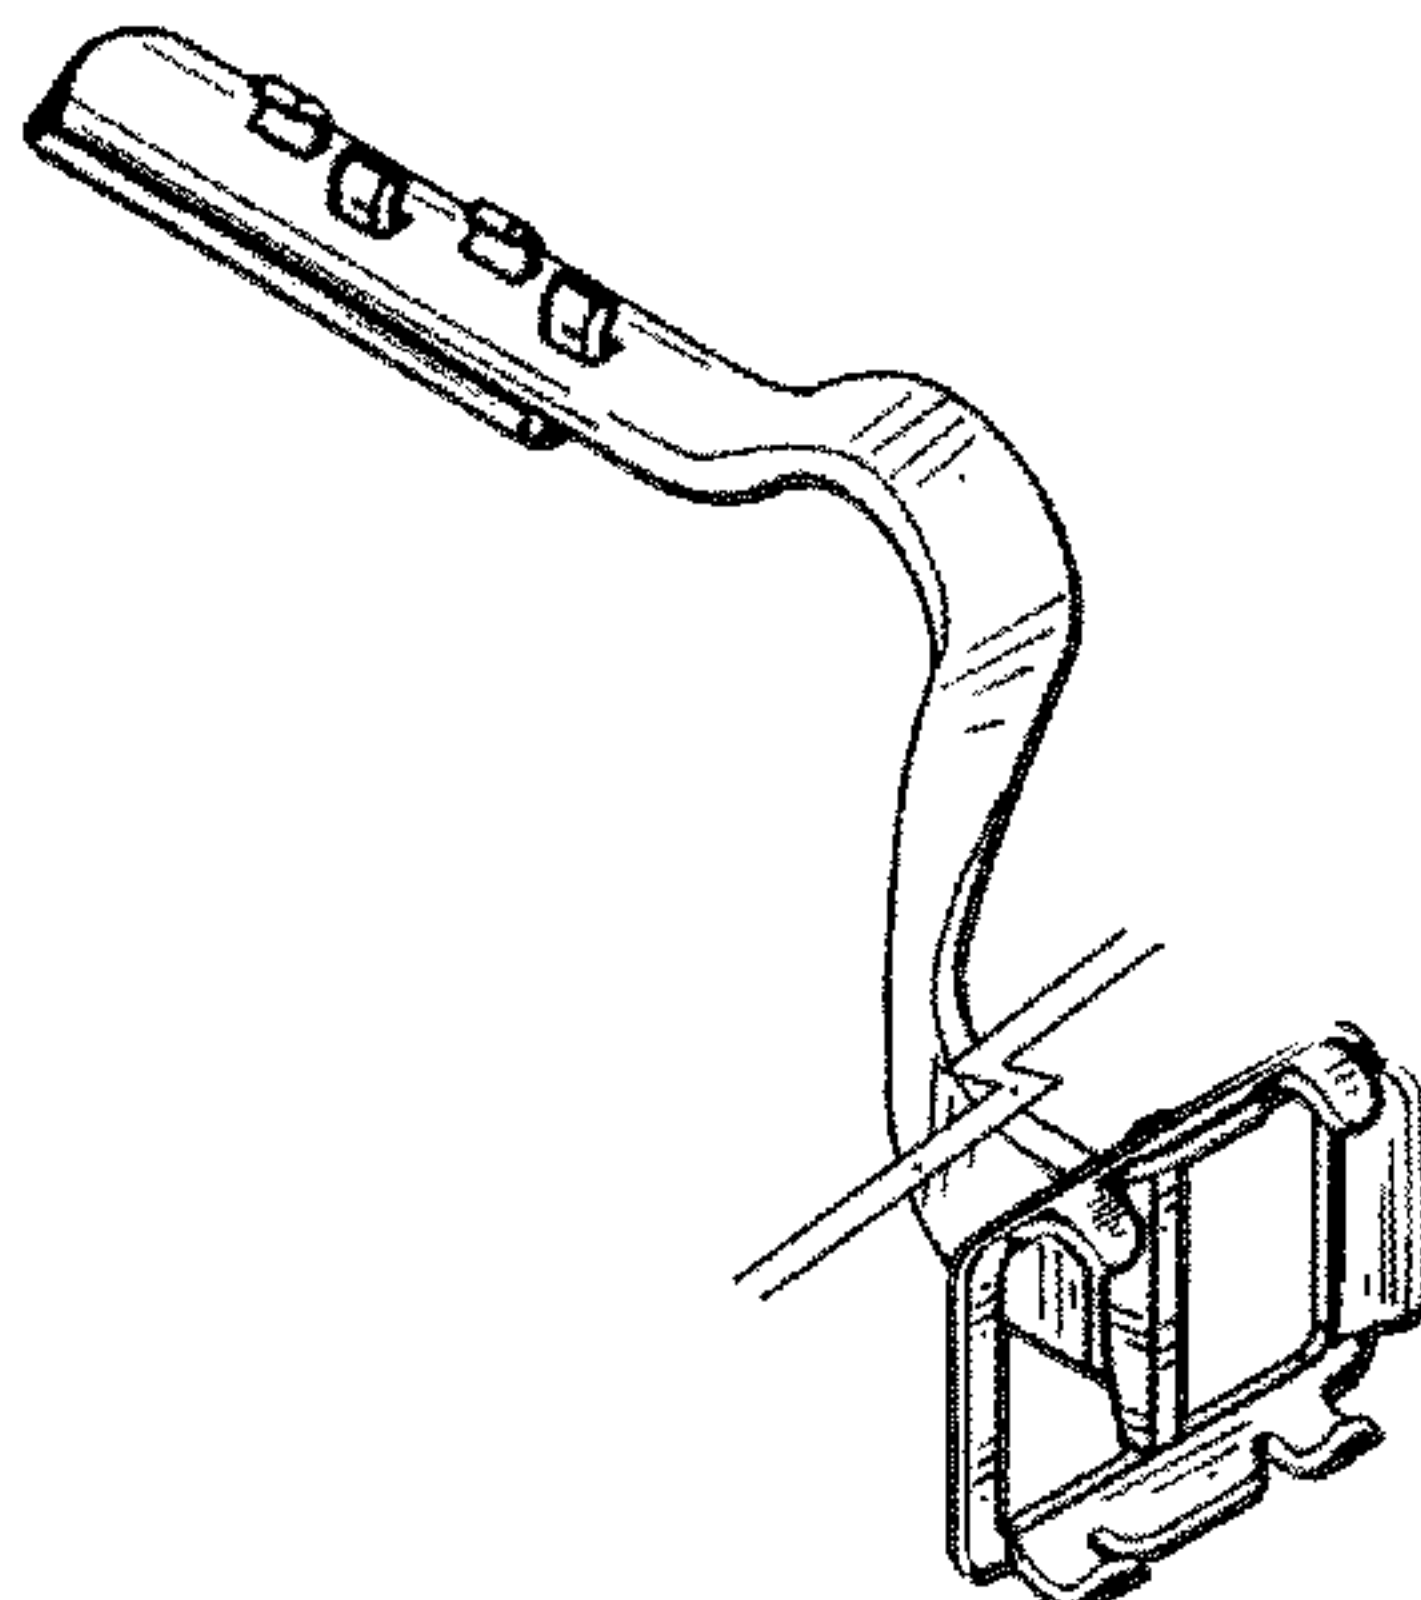

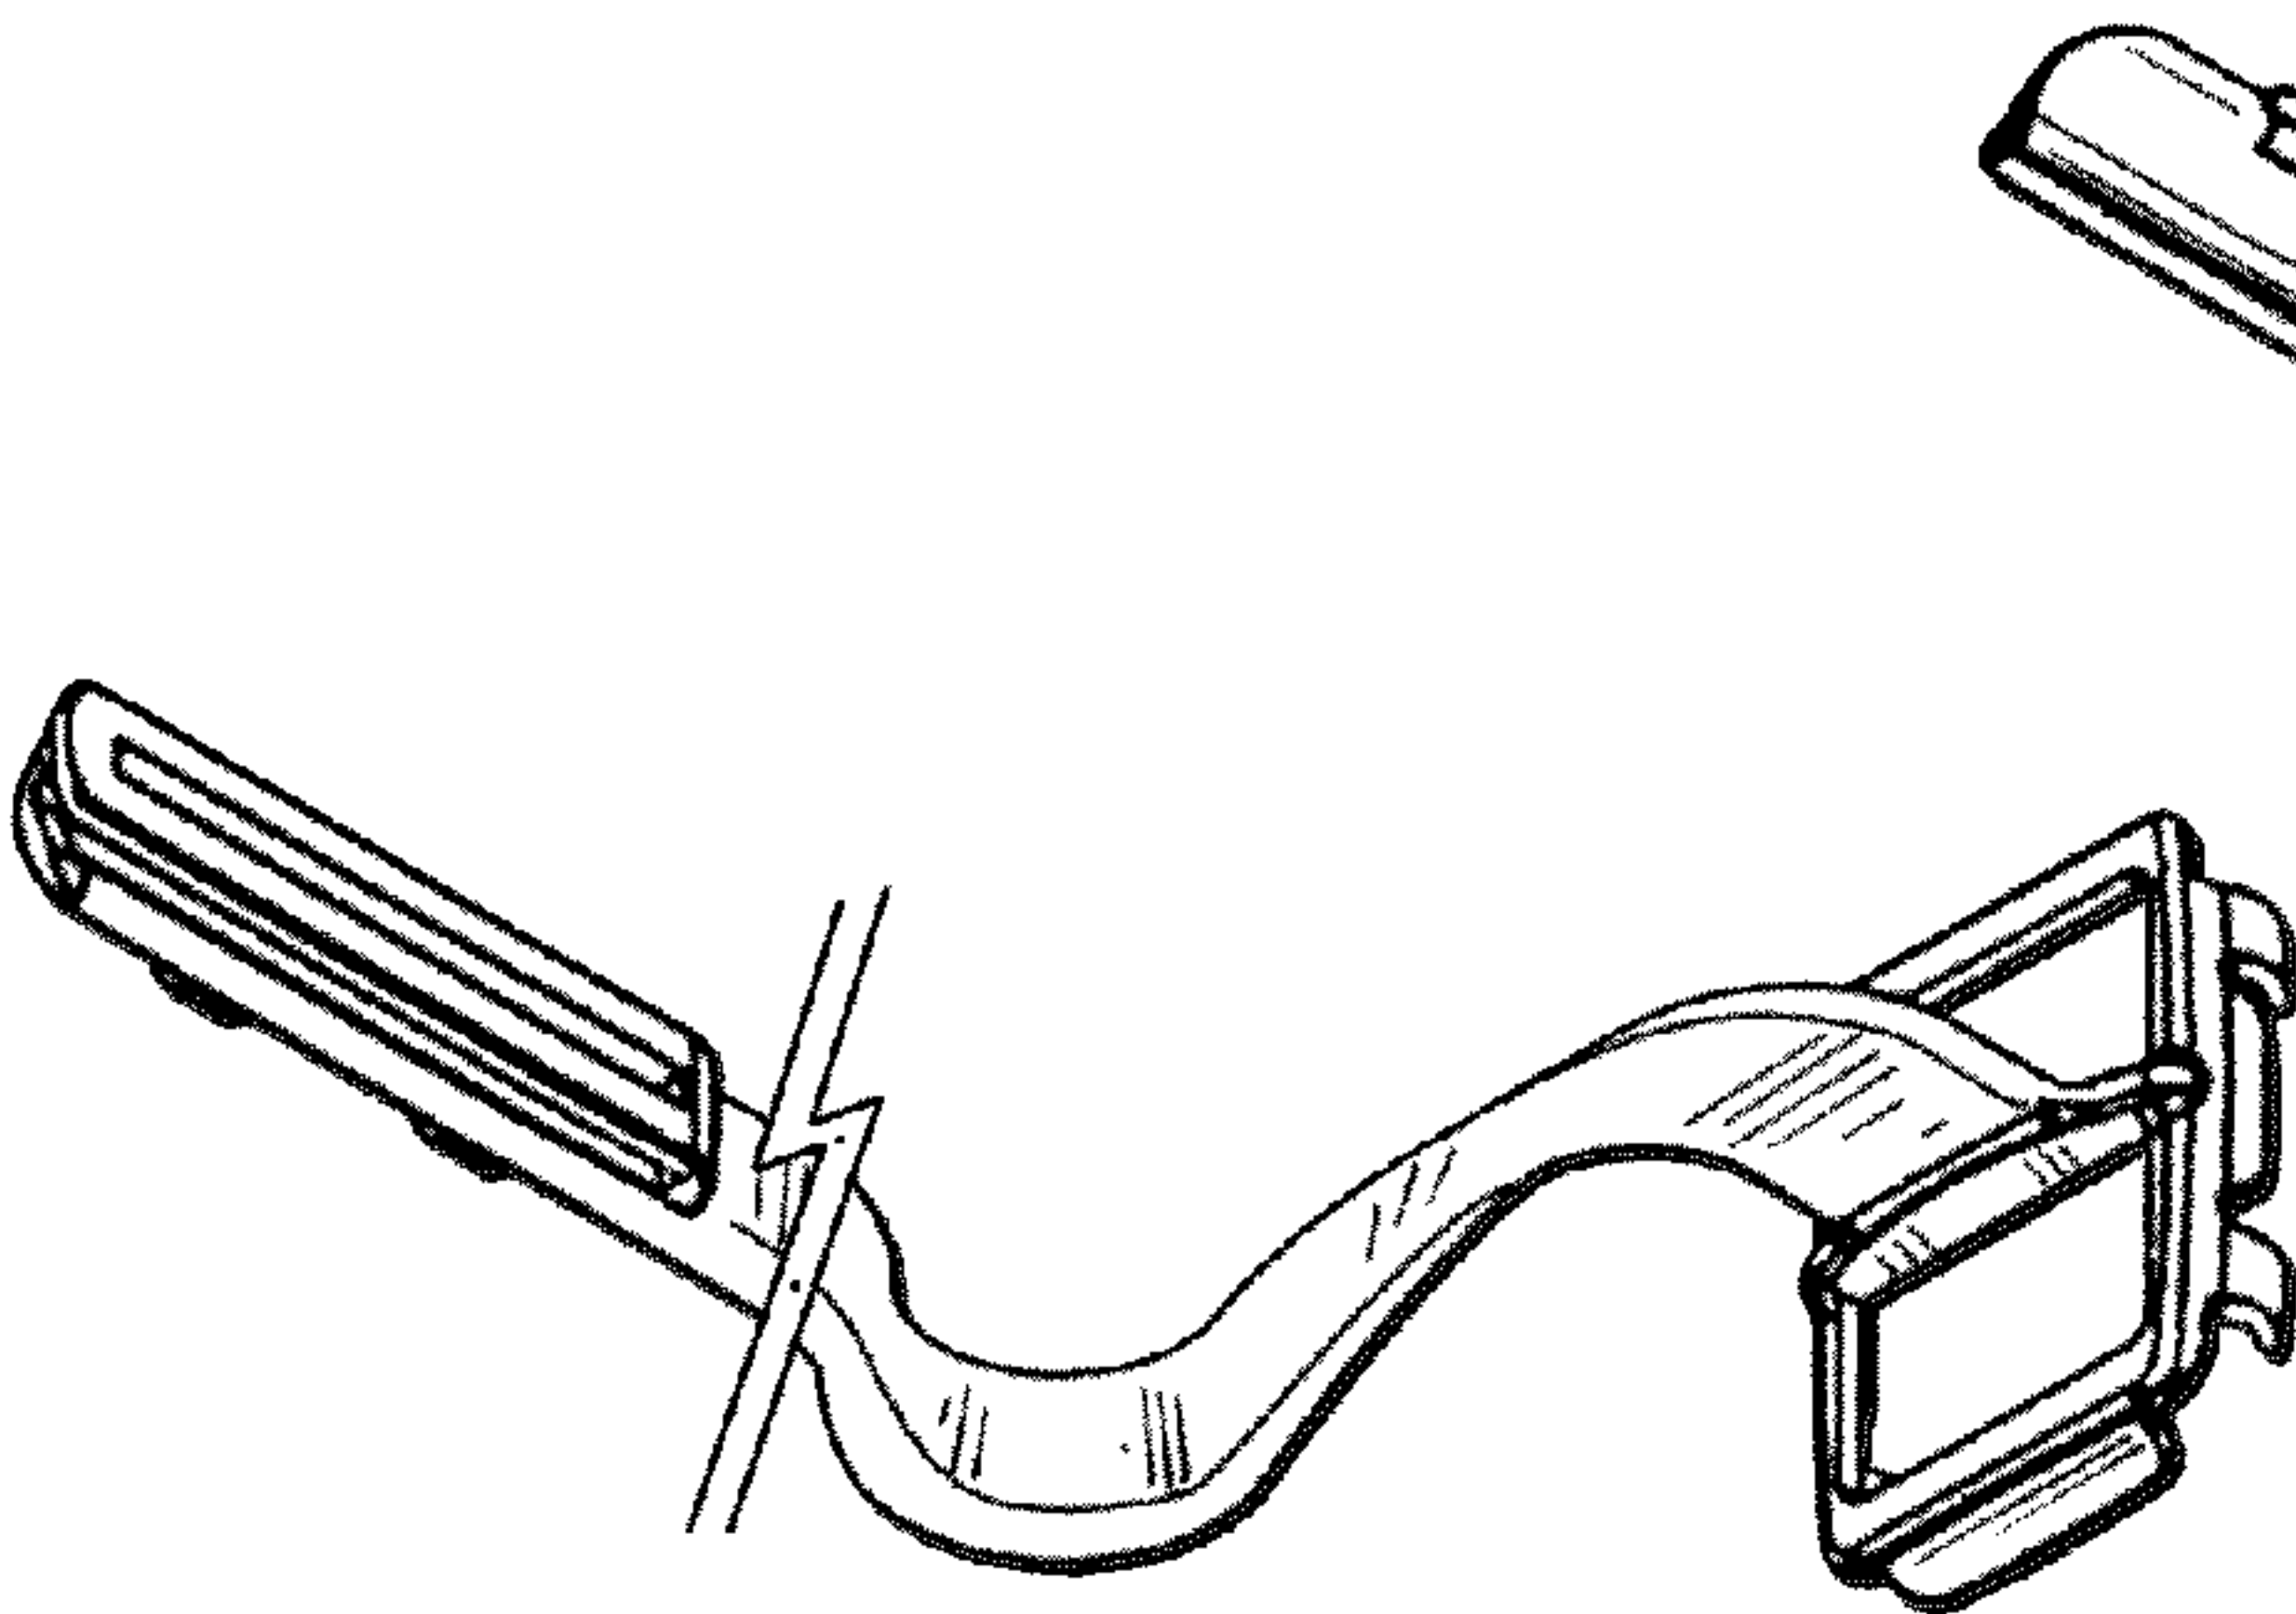


Fig. 1

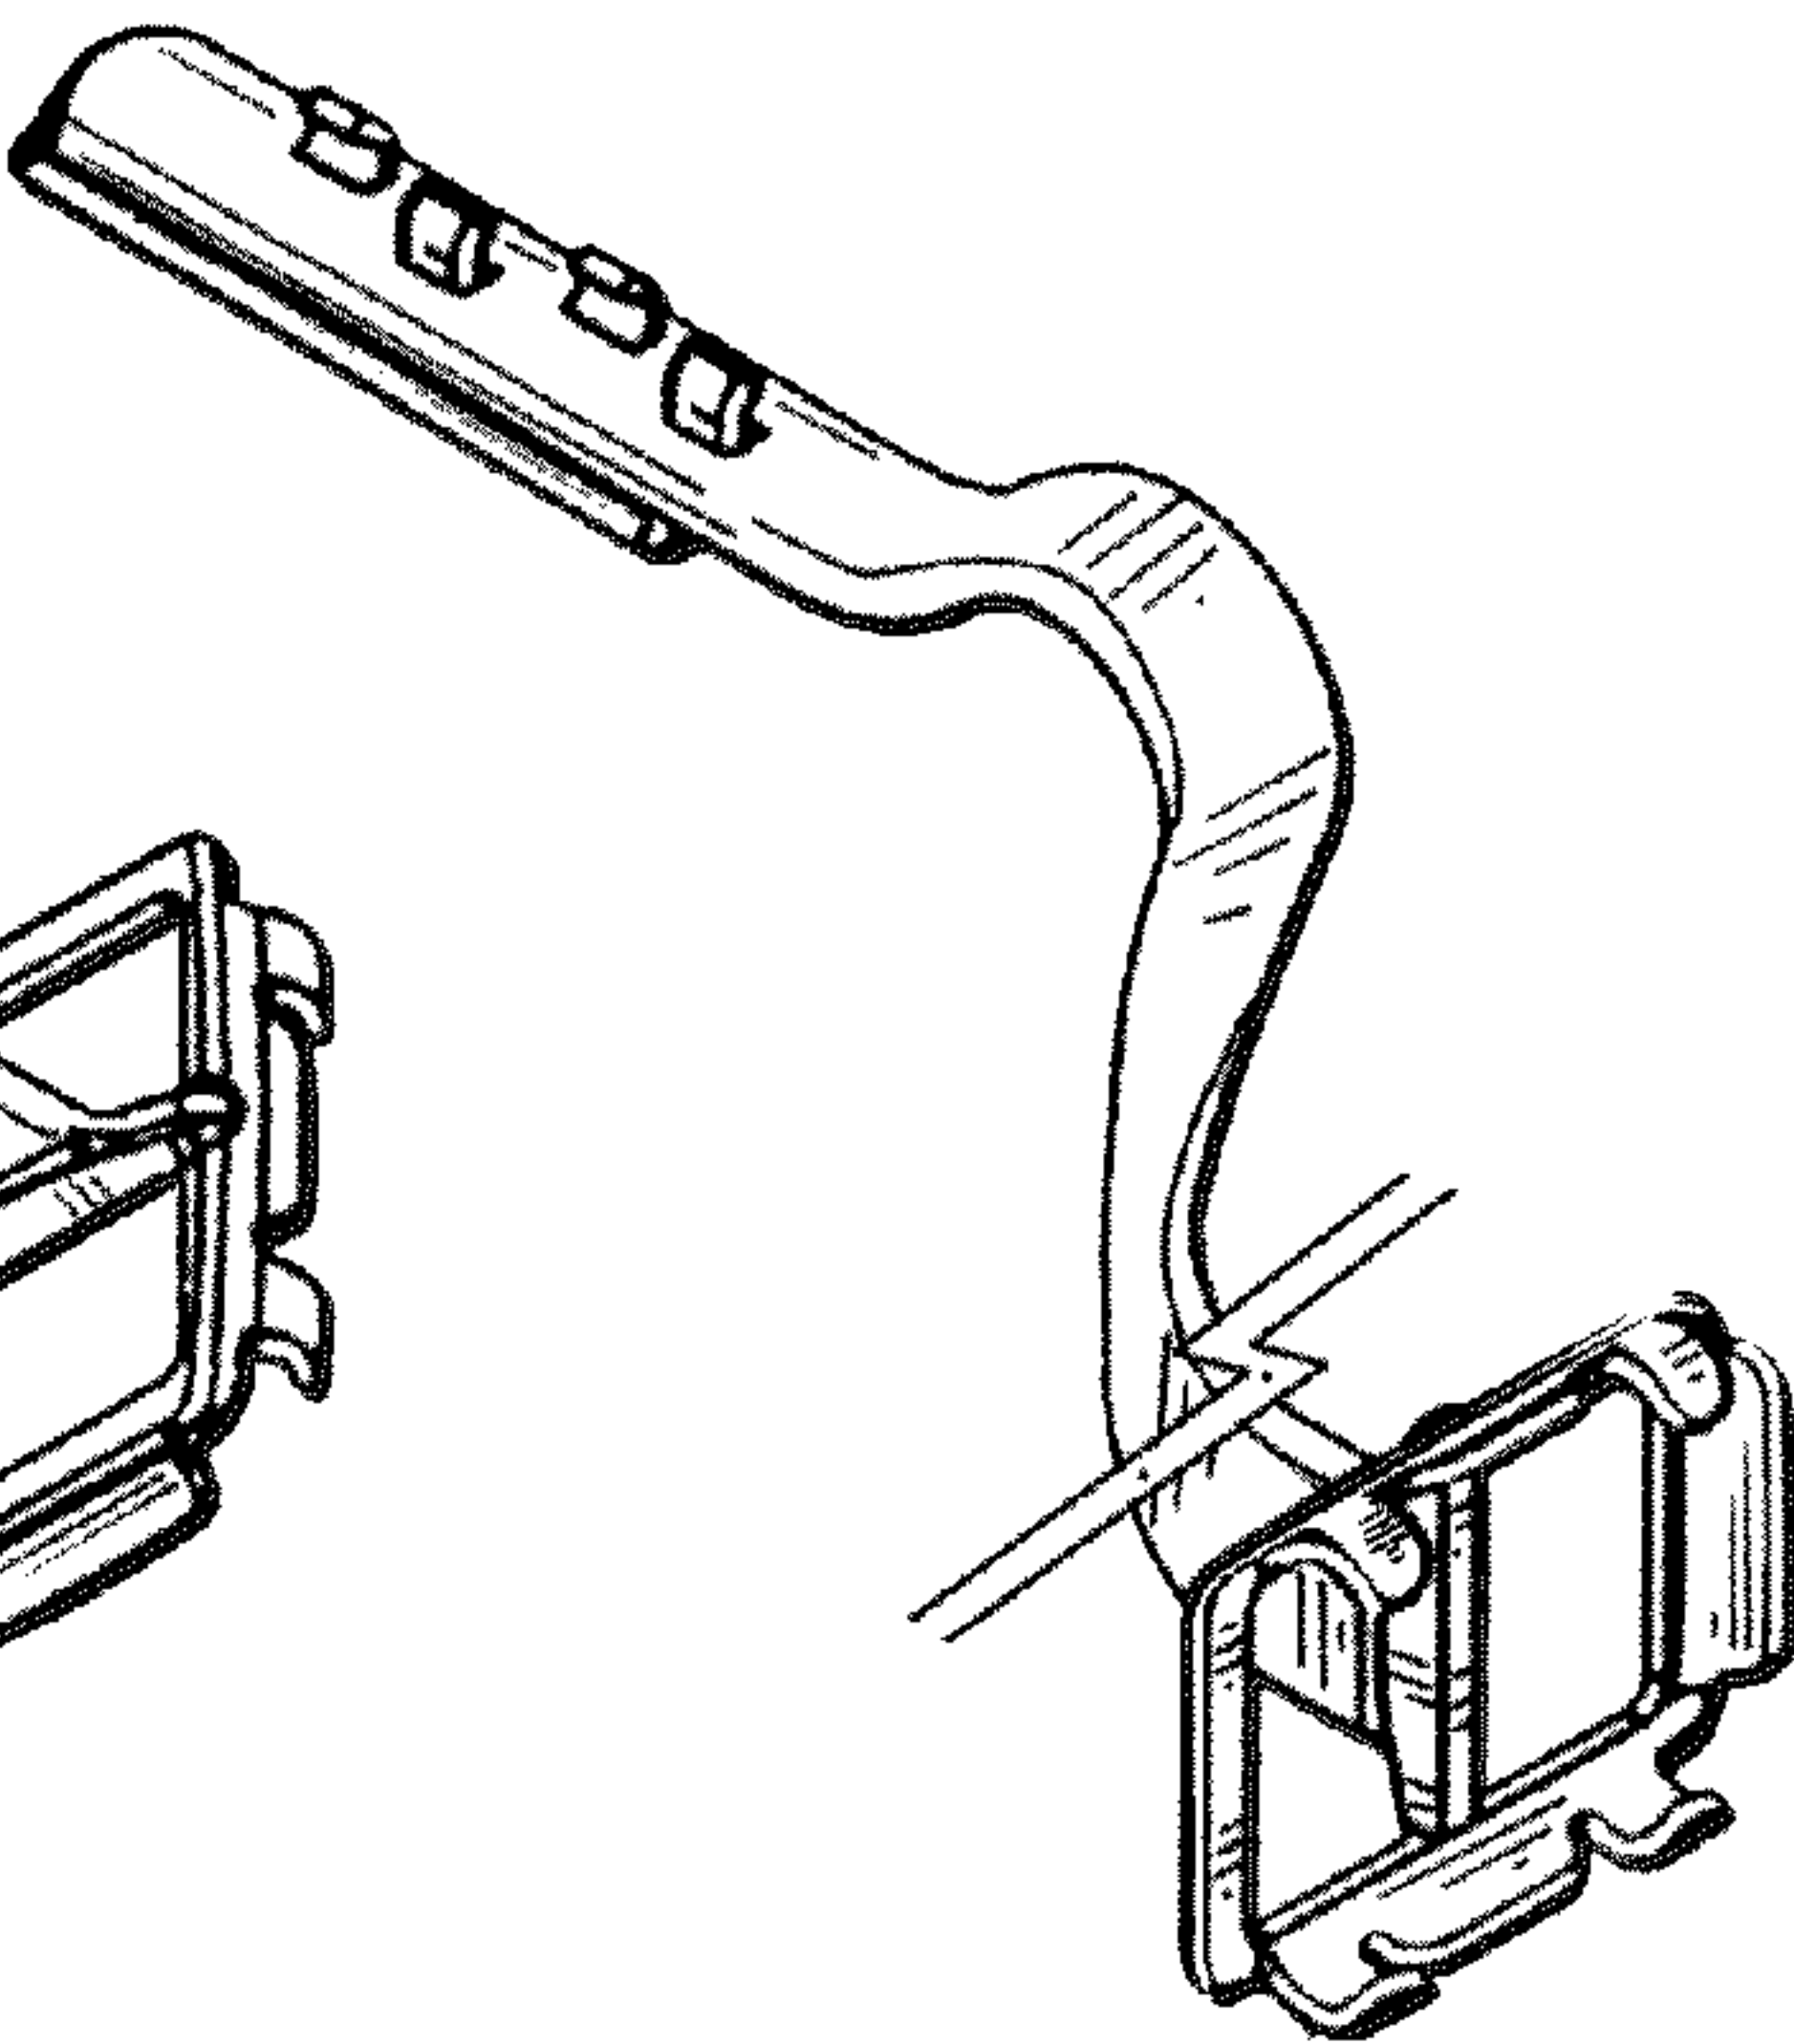


Fig. 2

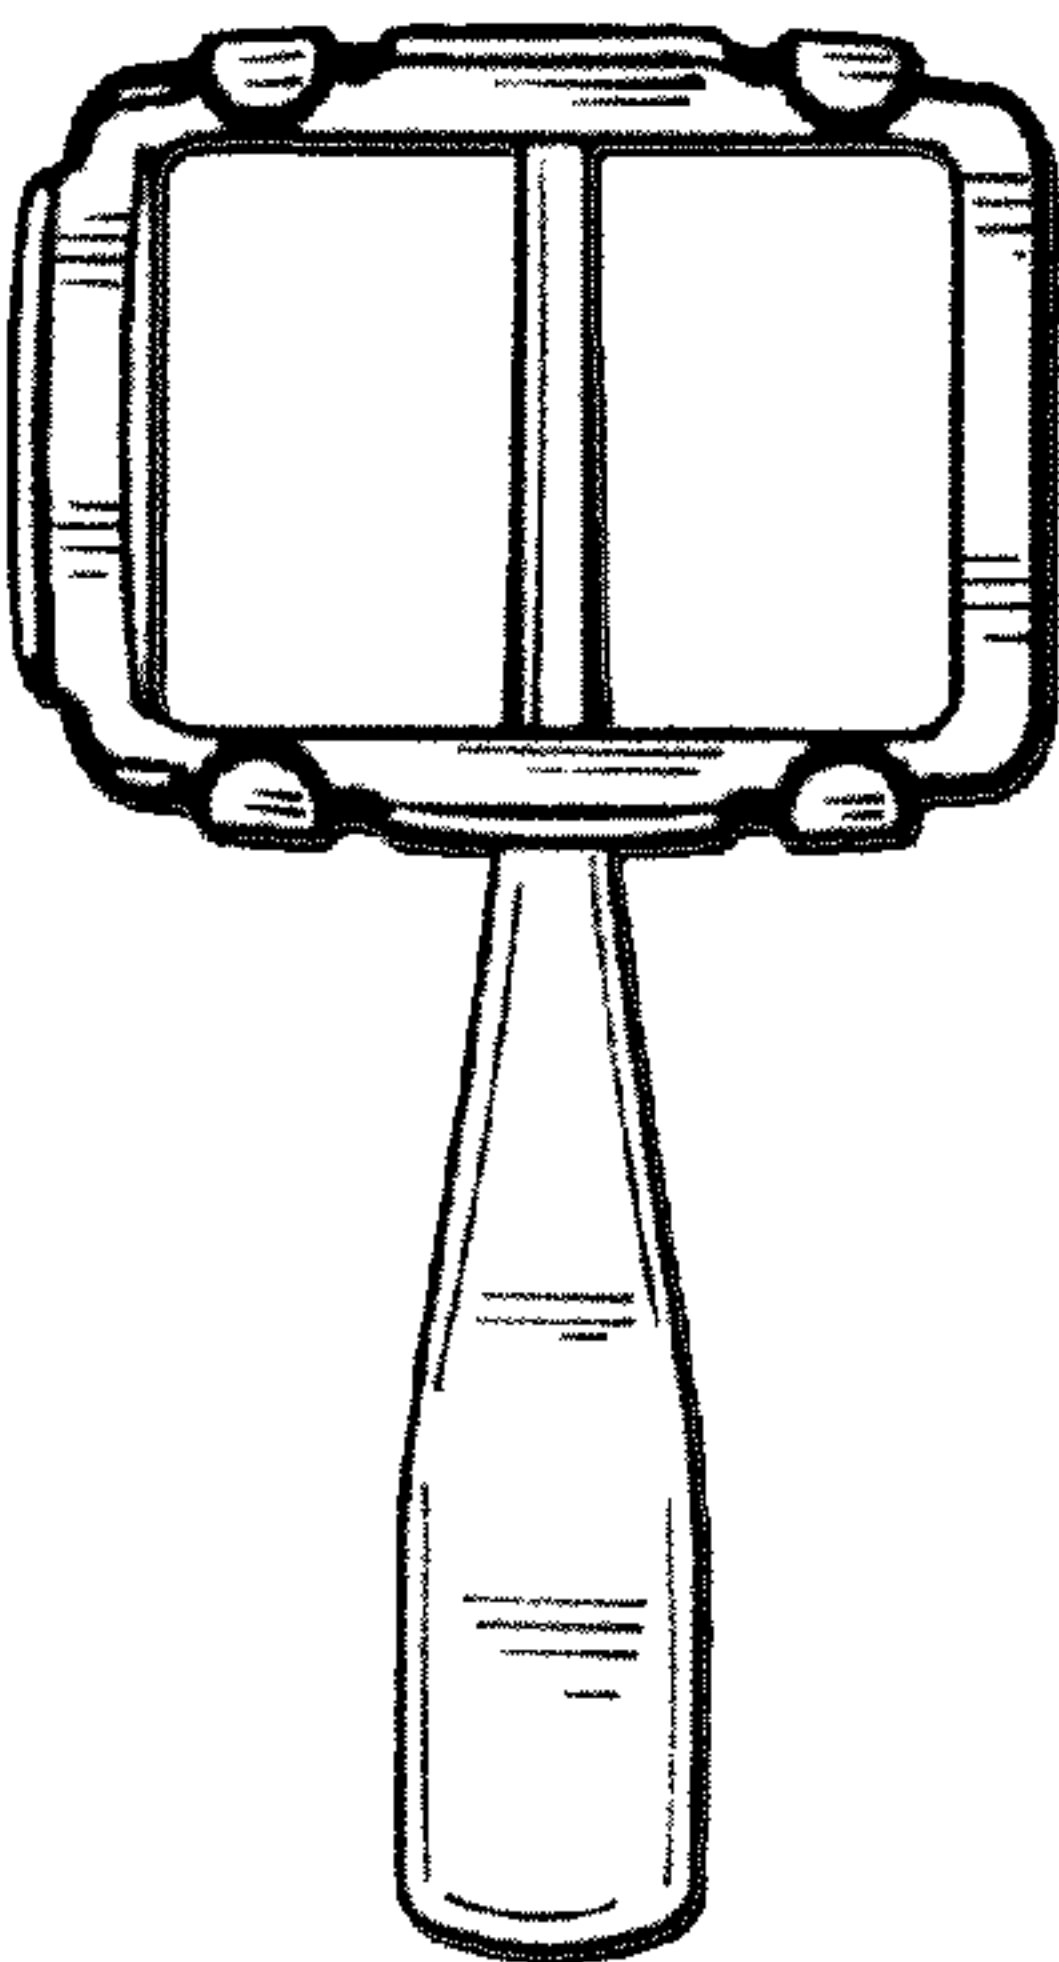


Fig. 3

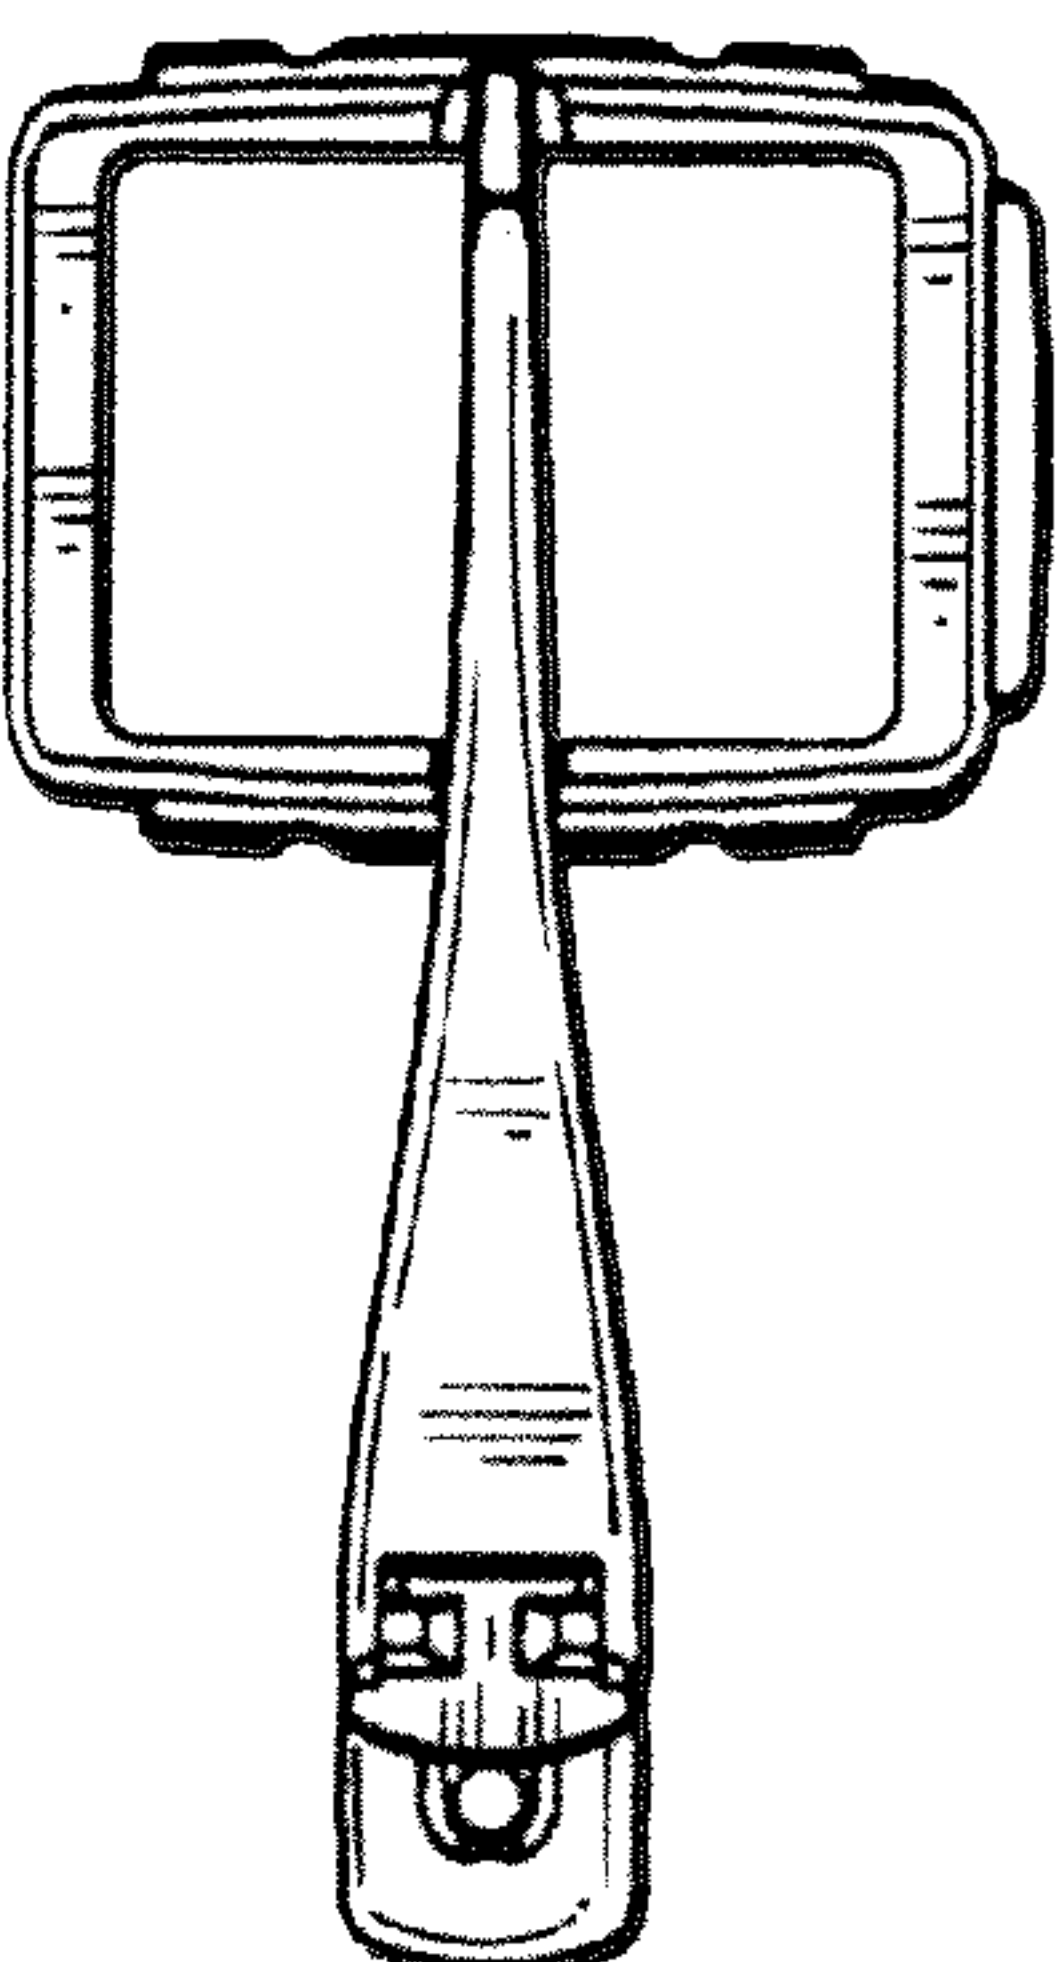


Fig. 4

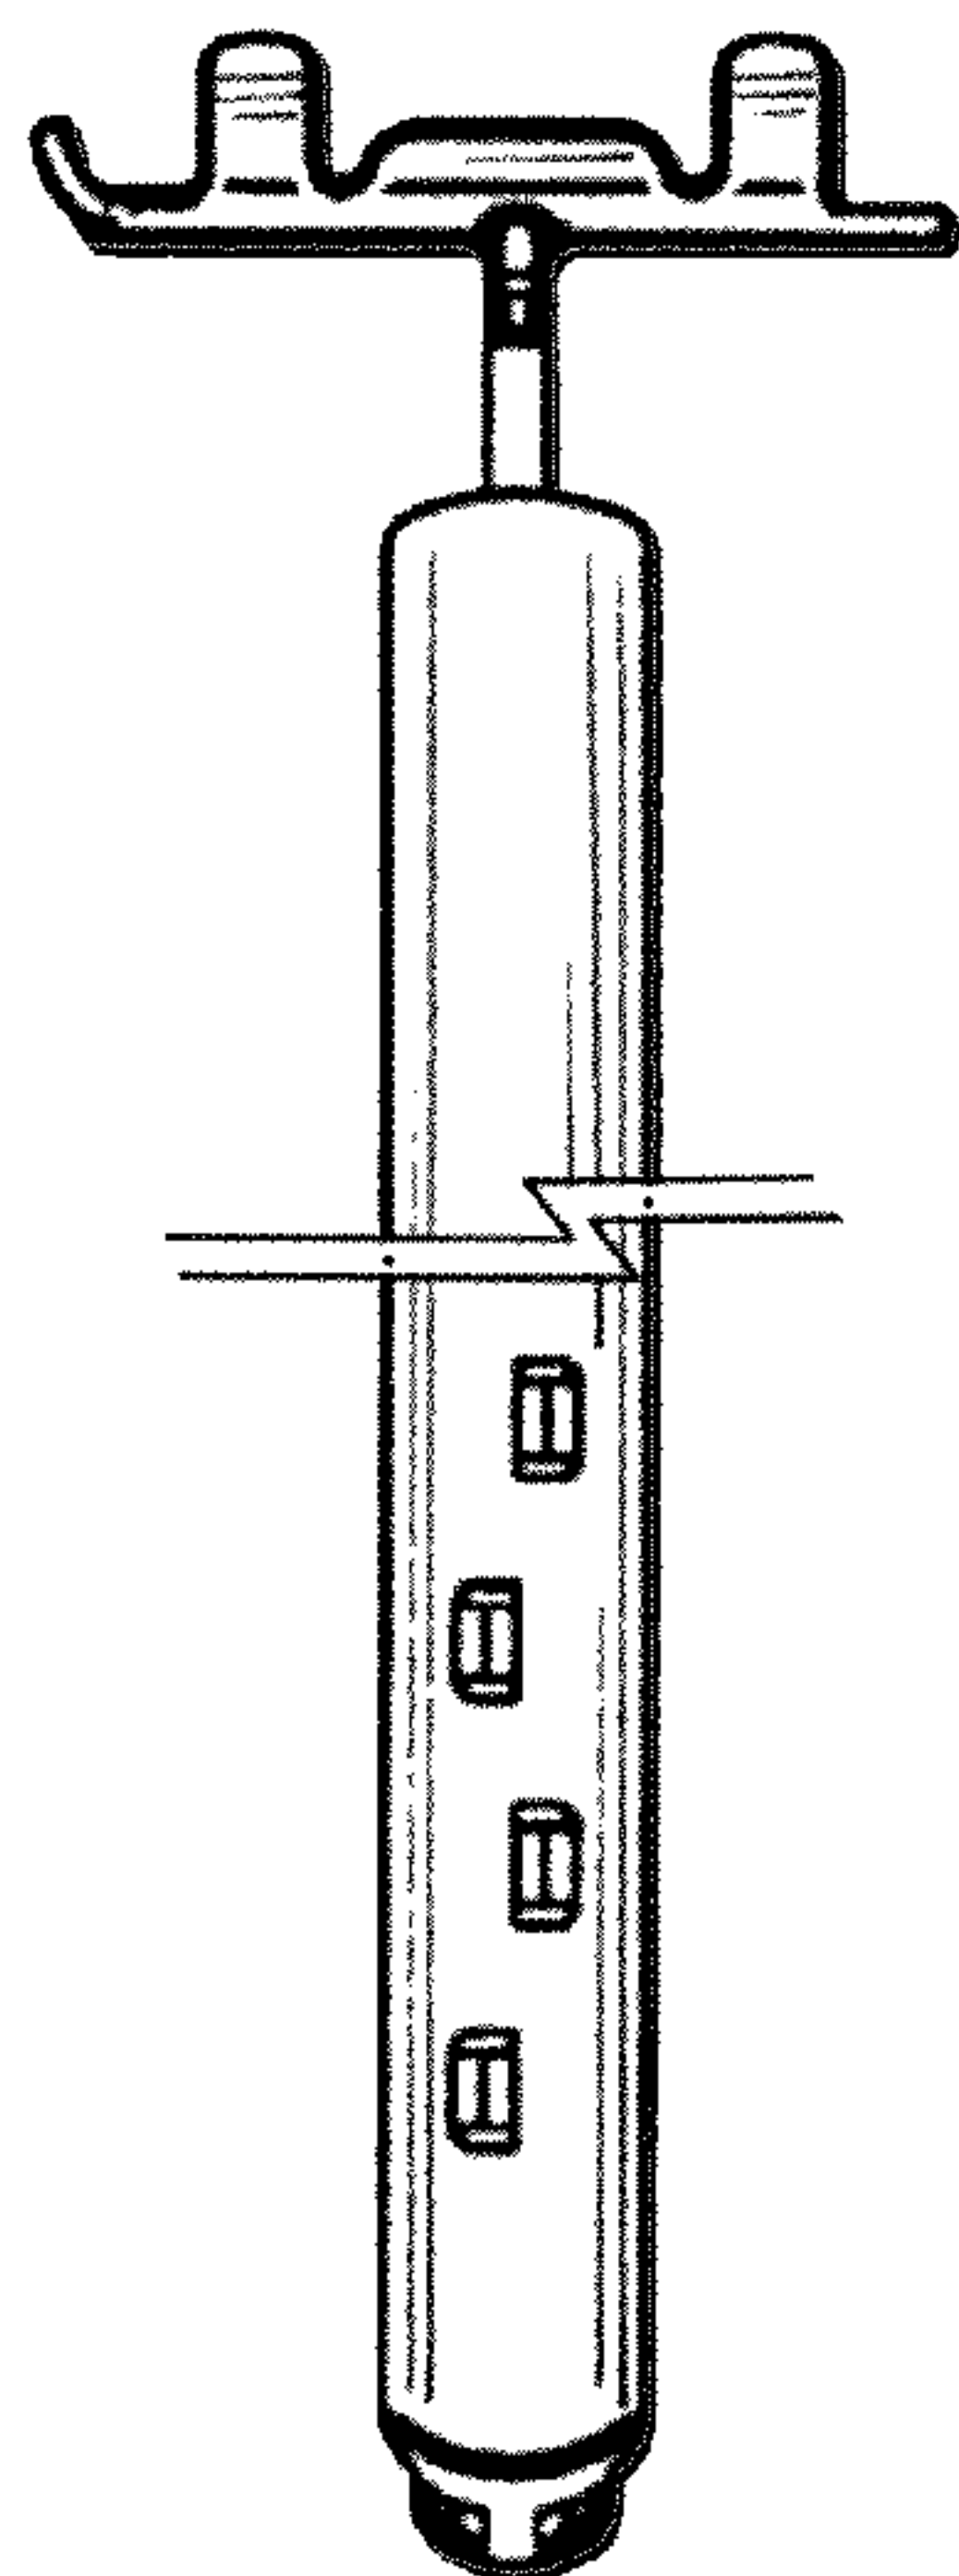


Fig. 5

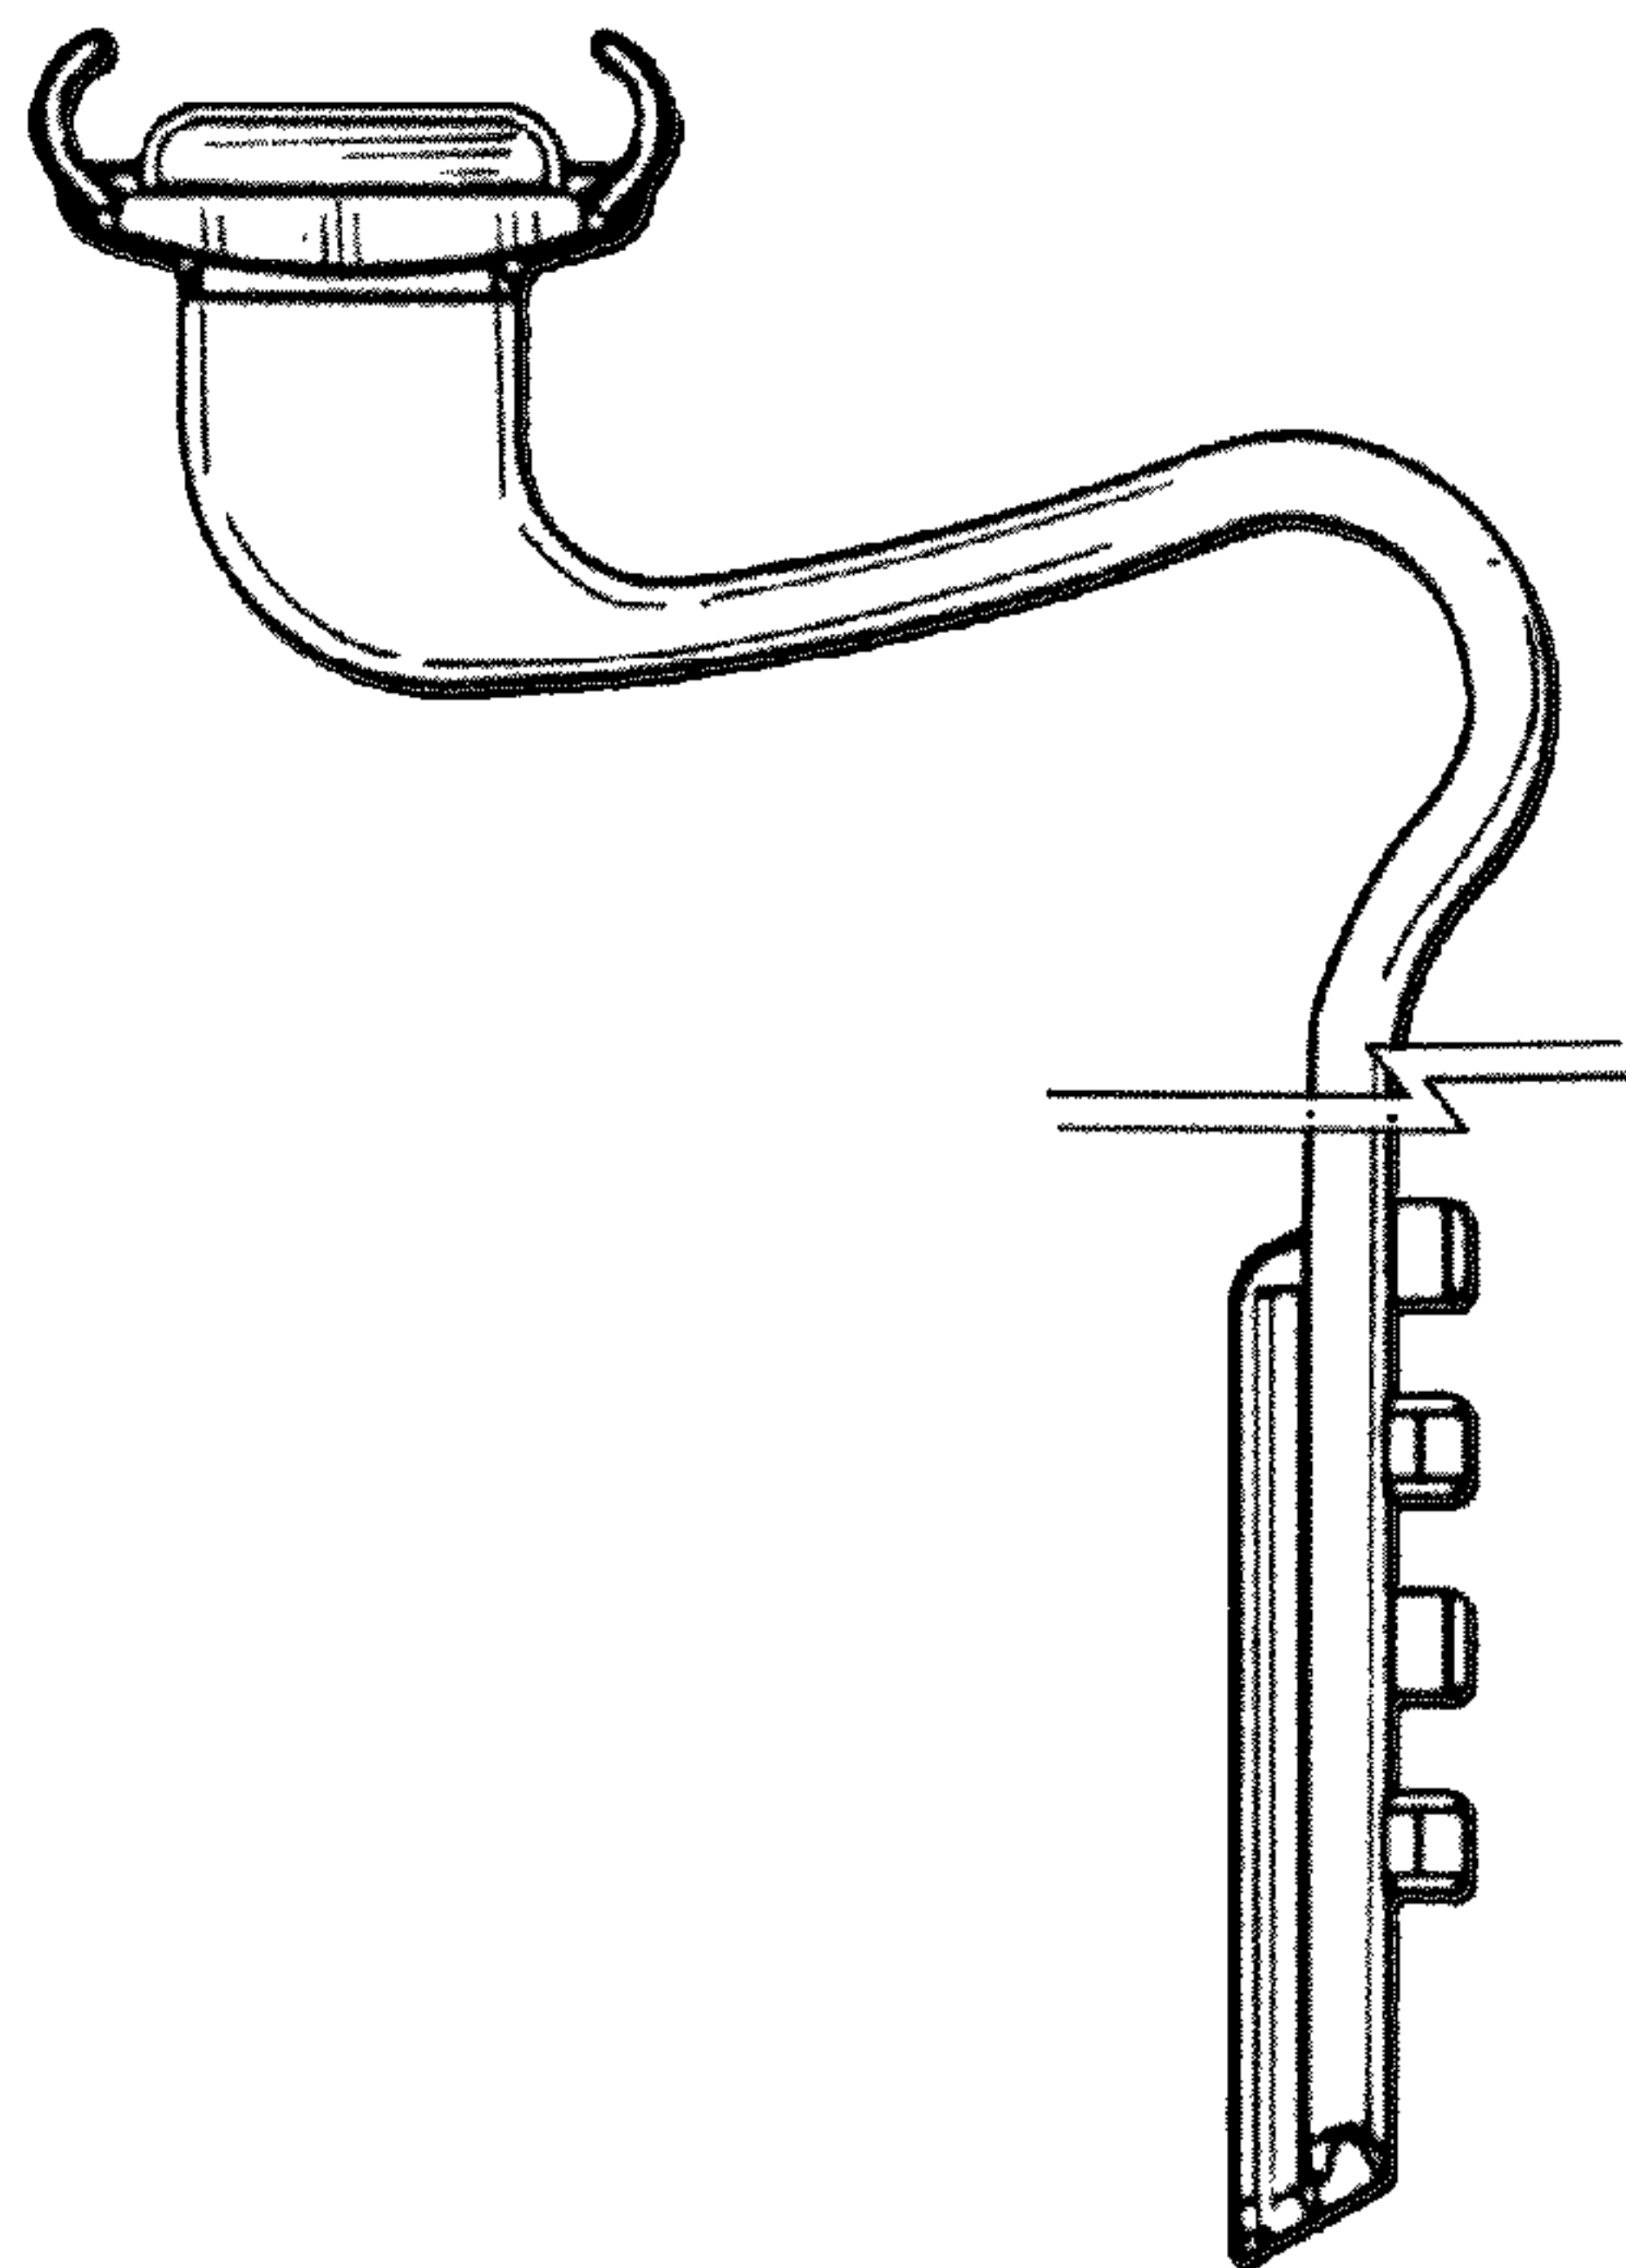


Fig. 6

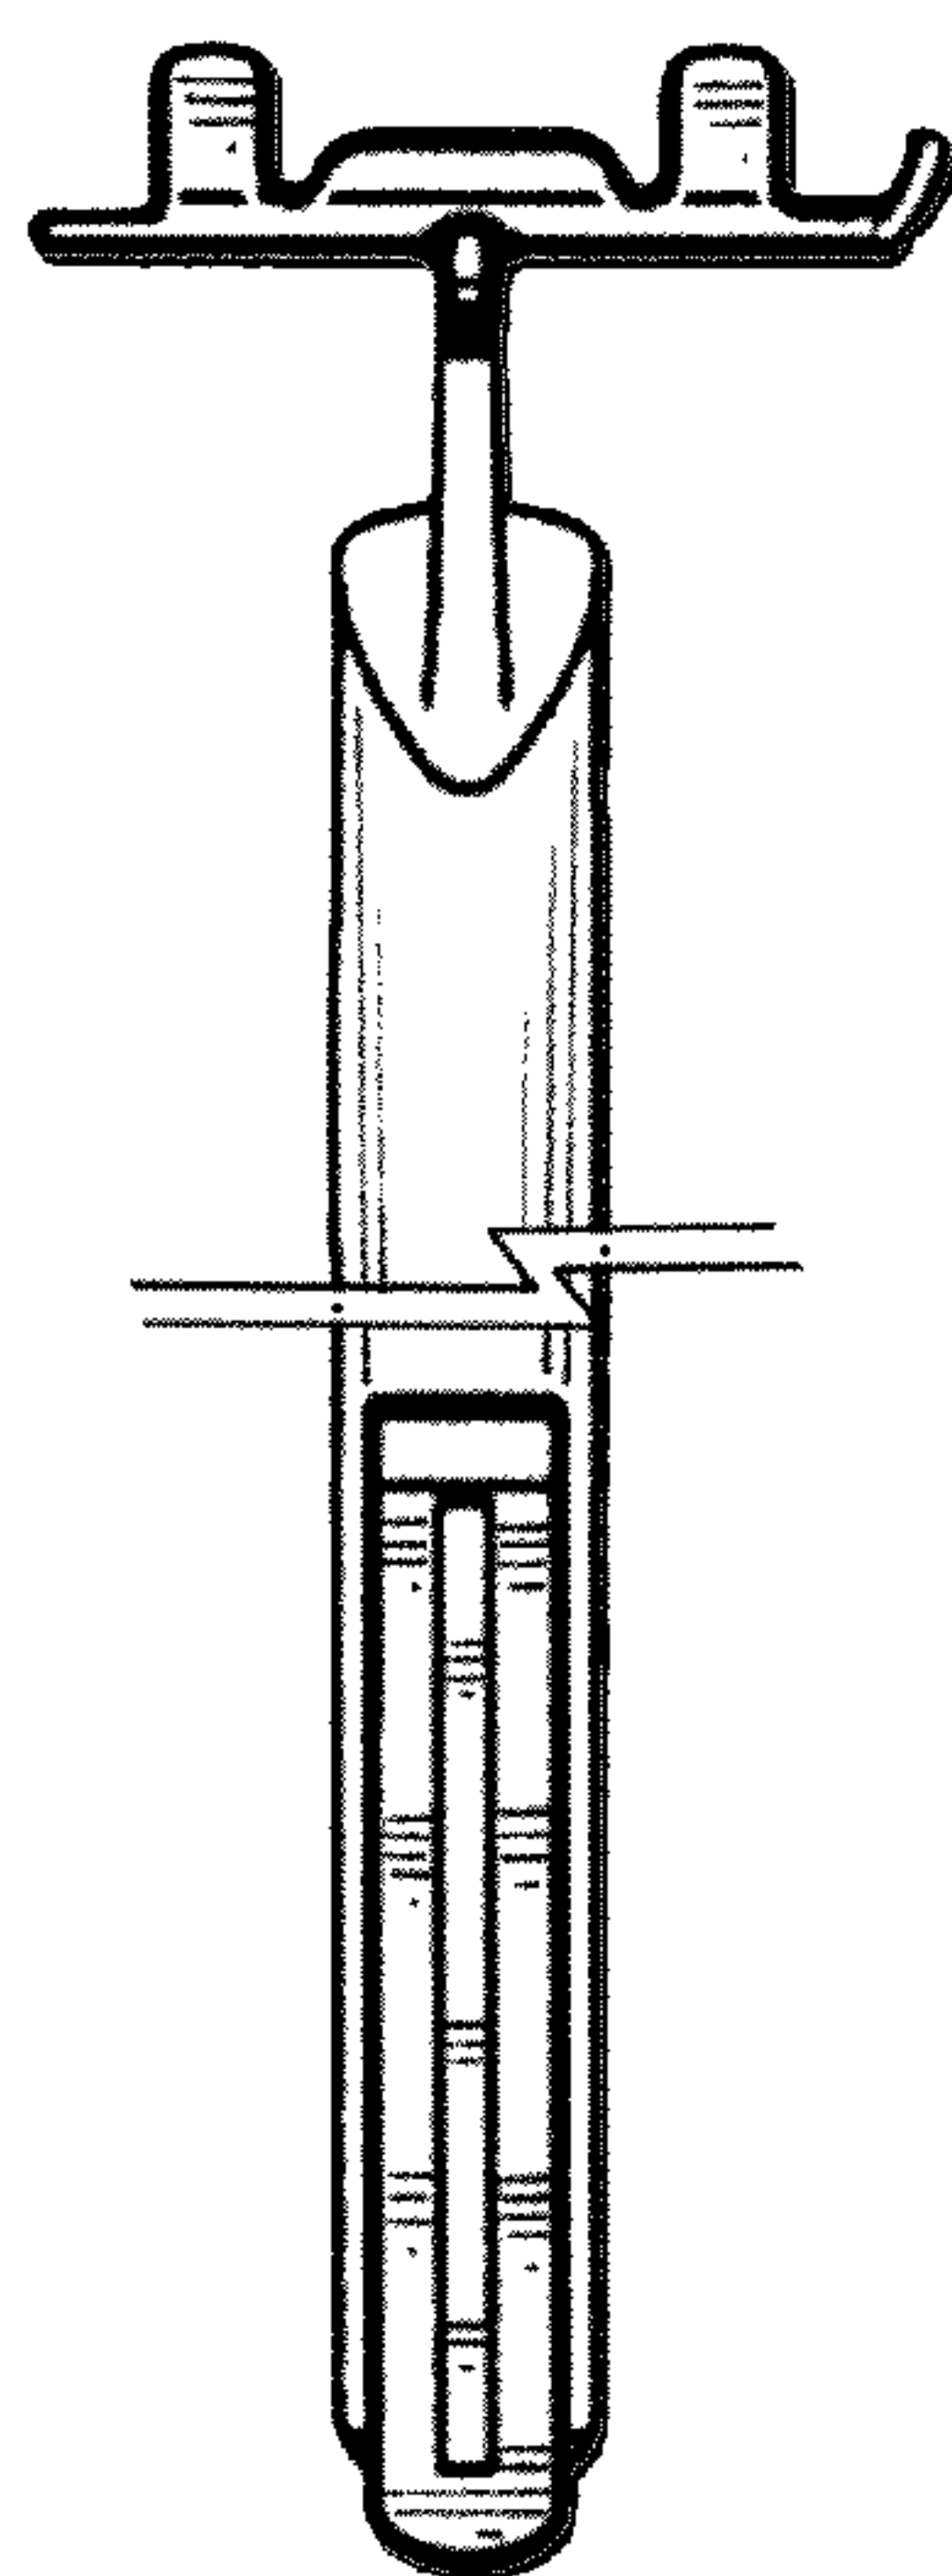


Fig. 7

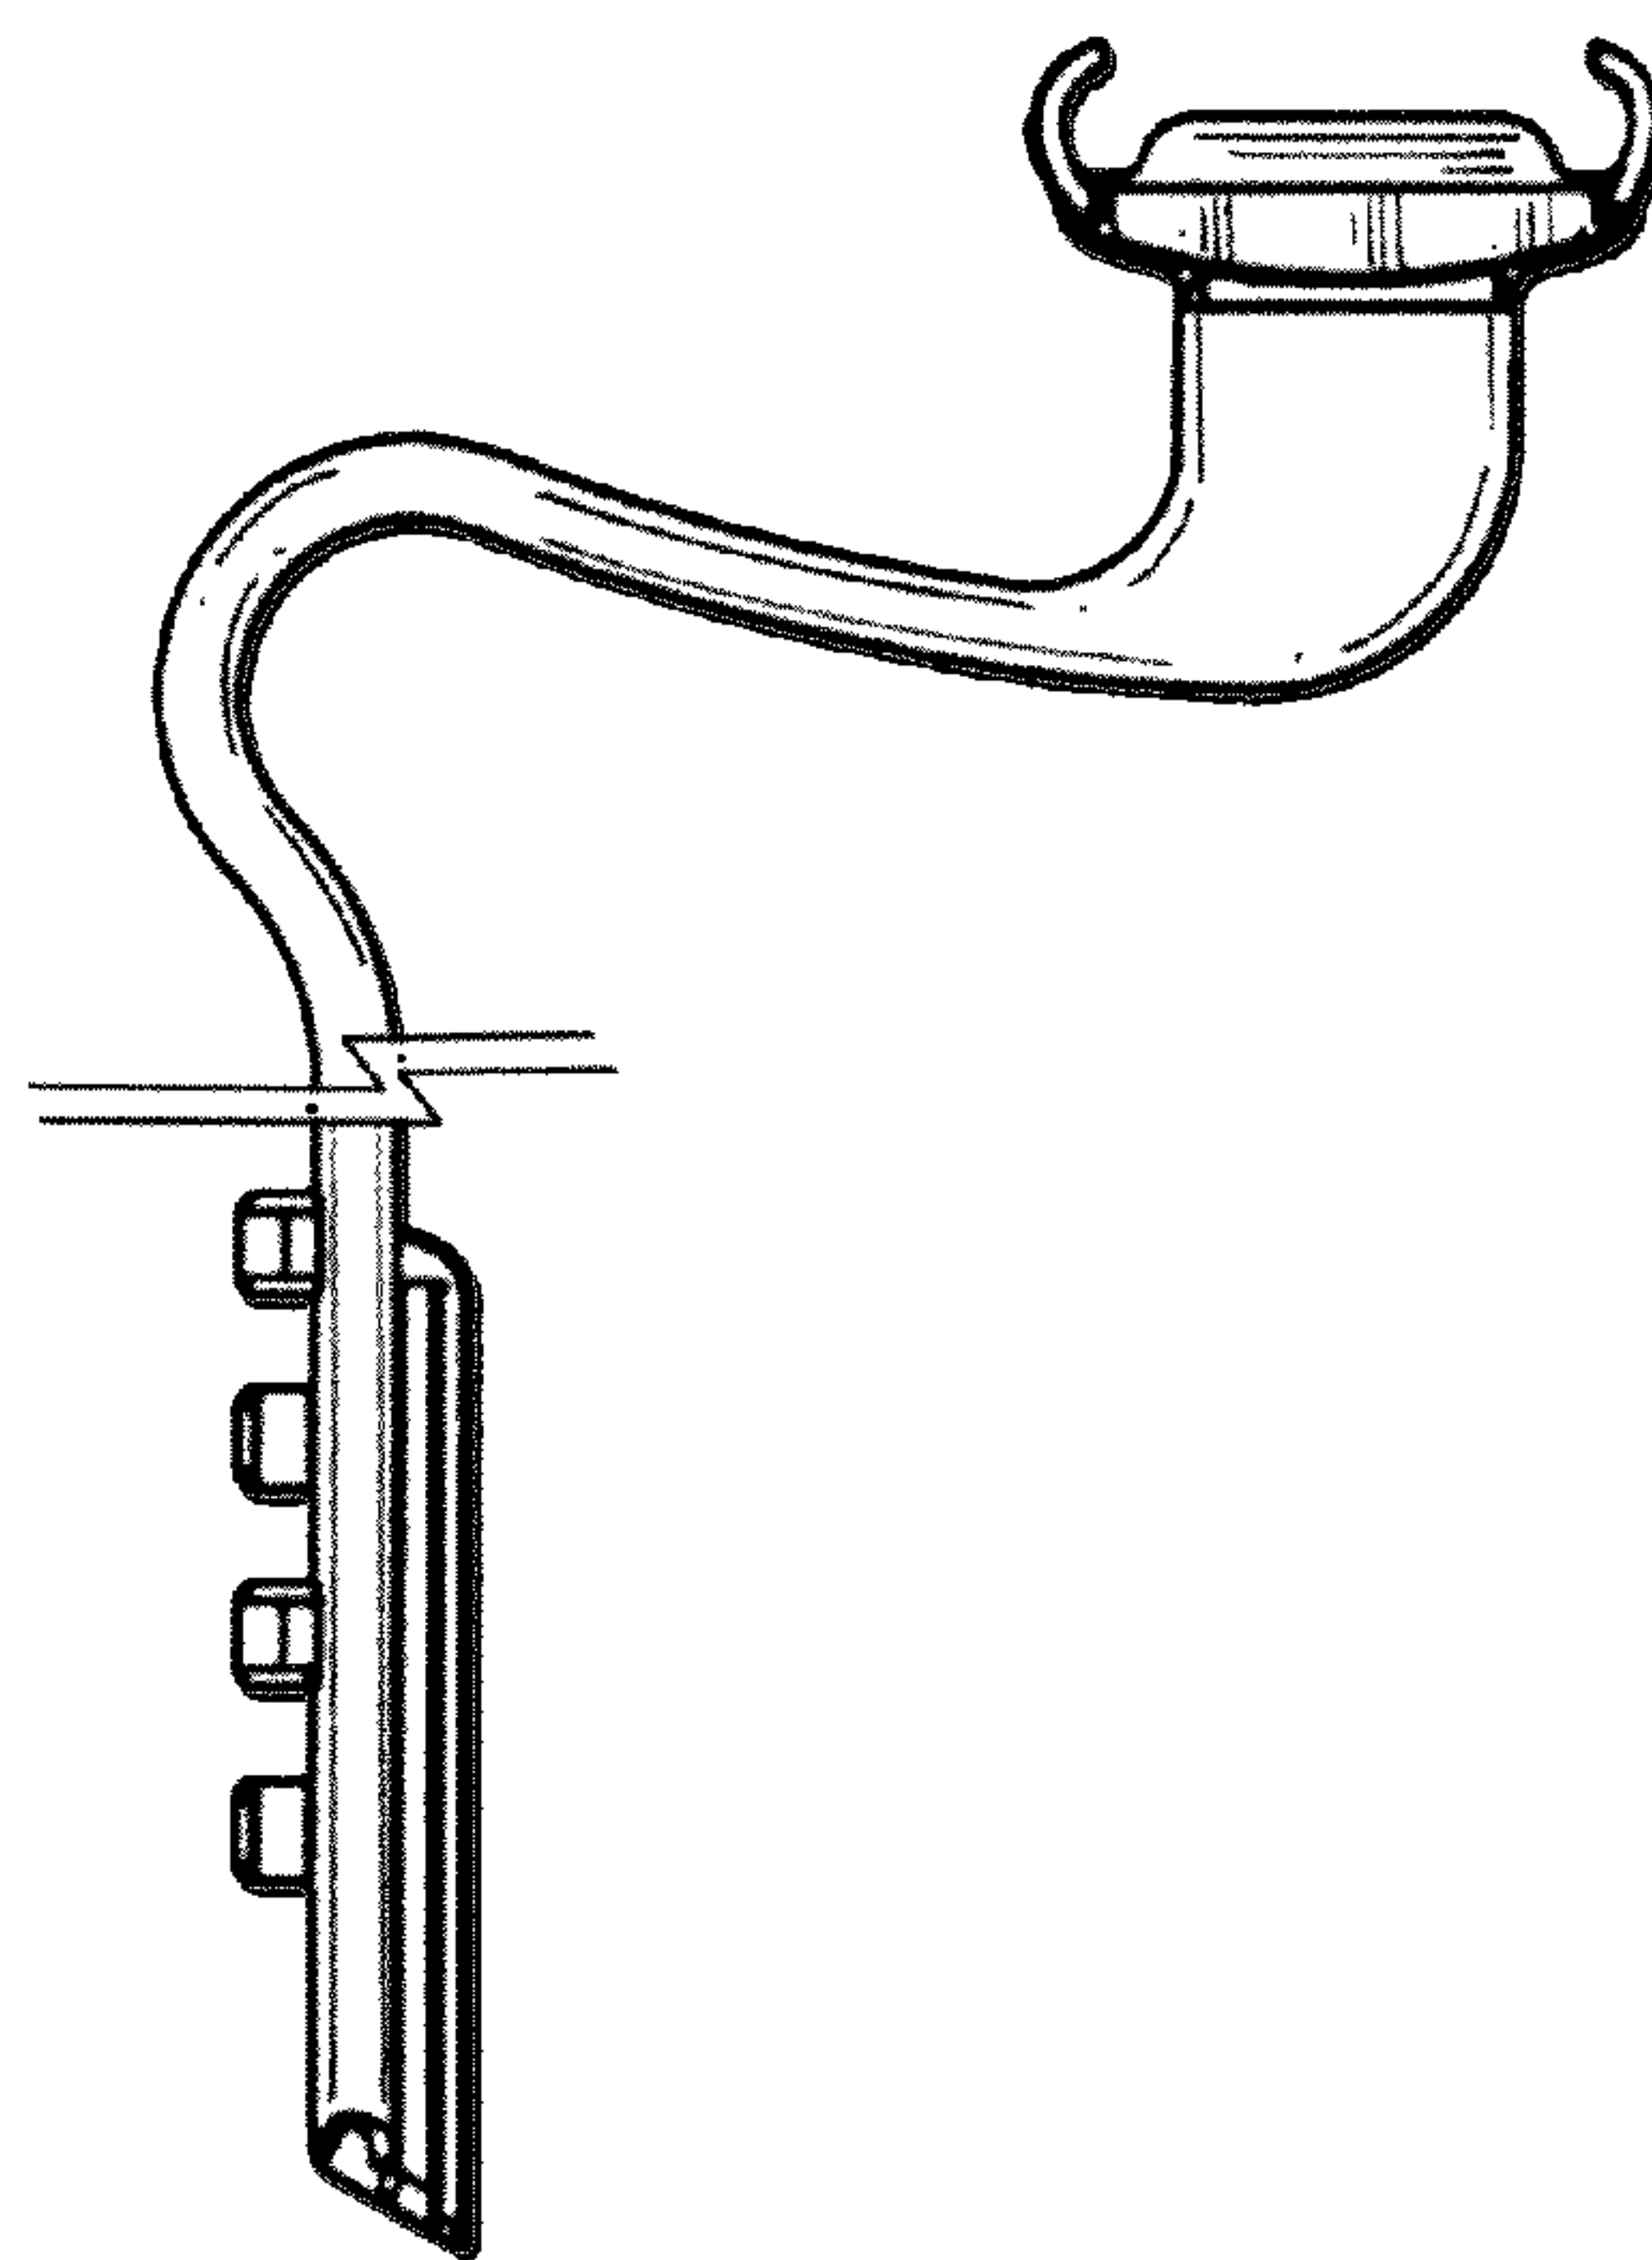


Fig. 8