



US00D713528S

(12) **United States Design Patent**  
**Li et al.**

(10) **Patent No.:** **US D713,528 S**  
(45) **Date of Patent:** **\*\* Sep. 16, 2014**

(54) **EXPOSURE SWITCH FOR X-RAY IMAGING SYSTEM**

(71) Applicant: **GE Medical Systems Global Technology Company, LLC**, Waukesha, WI (US)

(72) Inventors: **Jundong Li**, Beijing (CN); **Tianhui Wang**, Beijing (CN); **Yigang Xia**, Beijing (CN)

(73) Assignee: **Ge Medical Systems Global Technology Company, LLC**, Waukesha, WI (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/446,807**

(22) Filed: **Feb. 27, 2013**

(30) **Foreign Application Priority Data**

Aug. 28, 2012 (CN) ..... 2012 3 0409295

(51) **LOC (10) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/158**

(58) **Field of Classification Search**  
USPC ..... D24/158-161, 185, 186; 378/4, 21-27, 378/38, 40, 102, 196-198; D13/168, 171; D14/412; 200/6 A, 61.85, 293.1, 200/332.22, 505

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D300,023	S	*	2/1989	DeRamus, Jr.	.....	D13/171
D550,359	S	*	9/2007	Ogiwara	.....	D24/158
D589,464	S	*	3/2009	Ozoe	.....	D13/171
D606,947	S	*	12/2009	Caprio et al.	.....	D13/168
D683,022	S	*	5/2013	Moon et al.	.....	D24/158
D695,405	S	*	12/2013	Moon et al.	.....	D24/158

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Global Patent Operation; Marc A. Vivencio


(57) **CLAIM**

The ornamental design for an exposure switch for x-ray imaging system, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of an exposure switch for x-ray imaging system showing our new design; FIG. 2 is a front view of the exposure switch shown in FIG. 1; FIG. 3 is a rear view of the exposure switch shown in FIG. 1; FIG. 4 is a left side view of the exposure switch shown in FIG. 1; FIG. 5 is a right side view of the exposure switch shown in FIG. 1; and, FIG. 6 is a top view of the exposure switch shown in FIG. 1.

**1 Claim, 6 Drawing Sheets**

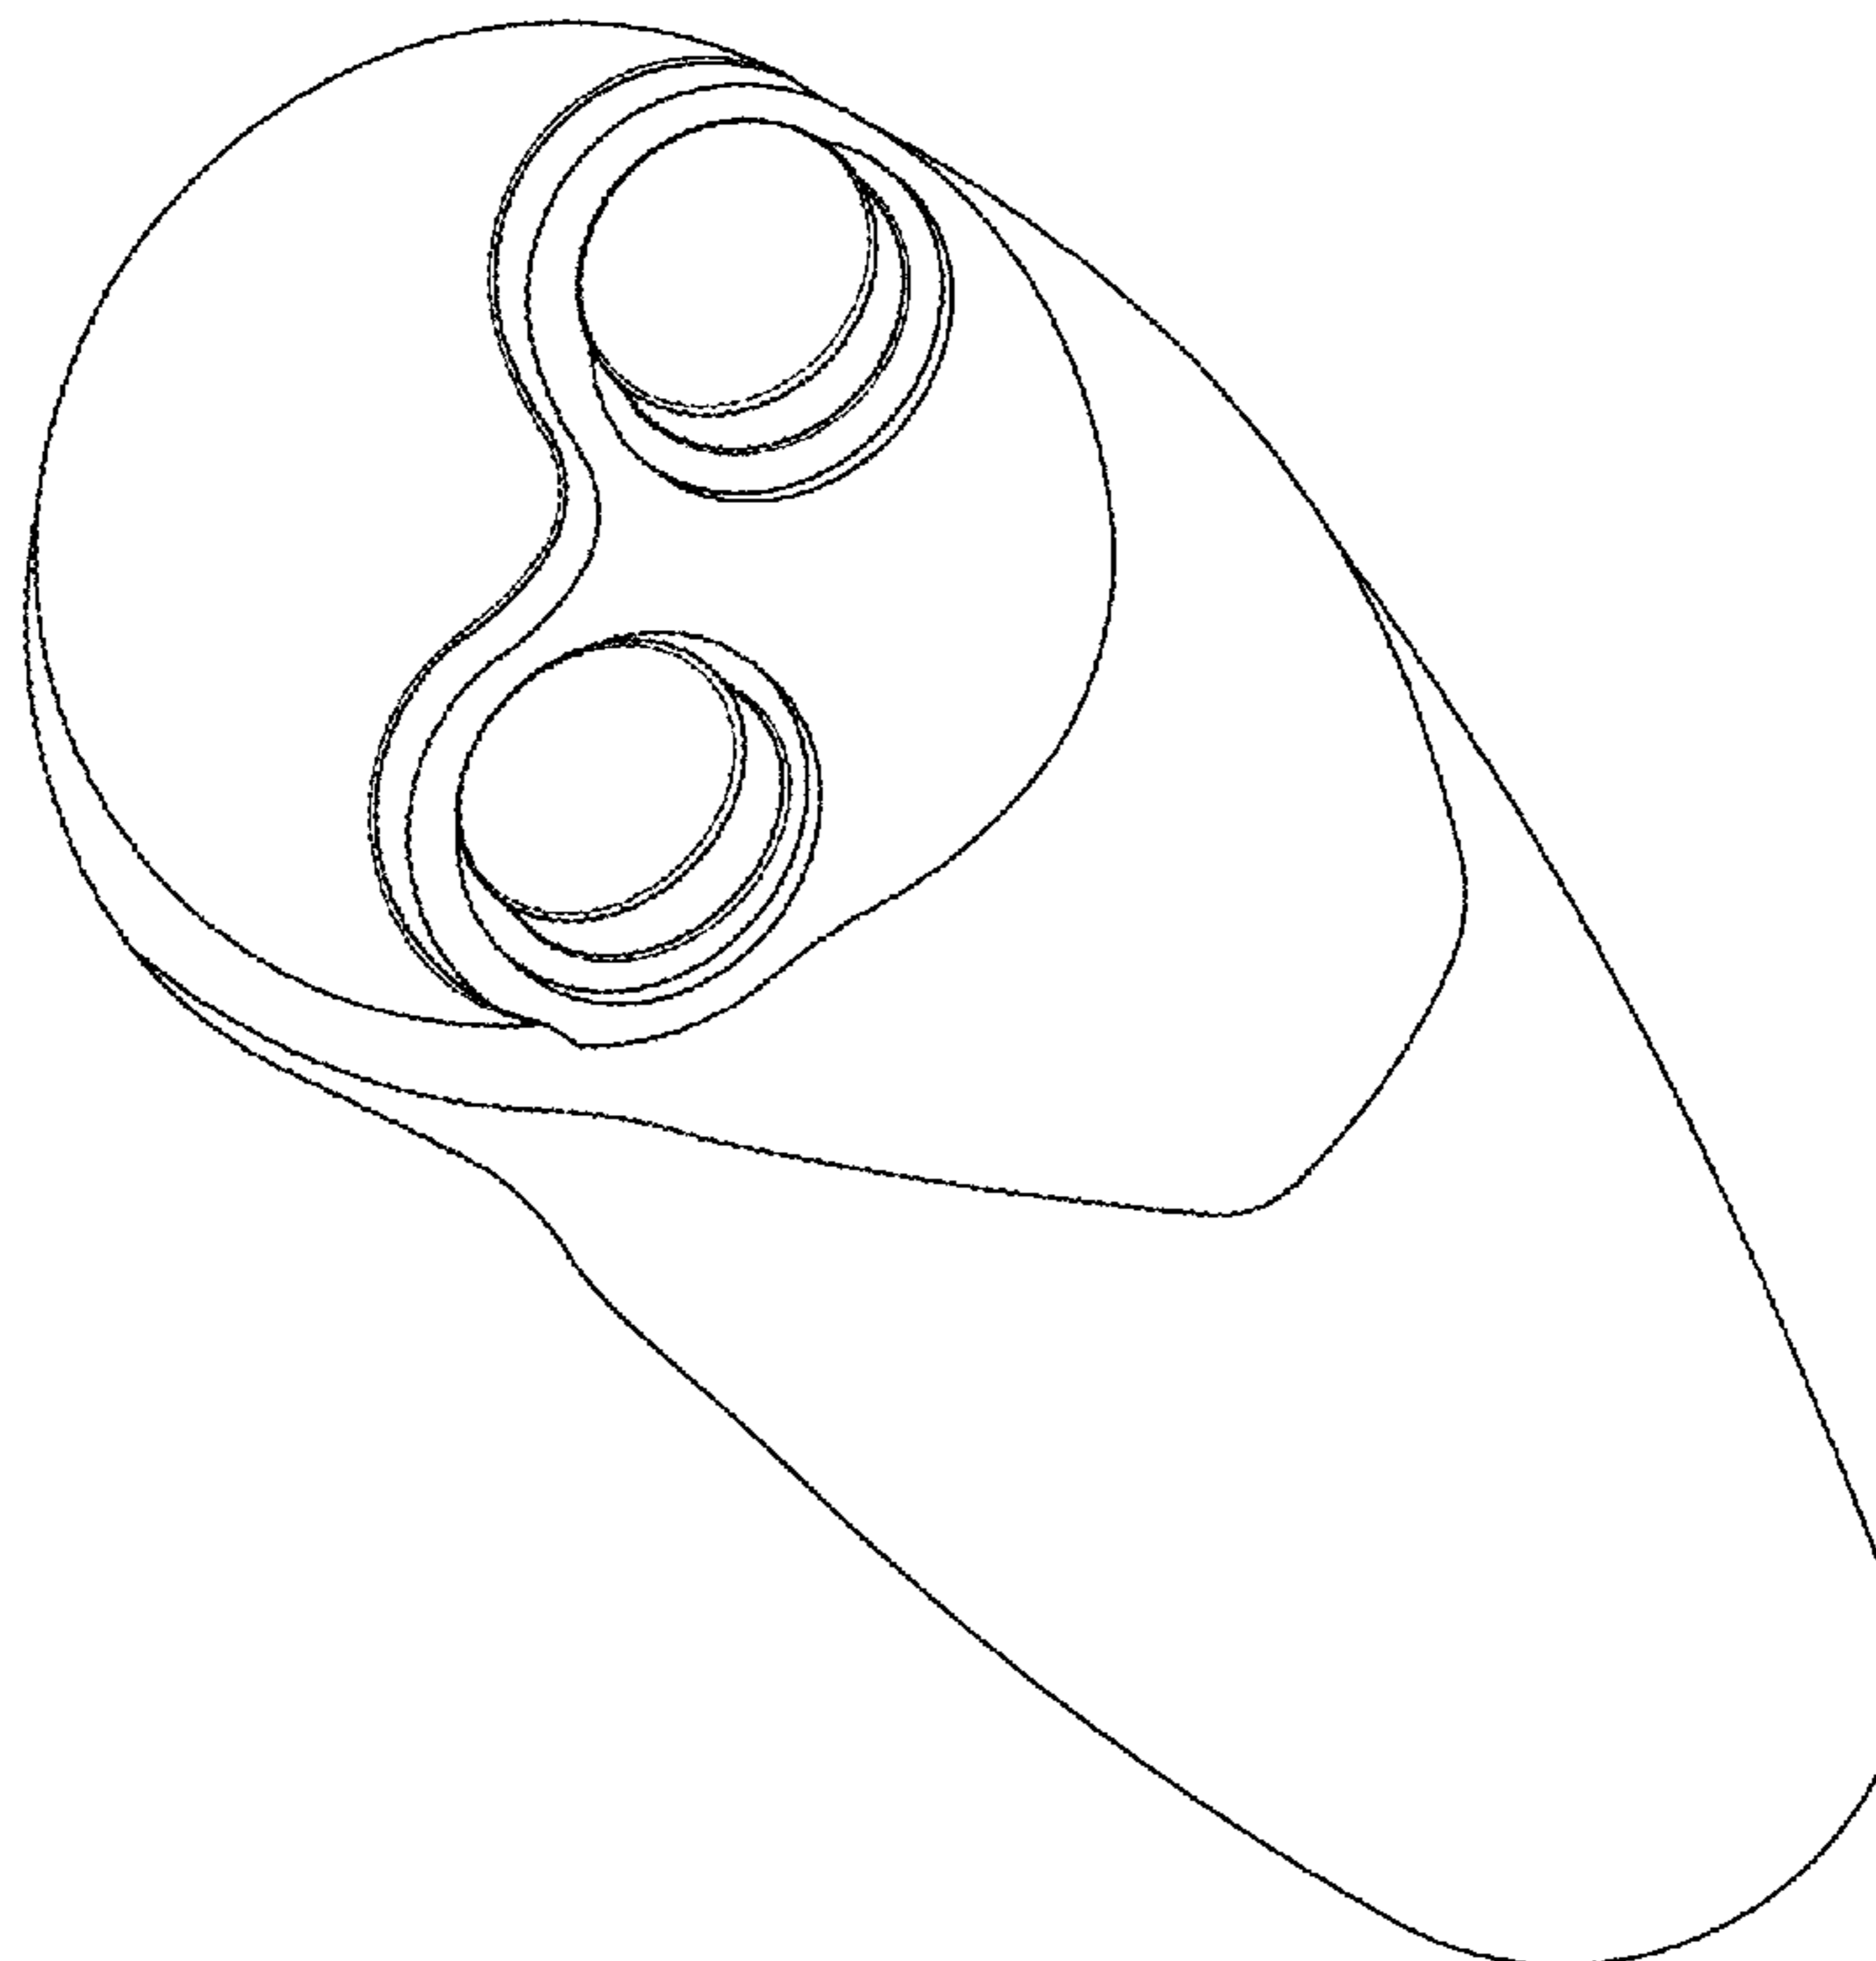

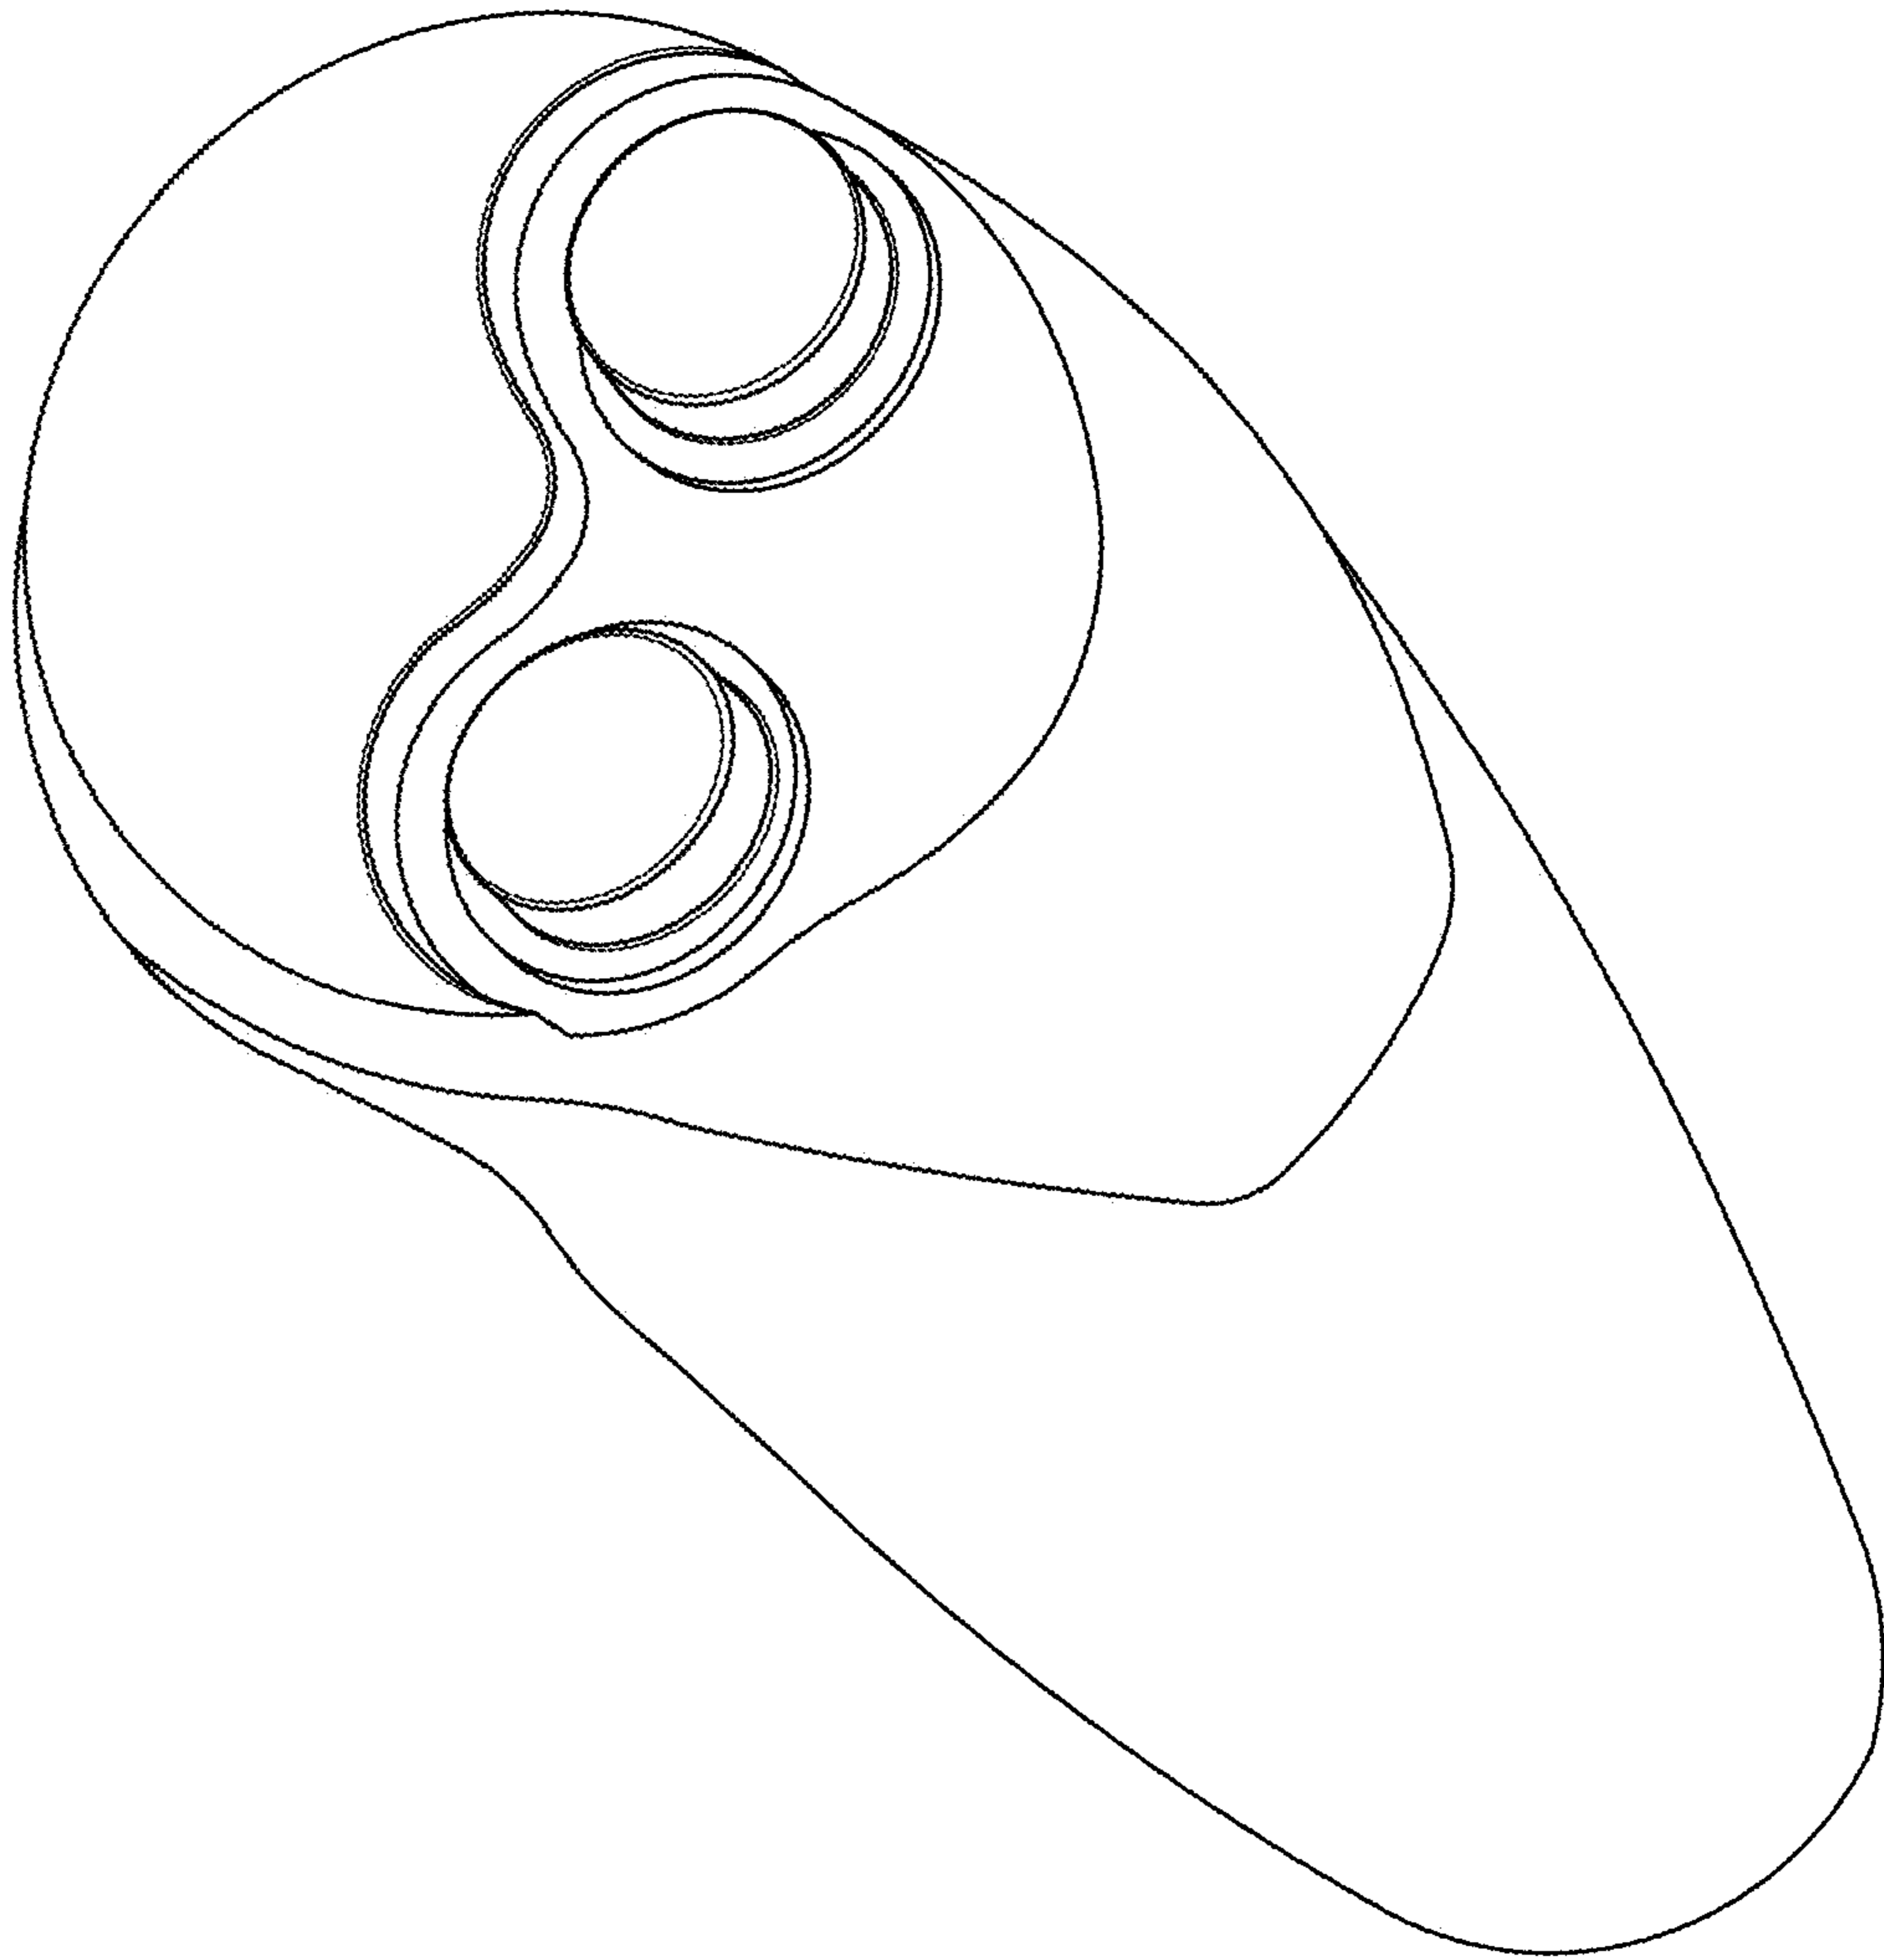


FIG. 1

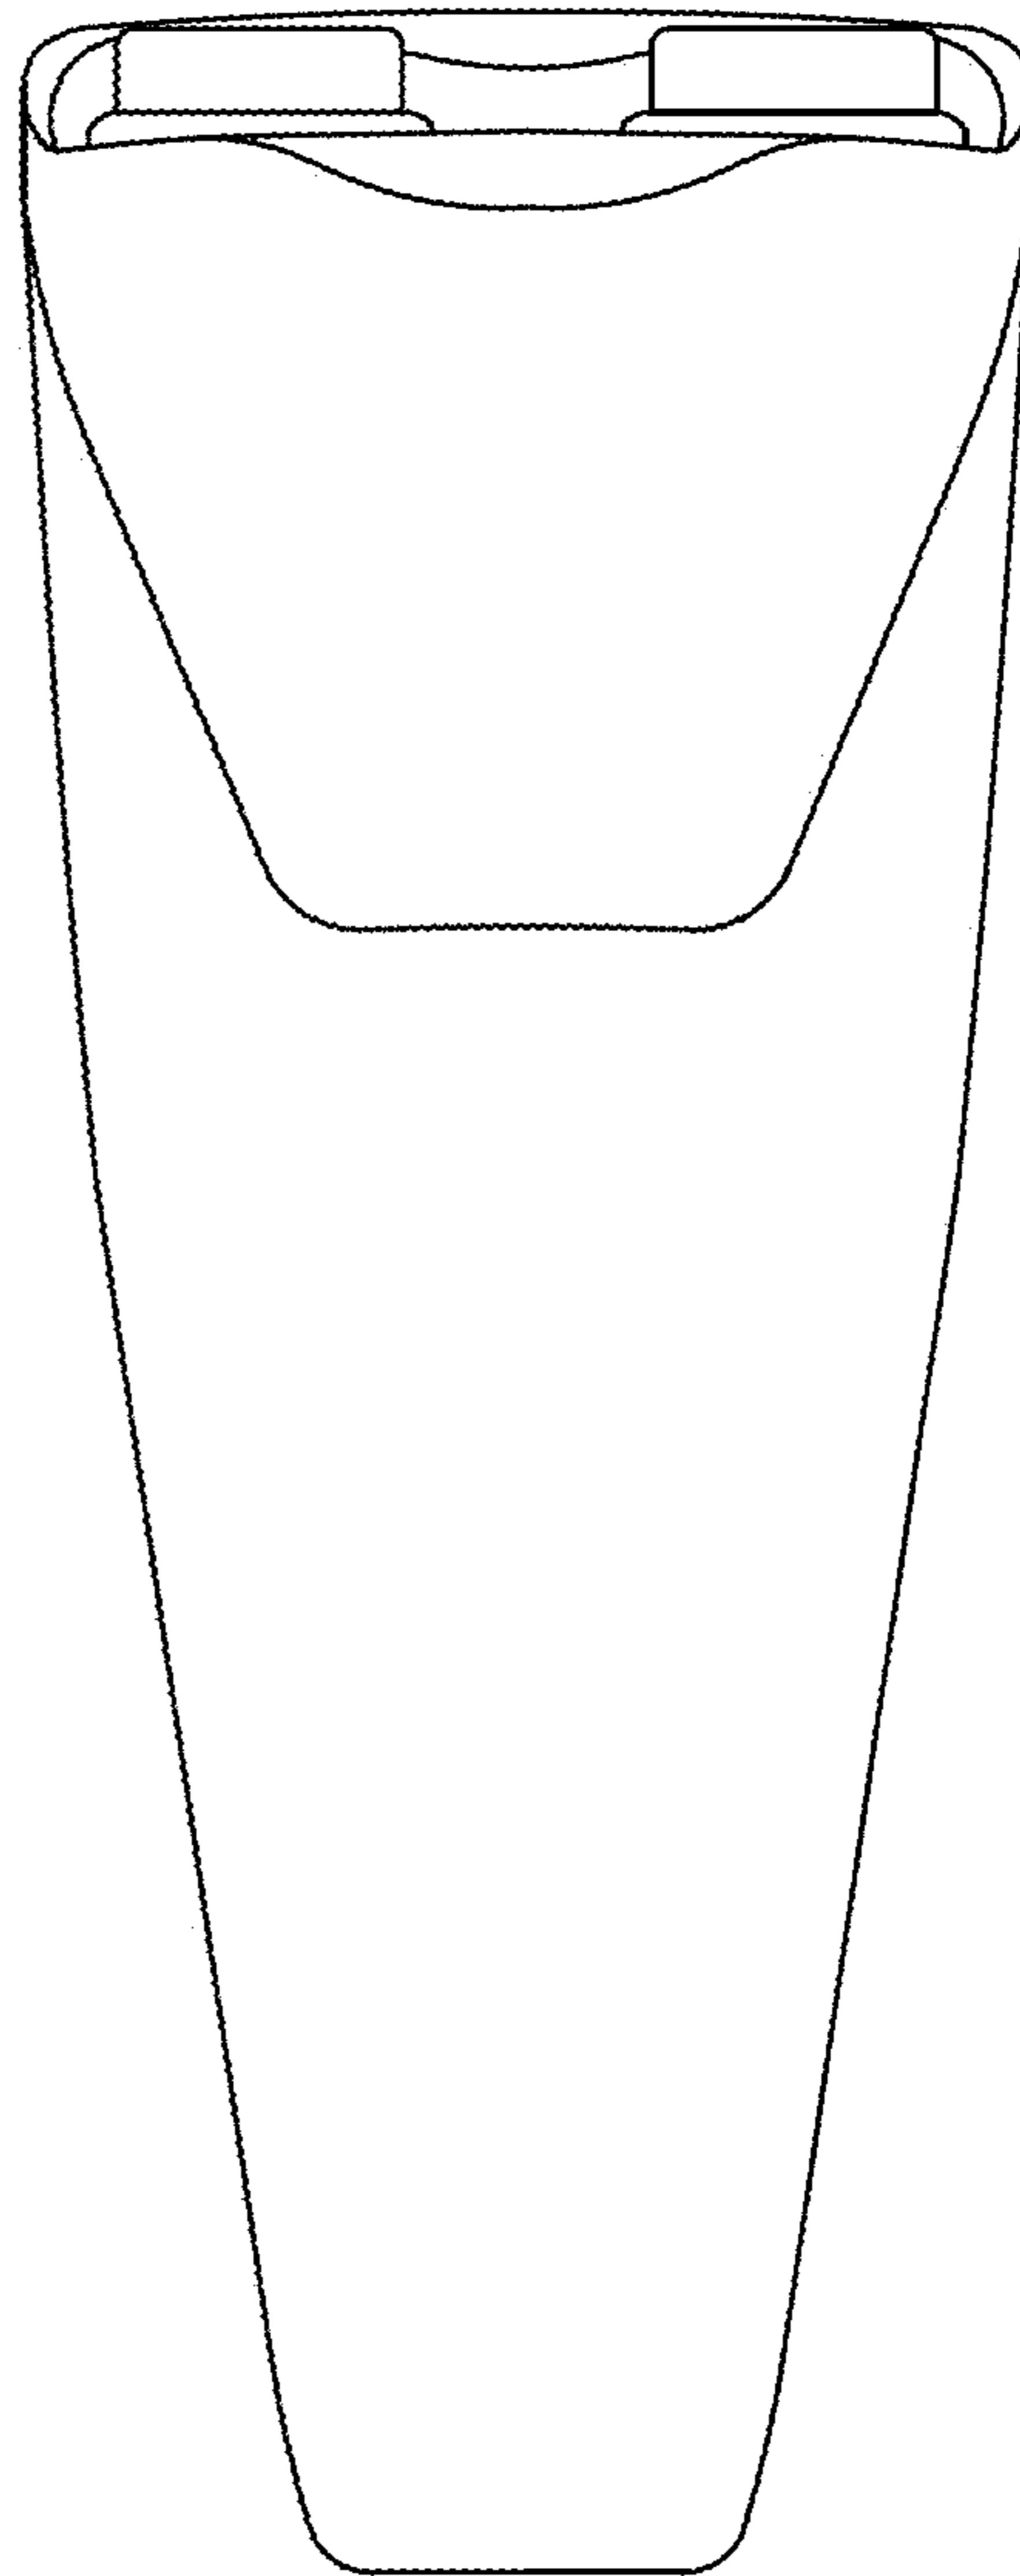


FIG. 2

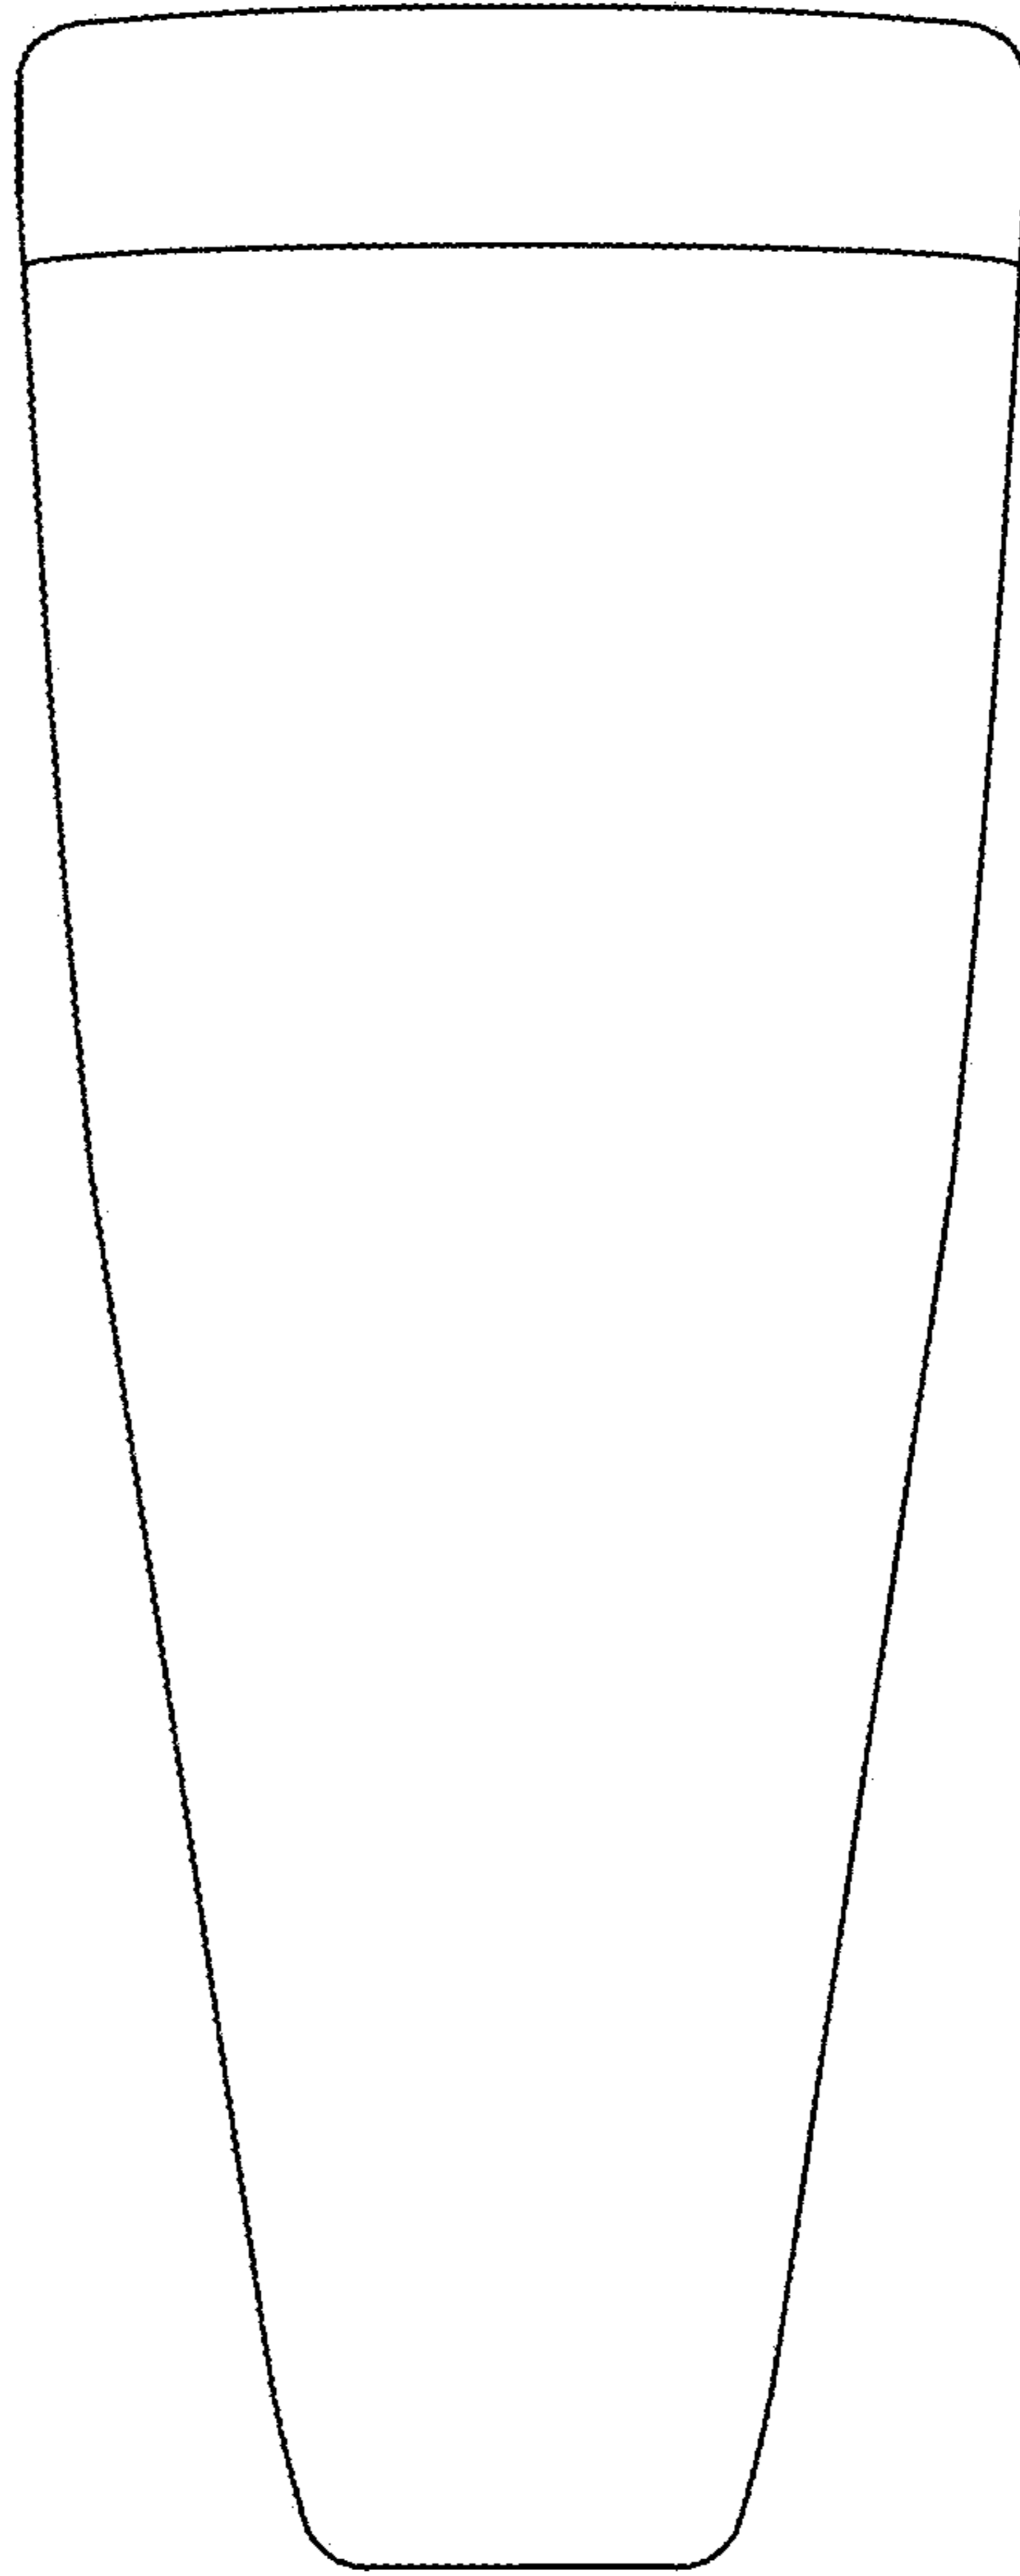


FIG. 3

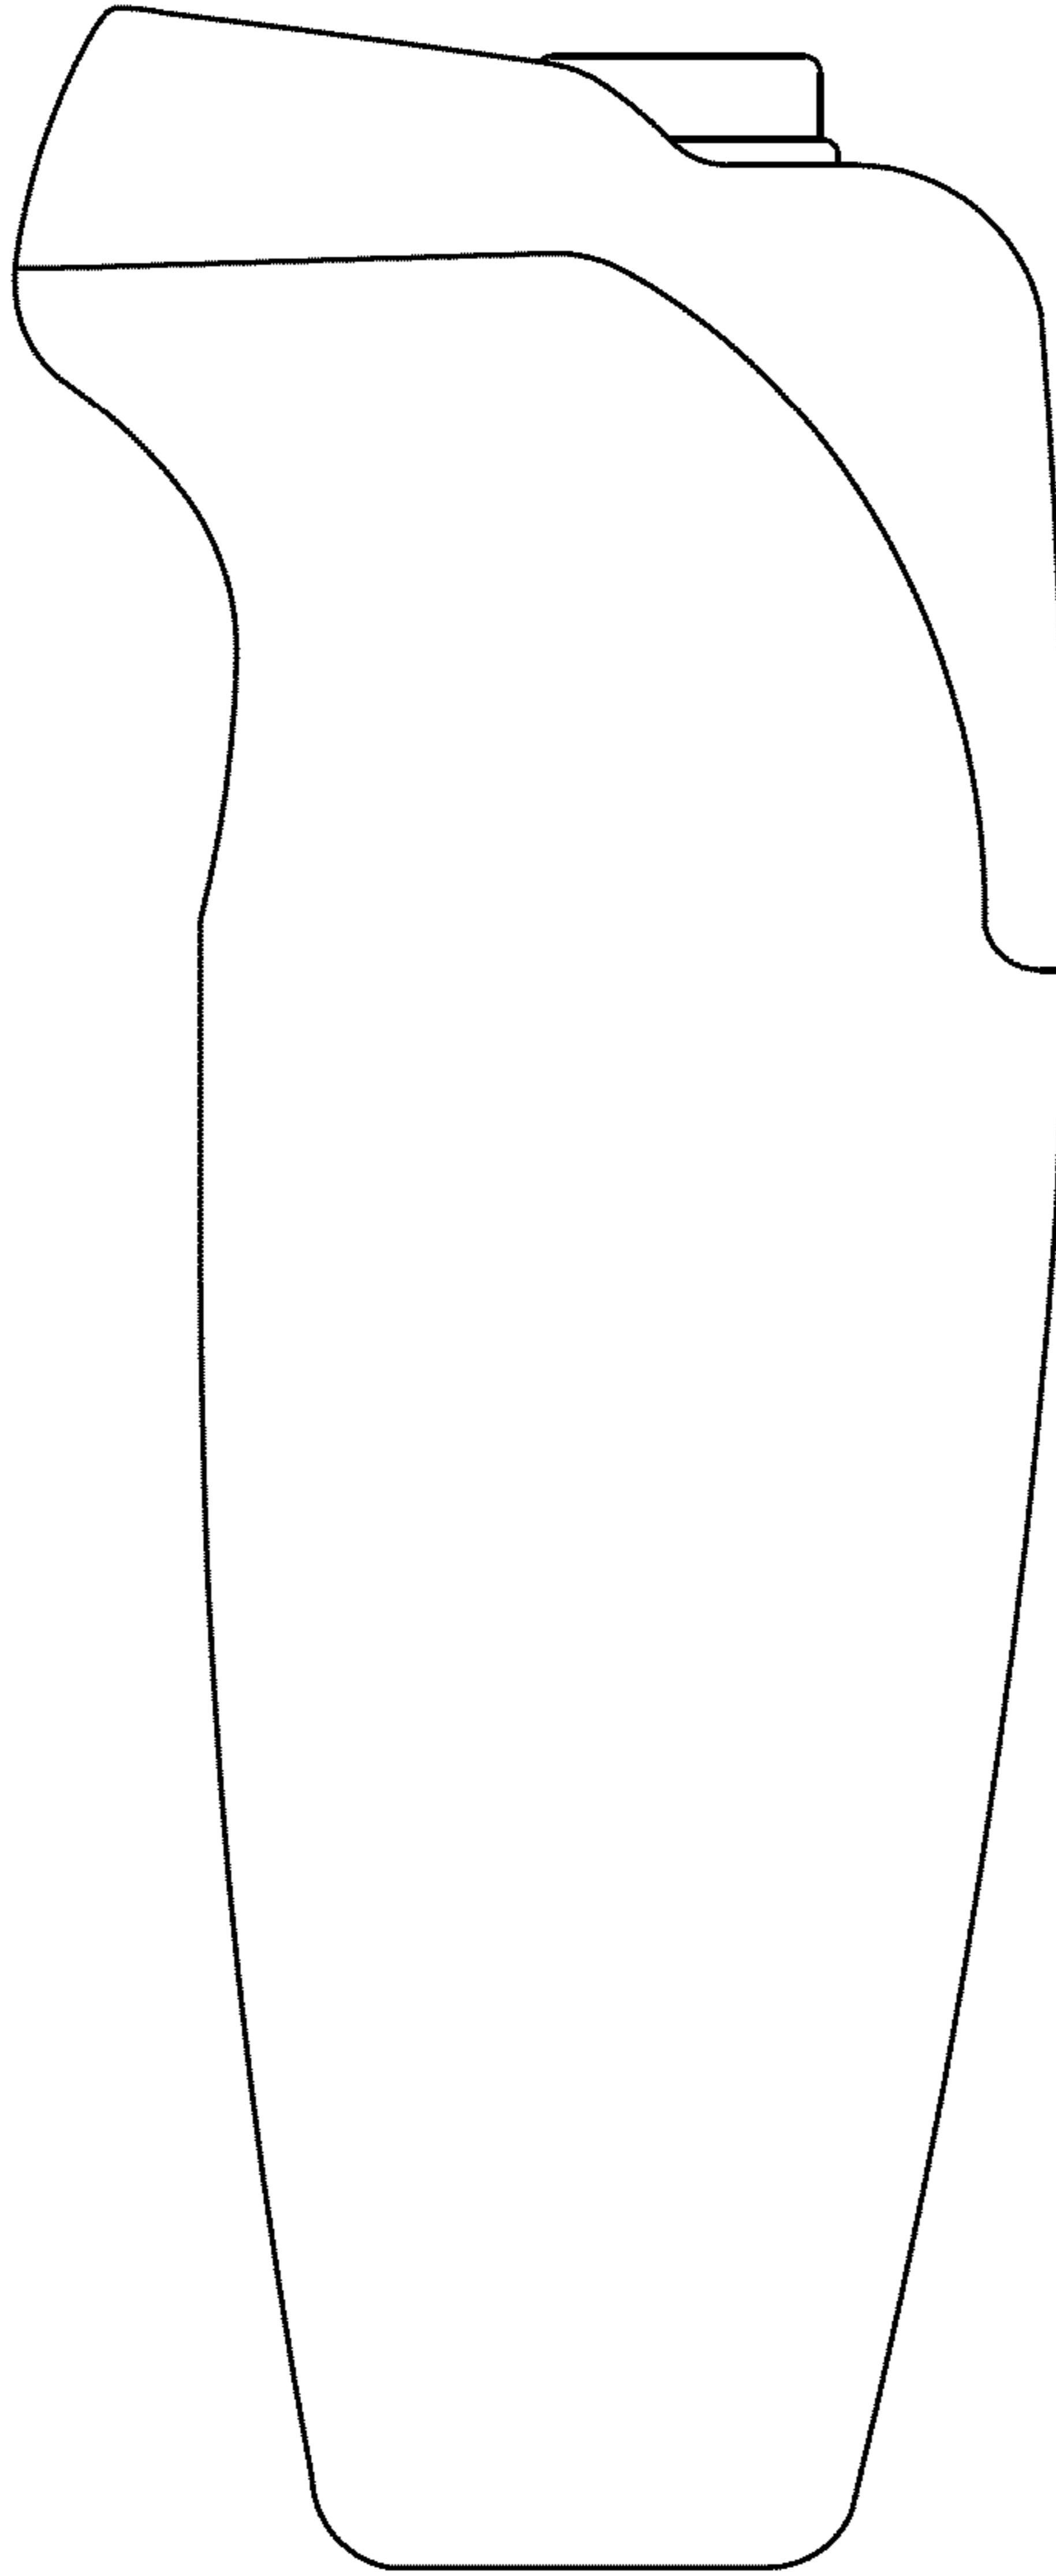


FIG. 4

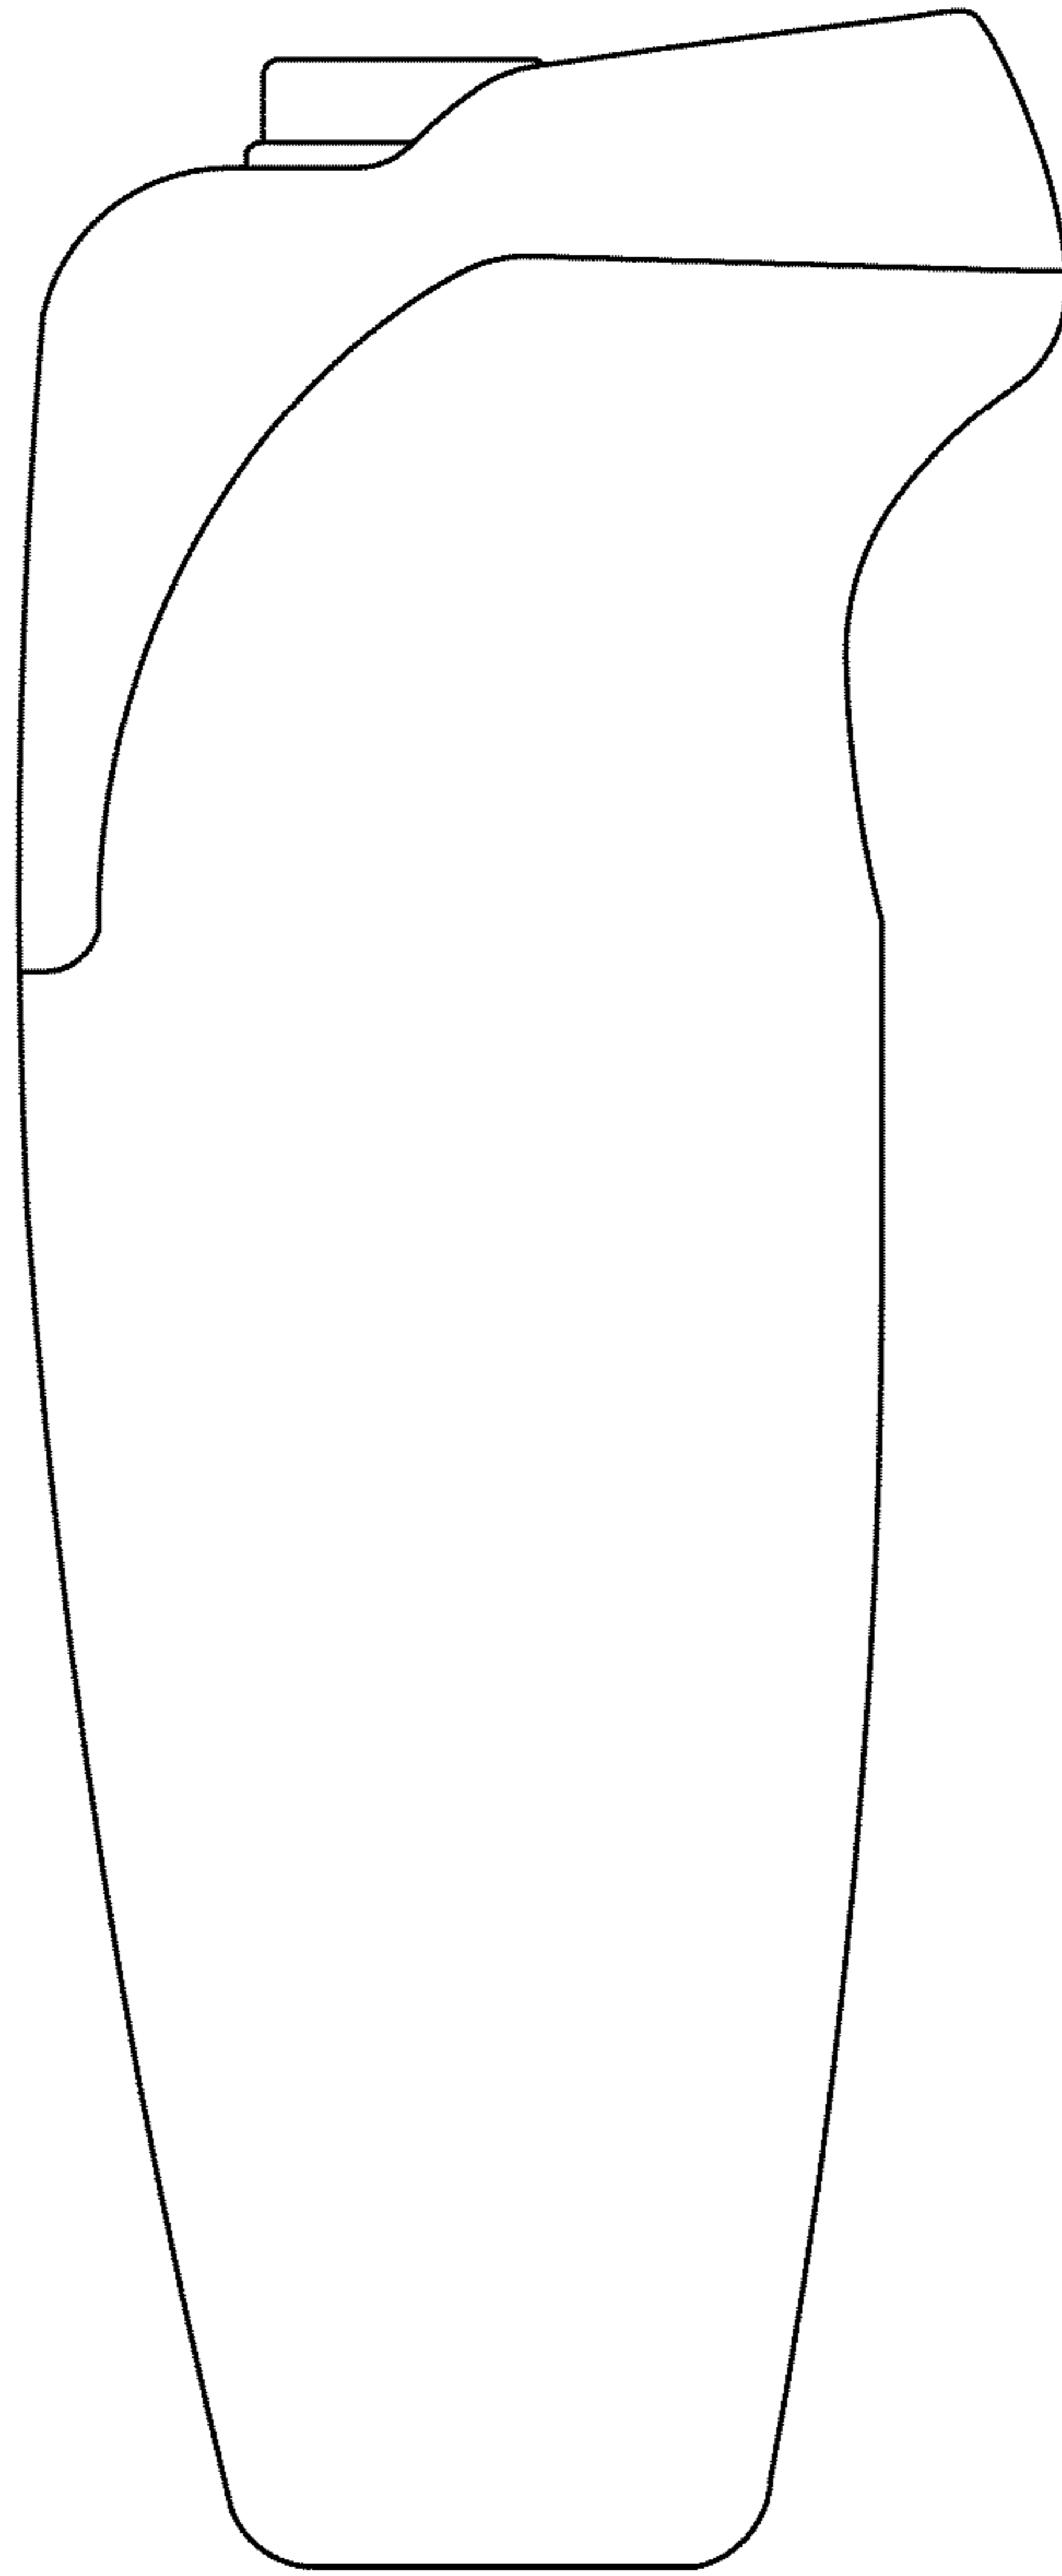


FIG. 5

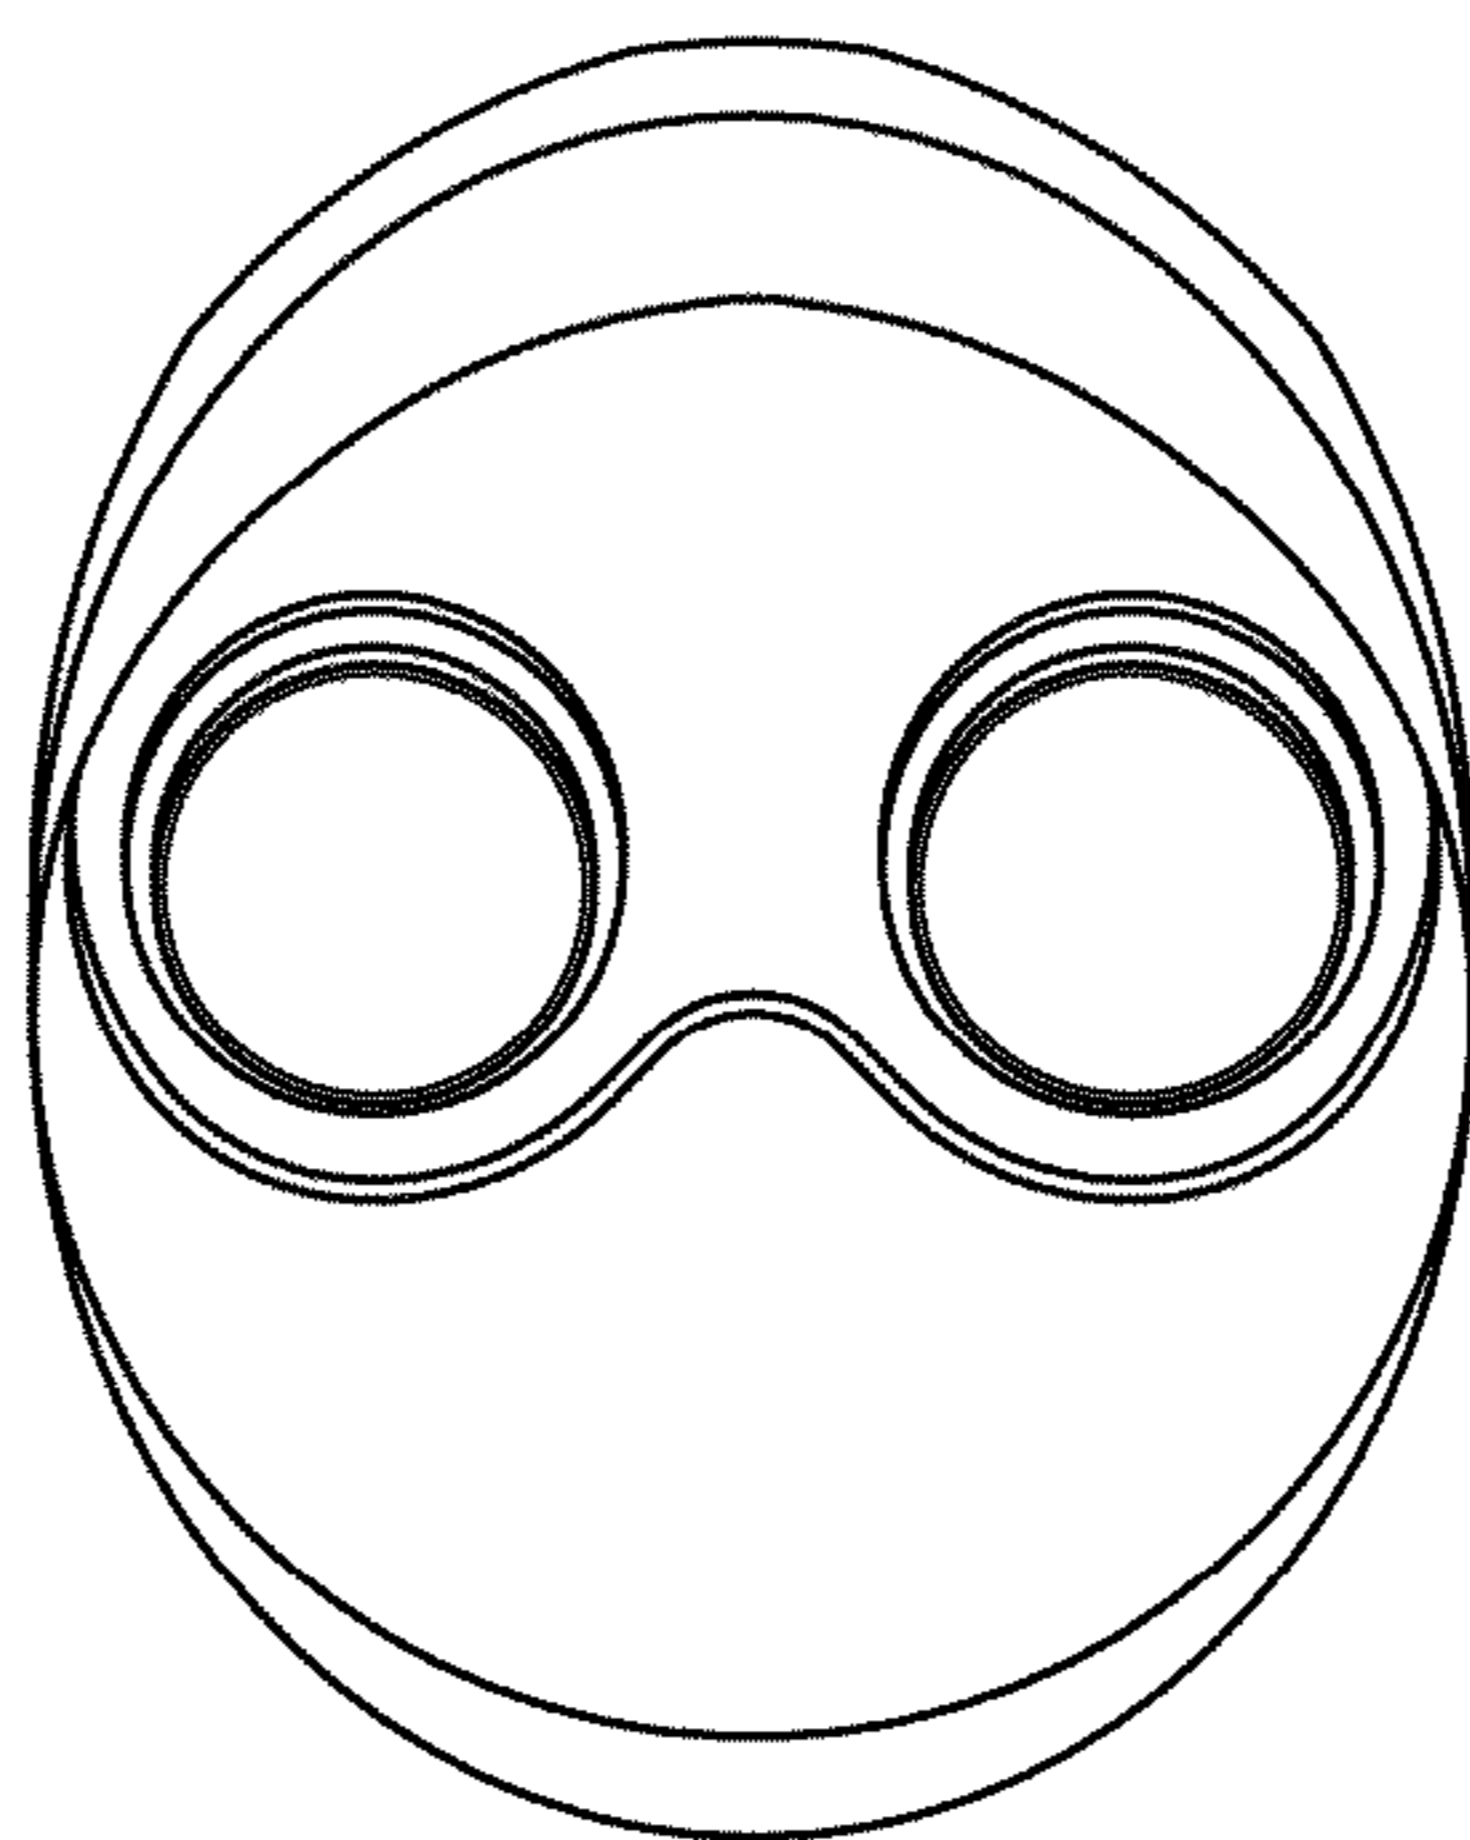


FIG. 6