



US00D714461S

(12) **United States Design Patent**
Judson et al.

(10) **Patent No.:** **US D714,461 S**
(45) **Date of Patent:** **** Sep. 30, 2014**

(54) **TISSUE SUSPENSION ADAPTOR**

(71) Applicant: **Paragonix Technologies, Inc.**,
Cambridge, MA (US)

(72) Inventors: **Jared Alden Judson**, Medford, MA
(US); **Lisa Maria Anderson**, Boston,
MA (US)

(73) Assignee: **Paragonix Technologies, Inc.**,
Braintree, MA (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/470,118**

(22) Filed: **Oct. 17, 2013**

Related U.S. Application Data

(62) Division of application No. 29/435,690, filed on Oct.
26, 2012, now Pat. No. Des. 692,160.

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/216**

(58) **Field of Classification Search**

USPC D24/216, 223, 224, 225, 226, 217, 227,
D24/231, 232, 129; D10/81; 62/78, 457.1,
62/457.2, 457.9; 435/1.1, 1.2, 1.3, 284.1,
435/307.1; 422/500, 547

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D243,070 S 1/1977 Burgheimer et al.
D358,469 S 5/1995 Mongeon

5,536,656 A	7/1996	Kemp et al.	
5,843,766 A	12/1998	Applegate et al.	
6,046,046 A	4/2000	Hassanein	
D458,997 S	6/2002	Crawford et al.	
D460,181 S	7/2002	Swenson	
D470,594 S	2/2003	Brassil et al.	
D473,941 S *	4/2003	Cise et al.	D24/129
D524,497 S	7/2006	Bruneau	
D671,639 S	11/2012	Trifilio	
2008/0038811 A1	2/2008	Alford et al.	
2008/0286746 A1 *	11/2008	Poo et al.	435/1.1
2012/0309078 A1	12/2012	Anderson et al.	

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Thomas C. Meyers; Brown
Rudnick LLP

(57) **CLAIM**

The ornamental design for a tissue suspension adaptor, as
shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of a tissue suspension
adaptor in accordance with the present invention;

FIG. 2 is a front view thereof, the rear view being a mirror
image;


FIG. 3 is a right side view thereof, the left side view being a
mirror image;

FIG. 4 is a top view thereof; and,

FIG. 5 is a bottom view thereof.

The broken lines are included for the purpose of illustrating
portions of the tissue suspension adaptor and form no part of
the claimed design.

1 Claim, 1 Drawing Sheet

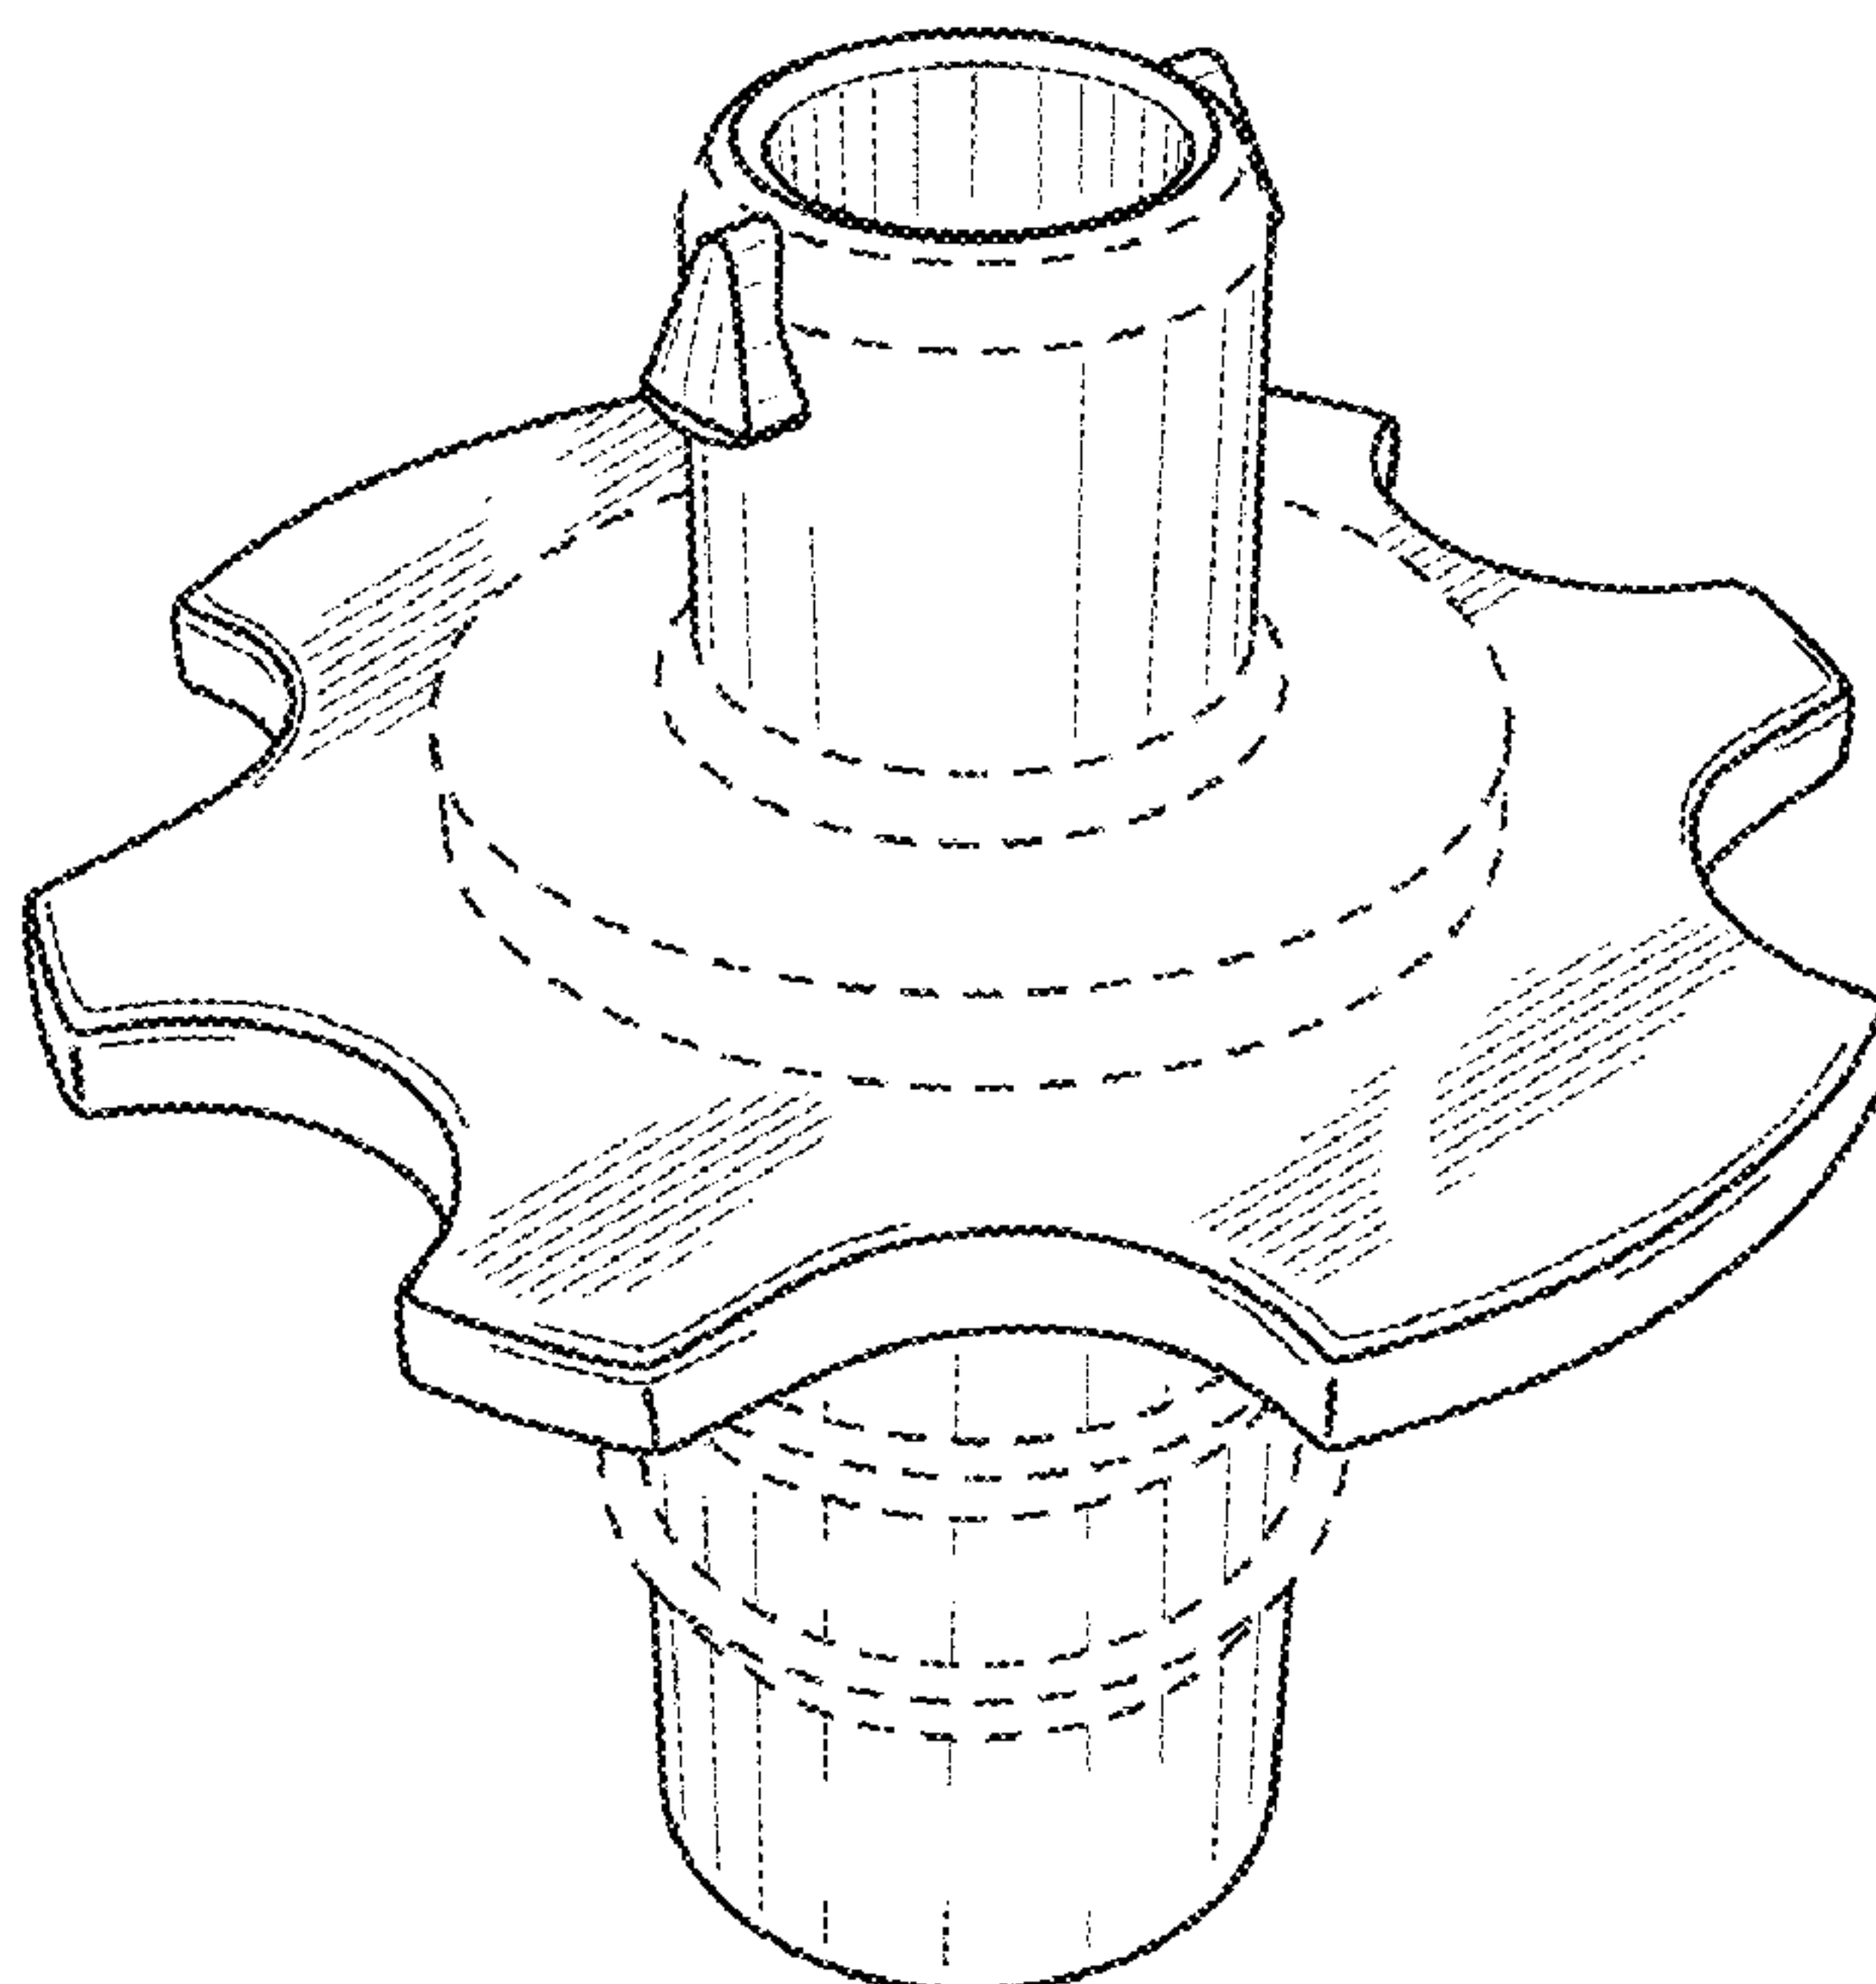

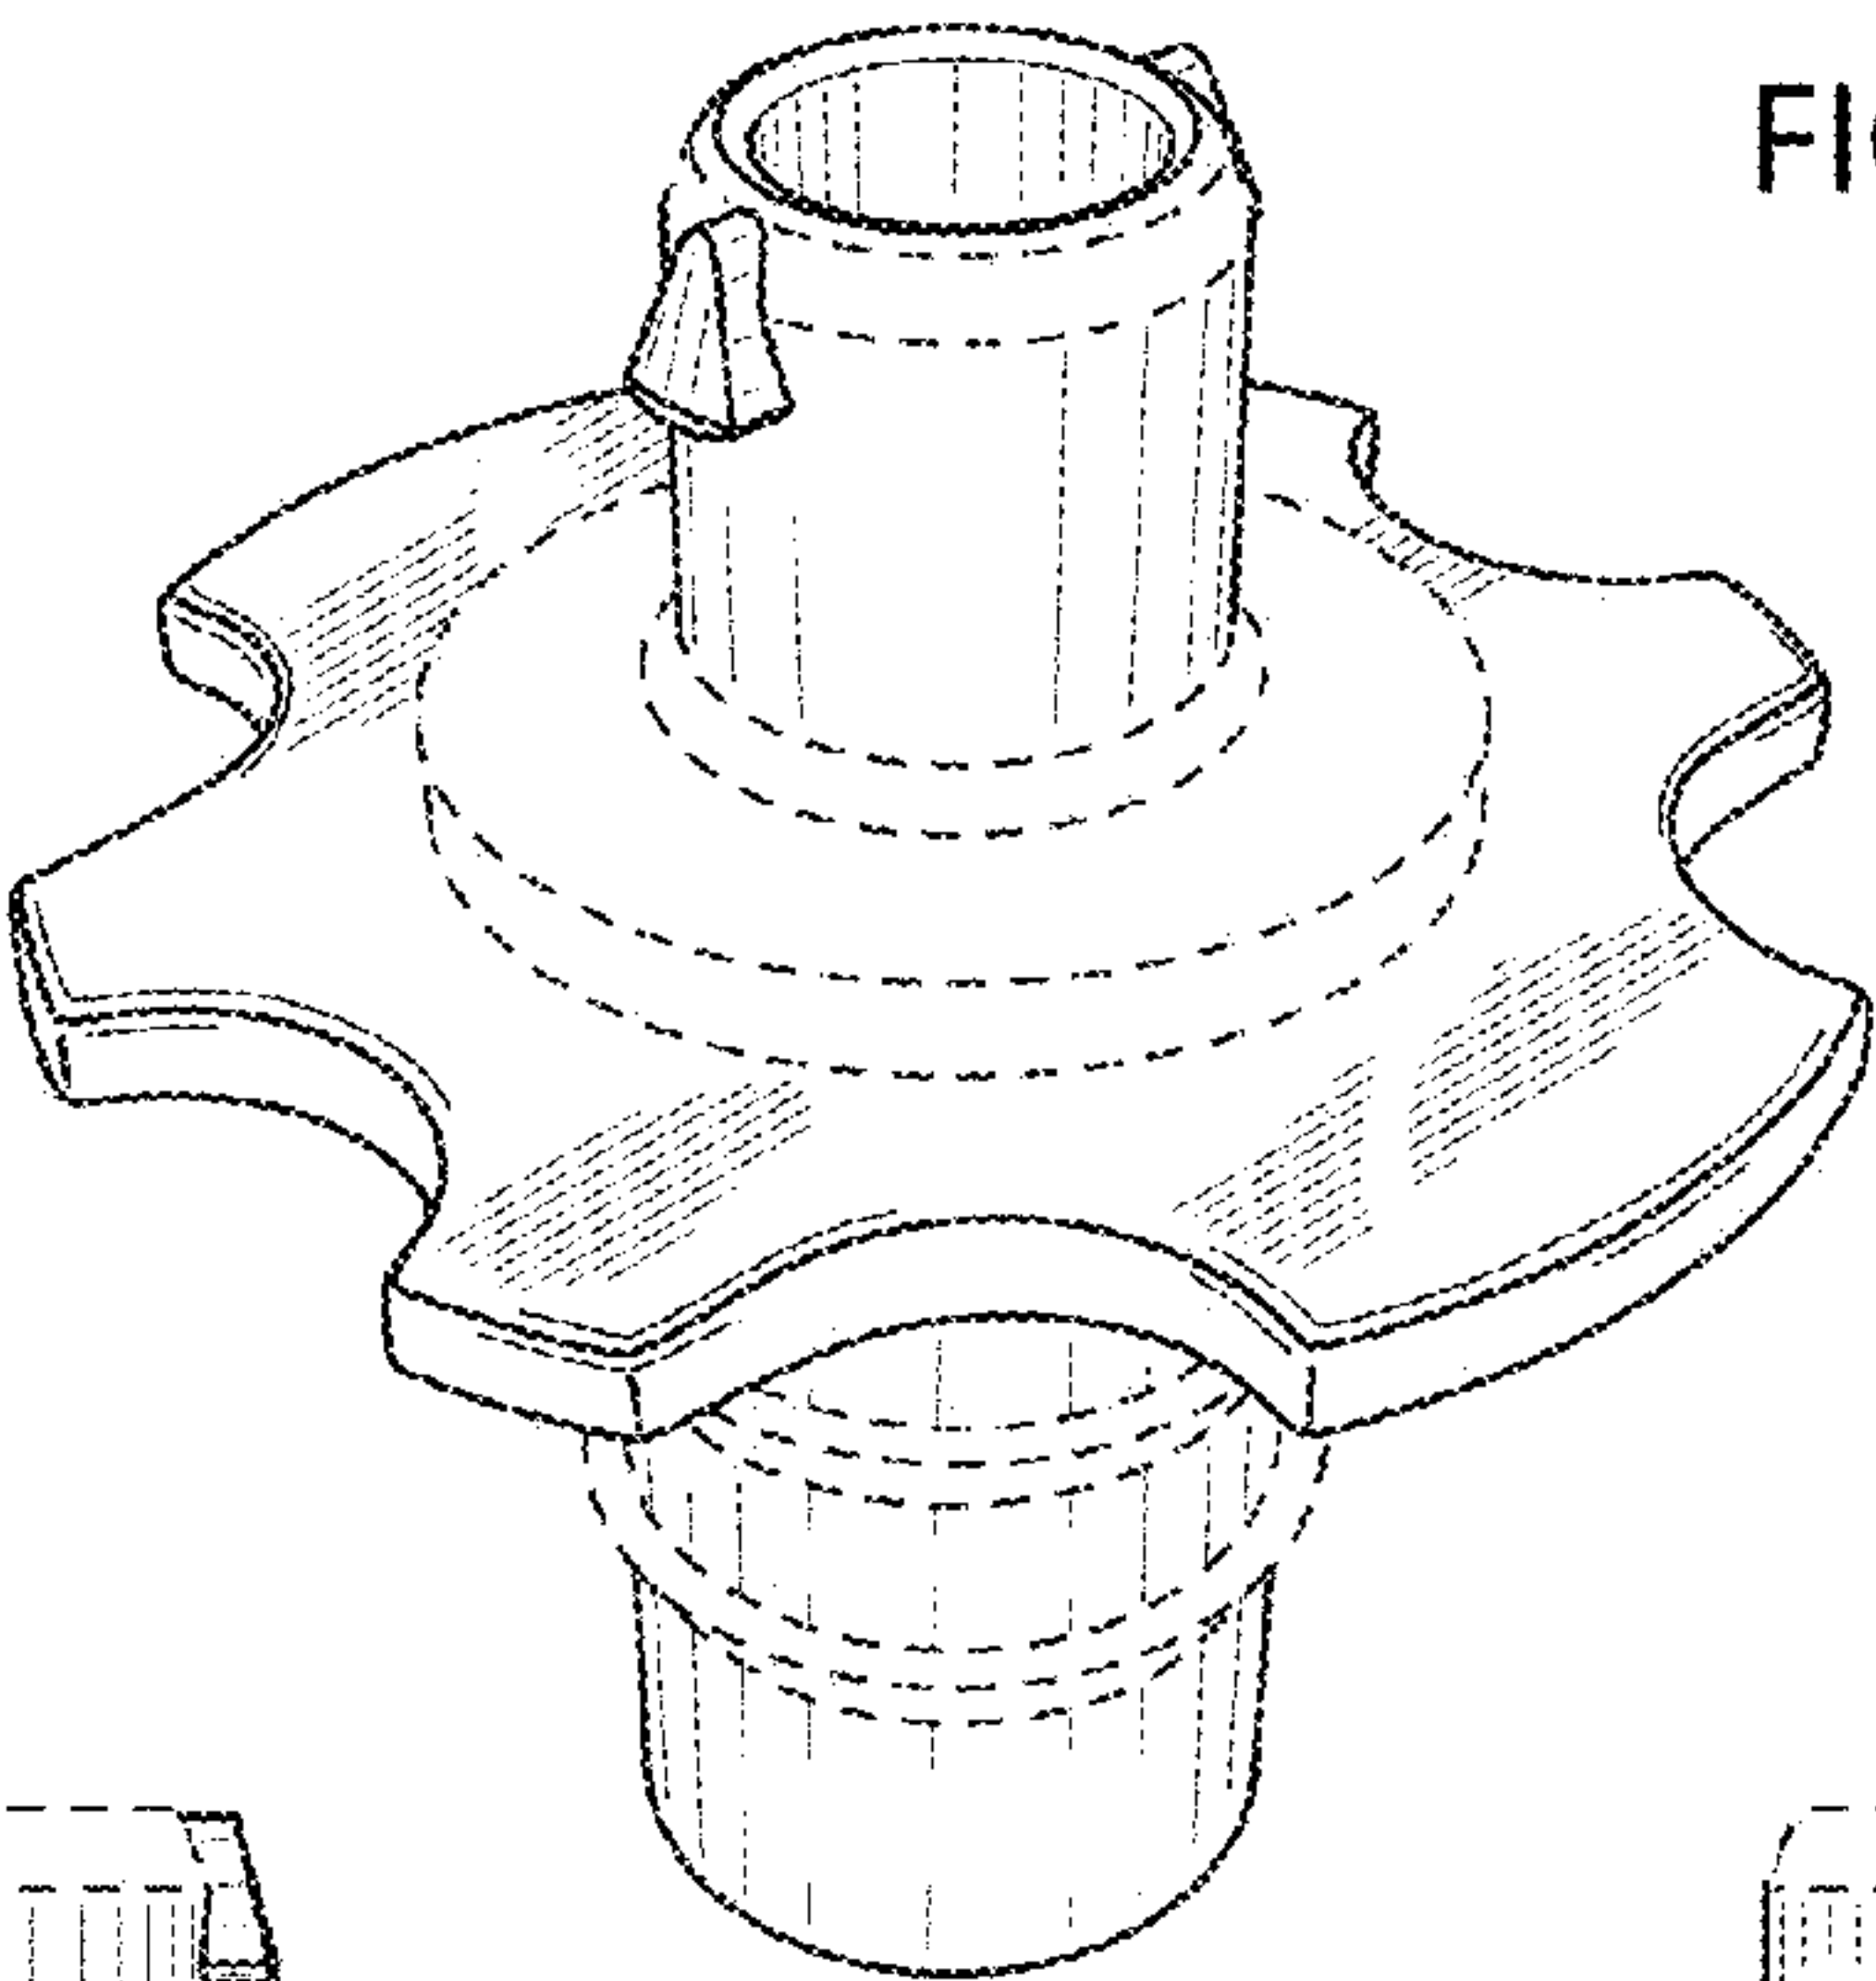


FIG. 1

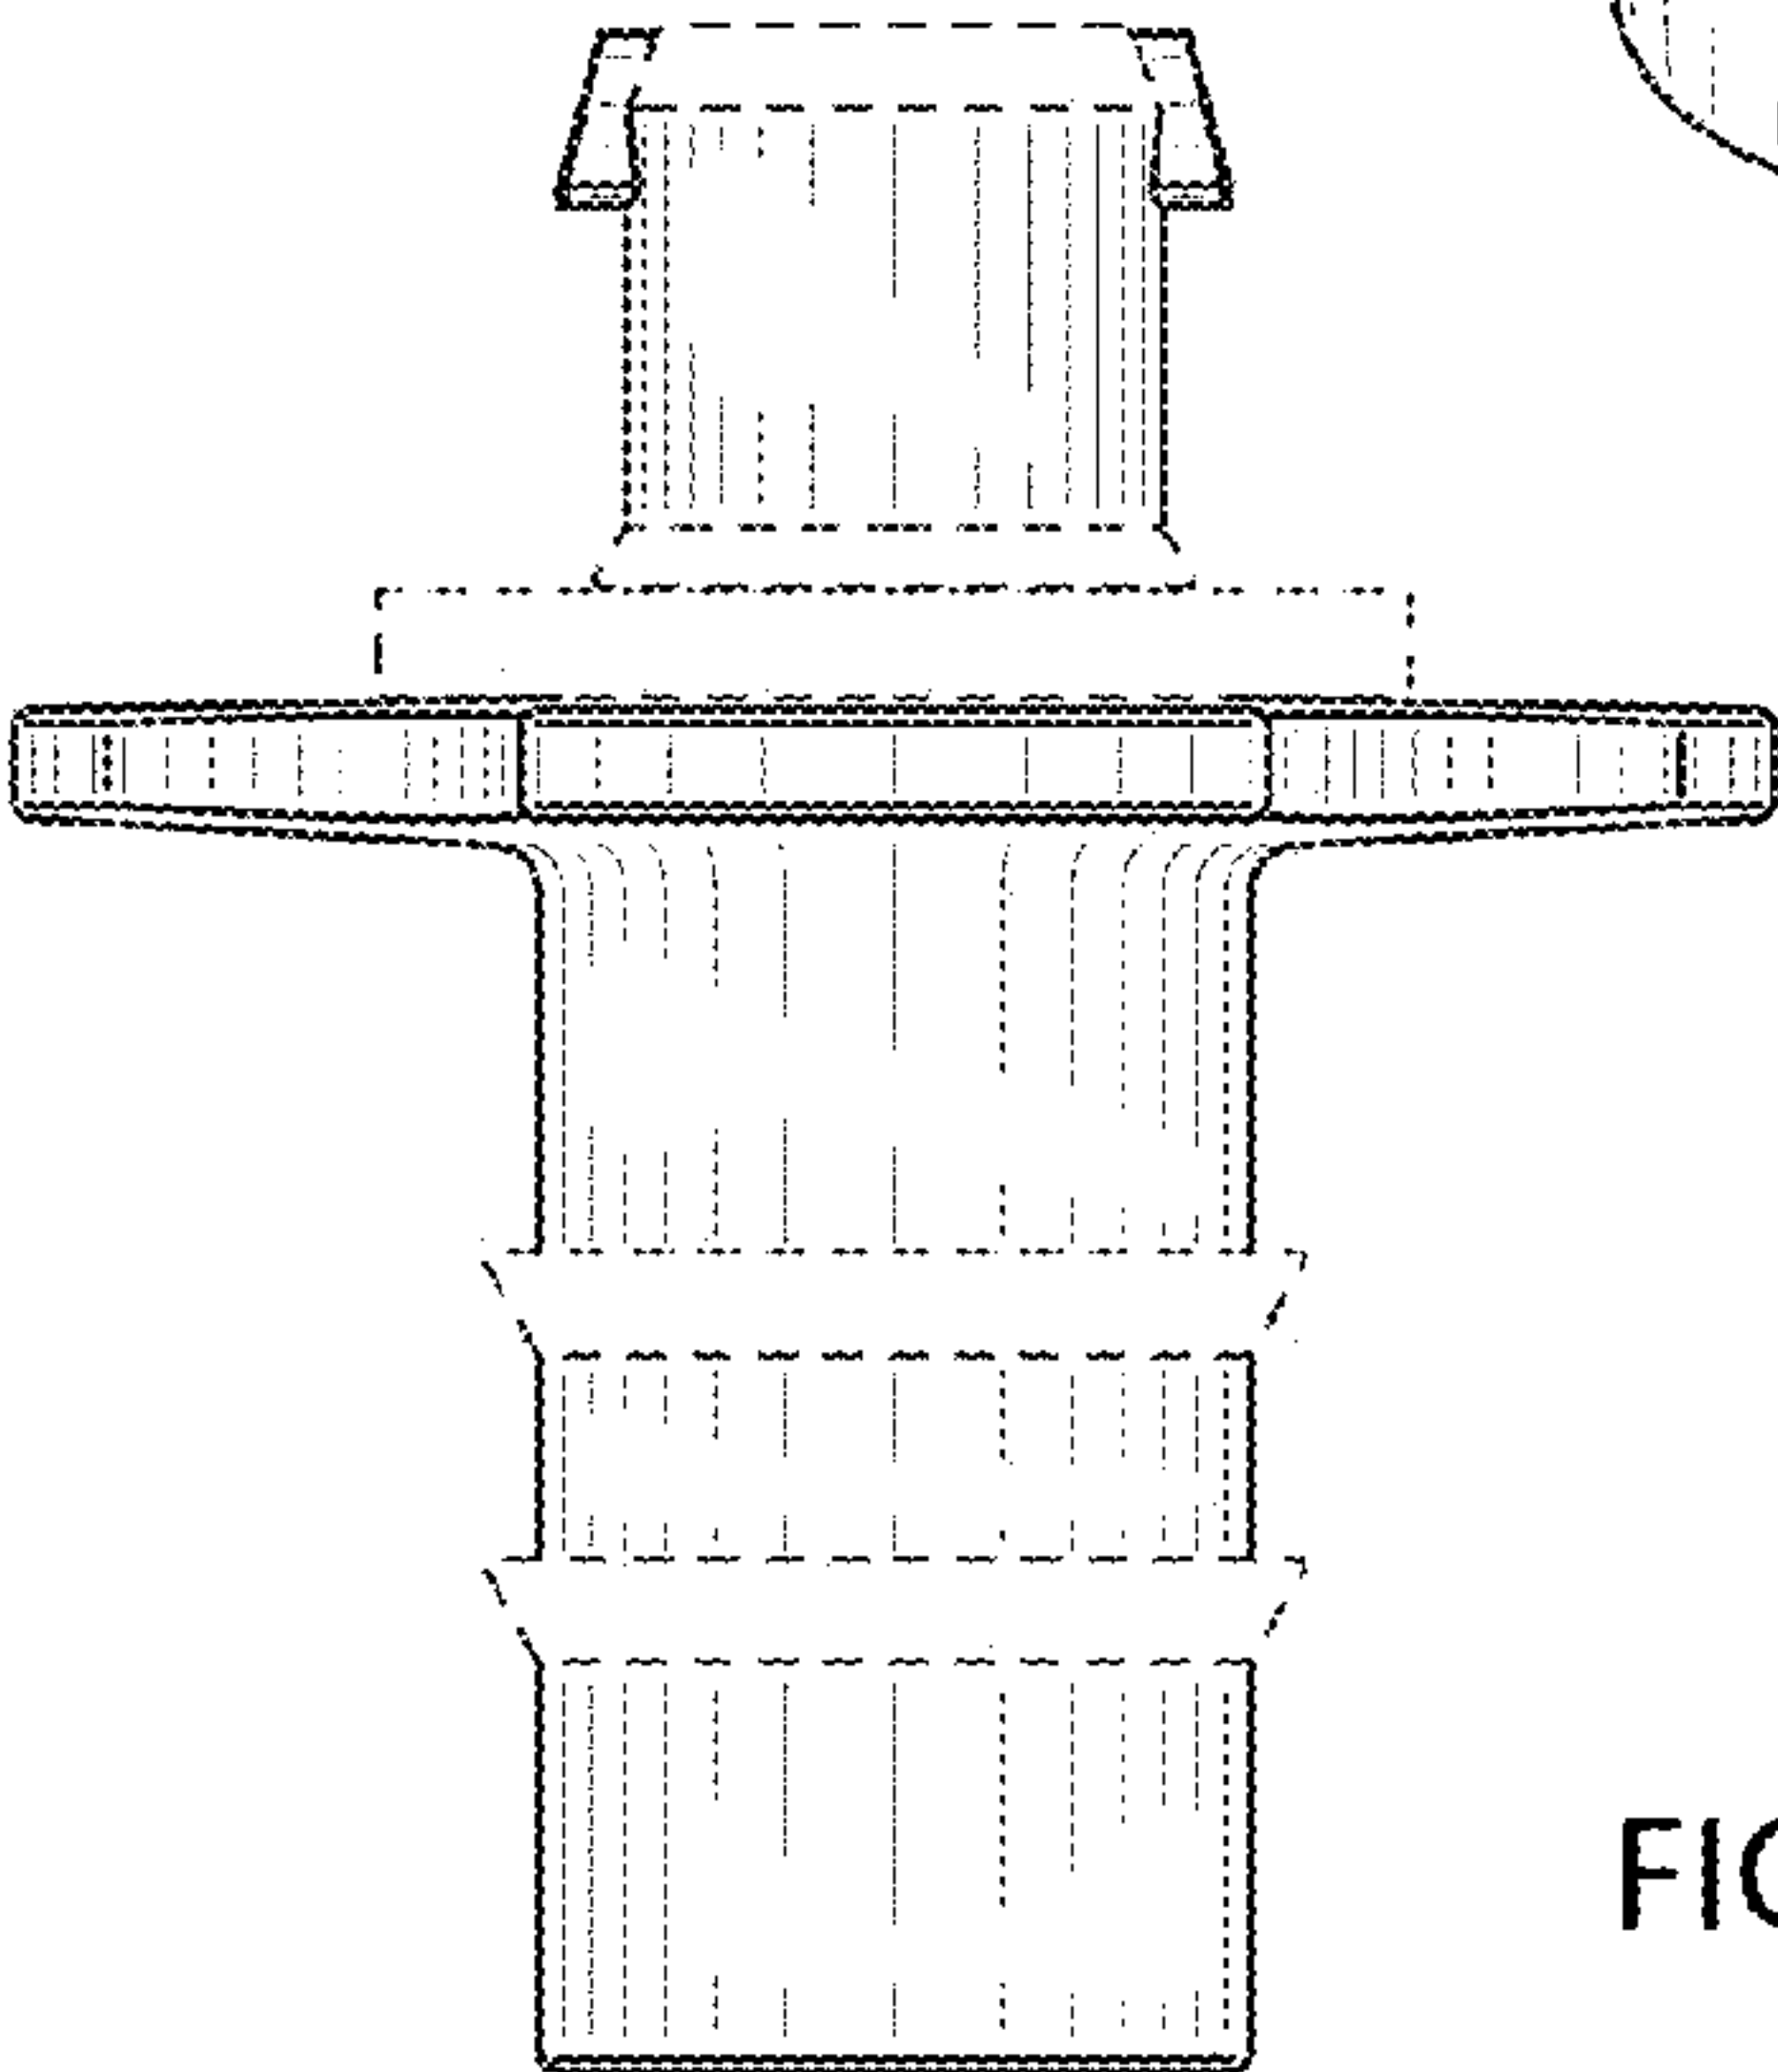


FIG. 2

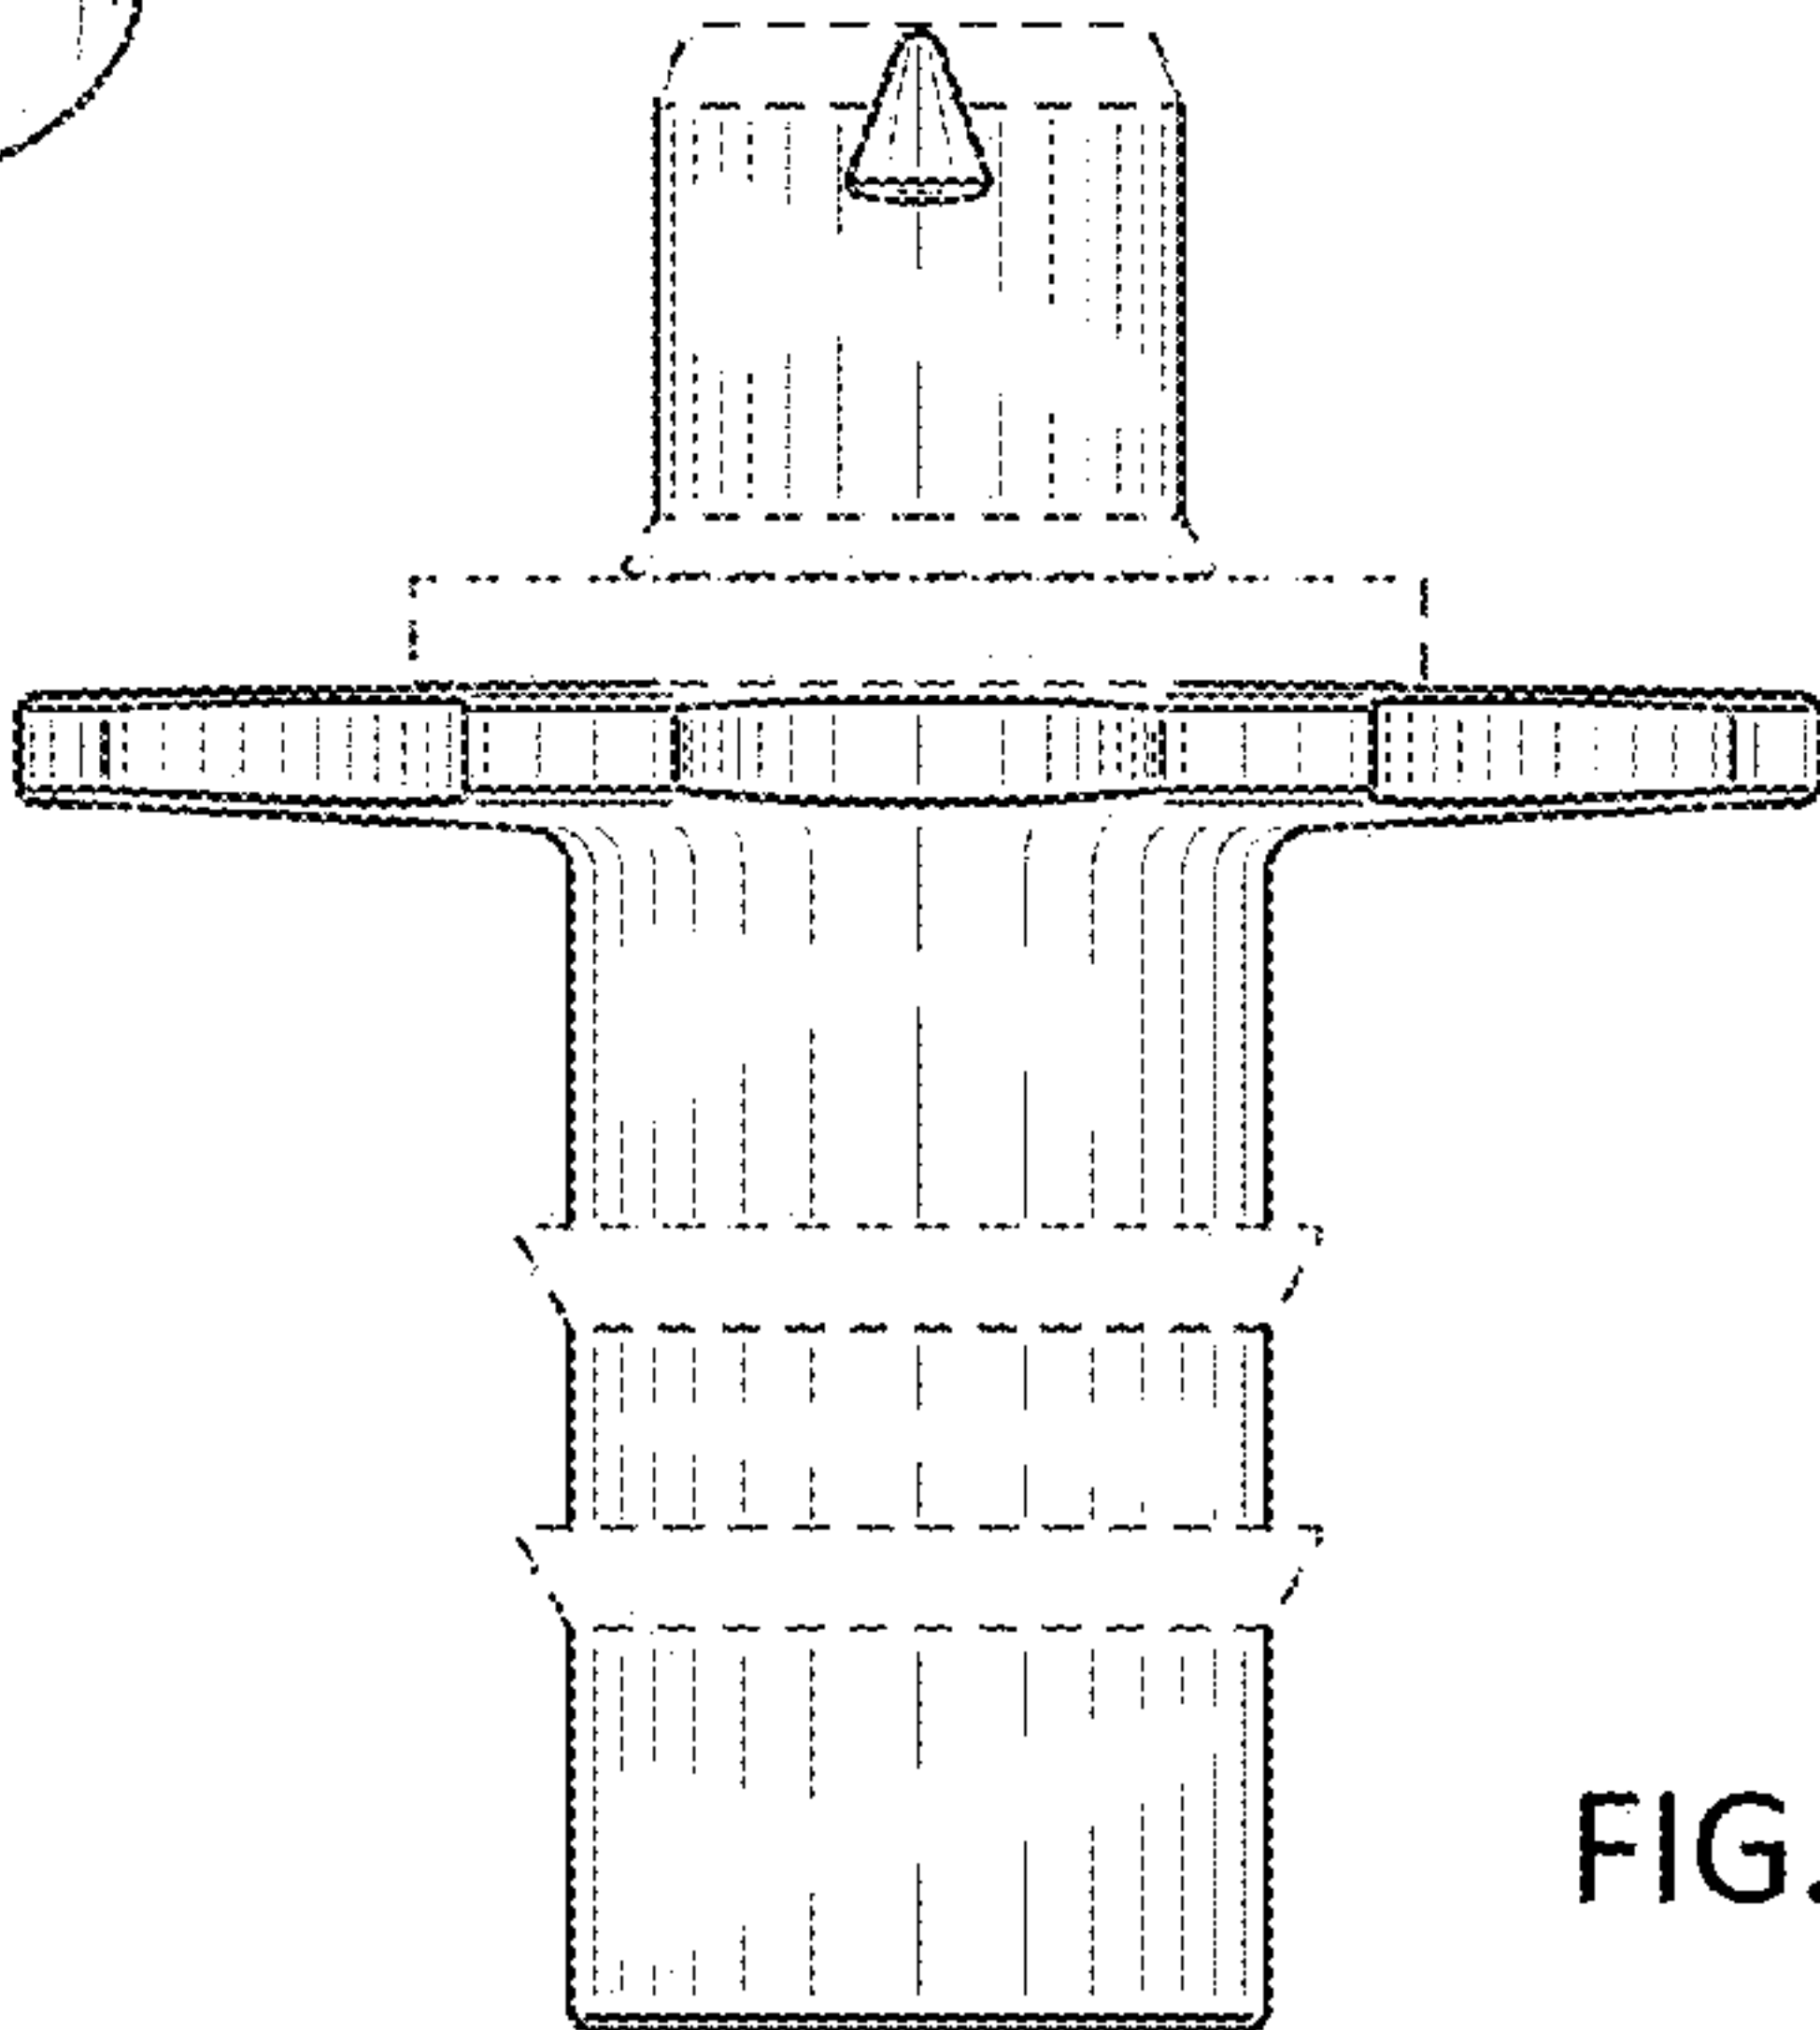


FIG. 3

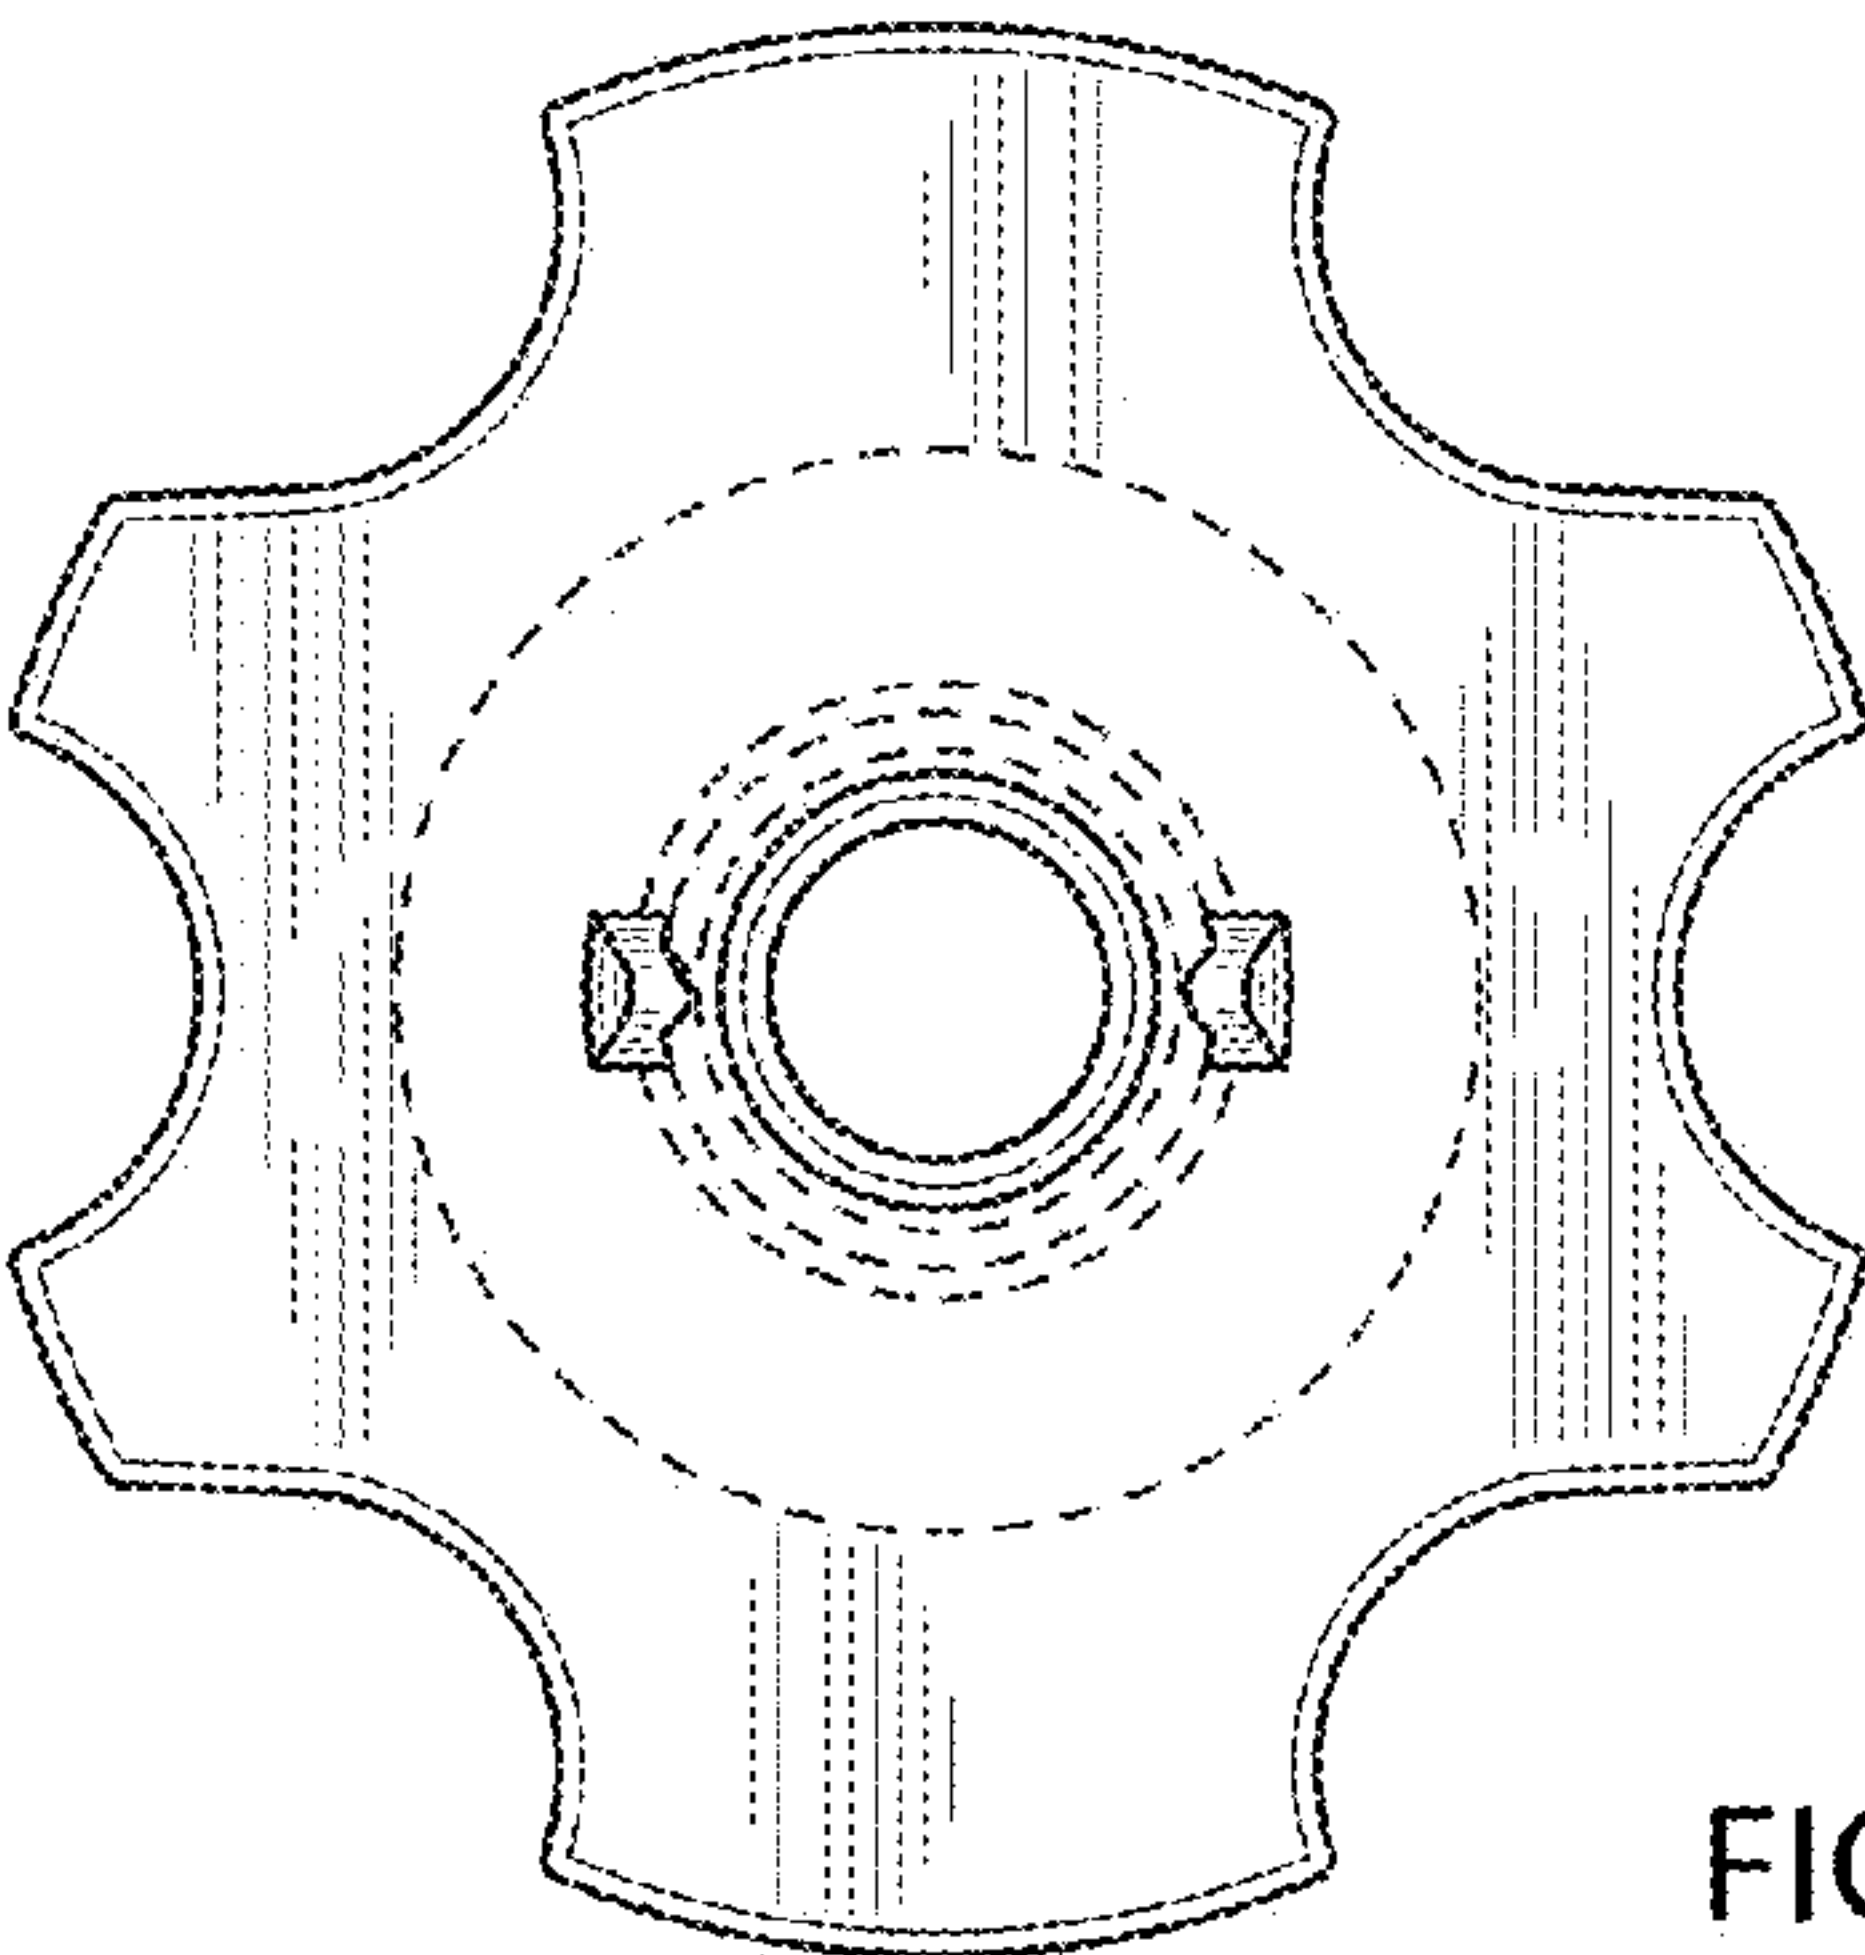


FIG. 4

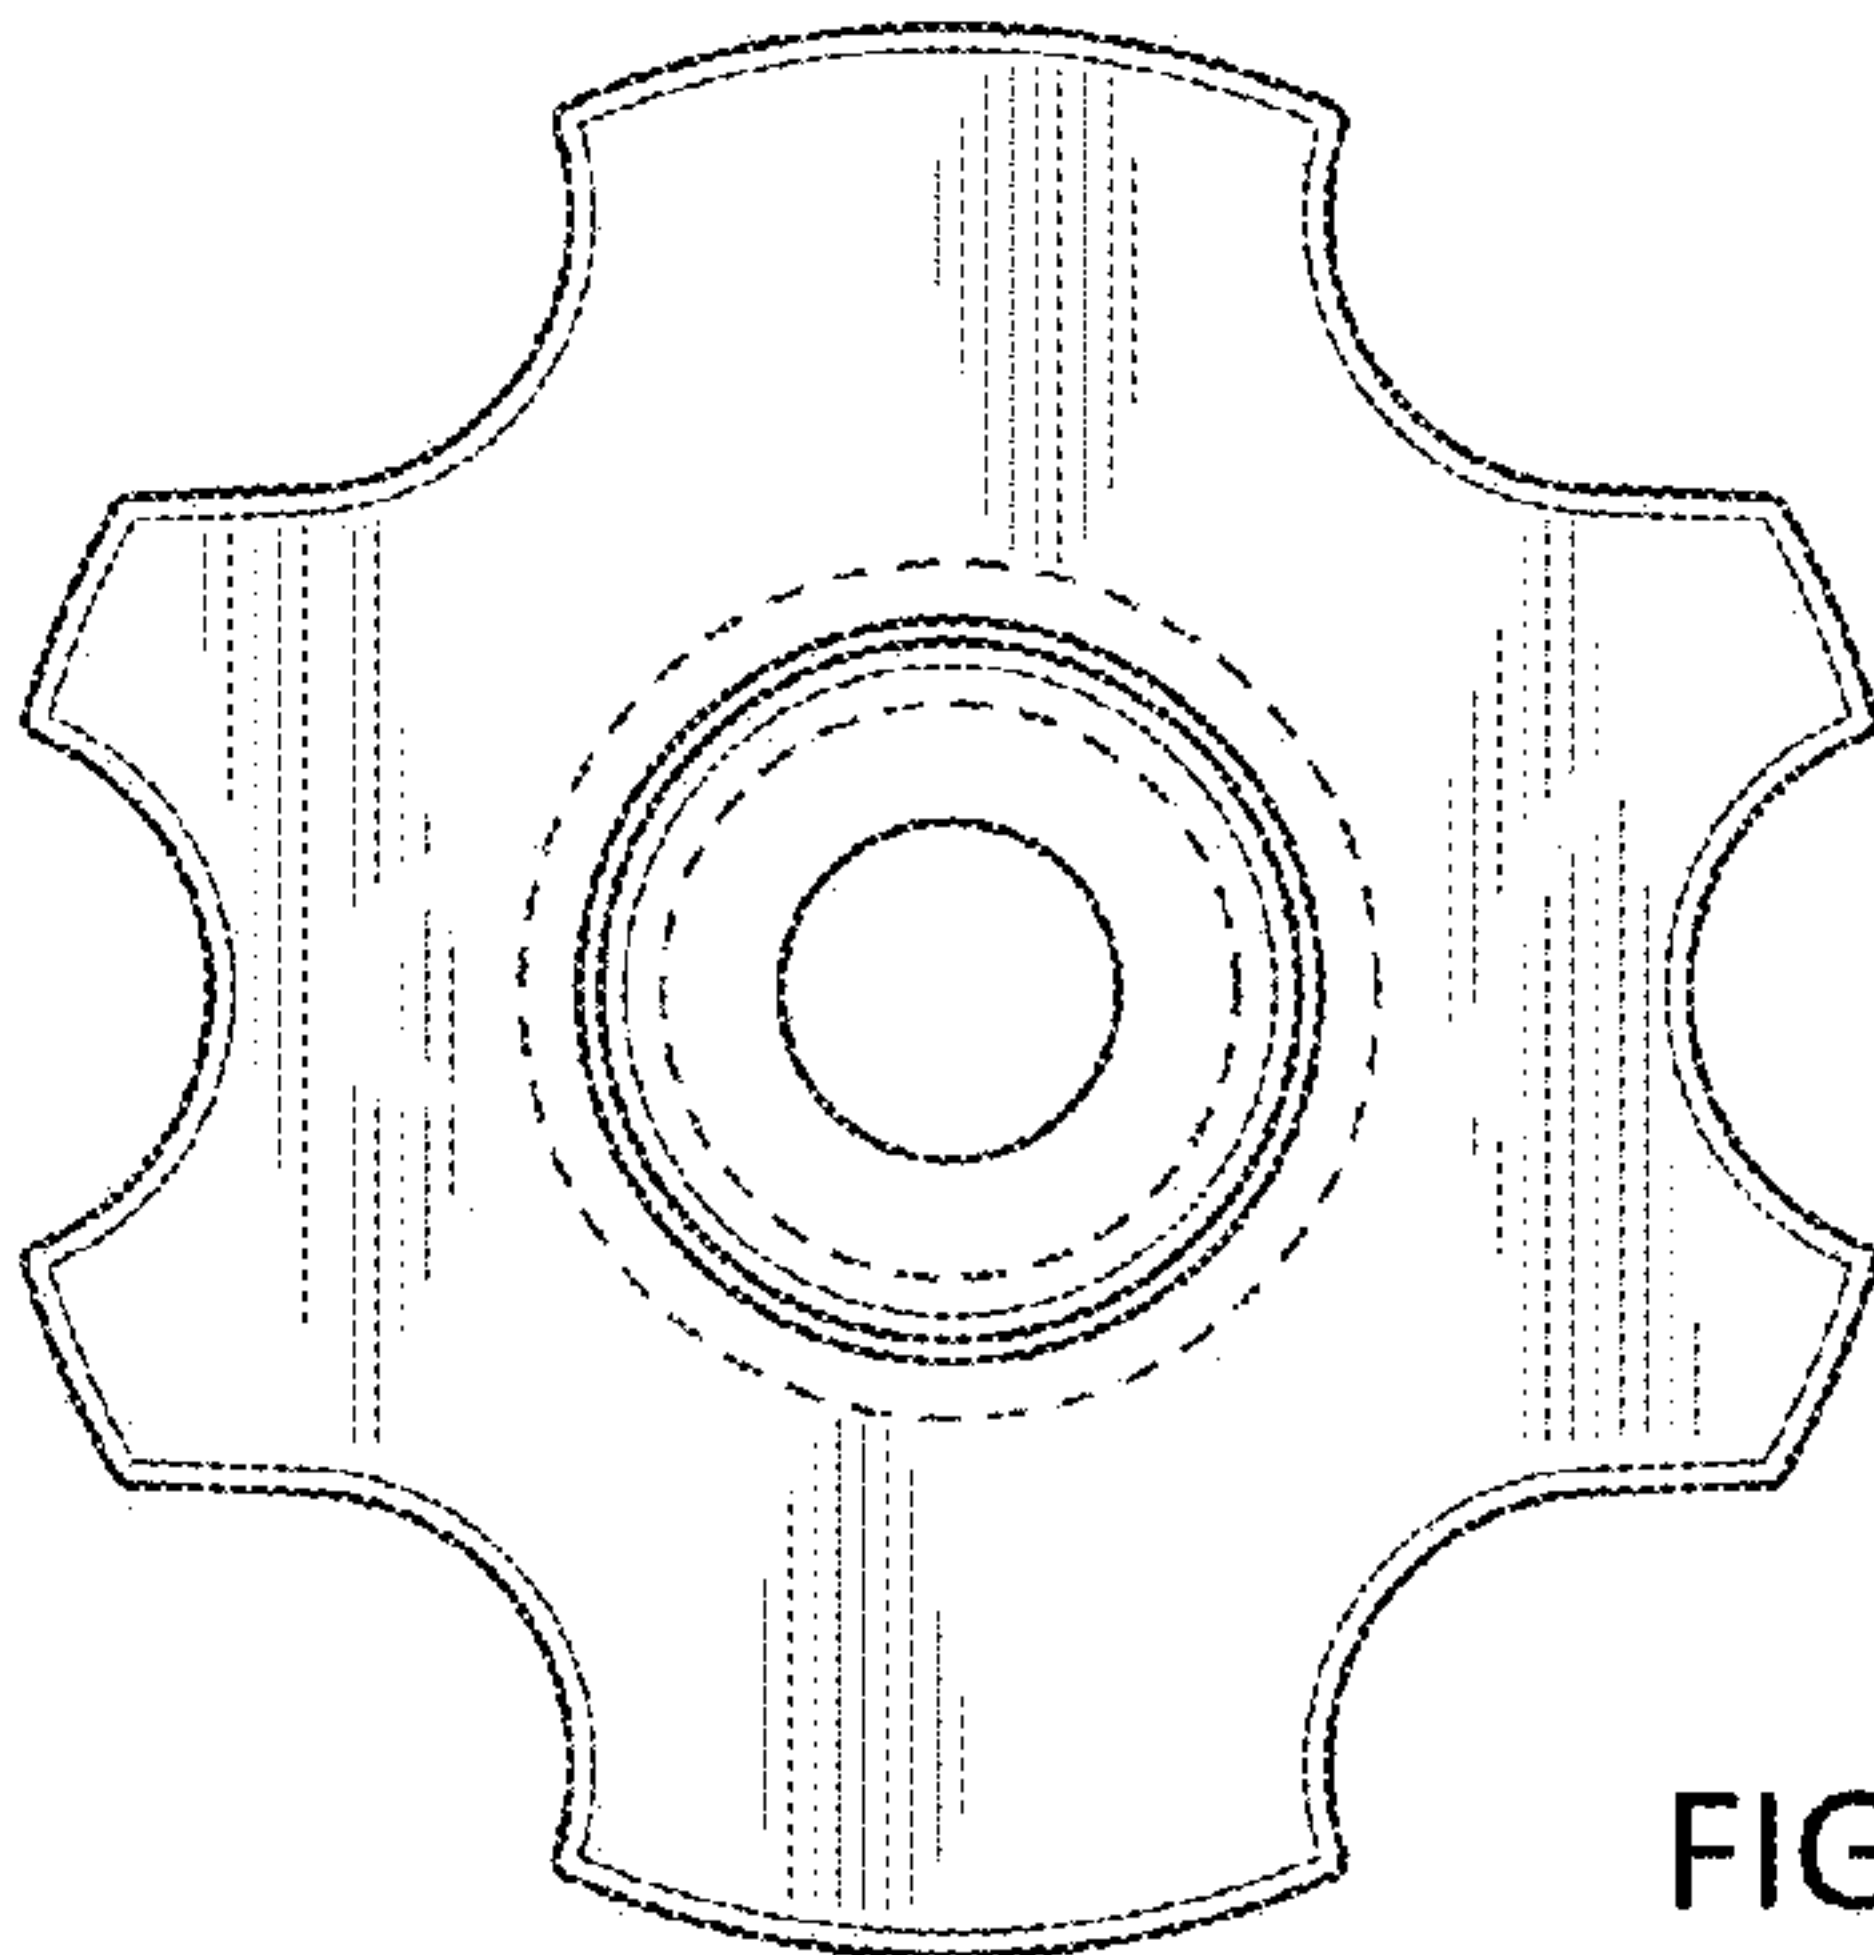


FIG. 5