



US00D715927S

(12) **United States Design Patent**
Kyvik et al.

(10) **Patent No.:** **US D715,927 S**
(45) **Date of Patent:** **** Oct. 21, 2014**

- (54) **DOUBLE NOTCHED CATHETER SECUREMENT DEVICE**
- (71) Applicant: **TIDI Securement Products, LLC**,
Neenah, WI (US)
- (72) Inventors: **Kurt Kyvik**, Ocala, FL (US); **Scott Ryan**, Ocala, FL (US); **Arthur Parkhurst**, Ocala, FL (US)
- (73) Assignee: **TIDI Securement Products, LLC**,
Neenah, WI (US)

- (**) Term: **14 Years**
- (21) Appl. No.: **29/464,264**
- (22) Filed: **Aug. 14, 2013**
- (51) **LOC (10) Cl.** **24-02**
- (52) **U.S. Cl.**
USPC **D24/128**
- (58) **Field of Classification Search**
USPC D24/127-128, 130, 112, 189;
600/391-392; 604/179-180, 187, 227;
128/DIG. 26; 602/58-59
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D364,922 S	*	12/1995	Bierman	D24/128
D375,356 S	*	11/1996	Bierman	D24/128
D401,329 S	*	11/1998	Bierman	D24/128
D424,691 S	*	5/2000	Yavitz	D24/128
D492,411 S	*	6/2004	Bierman	D24/128
D503,977 S	*	4/2005	Bierman	D24/128
D608,887 S		1/2010	Kyvik et al.		
D616,091 S	*	5/2010	Kyvik et al.	D24/128
D616,542 S	*	5/2010	Kyvik et al.	D24/128
D616,983 S		6/2010	Kyvik et al.		
D625,002 S		10/2010	Kyvik et al.		
8,251,957 B2		8/2012	Kyvik et al.		

D695,901 S * 12/2013 Heinecke et al. D24/189

* cited by examiner


Primary Examiner — Robert A. Delehanty
(74) *Attorney, Agent, or Firm* — Boyle Fredrickson, S.C.

(57) **CLAIM**
The ornamental design for a double notched catheter securement device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the catheter securement device with release layer, shown in an open position.
 FIG. 2 is a top view of the catheter securement device with release layer.
 FIG. 3 is a bottom view of the catheter securement device with release layer.
 FIG. 4 is a right side view of the catheter securement device with release layer.
 FIG. 5 is a left side view of the catheter securement device with release layer.
 FIG. 6 is a rear view of the catheter securement device with release layer.
 FIG. 7 is a front view of the catheter securement device with release layer.
 FIG. 8 is a top view of the catheter securement device with the release layer removed.
 FIG. 9 is a bottom view of the catheter securement device with the release layer removed.
 FIG. 10 is a right side view of the catheter securement device with the release layer removed.
 FIG. 11 is a left side view of the catheter securement device with the release layer removed.
 FIG. 12 is a rear view of the catheter securement device with the release layer removed; and,
 FIG. 13 is a front view of the catheter securement device with the release layer removed.

1 Claim, 5 Drawing Sheets

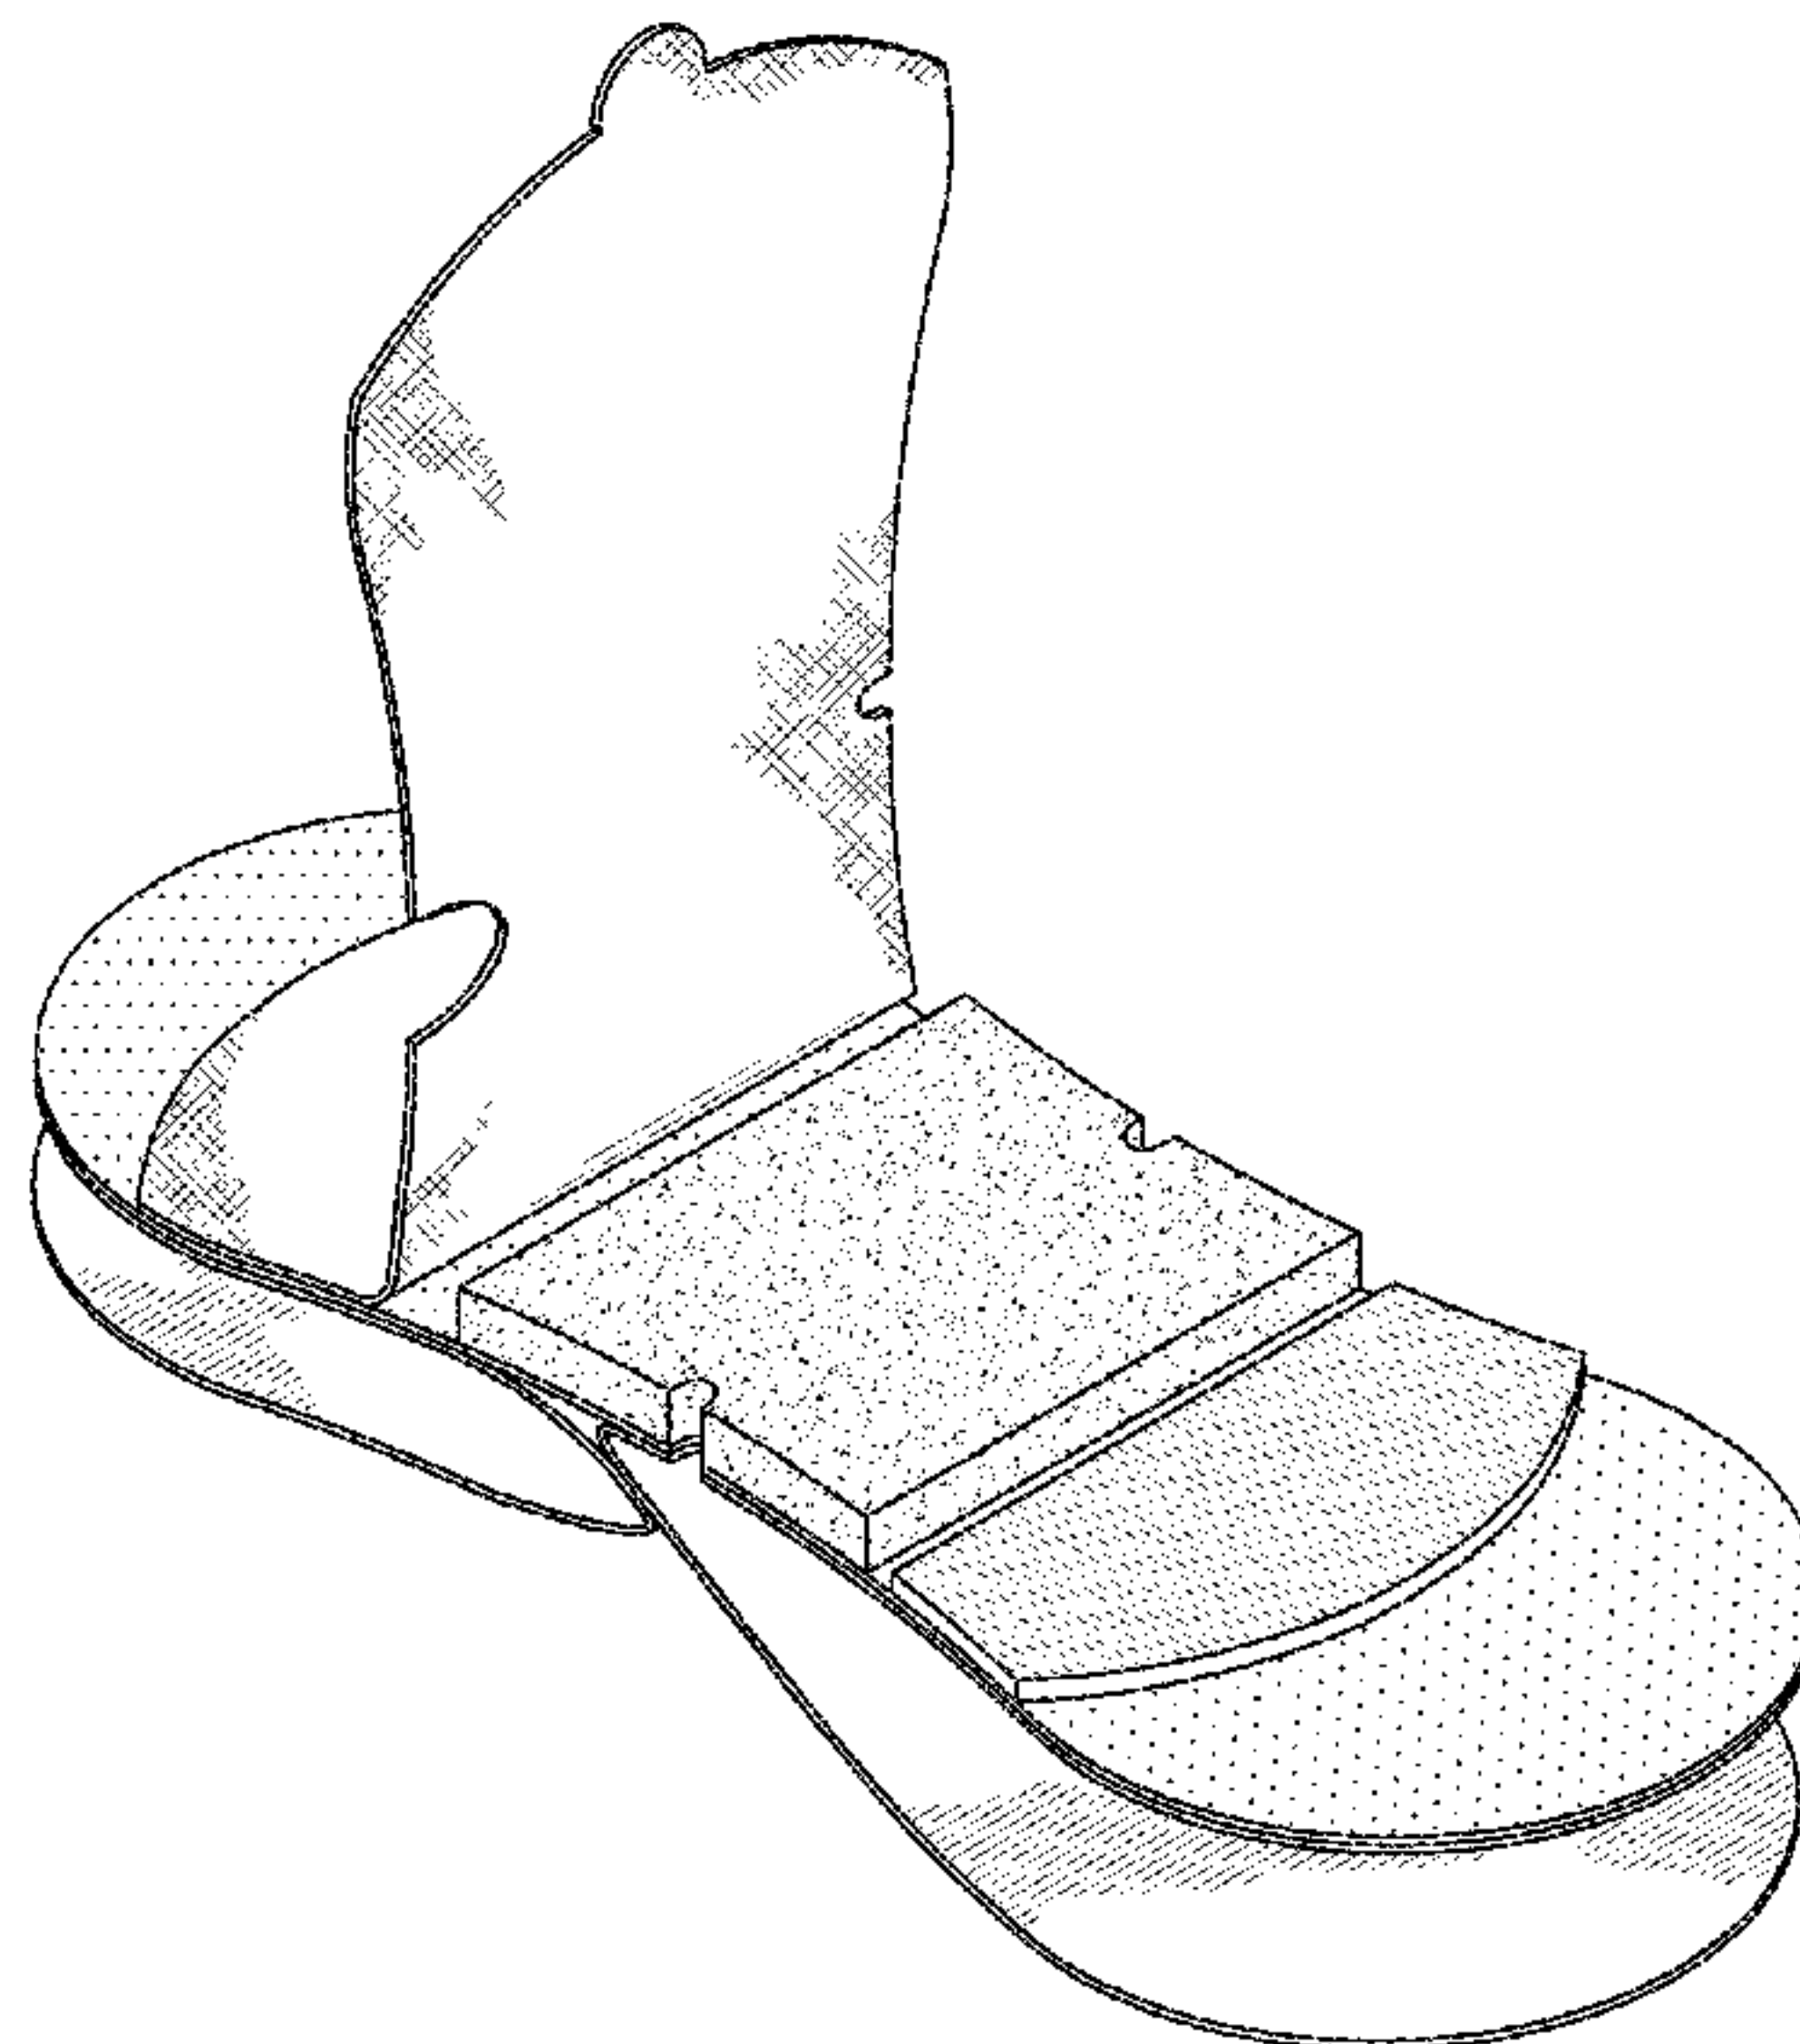

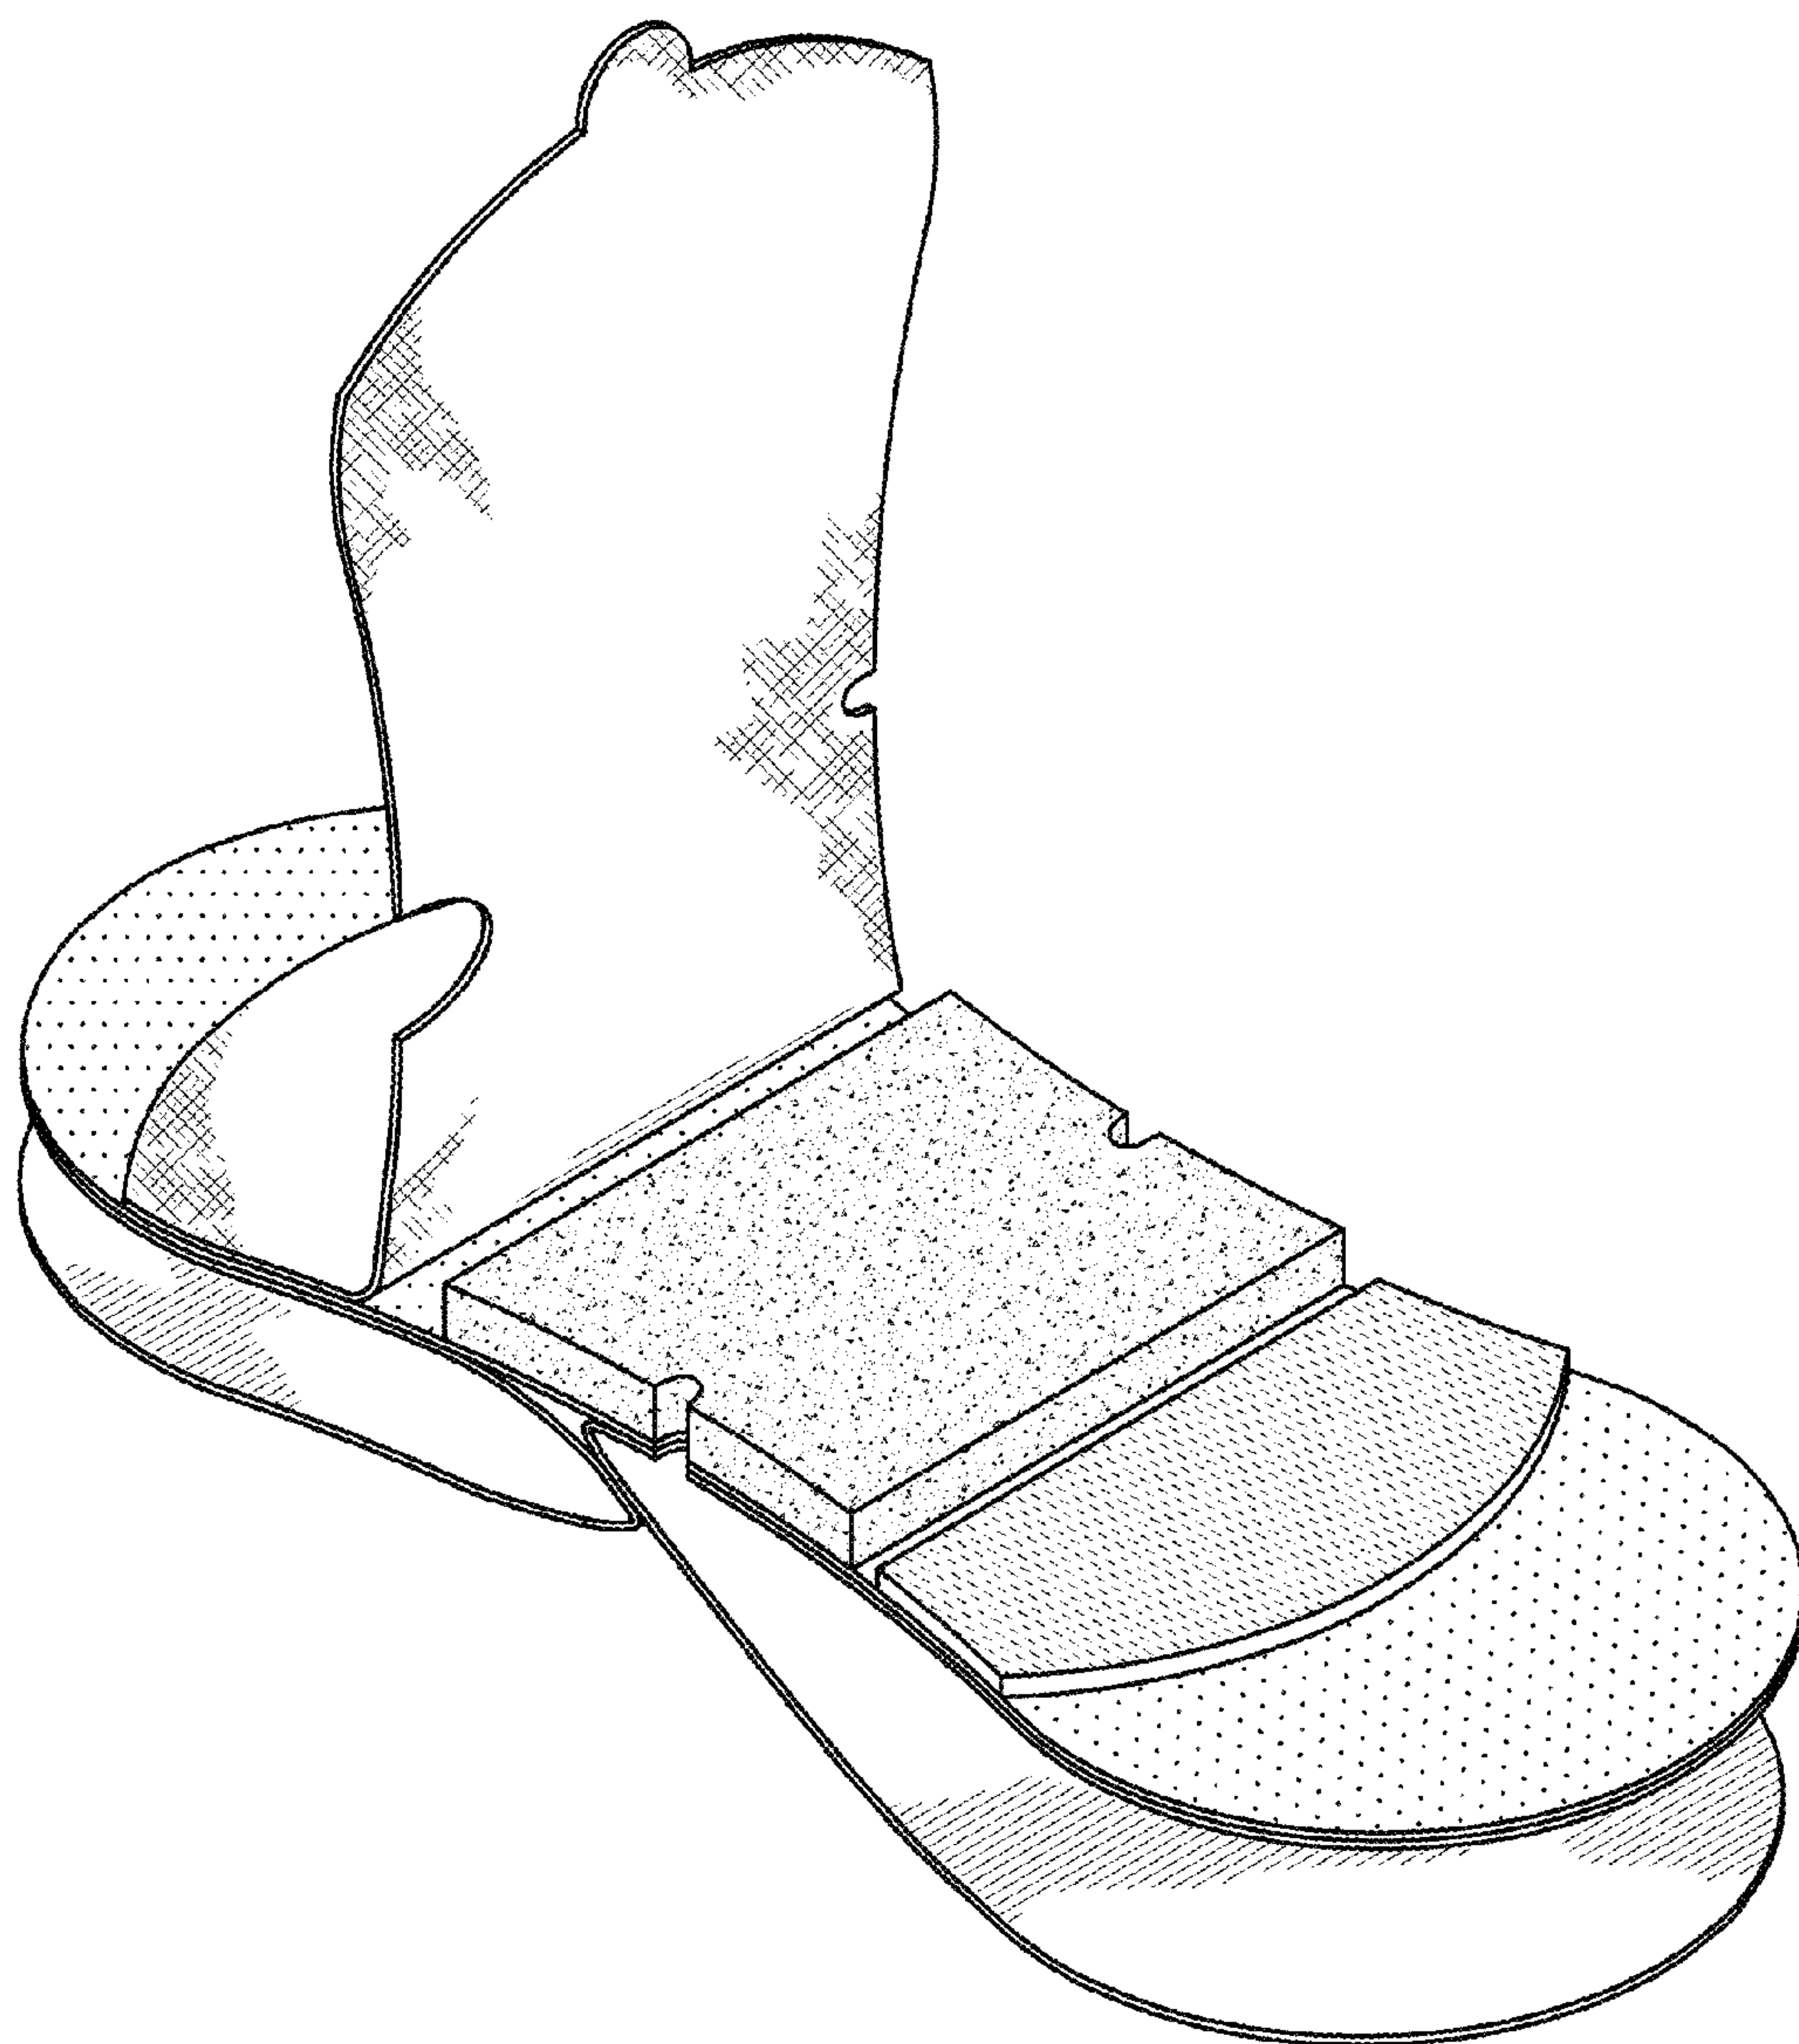


Fig. 1

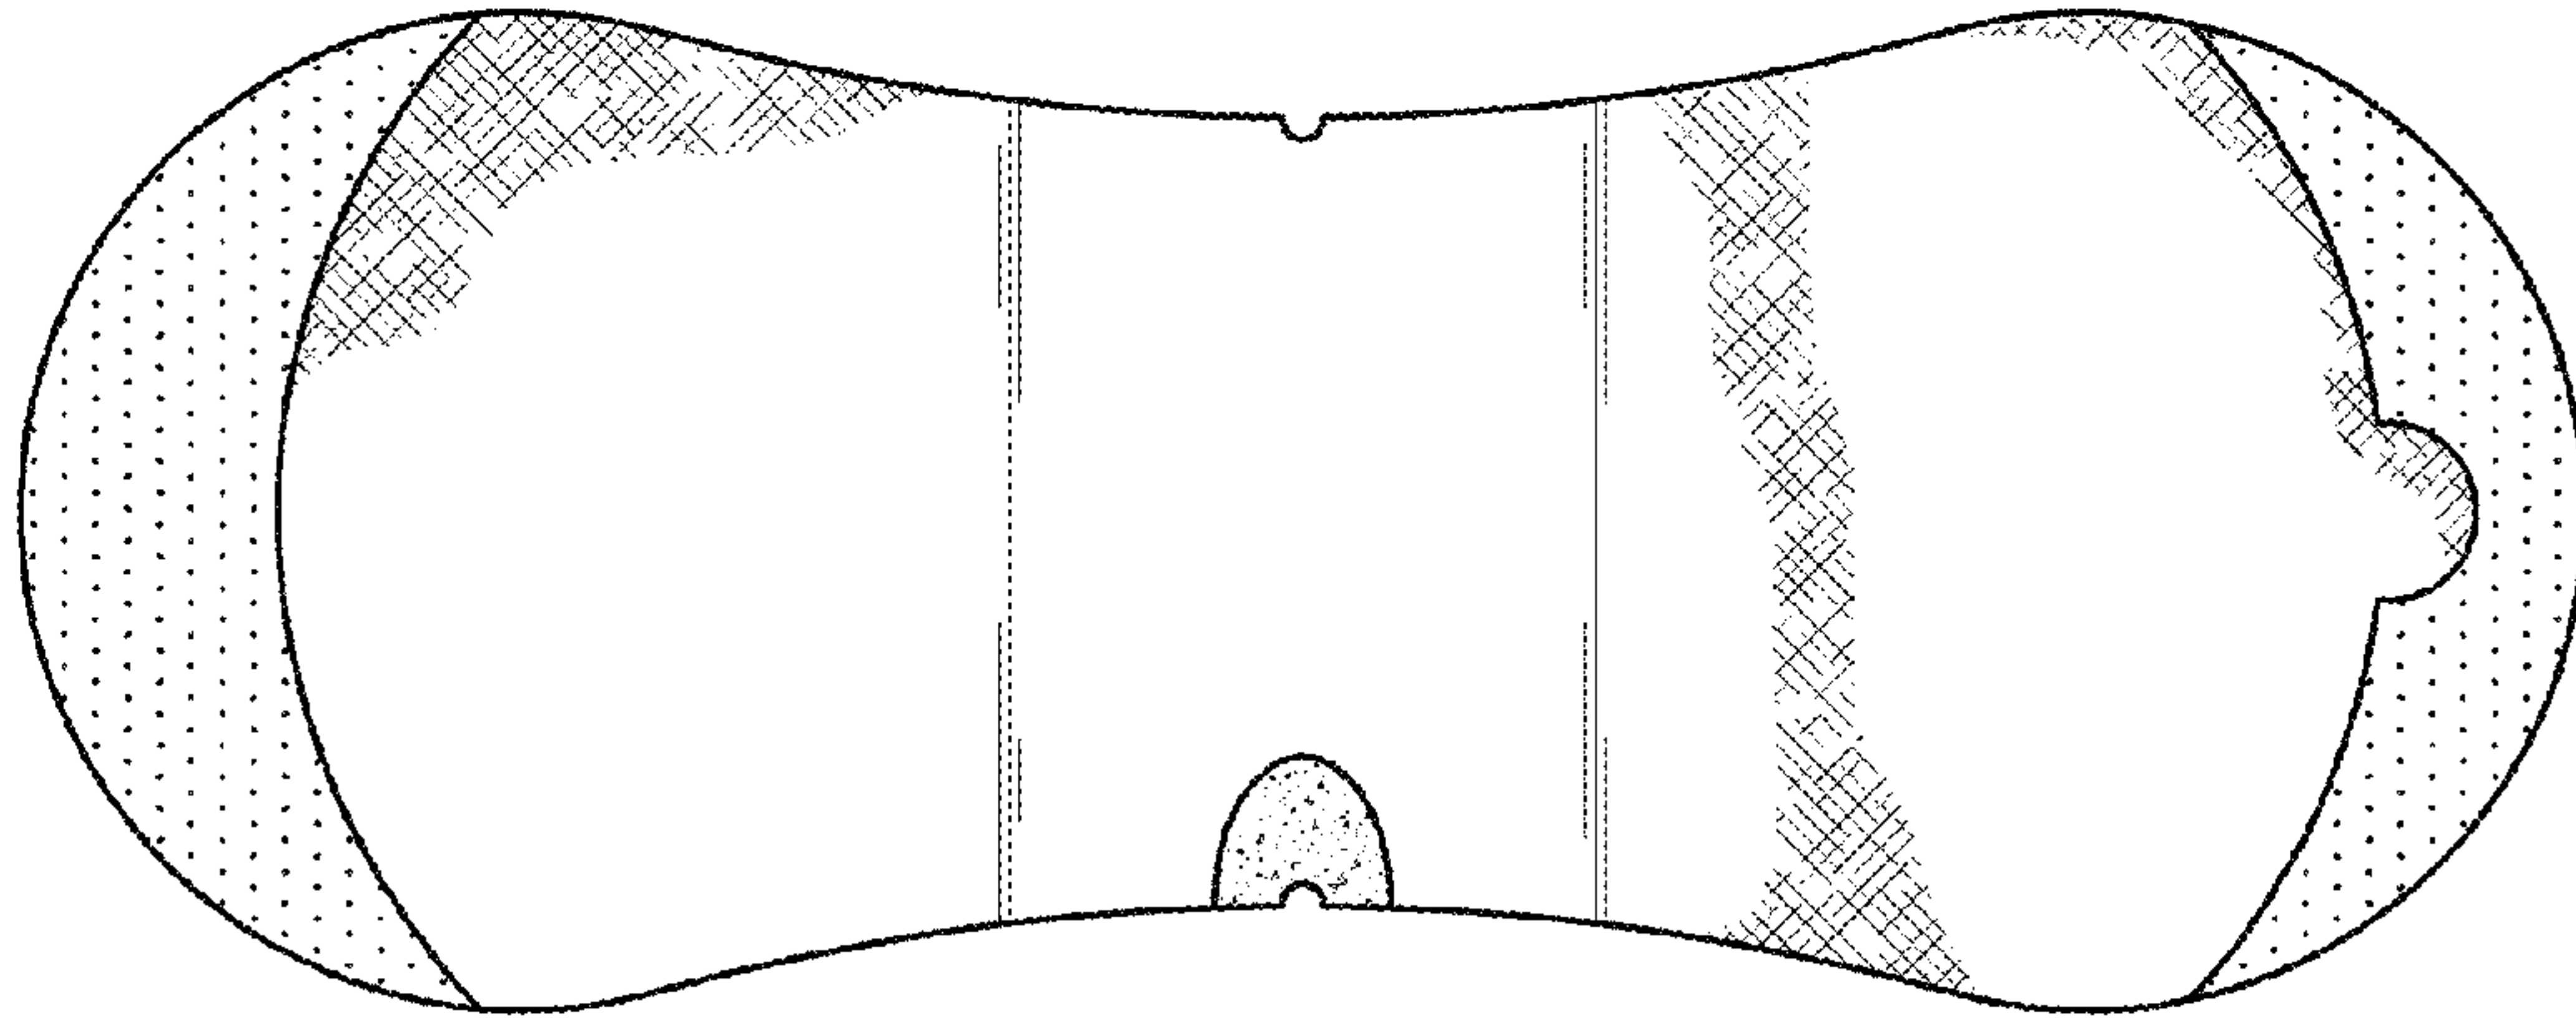


Fig. 2

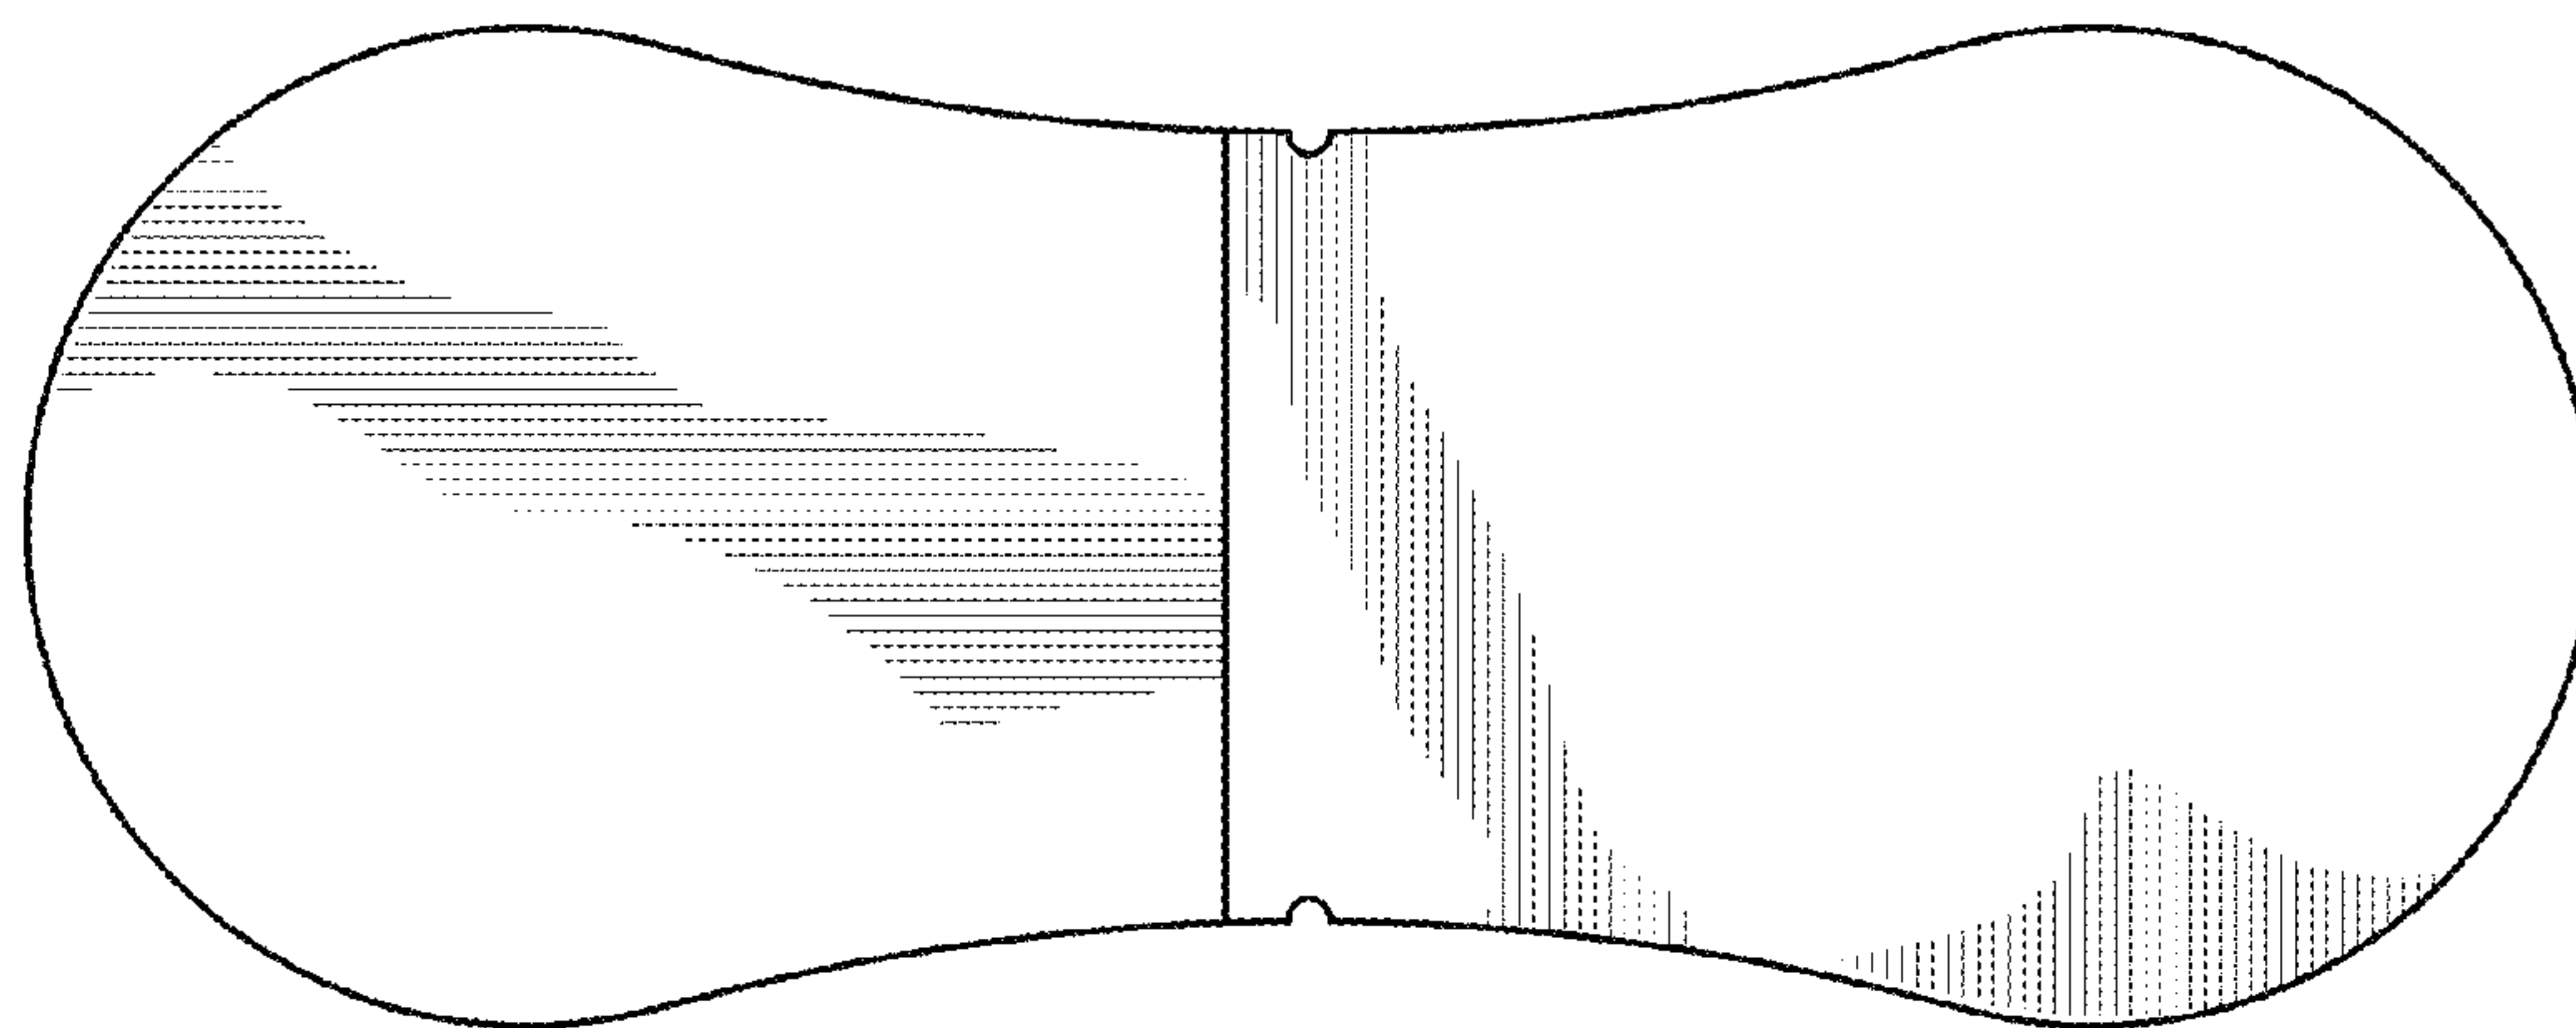


Fig. 3

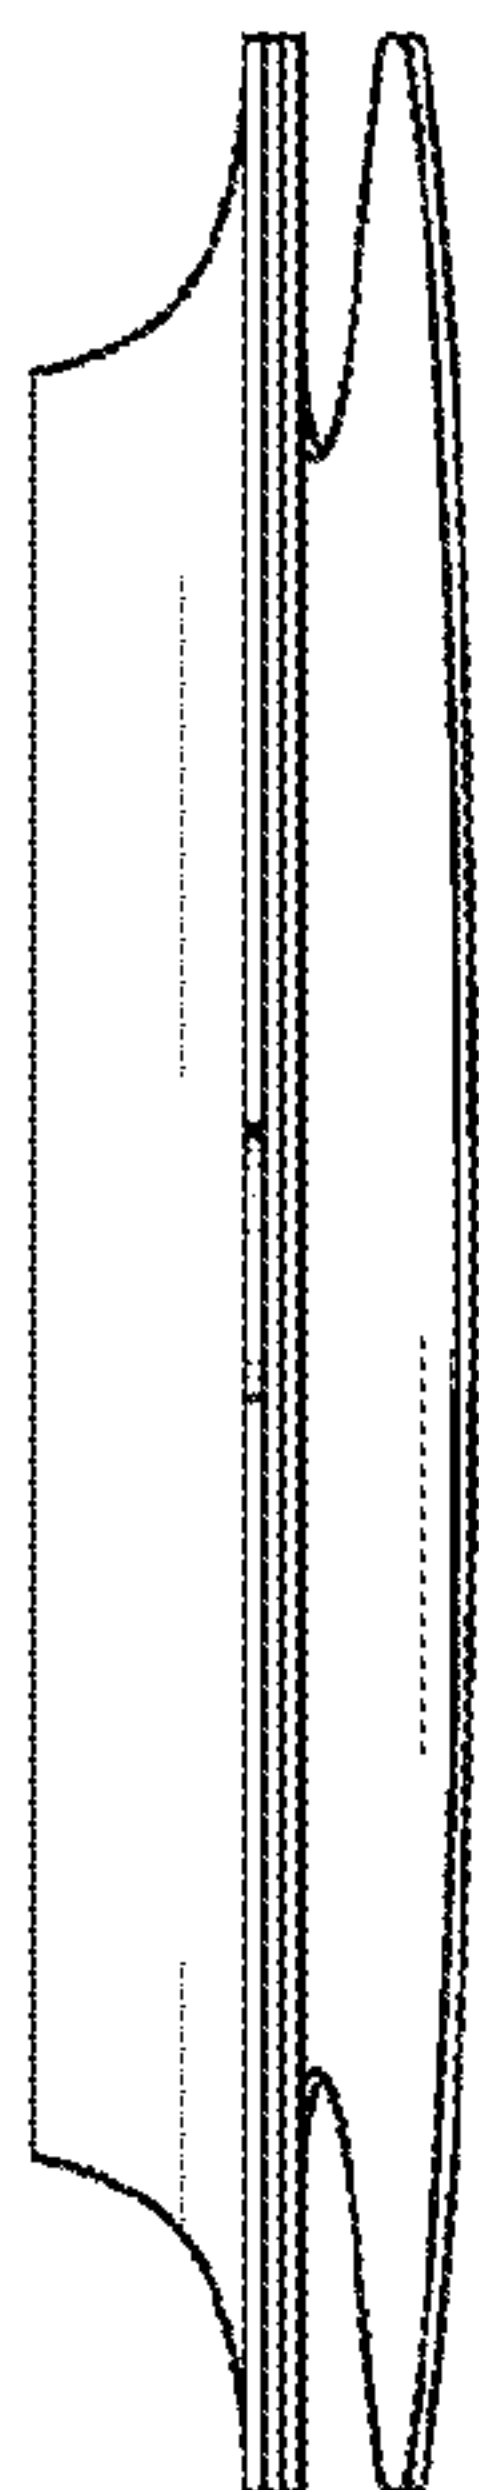


Fig. 4

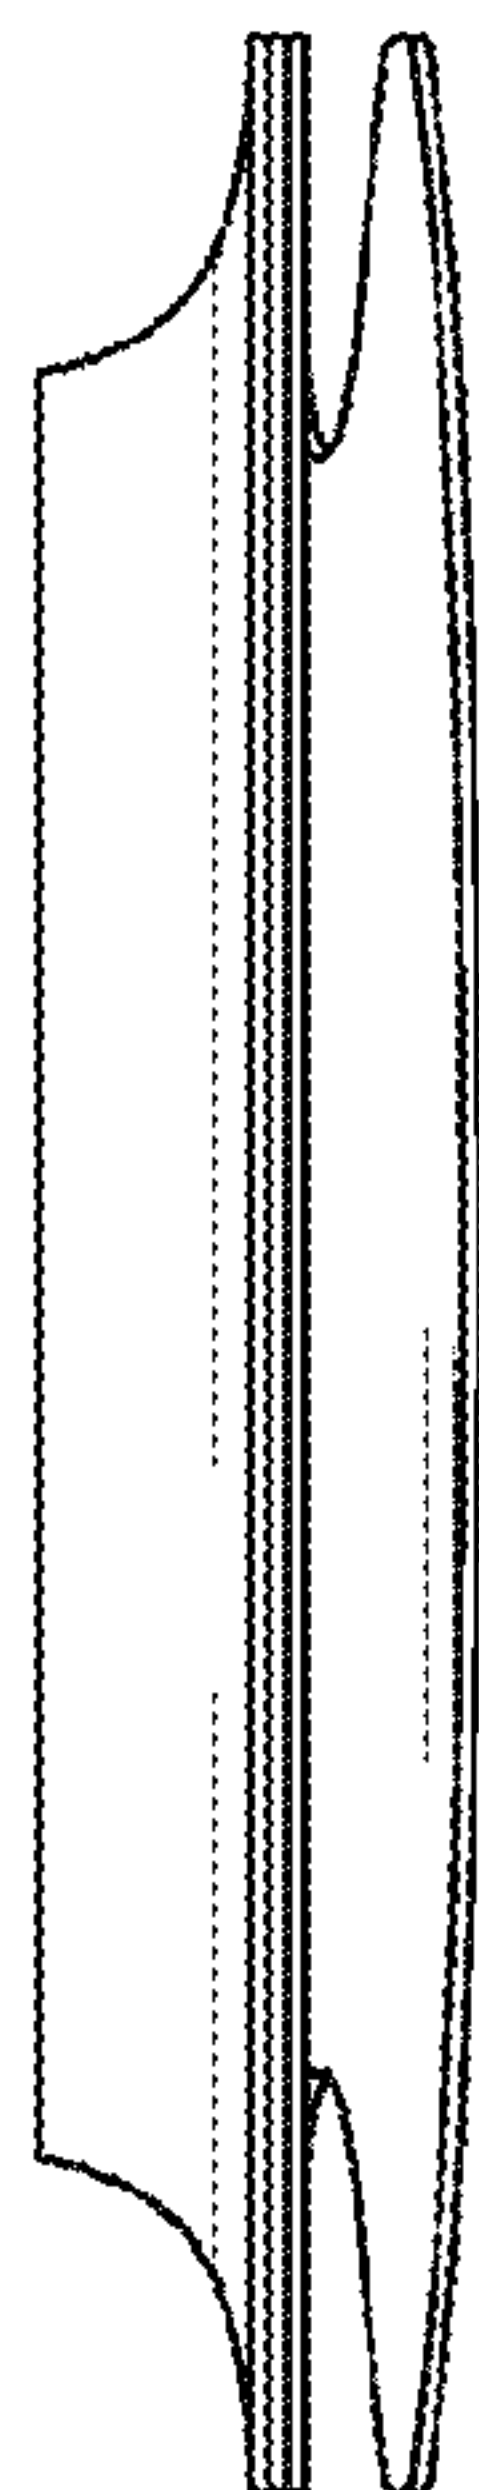


Fig. 5

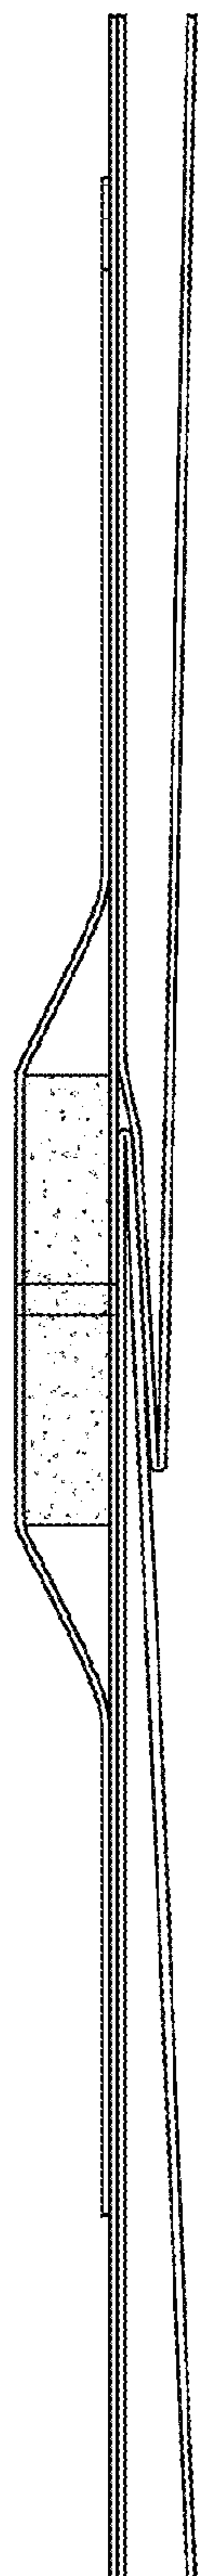


Fig. 6

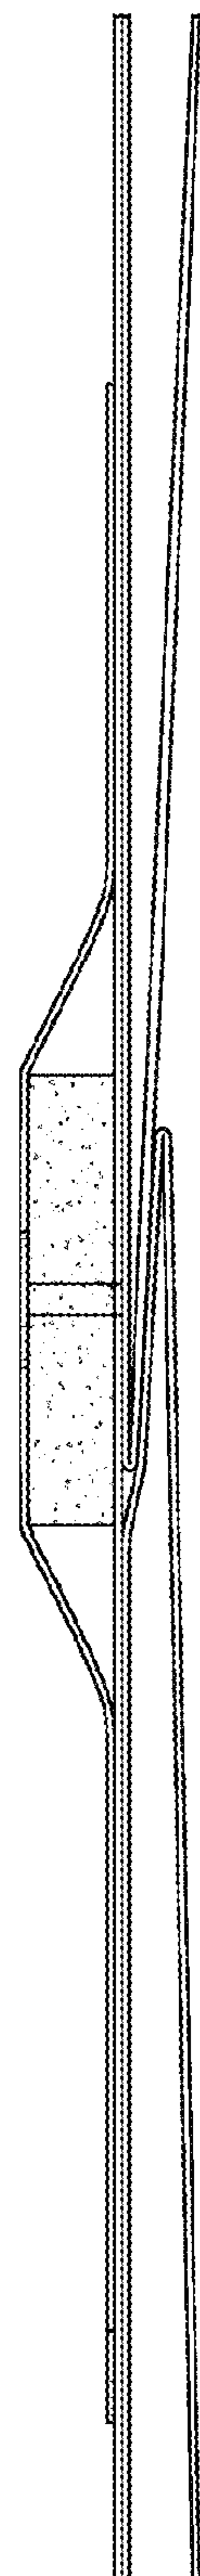


Fig. 7

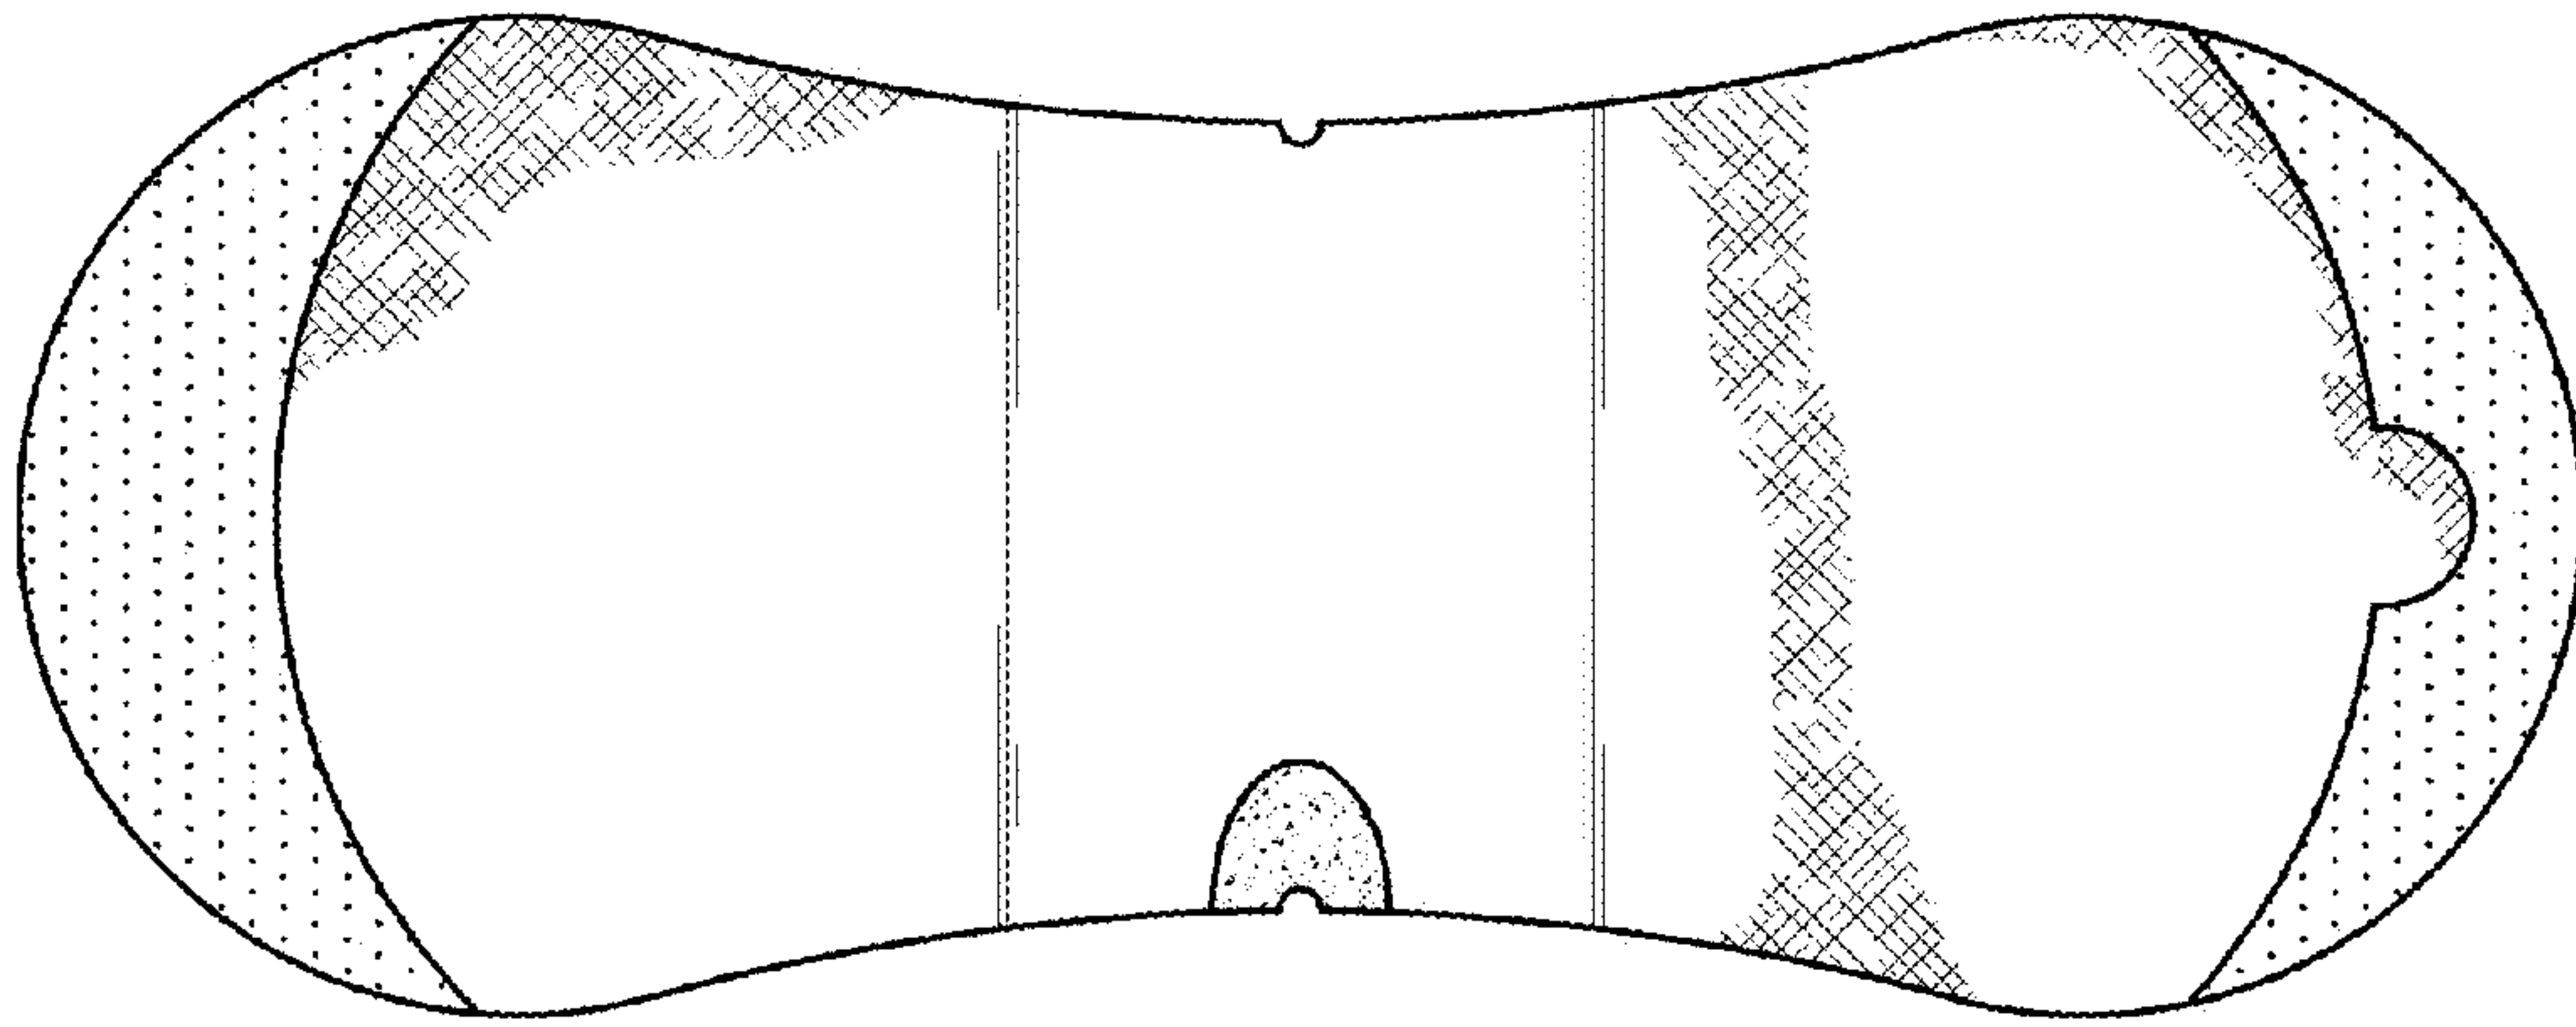


Fig. 8

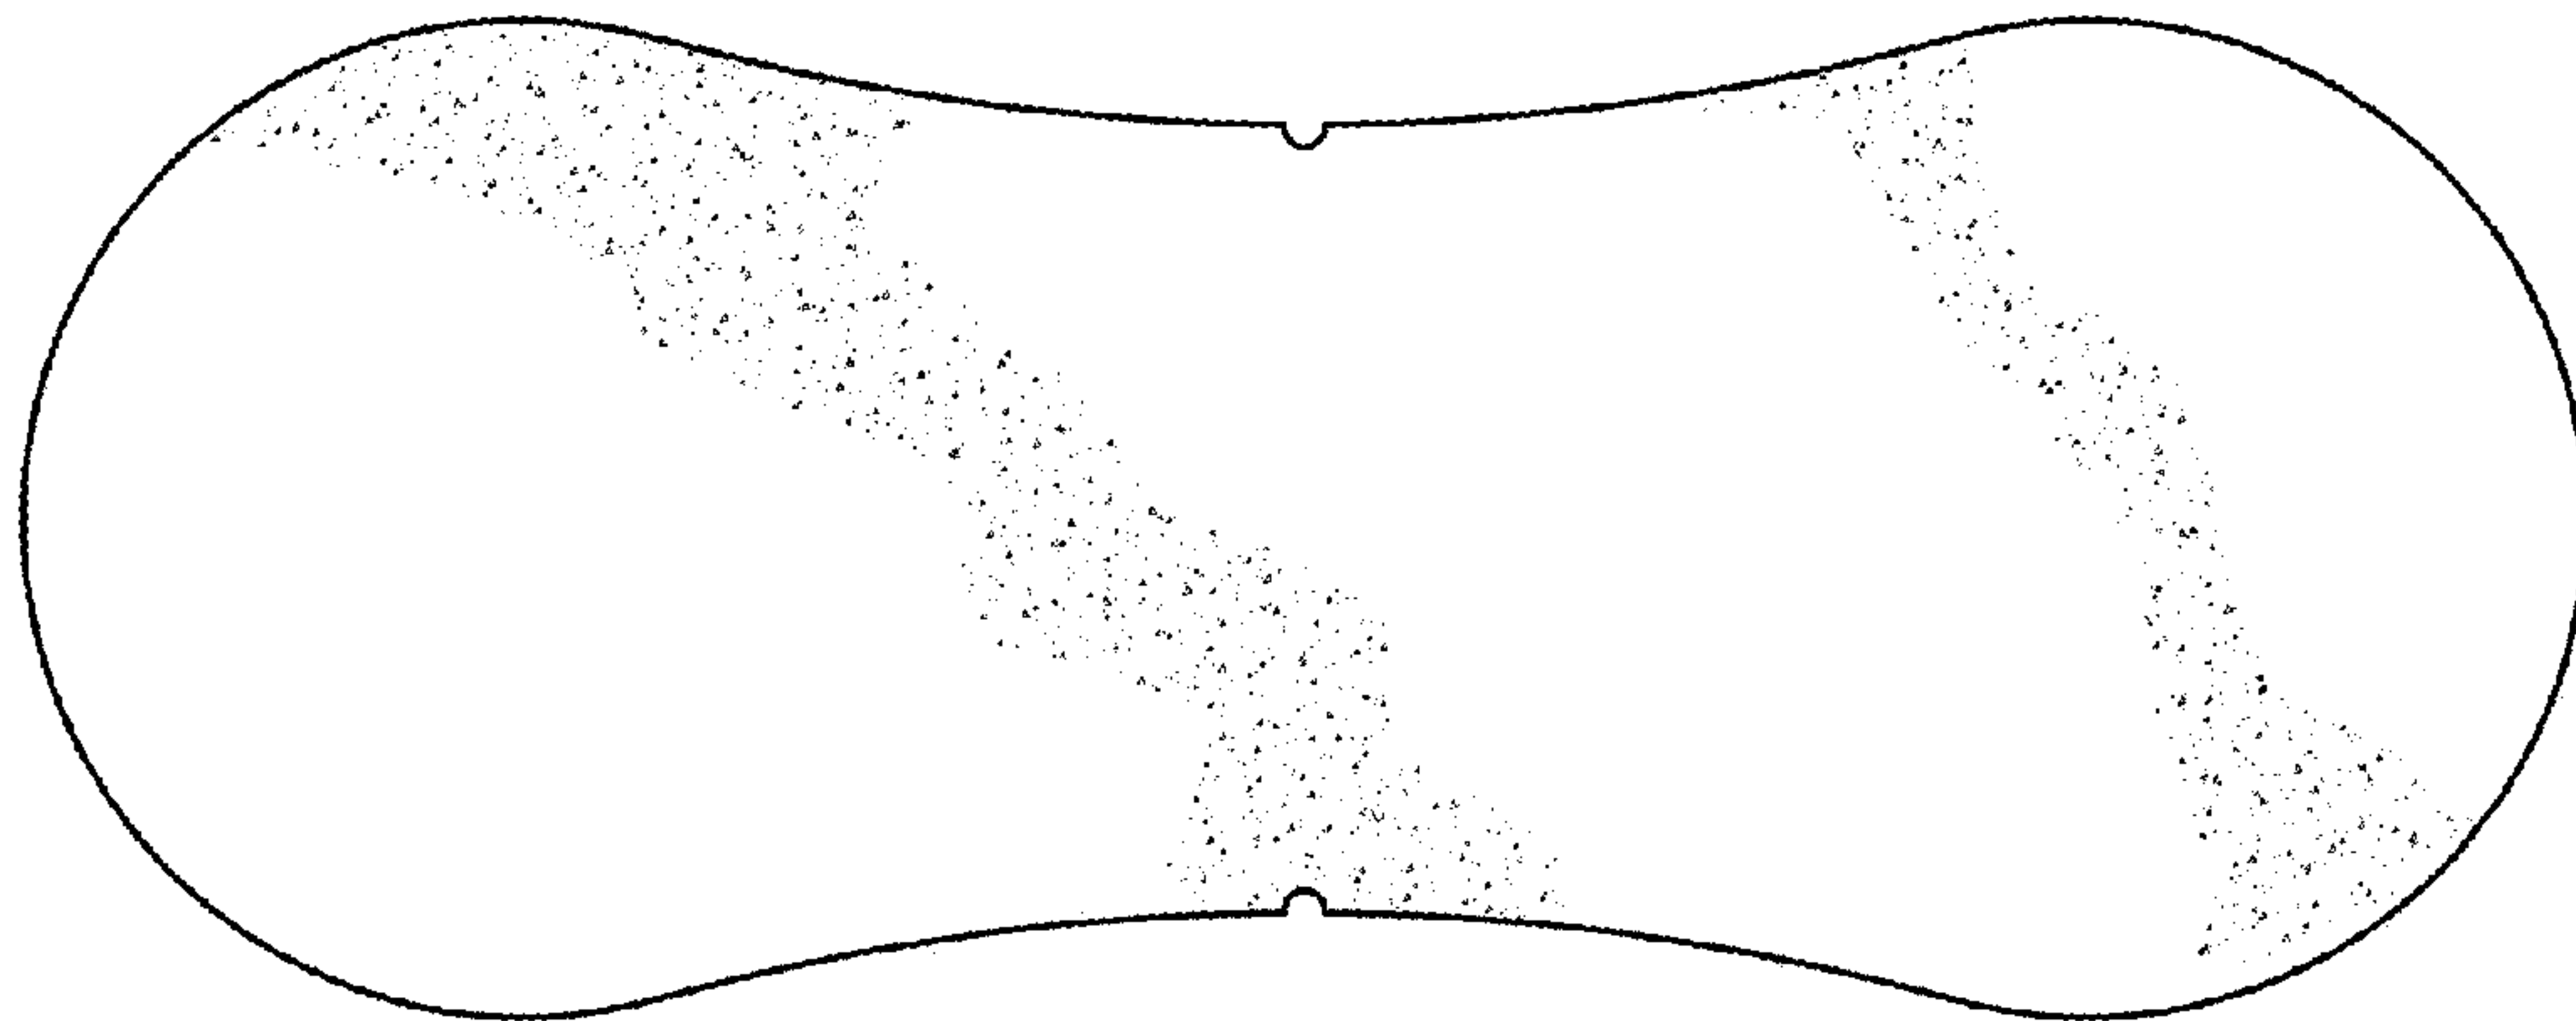


Fig. 9

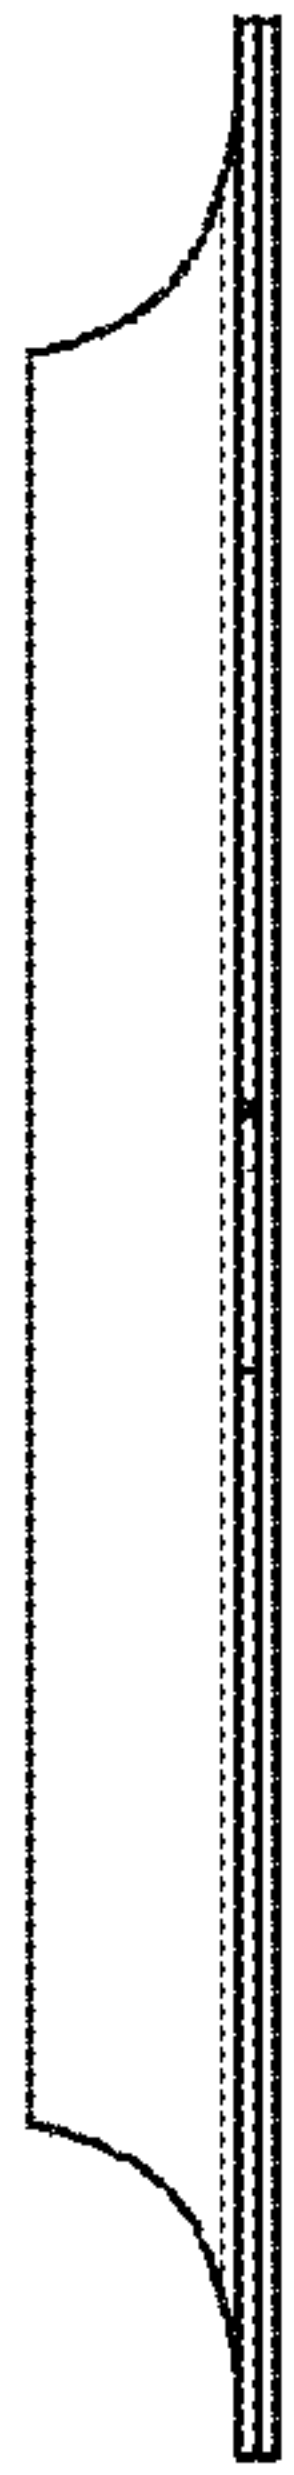


Fig. 10

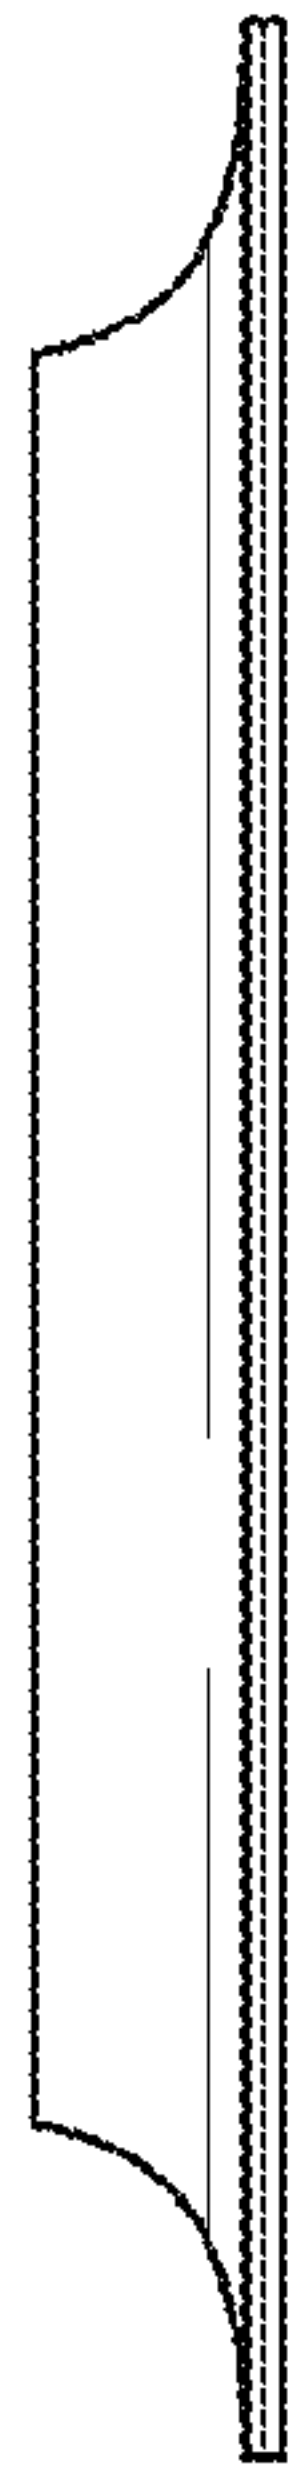


Fig. 11



Fig. 12

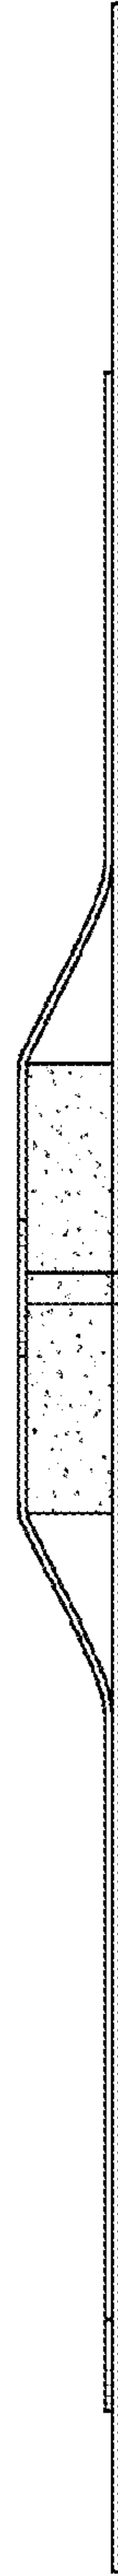


Fig. 13

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : D715,927 S
APPLICATION NO. : 29/464264
DATED : October 21, 2014
INVENTOR(S) : Kyvik et al.


Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the Title Page

---(72) Inventors: Please delete - "Scott Ryan, Ocala, FL (US)" - as an inventor---

Signed and Sealed this
Seventh Day of August, 2018

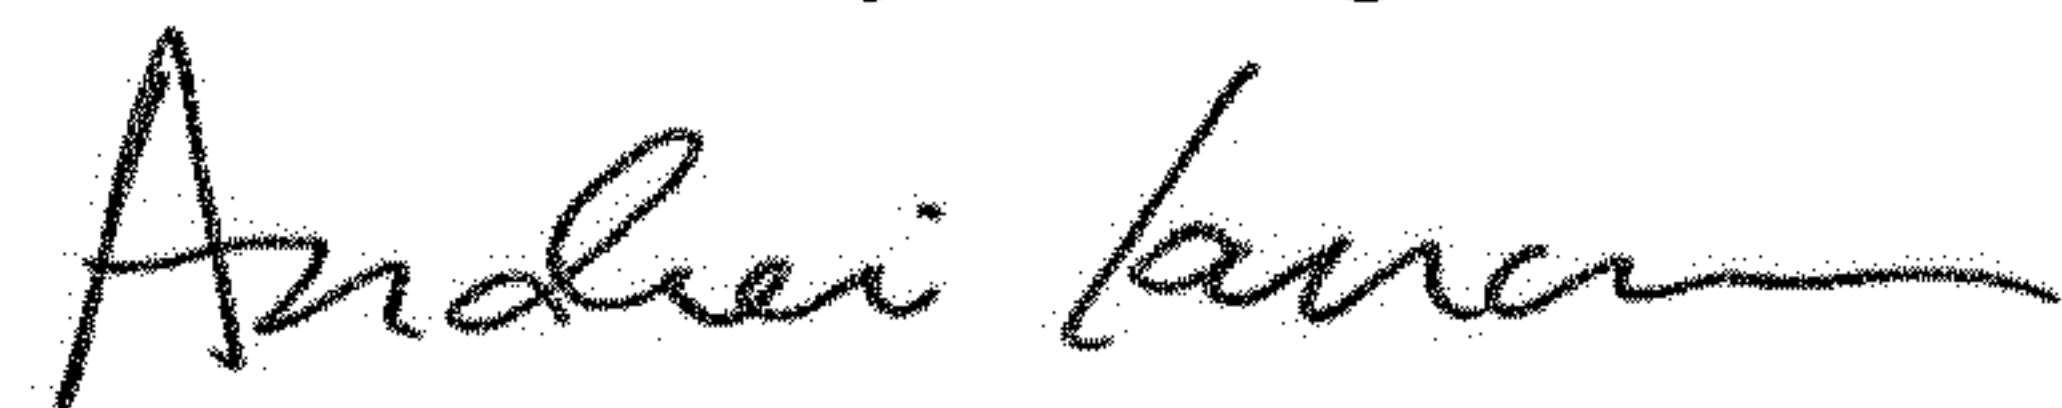

Andrei Iancu
Director of the United States Patent and Trademark Office