



US00D716375S

(12) **United States Design Patent**
Rastatter et al.

(10) **Patent No.:** **US D716,375 S**
(45) **Date of Patent:** **** Oct. 28, 2014**

(54) **MULTI-USER READING COMPREHENSION
THERAPY DEVICE**

(71) Applicant: **East Carolina University**, Greenville,
NC (US)

(72) Inventors: **Michael Rastatter**, Winterville, NC
(US); **Todd Carter**, Greenville, NC
(US); **Mark Allen**, Highlandville, MO
(US); **Ricardo Rodriguez**, Raleigh, NC
(US); **John Trainor**, Morrisville, NC
(US)

(73) Assignee: **East Carolina University**, Greenville,
NC (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/441,307**

(22) Filed: **Jan. 3, 2013**

(51) **LOC (10) Cl.** **19-07**

(52) **U.S. Cl.**
USPC **D19/60**

(58) **Field of Classification Search**

CPC G09B 21/00; G09B 21/006; G09B 19/04;
G09B 5/00; G09B 5/04; G09B 5/08–5/14;
G09B 17/00–17/04; H02G 3/08
USPC D19/59–64; 434/112, 116, 320,
434/178–179, 185; D13/147, 152;
D14/158, 229, 240; 174/53; 220/3.2

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D303,246	S	*	9/1989	Freeman et al.		D13/147
D372,703	S	*	8/1996	Hannon et al.		D13/152
D461,453	S	*	8/2002	Chen		D13/147
D462,953	S	*	9/2002	Jang		D14/299
D462,954	S	*	9/2002	Chen		D14/299

(Continued)

OTHER PUBLICATIONS

Declaration of Facts Describing Field Test of Prototype, executed
Jan. 28, 2013, 3 pages.

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Myers Bigel Sibley &
Sajovec, PA

(57) **CLAIM**

The ornamental design for a multi-user reading comprehen-
sion therapy device, as shown and described.

DESCRIPTION

FIG. 1 is a side perspective view of a multi-user reading
comprehension therapy device, showing our design;

FIG. 2 is a top view thereof;

FIG. 3 is a front view thereof;

FIG. 4 is a bottom view thereof;

FIG. 5 is a rear view thereof;

FIG. 6 is a side view thereof;

FIG. 7 is an opposing side view thereof;

FIG. 8 is a front perspective environmental view thereof;

FIG. 9 is a top side different environmental view thereof;

FIG. 10 is a side perspective view of a second embodiment of
a multi-user reading comprehension therapy device, showing
our design;

FIG. 11 is a top view thereof;

FIG. 12 is a front view thereof;

FIG. 13 is a bottom view thereof;

FIG. 14 is a rear view thereof;

FIG. 15 is a side view thereof;


FIG. 16 is an opposing side view thereof;

FIG. 17 is a front perspective environmental view thereof;
and,

FIG. 18 is a top side different environmental view thereof.

The broken lines in the drawings are for purposes of illustrat-
ing portions of the multi-user reading comprehension therapy
device, as well as environmental structure, which form no part
of the claimed design.

1 Claim, 10 Drawing Sheets

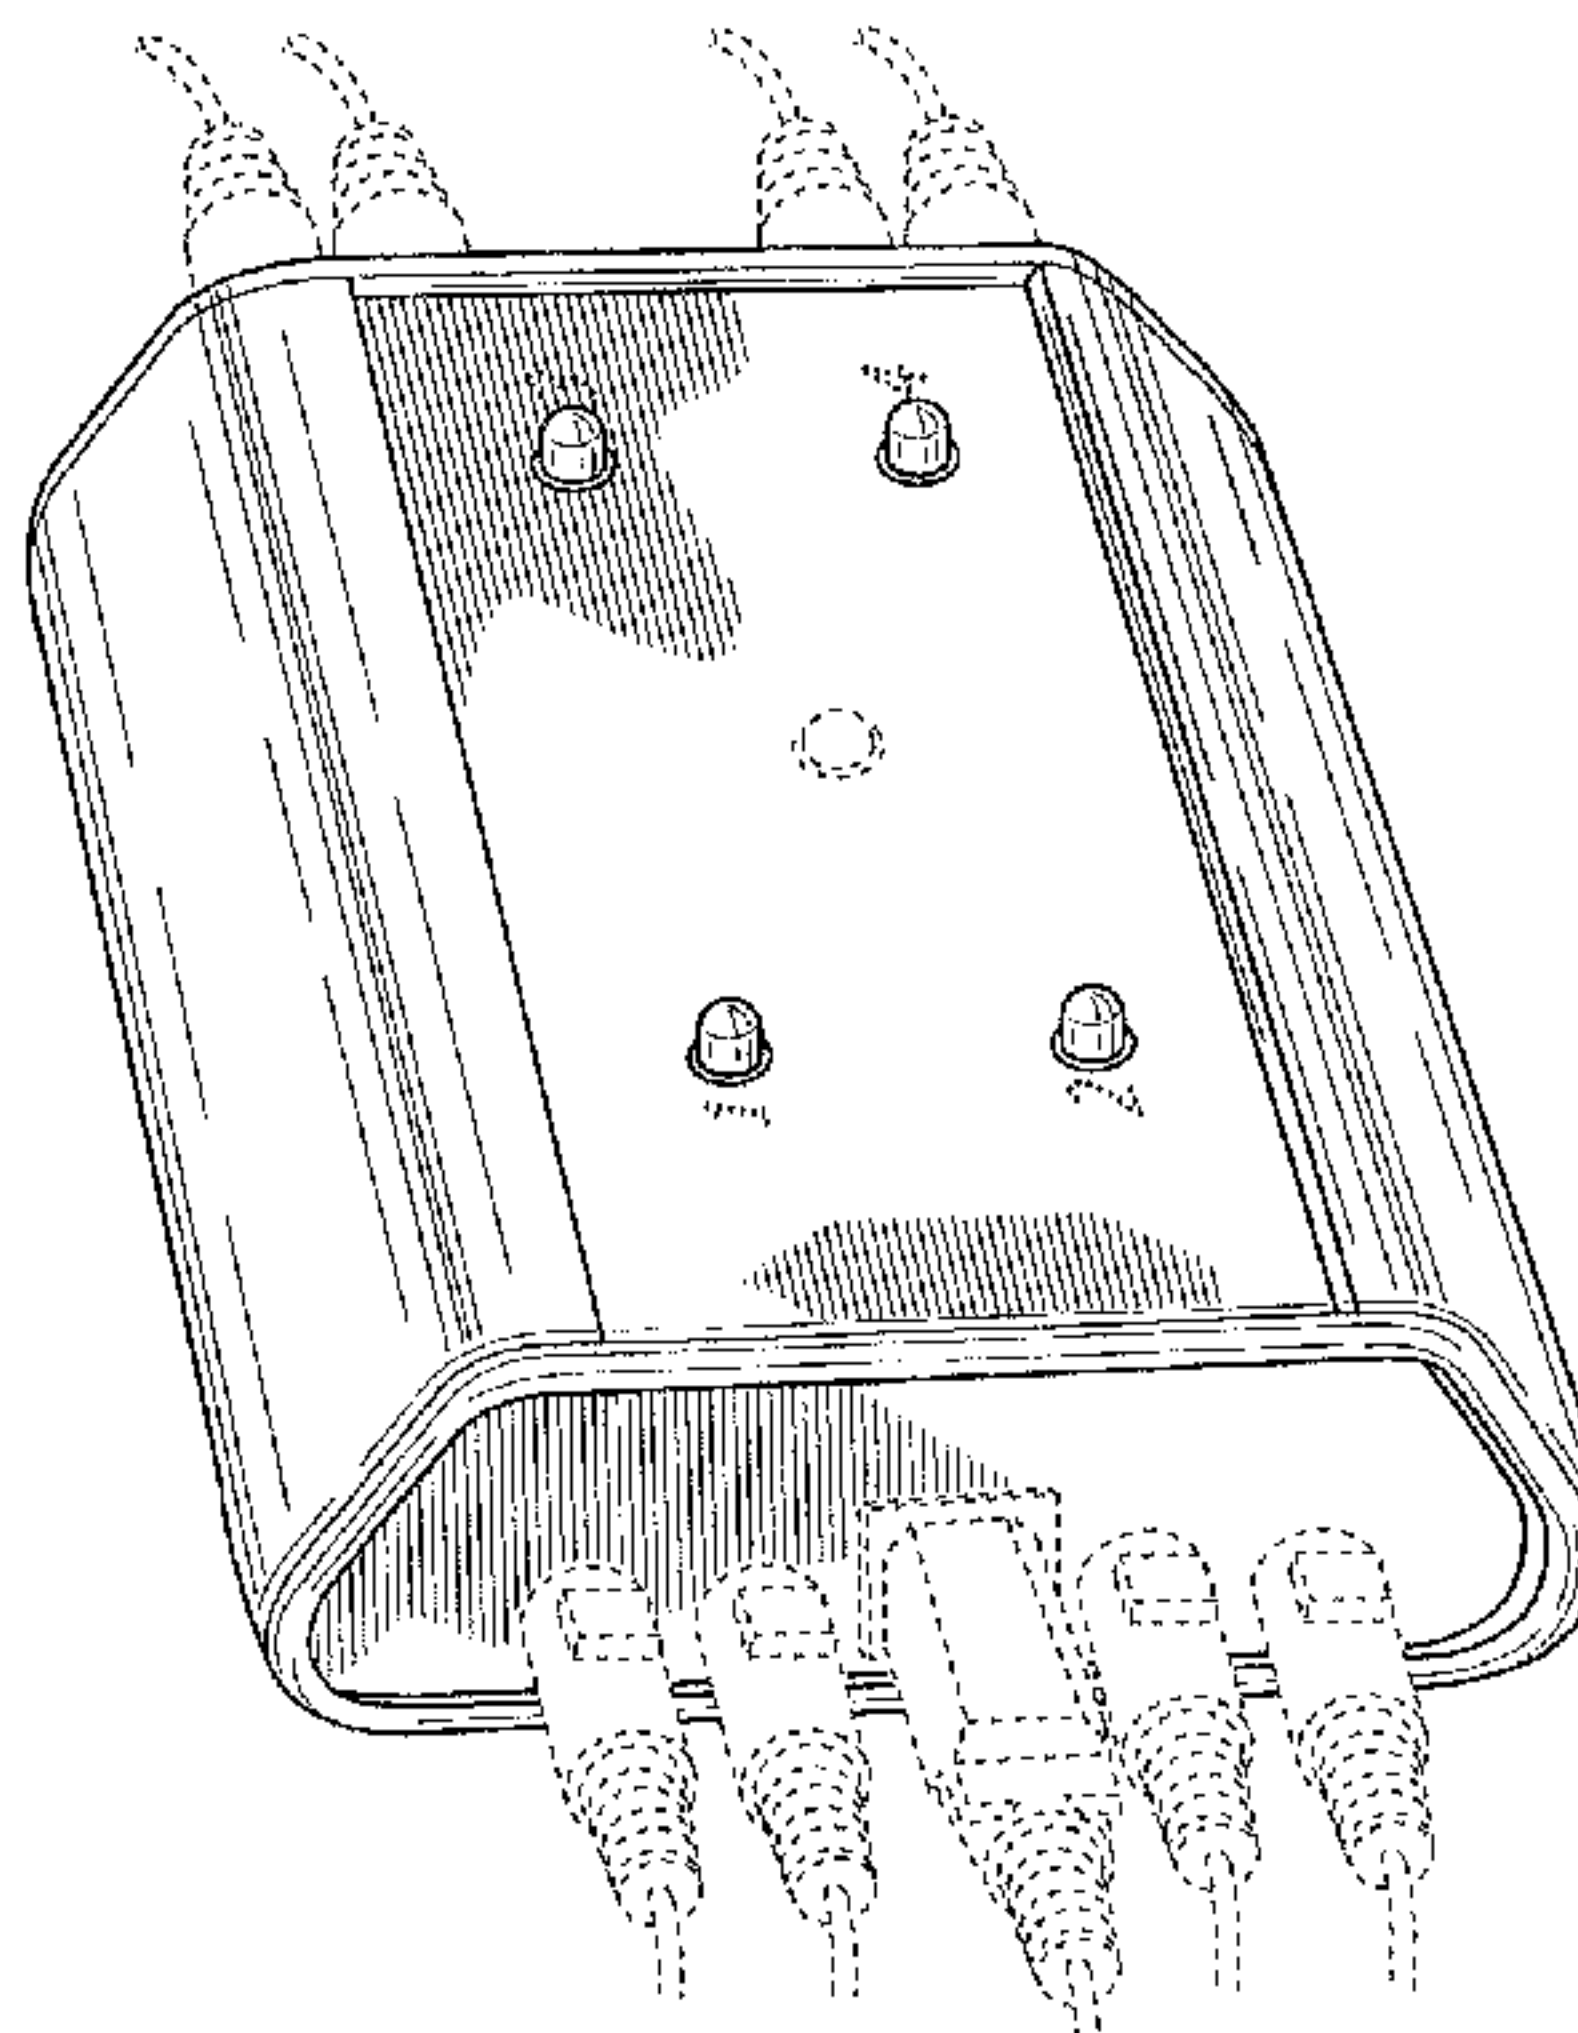

(56)

References Cited

U.S. PATENT DOCUMENTS

D485,830 S * 1/2004 Chen D14/240

D487,074 S * 2/2004 McGoldrick D14/158

D503,384 S * 3/2005 Weatherley D13/147

D521,504 S * 5/2006 Nagel et al. D14/240

D531,129 S * 10/2006 Muto D13/152

D545,768 S * 7/2007 Hsu D13/147

D553,572 S * 10/2007 Yi et al. D13/147

D566,045 S * 4/2008 Chang D13/147

D595,239 S * 6/2009 Inoue et al. D13/158

D600,213 S * 9/2009 Inoue et al. D13/158

7,828,712 B2 11/2010 Rastatter et al.

D699,299 S * 2/2014 Bruker D19/60

* cited by examiner

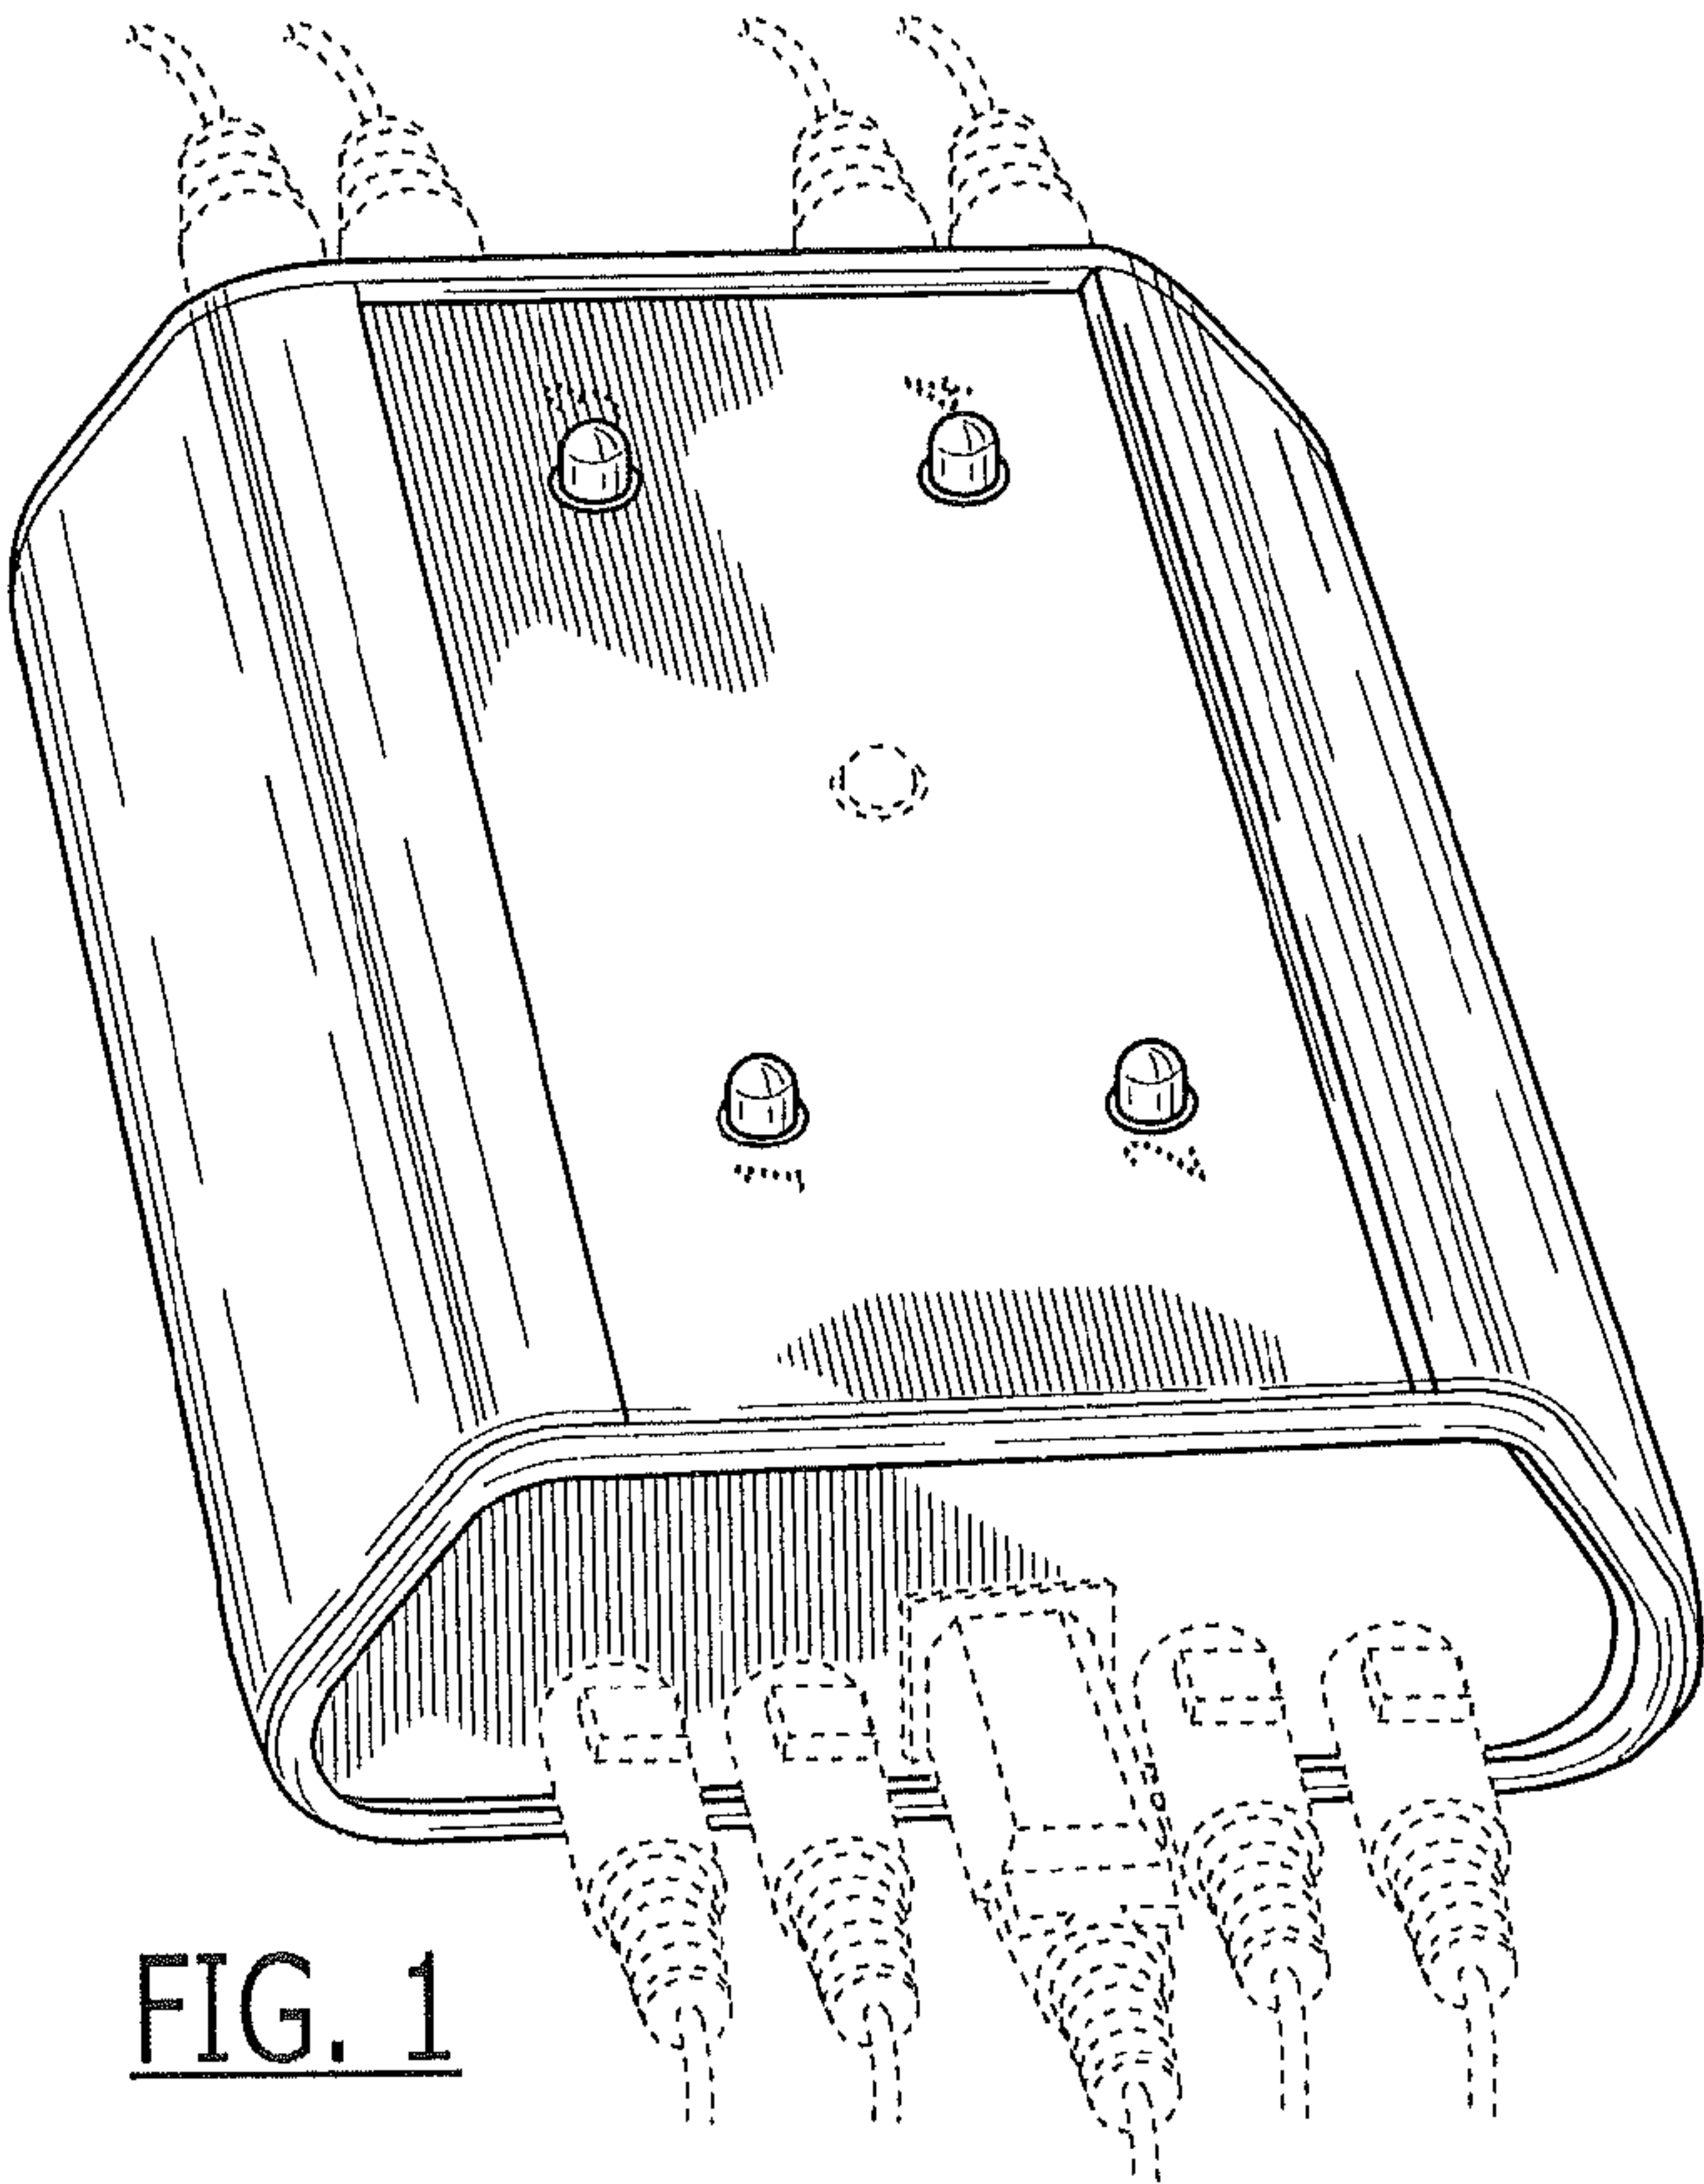


FIG. 1

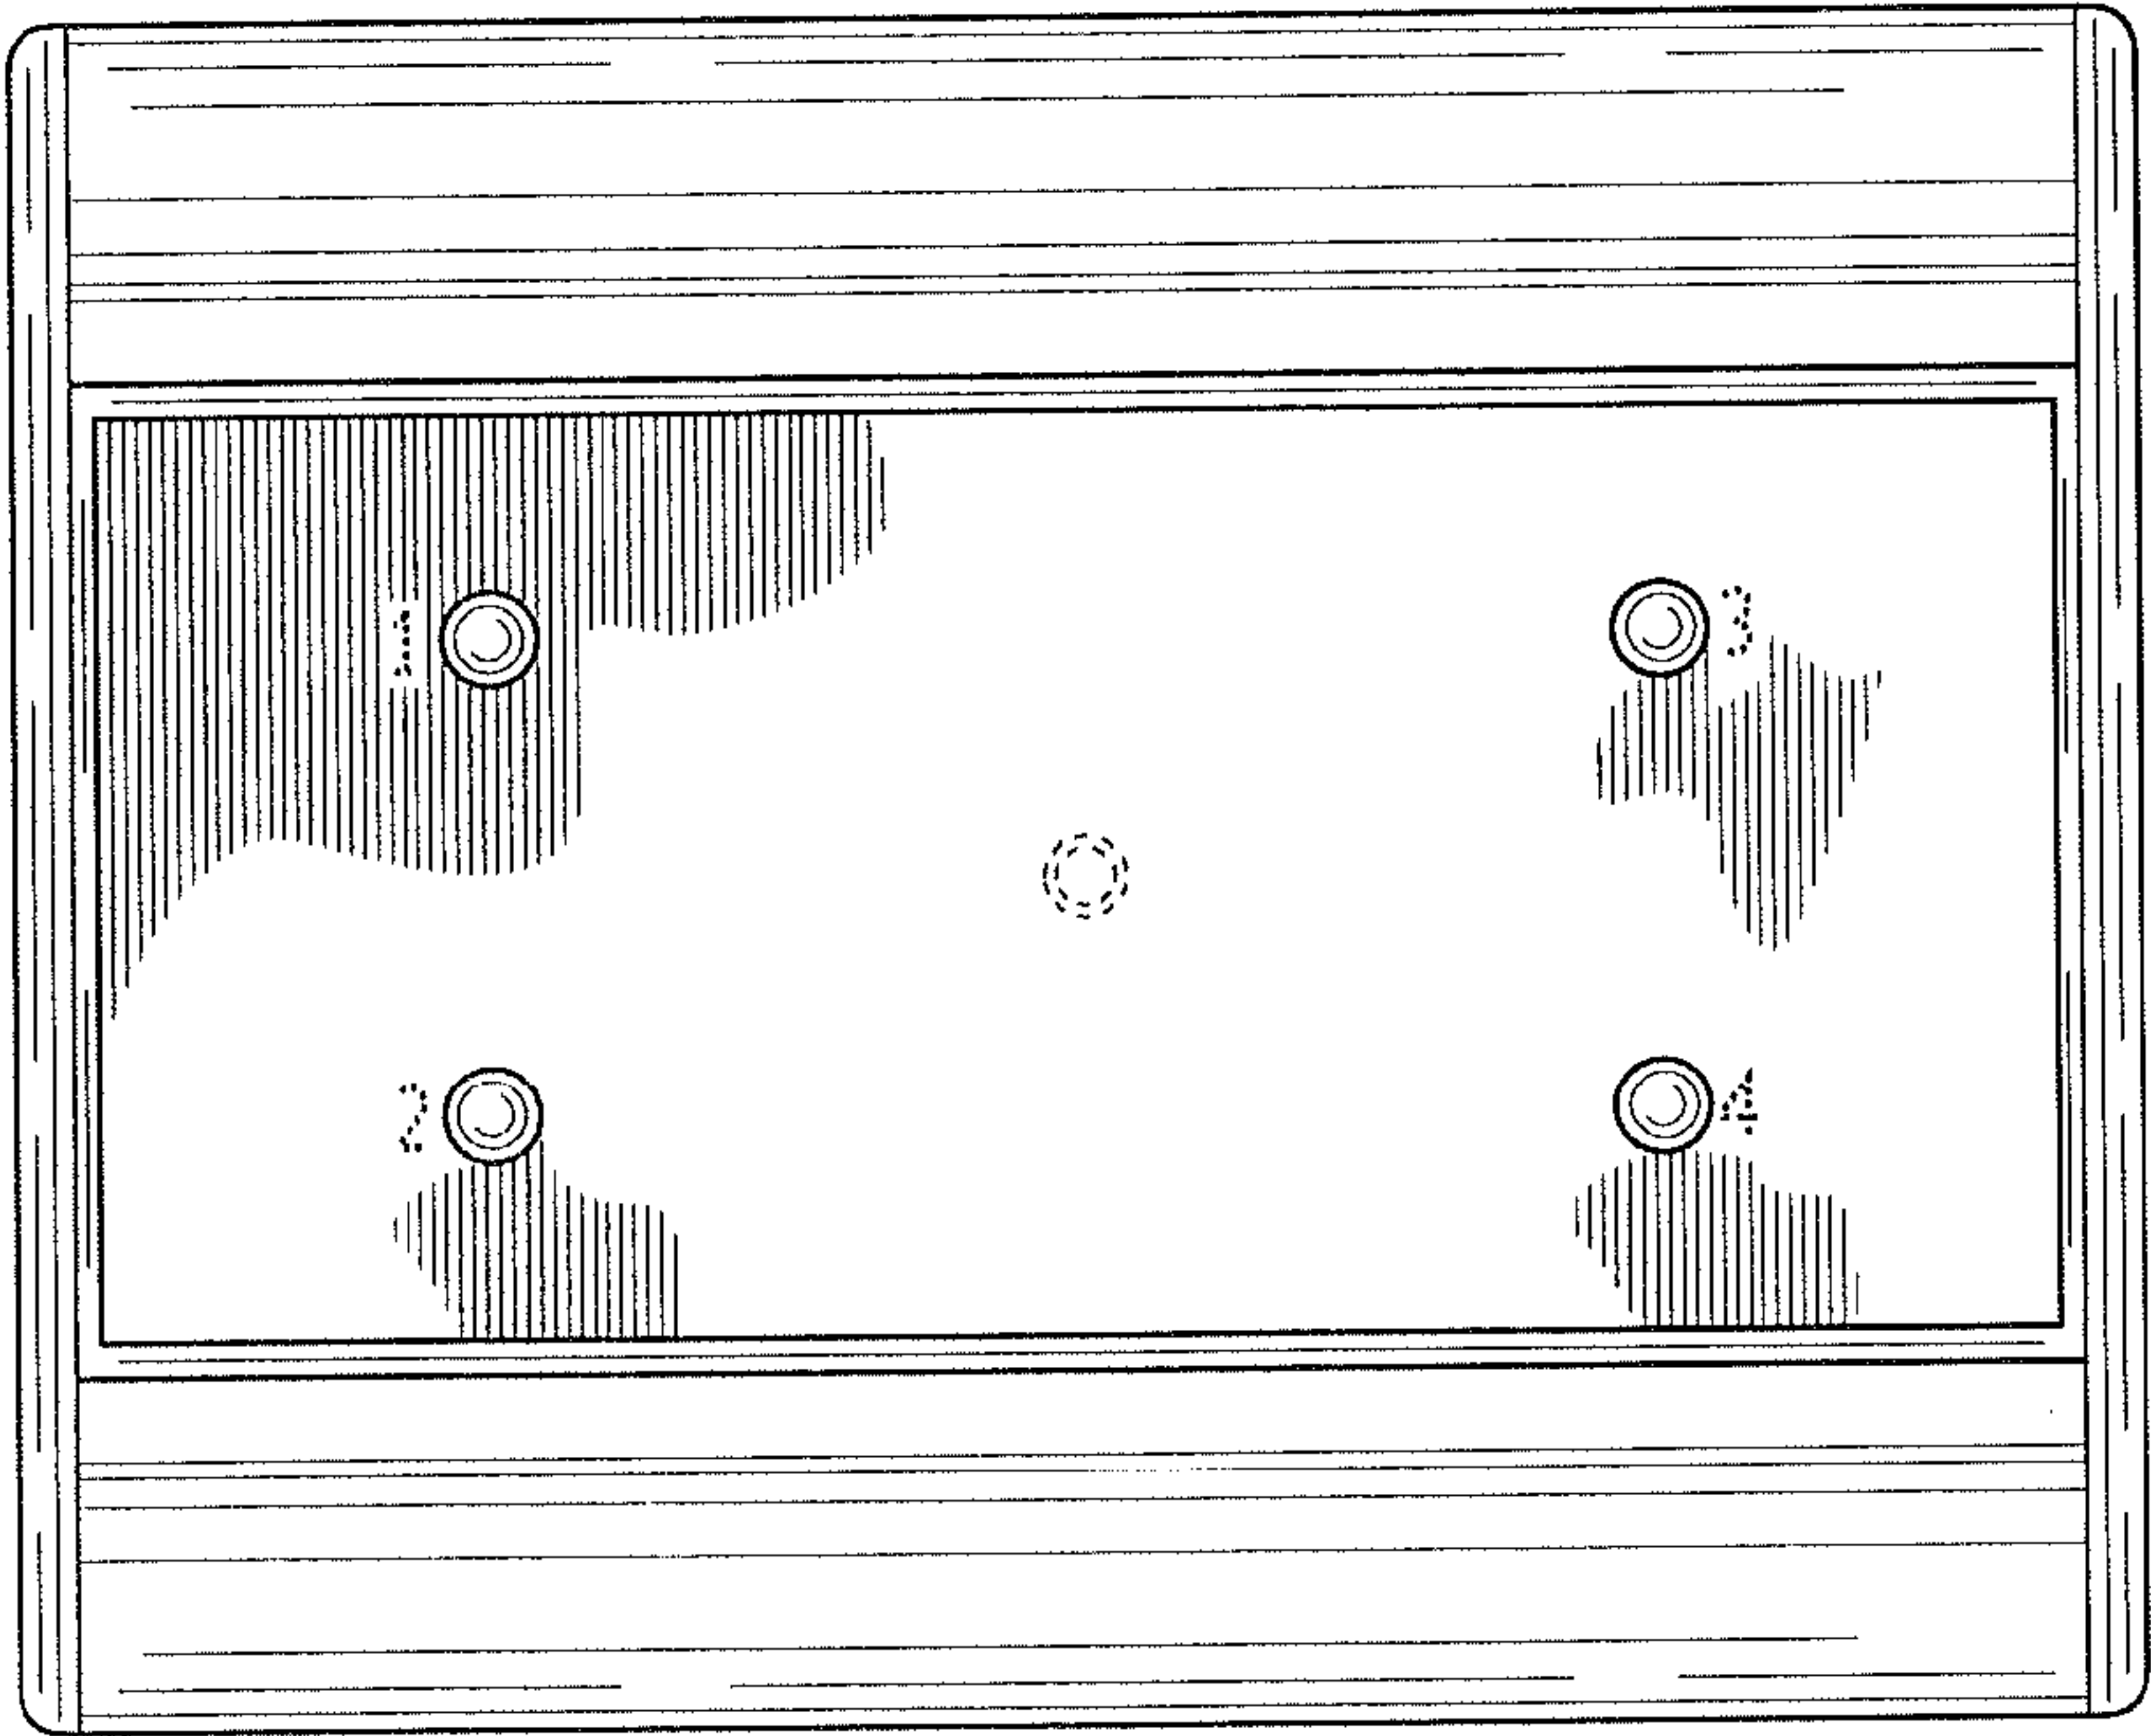


FIG. 2

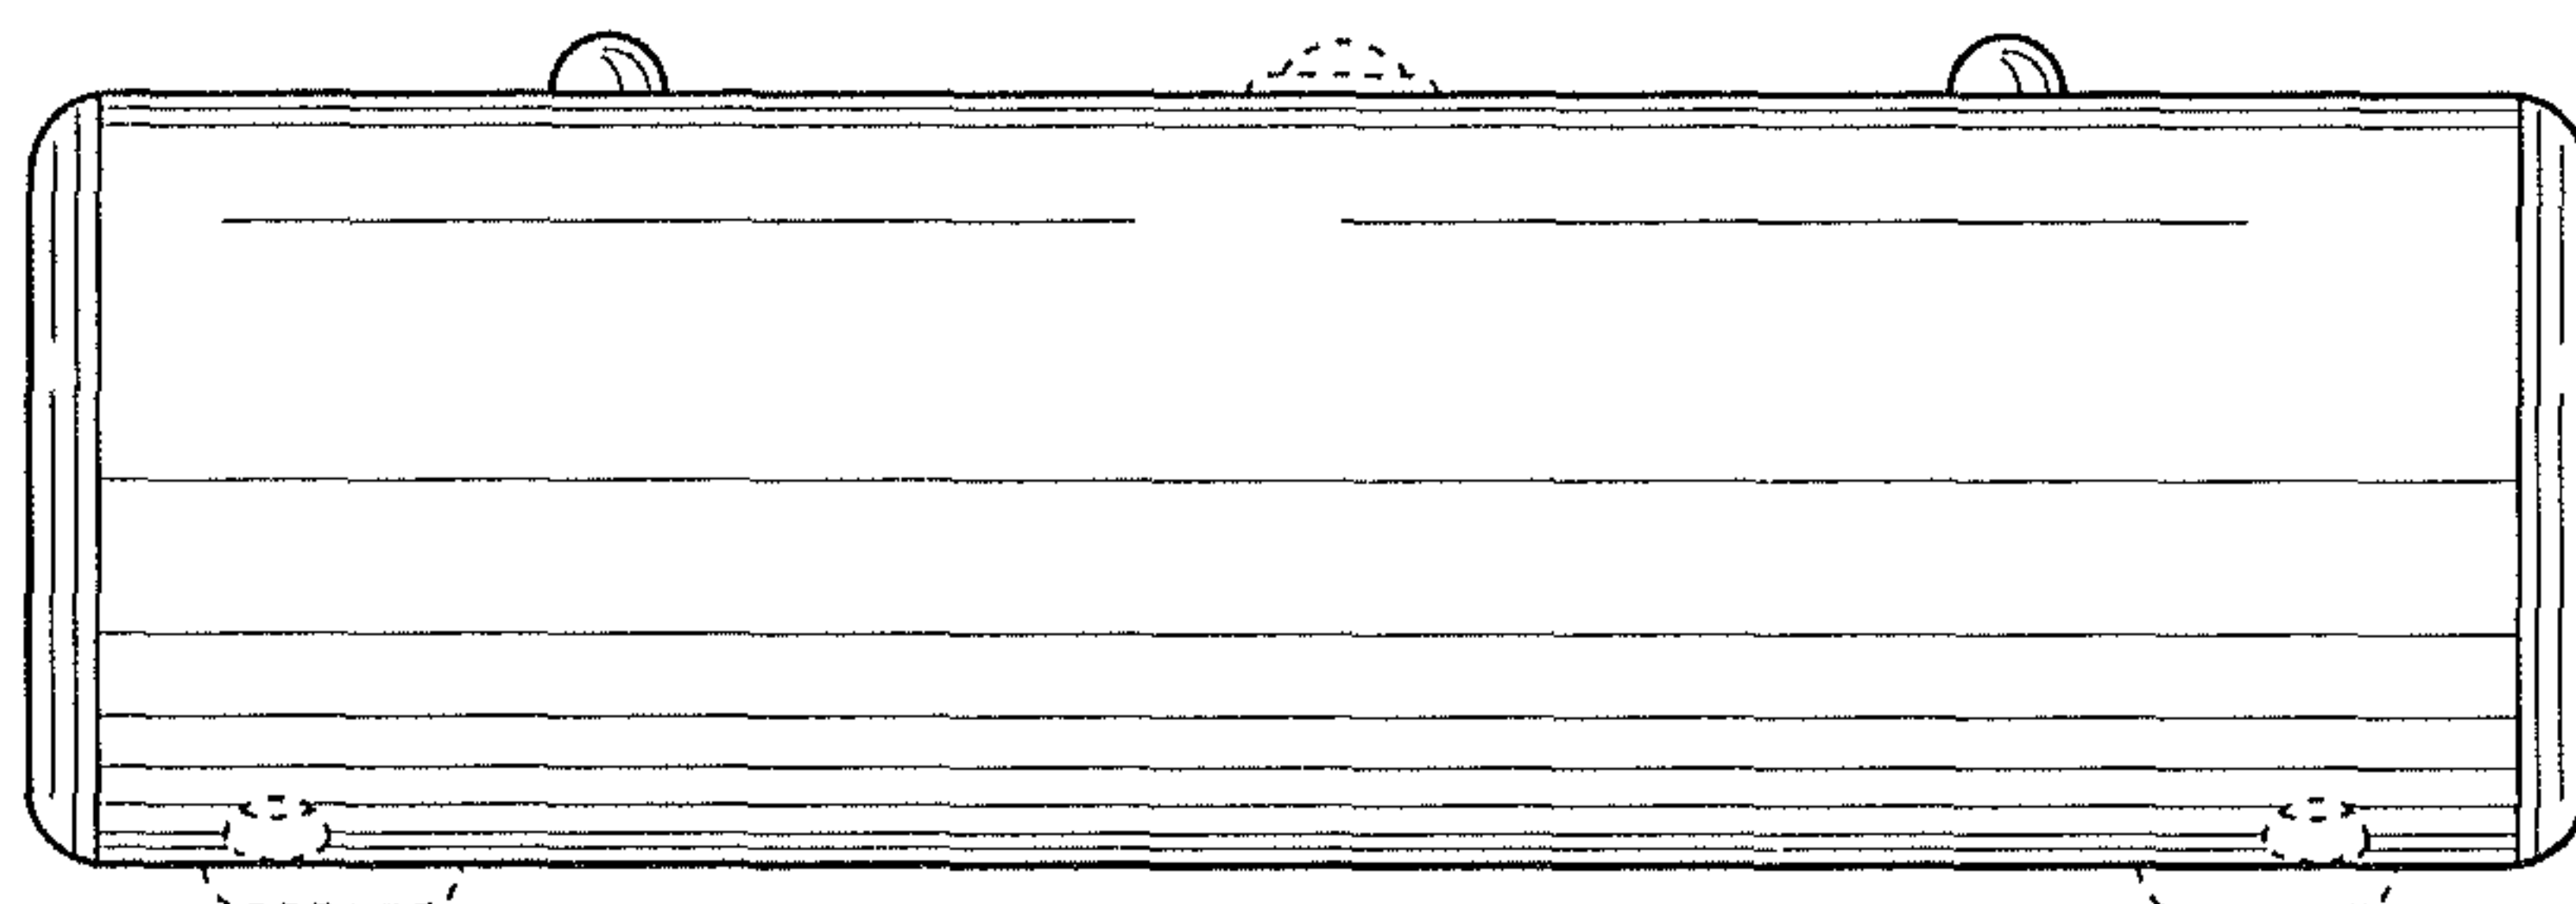


FIG. 3

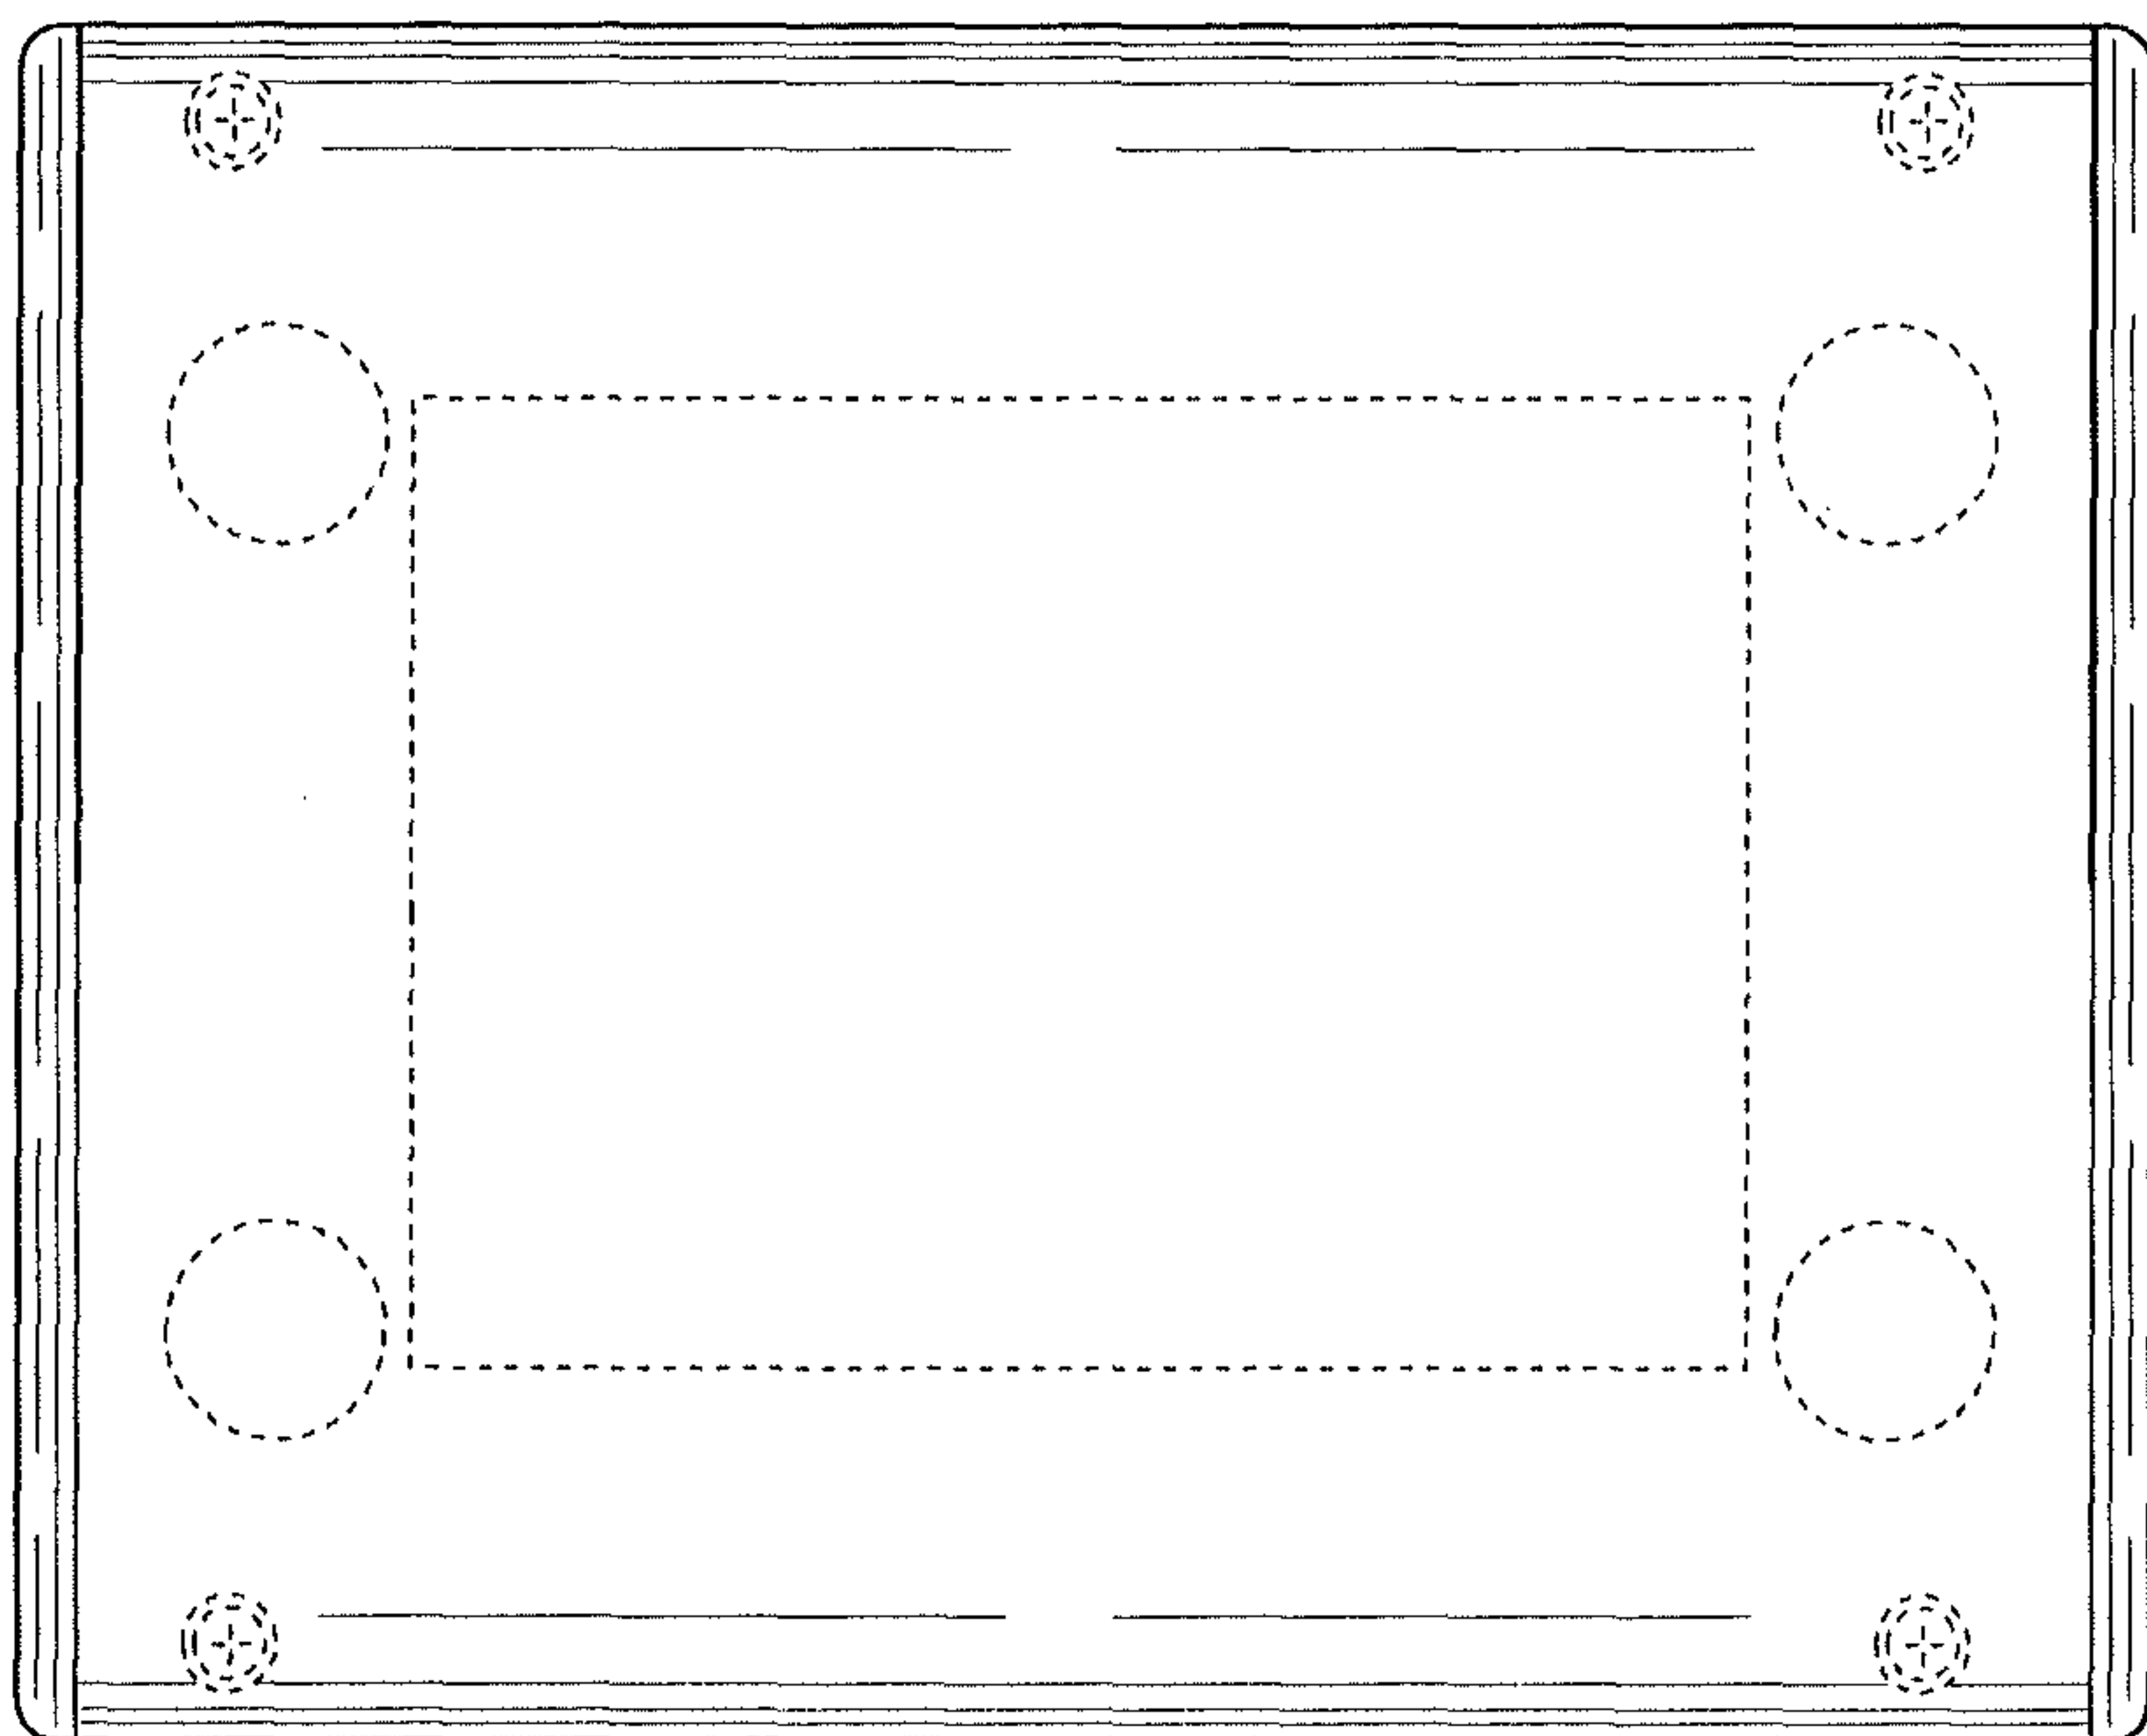


FIG. 4

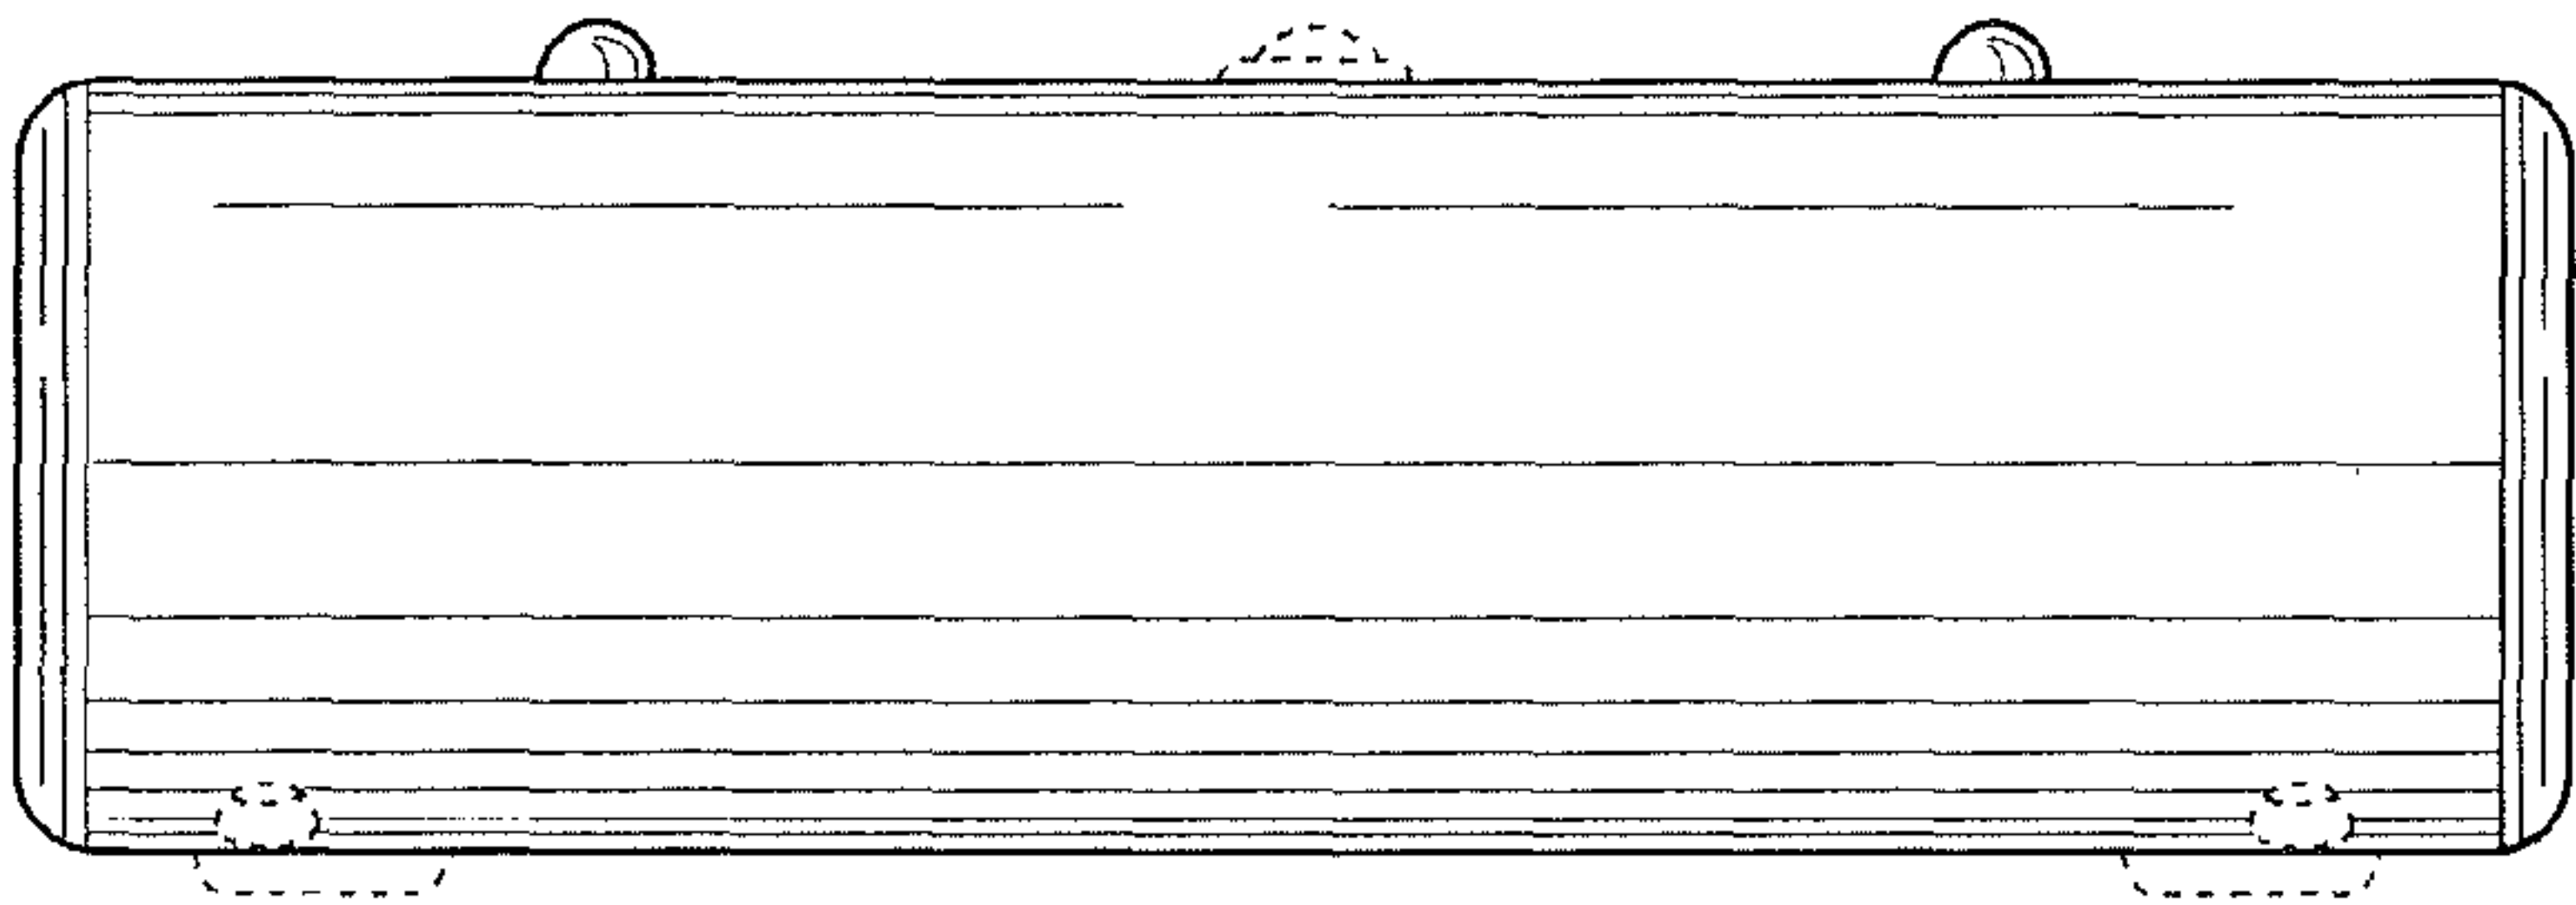


FIG. 5

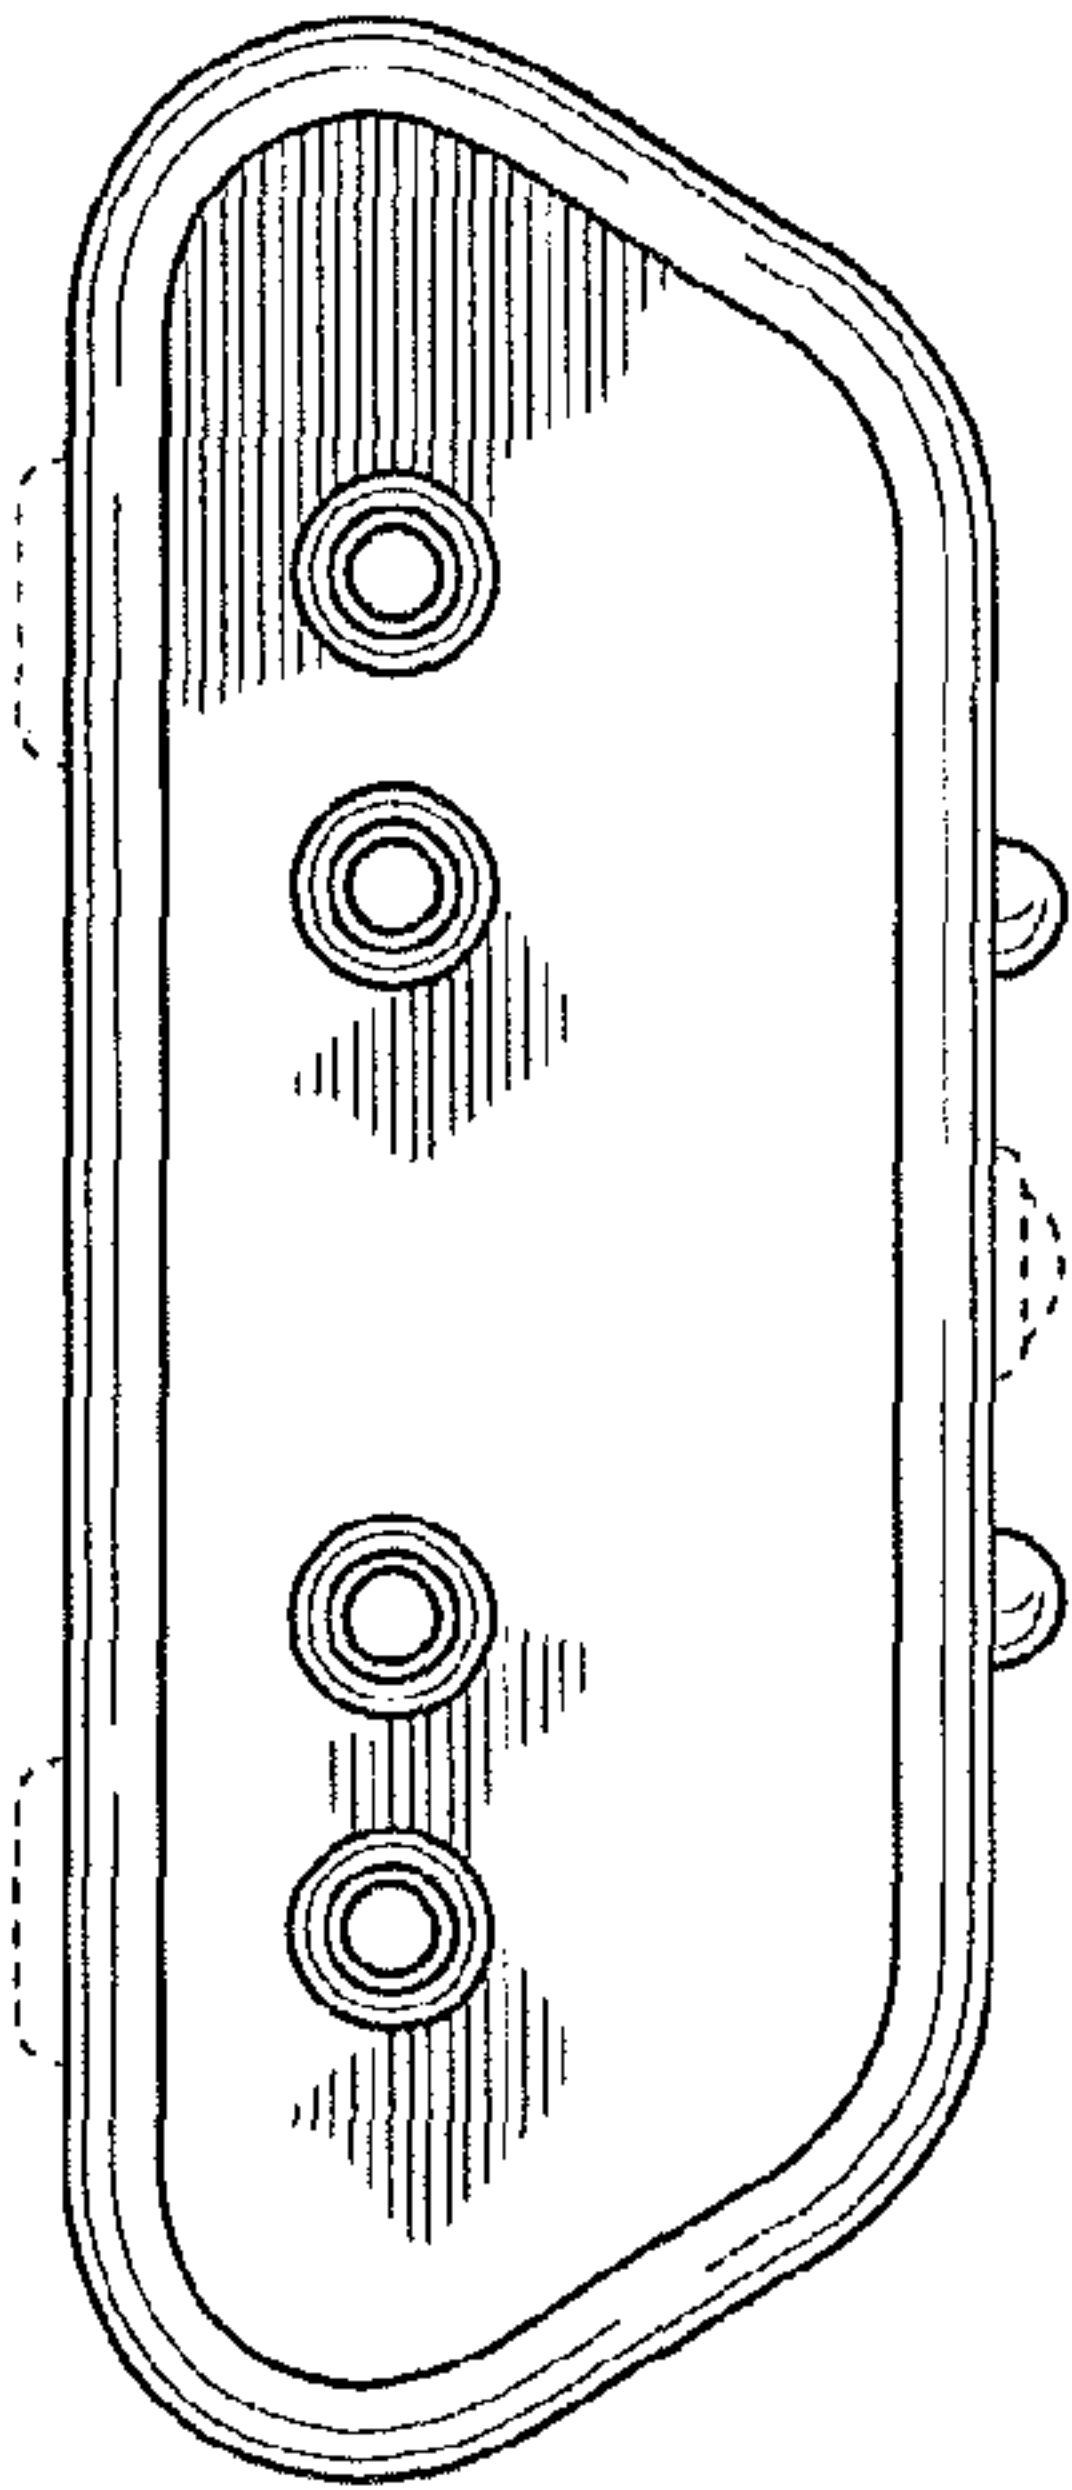


FIG. 6

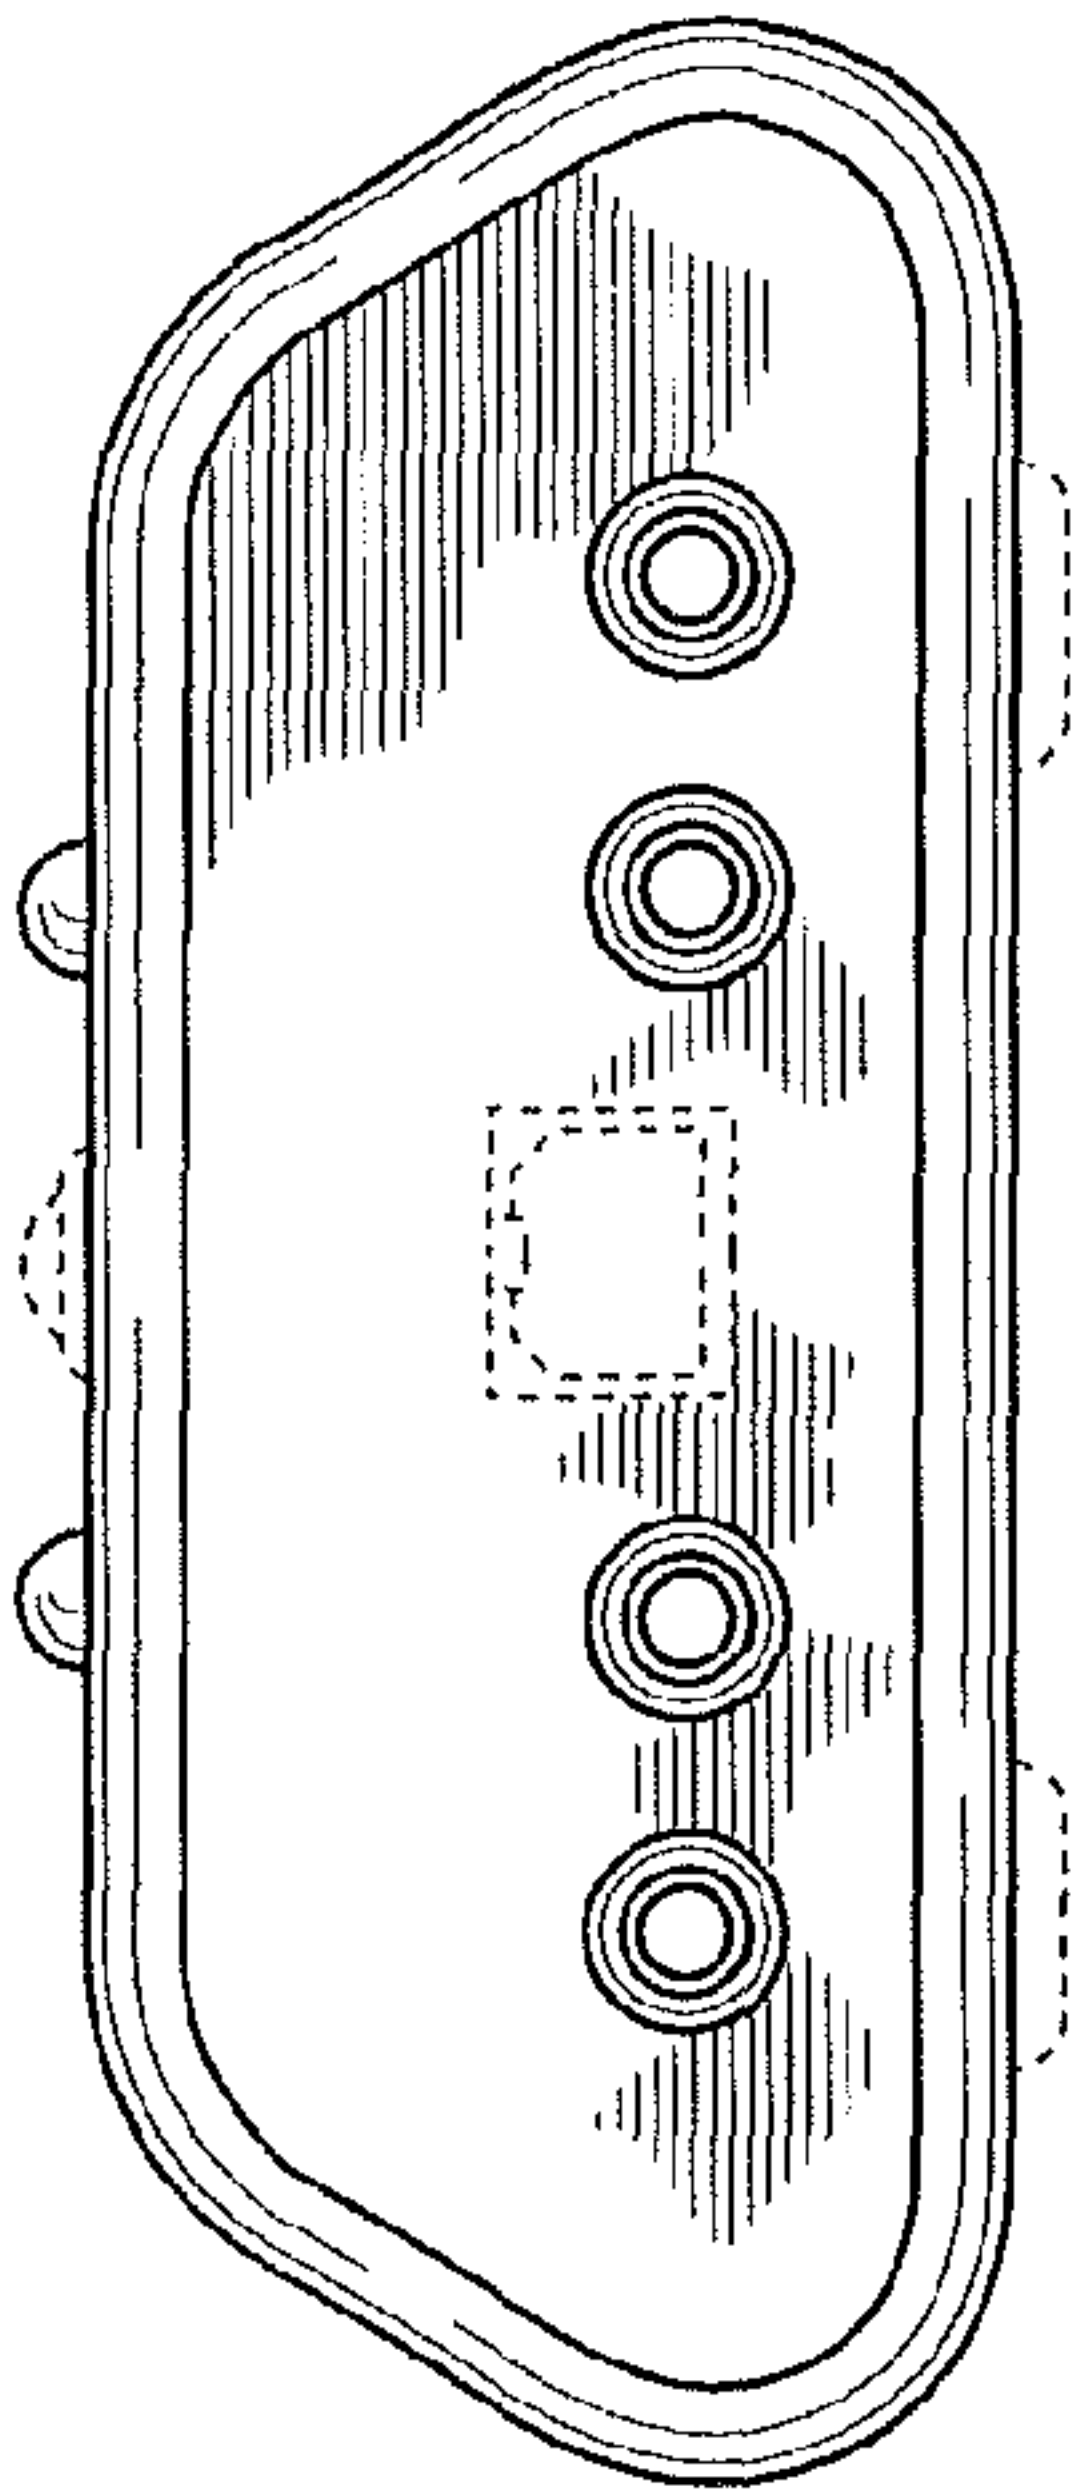


FIG. 7

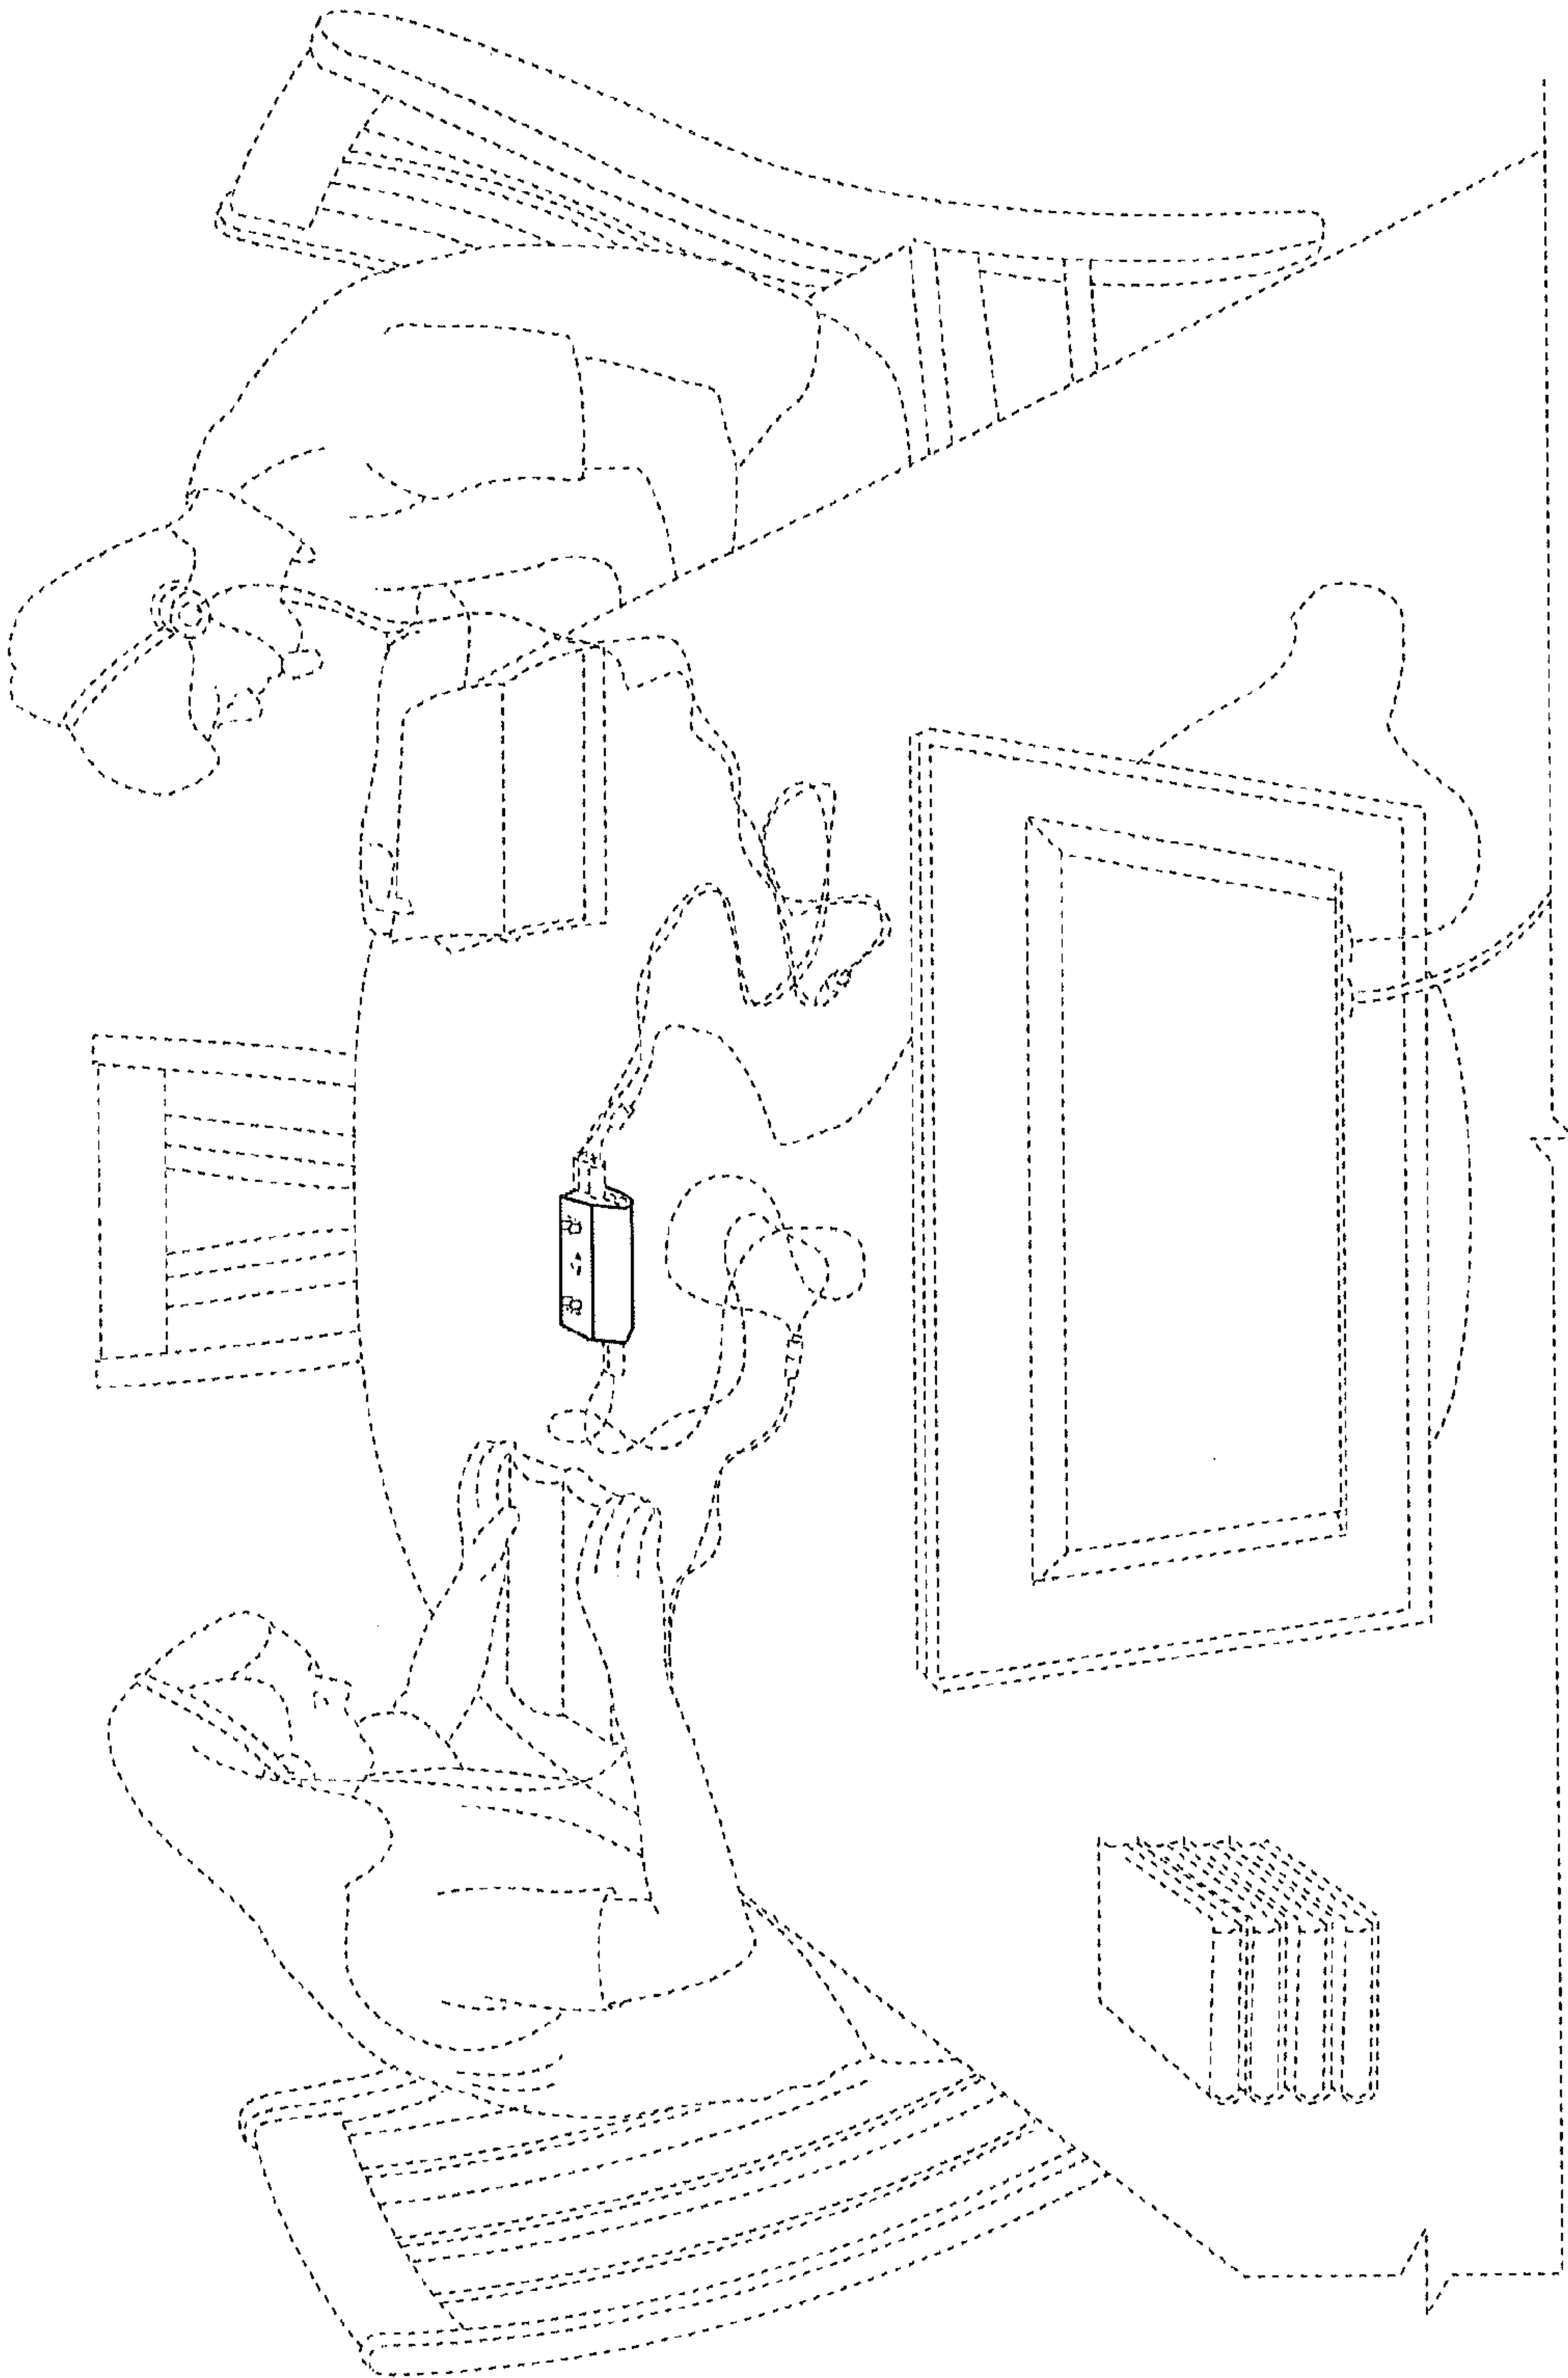


FIG. 8

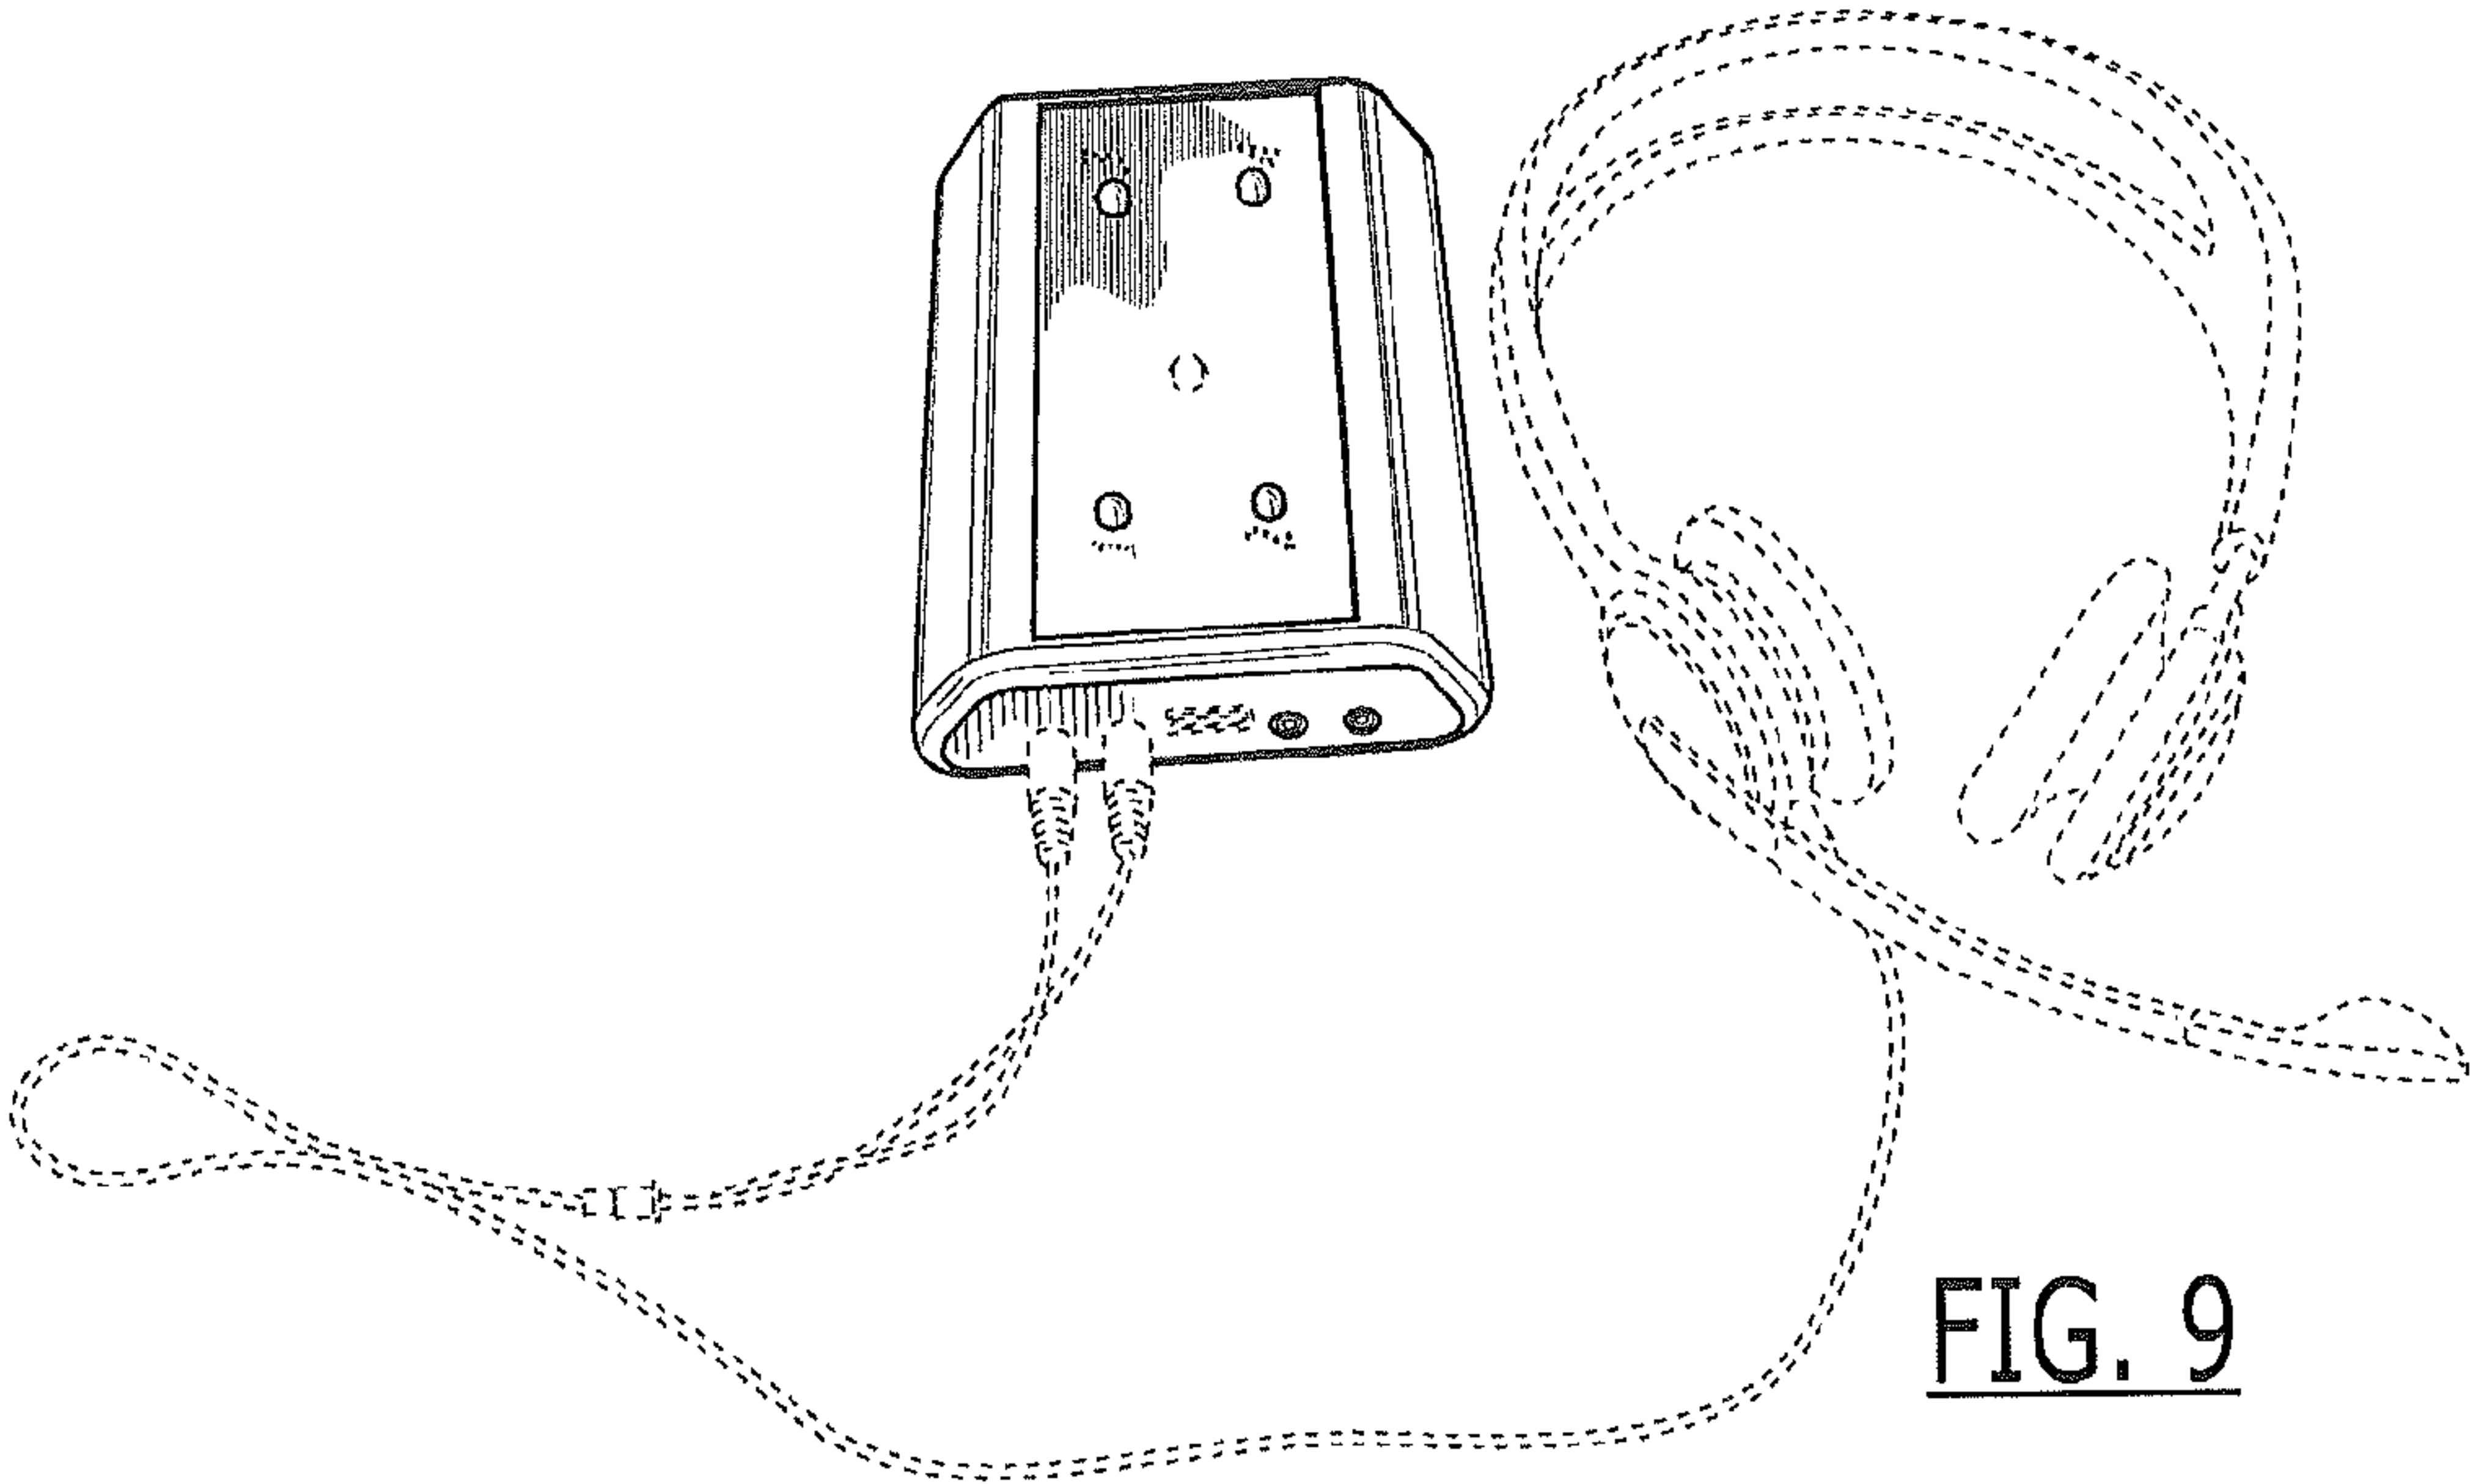


FIG. 9

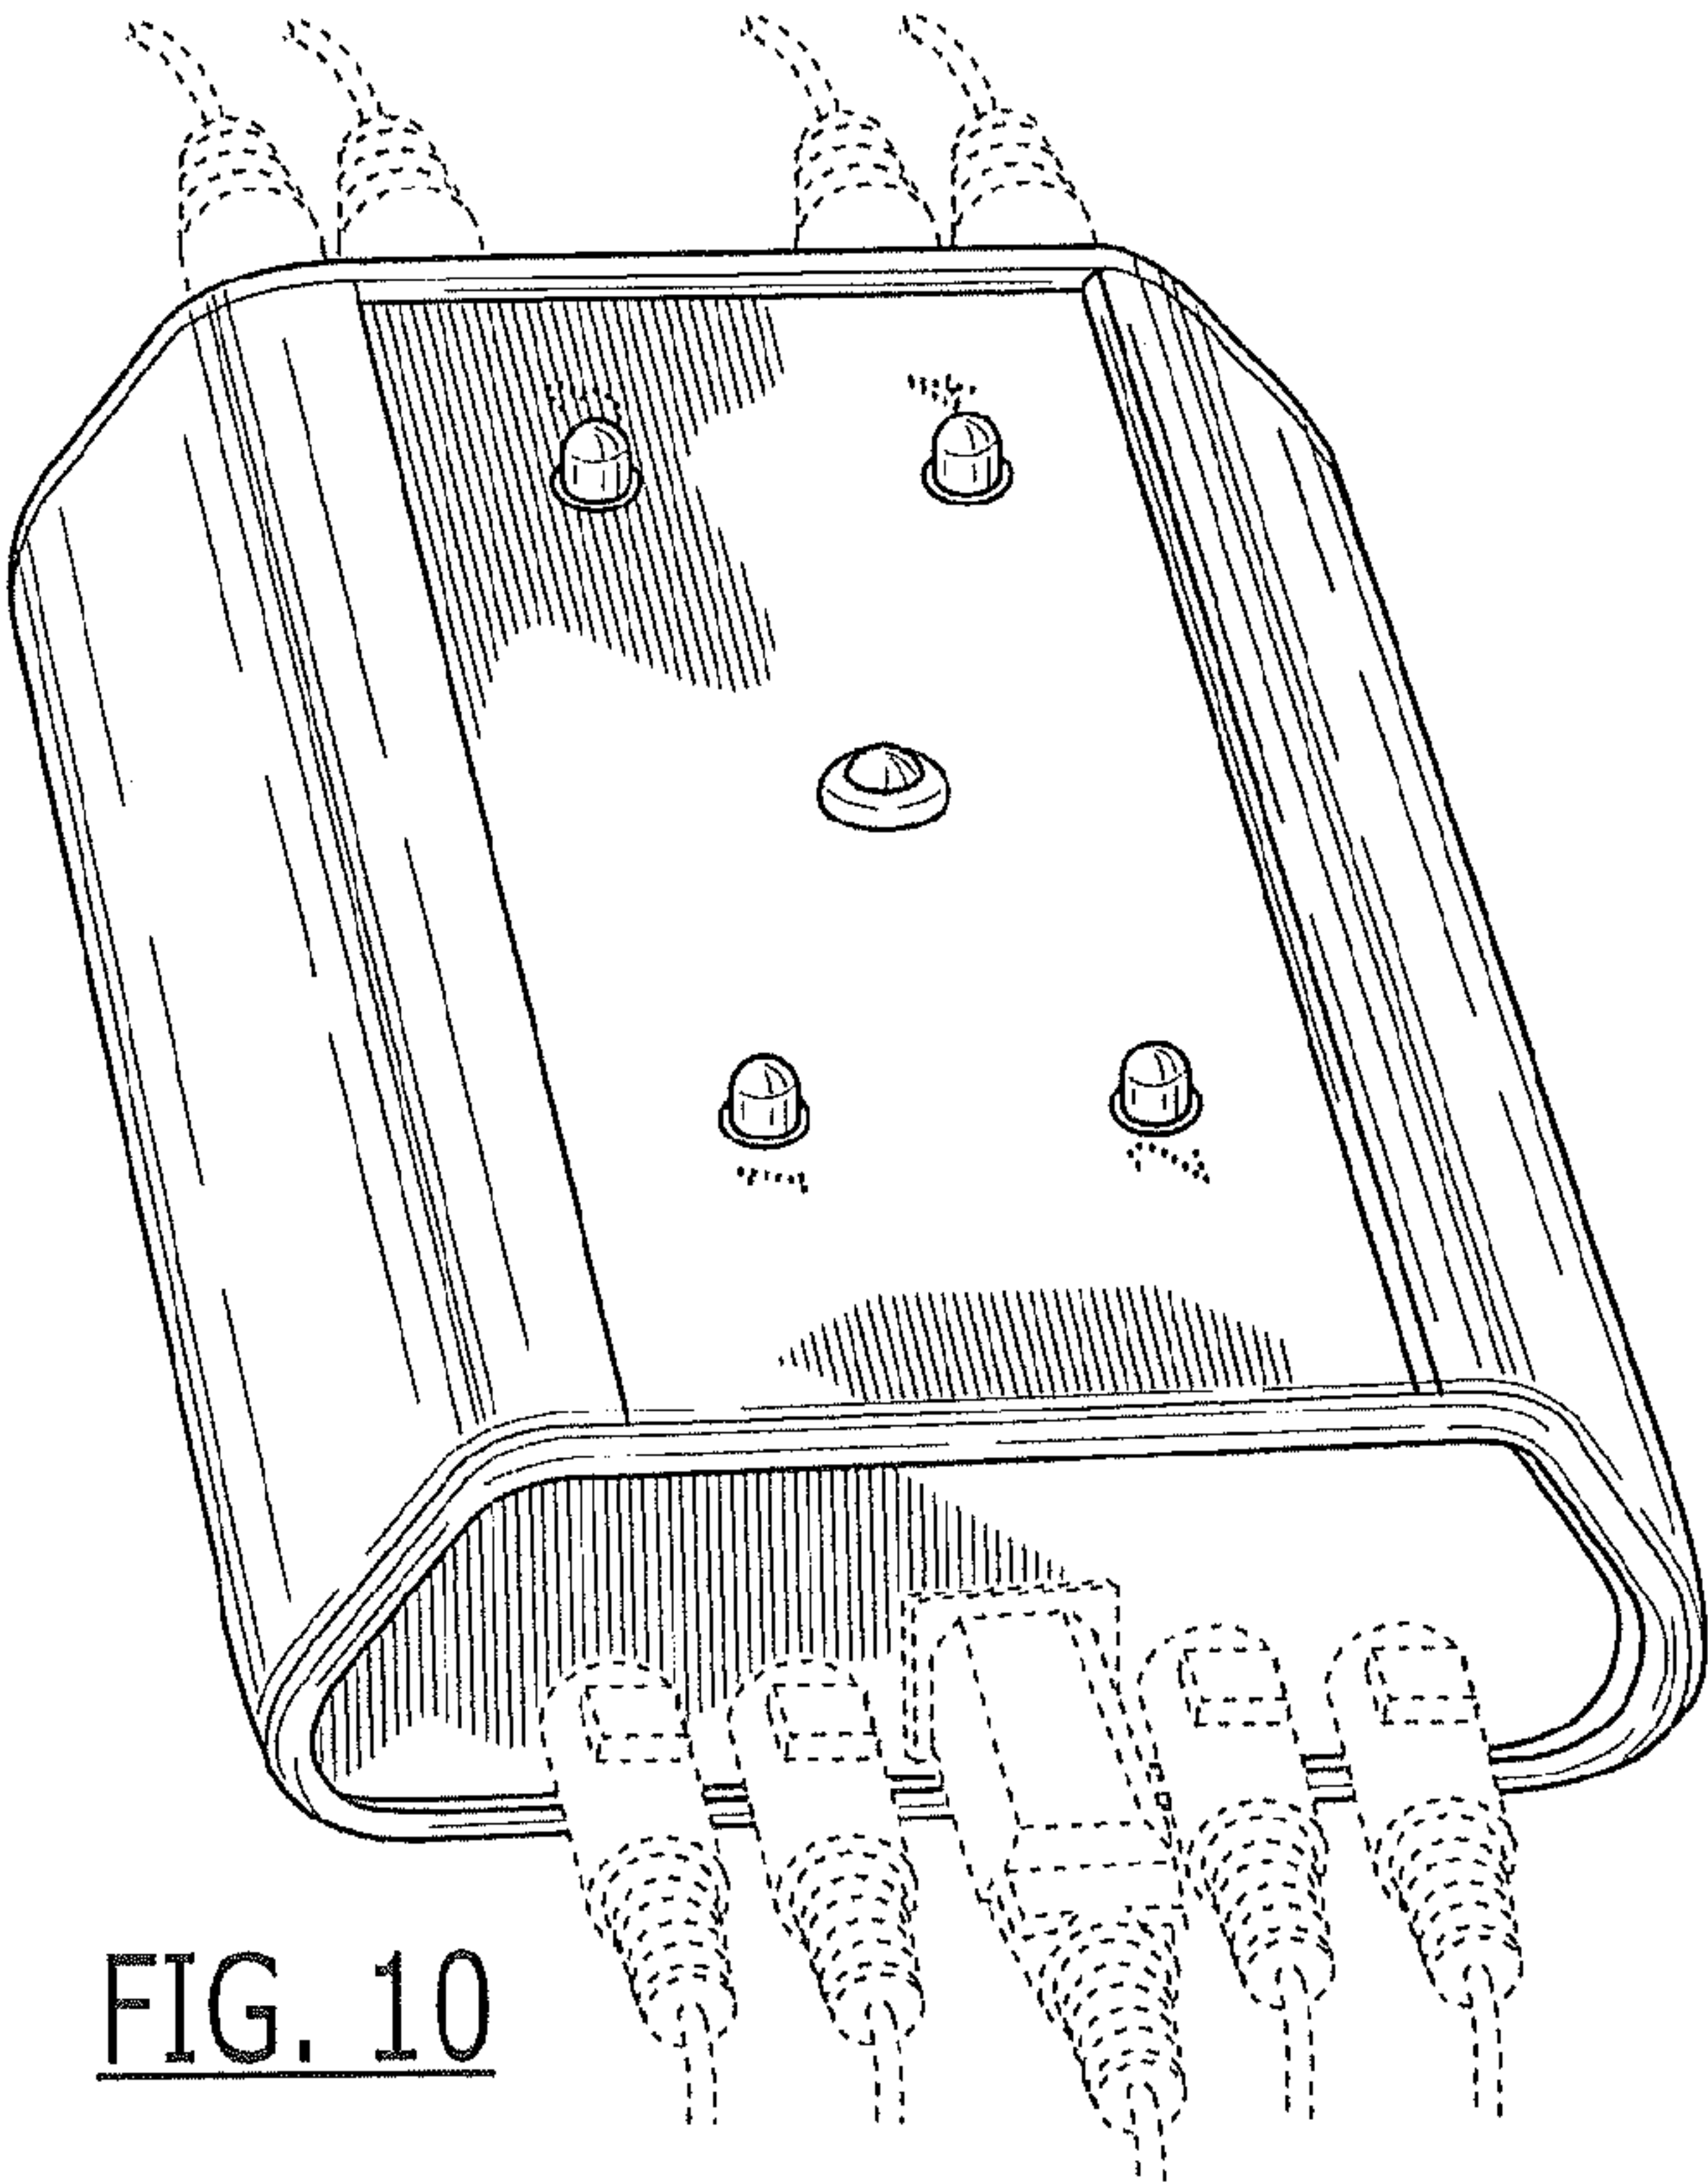


FIG. 10

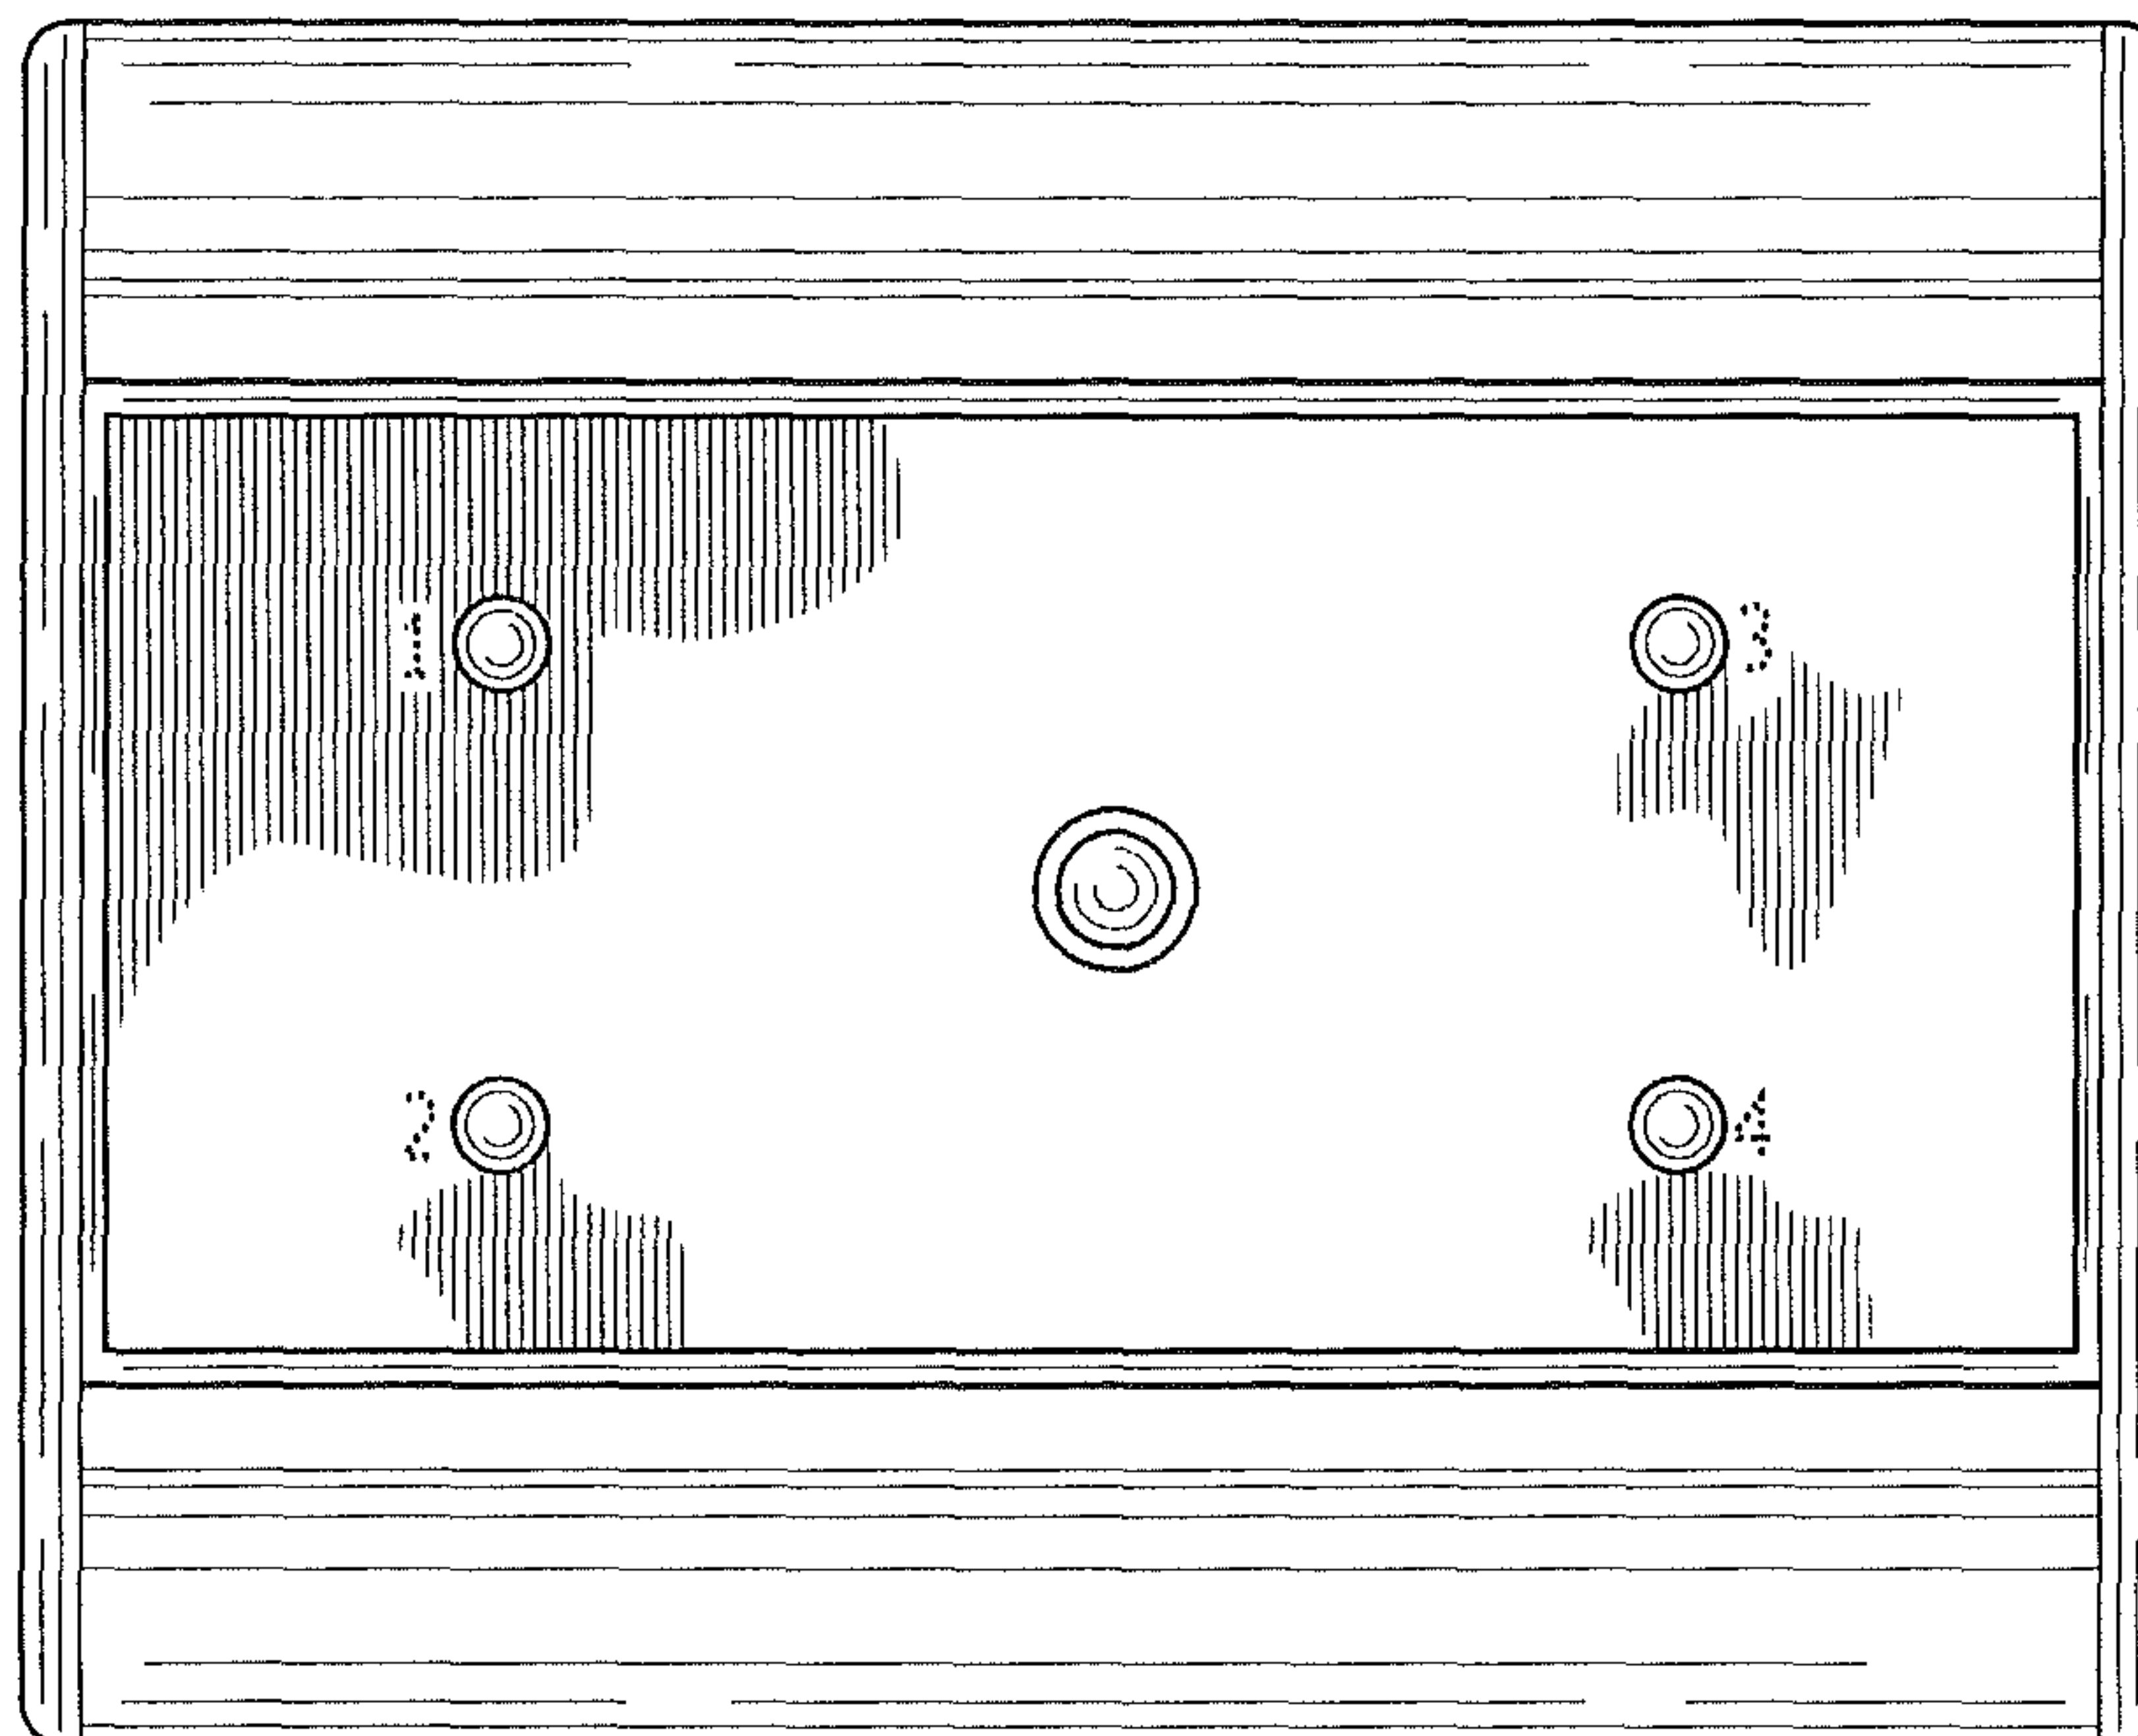


FIG. 11

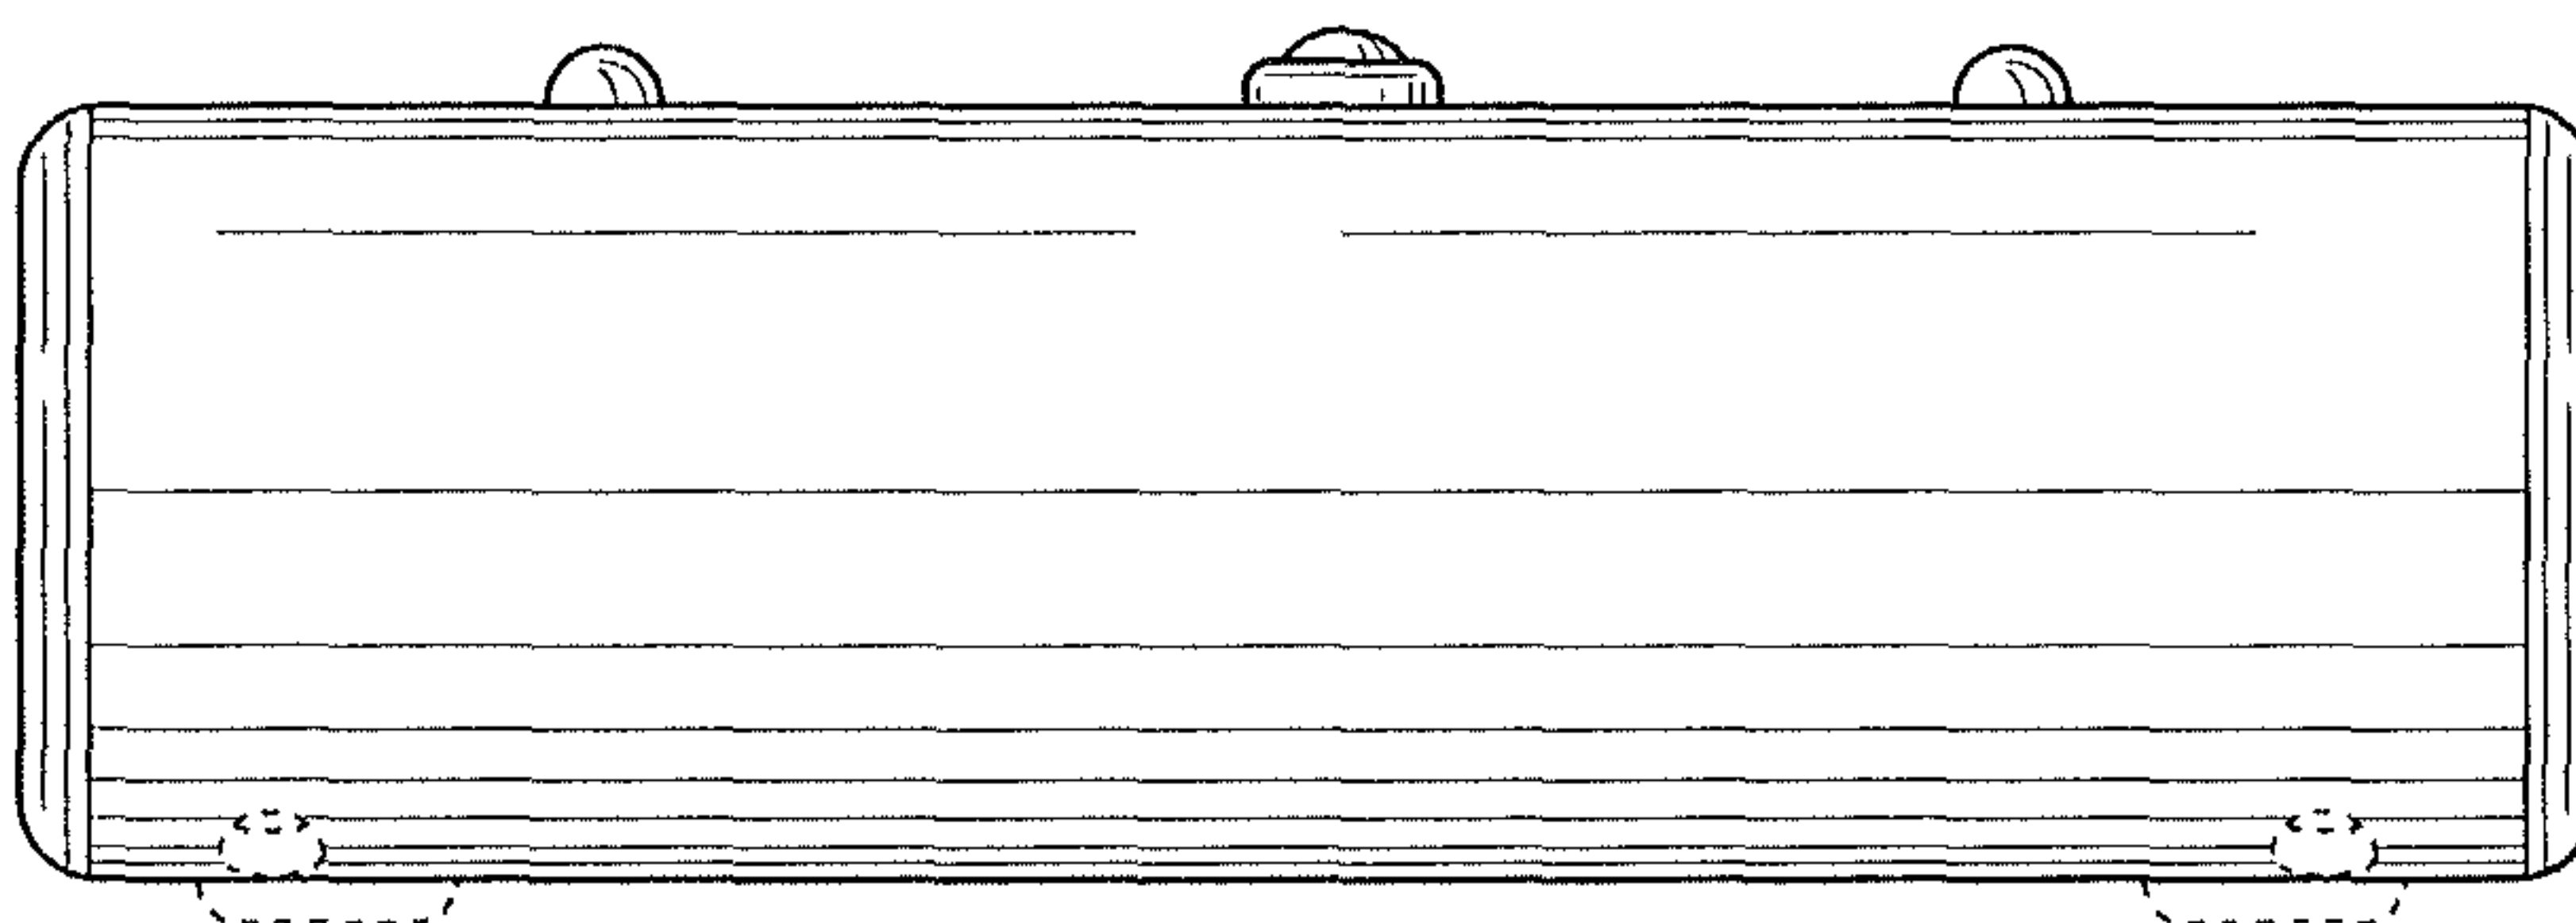


FIG. 12

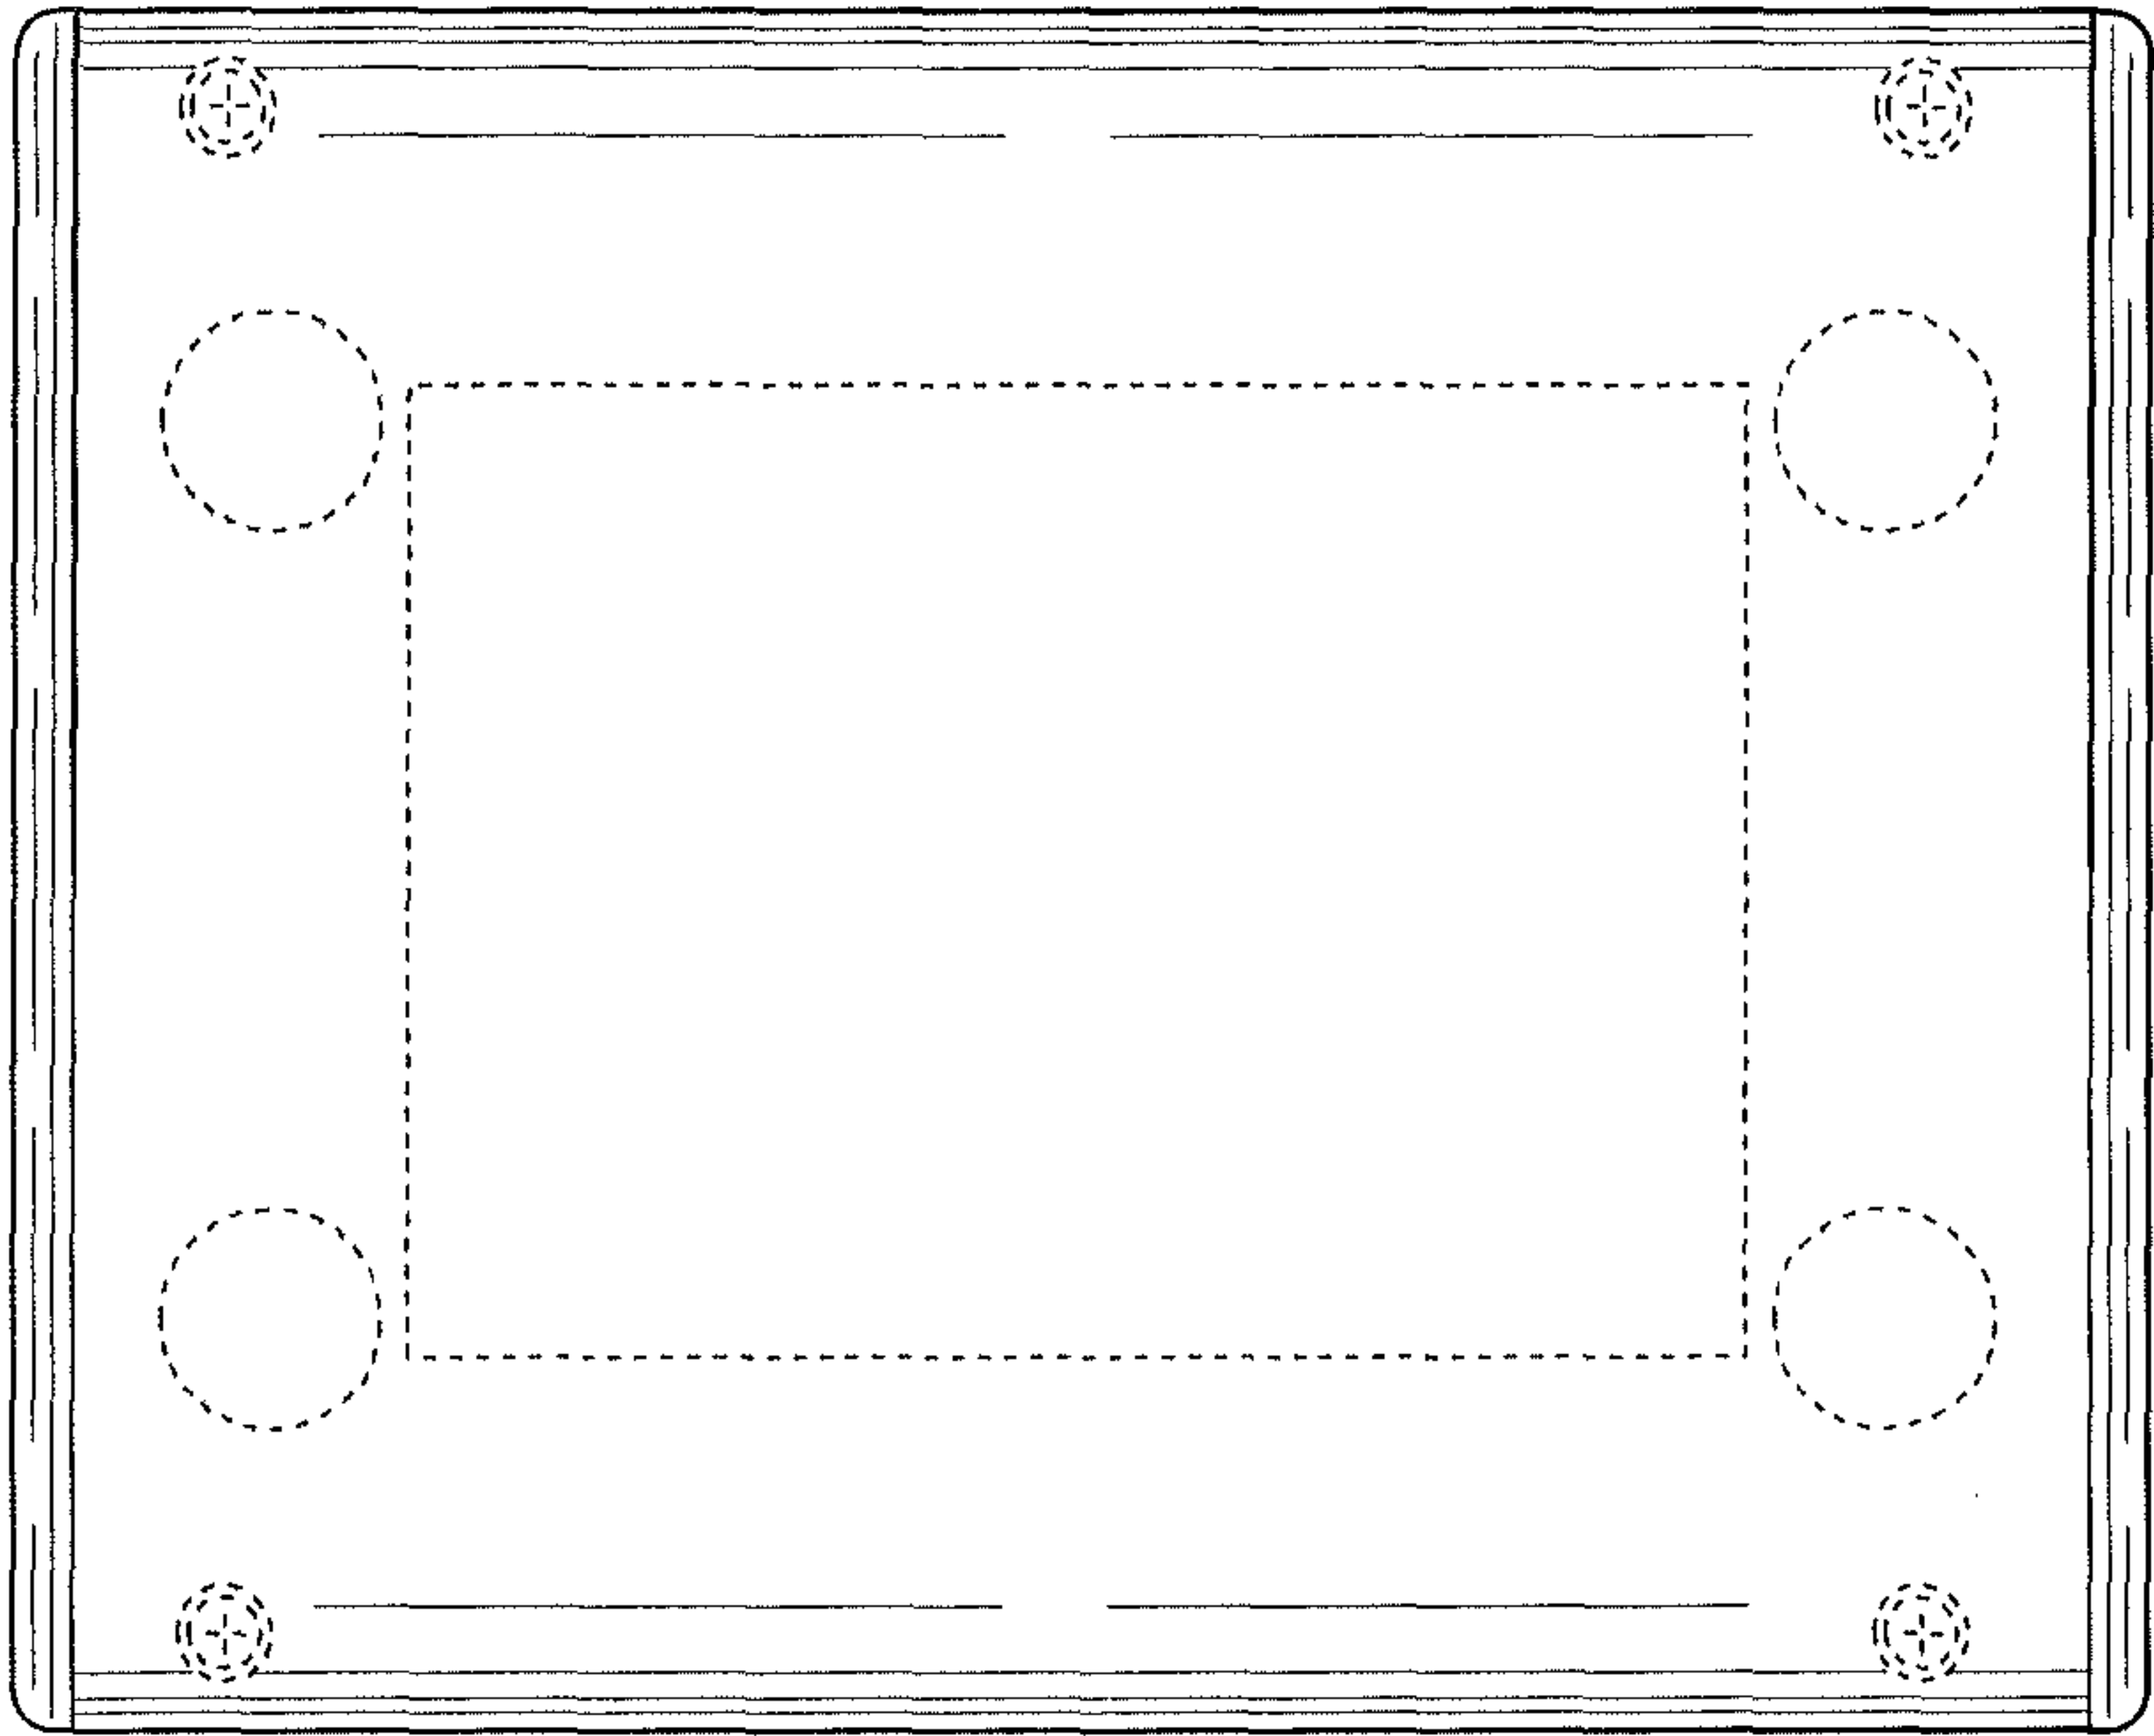


FIG. 13

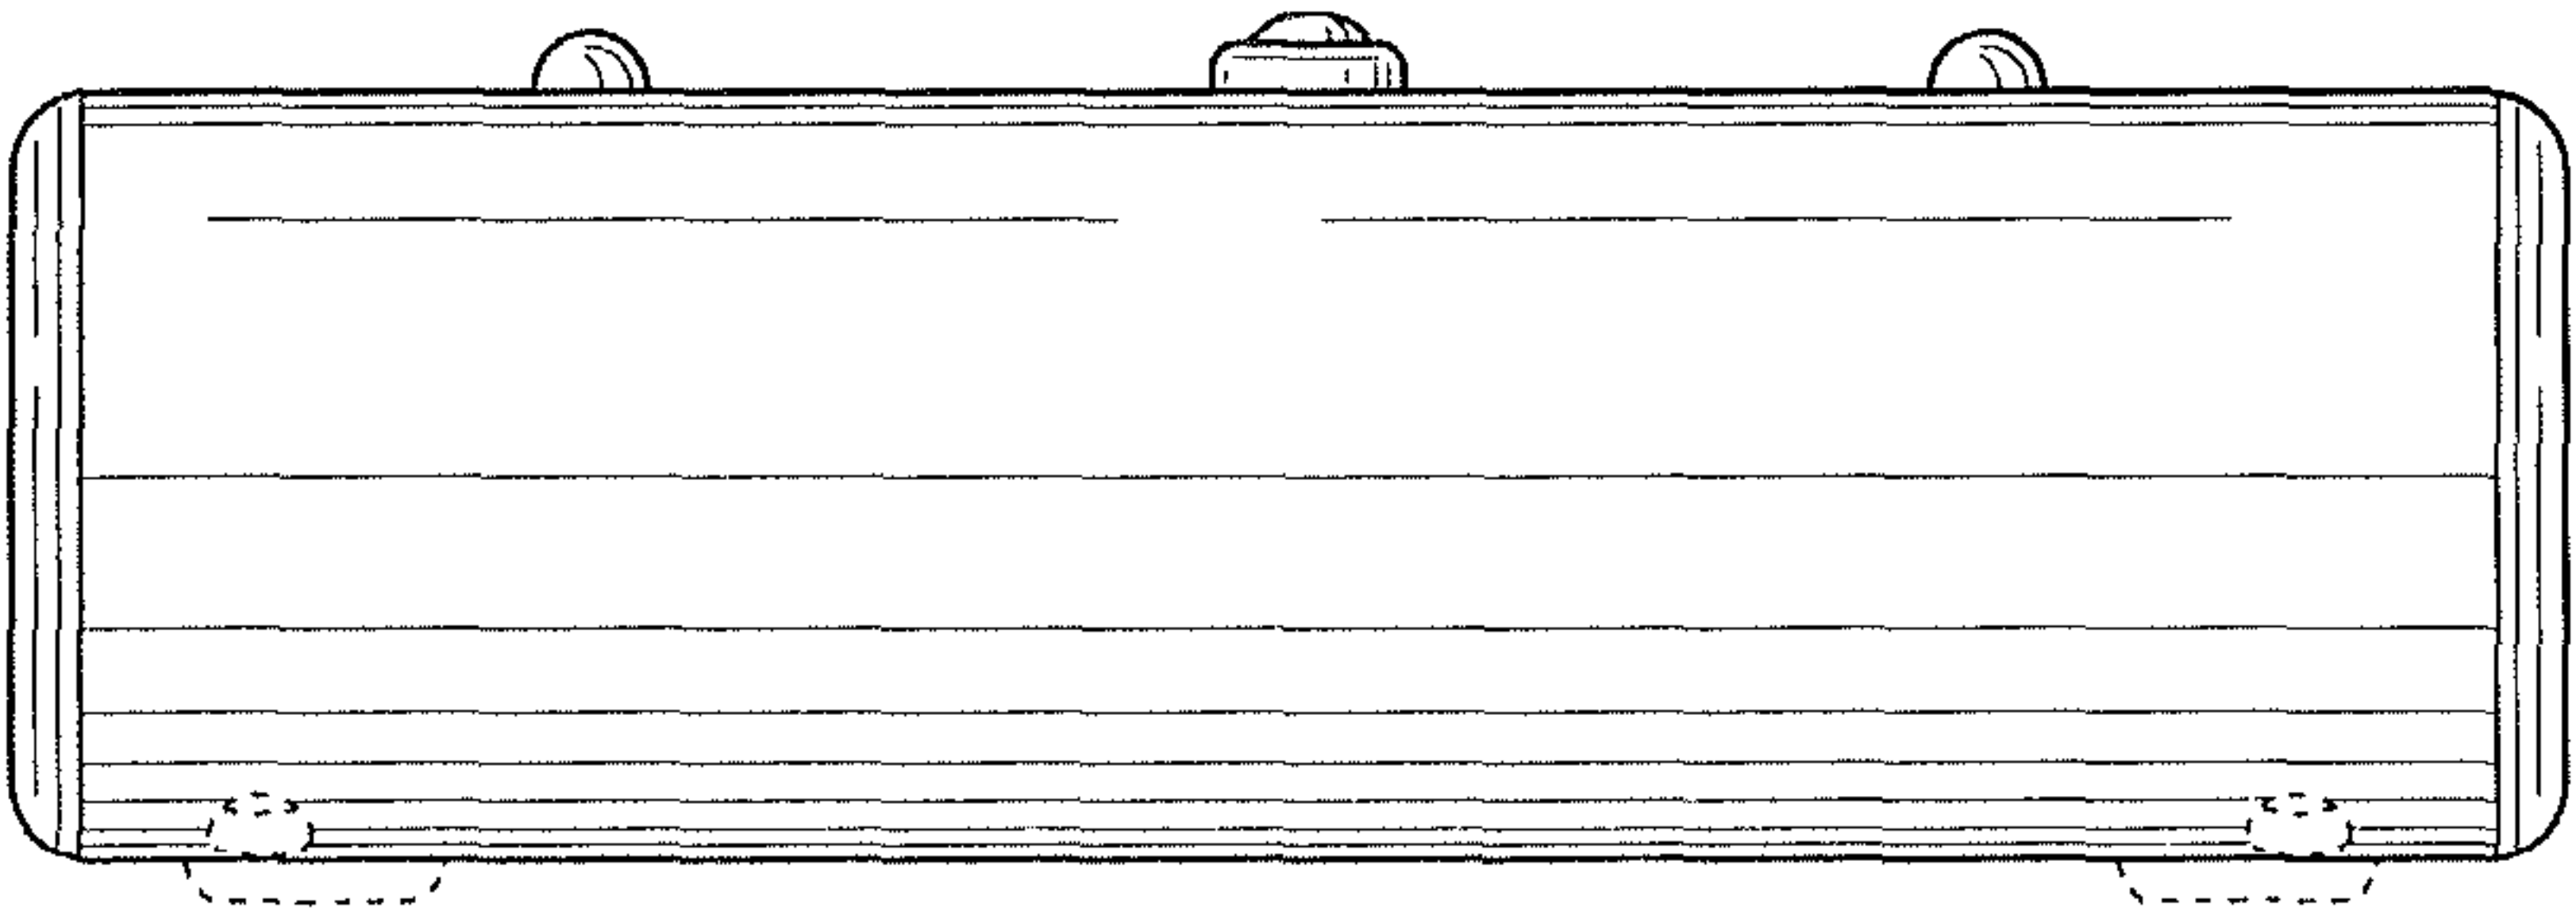


FIG. 14

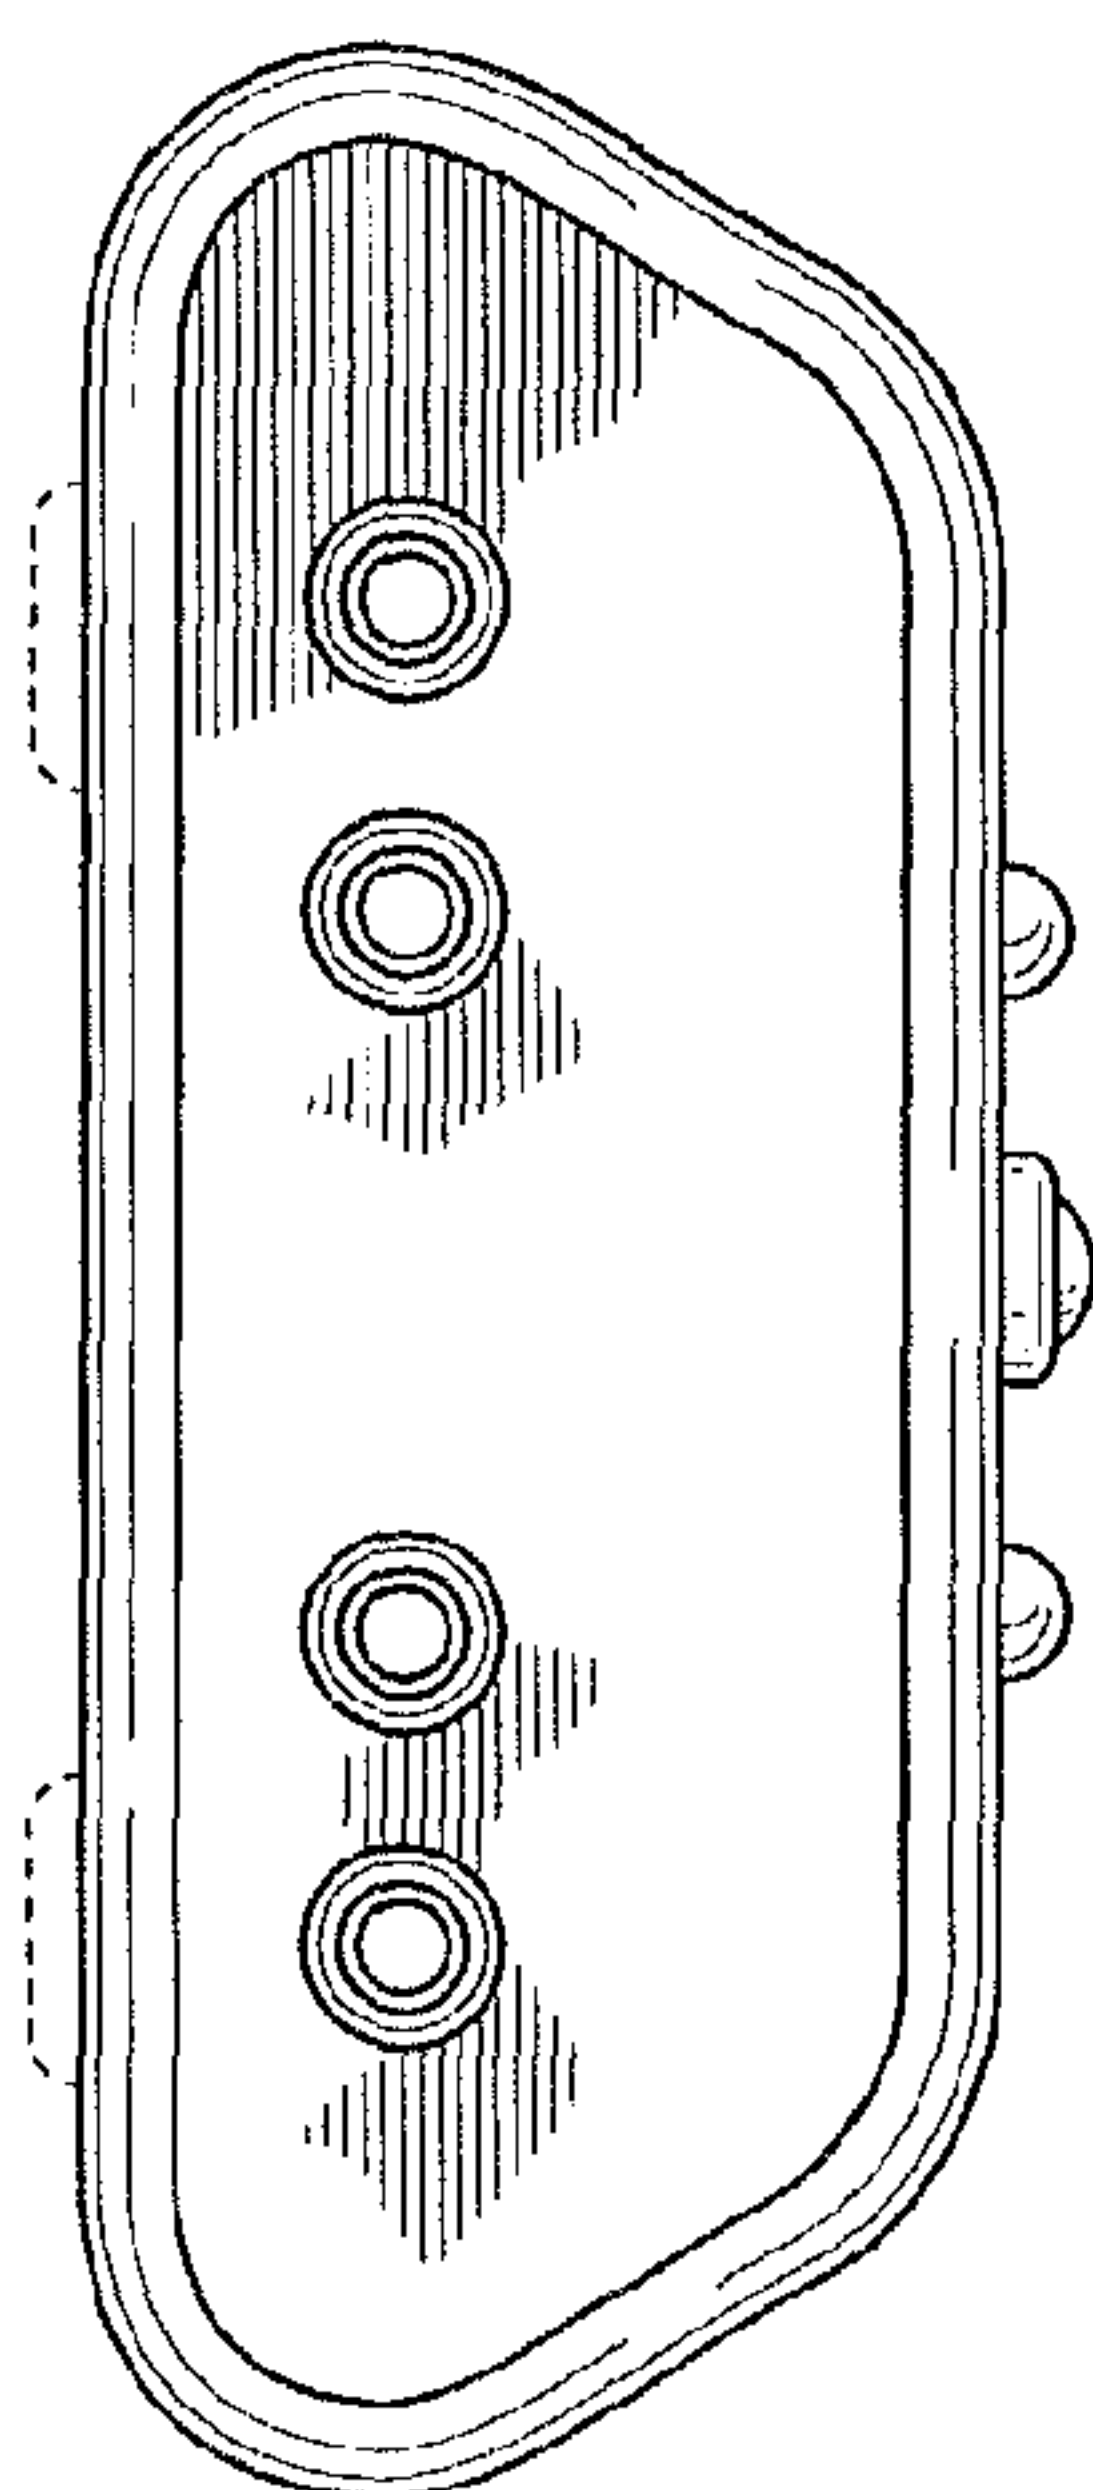


FIG. 15

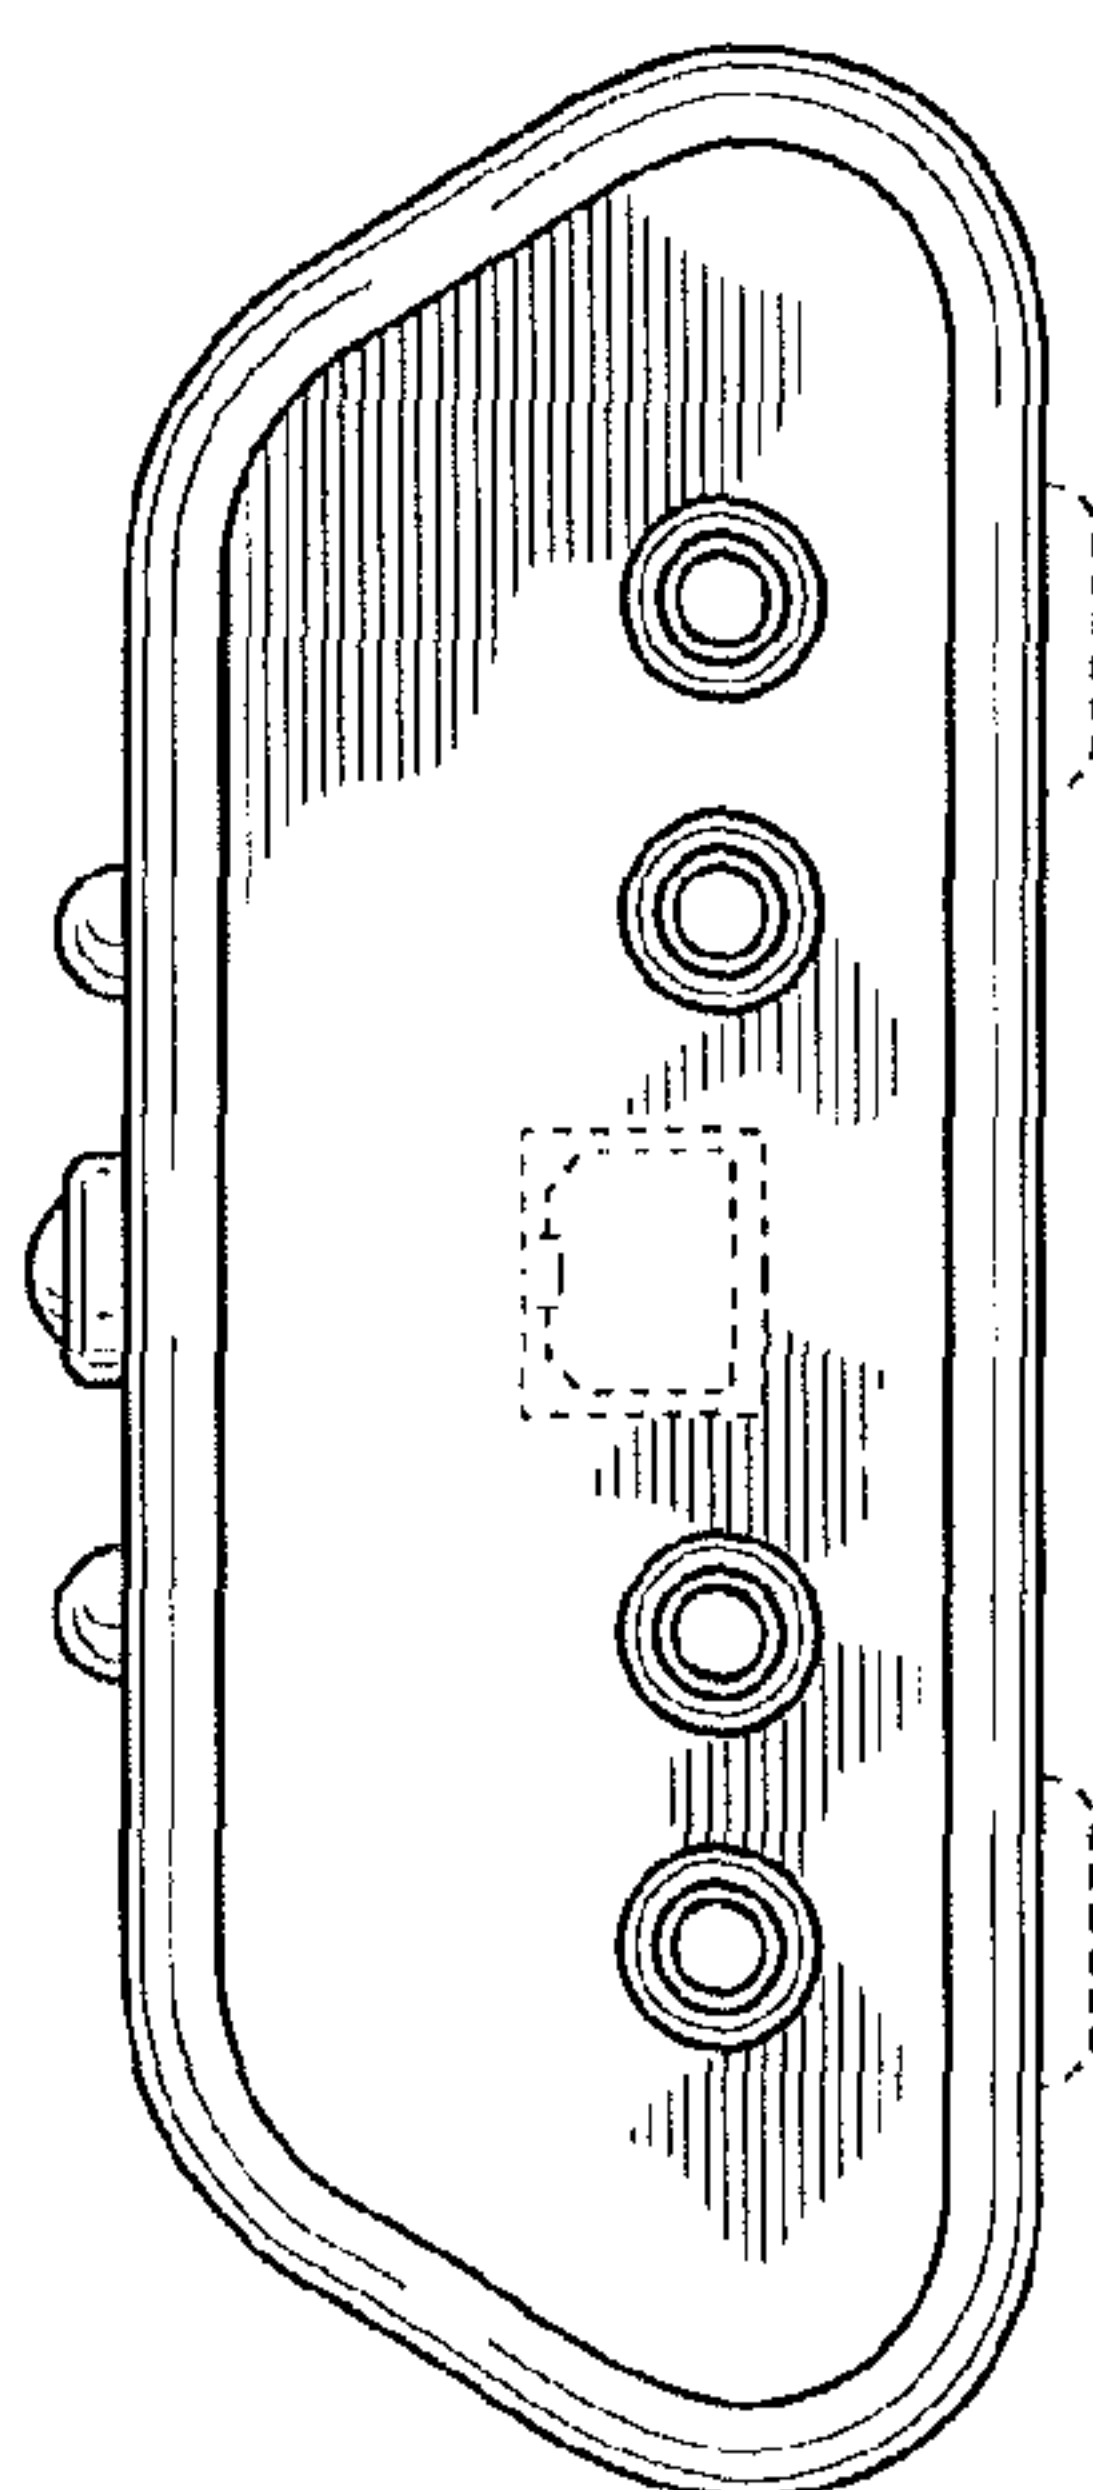


FIG. 16


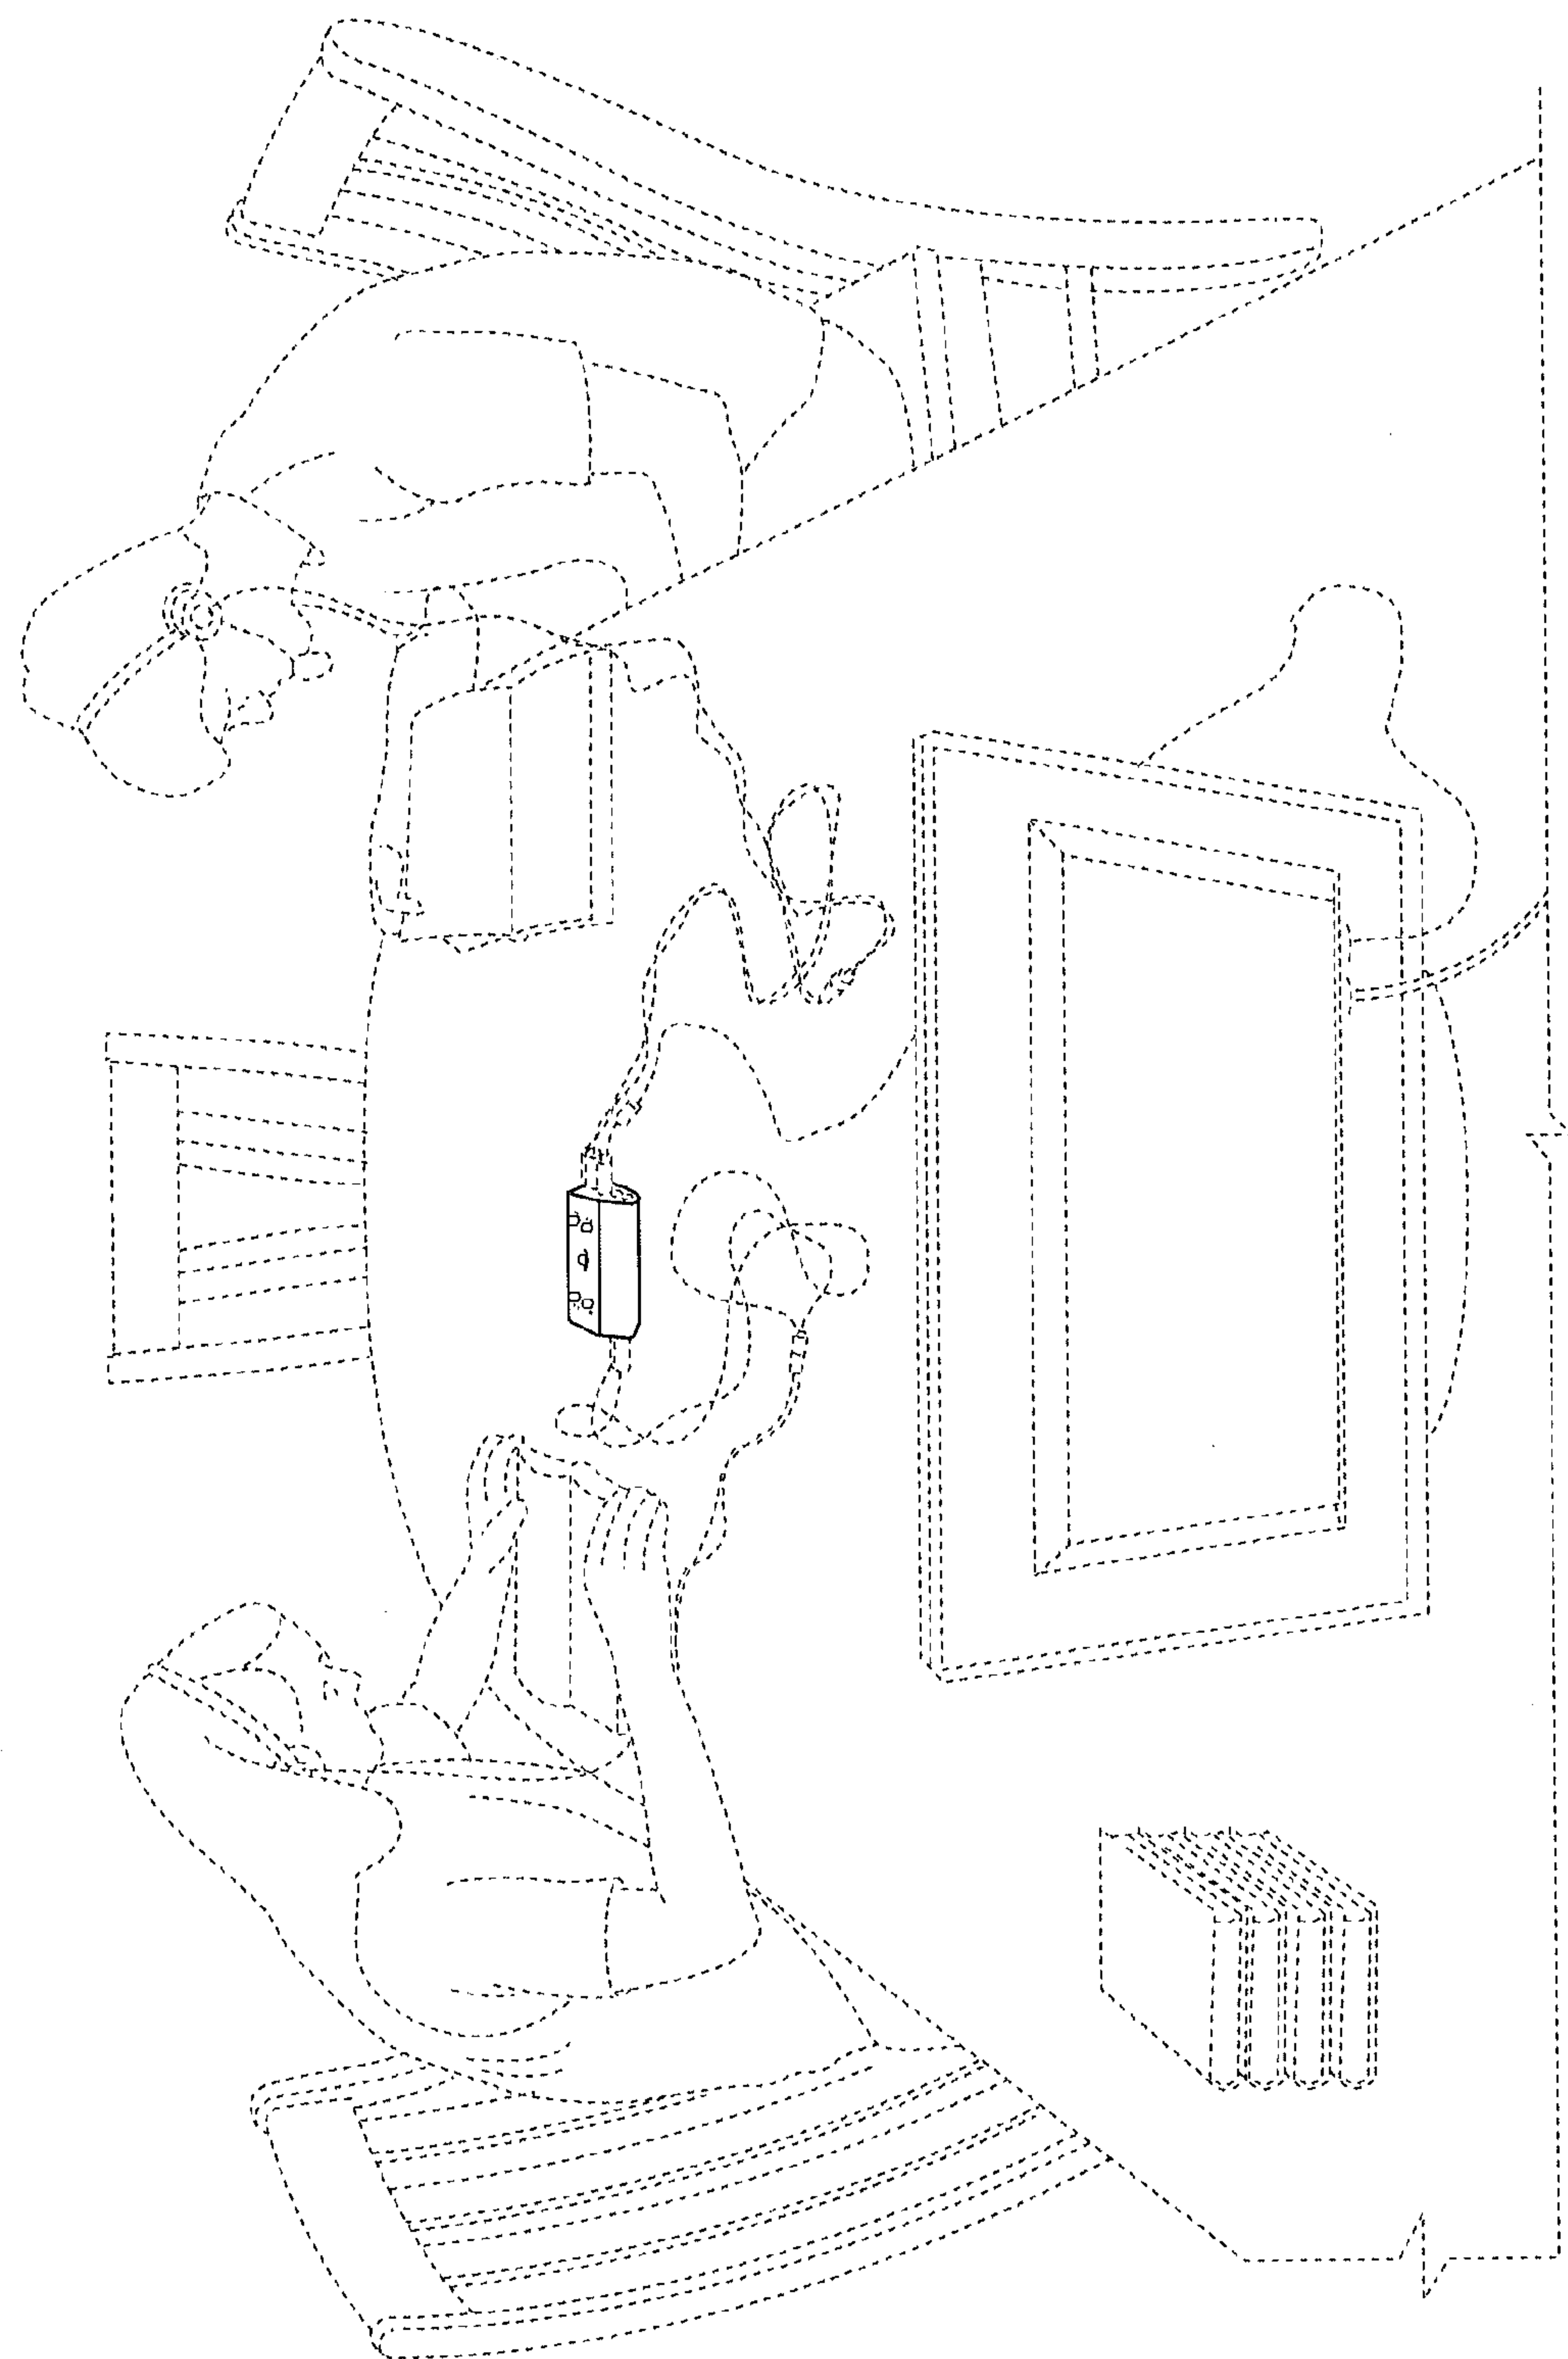


FIG. 17

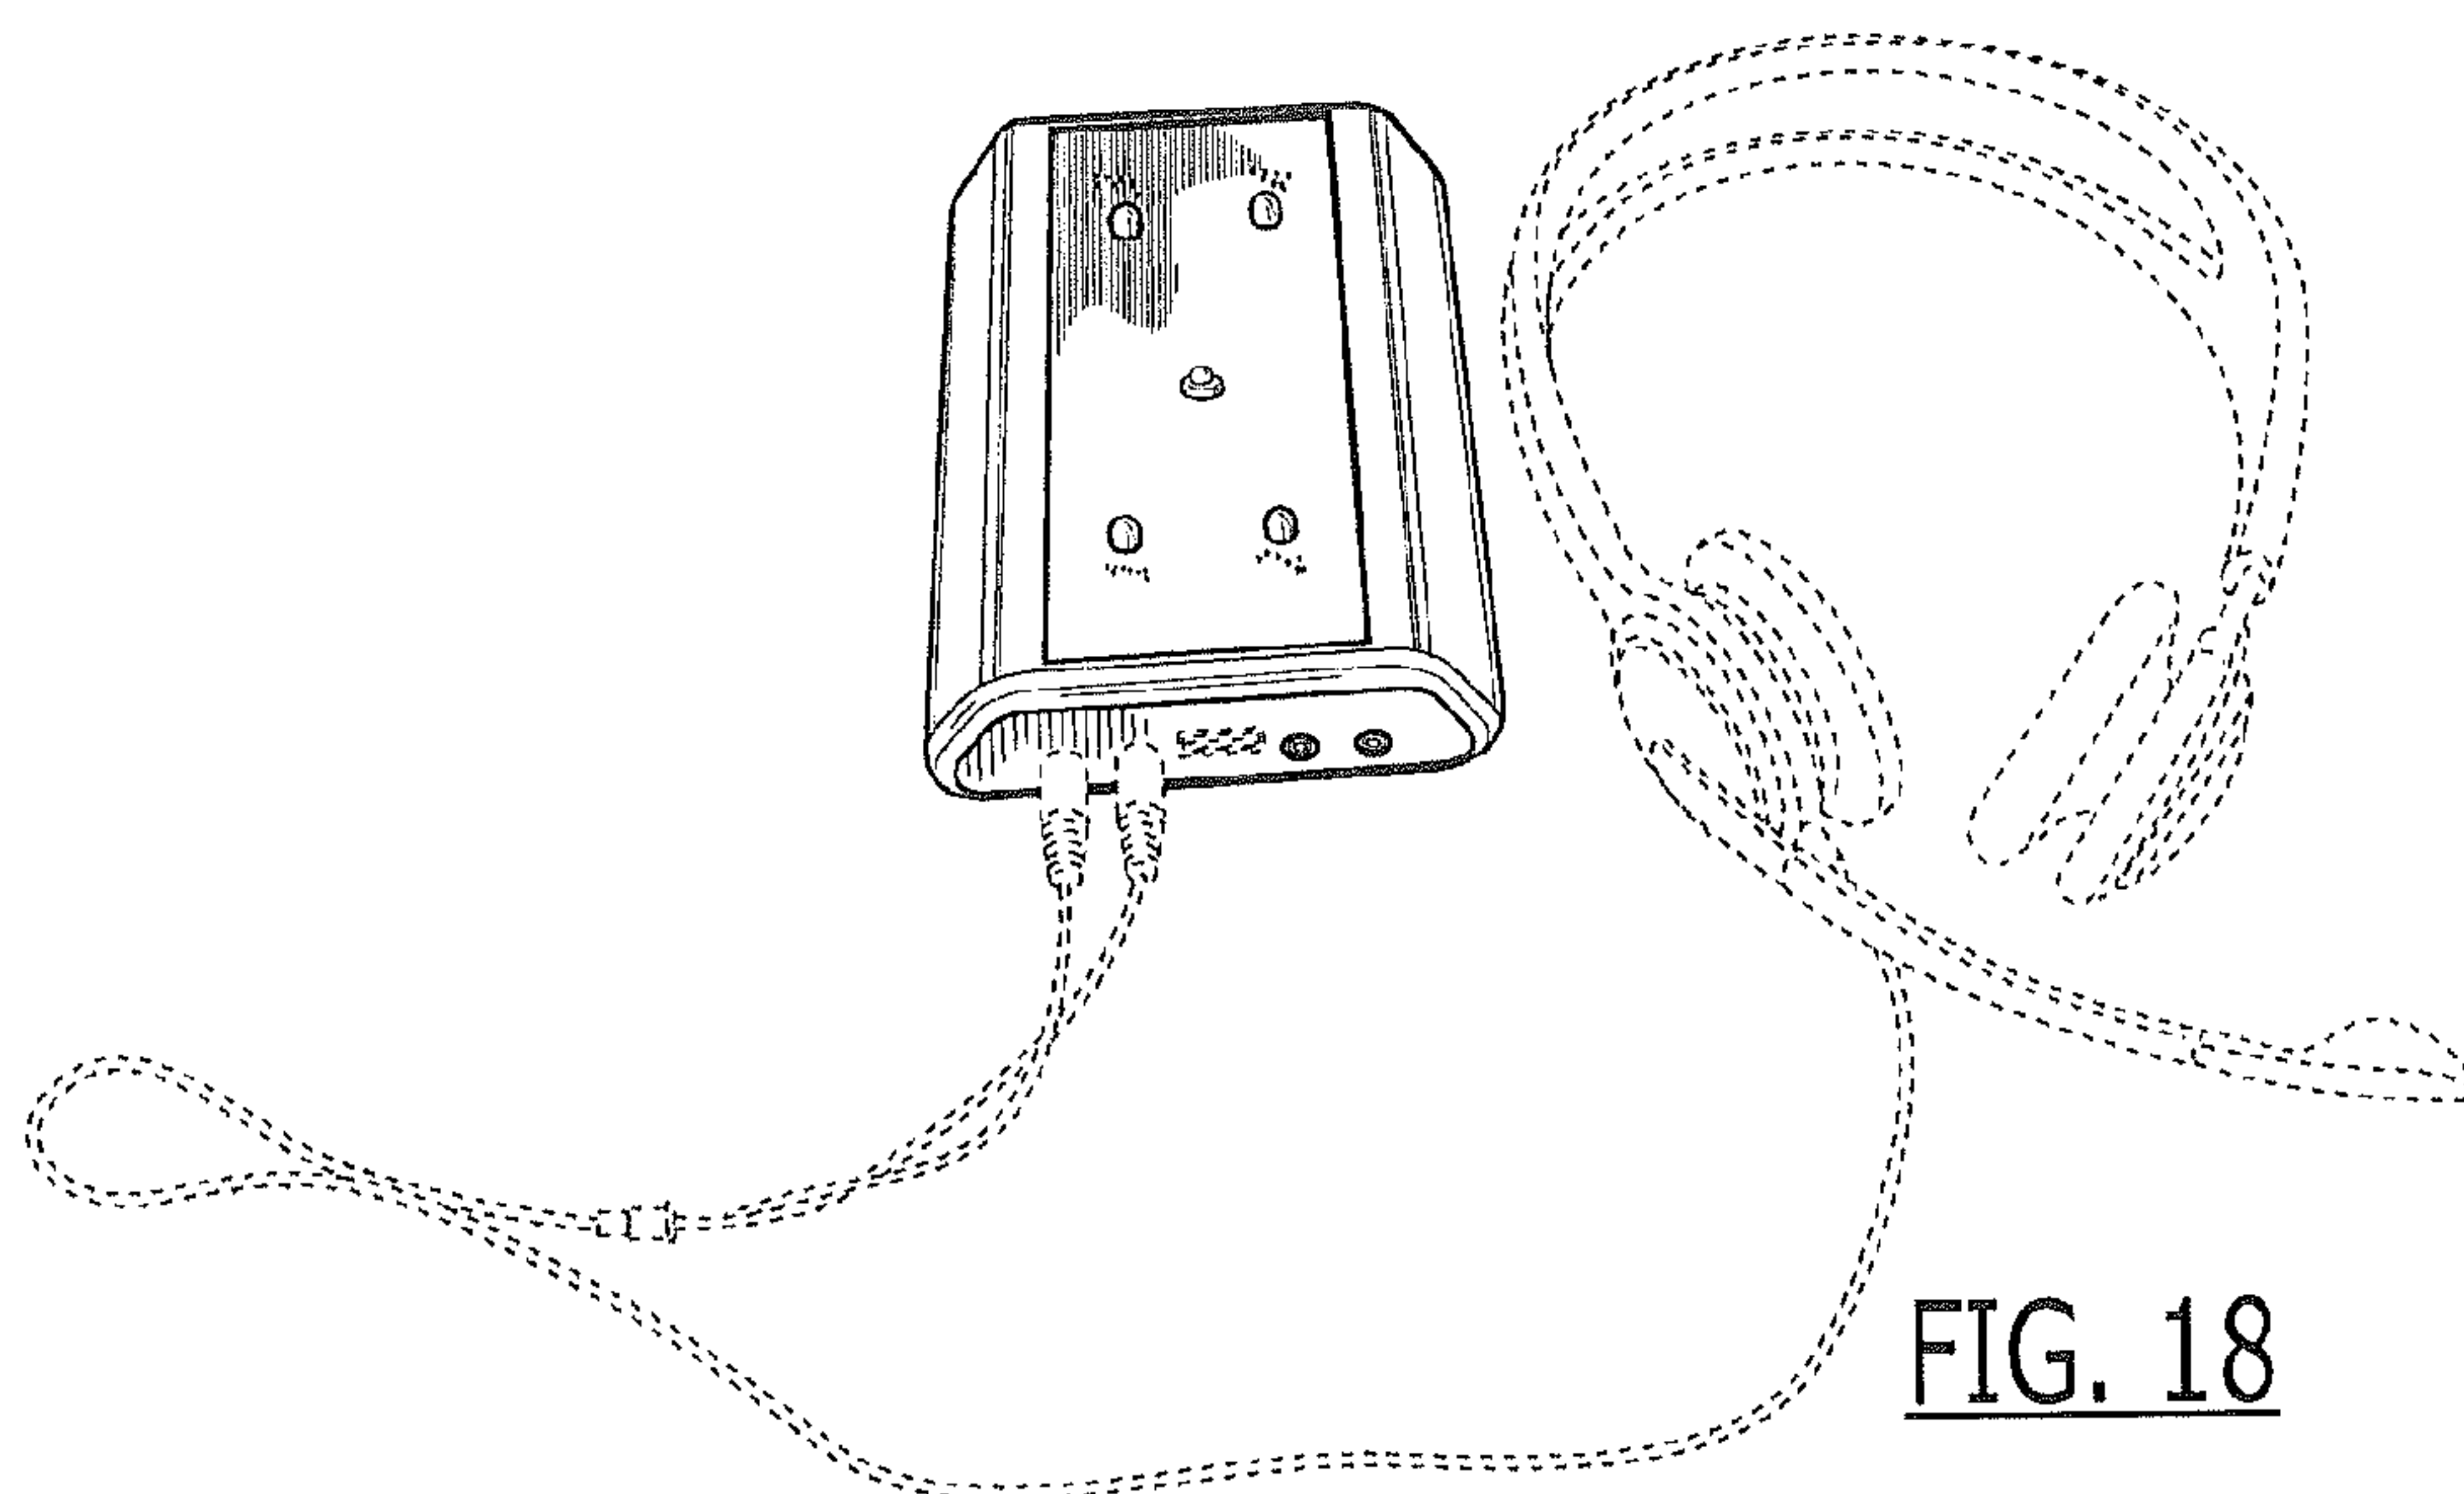

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : D716,375 S
APPLICATION NO. : 29/441307
DATED : October 28, 2014
INVENTOR(S) : Rastatter et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On Title Page:

Item (57), CLAIM, line 1:

Please correct "The ornamental design for a multi-user reading comprehension therapy device, as shown and described."

to read -- The ornamental design for a Multi-User Reading Comprehension Therapy Device as shown and described. --

Signed and Sealed this
Nineteenth Day of May, 2015



Michelle K. Lee
Director of the United States Patent and Trademark Office