



US00D717946S

(12) **United States Design Patent**  
**Kyvik et al.**

(10) **Patent No.:** **US D717,946 S**

(45) **Date of Patent:** **\*\* Nov. 18, 2014**

(54) **DUAL OVERLAP CATHETER ANCHOR PAD WITH RELEASE LAYERS**

(71) Applicant: **TIDI Securement Products, LLC**,  
Neenah, WI (US)

(72) Inventors: **Kurt Kyvik**, Ocala, FL (US); **Arthur Parkhurst**, Ocala, FL (US)

(73) Assignee: **TIDI Securement Products, LLC**,  
Neenah, WI (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/476,243**

(22) Filed: **Dec. 12, 2013**

(51) **LOC (10) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/128**

(58) **Field of Classification Search**  
USPC ..... D24/127-128, 130, 112, 189;  
600/391-392; 604/179-180, 187, 227;  
128/DIG. 26; 602/58-59  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D364,922 S \* 12/1995 Bierman ..... D24/128  
D375,356 S \* 11/1996 Bierman ..... D24/128

D401,329 S \* 11/1998 Bierman ..... D24/128  
D492,411 S \* 6/2004 Bierman ..... D24/128  
D503,977 S \* 4/2005 Bierman ..... D24/128  
D608,887 S \* 1/2010 Kyvik et al. .... D24/130  
D616,091 S \* 5/2010 Kyvik et al. .... D24/128  
D616,542 S \* 5/2010 Kyvik et al. .... D24/128  
D616,983 S \* 6/2010 Kyvik et al. .... D24/128  
8,486,004 B1 \* 7/2013 Propp ..... 604/180

\* cited by examiner

*Primary Examiner* — Robert A. Delehanty

(74) *Attorney, Agent, or Firm* — Boyle Fredrickson, S.C.

(57) **CLAIM**

The ornamental design for a dual overlap catheter anchor pad with release layers, as shown and described.

**DESCRIPTION**


FIG. 1 is a perspective view of the dual overlap catheter anchor pad with release layers, shown in a spread position with two portions of the upper release layer slightly separated from the underlying adhesive layer.


FIG. 2 is a top view of the dual overlap catheter anchor pad with release layers.

FIG. 3 is a bottom view of the dual overlap catheter anchor pad with release layers.


FIG. 4 is a front view of the dual overlap catheter anchor pad with release layers, the rear view being a mirror image; and, FIG. 5 is a right side view of the dual overlap catheter anchor pad with release layers, the left side view being a mirror image.

**1 Claim, 3 Drawing Sheets**

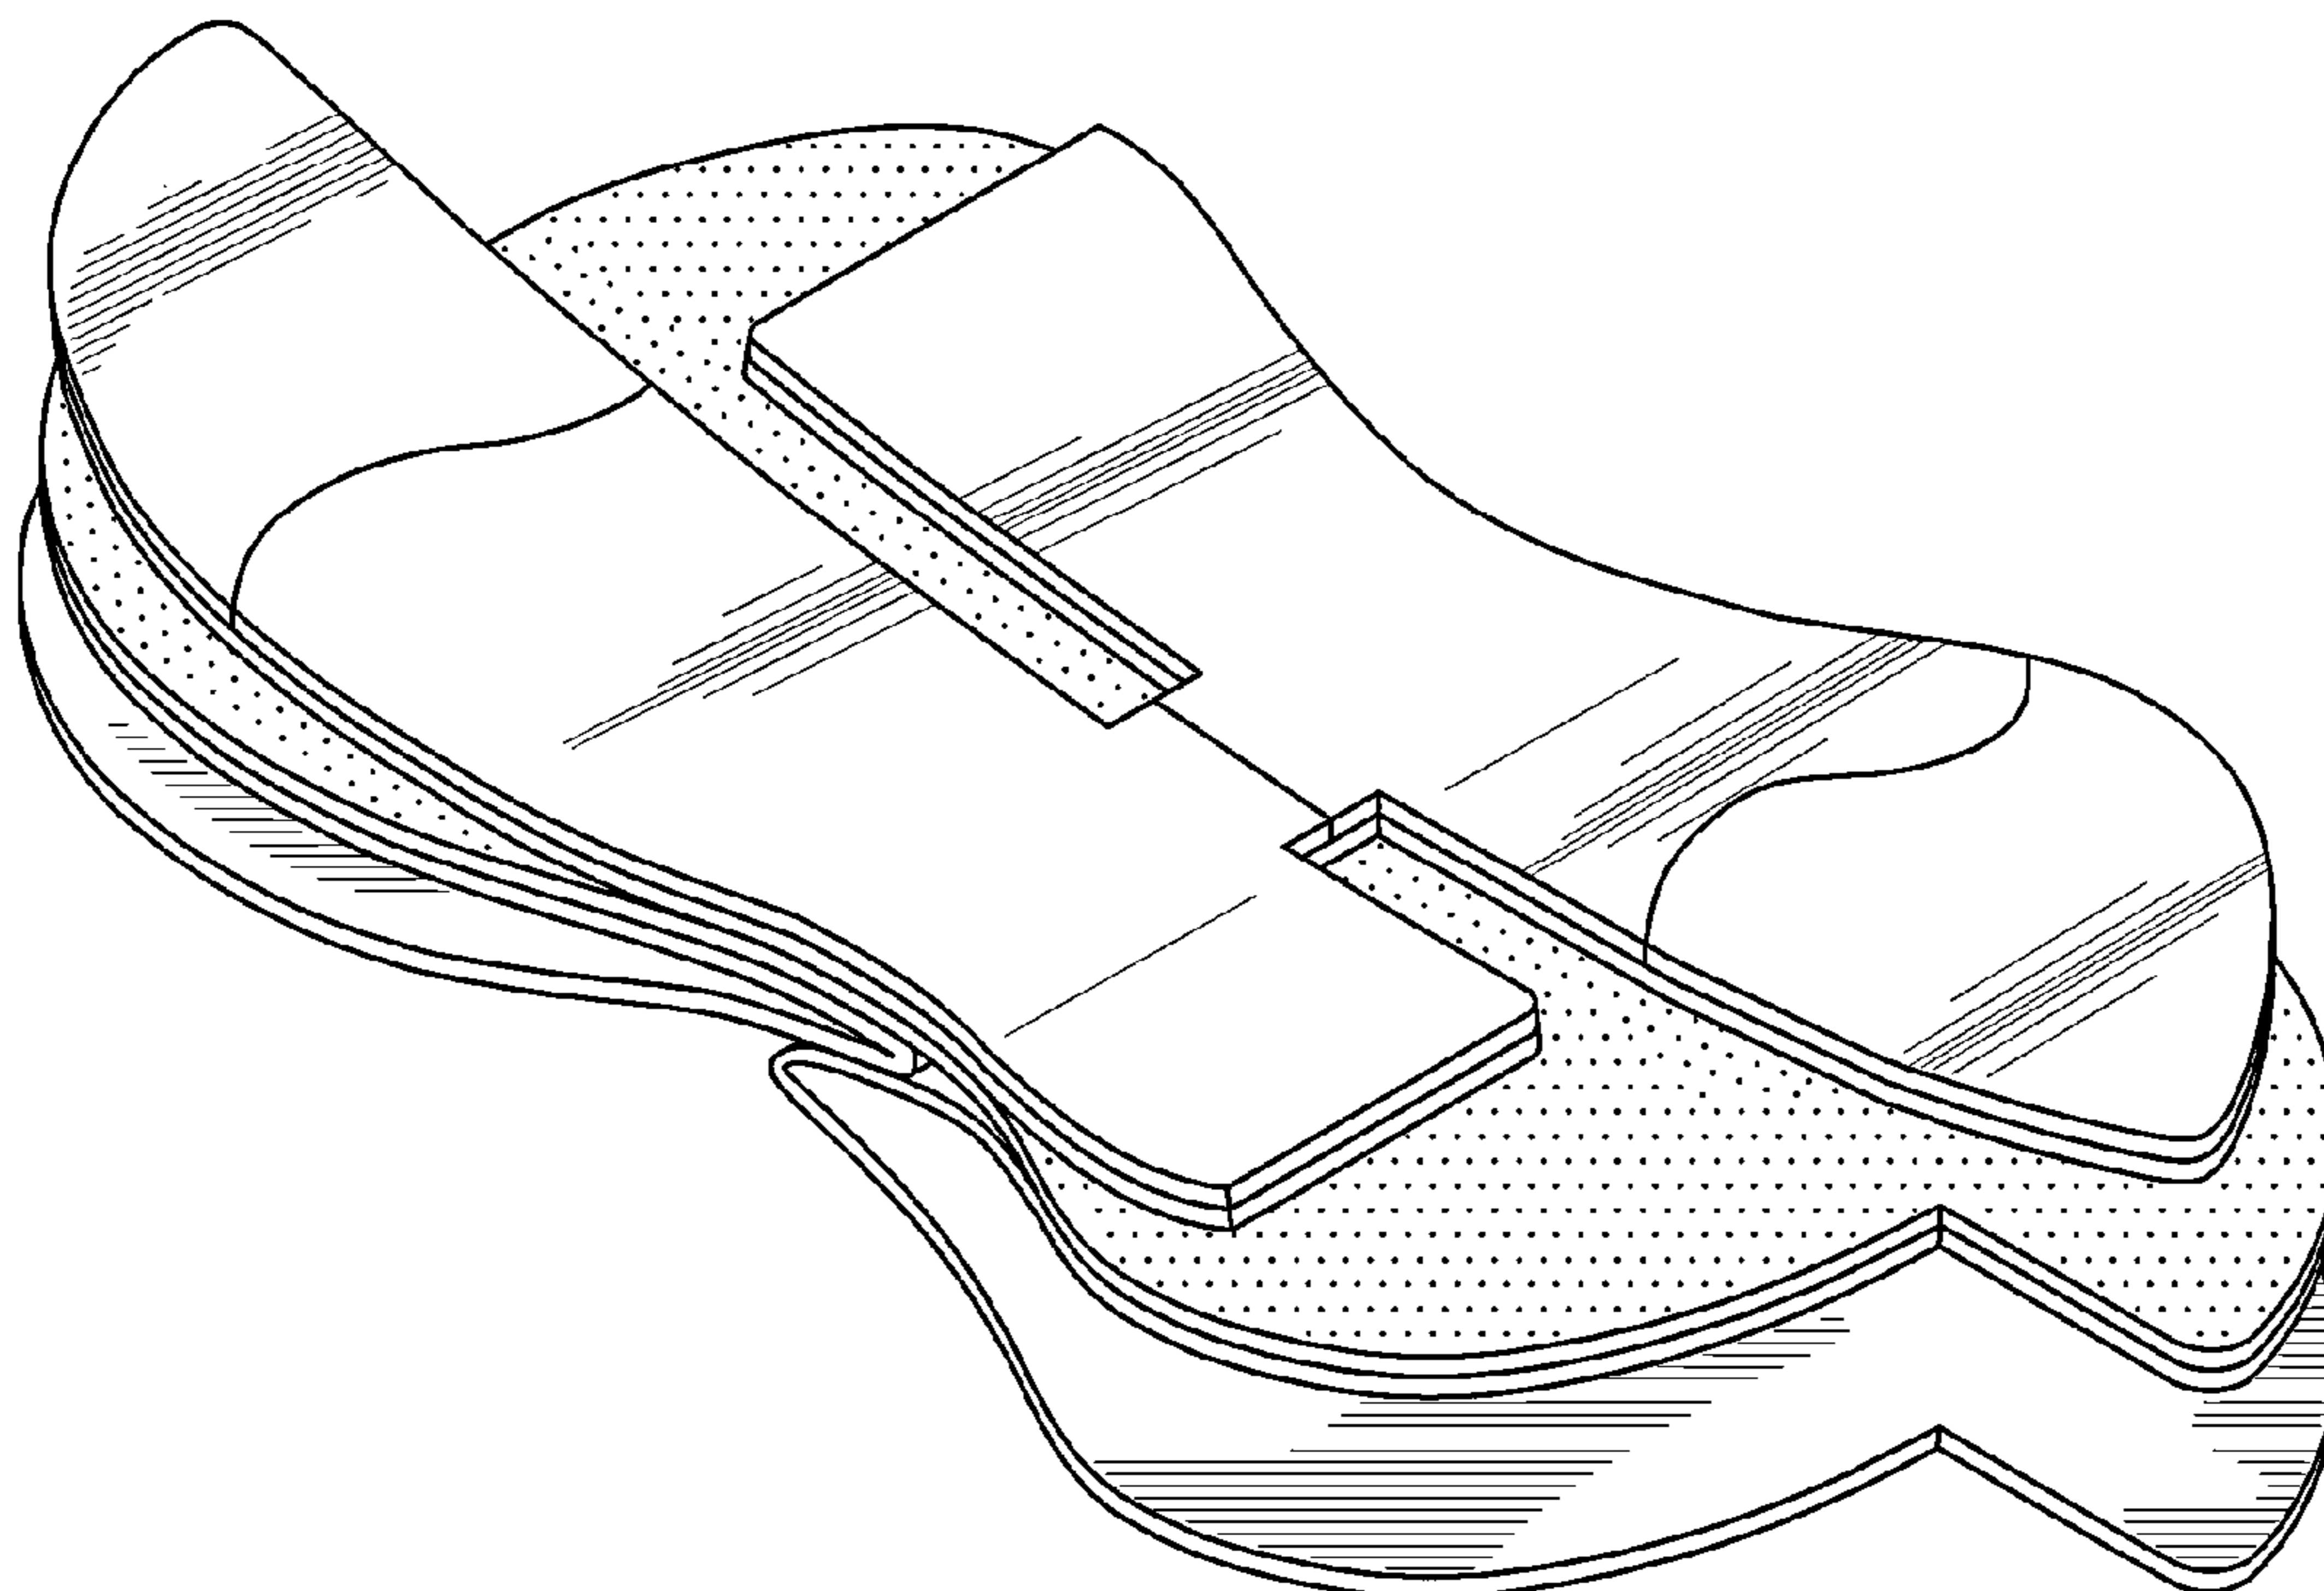


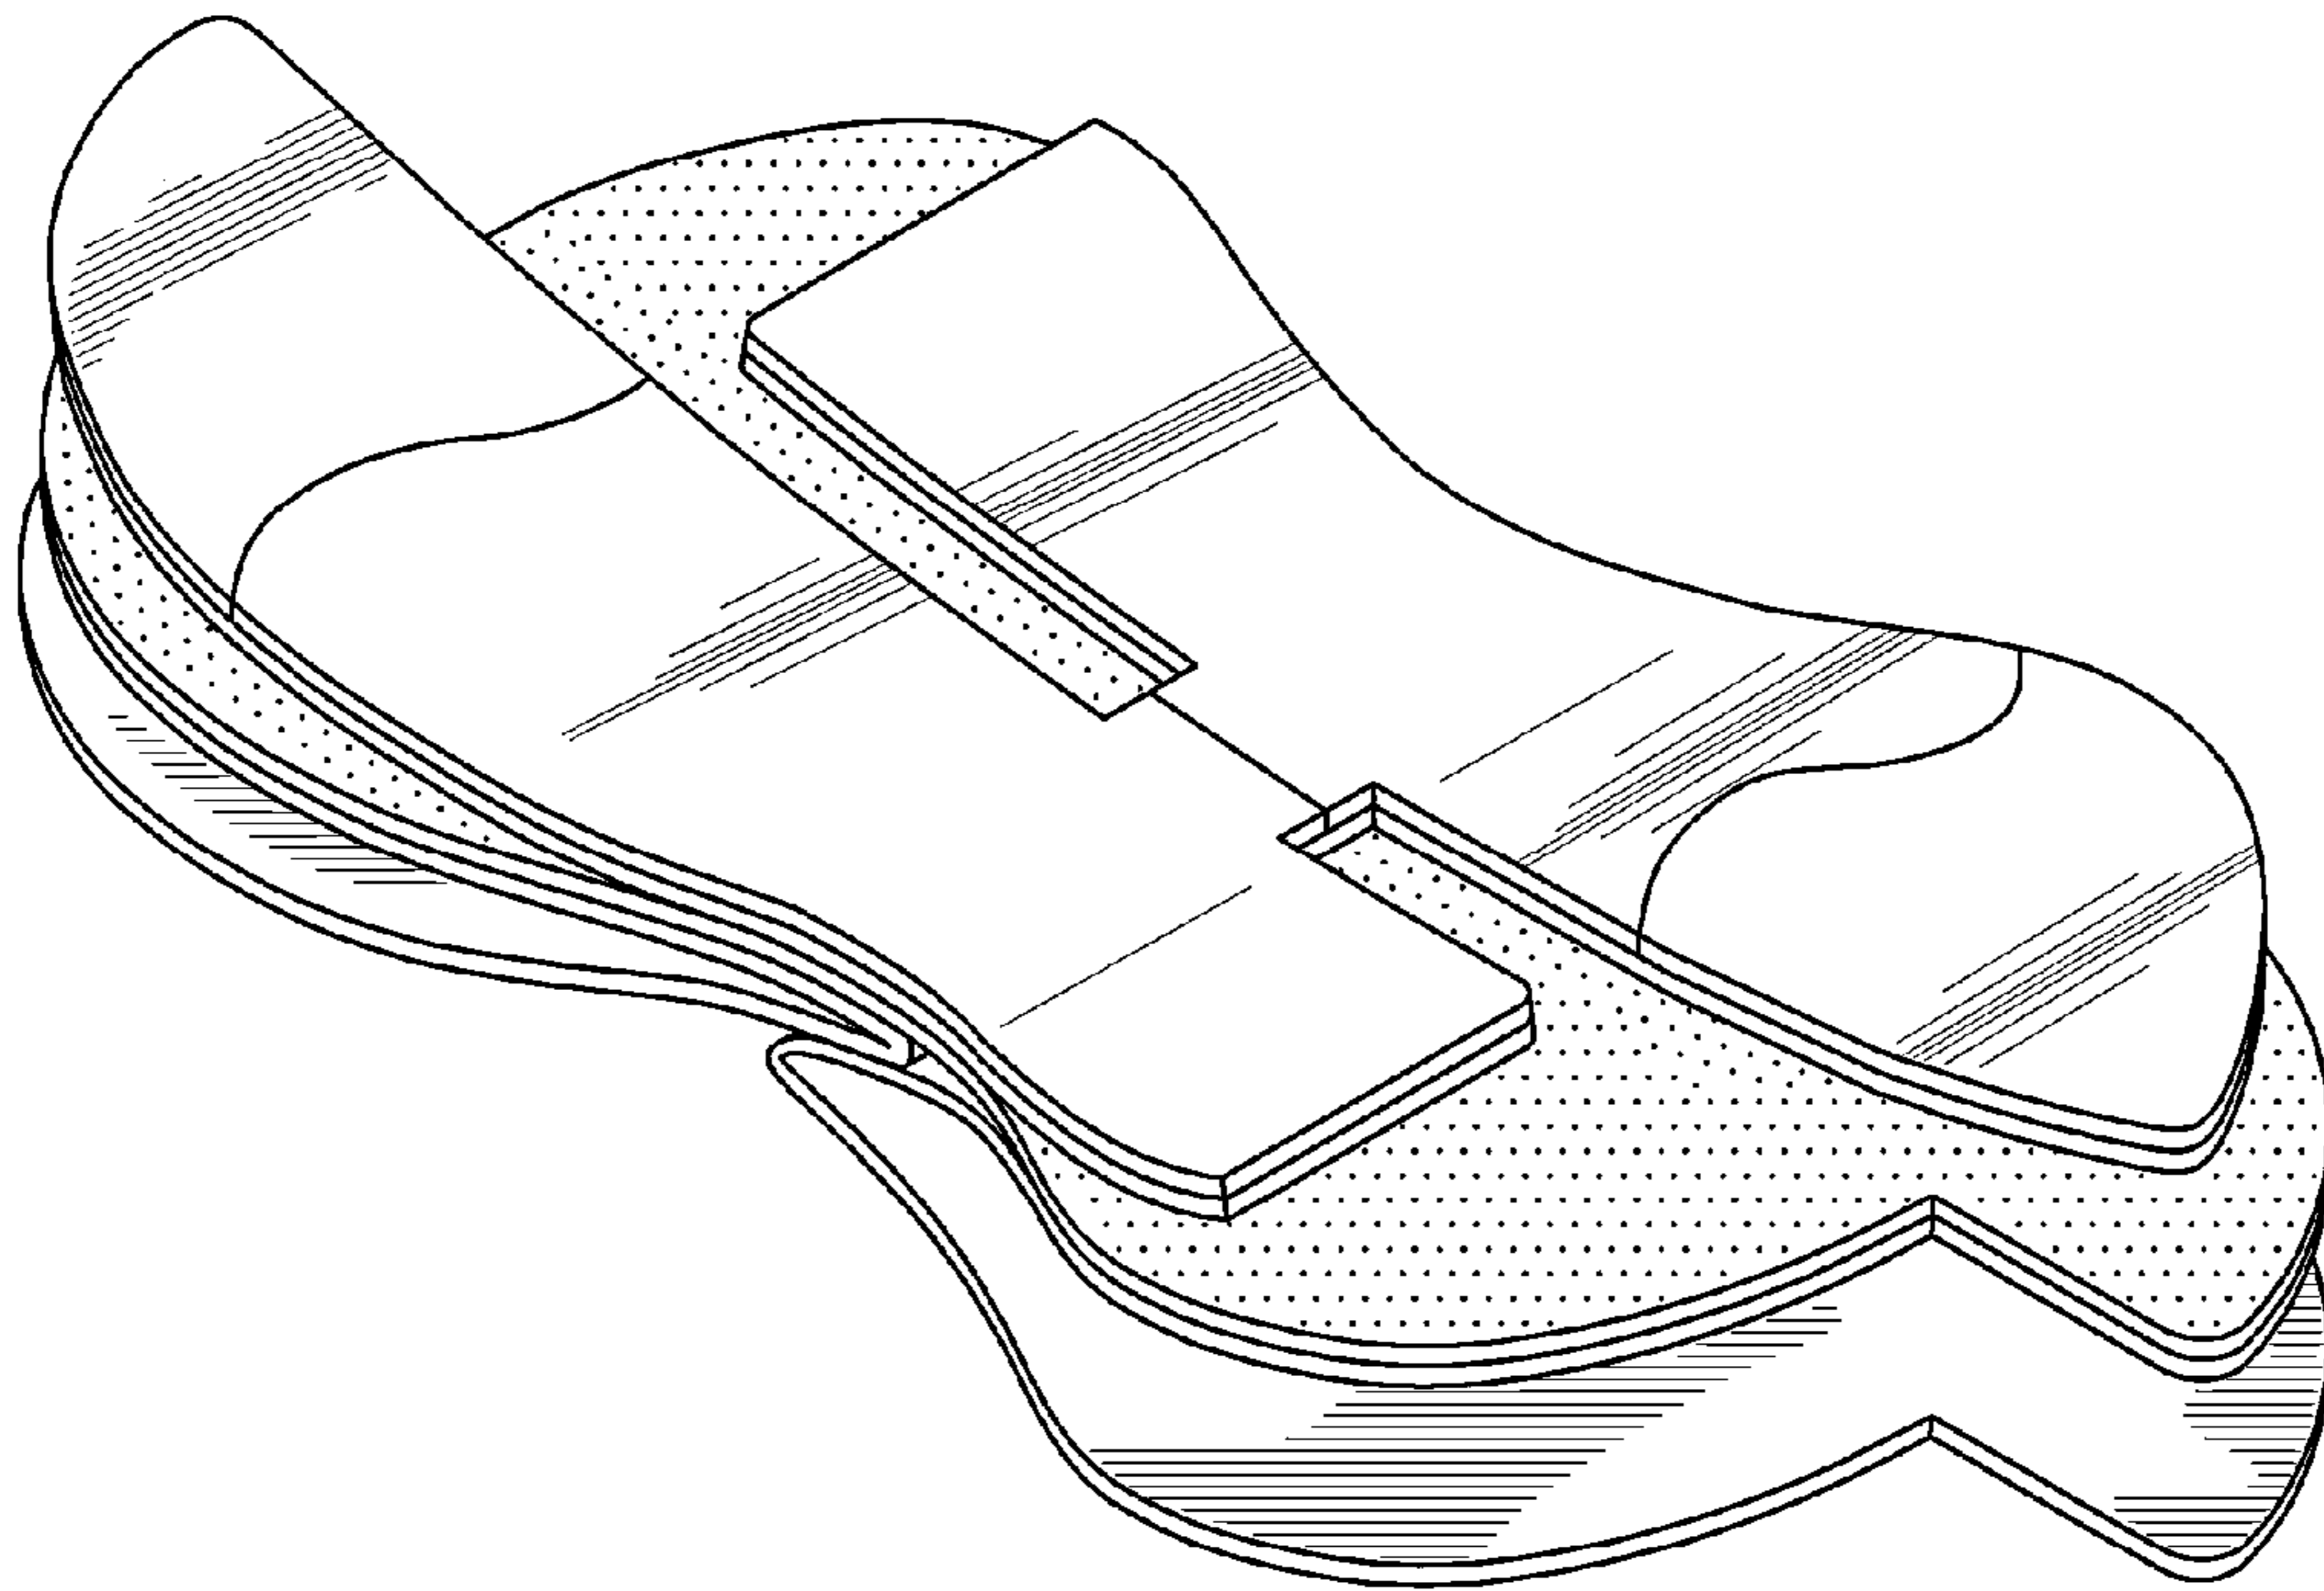


*Fig. 1*

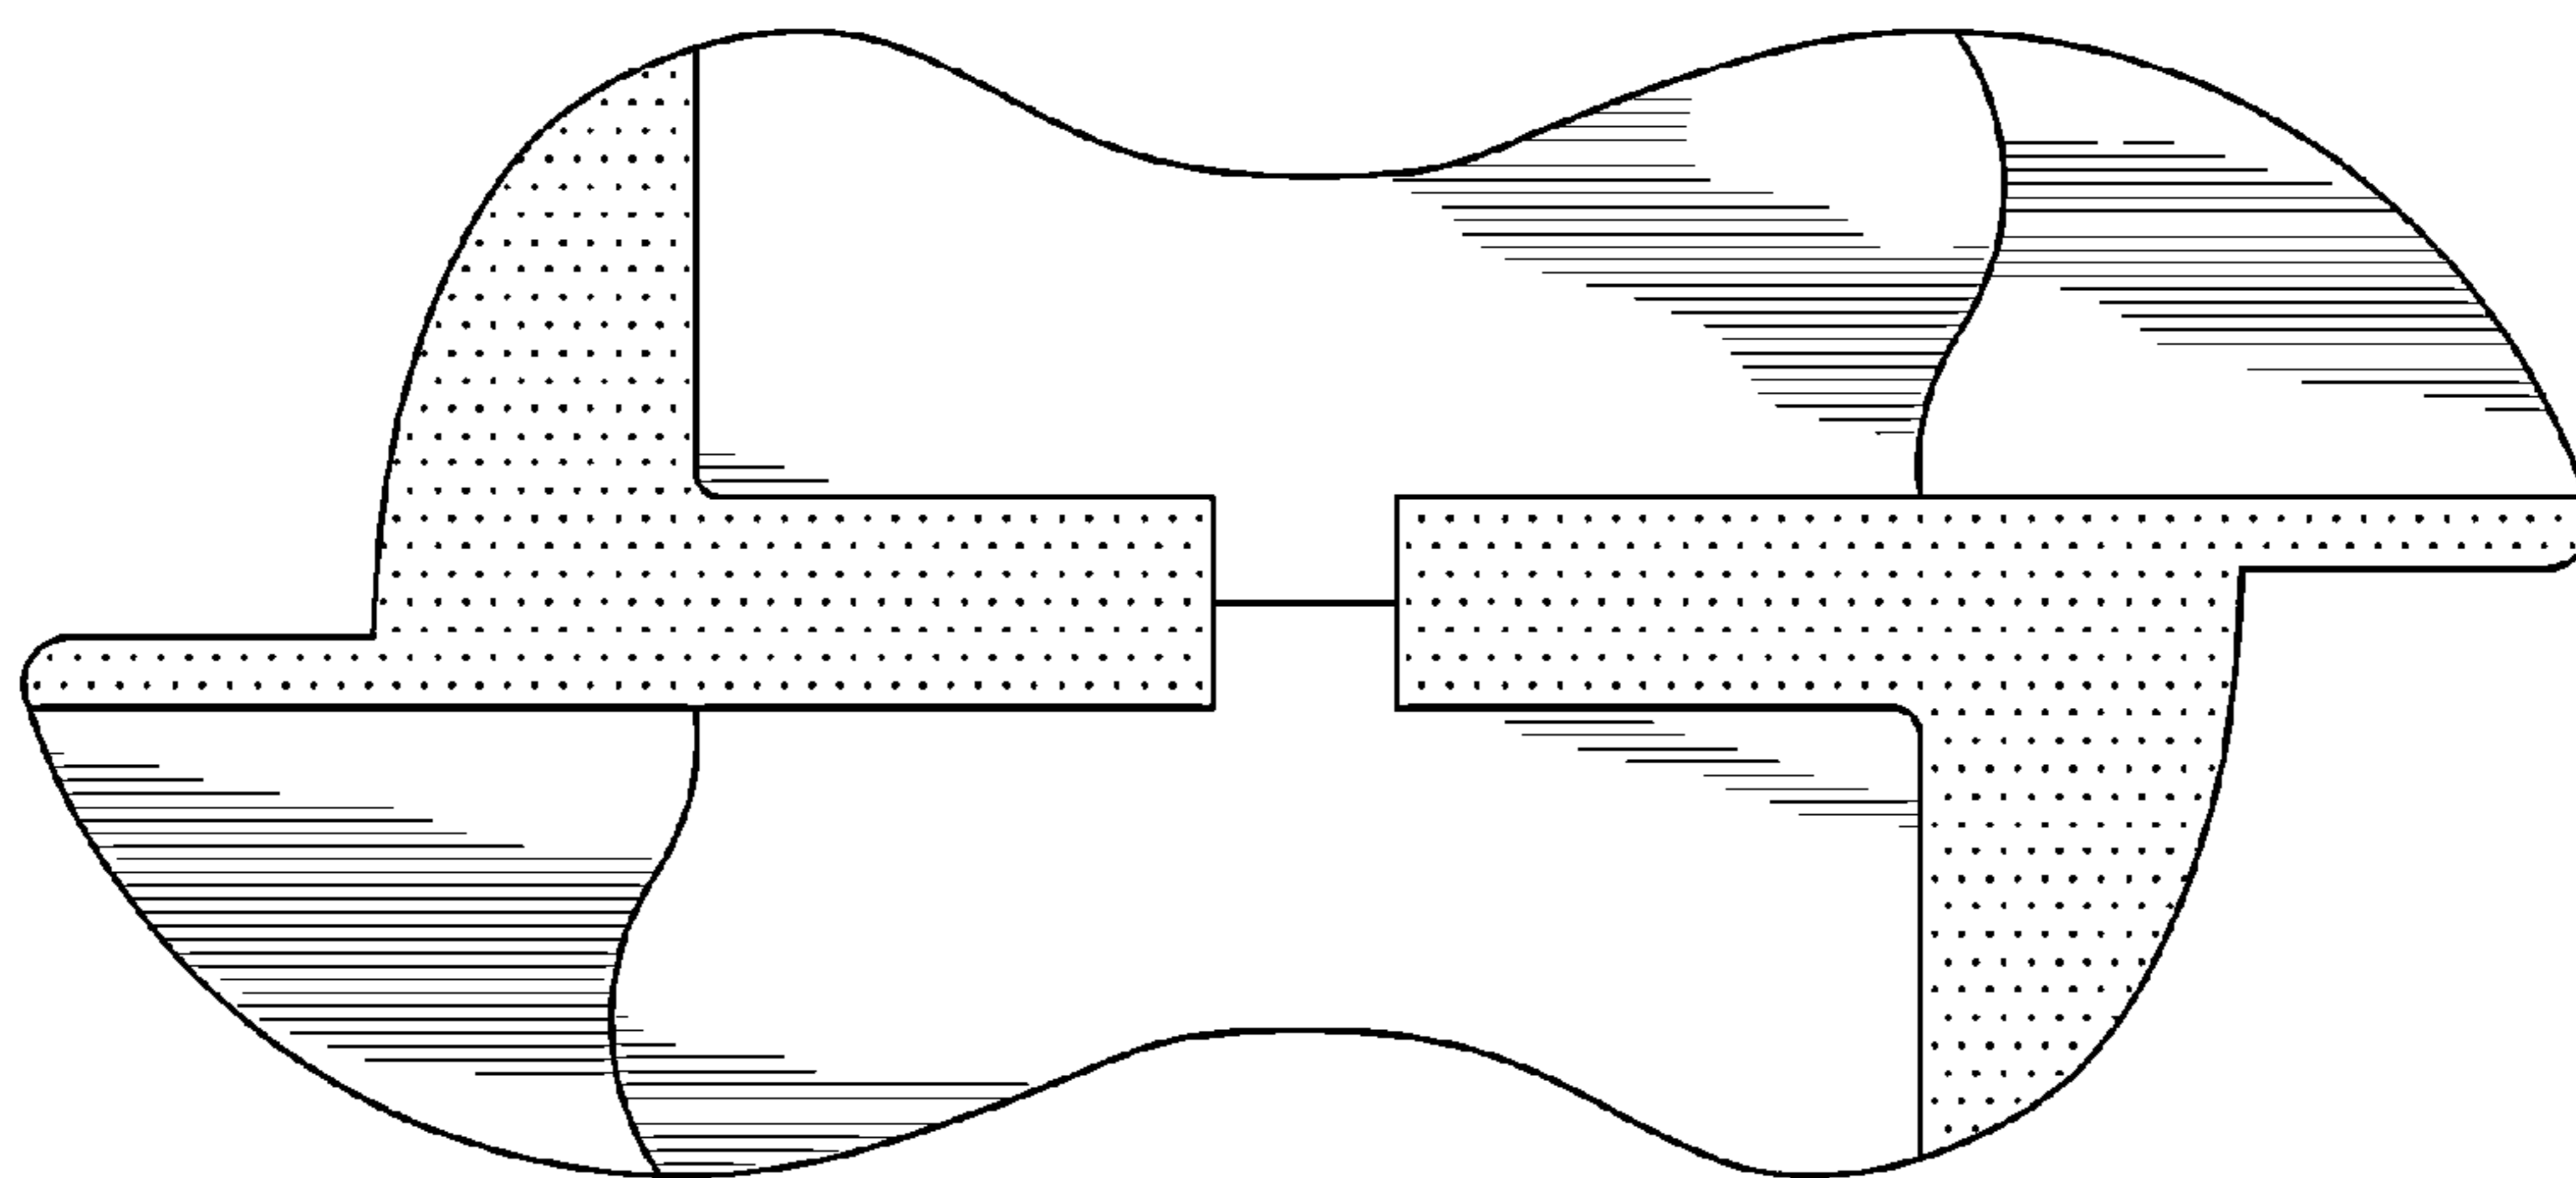


*Fig. 2*

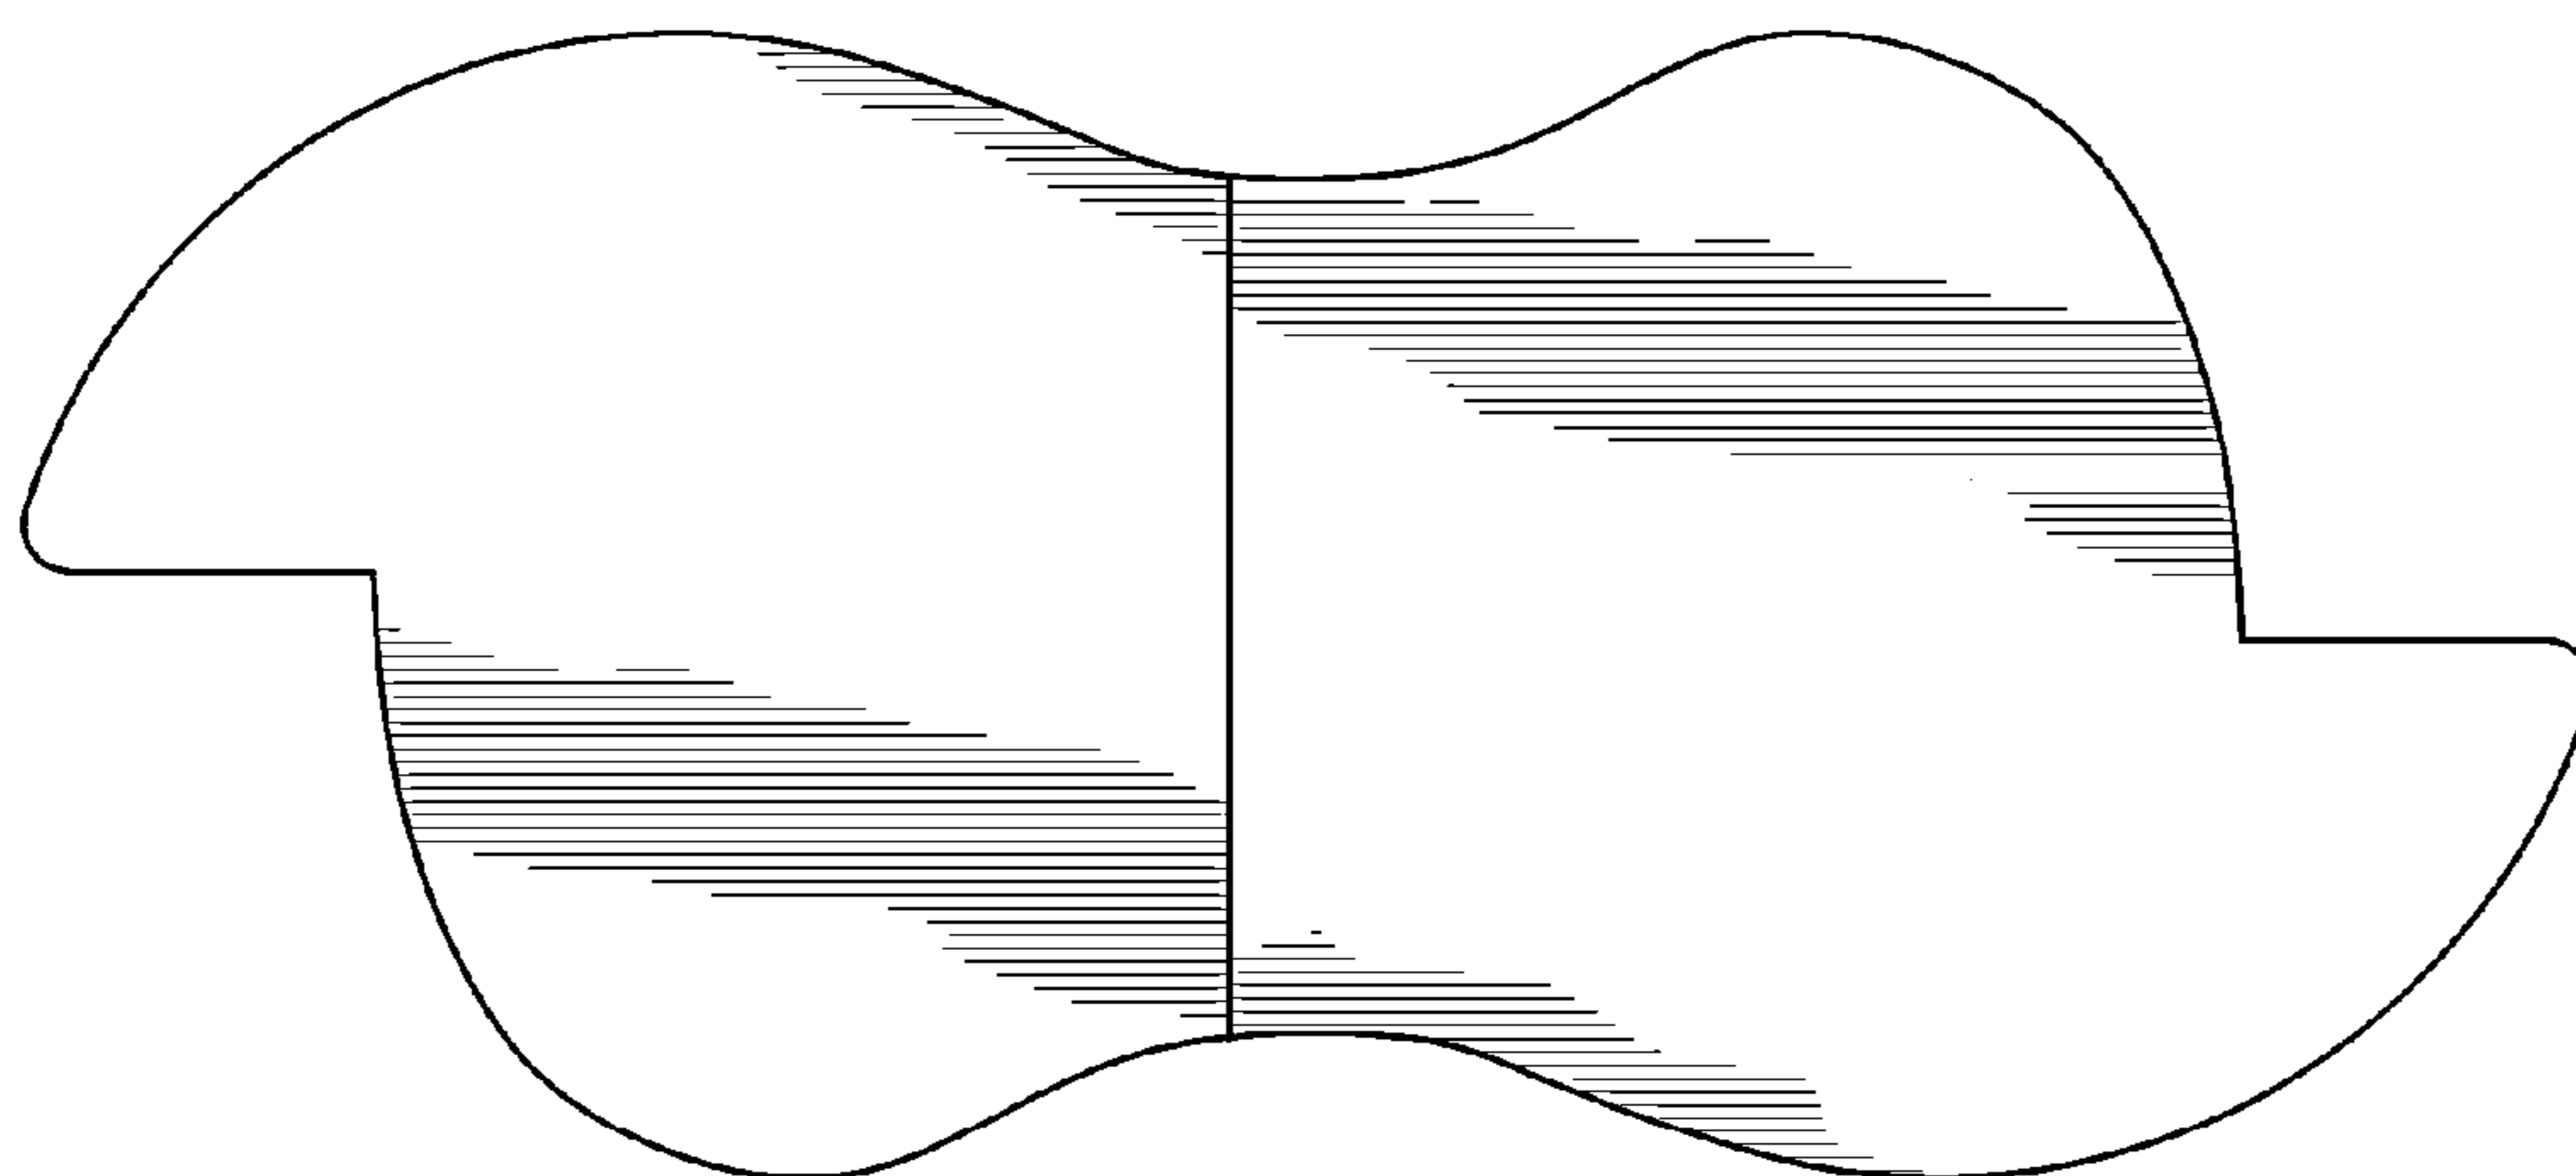

*Fig. 3*

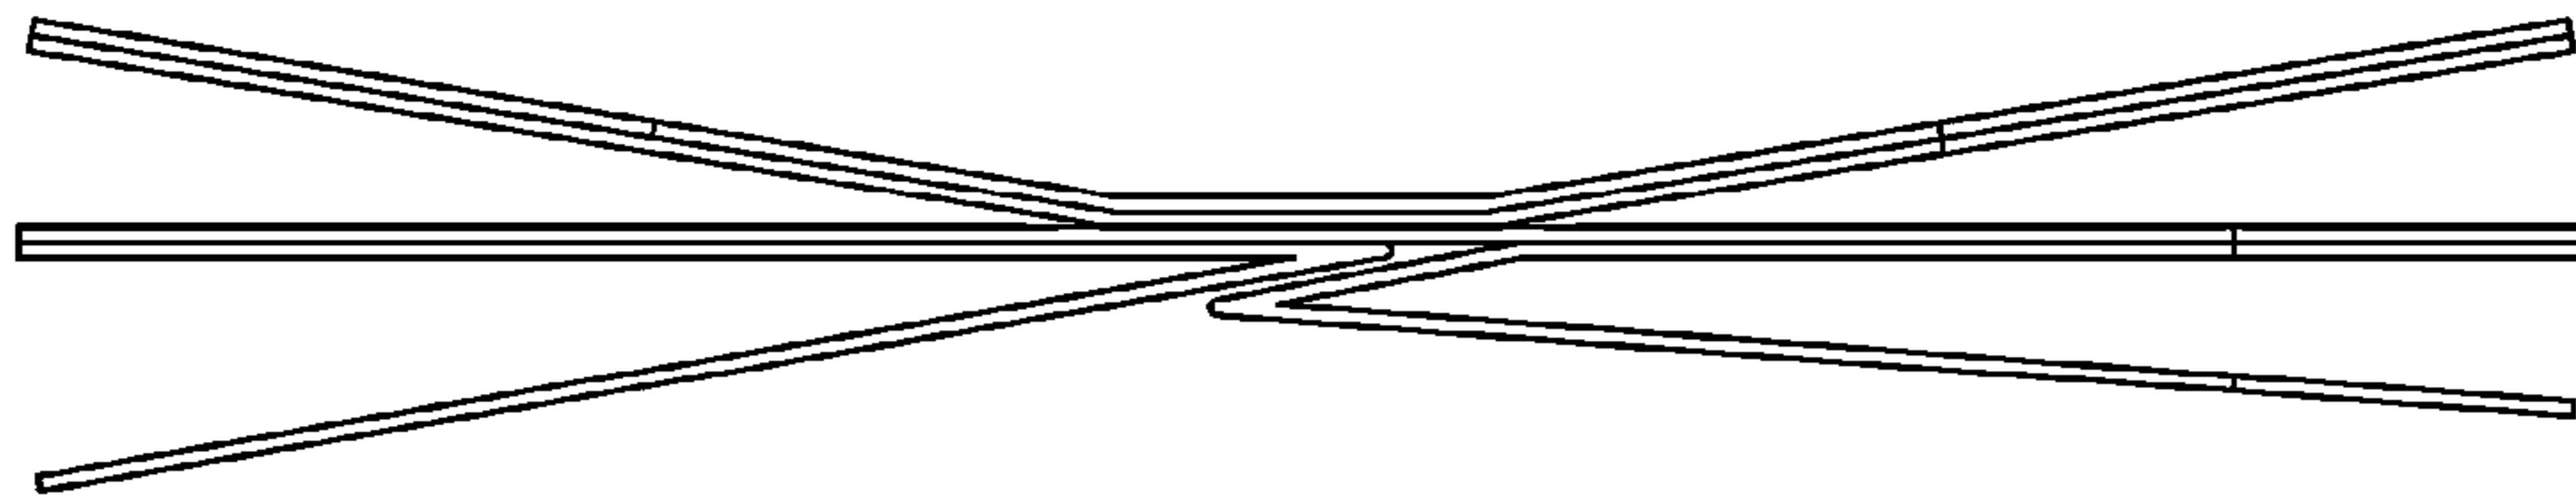

*Fig. 4*

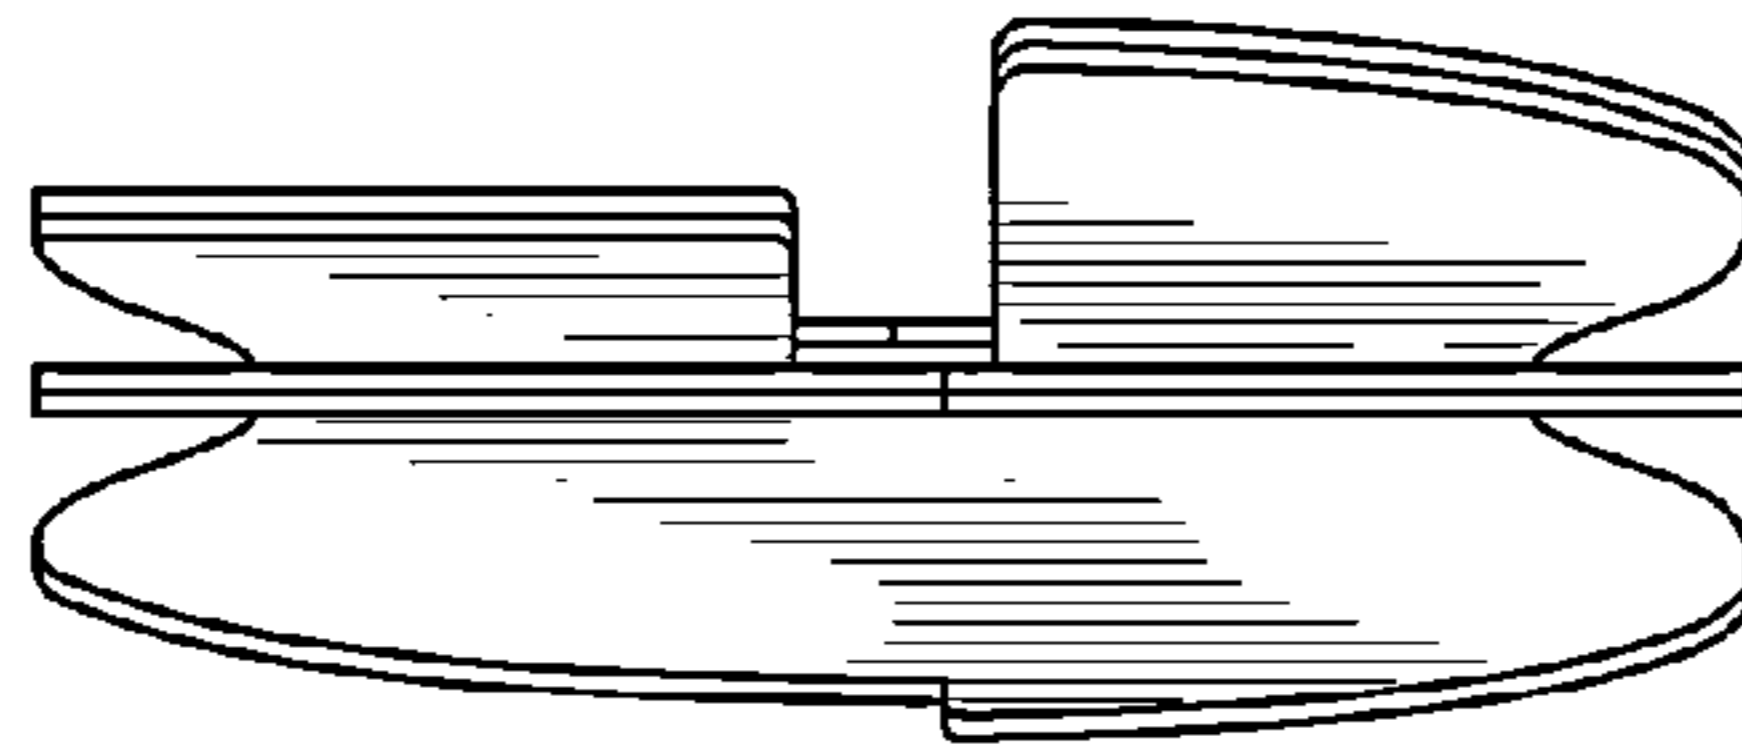

*Fig. 5*