



US00D718445S

(12) **United States Design Patent**
Yoshida et al.

(10) **Patent No.:** **US D718,445 S**

(45) **Date of Patent:** **** Nov. 25, 2014**

(54) **OPERATING GRIP FOR ENDOSCOPE**

(71) Applicant: **FUJIFILM Corporation**, Minato-ku,
Tokyo (JP)

(72) Inventors: **Koji Yoshida**, Ashigarakami-gun (JP);
Kunihiko Tanaka, Ashigarakami-gun
(JP)

(73) Assignee: **FUJIFILM Corporation**, Tokyo (JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/448,254**

(22) Filed: **Mar. 11, 2013**

(30) **Foreign Application Priority Data**

Sep. 12, 2012 (JP) 2012-022106

(51) **LOC (10) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/138**

(58) **Field of Classification Search**
CPC .. A61B 1/00; A61B 1/00064; A61B 1/00066;
A61B 1/0669
USPC D24/138, 137, 133, 135, 140;
600/101-183
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | | | |
|-----------|----|---|---------|-----------------|-------|---------|
| D277,406 | S | * | 1/1985 | Imada | | D24/138 |
| D486,910 | S | * | 2/2004 | Hayamizu et al. | | D24/138 |
| D493,529 | S | * | 7/2004 | Hayamizu et al. | | D24/138 |
| D498,846 | S | * | 11/2004 | Hayamizu et al. | | D24/138 |
| 6,852,077 | B2 | * | 2/2005 | Ouchi et al. | | 600/122 |
| D548,327 | S | * | 8/2007 | Fedenia et al. | | D24/108 |

| | | | | | | |
|--------------|----|---|---------|-----------------|-------|---------|
| D553,242 | S | * | 10/2007 | Fedenia et al. | | D24/108 |
| D638,937 | S | * | 5/2011 | Tanaka | | D24/138 |
| D641,470 | S | * | 7/2011 | Hayamizu | | D24/138 |
| D648,023 | S | * | 11/2011 | Nohara et al. | | D24/138 |
| D649,244 | S | * | 11/2011 | Nohara et al. | | D24/138 |
| 8,182,419 | B2 | * | 5/2012 | Kohno | | 600/158 |
| D668,762 | S | * | 10/2012 | Makowski et al. | | D24/138 |
| D669,174 | S | * | 10/2012 | Makowski et al. | | D24/138 |
| D669,175 | S | * | 10/2012 | Makowski et al. | | D24/138 |
| 2001/0018552 | A1 | * | 8/2001 | Akiba | | 600/146 |
| 2002/0091303 | A1 | * | 7/2002 | Ootawara et al. | | 600/106 |
| 2002/0188174 | A1 | * | 12/2002 | Aizawa et al. | | 600/118 |
| 2003/0216613 | A1 | * | 11/2003 | Suzuki et al. | | 600/104 |
| 2008/0119696 | A1 | * | 5/2008 | Moriyama | | 600/146 |
| 2009/0048487 | A1 | * | 2/2009 | Yanuma | | 600/139 |
| 2011/0046442 | A1 | * | 2/2011 | Matsushita | | 600/114 |
| 2011/0077463 | A1 | * | 3/2011 | Hirota | | 600/114 |
| 2013/0012780 | A1 | * | 1/2013 | Nakamura et al. | | 600/122 |
| 2014/0187864 | A1 | * | 7/2014 | Kubo | | 600/139 |

* cited by examiner

Primary Examiner — Bridget L Eland

(74) *Attorney, Agent, or Firm* — Sughrue Mion, PLLC

(57) **CLAIM**

The ornamental design for an operating grip for endoscope, as shown and described.

DESCRIPTION

FIG. 1 is a top, front and side perspective view of an operating grip for endoscope showing our new design;
FIG. 2 is a bottom, front and side perspective view thereof;
FIG. 3 is a top, rear and side perspective view thereof;
FIG. 4 is a front elevational view thereof;
FIG. 5 is a rear elevational view thereof;
FIG. 6 is a top plan view thereof;
FIG. 7 is a bottom plan view thereof;
FIG. 8 is a left side elevational view thereof; and,
FIG. 9 is a right side elevational view thereof.

1 Claim, 9 Drawing Sheets

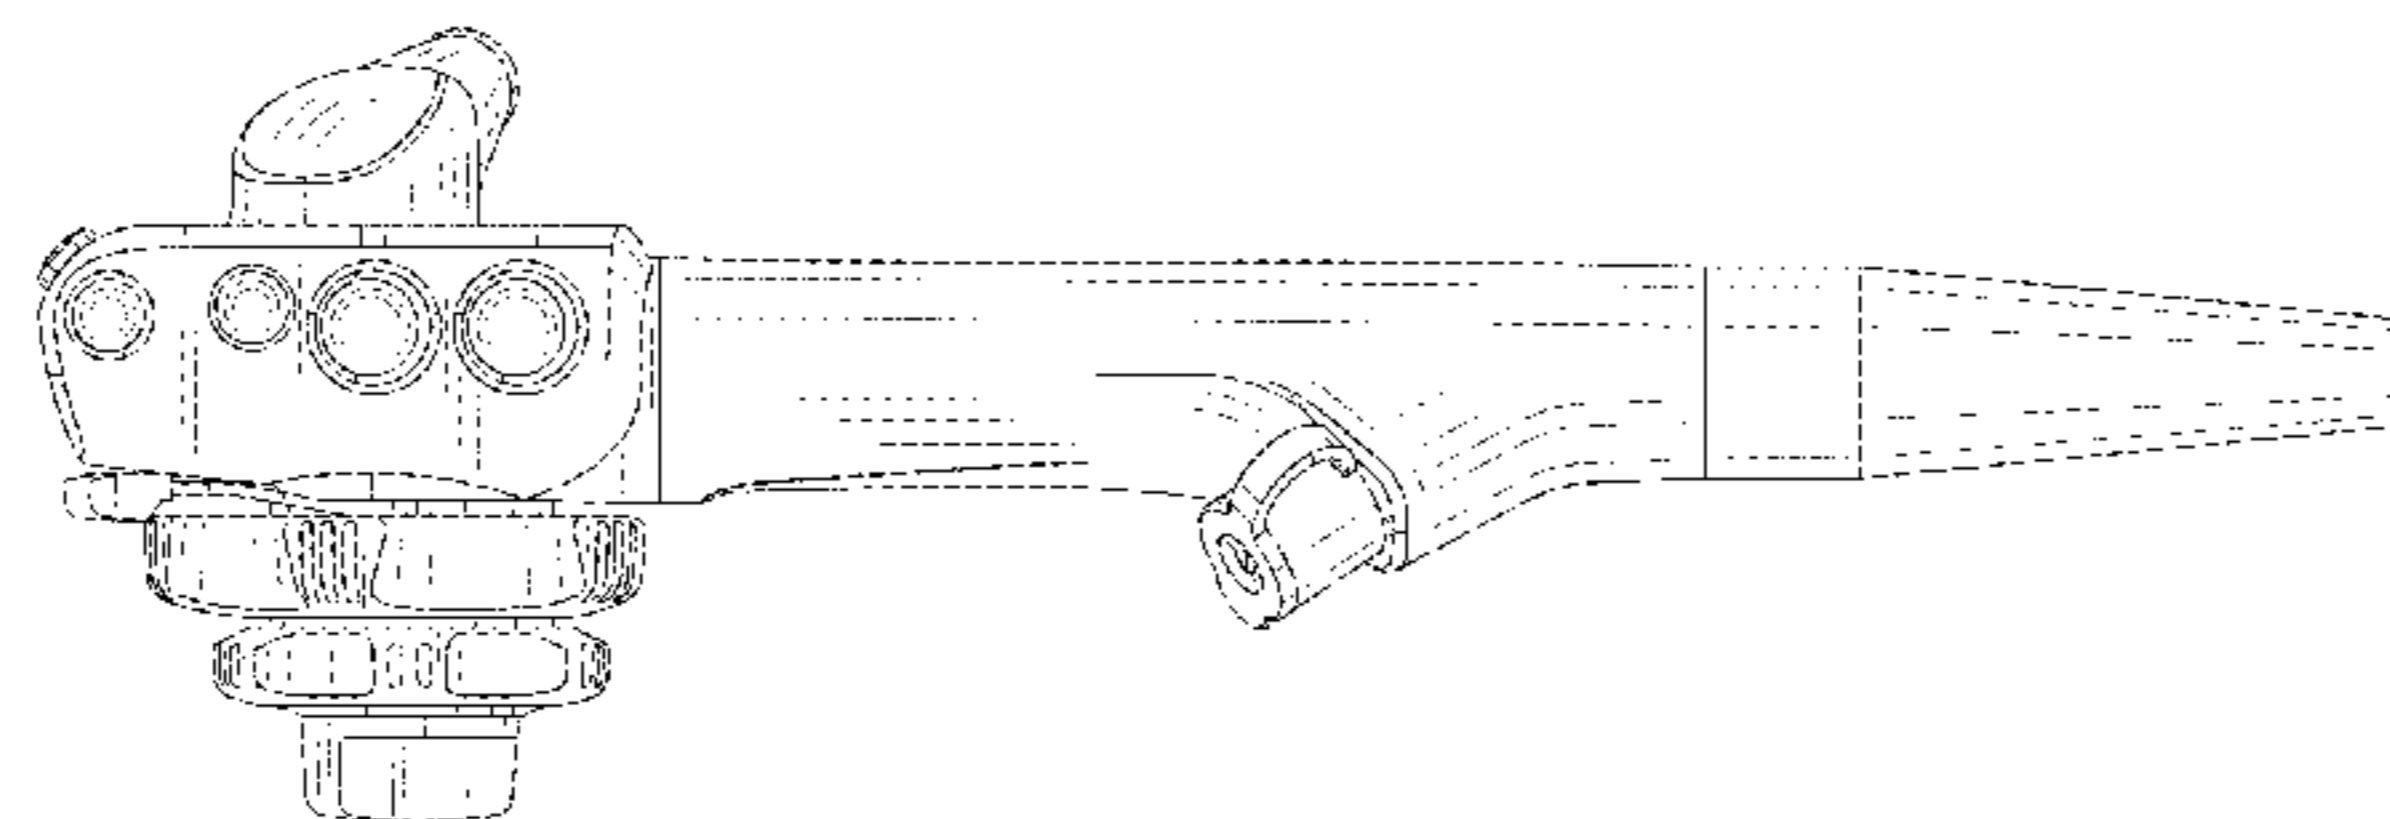
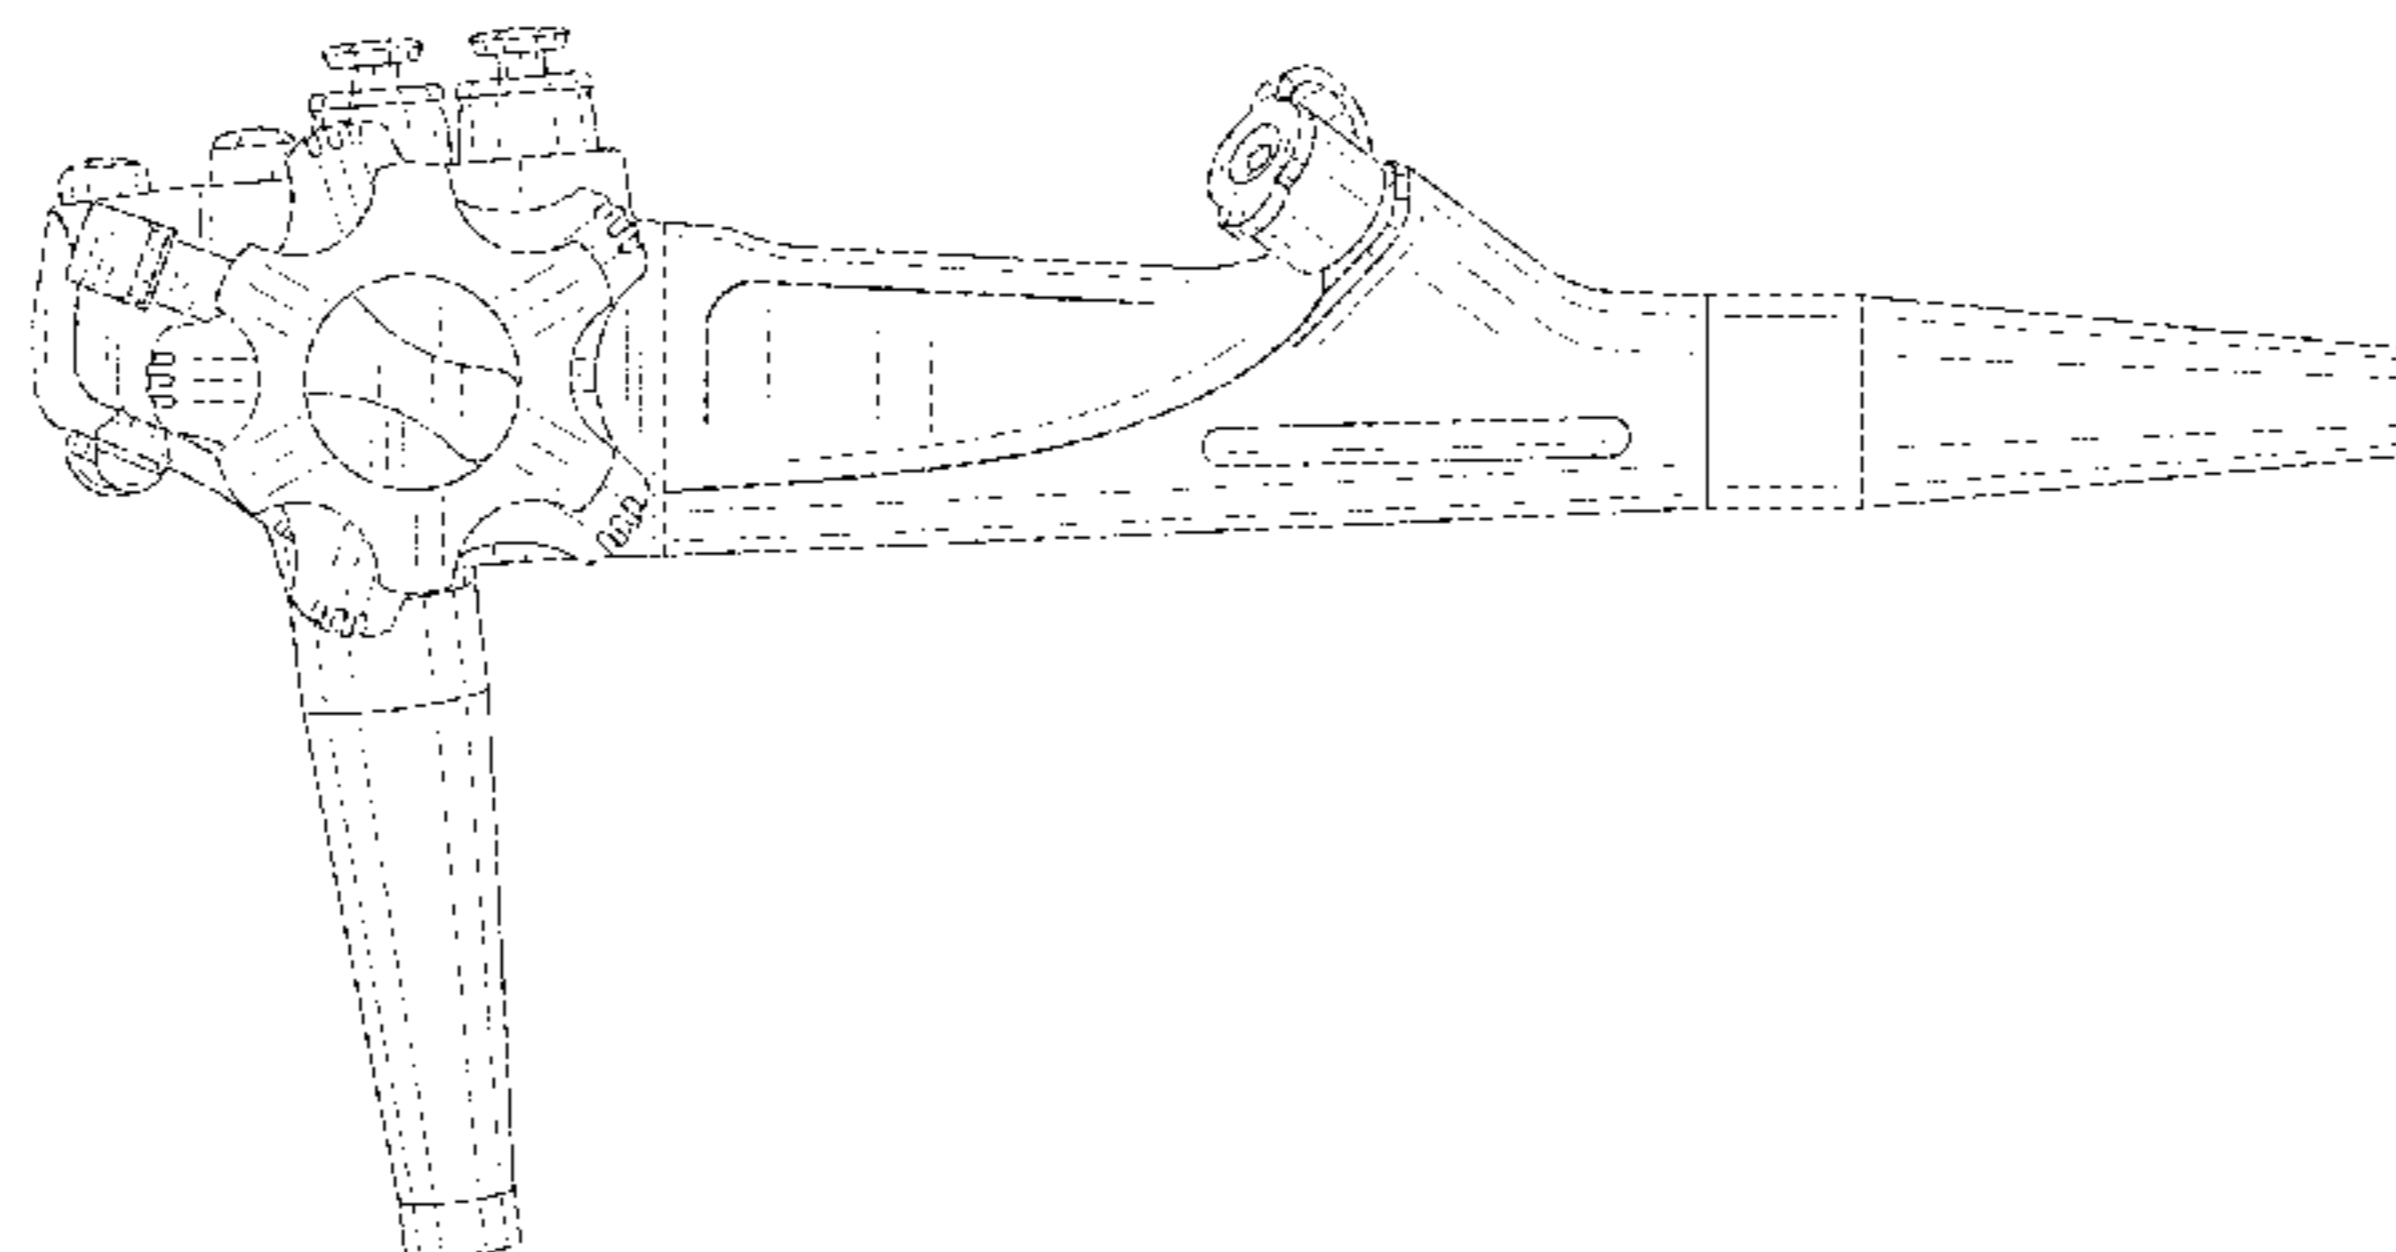


FIG.1

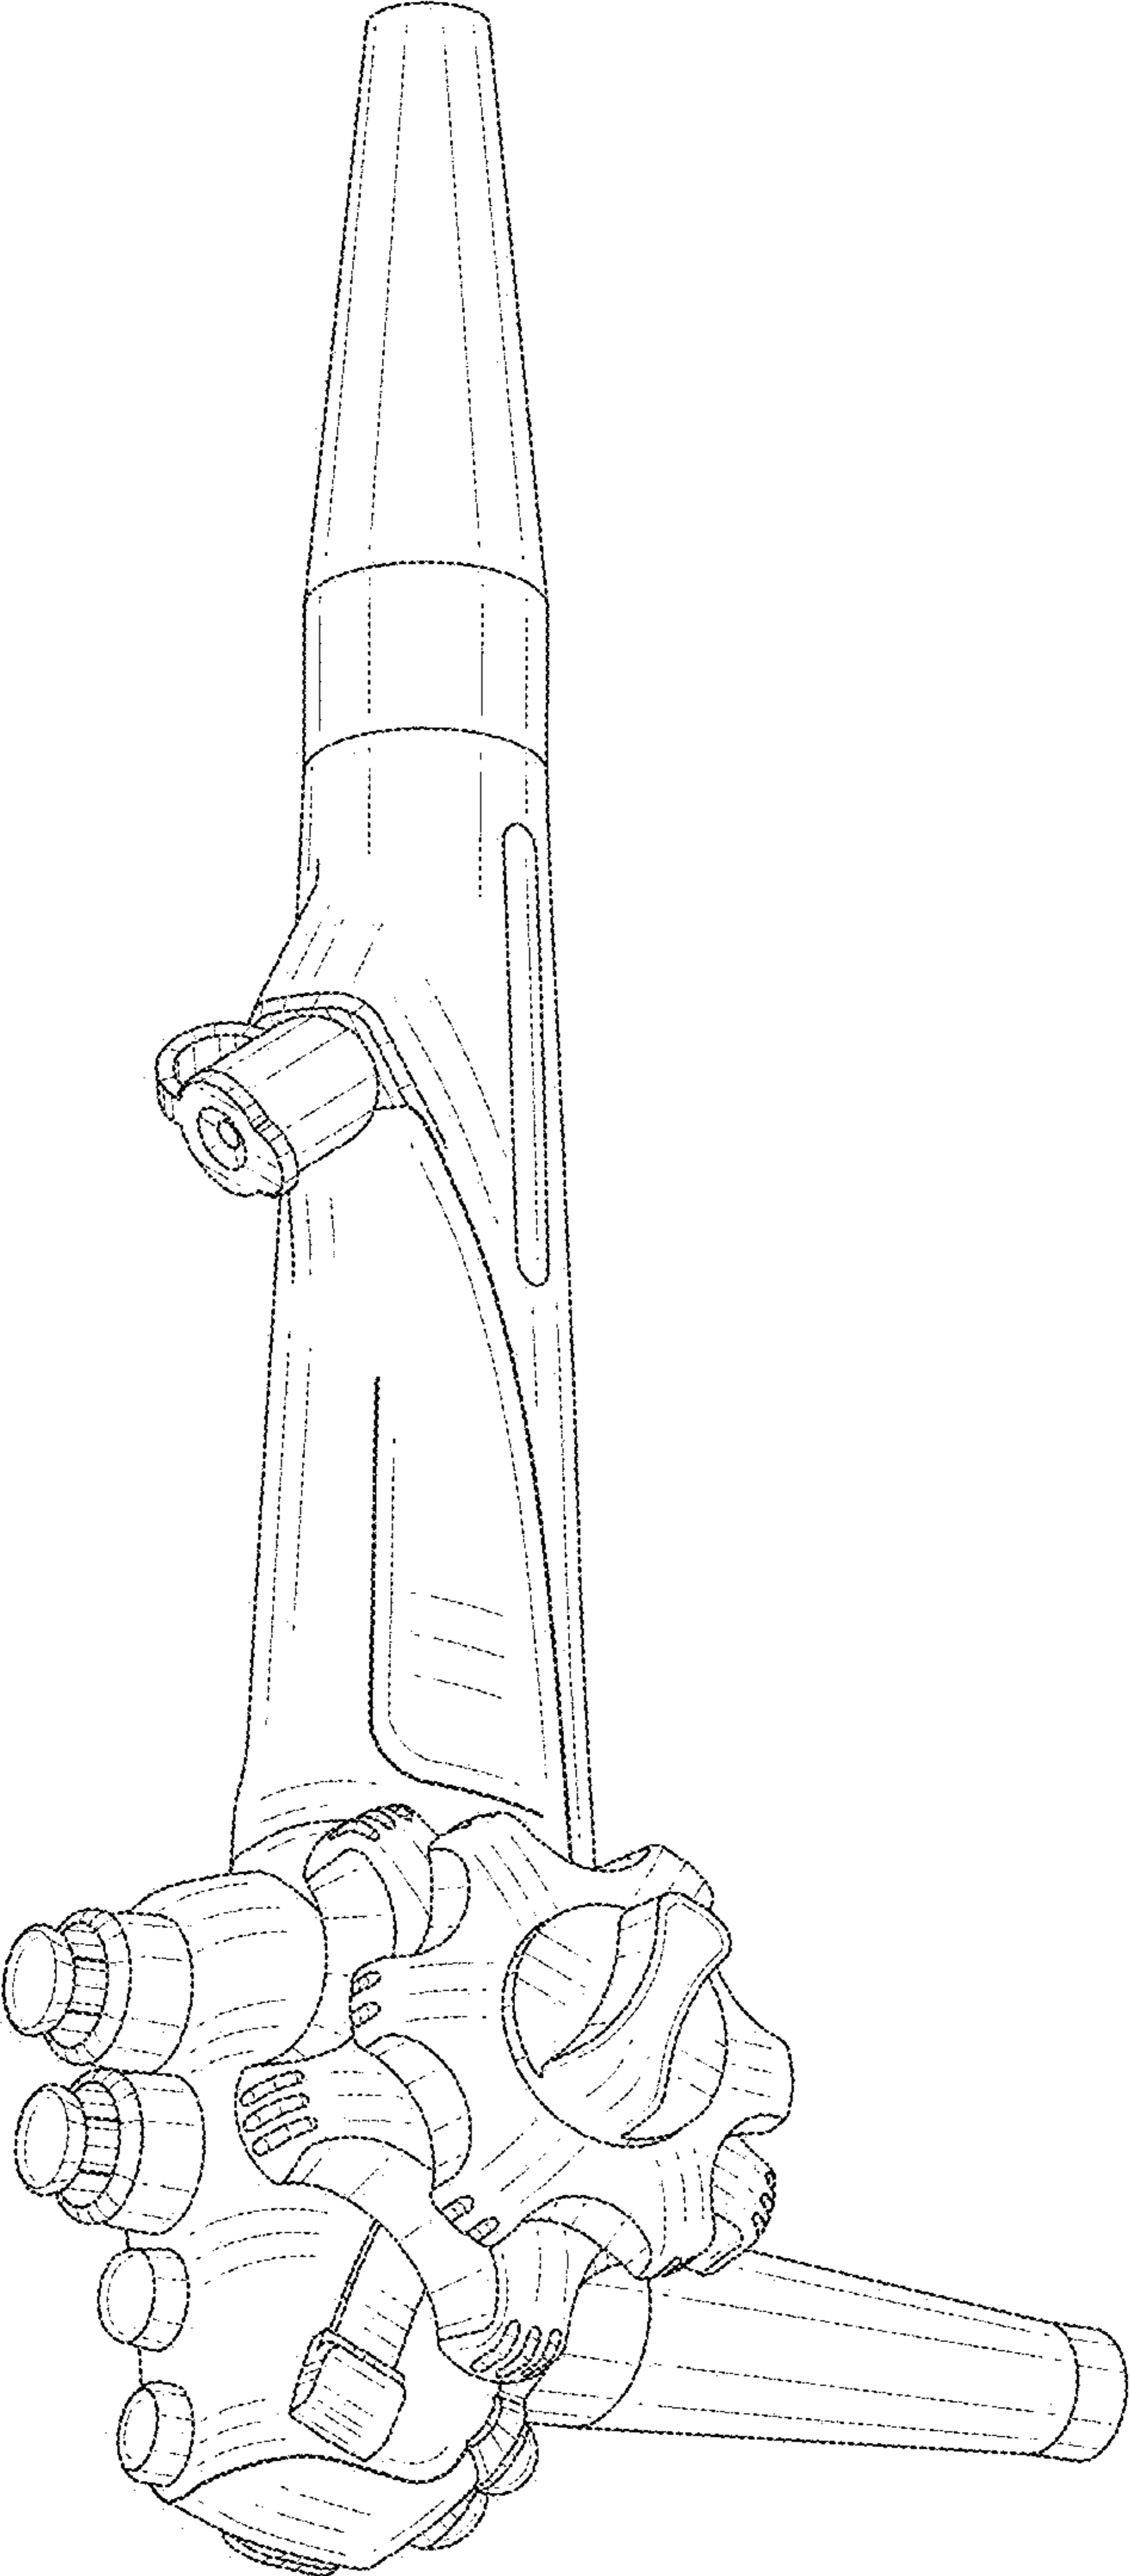


FIG.2

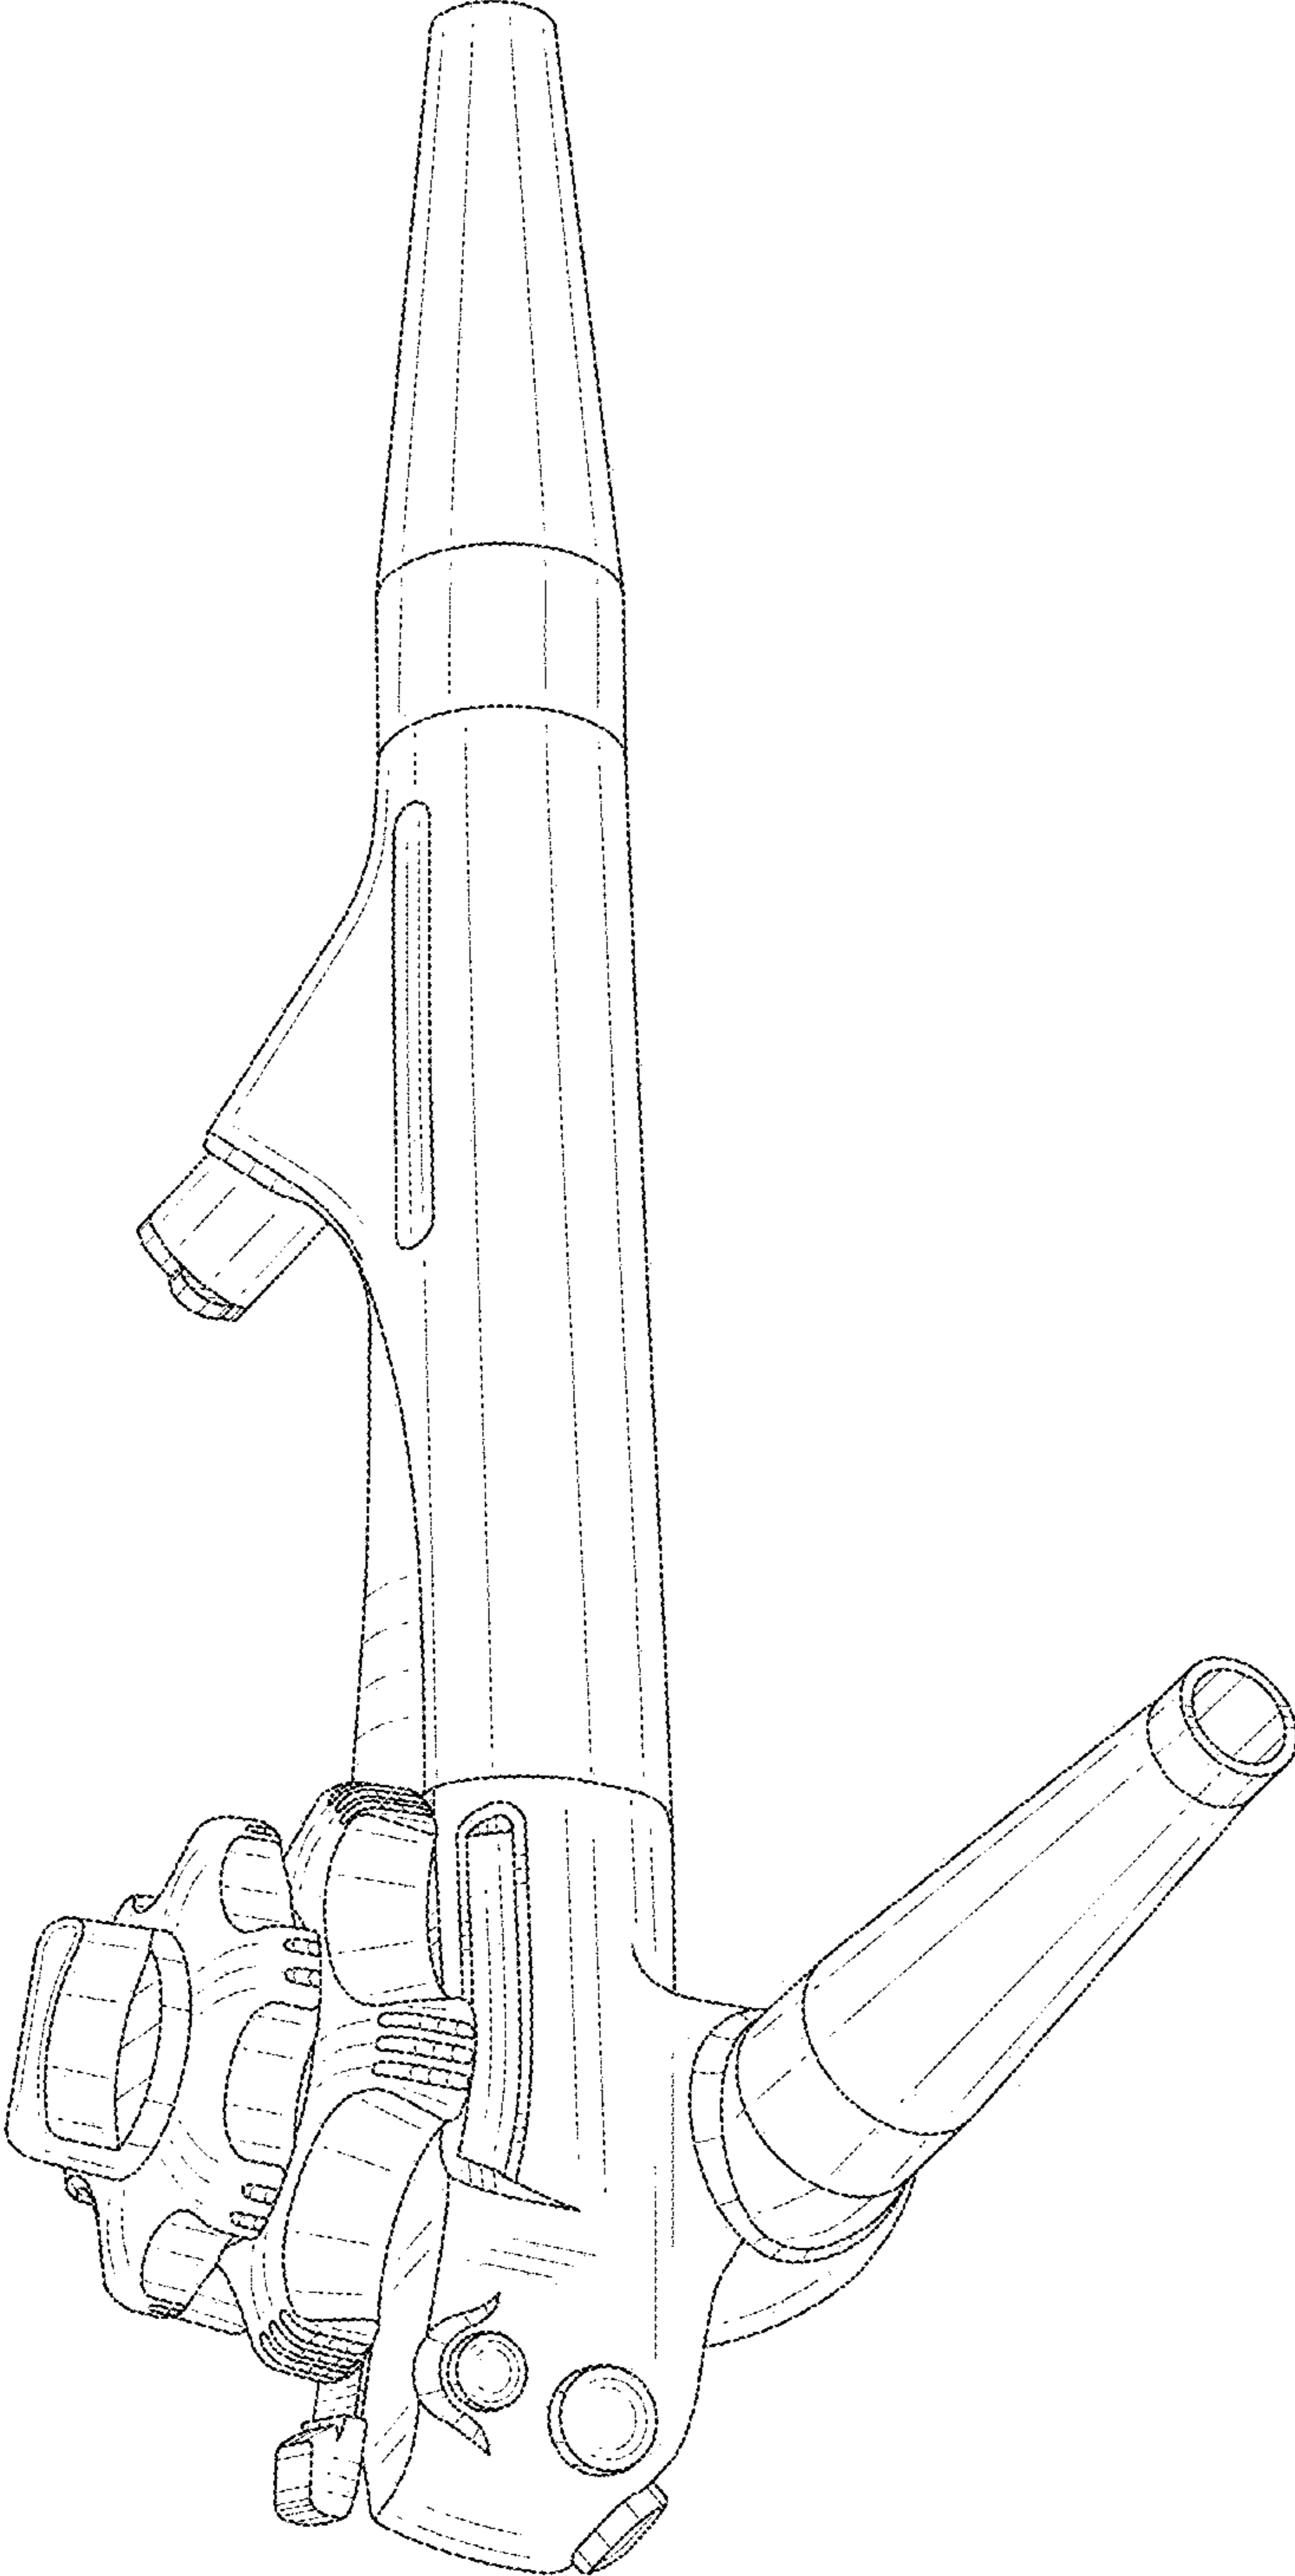


FIG.3

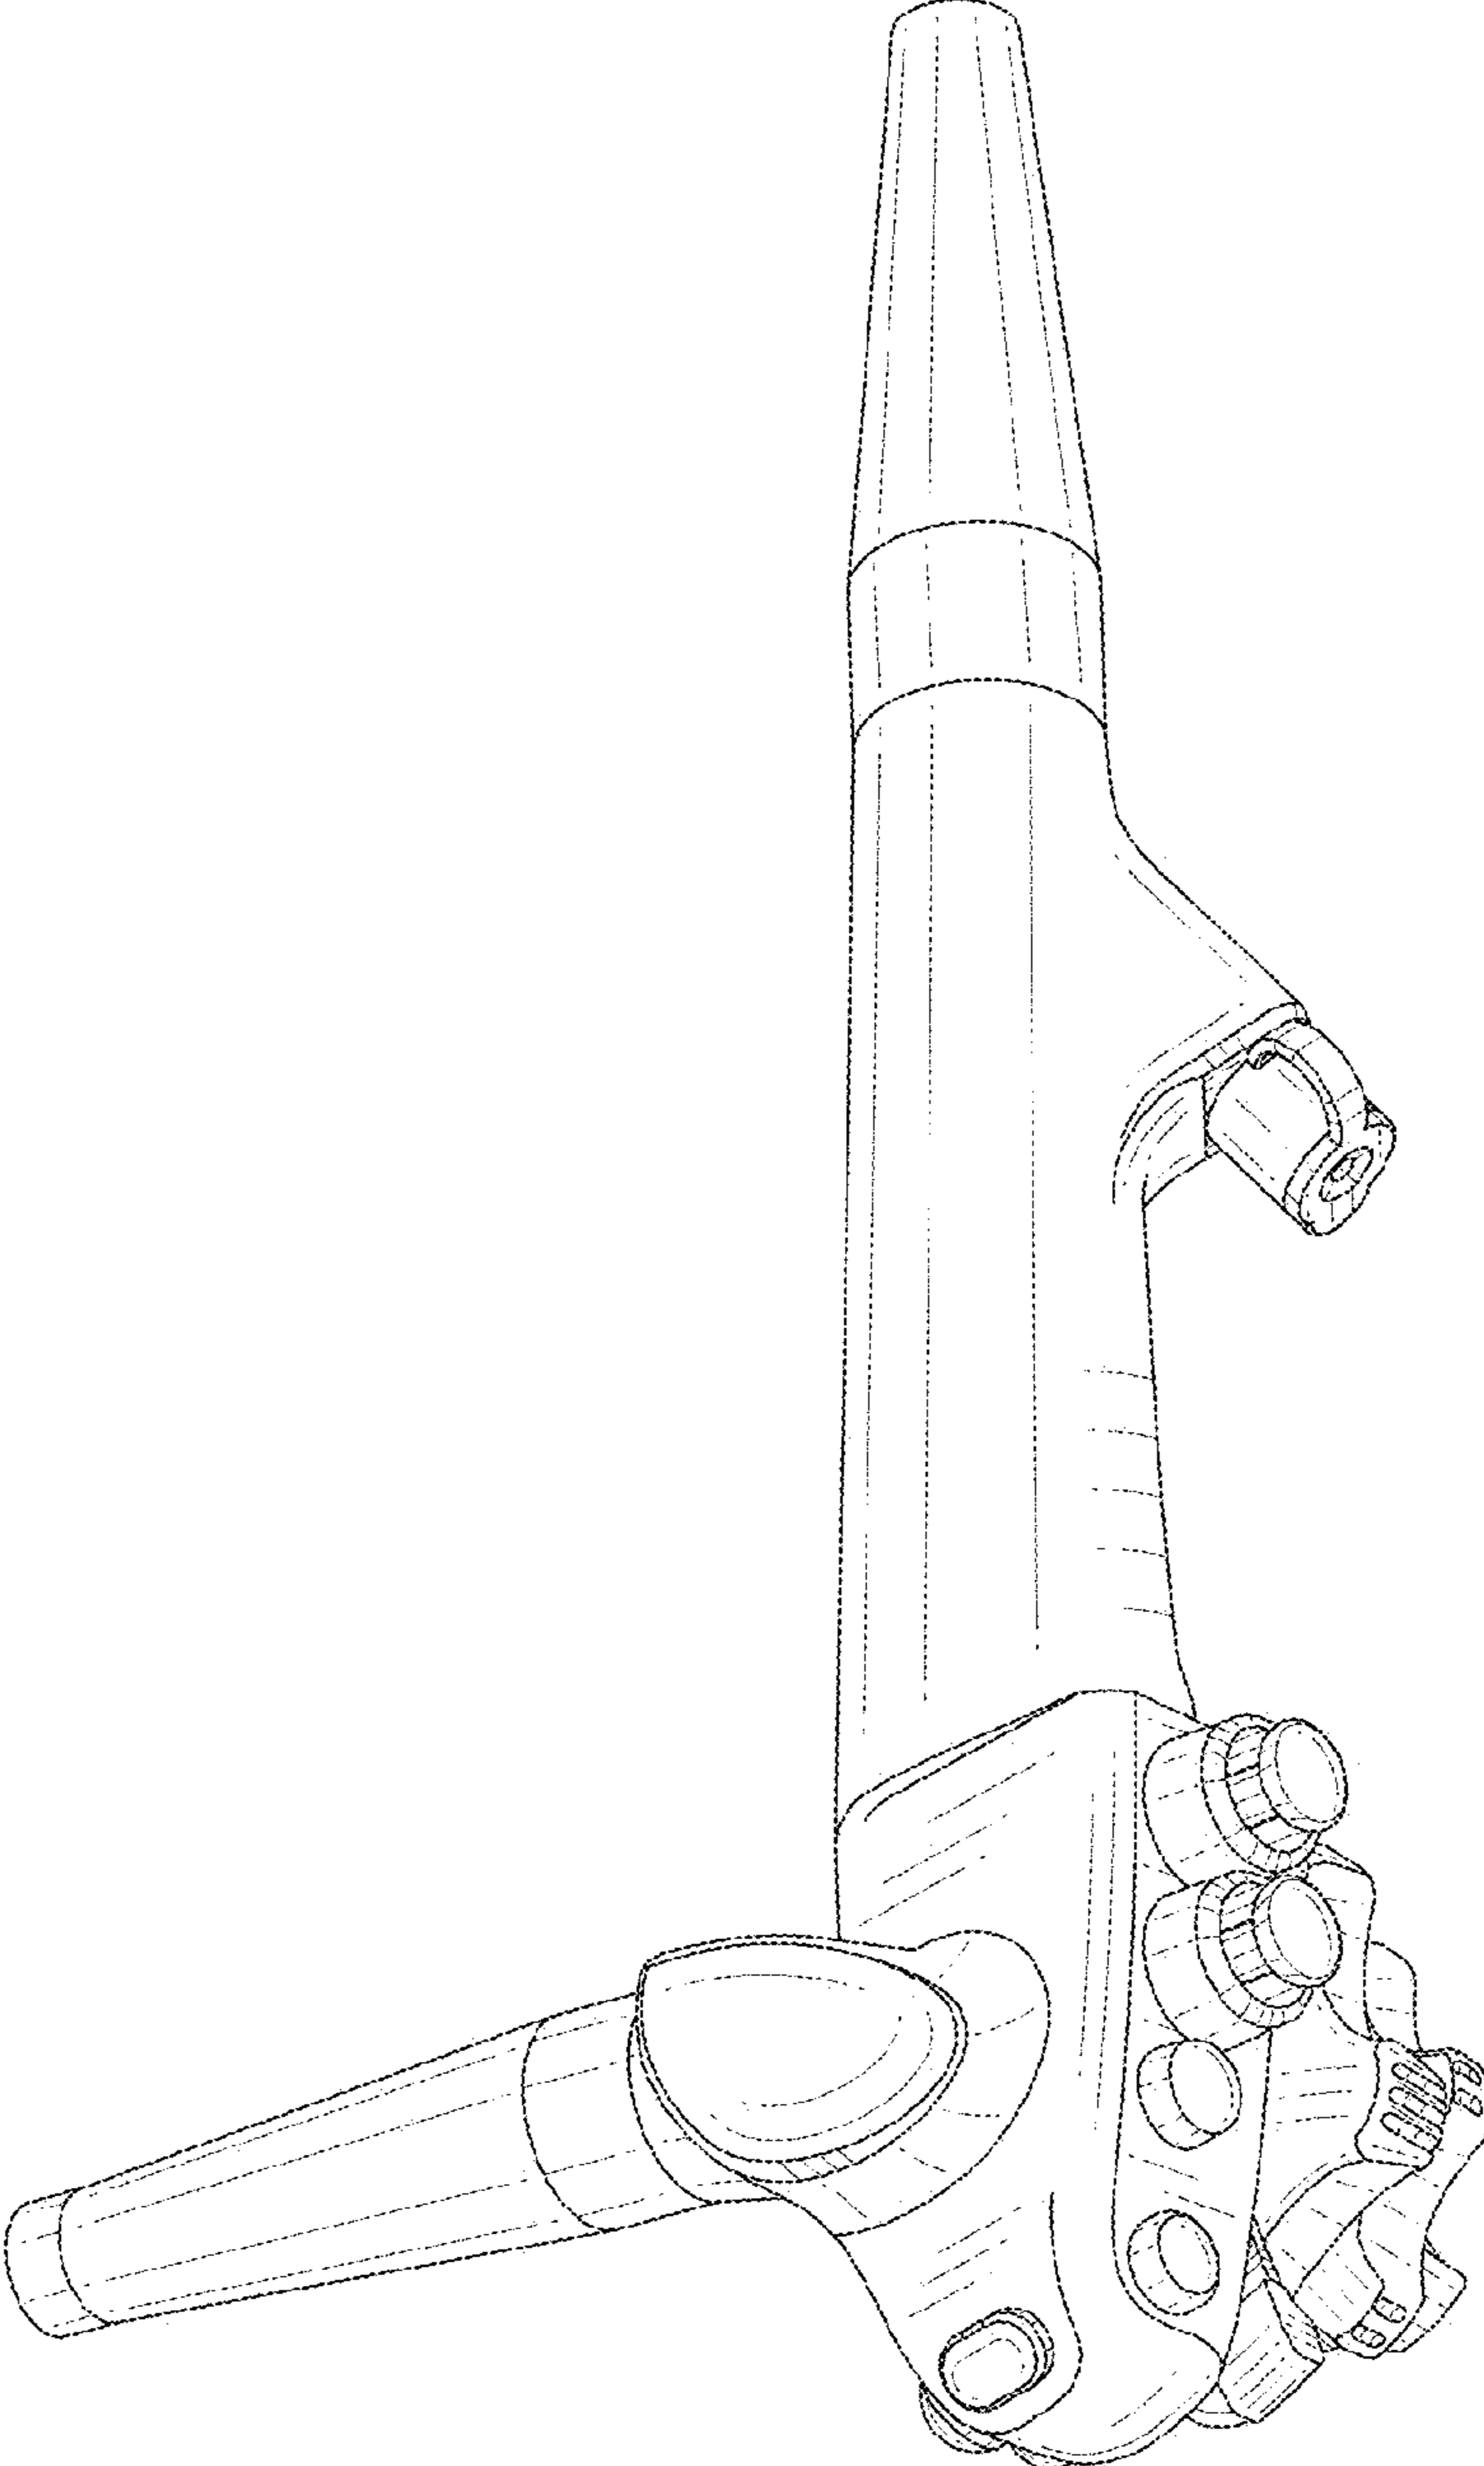


FIG.4

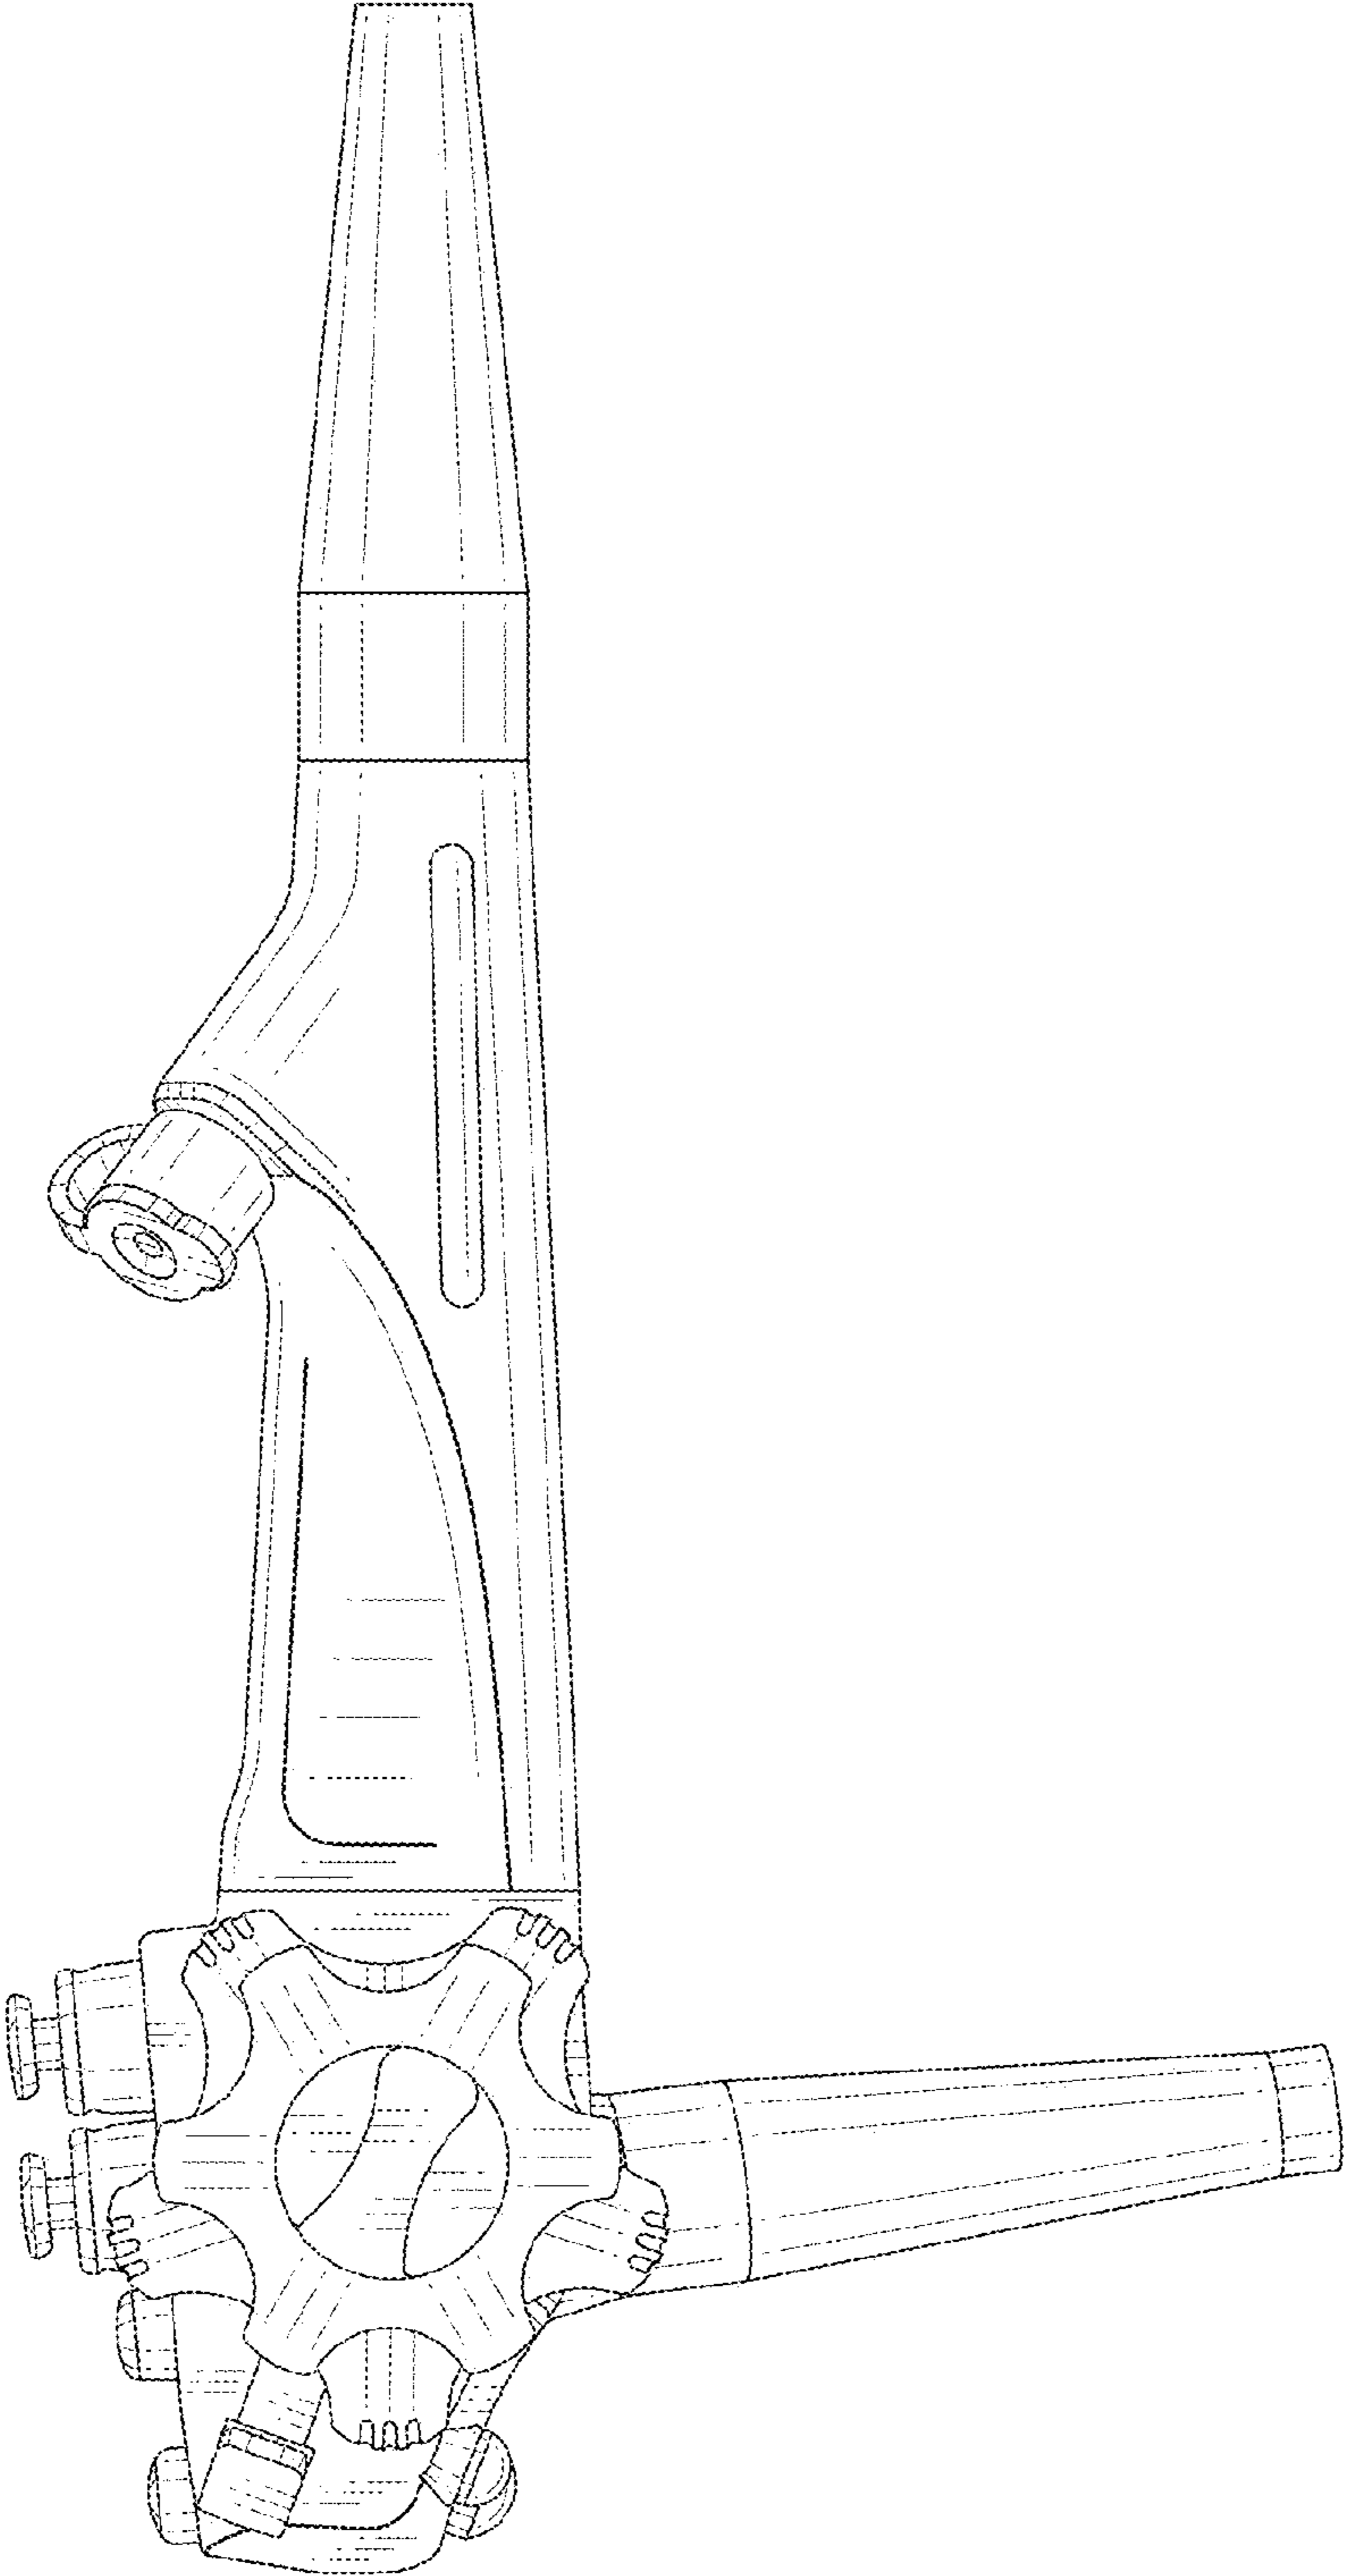


FIG. 5

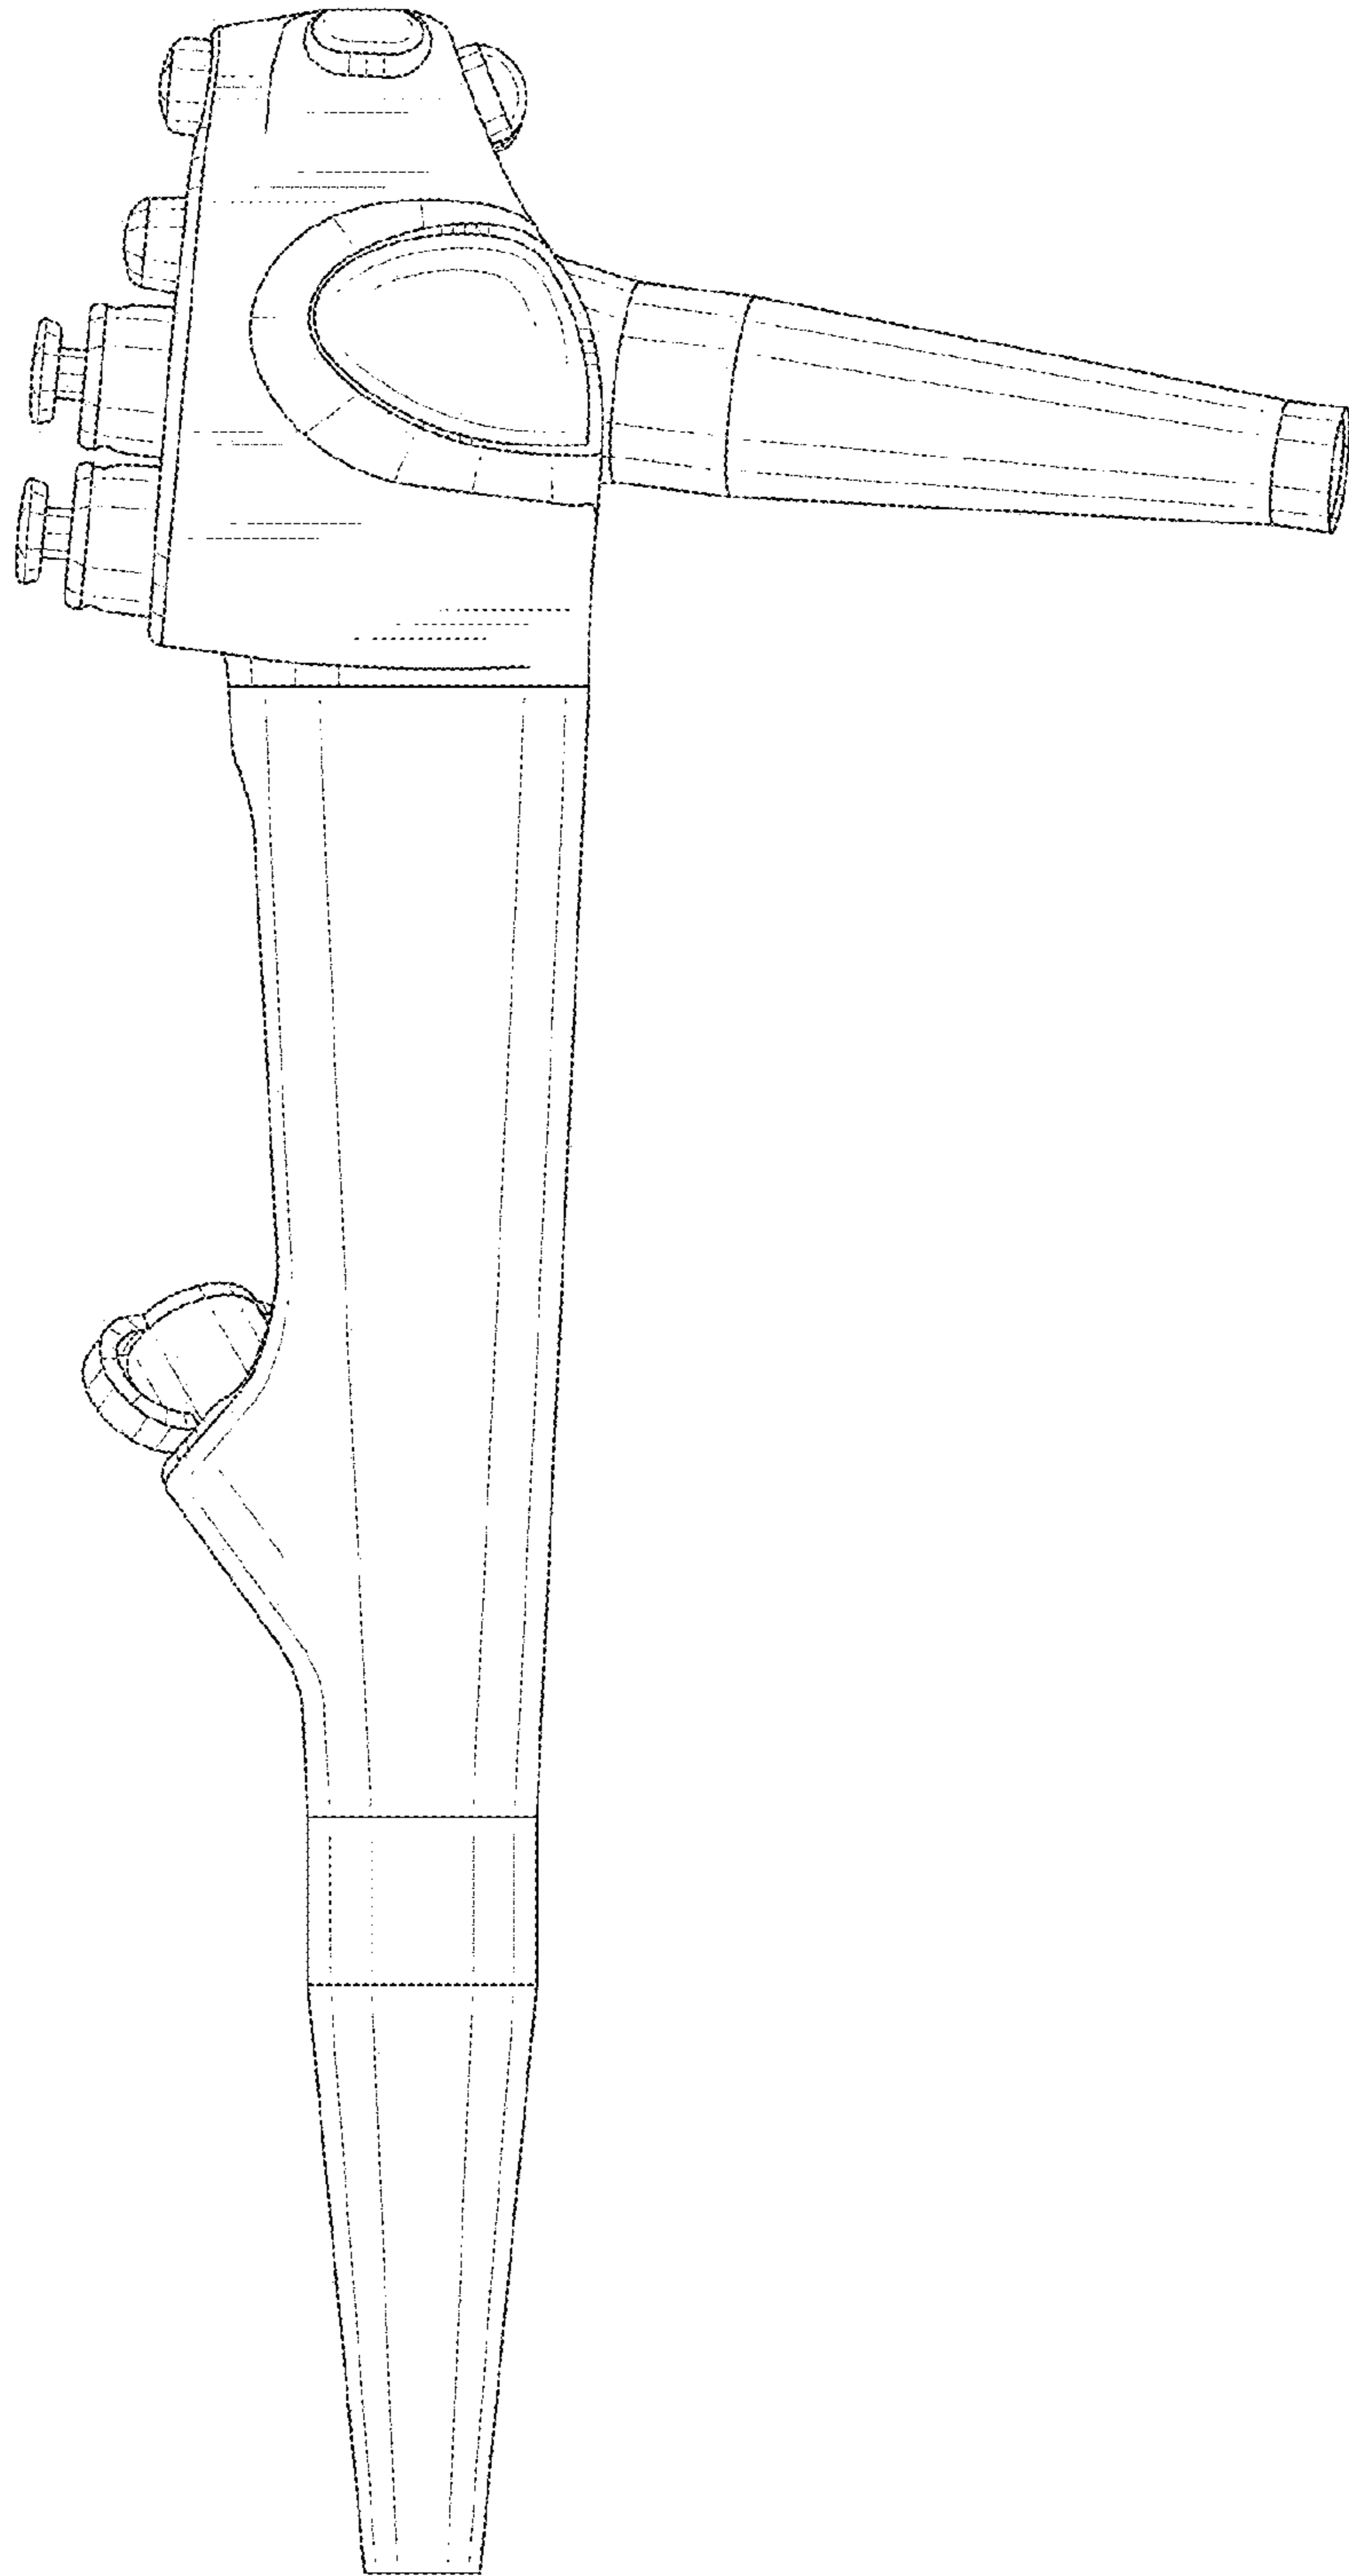


FIG.6

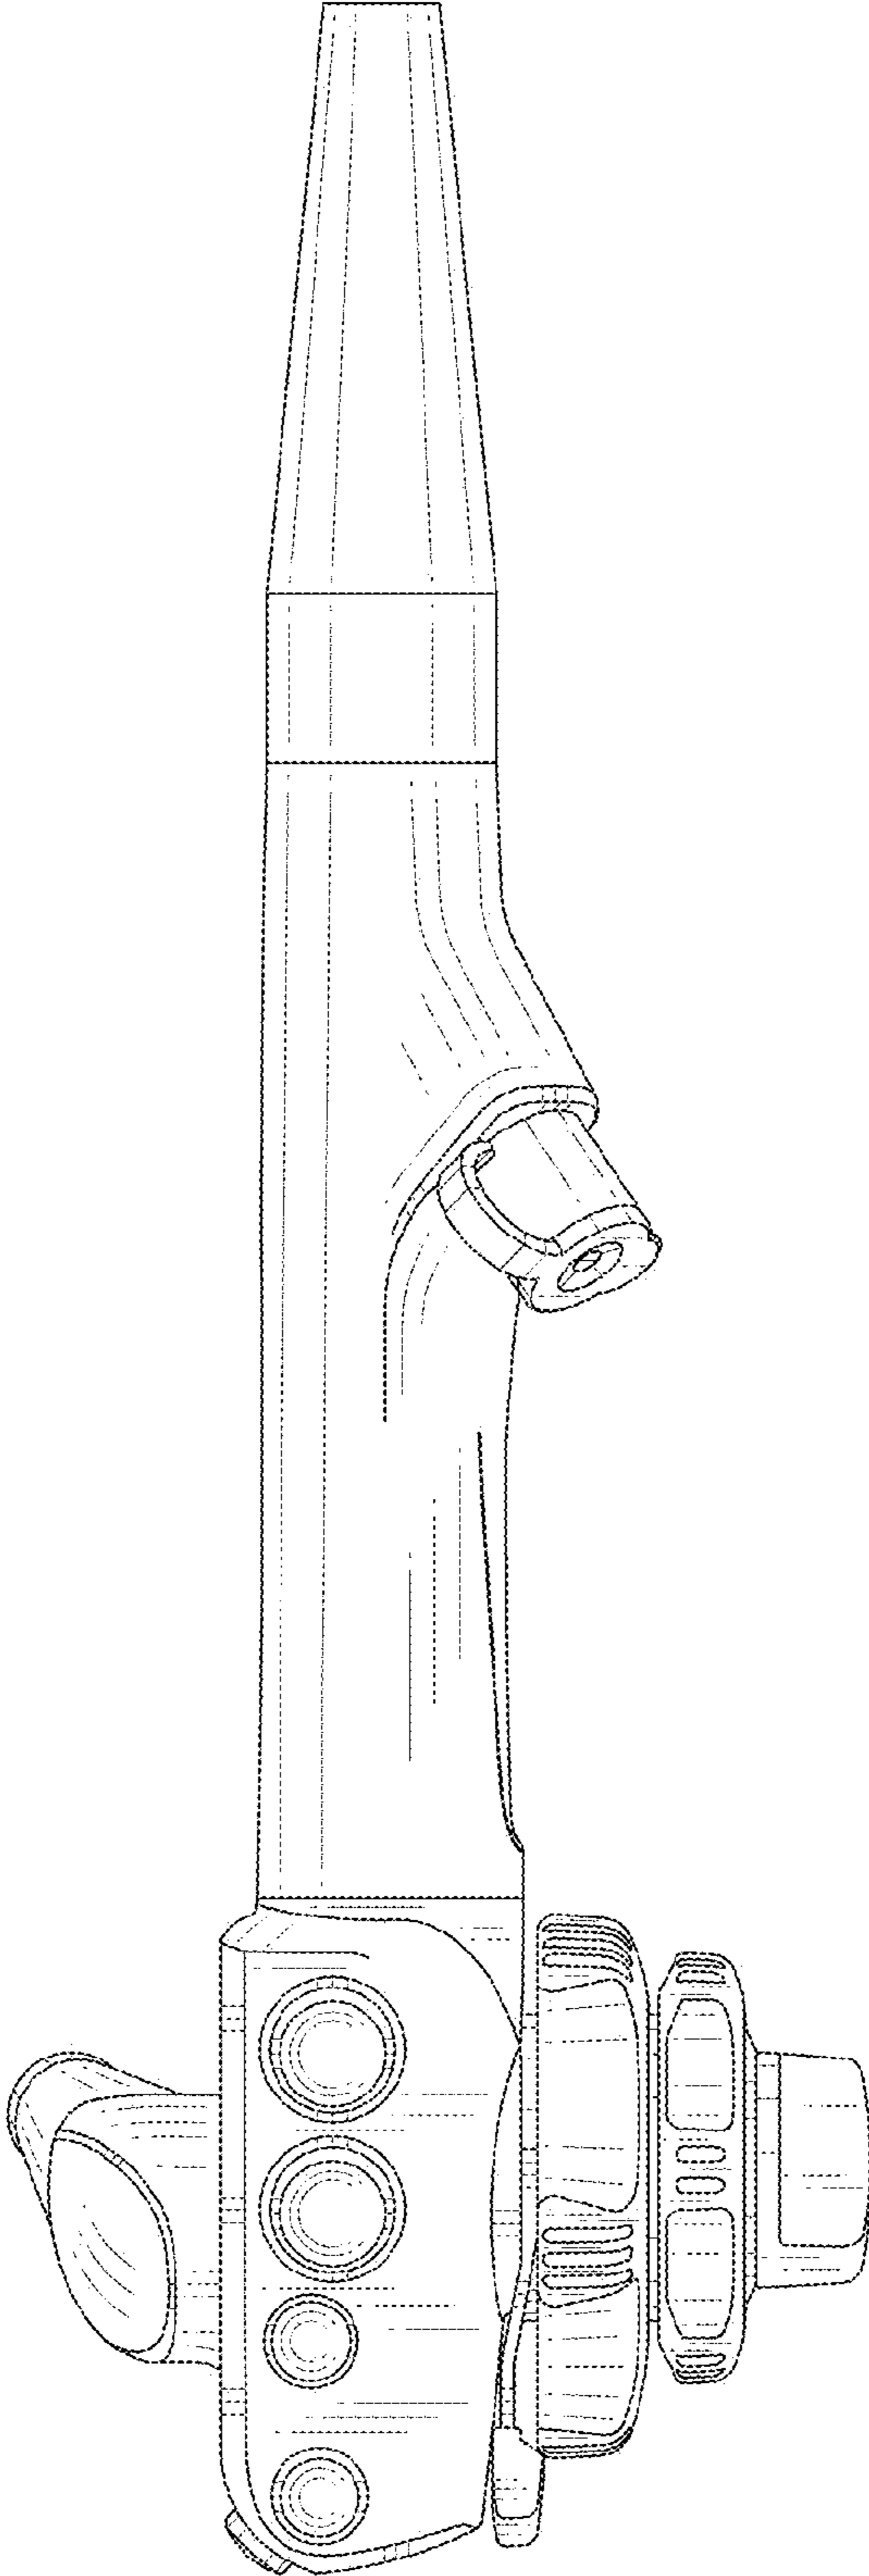


FIG. 7

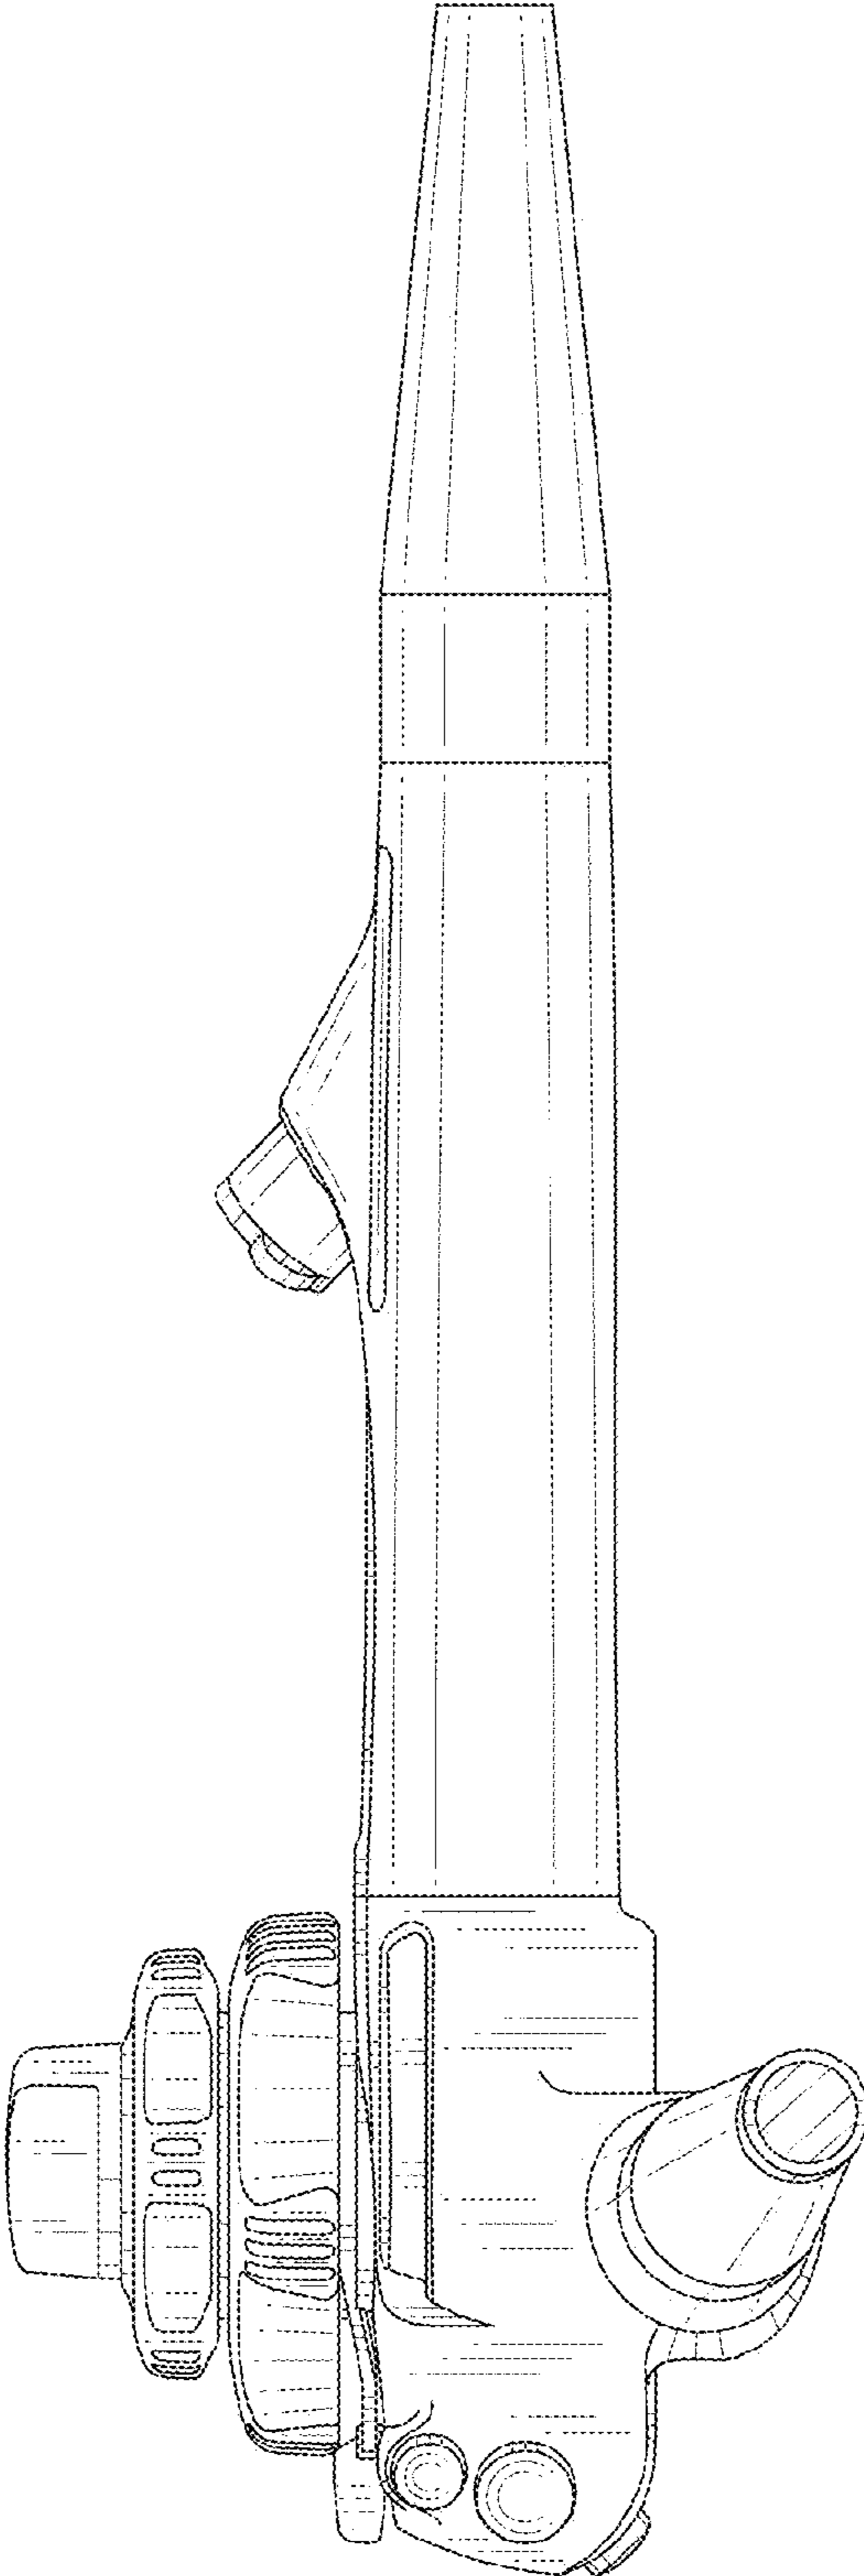


FIG. 8

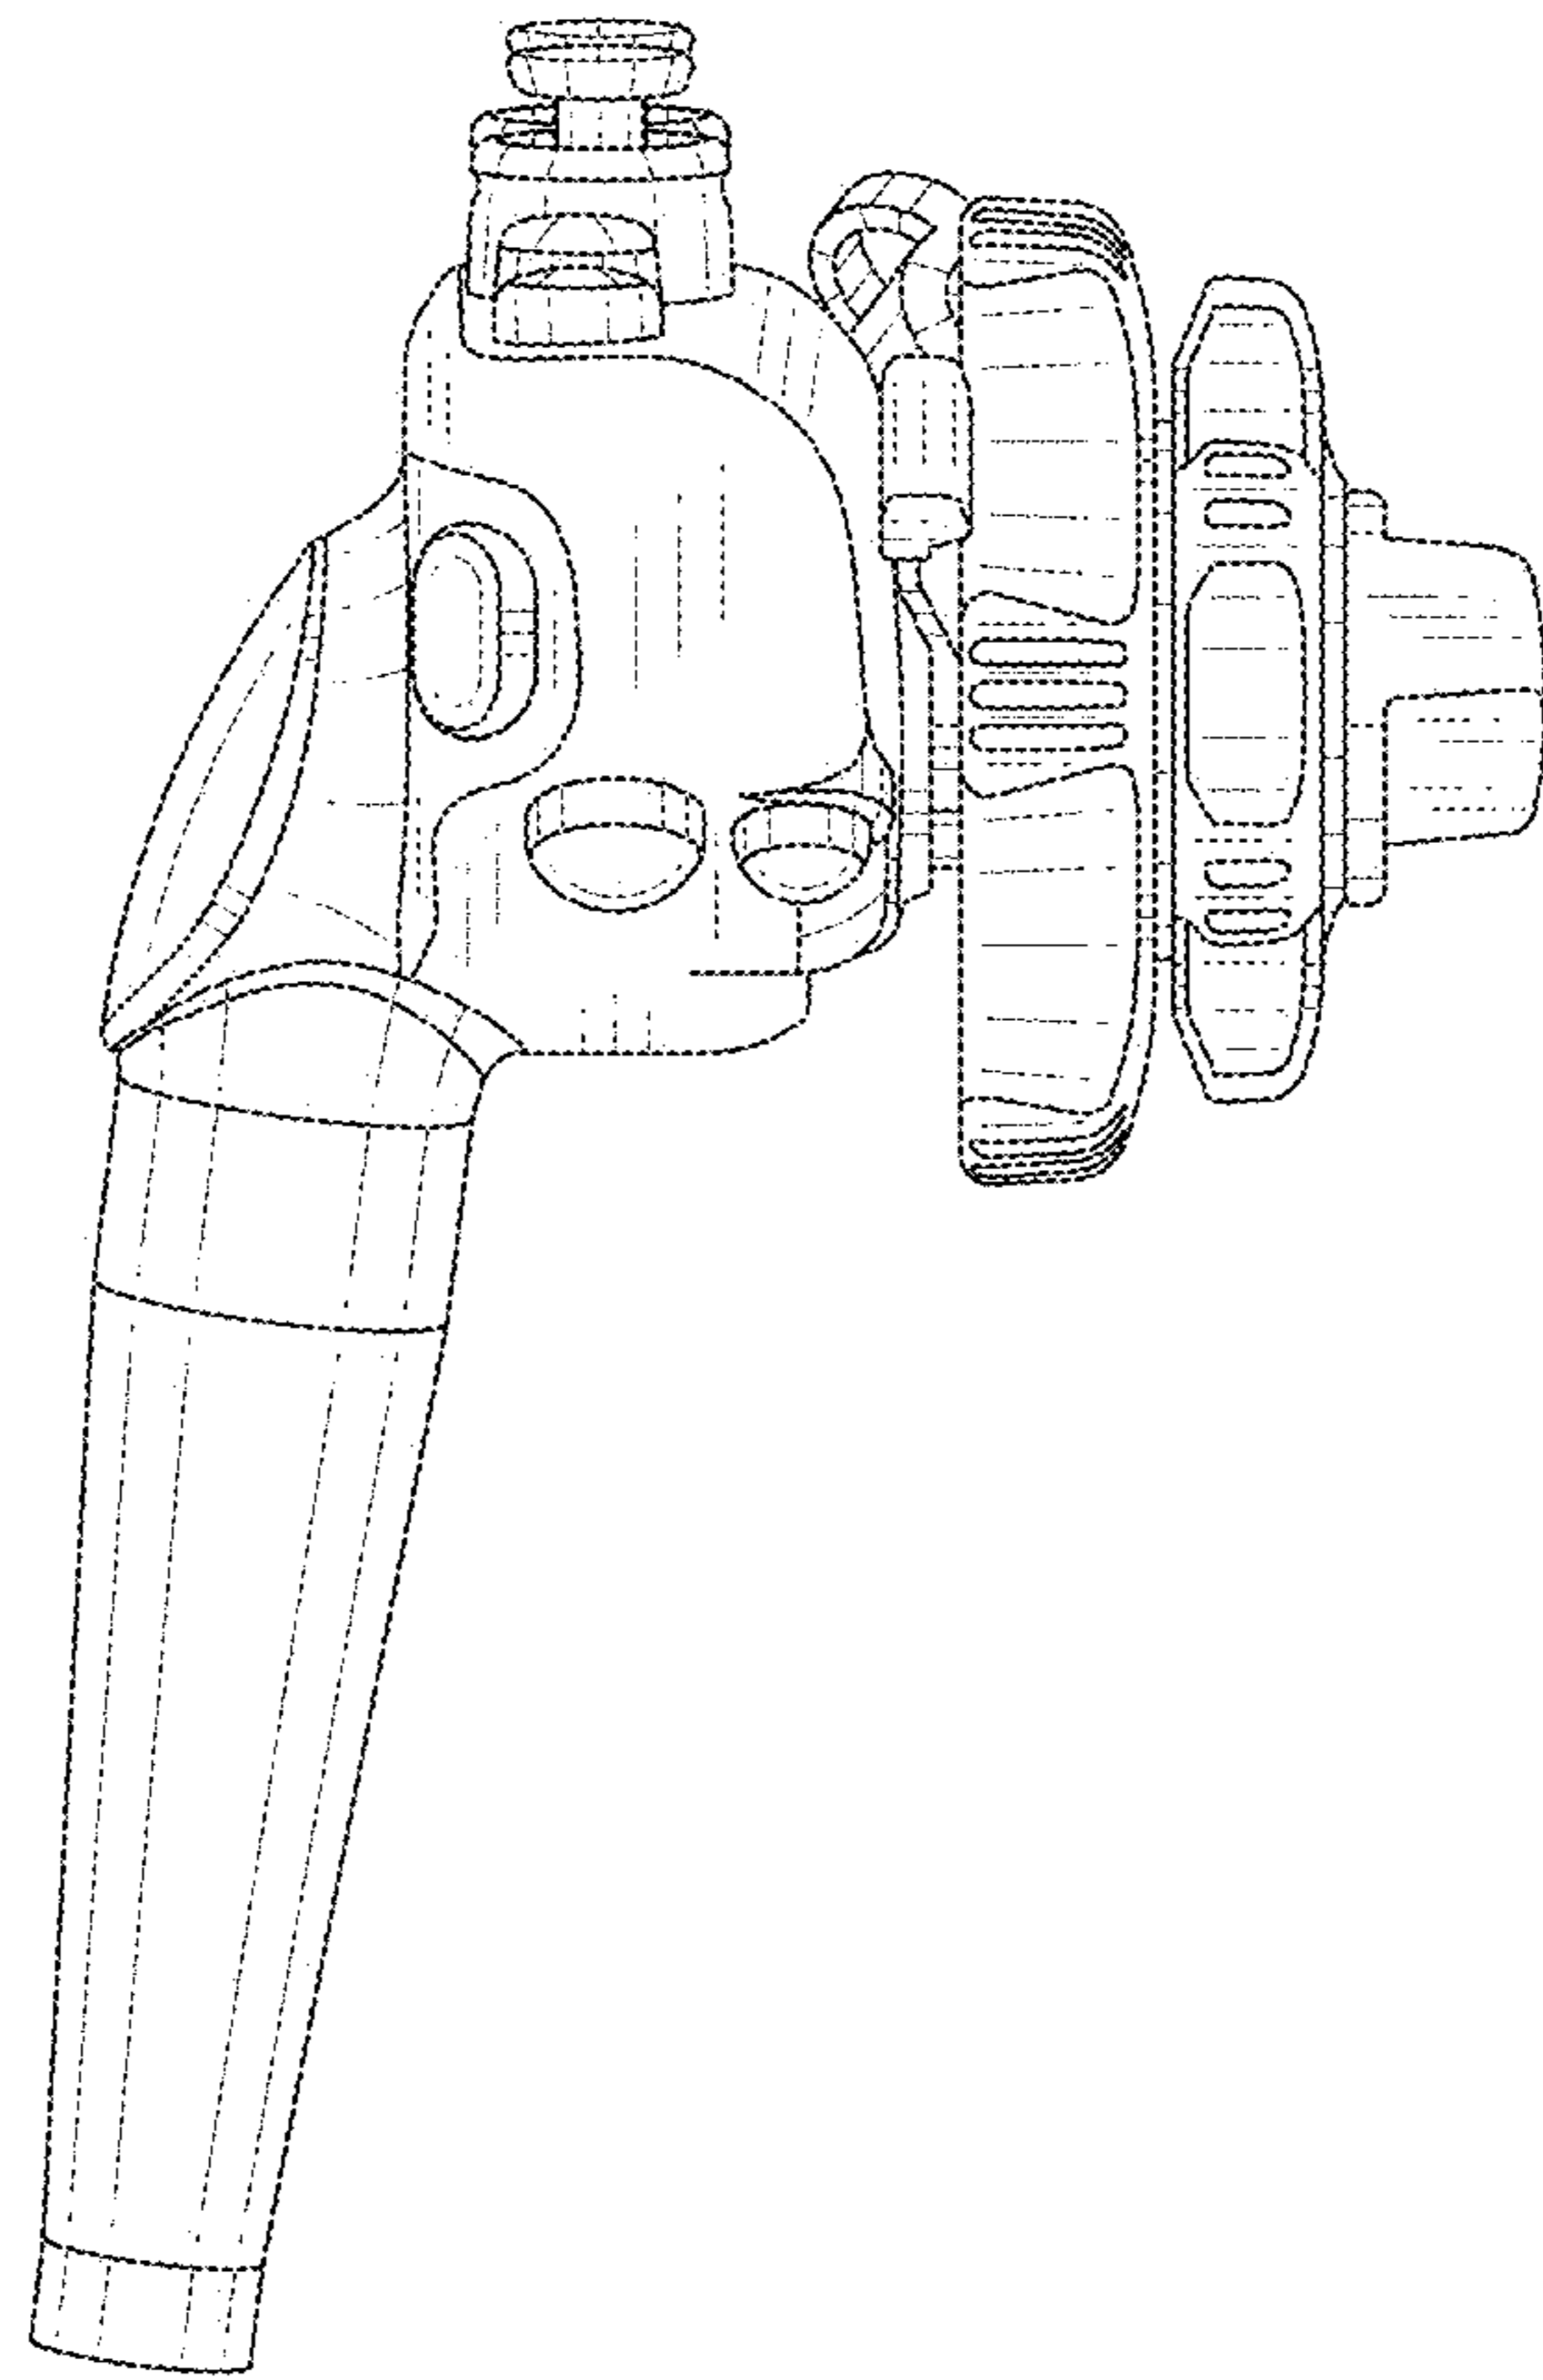


FIG. 9

