



US00D721437S

(12) **United States Design Patent**
Oka et al.

(10) **Patent No.:** **US D721,437 S**
(45) **Date of Patent:** **** Jan. 20, 2015**

(54) **BLOOD GLUCOSE TEST METER**
(71) Applicant: **ARKRAY, Inc.**, Kyoto-Shi (JP)
(72) Inventors: **Junichi Oka**, Kyoto (JP); **Kazuyoshi Kamekawa**, Kyoto (JP)
(73) Assignee: **ARKRAY, Inc.**, Kyoto-shi (JP)
(**) Term: **14 Years**

(21) Appl. No.: **29/476,628**

(22) Filed: **Dec. 16, 2013**

(30) **Foreign Application Priority Data**

Jul. 12, 2013 (JP) 2013-15969

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/169**

(58) **Field of Classification Search**
USPC D24/216, 223, 231, 232, 107, 169, 186;
D10/81; 422/68.1, 420, 500;
435/287.1, 287.3; 436/43, 45, 47;
600/309, 365, 368, 583, 584

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D546,457 S *	7/2007	Hannant et al.	D24/186
D600,349 S *	9/2009	Bell et al.	D24/169
D630,113 S *	1/2011	Orr et al.	D10/81
D633,814 S *	3/2011	Nishiyama	D24/186
D679,400 S *	4/2013	Hiramura	D24/169
D686,731 S *	7/2013	Oka	D24/169
D690,422 S *	9/2013	Oka	D24/169

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Fox Rothschild LLP

(57) **CLAIM**

The ornamental design for a blood glucose test meter, as shown and described.

DESCRIPTION

FIG. 1 is a front elevational view of the test meter.
FIG. 2 is a rear elevational view of the test meter.
FIG. 3 is a left elevational view of the test meter.
FIG. 4 is a right elevational view of the test meter.
FIG. 5 is a top plan view of the test meter.
FIG. 6 is a bottom plan view of the test meter.
FIG. 7 is a front perspective view 1 of the test meter.
FIG. 8 is a front perspective view 2 of the test meter; and,
FIG. 9 is a rear perspective view of the test meter.

1 Claim, 5 Drawing Sheets



Fig. 1

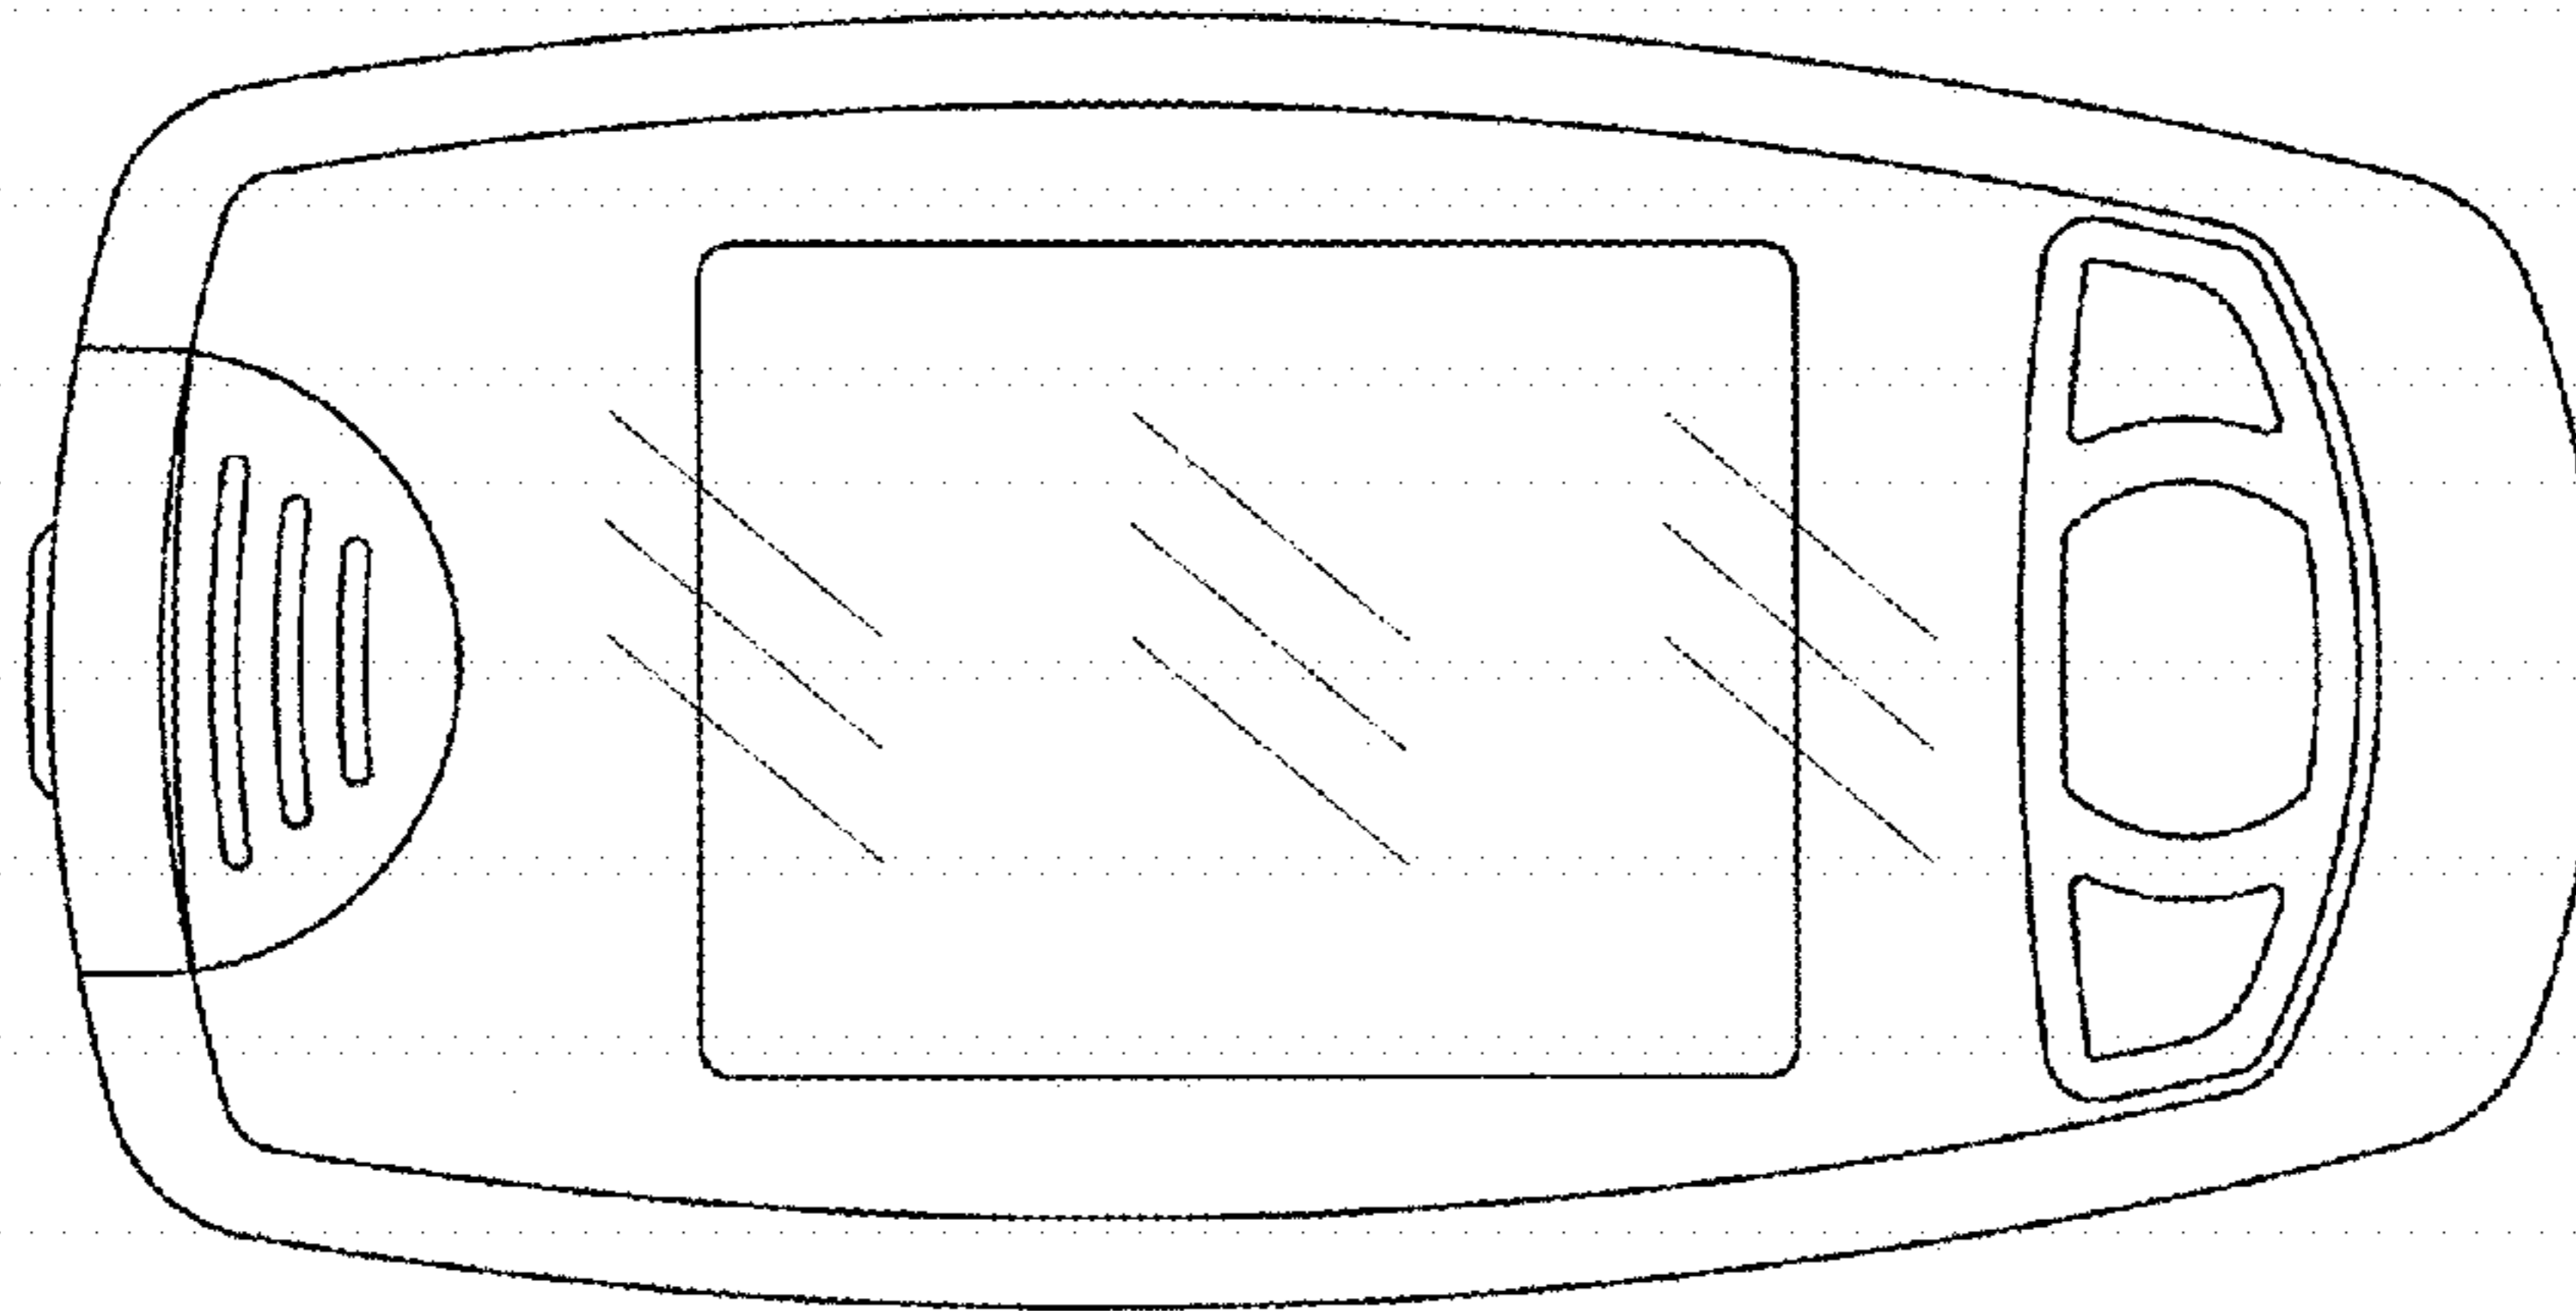


Fig. 2

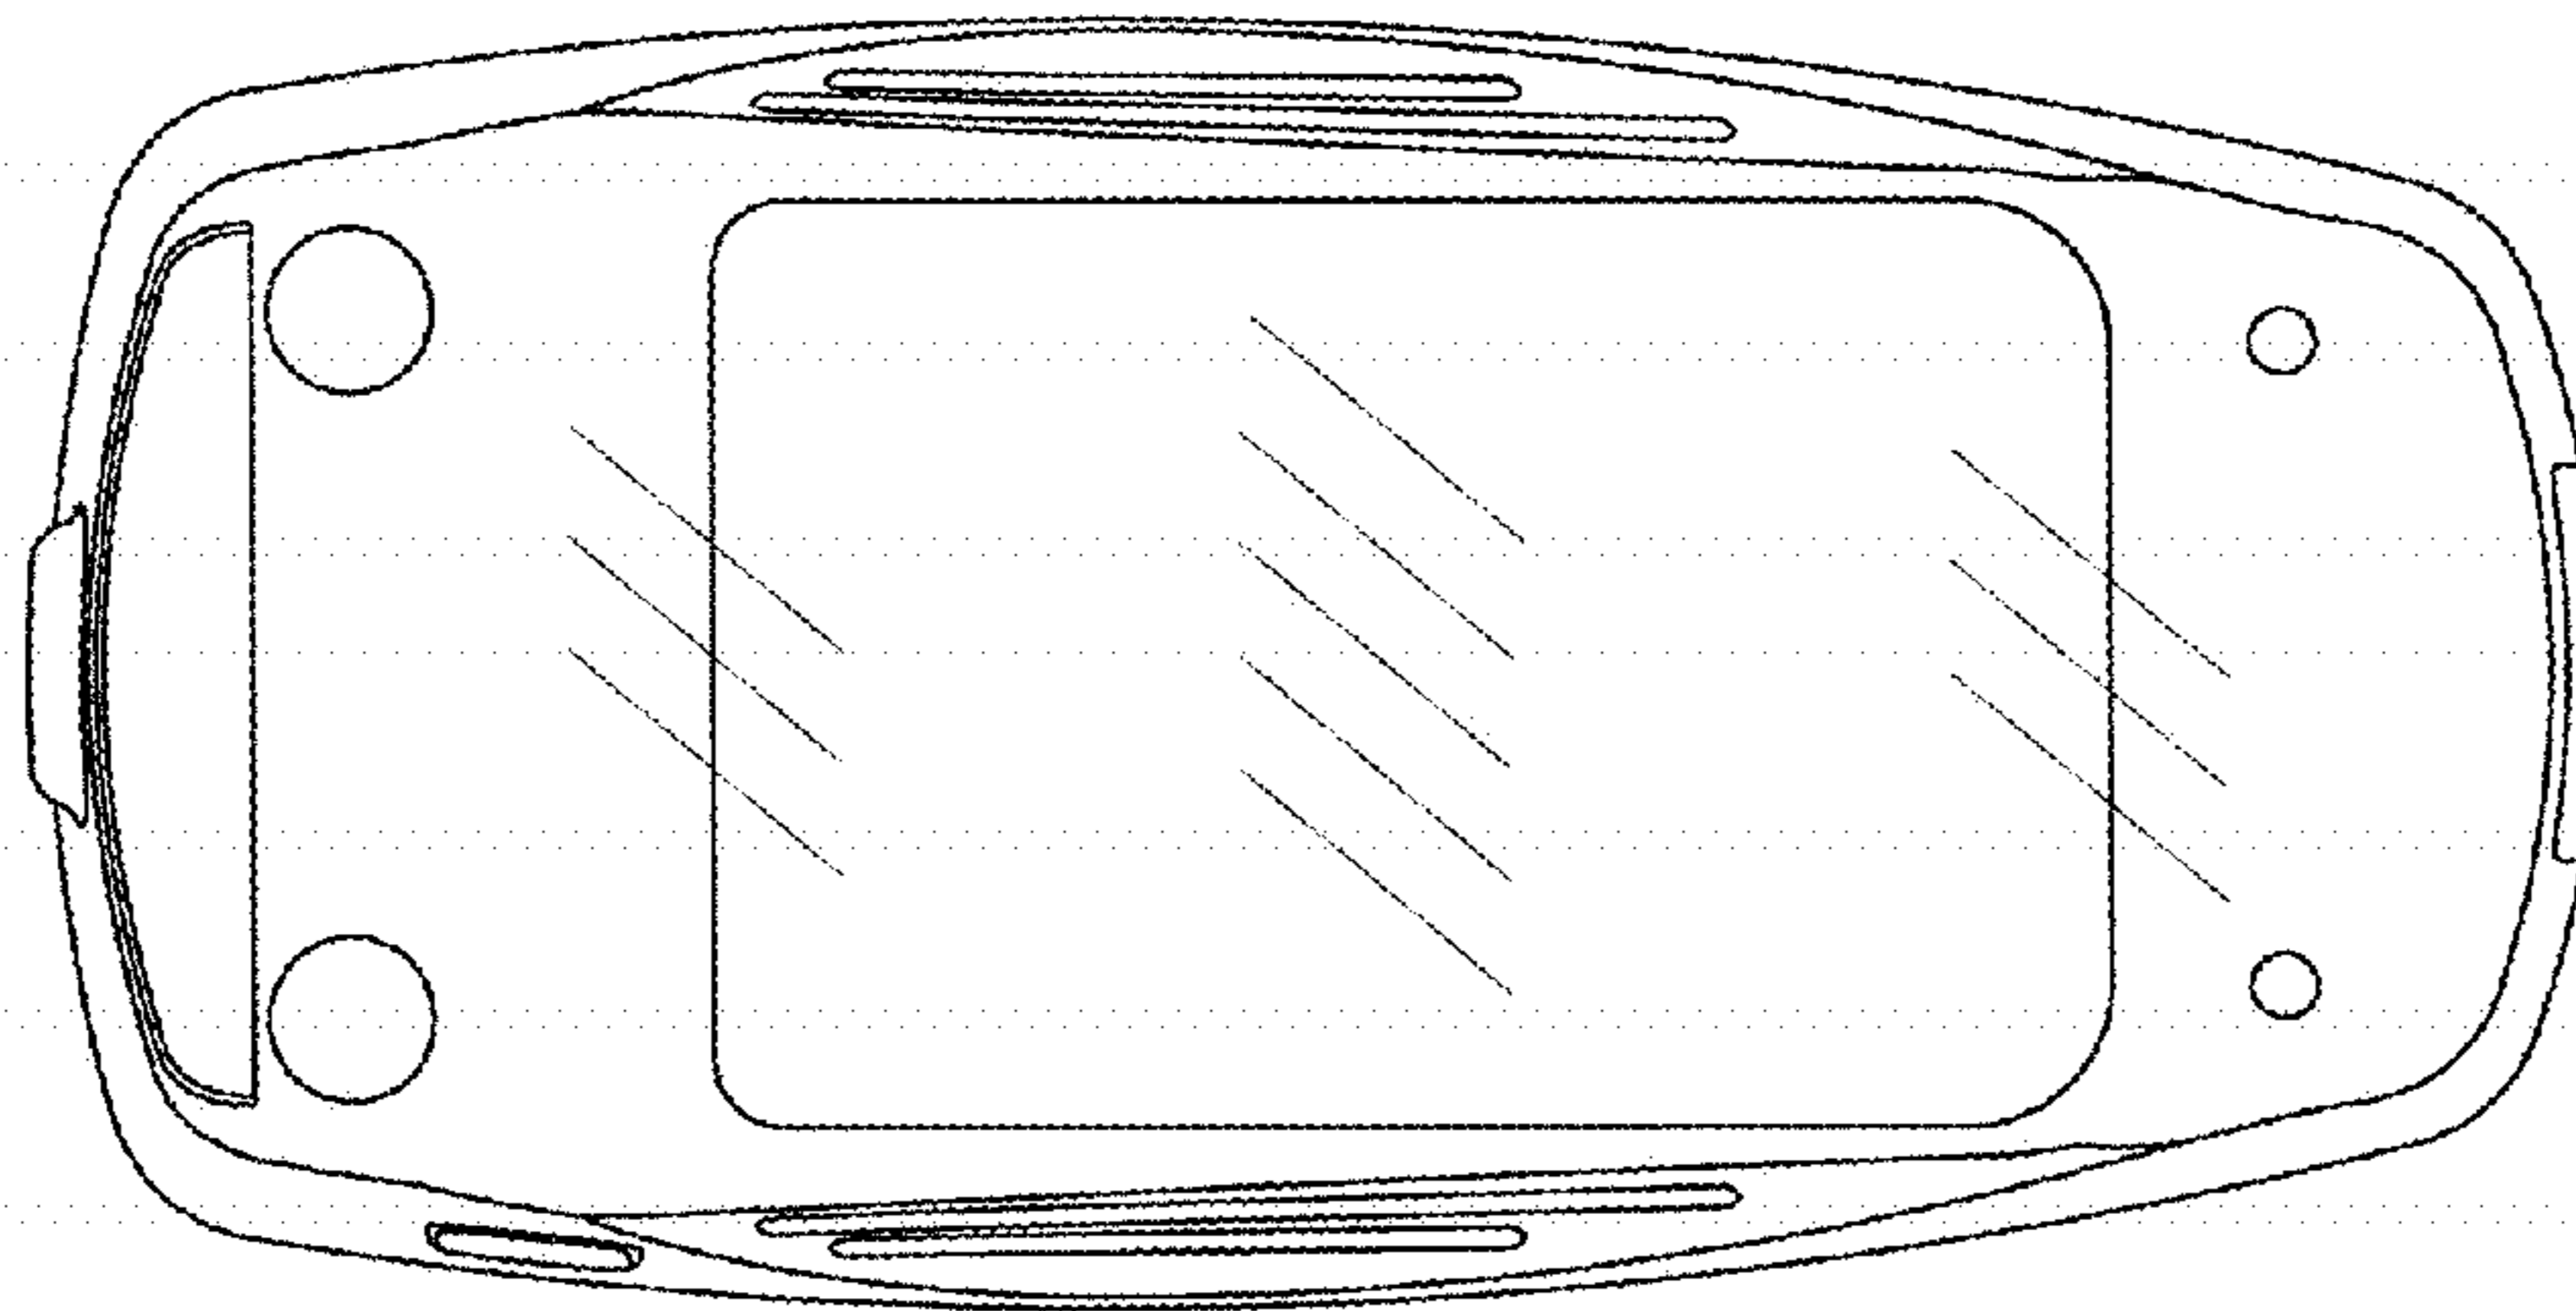


Fig. 3

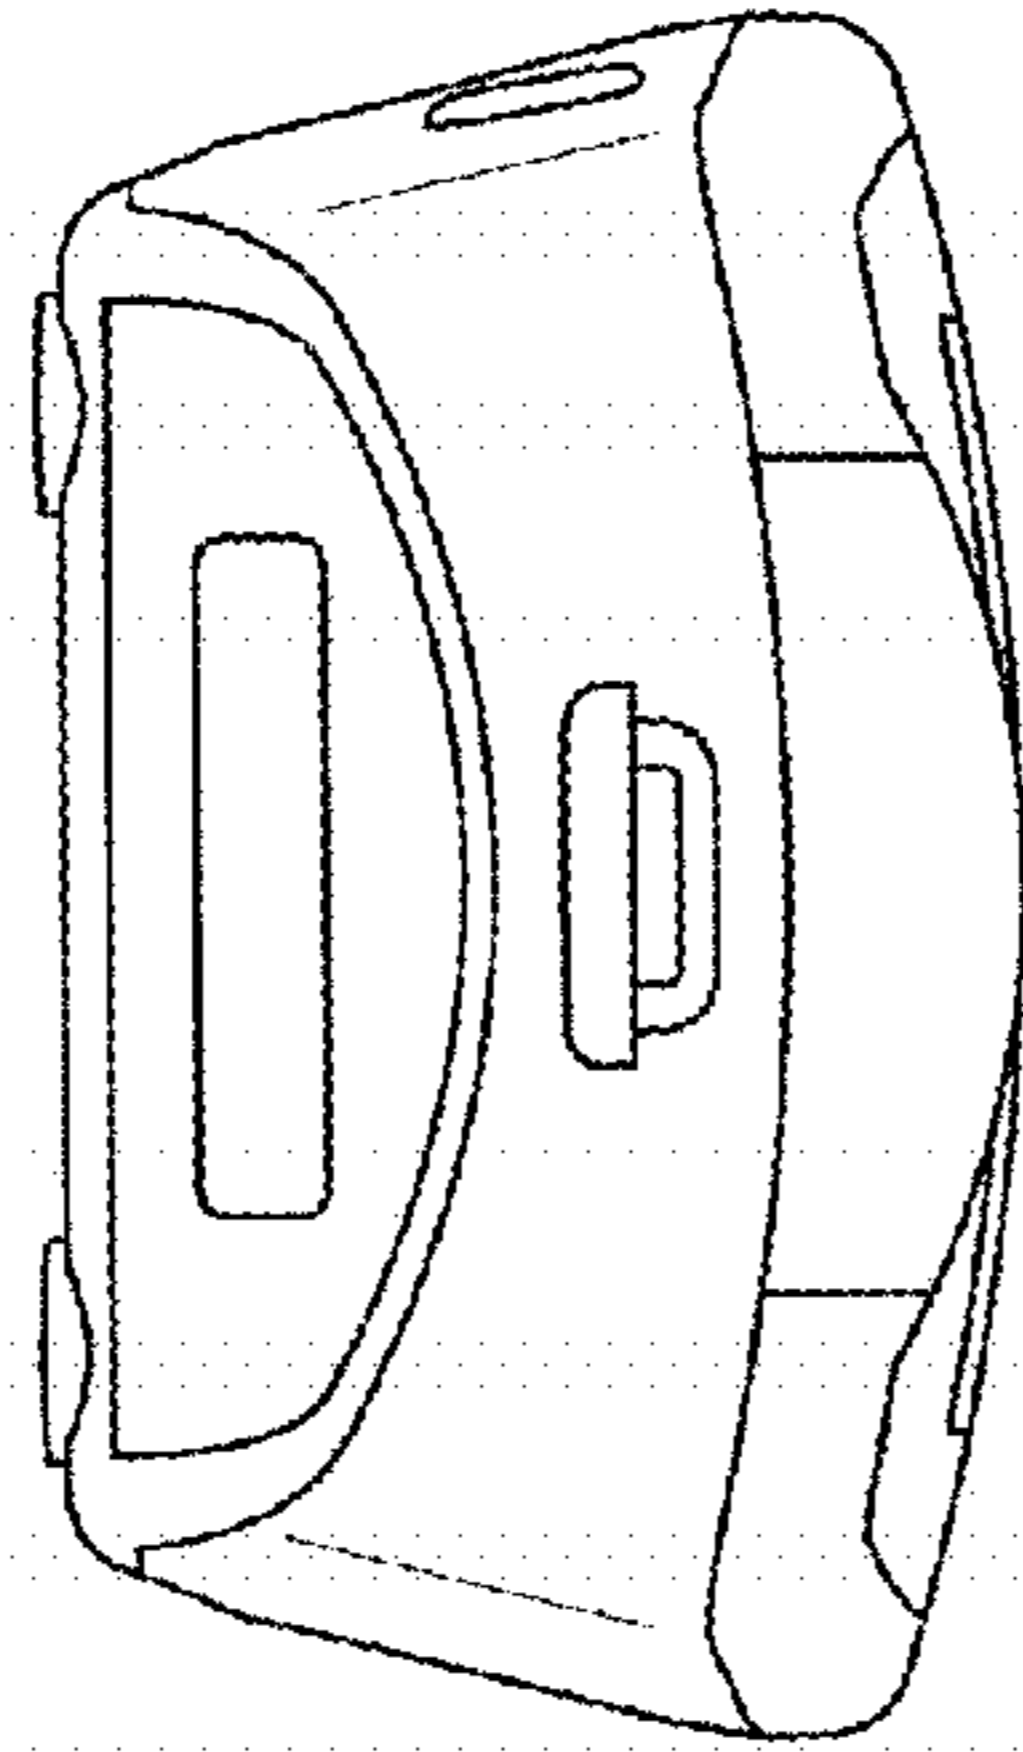


Fig. 4

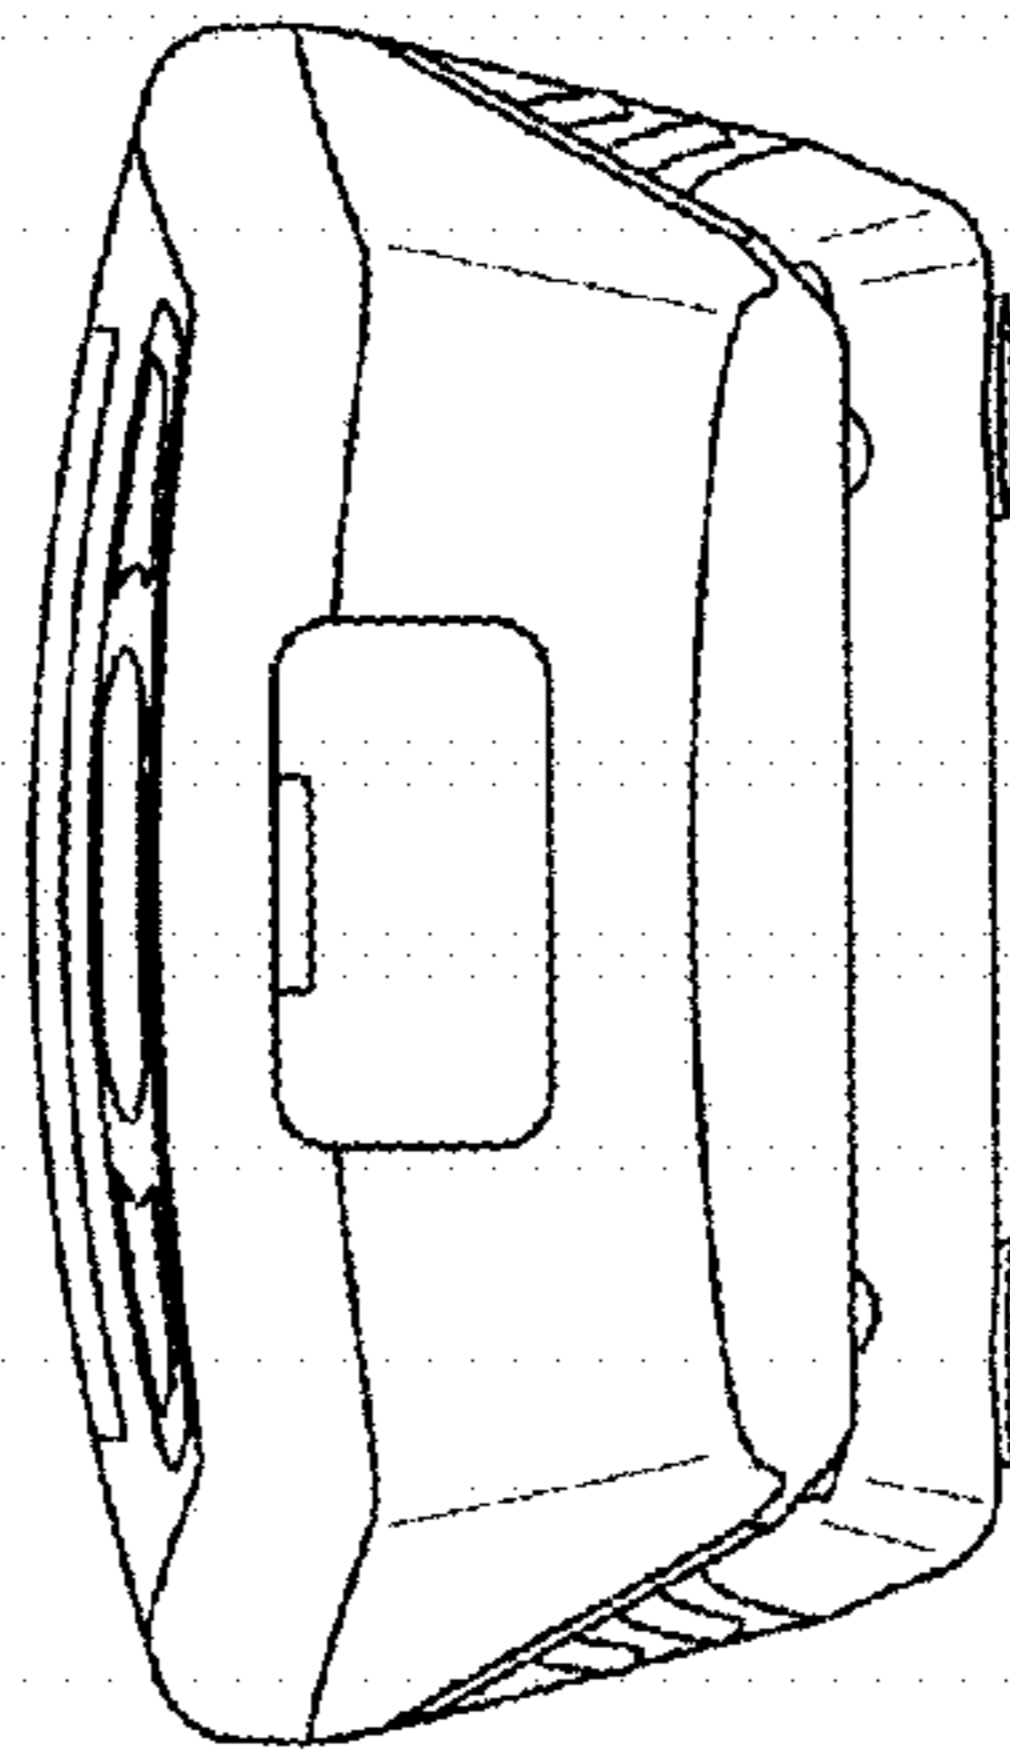


Fig. 5

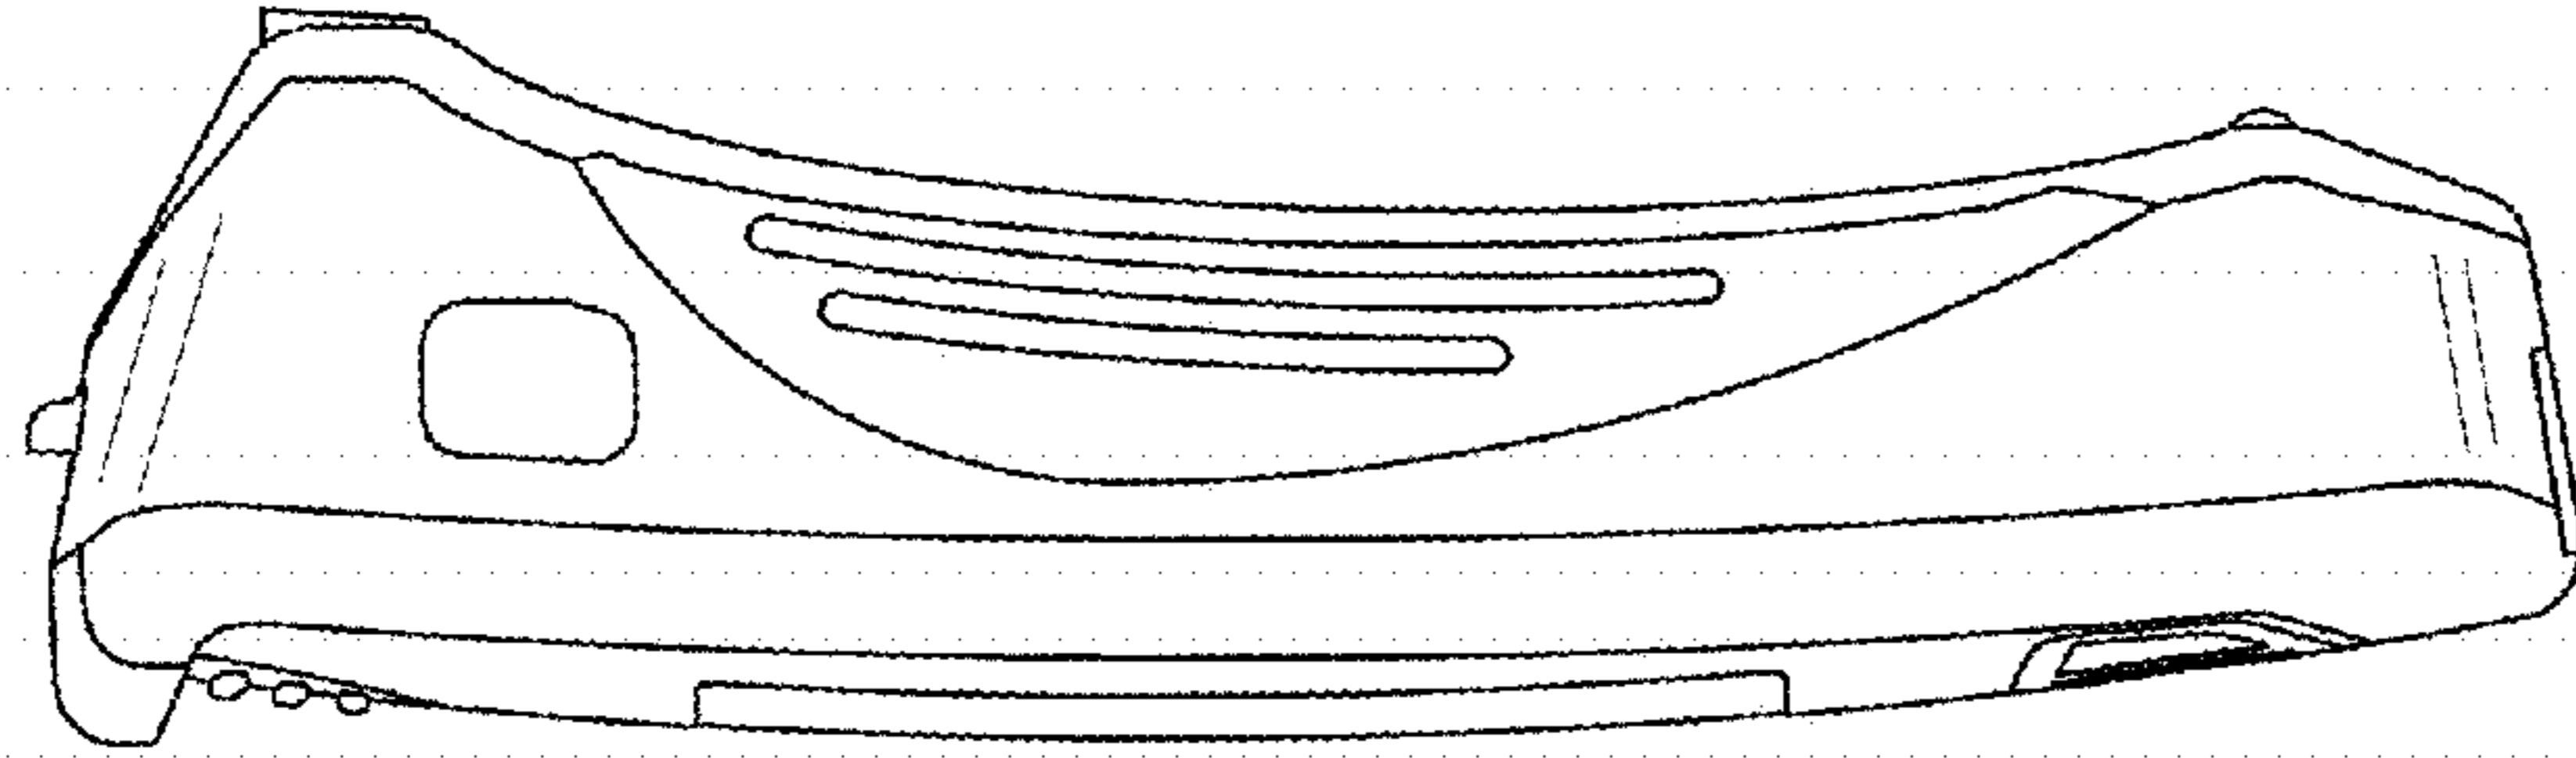


Fig. 6

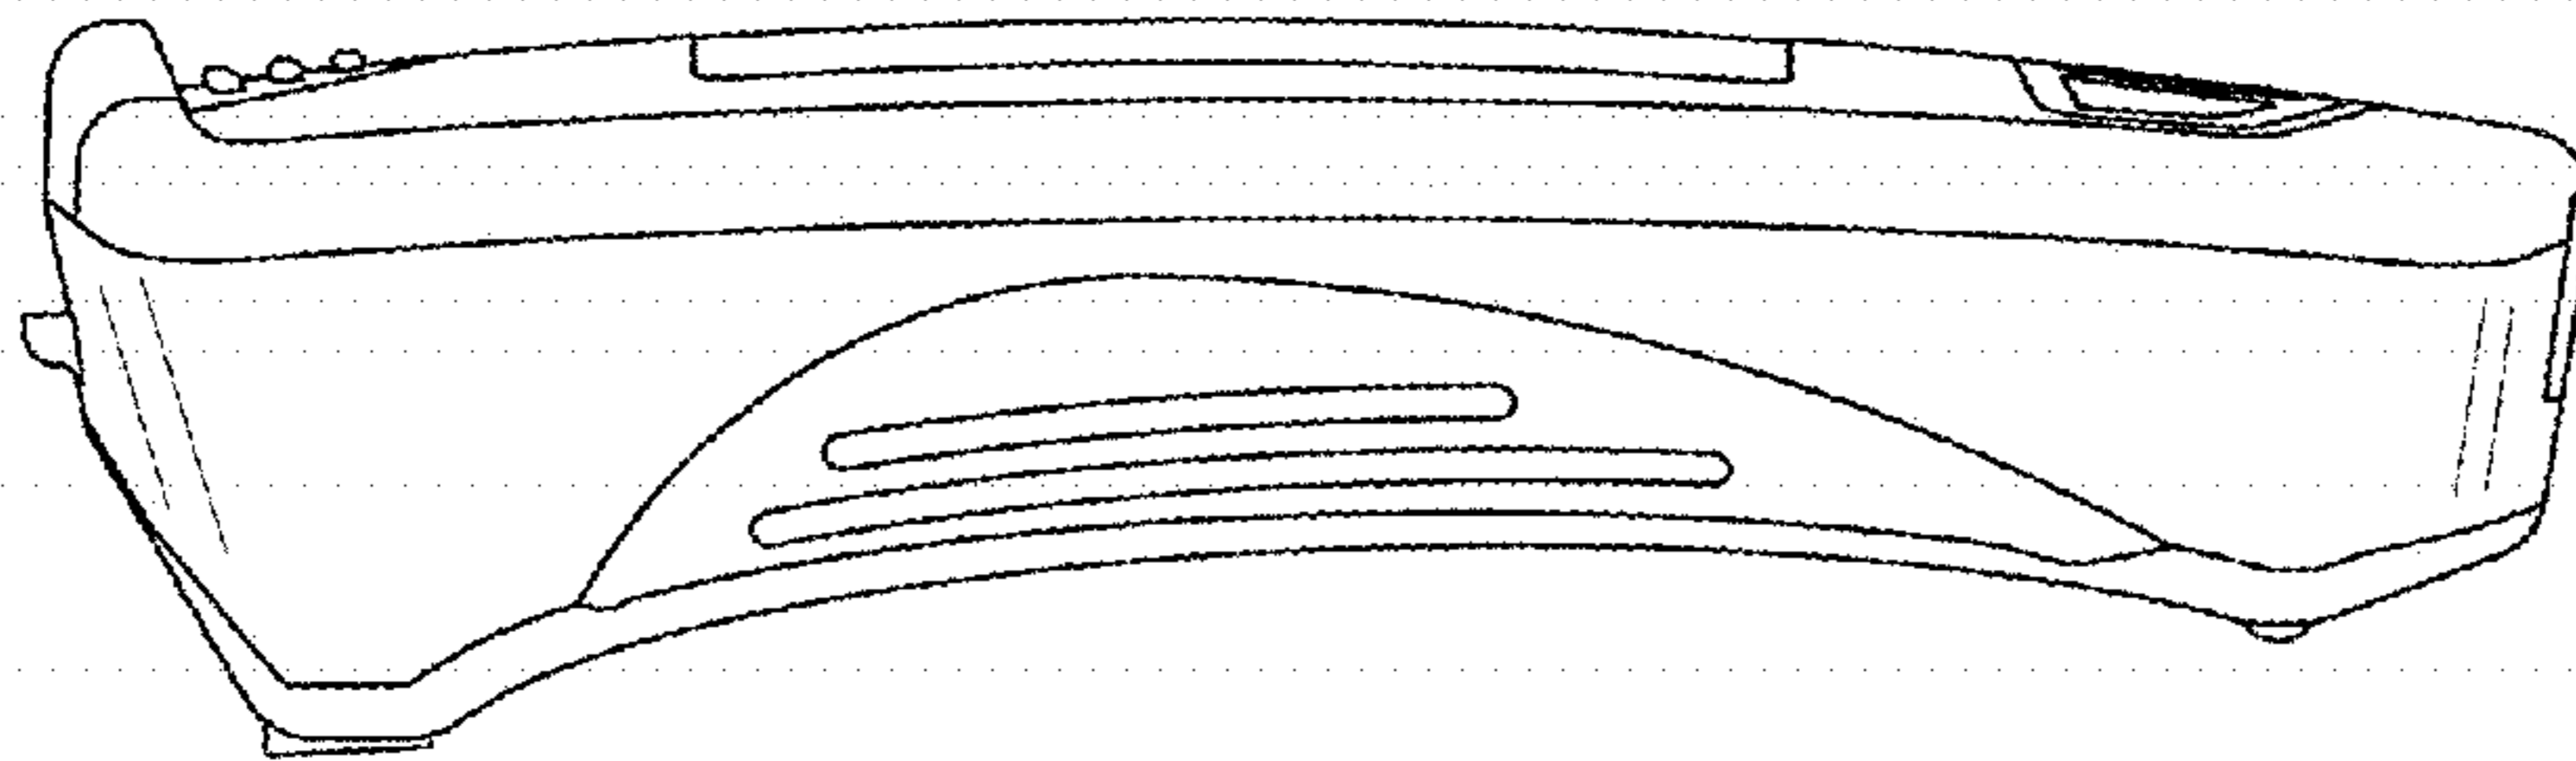


Fig. 7



Fig. 8

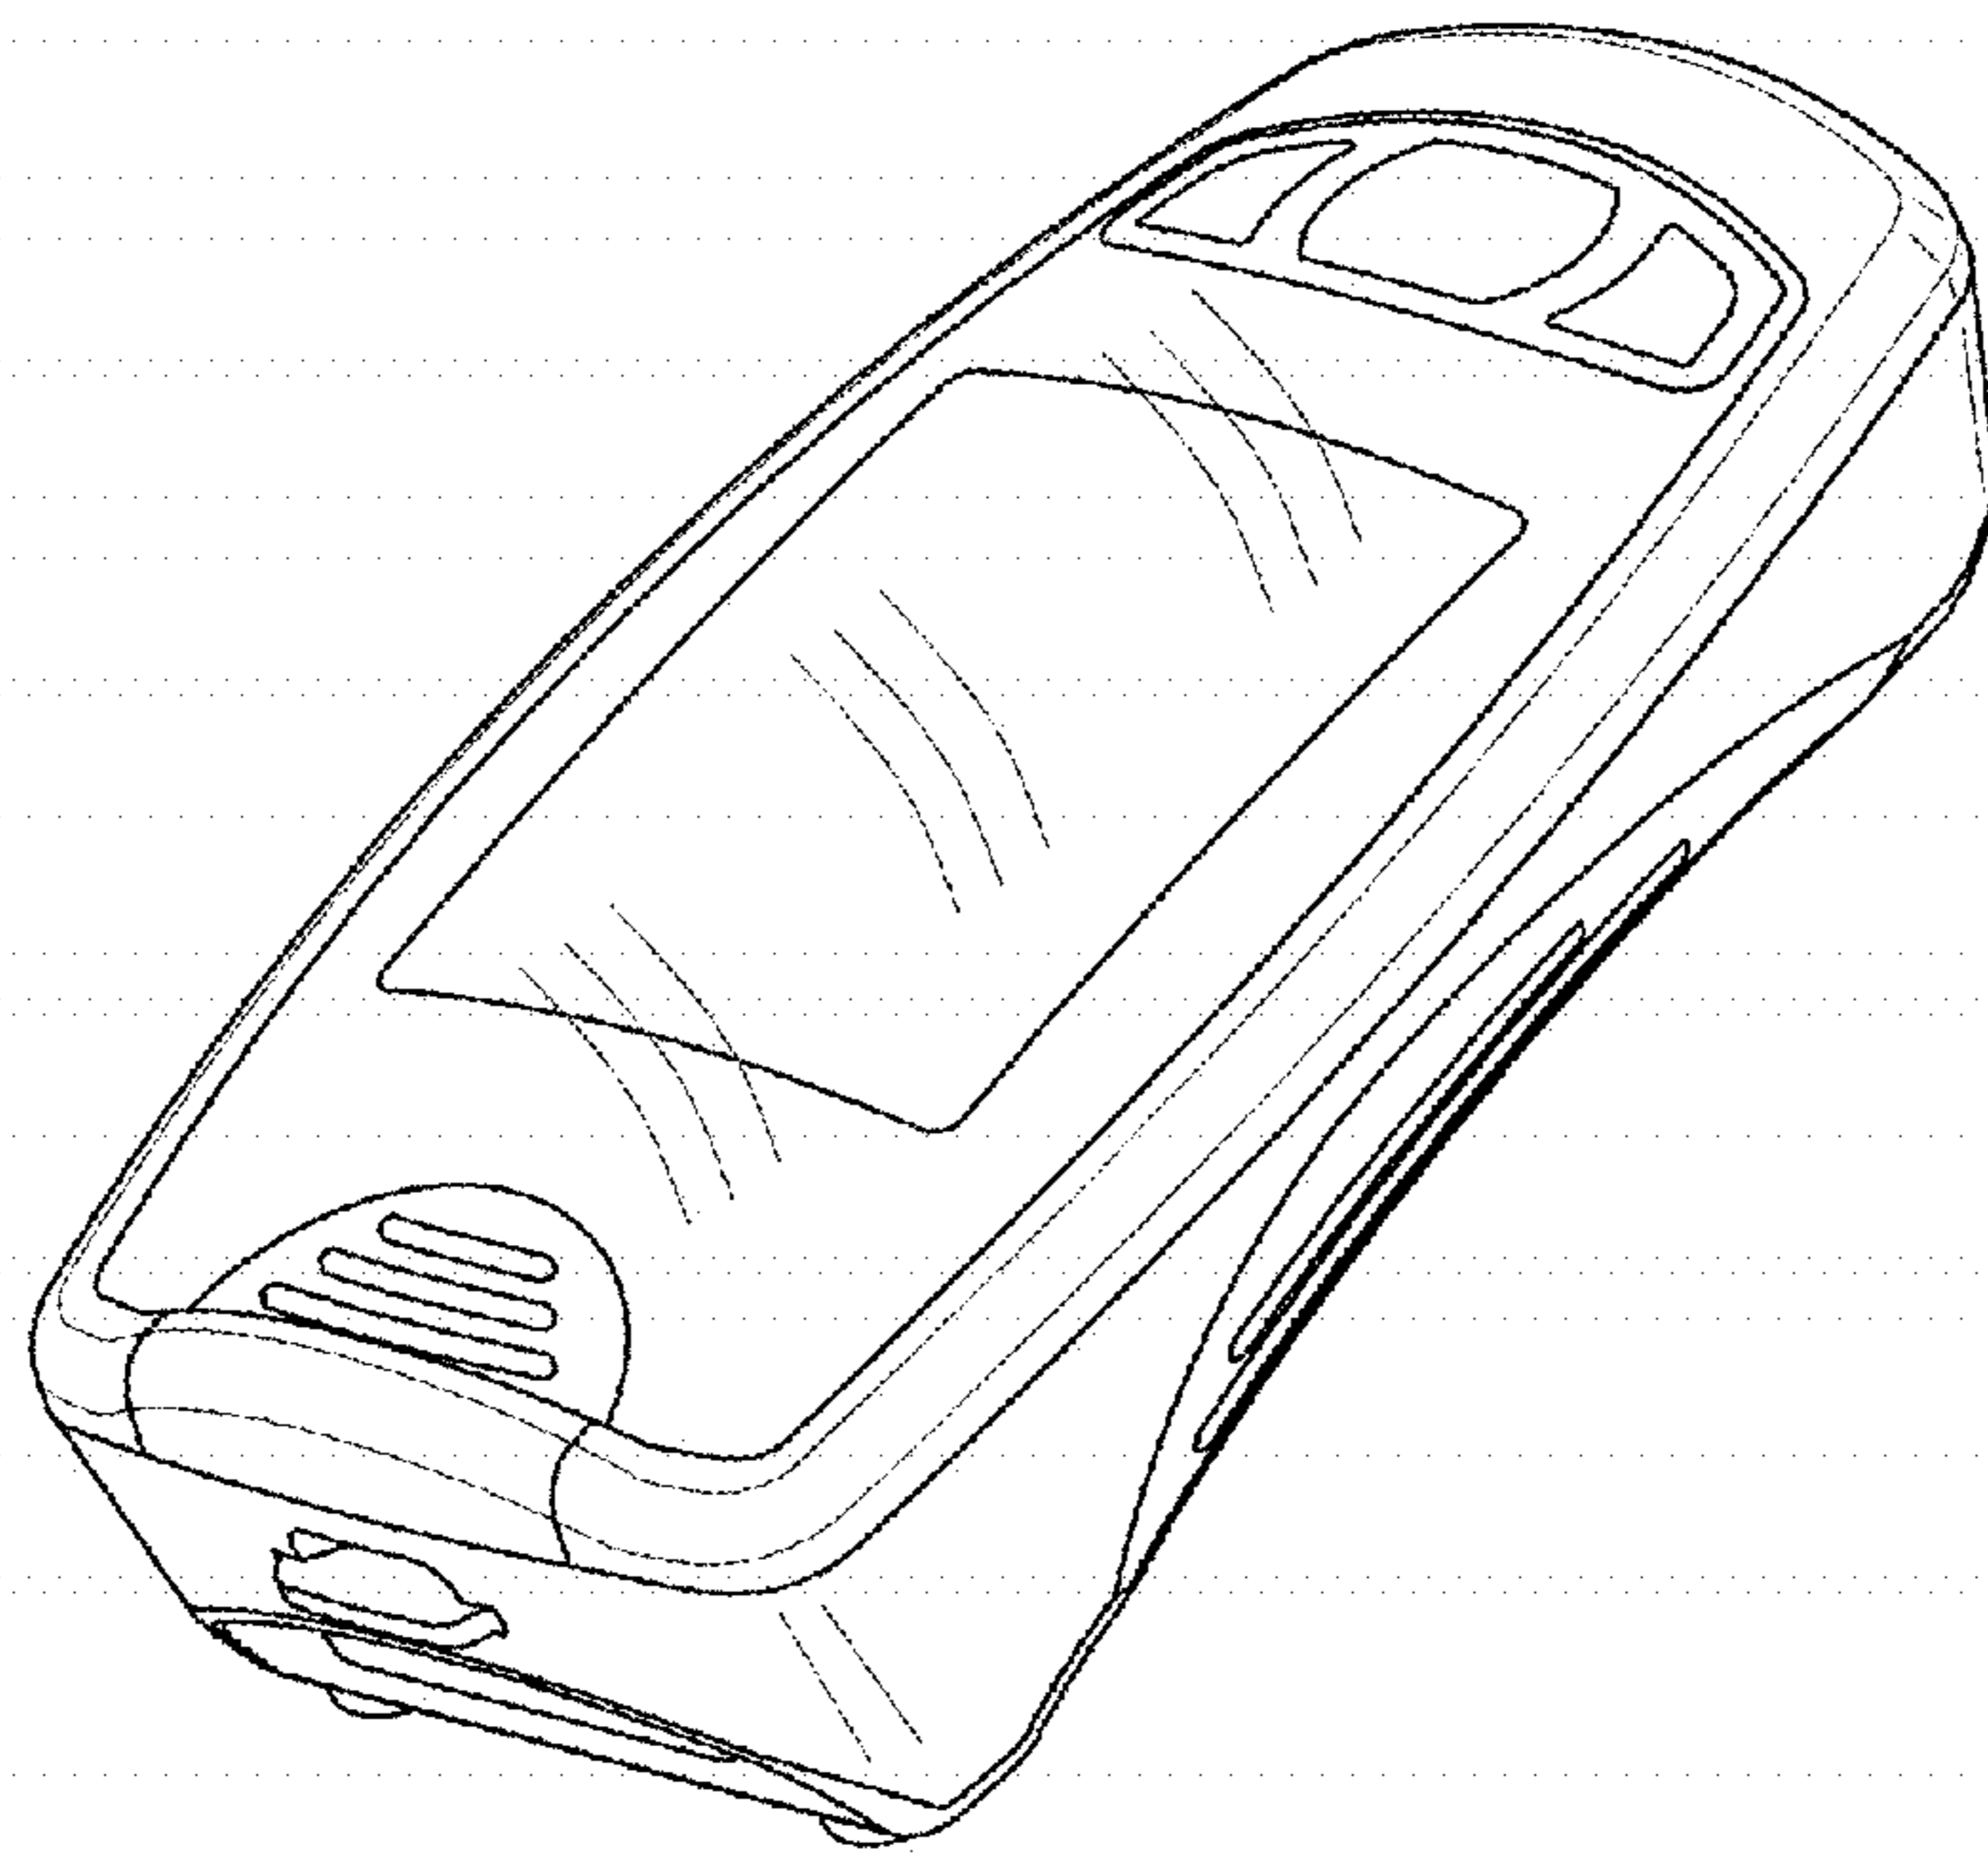


Fig. 9

