



US00D721704S

(12) **United States Design Patent**
Carreon et al.

(10) **Patent No.:** **US D721,704 S**
(45) **Date of Patent:** **** Jan. 27, 2015**

(54) **CHEMILUMINESCENCE COMPACT
IMAGING SCANNER LID**

(71) Applicant: **Li-Cor, Inc.**, Lincoln, NE (US)

(72) Inventors: **Ronaldo Carreon**, Oakland, CA (US);
Matthew Presta, San Mateo, CA (US);
Phil Halbert, San Francisco, CA (US);
Peter Gleason, Berkeley, CA (US)

(73) Assignee: **Li-Cor, Inc.**, Lincoln, NE (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/457,100**

(22) Filed: **Jun. 6, 2013**

(51) **LOC (10) Cl.** **14-02**

(52) **U.S. Cl.**
USPC **D14/425; D14/453**

(58) **Field of Classification Search**
USPC D14/420, 422, 424, 425, 464, 453;
D18/36-39; 235/470; 355/72, 75, 40;
358/474, 486, 488, 494, 497
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | | | |
|-----------|---|---|---------|-----------------|-------|---------|
| D264,345 | S | * | 5/1982 | Masaki et al. | | D18/37 |
| D267,802 | S | * | 2/1983 | Yasutani | | D18/36 |
| D269,274 | S | * | 6/1983 | Hofland et al. | | D18/36 |
| D286,296 | S | * | 10/1986 | Hara et al. | | D18/40 |
| D293,576 | S | * | 1/1988 | Hara | | D14/425 |
| D299,831 | S | * | 2/1989 | Hirata | | D18/37 |
| D304,204 | S | * | 10/1989 | Wada et al. | | D18/37 |
| D304,824 | S | * | 11/1989 | Hara et al. | | D14/425 |
| D304,825 | S | * | 11/1989 | Hara et al. | | D14/425 |
| D305,329 | S | * | 1/1990 | Hiroki et al. | | D14/425 |
| D318,654 | S | * | 7/1991 | Huang | | D14/425 |
| D318,686 | S | * | 7/1991 | Gotham et al. | | D18/36 |
| 5,069,769 | A | * | 12/1991 | Fujimiya et al. | | 204/461 |
| D328,382 | S | * | 7/1992 | Komada et al. | | D18/36 |
| D328,609 | S | * | 8/1992 | Isida | | D18/36 |
| D340,233 | S | * | 10/1993 | Takahashi | | D14/425 |

| | | | | | | |
|-----------|---|---|---------|-----------------|-------|---------|
| D350,769 | S | * | 9/1994 | Hattori et al. | | D18/49 |
| D365,341 | S | * | 12/1995 | Chen | | D14/453 |
| D365,807 | S | * | 1/1996 | Chen | | D14/425 |
| D388,773 | S | * | 1/1998 | Chang et al. | | D14/425 |
| D405,066 | S | * | 2/1999 | Wu et al. | | D14/425 |
| D405,068 | S | * | 2/1999 | Chang et al. | | D14/425 |
| D406,161 | S | * | 2/1999 | Yoshida et al. | | D18/36 |
| 5,953,133 | A | * | 9/1999 | Fujimiya et al. | | 358/474 |
| D416,874 | S | * | 11/1999 | Khovaylo et al. | | D14/453 |
| 5,991,030 | A | * | 11/1999 | Yamamoto et al. | | 356/451 |
| D421,042 | S | * | 2/2000 | Short et al. | | D18/36 |
| D423,040 | S | * | 4/2000 | Ohta et al. | | D18/36 |

(Continued)

Primary Examiner — Susan Moon Lee

(74) *Attorney, Agent, or Firm* — Kilpatrick Townsend & Stockton LLP; Mark P. Mathison

(57) **CLAIM**


The ornamental design for a chemiluminescence compact imaging scanner lid, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a chemiluminescence compact imaging scanner lid showing our new design;
 FIG. 2 is a front elevational view;
 FIG. 3 is a rear elevational view;
 FIG. 4 is a left side elevational view;
 FIG. 5 is a right side elevational view;
 FIG. 6 is a top plan view thereof;
 FIG. 7 is a bottom plan view partially occluded by a scanner base; and,
 FIG. 8 is a perspective view showing a bottom of the design. Portions or features of the chemiluminescence compact imaging scanner lid not shown in the drawings form no part of the claimed design. Broken lines and entirely unshaded portions contained within broken line are not claimed. Views that are not shown are not claimed.

The chemiluminescence compact imaging scanner lid is intended for use as a light-tight cover lid for a scanner that images molecular biology assays exhibiting chemiluminescence or other luminescence.

1 Claim, 6 Drawing Sheets

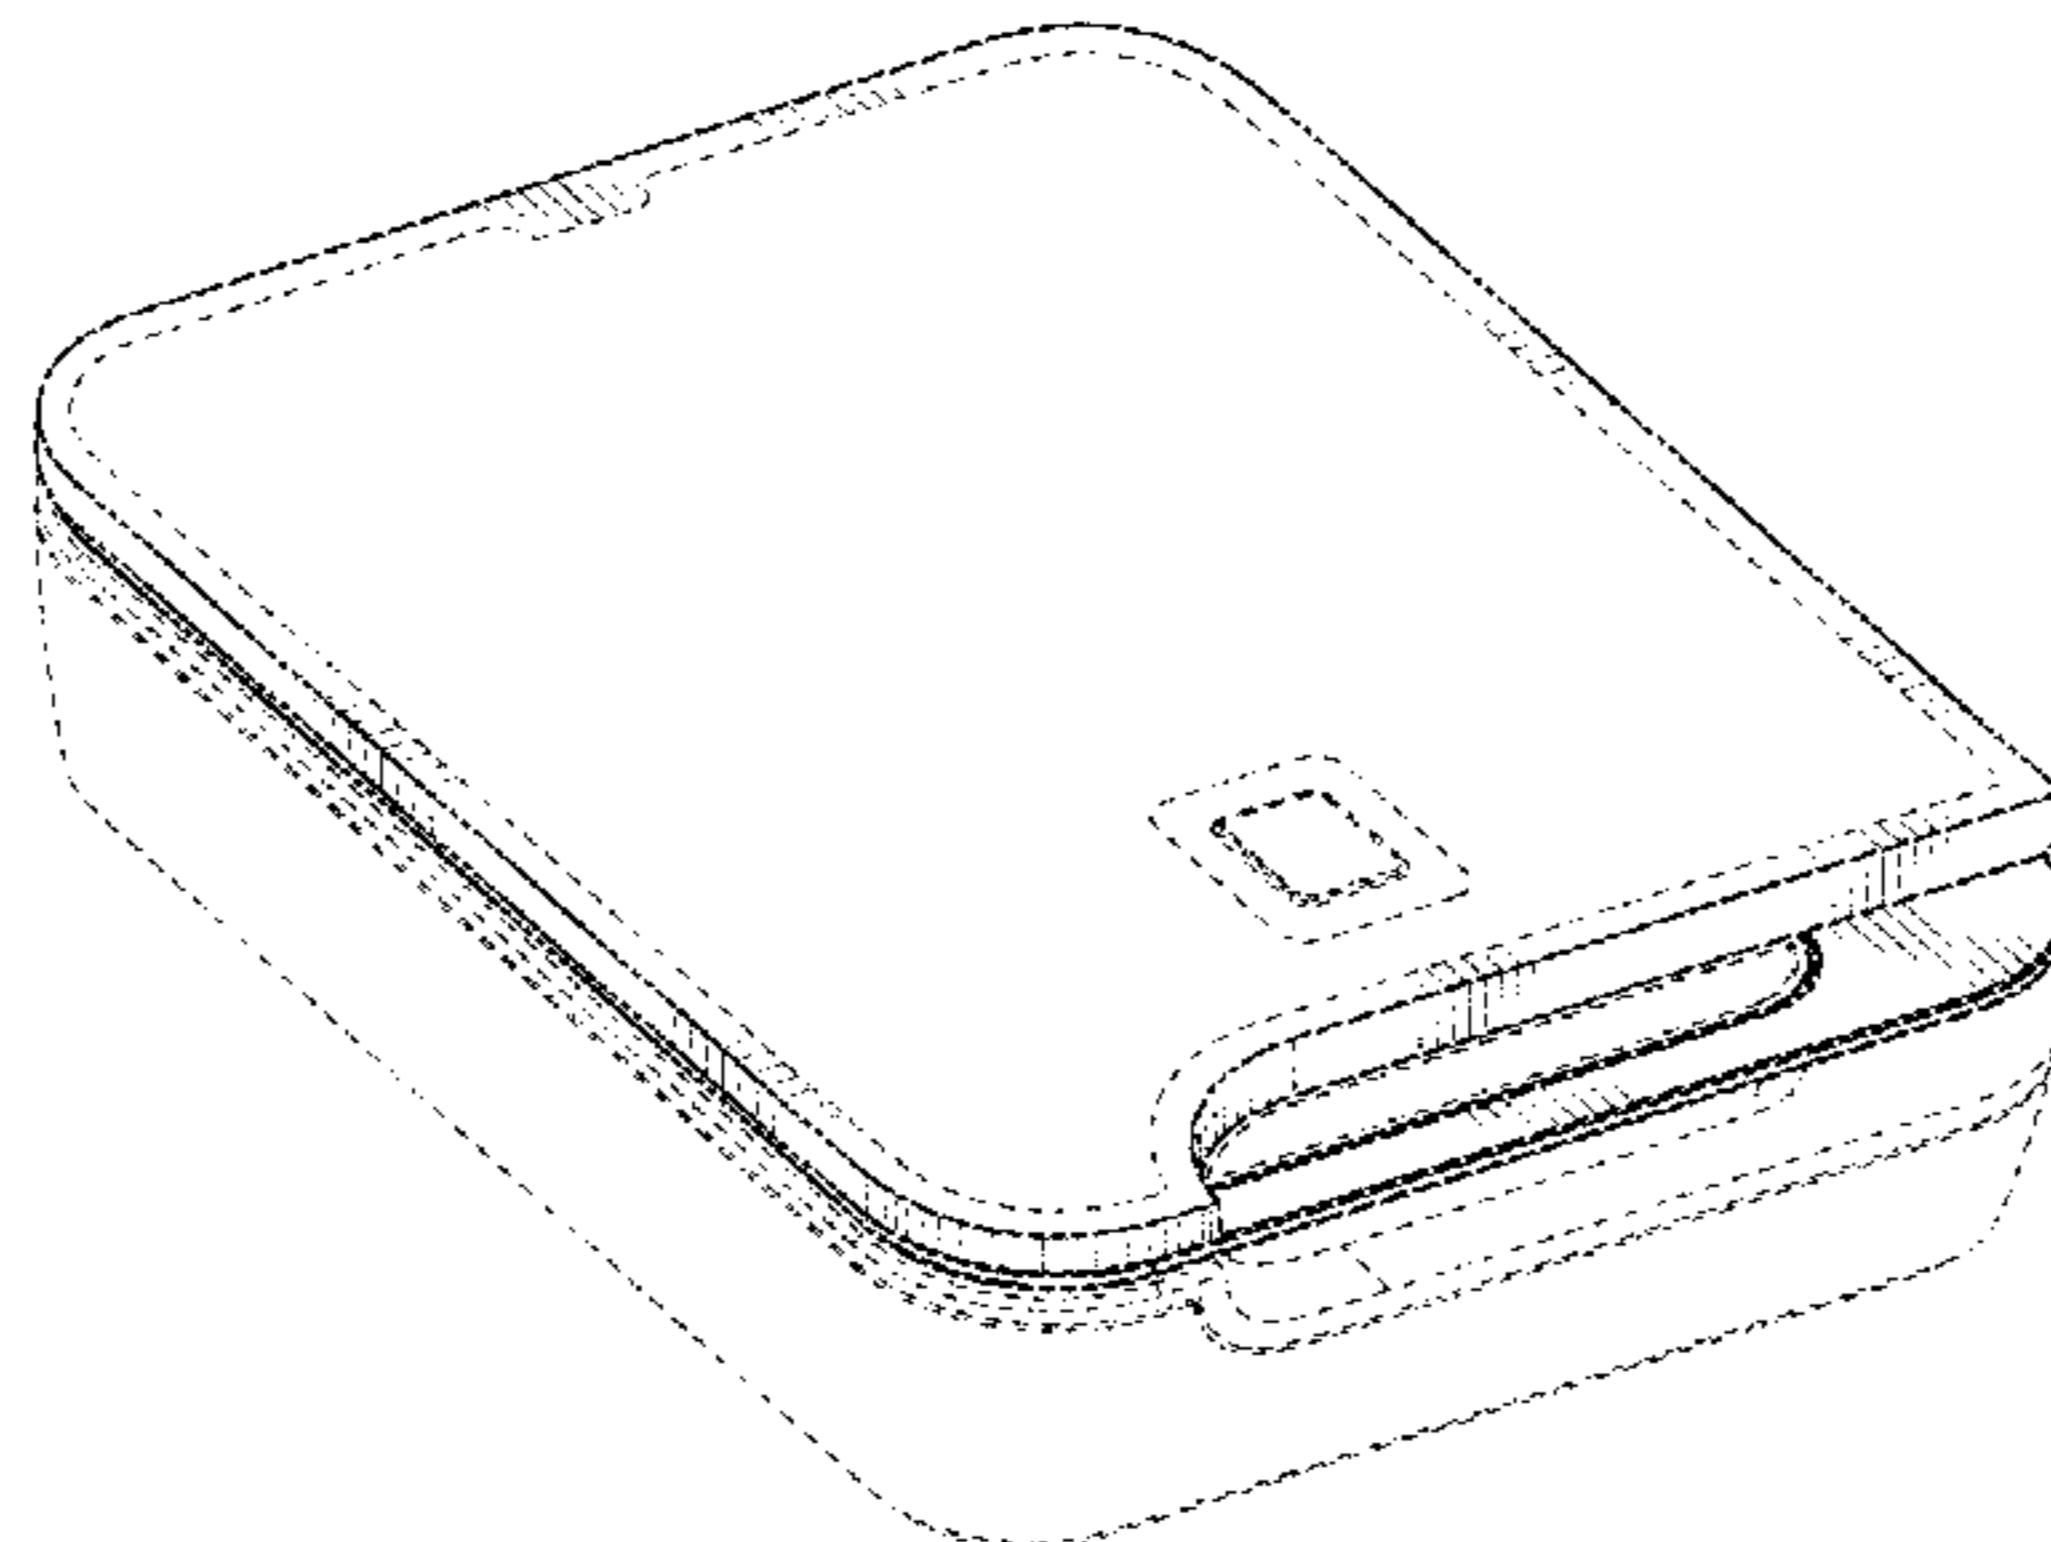

(56)

References Cited

U.S. PATENT DOCUMENTS

D440,571 S * 4/2001 Omuro et al. D14/425
 D447,765 S * 9/2001 Hatanaka et al. D18/39
 D448,382 S * 9/2001 Khovaylo et al. D14/425
 D467,927 S * 12/2002 Khovaylo et al. D14/425
 D469,096 S * 1/2003 Khovaylo et al. D14/425
 D494,211 S * 8/2004 Yoshida et al. D18/39
 6,782,223 B2 * 8/2004 Yoshida 399/124
 7,003,244 B2 * 2/2006 Cho 399/110
 D528,155 S * 9/2006 Katayama D18/55
 D532,450 S * 11/2006 Smith et al. D18/55
 D579,973 S * 11/2008 Park et al. D18/55
 D584,766 S * 1/2009 Tani D18/55
 D608,823 S * 1/2010 Tomono D18/55

7,649,618 B2 * 1/2010 Tuschel et al. 356/73
 7,773,223 B2 * 8/2010 Ikami 356/417
 D626,588 S * 11/2010 Kim et al. D18/39
 D639,851 S * 6/2011 Penke et al. D18/55
 D667,017 S * 9/2012 Tani D14/463
 8,486,644 B2 * 7/2013 Bouzid et al. 435/7.1
 8,722,346 B2 * 5/2014 Bouzid et al. 435/7.1
 2006/0072179 A1 * 4/2006 Caster et al. 359/202
 2008/0240747 A1 * 10/2008 Ikami 399/32
 2009/0141132 A1 * 6/2009 Lehmann et al. 348/207.99
 2010/0110509 A1 * 5/2010 Cui et al. 358/498
 2012/0142086 A1 * 6/2012 Haguët et al. 435/288.7
 2013/0157282 A1 * 6/2013 Bouzid et al. 435/7.1
 2013/0280737 A1 * 10/2013 Bouzid et al. 435/7.92
 2014/0206568 A1 * 7/2014 Bouzid et al. 506/9

* cited by examiner

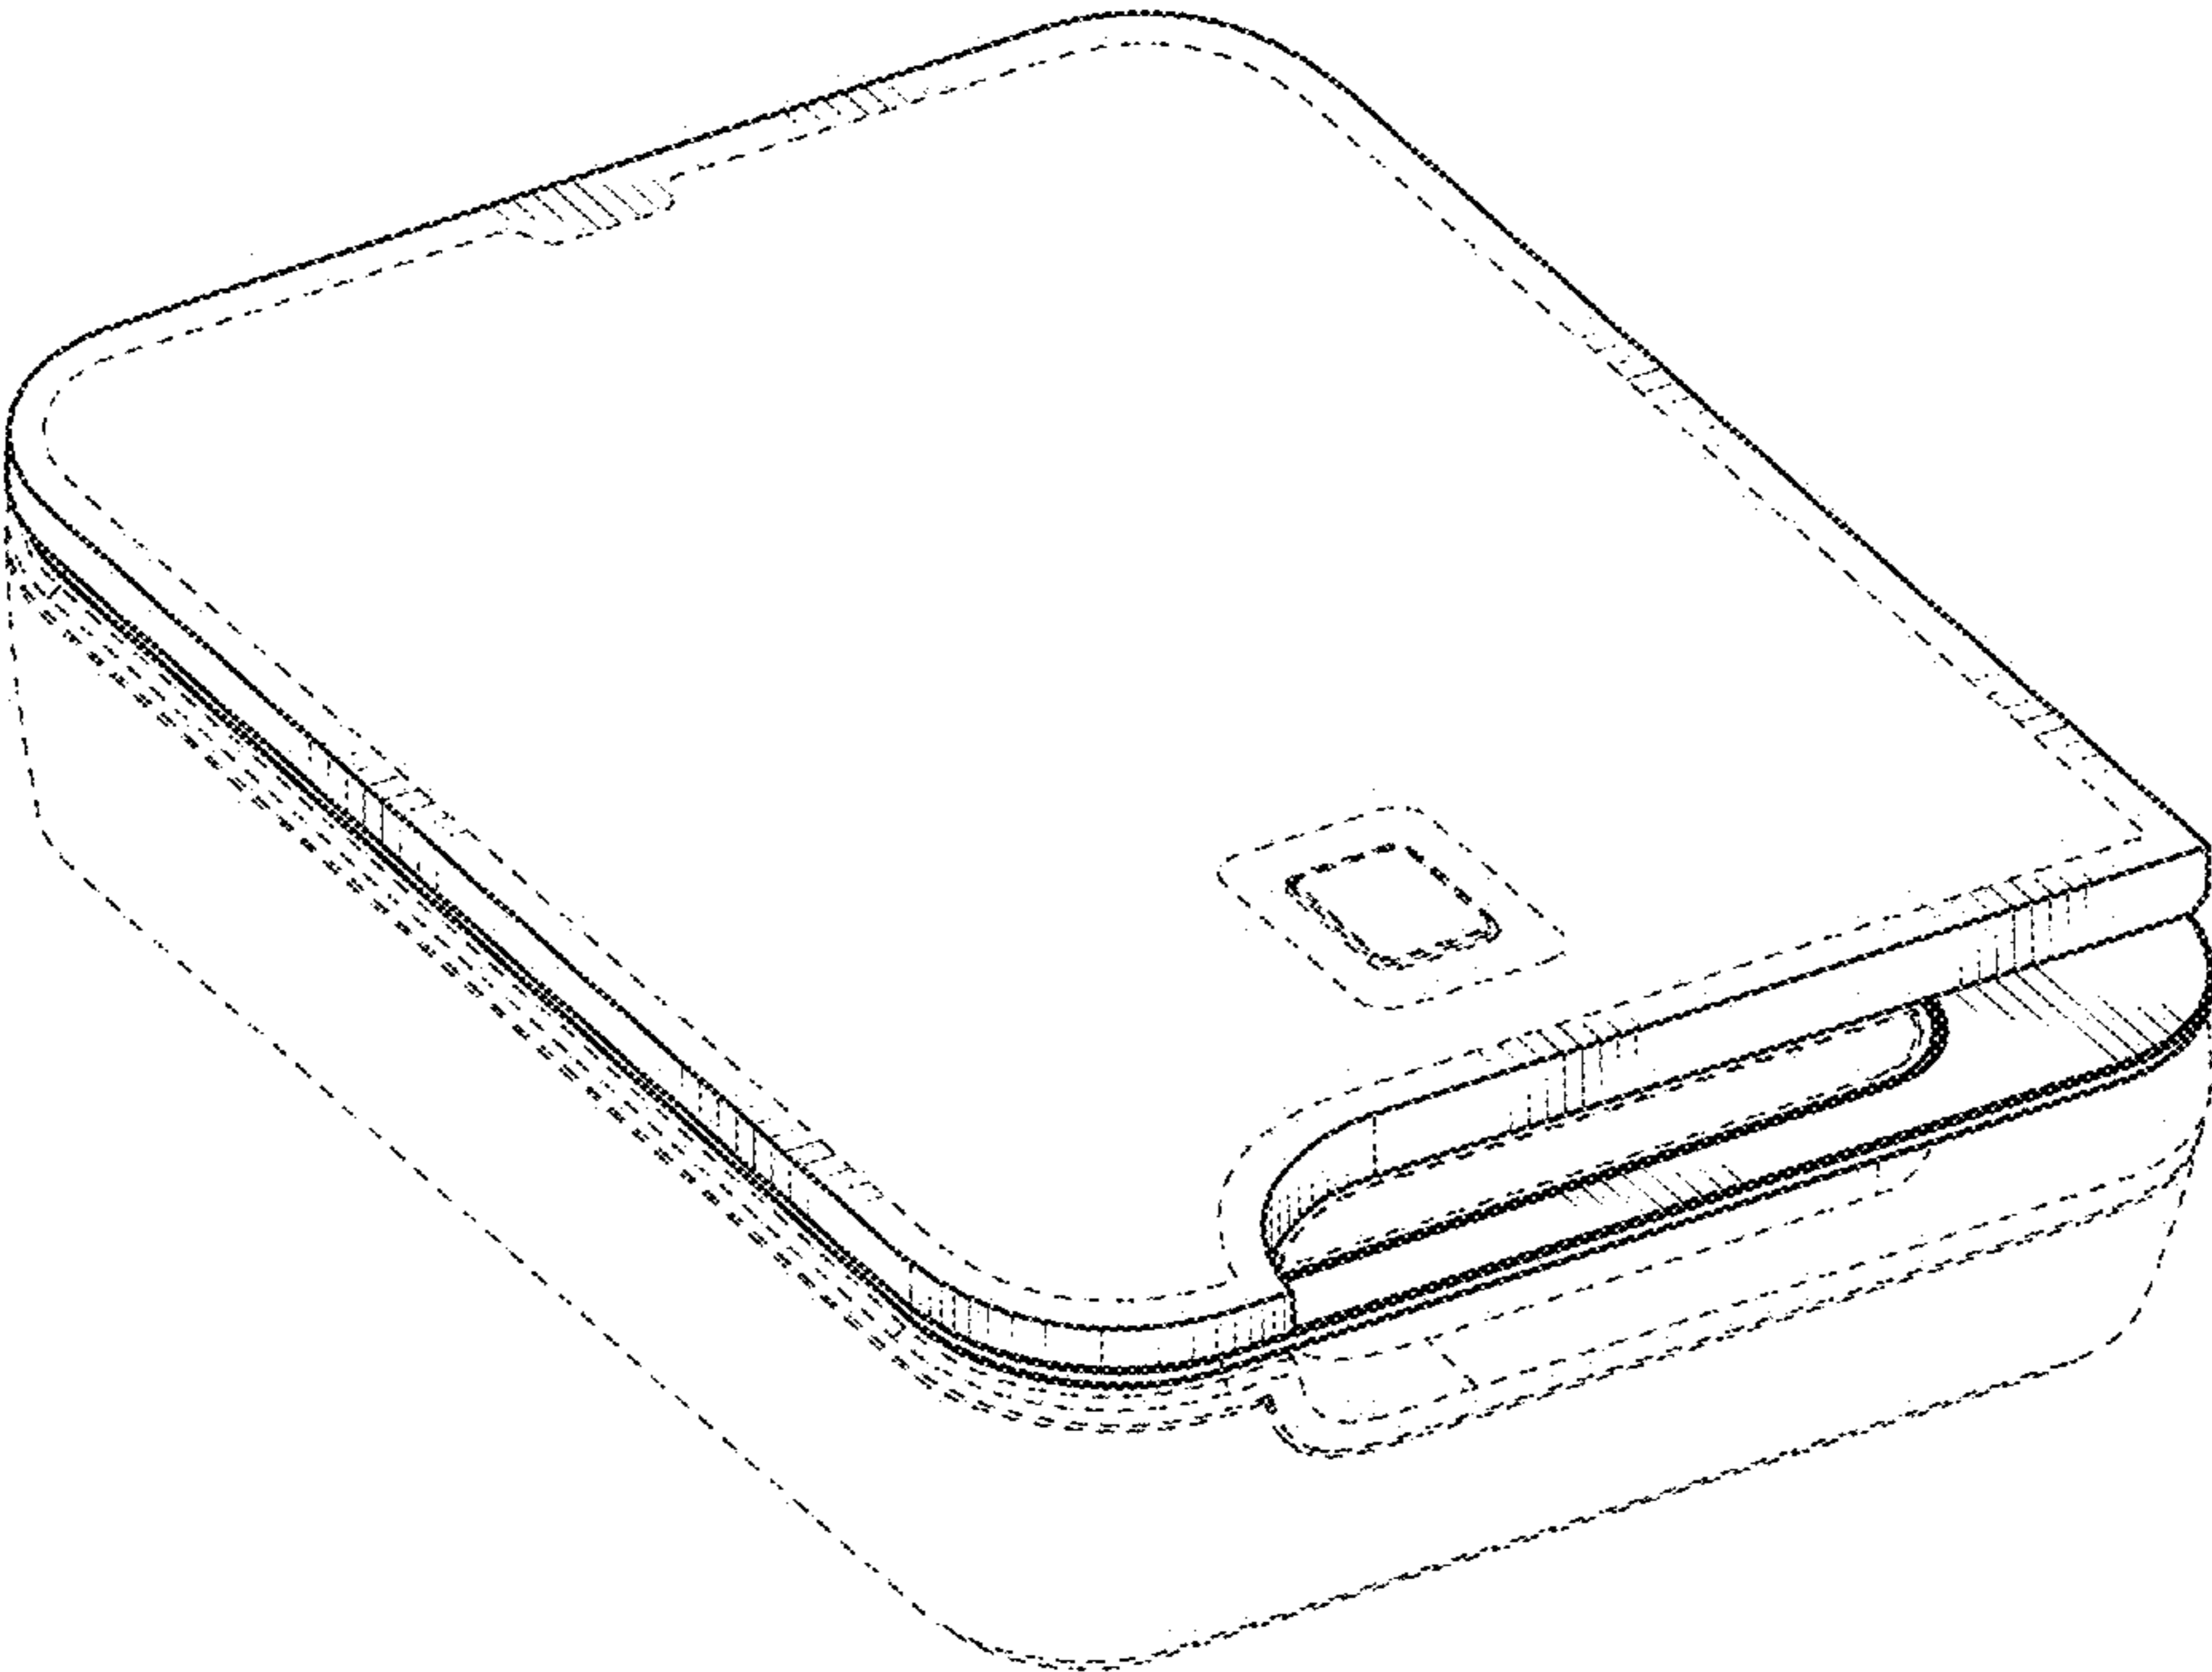


FIG. 1

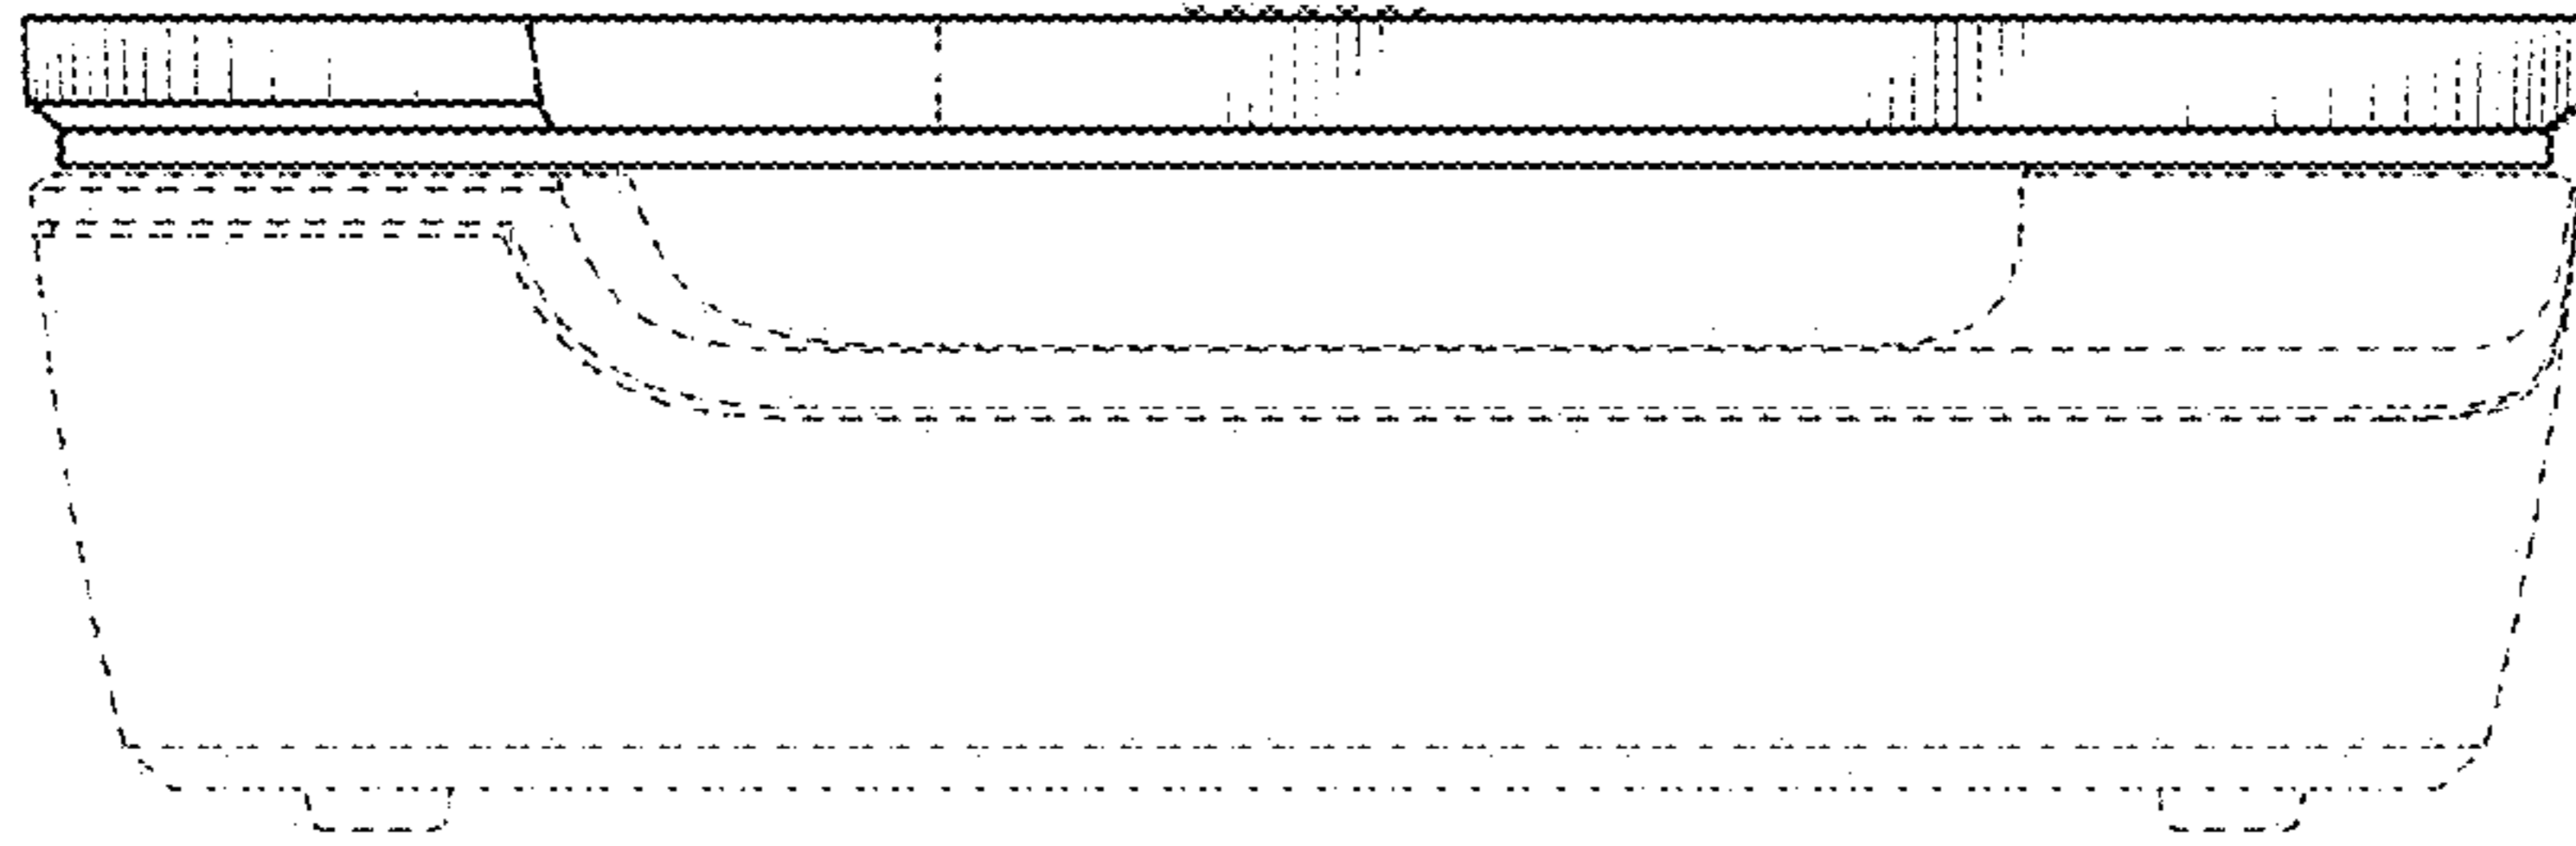


FIG. 2

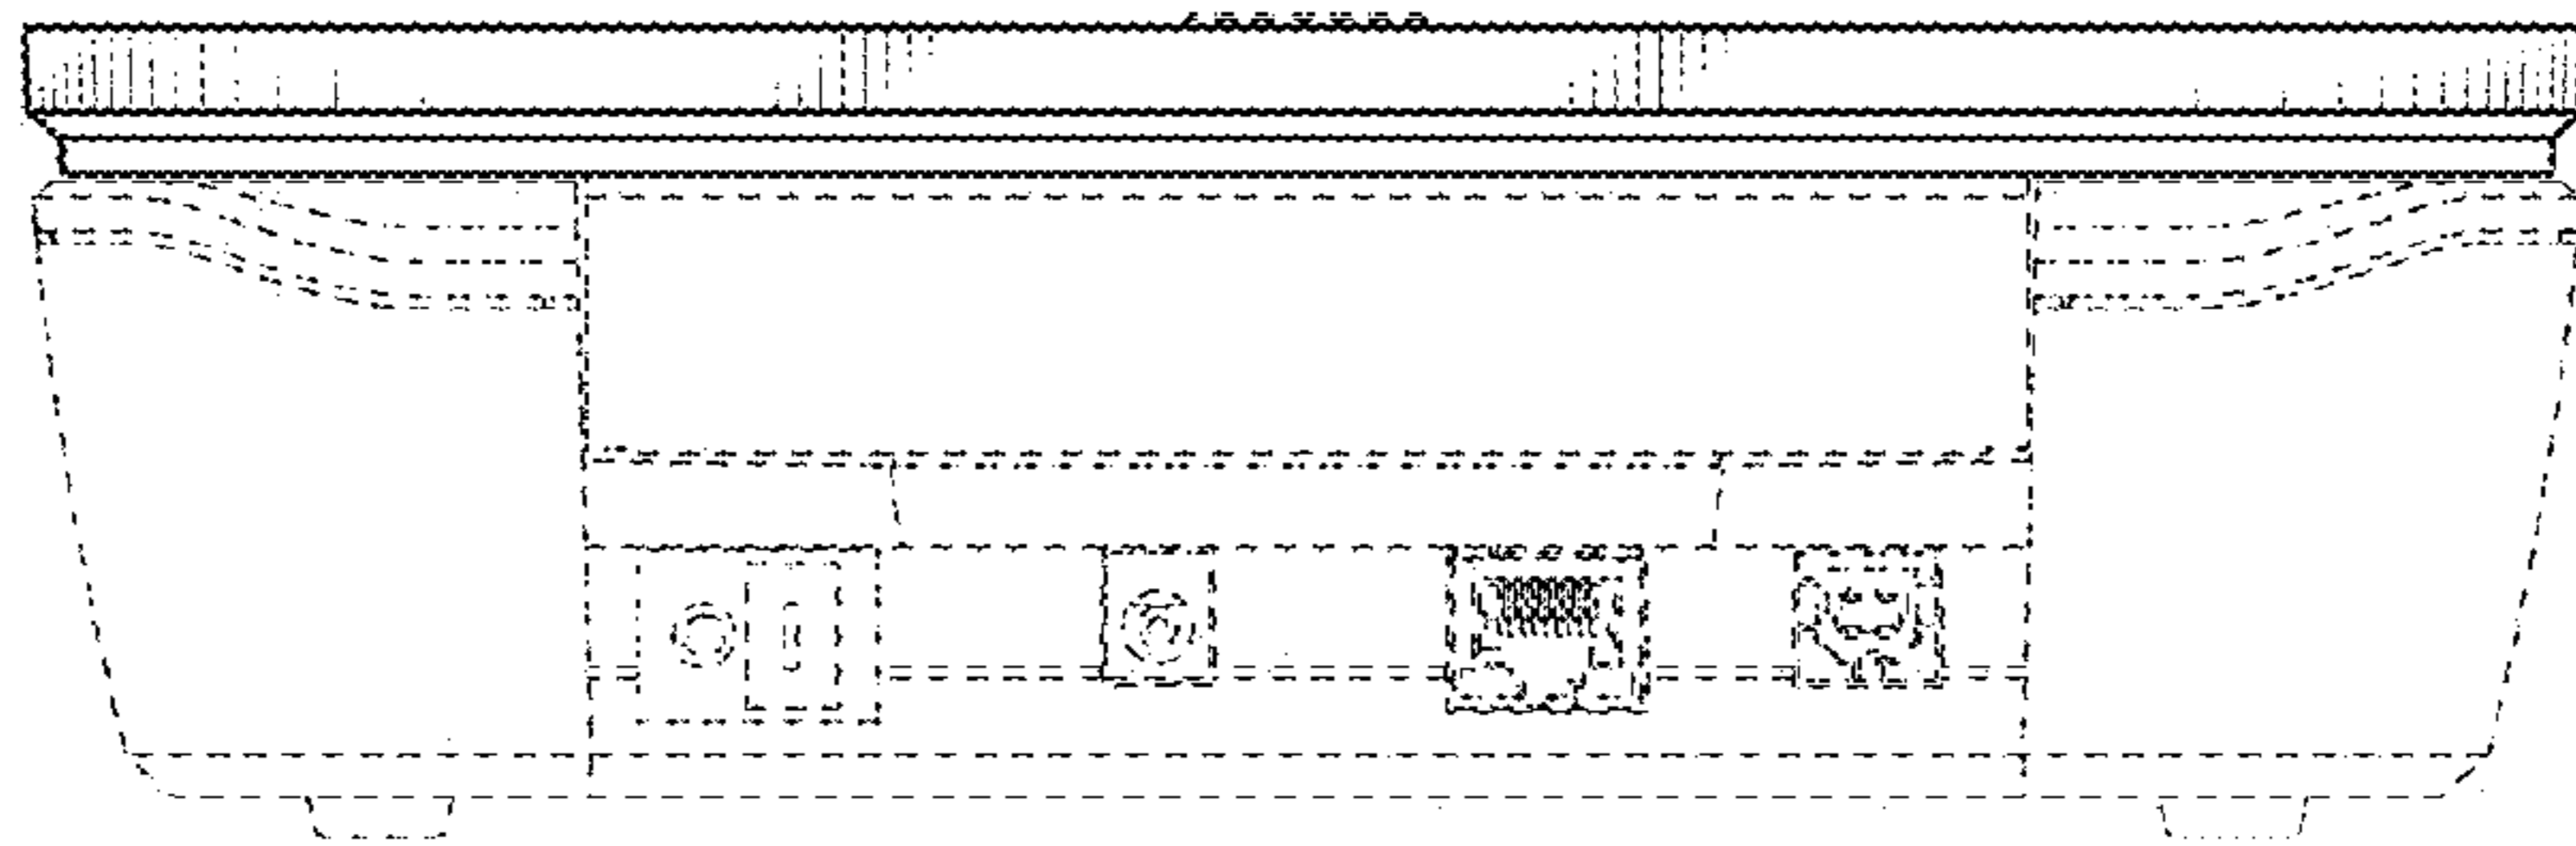


FIG. 3

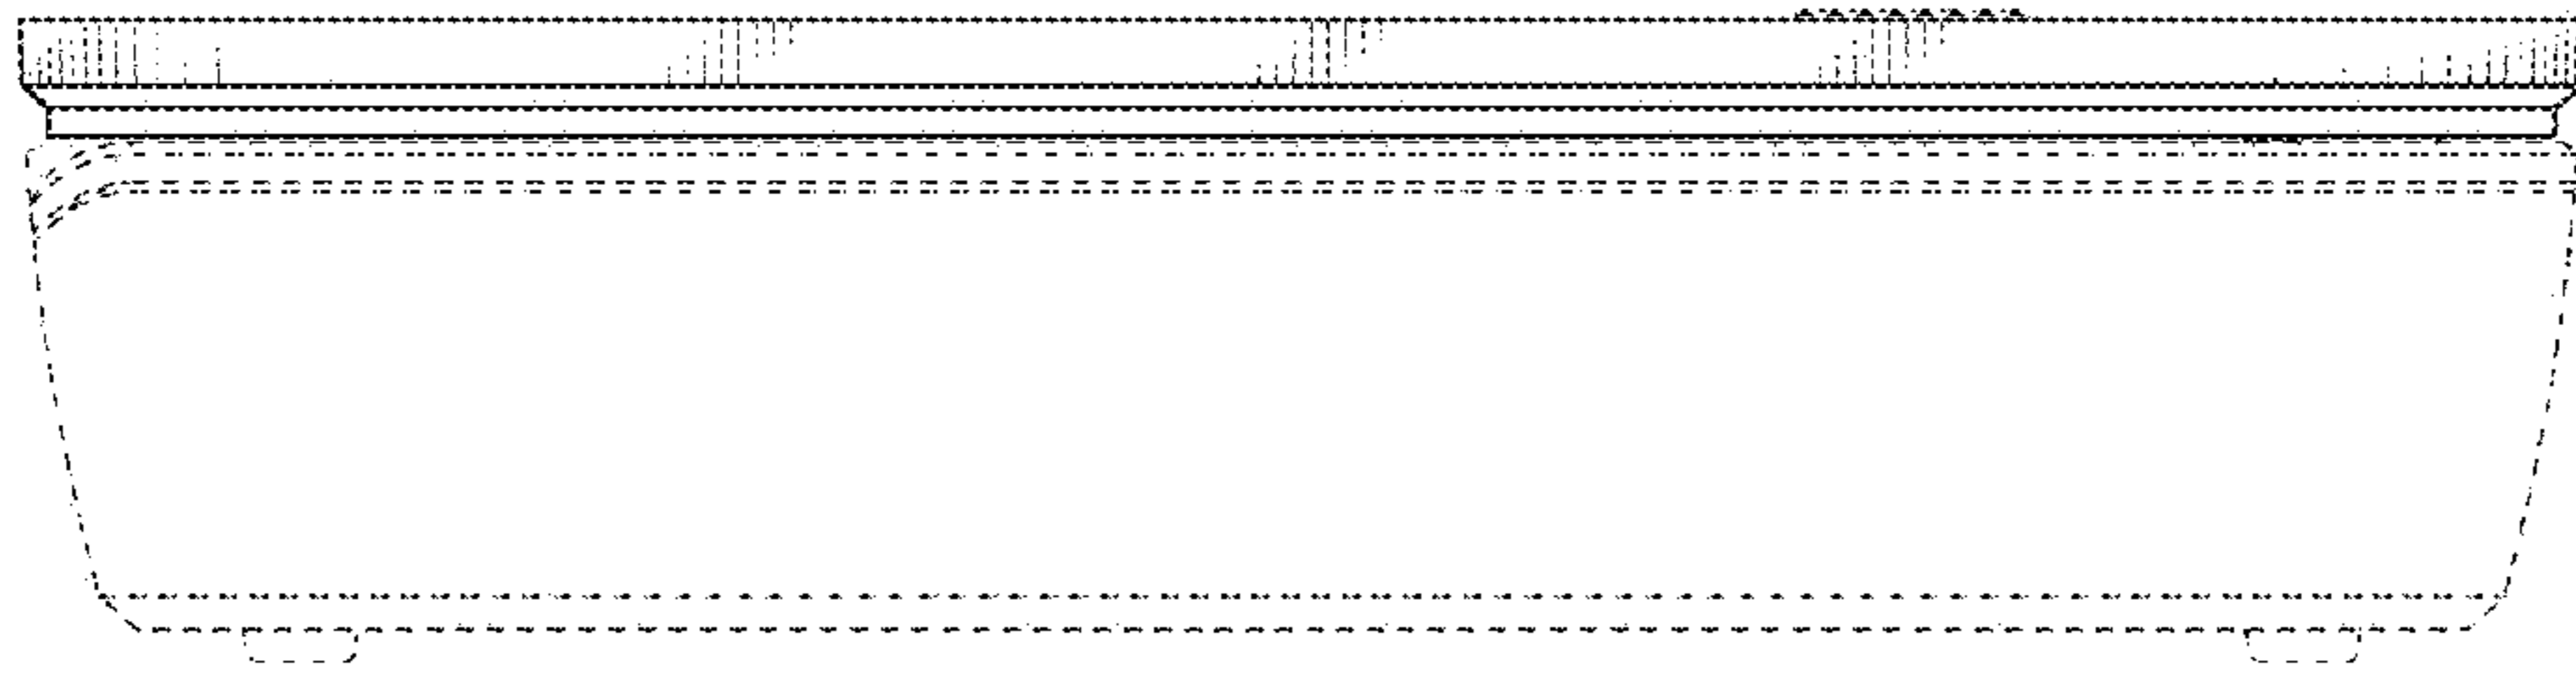


FIG. 4

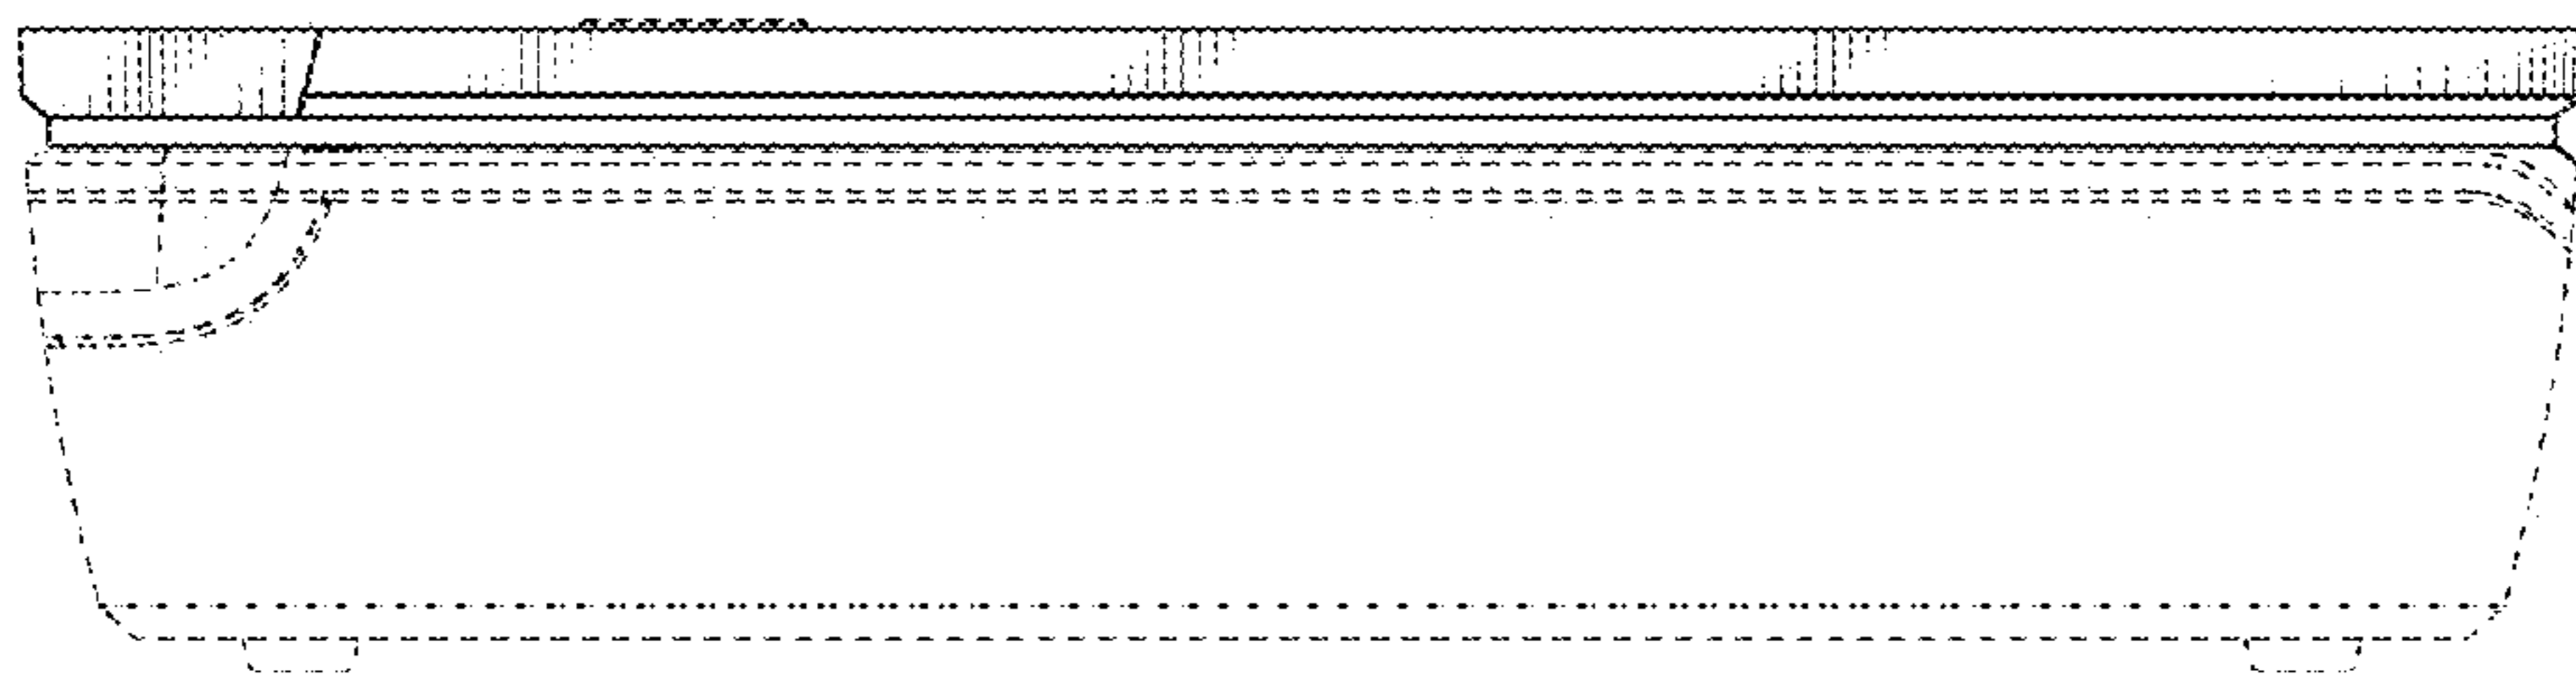


FIG. 5

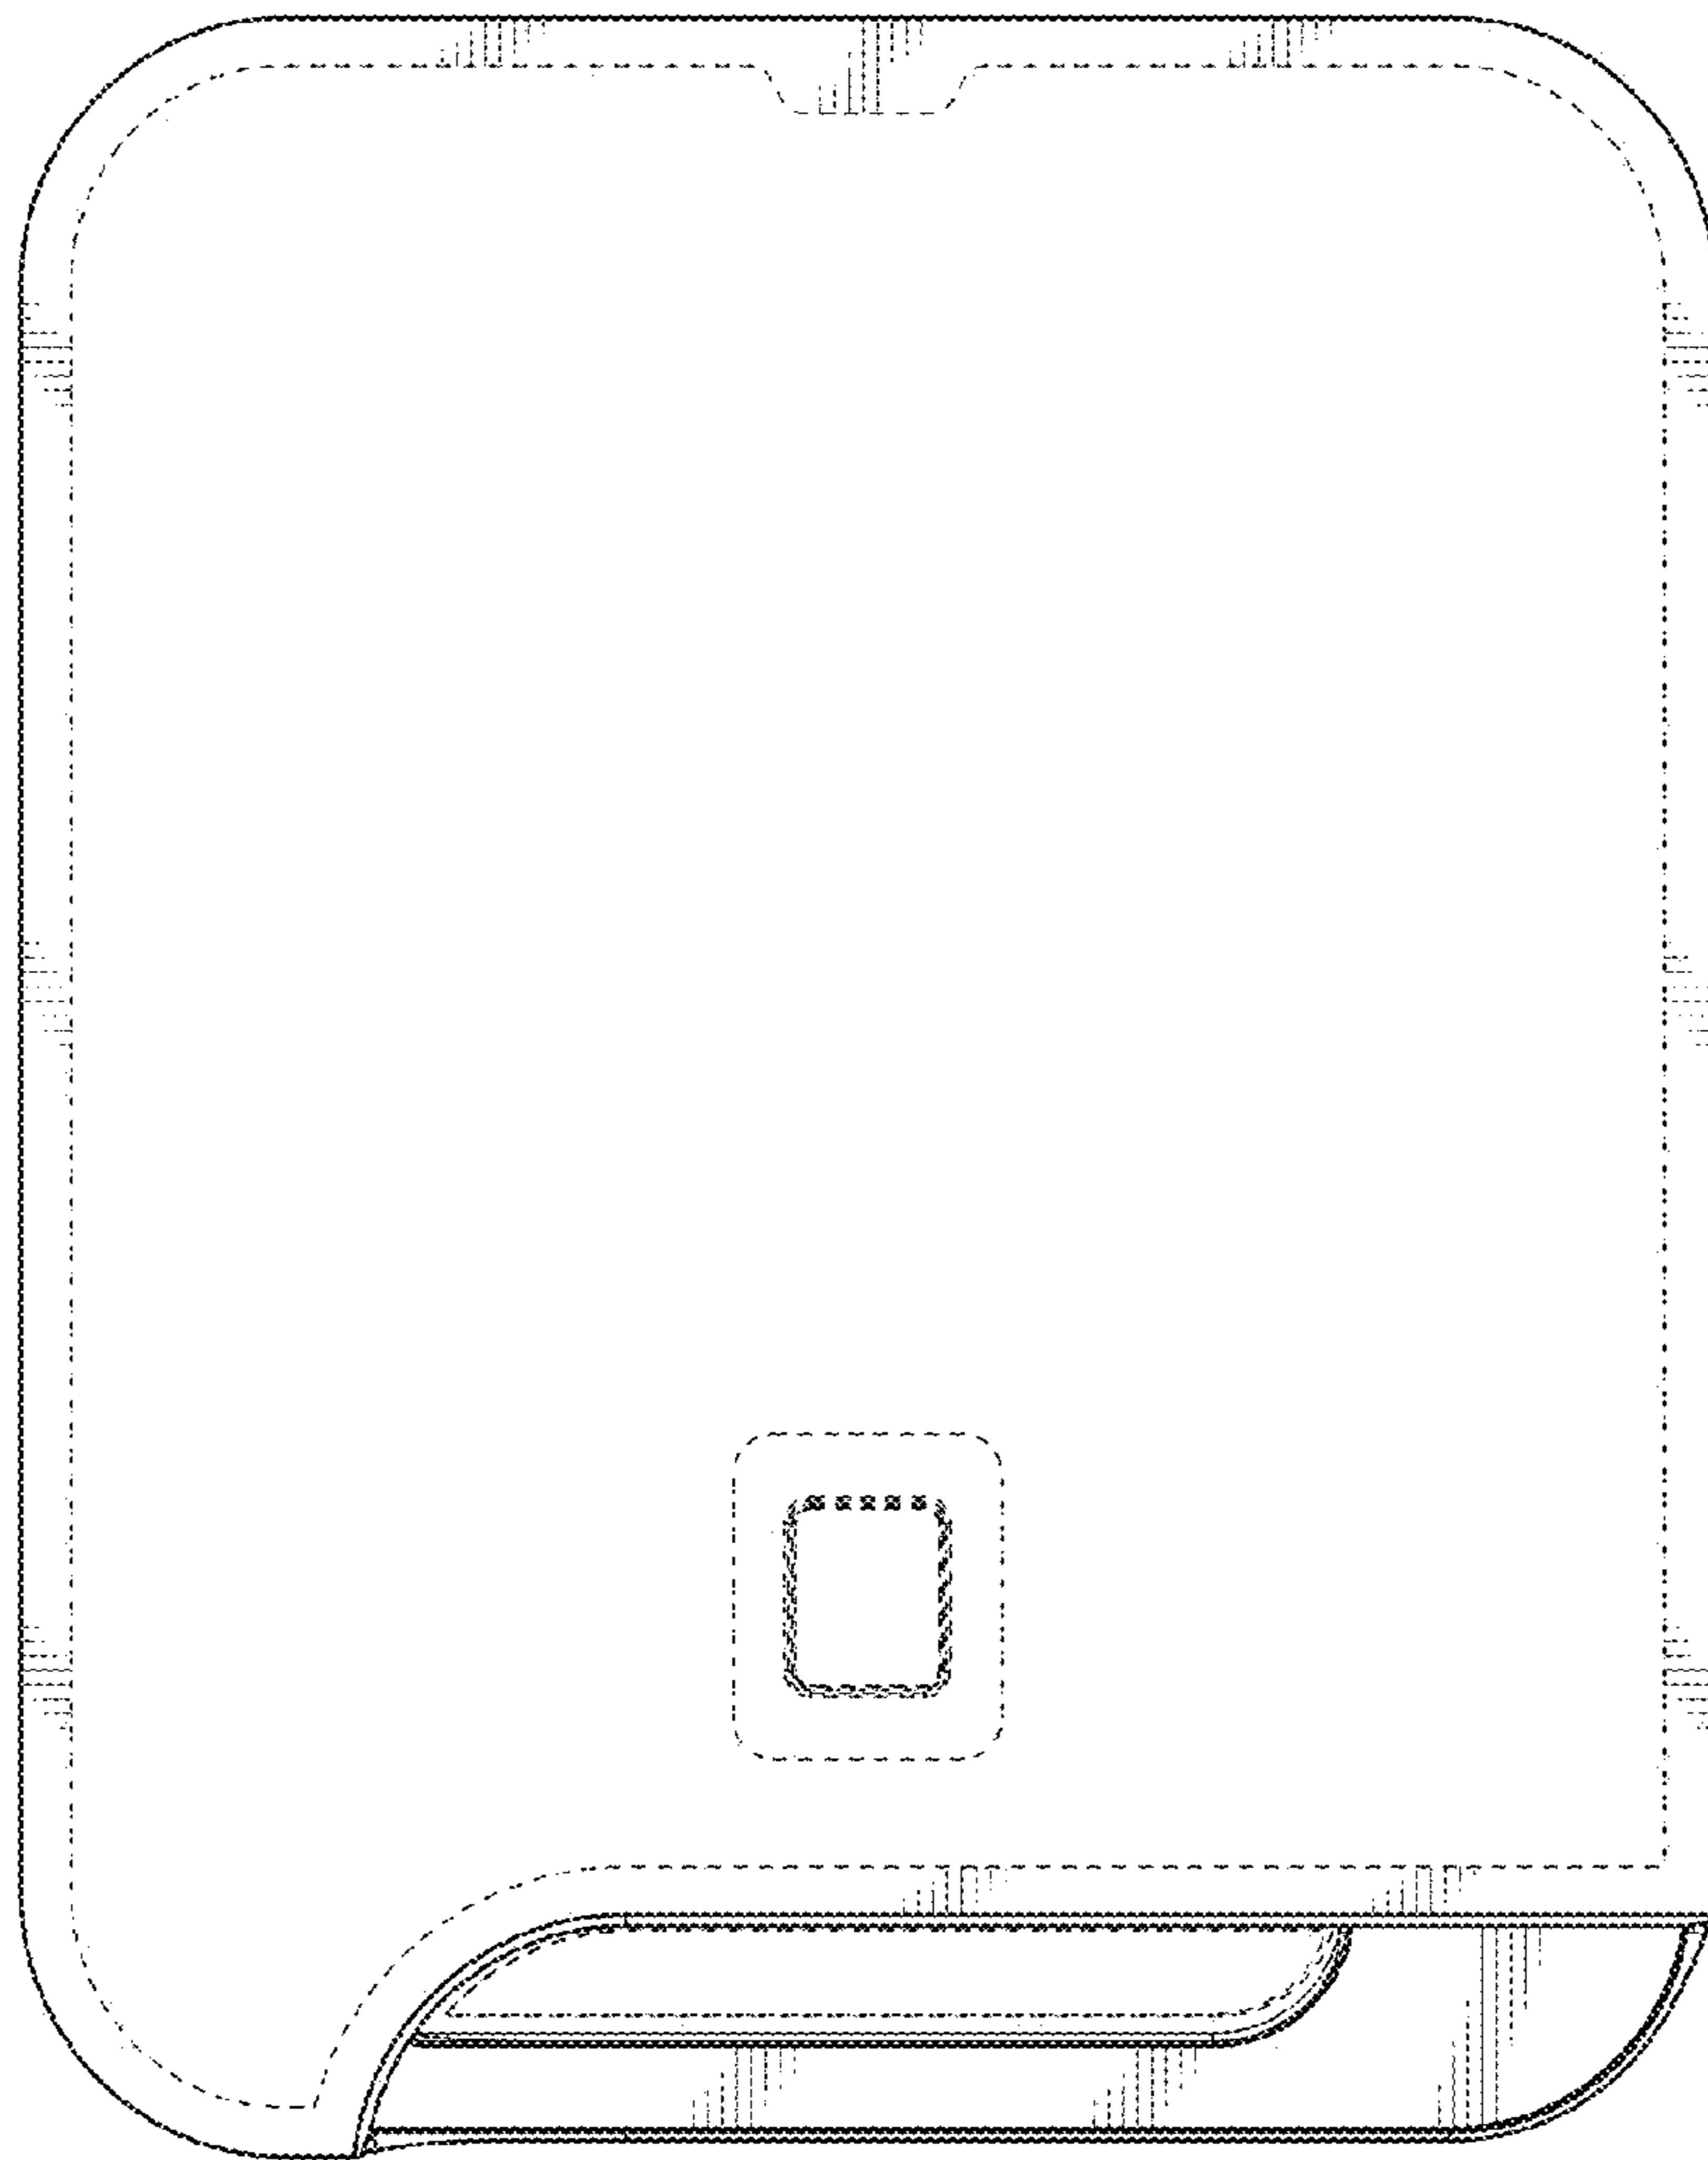


FIG. 6

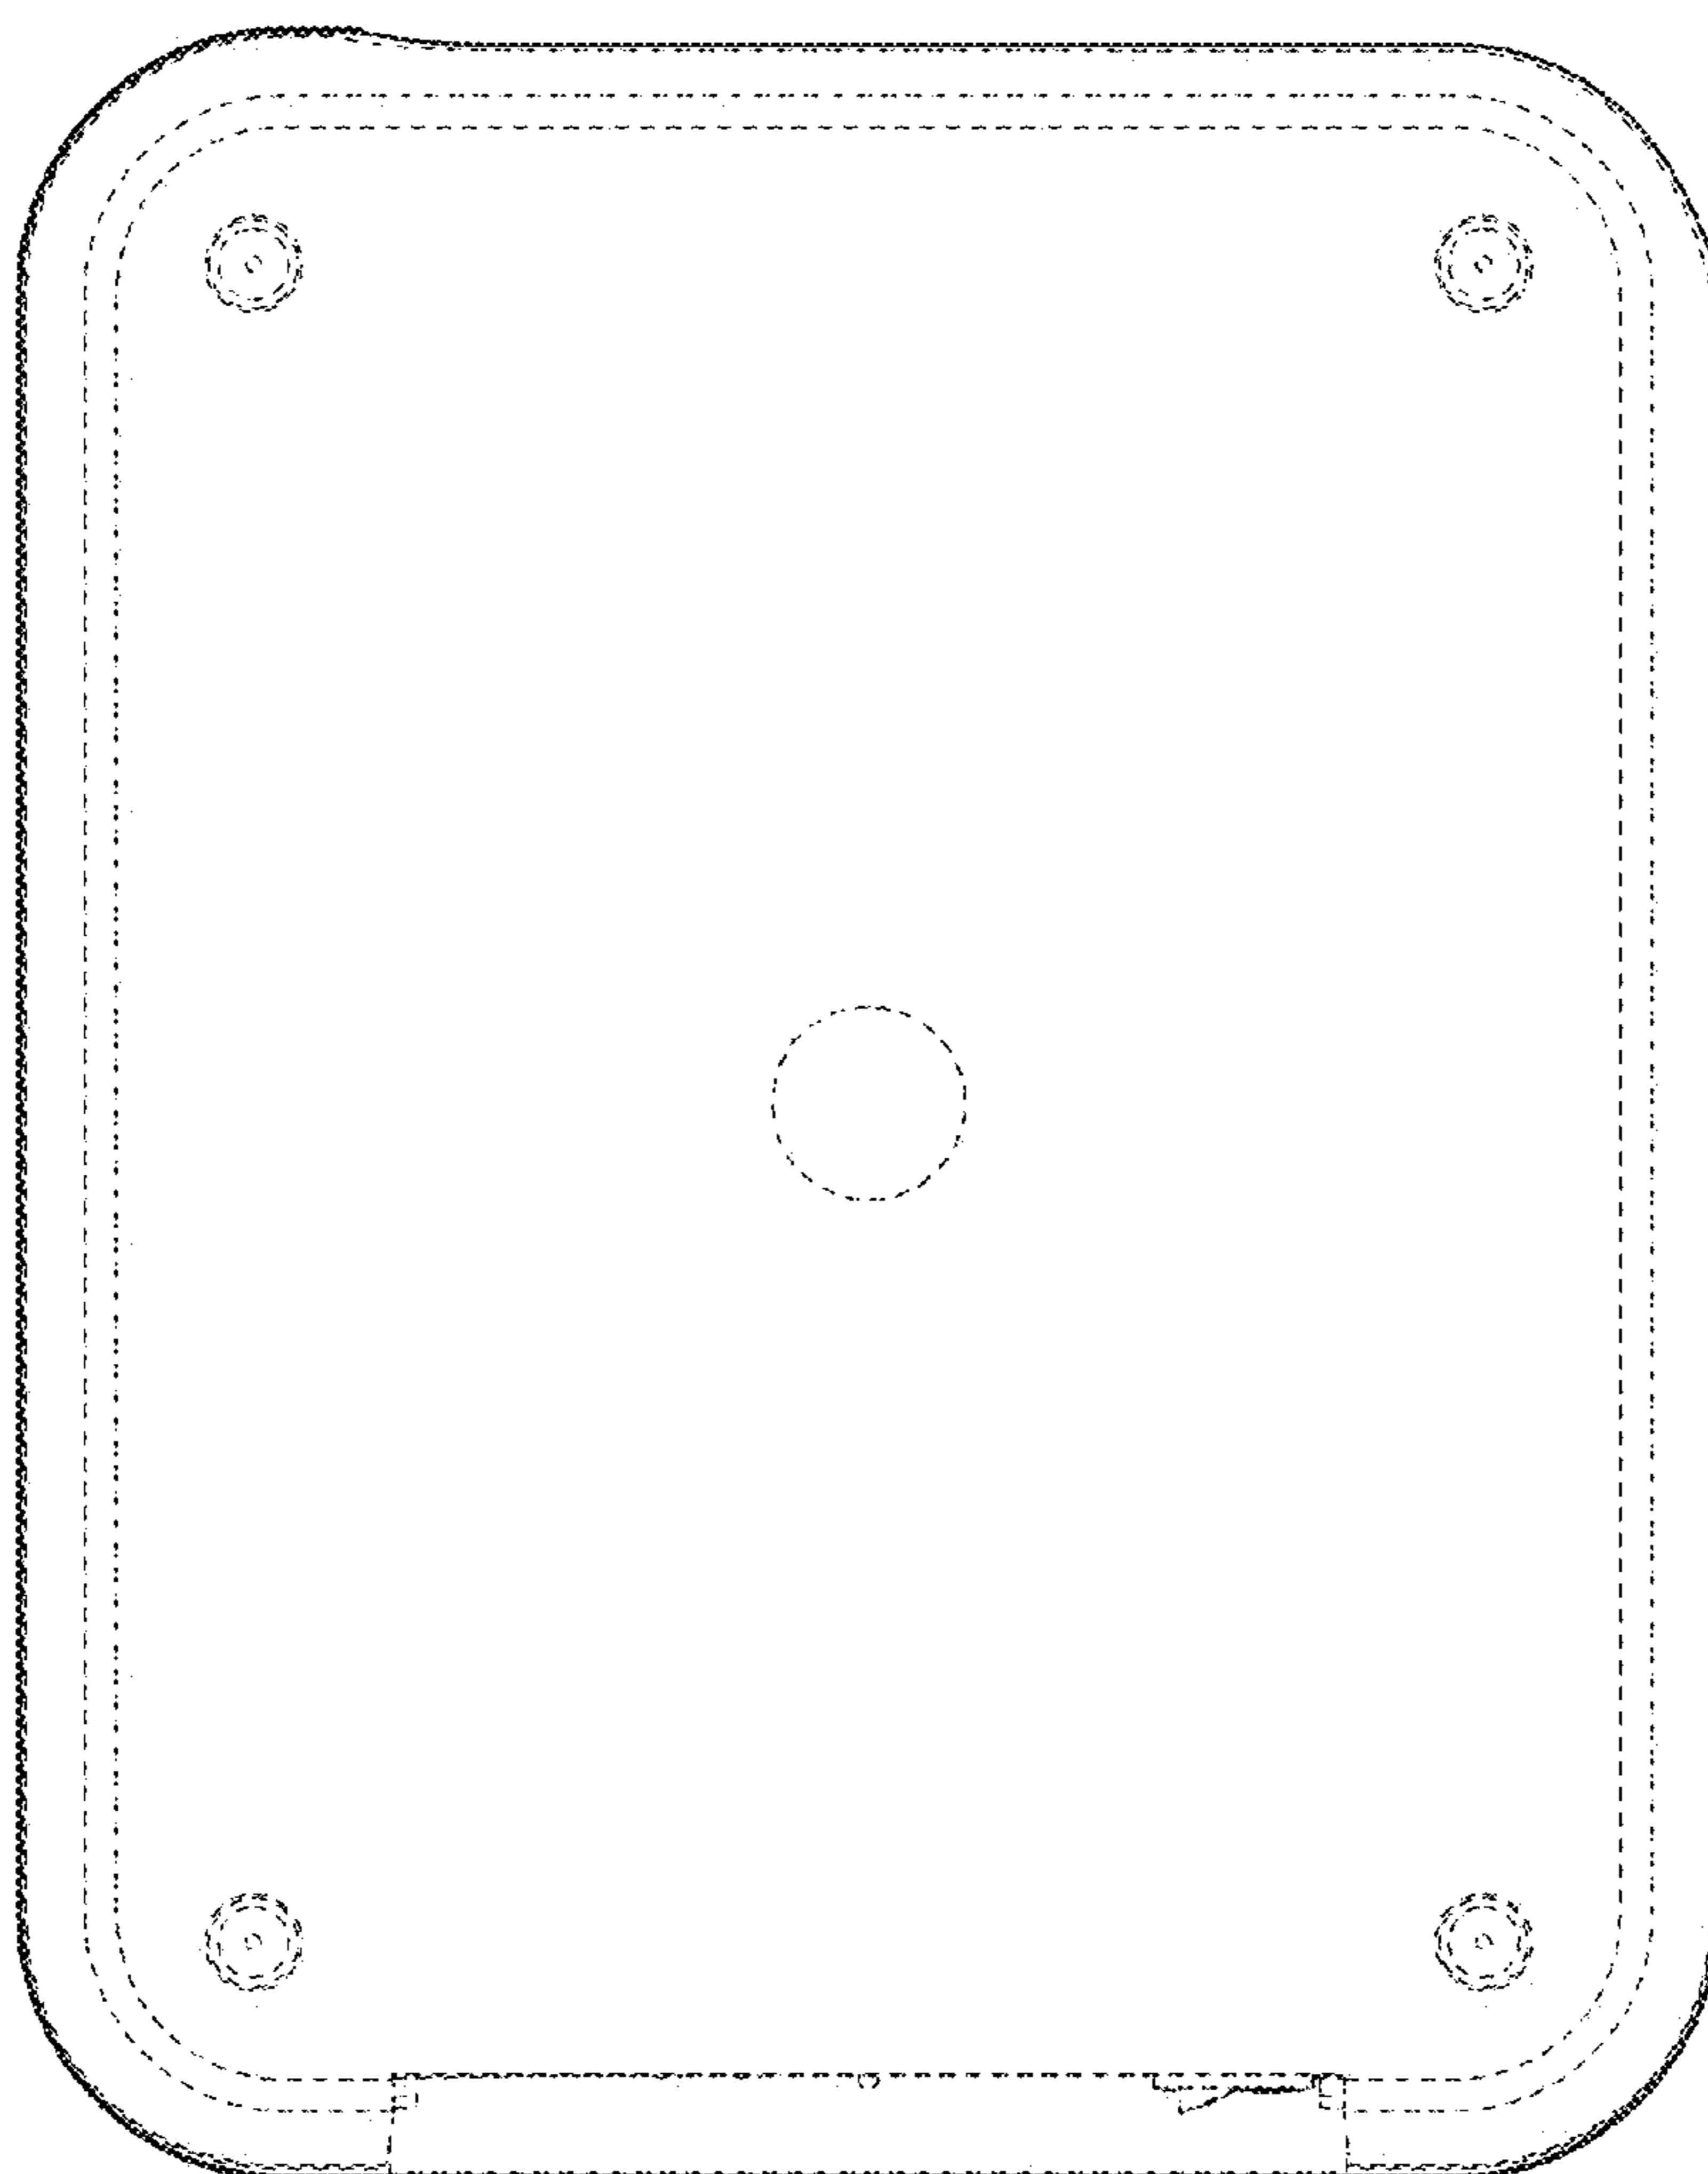


FIG. 7

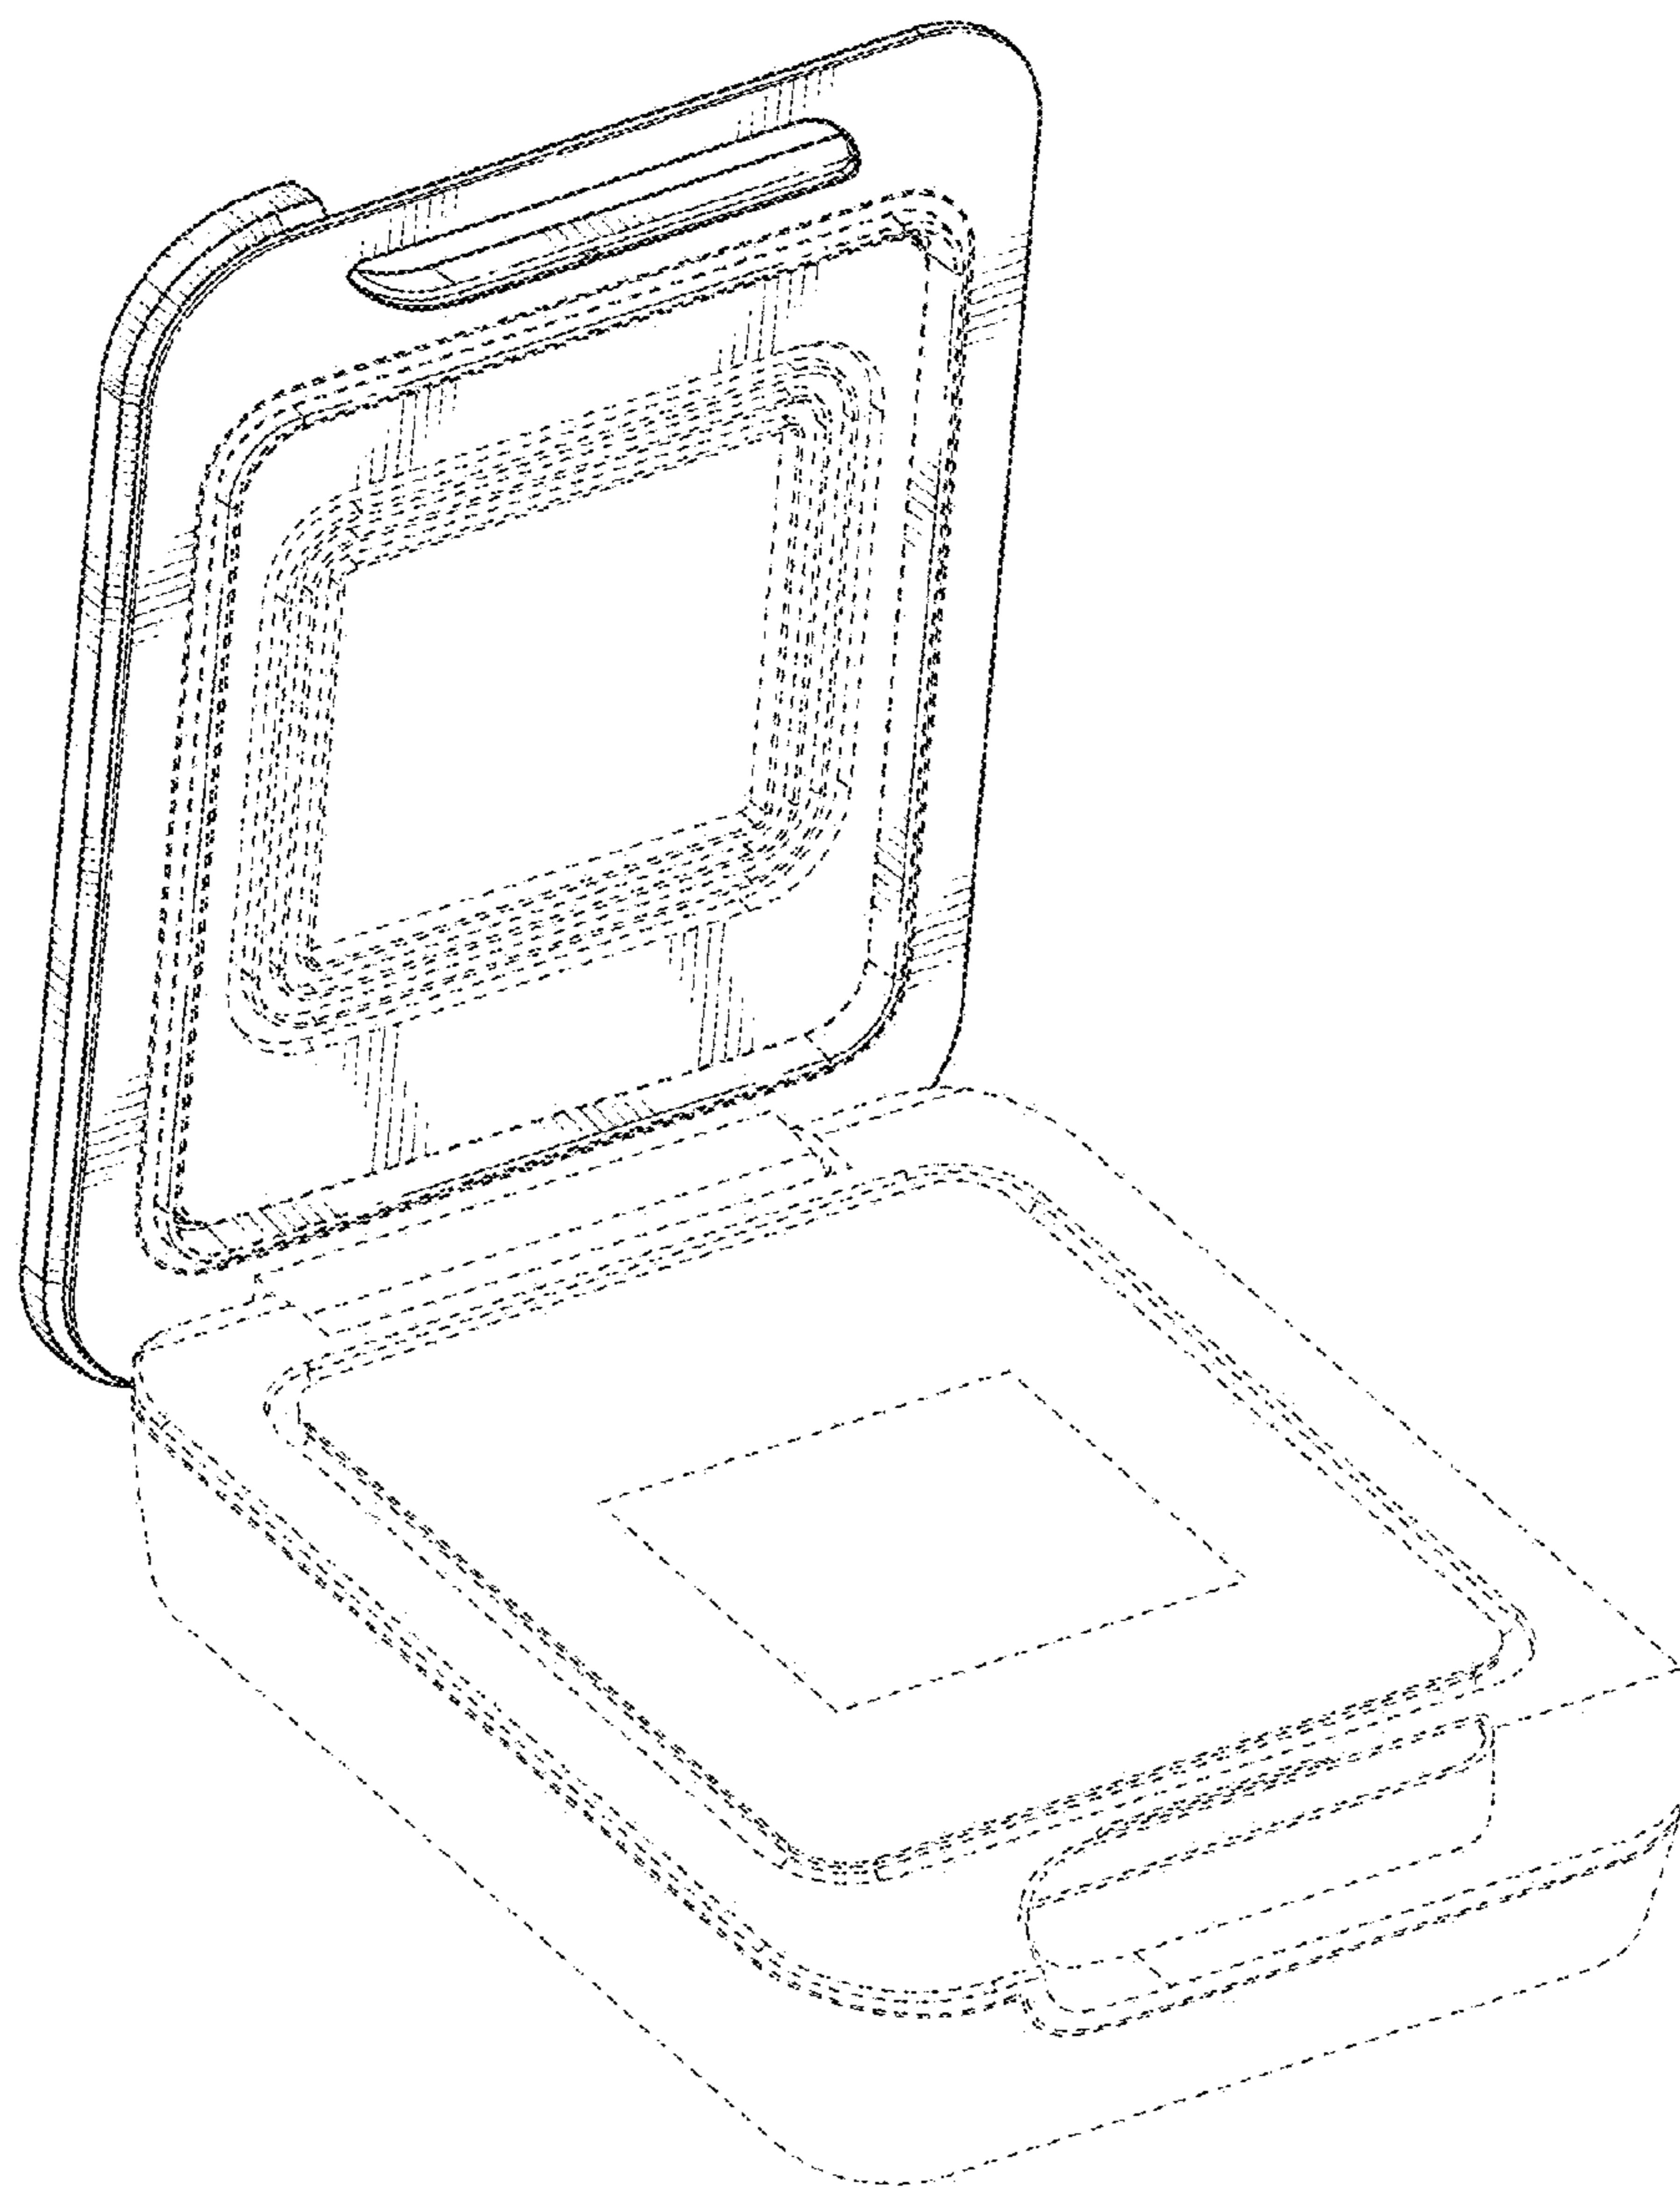


FIG. 8