



US00D722703S

(12) **United States Design Patent**  
**Fuller et al.**

(10) **Patent No.:** **US D722,703 S**  
(45) **Date of Patent:** **\*\* Feb. 17, 2015**

(54) **SALIVA TEST DEVICE**

(71) Applicants: **Kevin S. Fuller**, Lake Elmo, MN (US);  
**Wayde J. Altendorf**, Hickson, ND (US)

(72) Inventors: **Kevin S. Fuller**, Lake Elmo, MN (US);  
**Wayde J. Altendorf**, Hickson, ND (US)

(73) Assignee: **Premier Biotech, Inc.**, Excelsior, MN  
(US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/437,140**

(22) Filed: **Nov. 13, 2012**

(51) **LOC (10) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/216; D24/223**

(58) **Field of Classification Search**  
USPC ..... D24/169, 186, 216, 223–226, 231, 232,  
D24/121; D10/81; 436/165, 169; 422/68.1,  
422/82.1, 400, 401, 402, 403, 565, 64, 65,  
422/67, 102, 104, 547, 549–559;  
435/305.1, 307.1, 288.1–288.4  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D494,279 S \* 8/2004 Cogan et al. .... D24/224  
D507,351 S \* 7/2005 Birnboim ..... D24/224  
7,507,374 B2 \* 3/2009 Gould et al. .... 422/417

D594,131 S \* 6/2009 Nguyen ..... D24/216  
D608,455 S \* 1/2010 Pasmore et al. .... D24/224  
D639,446 S \* 6/2011 Smith ..... D24/224  
D641,890 S \* 7/2011 Nardo ..... D24/224

\* cited by examiner

*Primary Examiner* — Anhdao Doan  
(74) *Attorney, Agent, or Firm* — Christensen Fonder P.A.

(57) **CLAIM**

We claim the ornamental design for a saliva test device, as shown and described.

**DESCRIPTION**

FIG. 1 is a front perspective view of a saliva test device according to an embodiment of the invention. The view for the adjacent front corner being a mirror image thereto.

FIG. 2 is a front elevational view of the saliva test device depicted in FIG. 1.

FIG. 3 is a rear elevational view of the saliva test device depicted in FIG. 1.

FIG. 4 is a right side view of the saliva test device depicted in FIG. 1.


FIG. 5 is a left side view of the saliva test device depicted in FIG. 1.

FIG. 6 is a top plan view of the saliva test device depicted in FIG. 1; and,

FIG. 7 is a bottom plan view of the saliva test device depicted in FIG. 1.

The broken lines represent unclaimed portions of the saliva test device and form no part of the claimed design.

**1 Claim, 2 Drawing Sheets**

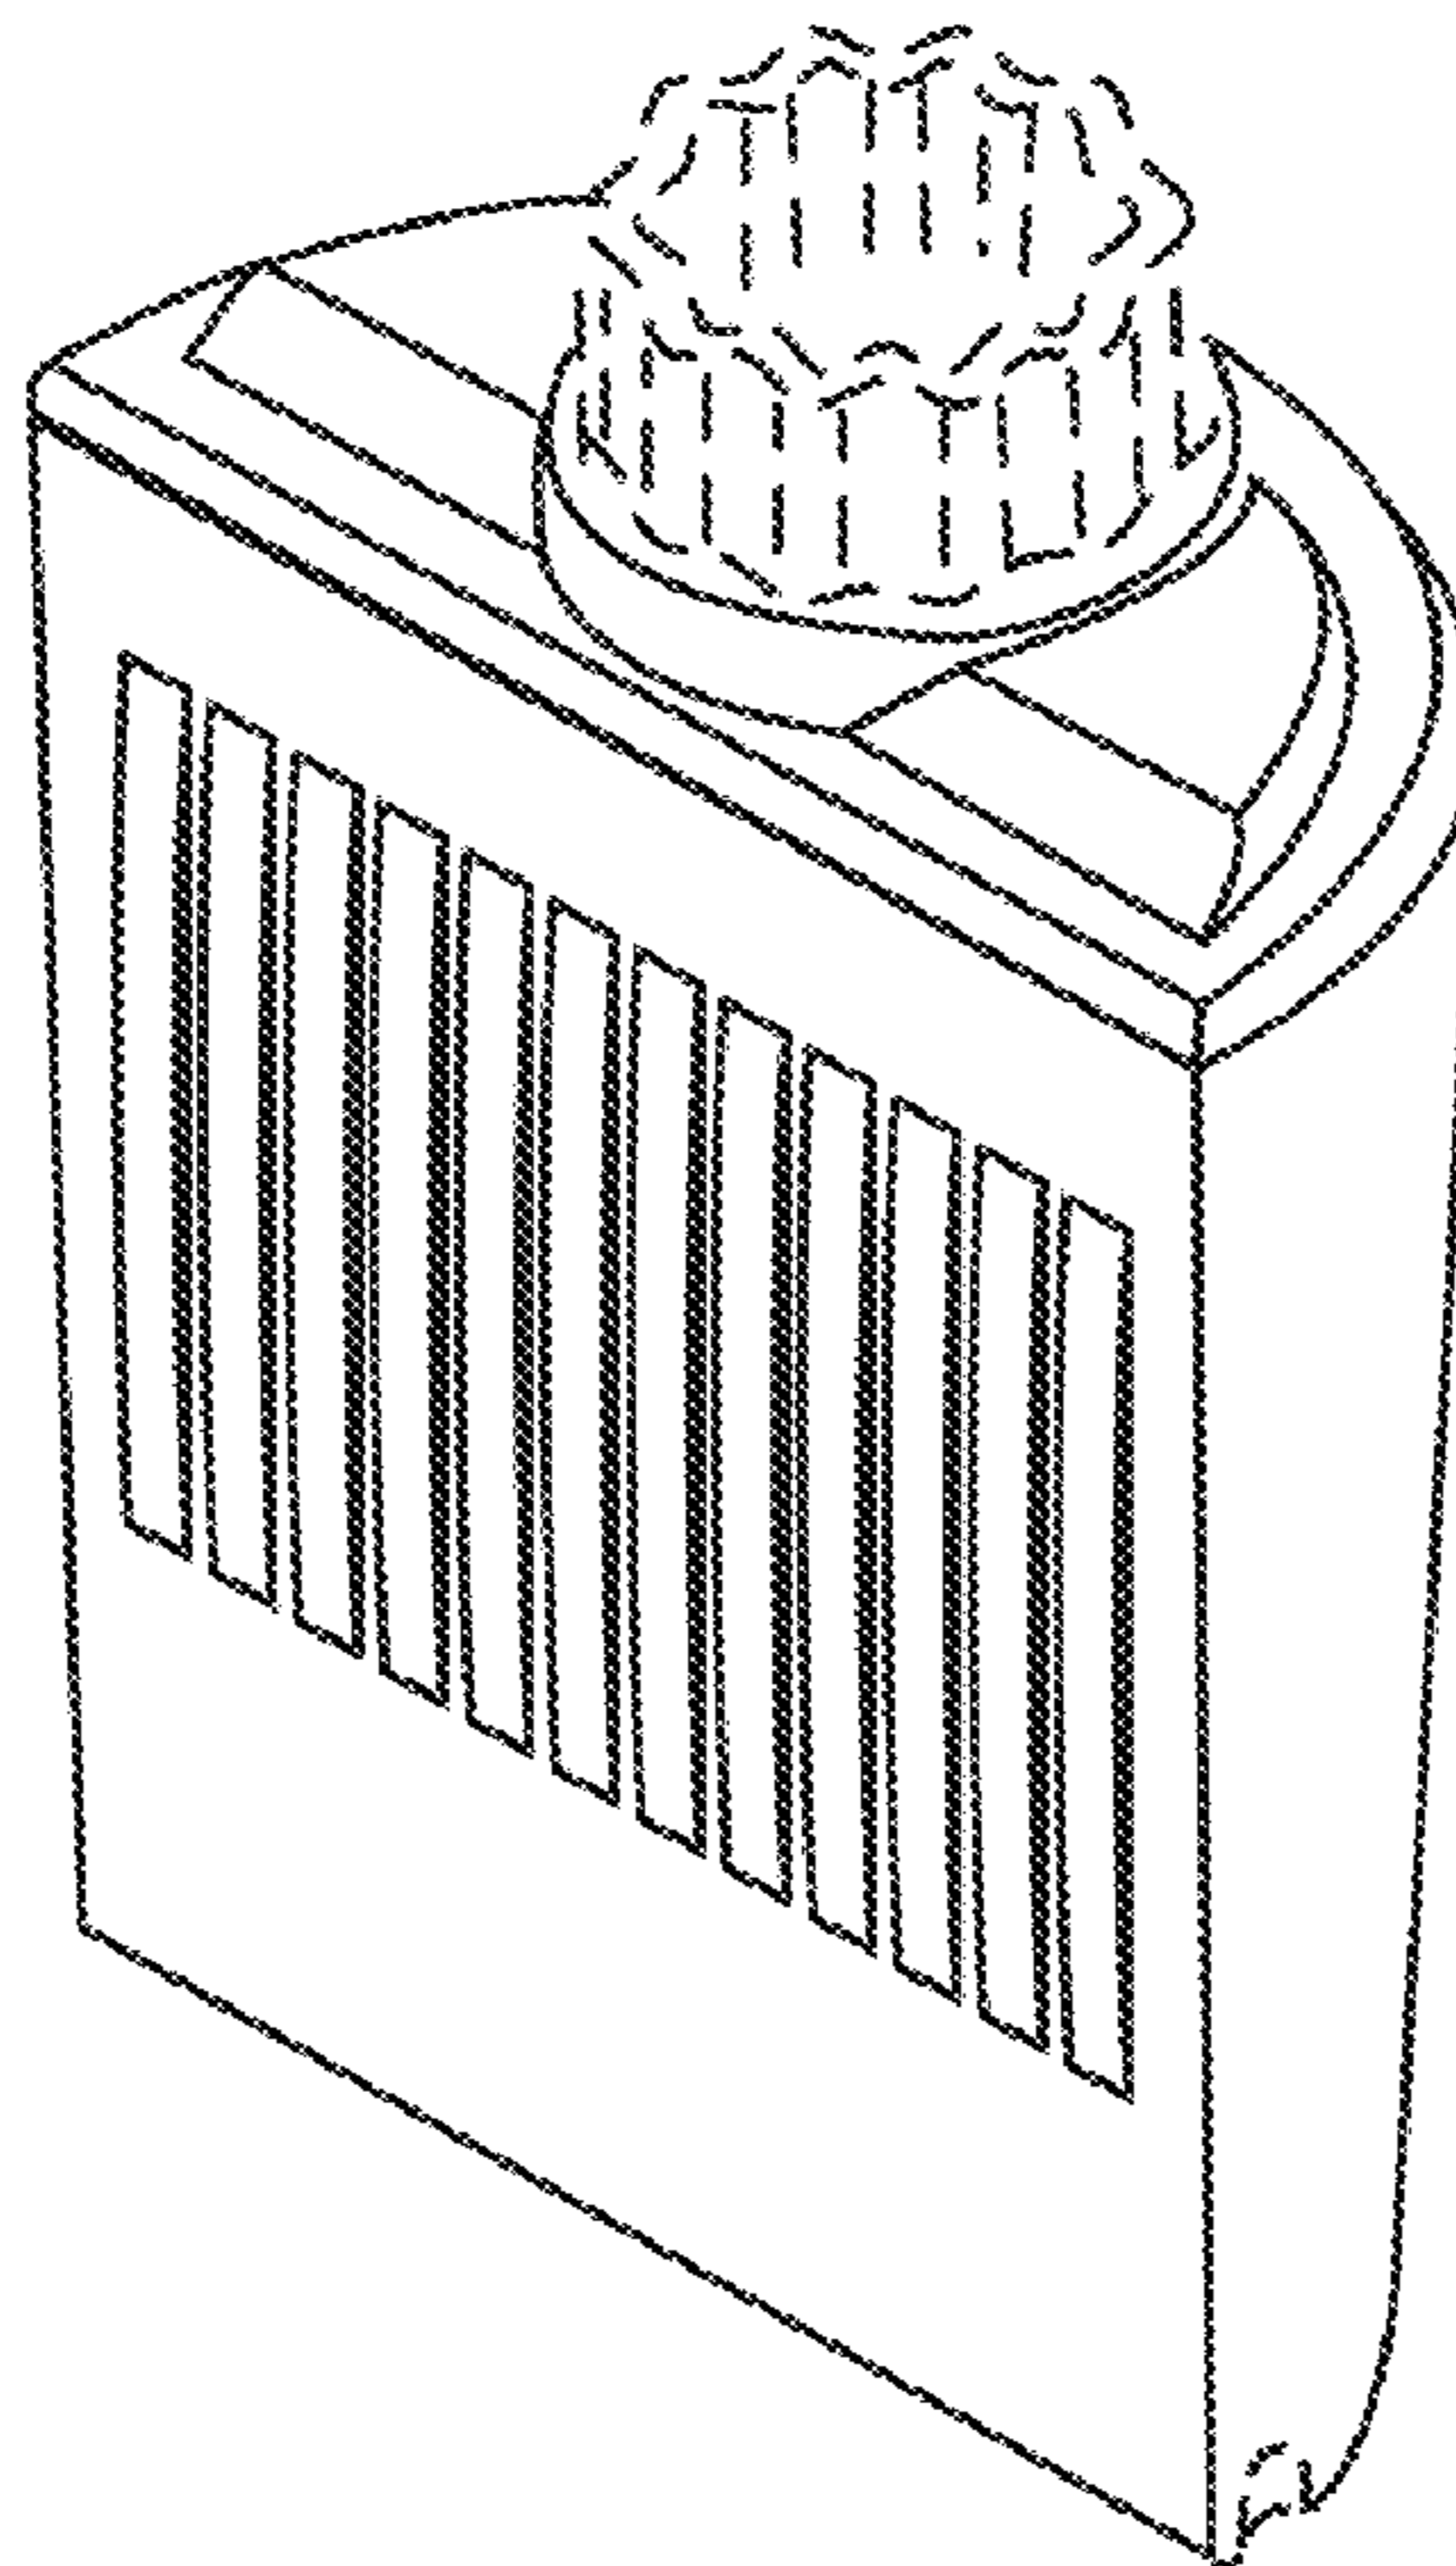

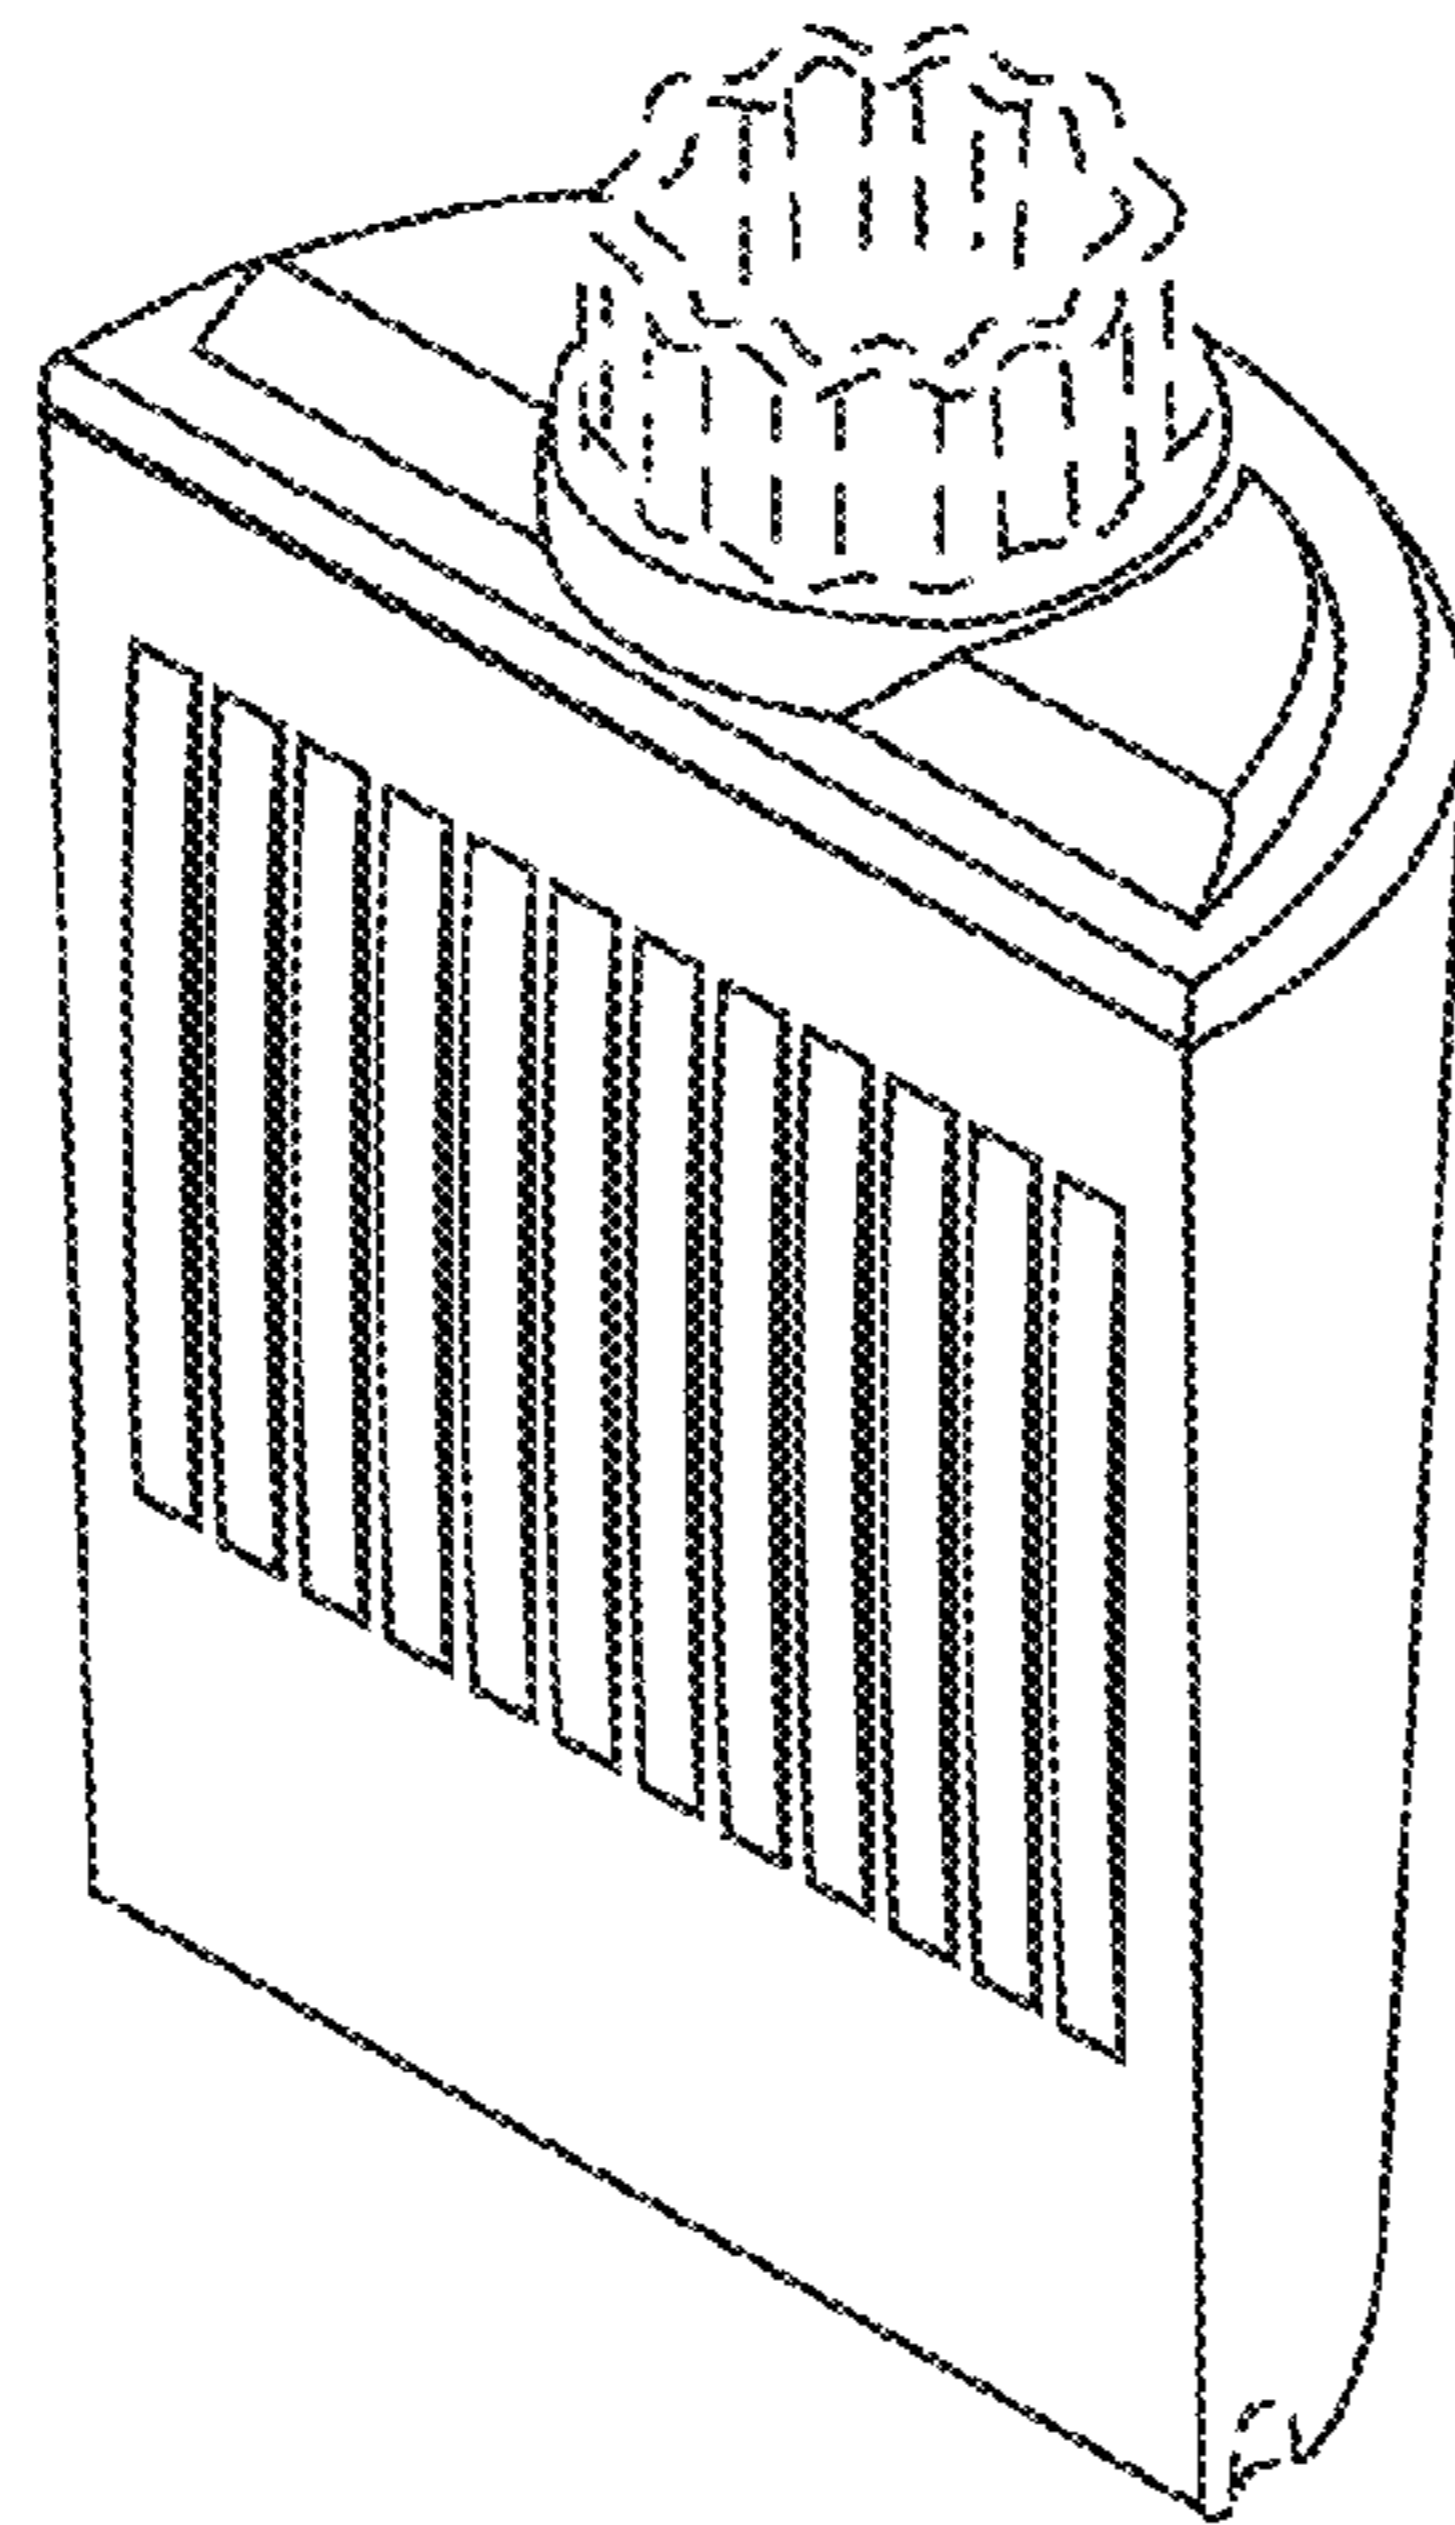


FIG. 1

FIG. 2

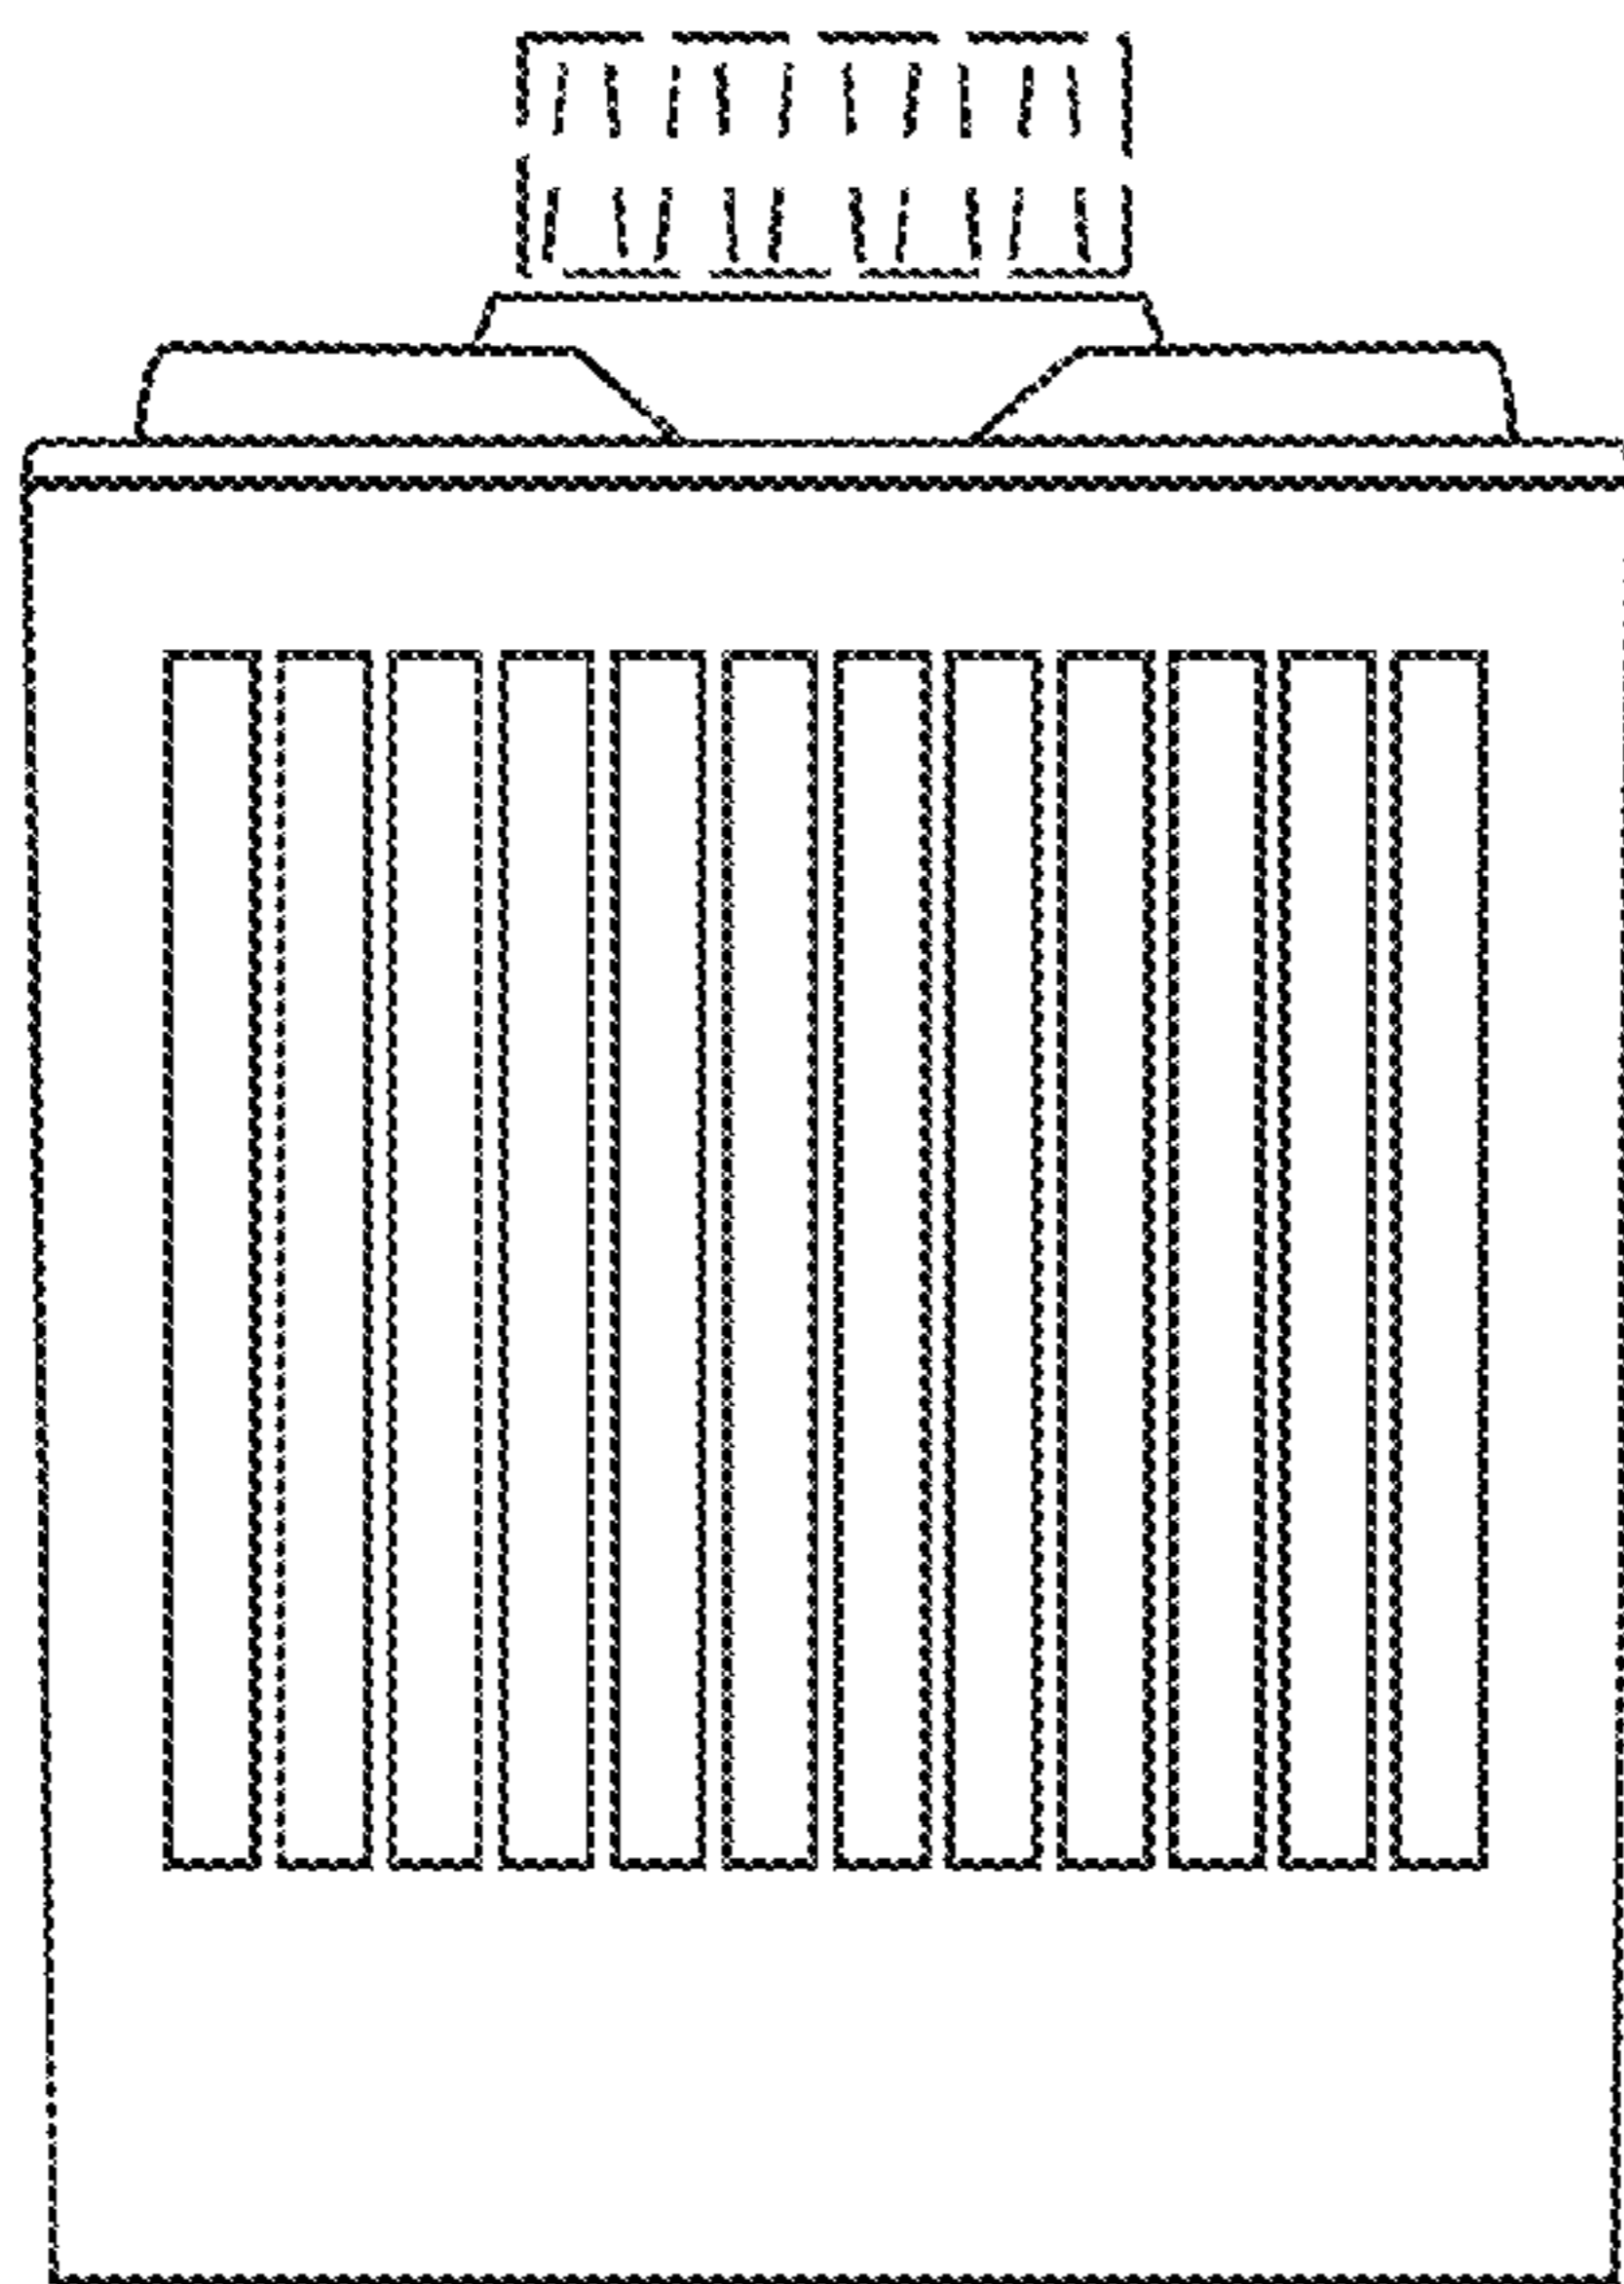
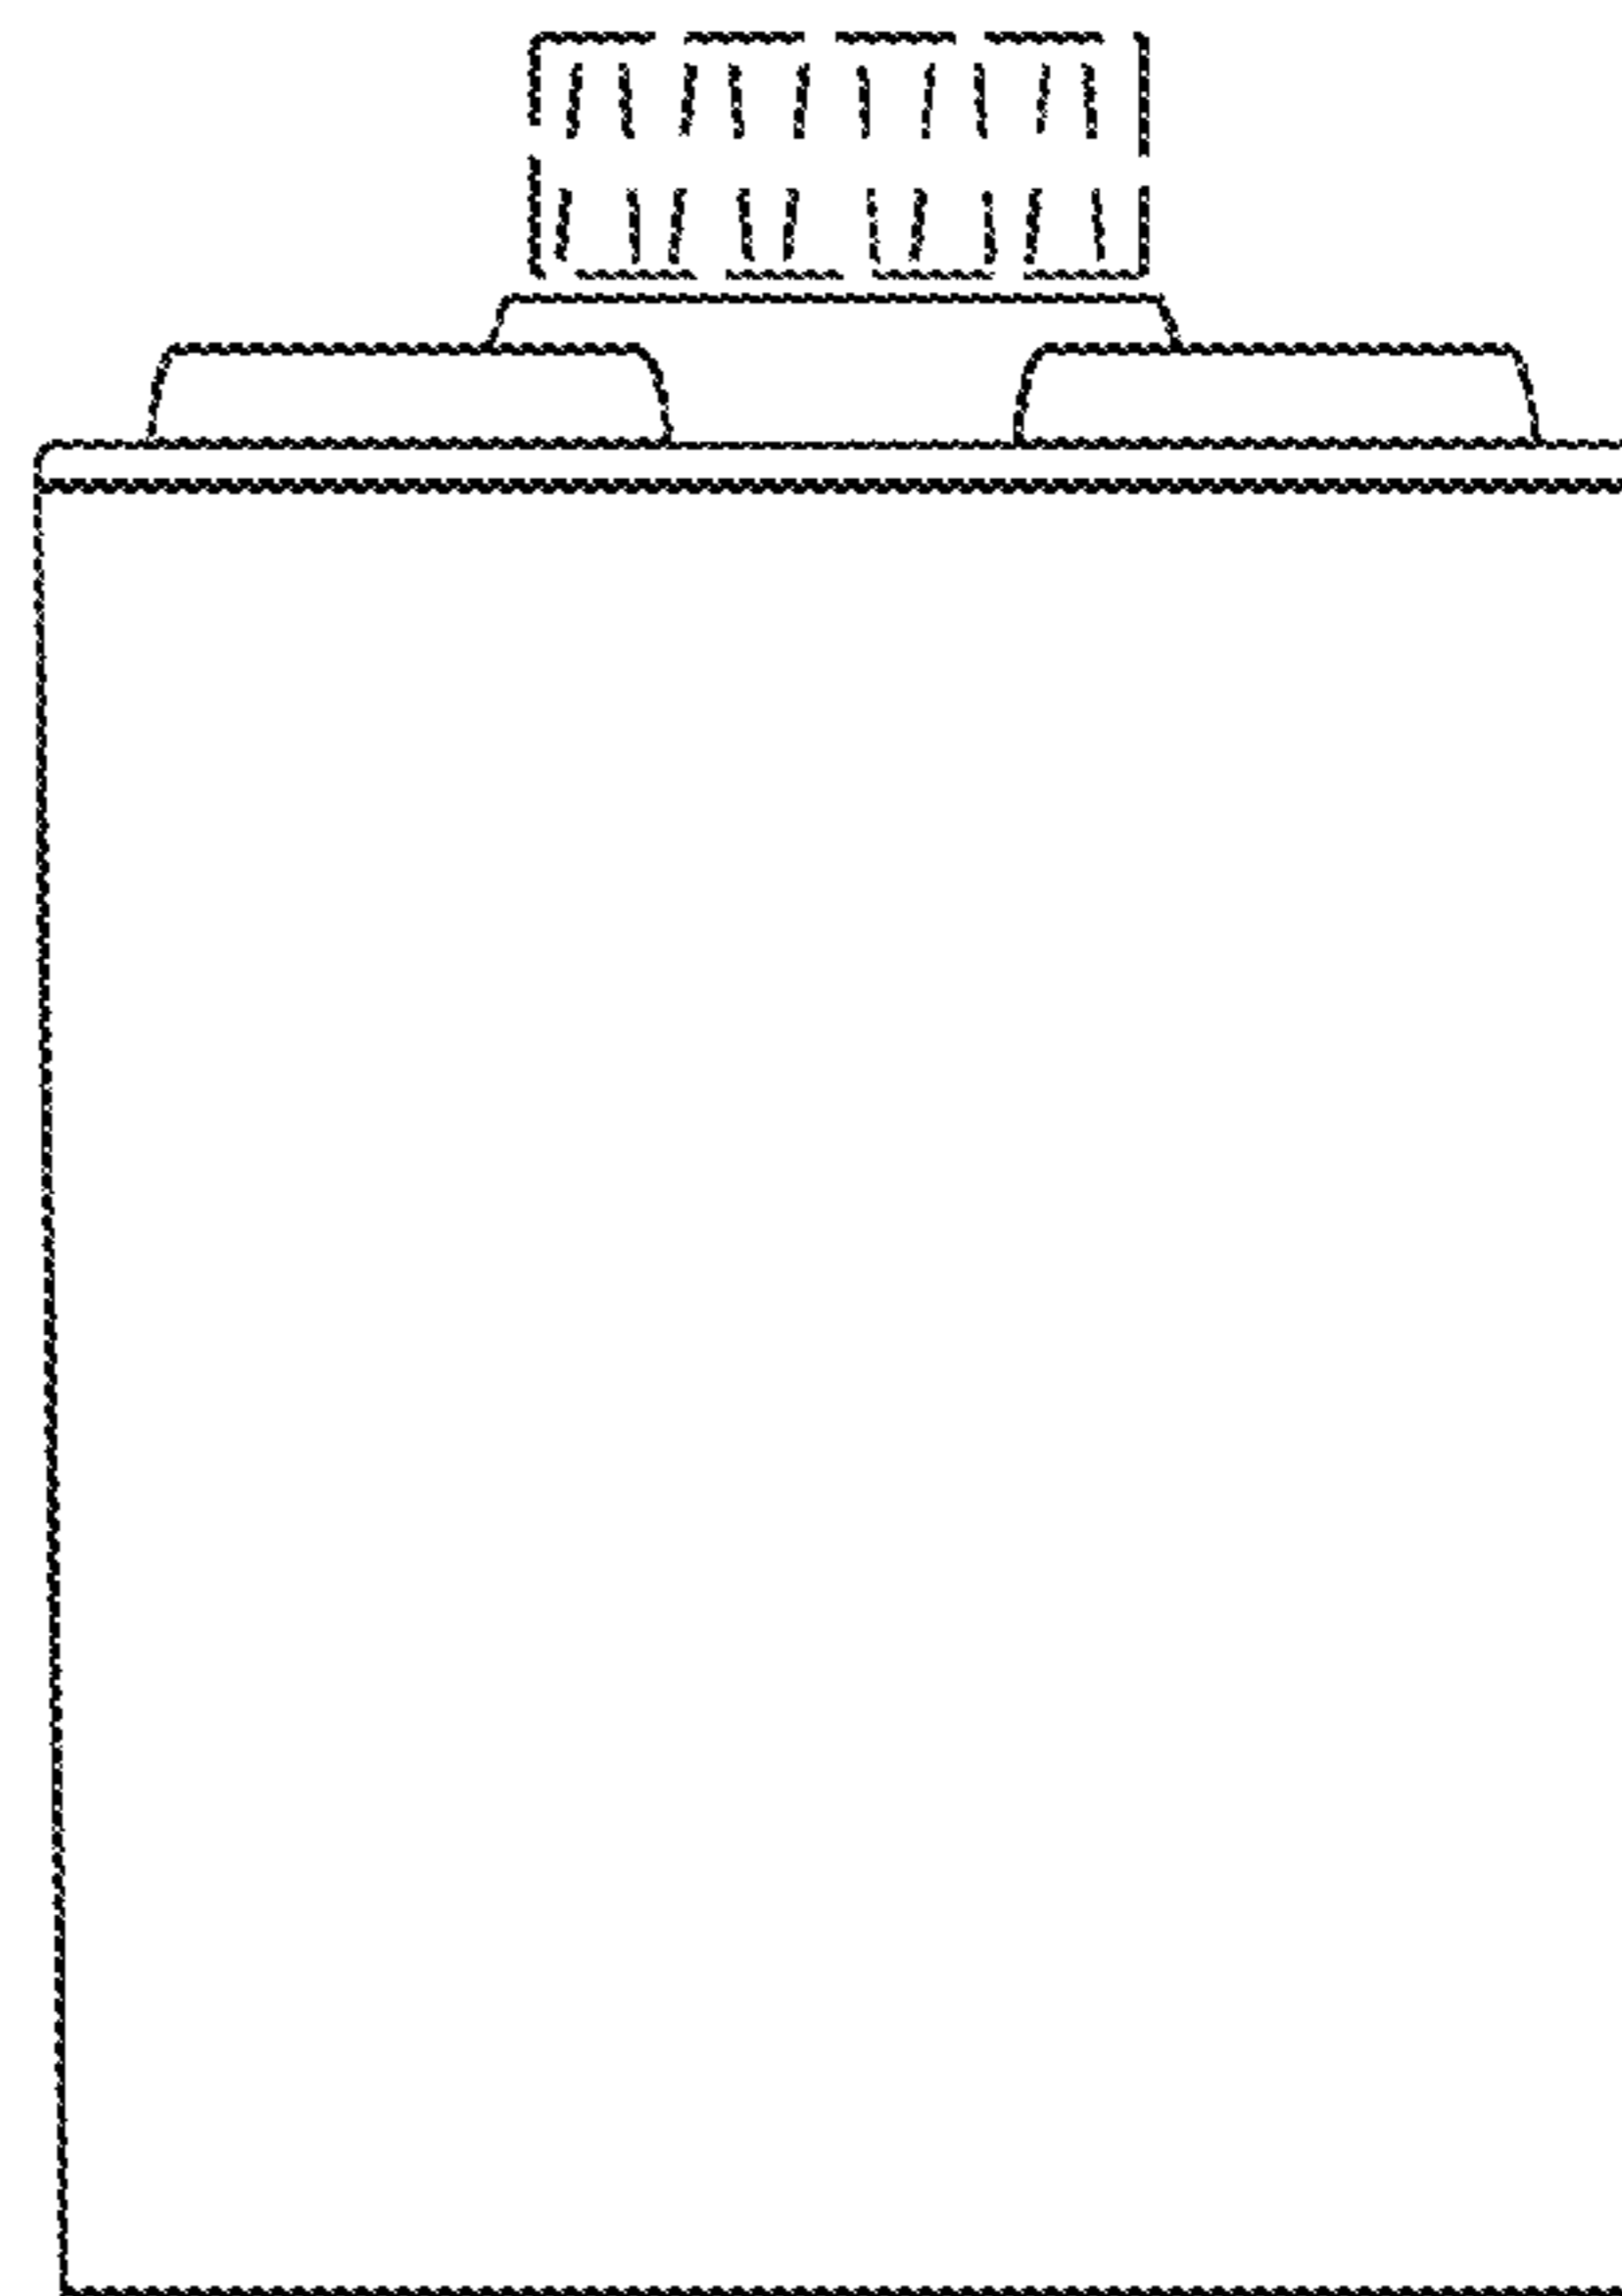


FIG. 3



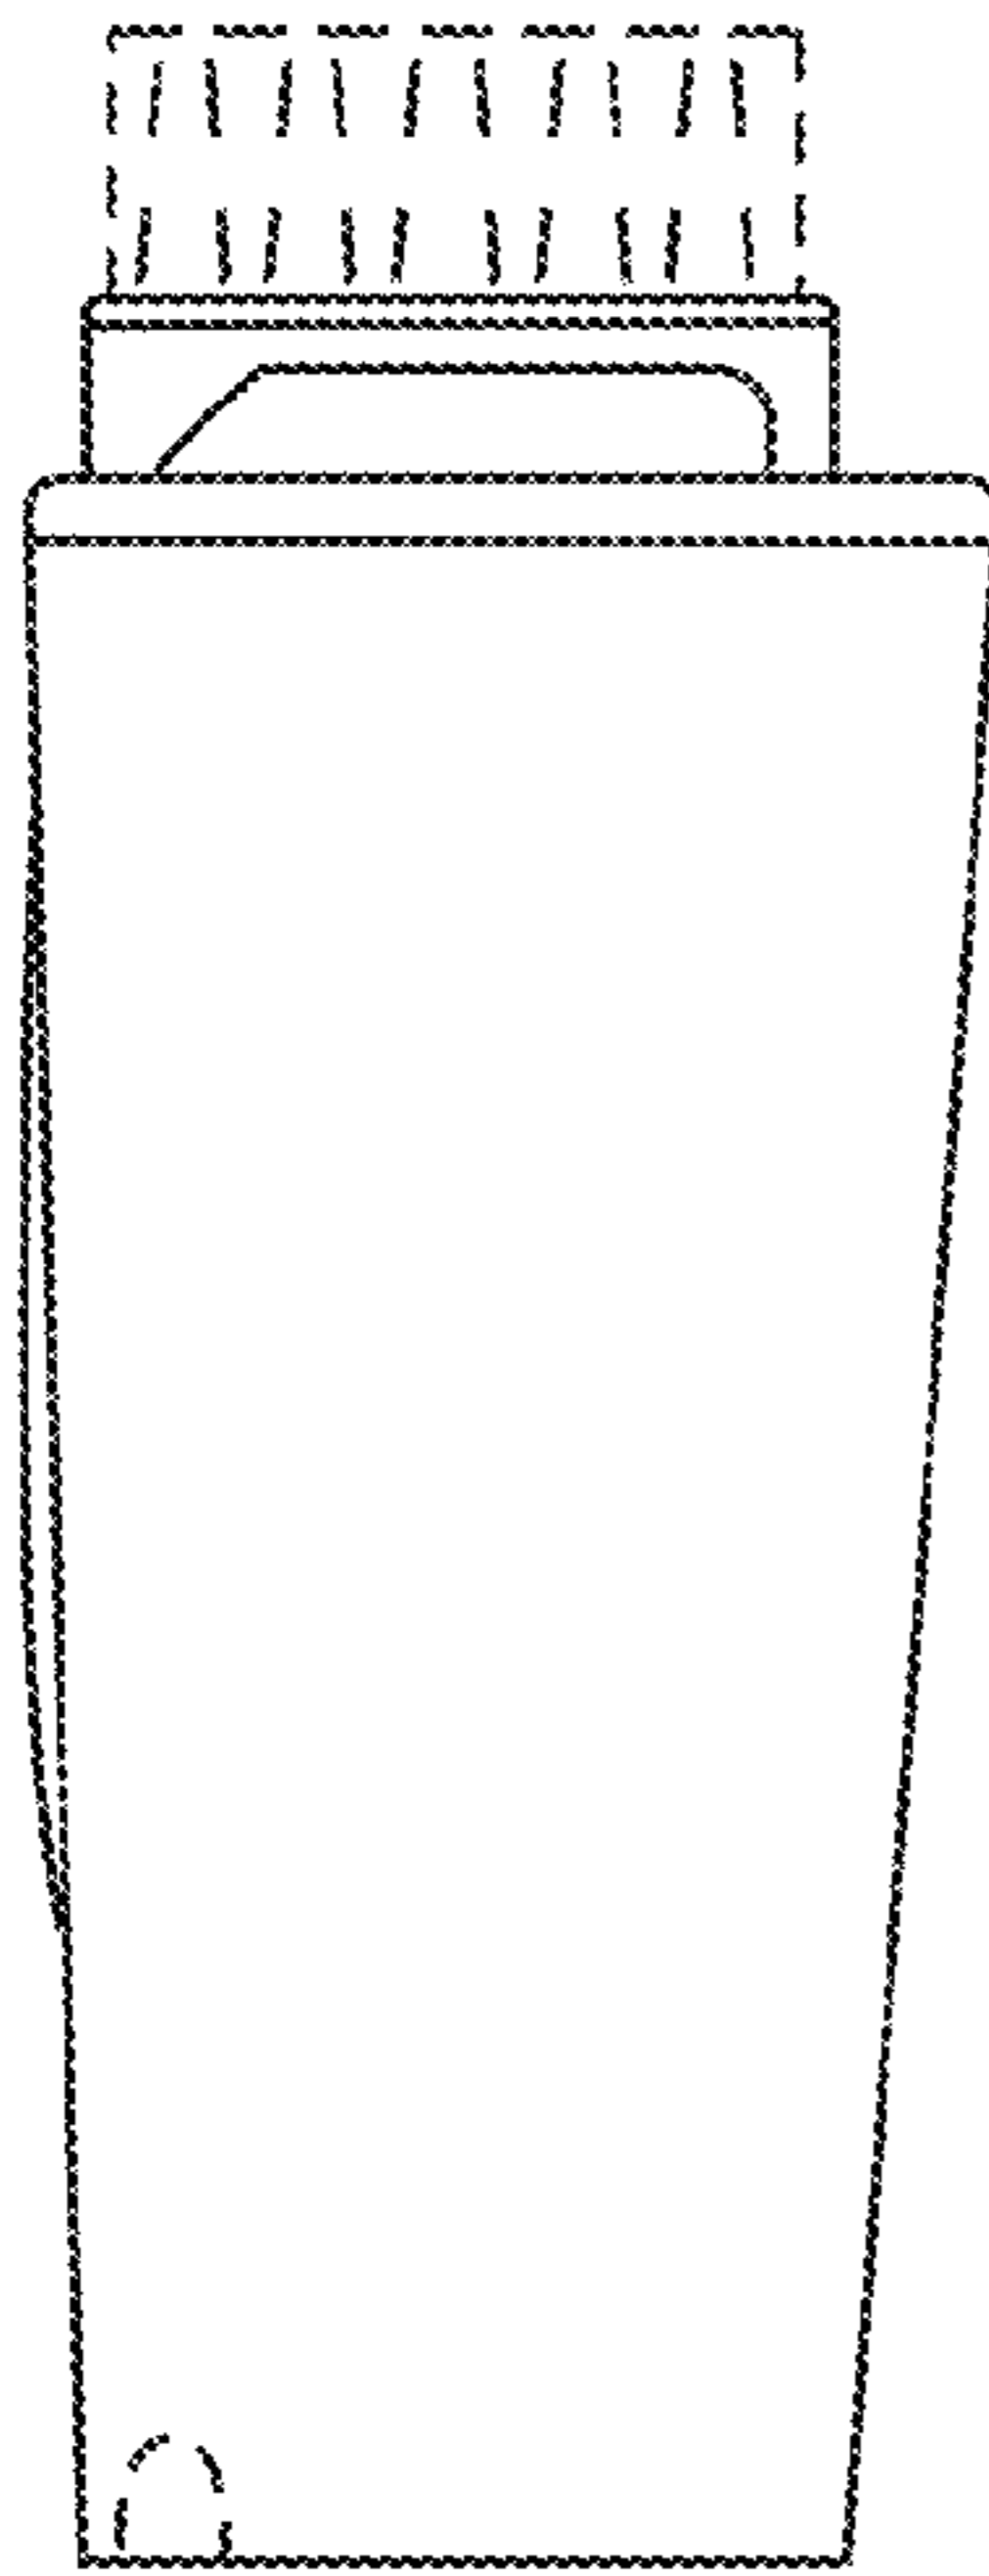


FIG. 4

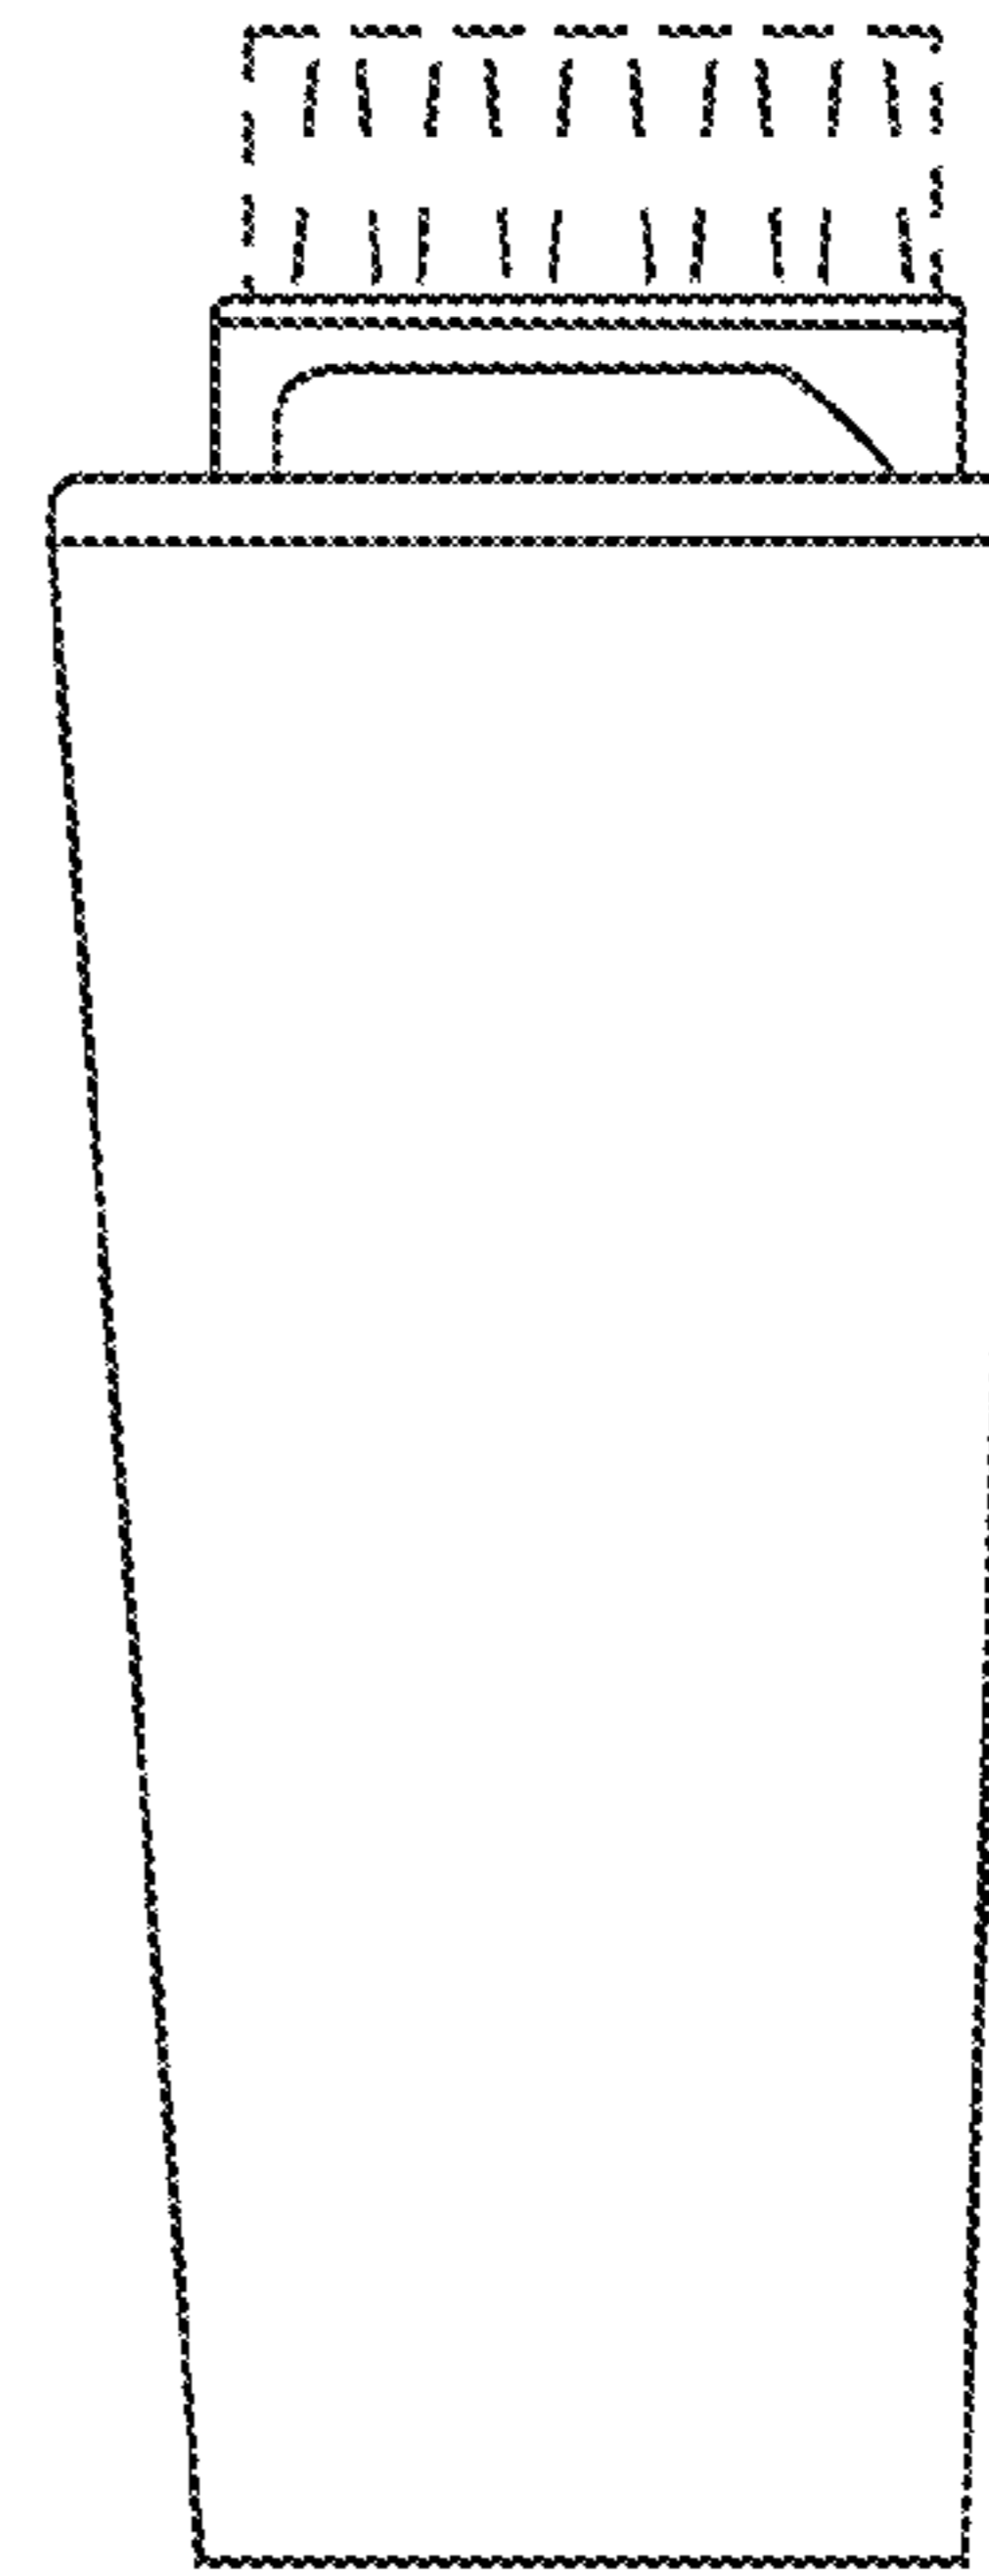


FIG. 5

FIG. 6

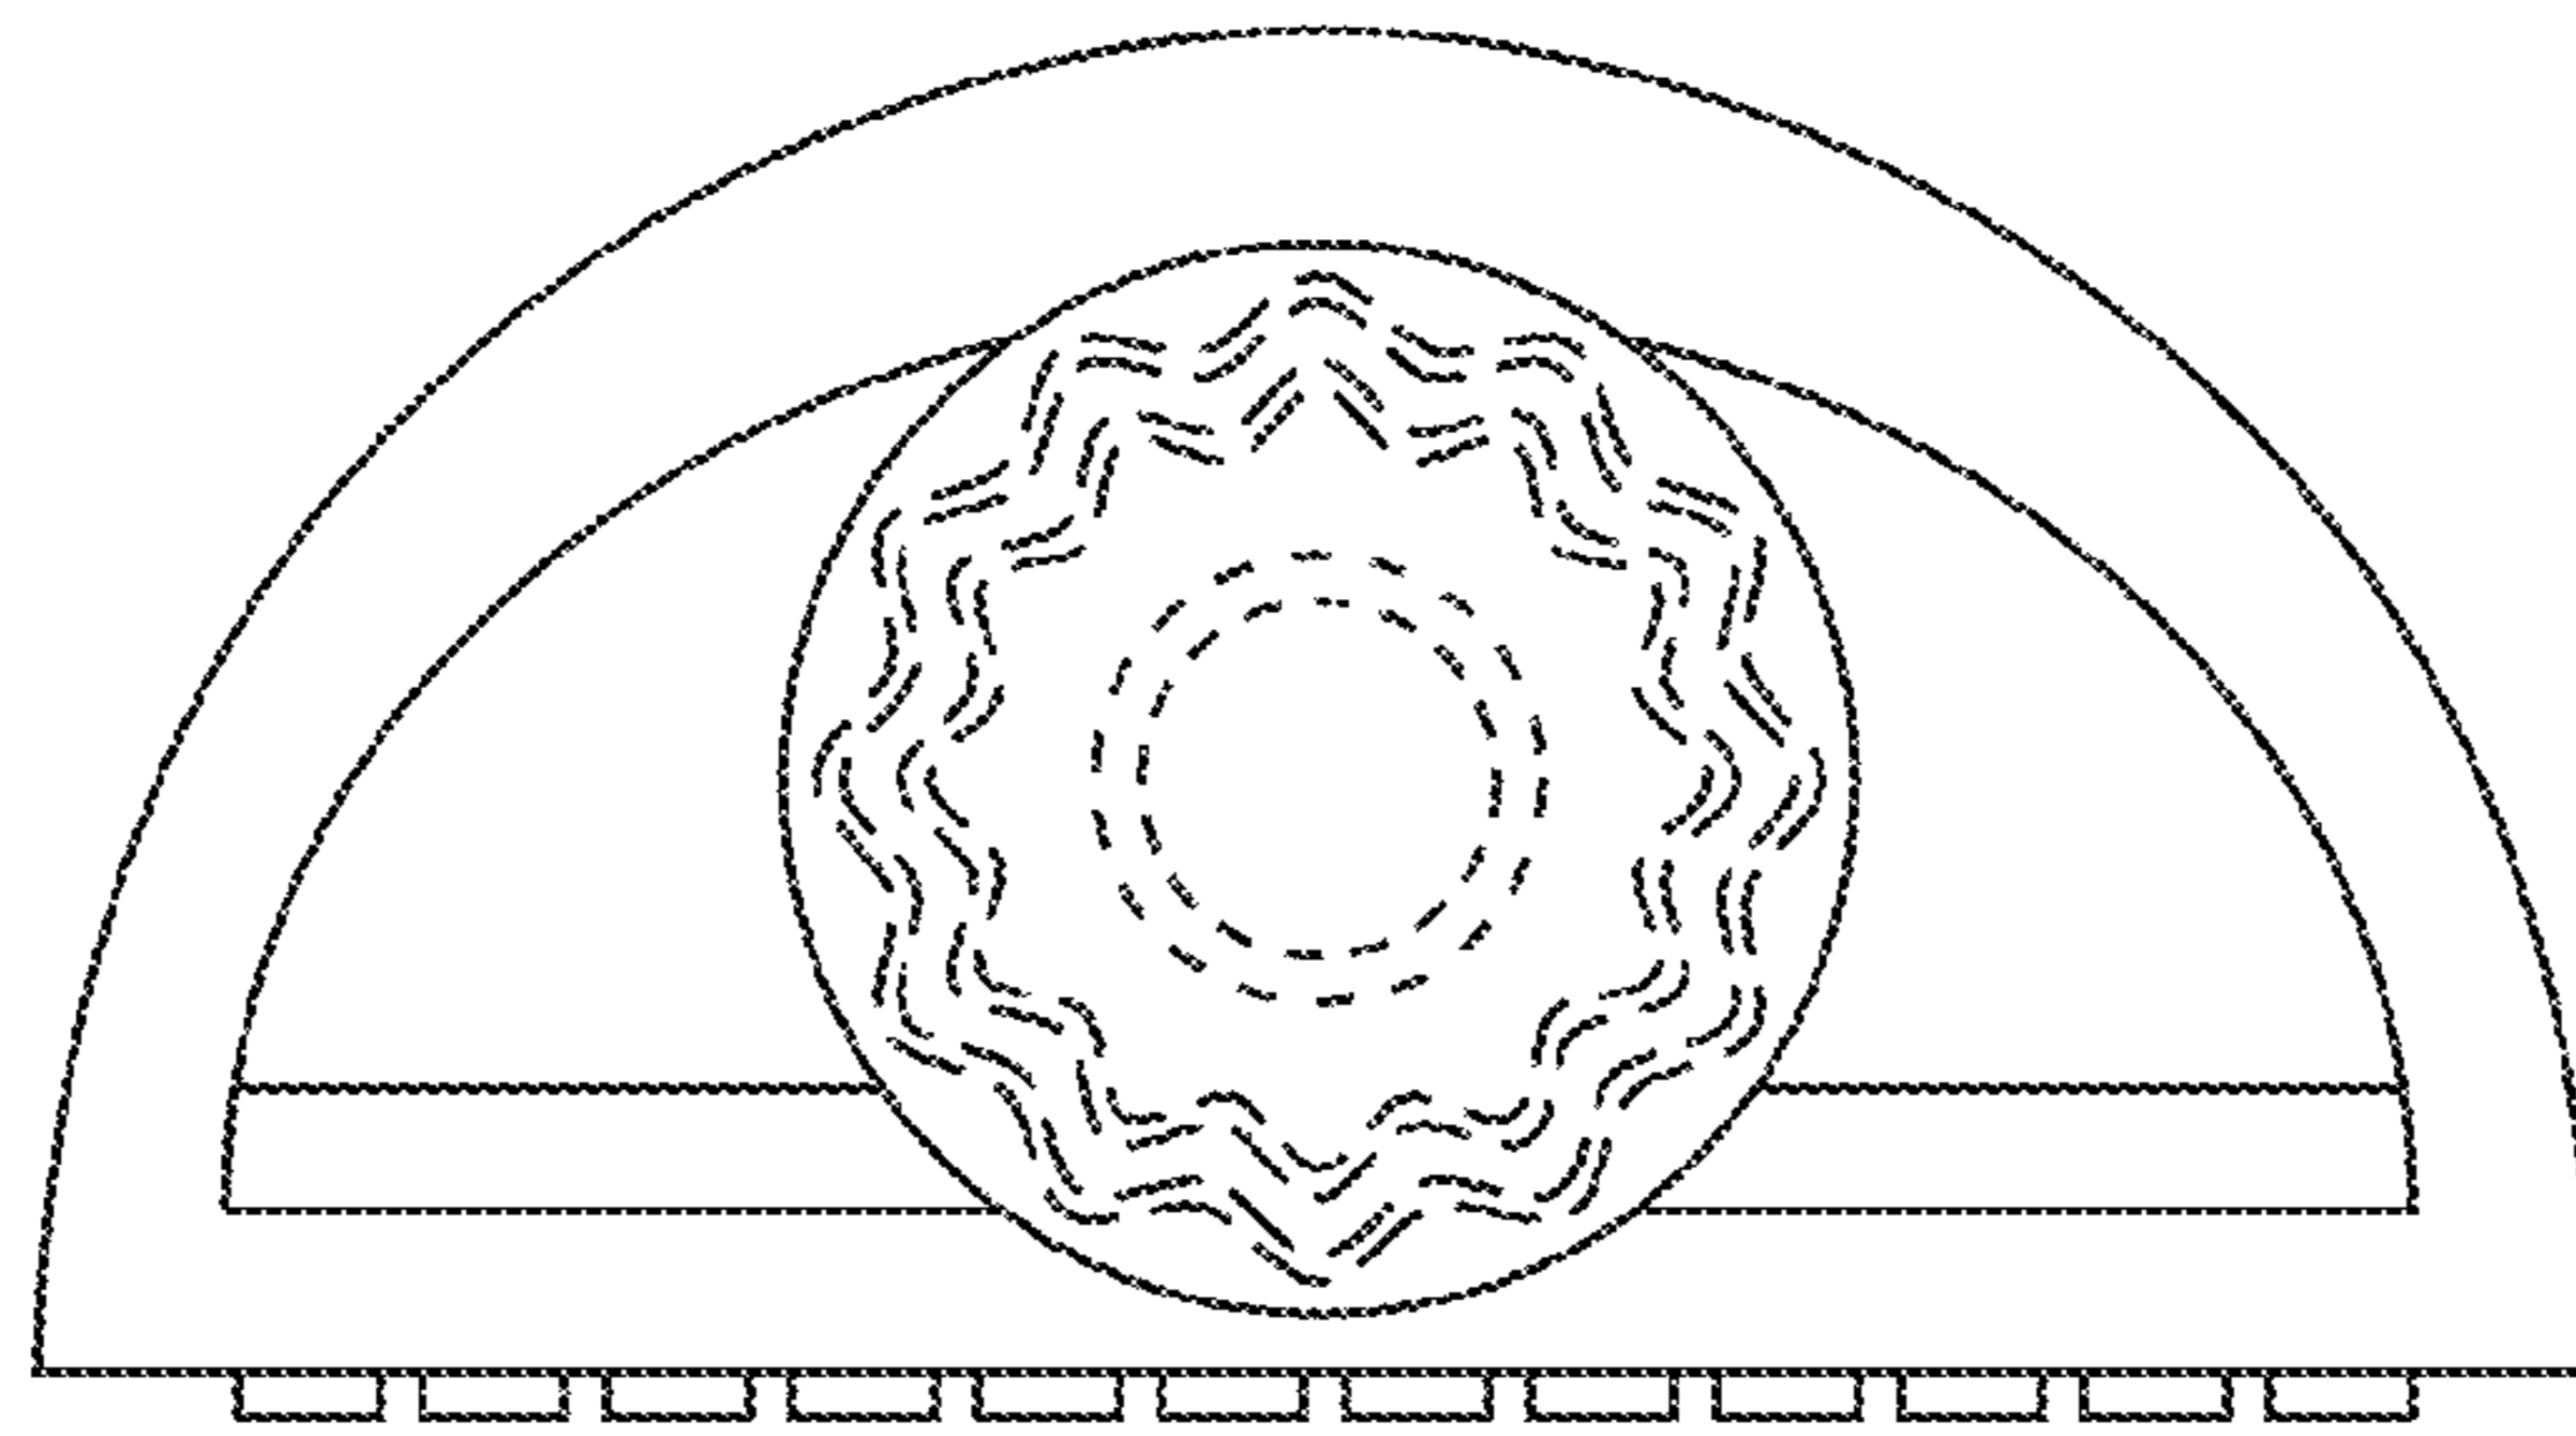


FIG. 7

