



US00D722703S

(12) **United States Design Patent**
Fuller et al.

(10) **Patent No.:** **US D722,703 S**
(45) **Date of Patent:** **** Feb. 17, 2015**

(54) **SALIVA TEST DEVICE**

(71) Applicants: **Kevin S. Fuller**, Lake Elmo, MN (US);
Wayde J. Altendorf, Hickson, ND (US)

(72) Inventors: **Kevin S. Fuller**, Lake Elmo, MN (US);
Wayde J. Altendorf, Hickson, ND (US)

(73) Assignee: **Premier Biotech, Inc.**, Excelsior, MN
(US)

(**) Term: **14 Years**

(21) Appl. No.: **29/437,140**

(22) Filed: **Nov. 13, 2012**

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/216; D24/223**

(58) **Field of Classification Search**
USPC D24/169, 186, 216, 223–226, 231, 232,
D24/121; D10/81; 436/165, 169; 422/68.1,
422/82.1, 400, 401, 402, 403, 565, 64, 65,
422/67, 102, 104, 547, 549–559;
435/305.1, 307.1, 288.1–288.4
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D494,279 S * 8/2004 Cogan et al. D24/224
D507,351 S * 7/2005 Birnboim D24/224
7,507,374 B2 * 3/2009 Gould et al. 422/417

D594,131 S * 6/2009 Nguyen D24/216
D608,455 S * 1/2010 Pasmore et al. D24/224
D639,446 S * 6/2011 Smith D24/224
D641,890 S * 7/2011 Nardo D24/224

* cited by examiner

Primary Examiner — Anhdao Doan
(74) *Attorney, Agent, or Firm* — Christensen Fonder P.A.

(57) **CLAIM**

We claim the ornamental design for a saliva test device, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of a saliva test device according to an embodiment of the invention. The view for the adjacent front corner being a mirror image thereto.

FIG. 2 is a front elevational view of the saliva test device depicted in FIG. 1.

FIG. 3 is a rear elevational view of the saliva test device depicted in FIG. 1.

FIG. 4 is a right side view of the saliva test device depicted in FIG. 1.


FIG. 5 is a left side view of the saliva test device depicted in FIG. 1.

FIG. 6 is a top plan view of the saliva test device depicted in FIG. 1; and,

FIG. 7 is a bottom plan view of the saliva test device depicted in FIG. 1.

The broken lines represent unclaimed portions of the saliva test device and form no part of the claimed design.

1 Claim, 2 Drawing Sheets

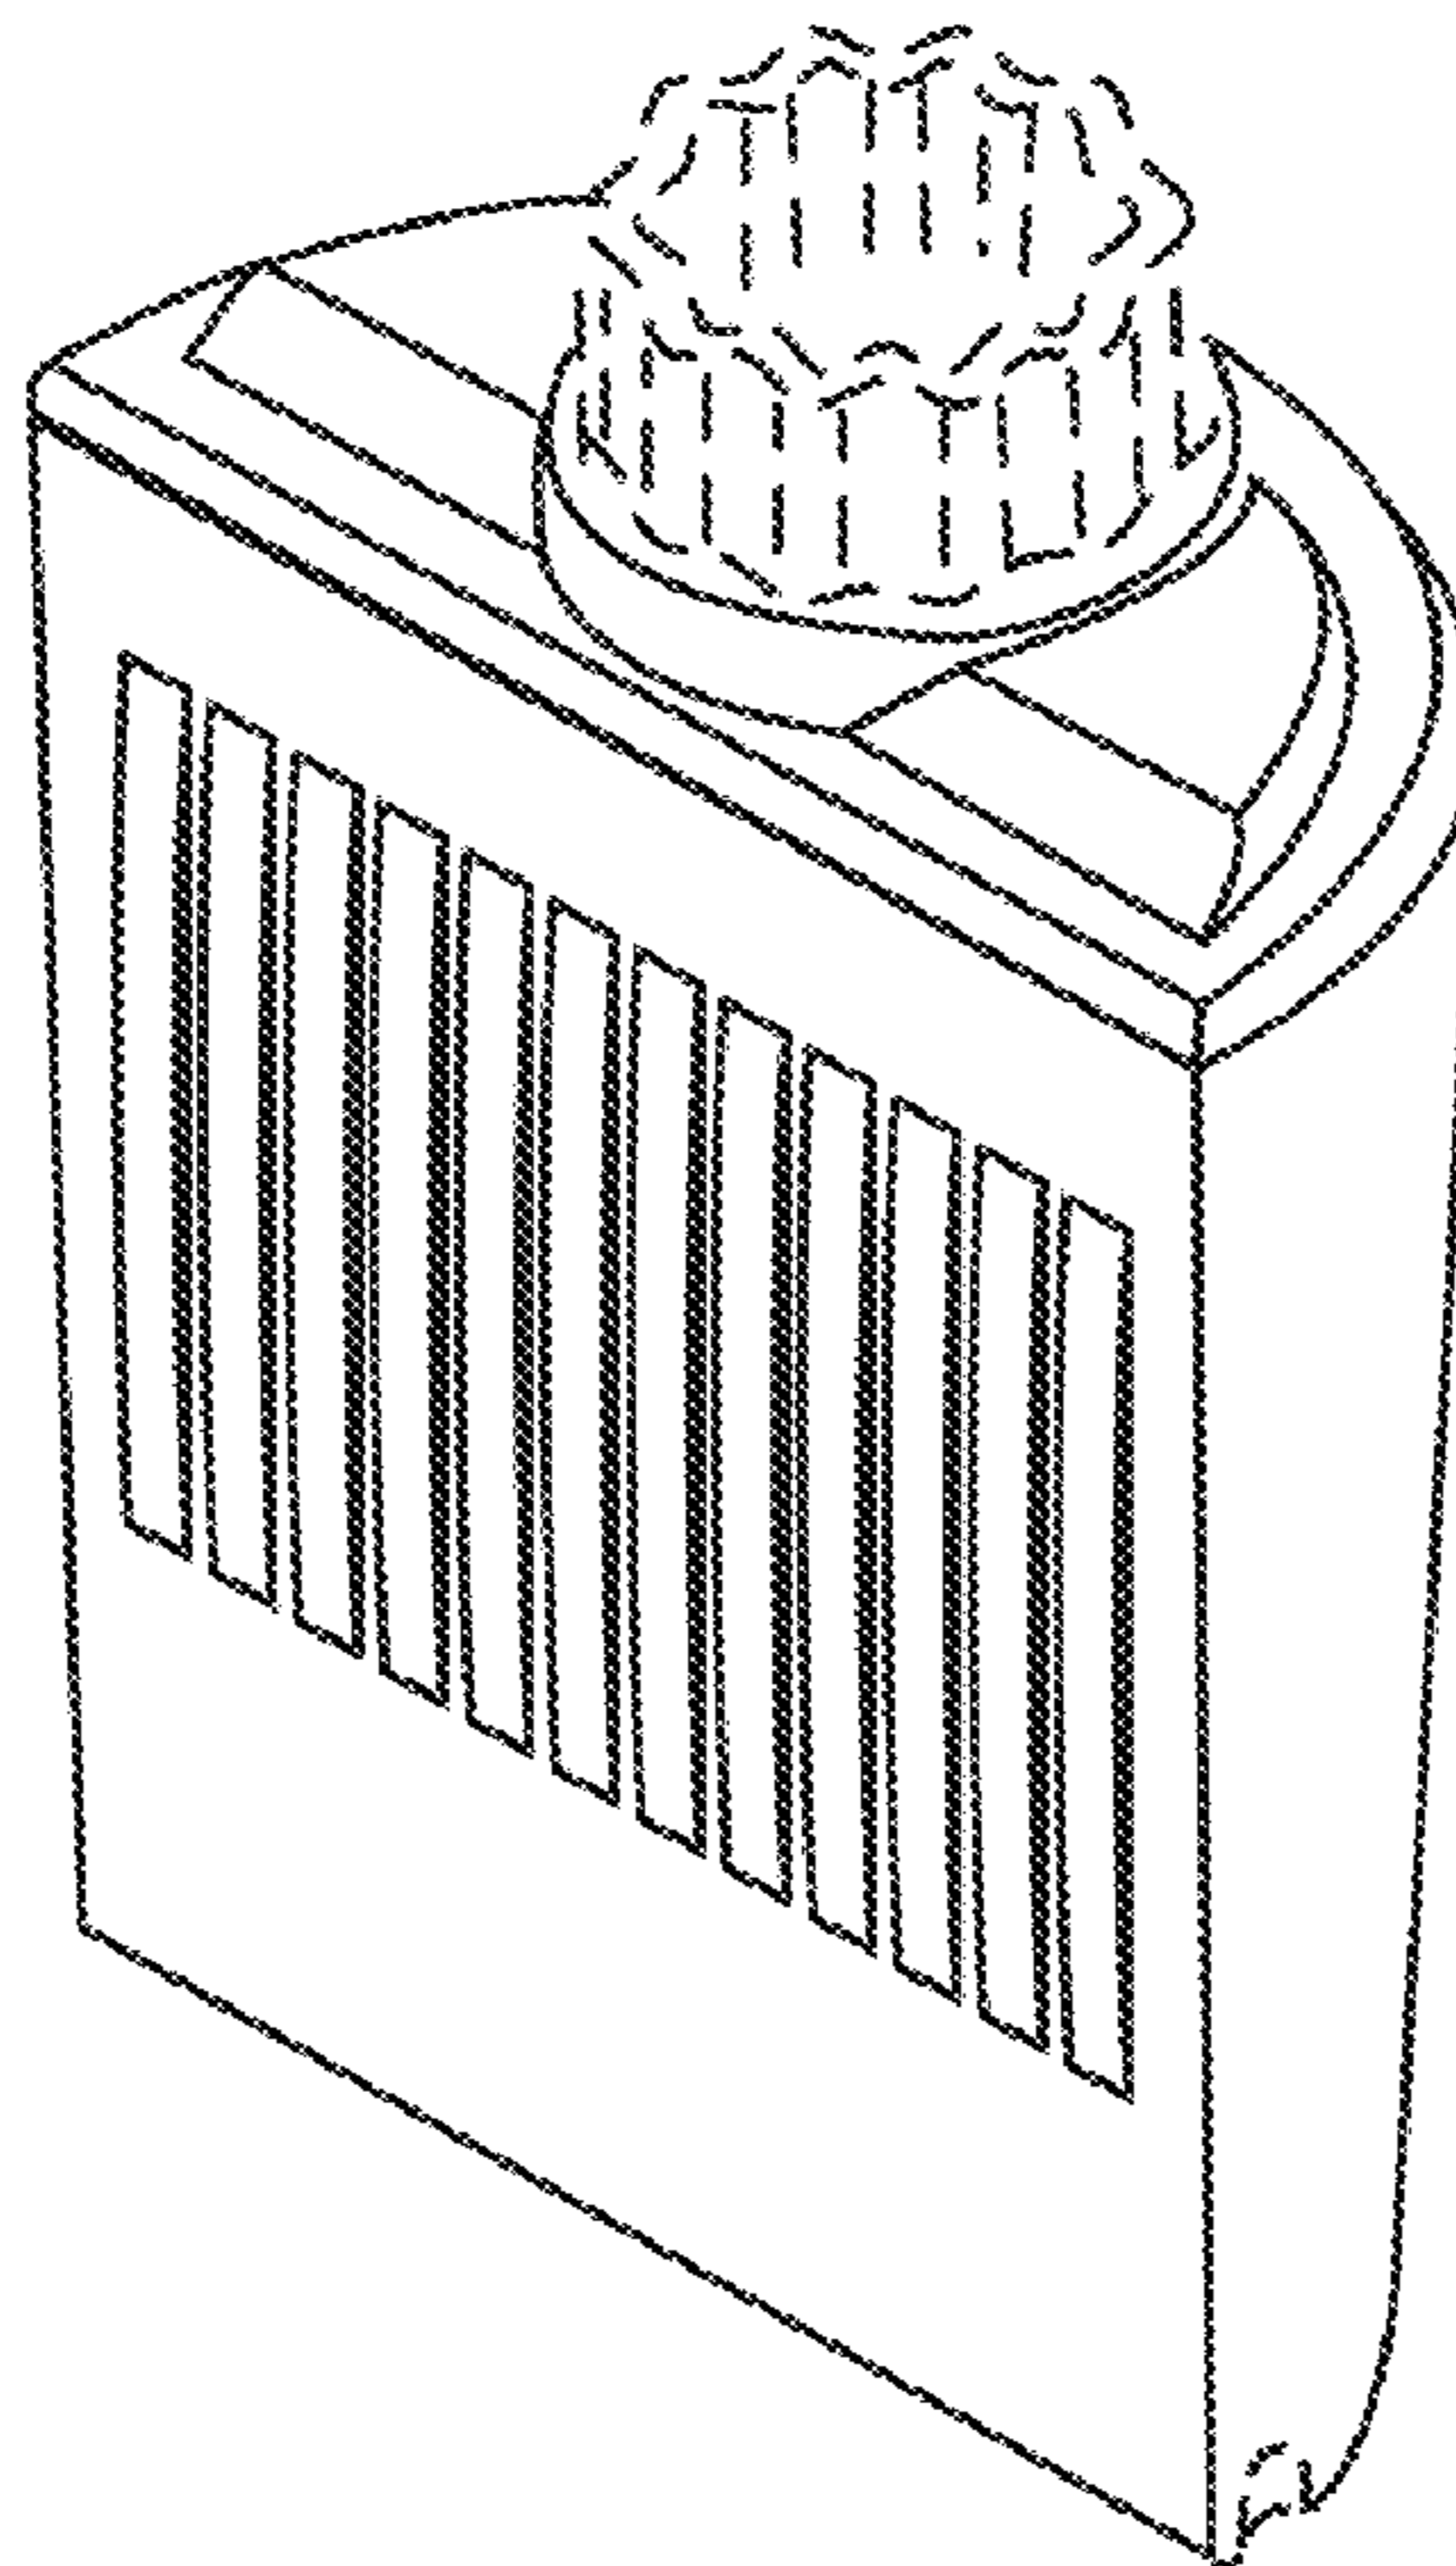

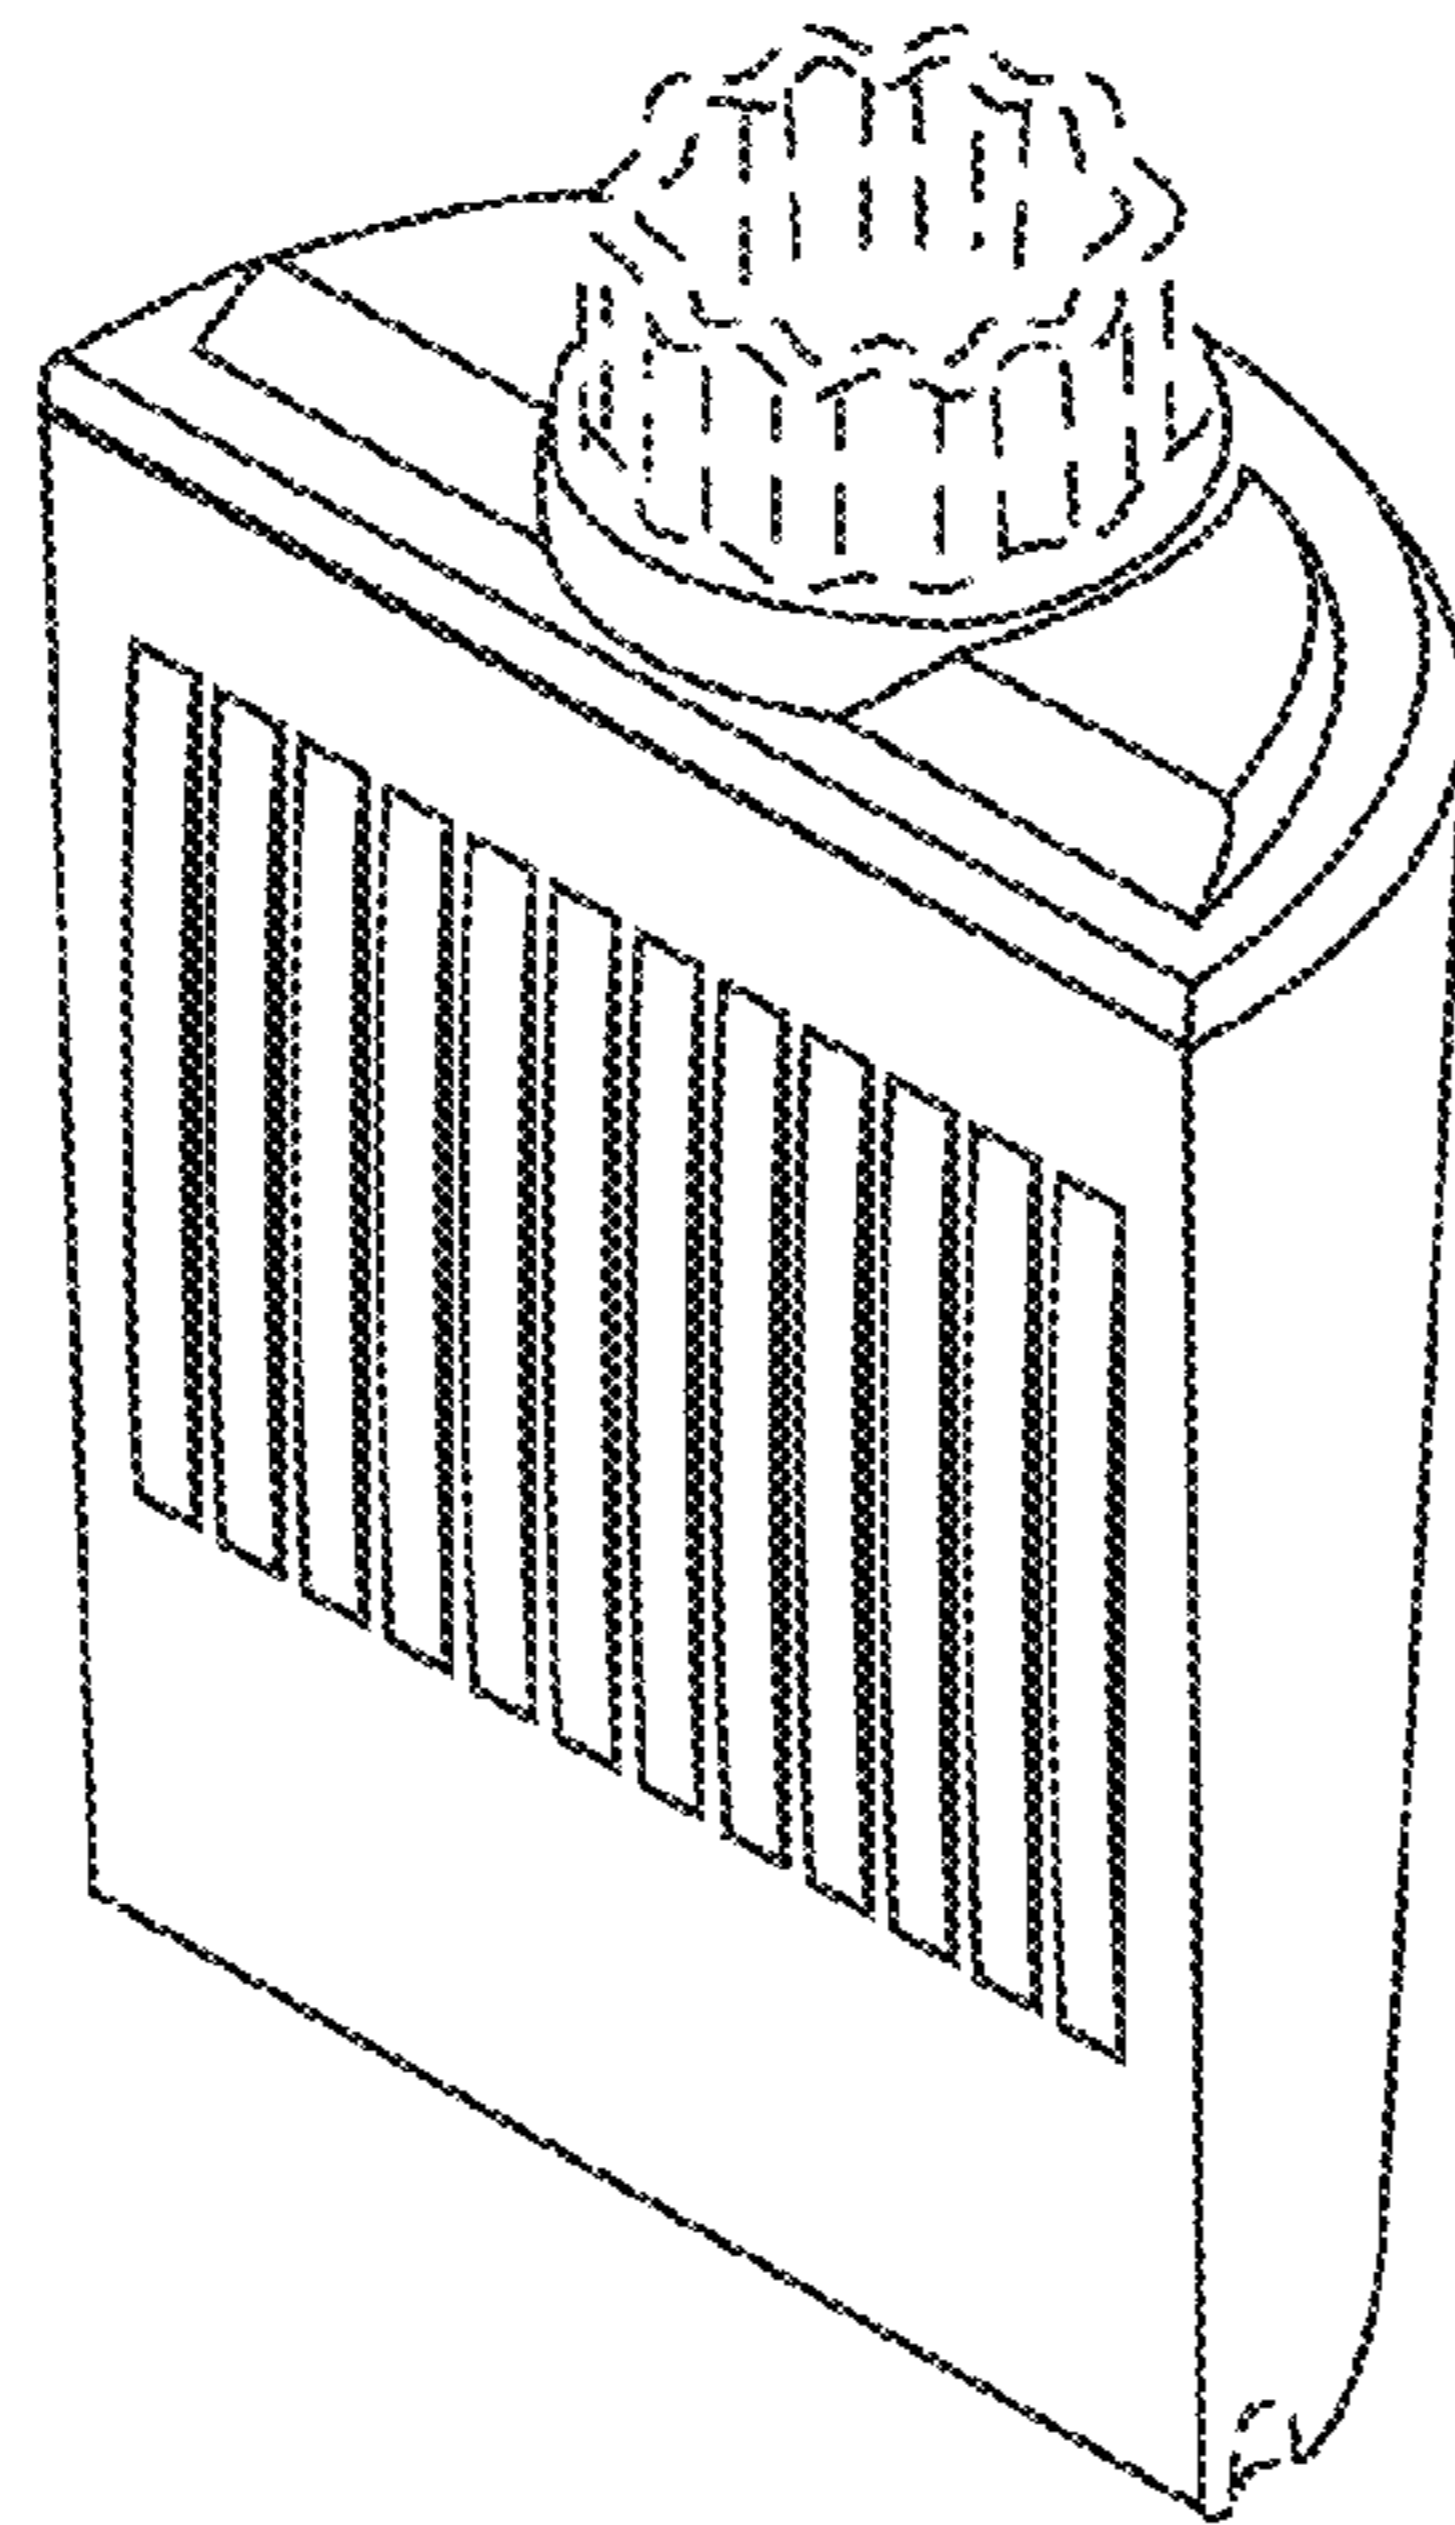


FIG. 1

FIG. 2

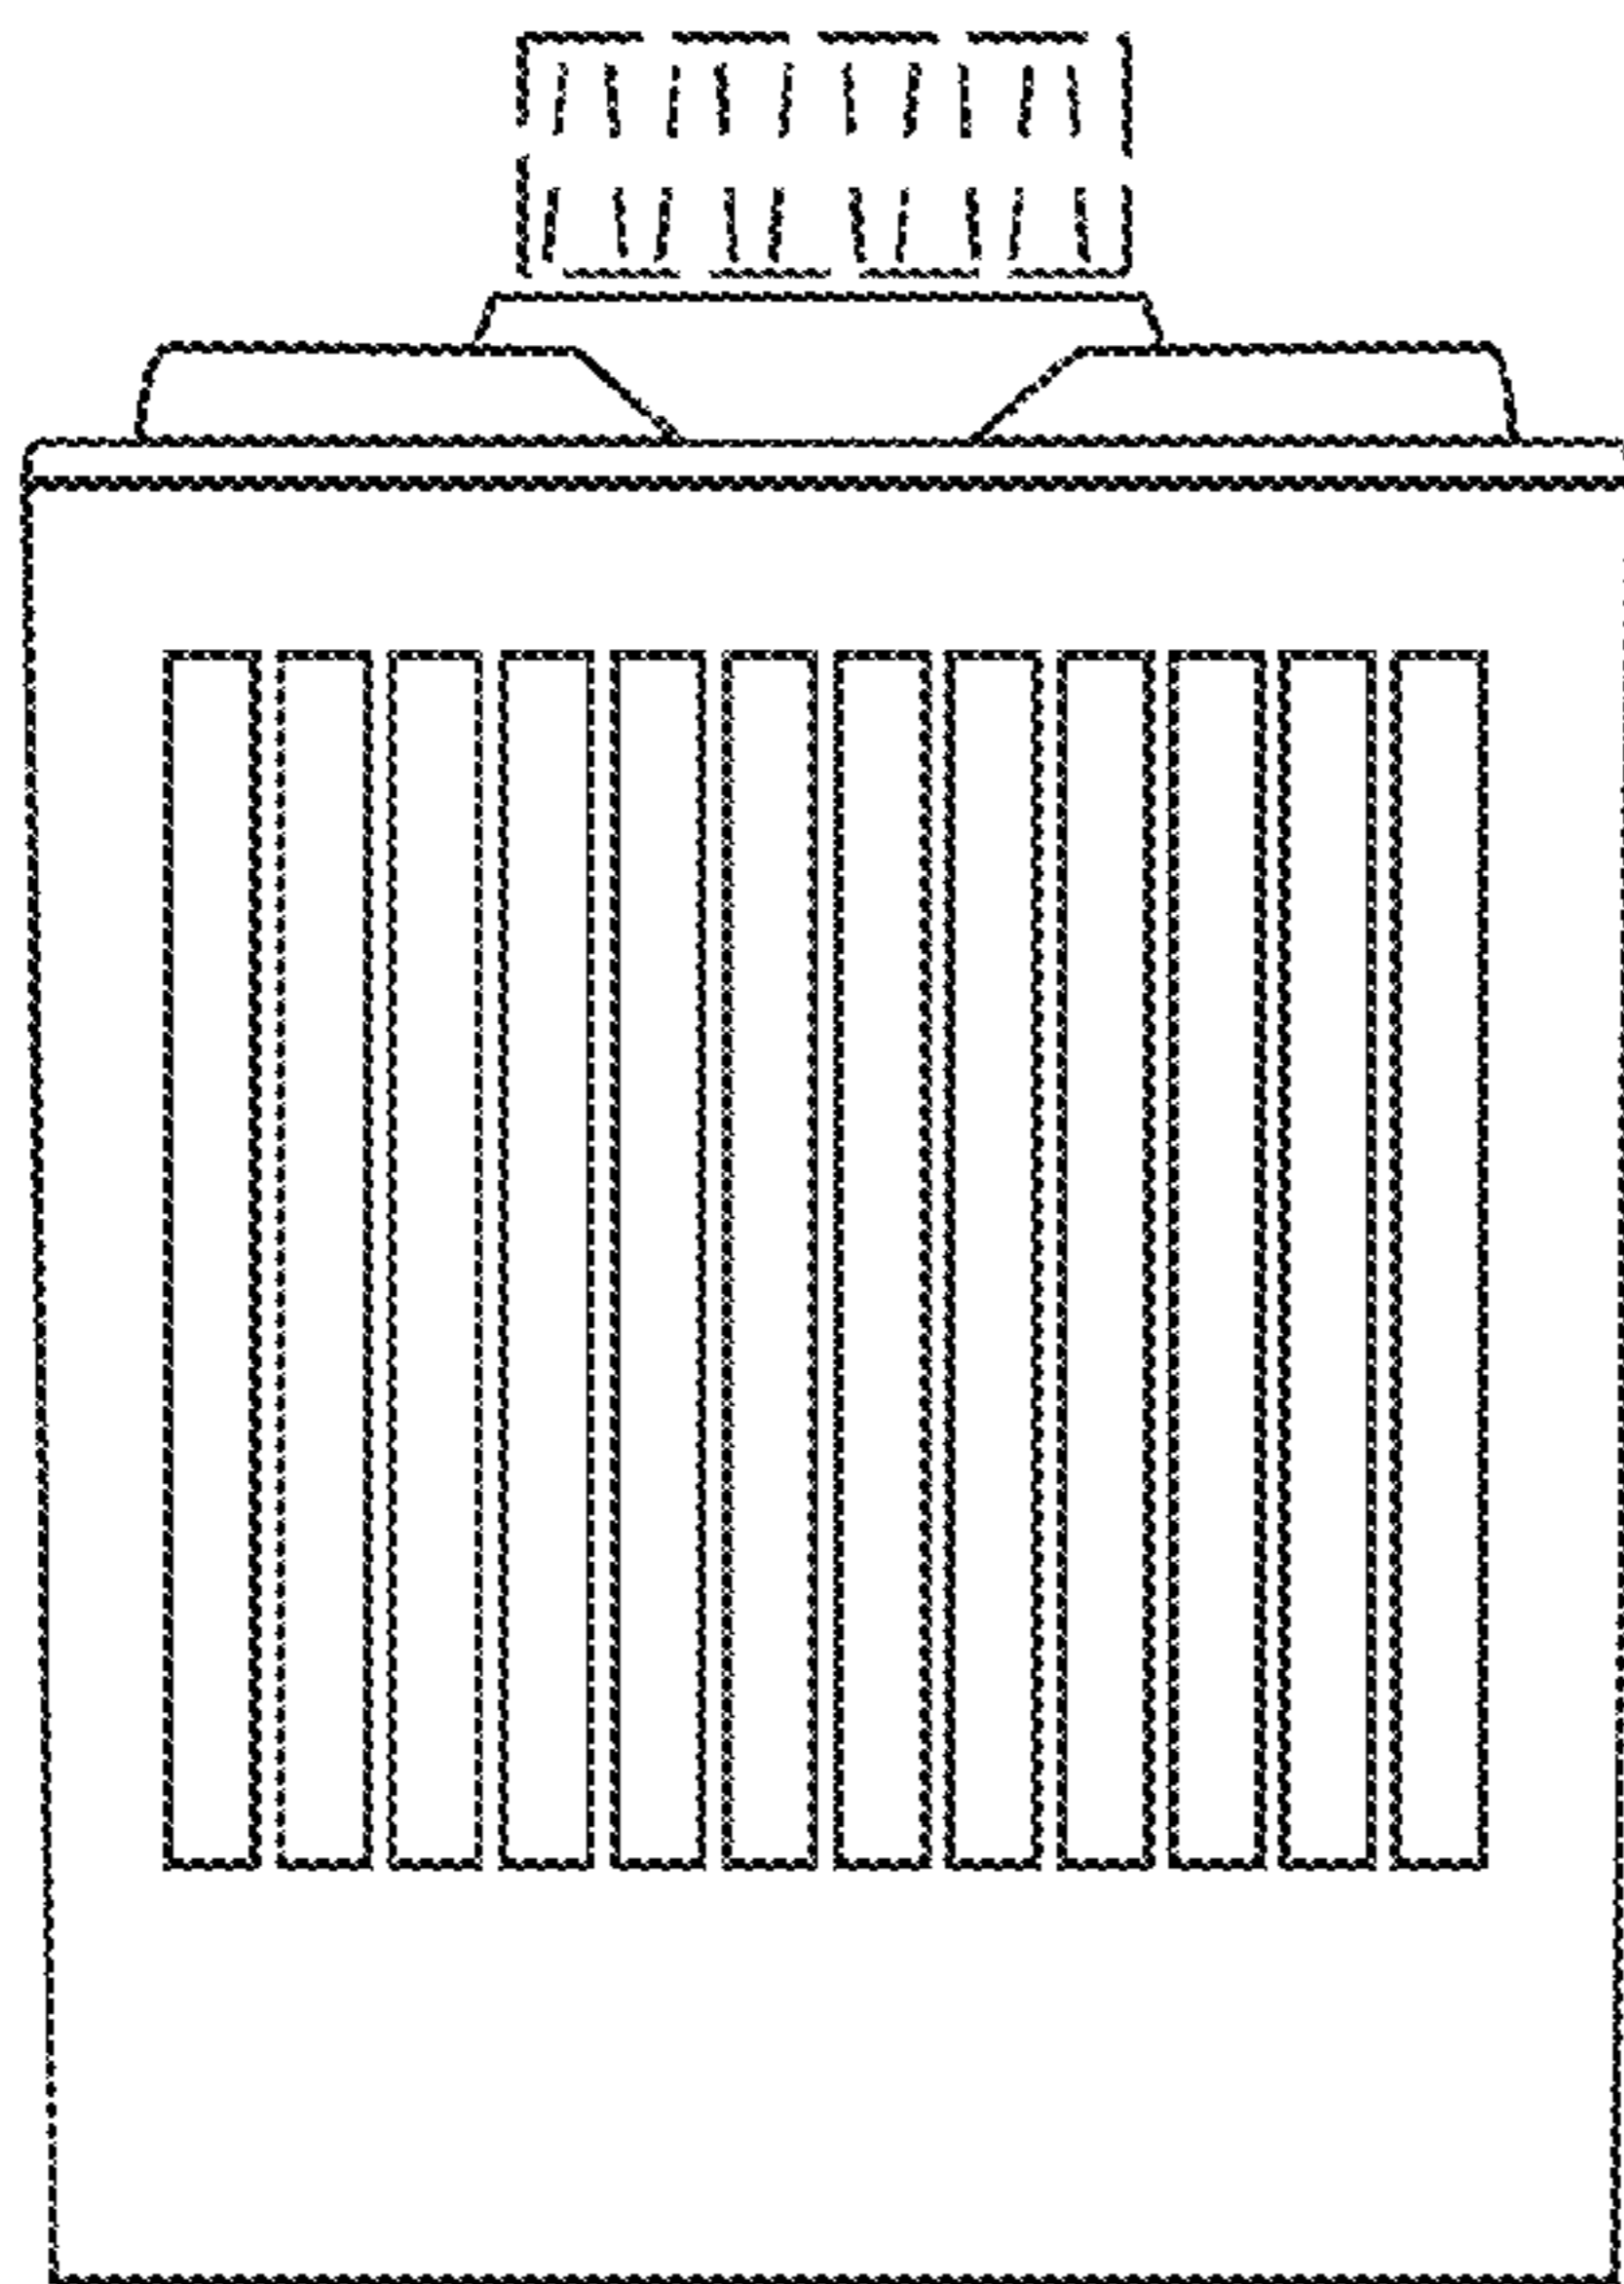
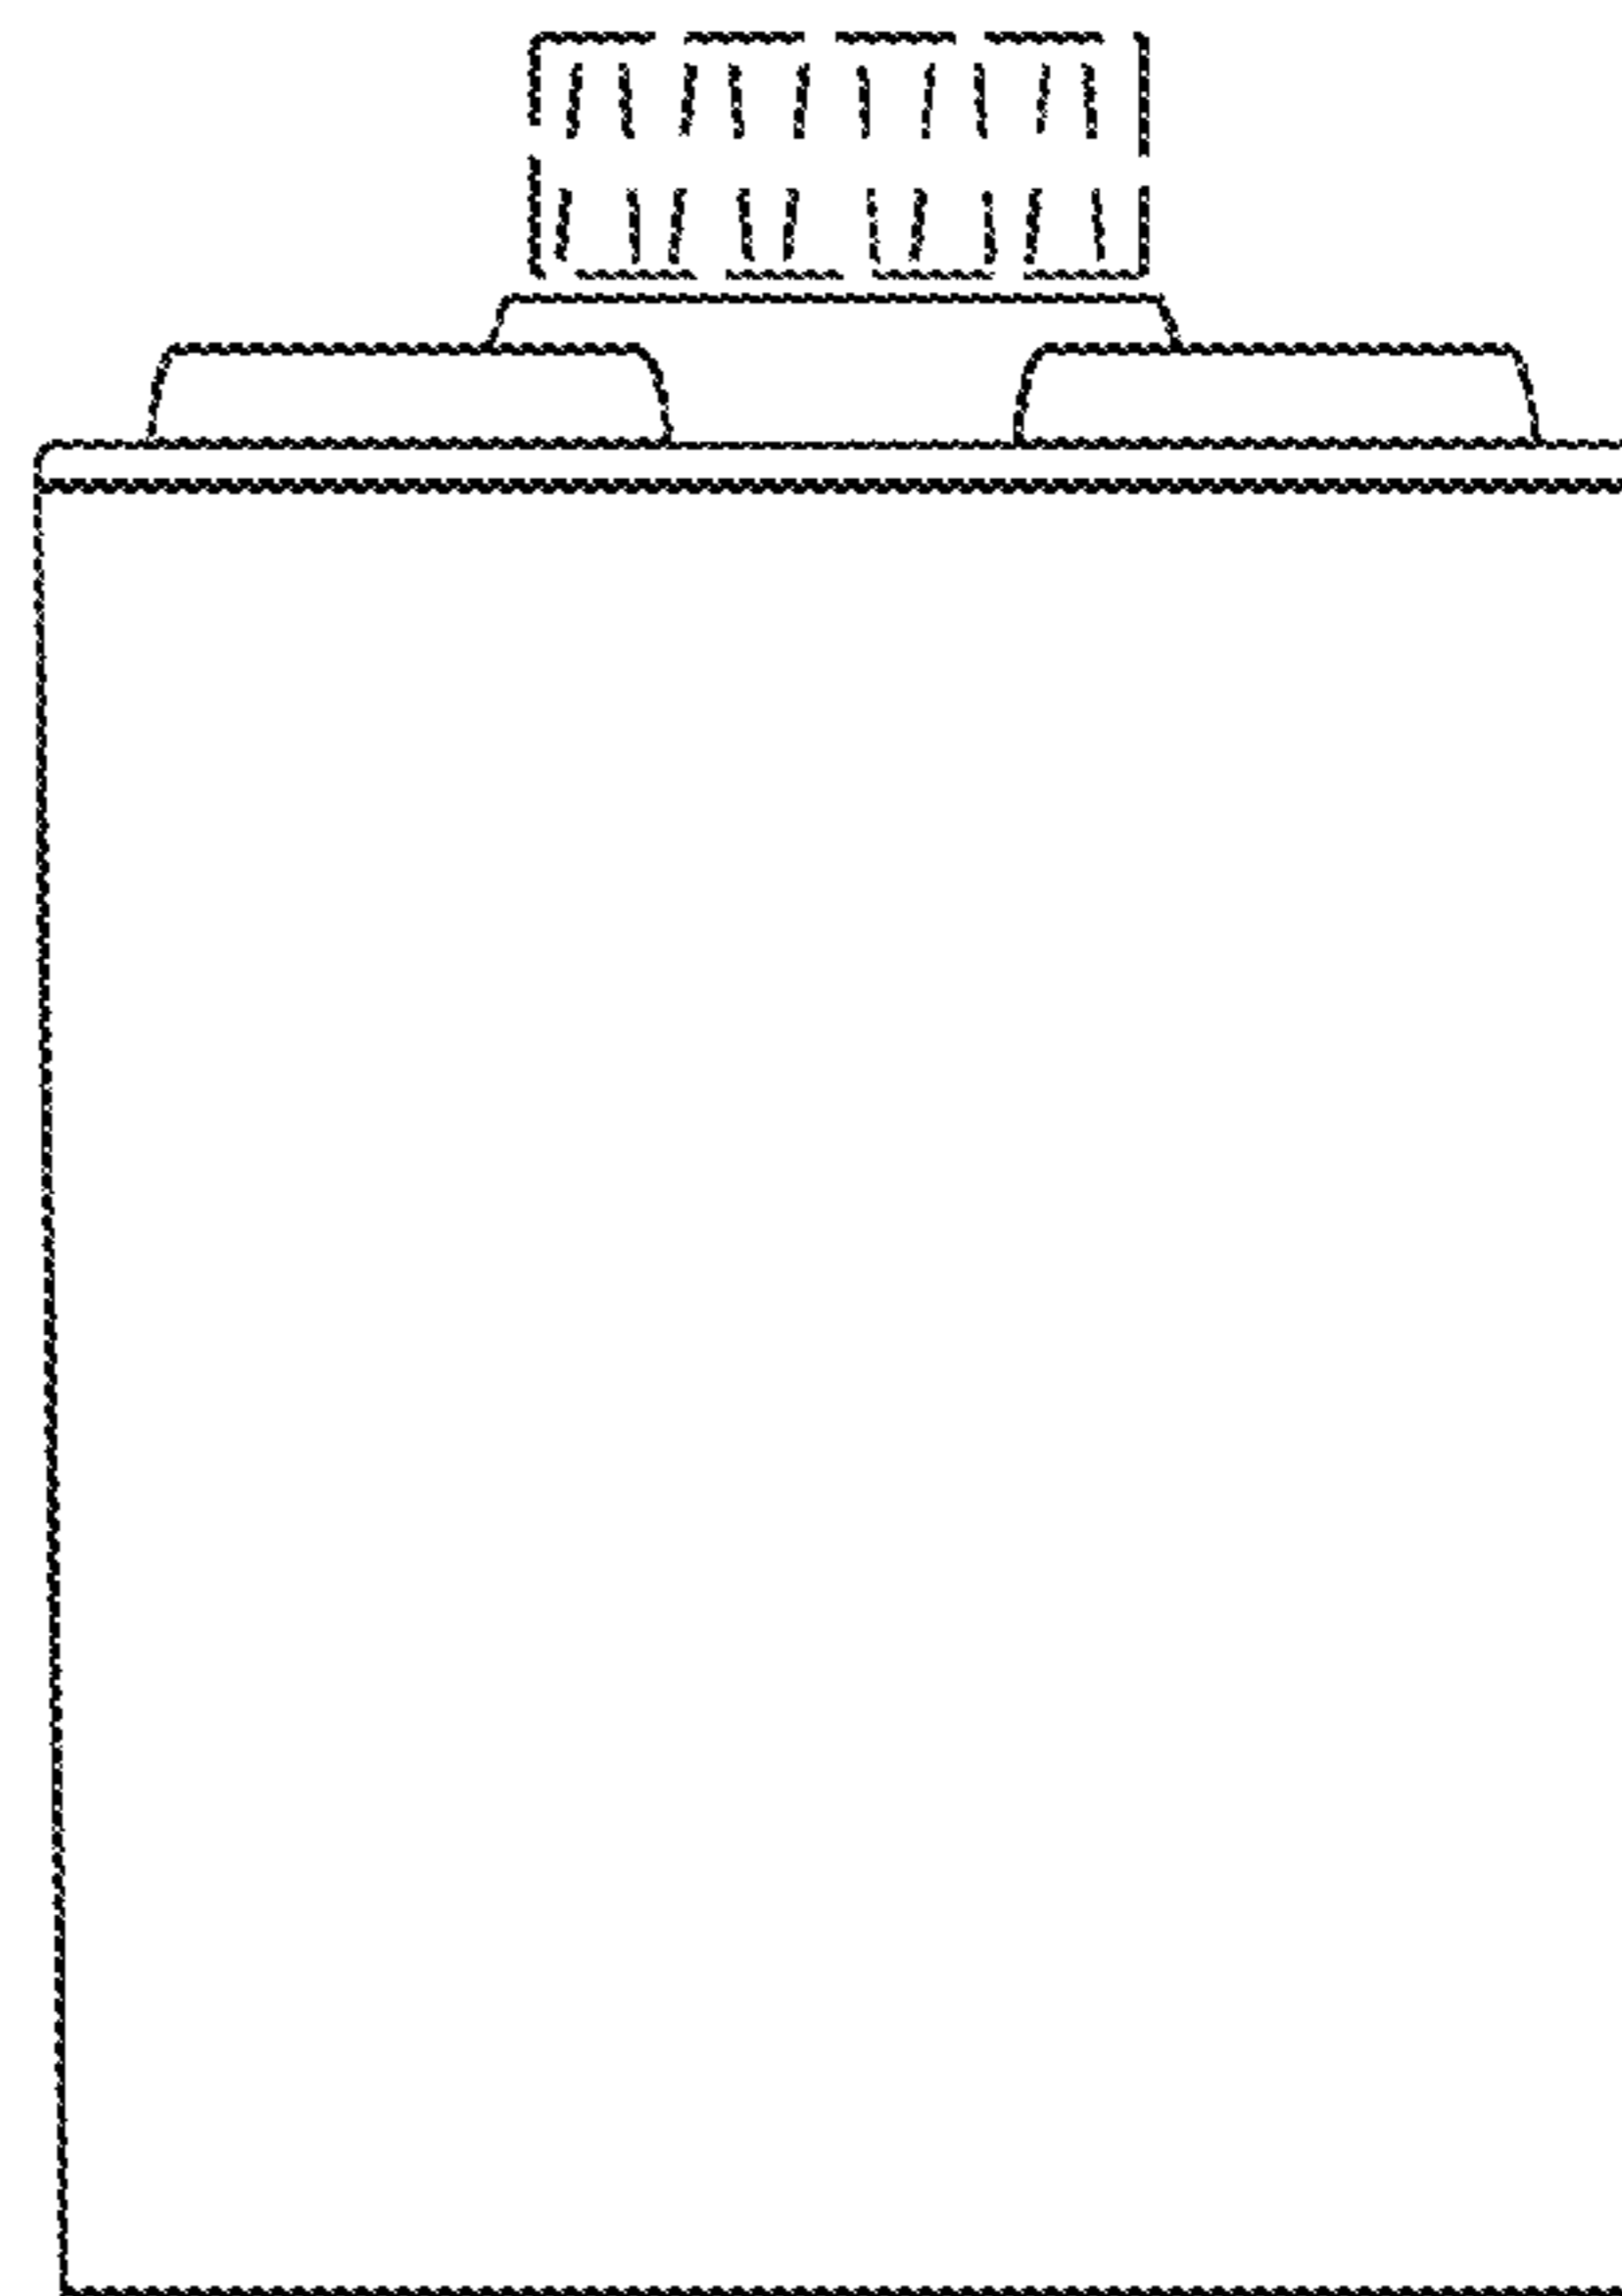


FIG. 3



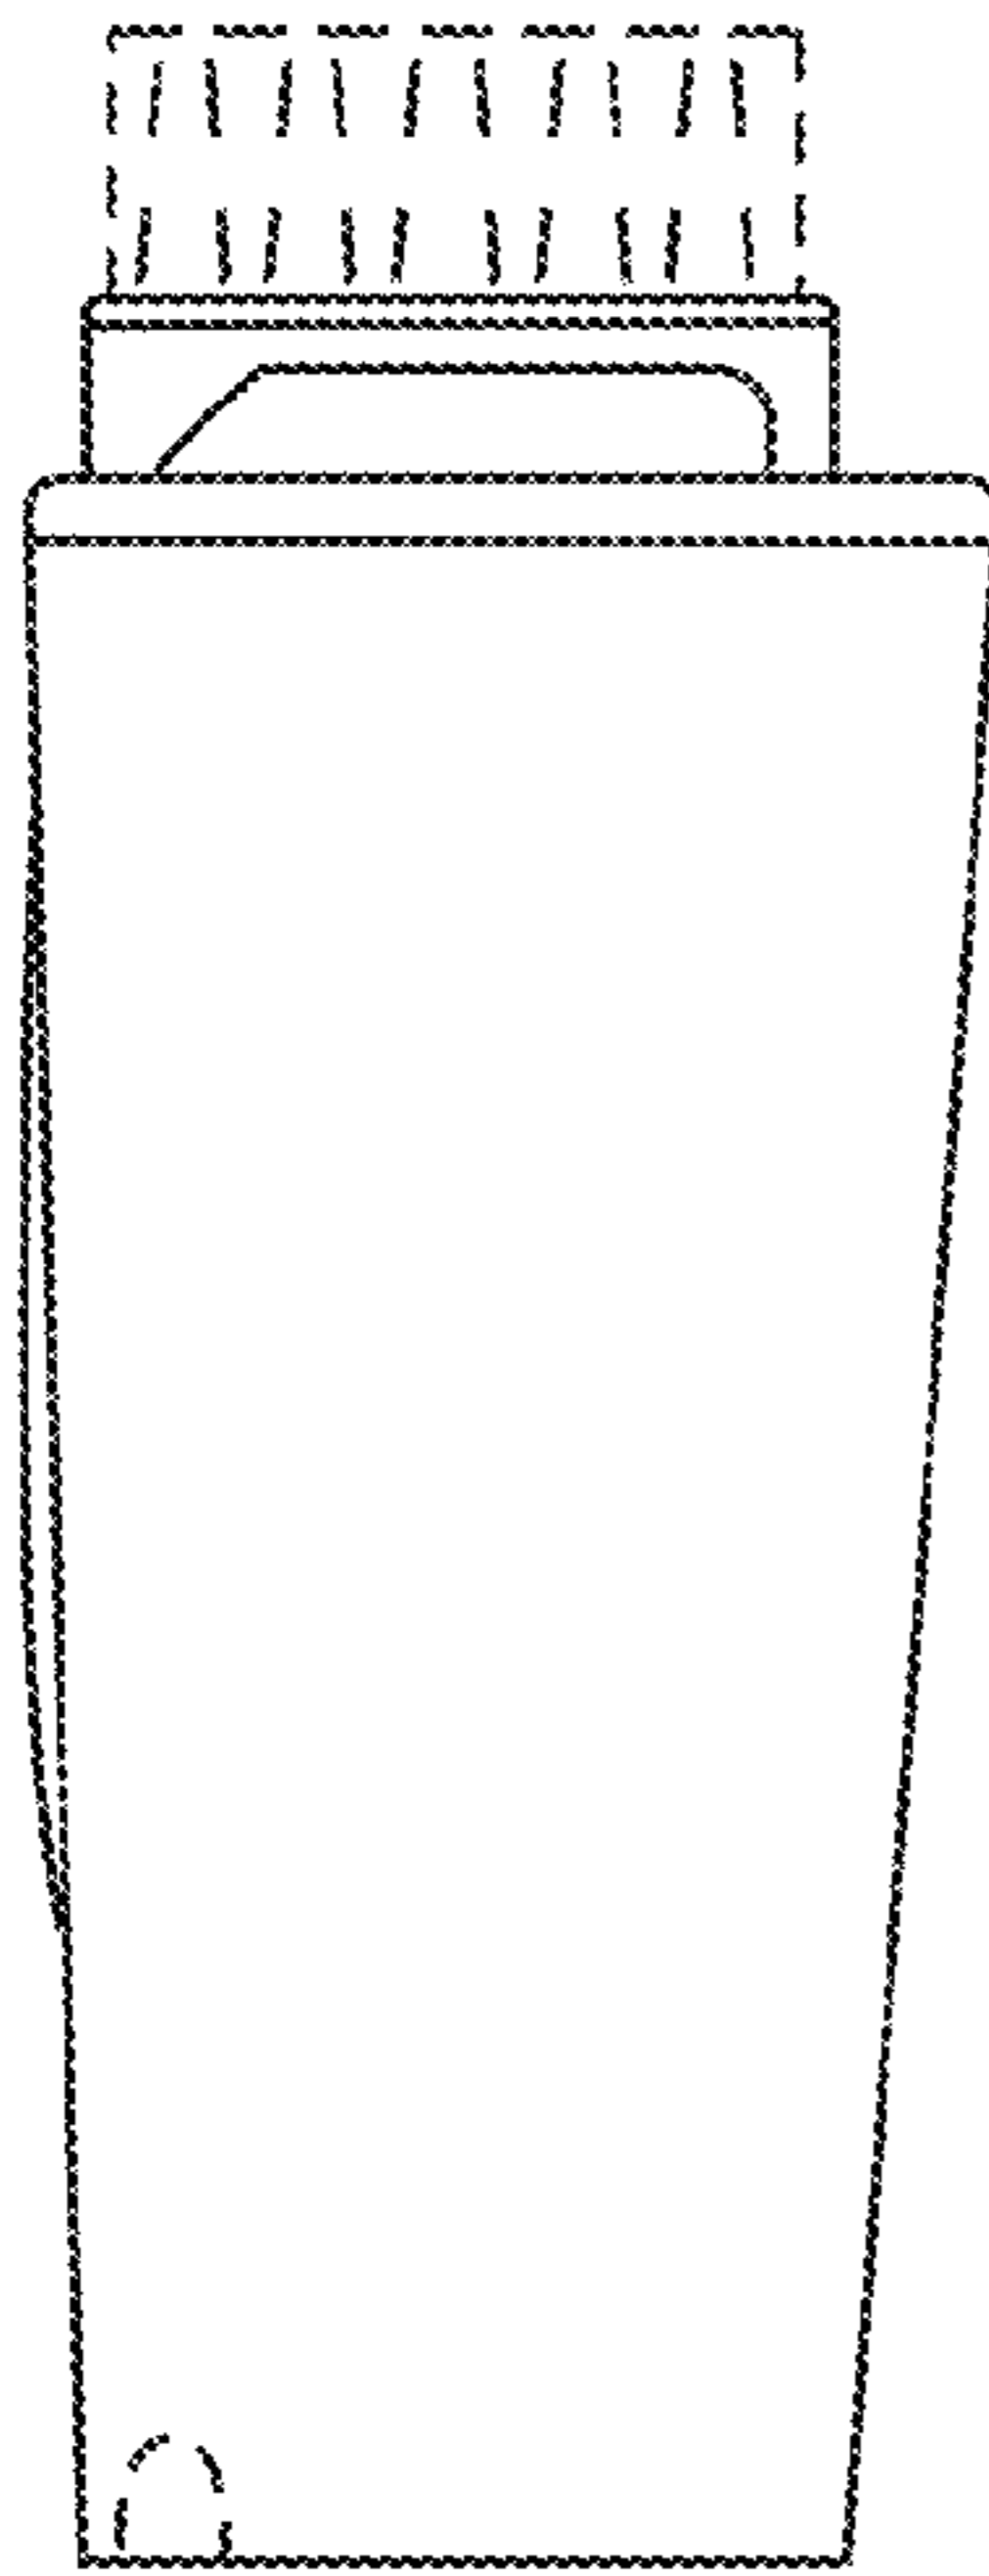


FIG. 4

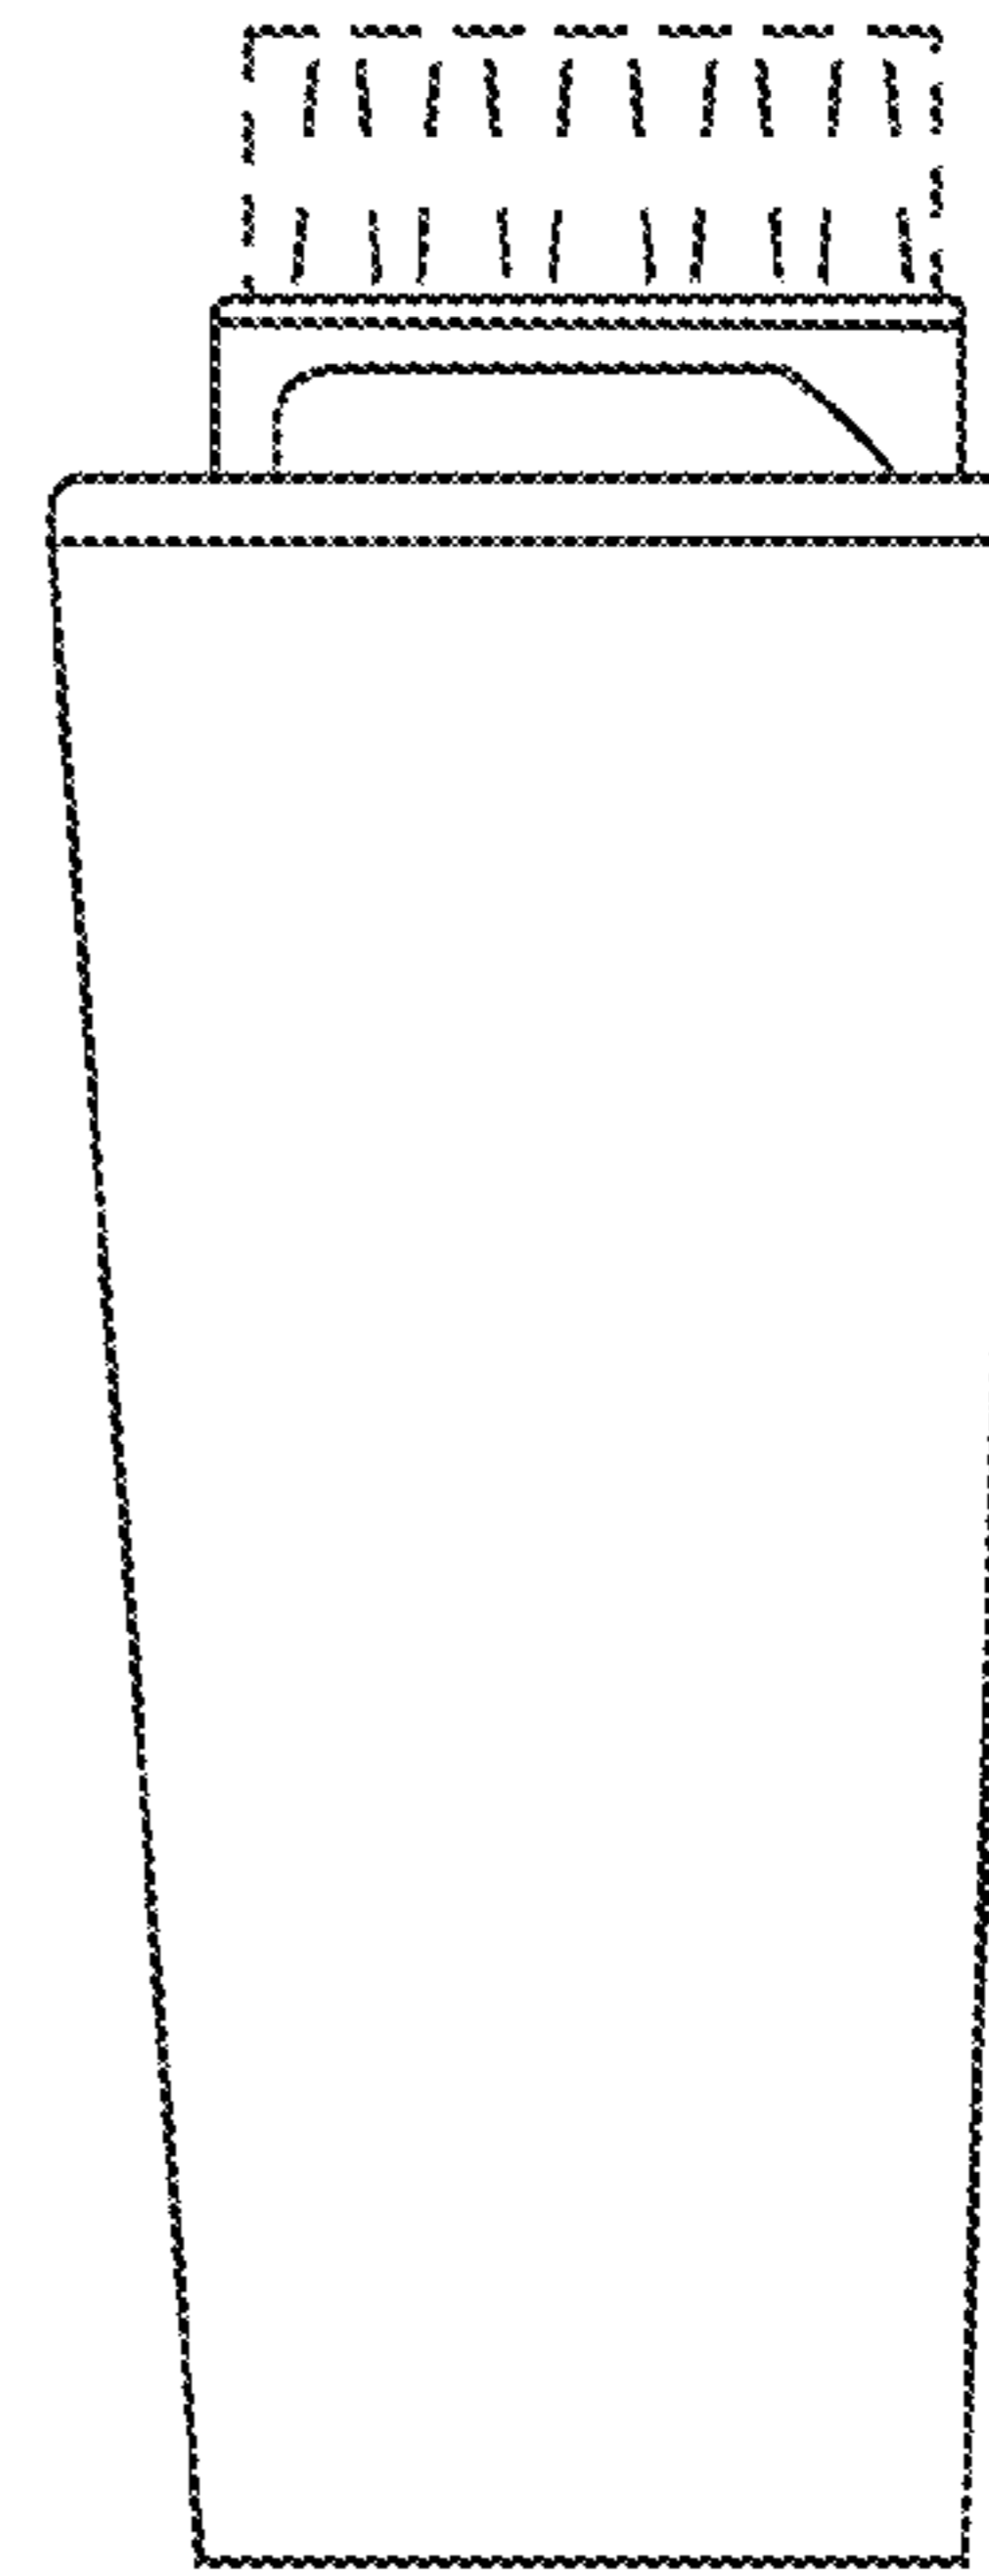


FIG. 5

FIG. 6

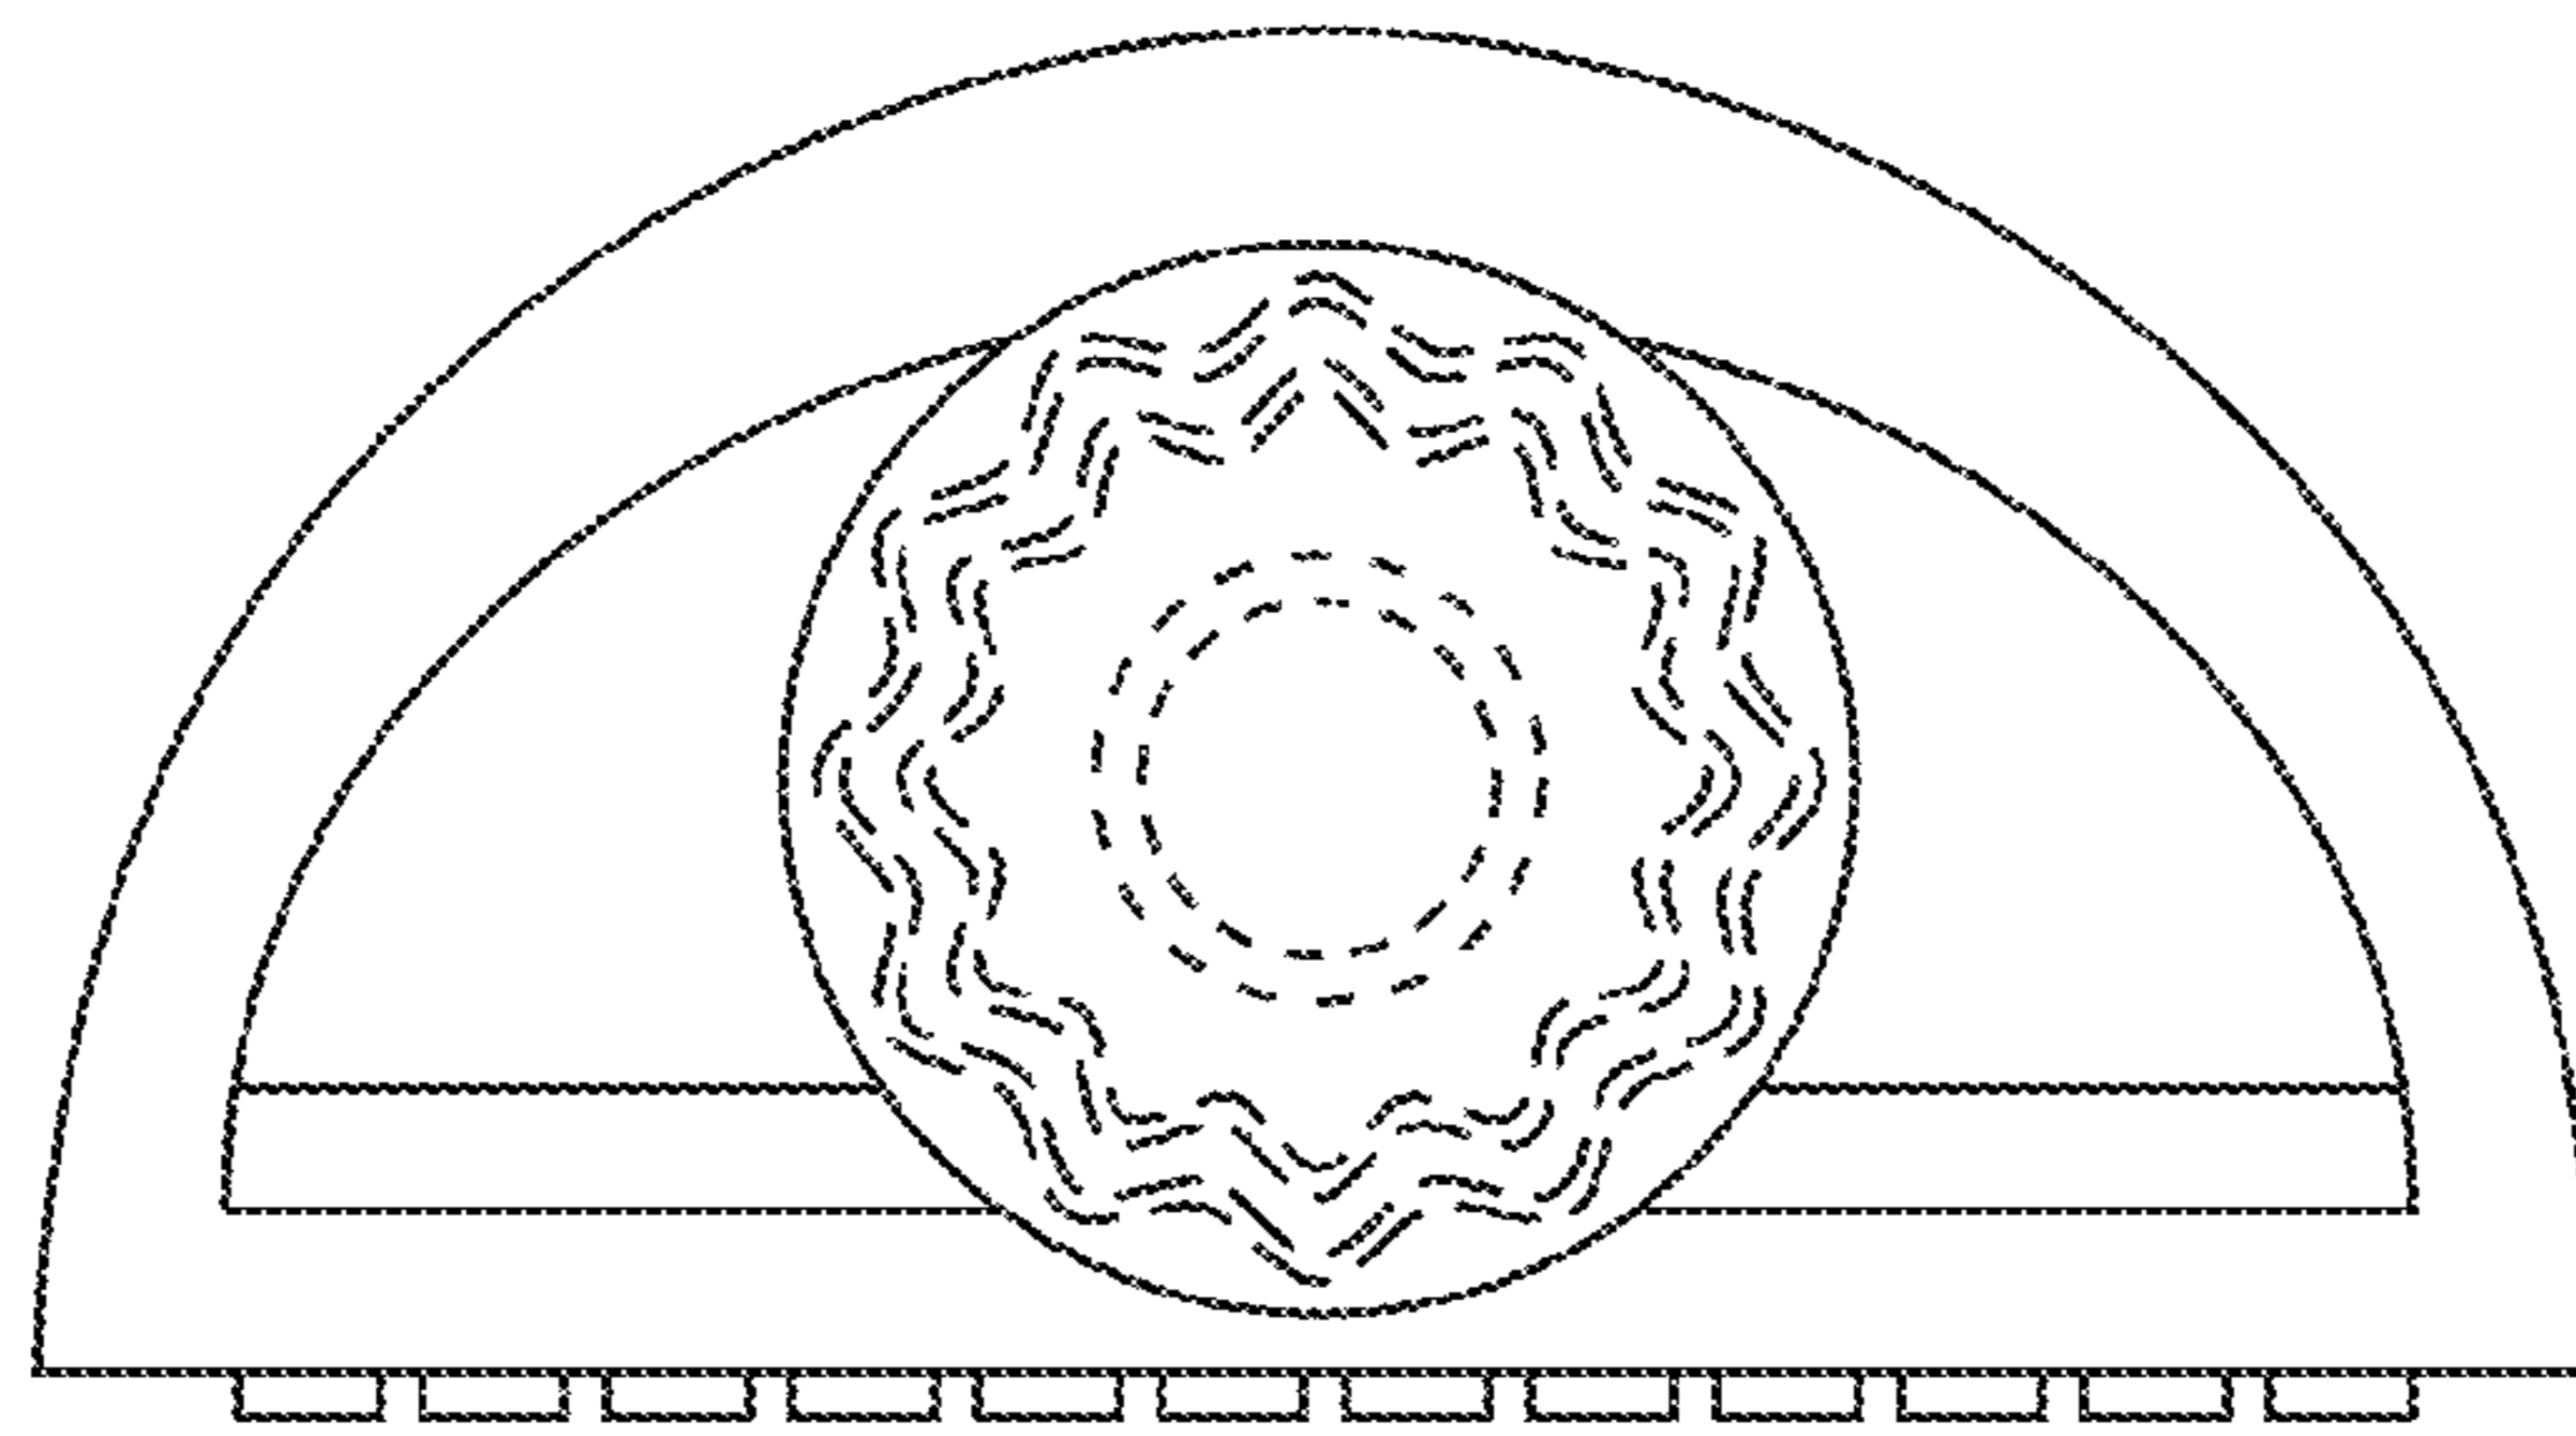


FIG. 7

