



US00D724727S

(12) **United States Design Patent**  
**Lubensky et al.**

(10) **Patent No.:** **US D724,727 S**  
(45) **Date of Patent:** **\*\* Mar. 17, 2015**

(54) **SURGICAL HANDLE**  
(71) Applicants: **Janelle M. Lubensky**, Winona Lake, IN (US); **Duncan G. Young**, Yorkshire (GB); **Francisco A. Amaral**, Acushnet, MA (US); **Craig S. Tsukayama**, Fort Wayne, IN (US); **Carl F. Livorsi**, Lakeville, MA (US); **Jeffrey M. Walcutt**, Fort Wayne, IN (US)

(72) Inventors: **Janelle M. Lubensky**, Winona Lake, IN (US); **Duncan G. Young**, Yorkshire (GB); **Francisco A. Amaral**, Acushnet, MA (US); **Craig S. Tsukayama**, Fort Wayne, IN (US); **Carl F. Livorsi**, Lakeville, MA (US); **Jeffrey M. Walcutt**, Fort Wayne, IN (US)

(73) Assignee: **DePuy (Ireland) (IE)**

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/457,179**

(22) Filed: **Jun. 7, 2013**

(51) **LOC (10) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/133**

(58) **Field of Classification Search**  
CPC ..... A61B 17/17; A61B 17/1725; A61B 2017/2925; A61B 2017/305; A61B 17/8819; A61F 2/46; A61F 2/4601; A61F 2/4603; A61F 2/4607; A61F 2/461  
USPC ..... D24/133, 140, 143, 144, 145, 146, 147, D24/155, 171  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D47,034 S \* 3/1915 Dickinson ..... D24/133  
D646,384 S \* 10/2011 Gauthier et al. .... D24/133  
D646,386 S \* 10/2011 Miller et al. .... D24/133  
2009/0125114 A1 5/2009 May et al.

2013/0006370 A1\* 1/2013 Wogoman et al. .... 623/20.16  
2013/0325014 A1 12/2013 Sordelet et al.  
2013/0325016 A1 12/2013 Sordelet et al.  
2013/0325018 A1 12/2013 Thomas et al.  
2013/0325019 A1 12/2013 Thomas et al.  
2013/0325021 A1 12/2013 Sordelet et al.  
2013/0325136 A1 12/2013 Thomas et al.  
2014/0276838 A1\* 9/2014 Tsukayama et al. .... 606/80  
2014/0276850 A1\* 9/2014 Chaney et al. .... 606/84

**OTHER PUBLICATIONS**

Zimmer NexGen LCCK, Surgical Technique for use with LCCK 4-in-1 Instrument, 2009, 52 pages.  
DePuy Orthopaedics, Inc., Sigma Revision and M.B.T. Revision Tray, Surgical Technique, 2008, 82 pages.  
Smith & Nephew, Legion, Revision Knee System, Surgical Technique, 2005, 40 pages.  
Biomet, Vanguard SSK, Revision System, Surgical Technique, Feb. 2008, 64 pages.

(Continued)

*Primary Examiner* — Bridget L Eland

(74) *Attorney, Agent, or Firm* — Barnes & Thornburg LLP

(57) **CLAIM**


We claim the ornamental design for a surgical handle, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view for a surgical handle showing our new design;  
FIG. 2 is a first side elevation view of the surgical handle of FIG. 1;  
FIG. 3 is a second side elevation view opposite the first side elevation view of FIG. 2;  
FIG. 4 is a bottom plan view of the surgical handle of FIG. 1;  
FIG. 5 is a top plan view of the surgical handle of FIG. 1; and  
FIG. 6 is a front elevation view of the surgical handle of FIG. 1; and,  
FIG. 7 is a rear elevation view of the surgical handle of FIG. 1.

The features shown in broken lines depict environmental subject matter only and form no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

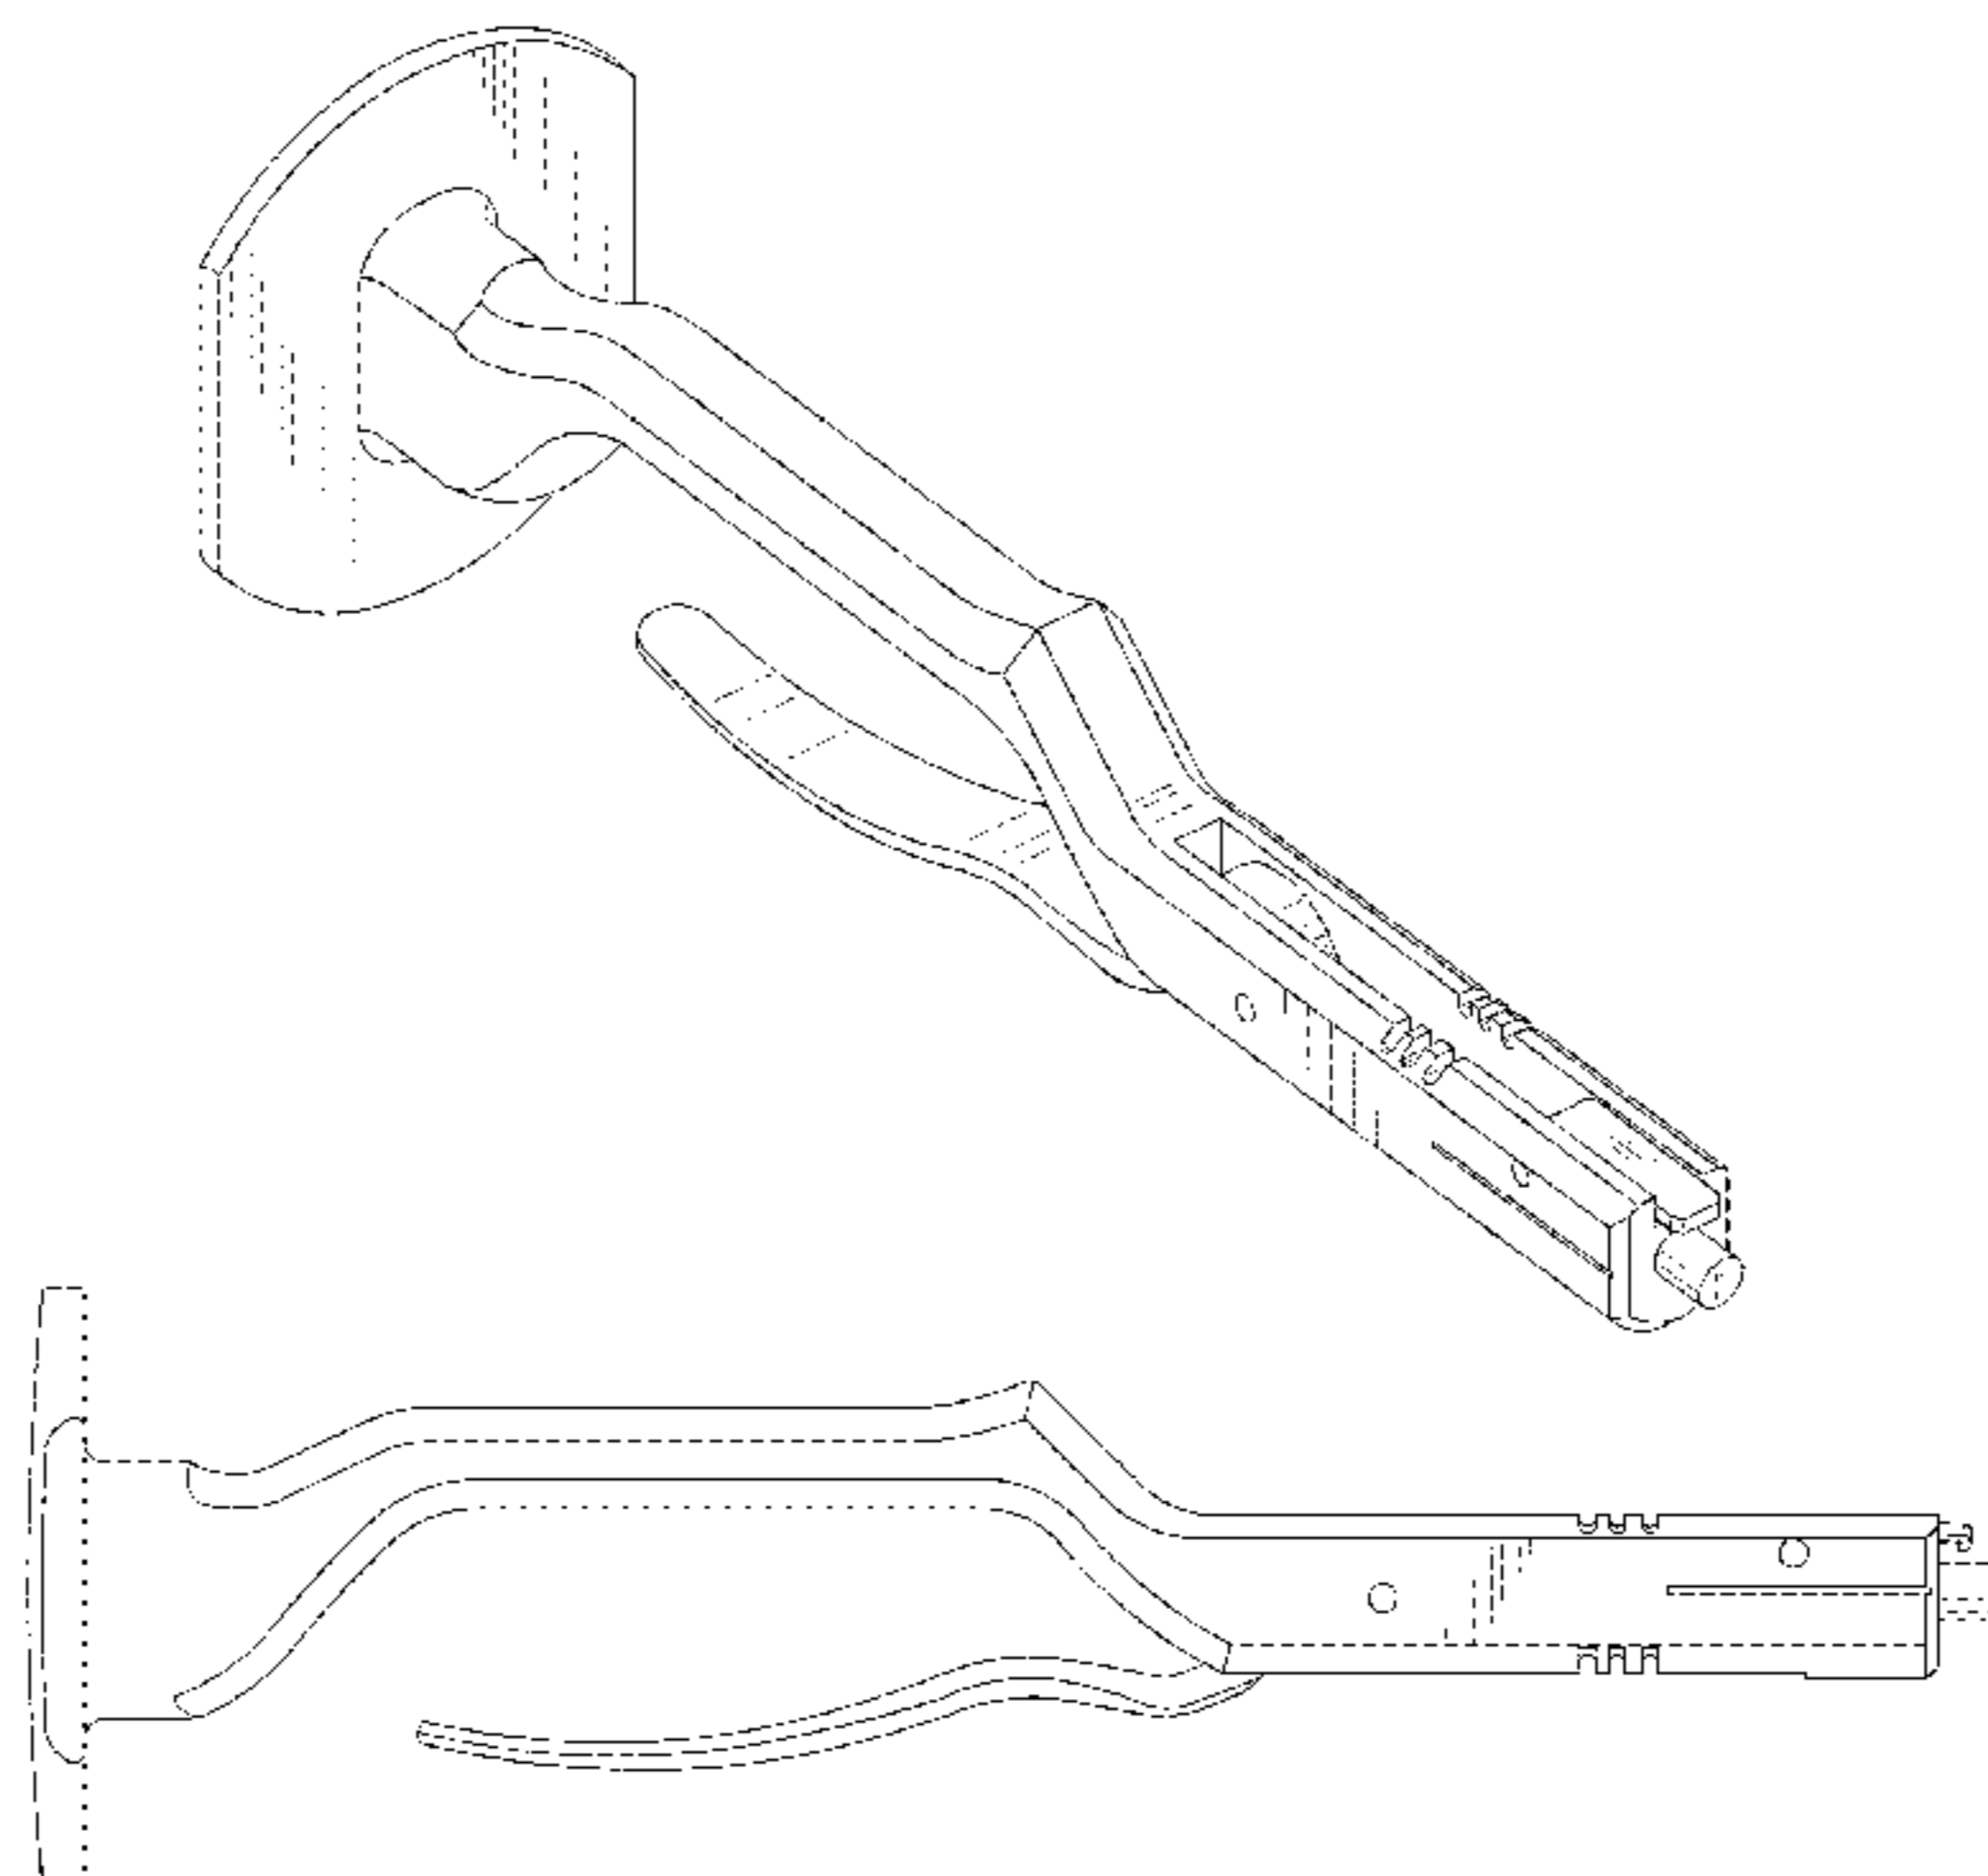

(56)

**References Cited**

OTHER PUBLICATIONS

GMK Revision, Surgical Technique, Ref. 99.27.12US rev. 1, 1999, 74 pages.

PFC Sigma RP-F, Specialist 2 Instruments, Surgical Technique, Performance in Flexion, 2007, 32 pages.

P.F.C. Sigma Rotating Platform Knee System with M.B.T Tray, Primary Procedure with a Curved or Posterior Stabilised Implant, 2003, 43 pages.

LCS High Performance Instruments, Surgical Technique, 2008, 44 pages.

Sigma High Performance Instruments, Design Rationale, 2007, 12 pages.

Sigma High Performance Instruments, Classic Surgical Technique, 2010, 52 pages.

Attune Knee System Surgical Technique, 2013, 73 pages.

\* cited by examiner

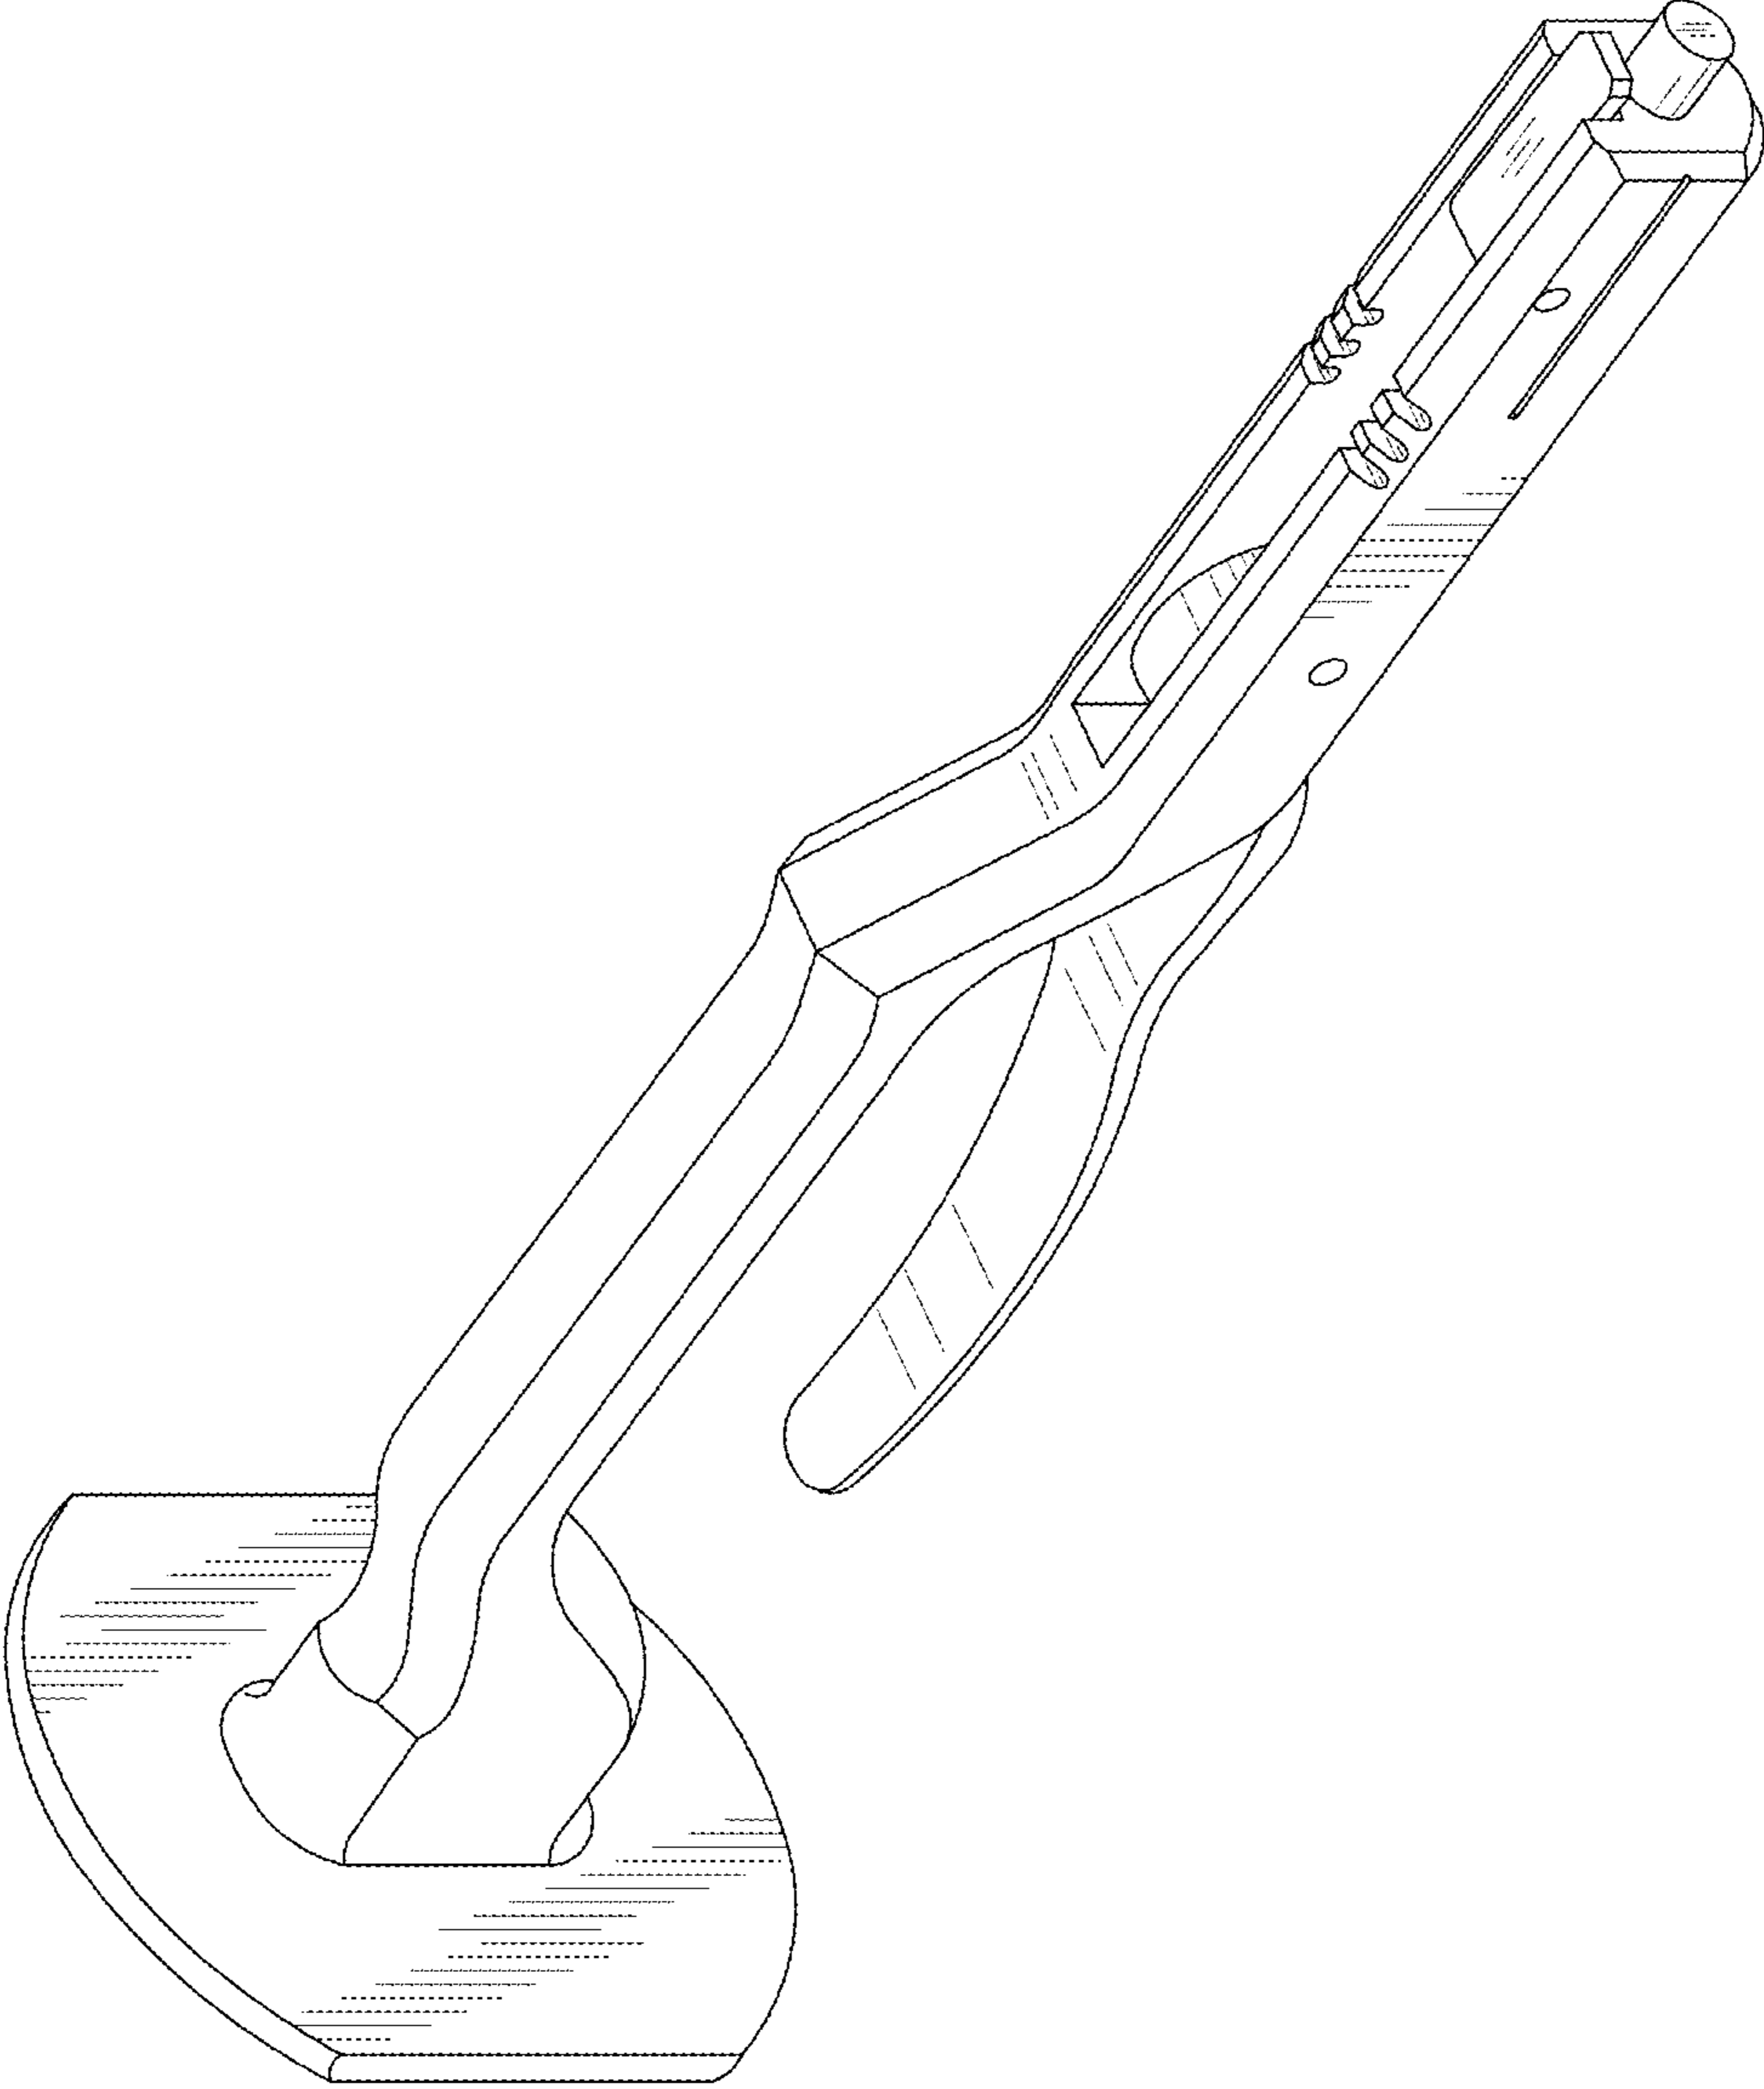


Fig. 1

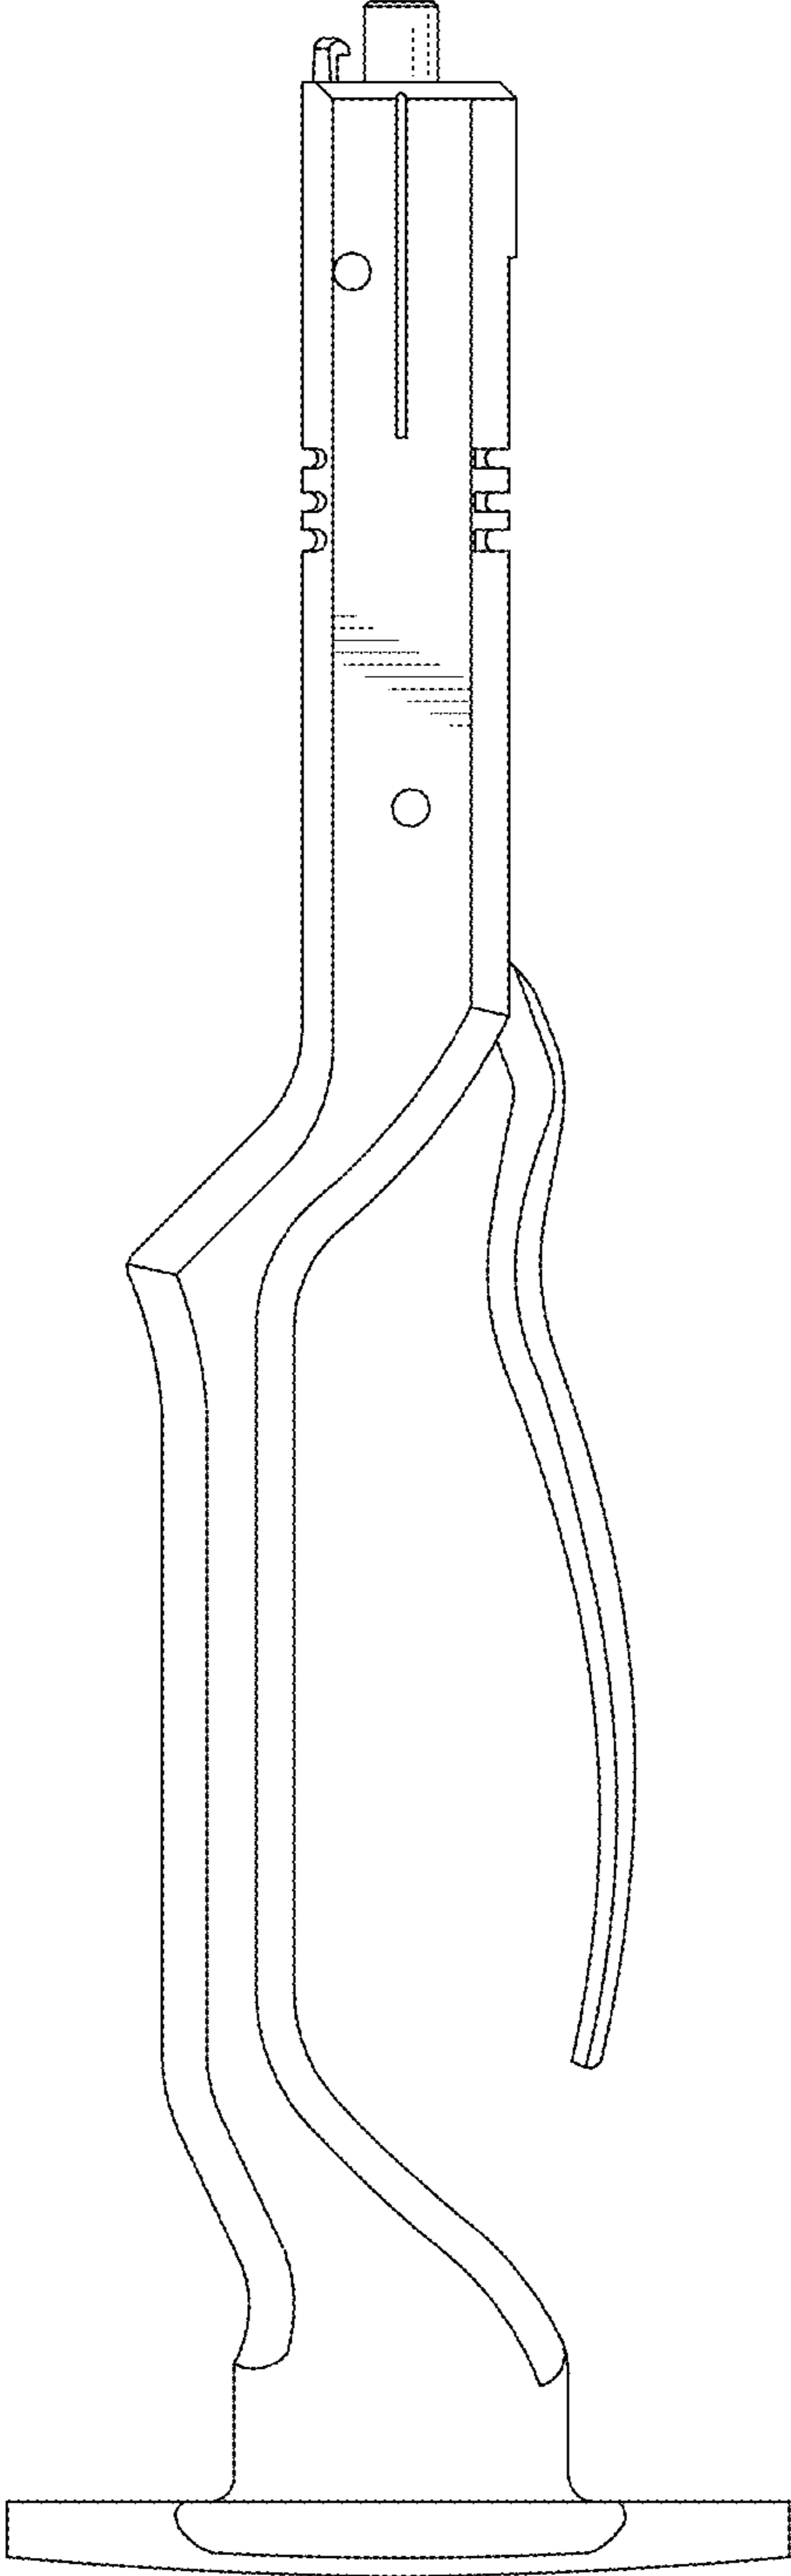


Fig. 2

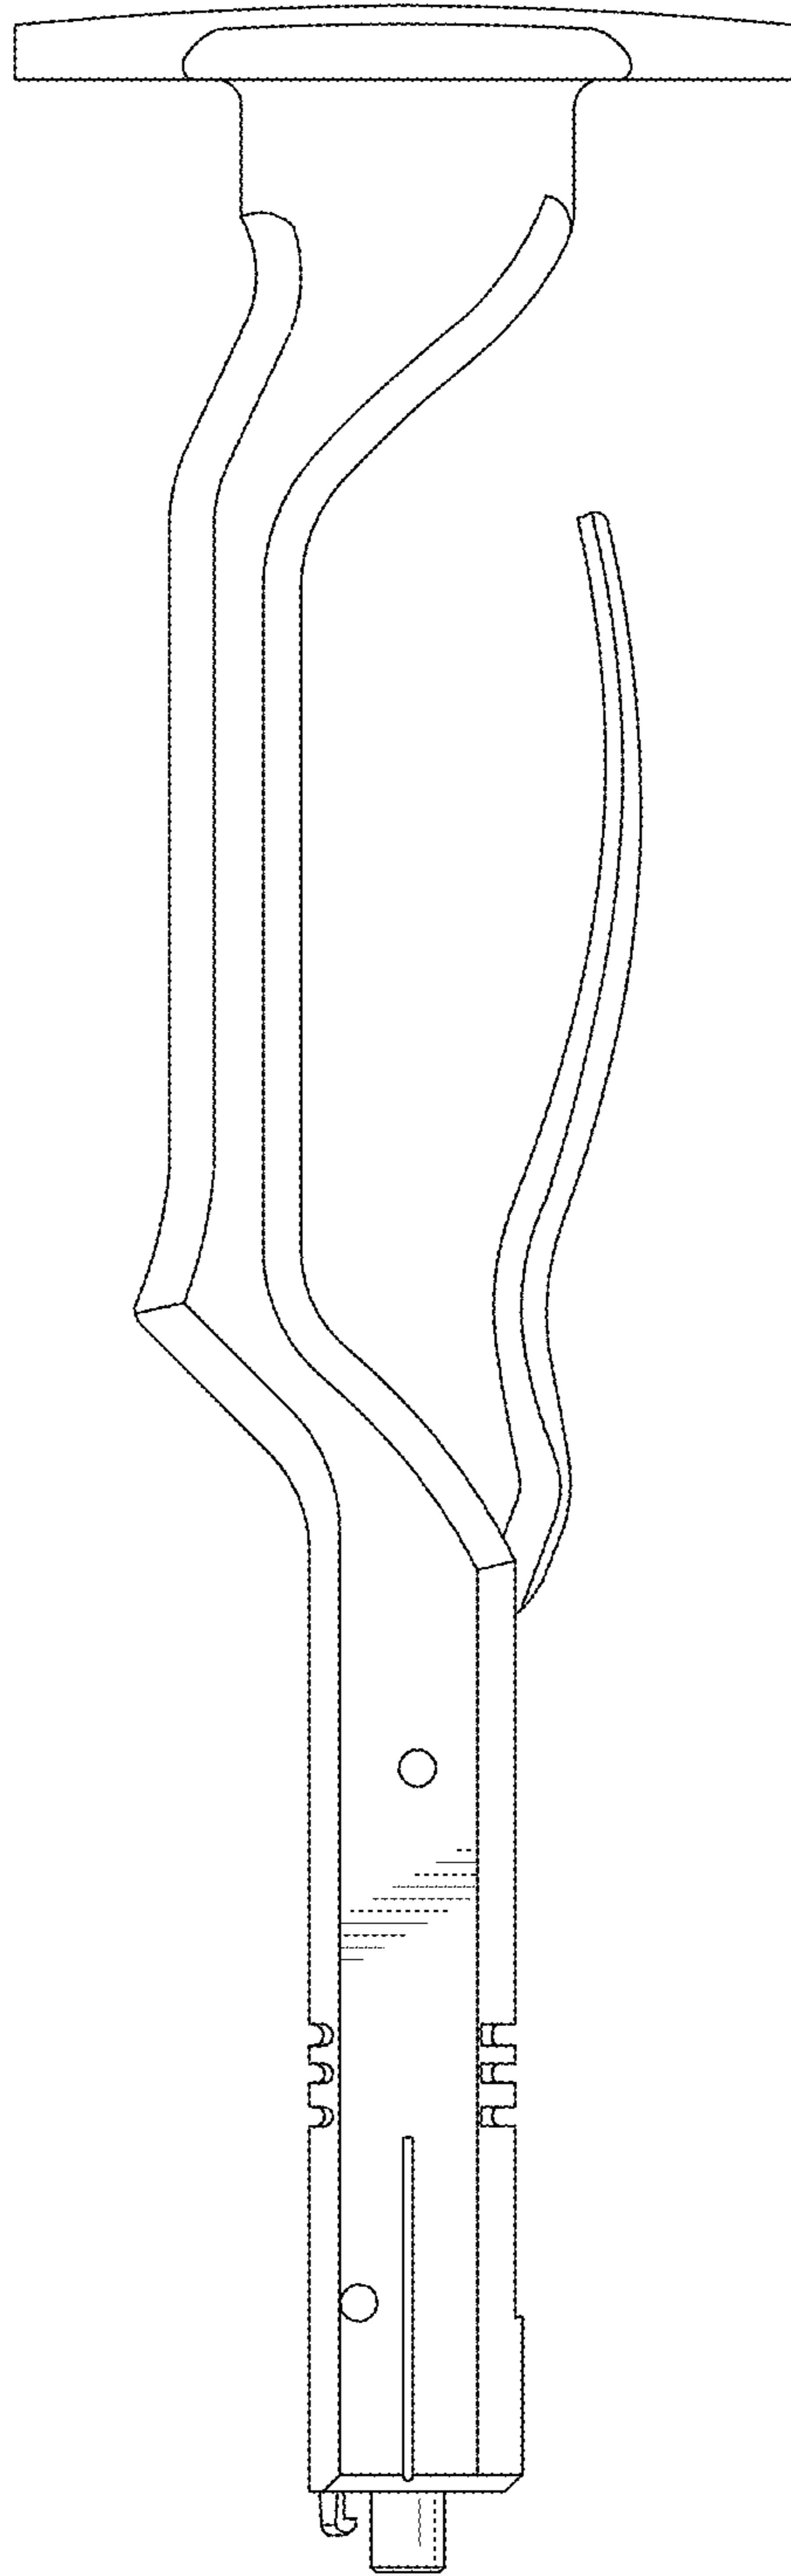


Fig. 3

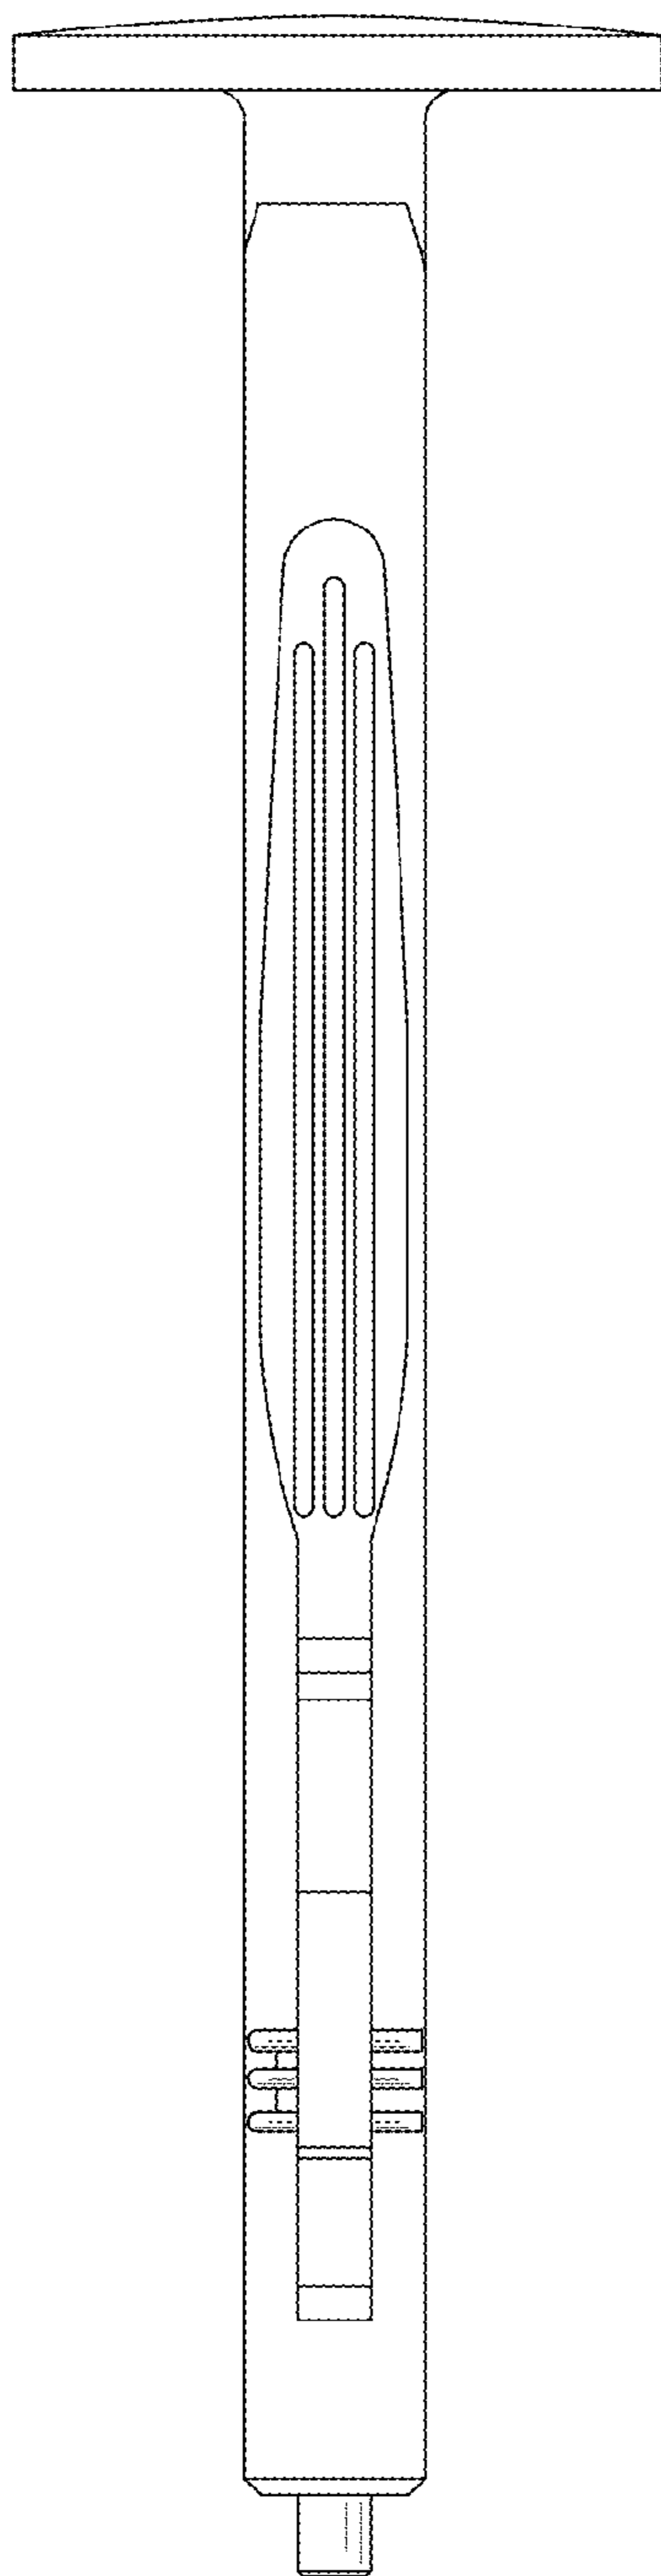


Fig. 4

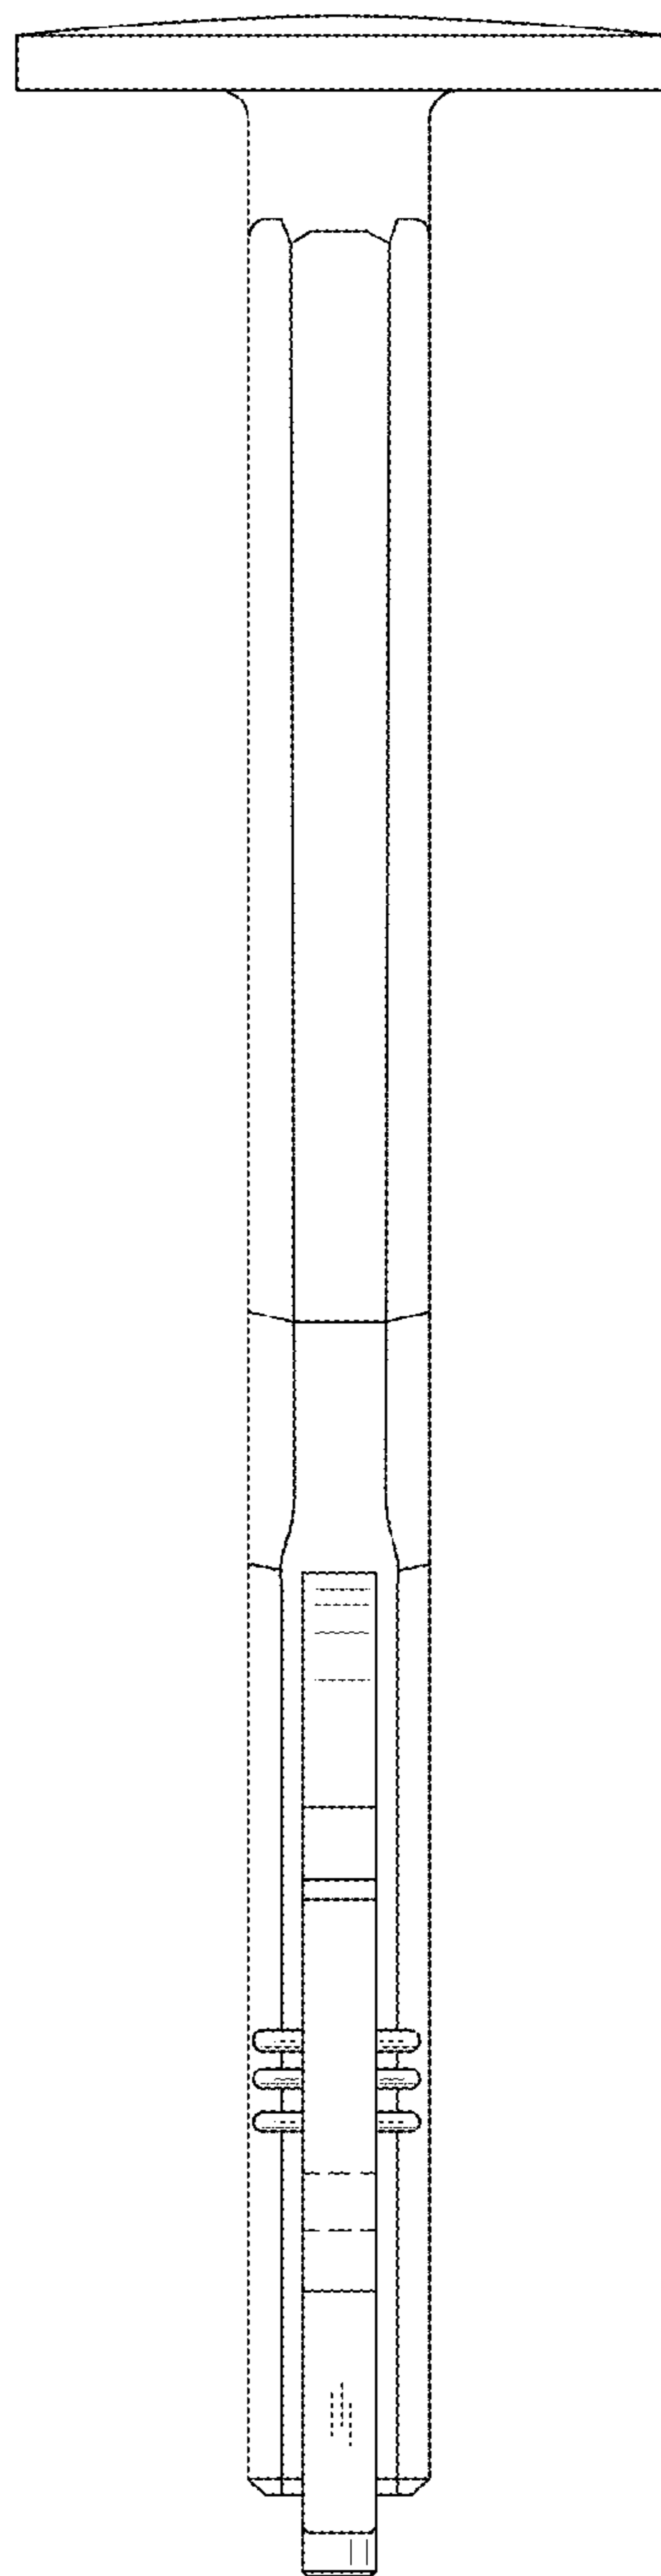


Fig. 5

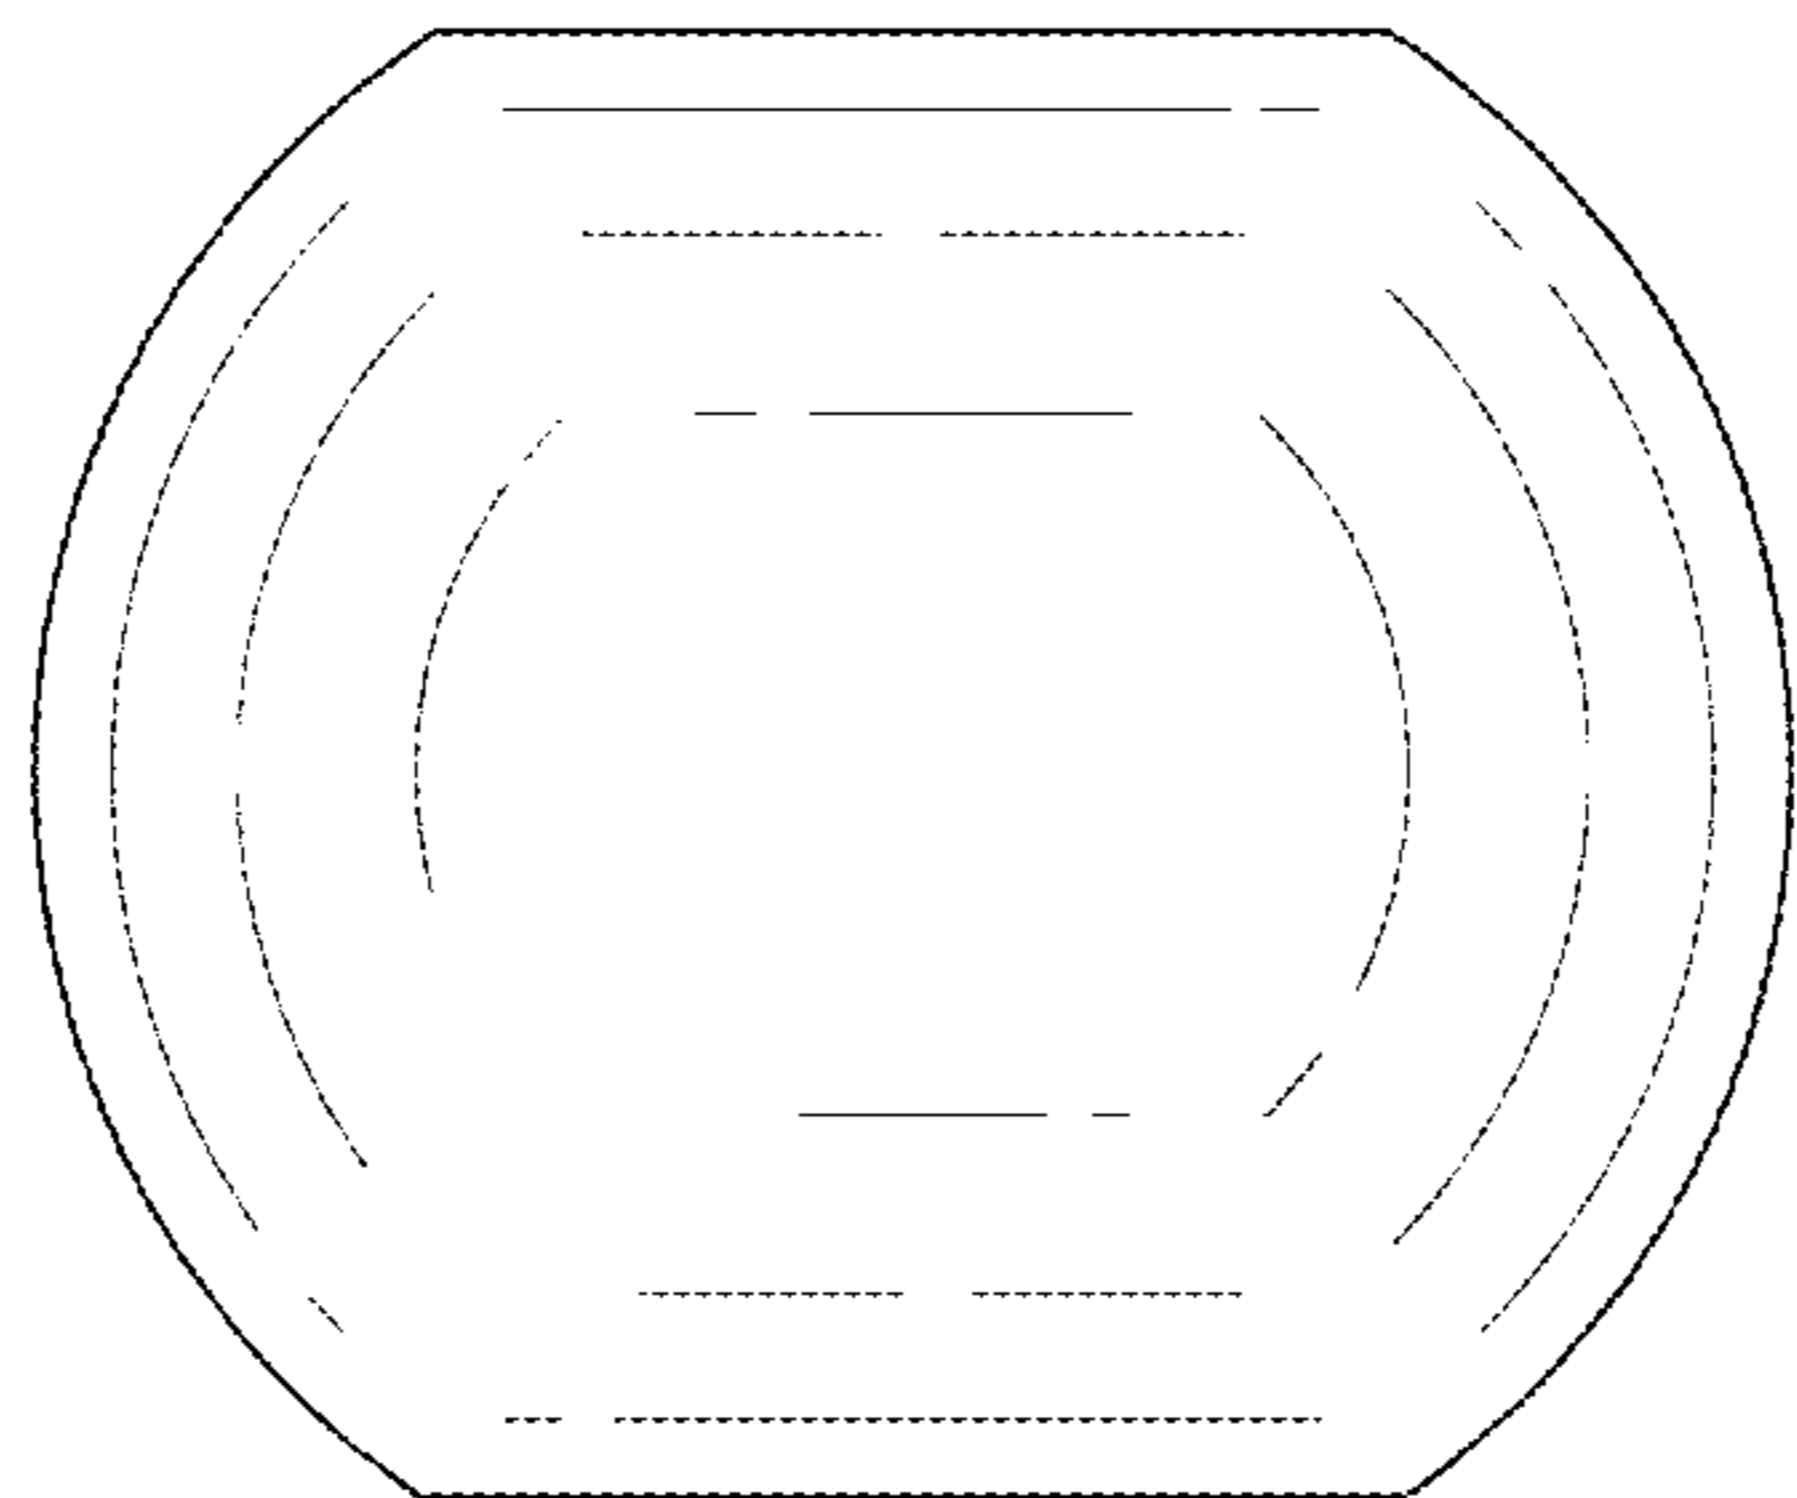


Fig. 7

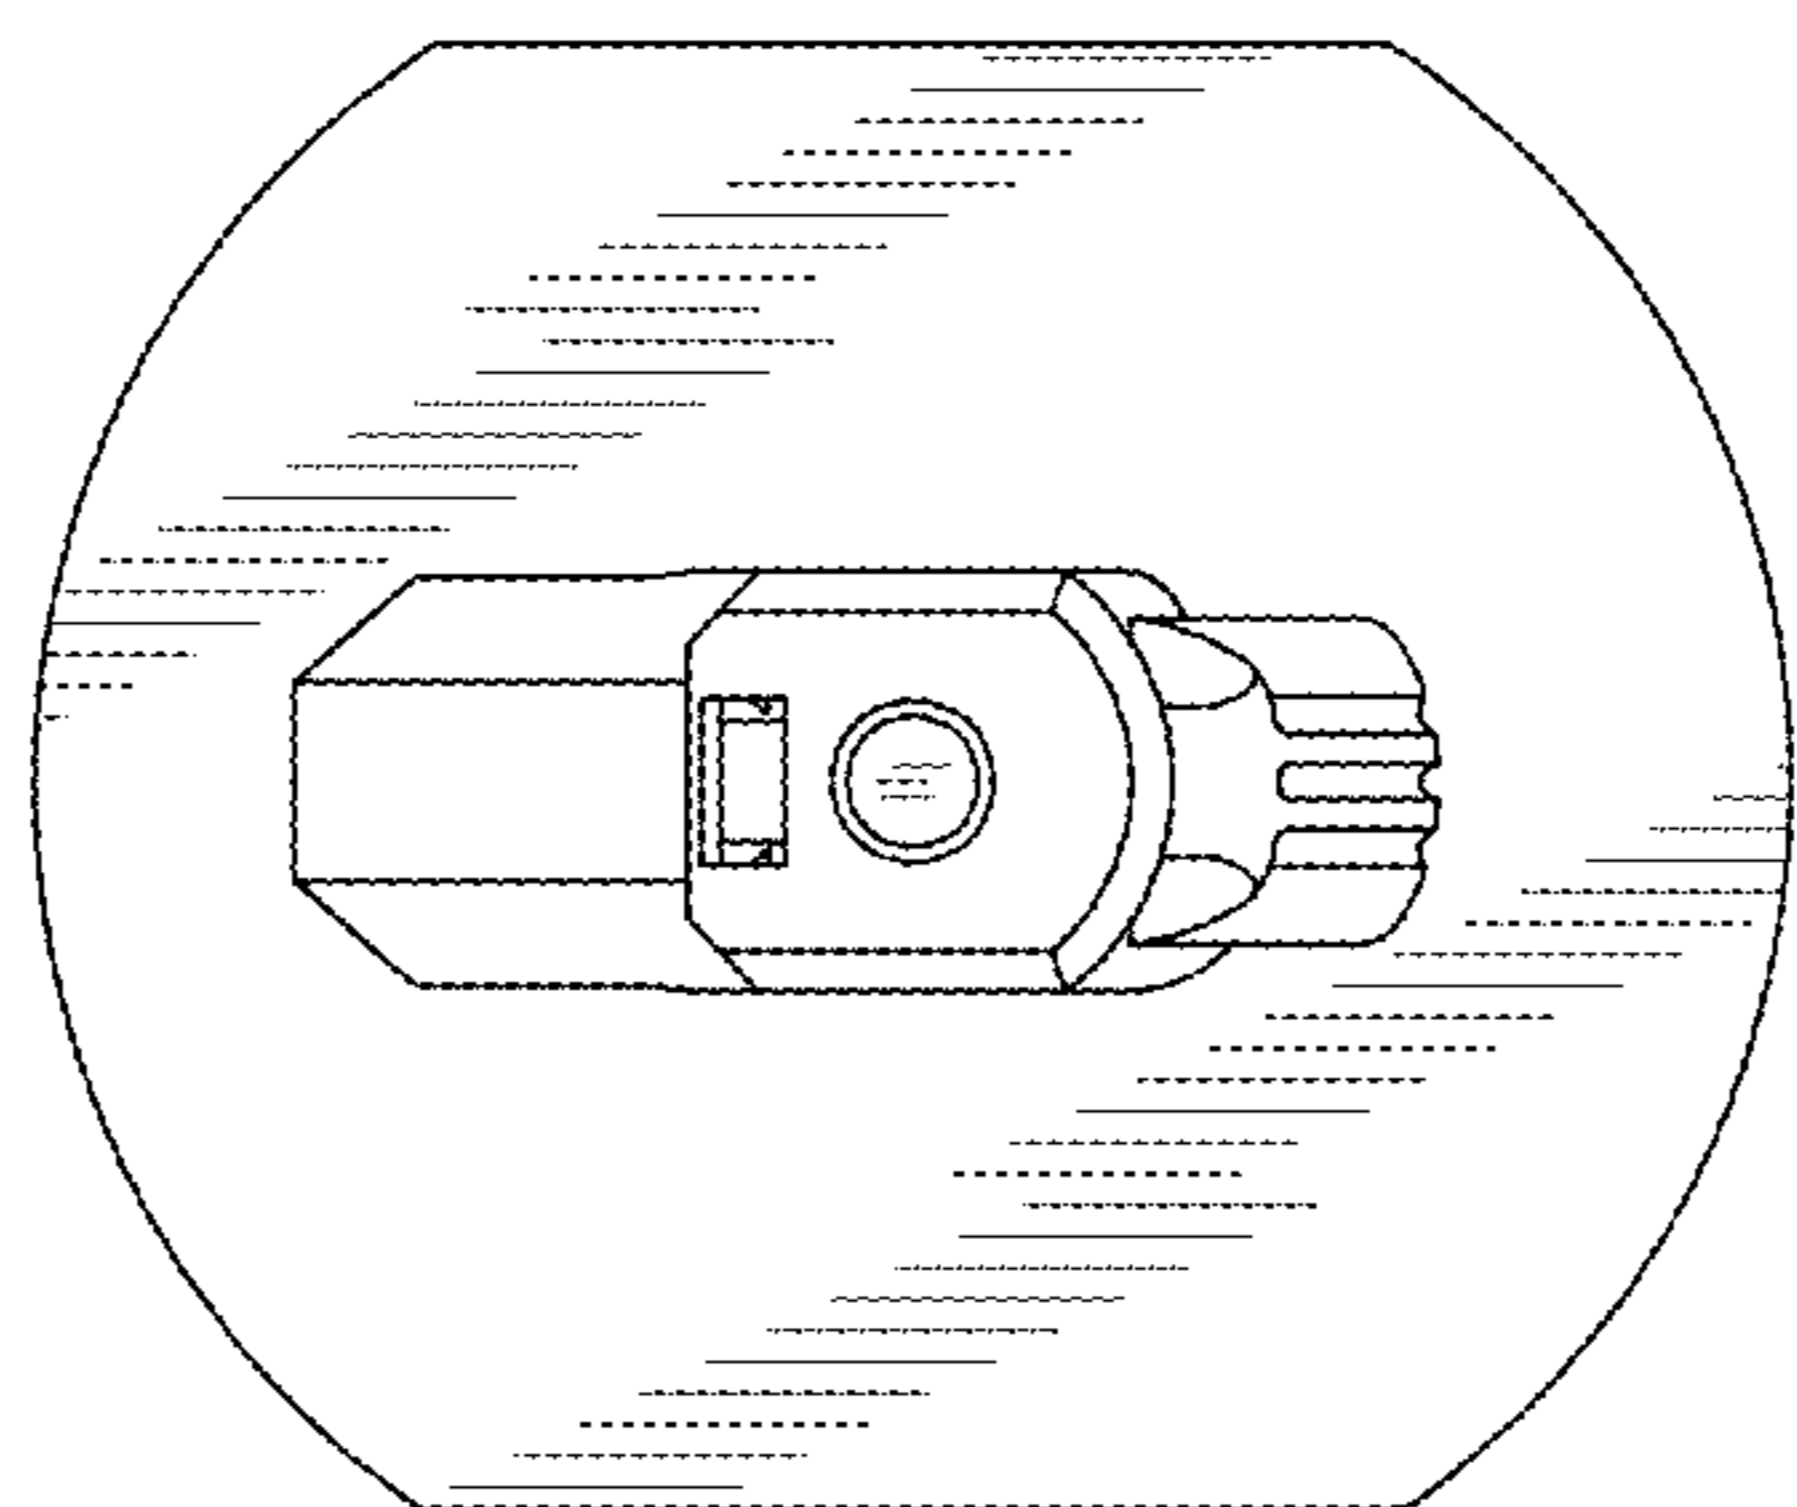


Fig. 6