



US00D725774S

(12) **United States Design Patent**  
**Lubensky et al.**

(10) **Patent No.:** **US D725,774 S**  
(45) **Date of Patent:** **\*\* Mar. 31, 2015**

(54) **SIZING ORTHOPAEDIC SURGICAL INSTRUMENT**

(71) Applicants: **Janelle M. Lubensky**, Winona Lake, IN (US); **Jeffrey M. Walcutt**, Fort Wayne, IN (US); **Rebecca L. Chaney**, Warsaw, IN (US); **Craig S. Tsukayama**, Fort Wayne, IN (US); **Jonathan C. Lee**, Mishawaka, IN (US); **Duncan G. Young**, Yorkshire (GB); **Timothy J. Phillips**, Walsall (GB)

(72) Inventors: **Janelle M. Lubensky**, Winona Lake, IN (US); **Jeffrey M. Walcutt**, Fort Wayne, IN (US); **Rebecca L. Chaney**, Warsaw, IN (US); **Craig S. Tsukayama**, Fort Wayne, IN (US); **Jonathan C. Lee**, Mishawaka, IN (US); **Duncan G. Young**, Yorkshire (GB); **Timothy J. Phillips**, Walsall (GB)

(73) Assignee: **DePuy (Ireland) (IE)**

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/457,168**

(22) Filed: **Jun. 7, 2013**

(51) **LOC (10) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/140**

(58) **Field of Classification Search**  
CPC ..... A61B 17/17; A61B 17/1725; A61F 2/46; A61F 2/4601; A61F 2/4603; A61F 2/4607; A61F 2/461  
USPC ..... D24/133, 140, 143, 144, 145, 146, 147, D24/155, 171; 606/86 R, 88, 89  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D245,918 S \* 9/1977 Shen ..... D24/140  
4,211,228 A \* 7/1980 Cloutier ..... 606/102

D449,689 S \* 10/2001 Comeau et al. .... D24/135  
D450,120 S \* 11/2001 Adler et al. .... D24/143  
6,673,077 B1 \* 1/2004 Katz ..... 606/88  
D701,302 S \* 3/2014 Jeffery ..... D24/107  
2007/0282451 A1 \* 12/2007 Metzger et al. .... 623/20.28  
2009/0125114 A1 5/2009 May et al.  
2012/0316563 A1 \* 12/2012 Metzger et al. .... 606/80  
2013/0123787 A1 \* 5/2013 Wilkinson ..... 606/88  
2013/0325014 A1 12/2013 Sordelet et al.  
2013/0325016 A1 12/2013 Sordelet et al.  
2013/0325018 A1 12/2013 Thomas et al.  
2013/0325019 A1 12/2013 Thomas et al.  
2013/0325021 A1 12/2013 Sordelet et al.  
2013/0325136 A1 12/2013 Thomas et al.  
2014/0243834 A1 \* 8/2014 Chaney et al. .... 606/88  
2014/0276838 A1 \* 9/2014 Tsukayama et al. .... 606/80

(Continued)

**OTHER PUBLICATIONS**

Zimmer NexGen LCCK, Surgical Technique for use with LCCK 4-in-1 Instrument, 2009, 52 pages.

(Continued)

*Primary Examiner* — Bridget L Eland

(74) *Attorney, Agent, or Firm* — Barnes & Thornburg LLP


(57) **CLAIM**

We claim the ornamental design for a sizing orthopaedic surgical instrument, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a sizing orthopaedic surgical instrument showing our new design;  
FIG. 2 is a front elevation view of the sizing orthopaedic surgical instrument of FIG. 1;  
FIG. 3 is a rear elevation view of the sizing orthopaedic surgical instrument of FIG. 1;  
FIG. 4 is a first side elevation view of the sizing orthopaedic surgical instrument of FIG. 1;  
FIG. 5 is a second side elevation view of the sizing orthopaedic surgical instrument of FIG. 1;  
FIG. 6 is a top plan view of the sizing orthopaedic surgical instrument of FIG. 1; and,  
FIG. 7 is a bottom plan view of the sizing orthopaedic surgical instrument of FIG. 1.

**1 Claim, 5 Drawing Sheets**

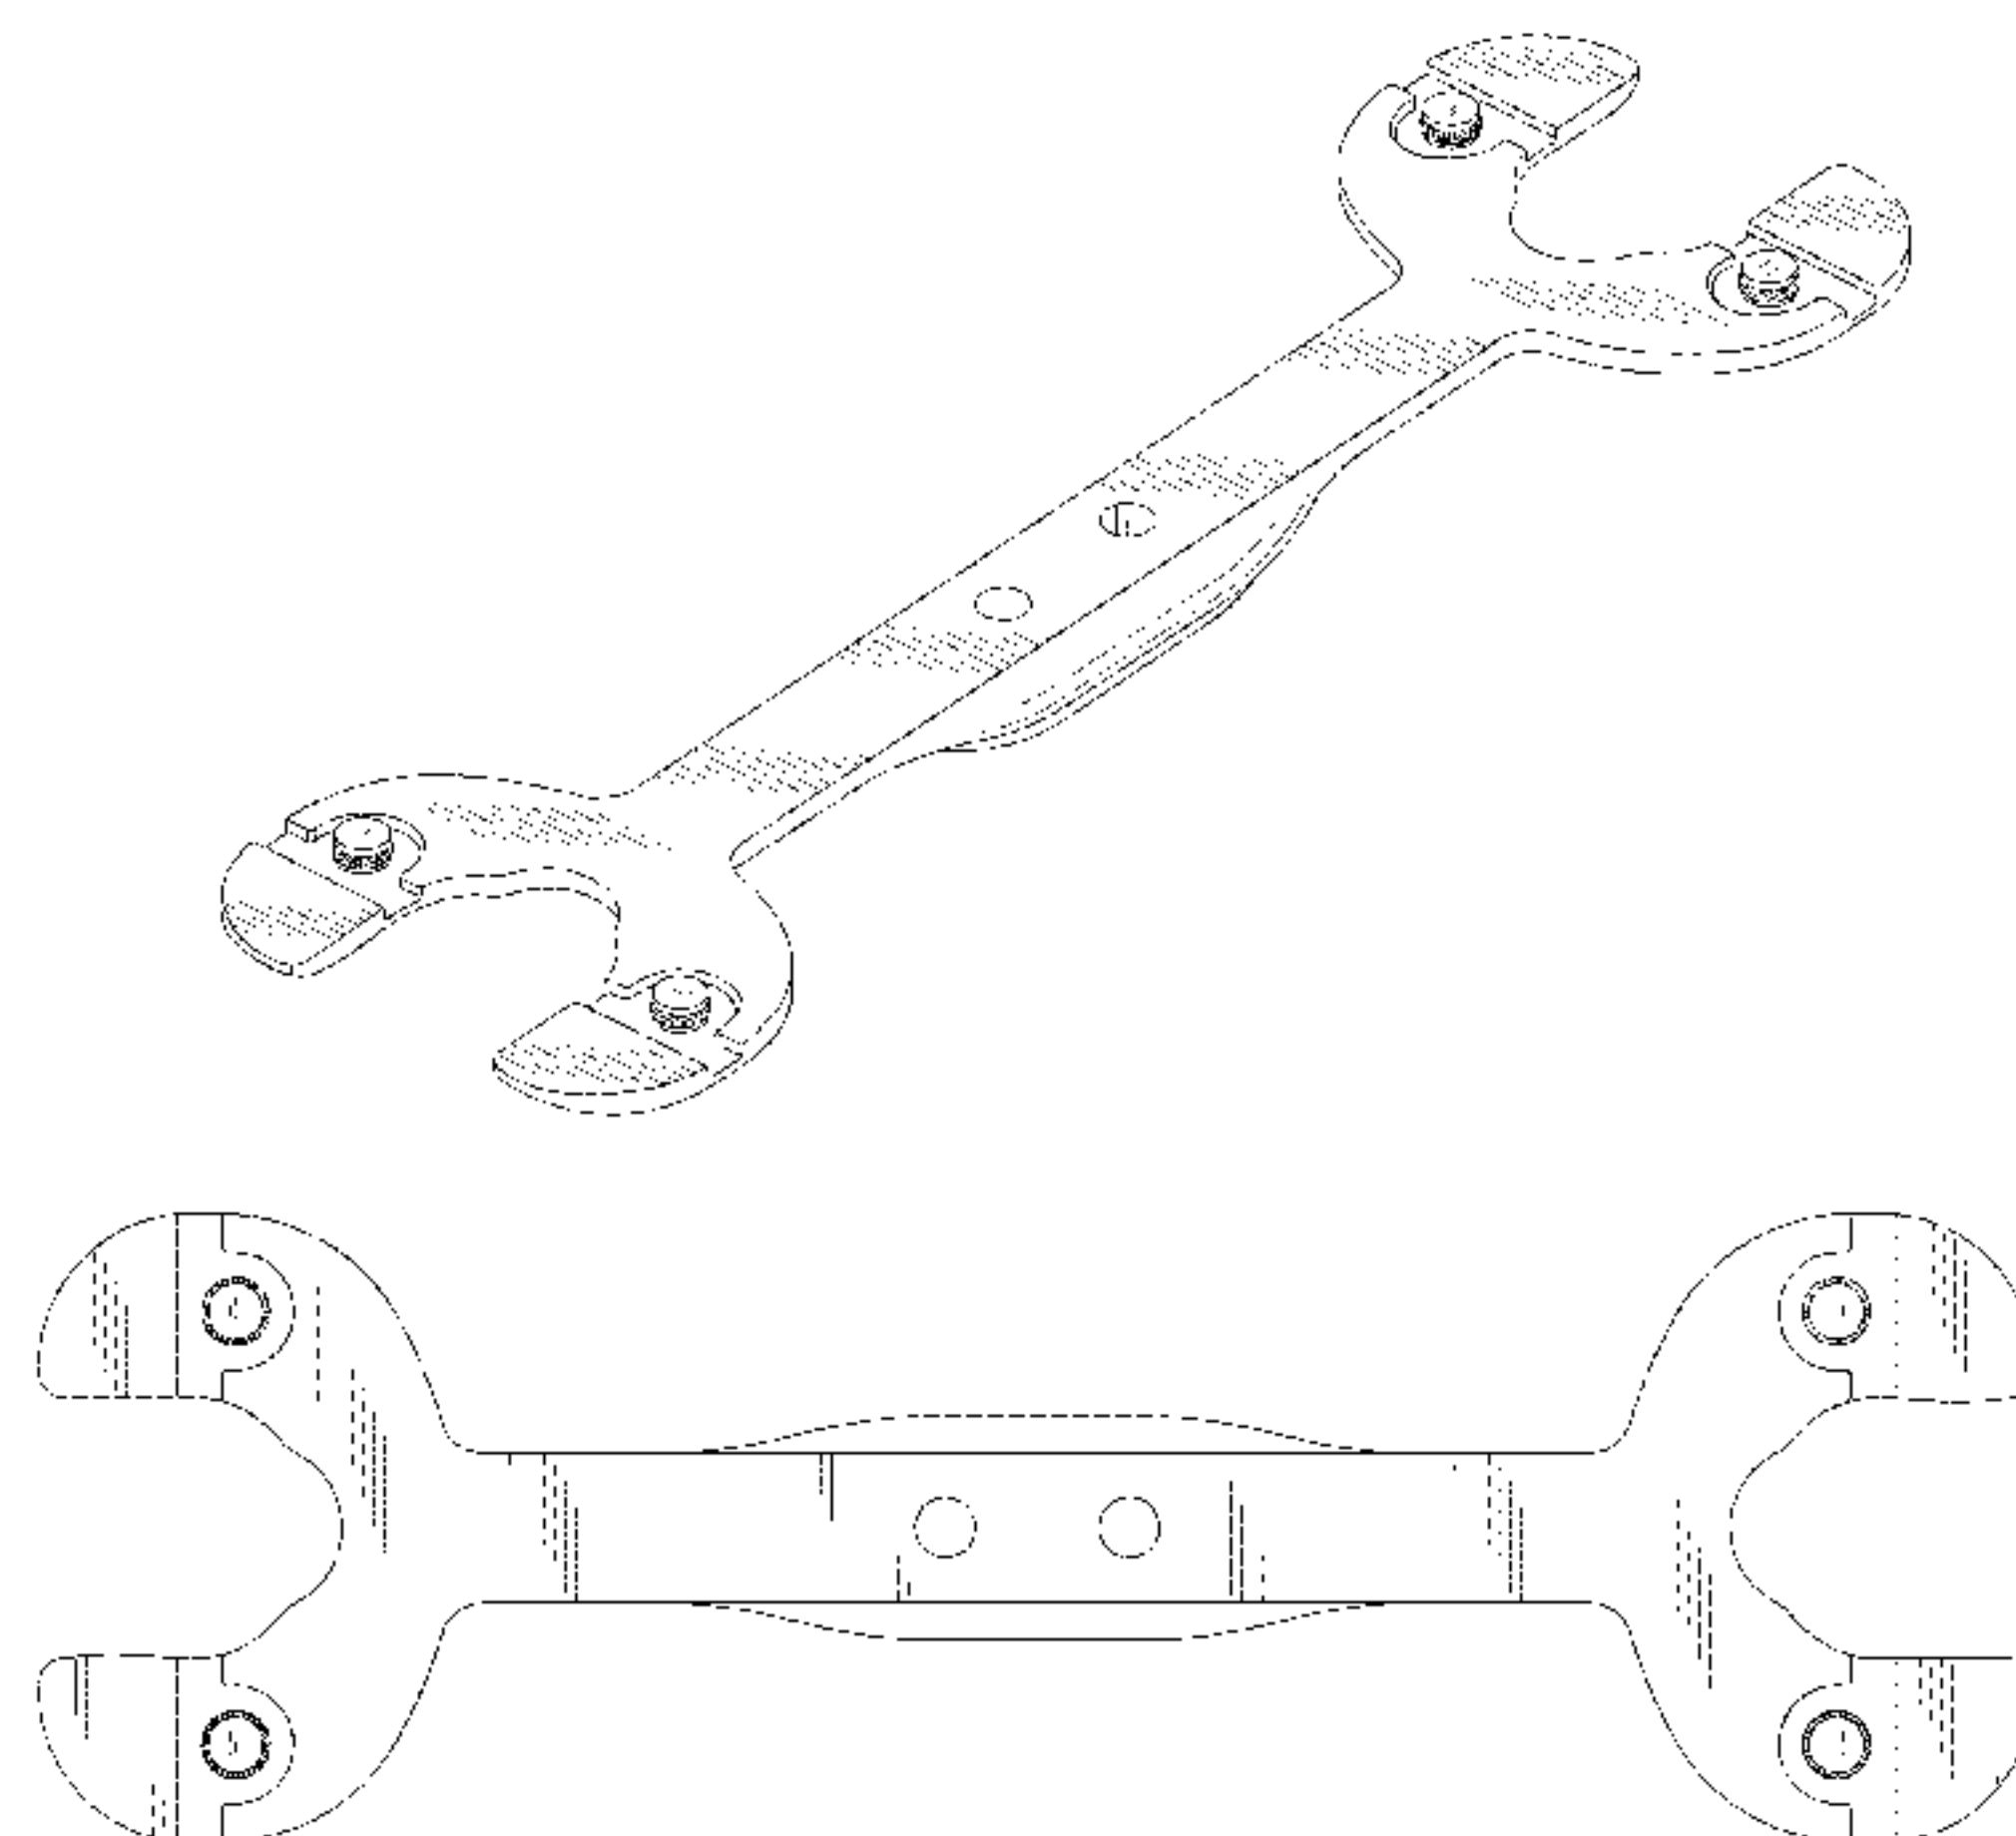

(56)

**References Cited**

U.S. PATENT DOCUMENTS

2014/0276850 A1\* 9/2014 Chaney et al. .... 606/84  
2014/0276859 A1\* 9/2014 Chaney et al. .... 606/88

OTHER PUBLICATIONS

DePuy Orthopaedics, Inc., Sigma Revision and M.B.T. Revision Tray, Surgical Technique, 2008, 82 pages.  
Smith & Nephew, Legion, Revision Knee System, Surgical Technique, 2005, 40 pages.  
Biomet, Vanguard SSK, Revision System, Surgical Technique, Feb. 2008, 64 pages.

GMK Revision, Surgical Technique, Ref. 99.27.12US rev. 1, 1999, 74 pages.  
PFC Sigma RP-F, Specialist 2 Instruments, Surgical Technique, Performance in Flexion, 2007, 32 pages.  
P.F.C. Sigma Rotating Platform Knee System with M.B.T Tray, Primary Procedure with a Curved or Posterior Stabilised Implant, 2003, 43 pages.  
LCS High Performance Instruments, Surgical Technique, 2008, 44 pages.  
Sigma High Performance Instruments, Design Rationale, 2007, 12 pages.  
Sigma High Performance Instruments, Classic Surgical Technique, 2010, 52 pages.  
Attune Knee System Surgical Technique, 2013, 73 pages.

\* cited by examiner

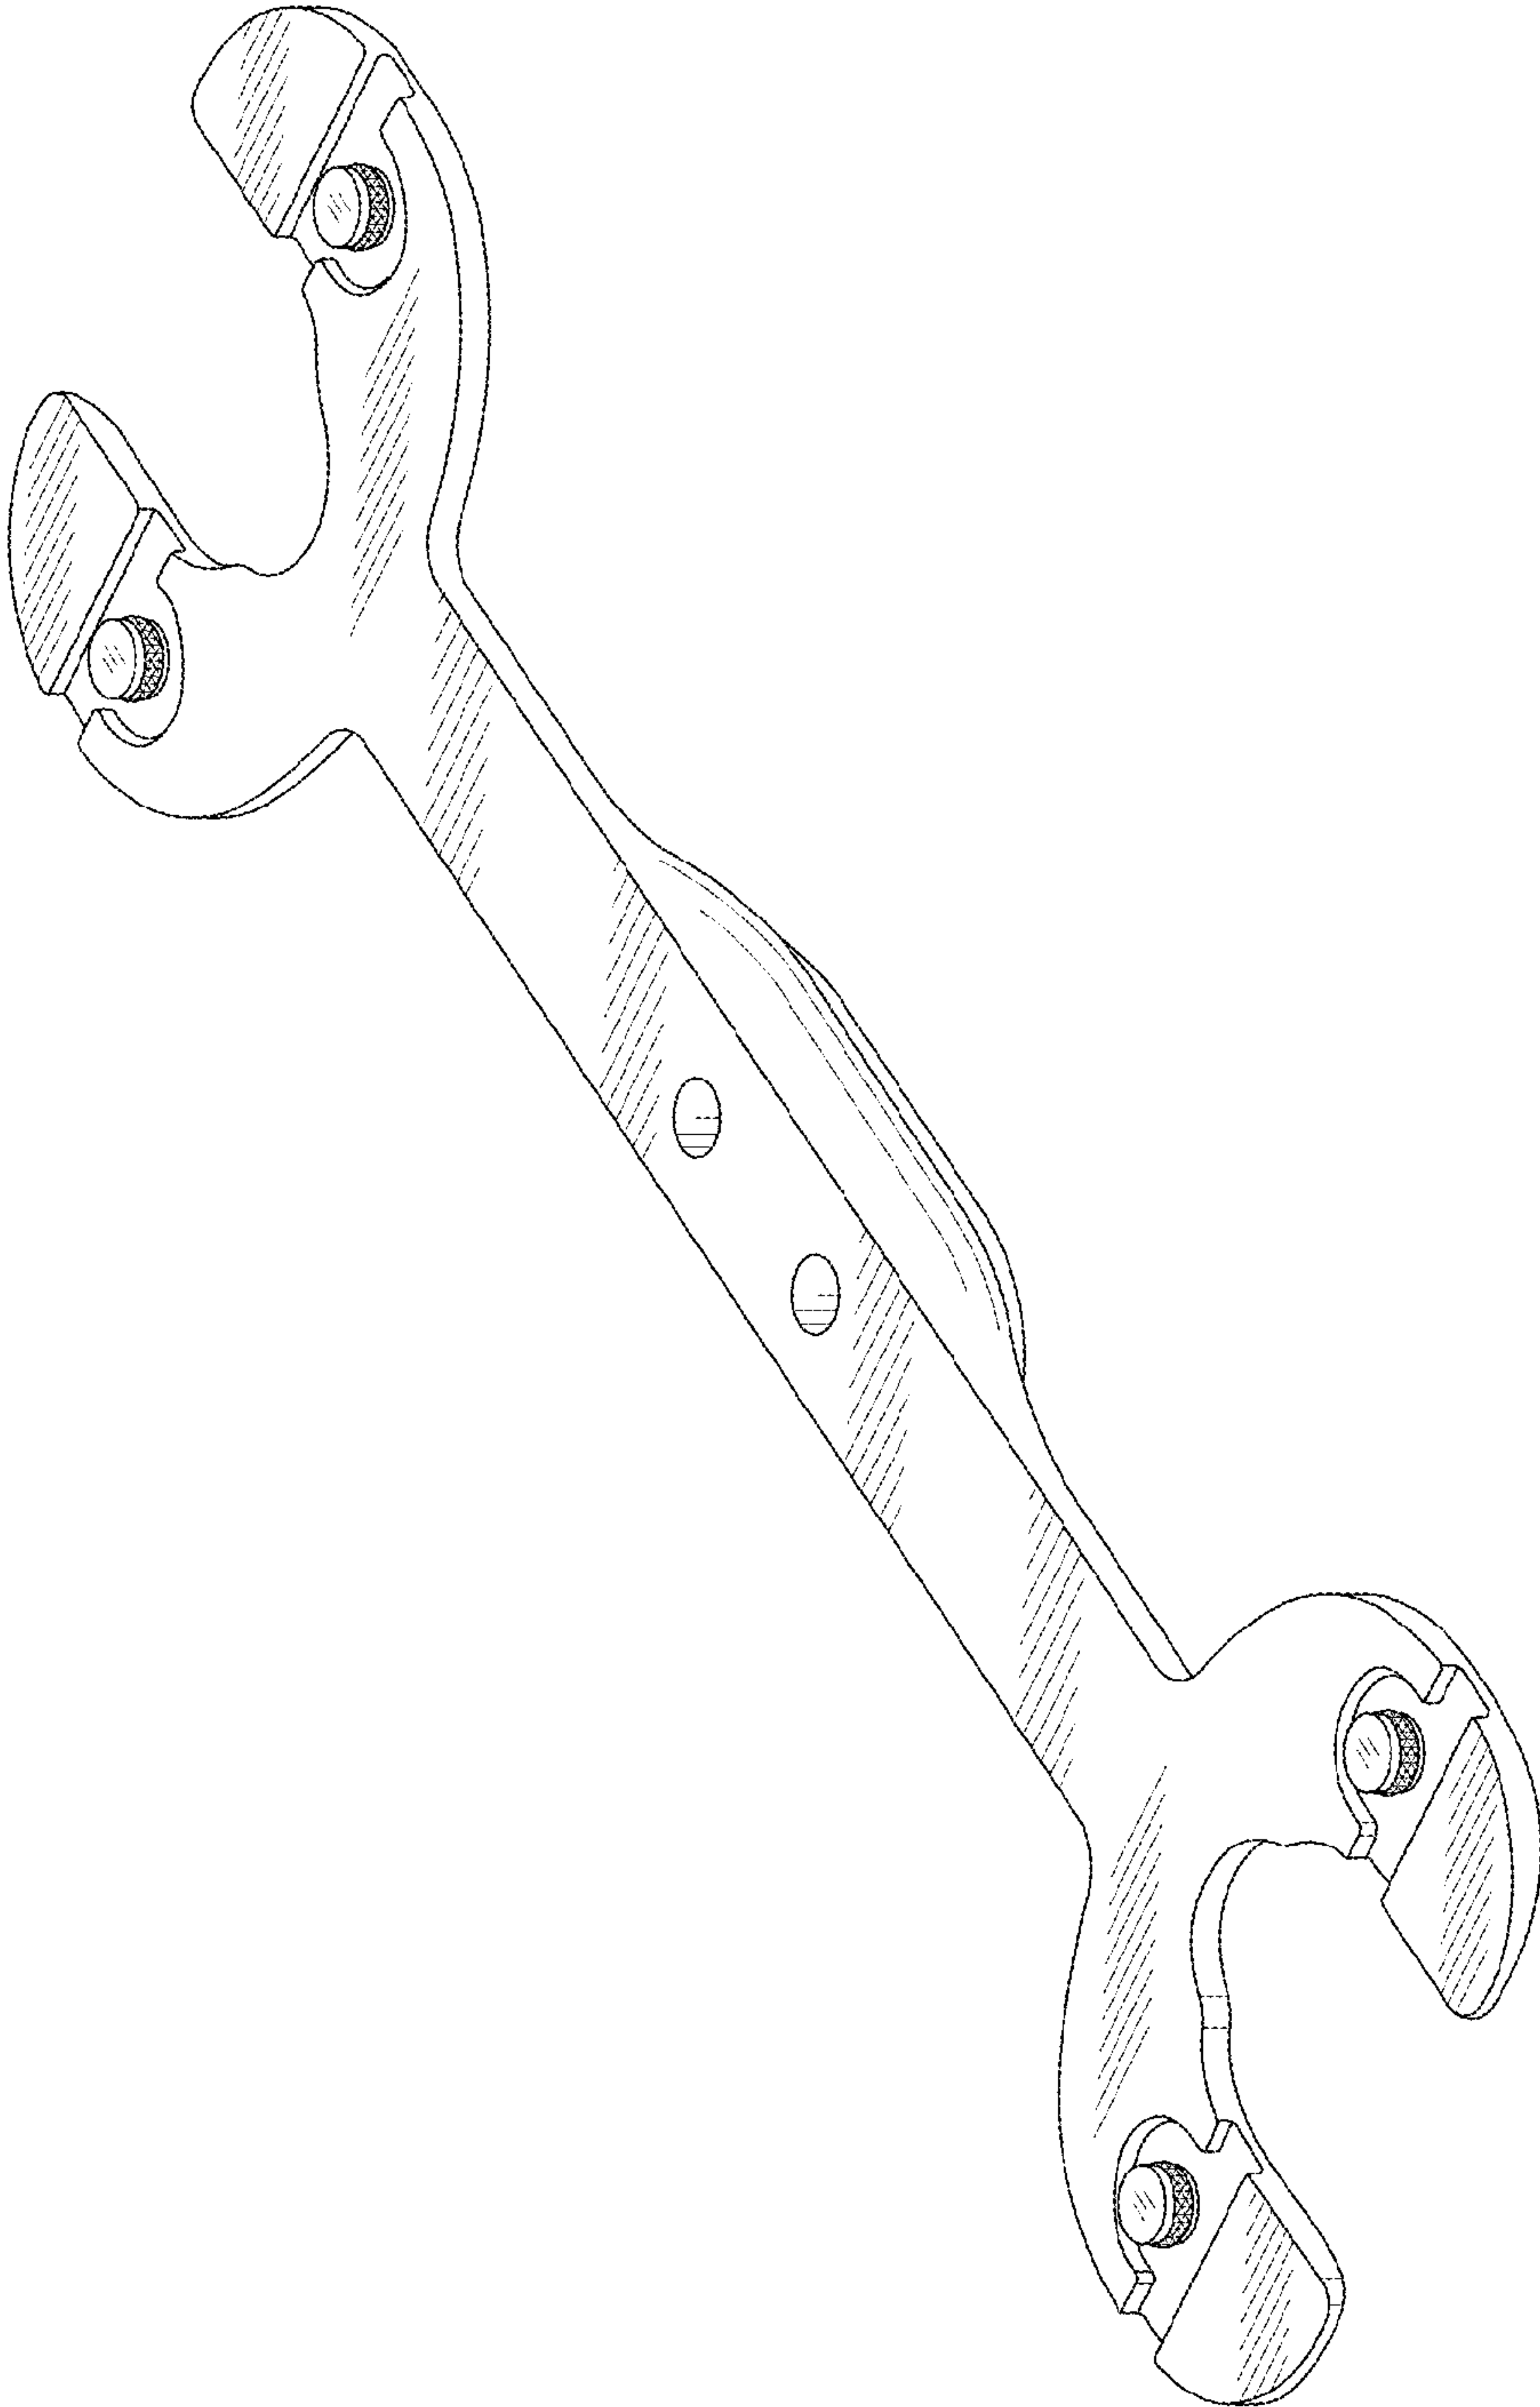


Fig. 1

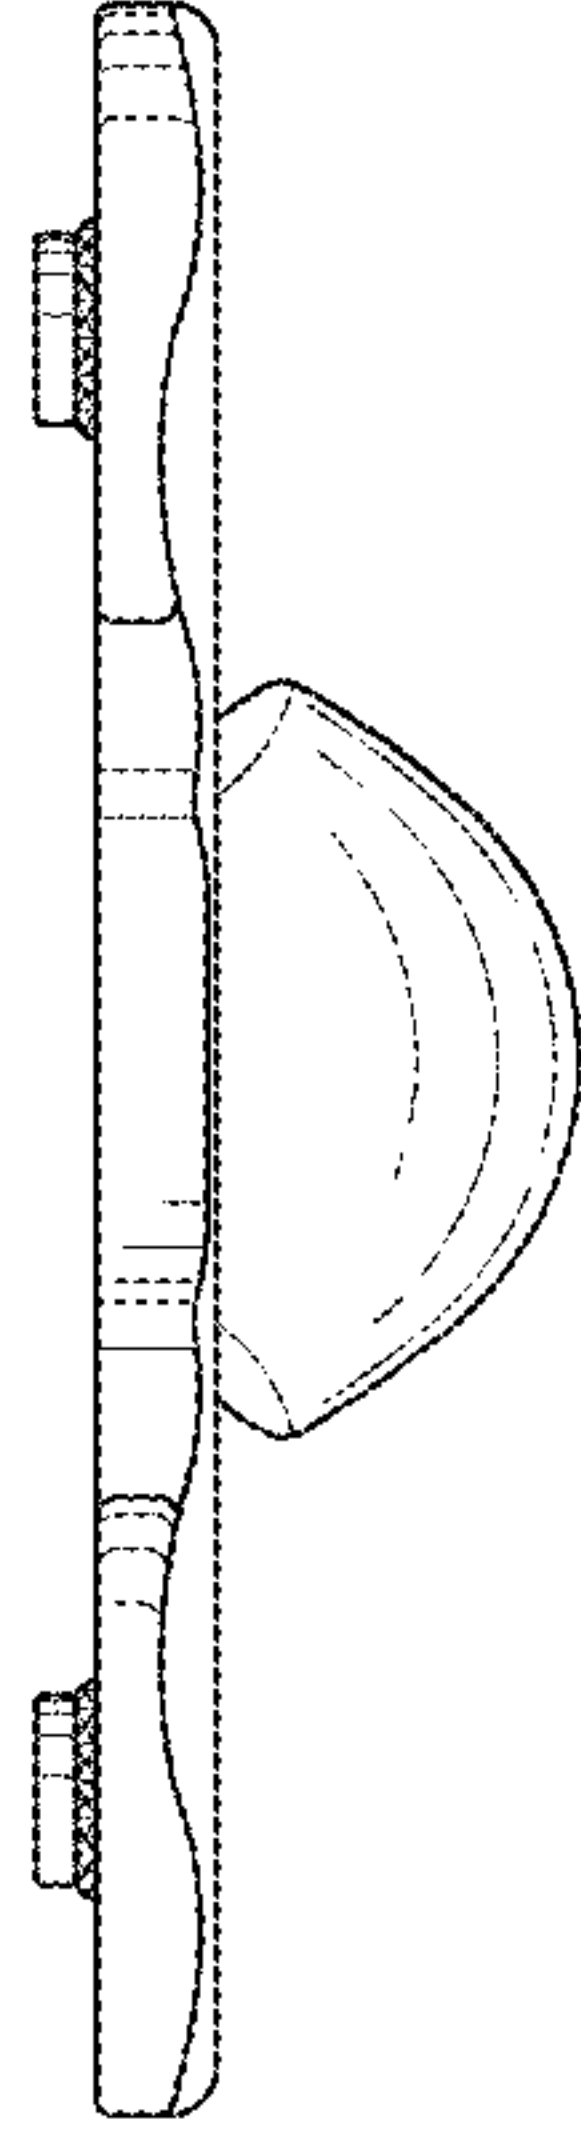


Fig. 3

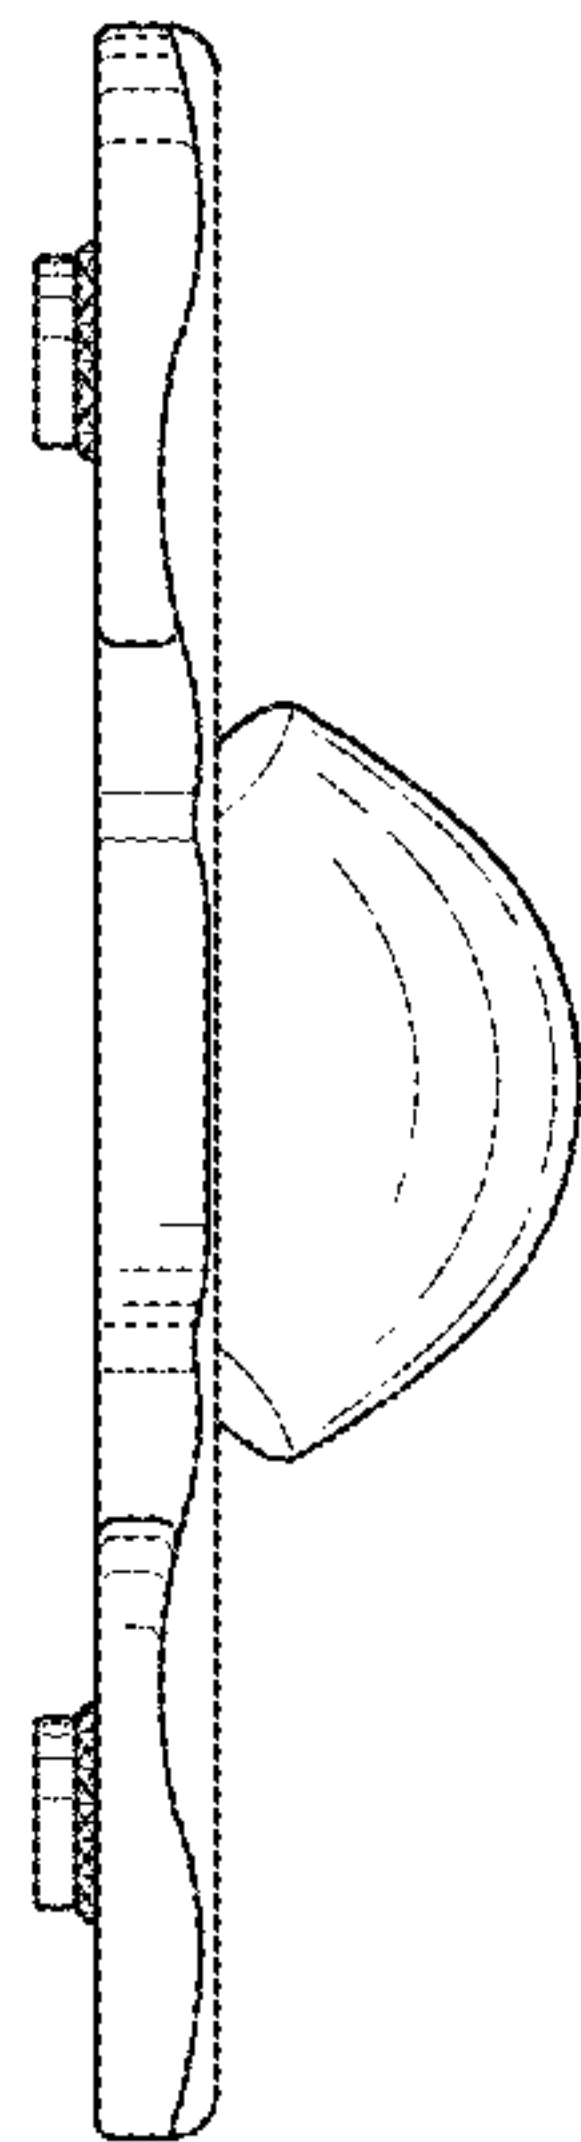


Fig. 2

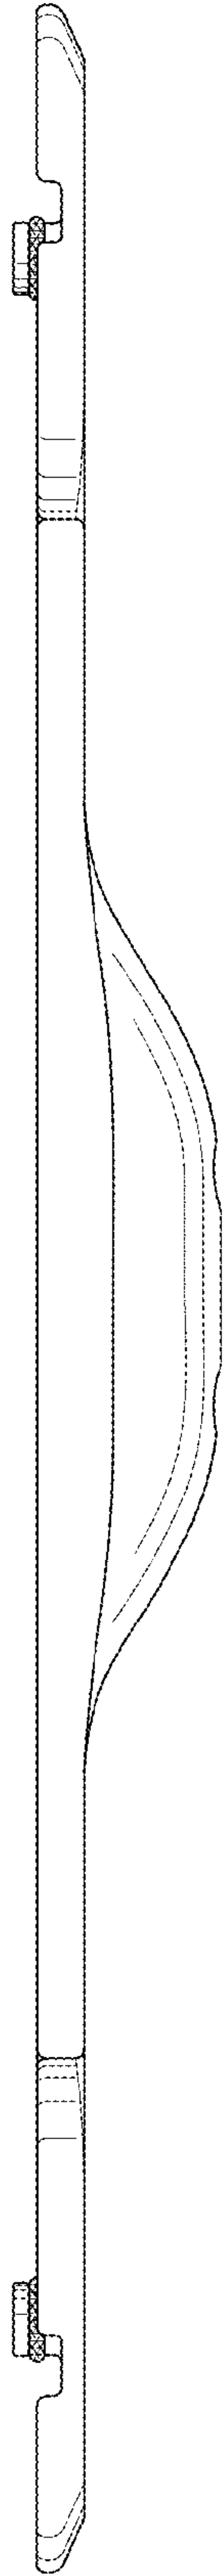


Fig. 4

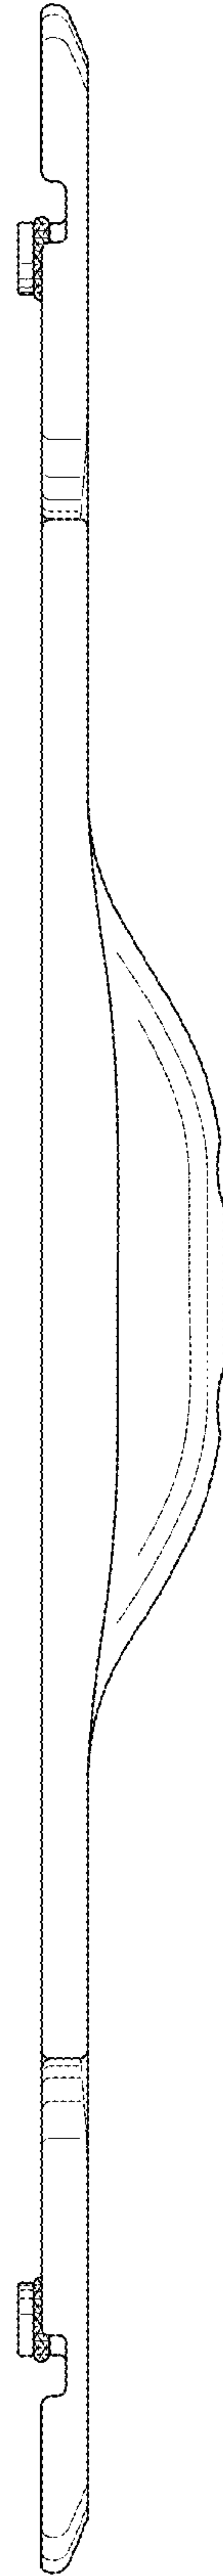


Fig. 5

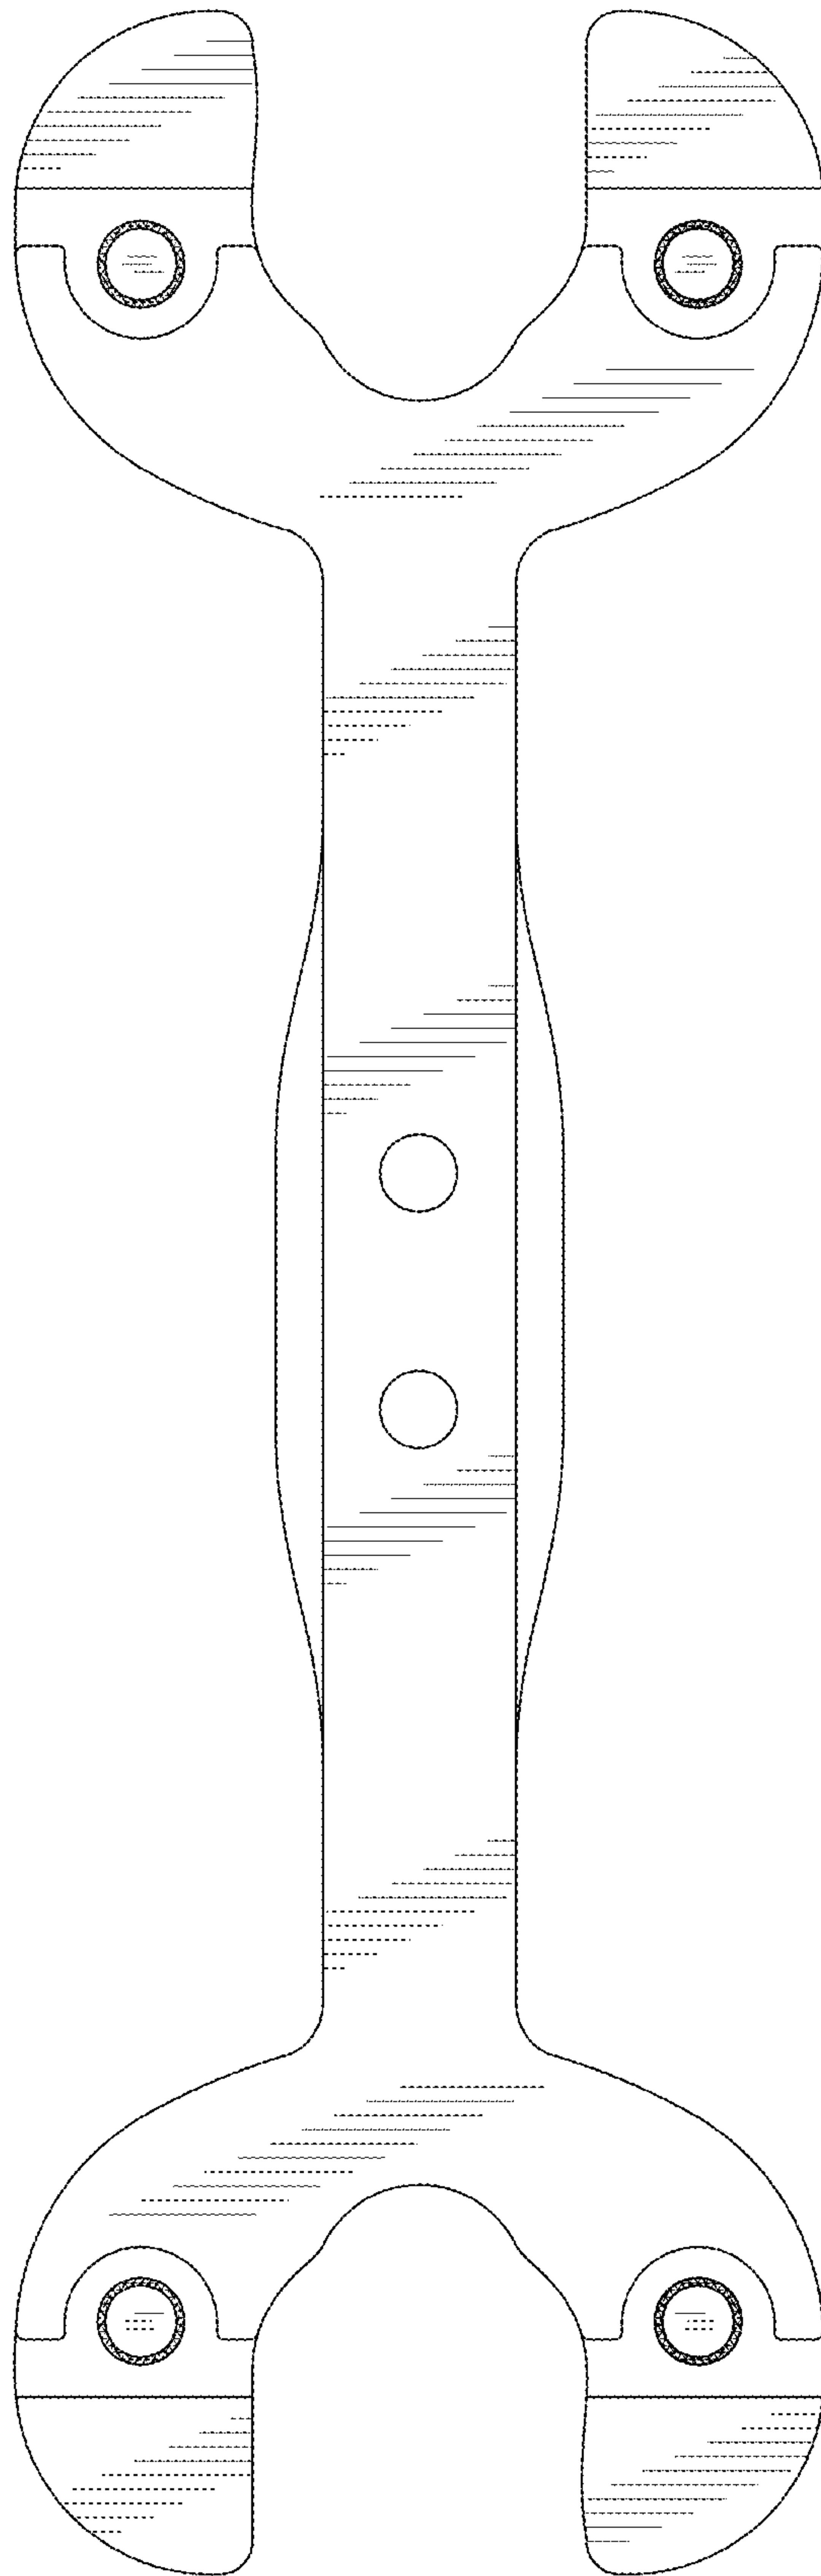


Fig. 6



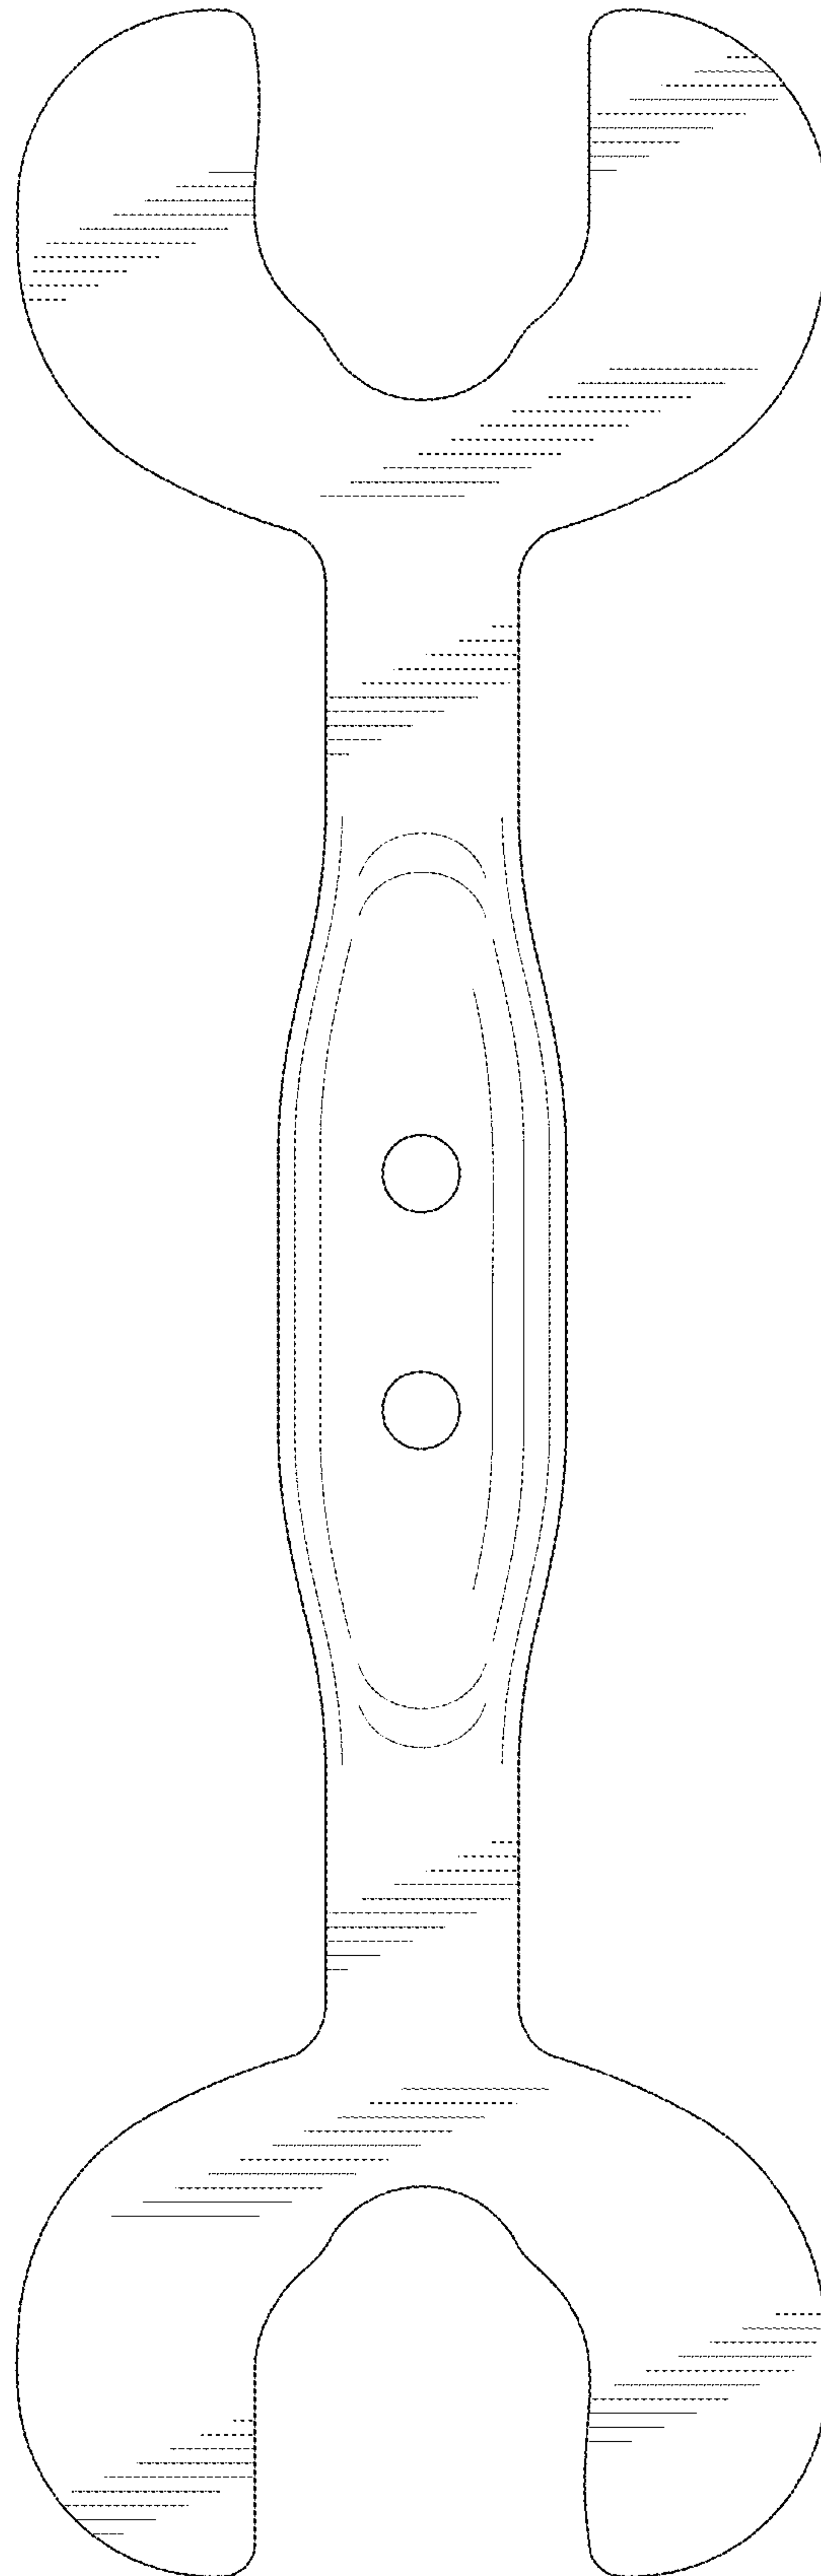


Fig. 7