



US00D726321S

(12) **United States Design Patent**  
**Jackson**

(10) **Patent No.:** **US D726,321 S**

(45) **Date of Patent:** **\*\* Apr. 7, 2015**

(54) **GLYCAEMIC ASSESSMENT TEST DEVICE**

(56)

**References Cited**

U.S. PATENT DOCUMENTS

(71) Applicant: **Smartsensor Telemed Limited**,  
Abingdon, Oxfordshire (GB)

(72) Inventor: **James Jackson**, Cliddesden (GB)

(73) Assignee: **Smartsensor Telemed Limited**,  
Abingdon, Oxfordshire (GB)

(\*\*) Term: **14 Years**

D598,126	S *	8/2009	Alvarez-Icaza et al. ....	D24/225
7,901,875	B2 *	3/2011	Stiene .....	435/4
7,947,490	B2 *	5/2011	Jackson .....	435/287.2
8,196,374	B2 *	6/2012	Chan et al. ....	53/426
D663,223	S *	7/2012	Wang .....	D10/81
2006/0030789	A1 *	2/2006	Allen .....	600/583
2006/0079810	A1 *	4/2006	Patel et al. ....	600/583
2008/0053222	A1 *	3/2008	Ehrensvar et al. ....	73/431
2010/0240079	A1 *	9/2010	Jackson .....	435/14
2013/0050459	A1 *	2/2013	Fan et al. ....	348/77

\* cited by examiner

Primary Examiner — Anhdao Doan

(21) Appl. No.: **29/447,562**

(22) Filed: **Mar. 5, 2013**

(51) **LOC (10) Cl.** ..... **24-01**

(52) **U.S. Cl.**

USPC ..... **D24/169**

(58) **Field of Classification Search**

USPC ..... D24/216, 223, 231, 232, 107, 169, 186;  
D10/81; 600/309, 365, 368, 583, 584;  
435/287.1, 287.2, 288.4, 810; 422/55,  
422/56, 57, 58


See application file for complete search history.

(57) **CLAIM**  
The ornamental design for a glycaemic assessment test device, as shown and described.

**DESCRIPTION**

FIG. 1 is a front view of a glycaemic assessment test device showing my new design;  
FIG. 2 is a perspective view thereof;  
FIG. 3 is a left side view thereof; and,  
FIG. 4 is a rear view thereof.  
The parts shown as broken lines in FIGS. 1 and 2 represent either an actual perforation in the sheet which sits on top of the device casing, or is a dotted or hatched printed line.

**1 Claim, 4 Drawing Sheets**

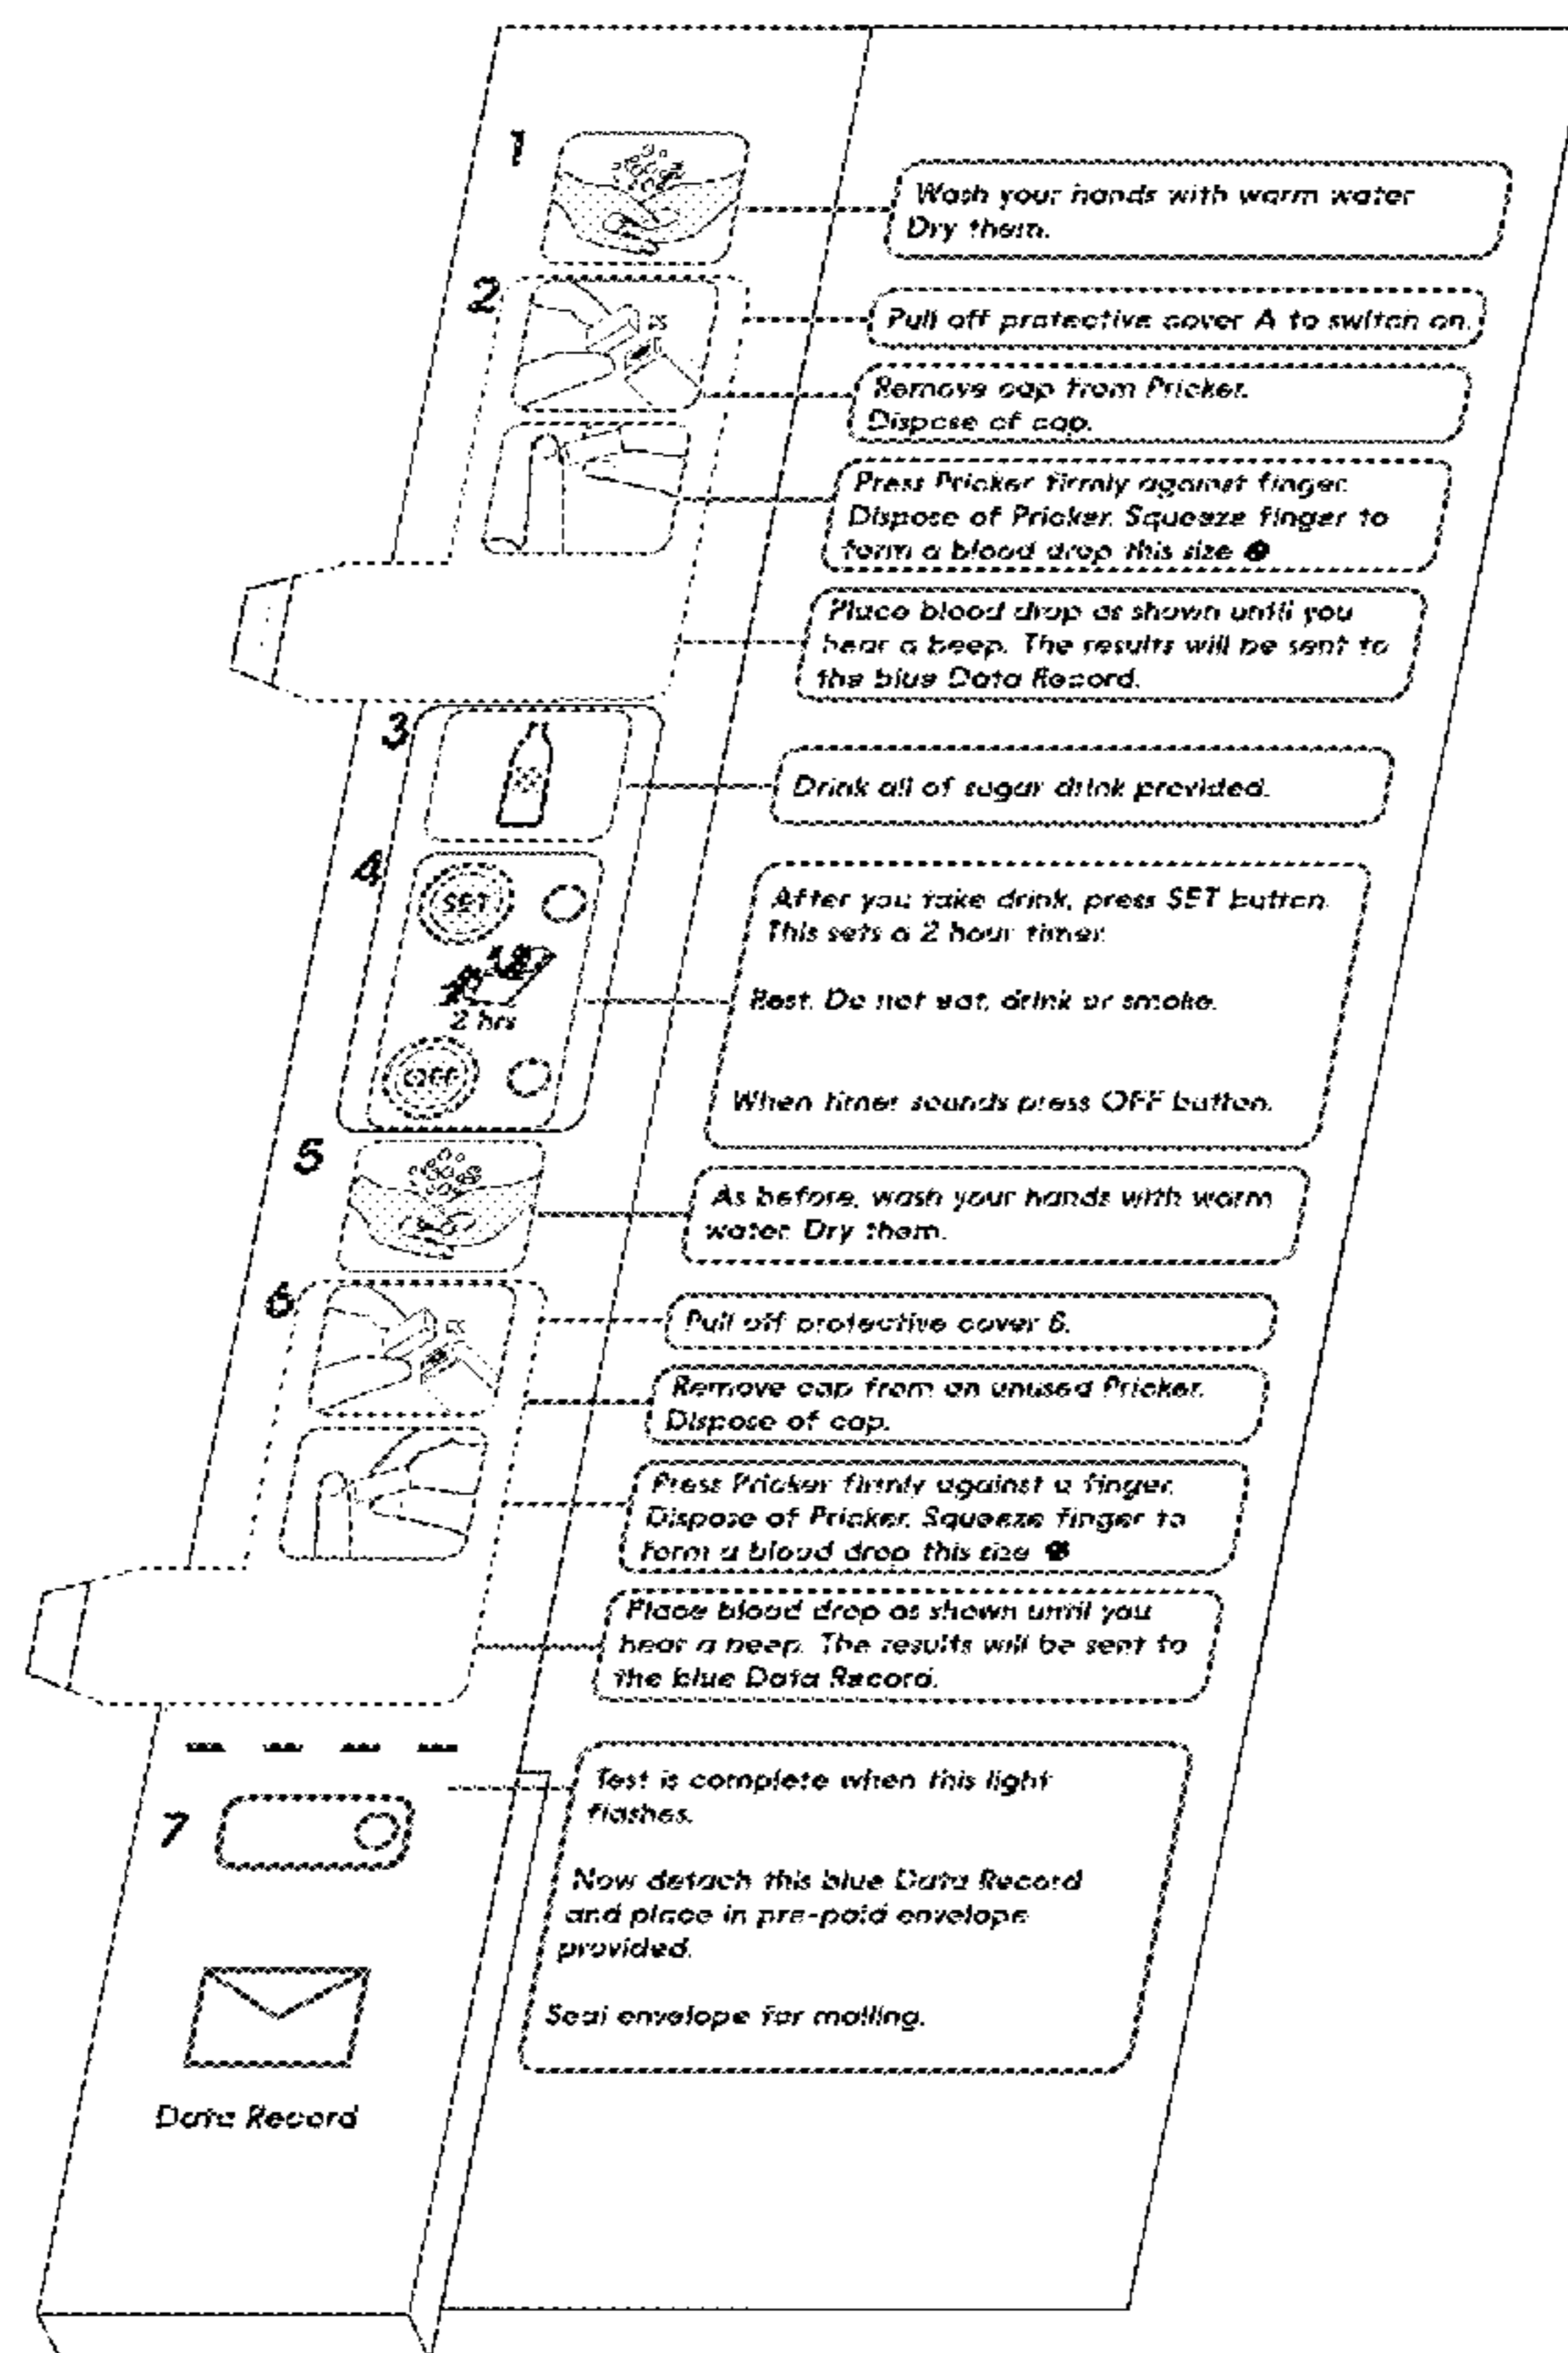

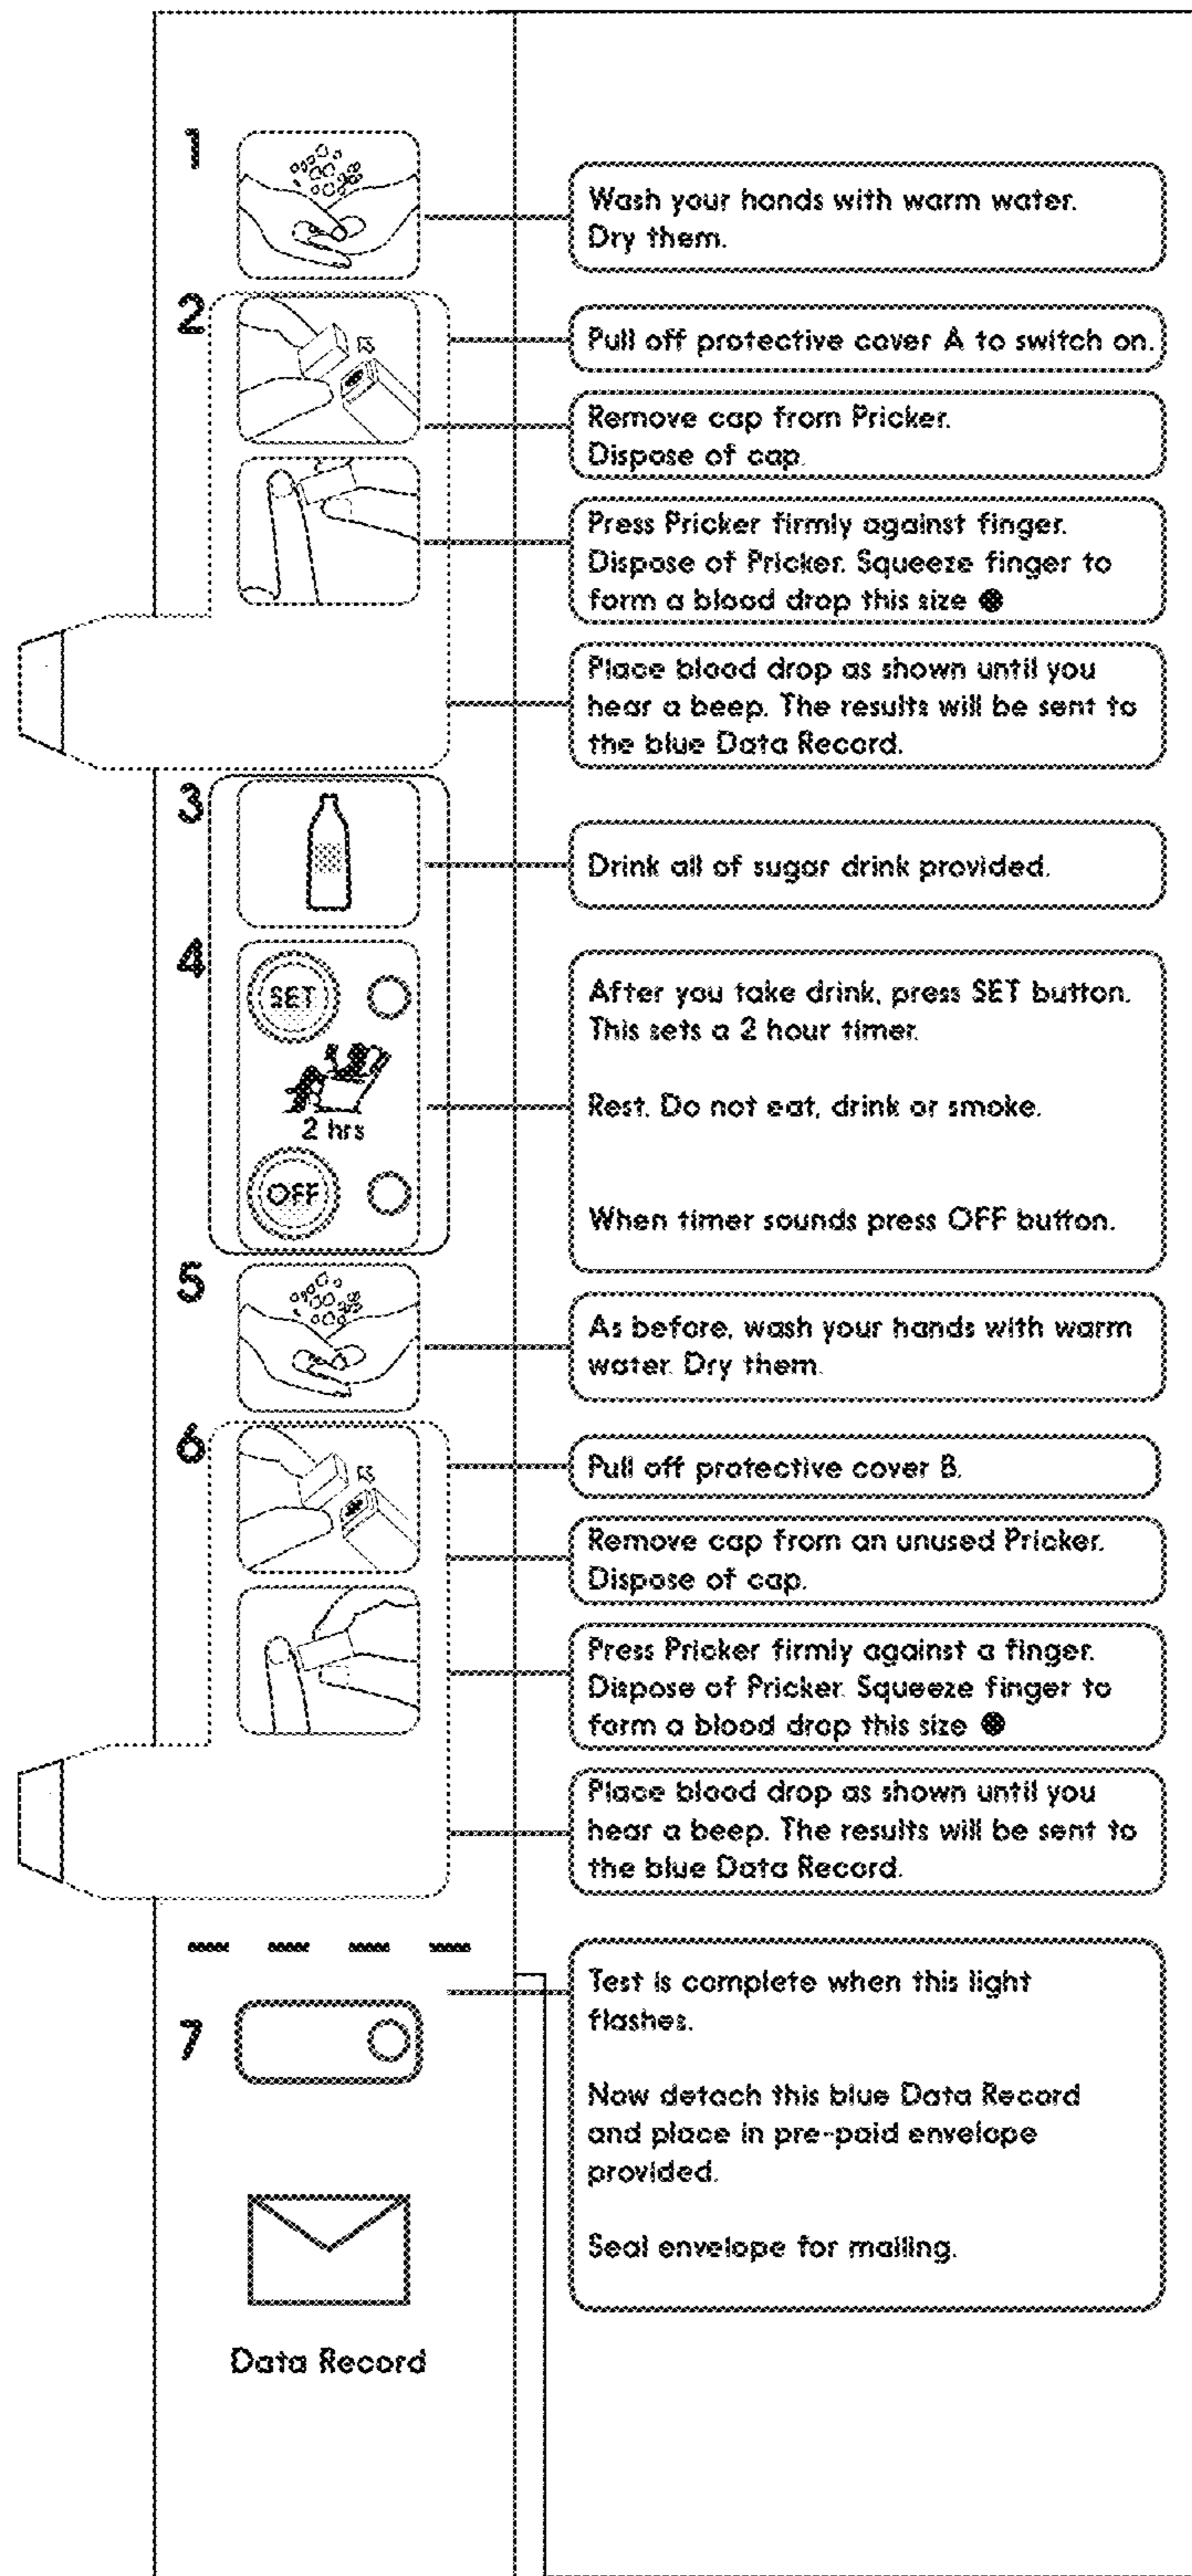


FIG 1.

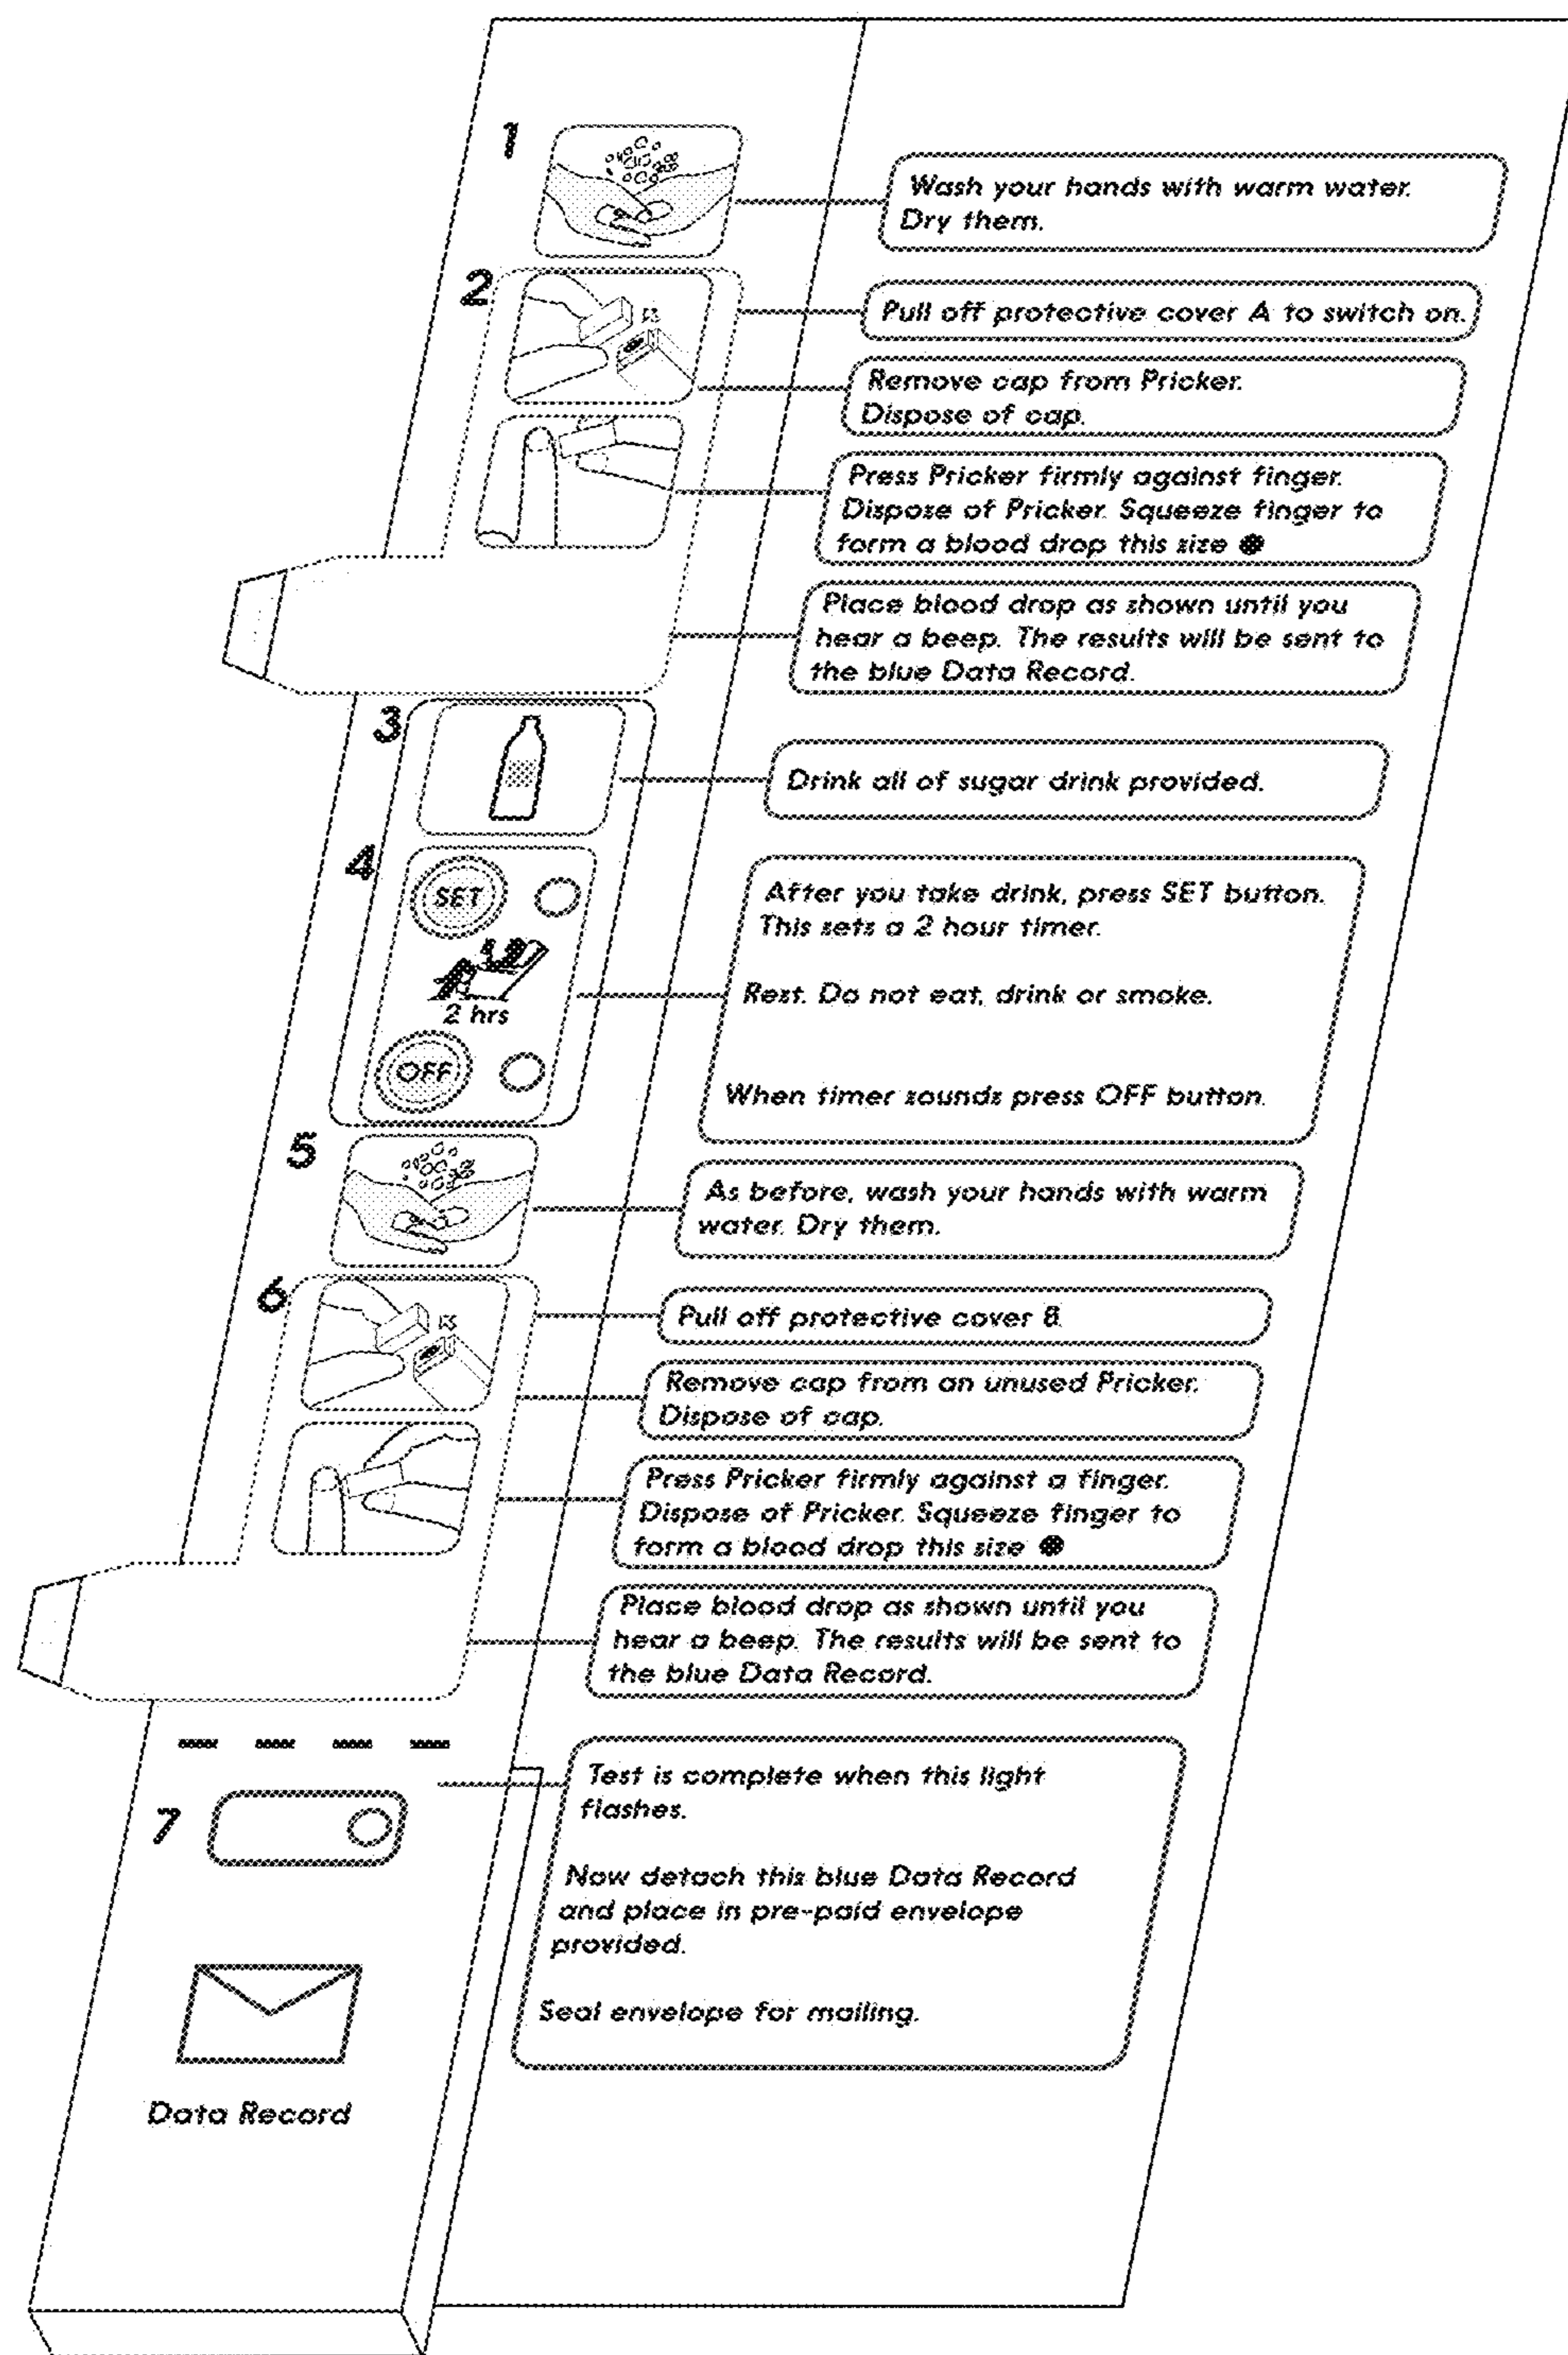


FIG 2.



**FIG 3.**

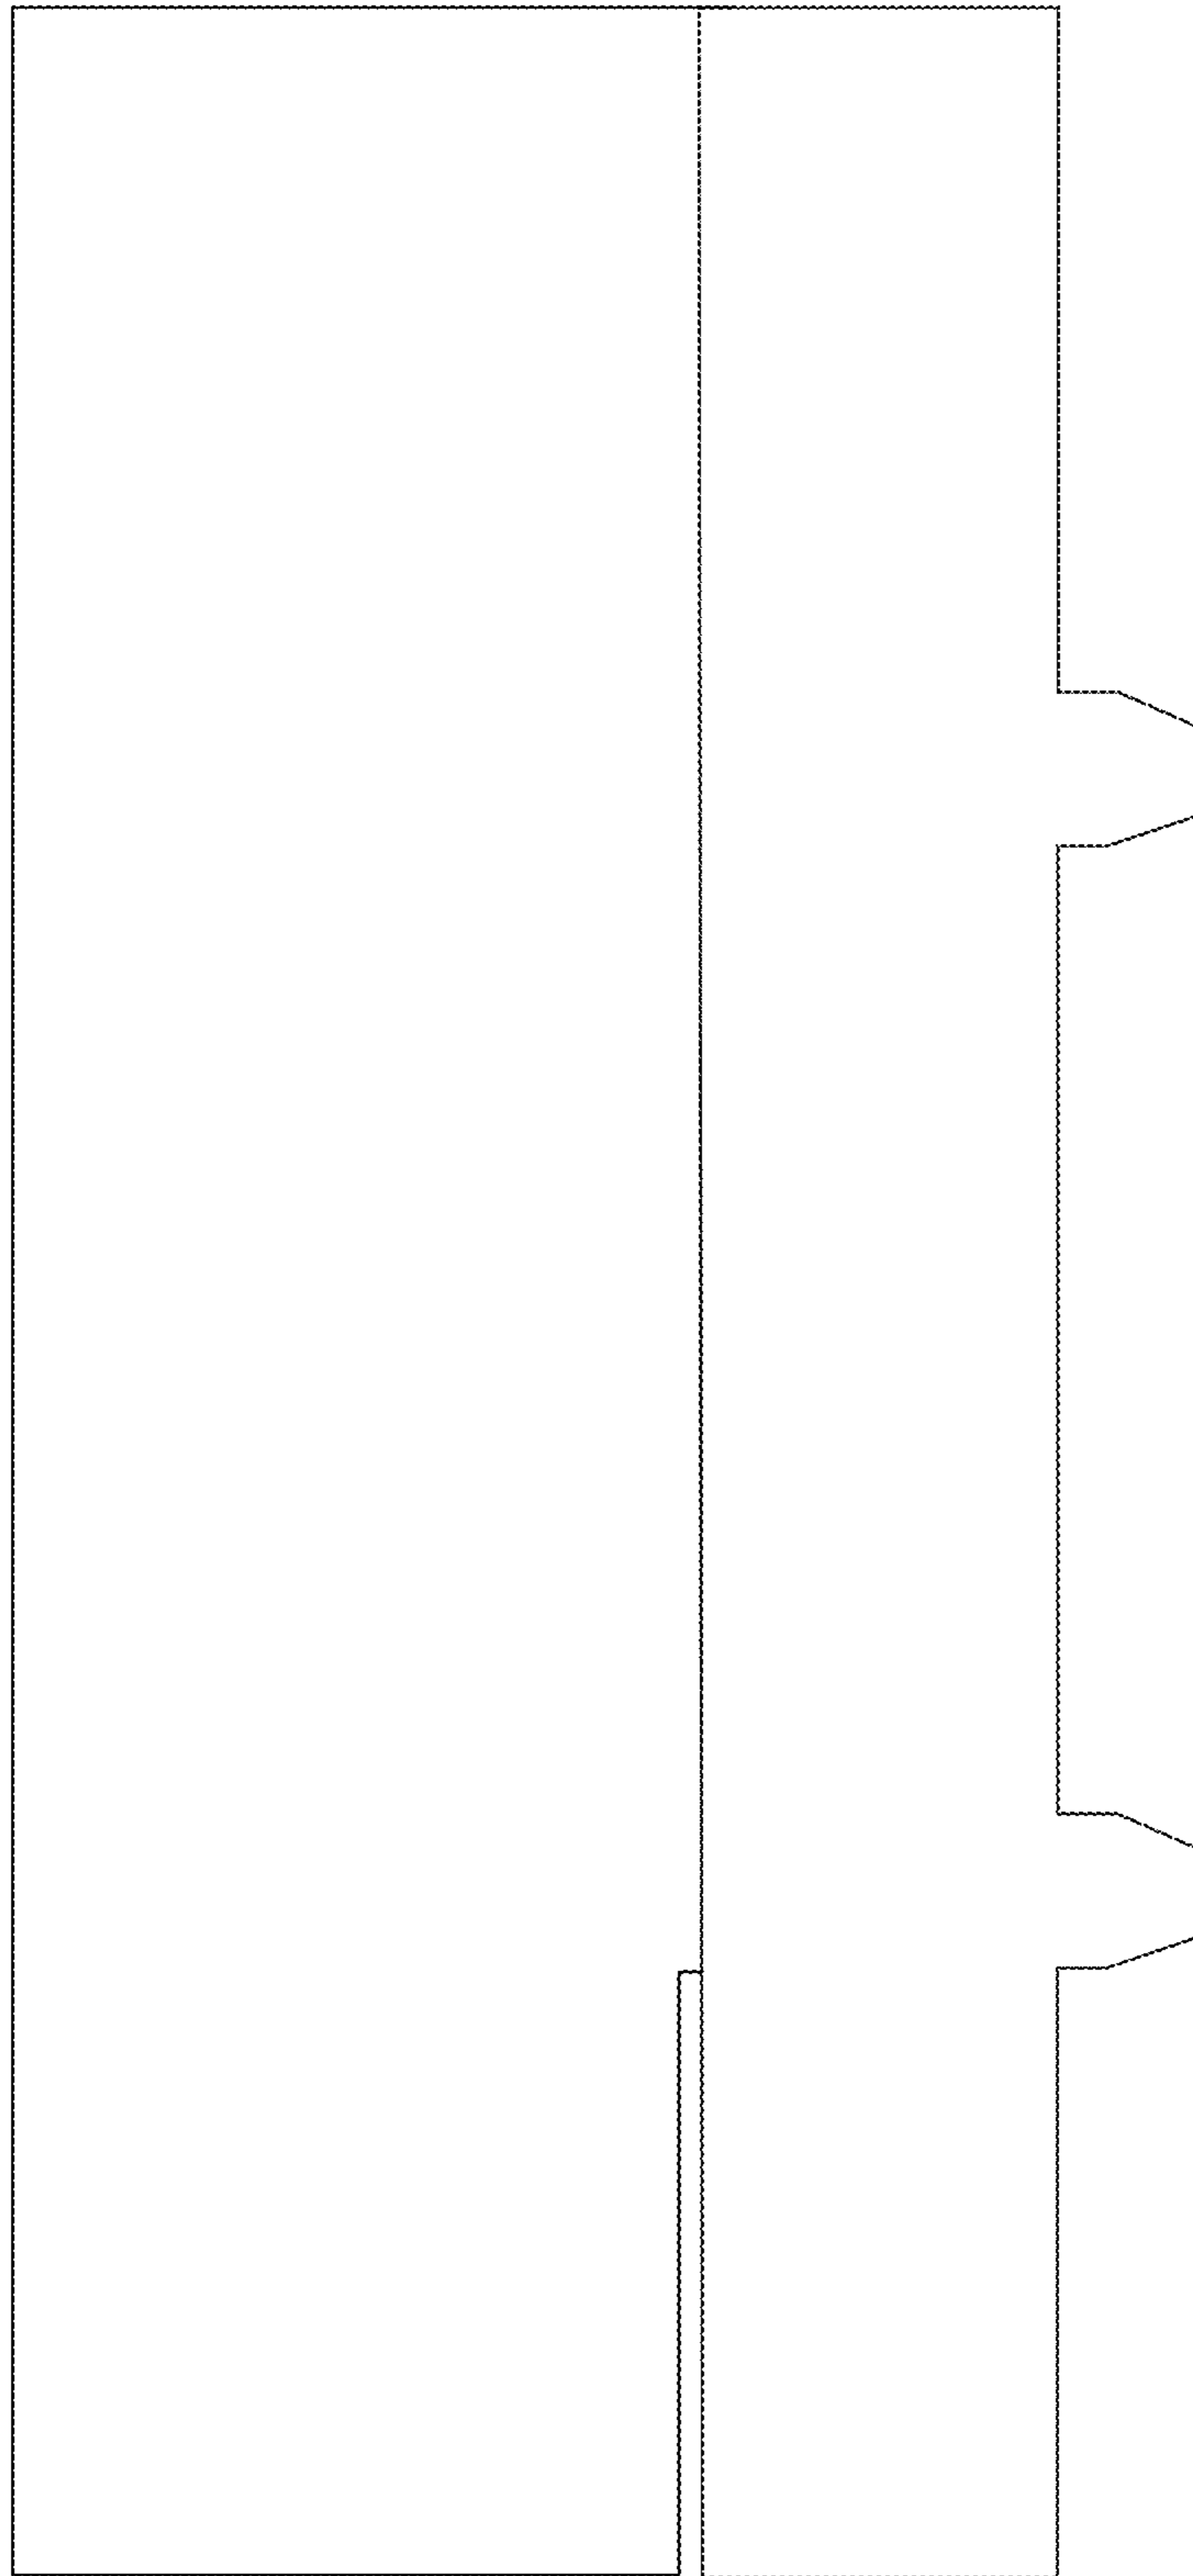


FIG 4.