



US00D726905S

(12) **United States Design Patent**
Tegg et al.

(10) **Patent No.:** **US D726,905 S**
(45) **Date of Patent:** **** Apr. 14, 2015**

(54) **CONTROL HANDLE FOR A MEDICAL DEVICE**

(75) Inventors: **Troy T. Tegg**, Elk River, MN (US);
Andrew O. Senn, Minneapolis, MN (US)

(73) Assignee: **St. Jude Medical, Atrial Fibrillation Division, Inc.**, St. Paul, MN (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/420,265**

(22) Filed: **May 7, 2012**

Related U.S. Application Data

(63) Continuation-in-part of application No. 13/105,646, filed on May 11, 2011, now Pat. No. 8,676,290.

(51) **LOC (10) Cl.** **23-01**

(52) **U.S. Cl.**
USPC **D24/130**

(58) **Field of Classification Search**
USPC D24/127, 130, 112-113, 186, 133;
606/181, 185; 604/533, 534, 284, 115,
604/19, 48, 164.01-164.09; 600/226,
600/372-374, 585, 114; 128/200.24,
128/207.14, 207.15

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D304,616 S * 11/1989 Dunlap et al. D24/112
4,924,092 A 5/1990 Crist, Jr.
4,944,727 A 7/1990 McCoy
D312,306 S * 11/1990 Michelson D24/112
5,108,368 A 4/1992 Hammerslag et al.
5,125,895 A 6/1992 Buchbinder et al.
5,125,896 A 6/1992 Hojeibane
5,170,803 A 12/1992 Hewson et al.
5,195,968 A 3/1993 Lundquist et al.

5,203,772 A 4/1993 Hammerslag et al.
5,254,088 A 10/1993 Lundquist et al.
5,273,535 A 12/1993 Edwards et al.
5,318,525 A 6/1994 West et al.
5,325,845 A 7/1994 Adair
5,342,299 A 8/1994 Snoke et al.
5,354,297 A 10/1994 Avitall
5,383,852 A 1/1995 Stevens-Wright
5,397,304 A 3/1995 Truckai

(Continued)

FOREIGN PATENT DOCUMENTS

EP 0431206 7/1995
WO 98/33429 8/1998

OTHER PUBLICATIONS

Blazer II XP, Temperature Ablation Catheter, "Extra Power . . . Controlled. Create Larger, deeper lesions for exceptional outcomes in atrial flutter", Boston Scientific Corporation, pp. 4 (2009).

(Continued)

Primary Examiner — Robert Delehanty

(74) *Attorney, Agent, or Firm* — Dykema Gossett PLLC

(57) **CLAIM**

The ornamental design for a control handle for a medical device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an embodiment of a control handle for a medical device showing a new design;

FIG. 2 is a top view thereof;

FIG. 3 is a front view thereof;

FIG. 4 is a bottom view thereof;


FIG. 5 is a back view thereof;

FIG. 6 is a left side view thereof; and,

FIG. 7 is a right side view thereof.

The broken lines are for purposes of illustration only and form no part of the claimed design.

1 Claim, 7 Drawing Sheets

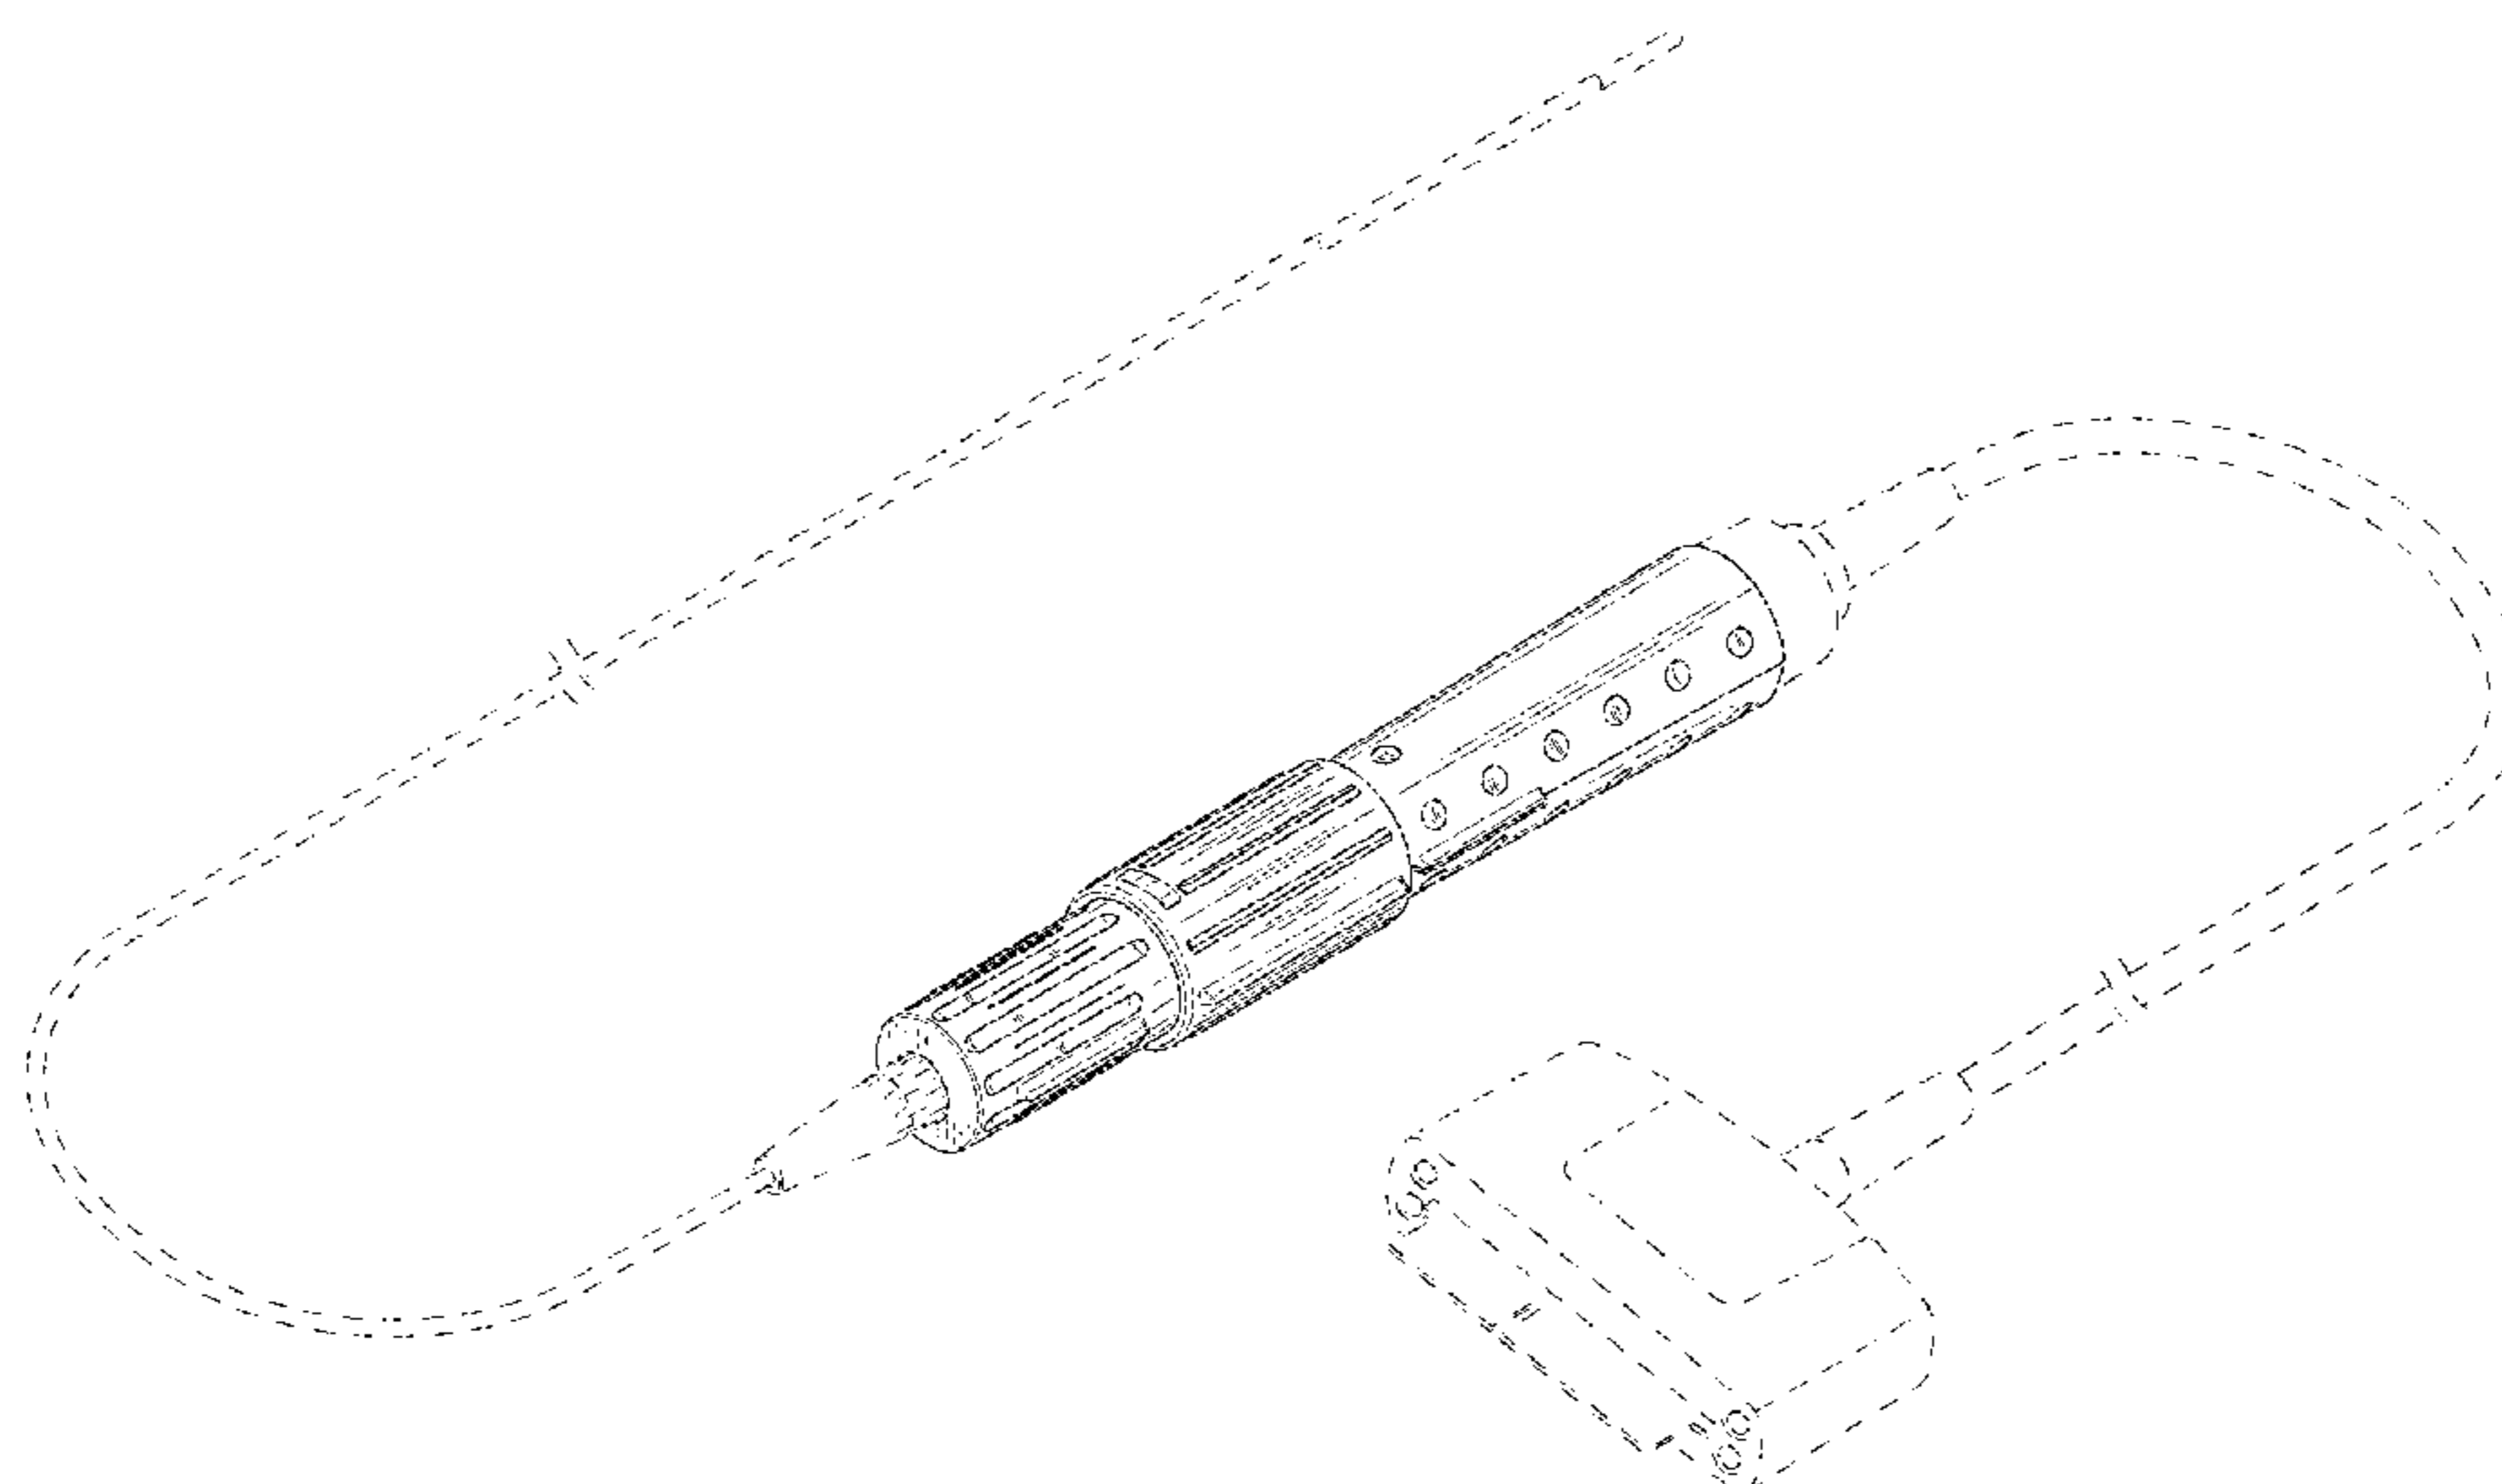

(56)

References Cited

U.S. PATENT DOCUMENTS

5,415,633 A 5/1995 Lazarus et al.
 5,487,757 A 1/1996 Truckai et al.
 5,520,644 A 5/1996 Imran
 5,531,721 A 7/1996 Pepin et al.
 5,549,542 A 8/1996 Kovalcheck
 5,662,606 A 9/1997 Cimino et al.
 D384,740 S * 10/1997 Musgrave et al. D24/112
 5,702,433 A 12/1997 Taylor et al.
 5,715,817 A 2/1998 Stevens-Wright et al.
 5,769,781 A * 6/1998 Chappuis 600/202
 5,842,984 A 12/1998 Avitall
 5,853,409 A 12/1998 Swanson et al.
 5,860,974 A 1/1999 Abele
 5,861,024 A 1/1999 Rashidi
 5,876,340 A 3/1999 Tu et al.
 5,891,138 A 4/1999 Tu et al.
 5,897,554 A 4/1999 Chia et al.
 5,921,924 A 7/1999 Avitall
 5,931,577 A 8/1999 Ishibashi
 5,931,811 A * 8/1999 Haissaguerre et al. 604/95.03
 5,938,616 A 8/1999 Eaton
 5,941,845 A * 8/1999 Tu et al. 600/374
 5,944,690 A 8/1999 Falwell et al.
 5,987,344 A 11/1999 West
 6,066,125 A 5/2000 Webster, Jr.
 6,068,629 A * 5/2000 Haissaguerre et al. 600/374
 6,071,274 A 6/2000 Thompson et al.
 6,071,279 A 6/2000 Whayne et al.
 6,076,012 A 6/2000 Swanson et al.
 6,211,936 B1 4/2001 Nakamura
 6,233,476 B1 5/2001 Strommer et al.
 6,241,727 B1 6/2001 Tu et al.
 6,308,091 B1 10/2001 Avitall
 6,330,473 B1 12/2001 Swanson et al.
 D455,210 S 4/2002 Henderson
 6,402,746 B1 6/2002 Whayne et al.
 6,430,426 B2 8/2002 Avitall
 6,454,758 B1 9/2002 Thompson et al.
 6,464,645 B1 10/2002 Park
 6,497,667 B1 12/2002 Miller
 6,554,794 B1 4/2003 Mueller
 6,582,536 B2 6/2003 Shimada
 6,690,963 B2 2/2004 Ben-Haim et al.
 6,942,661 B2 9/2005 Swanson et al.
 7,130,700 B2 10/2006 Gardeski et al.
 7,197,354 B2 3/2007 Sobe

7,263,397 B2 8/2007 Hauck et al.
 D550,356 S 9/2007 Anderson et al.
 7,386,339 B2 6/2008 Strommer et al.
 7,507,229 B2 3/2009 Hewitt et al.
 7,536,218 B2 5/2009 Govari et al.
 D612,044 S * 3/2010 Scheibe D24/130
 7,691,095 B2 4/2010 Bednarek
 7,715,204 B2 5/2010 Miller
 7,785,252 B2 8/2010 Danitz et al.
 7,848,789 B2 12/2010 Govari et al.
 D634,421 S * 3/2011 El-Gad et al. D24/113
 D634,422 S * 3/2011 El-Gad et al. D24/113
 7,901,358 B2 3/2011 Mehi
 8,123,721 B2 2/2012 Tegg
 D695,891 S * 12/2013 Biel et al. D24/112
 D696,397 S * 12/2013 Guarraia et al. D24/113
 8,620,399 B2 * 12/2013 Gonda 600/372
 8,676,290 B2 * 3/2014 Tegg 600/373
 2002/0077590 A1 6/2002 Ponzi et al.
 2002/0087166 A1 7/2002 Brock et al.
 2002/0087169 A1 7/2002 Brock et al.
 2003/0040684 A1 2/2003 Soukup et al.
 2004/0153049 A1 8/2004 Hewitt et al.
 2005/0038467 A1 2/2005 Hebert et al.
 2005/0107737 A1 5/2005 McDaniel
 2005/0267461 A1 12/2005 Cao et al.
 2006/0142694 A1 6/2006 Bednarek et al.
 2006/0142695 A1 6/2006 Knudson
 2007/0276324 A1 11/2007 Laduca et al.
 2008/0234660 A2 9/2008 Cumming et al.
 2008/0312536 A1 12/2008 Dala-Krishna
 2009/0105640 A1 4/2009 Bednarek et al.
 2009/0264817 A1 10/2009 Flach et al.
 2010/0004592 A1 1/2010 Butler
 2010/0130924 A1 5/2010 Martin et al.
 2010/0262075 A1 10/2010 Danitz et al.
 2010/0280449 A1 11/2010 Alvarez et al.
 2011/0264074 A1 10/2011 Tegg et al.
 2011/0282176 A1 11/2011 Tegg
 2012/0029334 A1 2/2012 Tegg

OTHER PUBLICATIONS

EZ Steer, Bi-Directional Catheters, "Micro Movements. Macro Control.", Biosense Webster, Inc., a Johnson & Johnson Company, pp. 6 (2006).
 Title: International Search Report and Written Opinion Citation: PCT/US2013/026990 Publication Date: Apr. 29, 2013.

* cited by examiner

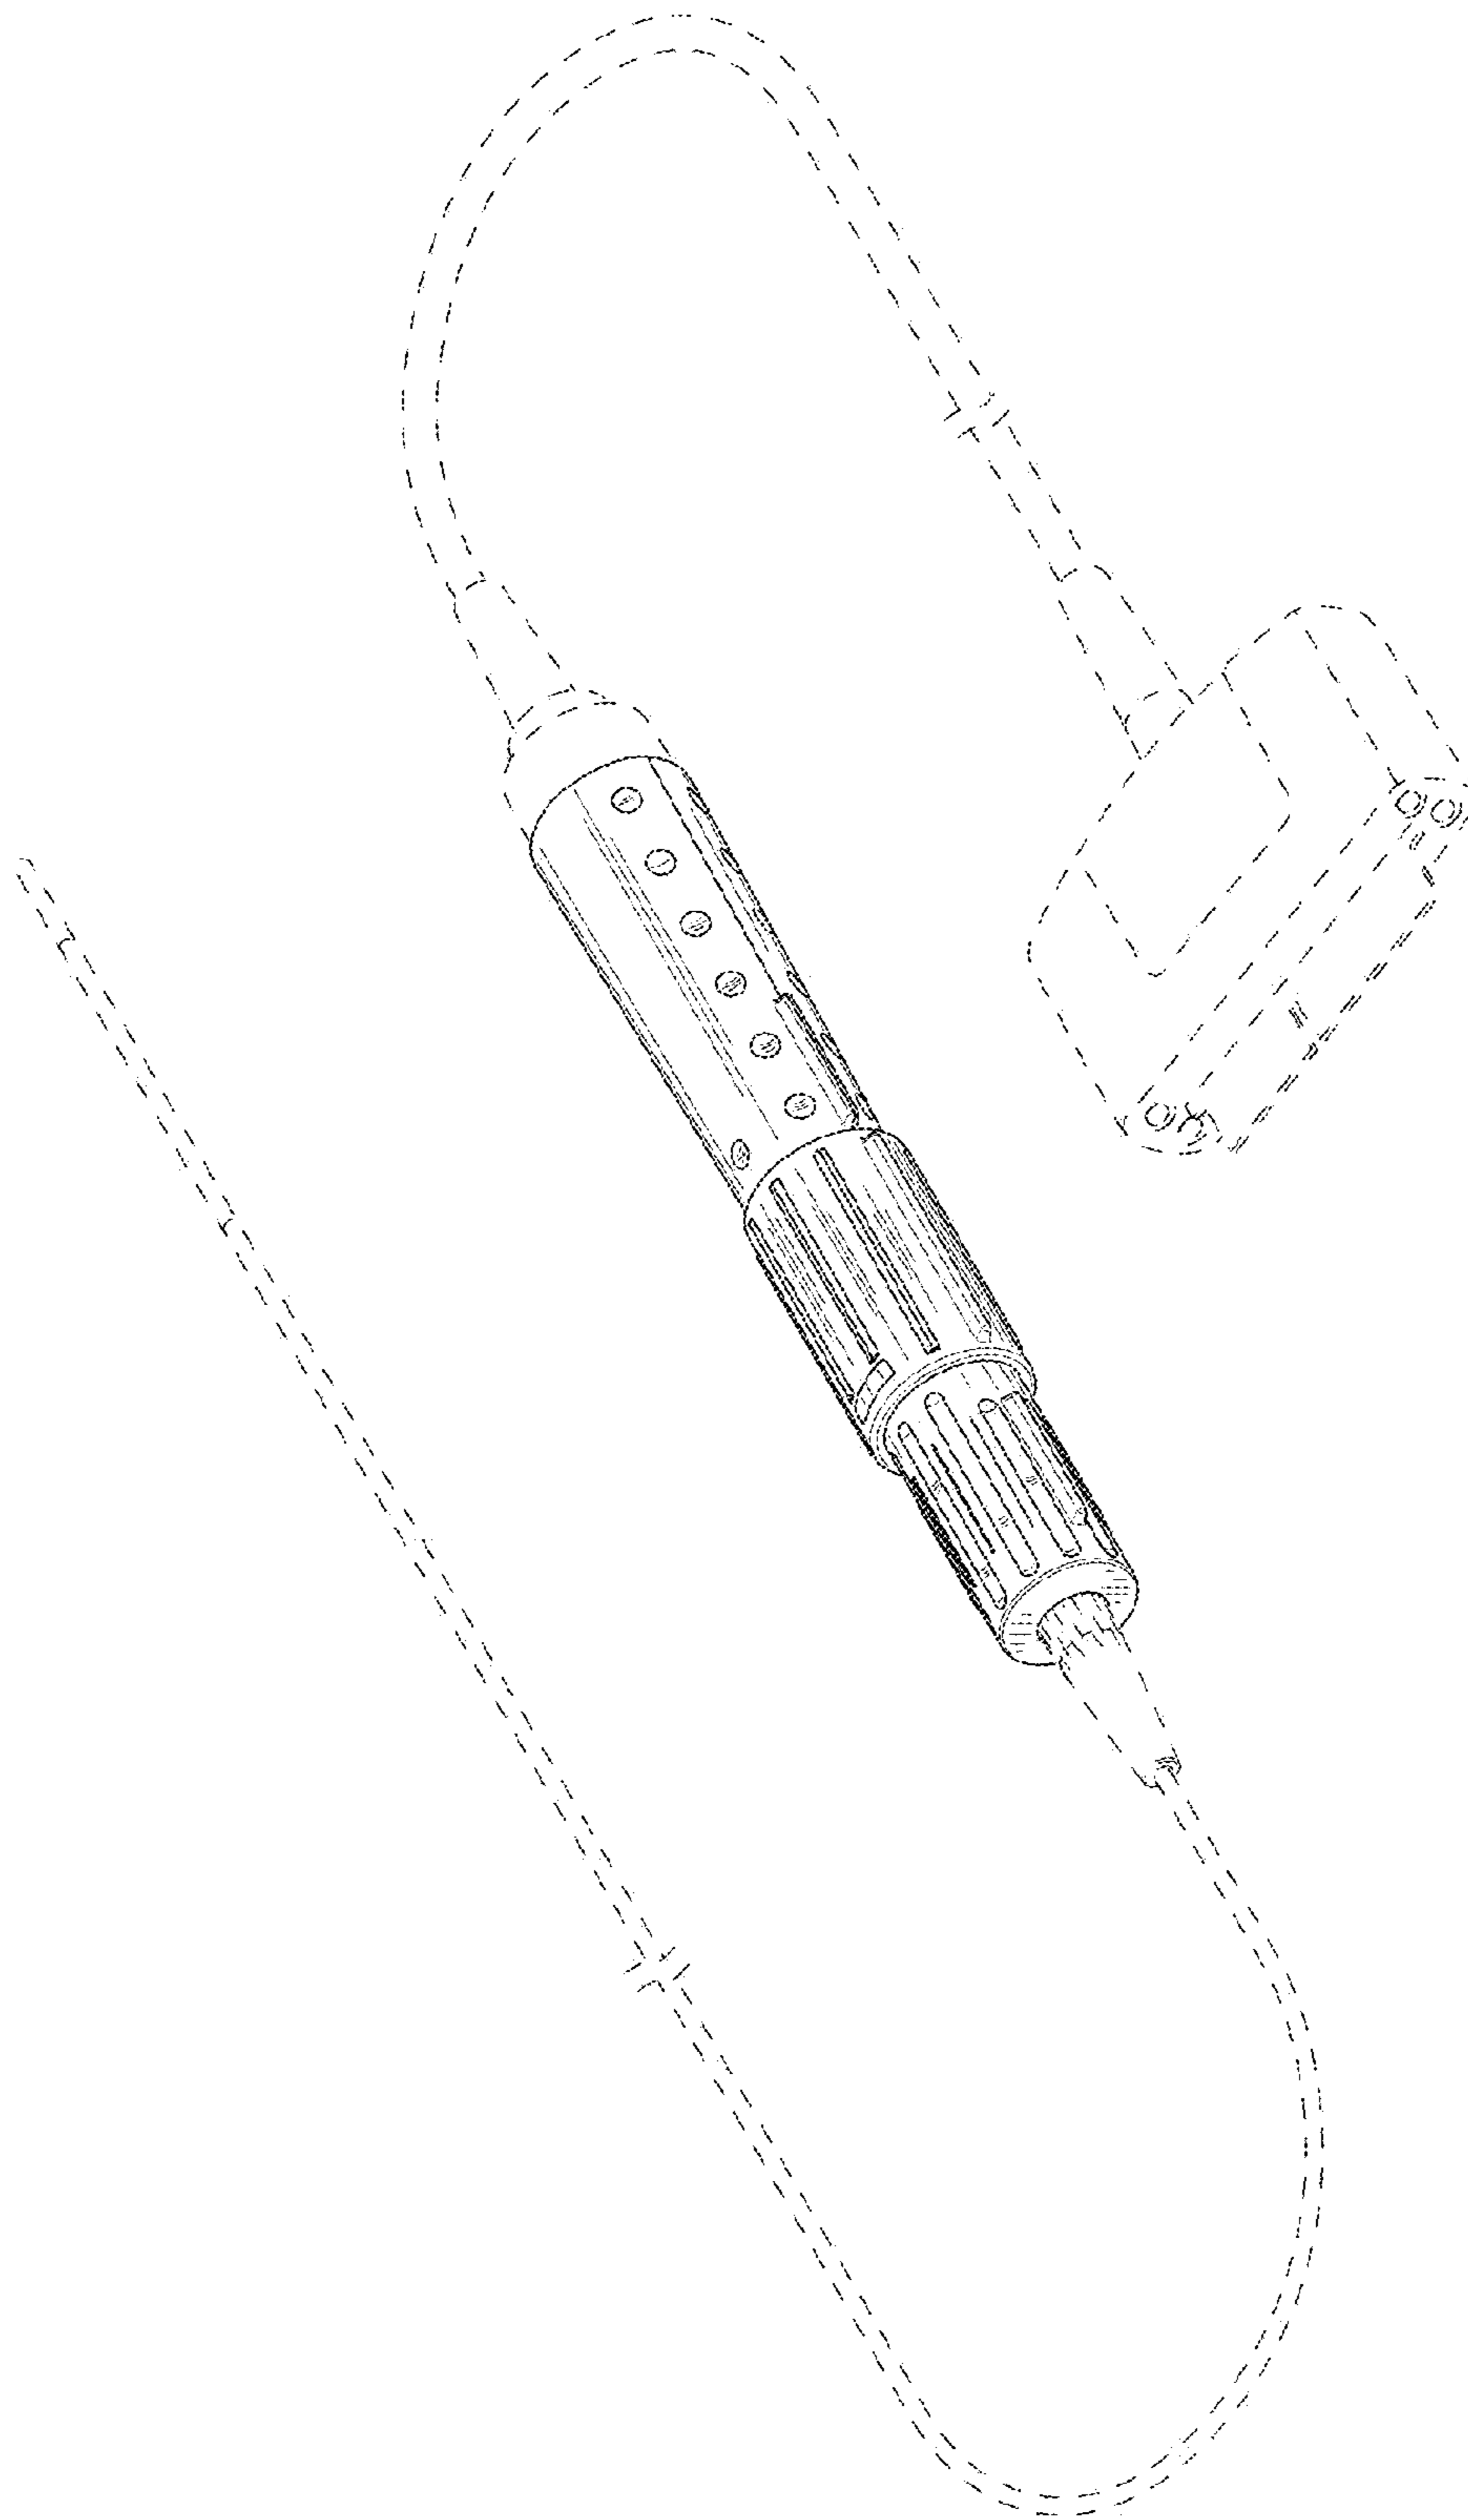


FIG. 1

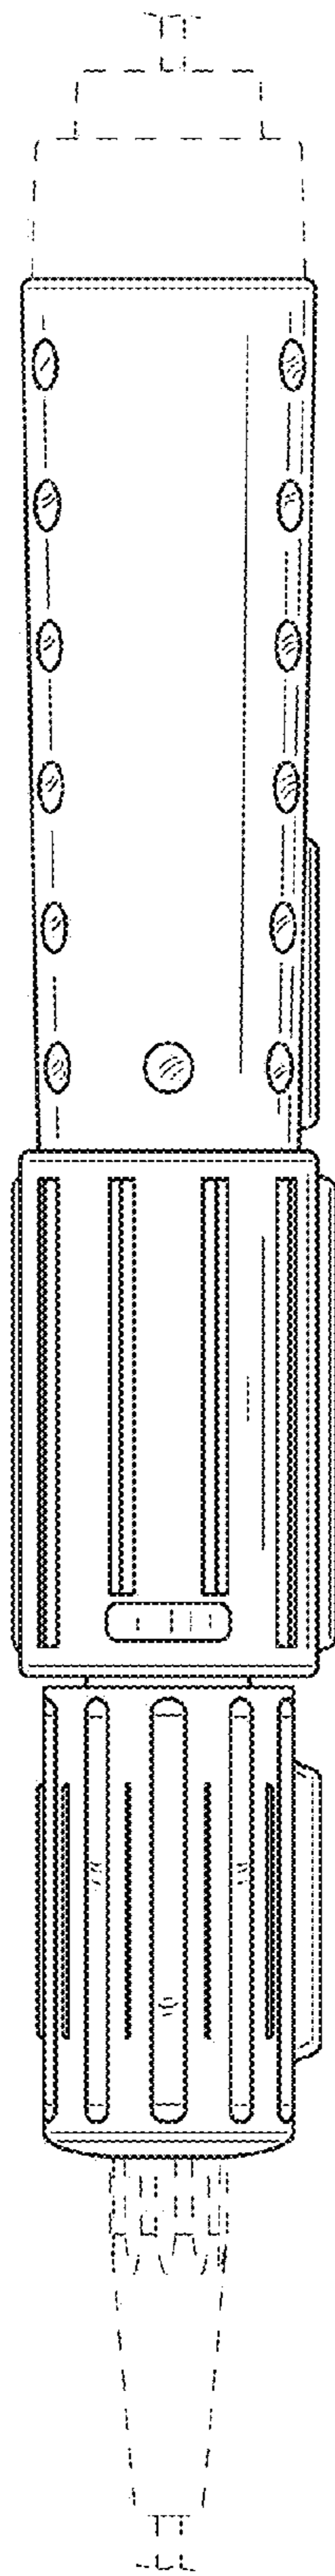


FIG. 2

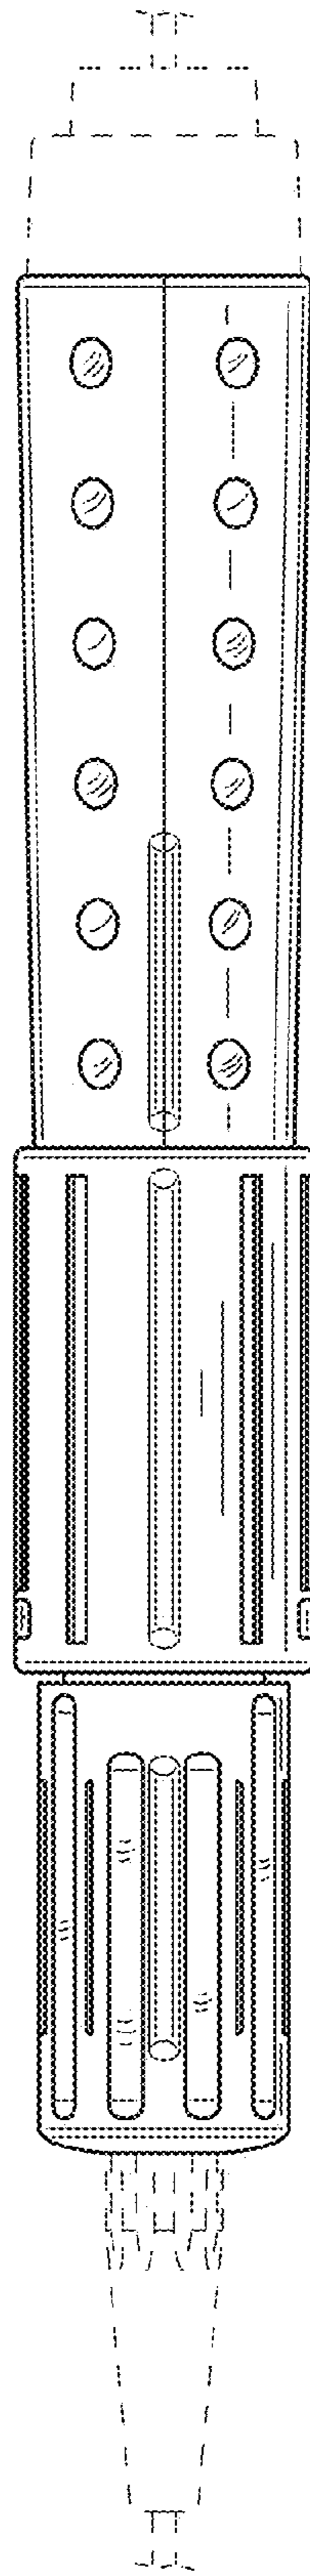


FIG. 3

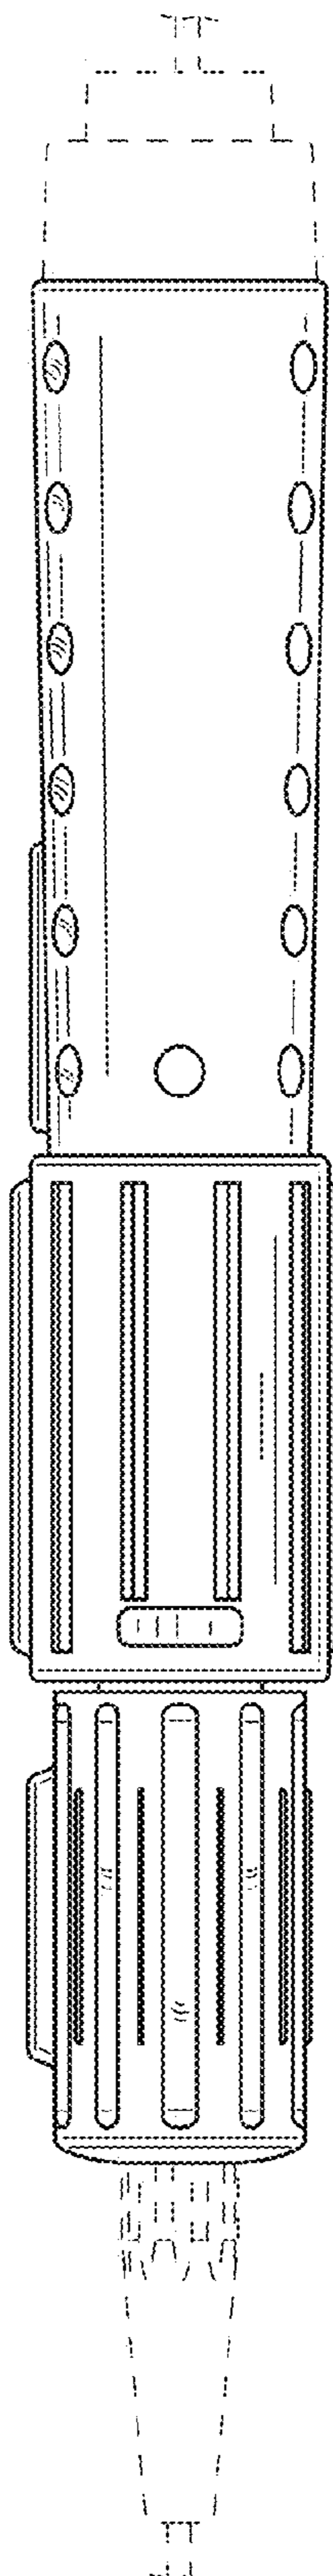


FIG. 4

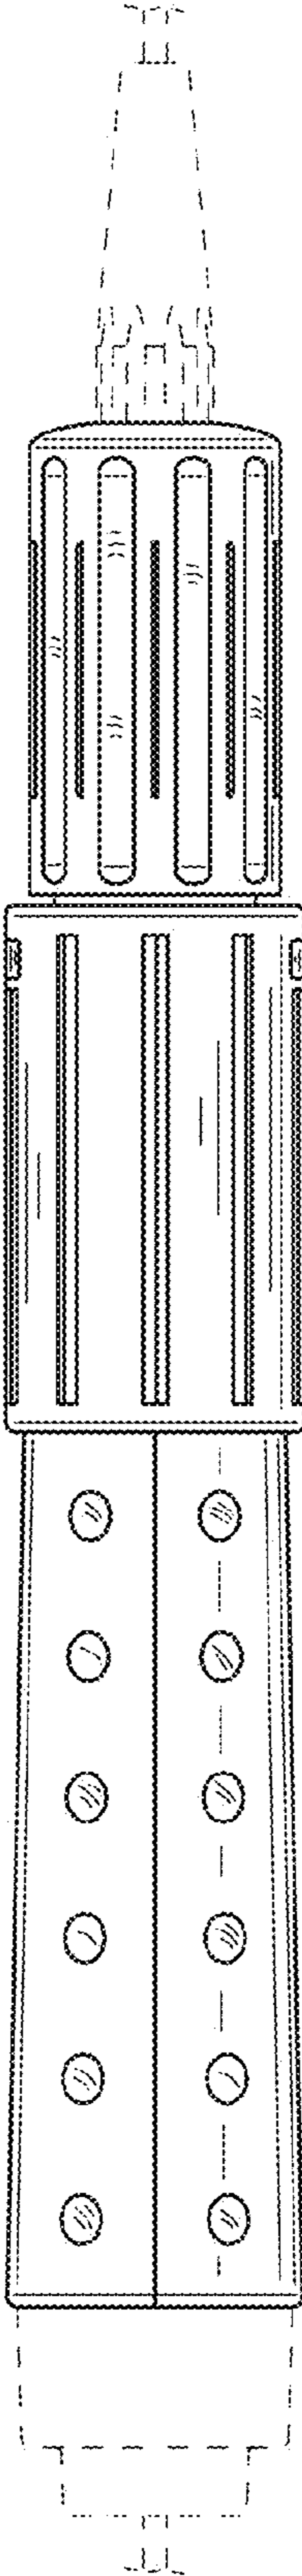


FIG. 5

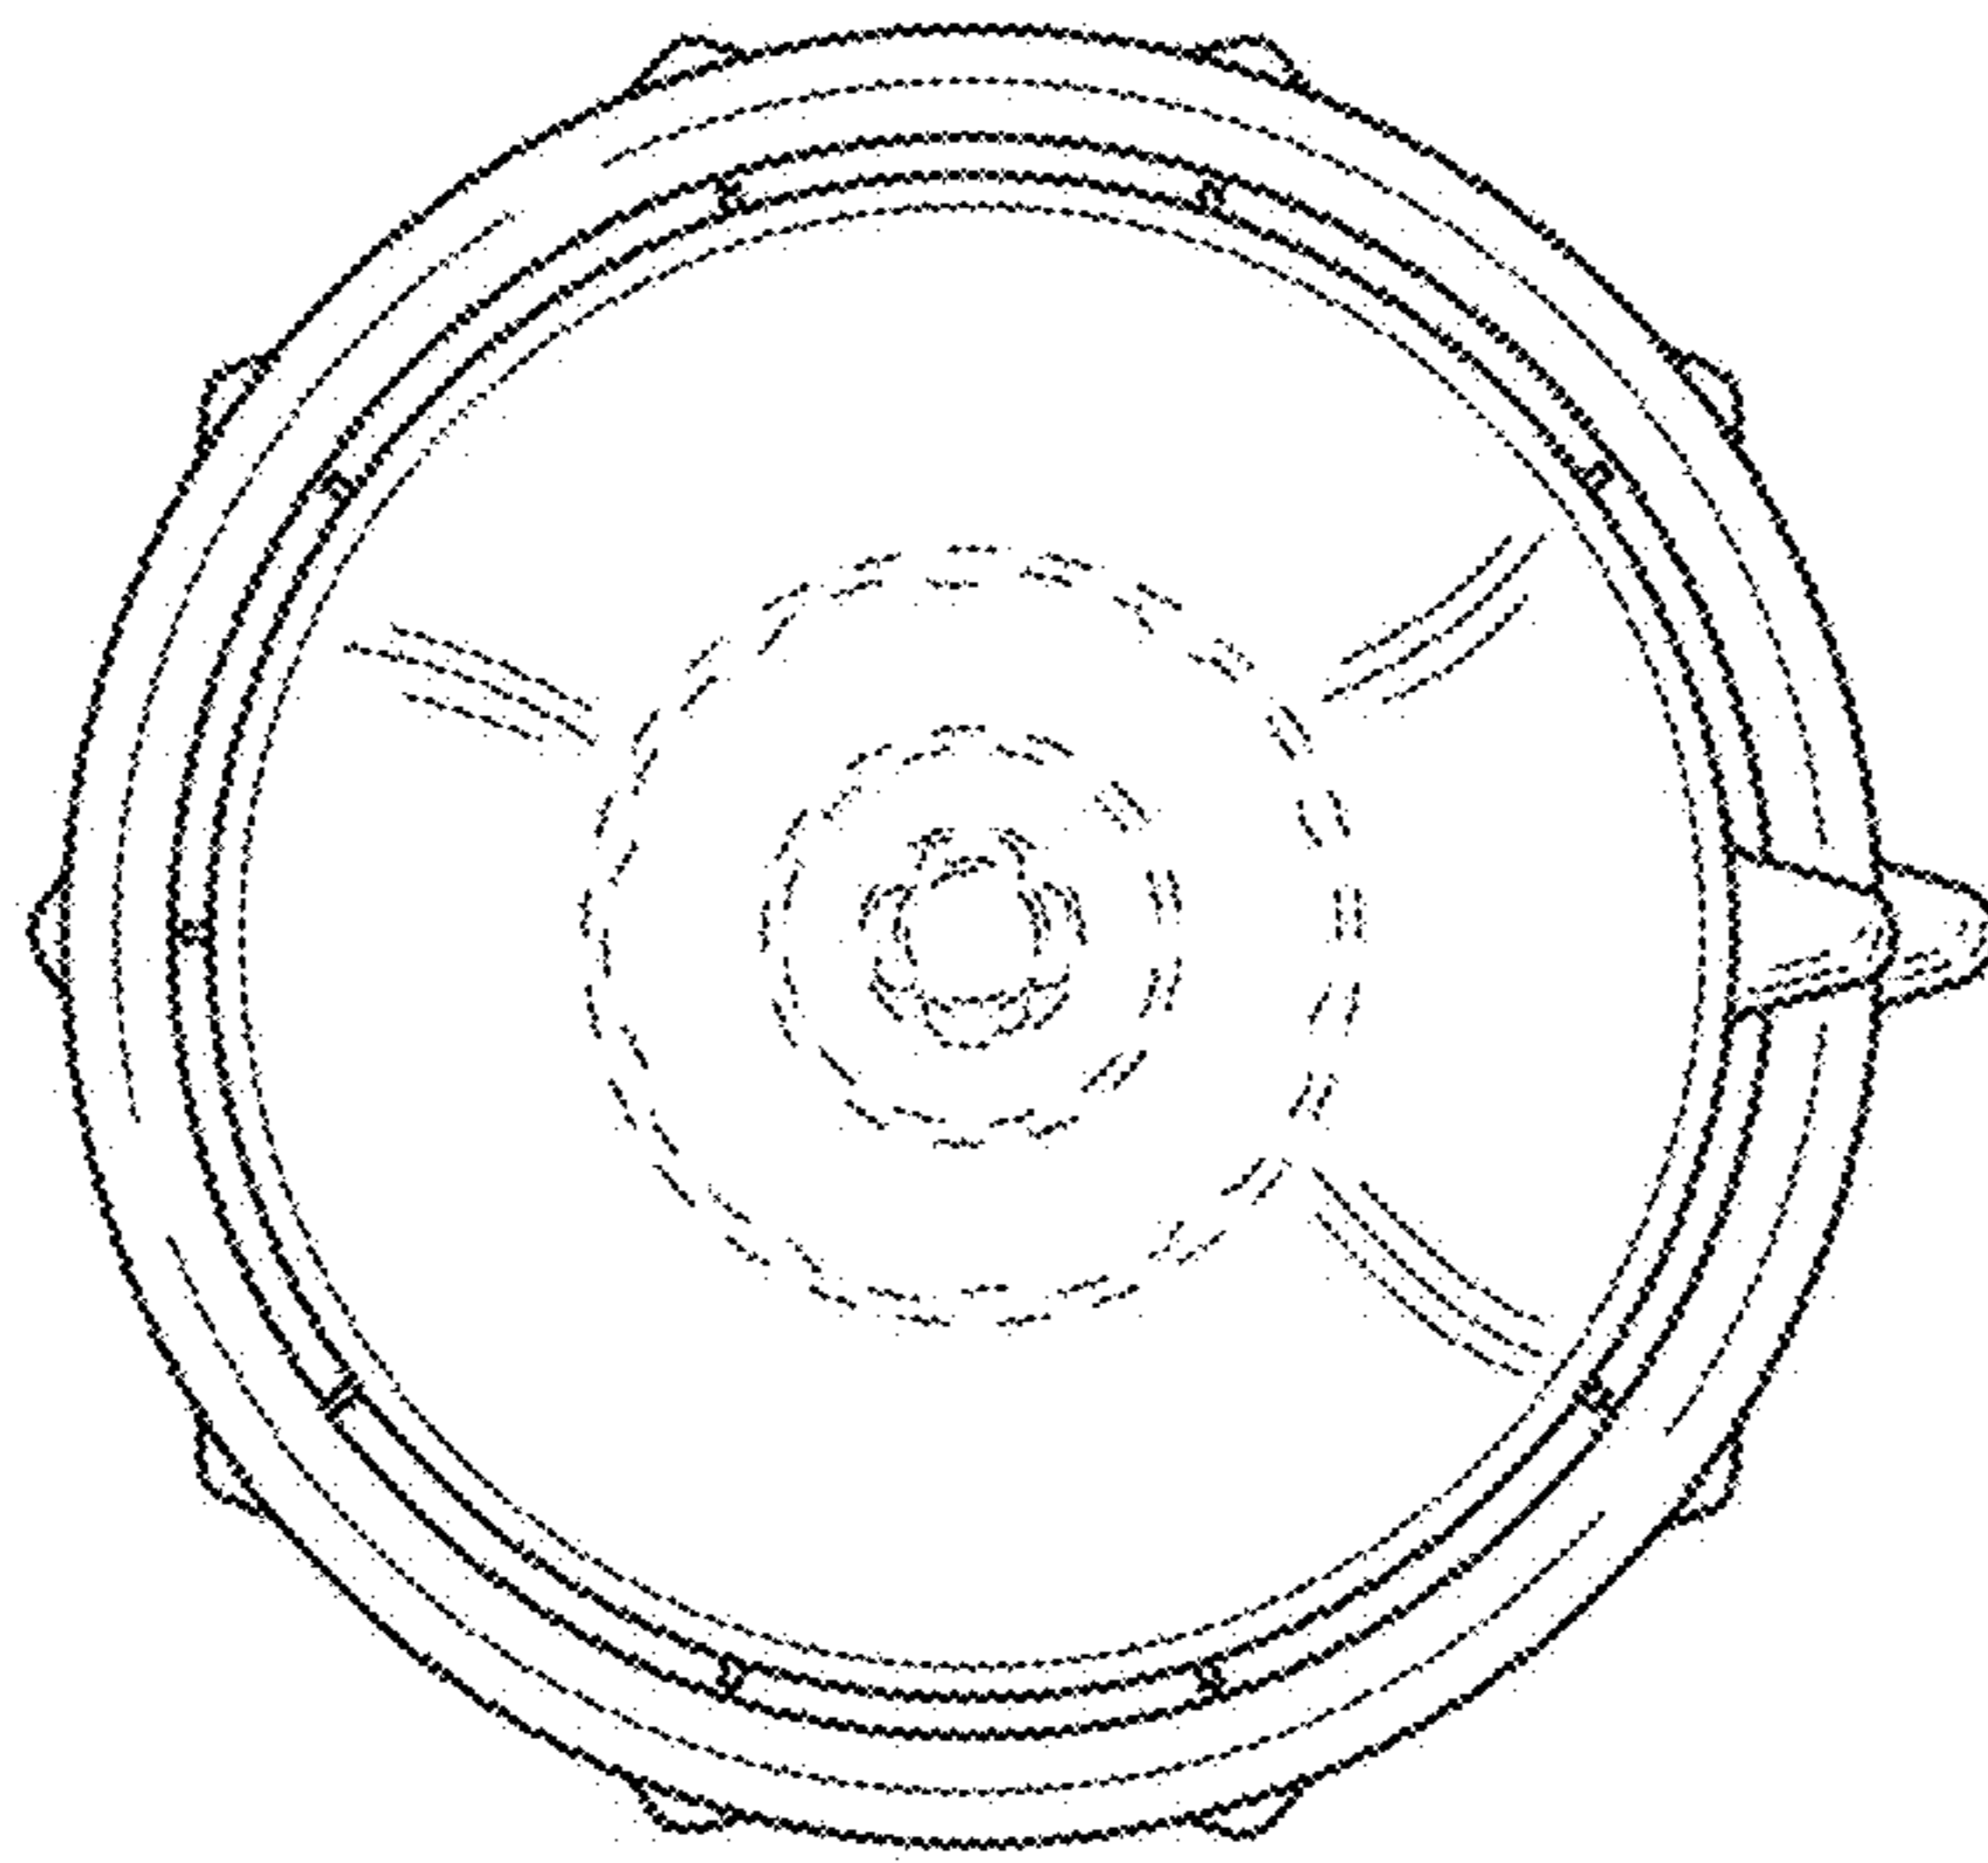


FIG.6

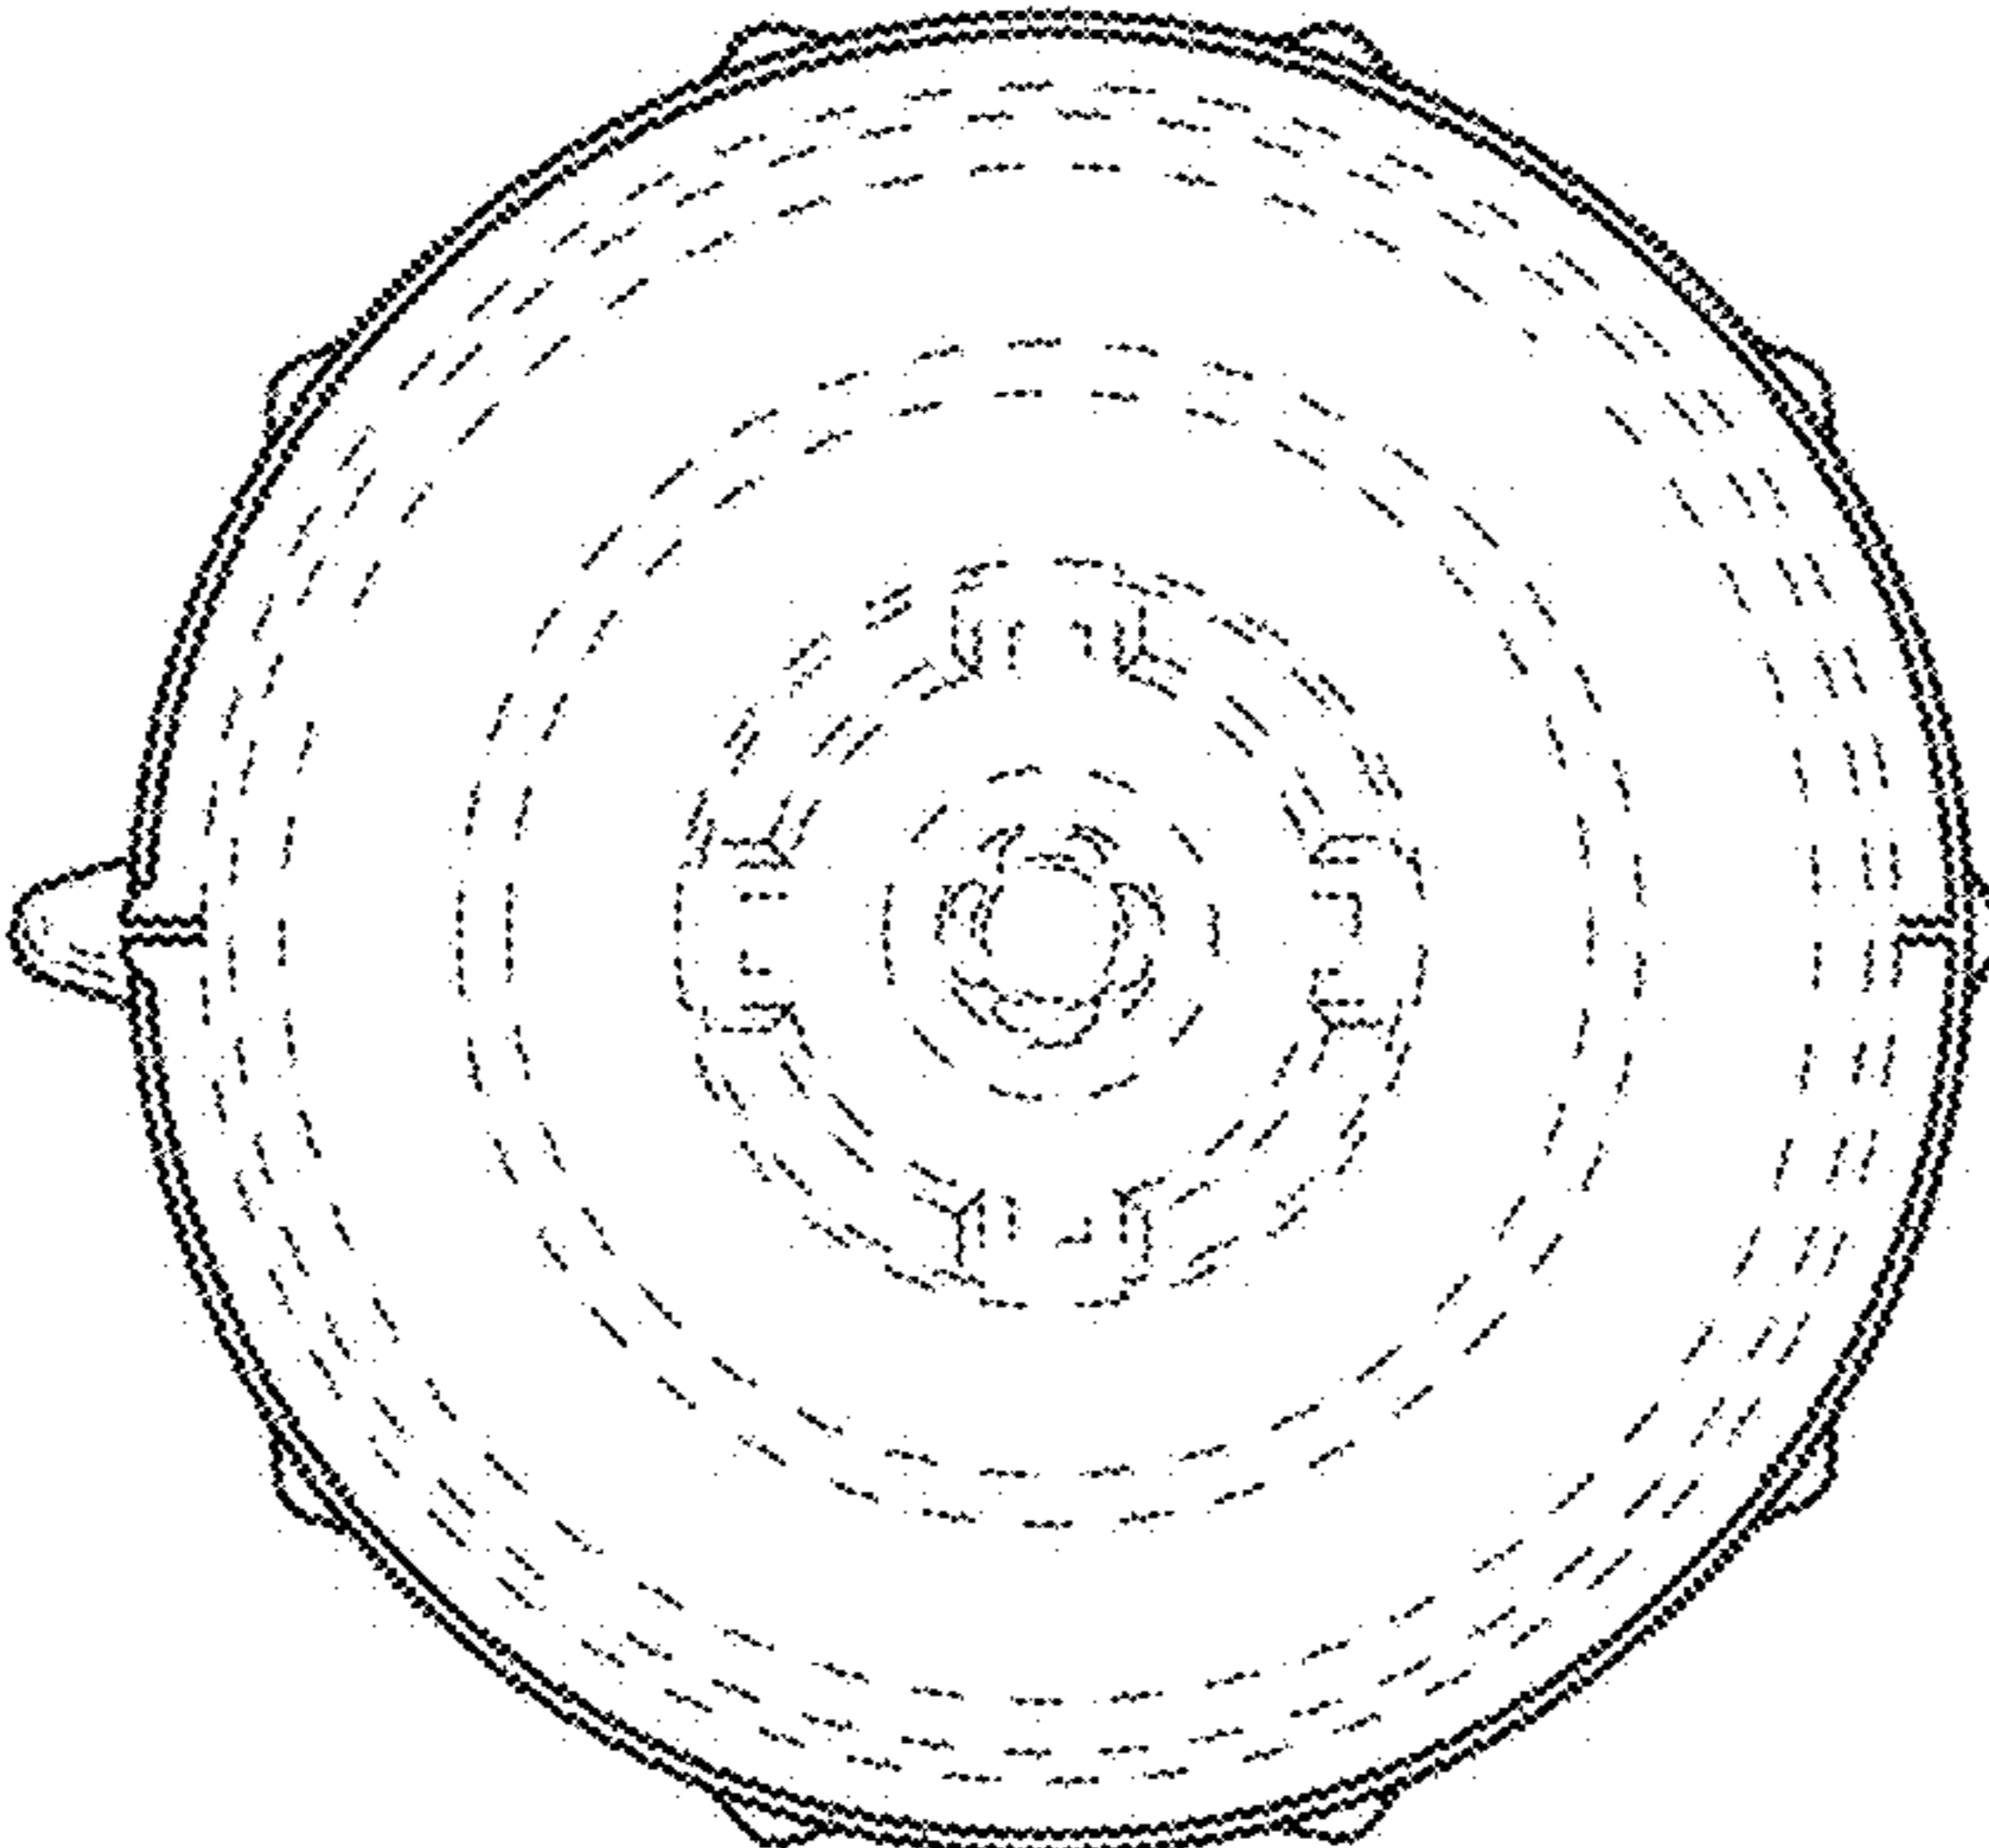


FIG. 7