

US00D730212S

(12) **United States Design Patent**  
**Biselx et al.**

(10) **Patent No.:** **US D730,212 S**

(45) **Date of Patent:** **\*\* May 26, 2015**

(54) **MICROMETER**

(71) Applicant: **TESA SA**, Renens (CH)

(72) Inventors: **Frédéric Biselx**, Yens (CH); **Stéphane Karawa**, Luasanne (CH)

(73) Assignee: **TESA SA**, Renens (CH)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/492,826**

(22) Filed: **Jun. 3, 2014**

(30) **Foreign Application Priority Data**

Dec. 11, 2013 (WO) ..... 780199301

(51) **LOC (10) Cl.** ..... **10-04**

(52) **U.S. Cl.**  
USPC ..... **D10/73**

(58) **Field of Classification Search**  
CPC ..... G01B 3/20; G01B 3/205; G01B 3/24;  
G01B 3/18; G01B 3/008; G01J 3/02; G01J  
3/0208; G01J 3/0291; G01J 3/50; G01J 3/501;  
G01J 3/0289; G01J 3/0243  
USPC ..... D10/73  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

4,255,861 A \* 3/1981 Nakata et al. .... 33/819  
D263,809 S \* 4/1982 Suwa et al. .... D10/73  
D273,468 S \* 4/1984 Ueda et al. .... D10/73

D273,469 S \* 4/1984 Ueda et al. .... D10/73  
4,578,868 A \* 4/1986 Sasaki et al. .... 33/819  
5,433,016 A \* 7/1995 Tachikake et al. .... 33/820  
5,495,677 A \* 3/1996 Tachikake et al. .... 33/784  
5,691,646 A \* 11/1997 Sasaki ..... 324/662  
5,920,198 A \* 7/1999 Suzuki et al. .... 324/662  
D429,172 S \* 8/2000 Reymond ..... D10/73  
6,247,244 B1 \* 6/2001 Zanier et al. .... 33/819  
6,308,433 B1 \* 10/2001 Takahashi et al. .... 33/819  
D611,371 S \* 3/2010 Ohtani et al. .... D10/73  
2013/0276319 A1 \* 10/2013 Tsuji ..... 33/819

\* cited by examiner

*Primary Examiner* — Antoine D Davis

(74) *Attorney, Agent, or Firm* — Maschoff Brennan


(57) **CLAIM**

The ornamental design for a micrometer, as shown and described.

**DESCRIPTION**

FIG. 1 is an upper perspective view of an exemplary micrometer;  
FIG. 2 is a front view of the micrometer;  
FIG. 3 is a rear view of the micrometer;  
FIG. 4 is a bottom view of the micrometer;  
FIG. 5 is a top view of the micrometer;  
FIG. 6 is a left side view of the micrometer;  
FIG. 7 is a front view of another exemplary micrometer, with the other views the same as shown above in connection with FIG. 1; and,  
FIG. 8 is a front view of still another exemplary micrometer, with the other view the same as shown above in connection with FIG. 1.

**1 Claim, 8 Drawing Sheets**

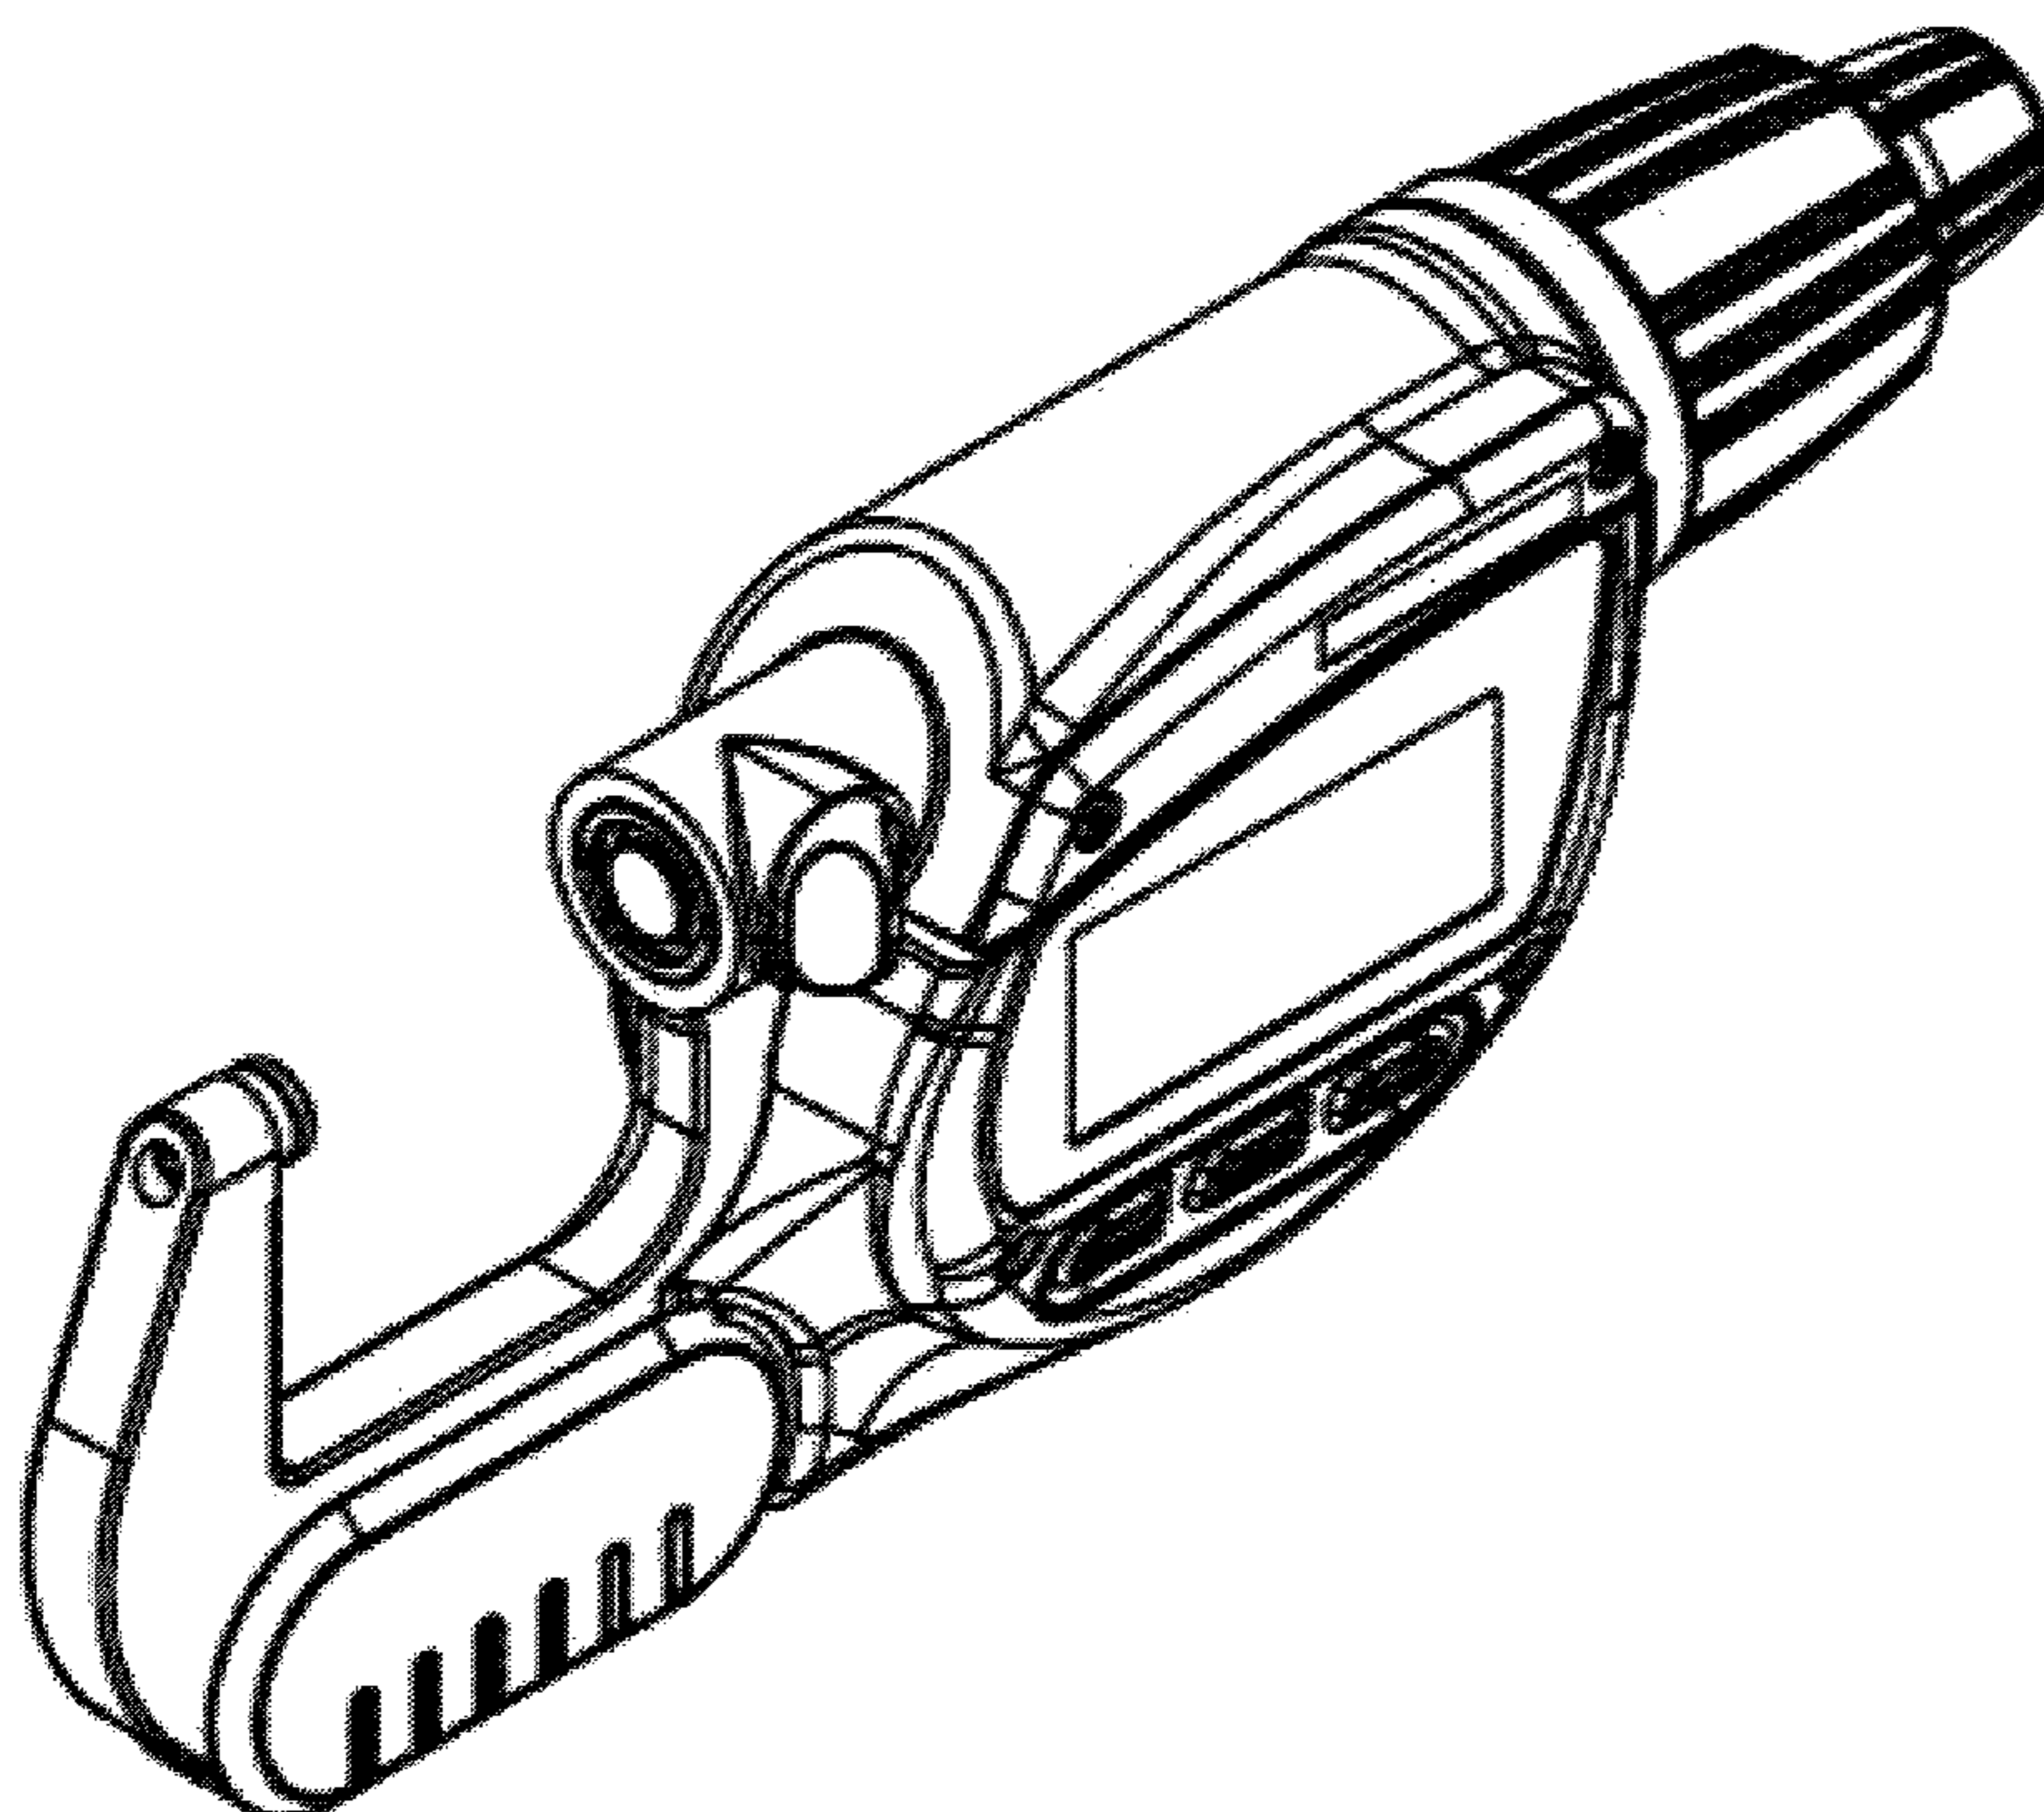

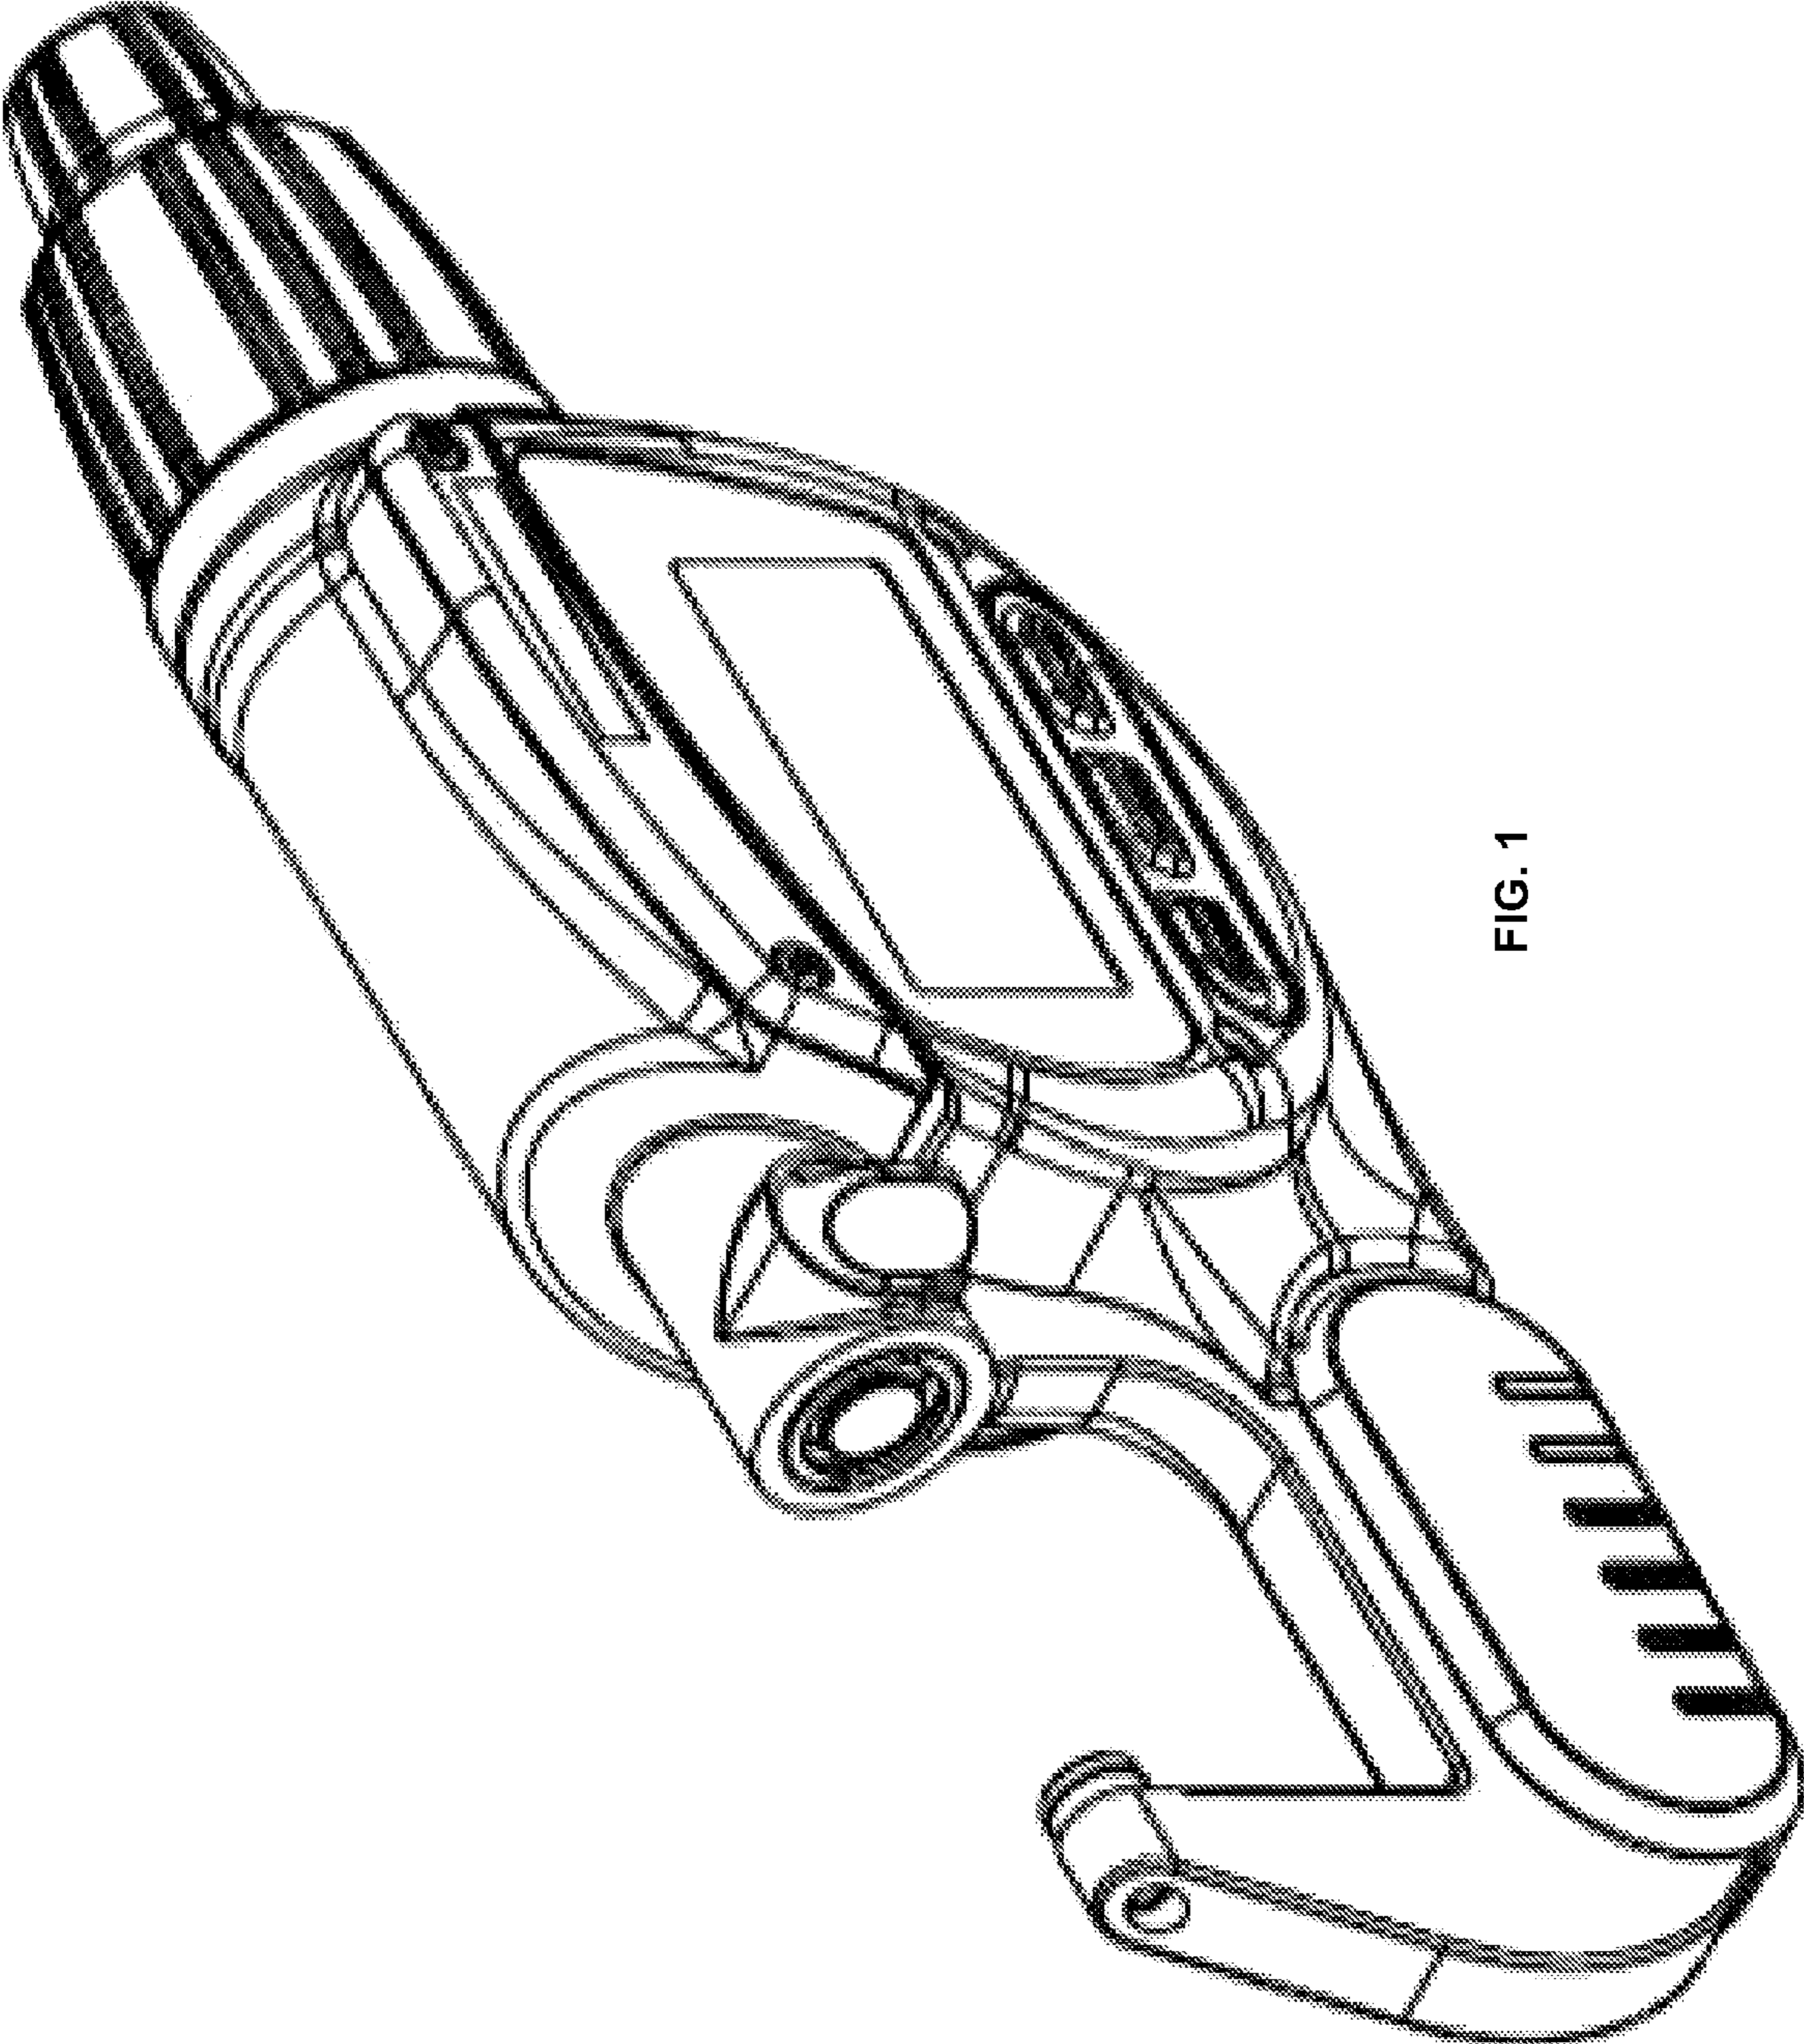


FIG. 1

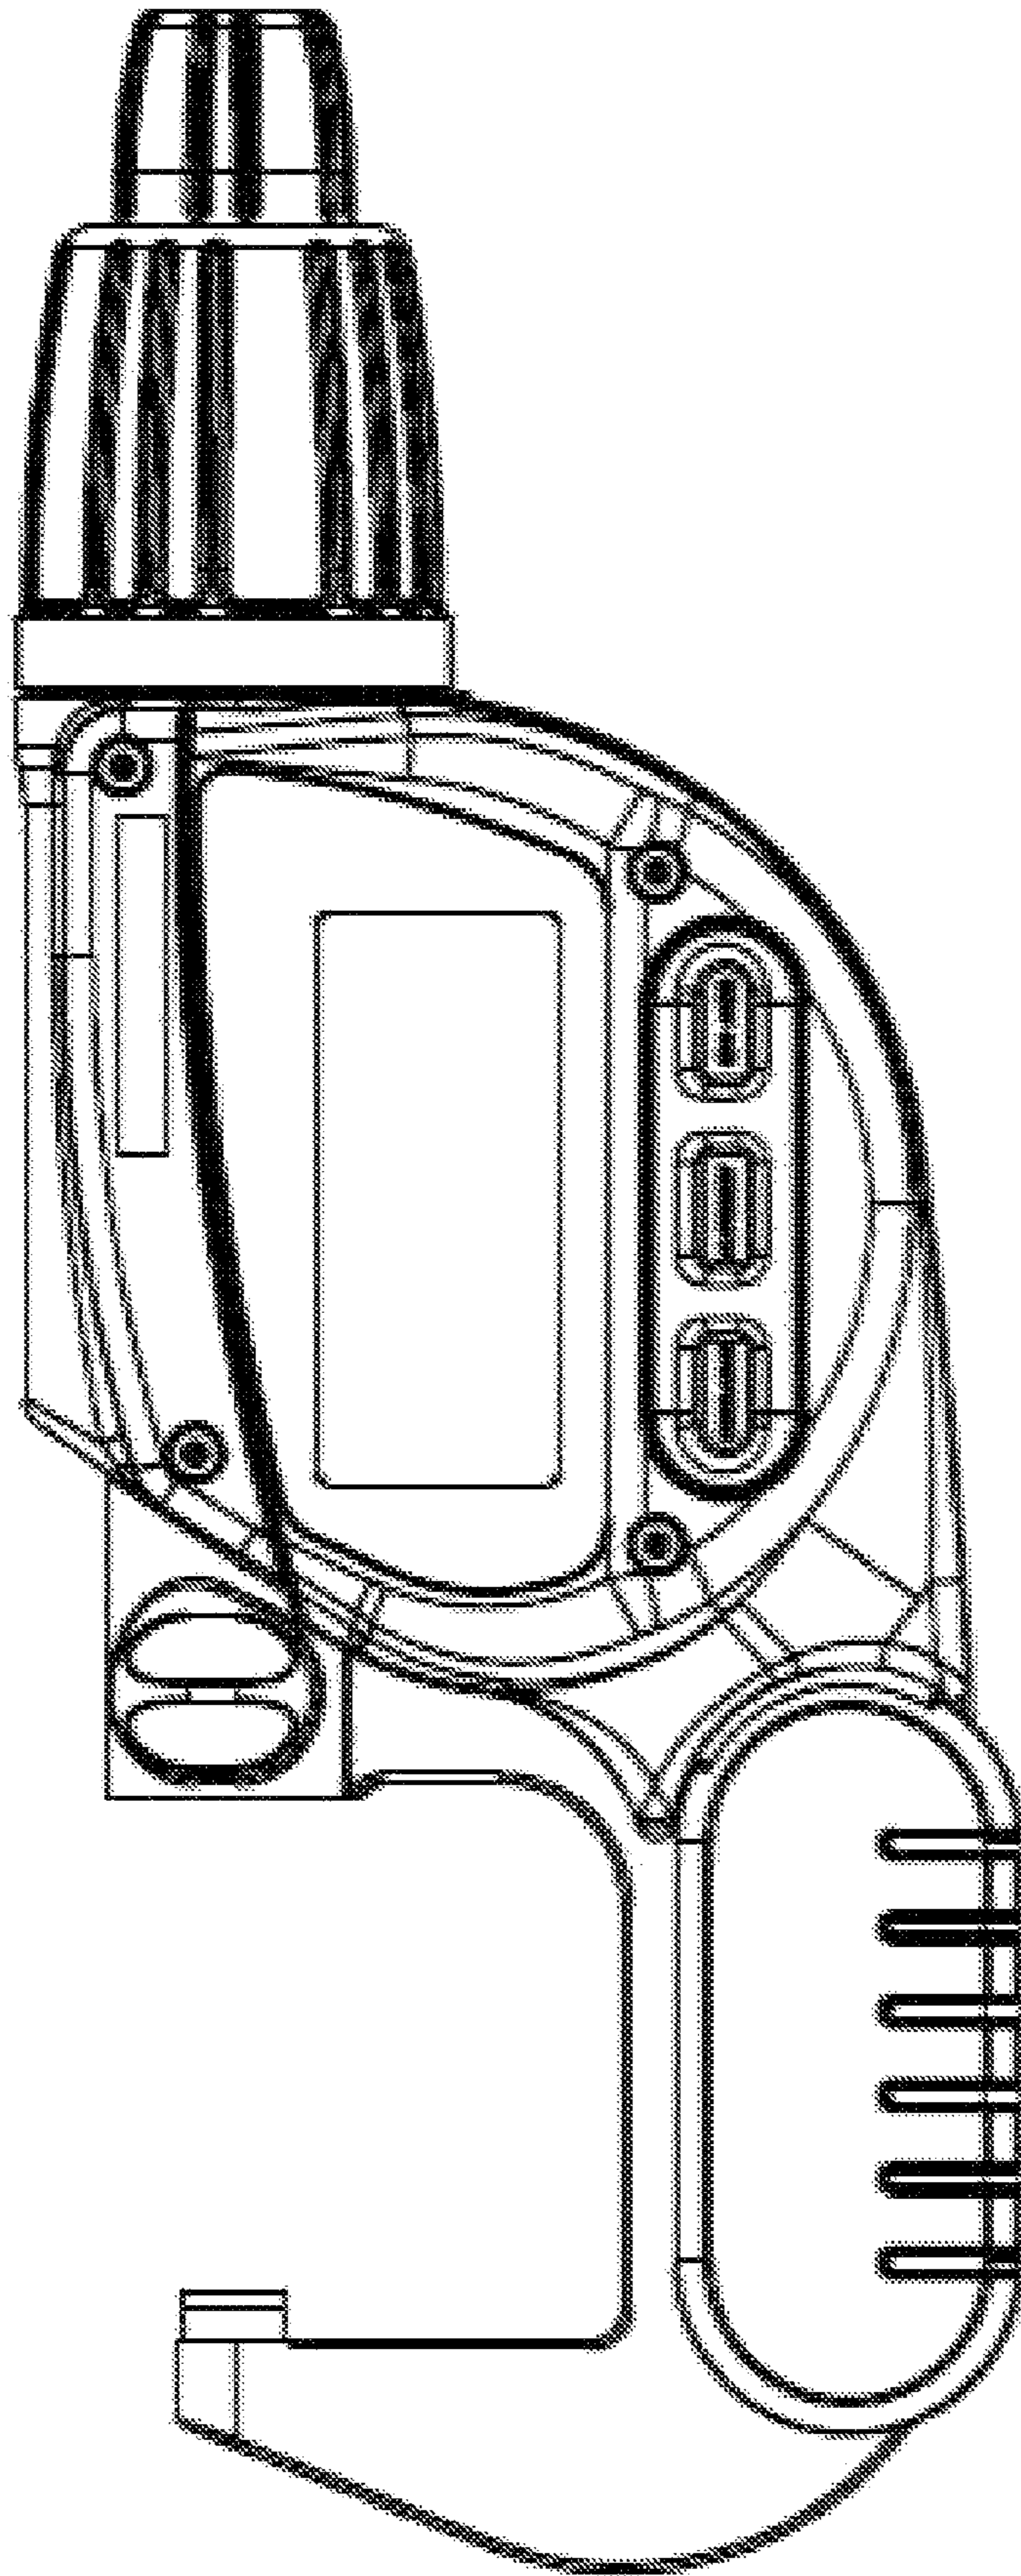


FIG. 2

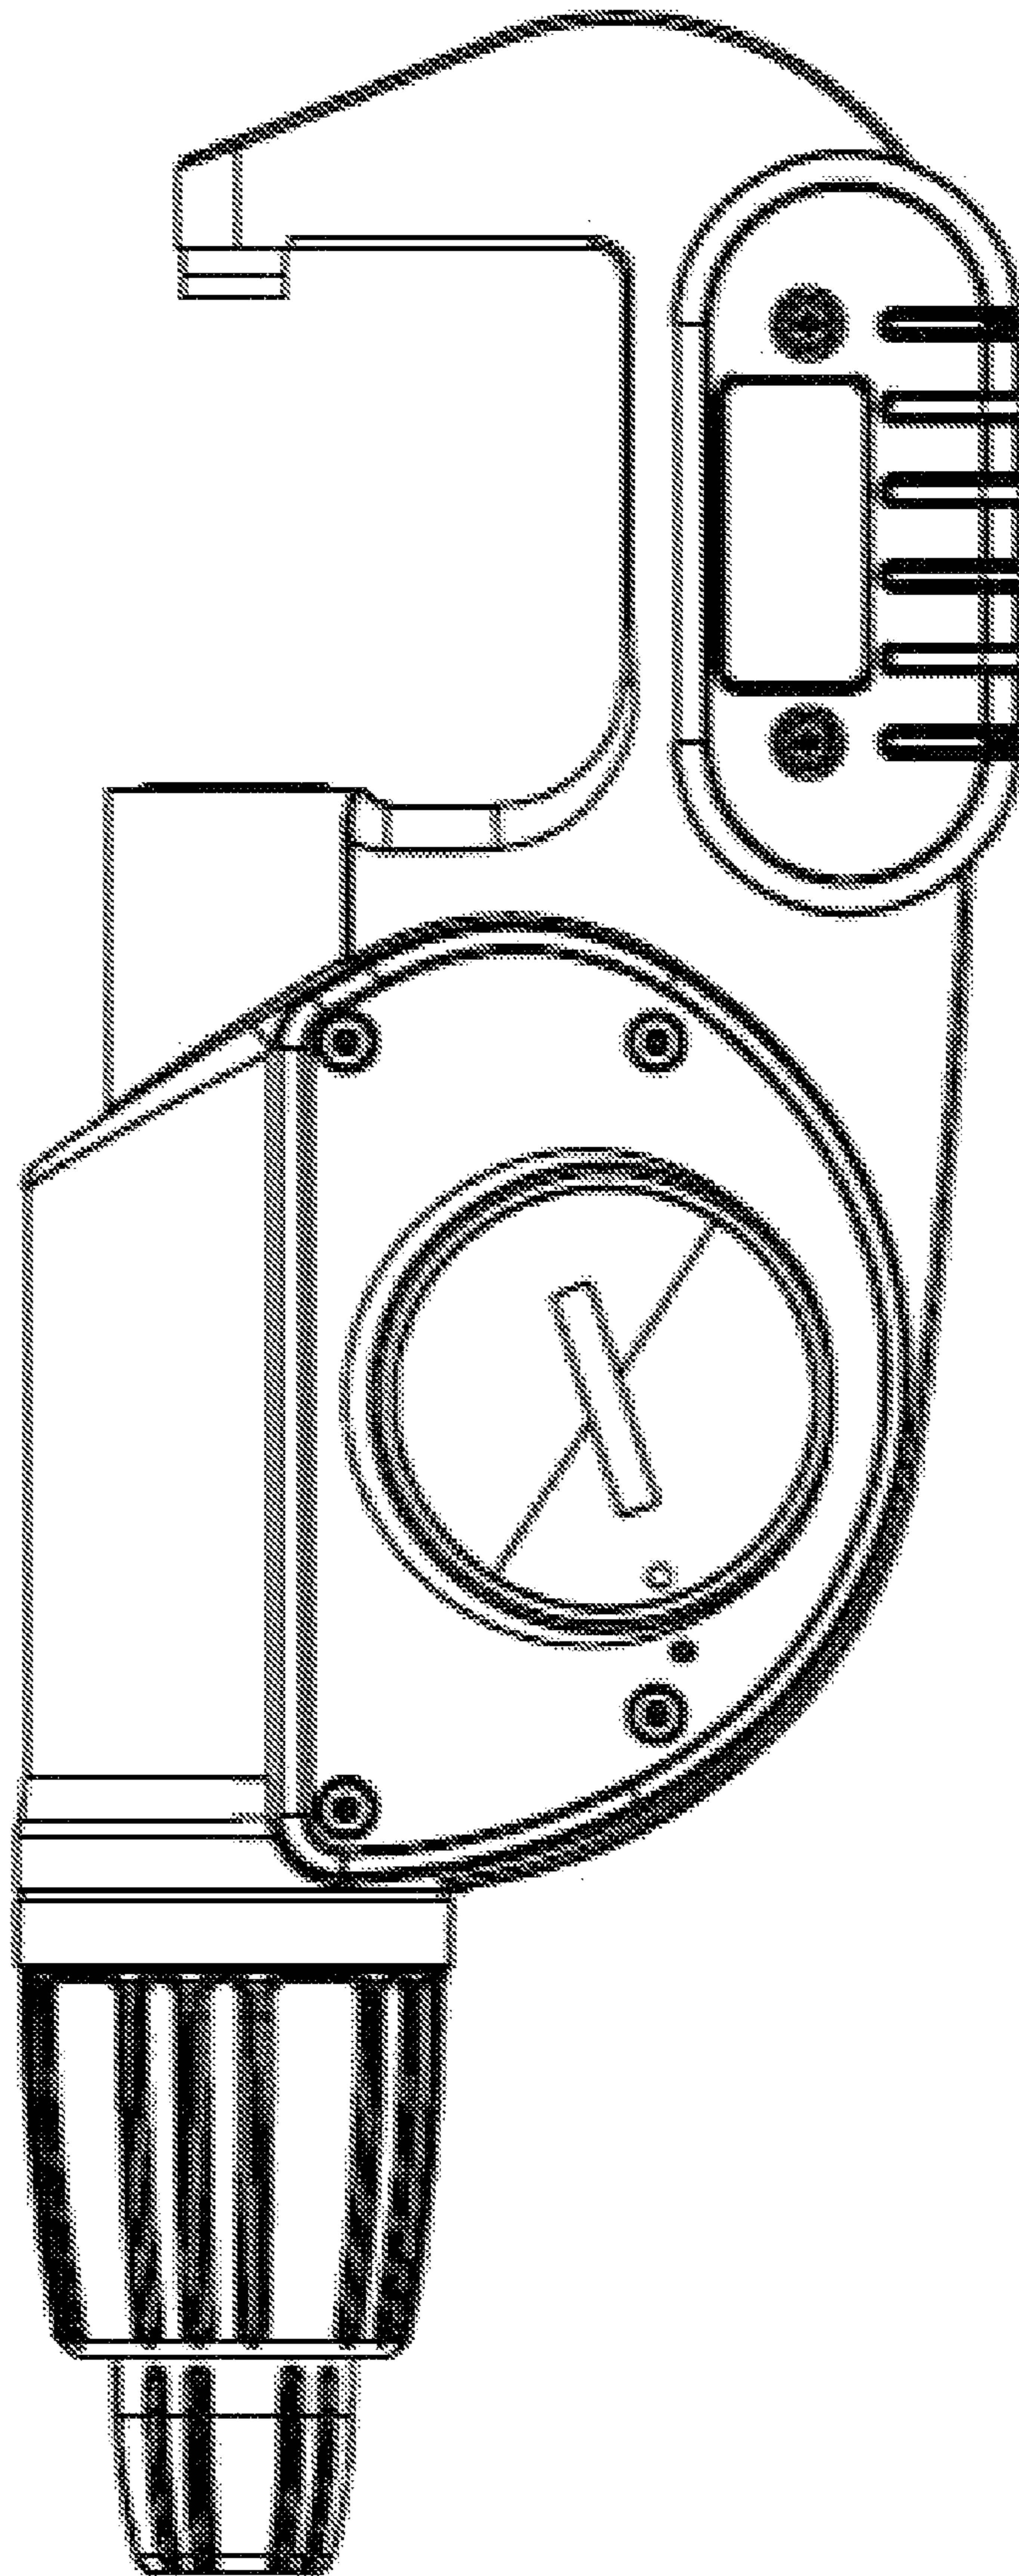


FIG. 3

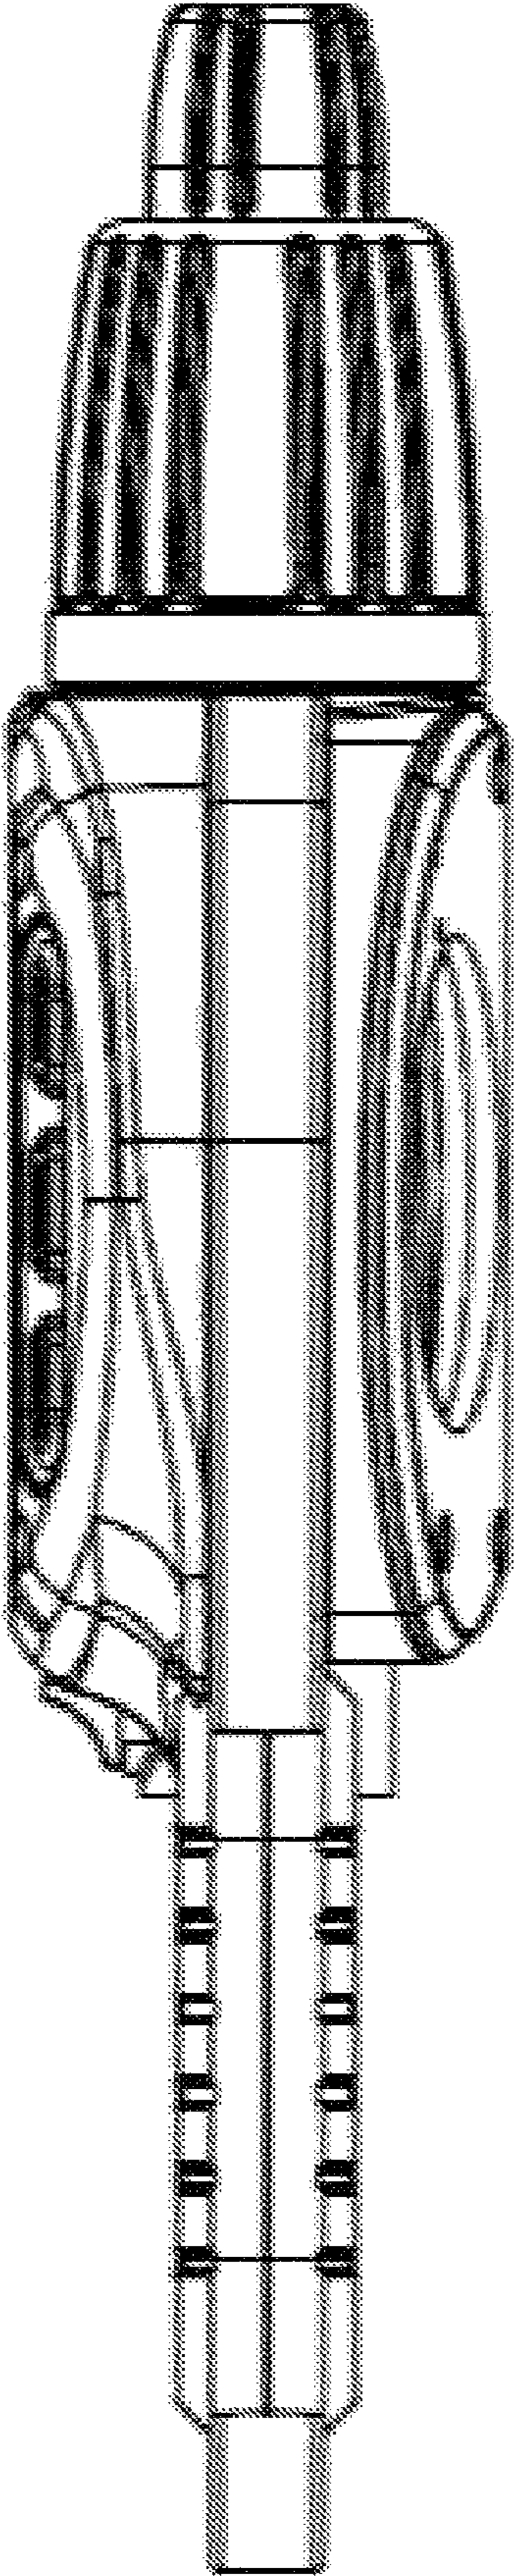


FIG. 4

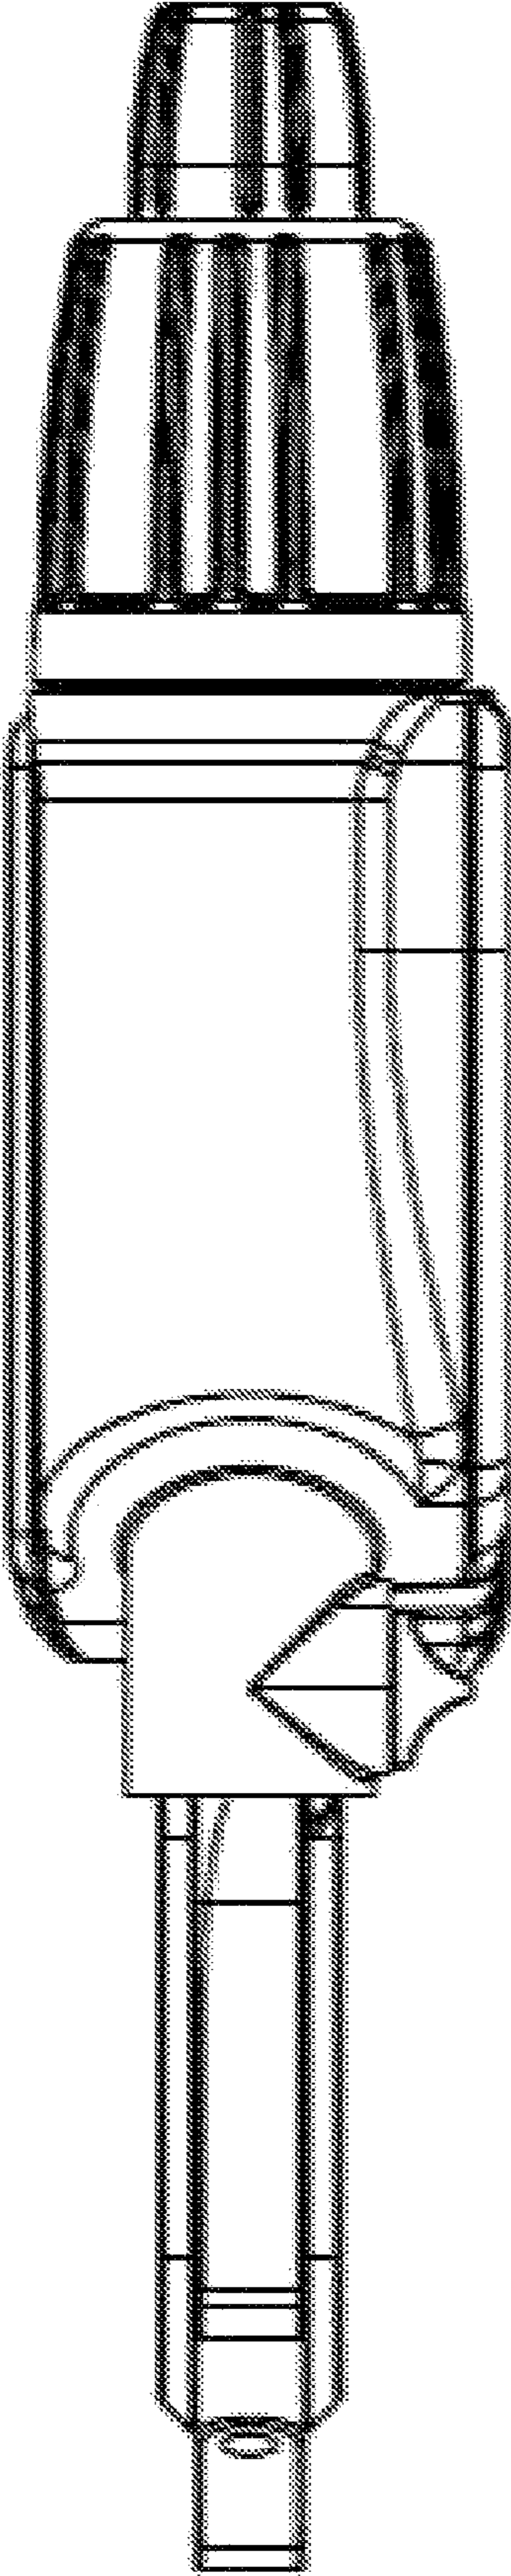


FIG. 5

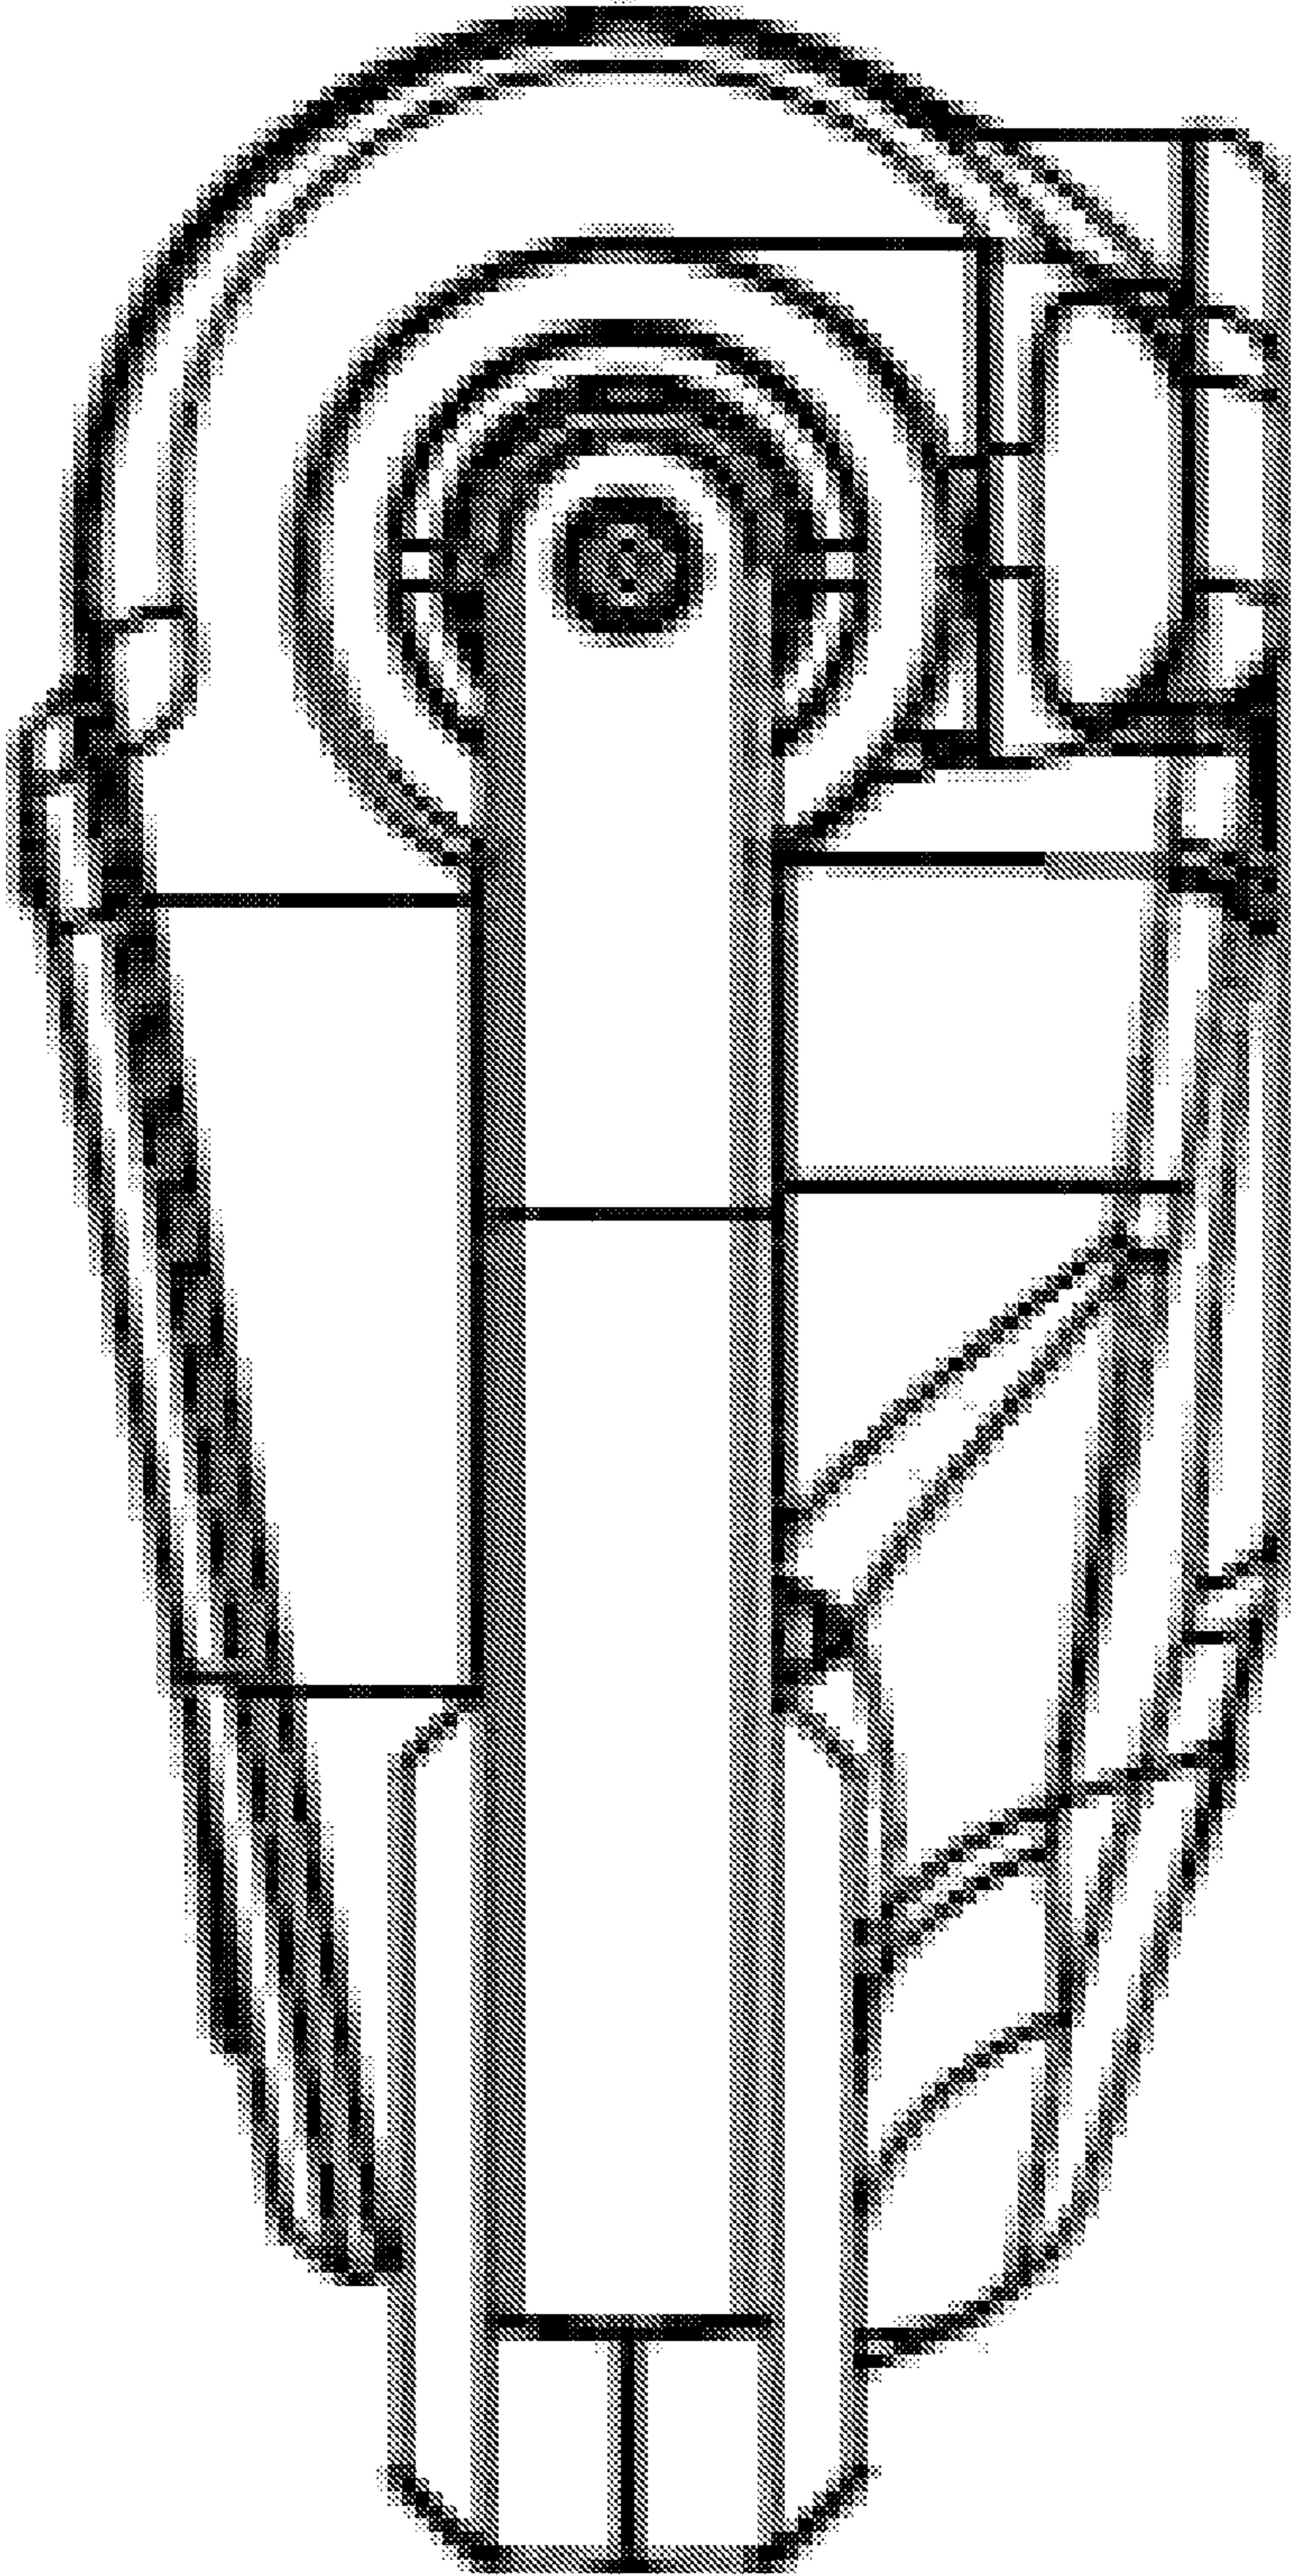


FIG. 6

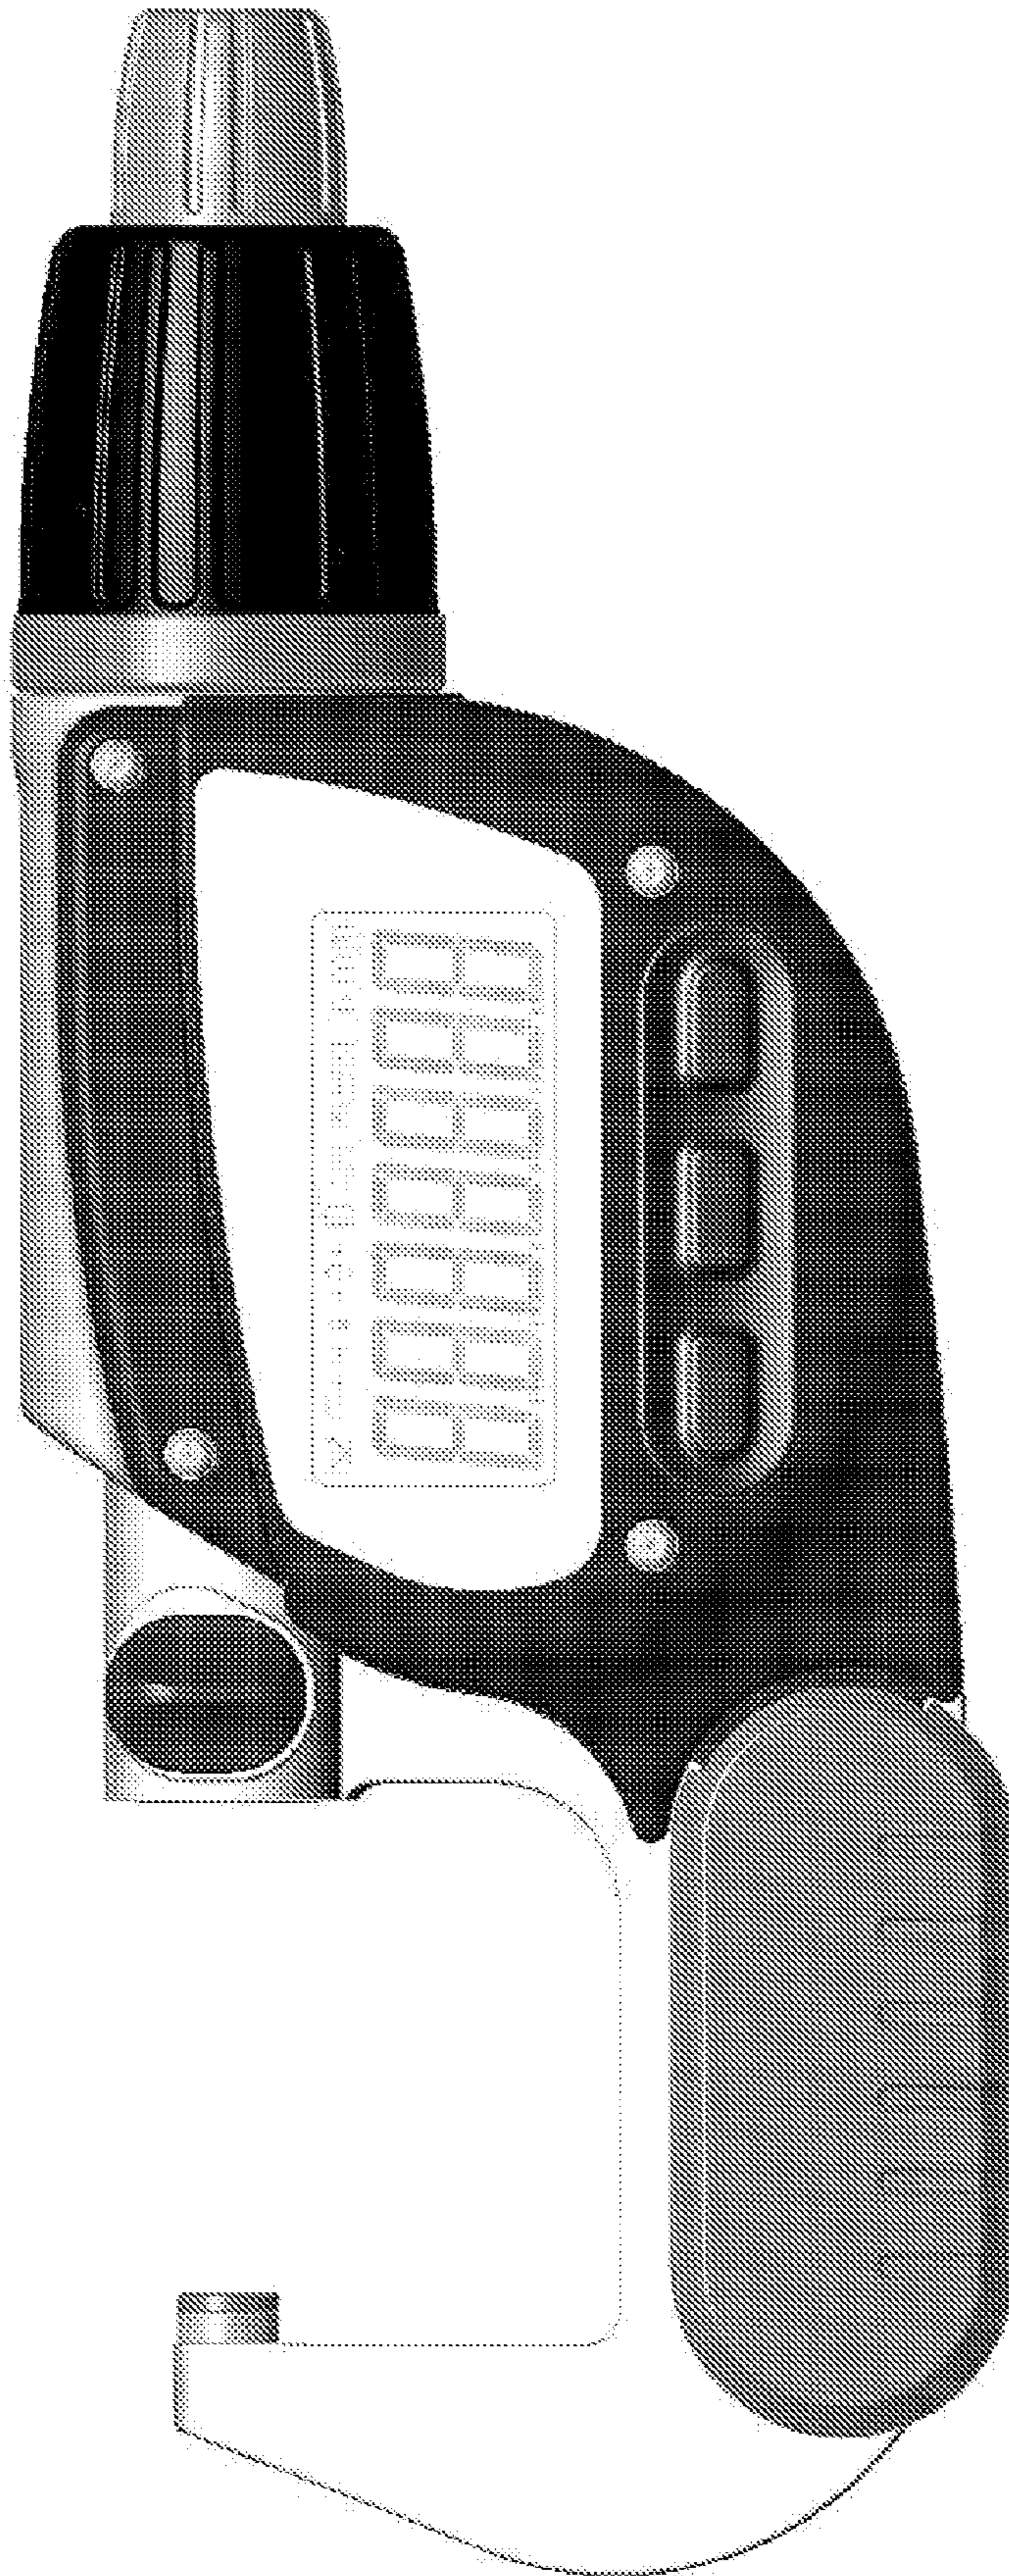


FIG. 7



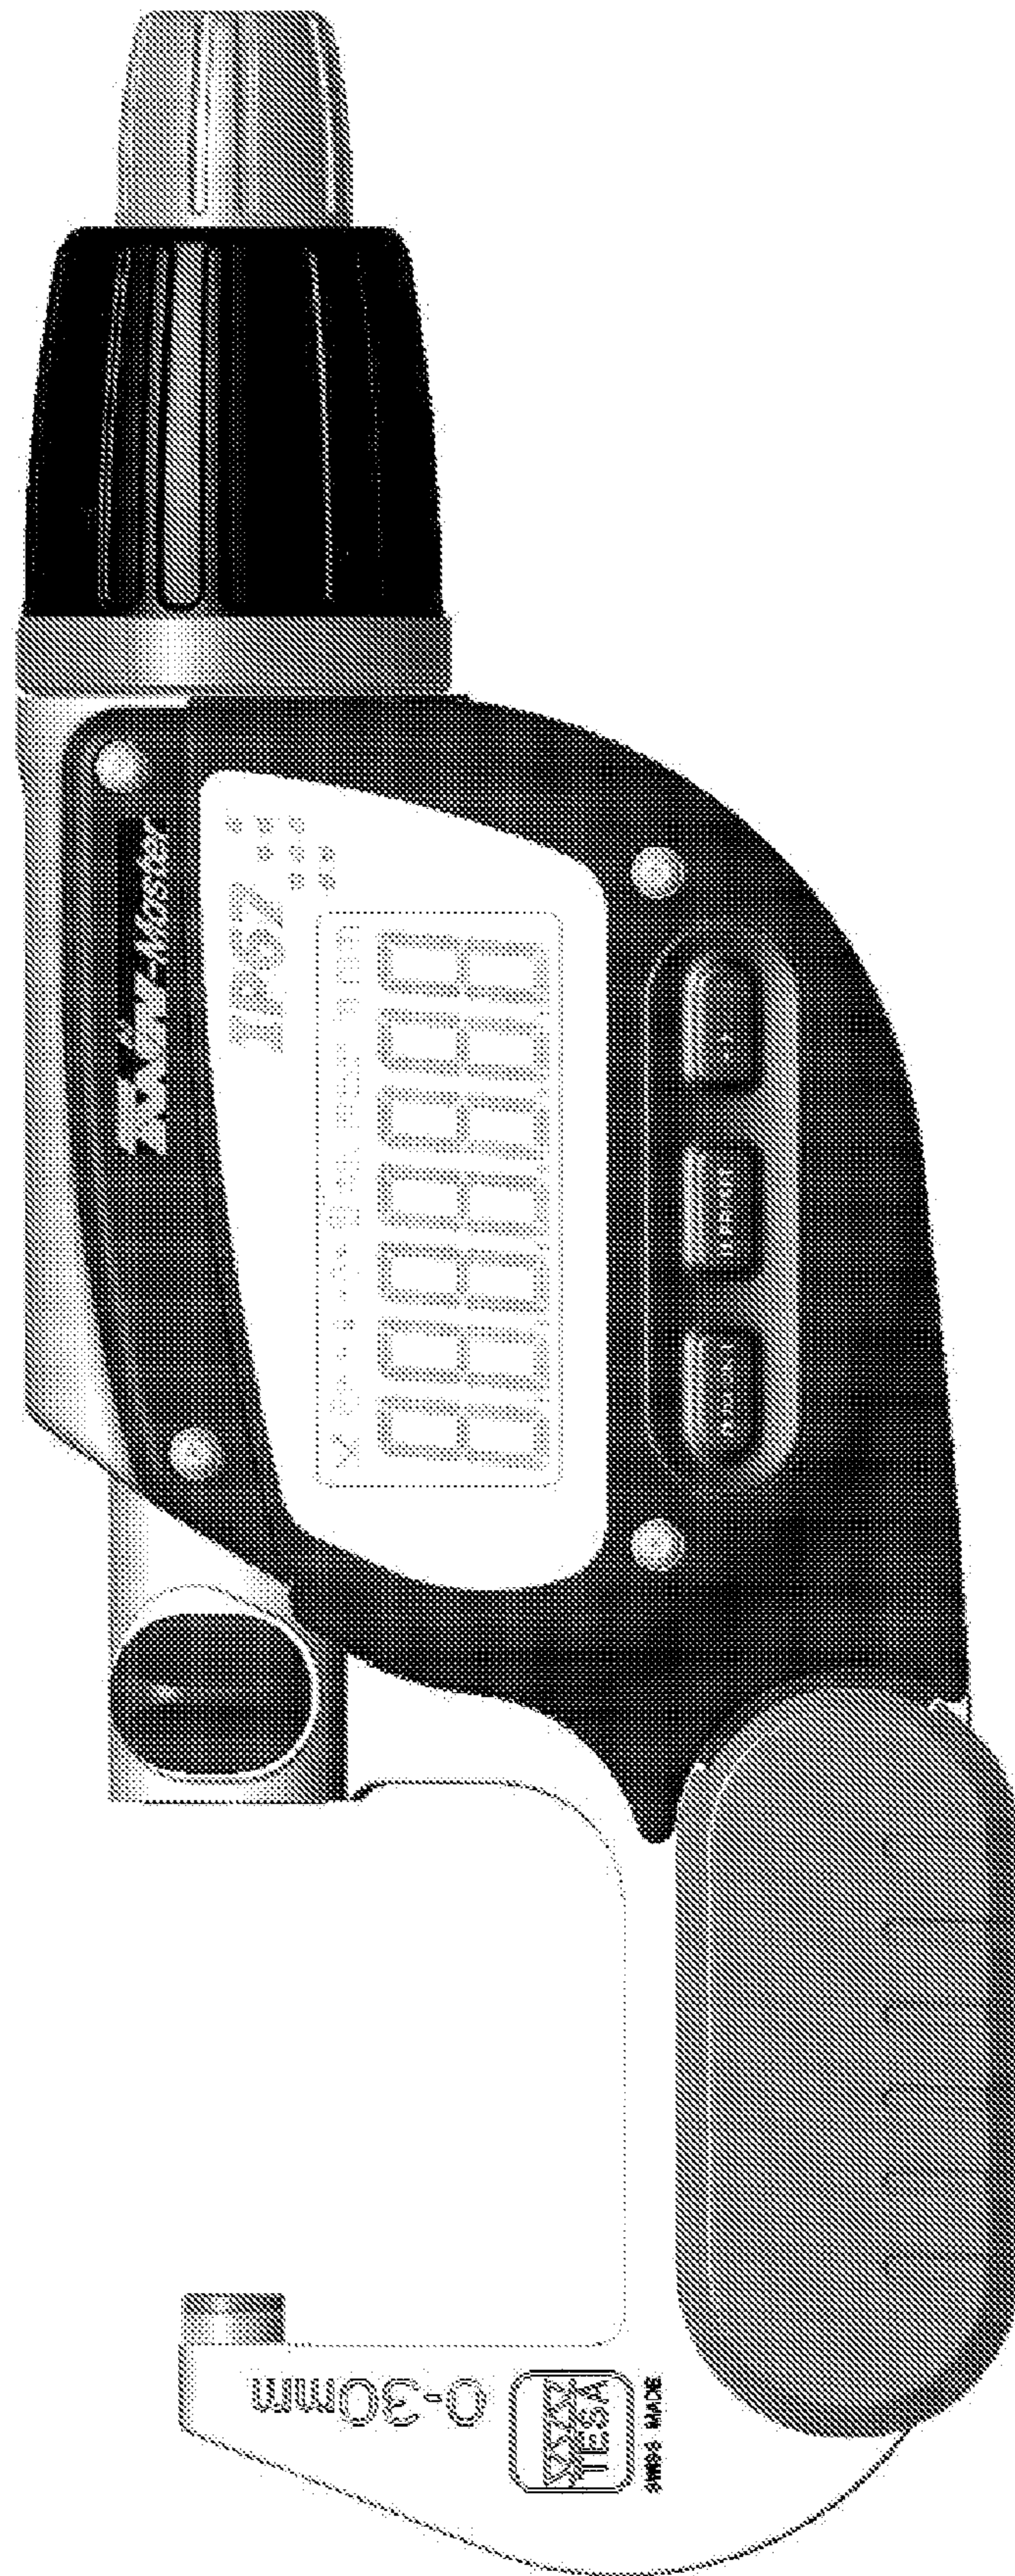


FIG. 8