



US00D730526S

(12) **United States Design Patent**
Shin et al.

(10) **Patent No.:** **US D730,526 S**
(45) **Date of Patent:** **** May 26, 2015**

(54) **HYBRID PULSE MEASURING DEVICE**

(71) Applicant: **SOLMITECH CO., LTD.**, Daejeon (KR)

(72) Inventors: **Seungcheol Shin**, Daejeon (KR);
Gangcheon Lee, Gyeryong-si (KR)

(73) Assignee: **SOLMITECH CO., LTD.**, Daejeon (KR)

(**) Term: **14 Years**

(21) Appl. No.: **29/473,140**

(22) Filed: **Nov. 19, 2013**

(51) **LOC (10) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/167; D24/165**

(58) **Field of Classification Search**
USPC D24/165–168, 169, 186, 107, 187;
D10/75, 98, 31, 32; 600/301, 481–483,
600/485, 490, 493–495, 500, 503, 509;
128/900; D11/3, 4; D14/138 R
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D365,285	S	*	12/1995	Nanayakkara	D10/31
6,928,317	B2	*	8/2005	Chen	600/509
D535,205	S	*	1/2007	Frederick et al.	D10/32
D645,360	S	*	9/2011	Kiser et al.	D10/32
D667,126	S	*	9/2012	Cho et al.	D24/186
D674,488	S	*	1/2013	McKay et al.	D24/167

D687,951	S	*	8/2013	Della Torre et al.	D24/167
D709,476	S	*	7/2014	Park et al.	D14/138 R
D711,002	S	*	8/2014	Ohnemus et al.	D24/186
2004/0138573	A1	*	7/2004	Chen	600/509
2010/0076331	A1	*	3/2010	Chan et al.	600/522
2011/0275940	A1	*	11/2011	Nims et al.	600/483
2013/0109984	A1	*	5/2013	Su	600/509

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Drinker Biddle & Reath LLP

(57) **CLAIM**

The ornamental design for a hybrid pulse measuring device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the hybrid pulse measuring device according to the present invention;
FIG. 2 is a front view of the hybrid pulse measuring device of FIG. 1;
FIG. 3 is a rear view of the hybrid pulse measuring device of FIG. 1;
FIG. 4 is a left side view of the hybrid pulse measuring device of FIG. 1;
FIG. 5 is a right side view of the hybrid pulse measuring device of FIG. 1;
FIG. 6 is a top view of the hybrid pulse measuring device of FIG. 1; and,
FIG. 7 is a bottom view of the hybrid pulse measuring device of FIG. 1.

1 Claim, 5 Drawing Sheets

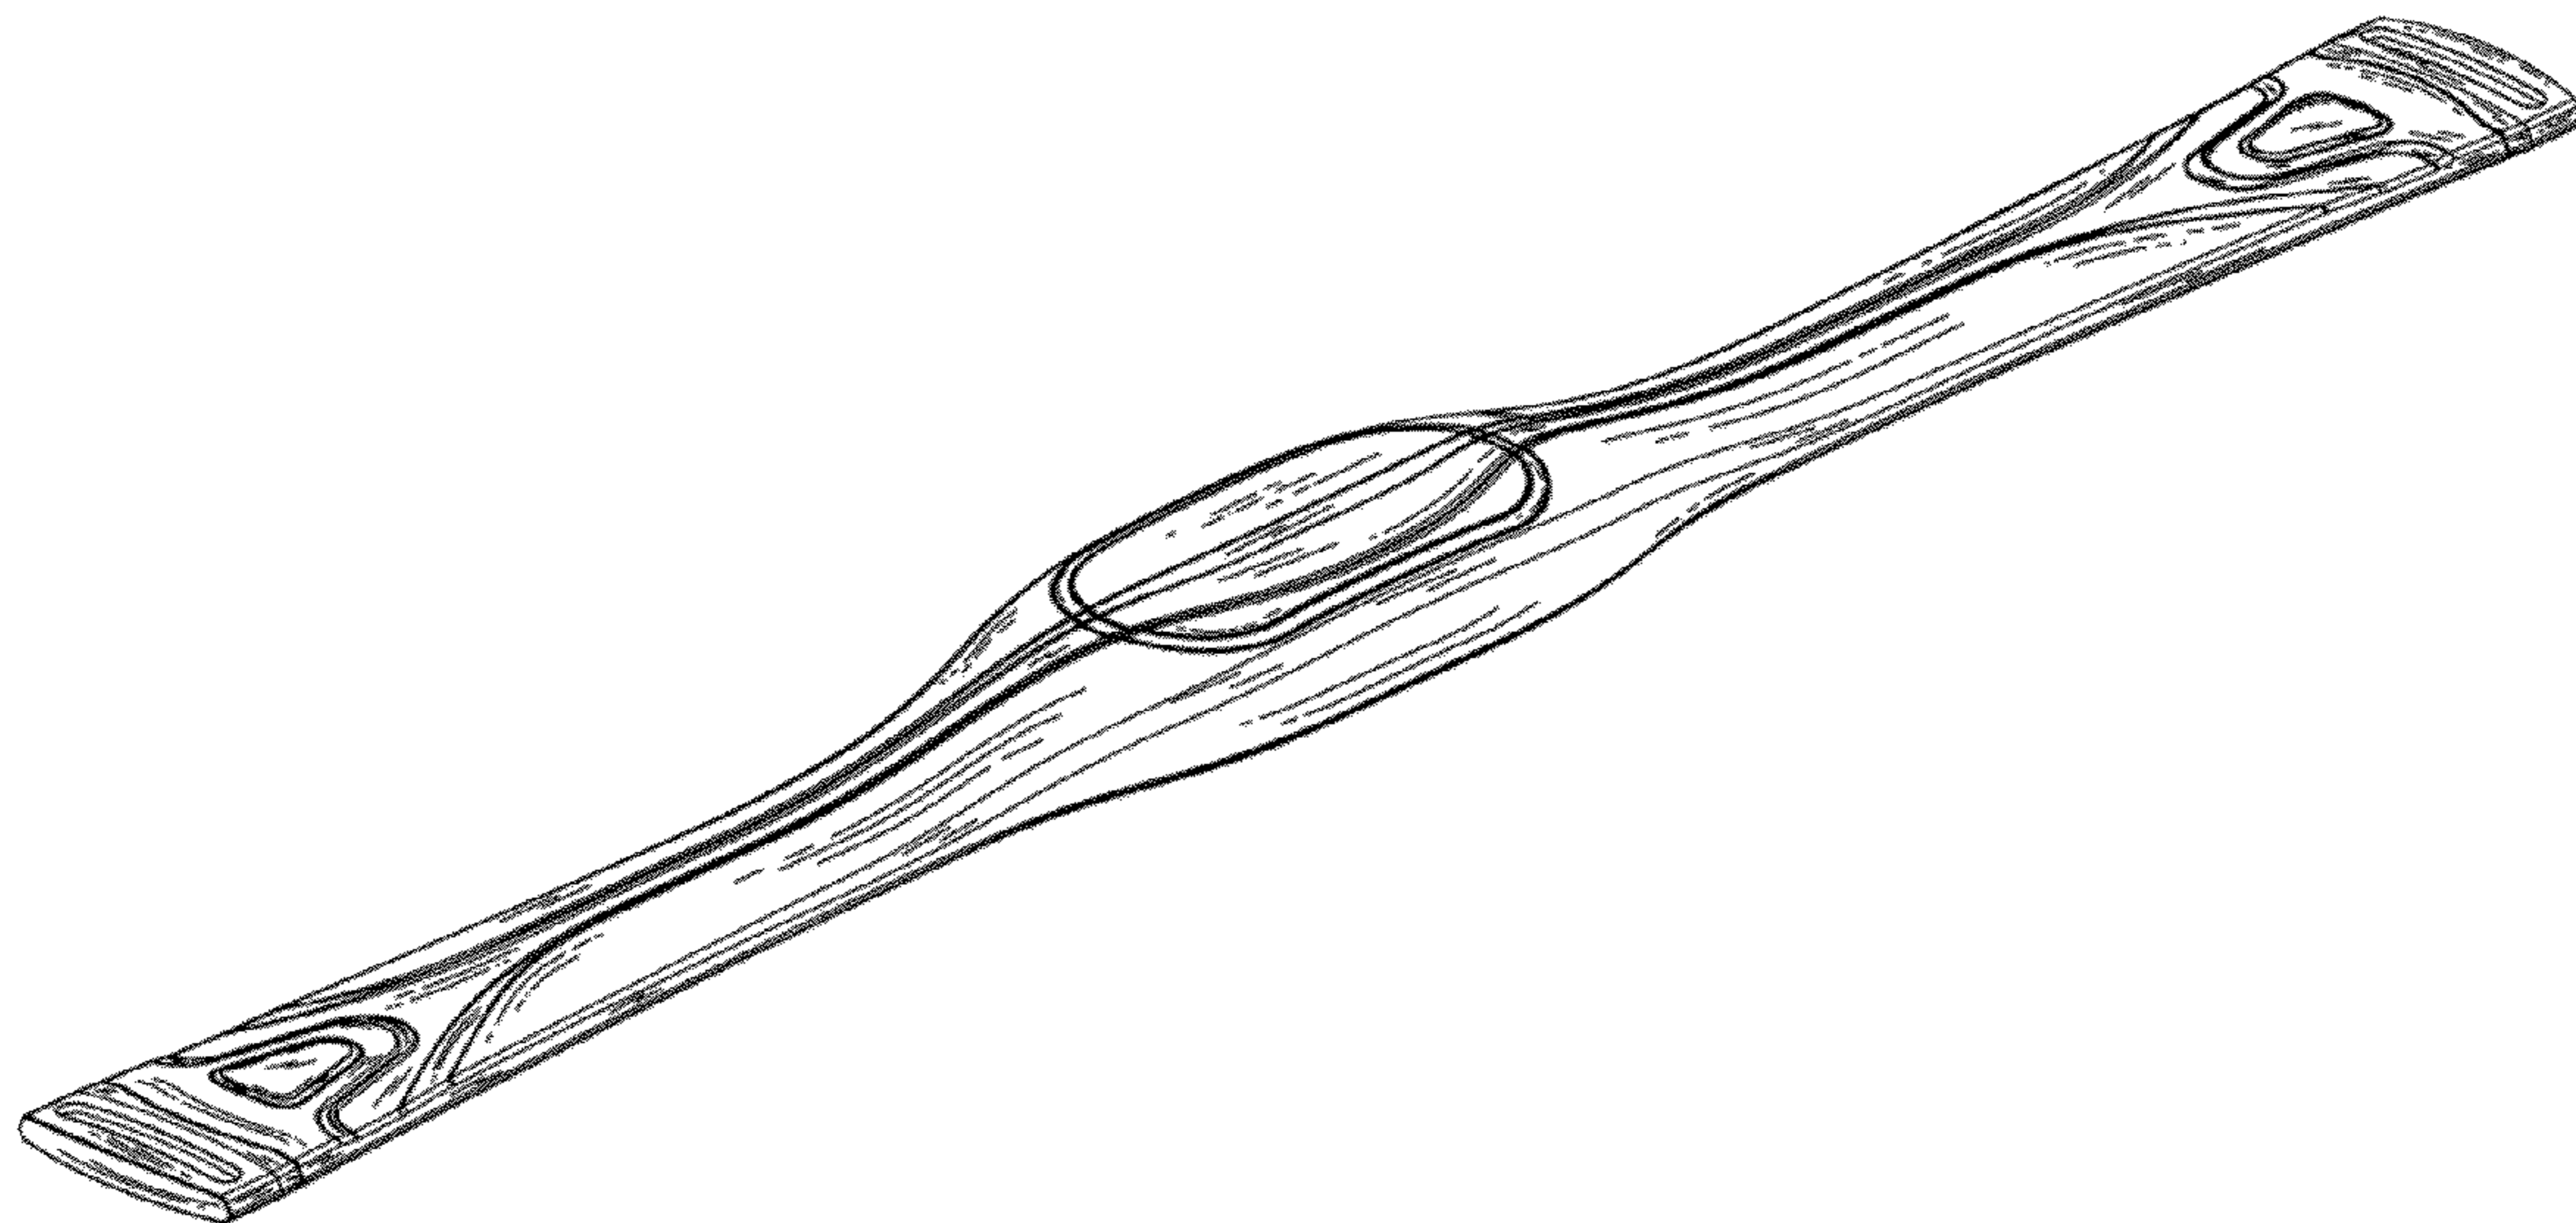


FIG. 1

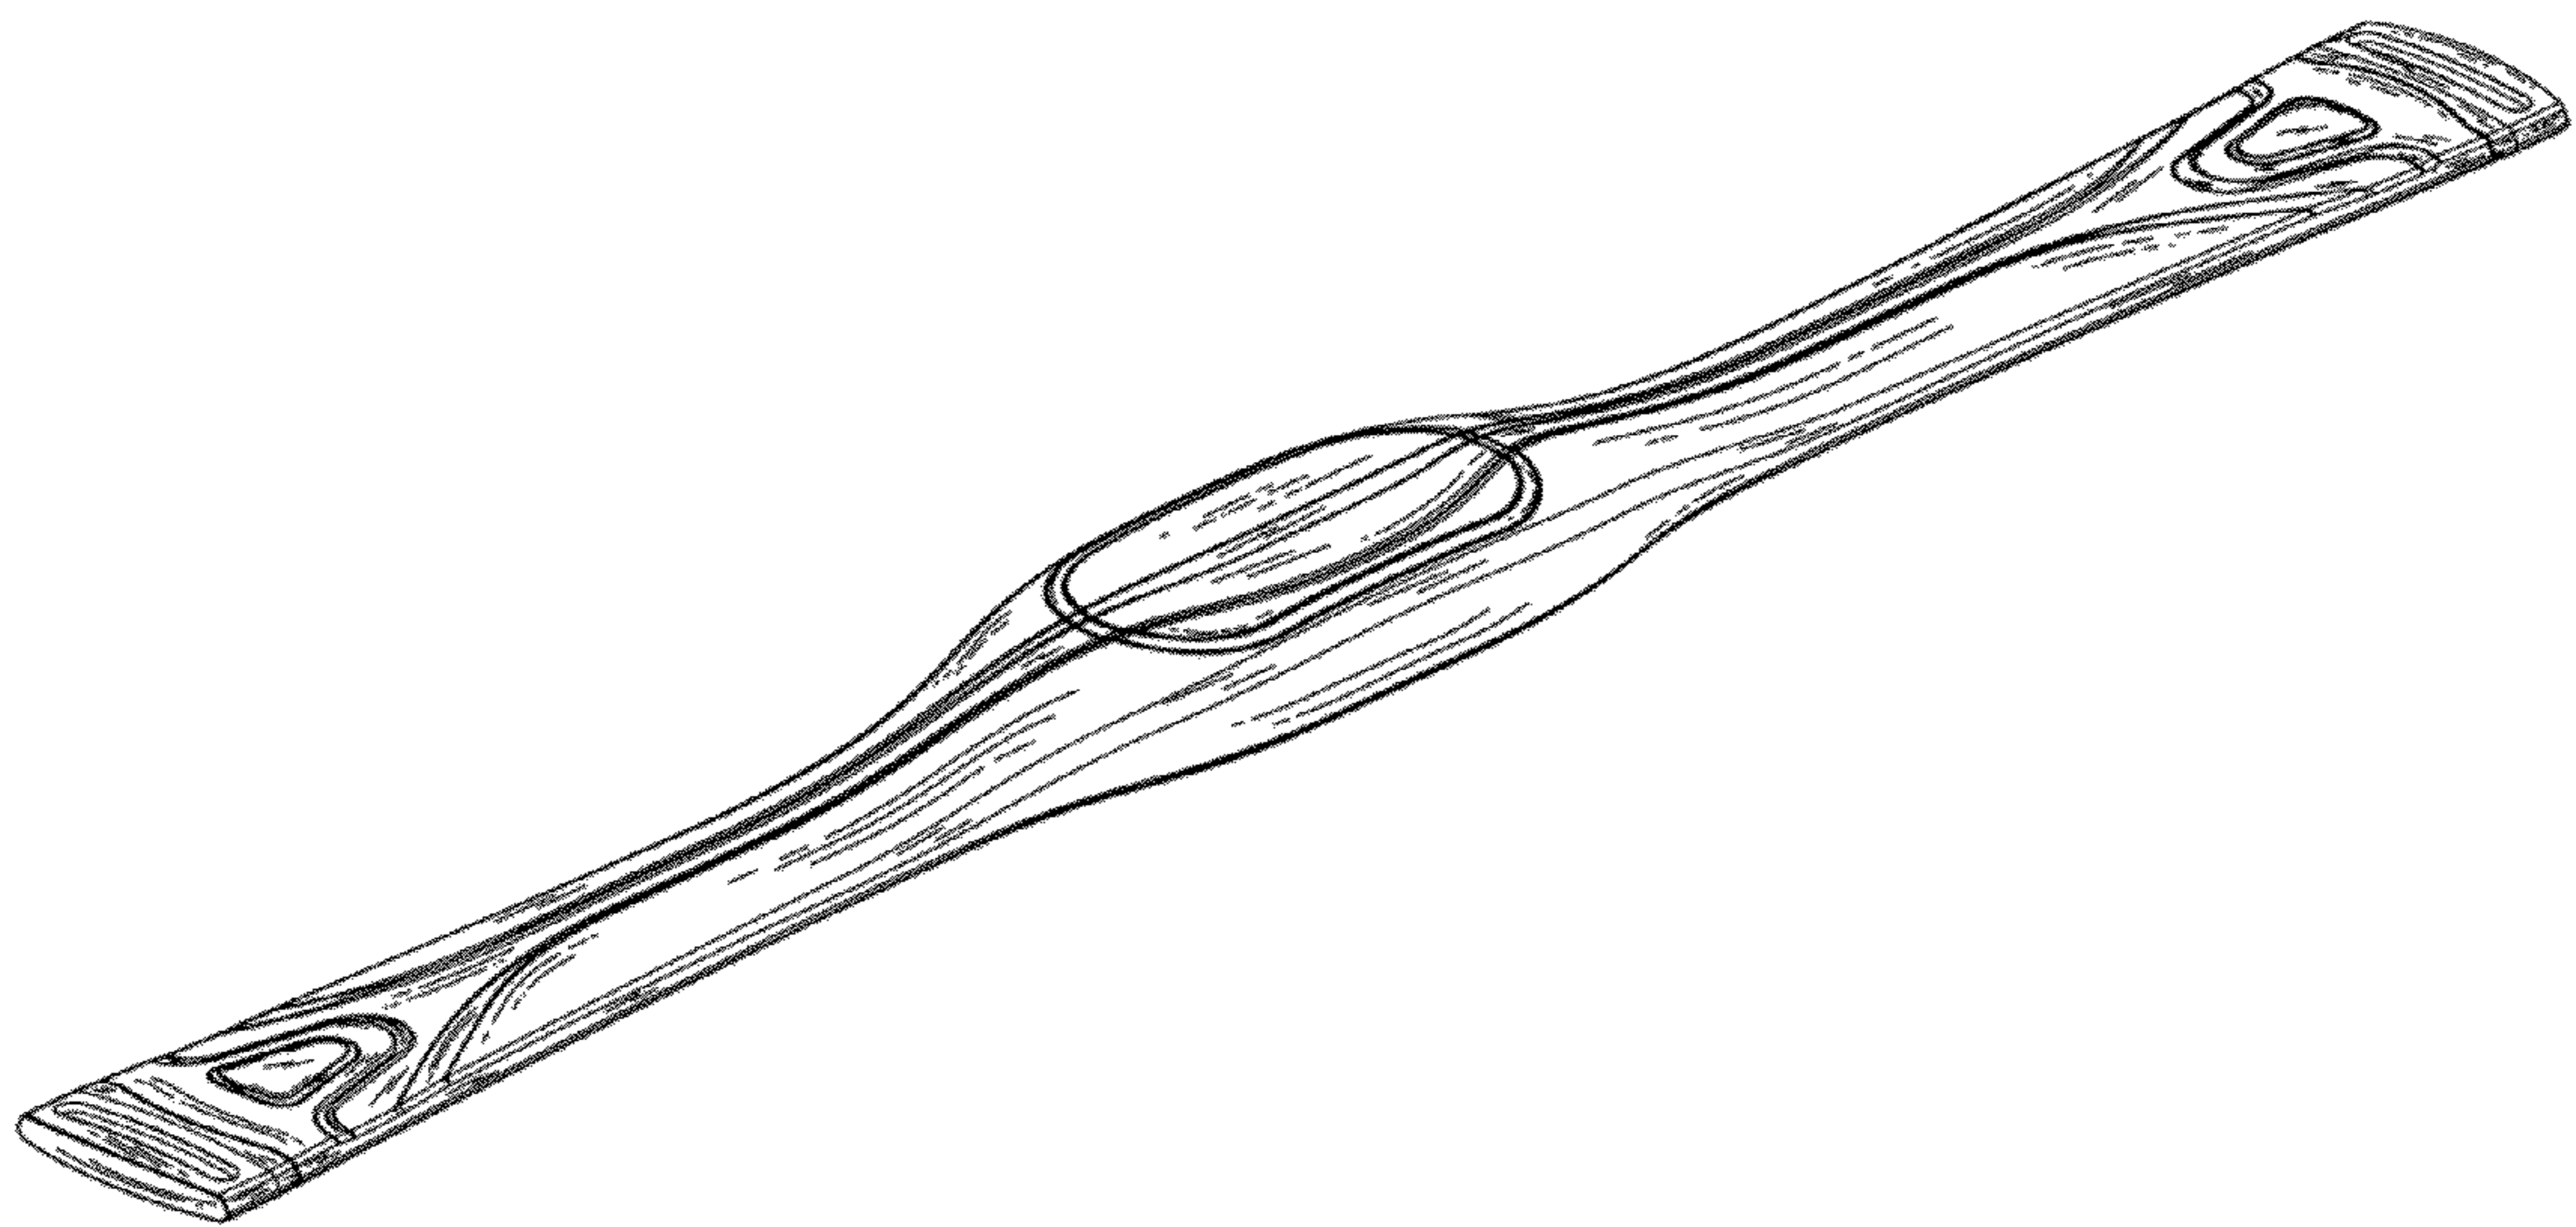


FIG. 2



FIG. 3



FIG. 4

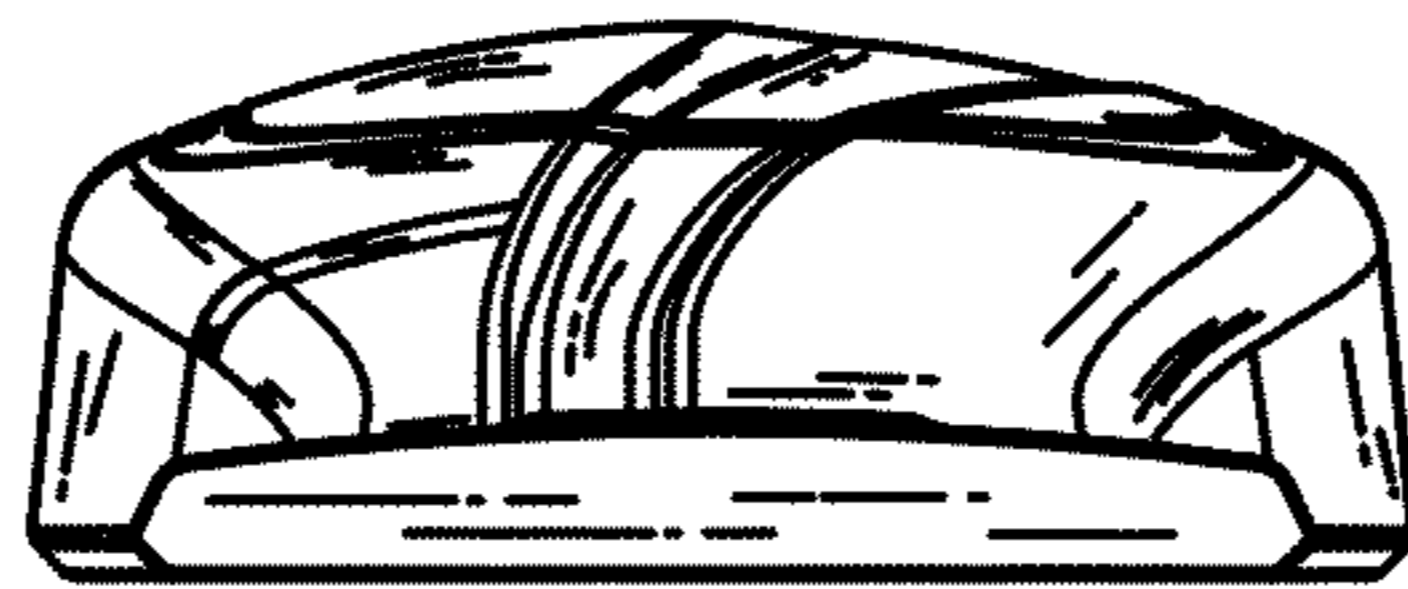


FIG. 5

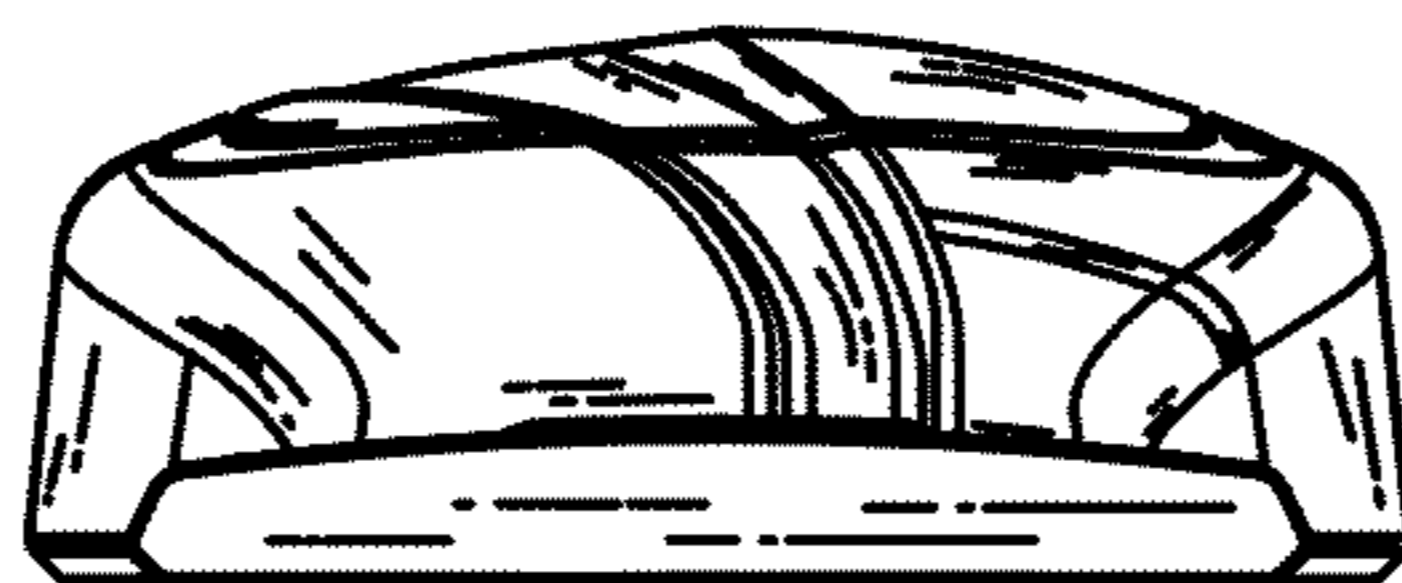


FIG. 6

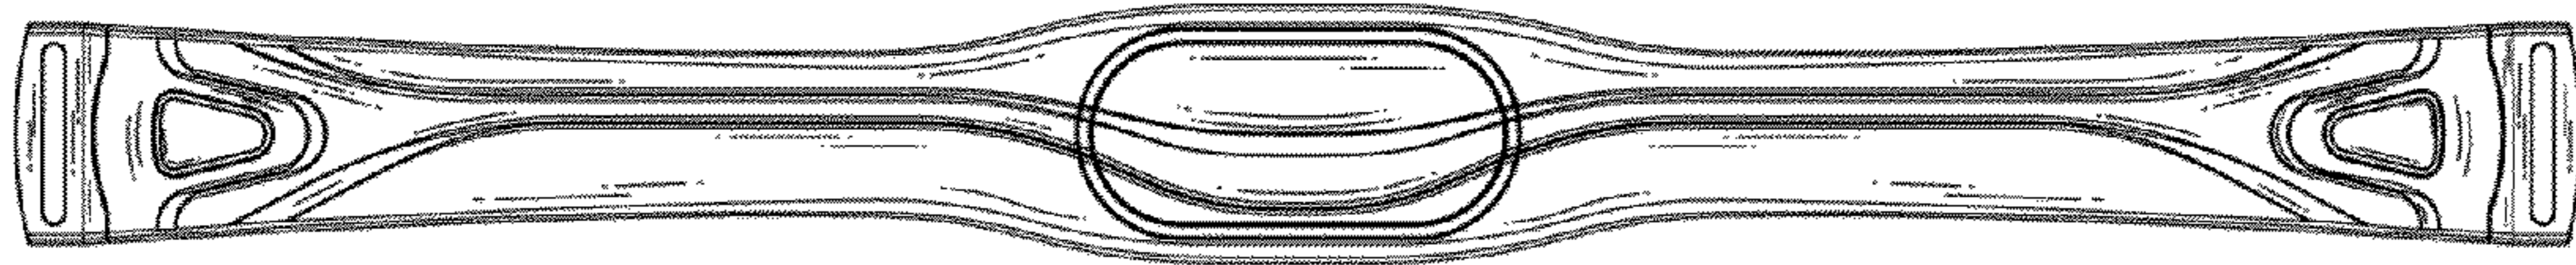


FIG. 7

