



US00D733874S

(12) **United States Design Patent**
Yu et al.

(10) **Patent No.:** **US D733,874 S**
(45) **Date of Patent:** **** Jul. 7, 2015**

- (54) **CONTROL HANDLE FOR A MEDICAL DEVICE**
- (71) Applicant: **St. Jude Medical, Atrial Fibrillation Division, Inc.**, St. Paul, MN (US)
- (72) Inventors: **Alex Yu**, Minneapolis, MN (US);
Stephen W. Evans, Plymouth, MN (US)
- (73) Assignee: **St. Jude Medical, Atrial Fibrillation Division, Inc.**, St. Paul, MN (US)
- (**) Term: **14 Years**
- (21) Appl. No.: **29/501,305**
- (22) Filed: **Sep. 3, 2014**

Related U.S. Application Data

- (62) Division of application No. 29/420,271, filed on May 7, 2012, now Pat. No. Des. 715,429.
- (51) **LOC (10) Cl.** **24-02**
- (52) **U.S. Cl.**
USPC **D24/130**
- (58) **Field of Classification Search**
USPC D24/127, 130, 112–113, 186, 133, 138;
606/181, 185; 604/533, 534, 284, 115,
604/19, 48, 164.01–164.09; 600/226,
600/372–374, 585, 114; 128/200.24,
128/207.14, 207.15
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D345,419 S *	3/1994	Horrigan et al.	D24/130
D351,652 S *	10/1994	Thompson et al.	D24/138
7,194,294 B2 *	3/2007	Panescu et al.	600/374
7,606,609 B2	10/2009	Muranushi et al.		
D612,044 S	3/2010	Scheibe		
D655,406 S *	3/2012	Ma et al.	D24/112
8,725,228 B2 *	5/2014	Koblish et al.	600/374

OTHER PUBLICATIONS

Title: Safire BLU Bi-Directional Ablation Catheter Irrigated 4 mm Tip Thermocouple Quadripolar, Citation: St. Jude Medical Electrophysiology International Catalogue, Reference pp. 169, Publication Date 2010.
Title: Therapy 4mm, Bidirectional Catheter Deflection, Citation: St. Jude Medical, Inc., Ordering Information and Accessories, Publication Date: 2010.

* cited by examiner

Primary Examiner — Robert Delehanty

(74) *Attorney, Agent, or Firm* — Dykema Gossett PLLC


(57) **CLAIM**

The ornamental design for a control handle for a medical device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an embodiment of a control handle for a medical device showing a new design;
FIG. 2 is a front view thereof;
FIG. 3 is a back view thereof;
FIG. 4 is a right view thereof;
FIG. 5 is a left view thereof;
FIG. 6 is a top side view thereof; and
FIG. 7 is a bottom side view thereof.
FIG. 8 is a perspective view of a second embodiment of a control handle for a medical device showing a new design;
FIG. 9 is a front view thereof;
FIG. 10 is a back view thereof;
FIG. 11 is a right view thereof;
FIG. 12 is a left view thereof;
FIG. 13 is a top side view thereof; and,
FIG. 14 is a bottom side view thereof.
The broken lines are for purposes of illustration only and form no part of the claimed design.

1 Claim, 12 Drawing Sheets

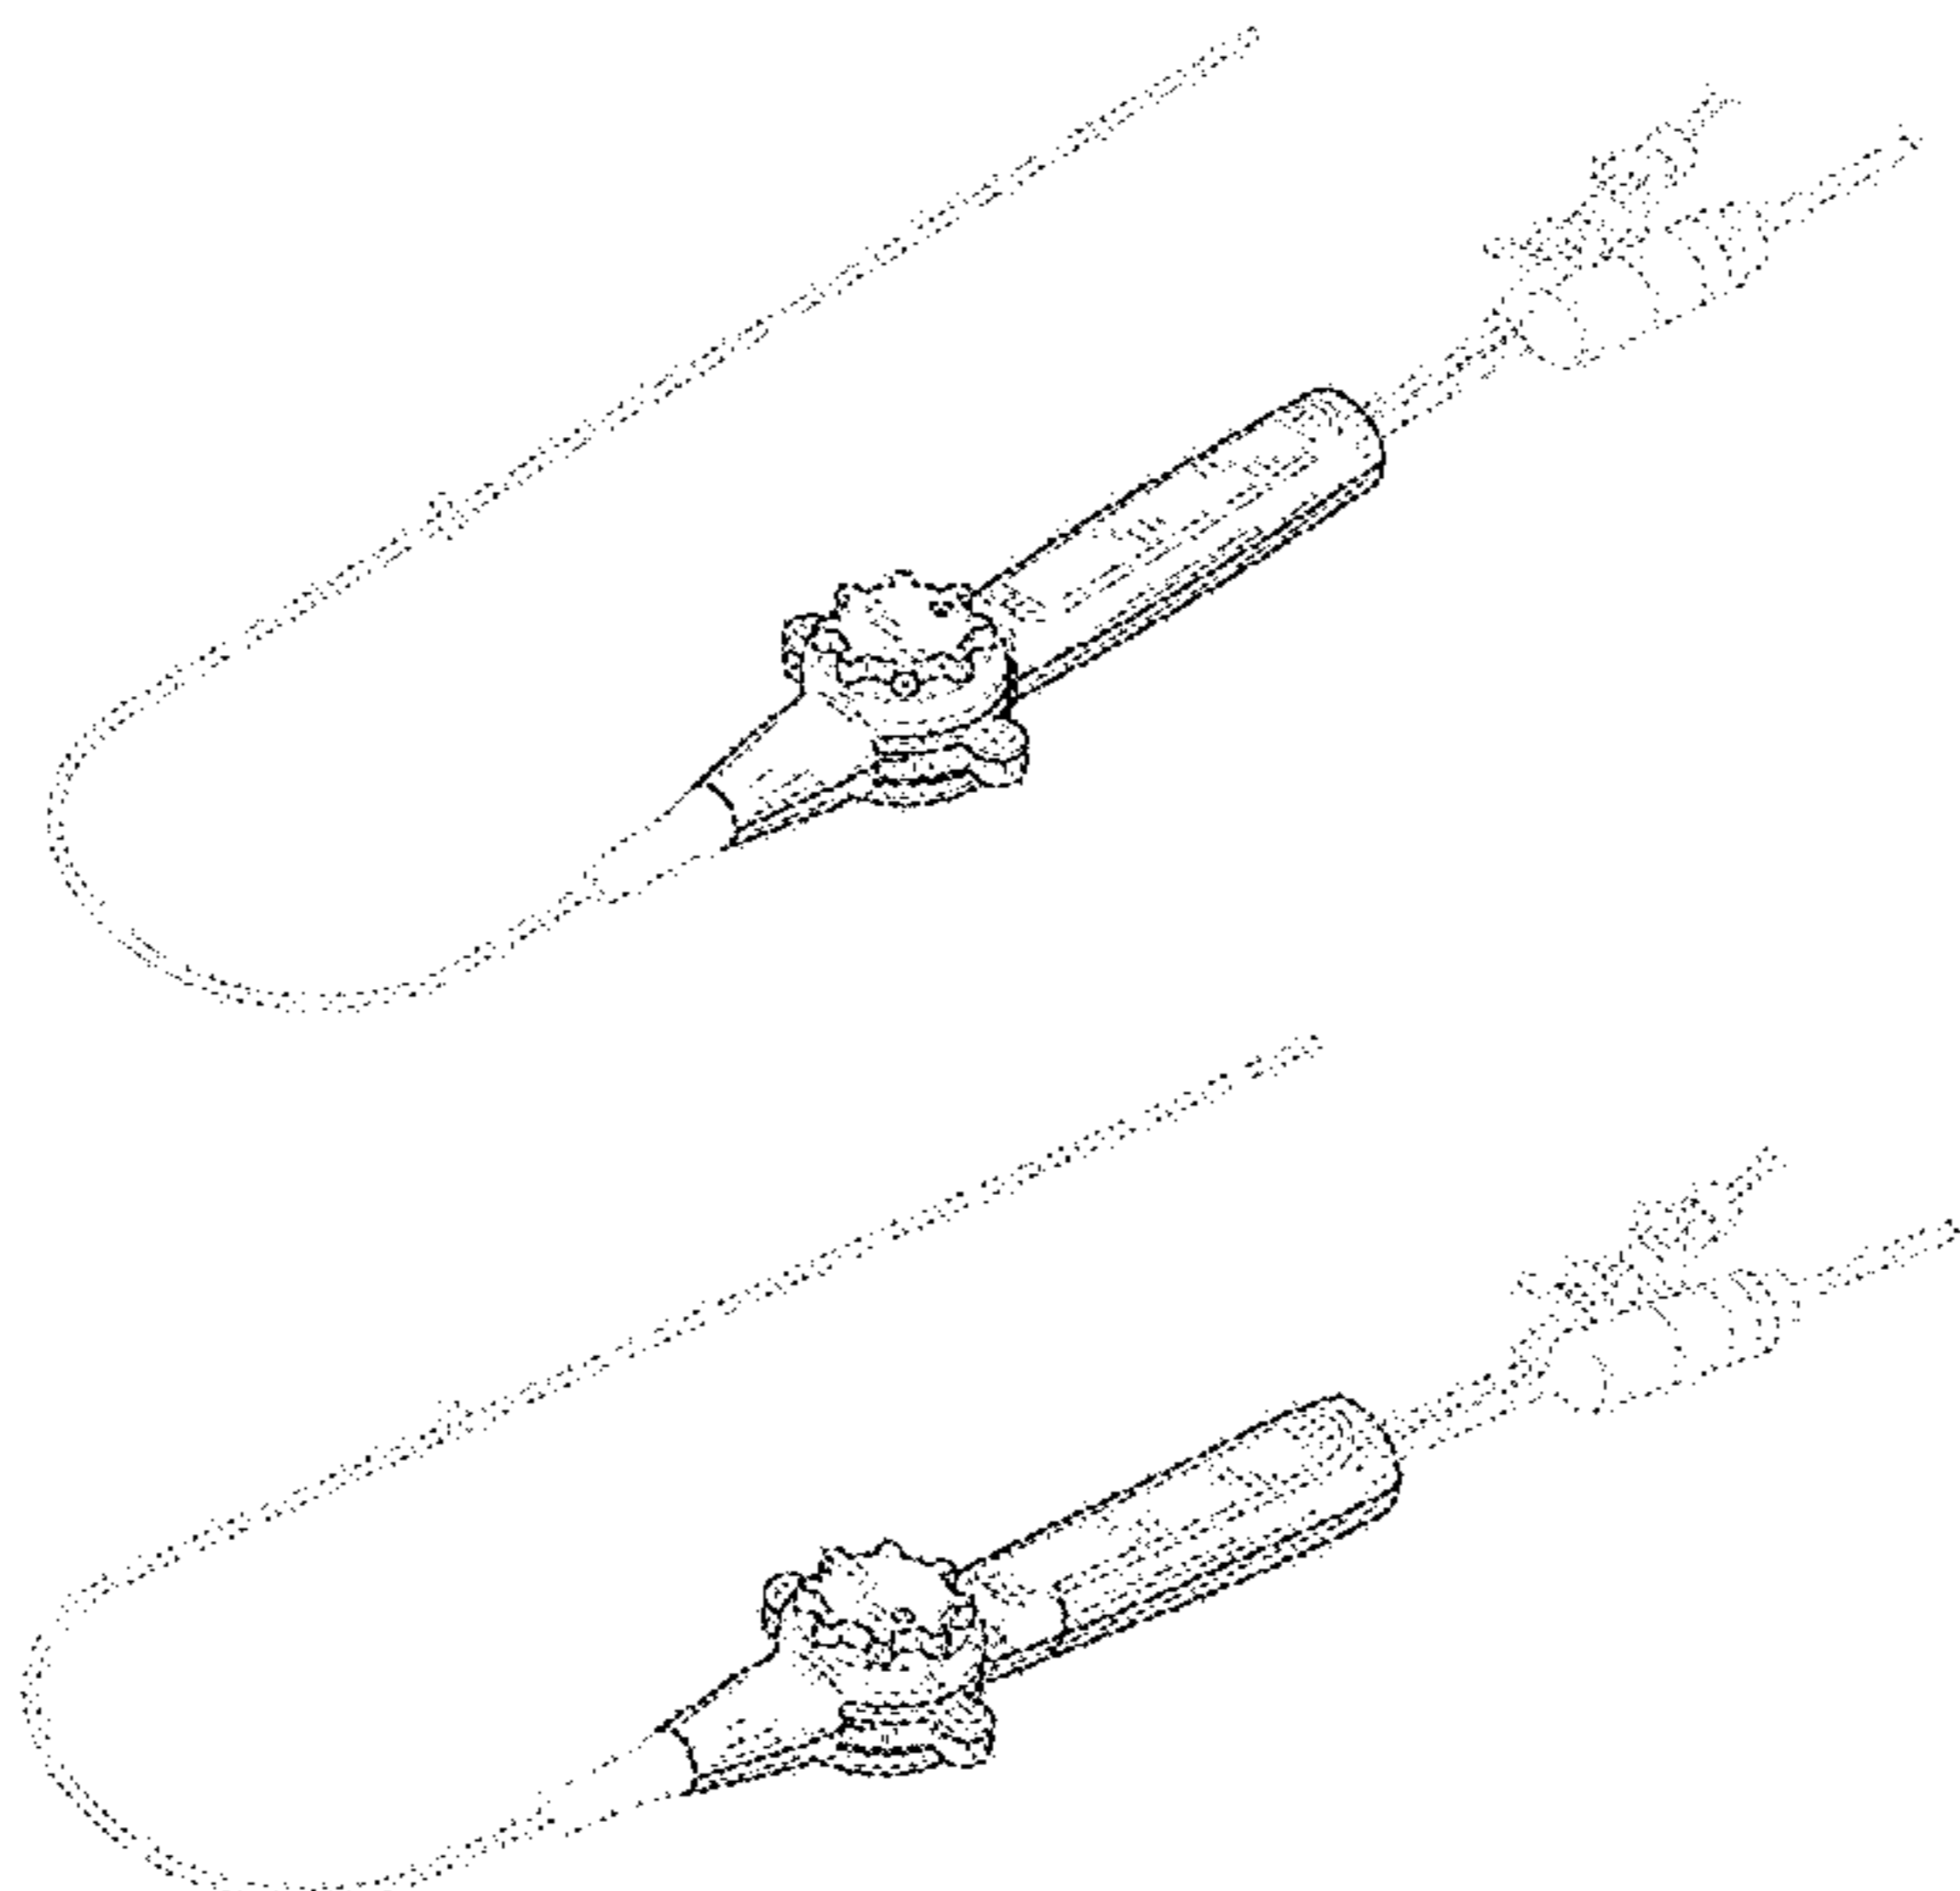

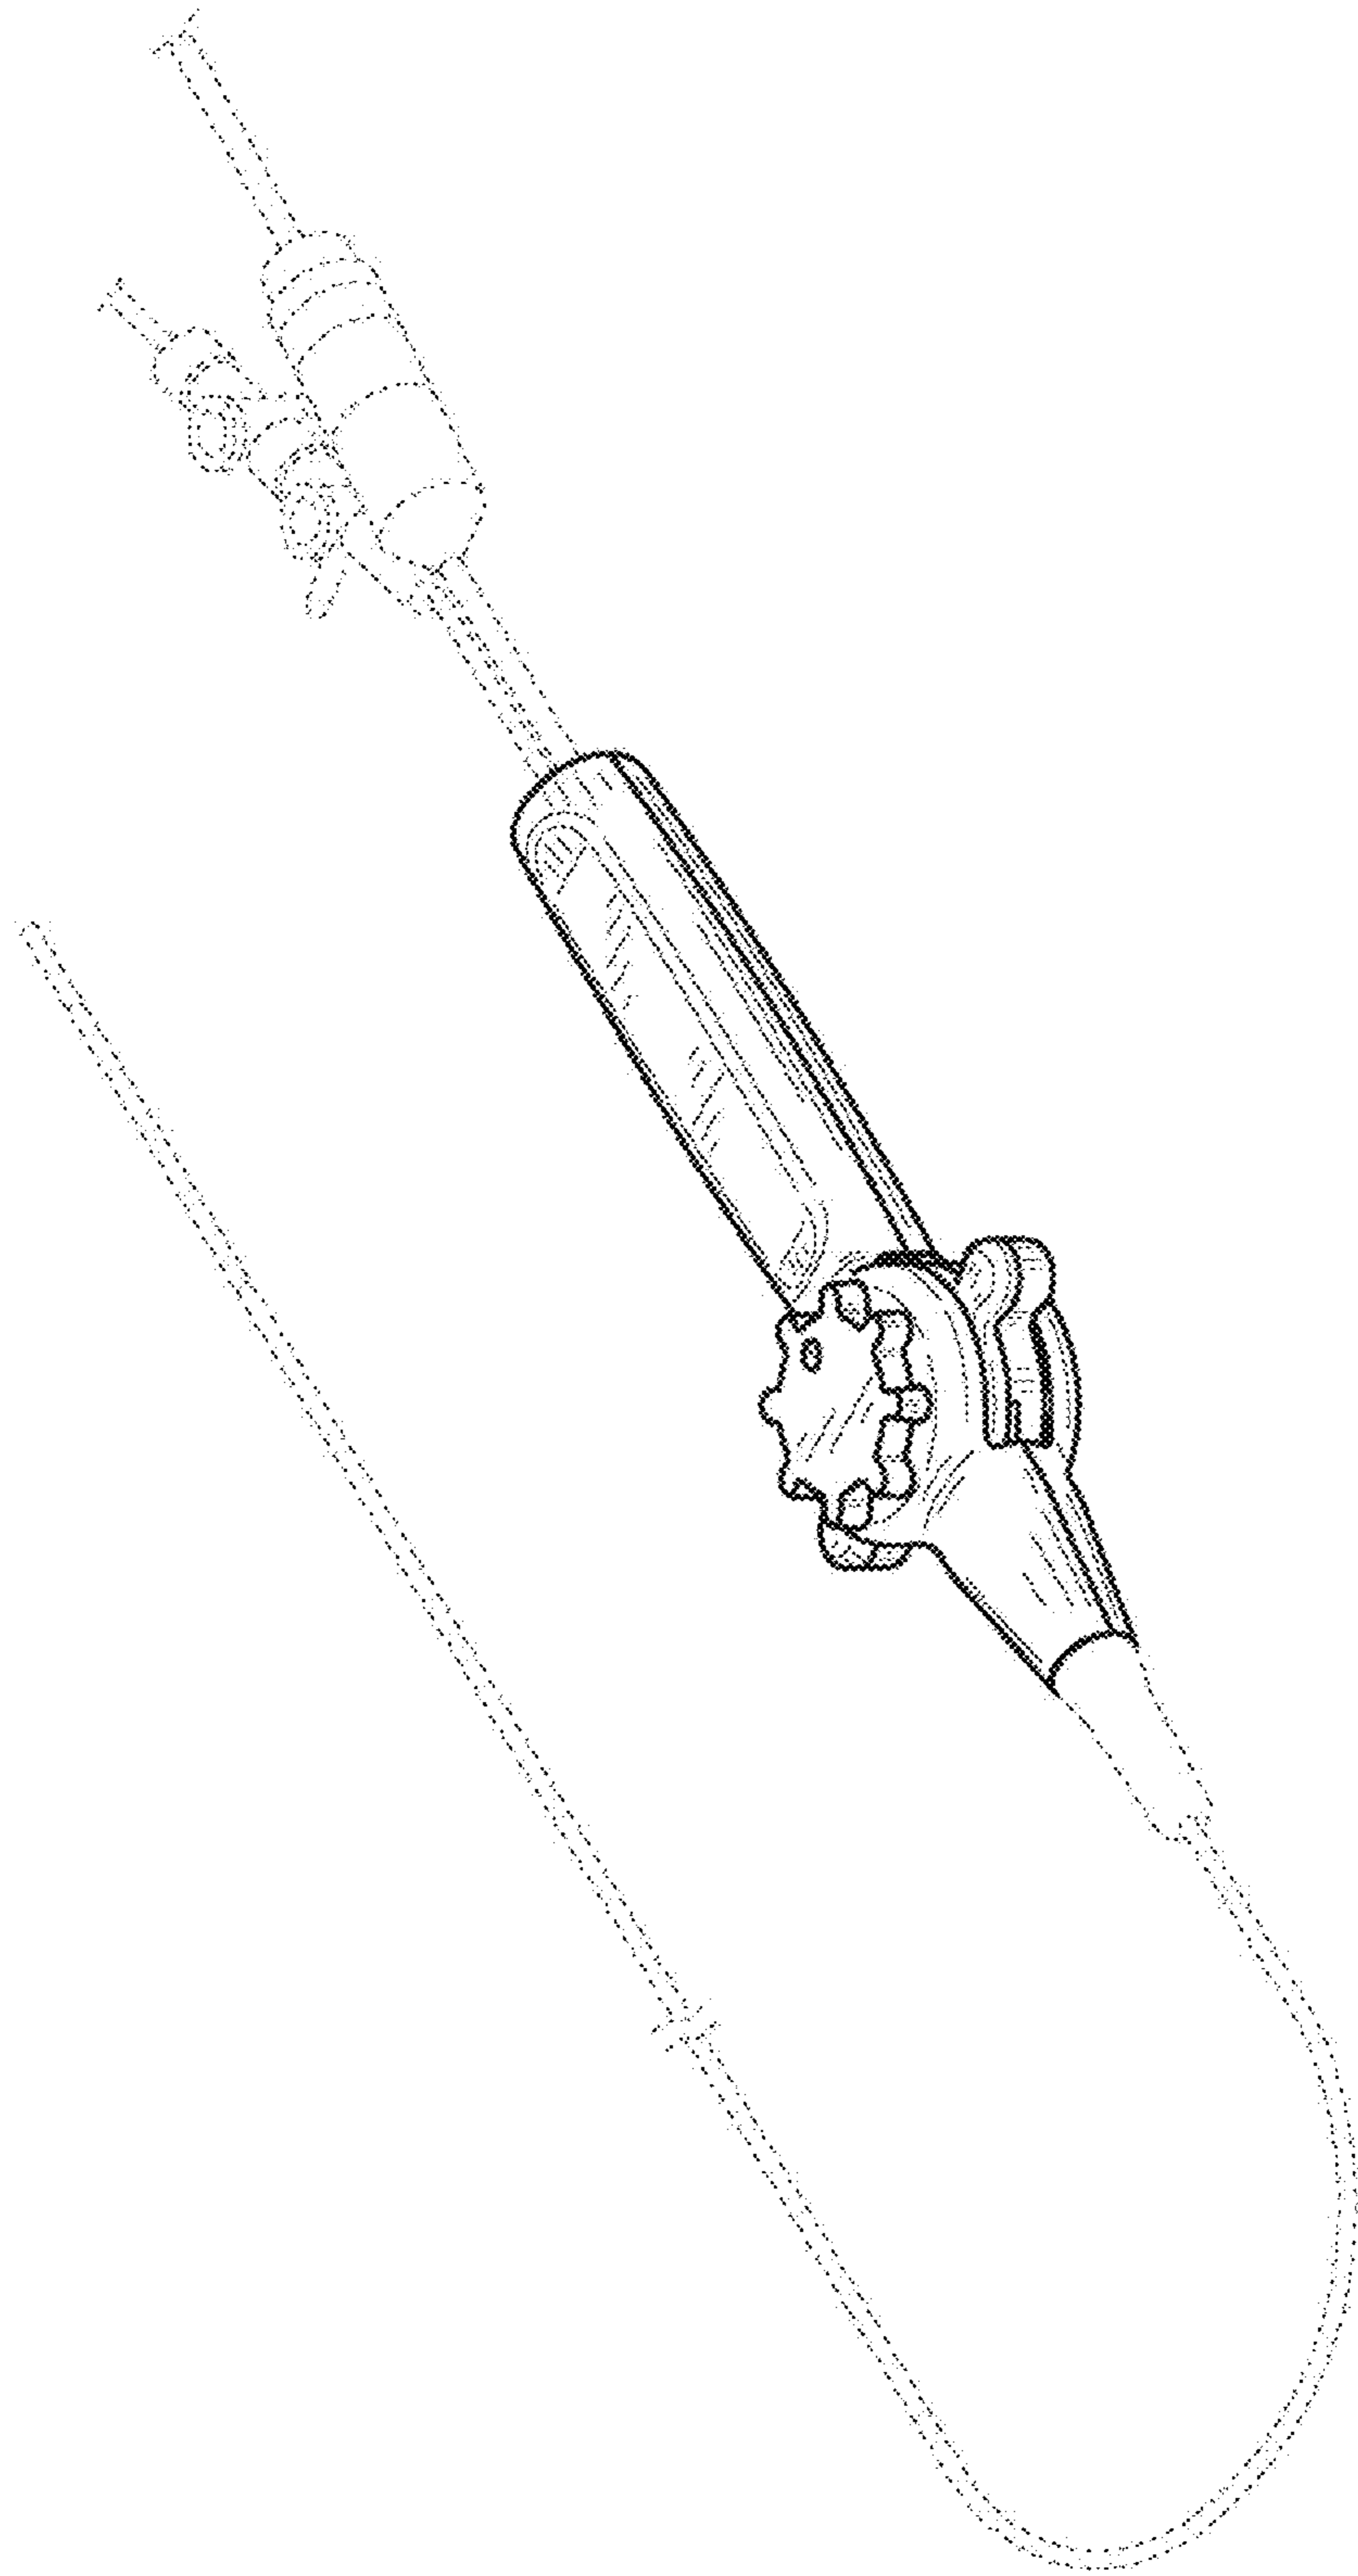


FIG. 1

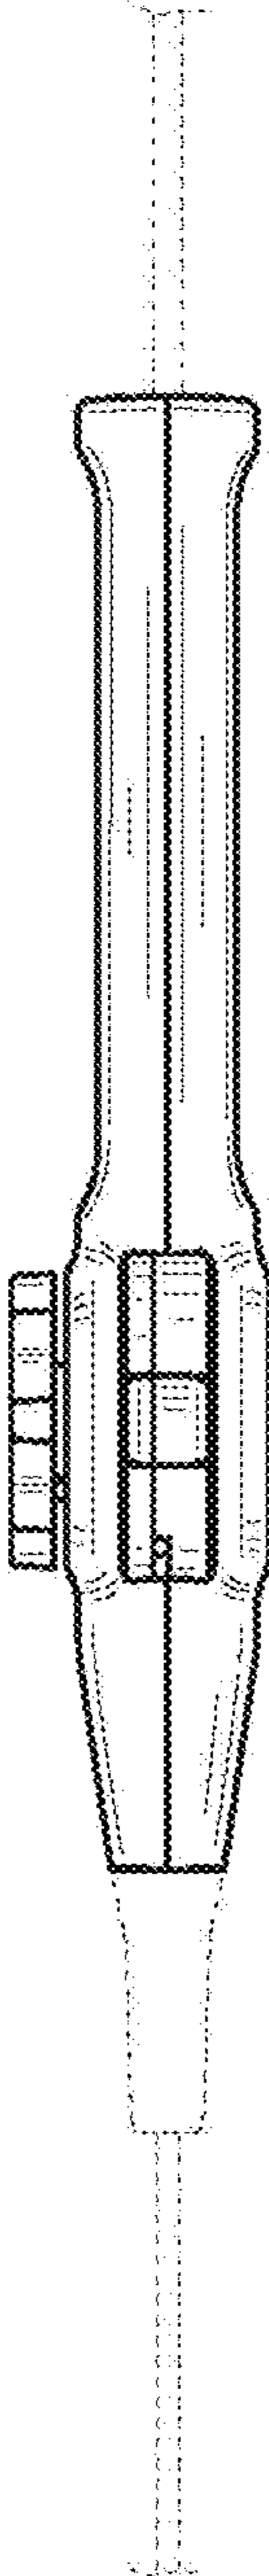


FIG. 2

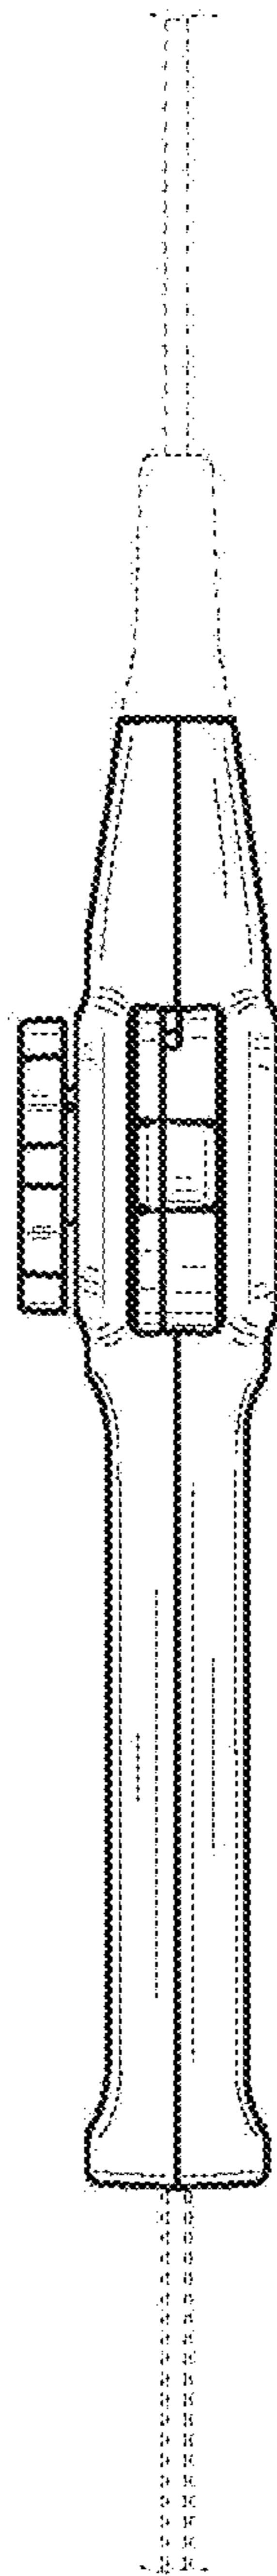


FIG. 3

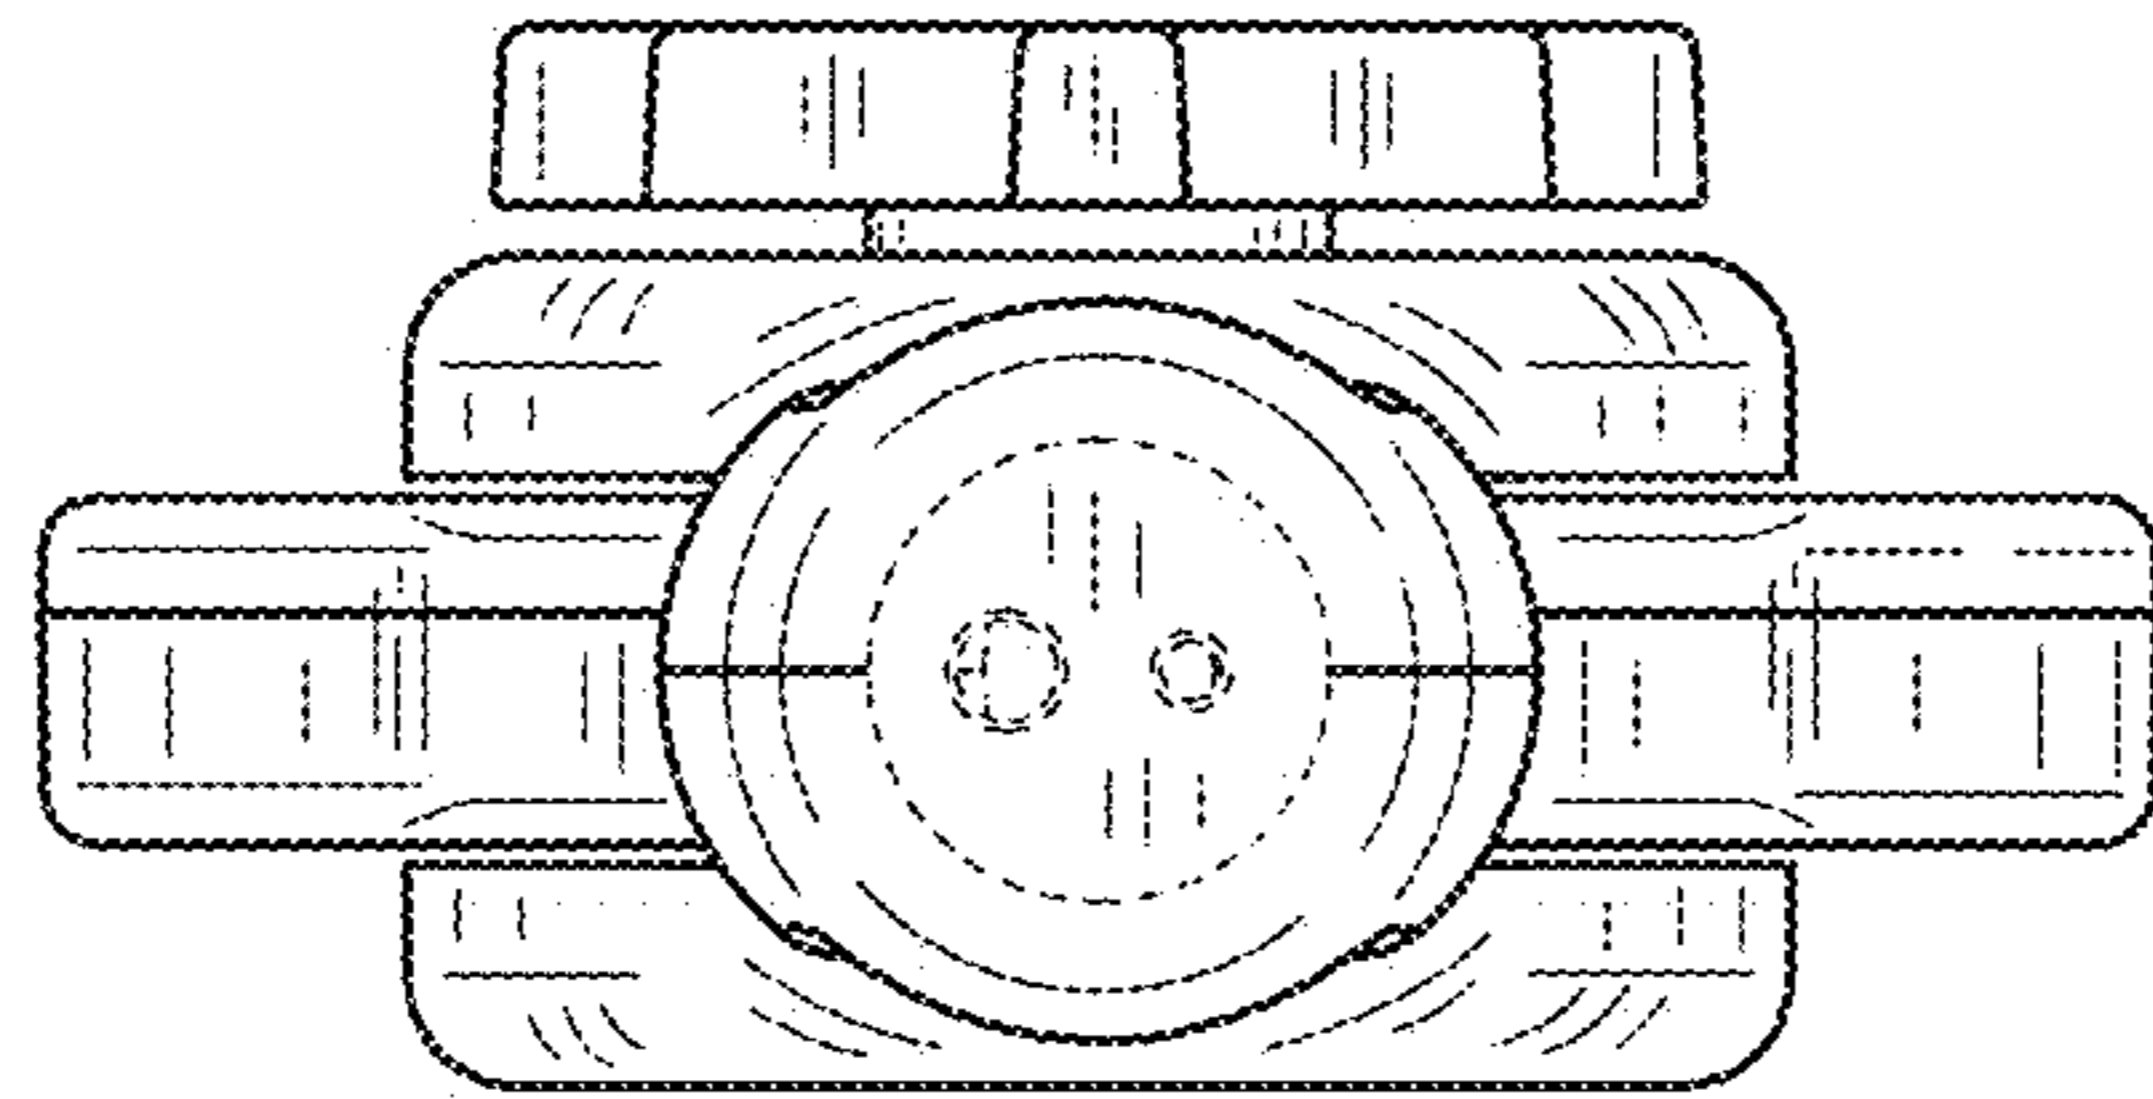


FIG. 4

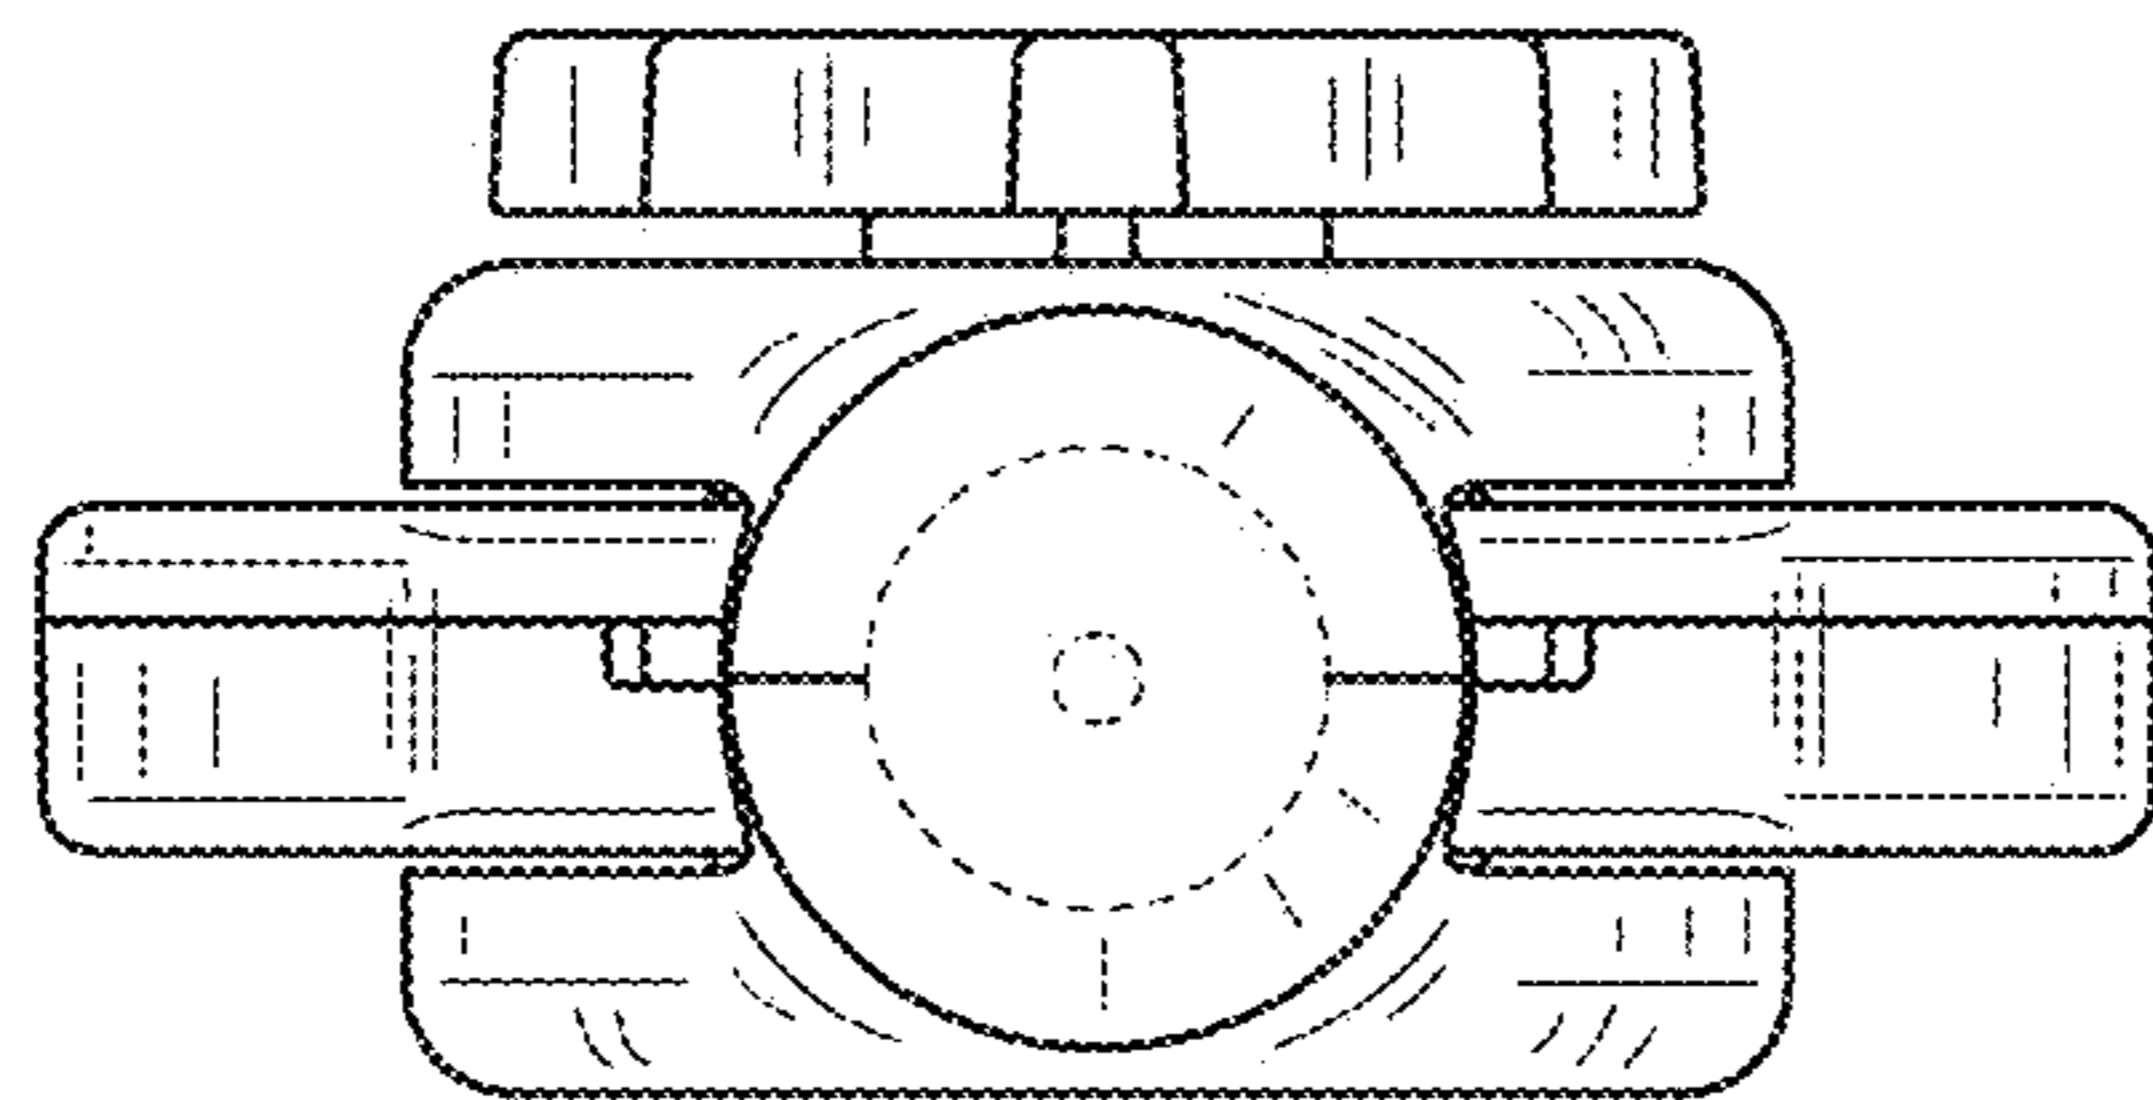


FIG. 5

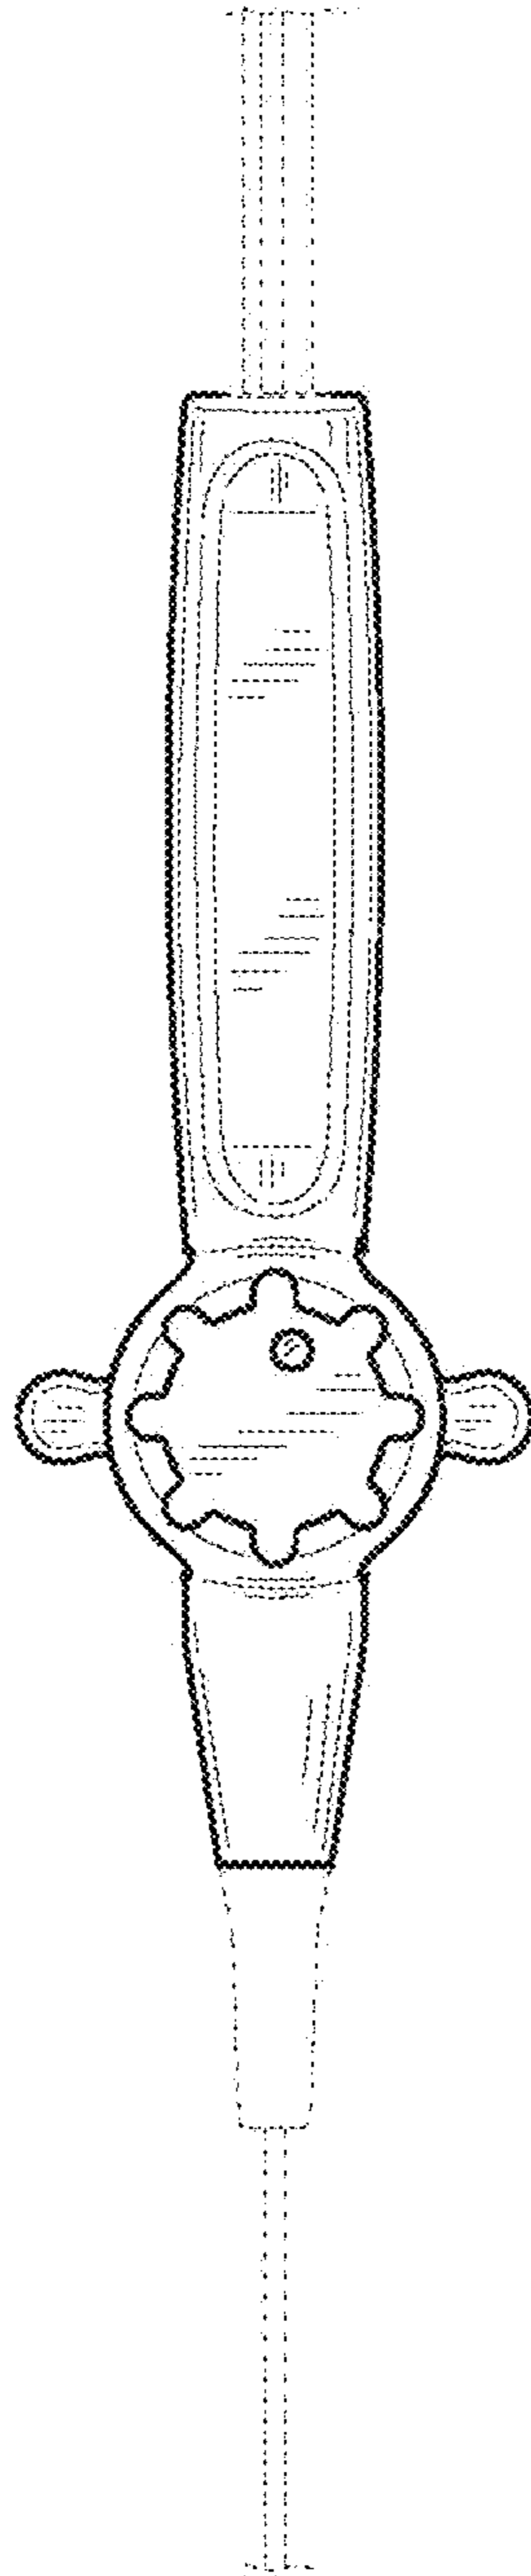


FIG. 6

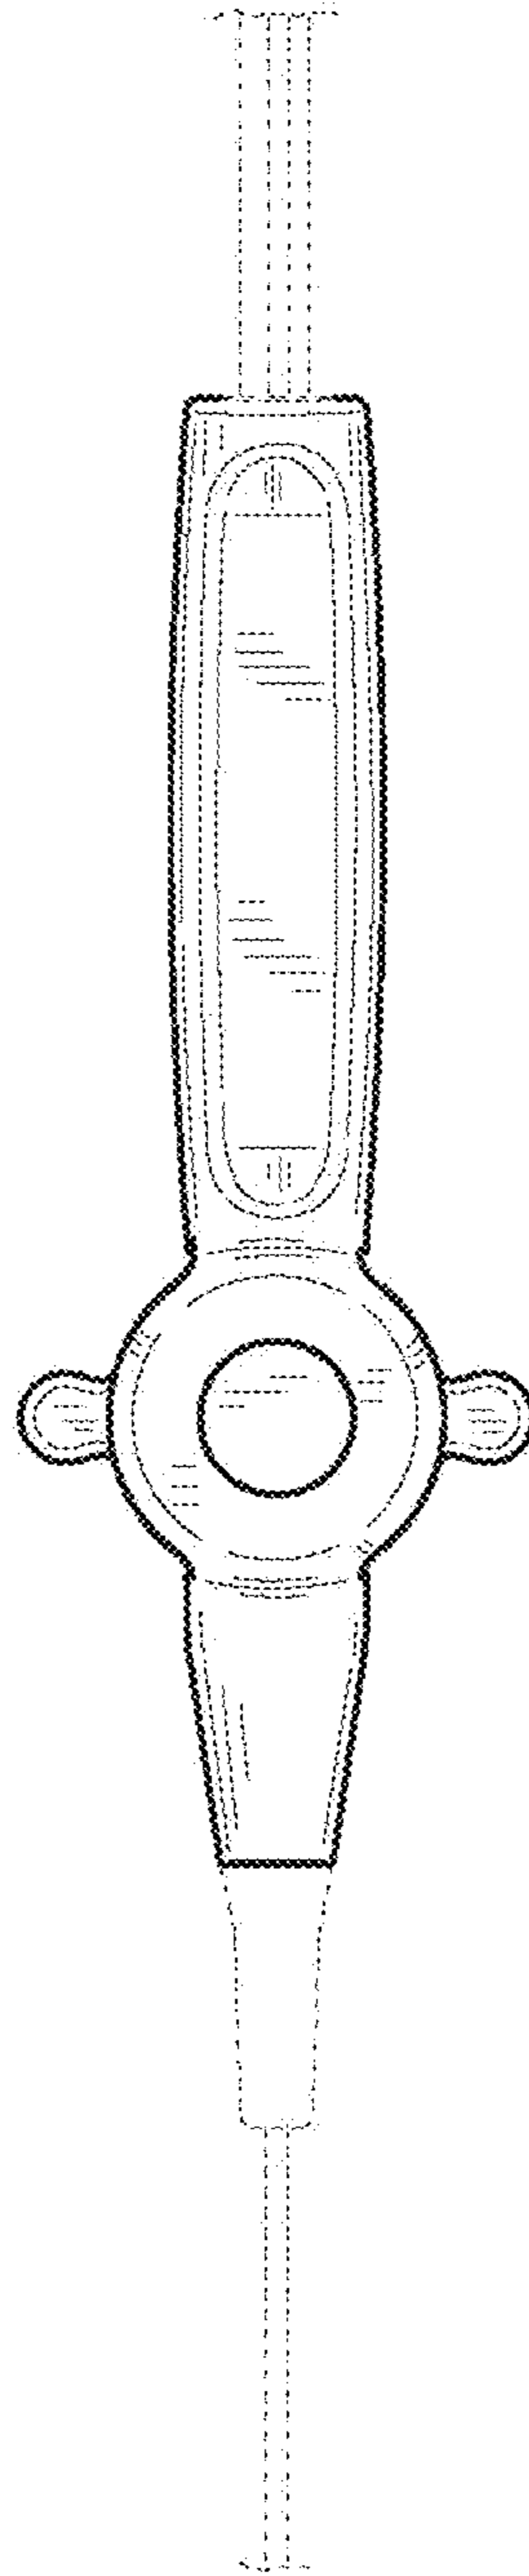


FIG. 7

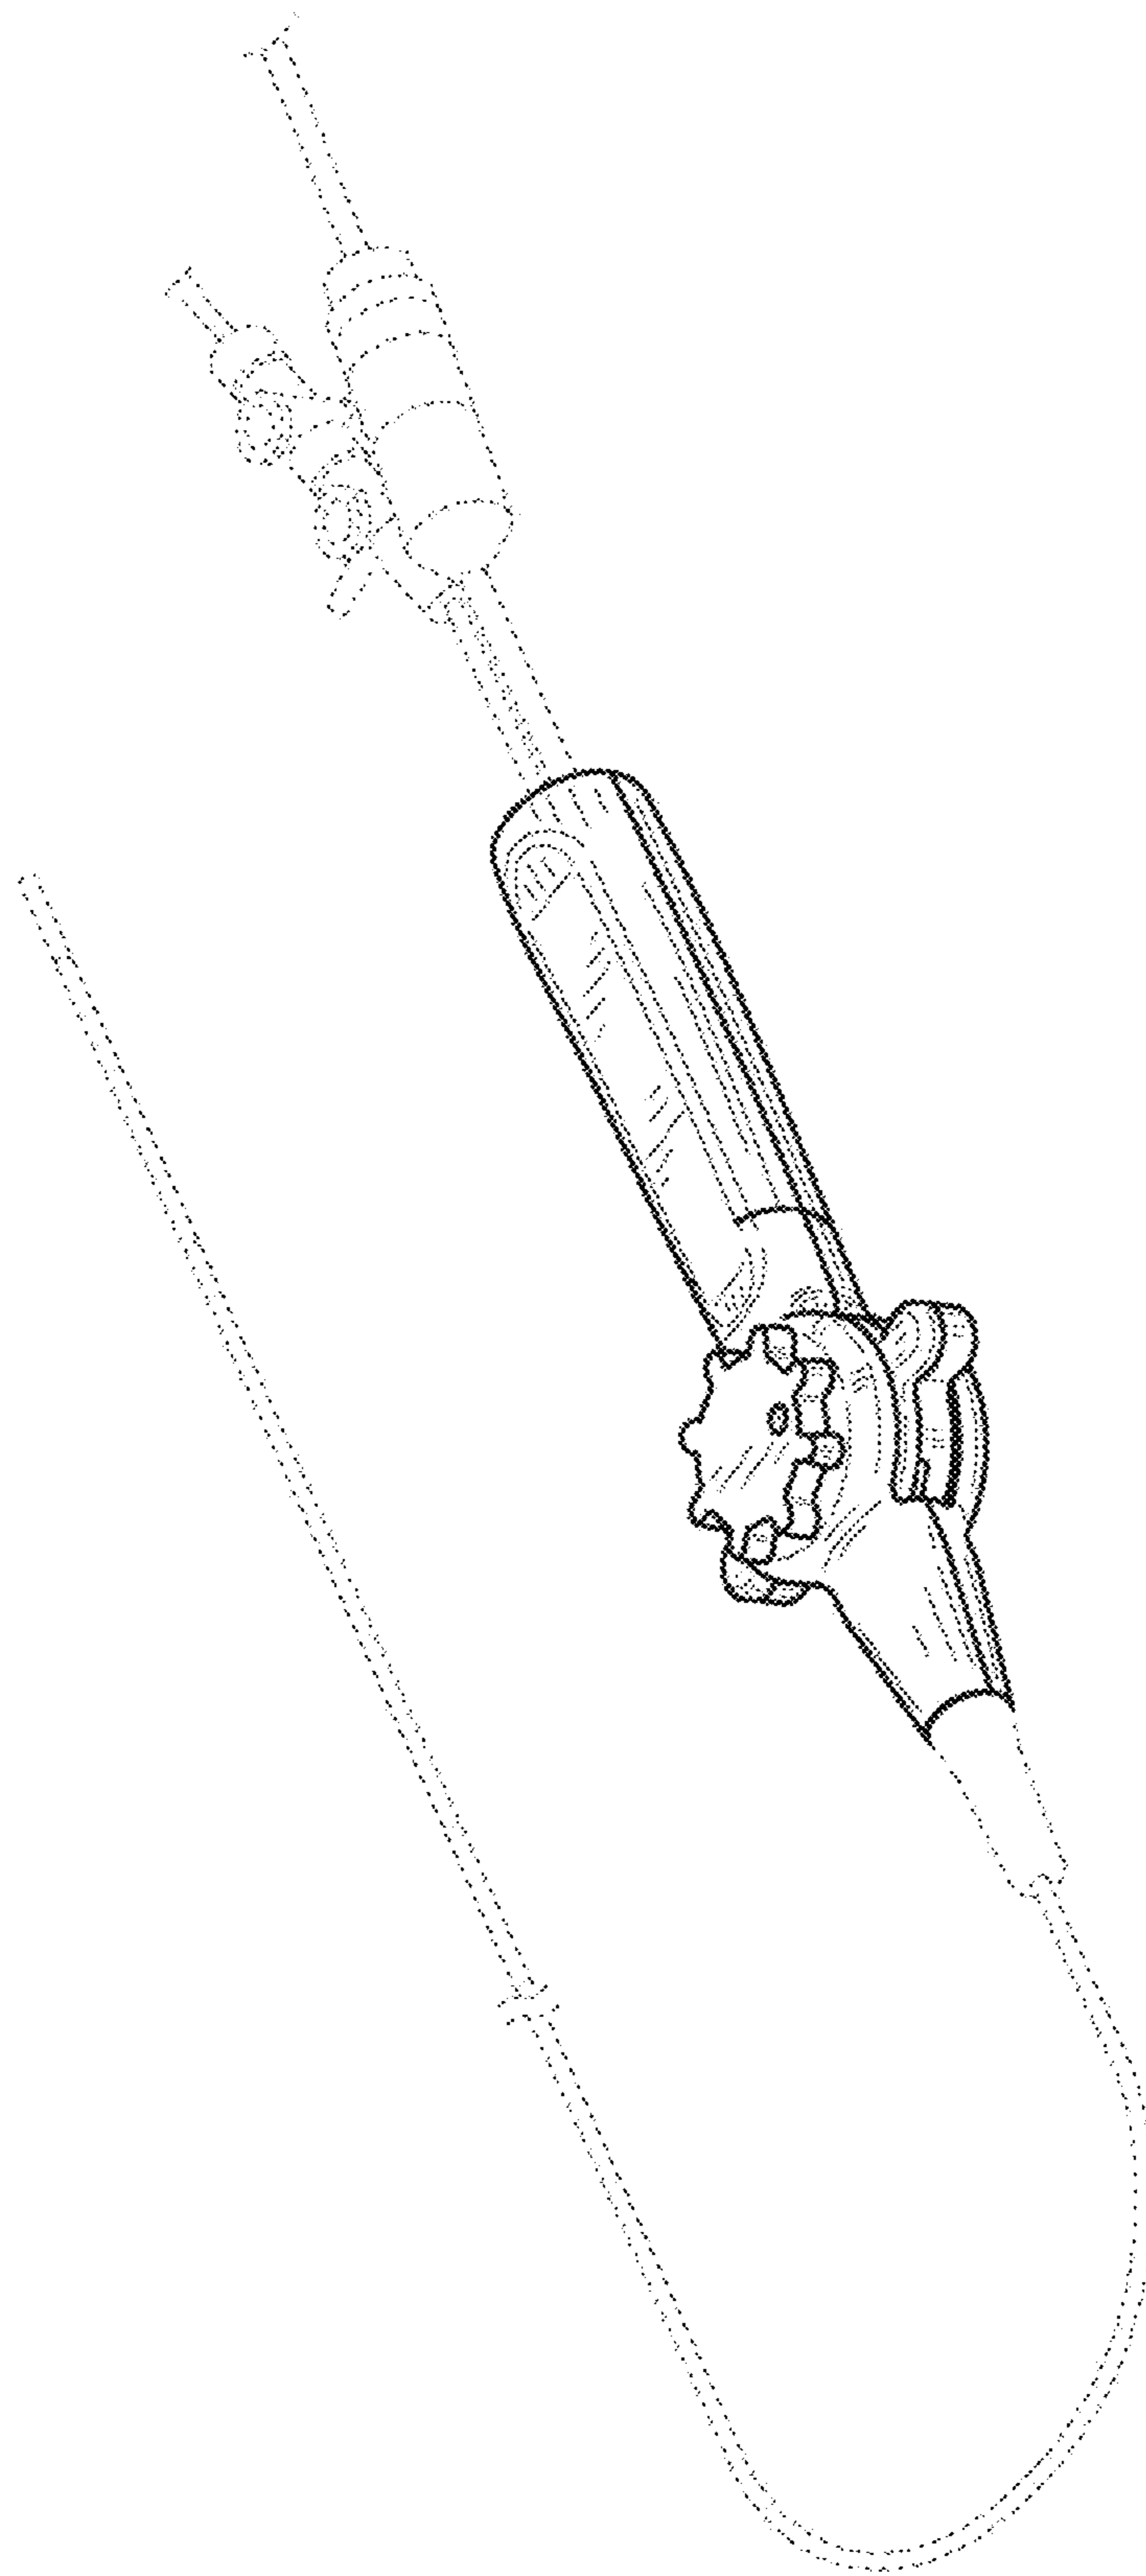


FIG. 8

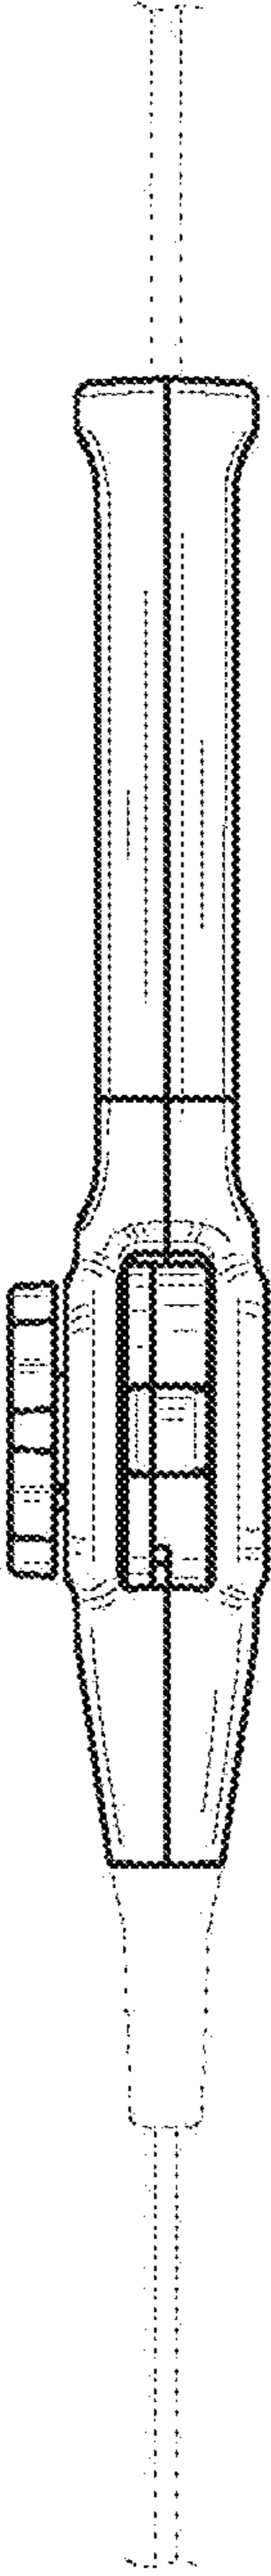


FIG. 9

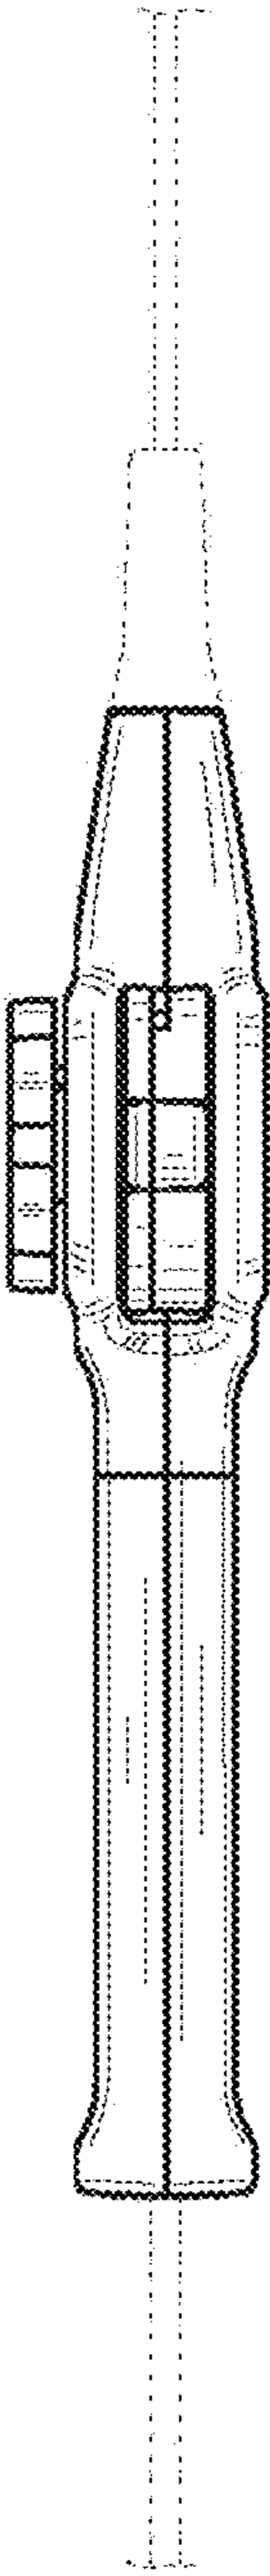


FIG. 10

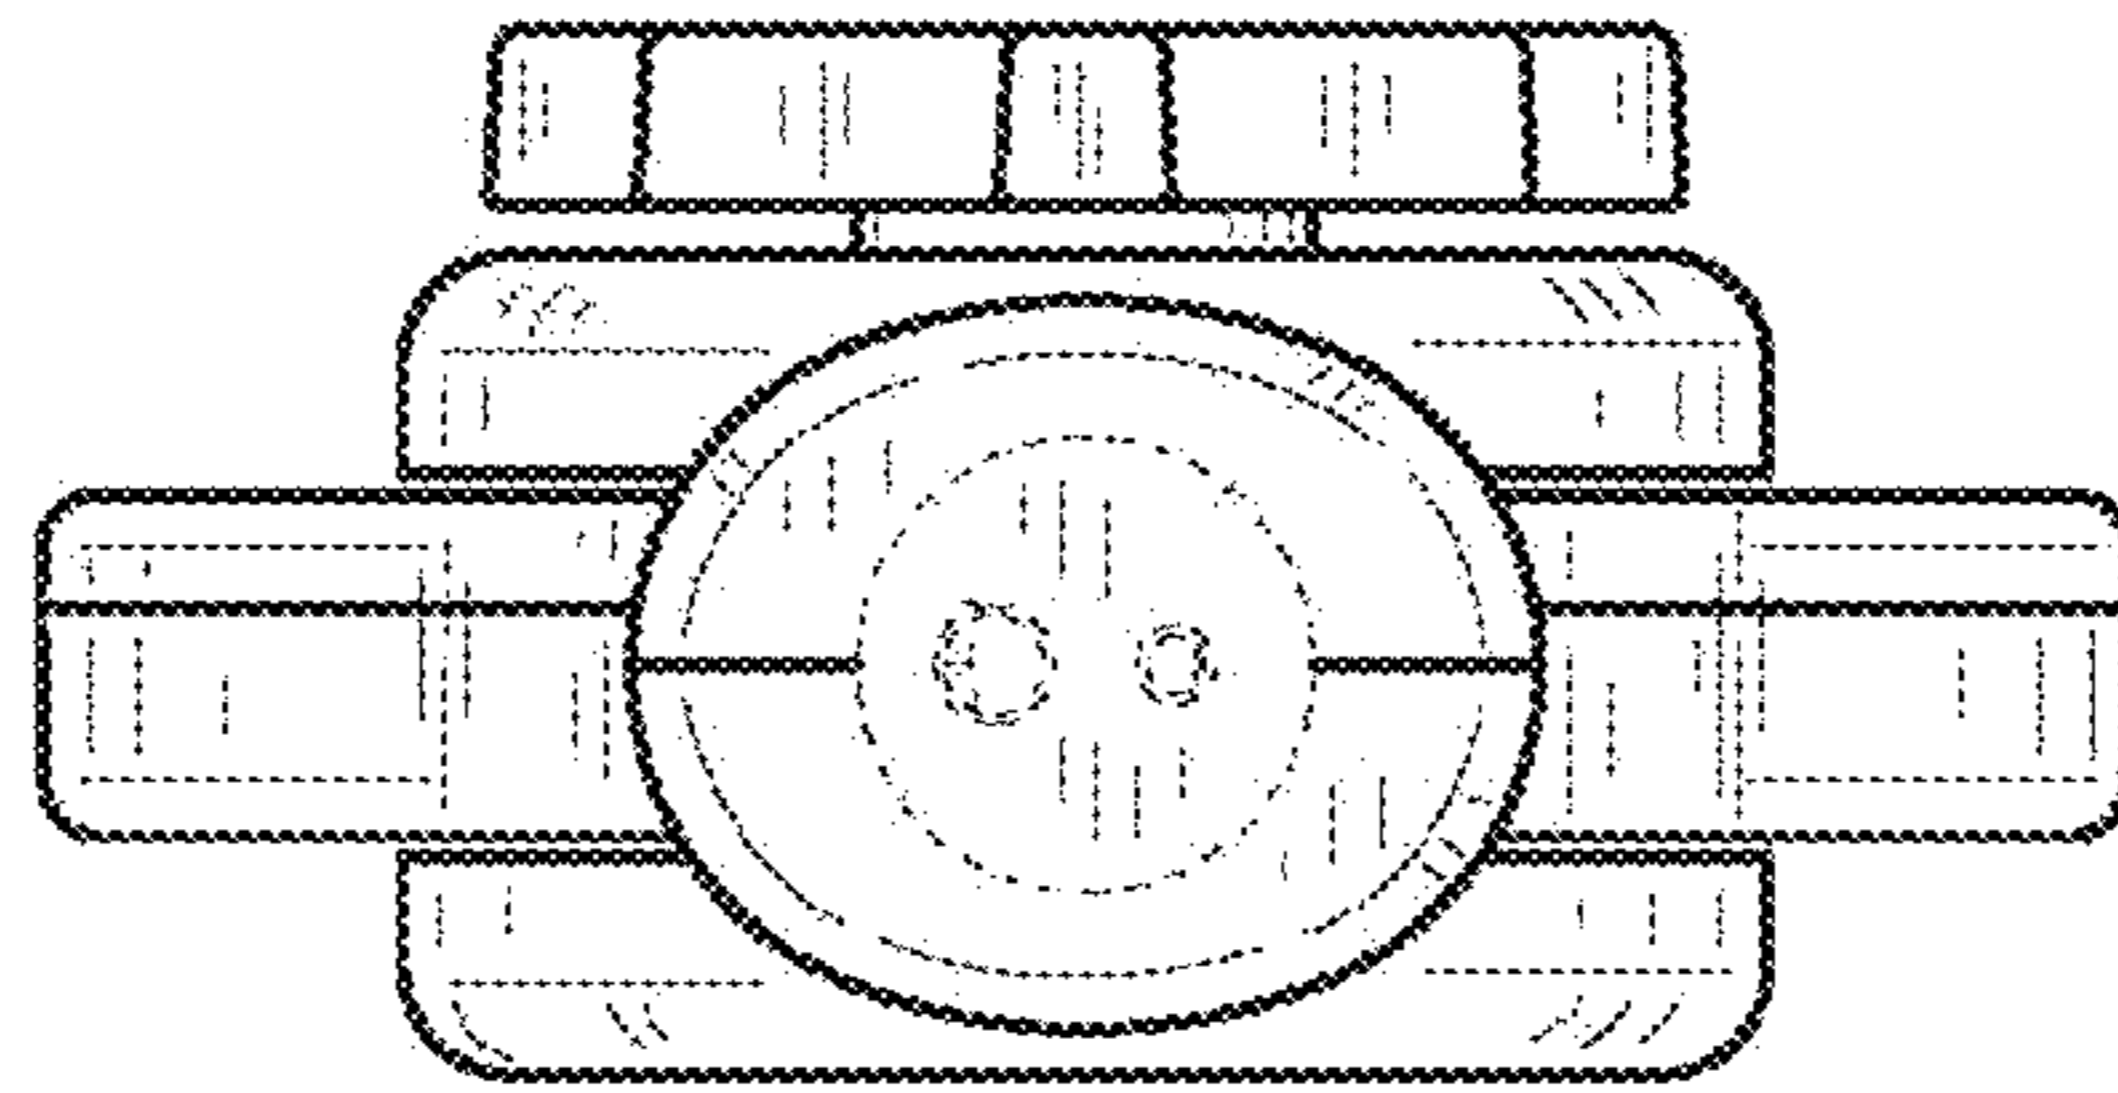


FIG. 11

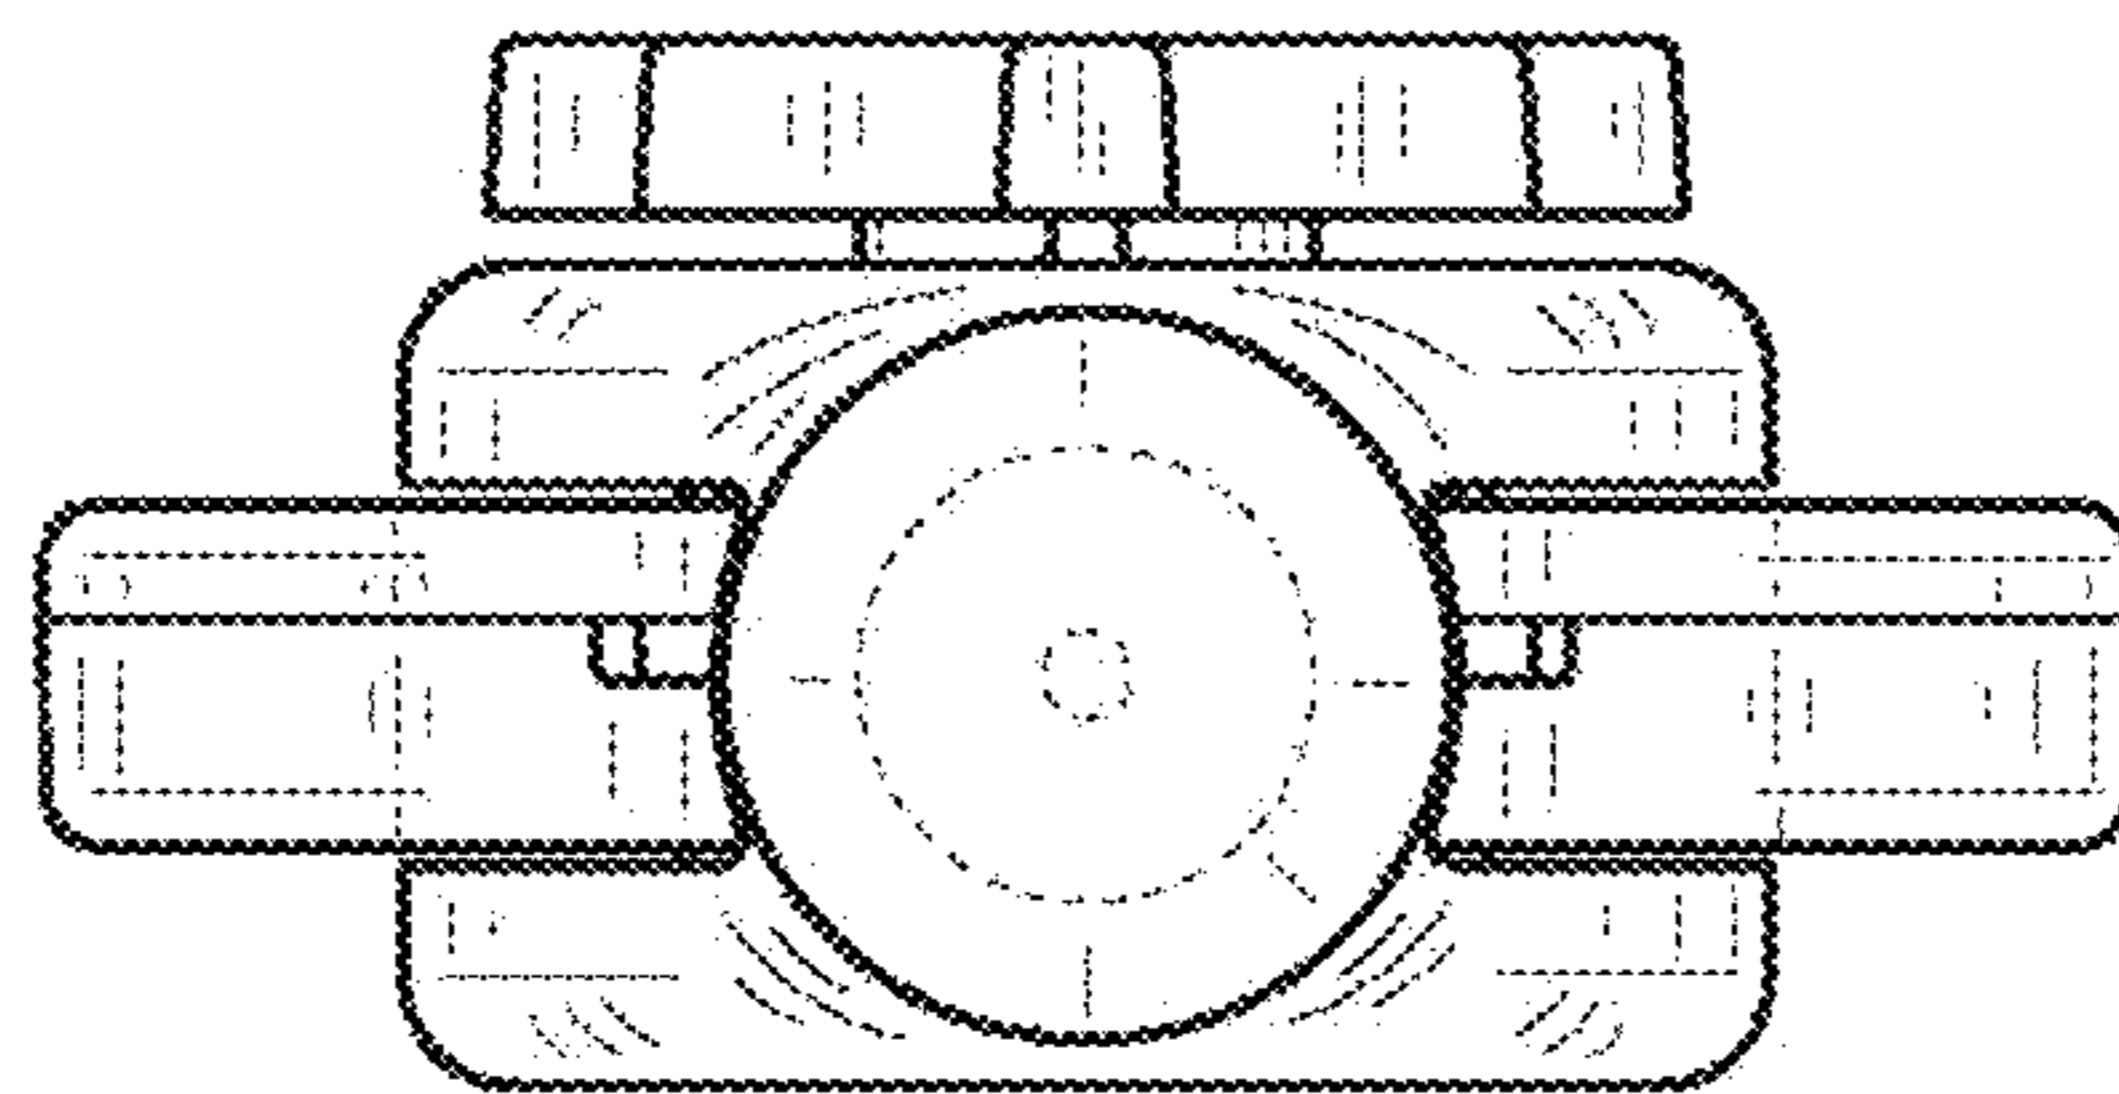


FIG. 12

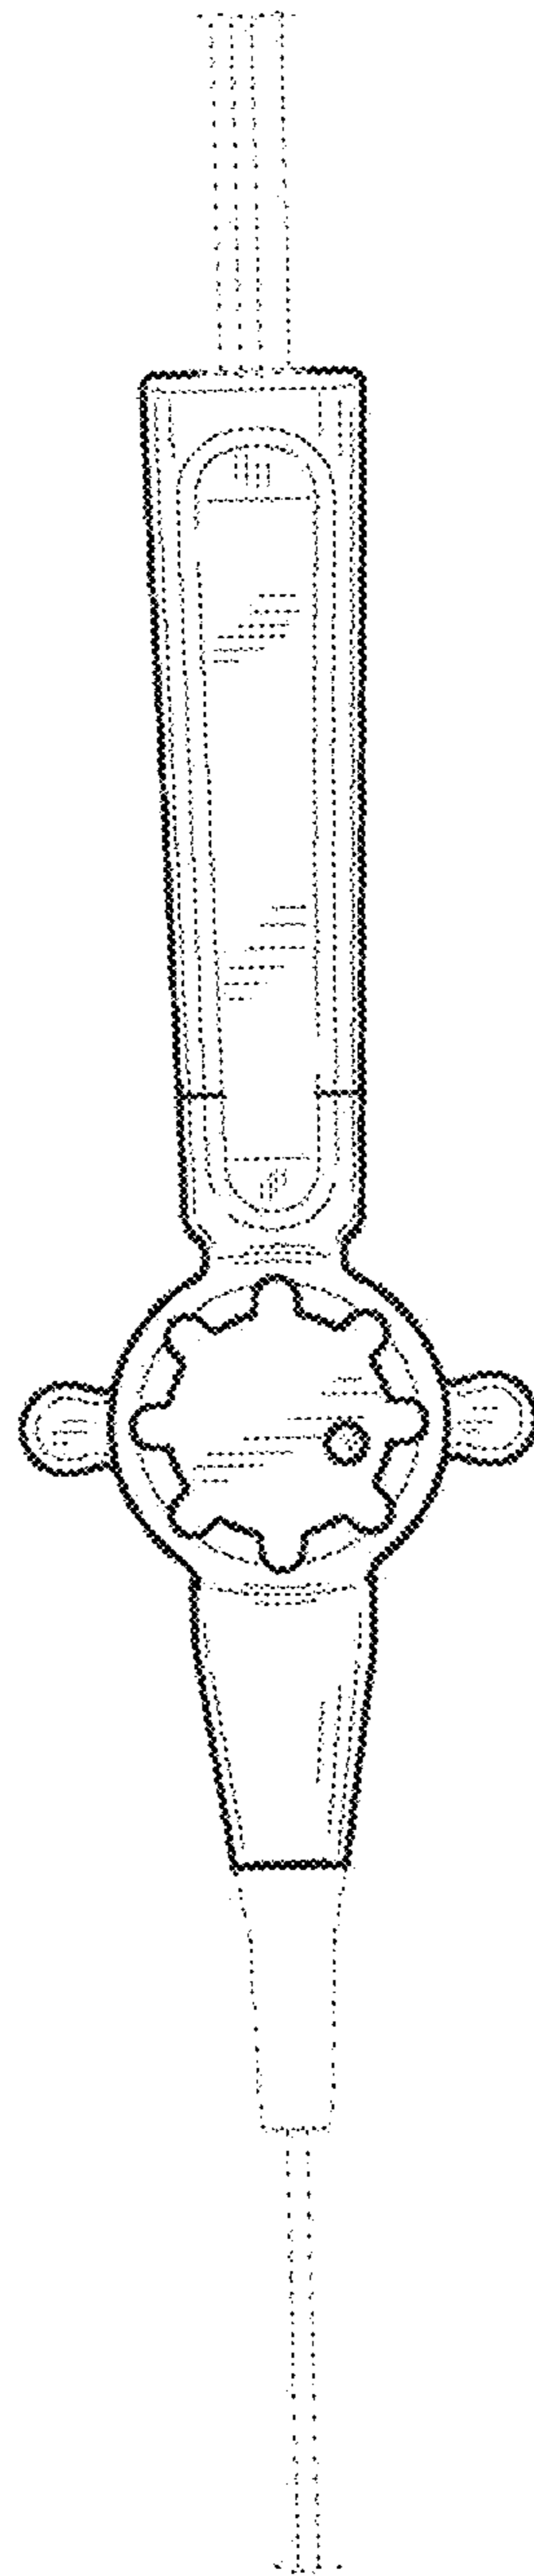


FIG. 13

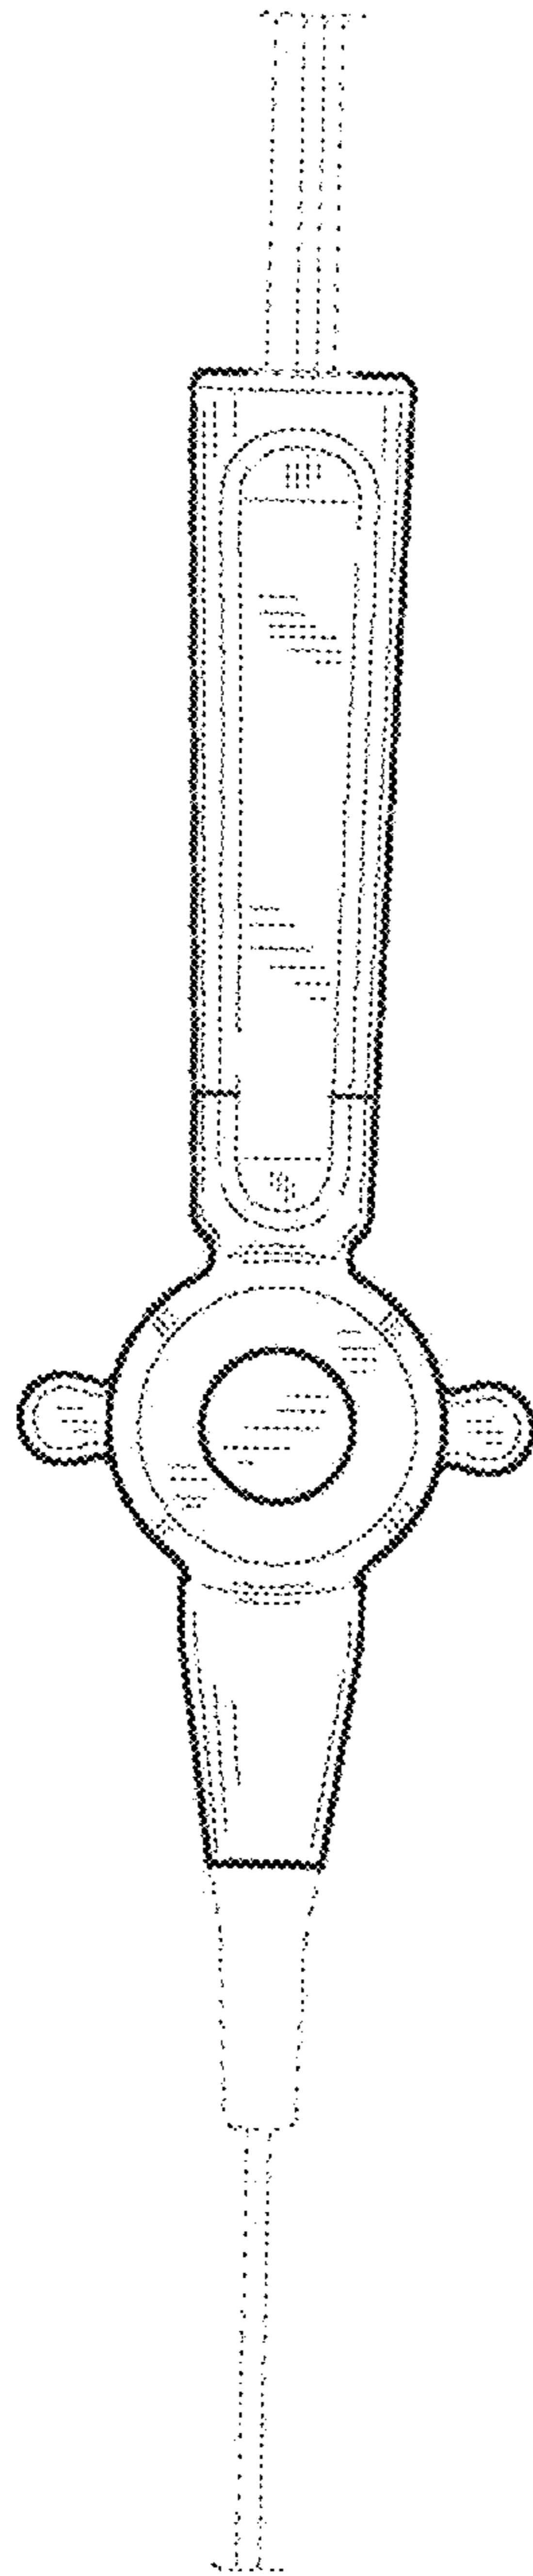


FIG. 14