

US00D734858S

(12) **United States Design Patent**
Weichert et al.

(10) **Patent No.:** **US D734,858 S**
(45) **Date of Patent:** **** Jul. 21, 2015**

(54) **MEDICAL MONITOR**
(71) Applicant: **KONINKLIJKE PHILIPS N.V.**,
Eindhoven (NL)
(72) Inventors: **Sven Weichert**, Eindhoven (NL); **Stefan**
Melles, Stuttgart (DE)
(73) Assignee: **KONINKLIJKE PHILIPS N.V.**,
Eindhoven (NL)
(**) Term: **14 Years**
(21) Appl. No.: **29/483,502**
(22) Filed: **Feb. 28, 2014**

D475,137	S	*	5/2003	Manke et al.	D24/165
D491,270	S	*	6/2004	Barker	D24/186
D512,151	S	*	11/2005	Ward et al.	D24/186
D536,794	S	*	2/2007	Knieriem et al.	D24/186
D536,795	S	*	2/2007	Knieriem et al.	D24/186
D549,831	S	*	8/2007	Ward et al.	D24/186
D552,741	S	*	10/2007	Zhou et al.	D24/186
D562,456	S	*	2/2008	Scruggs et al.	D24/160
D592,754	S	*	5/2009	Koike et al.	D24/186
D600,814	S	*	9/2009	Lathrop et al.	D24/186
D621,511	S	*	8/2010	Lathrop et al.	D24/167
D624,654	S	*	9/2010	Shimizu	D24/186
D632,397	S	*	2/2011	Edwards et al.	D24/186
D635,681	S	*	4/2011	Edwards et al.	D24/186
D638,543	S	*	5/2011	Geisser et al.	D24/138
D693,006	S	*	11/2013	Arimitsu et al.	D24/167
D697,214	S	*	1/2014	Rosenfeldt et al.	D24/186

* cited by examiner

(30) **Foreign Application Priority Data**
Sep. 3, 2013 (EM) 002301796-0004
(51) **LOC (10) Cl.** **24-01**
(52) **U.S. Cl.**
USPC **D24/186**
(58) **Field of Classification Search**
USPC D24/138, 160, 164-165, 167-169,
D24/185-186; 600/301, 481, 483-485, 509,
600/513, 519, 544; 128/900; D10/81, 104;
D14/381, 126, 371
See application file for complete search history.

Primary Examiner — T. Chase Nelson
Assistant Examiner — Mark Cavanna


(57) **CLAIM**
The ornamental design for a medical monitor, as shown and described.

(56) **References Cited**
U.S. PATENT DOCUMENTS
D303,255 S * 9/1989 Bratasevec D14/371
D328,645 S * 8/1992 Rogler et al. D24/186
D393,072 S * 3/1998 Rogler D24/186
D395,513 S * 6/1998 Rogler D24/186

DESCRIPTION

FIG. 1 is a perspective view showing my design;
FIG. 2 is a front elevational view thereof;
FIG. 3 is a rear elevational view thereof;
FIG. 4 is a right side elevational view thereof;
FIG. 5 is a left side elevational view thereof;
FIG. 6 is a top plan view thereof; and,
FIG. 7 is a bottom plan view thereof.
The broken lines are included for the purpose of illustrating unclaimed portions of the medical monitor and forms no part of the claimed design.

1 Claim, 6 Drawing Sheets

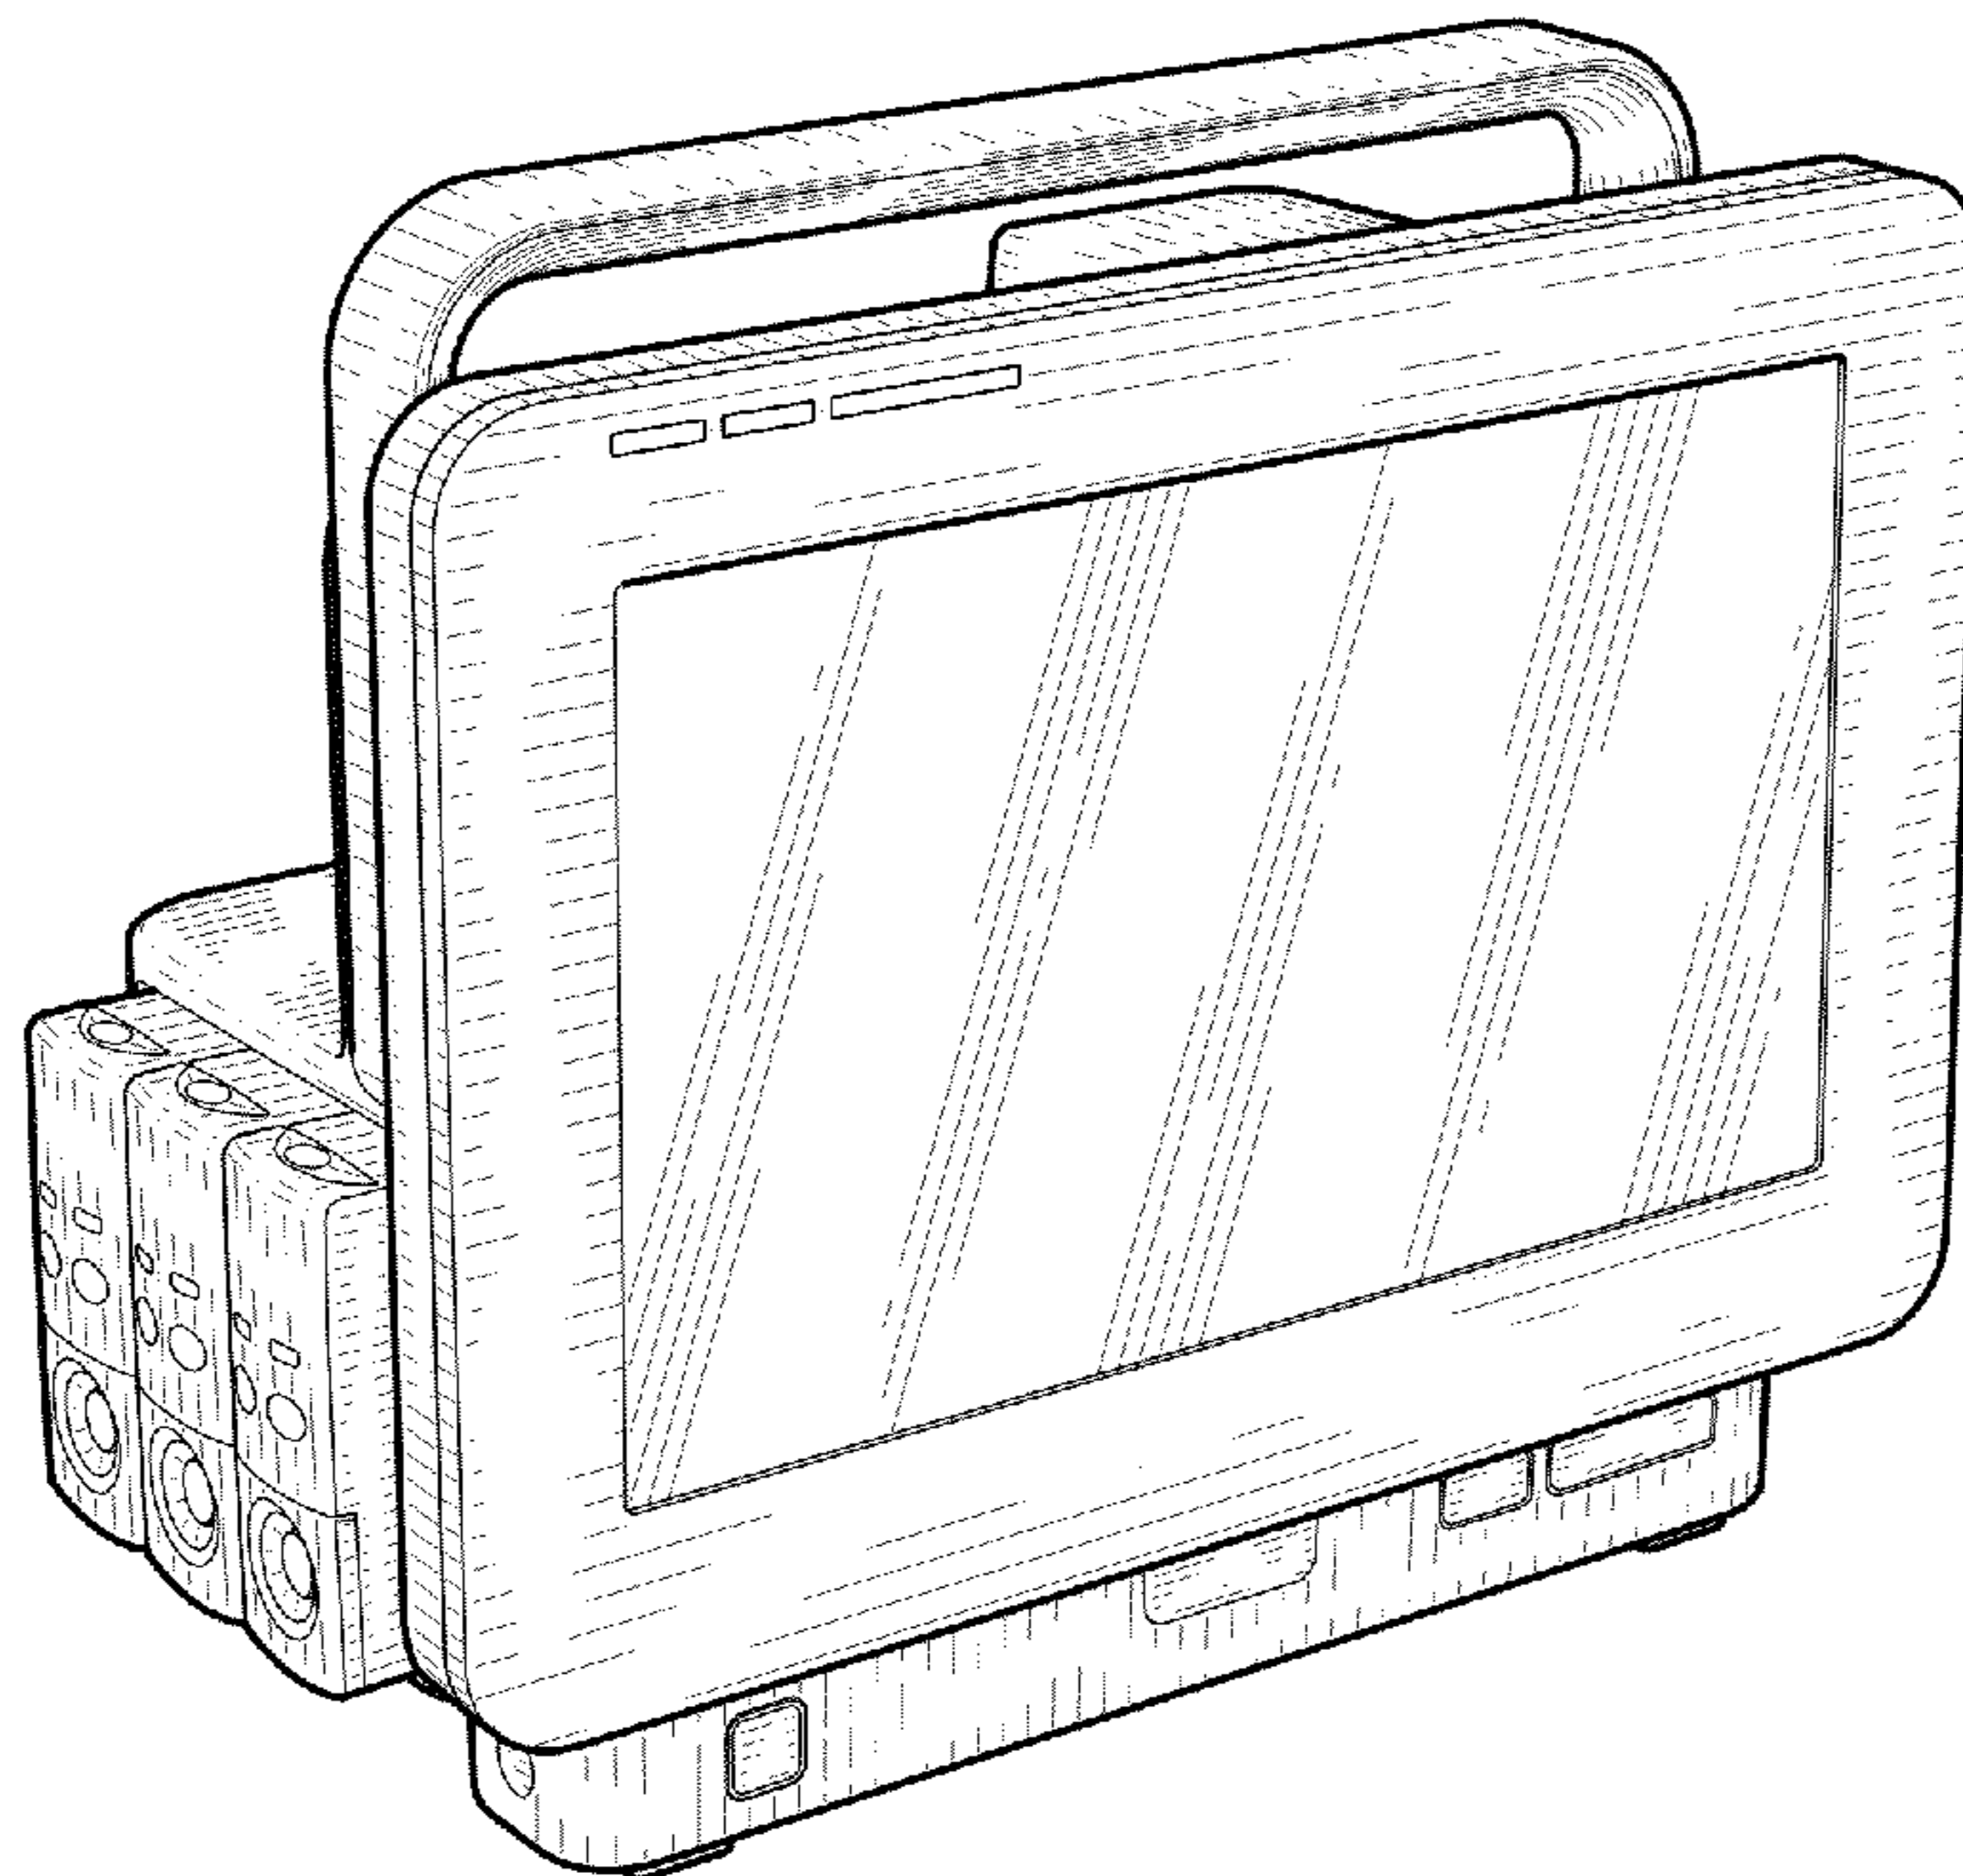

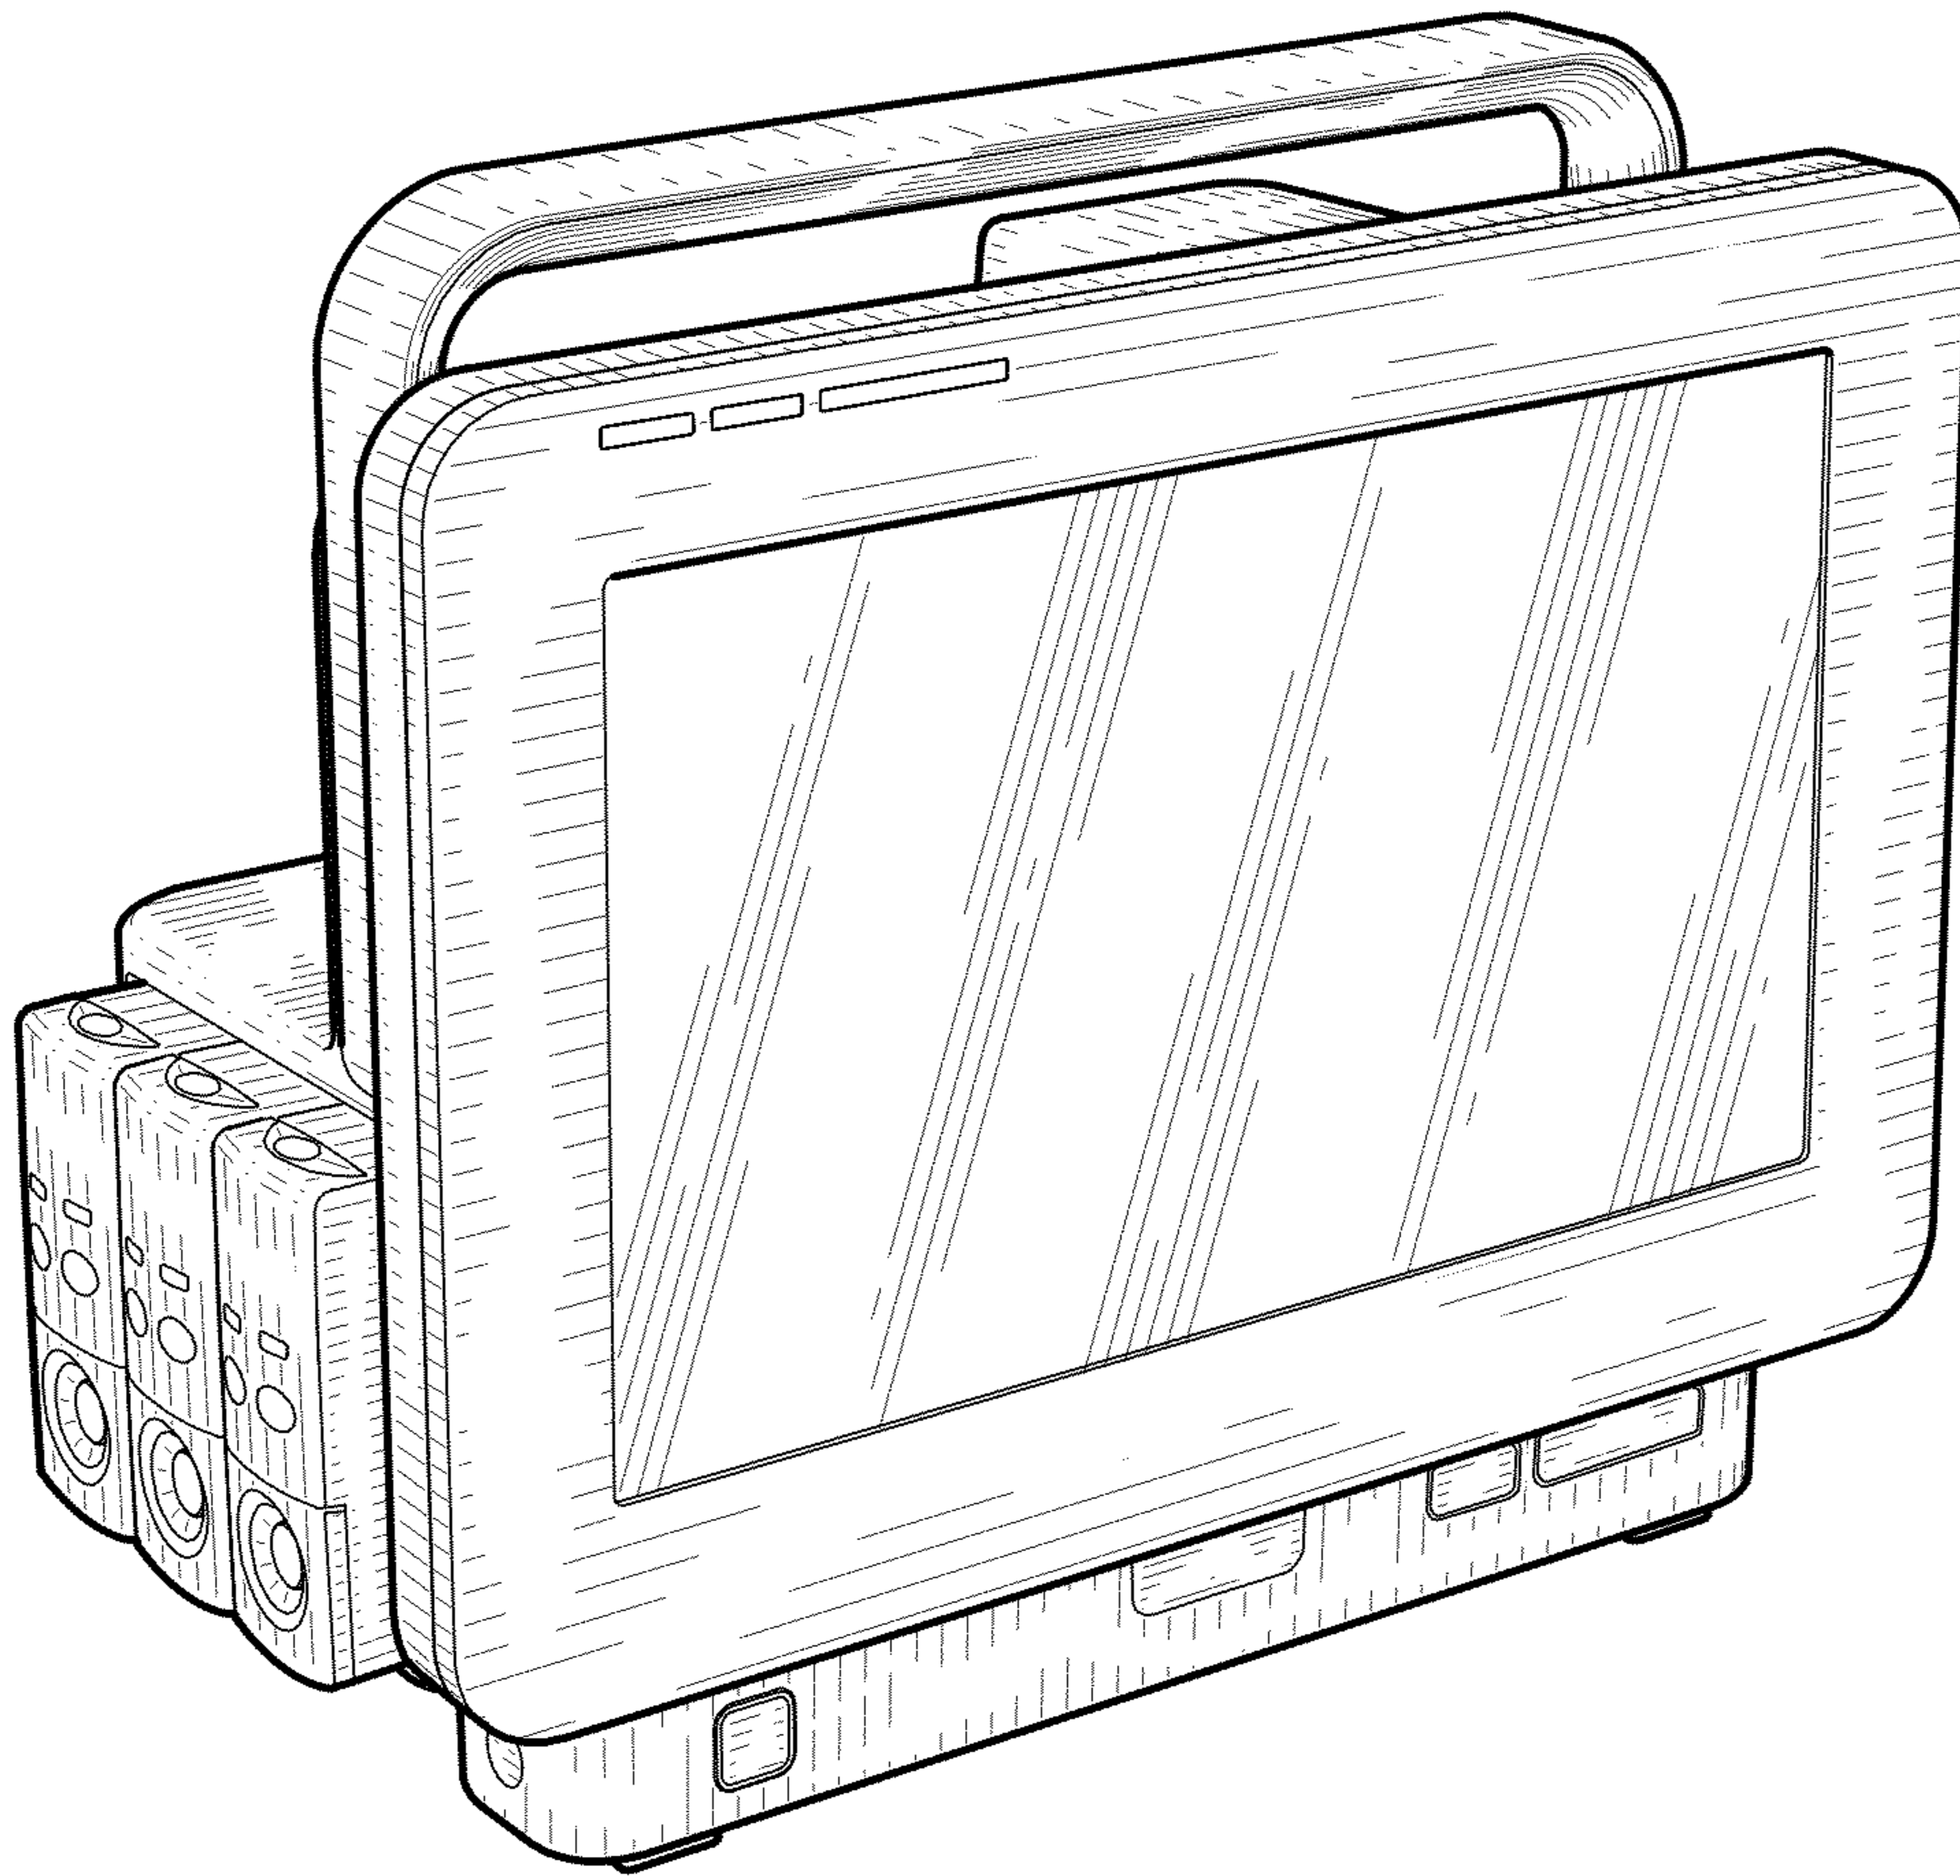


FIG. 1

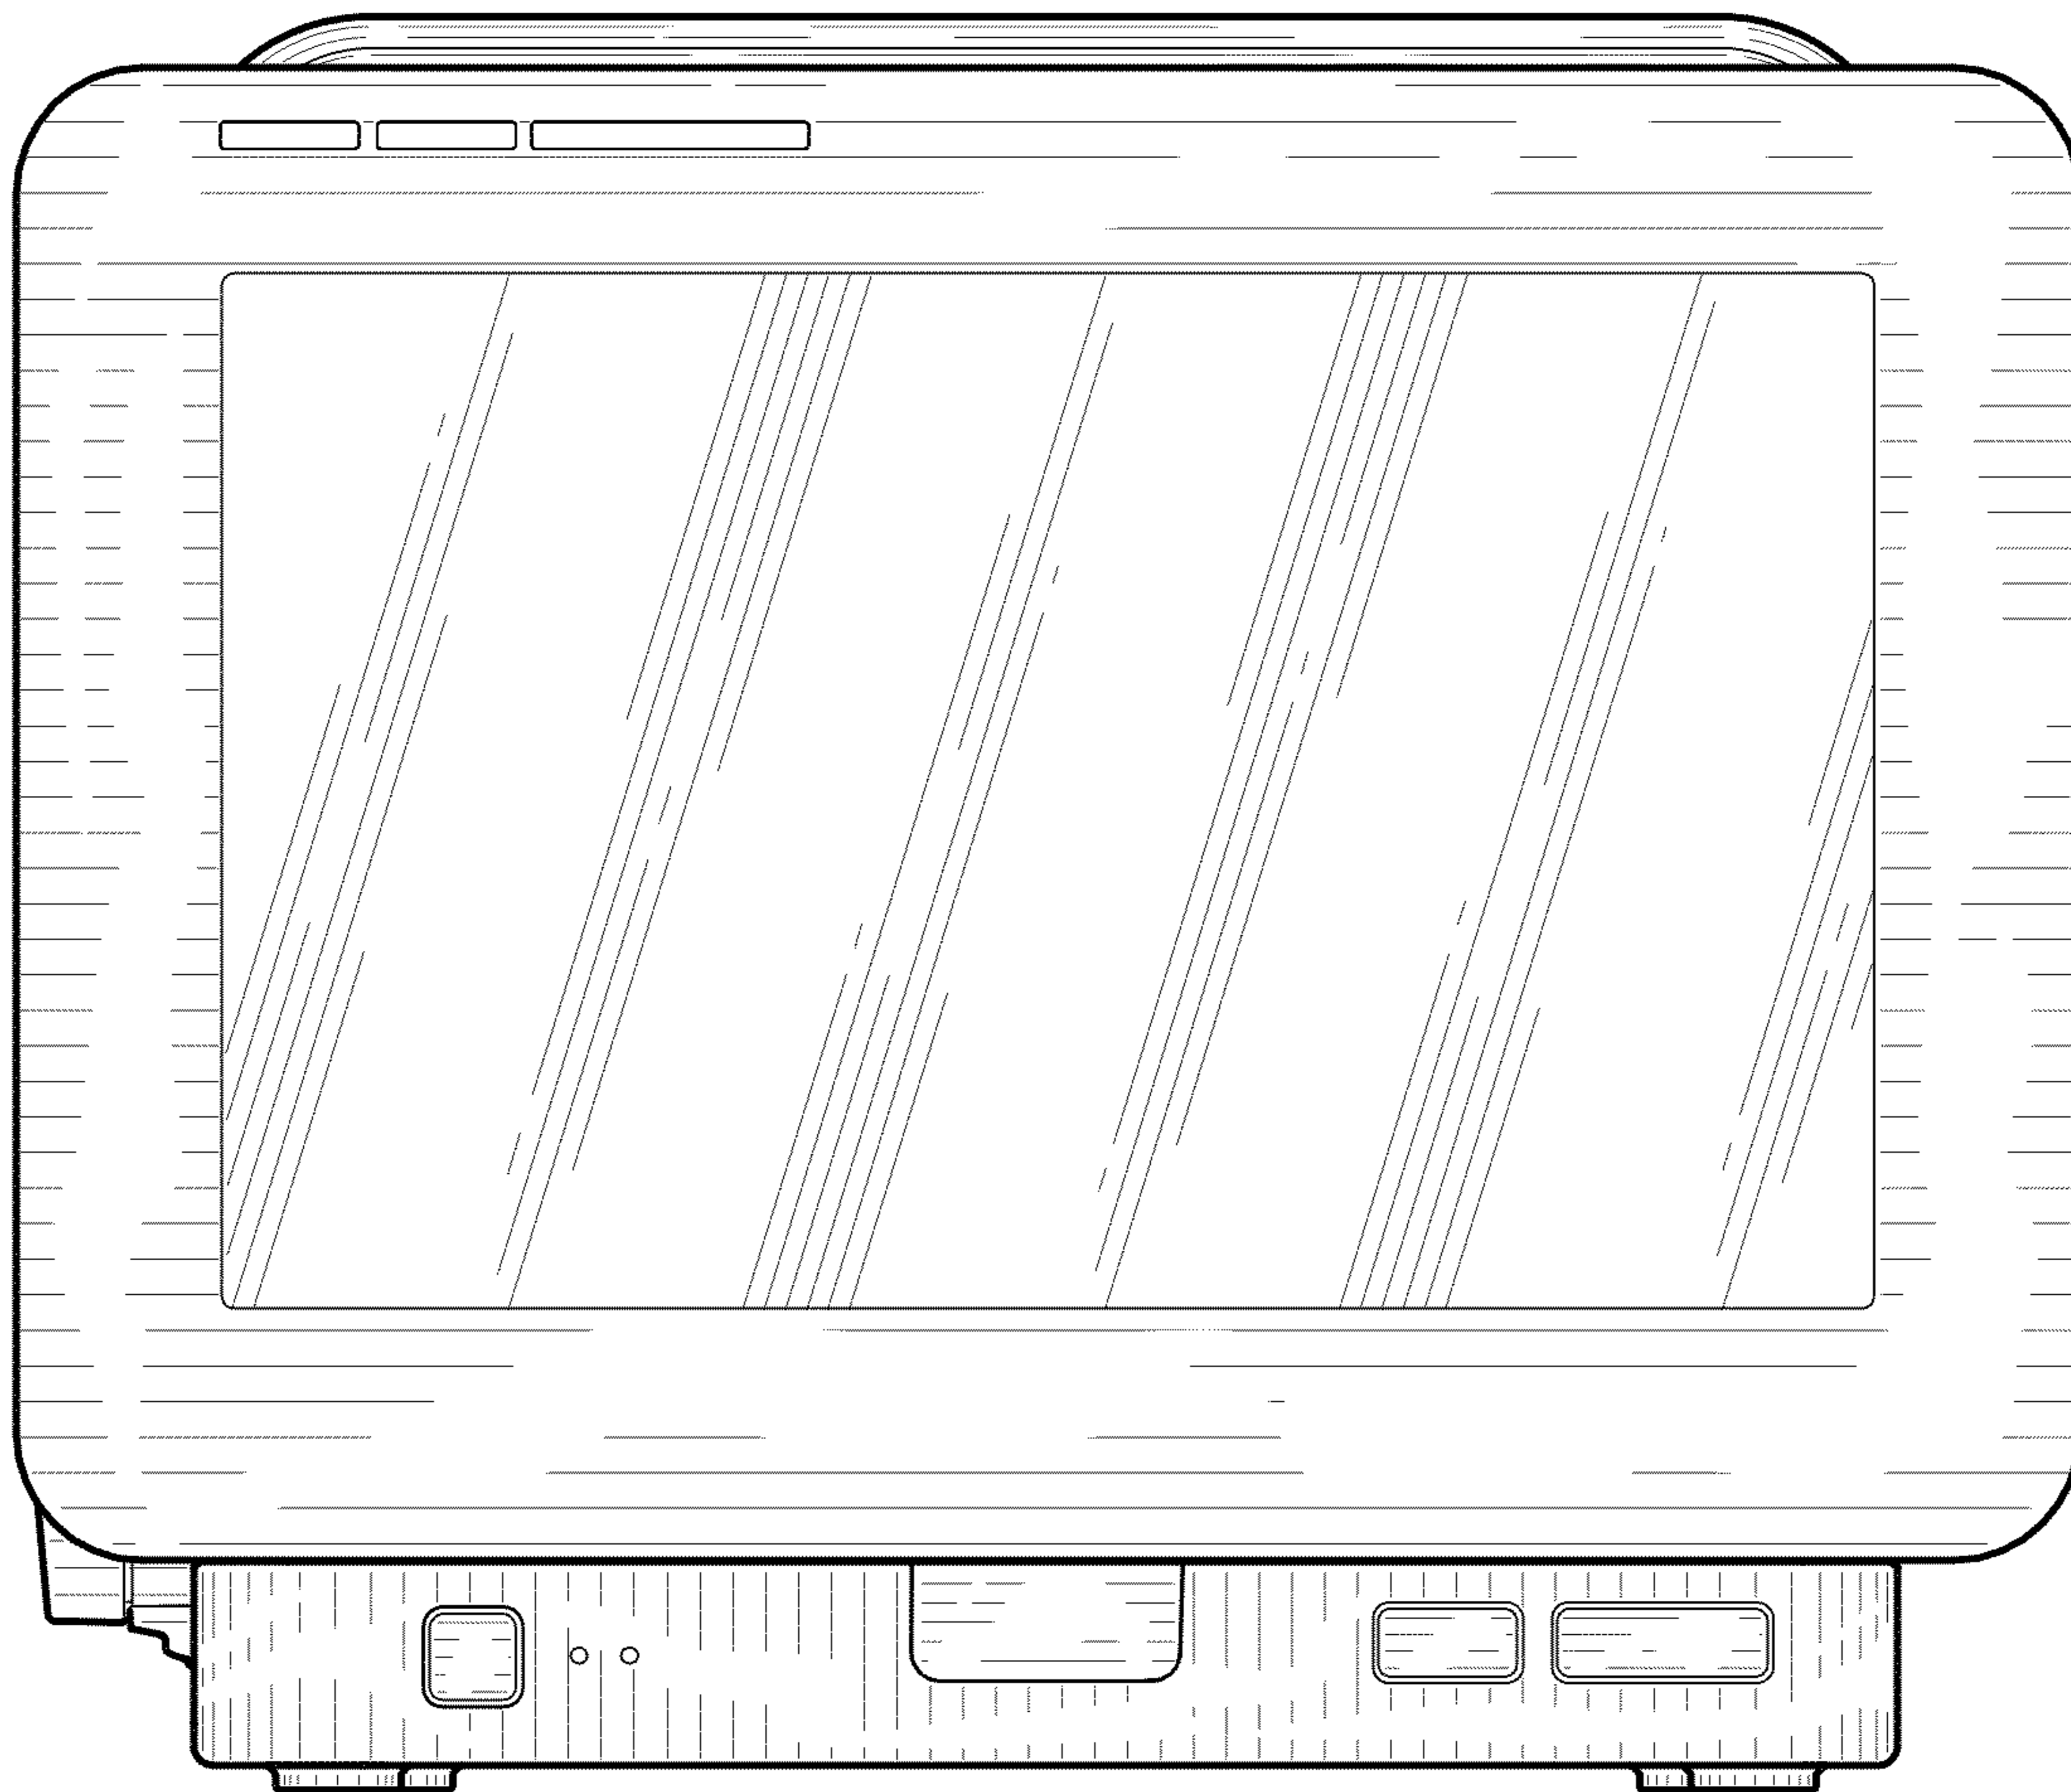


FIG. 2

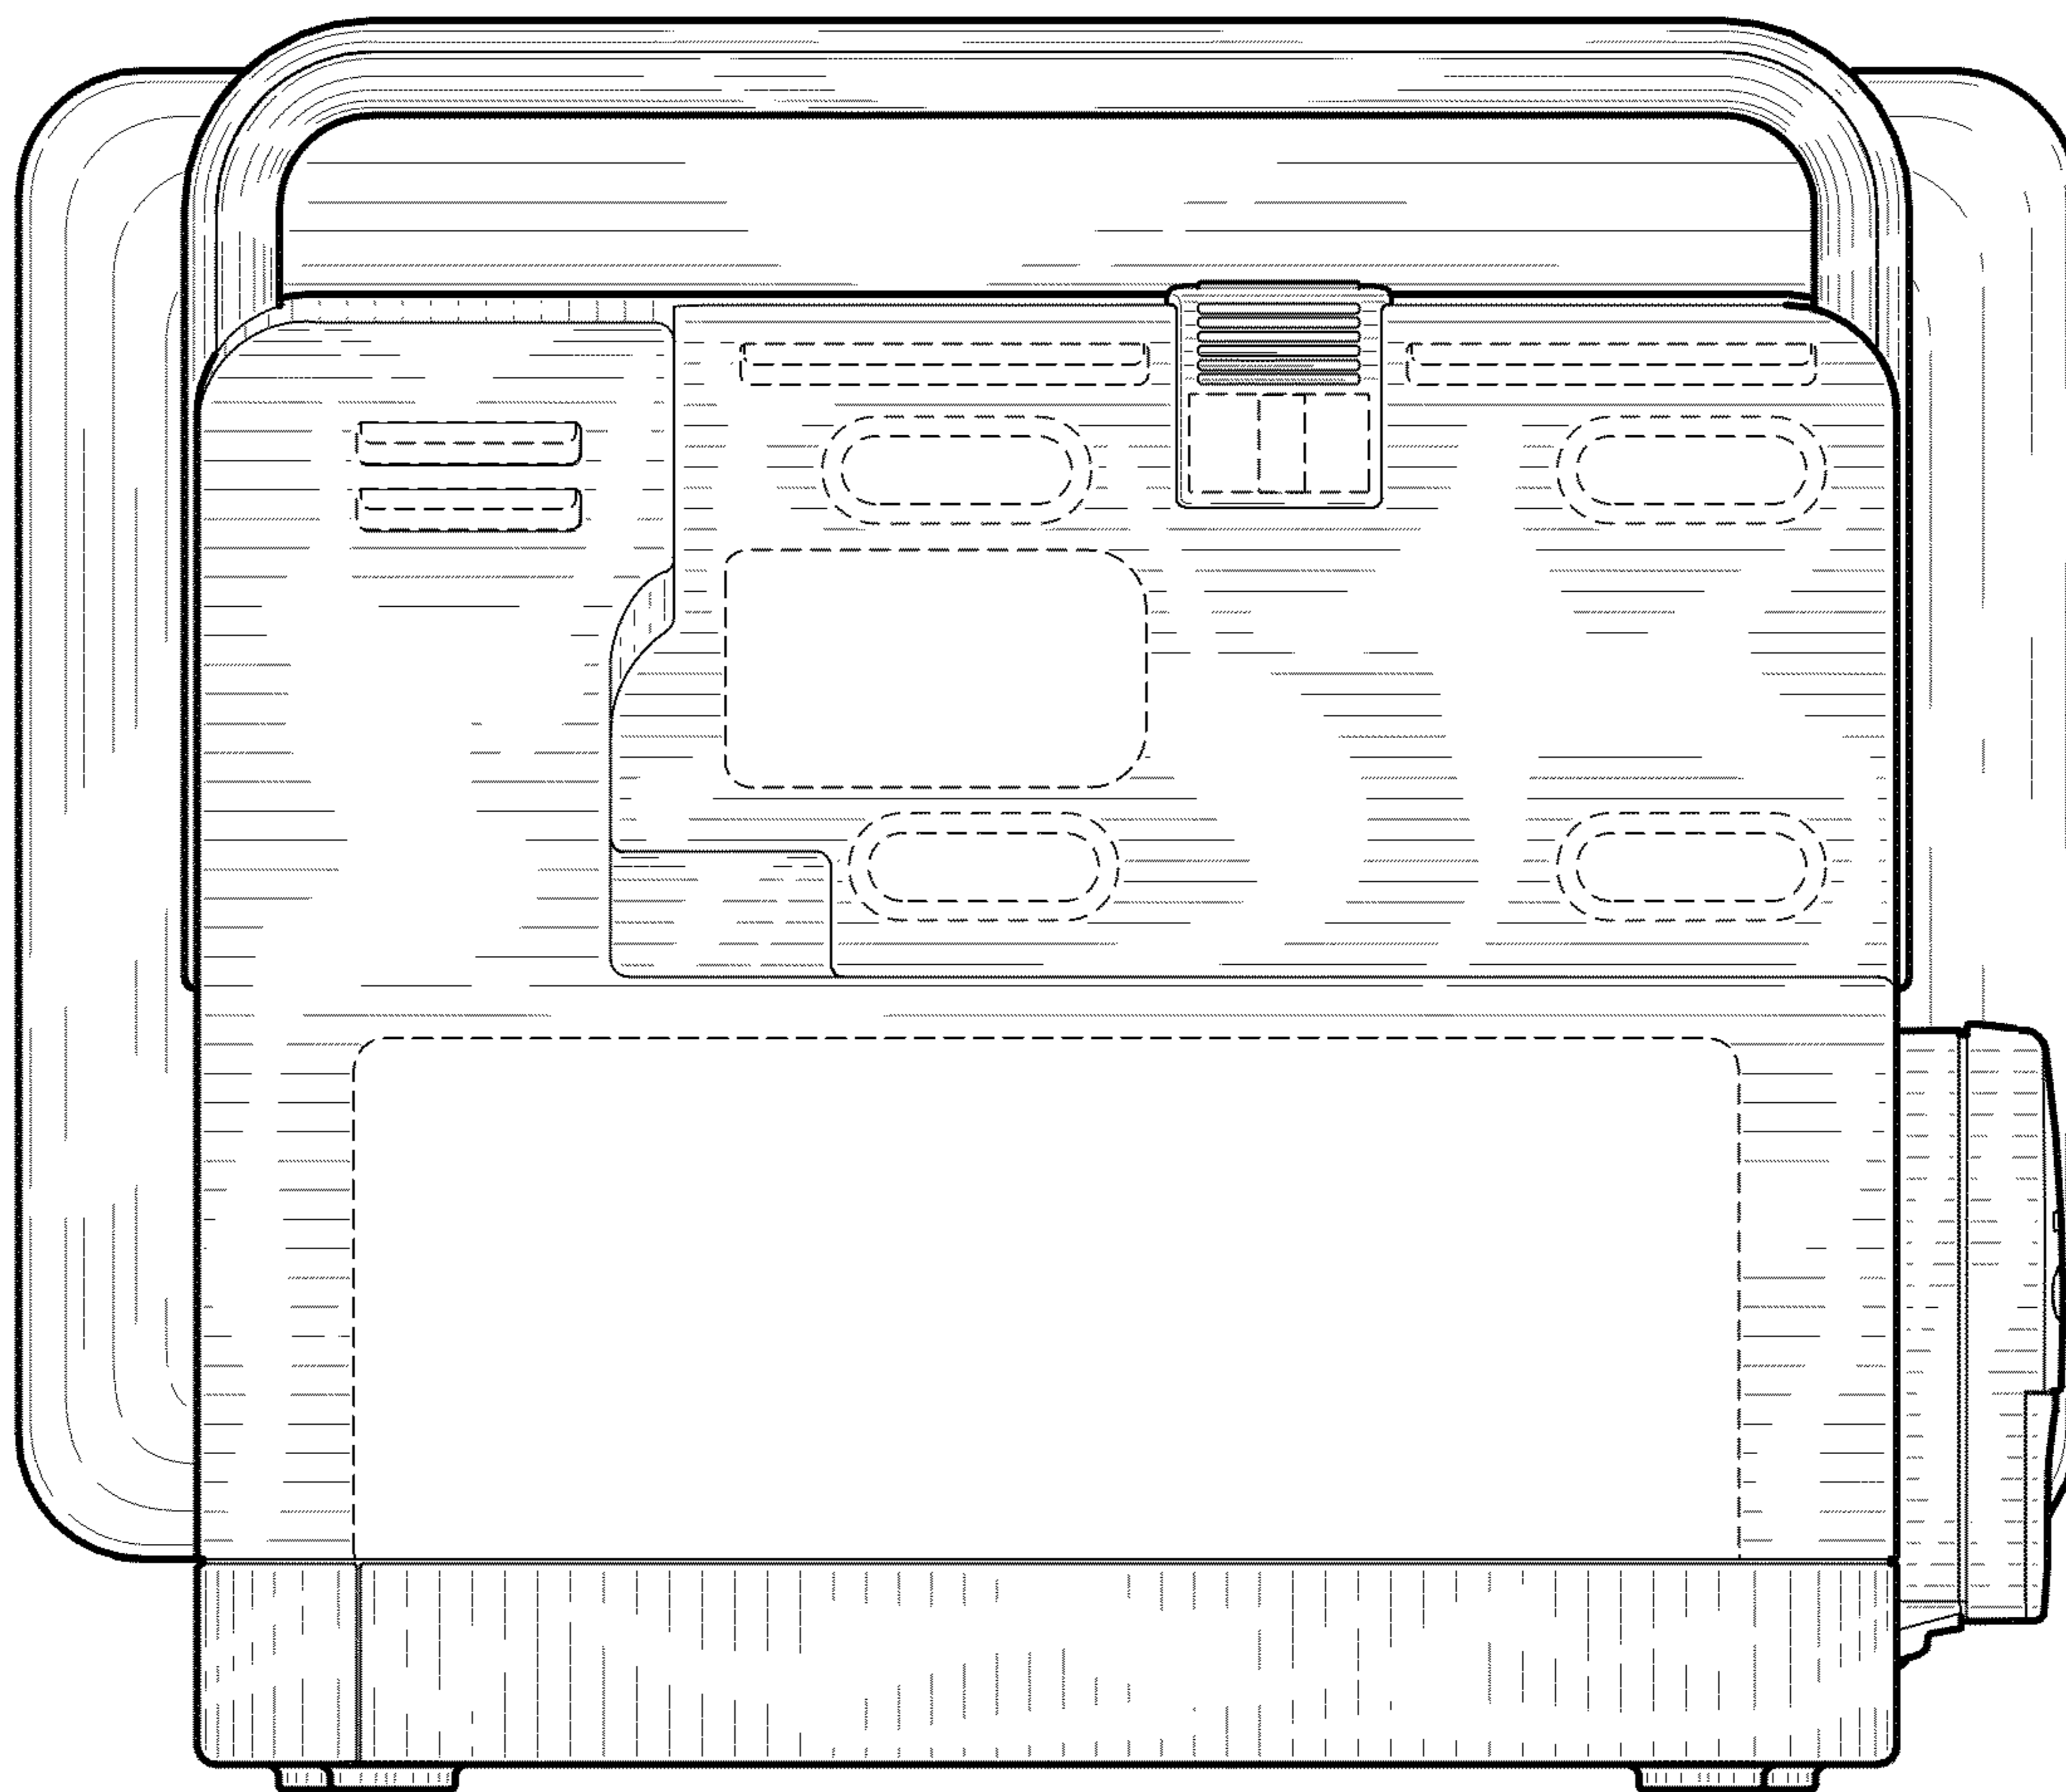


FIG. 3

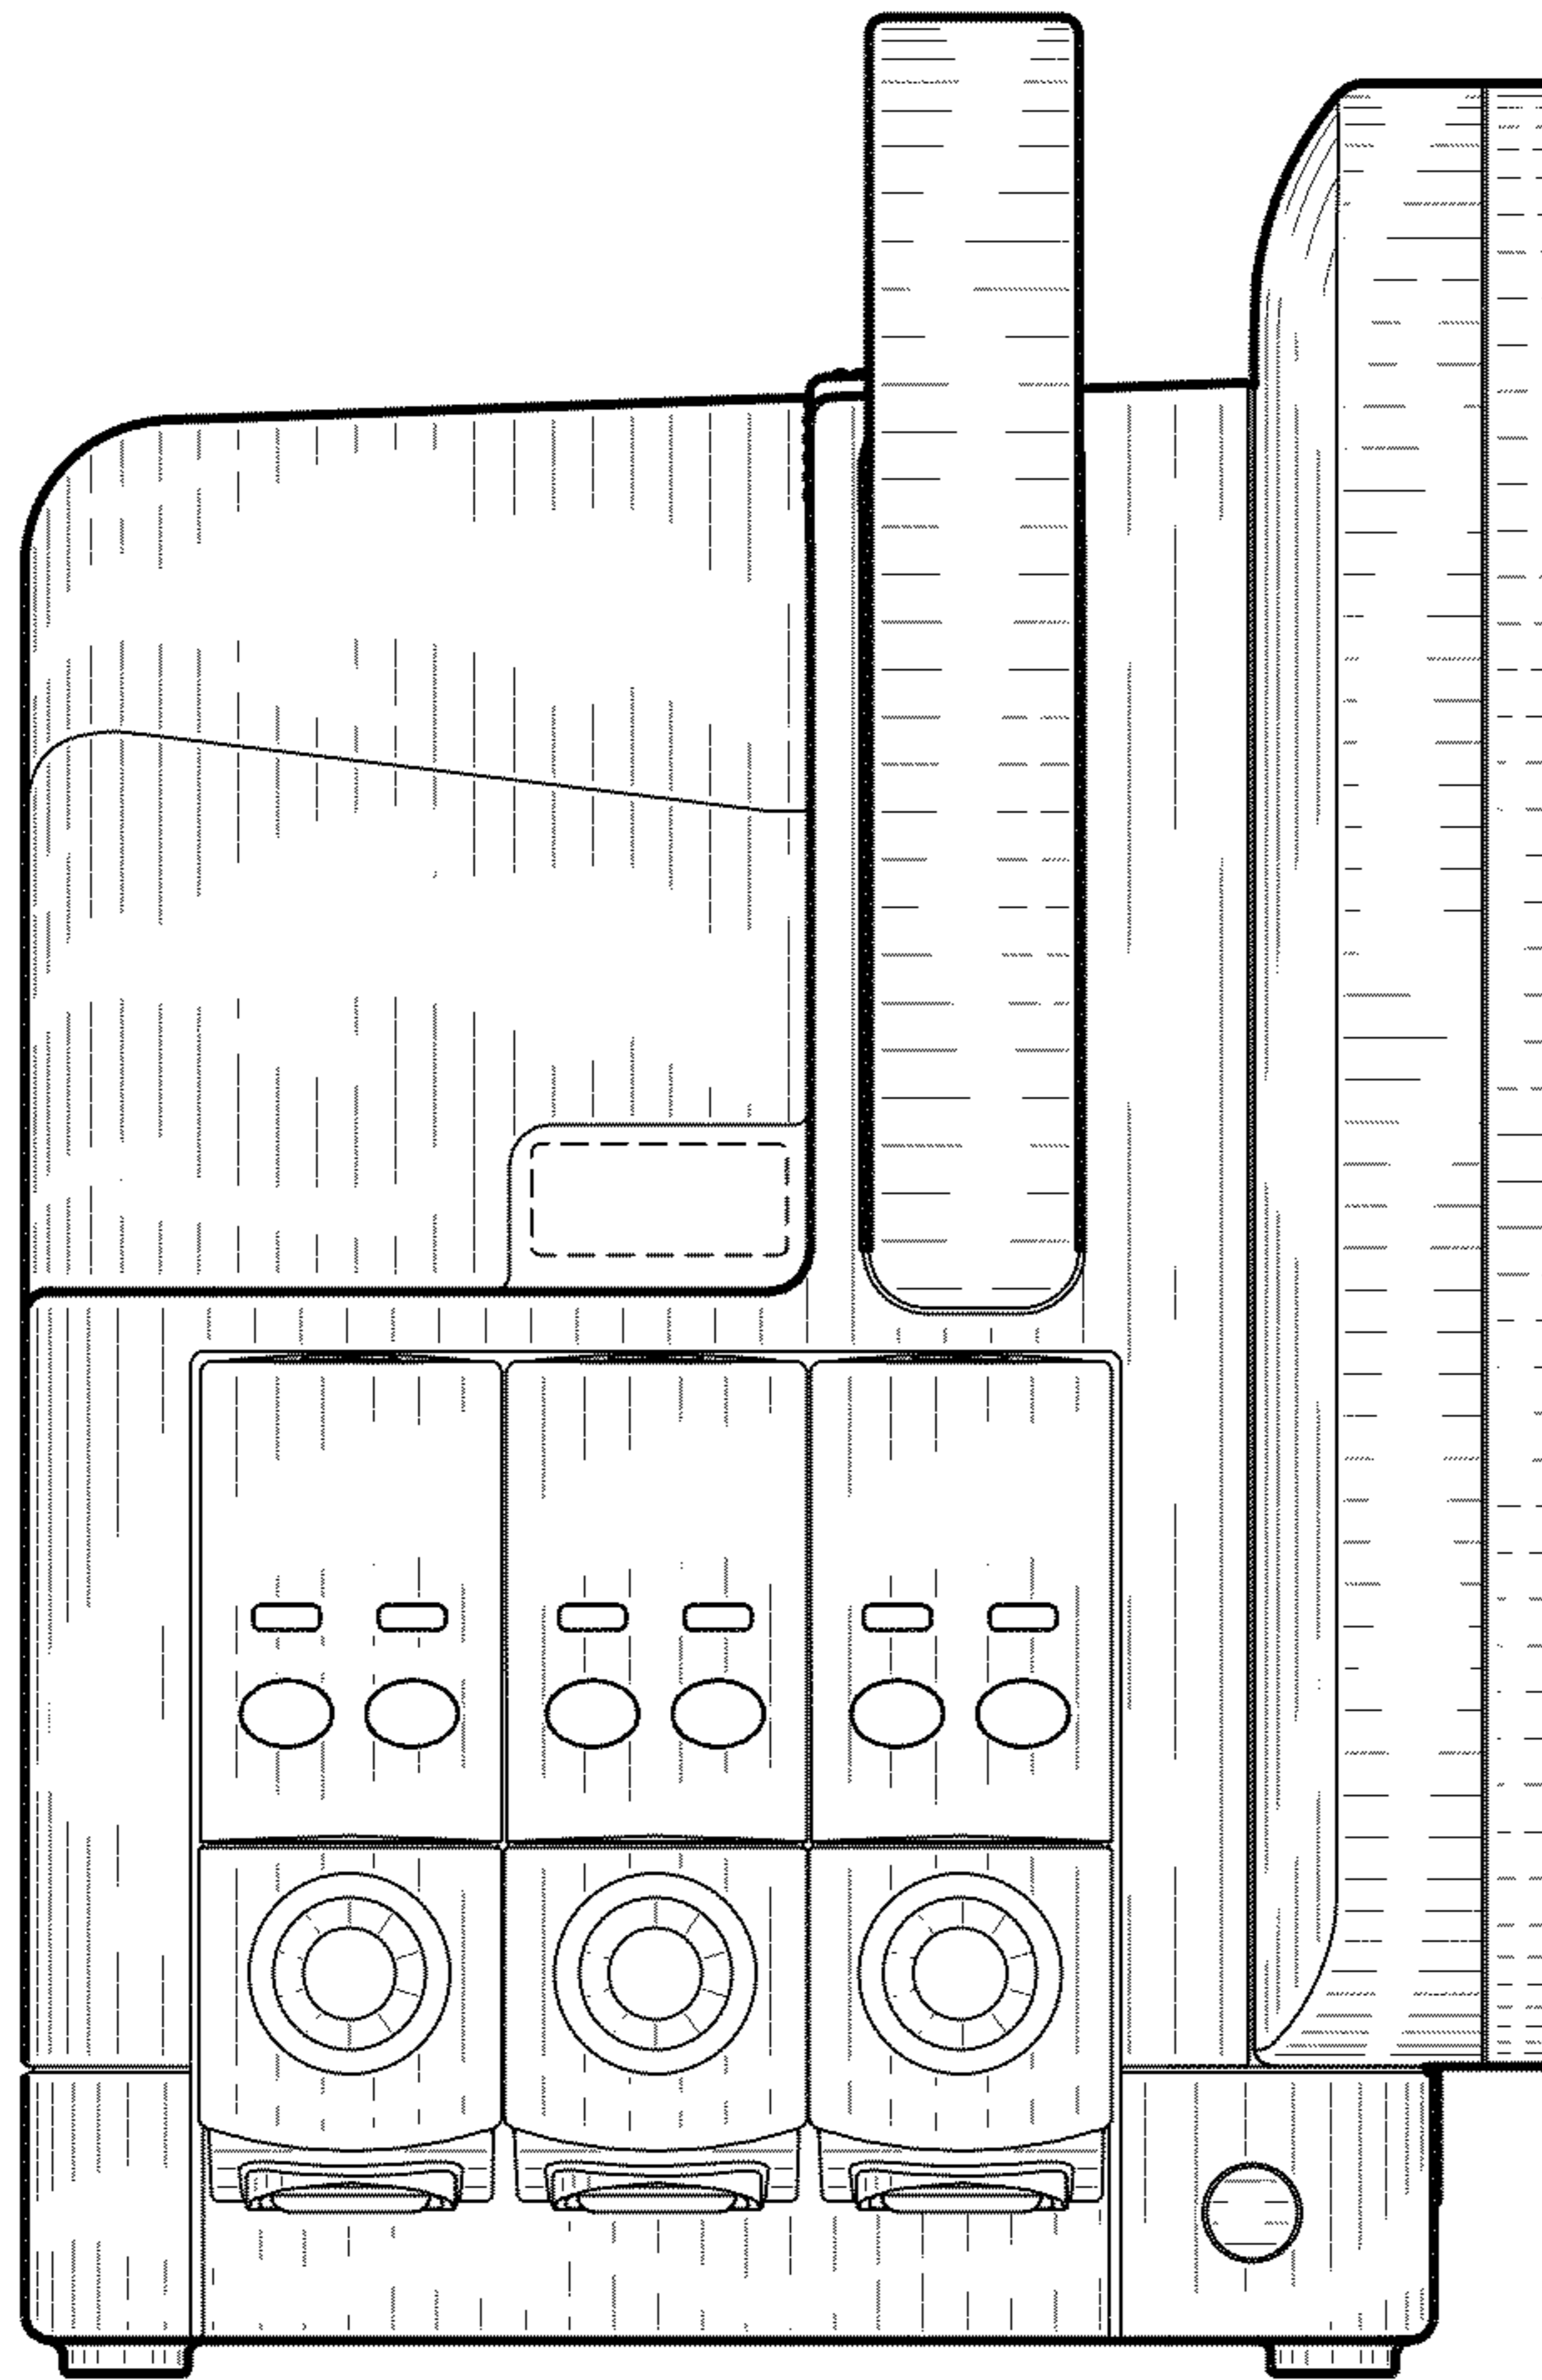


FIG. 4

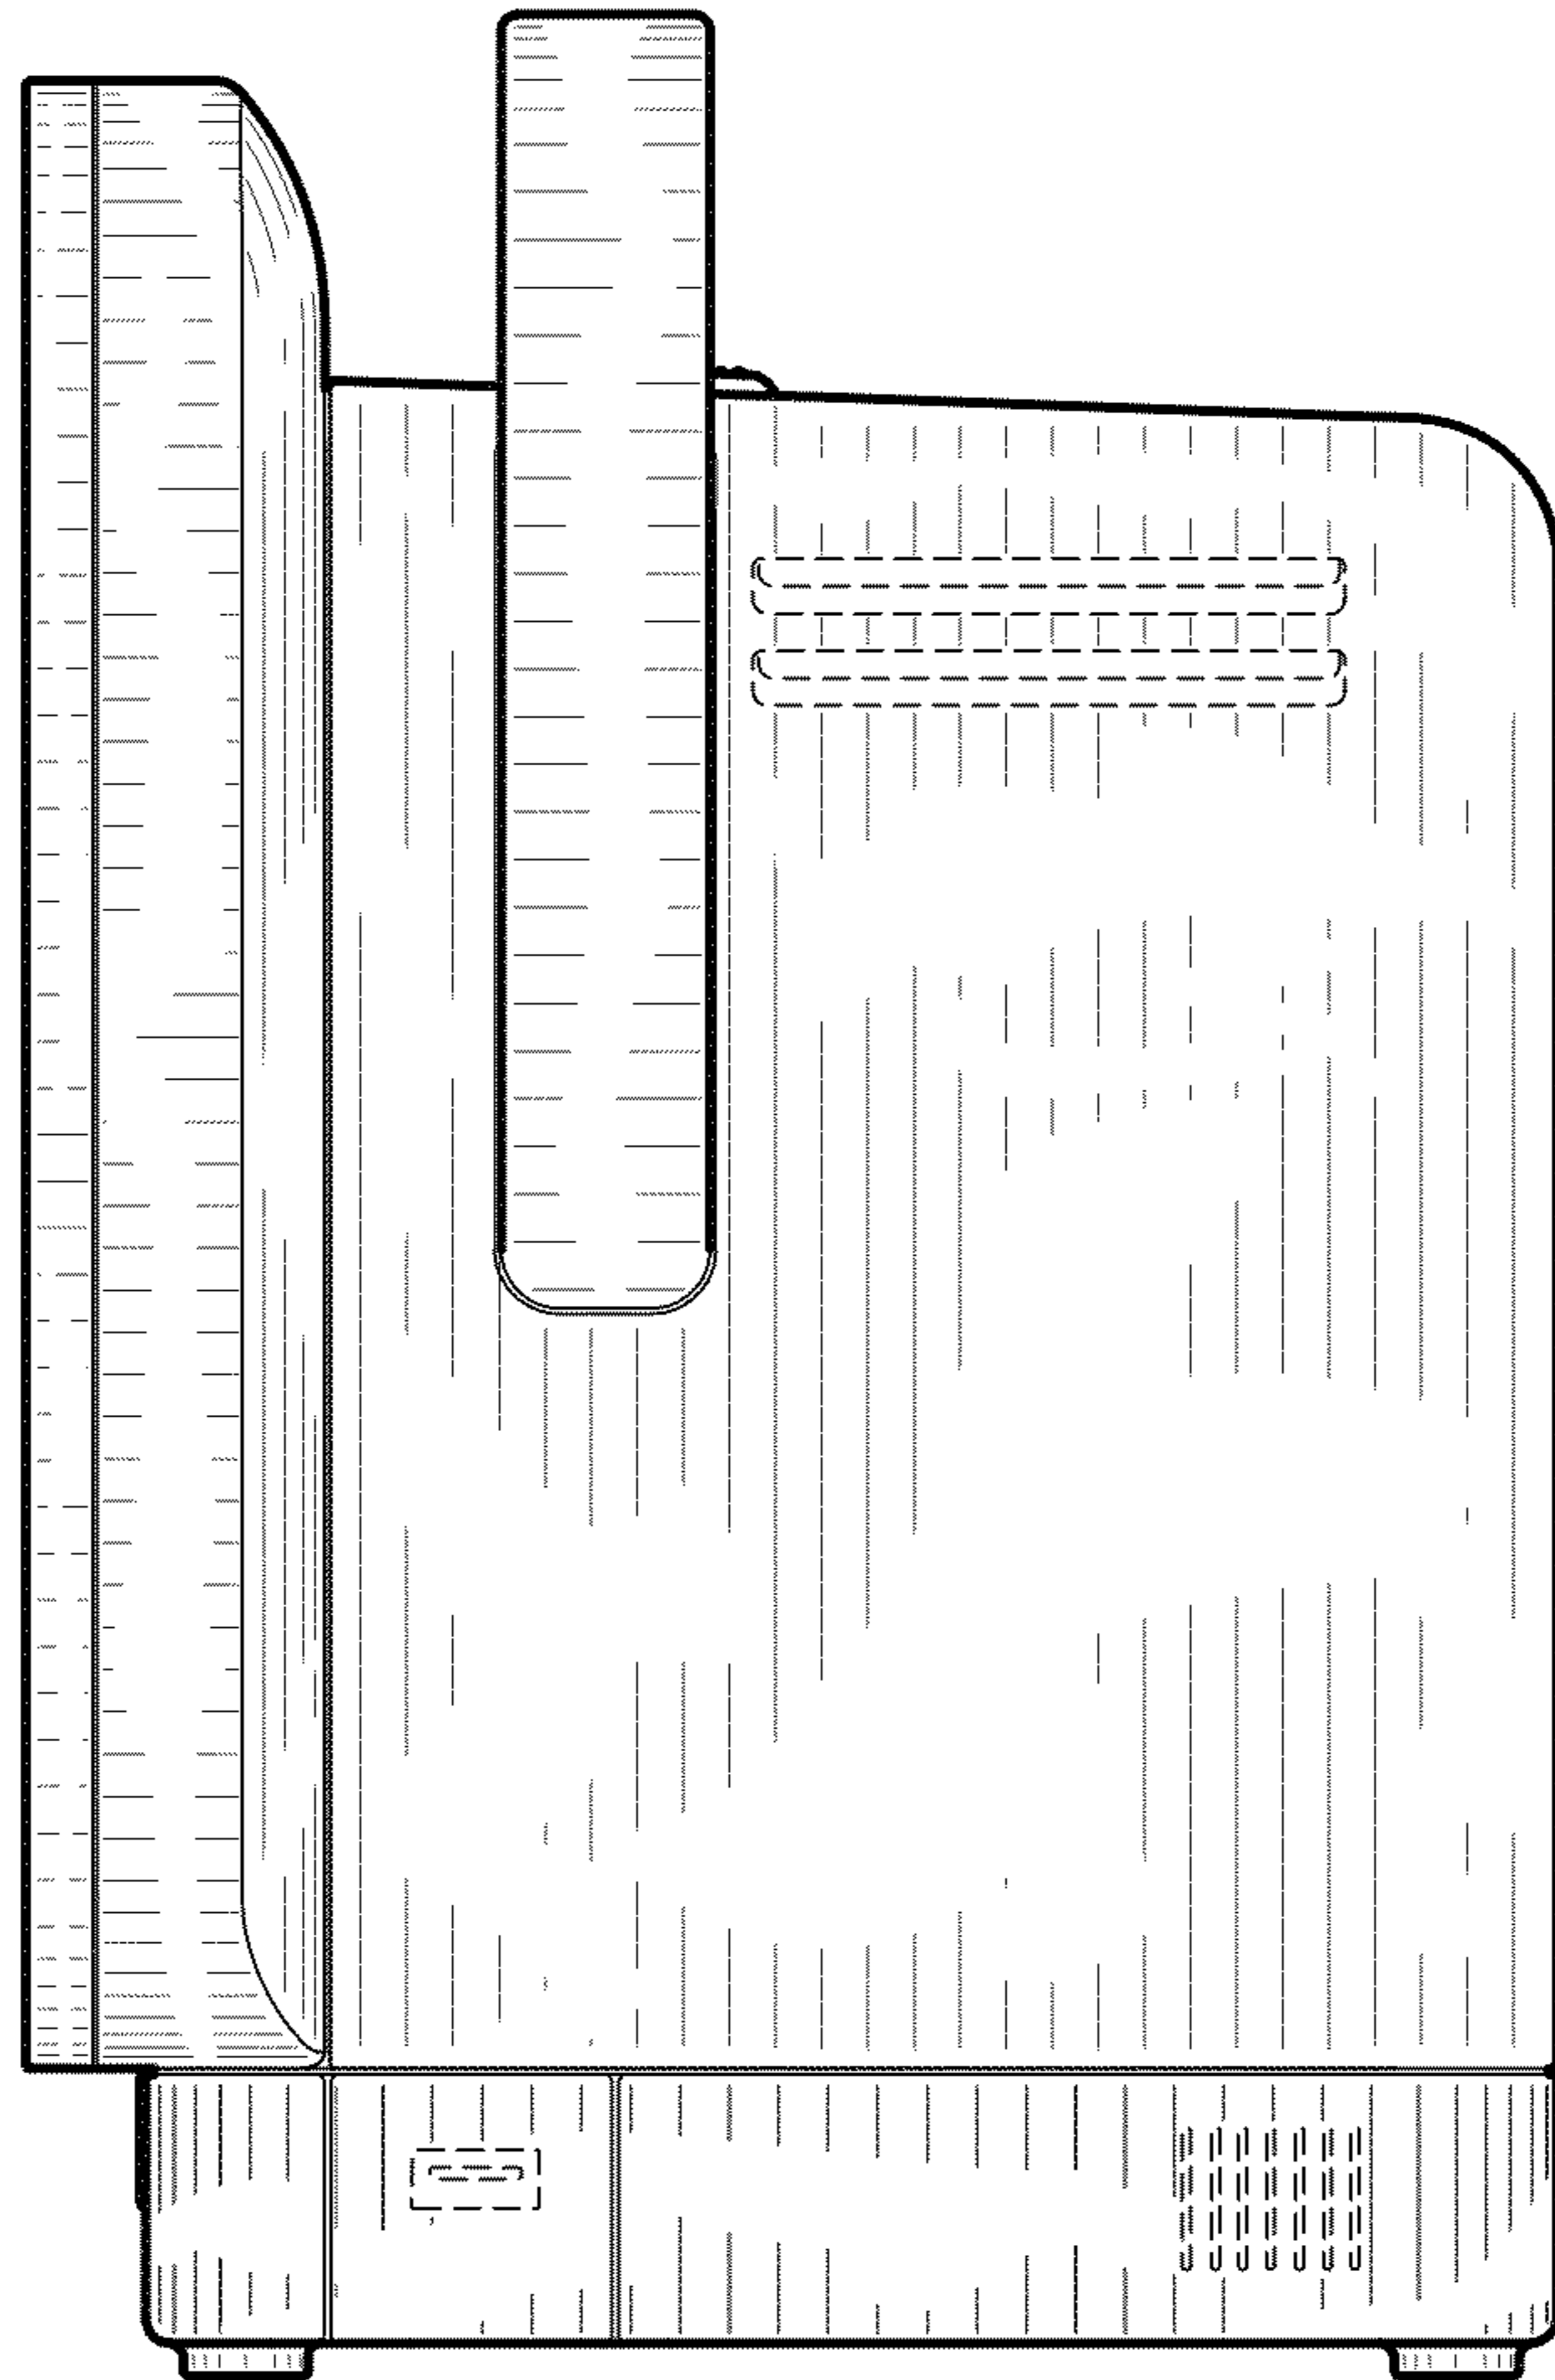


FIG. 5

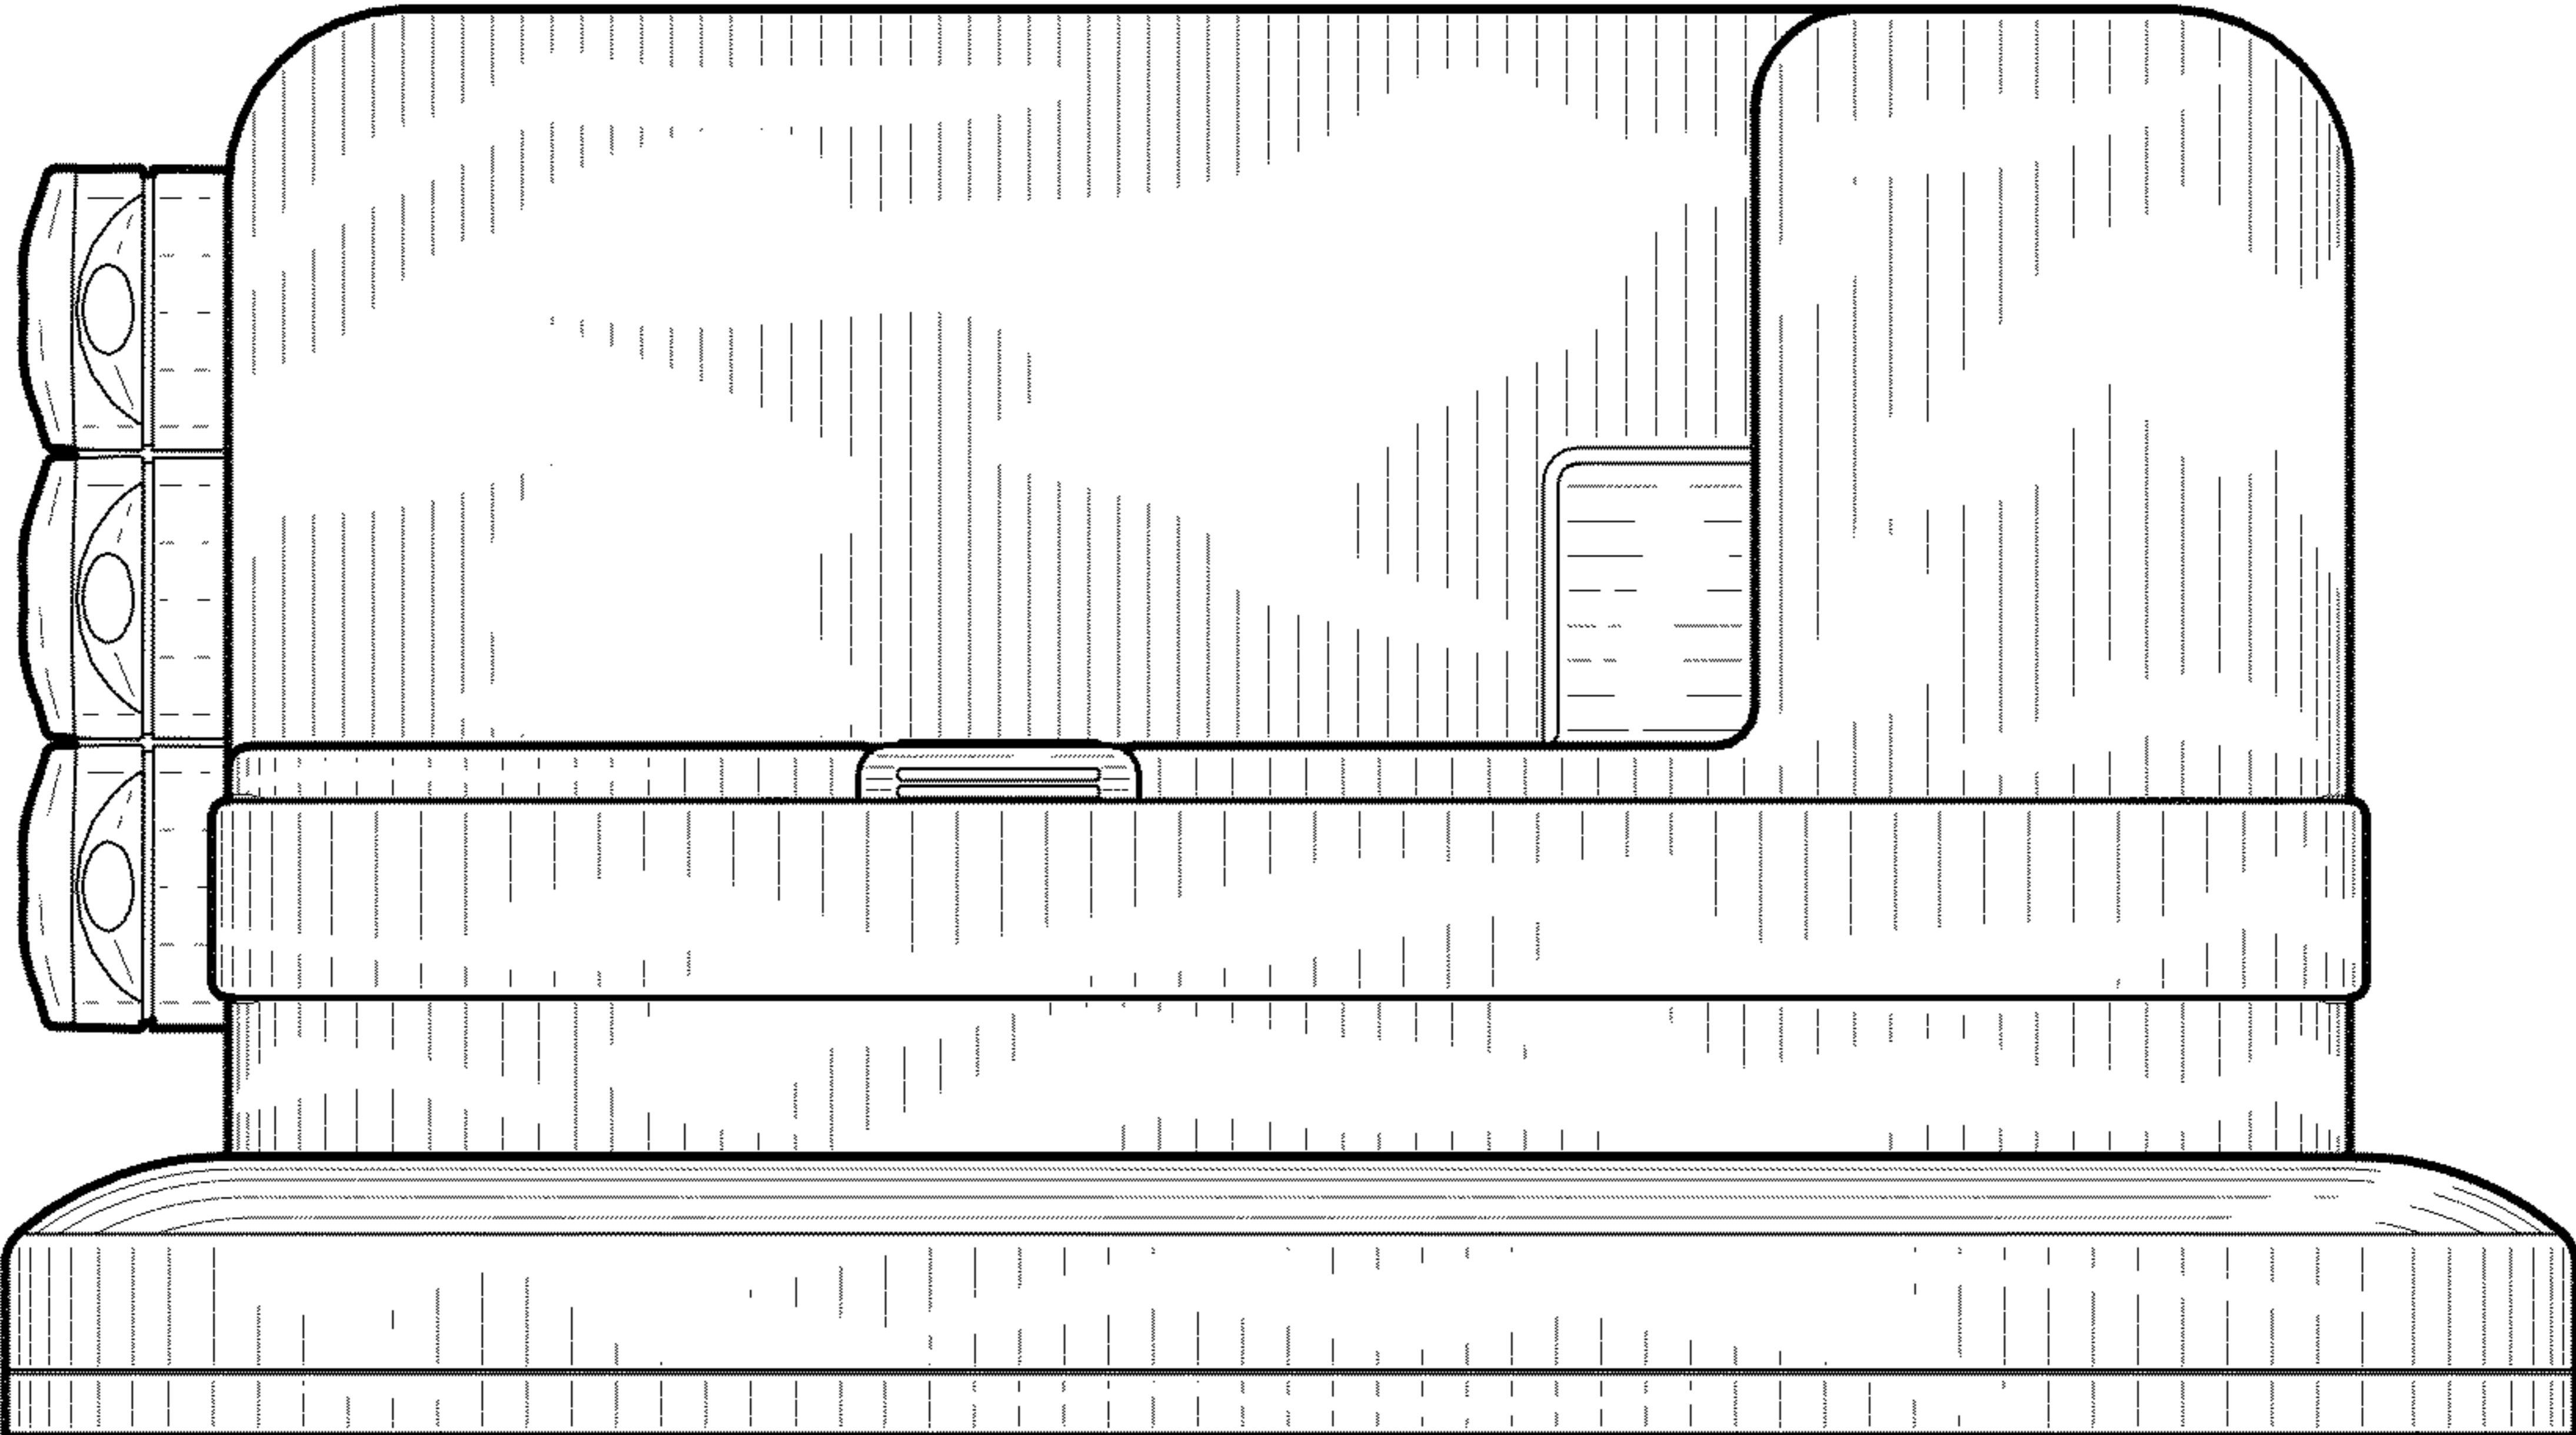


FIG. 6



FIG. 7