

US00D737980S

(12) **United States Design Patent**  
**Golnik et al.**

(10) **Patent No.:** **US D737,980 S**

(45) **Date of Patent:** **\*\* Sep. 1, 2015**

(54) **BLOOD GLUCOSE METER**

(71) Applicant: **Sanofi-Aventis Deutschland GmbH**,  
Frankfurt am Main (DE)

(72) Inventors: **Timothy Golnik**, Stoneham, MA (US);  
**Evan Brooks**, San Anselmo, CA (US)

(73) Assignee: **SANOFI DEUTSCHLAND GMBH**,  
Frankfurt am Main (DE)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/481,603**

(22) Filed: **Feb. 7, 2014**

(30) **Foreign Application Priority Data**

Aug. 7, 2013 (EM) ..... 002 288 266

(51) **LOC (10) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/169**

(58) **Field of Classification Search**  
USPC ..... D24/216, 223, 231, 232, 107, 169, 186;  
D10/81; 422/68.1, 420, 500;  
435/287.1, 287.3; 436/43, 45, 47;  
600/309, 365, 368, 583, 584  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D406,895	S *	3/1999	Byrd et al.	.....	D24/169
D473,310	S *	4/2003	Schlagheck et al.	.....	D24/169
D546,457	S *	7/2007	Hannant et al.	.....	D24/186
D562,458	S *	2/2008	Padain	.....	D24/169
D696,404	S *	12/2013	Golnik et al.	.....	D24/169
D713,963	S *	9/2014	Liedtke et al.	.....	D24/169
2010/0113896	A1 *	5/2010	Cadio et al.	.....	600/309
2011/0034786	A1 *	2/2011	Cadio et al.	.....	600/316

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Scully, Scott, Murphy & Presser, P.C.

(57) **CLAIM**

The ornamental design for a blood glucose meter, as shown and described.

**DESCRIPTION**

The patent or application file contains at least one drawing executed in color. Copies of this patent or patent application publication with color drawing(s) will be provided by the Office upon request and payment of the necessary fee.

FIG. 1 is a perspective view of a blood glucose meter, showing a first embodiment of our new design;

FIG. 2 is a front view of FIG. 1;

FIG. 3 is a rear view of FIG. 1;

FIG. 4 is a side view of FIG. 1;

FIG. 5 is an opposite side view of FIG. 1;

FIG. 6 is a top view of FIG. 1;

FIG. 7 is a bottom view of FIG. 1;

FIG. 8 is a perspective view of a blood glucose meter, showing a second embodiment of our new design;

FIG. 9 is a front view of FIG. 8;

FIG. 10 is a rear view of FIG. 8;

FIG. 11 is a side view of FIG. 8;

FIG. 12 is an opposite side view of FIG. 8;

FIG. 13 is a top view of FIG. 8;

FIG. 14 is a bottom view of FIG. 8;

FIG. 15 is a perspective view of a blood glucose meter, showing a third embodiment of our new design;

FIG. 16 is a front view of FIG. 15;

FIG. 17 is a rear view of FIG. 15;

FIG. 18 is a side view of FIG. 15;

FIG. 19 is an opposite side view of FIG. 15;

FIG. 20 is a top view of FIG. 15; and,

FIG. 21 is a bottom view of FIG. 15.

The portions indicated in broken lines are for illustrative purposes only and form no part of the claimed design.

**1 Claim, 21 Drawing Sheets**  
**(12 of 21 Drawing Sheet(s) Filed in Color)**

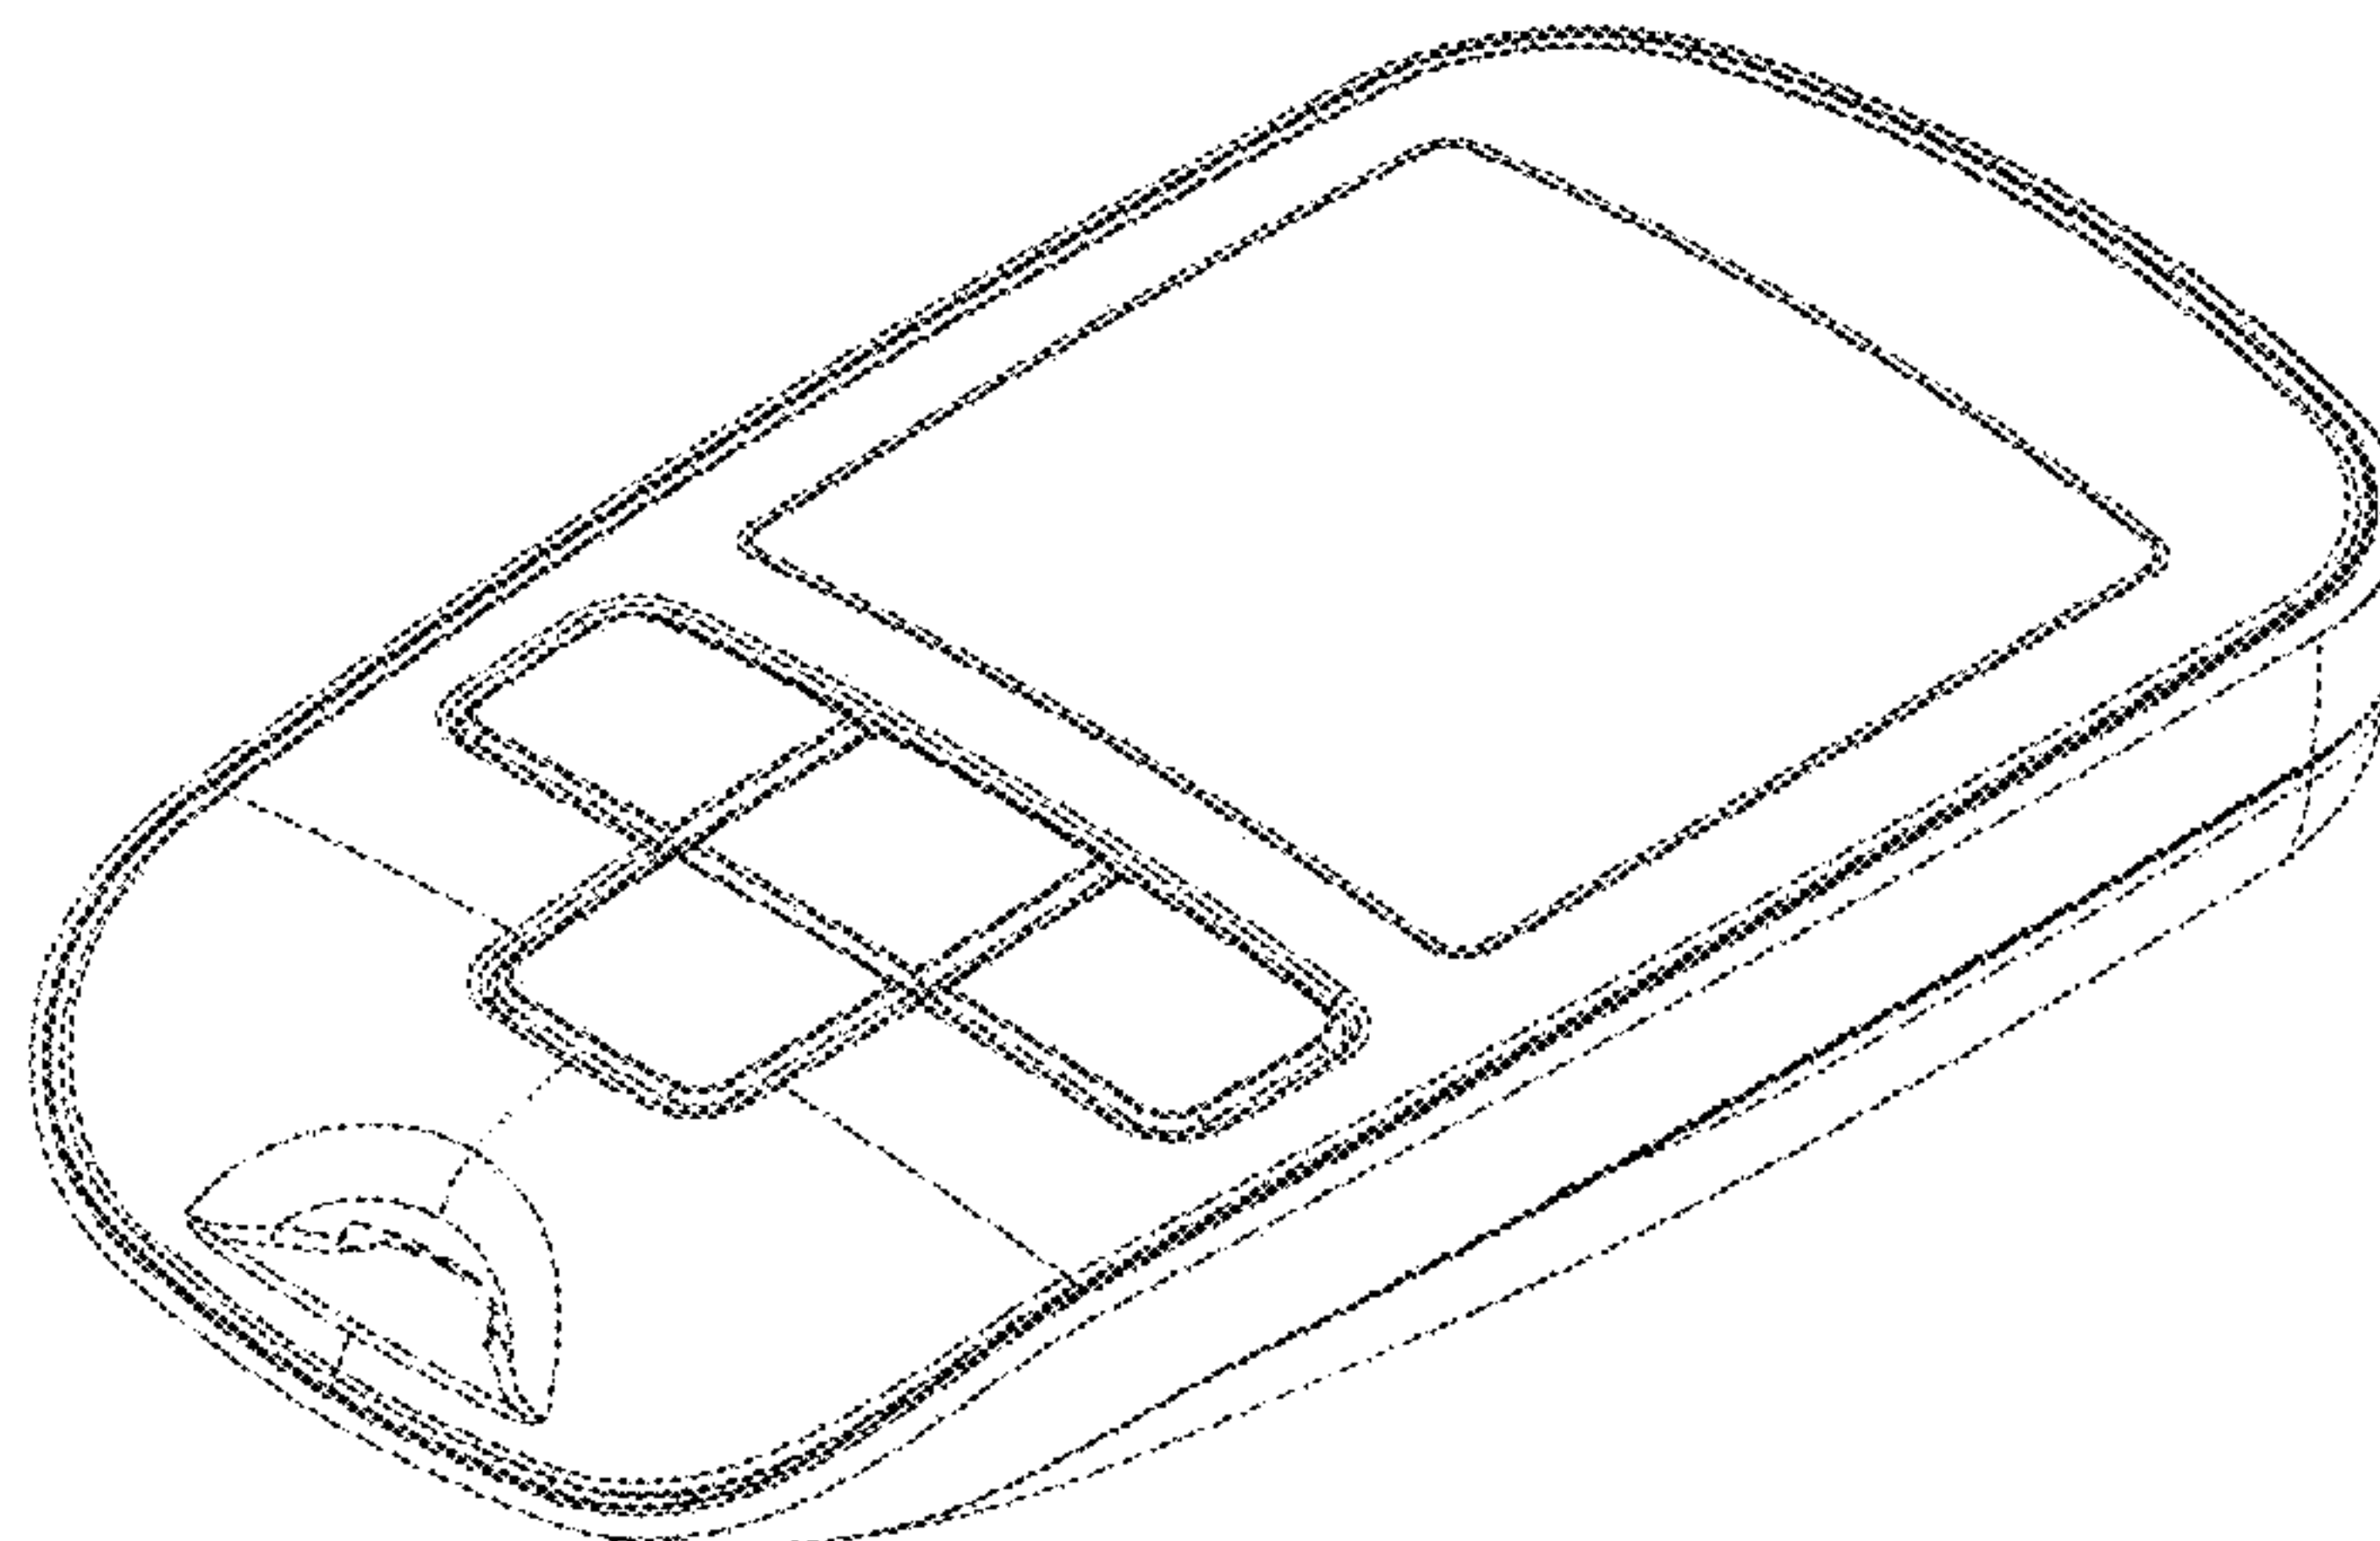






FIG. 1

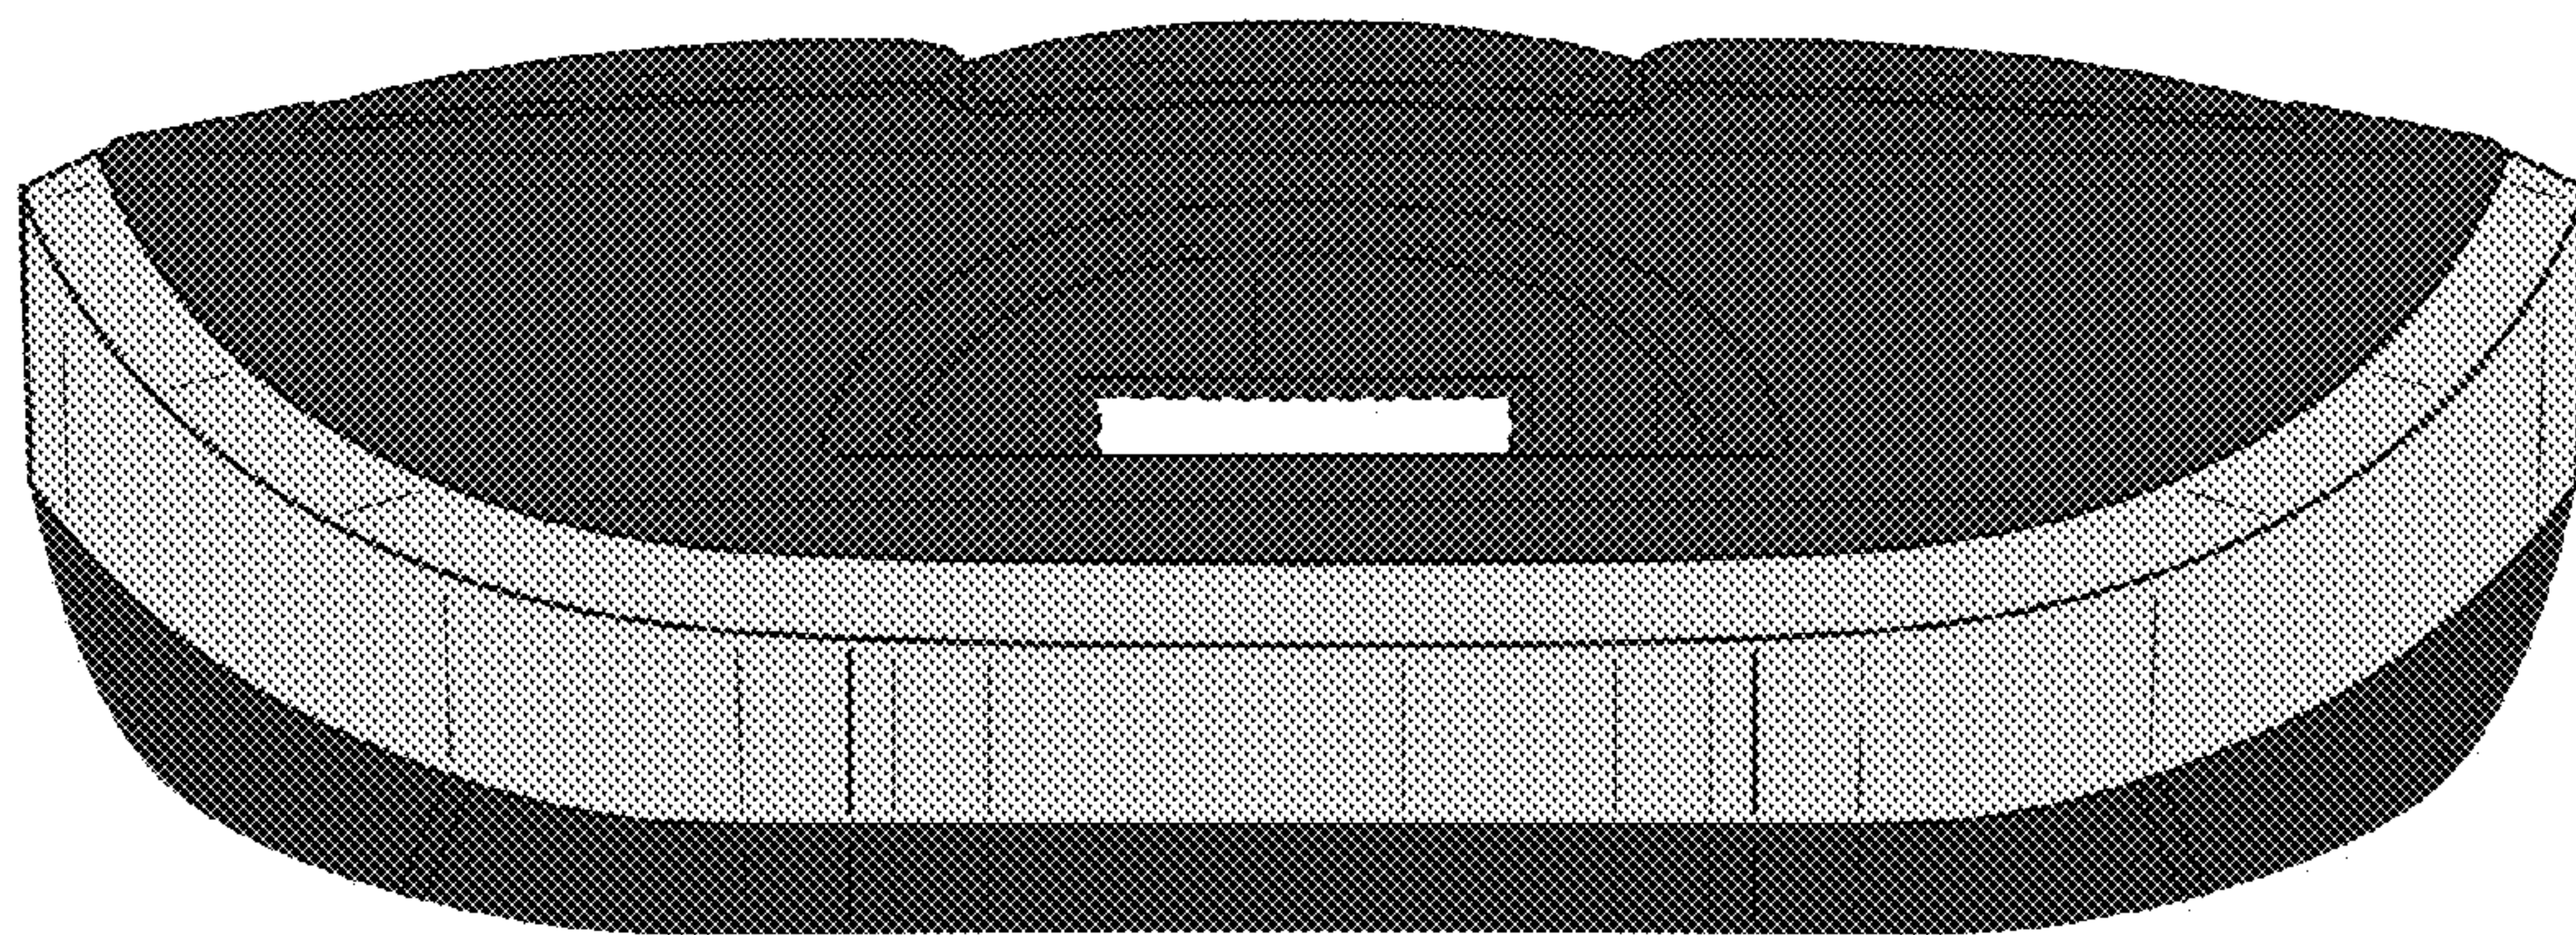


FIG. 2



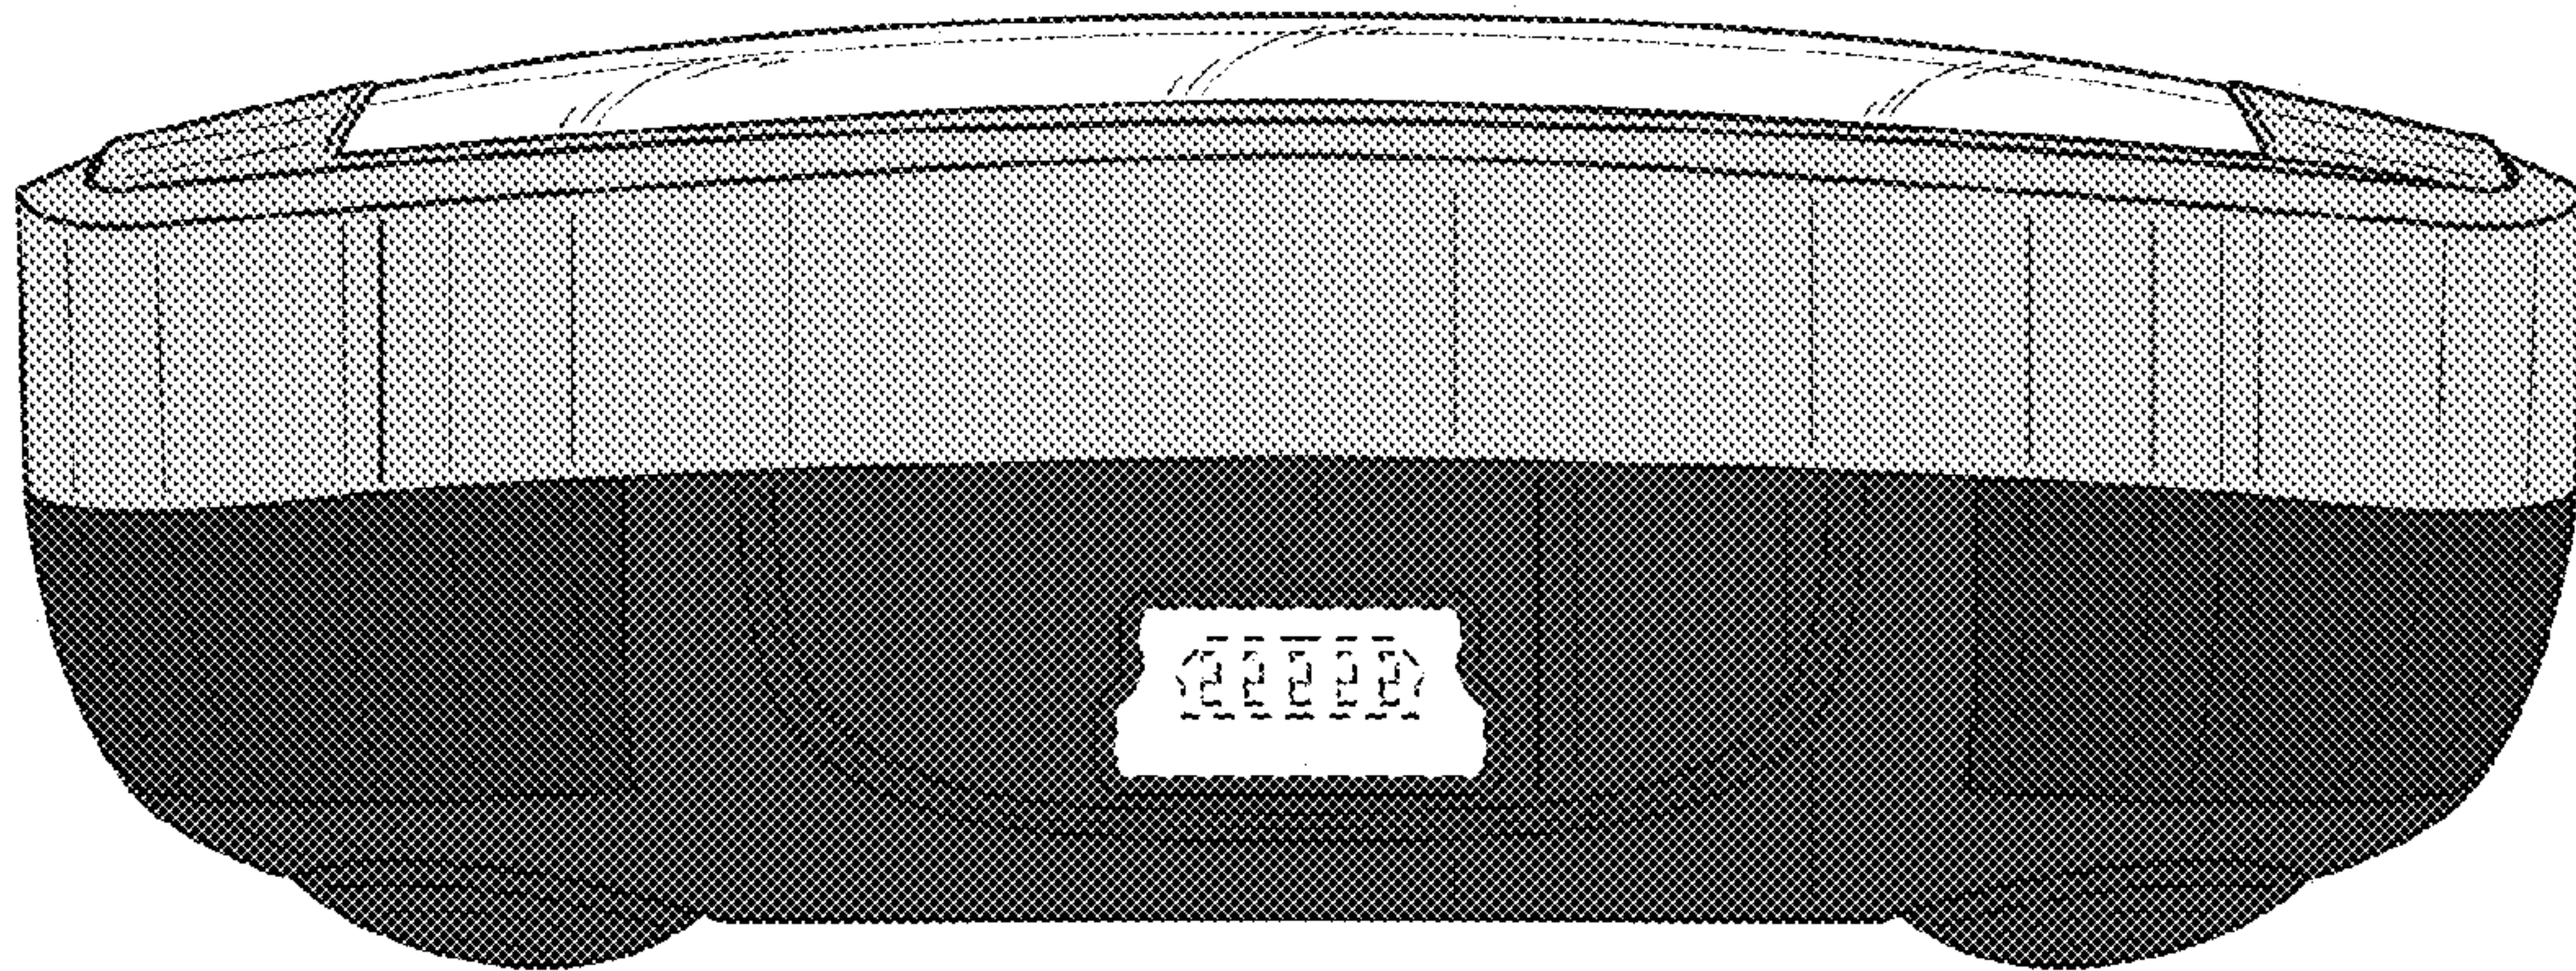


FIG. 3

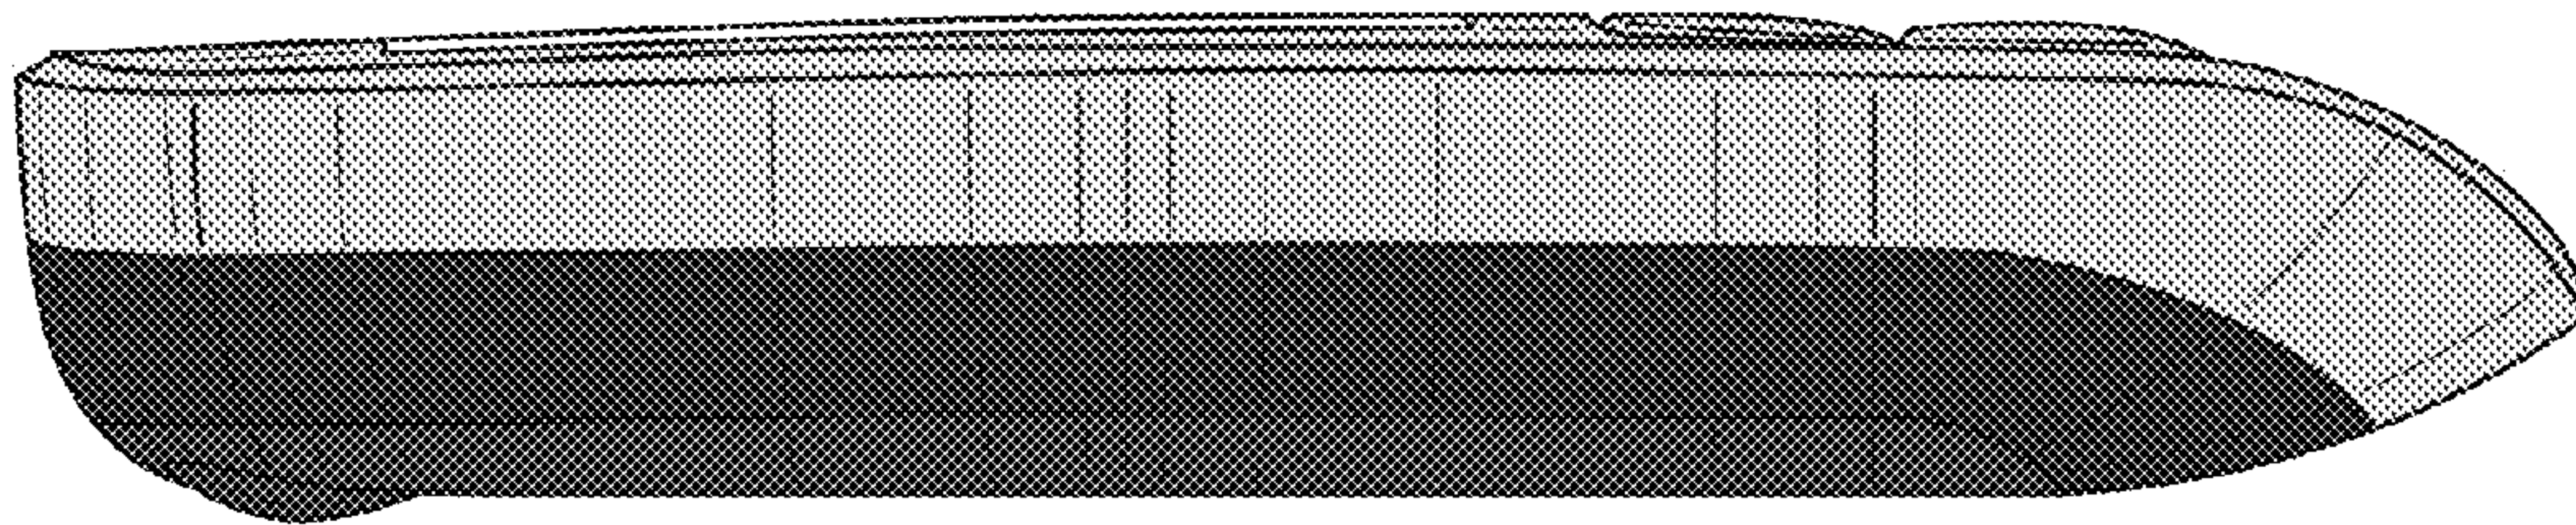


FIG. 4

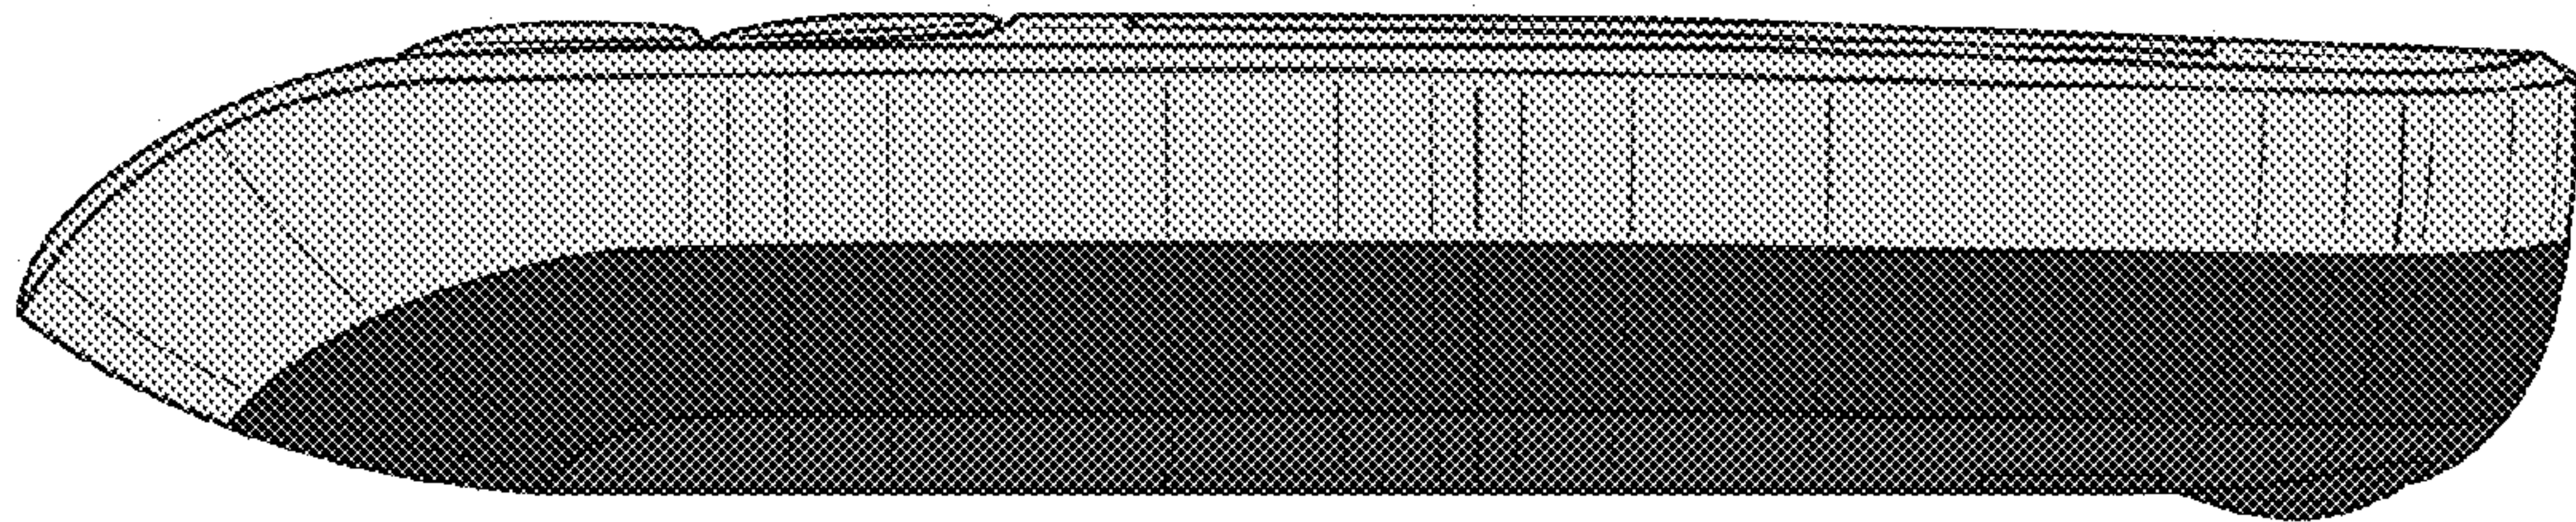


FIG. 5





FIG. 6





FIG. 7





FIG. 8



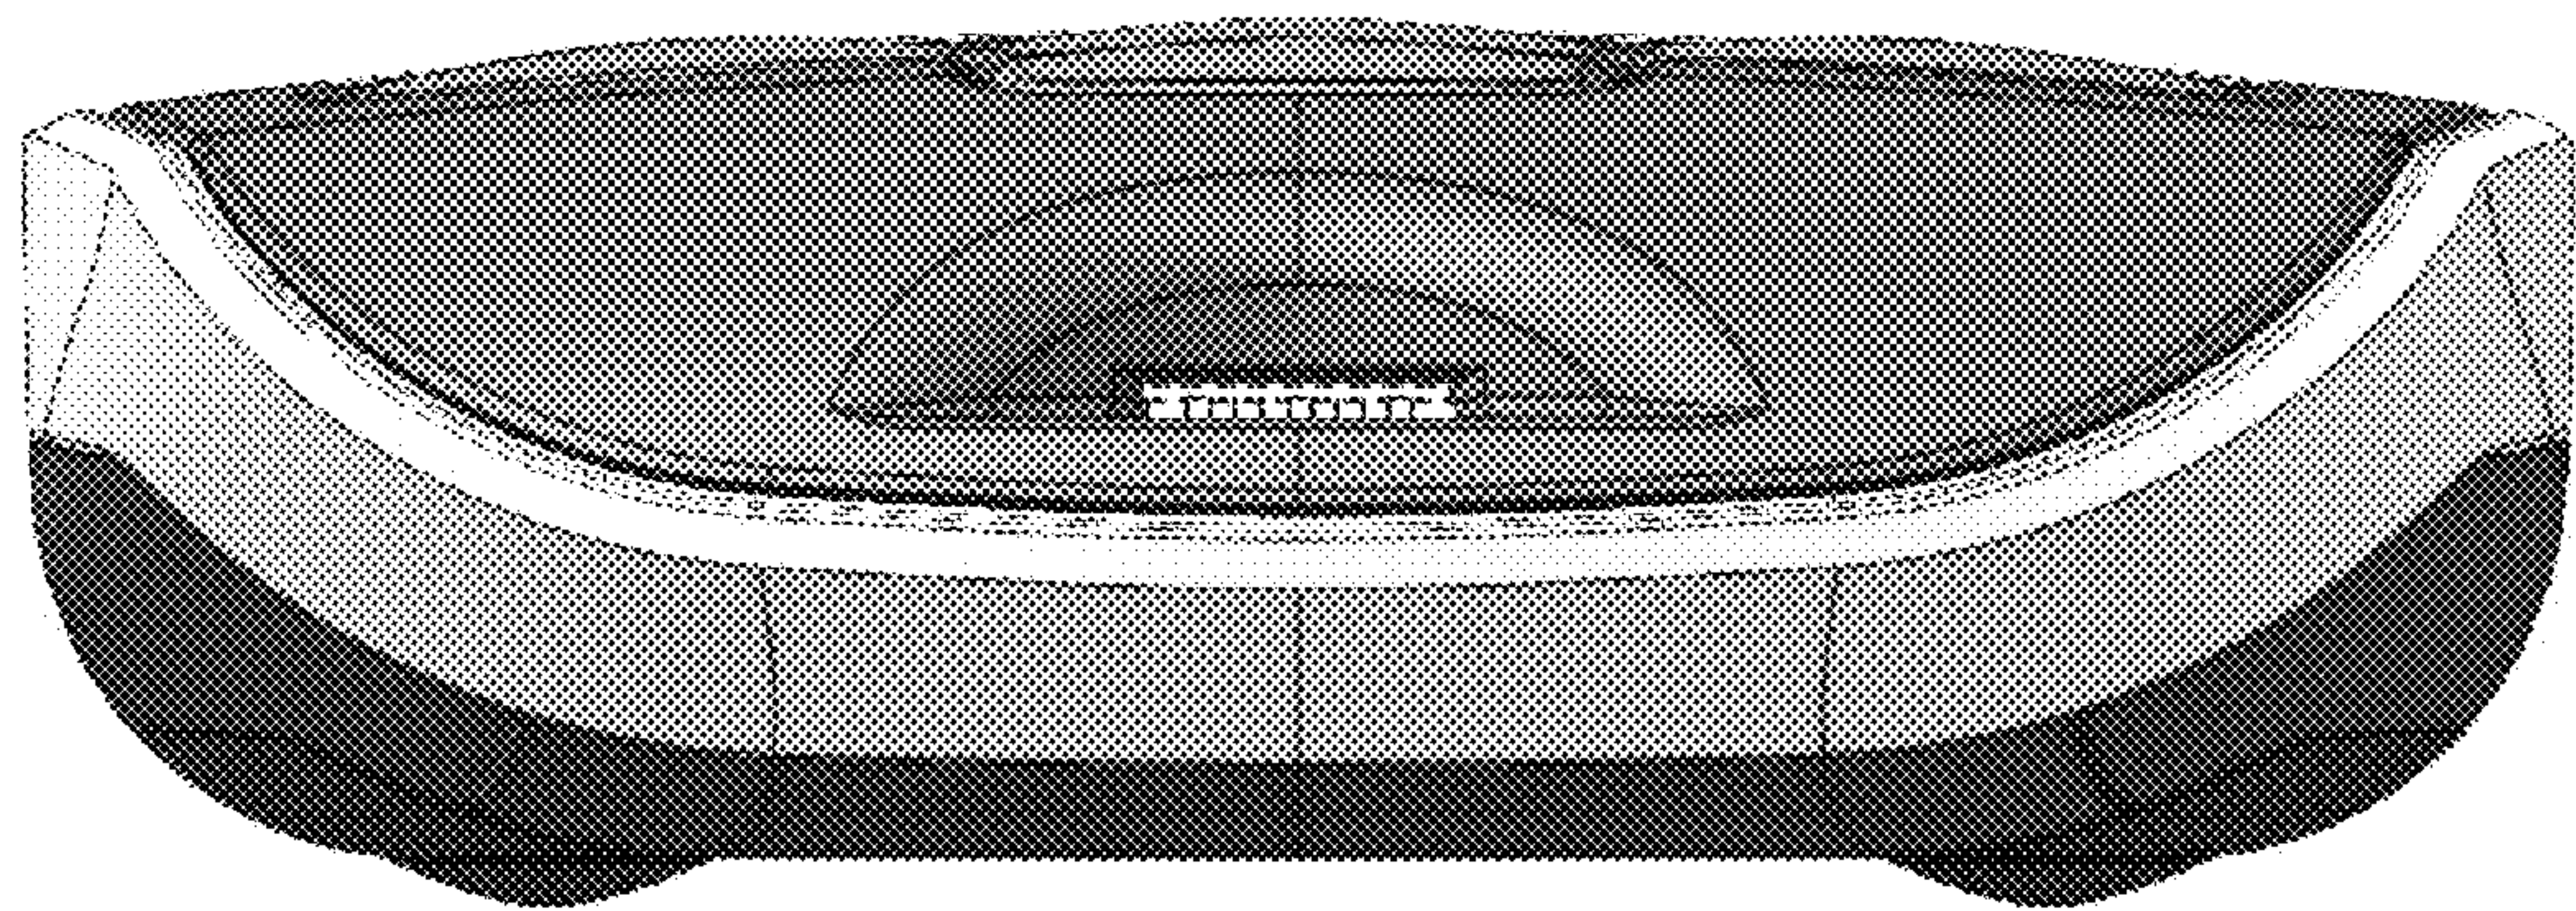


FIG. 9



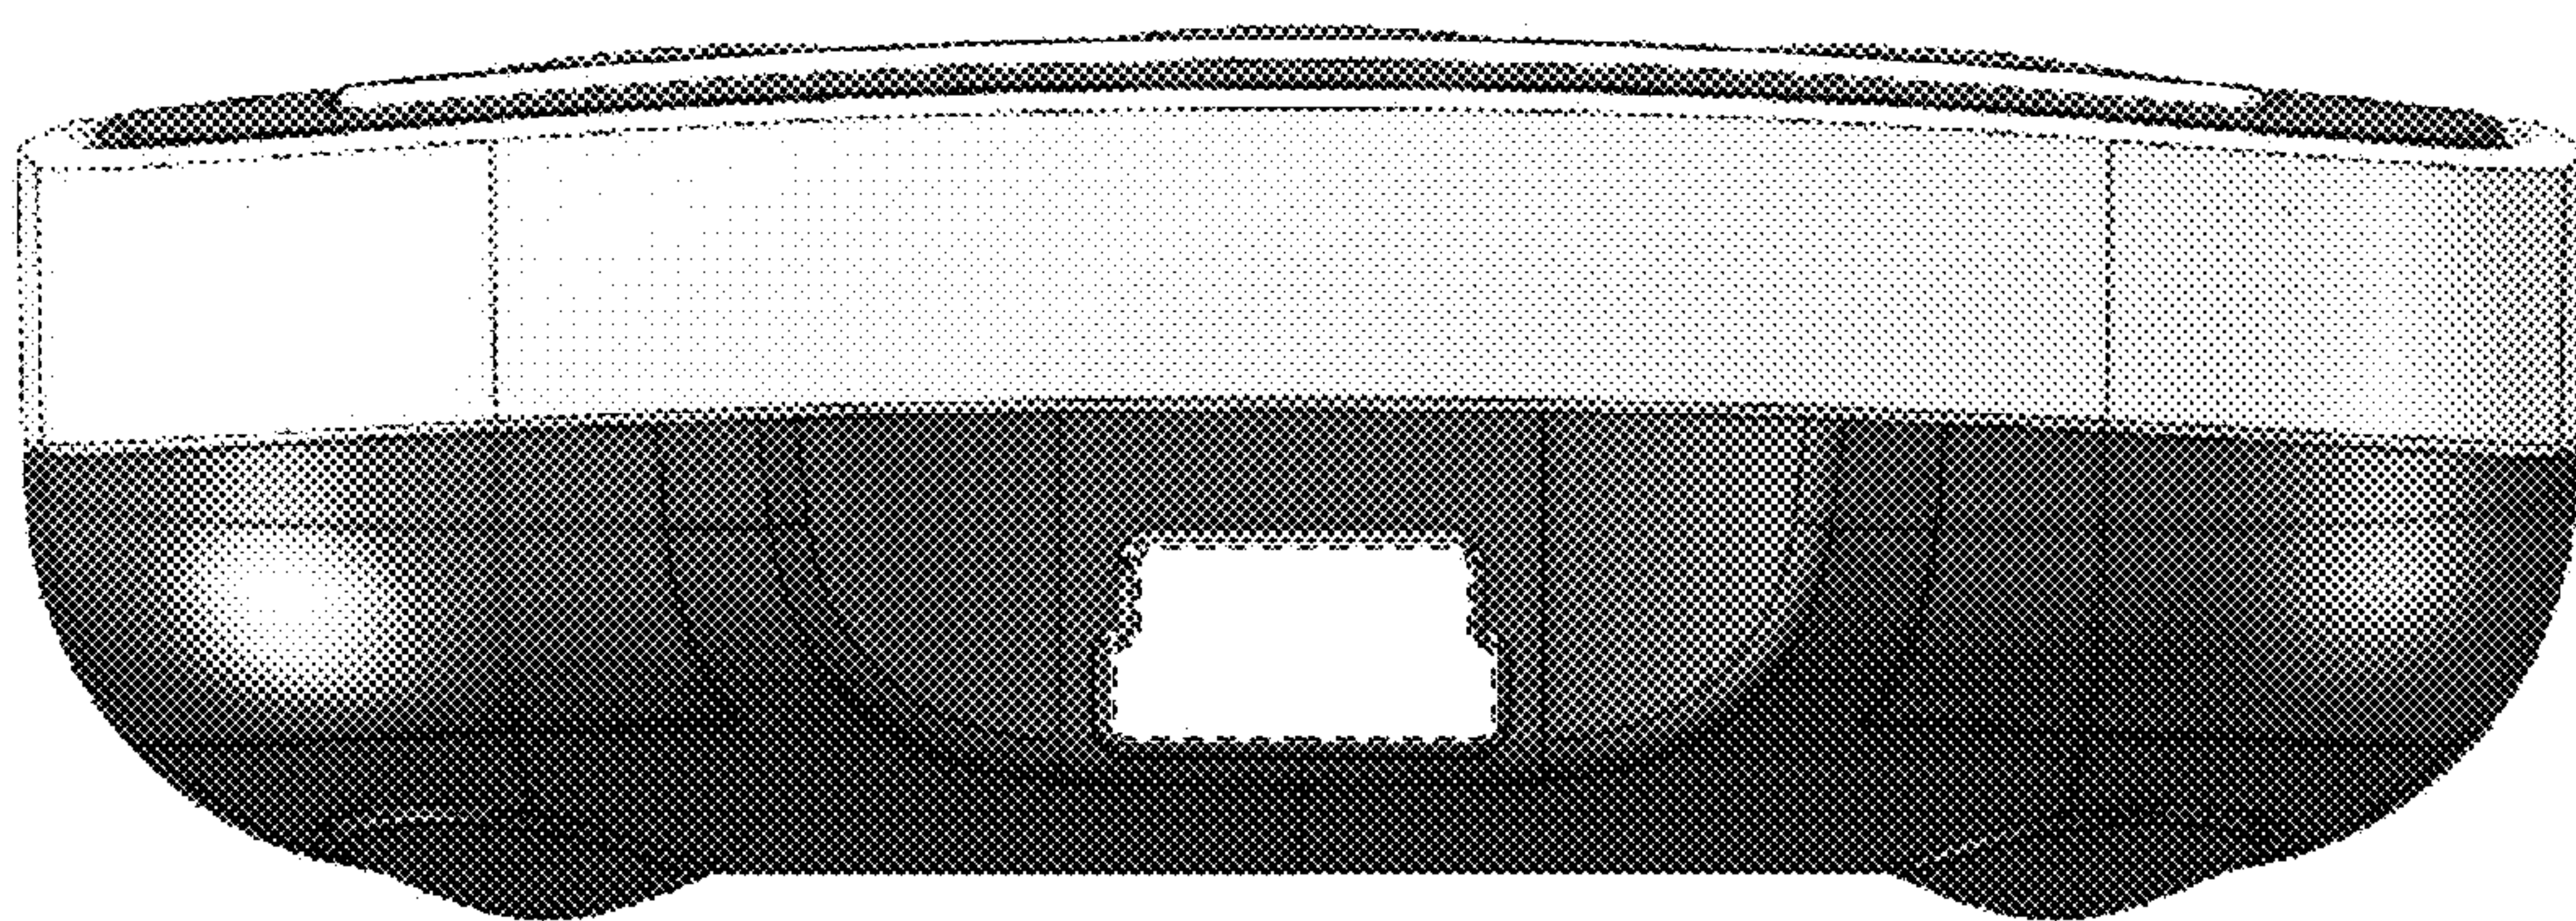


FIG. 10



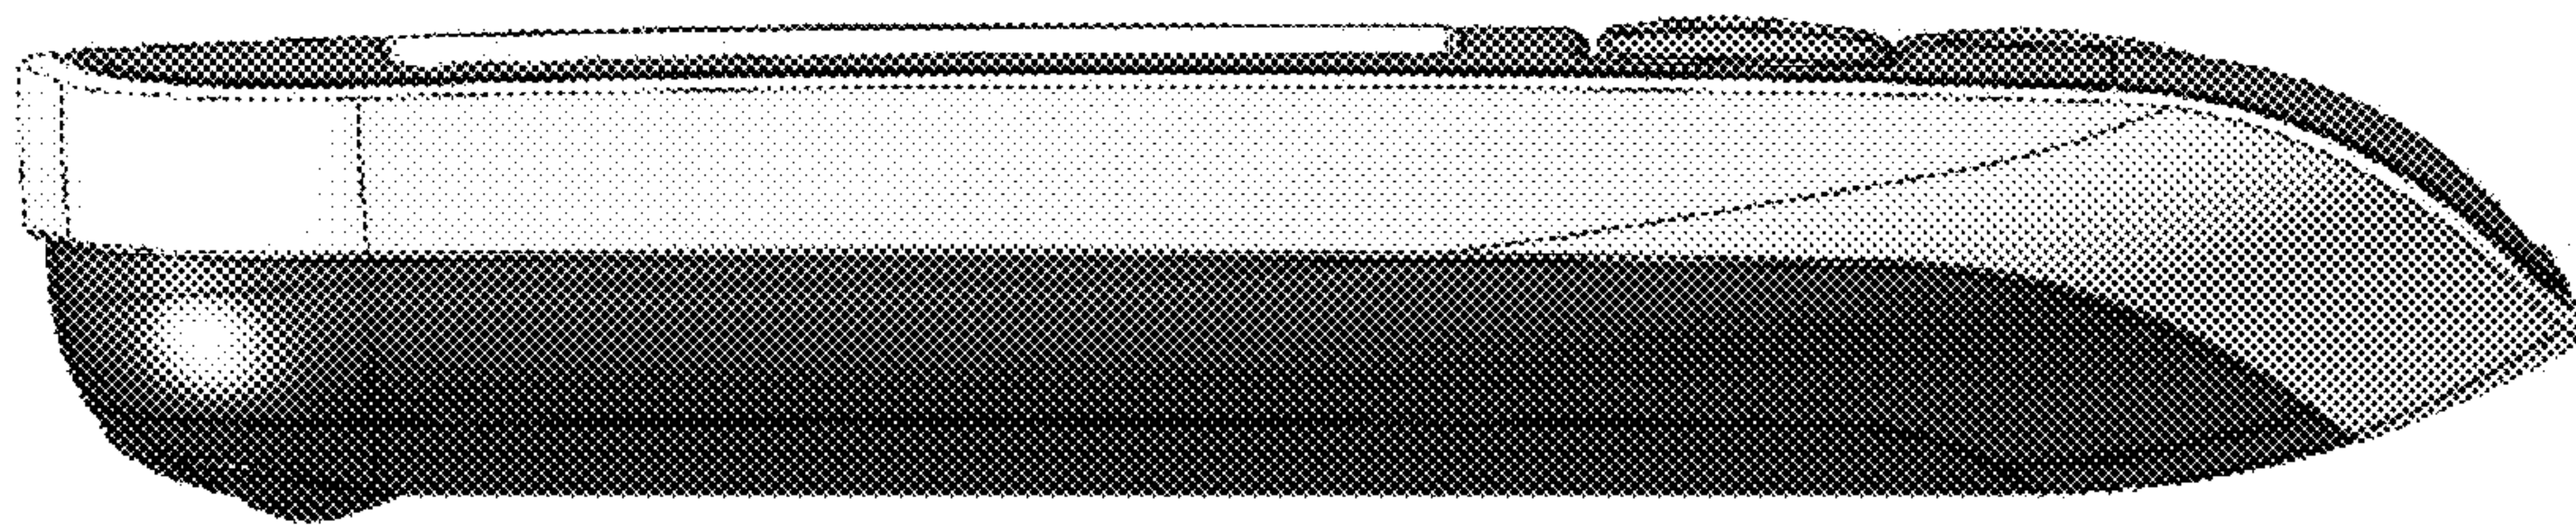


FIG. 11



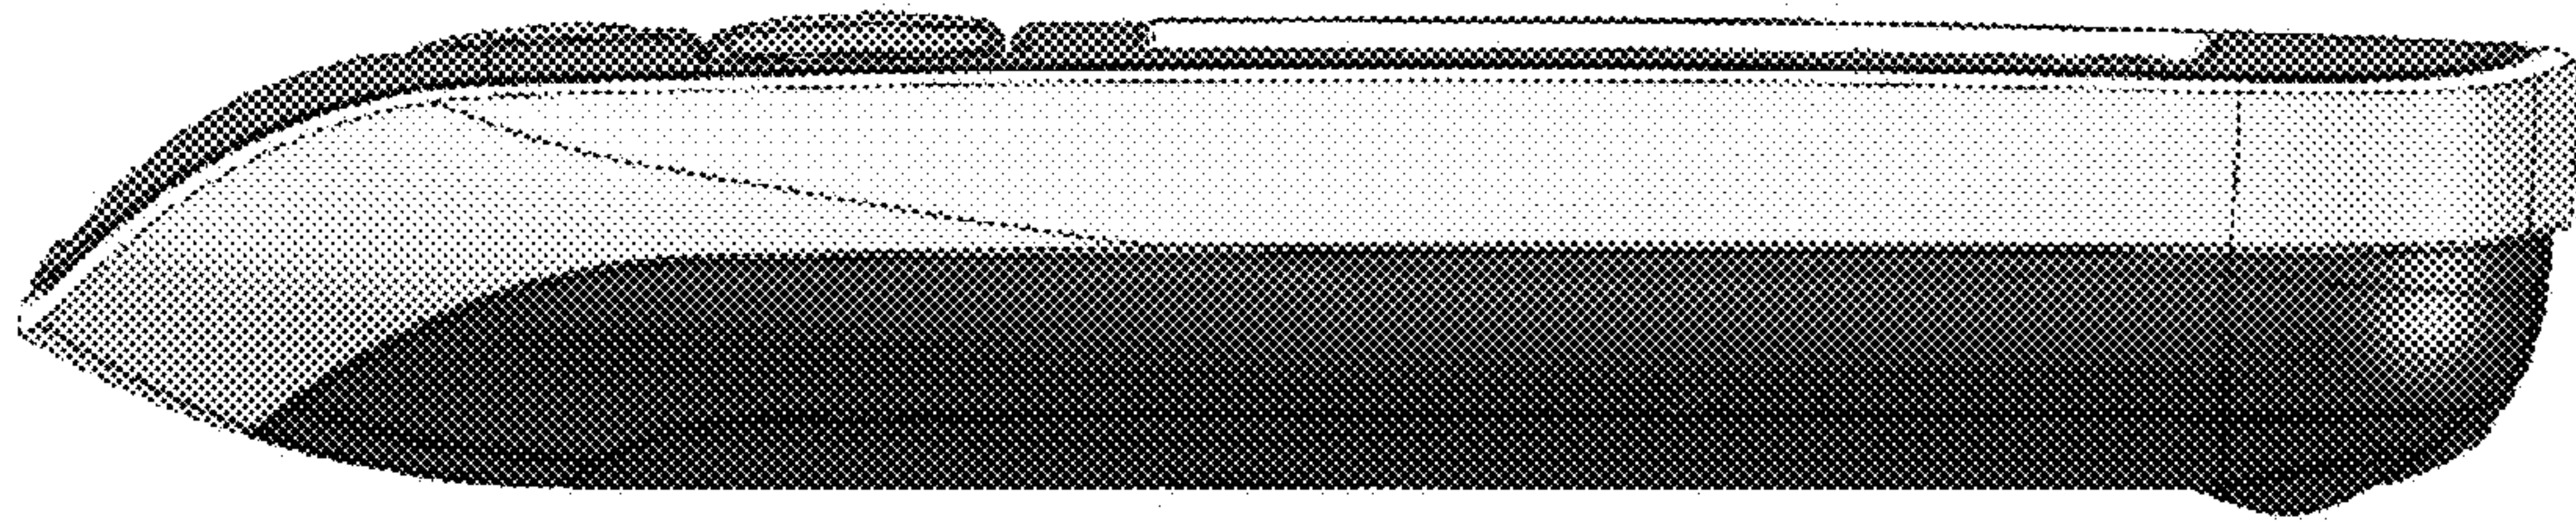


FIG. 12





FIG. 13



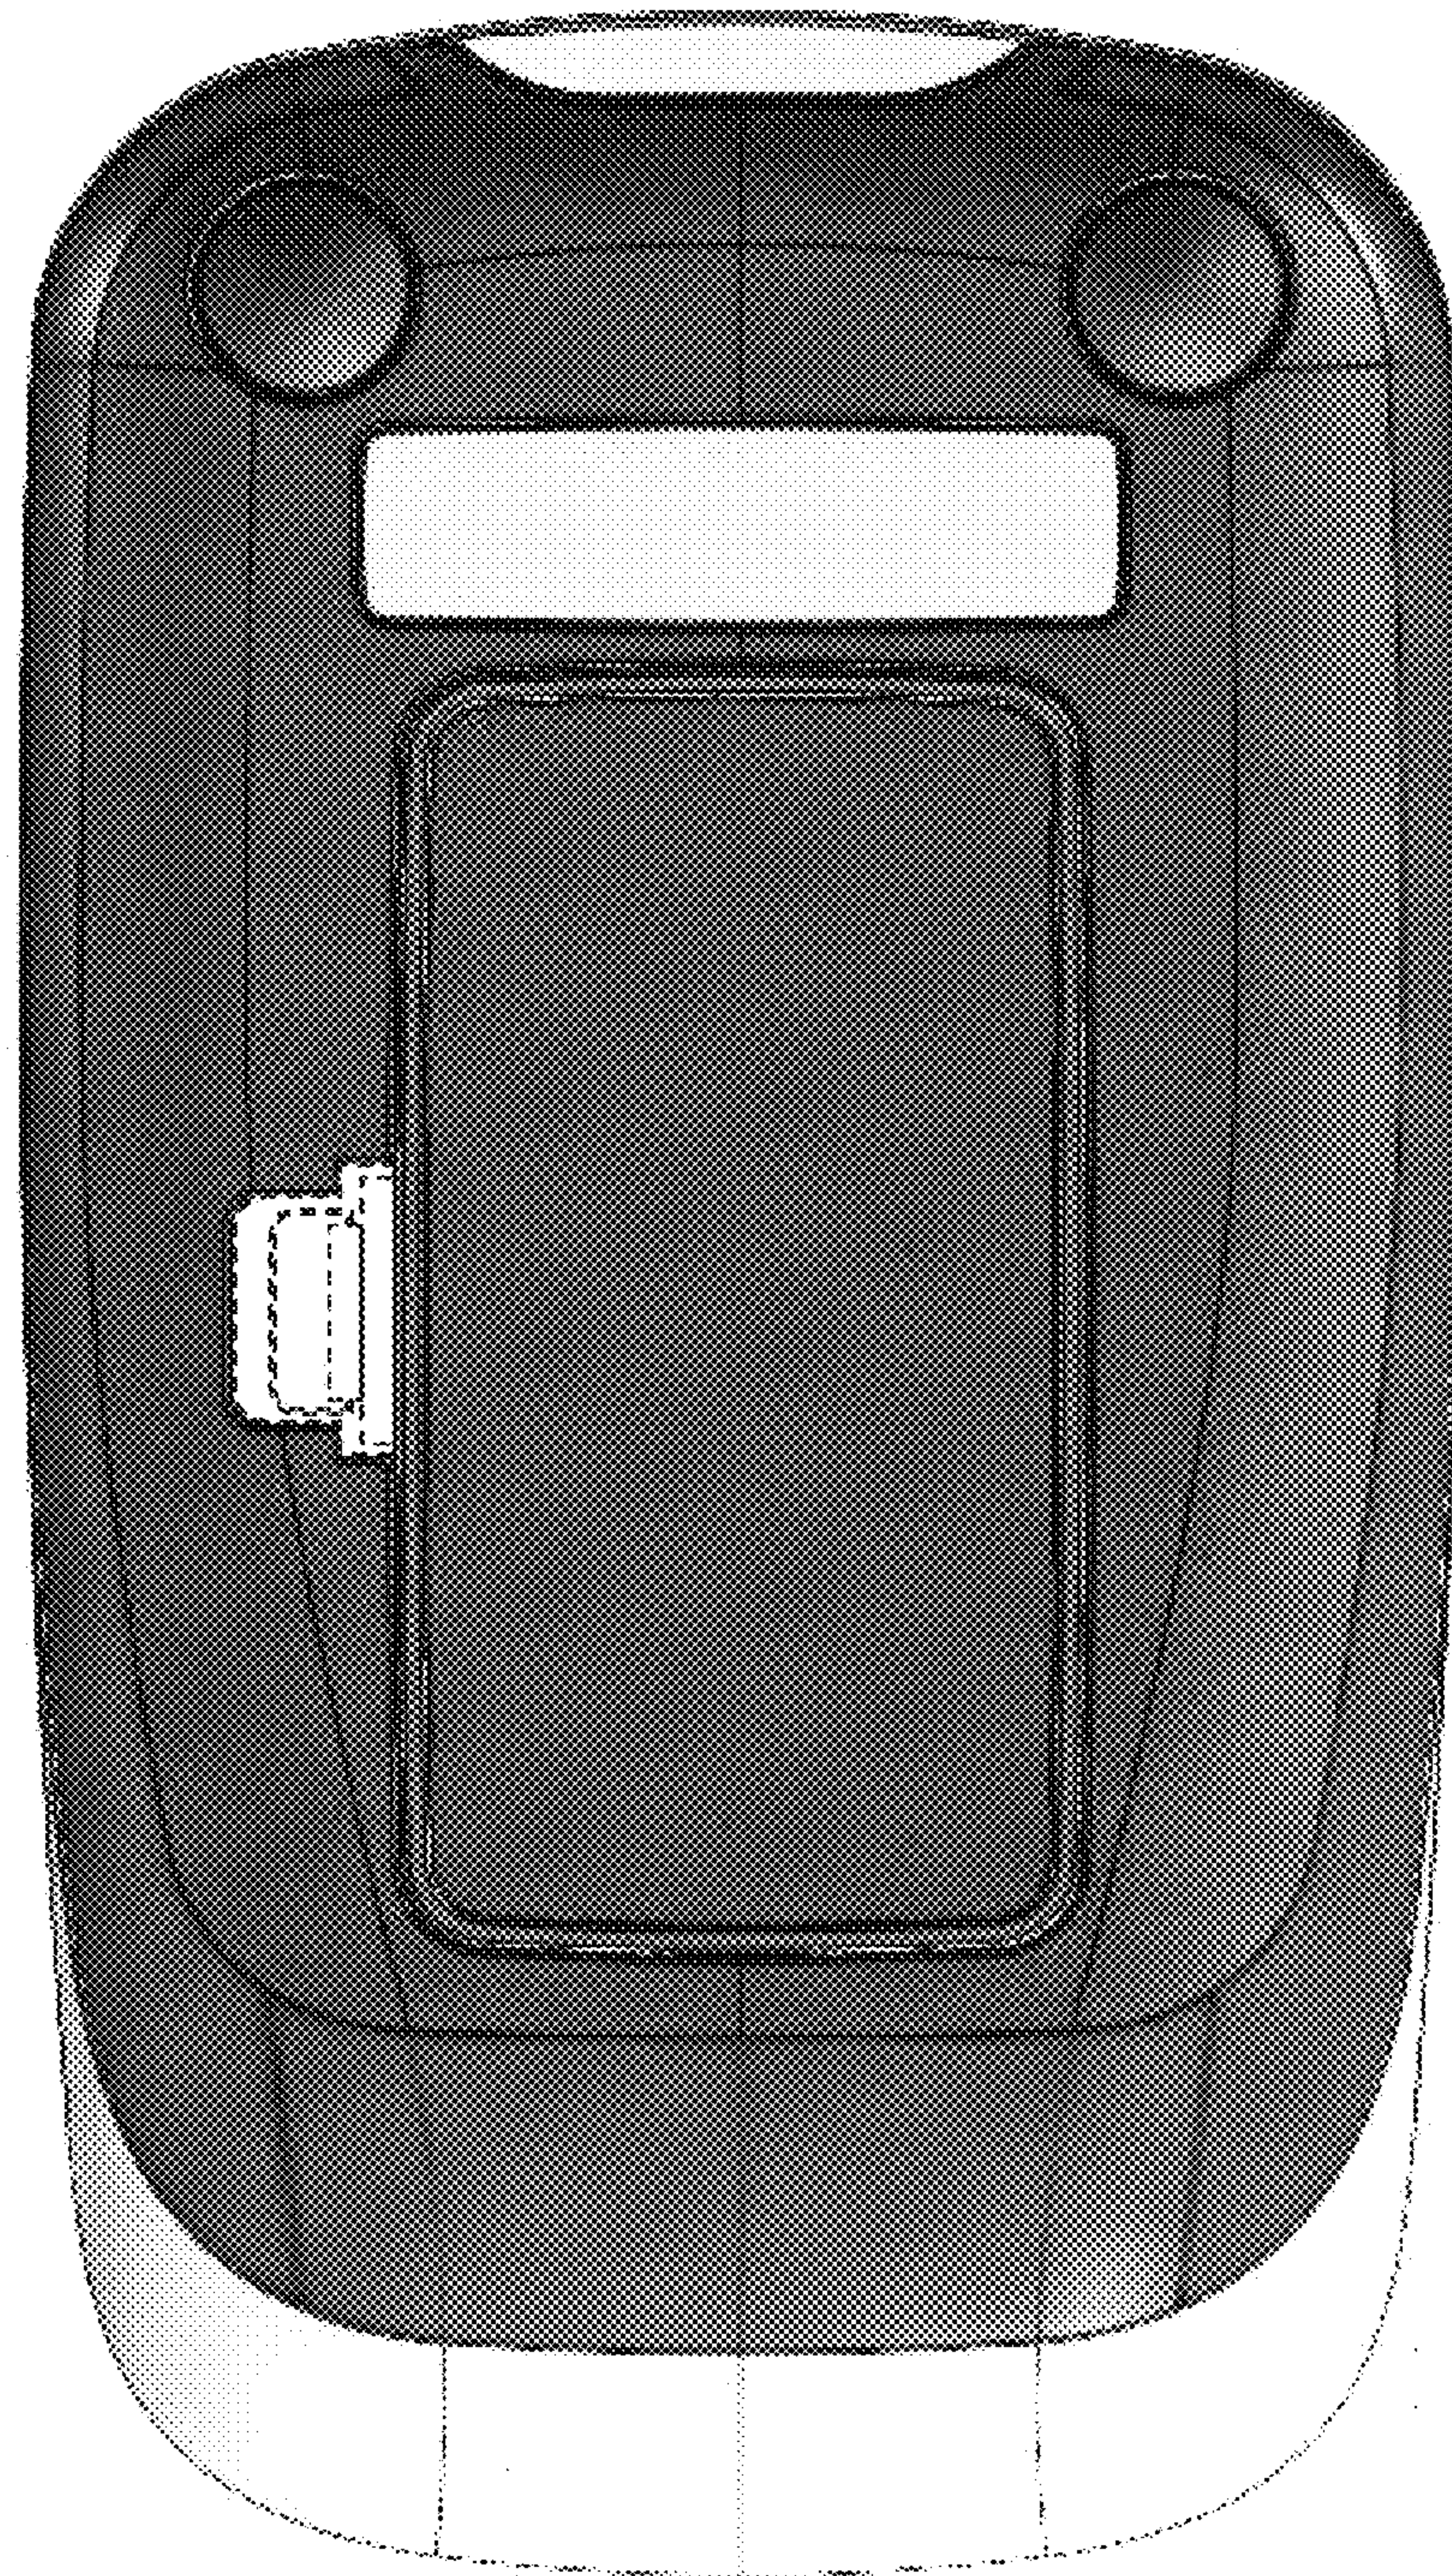


FIG. 14



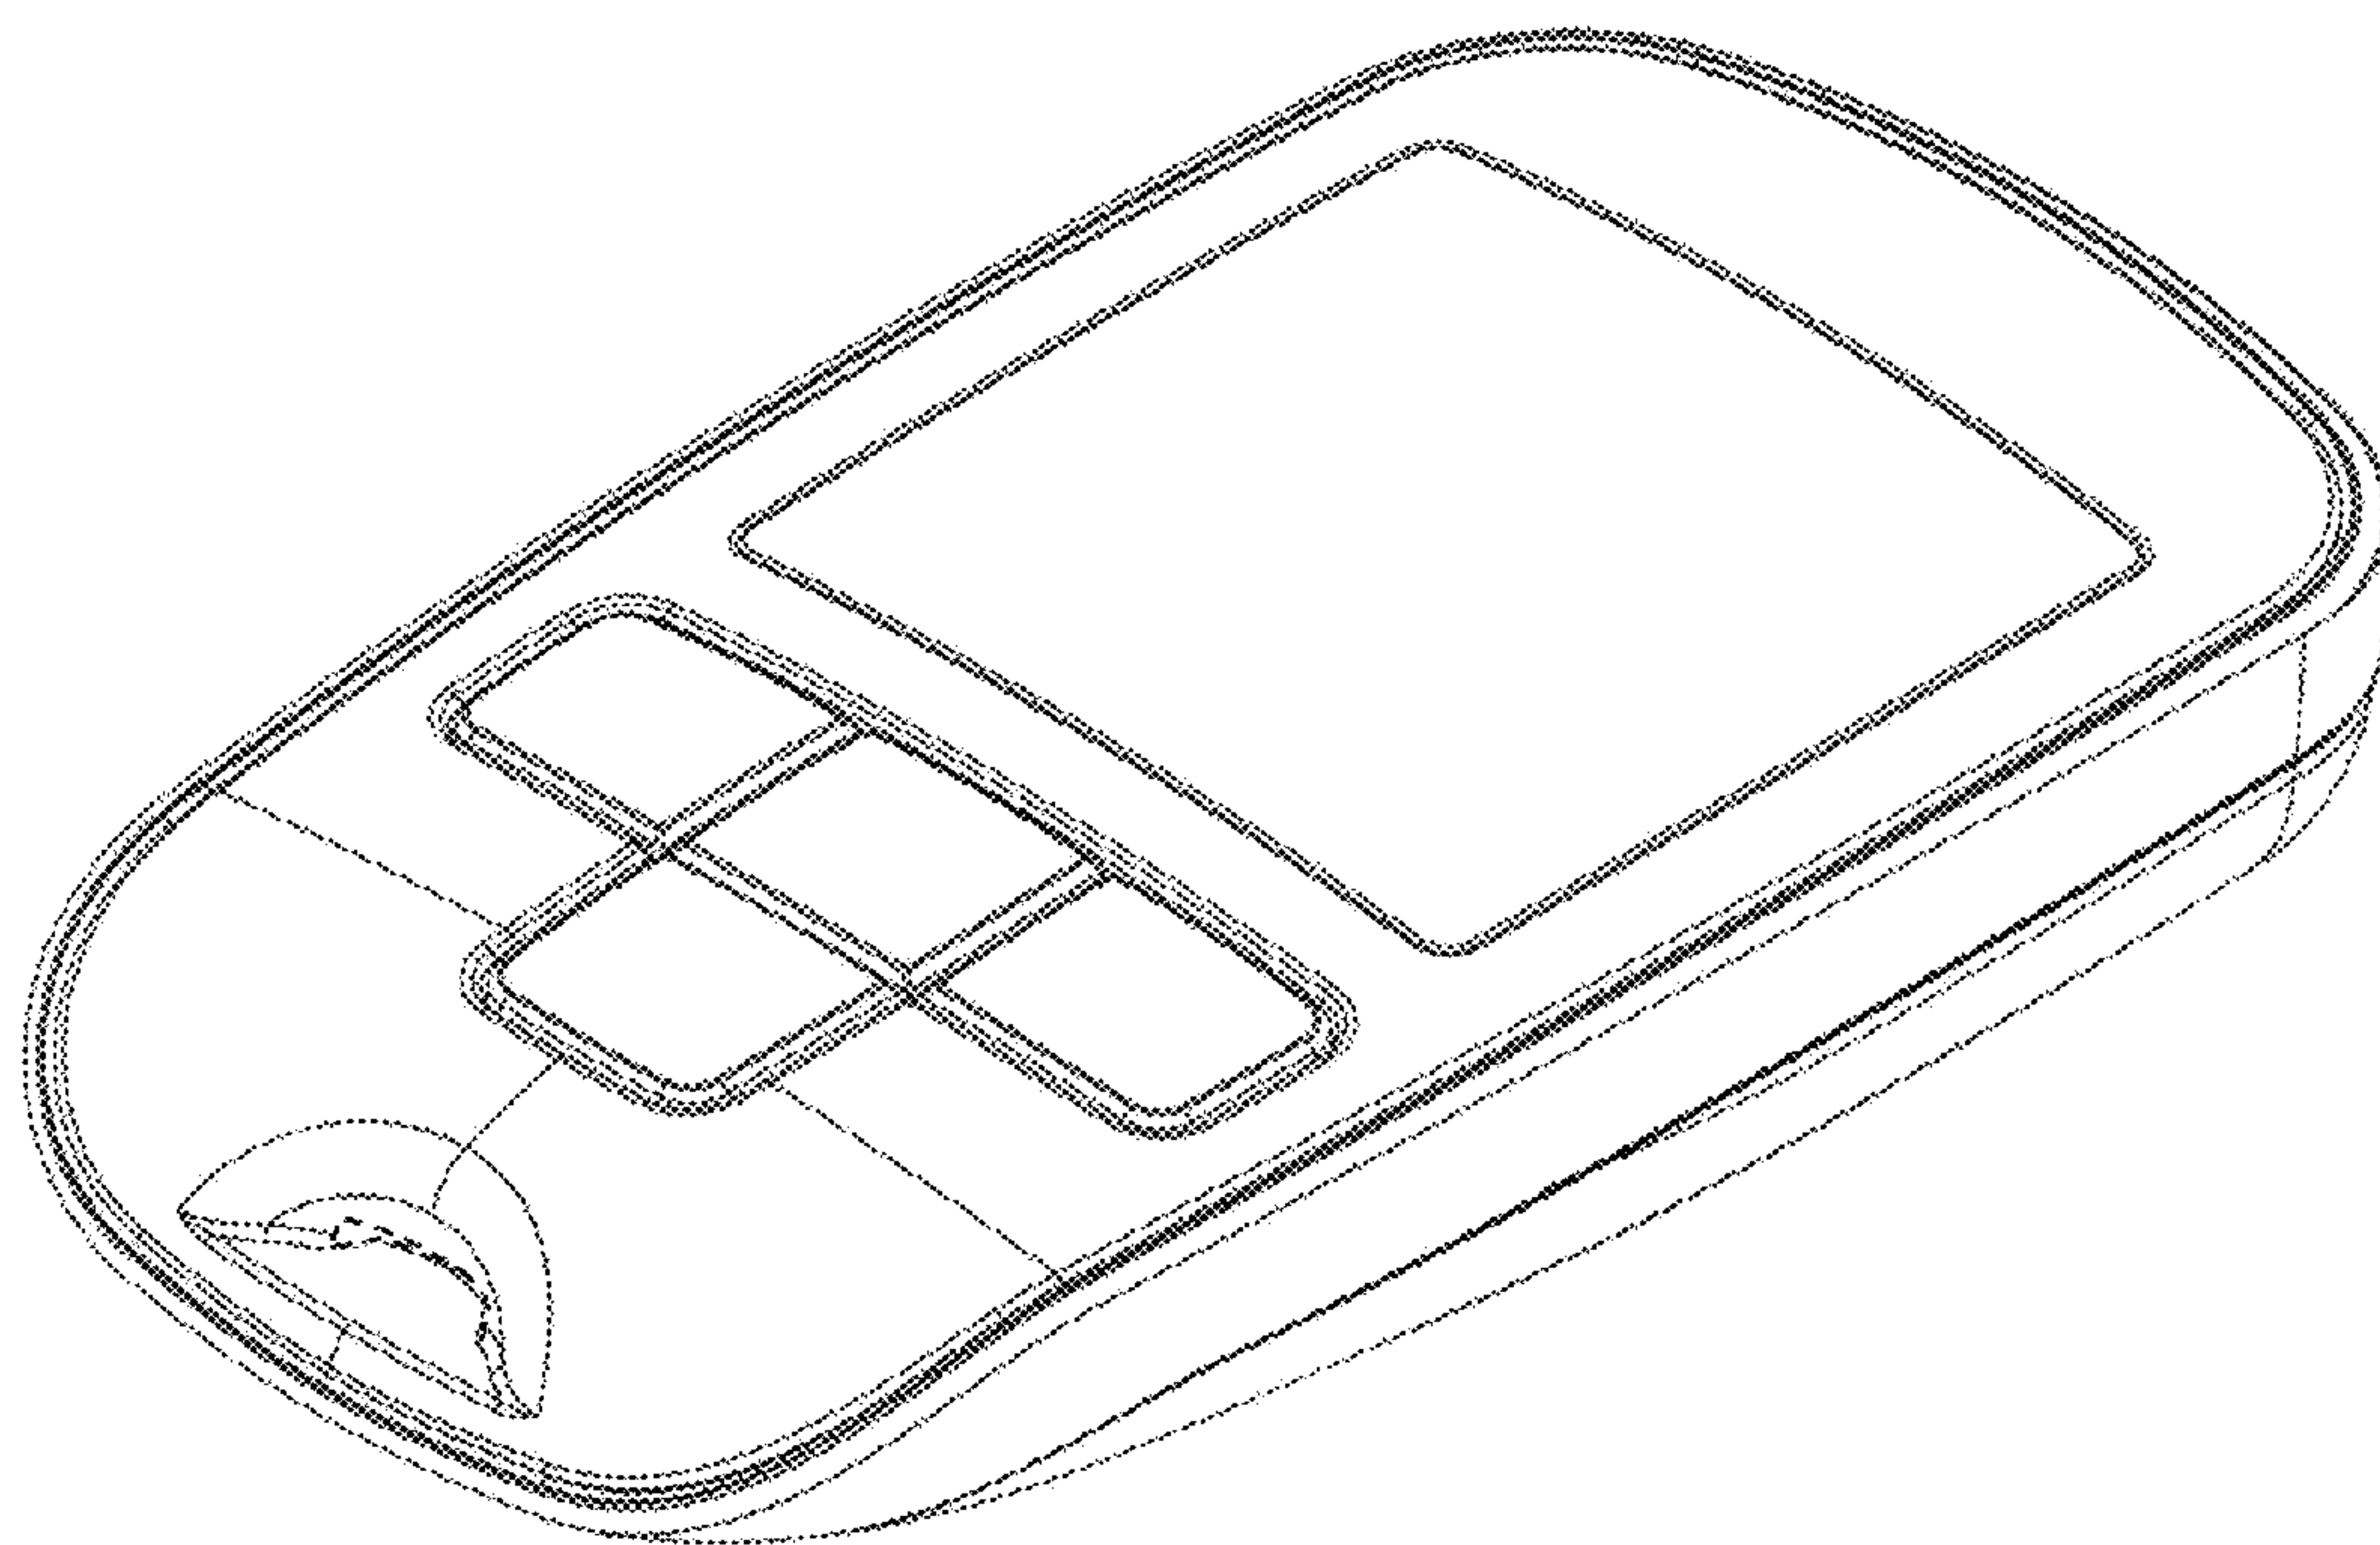


FIG. 15



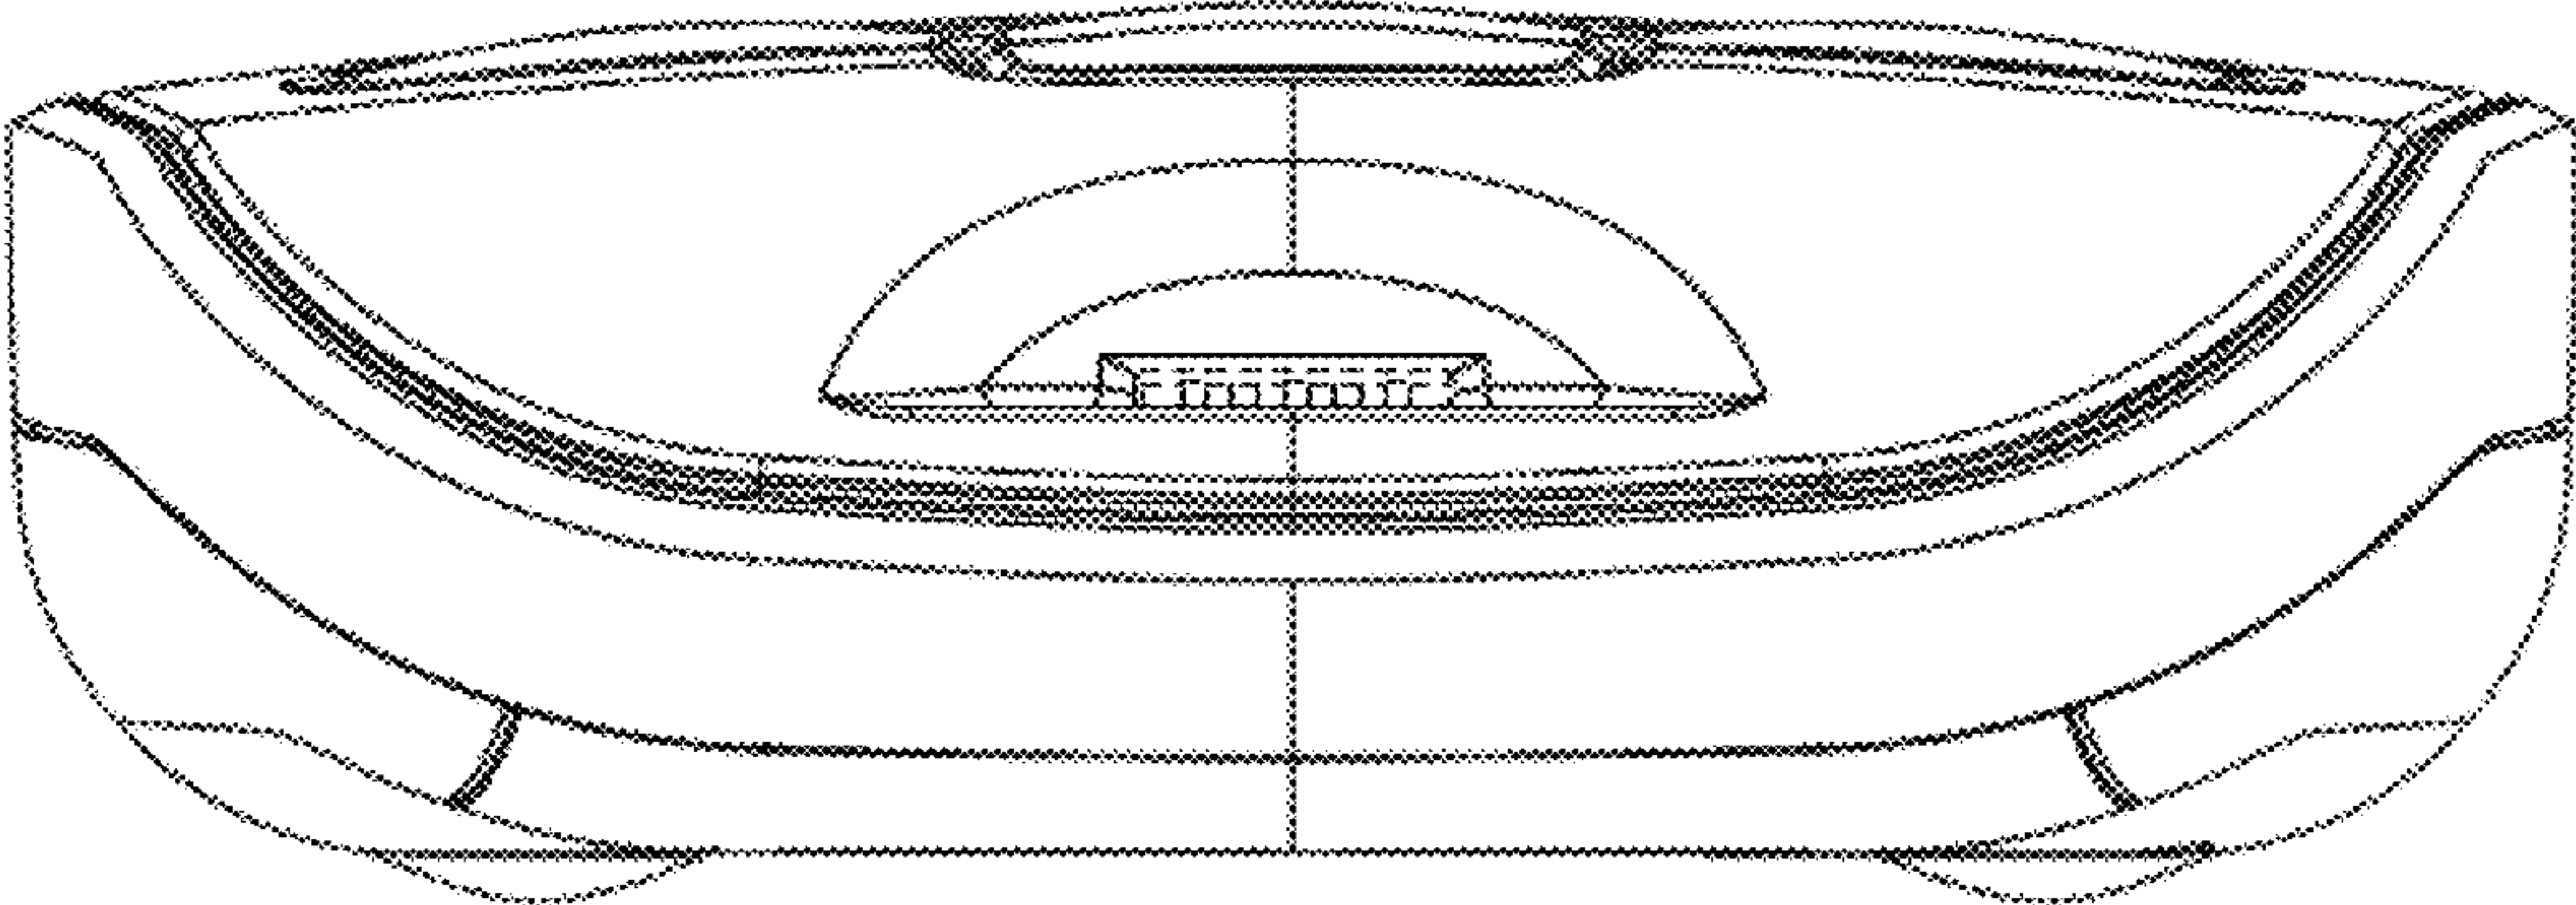


FIG. 16



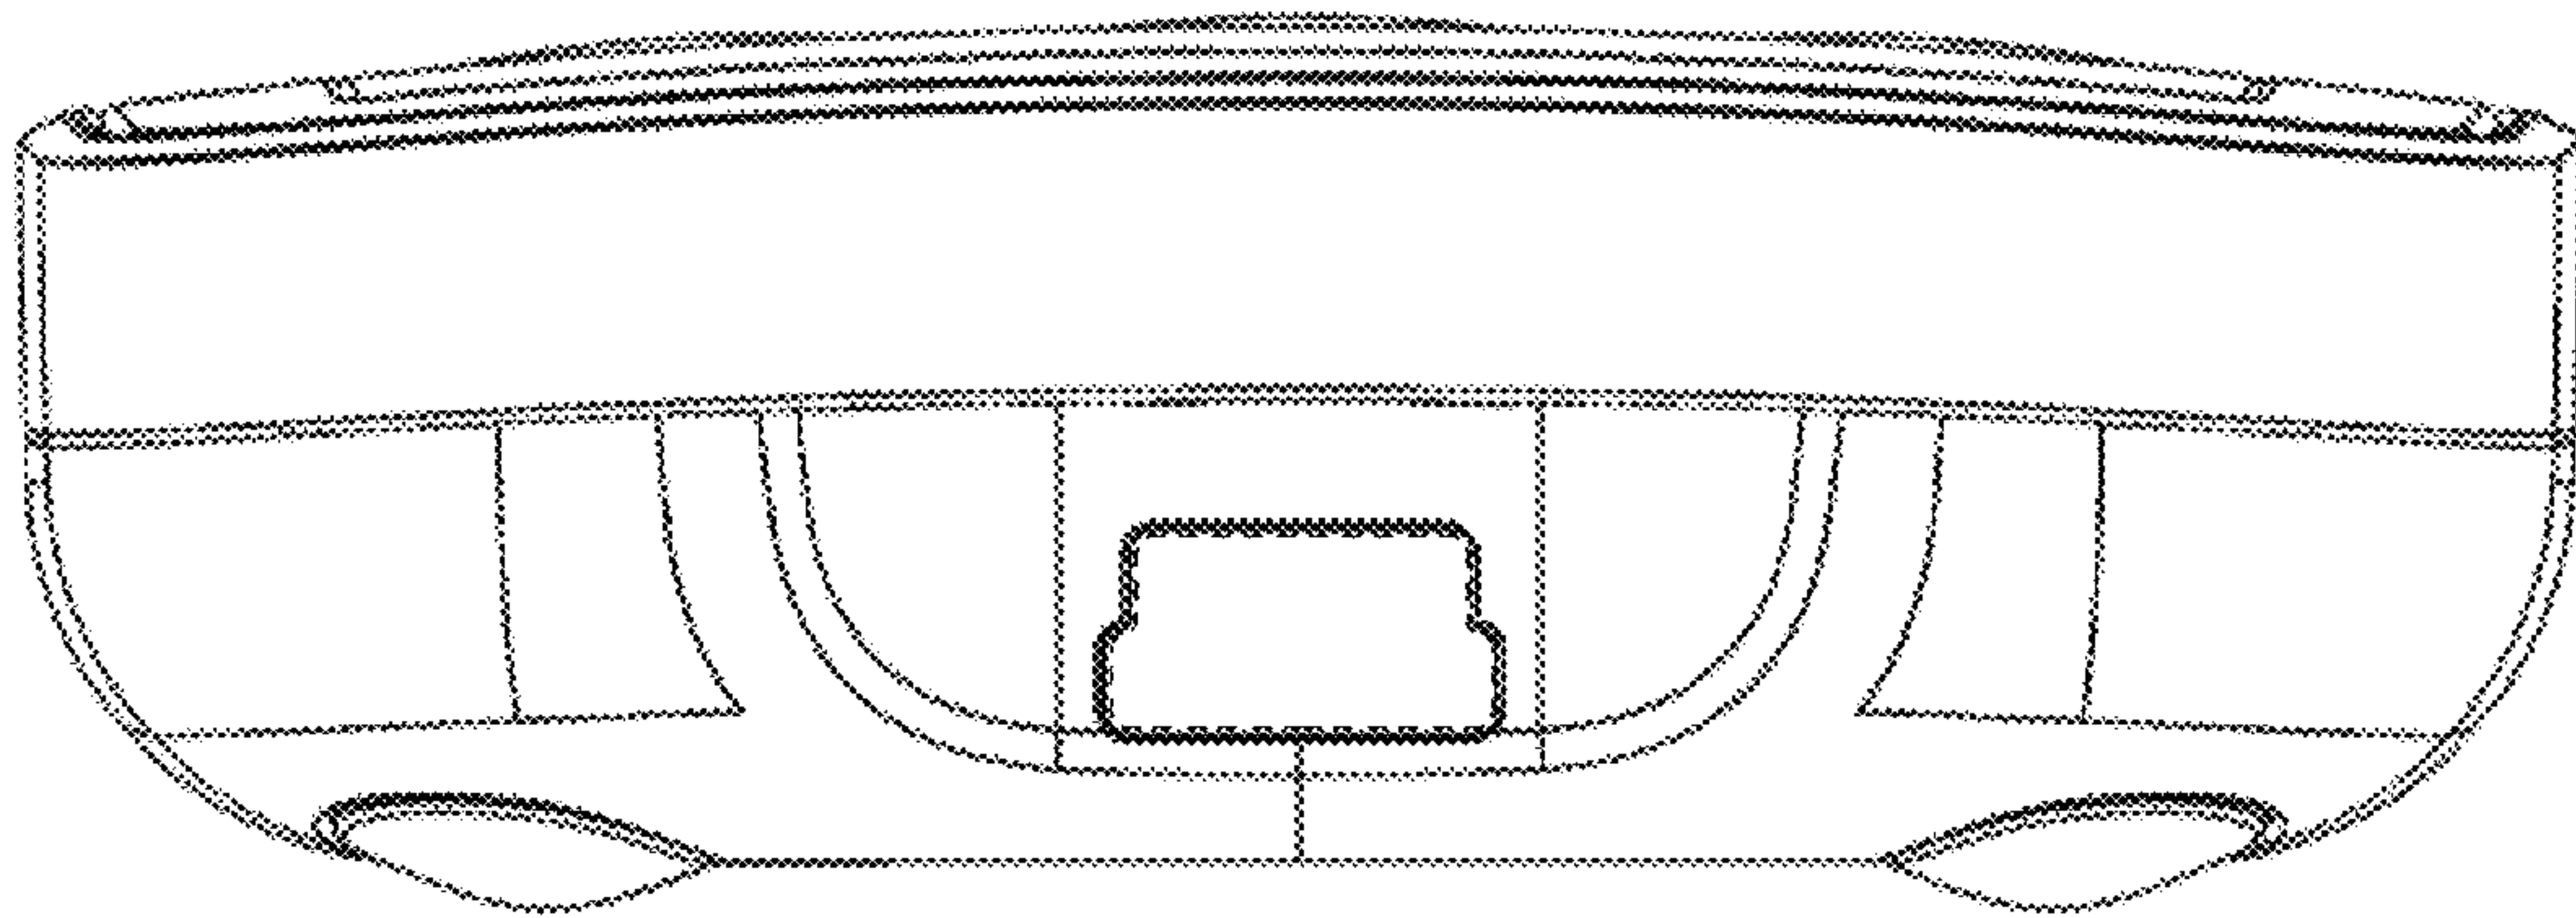


FIG. 17

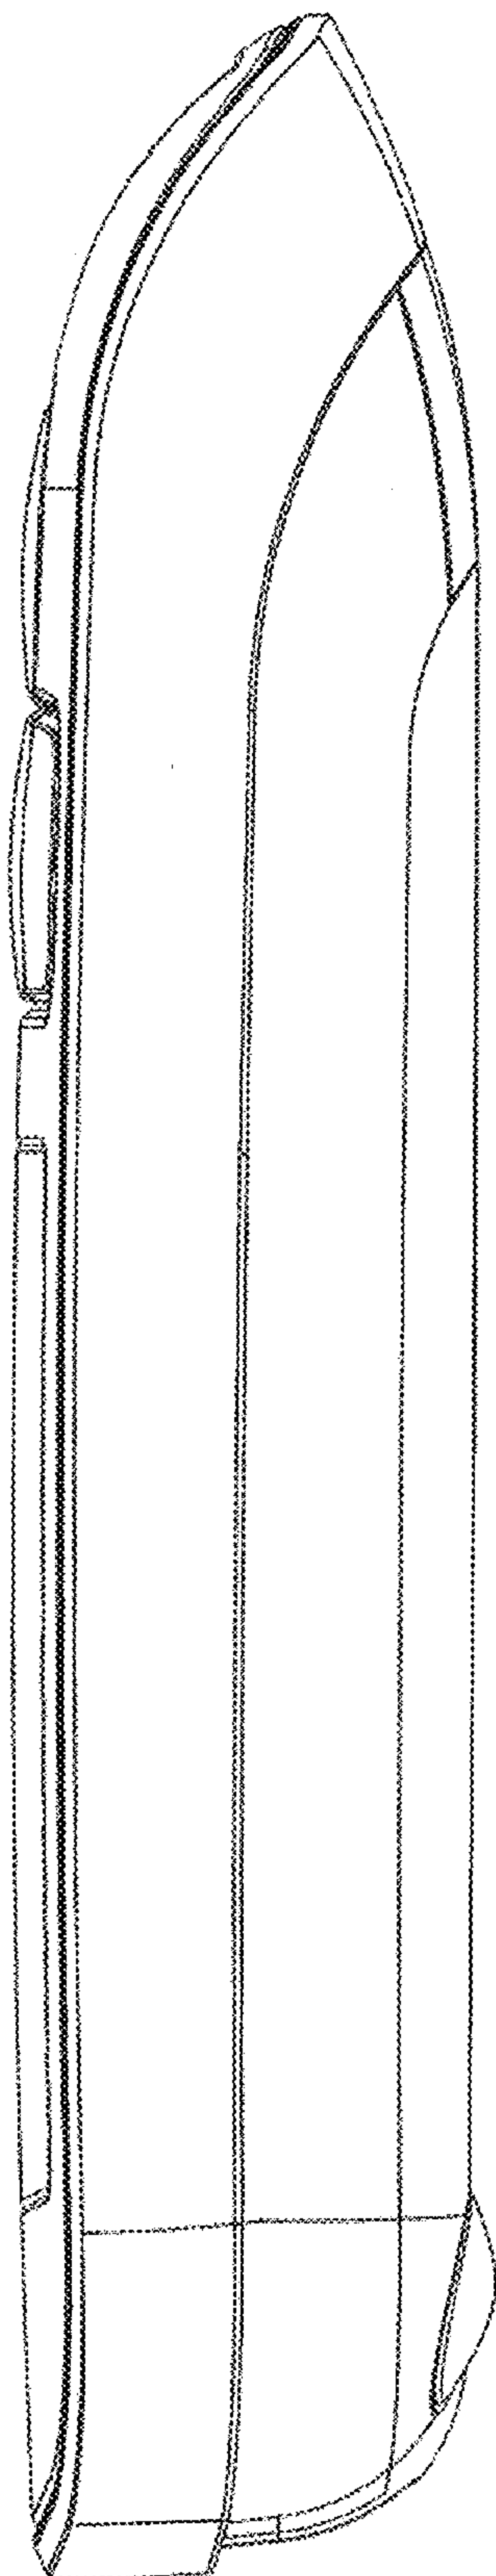


FIG. 18



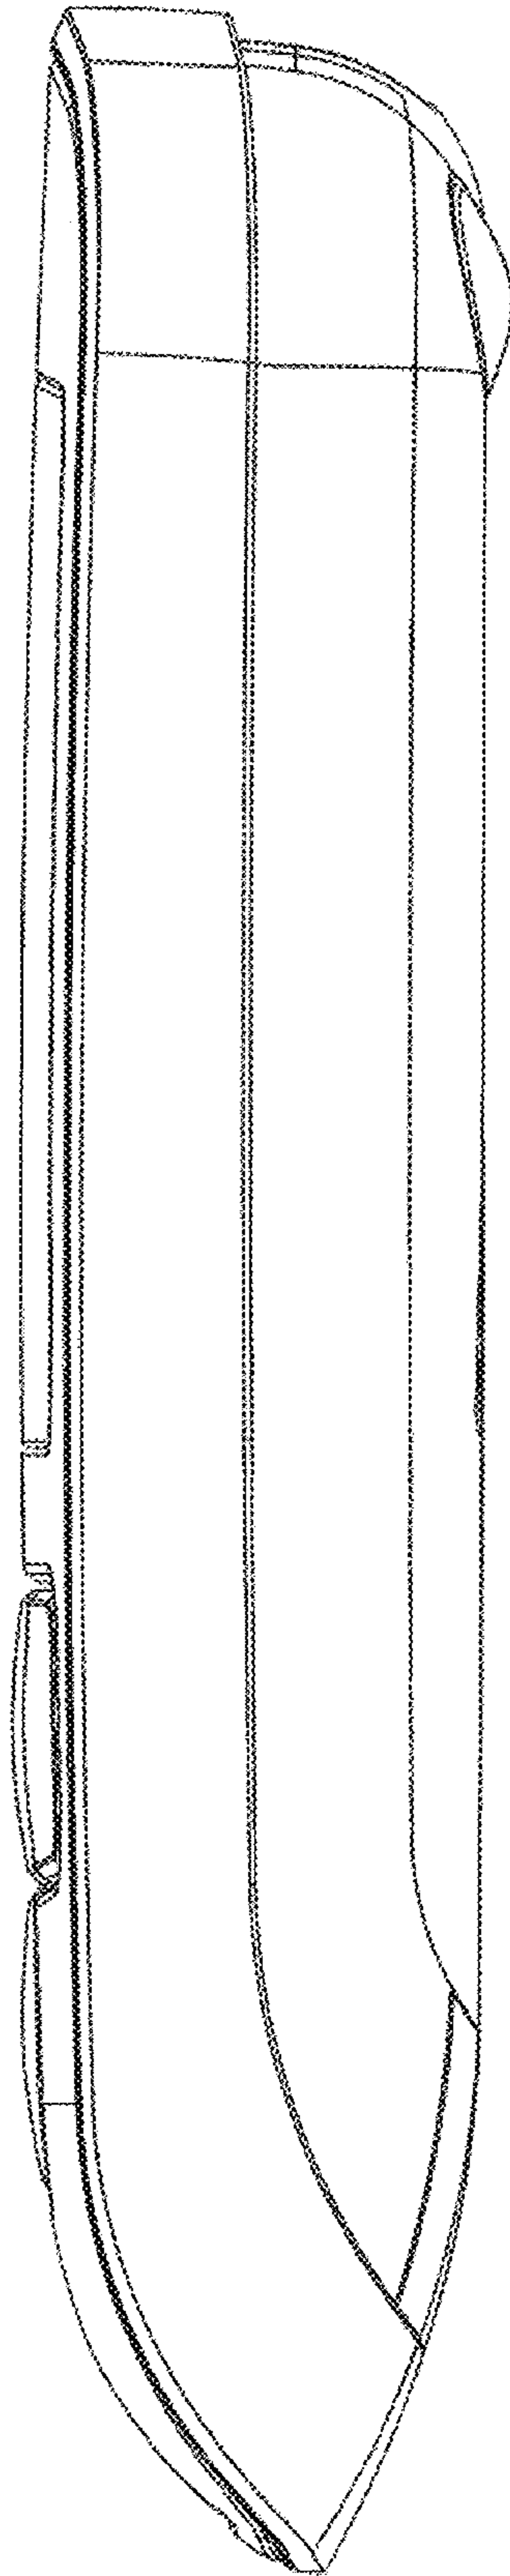


FIG. 19



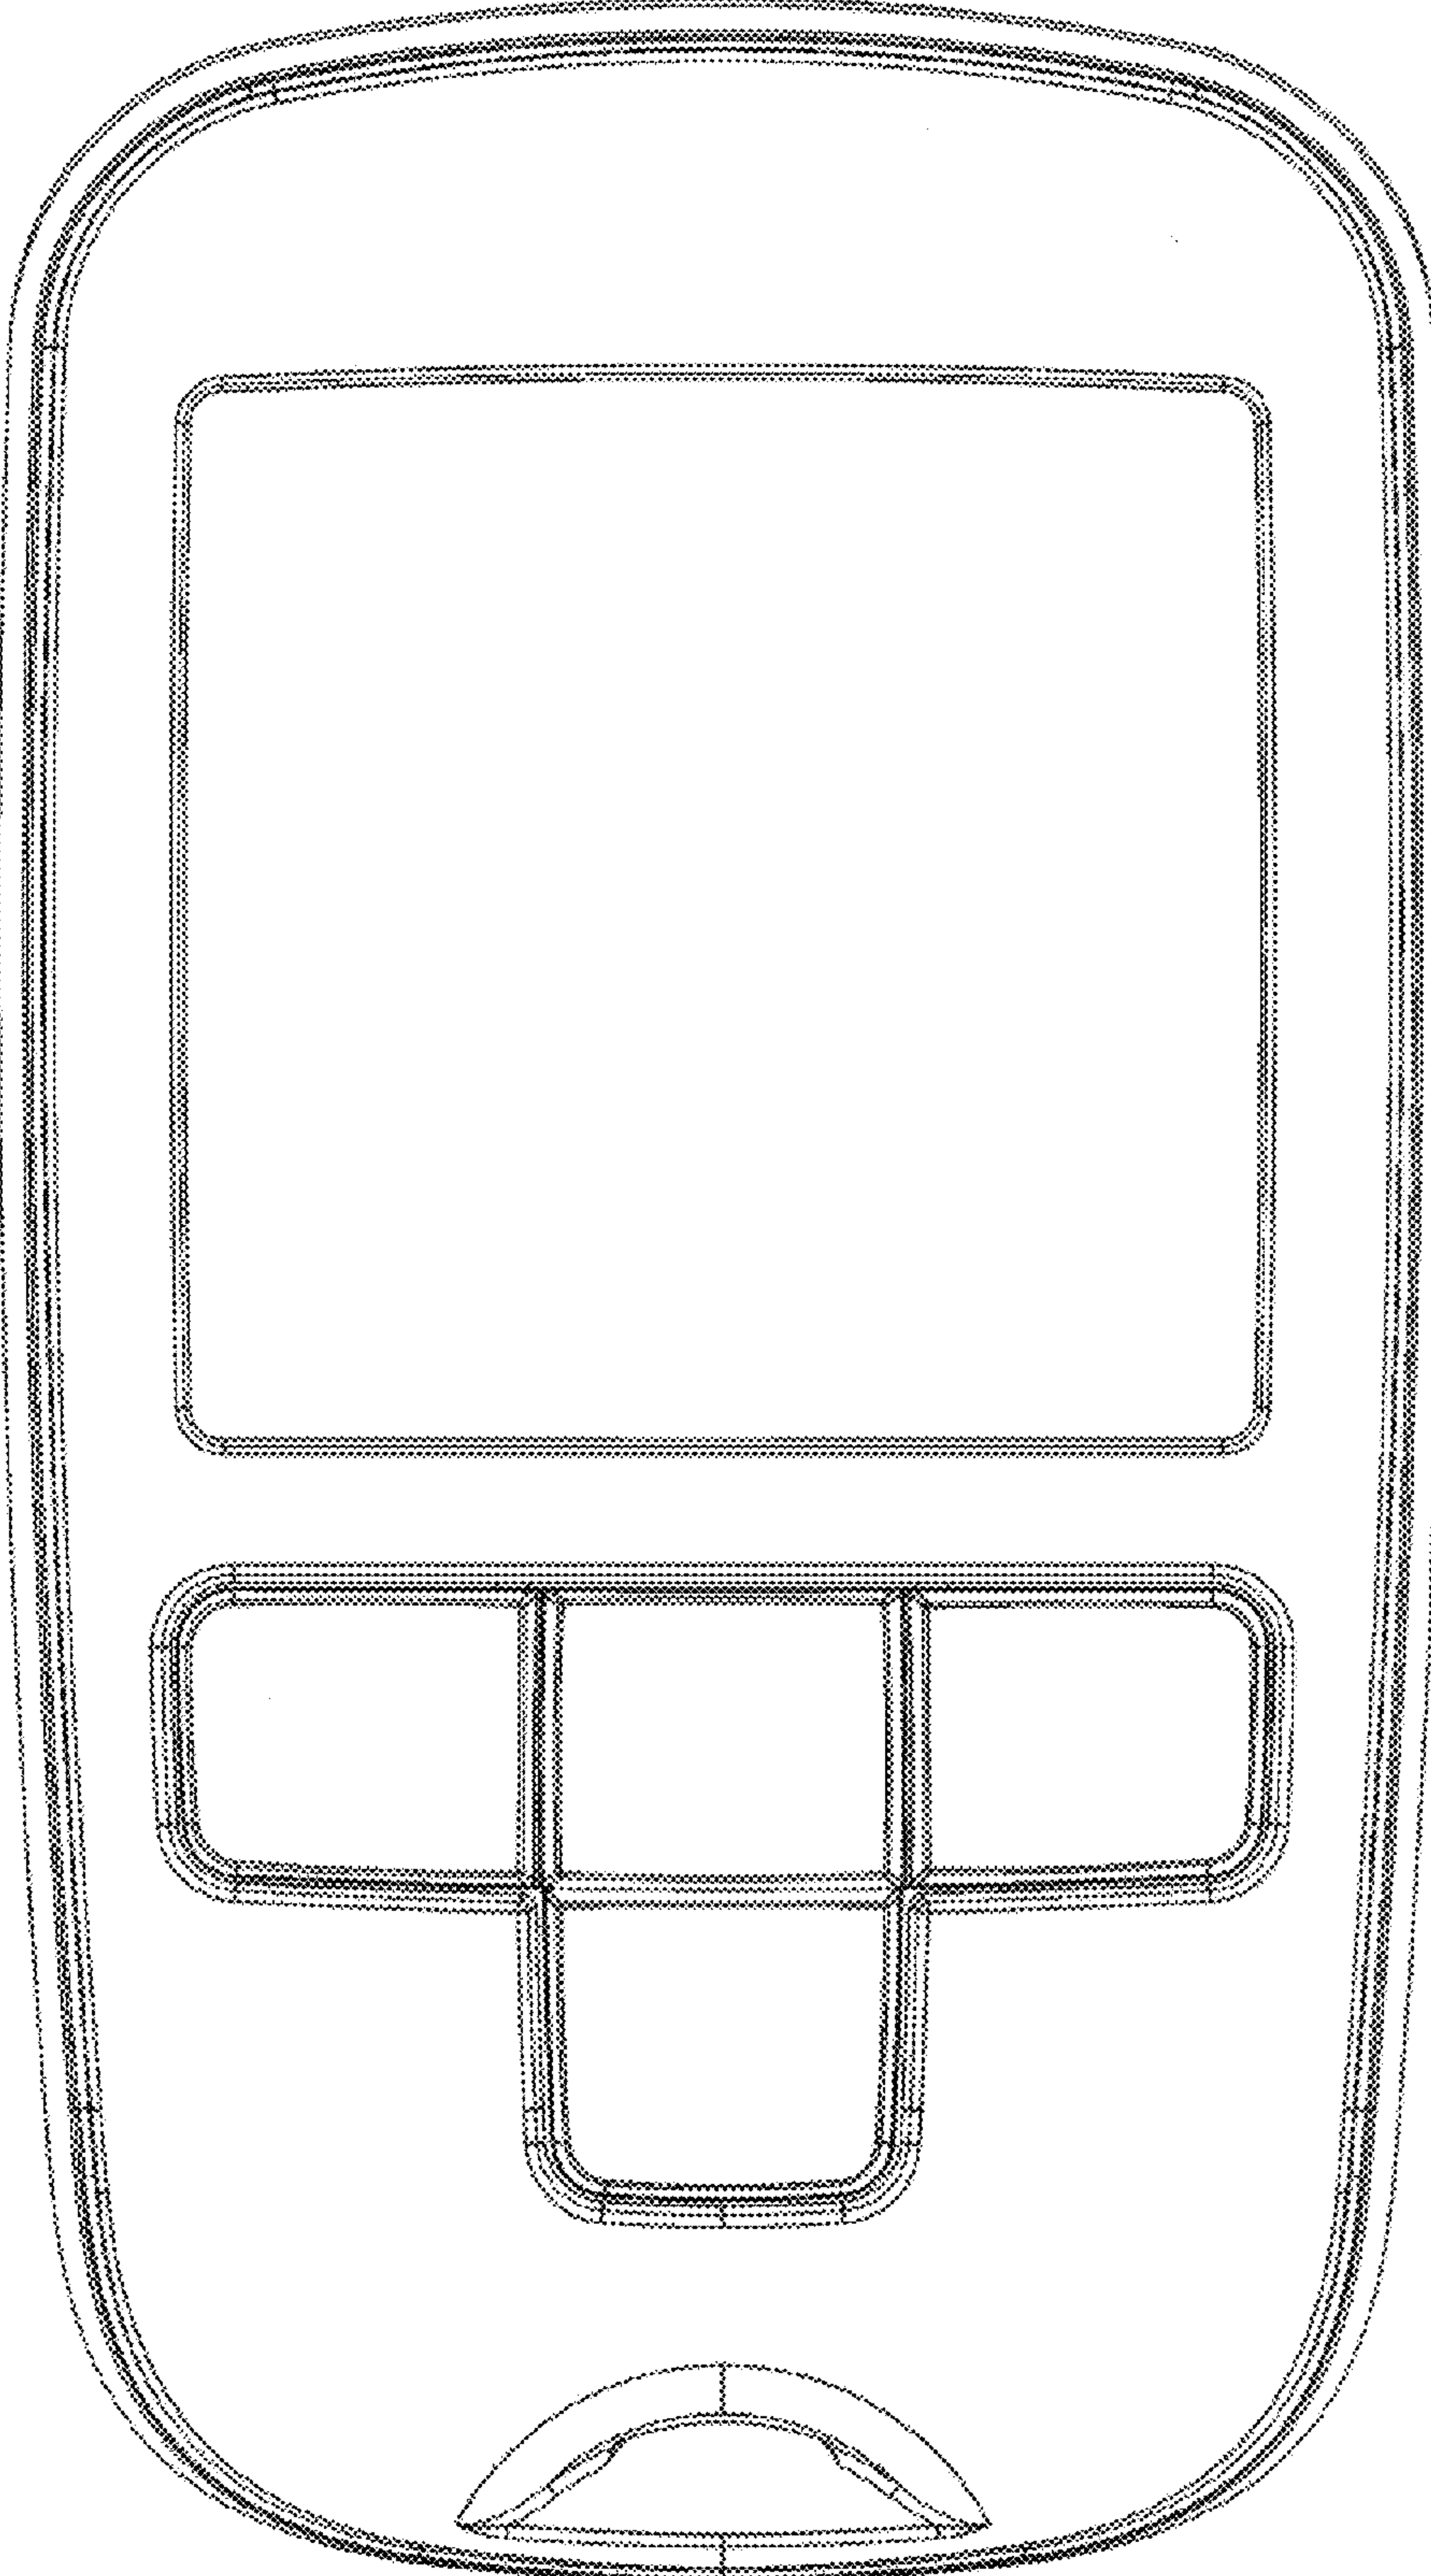


FIG. 20



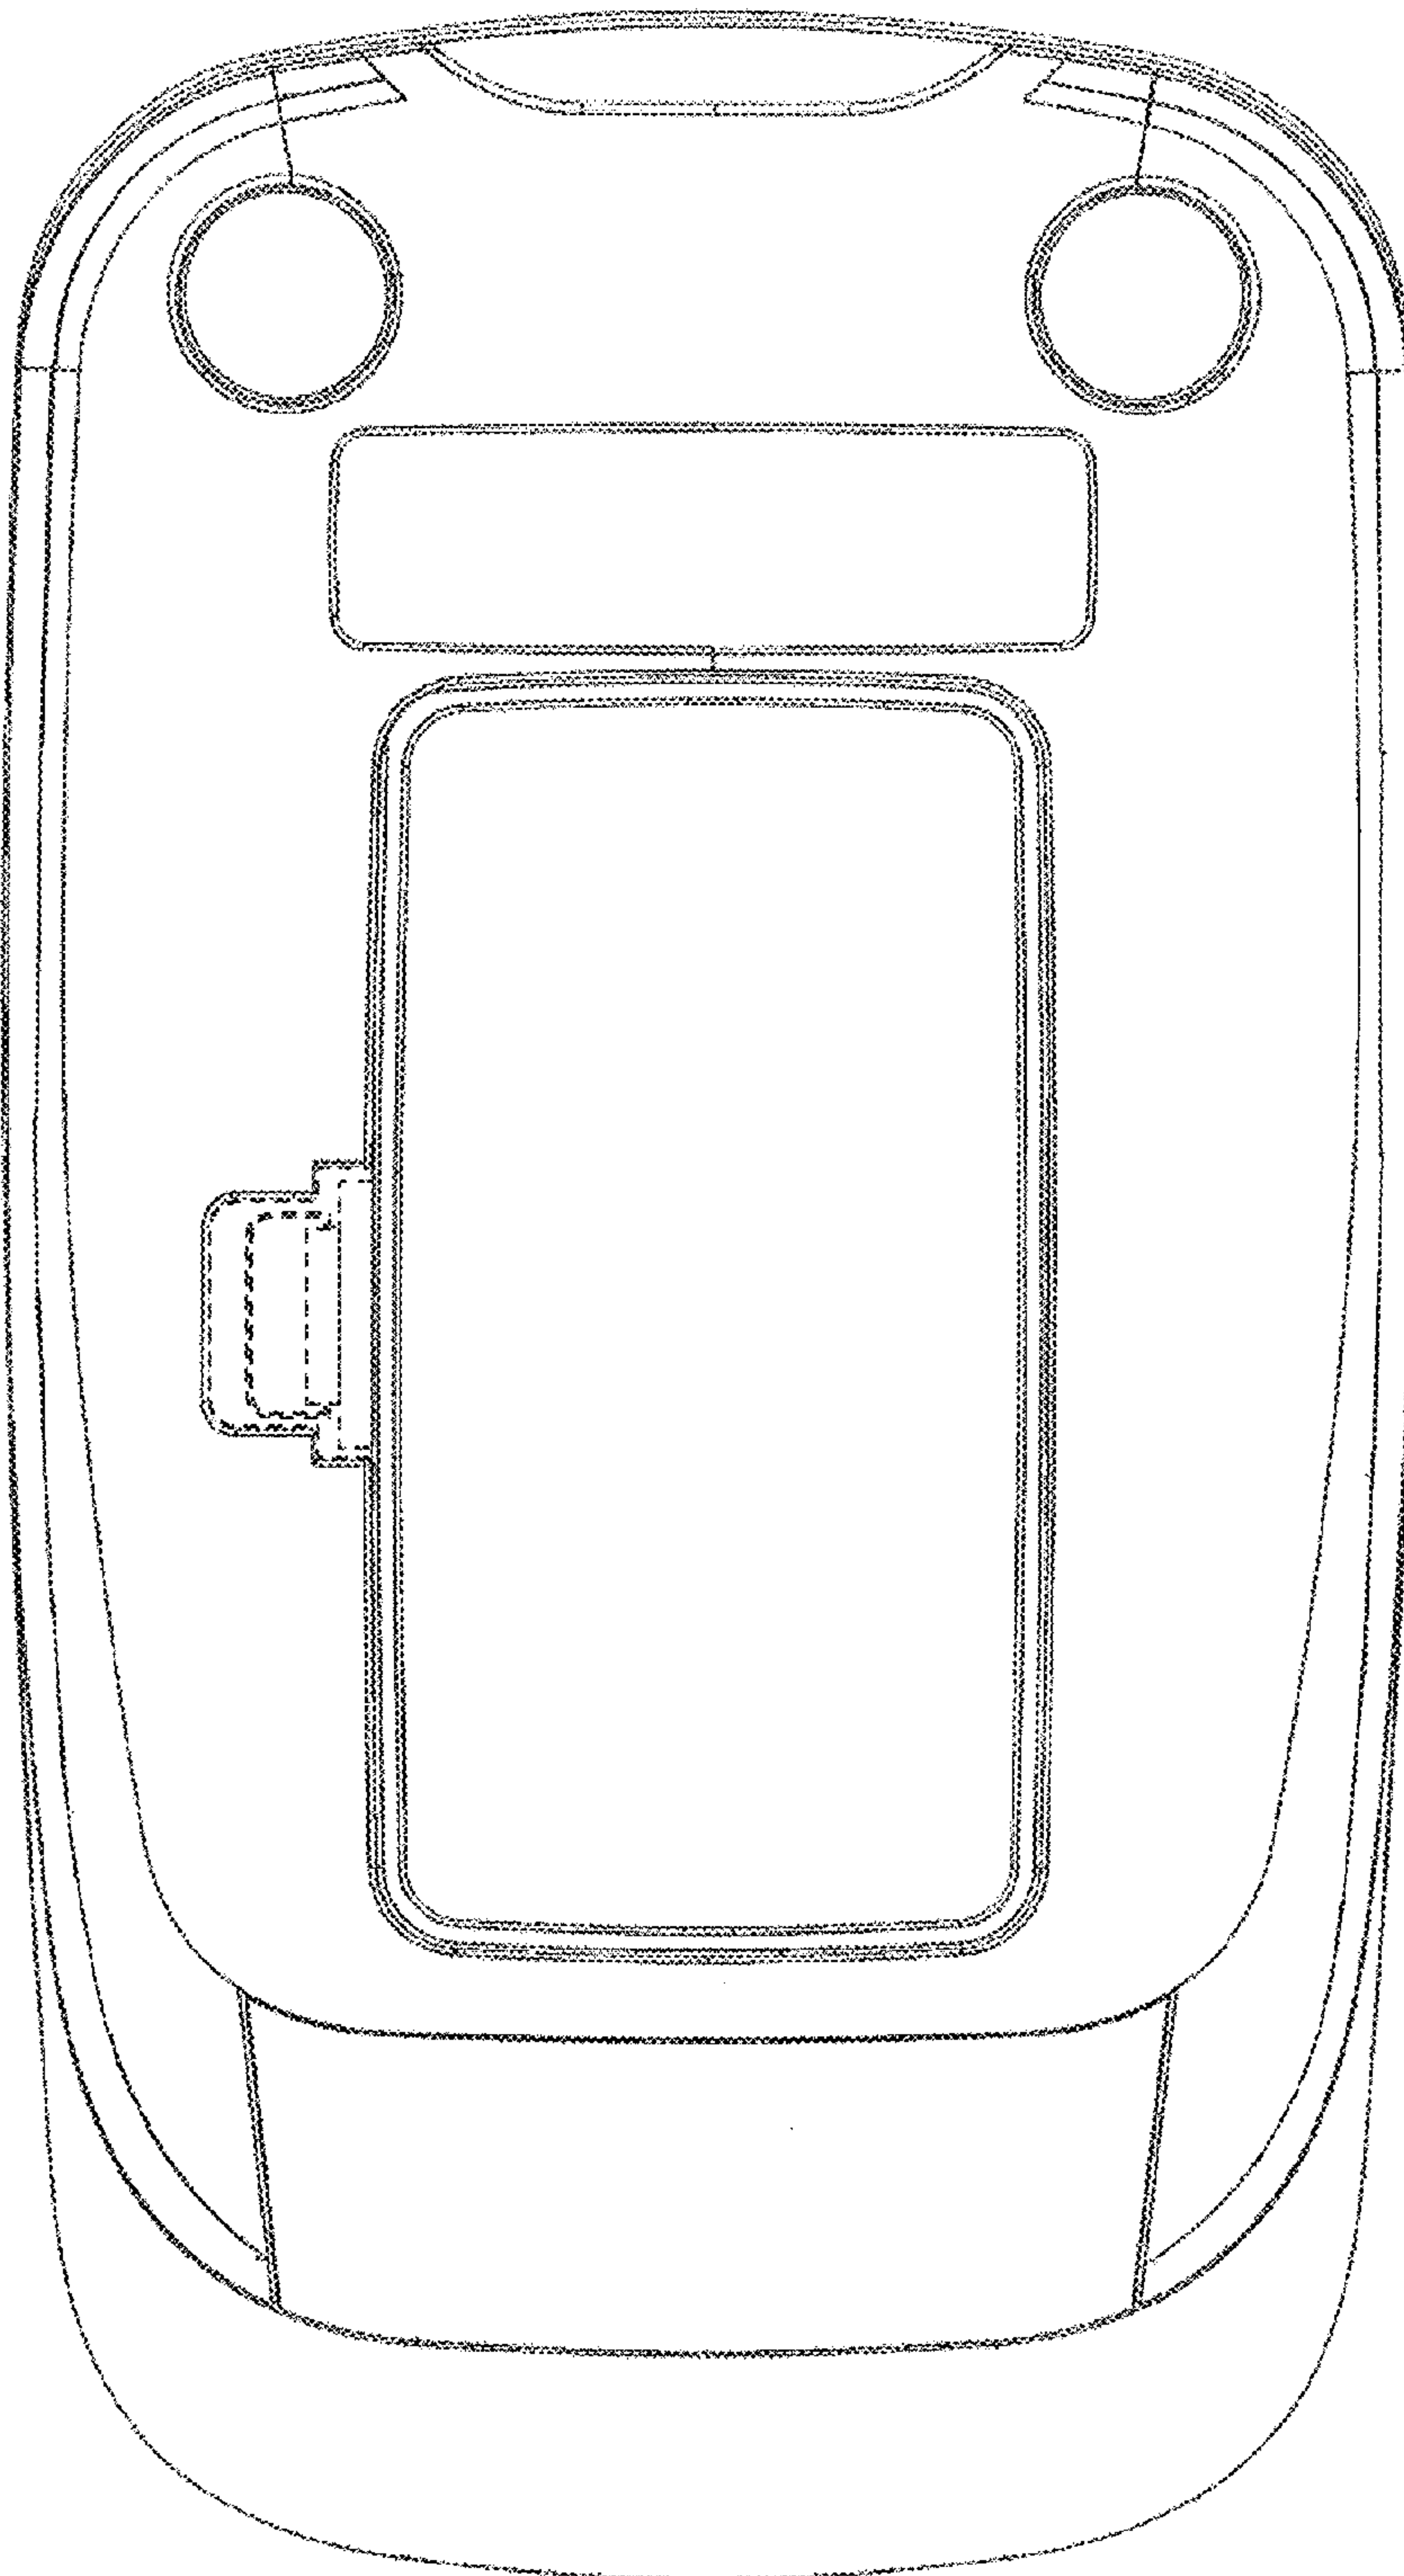


FIG. 21