



US00D739934S

(12) **United States Design Patent**  
**Broyles et al.**

(10) **Patent No.:** **US D739,934 S**

(45) **Date of Patent:** **\*\* Sep. 29, 2015**

(54) **COMPOSITE SYRINGE**

(56) **References Cited**

(71) Applicant: **3M INNOVATIVE PROPERTIES COMPANY**, St. Paul, MN (US)

U.S. PATENT DOCUMENTS

(72) Inventors: **Bruce R. Broyles**, Oakdale, MN (US); **Christopher J. Claypool**, Woodbury, MN (US); **Greg E. Schrank**, Bloomington, MN (US); **Steven J. Maxa**, Lakeville, MN (US); **Andreas J. Boehm**, Reichling (DE); **Stefan Eckstein**, Munich (DE); **Remus Feldman**, Munich (DE)

3,739,947 A	6/1973	Baumann	
D287,877 S *	1/1987	Holewinski et al. ....	D24/114
4,941,752 A	7/1990	Yant	
5,324,273 A *	6/1994	Discko, Jr. ....	433/90
5,392,904 A	2/1995	Frick	
D419,236 S *	1/2000	Carlson et al. ....	D24/114
D421,121 S *	2/2000	Prasad et al. ....	D24/114
D429,812 S *	8/2000	Hjertman et al. ....	D24/114
D472,323 S	3/2003	Sand	
6,884,071 B2	4/2005	Martin	
7,562,792 B2	7/2009	Nisbet	
D635,248 S *	3/2011	Coale .....	D24/114
D645,958 S *	9/2011	Assmann et al. ....	D24/113
D657,867 S *	4/2012	Effenberger .....	D24/114

(73) Assignee: **3M INNOVATIVE PROPERTIES COMPANY**, St. Paul, MN (US)

(Continued)

(\*\*) Term: **14 Years**

OTHER PUBLICATIONS

(21) Appl. No.: **29/500,184**

U.S. Appl. No. 29/483,999, filed Mar. 5, 2014, Broyles.

(22) Filed: **Aug. 22, 2014**

(Continued)

*Primary Examiner* — Wan Laymon

**Related U.S. Application Data**

(63) Continuation of application No. 29/483,999, filed on Mar. 5, 2014.

(51) **LOC (10) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/114; D24/176**

(58) **Field of Classification Search**  
USPC ..... D24/152, 176, 112-114, 130; 604/181, 604/187, 184, 227; 433/226, 229, 88-89, 433/80, 90, 215  
CPC .... A61C 5/062; A61C 5/064; A61C 17/0202; A61C 19/063; A61C 5/066; B05C 17/00593; B05C 17/00506; B05C 17/00553

See application file for complete search history.


(57) **CLAIM**

The ornamental design for a composite syringe, as shown and described.

**DESCRIPTION**

FIG. 1 is a top perspective view of a composite syringe in accordance with the present disclosure; FIG. 2 is a front plan view of the composite syringe of FIG. 1; FIG. 3 is a rear plan view of the composite syringe of FIG. 1; FIG. 4 is a top plan view of the composite syringe of FIG. 1; FIG. 5 is a bottom plan view of the composite syringe of FIG. 1; and, FIG. 6 is a side view of the composite syringe of FIG. 1, the opposite side view a mirror image. The broken lines shown in the figures represent portions of the composite syringe that form no part of the claimed design.

**1 Claim, 2 Drawing Sheets**

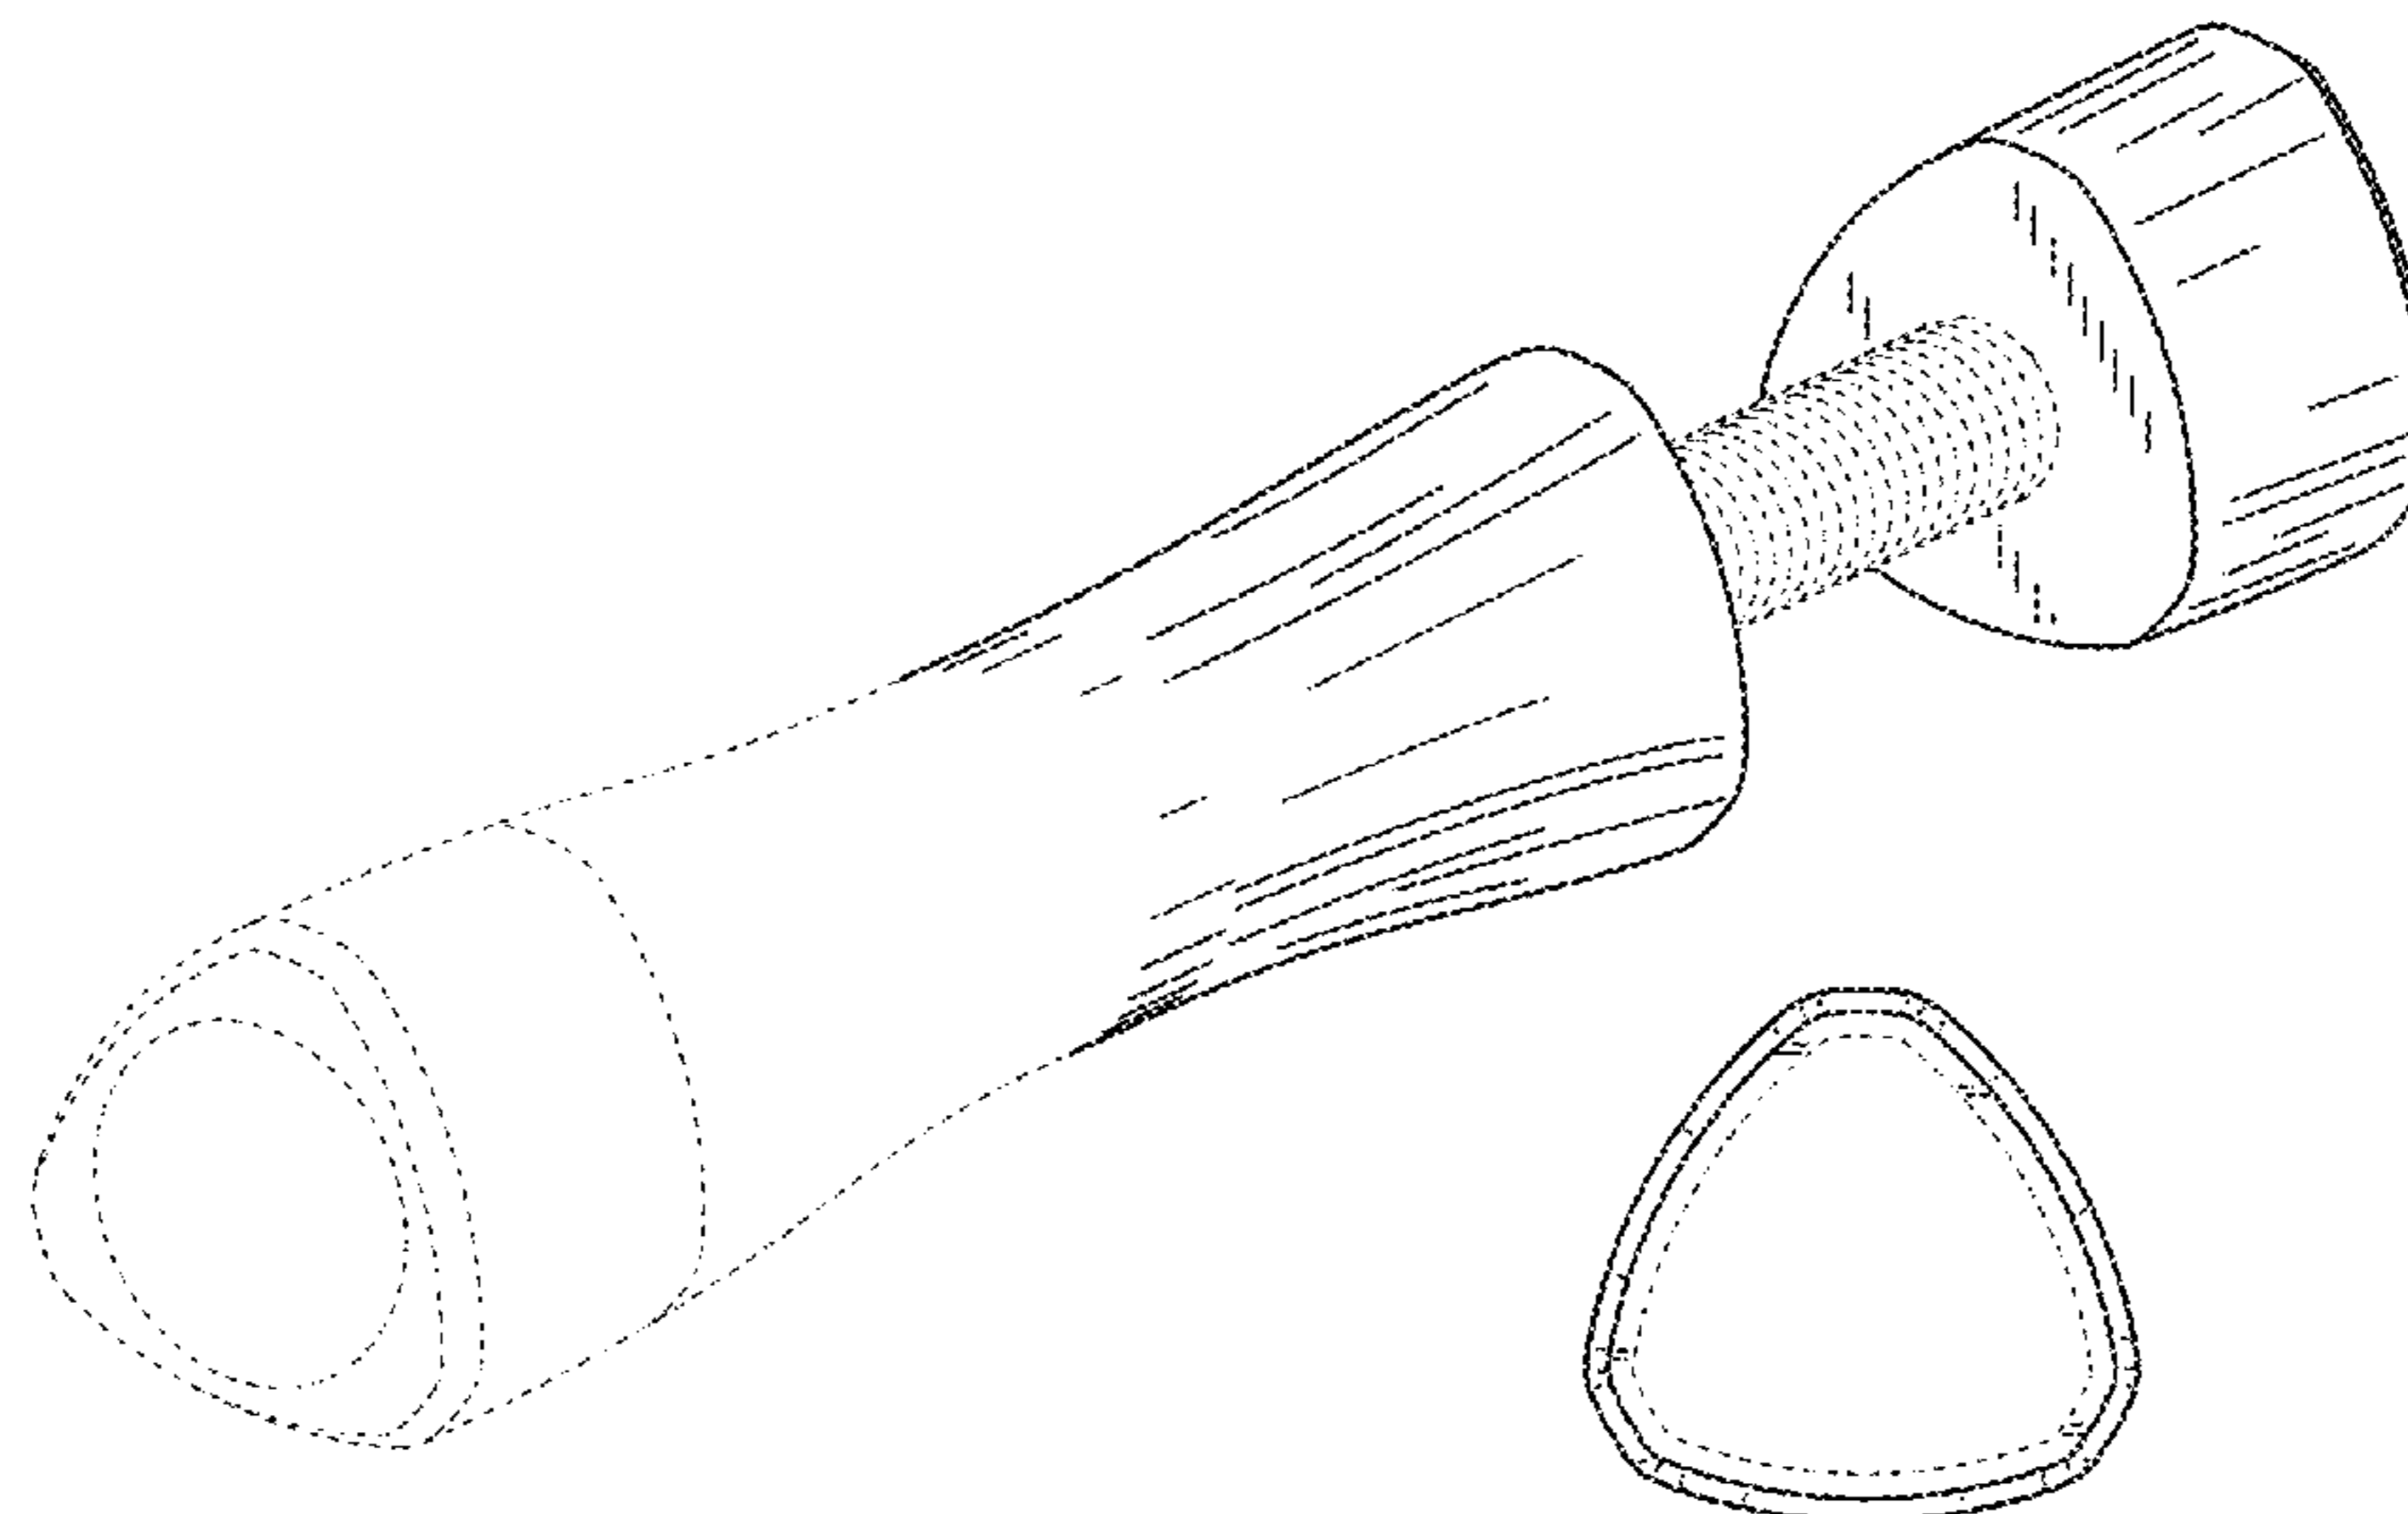

(56)

**References Cited**

U.S. PATENT DOCUMENTS


D672,873 S 12/2012 An  
D681,808 S \* 5/2013 Holaschke et al. .... D24/114  
D690,813 S 10/2013 Bizzell  
D693,940 S 11/2013 Walter  
D696,787 S 12/2013 Walter  
D698,918 S \* 2/2014 Leiner et al. .... D24/114  
2010/0240004 A1 9/2010 Zalsman

2011/0056985 A1 3/2011 Bubleitz  
2013/0101955 A1 4/2013 Broyles  
2013/0260335 A1 10/2013 Peuker


OTHER PUBLICATIONS

*Tetric EvoCeram & Tetric EvoFlow®*, Ivoclar Vivodent, Oct. 29, 2013, 10 pages.


\* cited by examiner

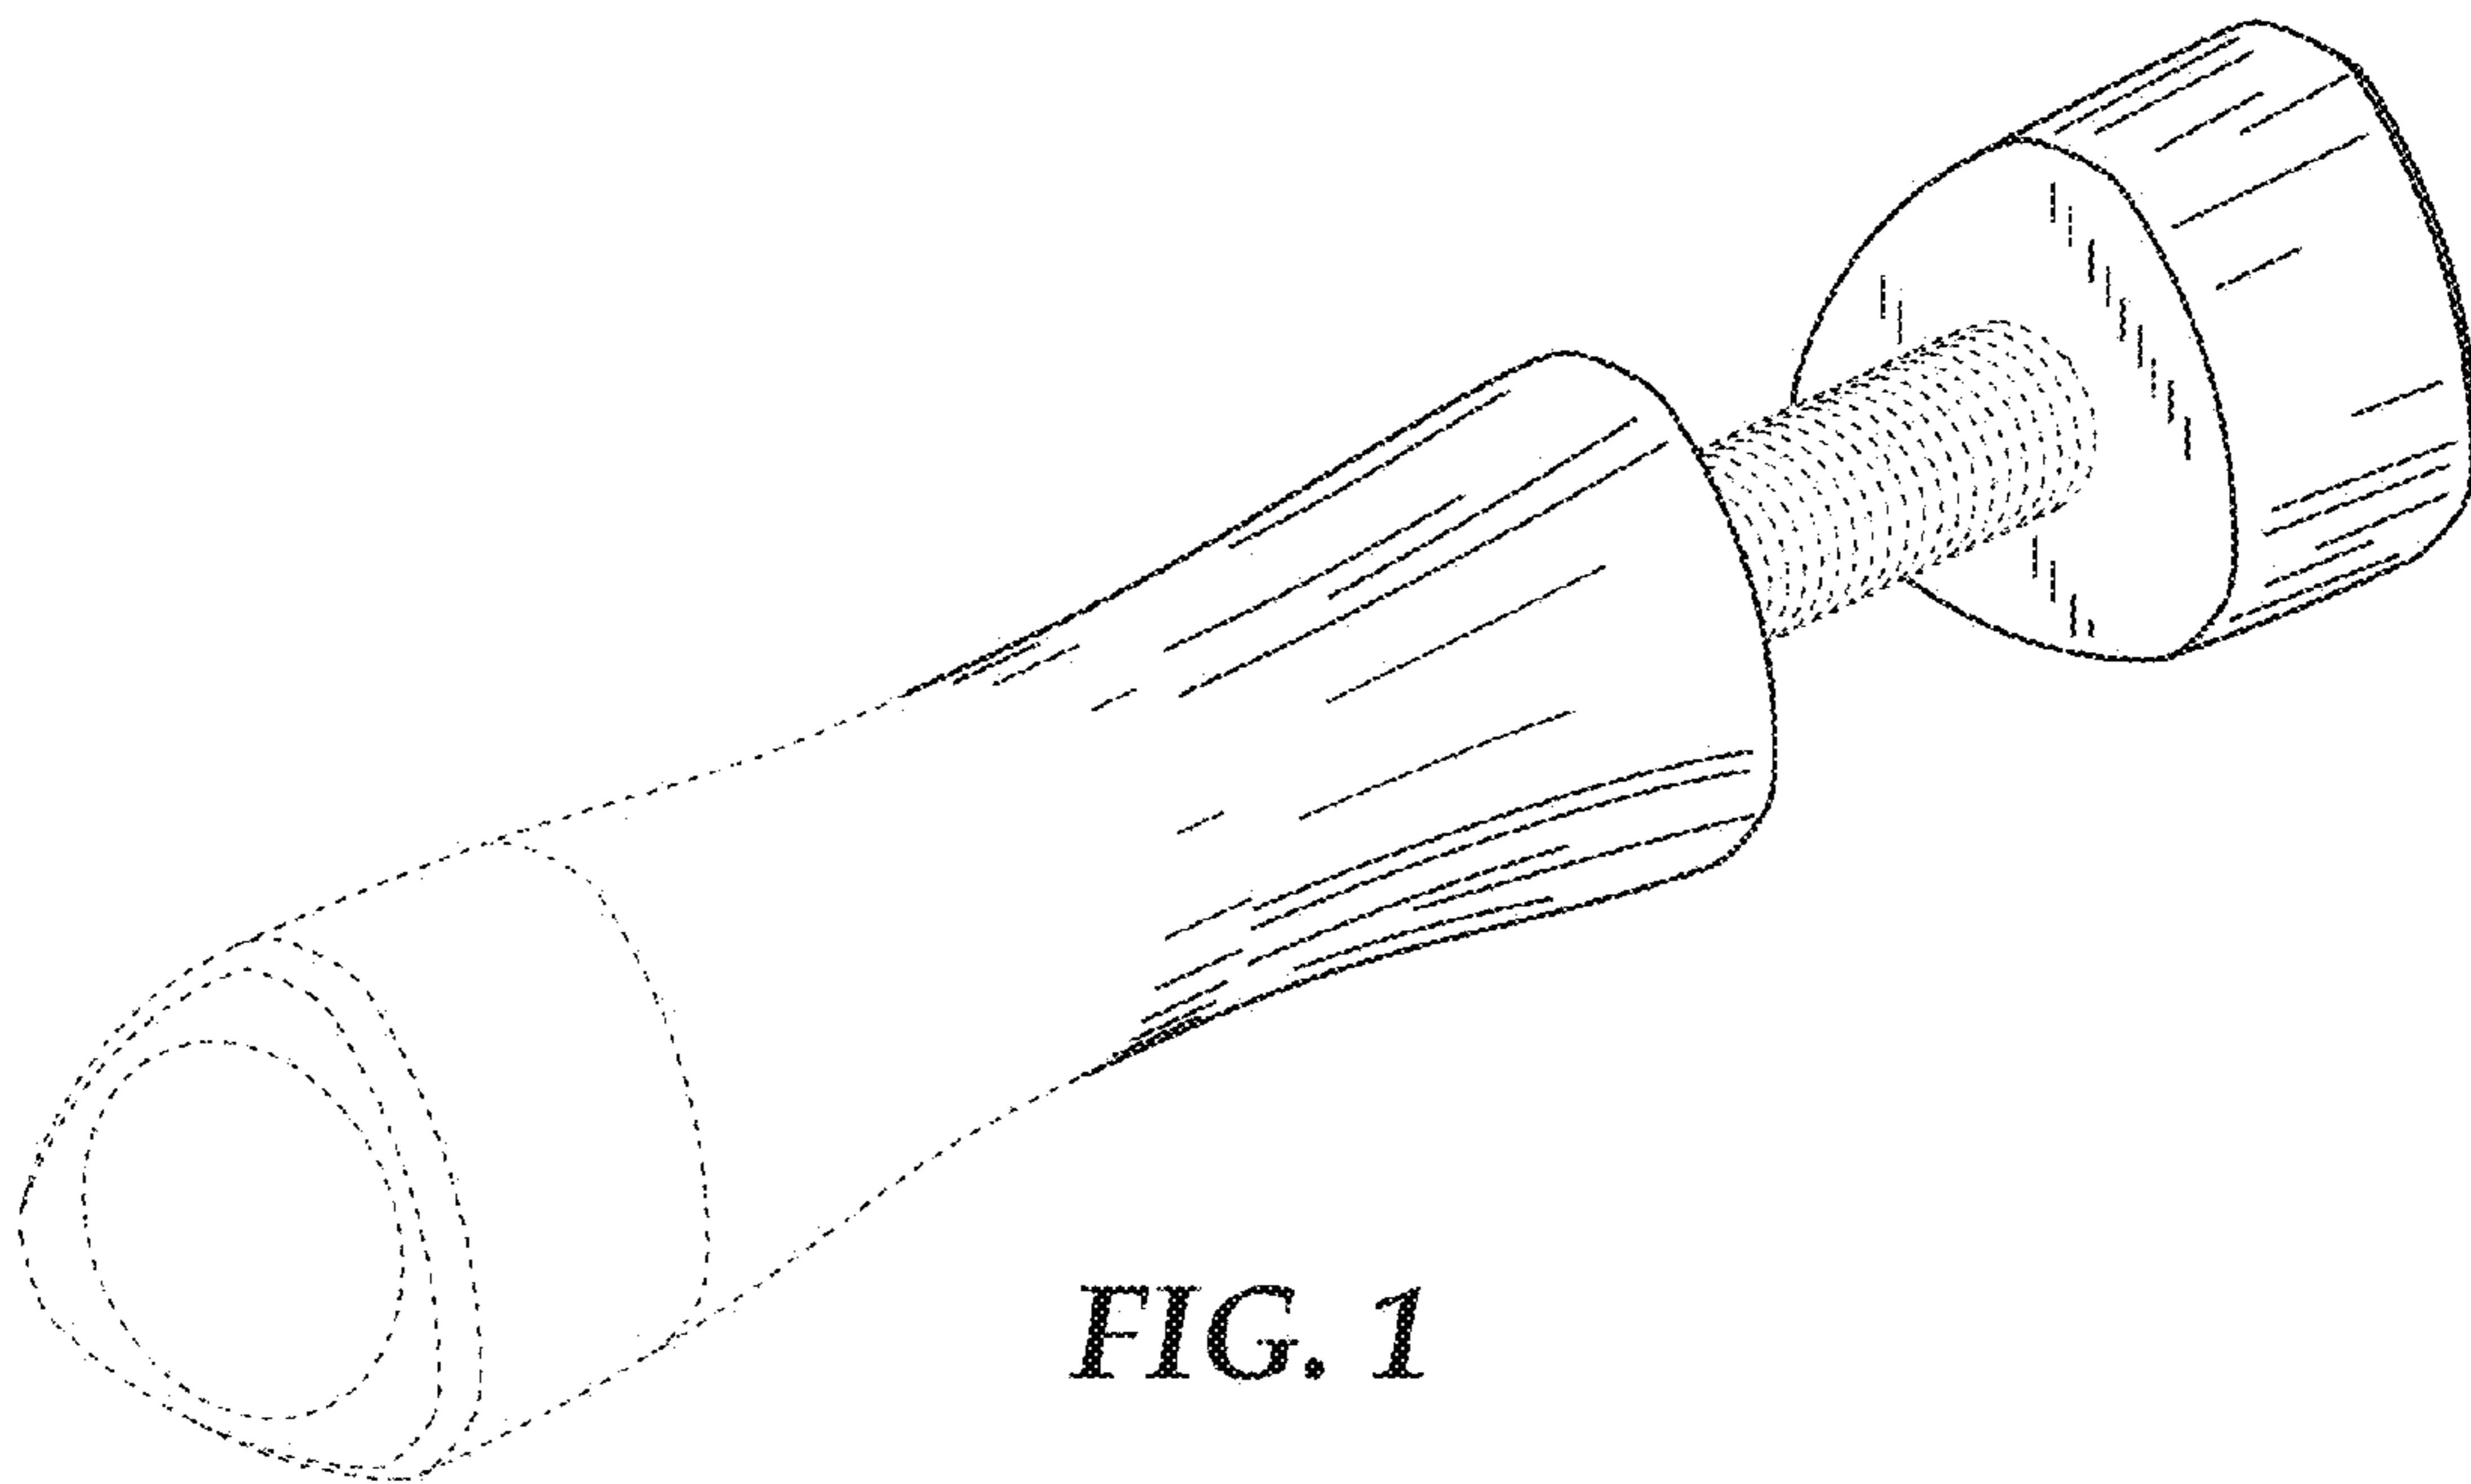


**FIG. 1**

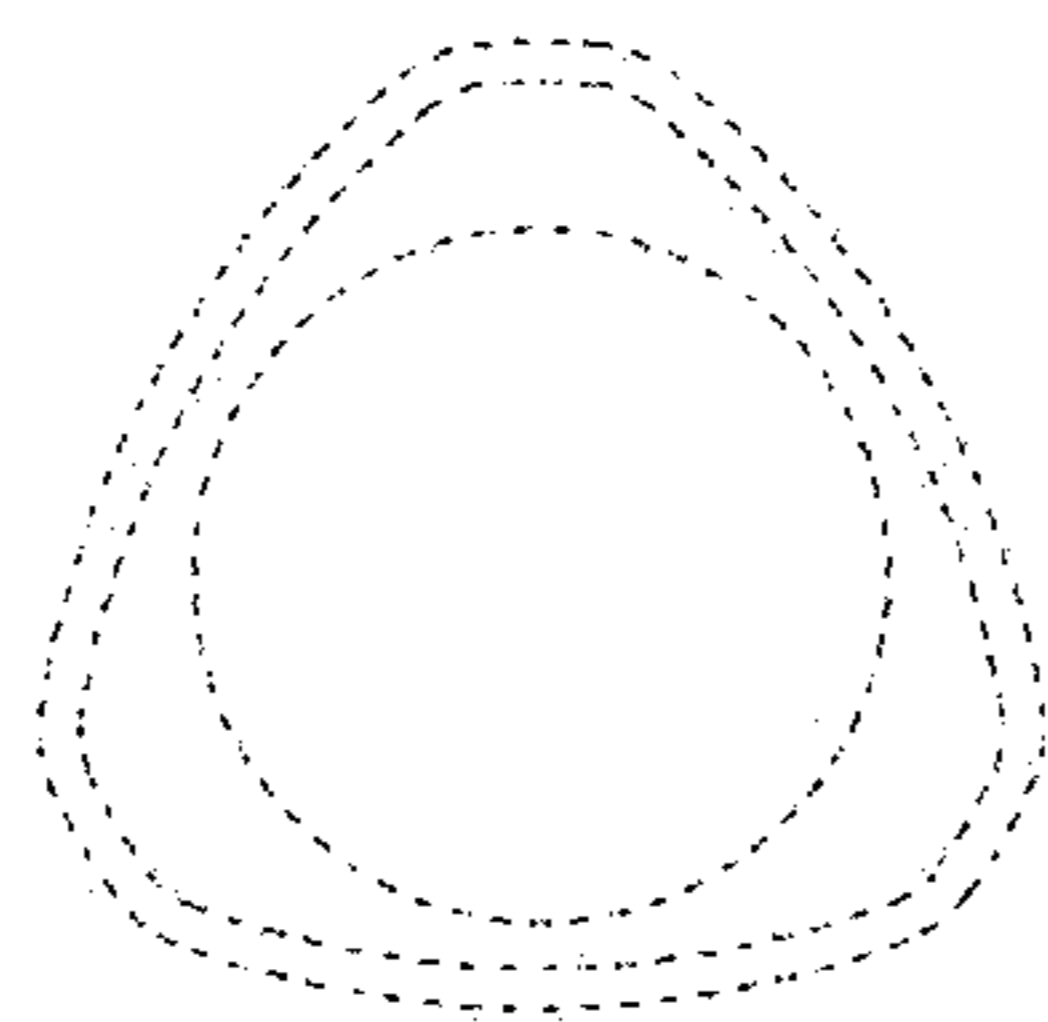


**FIG. 2**

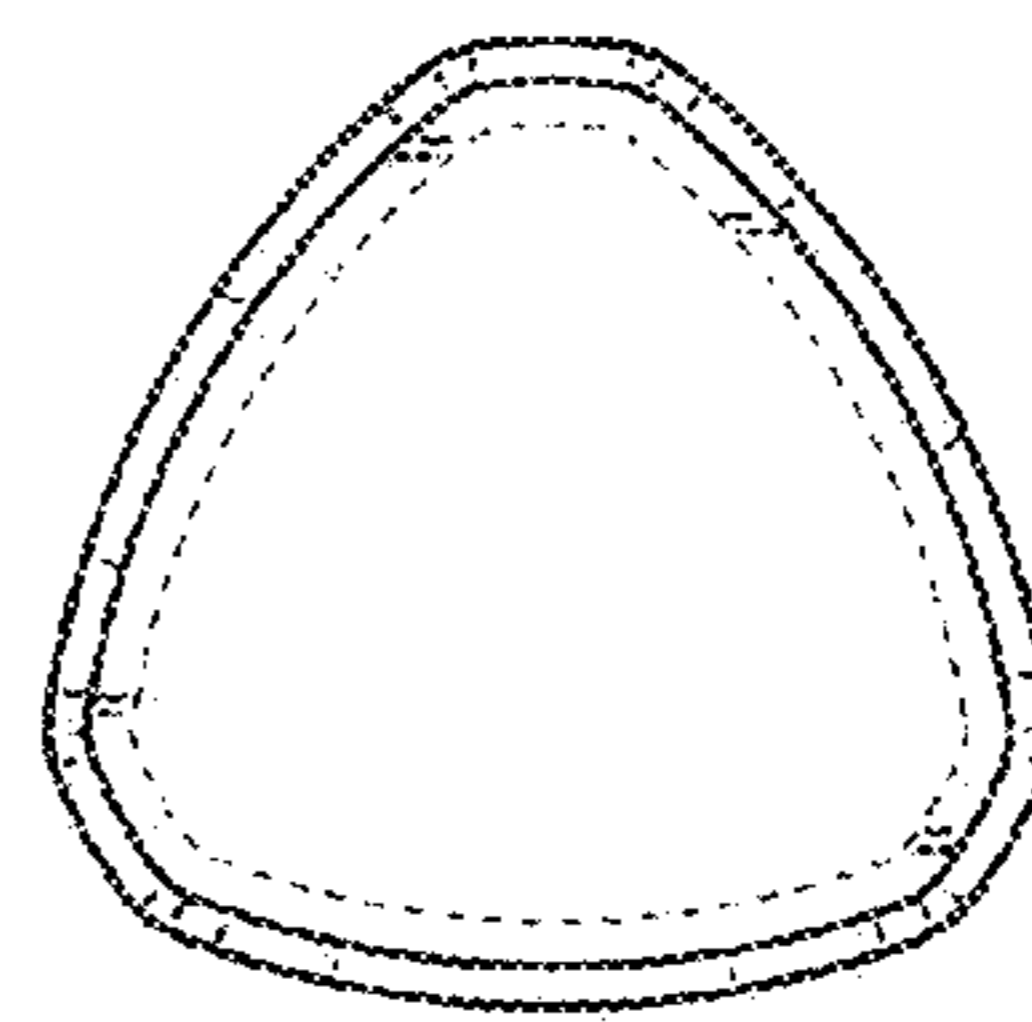


**FIG. 3**

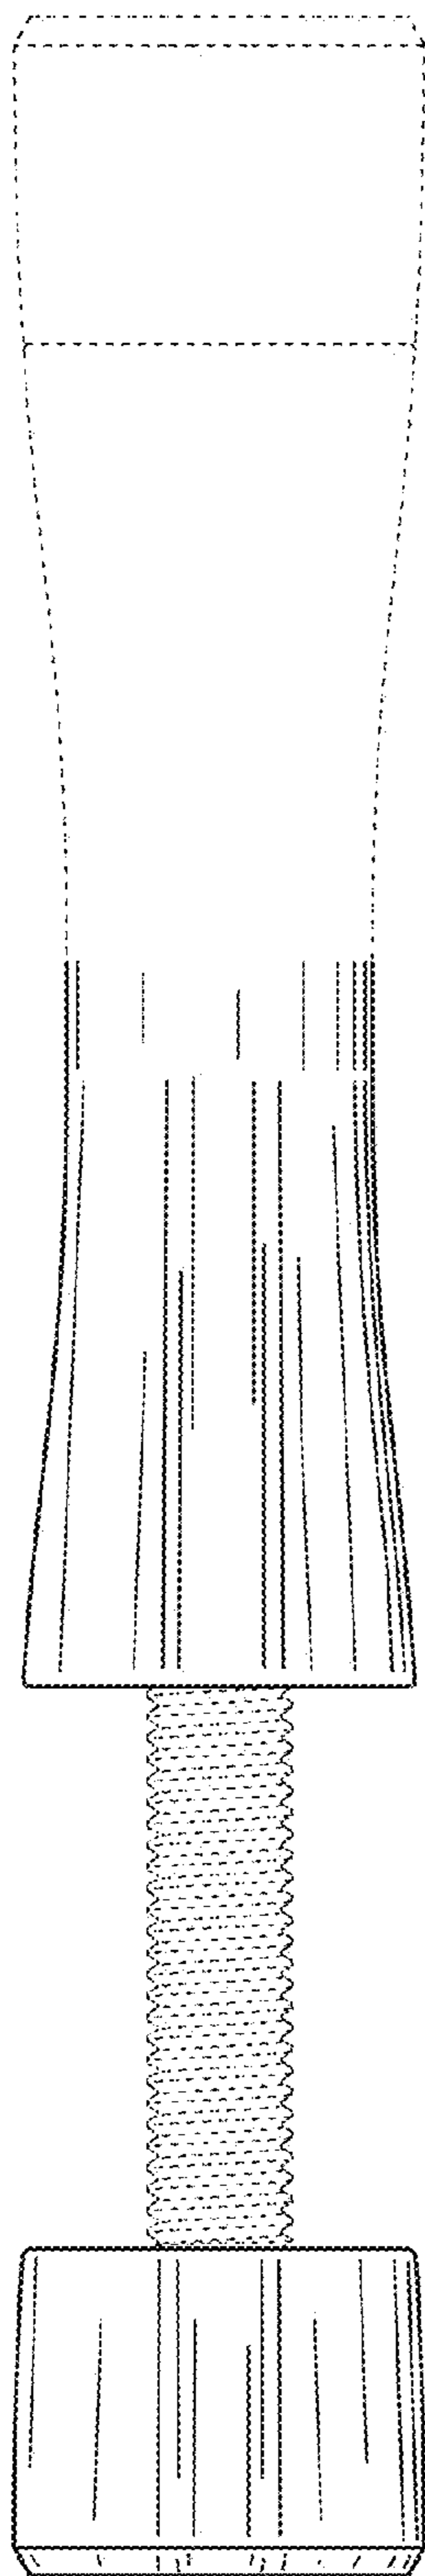

*FIG. 4*

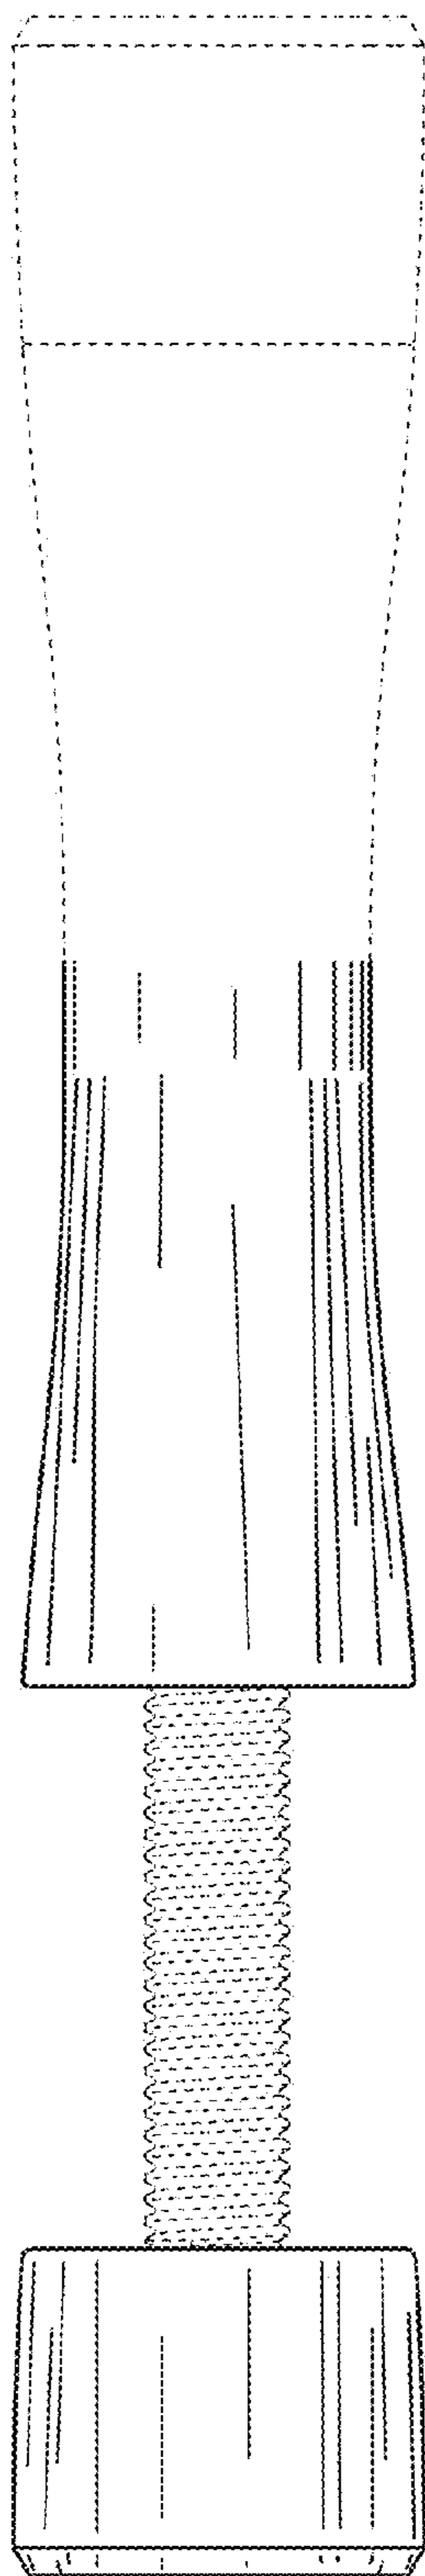

*FIG. 5*

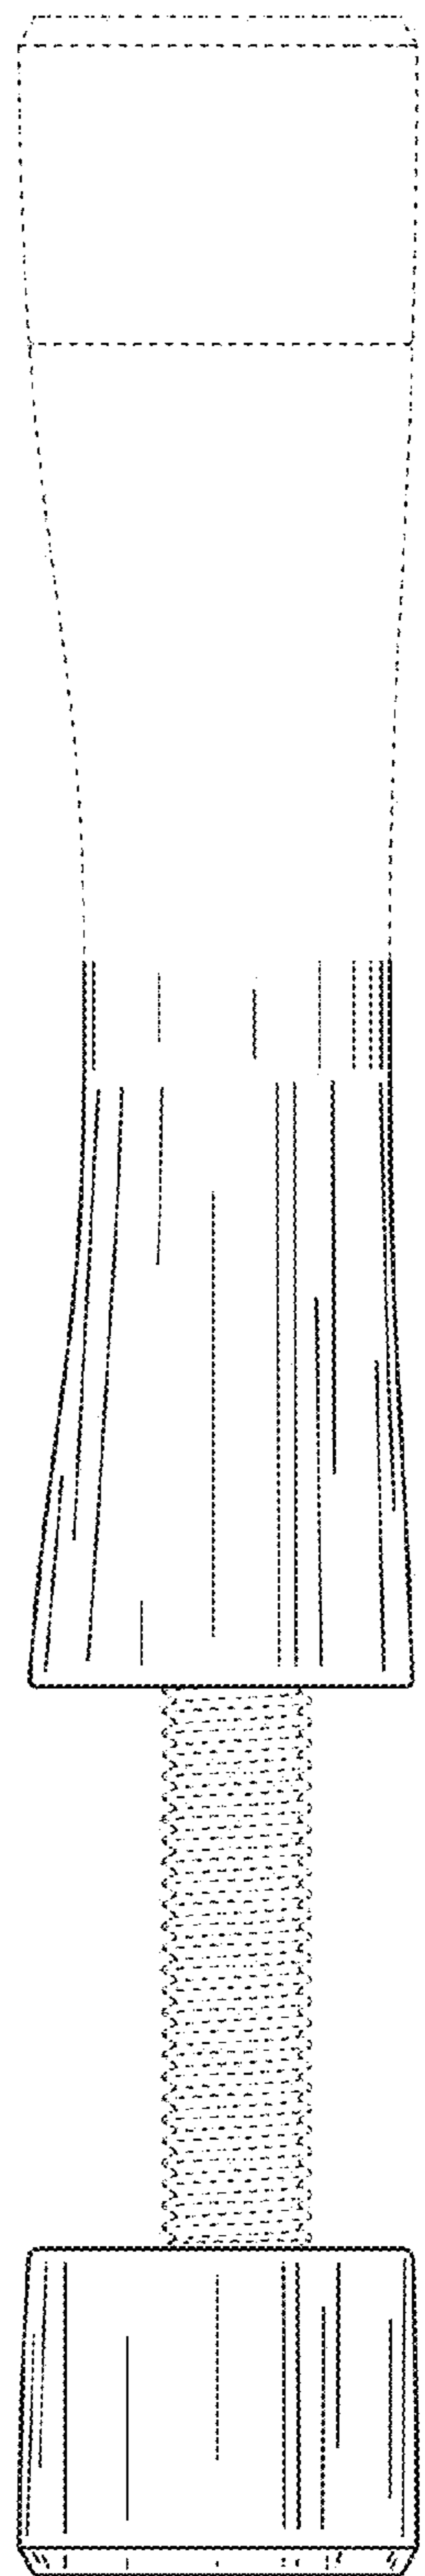

*FIG. 6*