

US00D740428S

(12) **United States Design Patent**
Suzuki

(10) **Patent No.:** **US D740,428 S**
(45) **Date of Patent:** **** Oct. 6, 2015**

(54) **BIOMEDICAL SIGNAL RECORDER WITH A RADIO FUNCTION**

(71) Applicant: **Kabushiki Kaisha Toshiba**, Minato-ku, Tokyo (JP)

(72) Inventor: **Takuji Suzuki**, Yokohama (JP)

(73) Assignee: **Kabushiki Kaisha Toshiba**, Minato-ku, Tokyo (JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/465,665**

(22) Filed: **Aug. 30, 2013**

(30) **Foreign Application Priority Data**

Mar. 4, 2013 (JP) 2013-004670

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/187**

(58) **Field of Classification Search**

USPC D24/168, 186–187, 200, 167; 600/301, 600/544, 546, 554, 372, 382, 384, 600/386–395; 601/21; 602/2; 606/32; 607/45, 46, 115, 139, 142, 148, 152; 29/842

CPC A61B 5/0002; A61B 5/0408; A61B 5/04085; A61B 5/0404; A61B 5/04082; A61B 5/6831; A61B 5/04087; A61B 5/0476; A61B 5/0488; A61B 5/05; A61B 18/1492; A61H 2201/10; A61F 7/007; A61N 1/3605; A61N 1/36021; A61N 1/05; A61N 1/0472; A61N 1/046; A61N 1/0476; A61N 1/0492

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D255,149 S * 5/1980 Bevilacqua D24/187
D326,717 S * 6/1992 Henderson et al. D24/168

D425,203 S * 5/2000 Sheehan et al. D24/187
D456,907 S * 5/2002 Sanfilippo D24/187
D468,433 S * 1/2003 Wagner et al. D24/187
D471,281 S * 3/2003 Baura et al. D24/187
D475,138 S * 5/2003 Baura et al. D24/187
D483,488 S * 12/2003 Luthy et al. D24/140
D492,783 S * 7/2004 Lax D24/167
D495,055 S * 8/2004 Silber D24/187
D511,384 S * 11/2005 Masuda D24/187
D536,673 S * 2/2007 Silber D24/187
D557,423 S * 12/2007 Chen D24/187
D558,352 S * 12/2007 Sanfilippo D24/187
D558,882 S * 1/2008 Brady D24/187

(Continued)

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Banner & Witcoff, Ltd.

(57) **CLAIM**

The ornamental design for a biomedical signal recorder with a radio function, as shown and described.

DESCRIPTION

FIG. 1 is a top view of a biomedical signal recorder with a radio function, showing my new design;

FIG. 2 is a front view thereof;

FIG. 3 is a right side view thereof; the left side being symmetrical;

FIG. 4 is a rear view thereof;


FIG. 5 is a bottom view thereof;

FIG. 6 is an enlarged cross sectional view thereof, taken along the line 6-6 in FIG. 2 with its internal mechanisms omitted; and,

FIG. 7 is an enlarged cross sectional view thereof, taken along the line 7-7 in FIG. 5 with its internal mechanisms omitted.

The uneven spaced broken lines define the bounds of the claimed design and form no part thereof. The even spaced broken lines are included for the purpose of illustrating unclaimed portions of the biomedical signal recorder with a radio function and form no part of the claimed design.

1 Claim, 3 Drawing Sheets

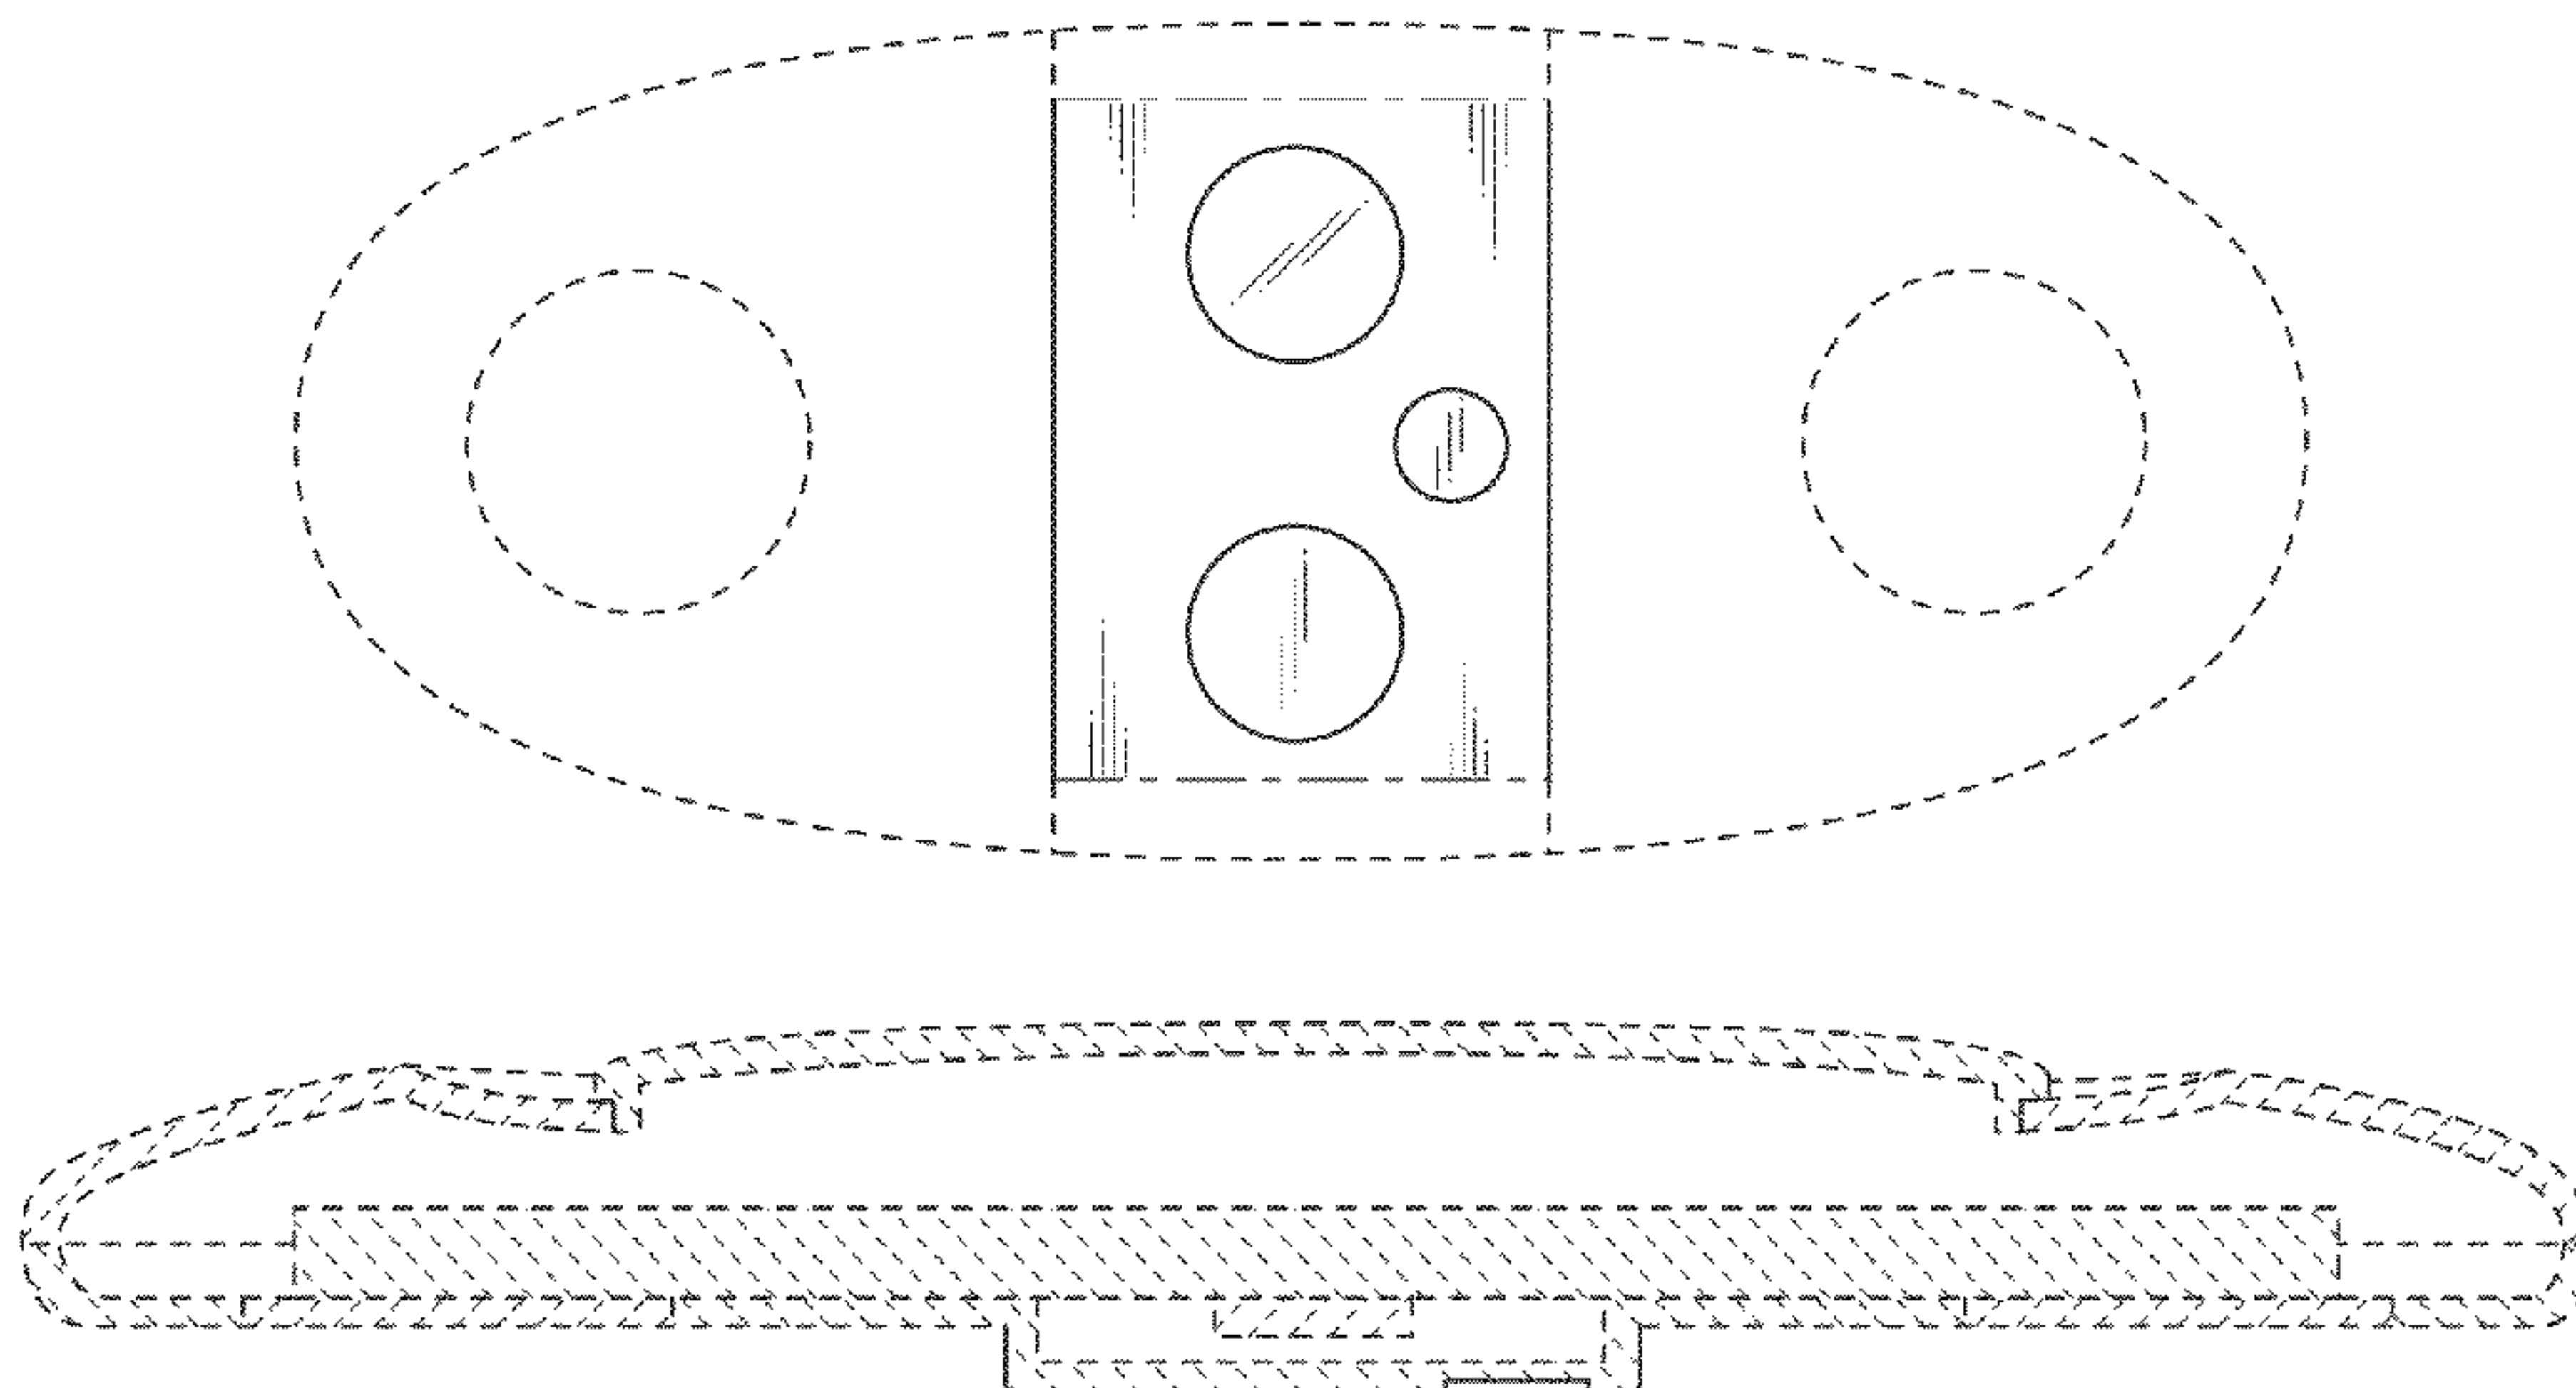

(56)

References Cited

U.S. PATENT DOCUMENTS

D565,183 S * 3/2008 Cheng et al. D24/168

D567,949 S * 4/2008 Lash et al. D24/168

D568,479 S * 5/2008 Mao et al. D24/168

D598,114 S * 8/2009 Cryan D24/187

D599,909 S * 9/2009 Rinott et al. D24/186

D608,451 S * 1/2010 Hanoun D24/186

D631,552 S * 1/2011 Kasabach et al. D24/186

D639,437 S * 6/2011 Bishay et al. D24/167

8,201,327 B2 * 6/2012 Hallin 29/842

8,238,996 B2 * 8/2012 Burnes et al. 600/382

8,738,112 B2 * 5/2014 Choe et al. 600/391

* cited by examiner

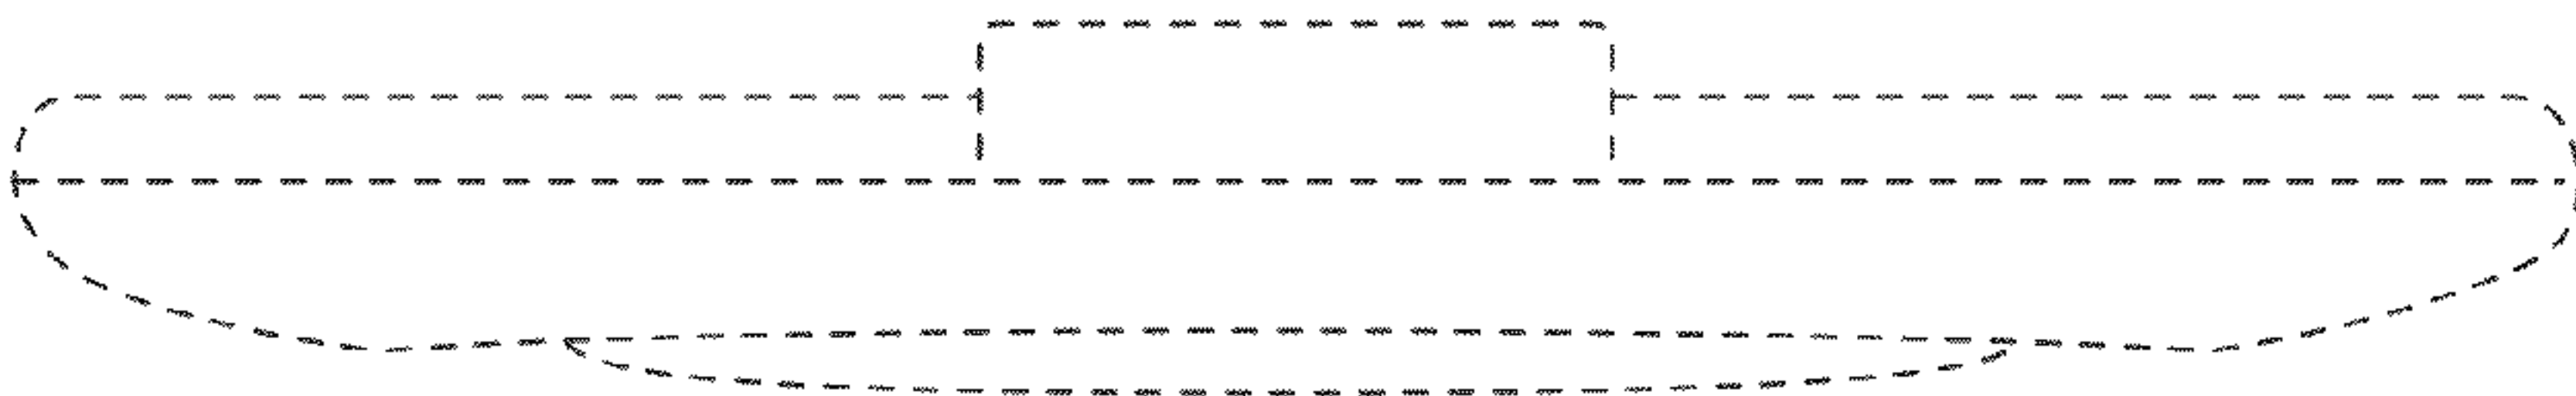


FIG. 1

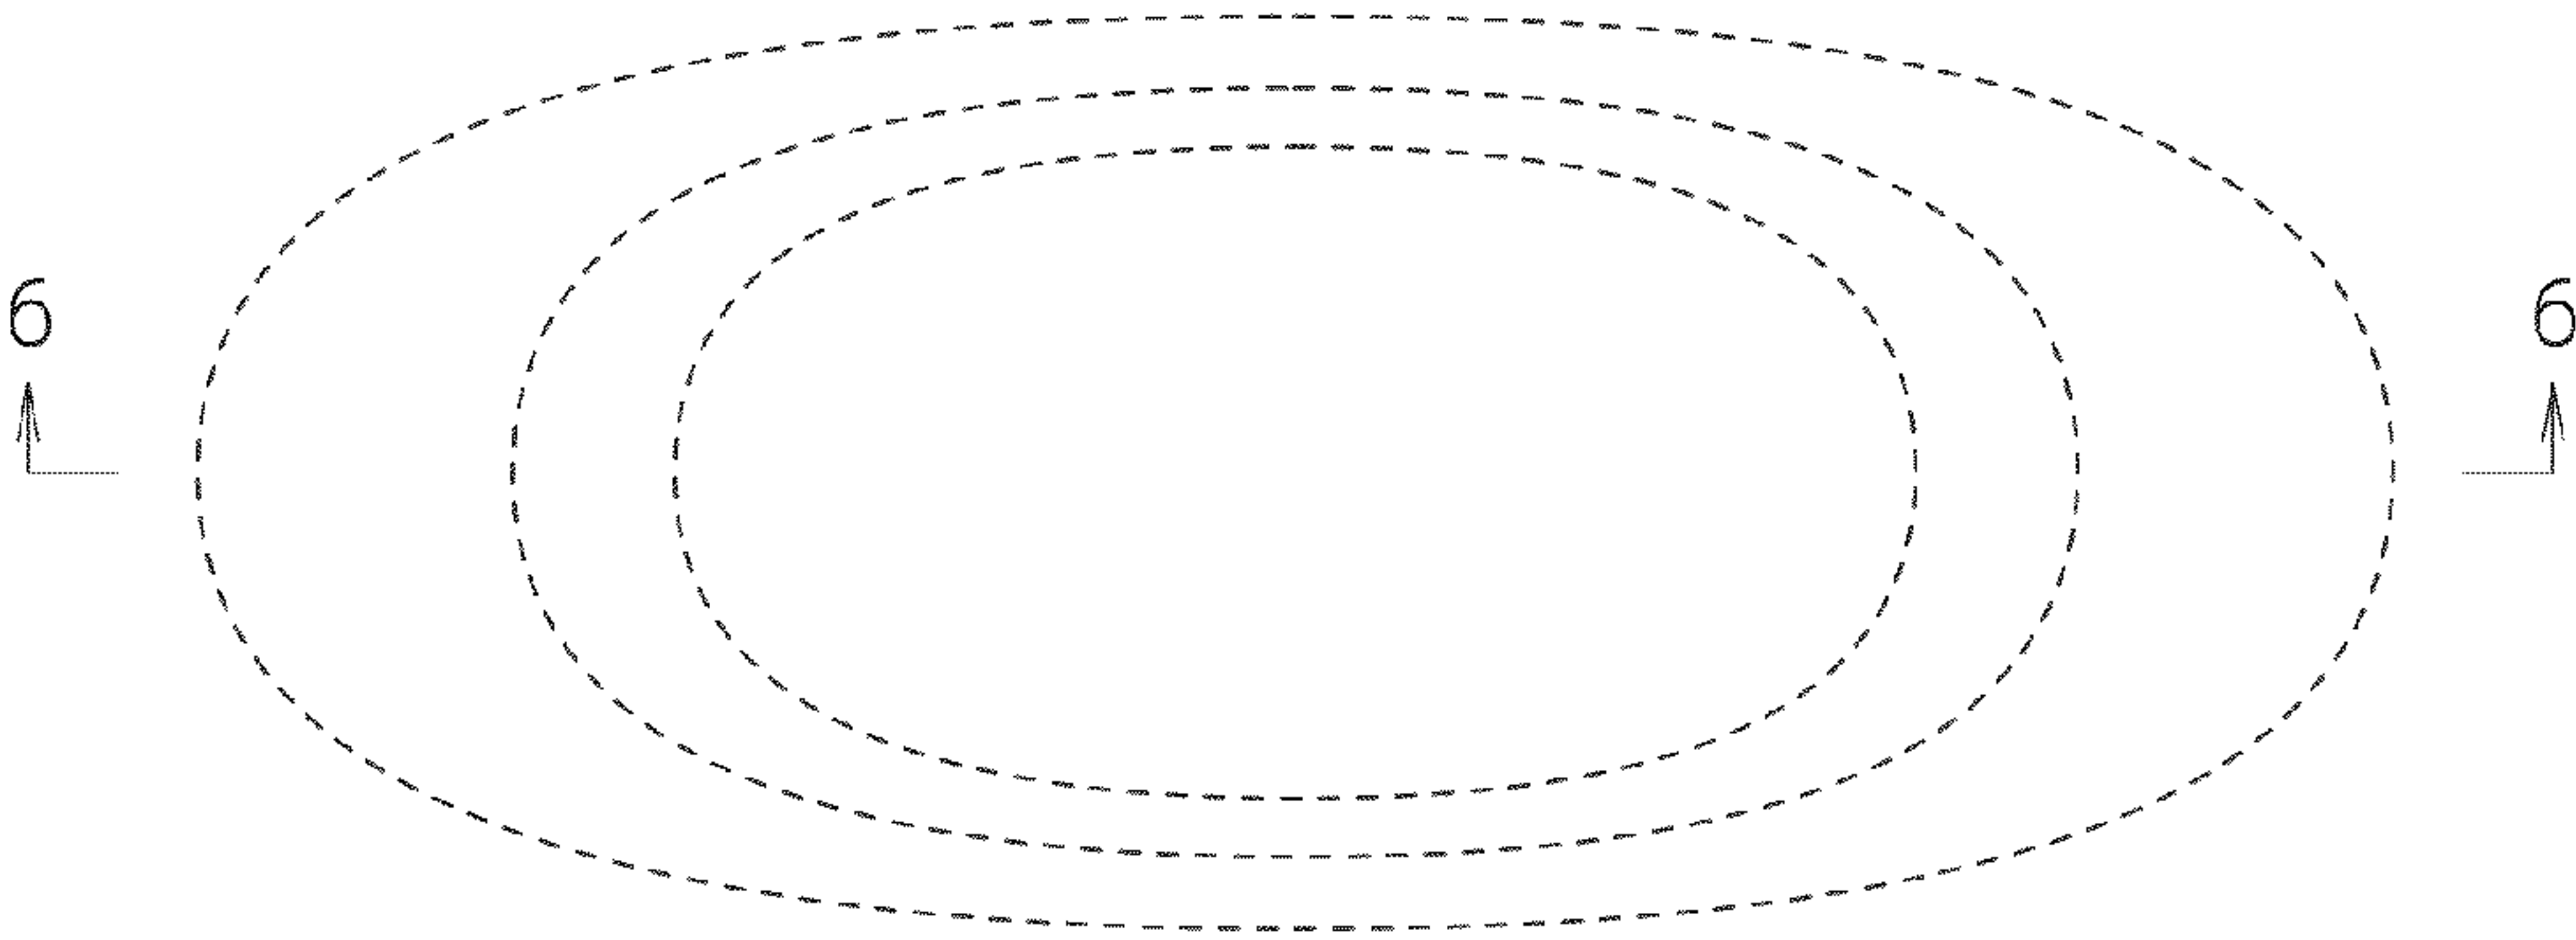


FIG. 2

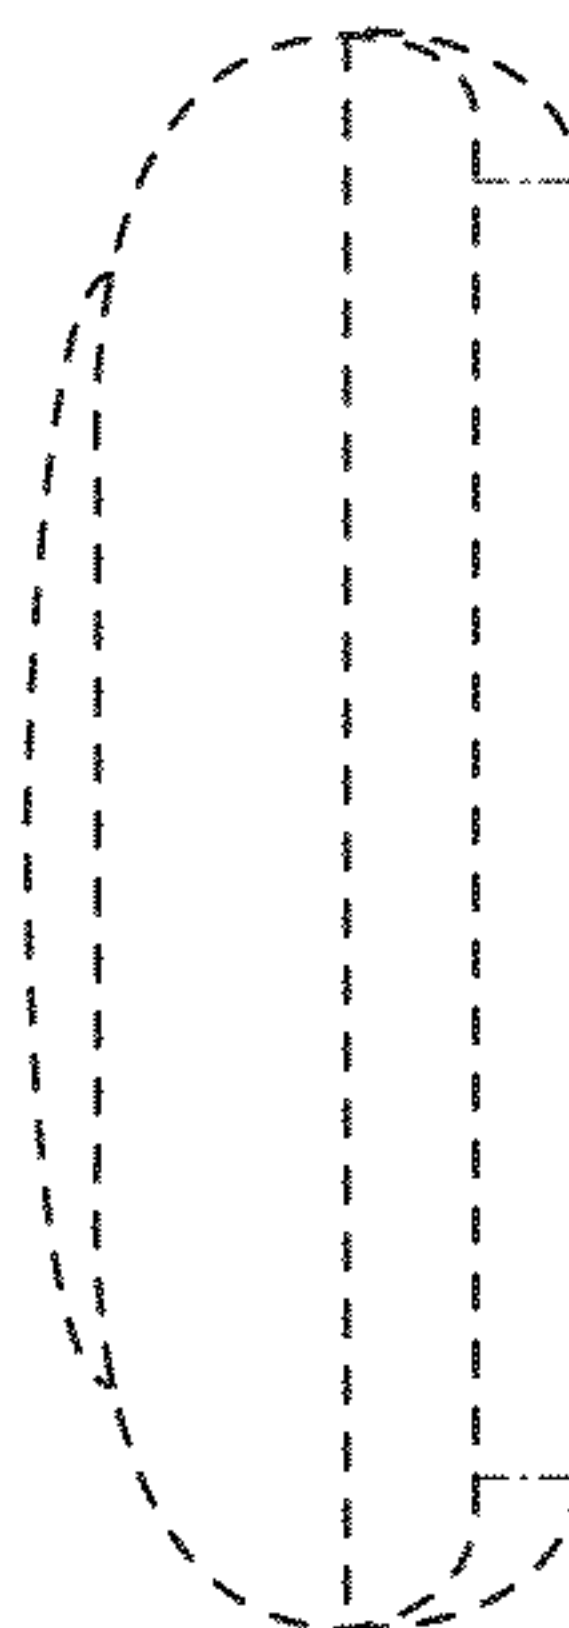


FIG. 3

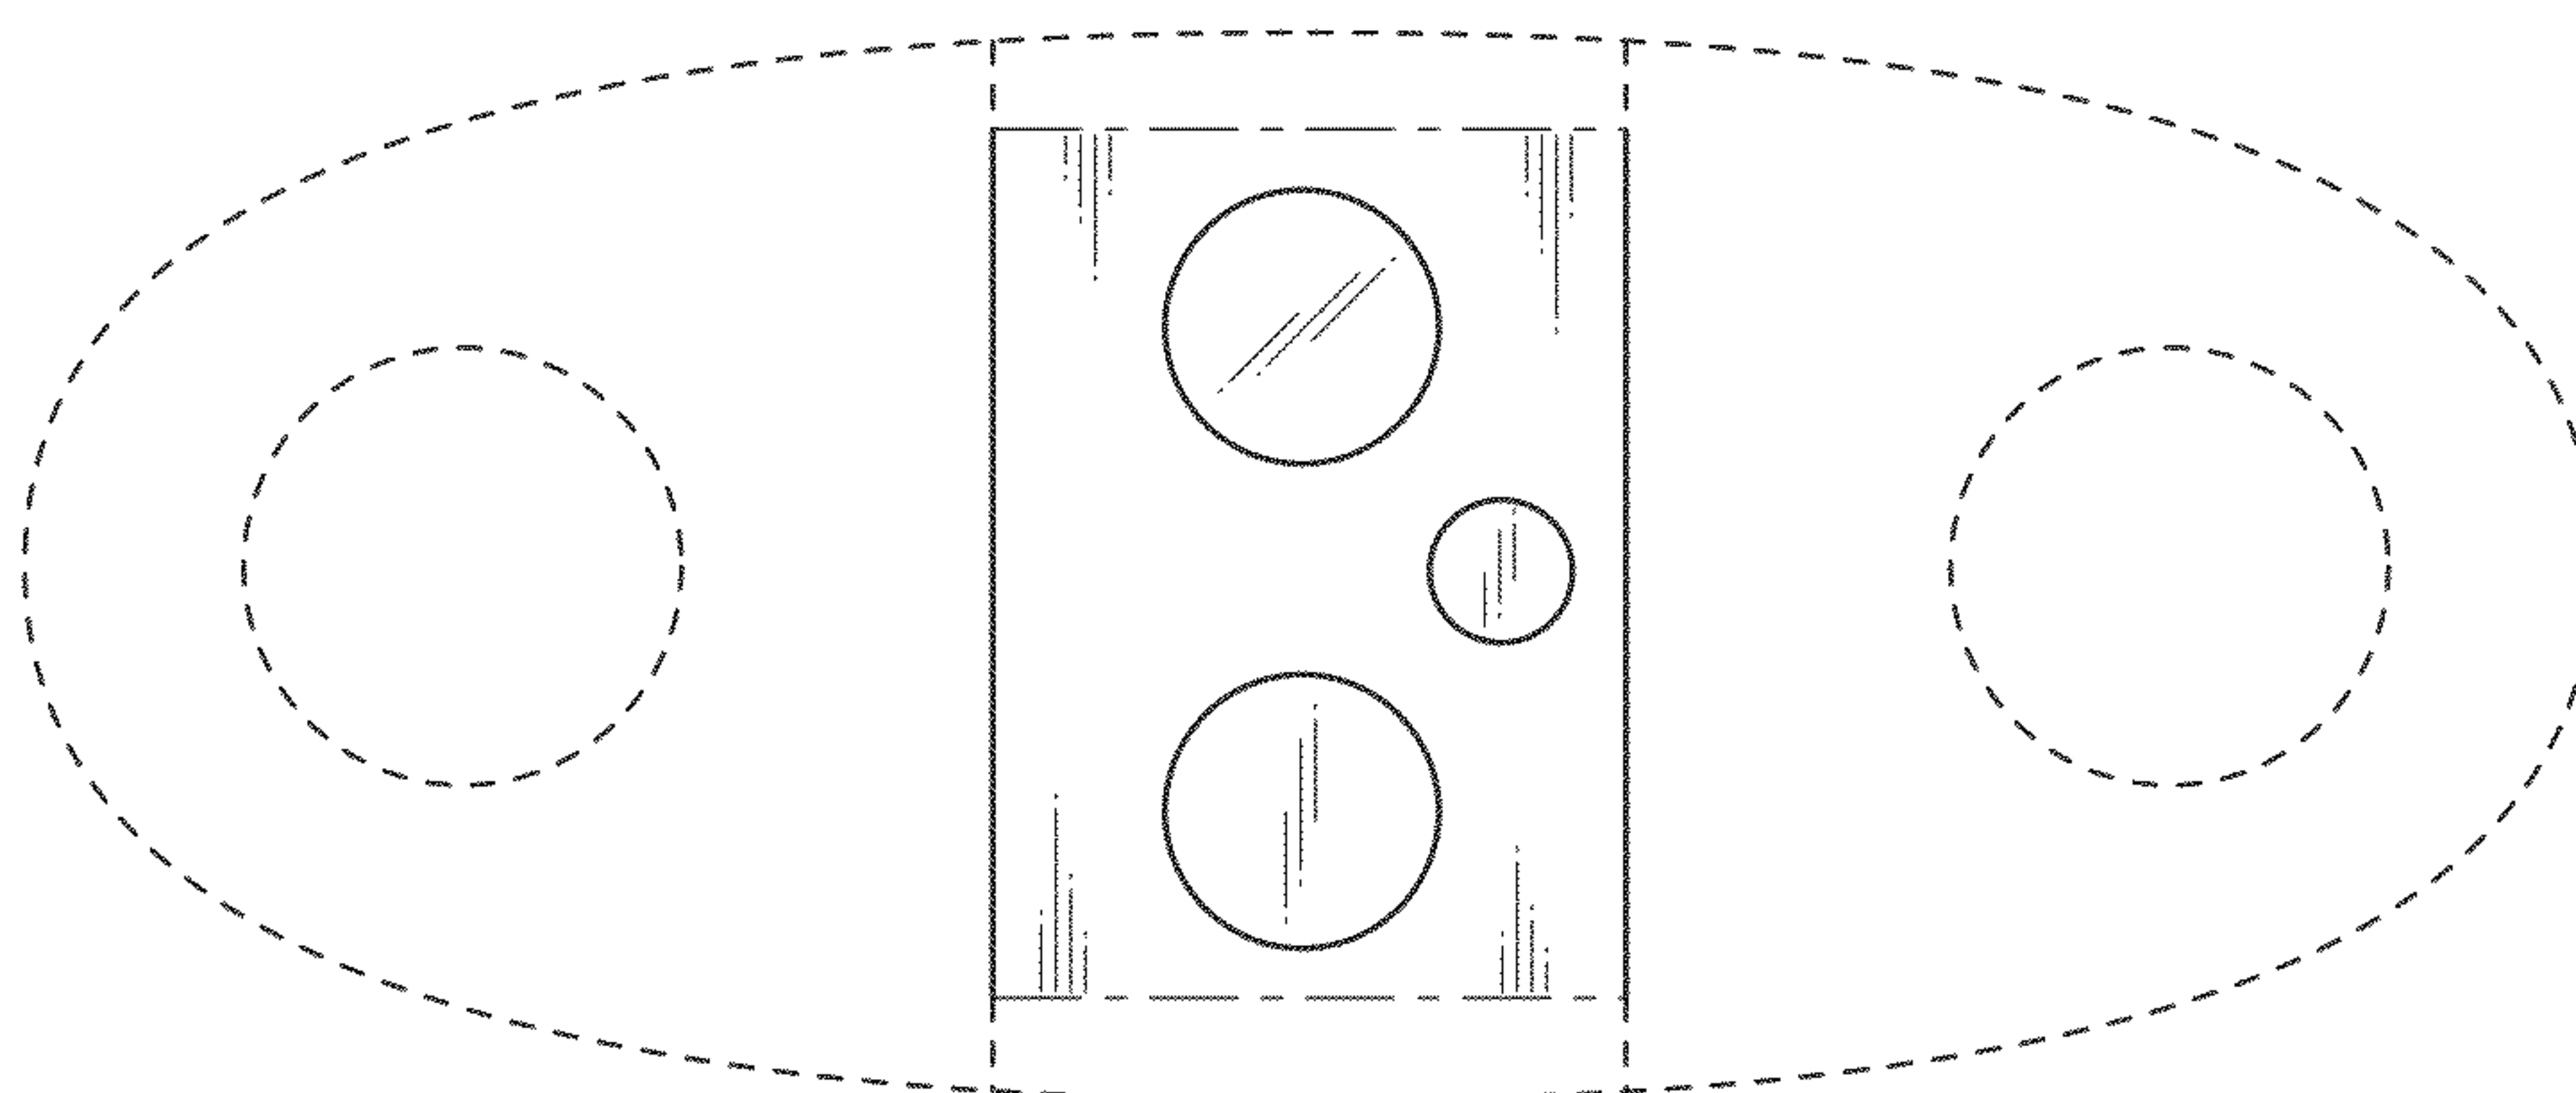


FIG. 4

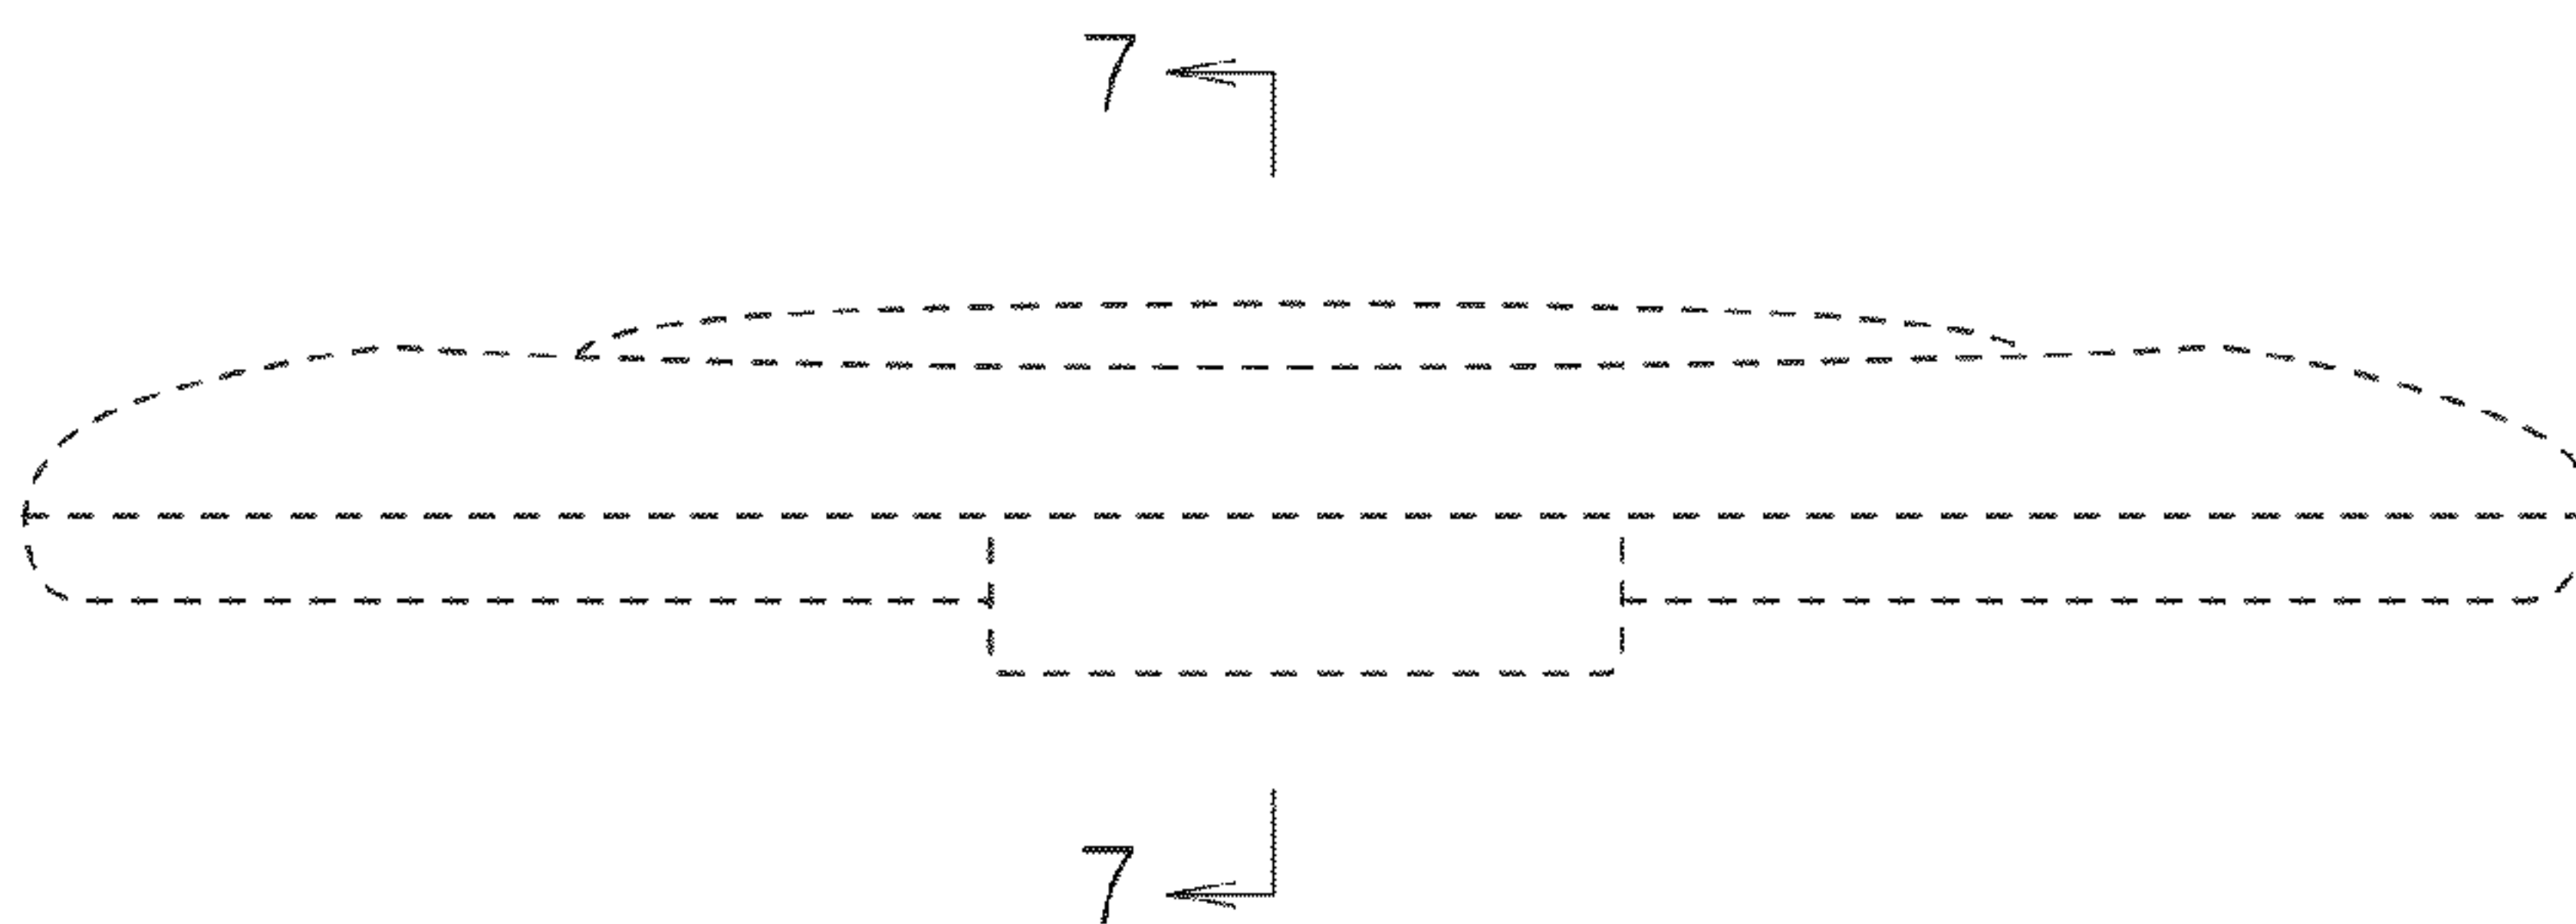


FIG. 5

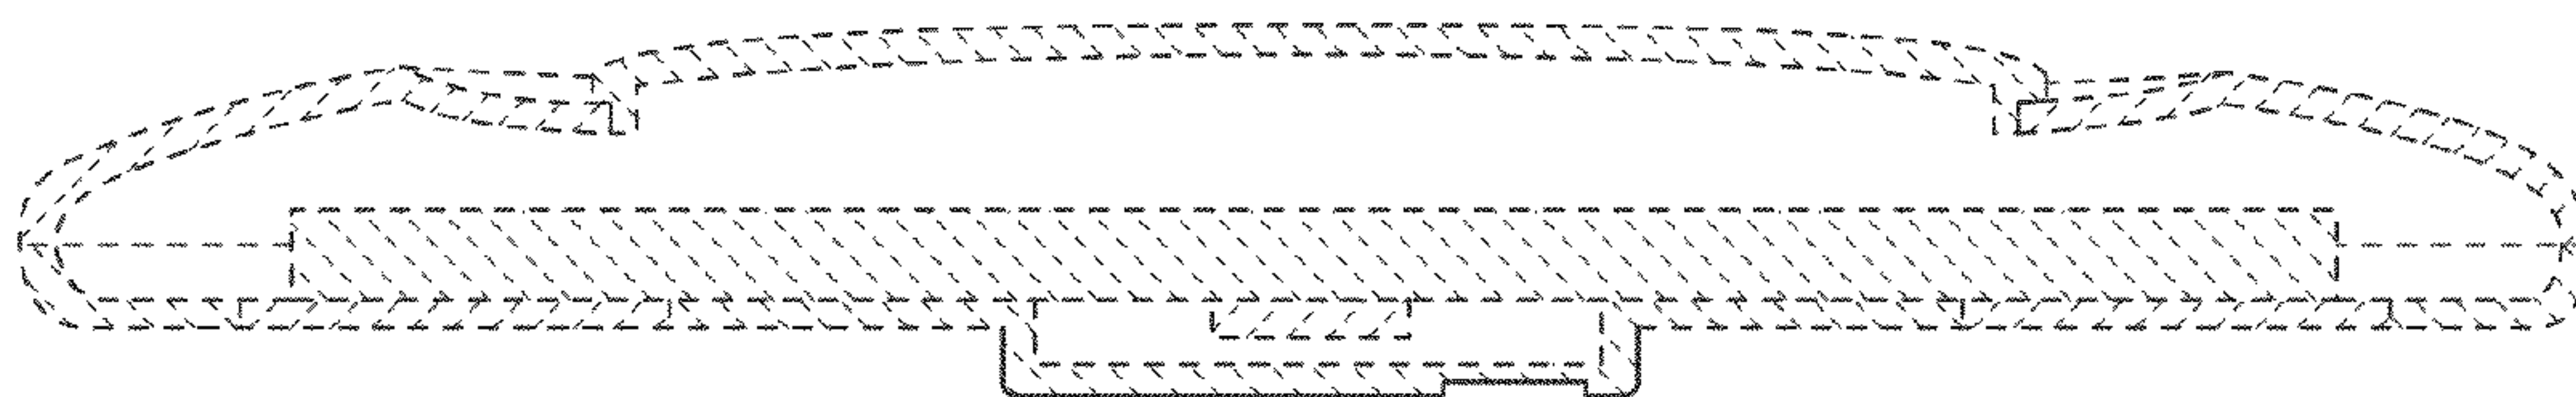


FIG. 6

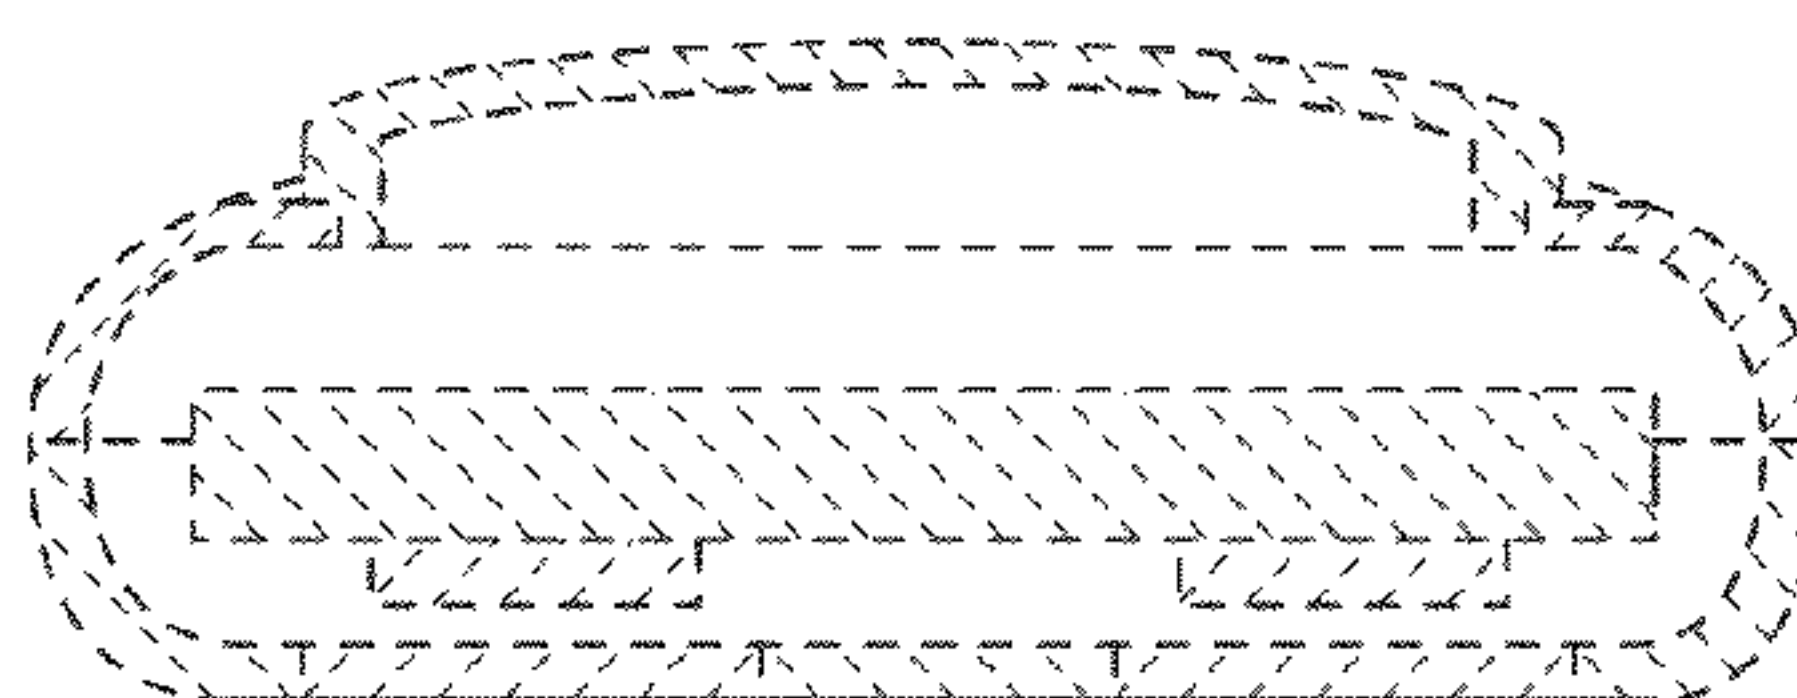


FIG. 7