



US00D741474S

(12) **United States Design Patent**
Chen et al.

(10) **Patent No.:** **US D741,474 S**
(45) **Date of Patent:** **** Oct. 20, 2015**

- (54) **SLEEP APNEA DEVICE ACCESSORY**
- (71) Applicant: **Fresca Medical, Inc.**, San Clemente, CA (US)
- (72) Inventors: **Eugene G. Chen**, Carlsbad, CA (US);
Alan M. Gordon, Del Mar, CA (US);
Samuel C. Wu, Cerritos, CA (US)
- (73) Assignee: **Fresca Medical, Inc.**, San Clemente, CA (US)
- (**) Term: **14 Years**
- (21) Appl. No.: **29/465,007**
- (22) Filed: **Aug. 22, 2013**
- (51) **LOC (10) Cl.** **29-02**
- (52) **U.S. Cl.**
USPC **D24/110.1**
- (58) **Field of Classification Search**
USPC D24/107, 110, 110.1, 110.2, 110.4,
D24/110.5, 127, 164, 173, 174; D14/205
CPC A61B 5/4818; A61M 16/06; A61M
16/0683; A61M 16/00; A61M 16/0666;
A61M 16/0672; A62B 9/00
See application file for complete search history.

- D397,334 S * 8/1998 Larian D14/372
- 6,421,031 B1 * 7/2002 Ronzani et al. 345/8
- D469,753 S * 2/2003 Andre et al. D14/205
- 6,526,974 B1 3/2003 Brydon et al.
- 6,729,726 B2 * 5/2004 Miller et al. 351/158
- 7,202,774 B2 * 4/2007 Hoyle 340/309.16
- D566,687 S * 4/2008 Duarte et al. D14/205
- D568,291 S * 5/2008 Andre et al. D14/205

(Continued)

FOREIGN PATENT DOCUMENTS

- EP 1893267 A1 11/2011
- EP 2287471 B1 6/2012
- EP 2530327 A2 12/2012

OTHER PUBLICATIONS

CPAP Systems and Accessories: Comfort Accuracy and High Flows. Vital Signs, Inc. General Electric Healthcare Company. 2009, 2 pages.

(Continued)

Primary Examiner — Deanna L Pratt
Assistant Examiner — Lilyana Bekic
(74) *Attorney, Agent, or Firm* — Manuel de la Cerra

(57) **CLAIM**
The ornamental design for sleep apnea device accessory, as shown and described herein.


DESCRIPTION

FIG. 1 is a perspective view of the sleep apnea device accessory showing our design;
FIG. 2 is a front elevation view thereof;
FIG. 3 is a rear elevation view thereof;
FIG. 4 is a left-side elevation view thereof;
FIG. 5 is a right-side elevation view thereof;
FIG. 6 is a top plan view thereof;
FIG. 7 is a bottom plan view thereof; and,
FIG. 8 is a partially-exploded, perspective view thereof.

1 Claim, 8 Drawing Sheets

(56) **References Cited**
U.S. PATENT DOCUMENTS

- 2,395,297 A * 2/1946 Shock, Jr. 2/447
- 2,537,768 A * 1/1951 Laporte 2/15
- 2,874,385 A * 2/1959 Wade 2/15
- 4,122,847 A * 10/1978 Craig 128/858
- 4,411,263 A * 10/1983 Cook 128/858
- 4,777,937 A * 10/1988 Rush et al. 600/27
- 4,779,291 A * 10/1988 Russell 2/439
- D309,465 S * 7/1990 Russell D16/312
- 5,106,179 A * 4/1992 Kamaya et al. 351/158
- 5,276,471 A * 1/1994 Yamauchi et al. 351/153
- 5,567,127 A 10/1996 Wentz
- 5,649,533 A 7/1997 Oren

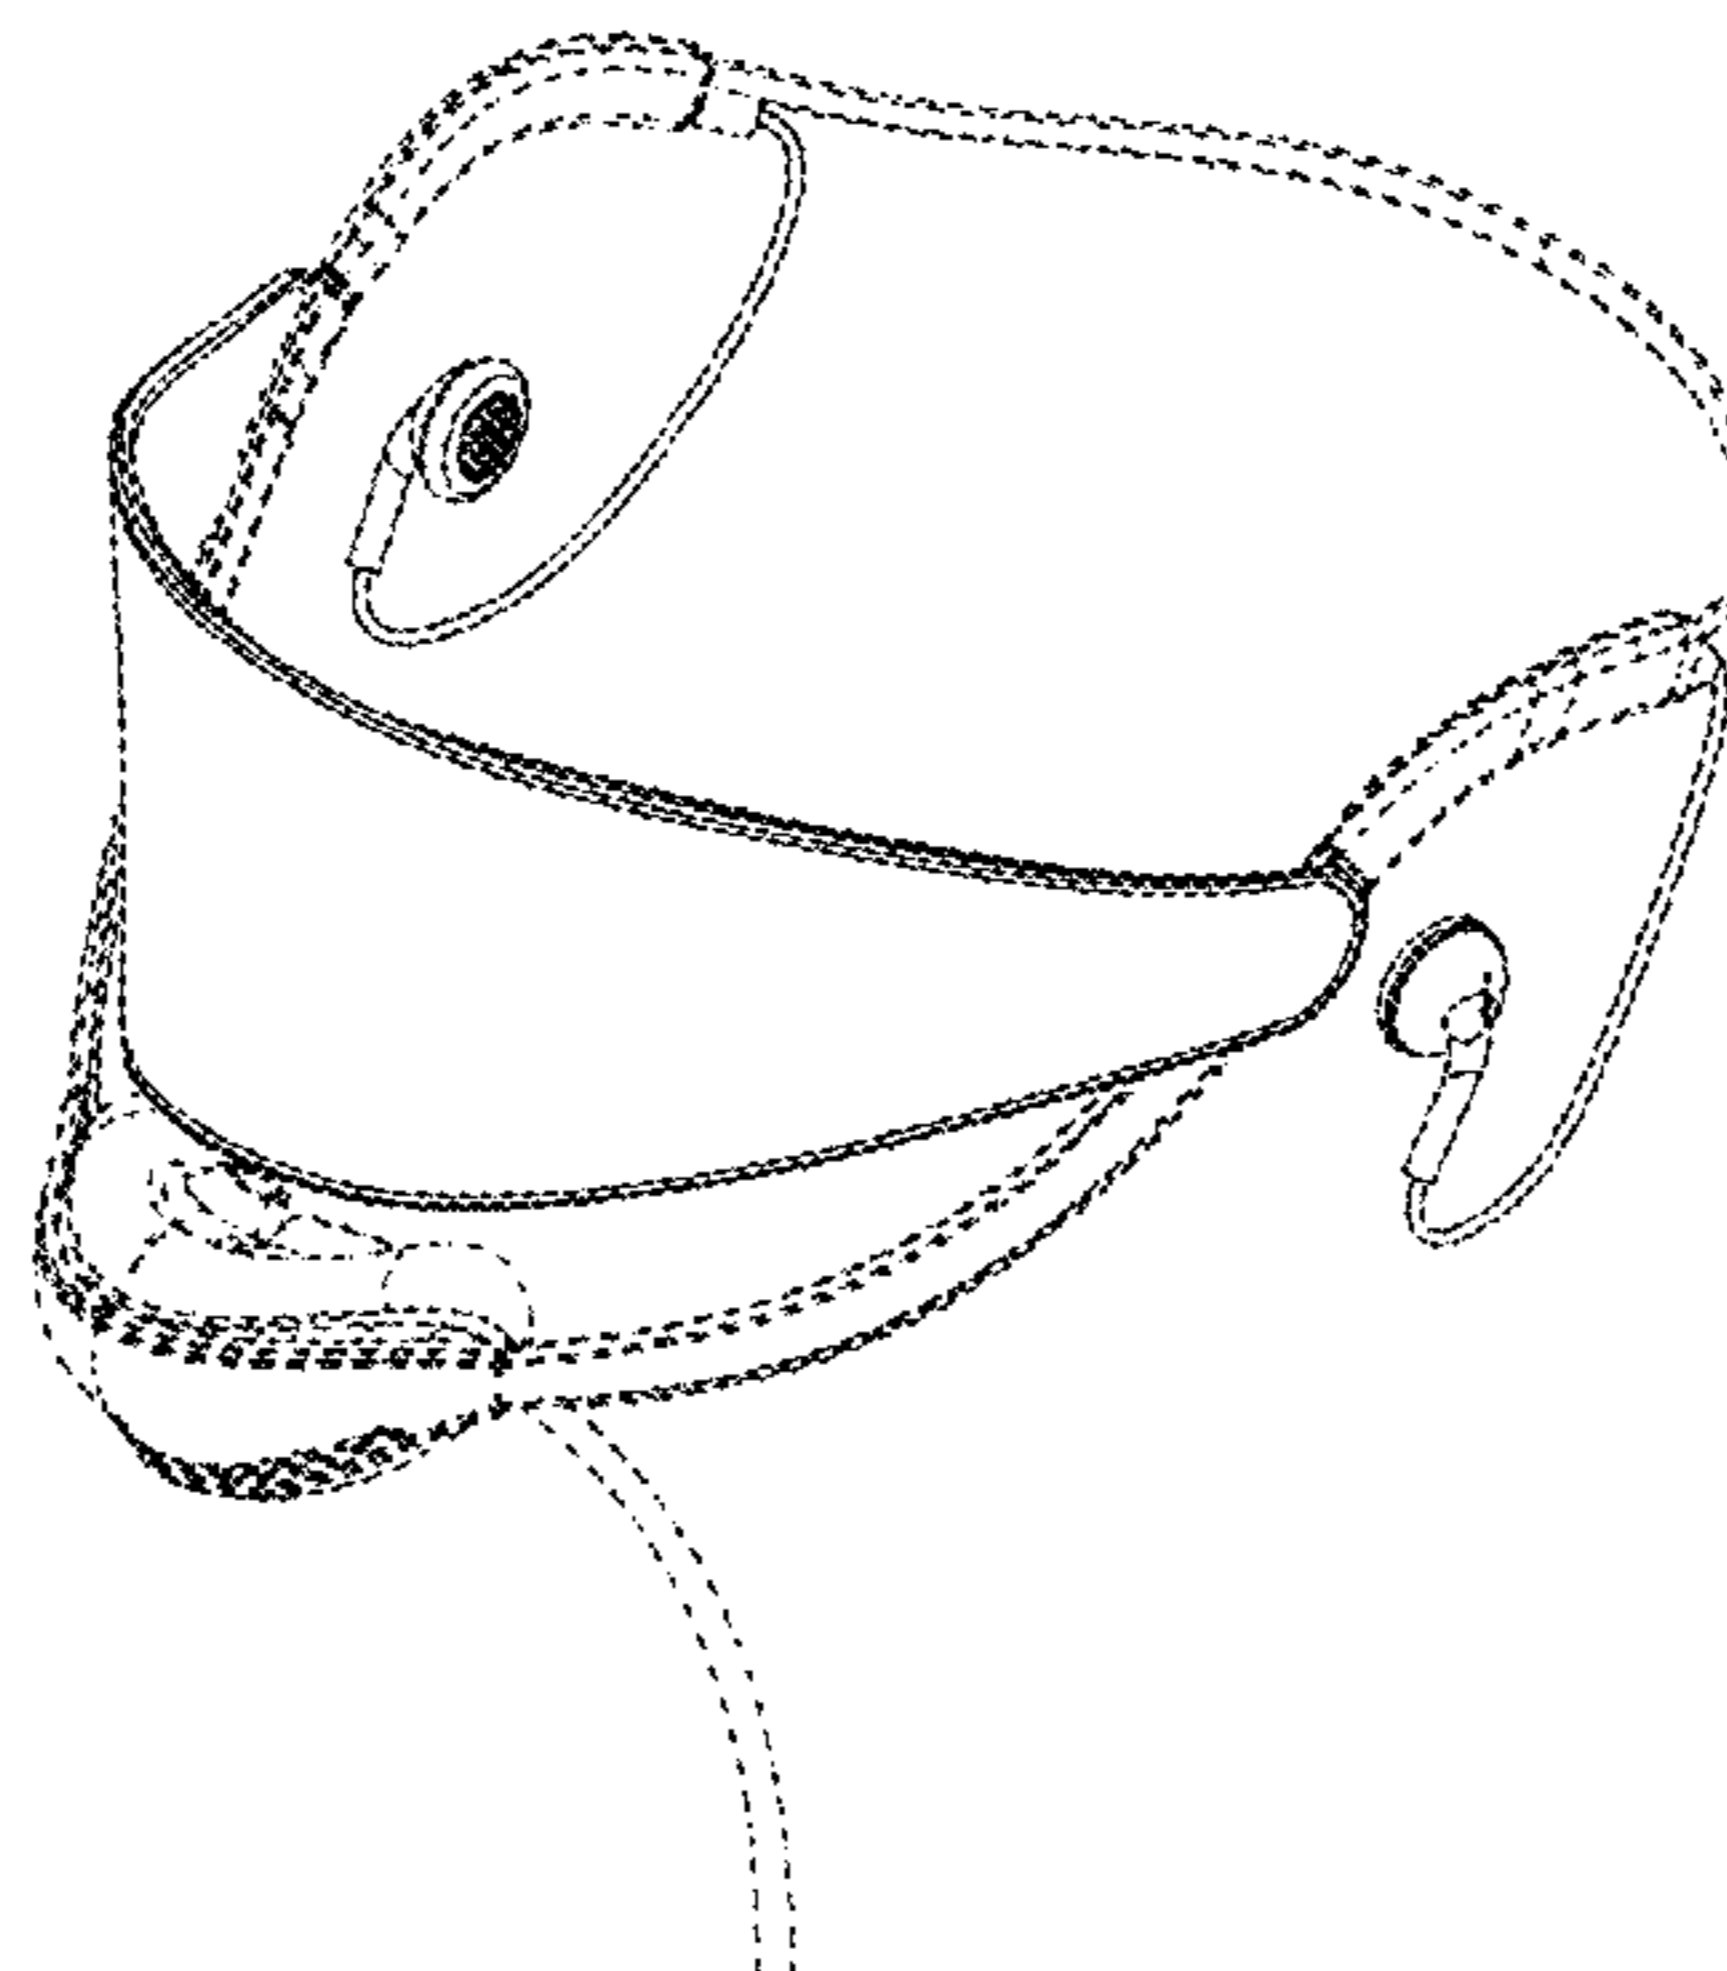

(56)

References Cited

U.S. PATENT DOCUMENTS

D587,243	S *	2/2009	Suzuki	D14/205
D587,677	S *	3/2009	Andre et al.	D14/205
D589,491	S *	3/2009	Andre et al.	D14/205
7,527,055	B2	5/2009	McAuliffe et al.		
D593,538	S *	6/2009	Chon et al.	D14/205
D594,442	S *	6/2009	Chon et al.	D14/205
7,603,723	B2 *	10/2009	Ulm	2/15
7,677,734	B2 *	3/2010	Wallace	353/18
7,735,492	B2	6/2010	Doshi et al.		
7,740,353	B2 *	6/2010	Jannard	351/158
7,806,120	B2	10/2010	Loomas et al.		
7,856,979	B2	12/2010	Doshi et al.		
D636,756	S *	4/2011	Fahrendorff et al.	D14/205
D637,295	S *	5/2011	McCartney	D24/174
7,992,564	B2	8/2011	Doshi et al.		
8,122,884	B2	2/2012	Daly et al.		
D656,481	S *	3/2012	McManigal	D14/205
D659,673	S *	5/2012	Fahrendorff et al.	D14/205
D662,079	S *	6/2012	Fahrendorff et al.	D14/205
8,215,308	B2	7/2012	Doshi et al.		
8,235,046	B2	8/2012	Doshi et al.		
8,240,309	B2	8/2012	Doshi et al.		
8,243,973	B2 *	8/2012	Rickards et al.	381/327
8,337,145	B2	12/2012	Frater et al.		
8,368,794	B2 *	2/2013	Sako et al.	348/333.01
D677,240	S *	3/2013	Coulter	D14/205
D706,745	S *	6/2014	Nakagawa	D14/205
D719,929	S *	12/2014	Rye et al.	D14/205
D731,999	S *	6/2015	Cepress et al.	D14/205
2003/0068057	A1 *	4/2003	Miller et al.	381/334
2005/0219152	A1 *	10/2005	Budd et al.	345/8
2005/0256675	A1 *	11/2005	Kurata	702/153
2007/0116318	A1 *	5/2007	Rickards	381/374

OTHER PUBLICATIONS

Deegan, P., et al. Effects of positive airway pressure on upper airway dilator muscle activity and ventilatory timing. *Journal of Applied Physiol.* Jul. 1996; 81(1): 470-9.

Duncan, A., et al. PEEP and CPAP. *Anaesth Intensive Care.* Aug. 1986; 14(3): 236-50.

Garrard, C., et al. The effects of expiratory positive airway pressure on functional residual capacity in normal subjects. *Crit Care Med.* Sep.-Oct. 1978; 6(5): 320-2.

Gillick, JS. Spontaneous positive end-expiratory pressure (sPEEP). *Anesthesia & Analgesia.* Sep.-Oct. 1977; 56(5): 627-32. PubMed PMID: 333990.

Heinzer R, et al. Effect of expiratory positive airway pressure on sleep disordered breathing. *Sleep.* Mar. 2008; 31(3): 429-32.

Juhász, J. et al. Proportional positive airway pressure: a new concept to treat obstructive sleep apnoea. *European Respiratory Journal.* 2001; 17: 467-473.

Layon, J., et al. Continuous positive airway pressure and expiratory positive airway pressure increase functional residual capacity equivalently. *Chest.* Apr. 1986;89(4):517-21.

Resta, O., et al. The role of the expiratory phase in obstructive sleep apnoea. *Respir Med.* Mar. 1999;93(3):190-5.

Sanders, M., et al. Obstructive sleep apnea treated by independently adjusted inspiratory and expiratory positive airway pressures via nasal mask. Physiologic and clinical implications. *Chest.* Aug. 1990; 98(2): 317-24.

Schlobohm, R., et al. Lung volumes, mechanics, and oxygenation during spontaneous positive-pressure ventilation: the advantage of CPAP over EPAP. *Anesthesiology.* Oct. 1981;55(4):416-22.

Schmidt, G., et al. EPAP without intubation. *Crit Care Med.* Jul.-Aug. 1977; 5(4): 207-9.

Sériès, F., et al. Changes in upper airway resistance with lung inflation and positive airway pressure. *American Physiological Society.* Mar. 1990; 68(3): 1075-1079.

Sturgeon, C. Jr, et al. PEEP and CPAP: cardiopulmonary effects during spontaneous ventilation. *Anesth Analg.* Sep.-Oct. 1977; 56(5):633-41. PubMed PMID: 20822.

Tummons, J. A positive end-expiratory pressure-nasal-assist device (PEEP-NAD) for treatment of respiratory distress syndrome. *Anesthesiology.* Jun. 1973; 38(6):592-5.

* cited by examiner

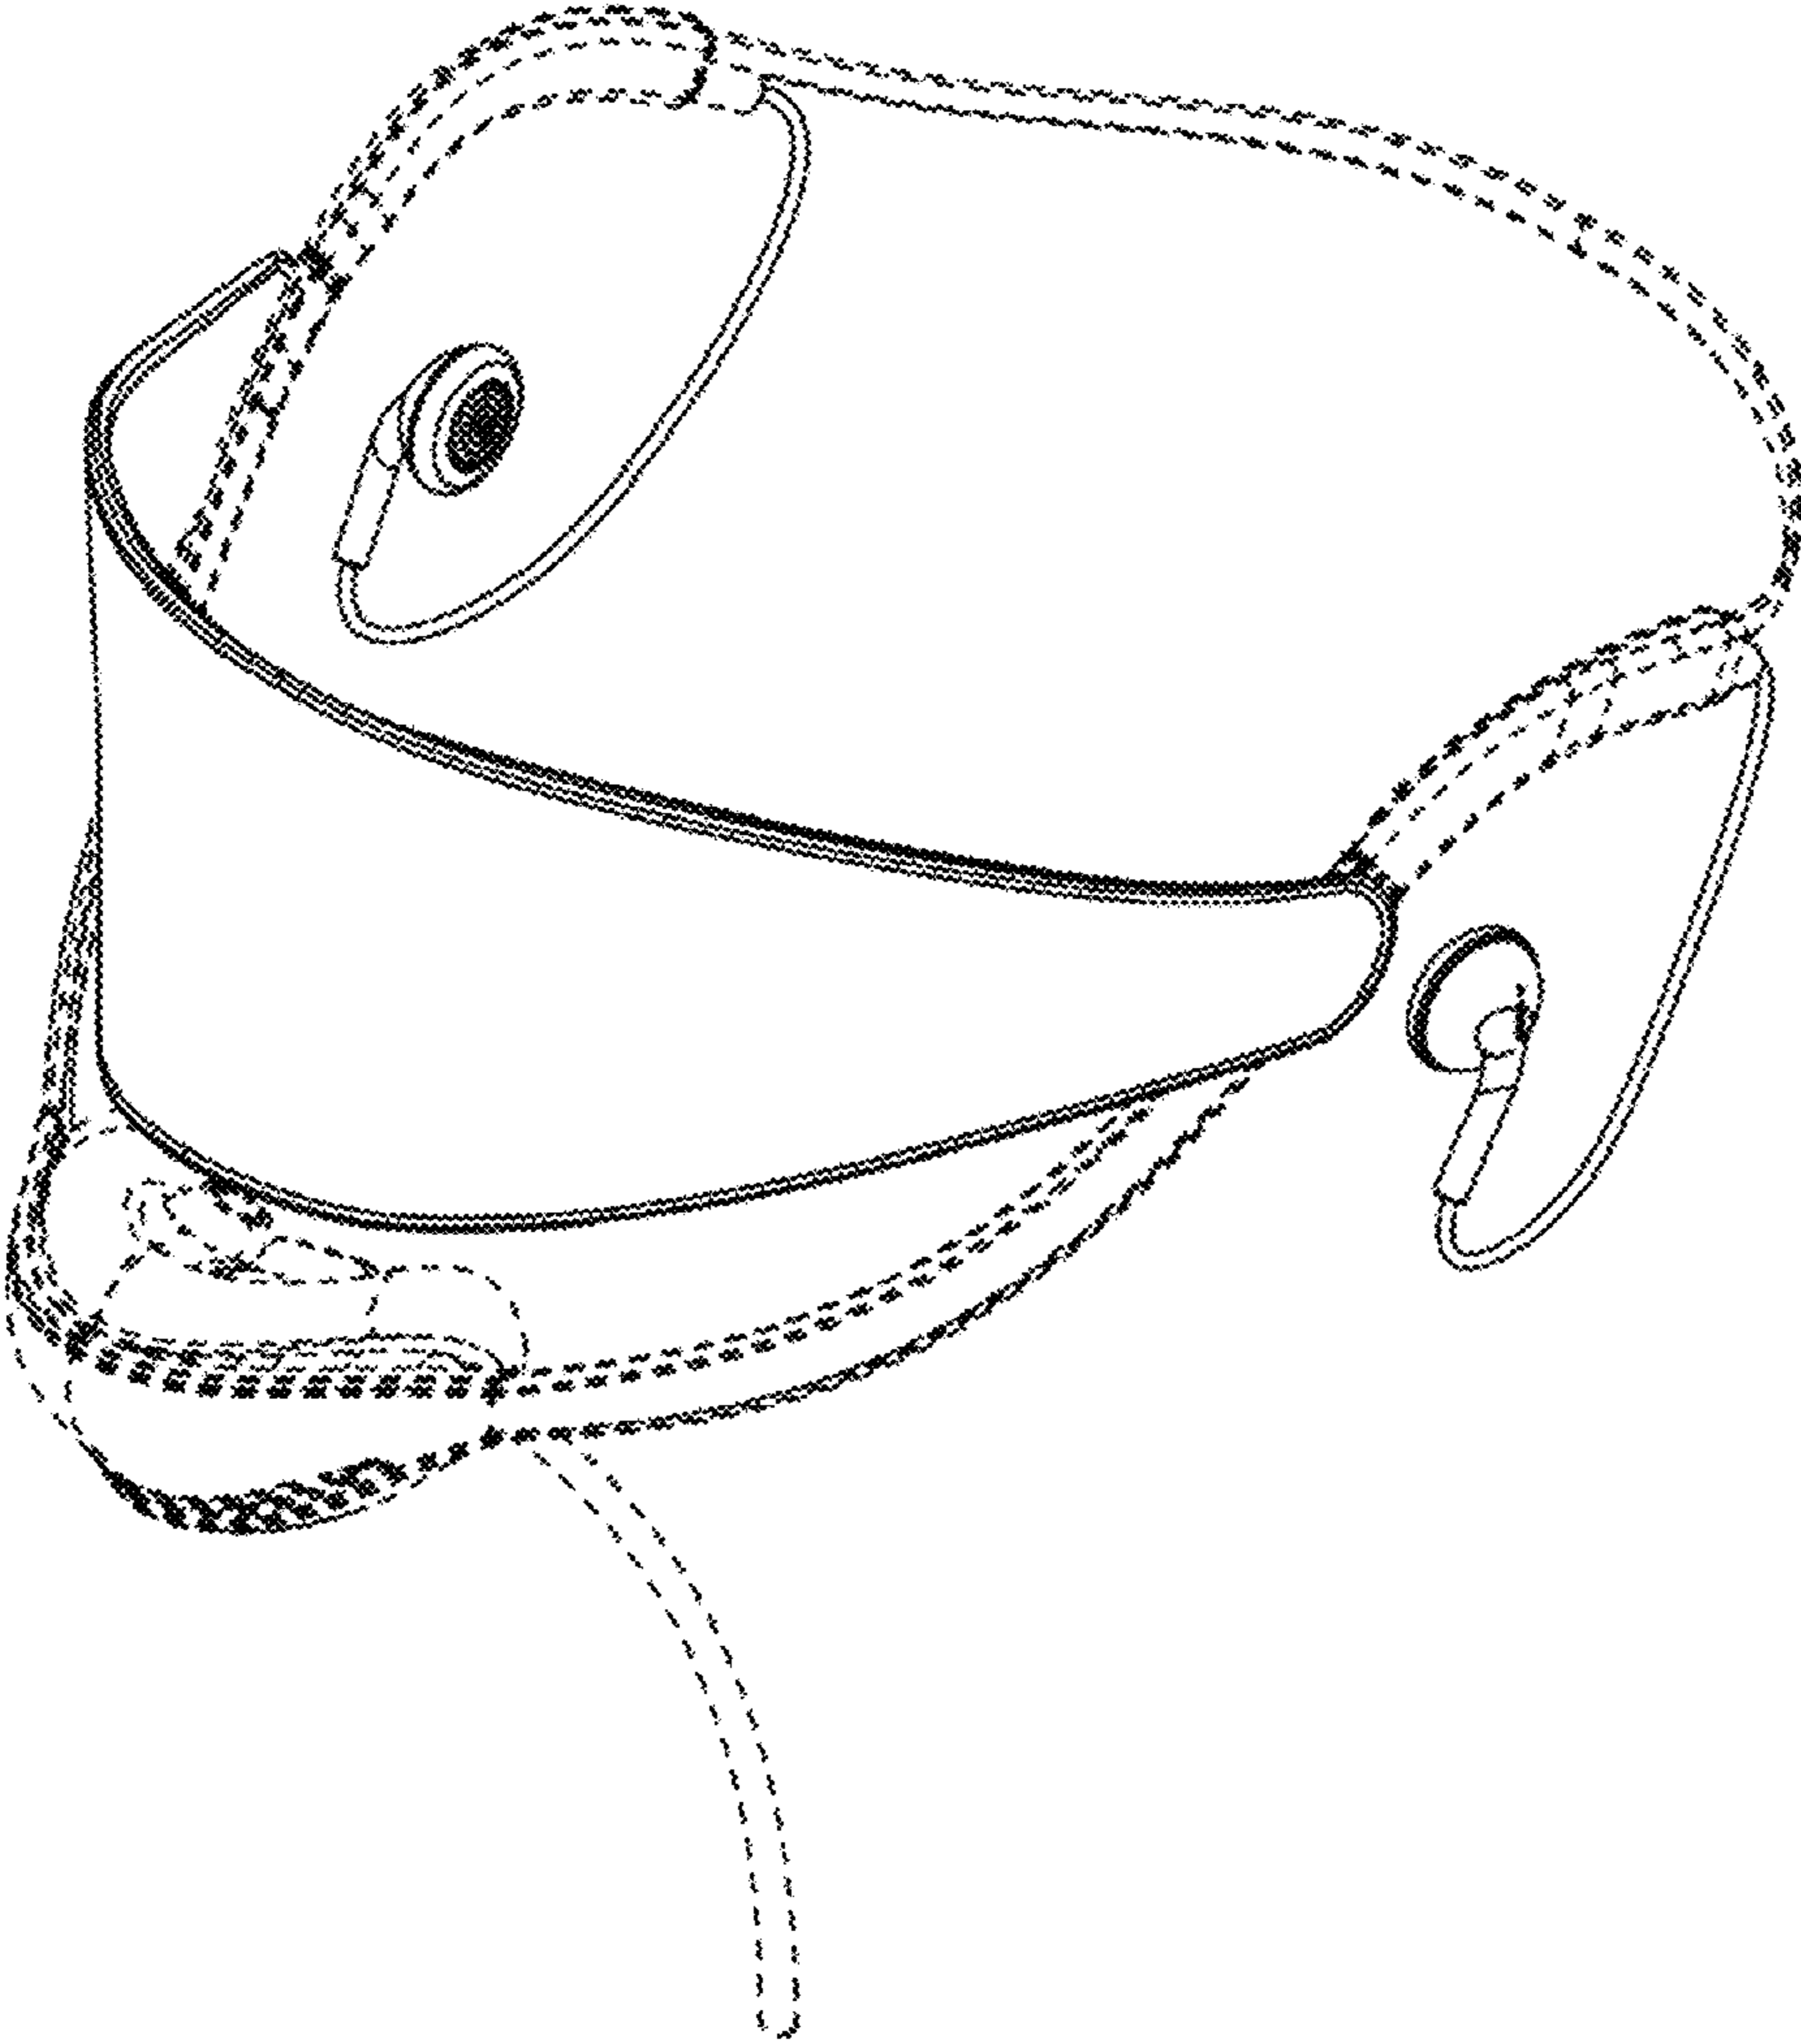


FIG. 1

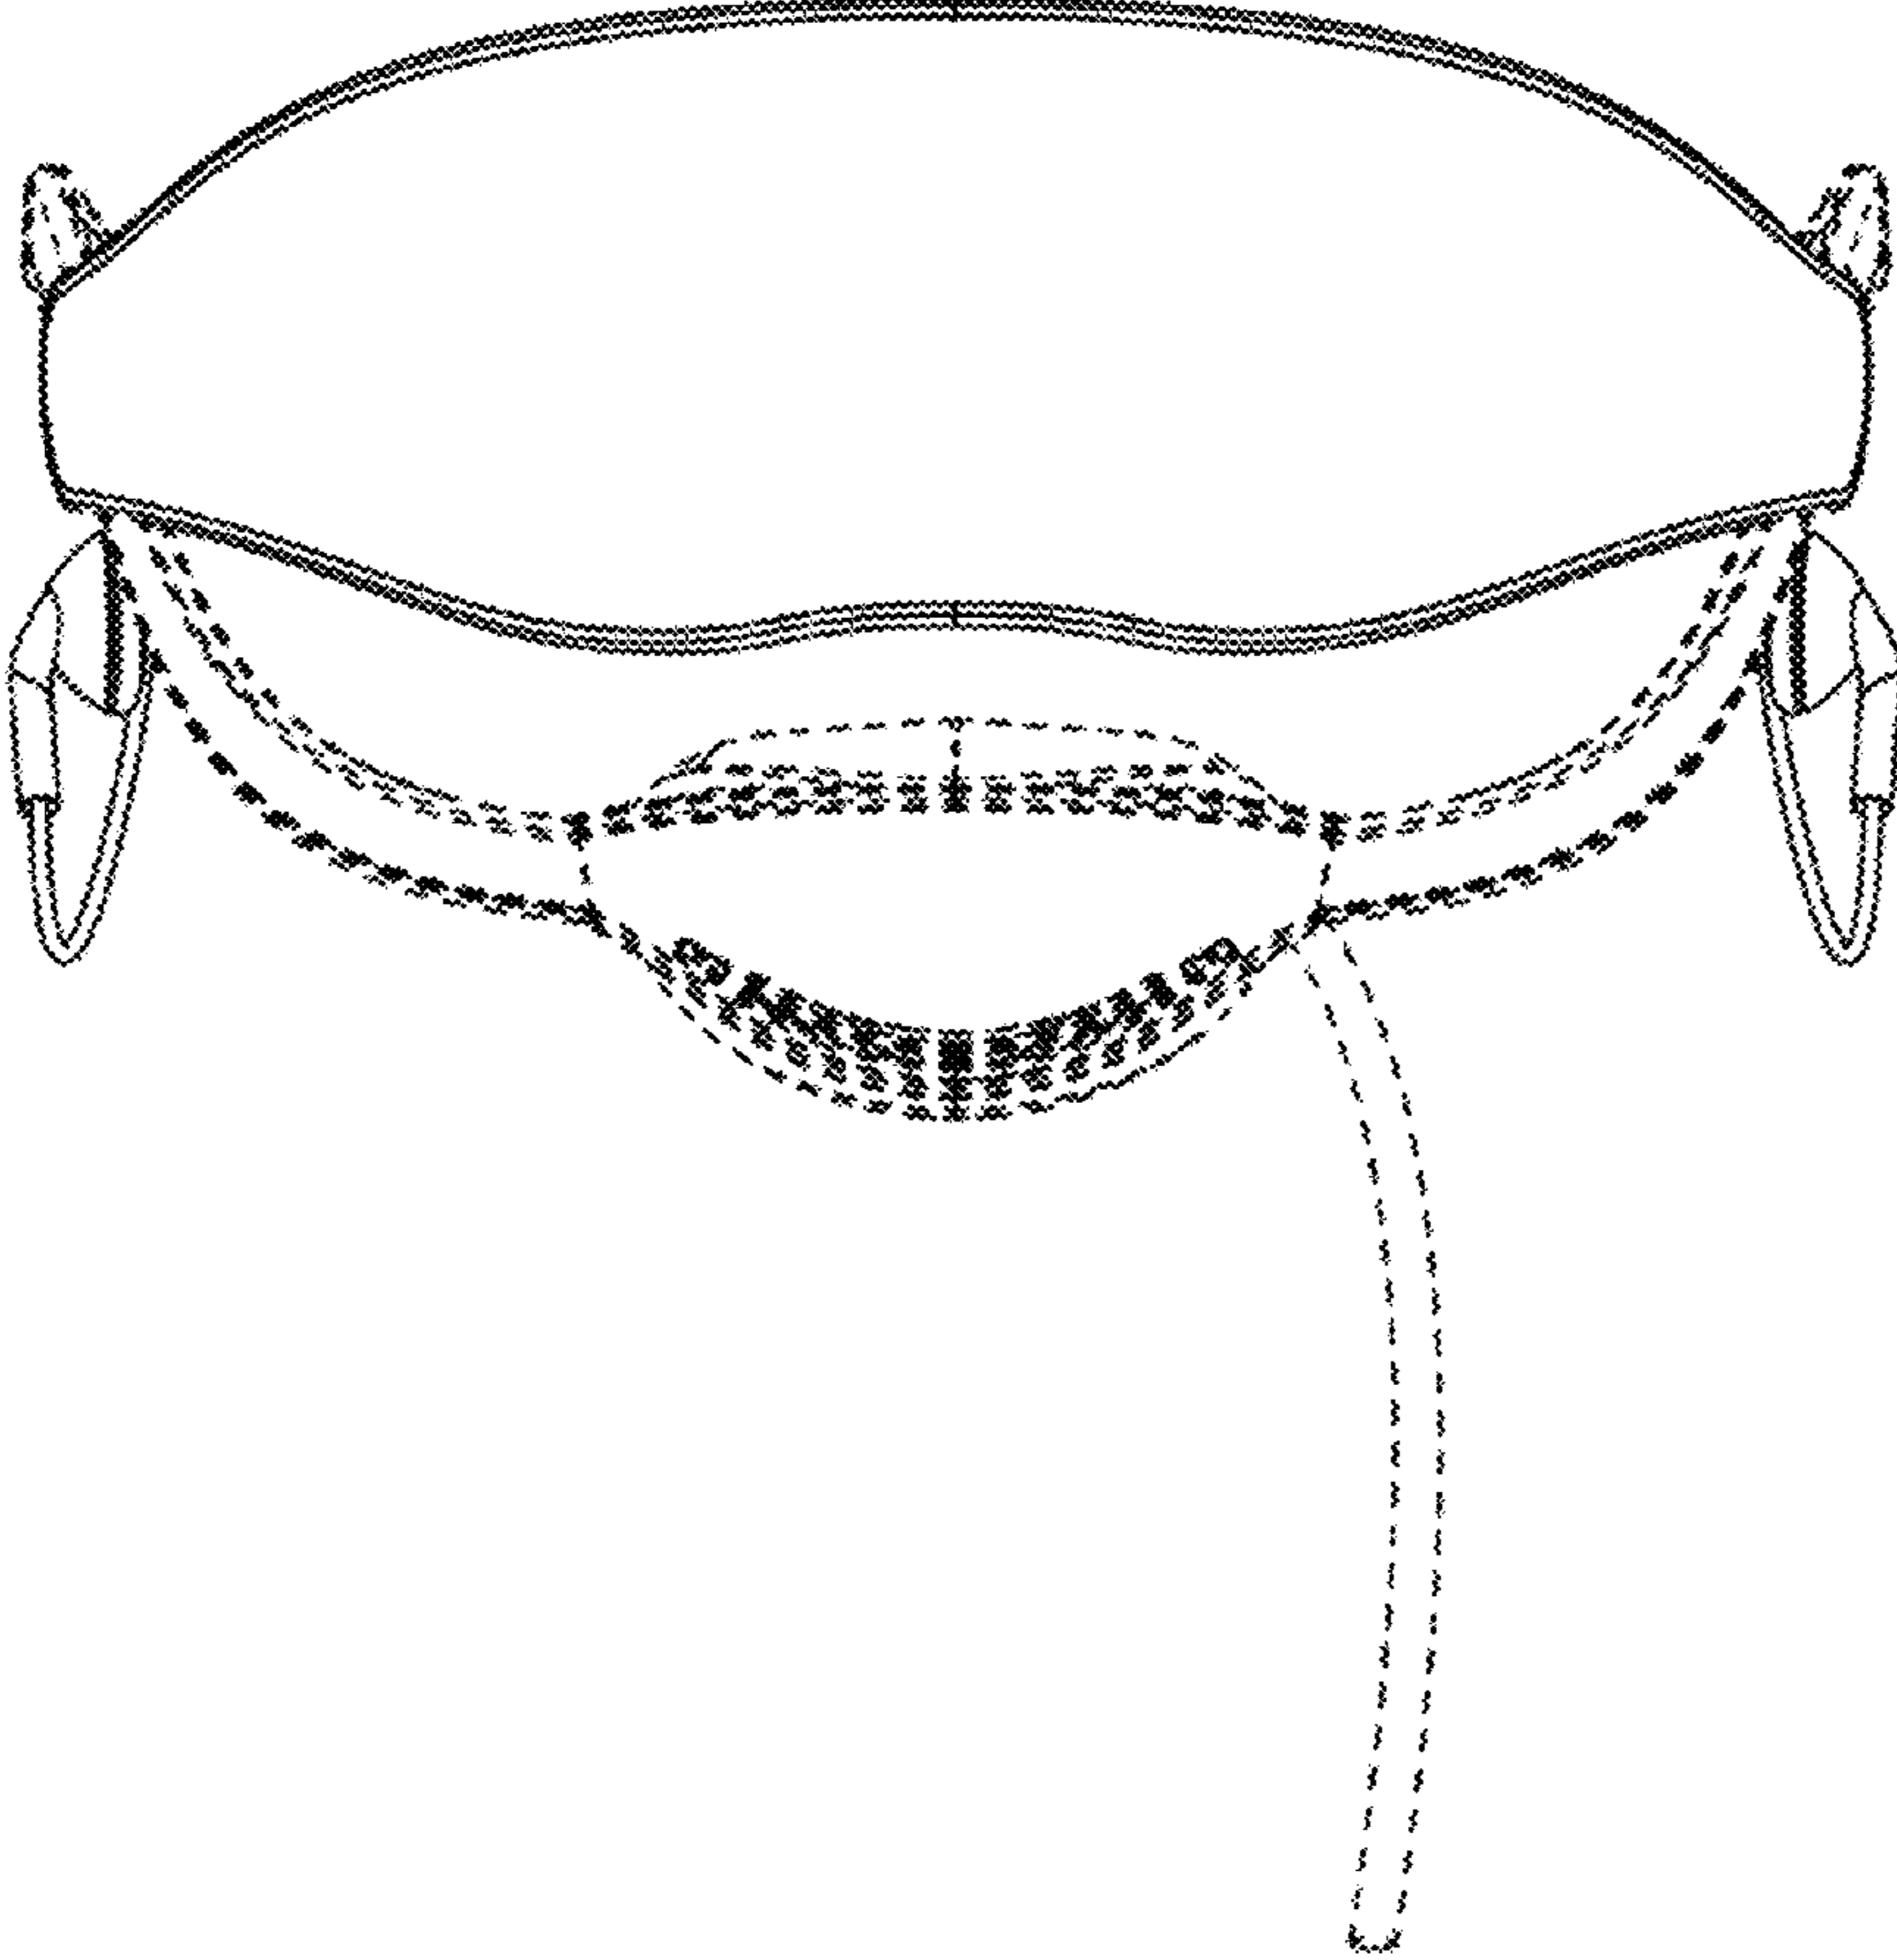


FIG. 2

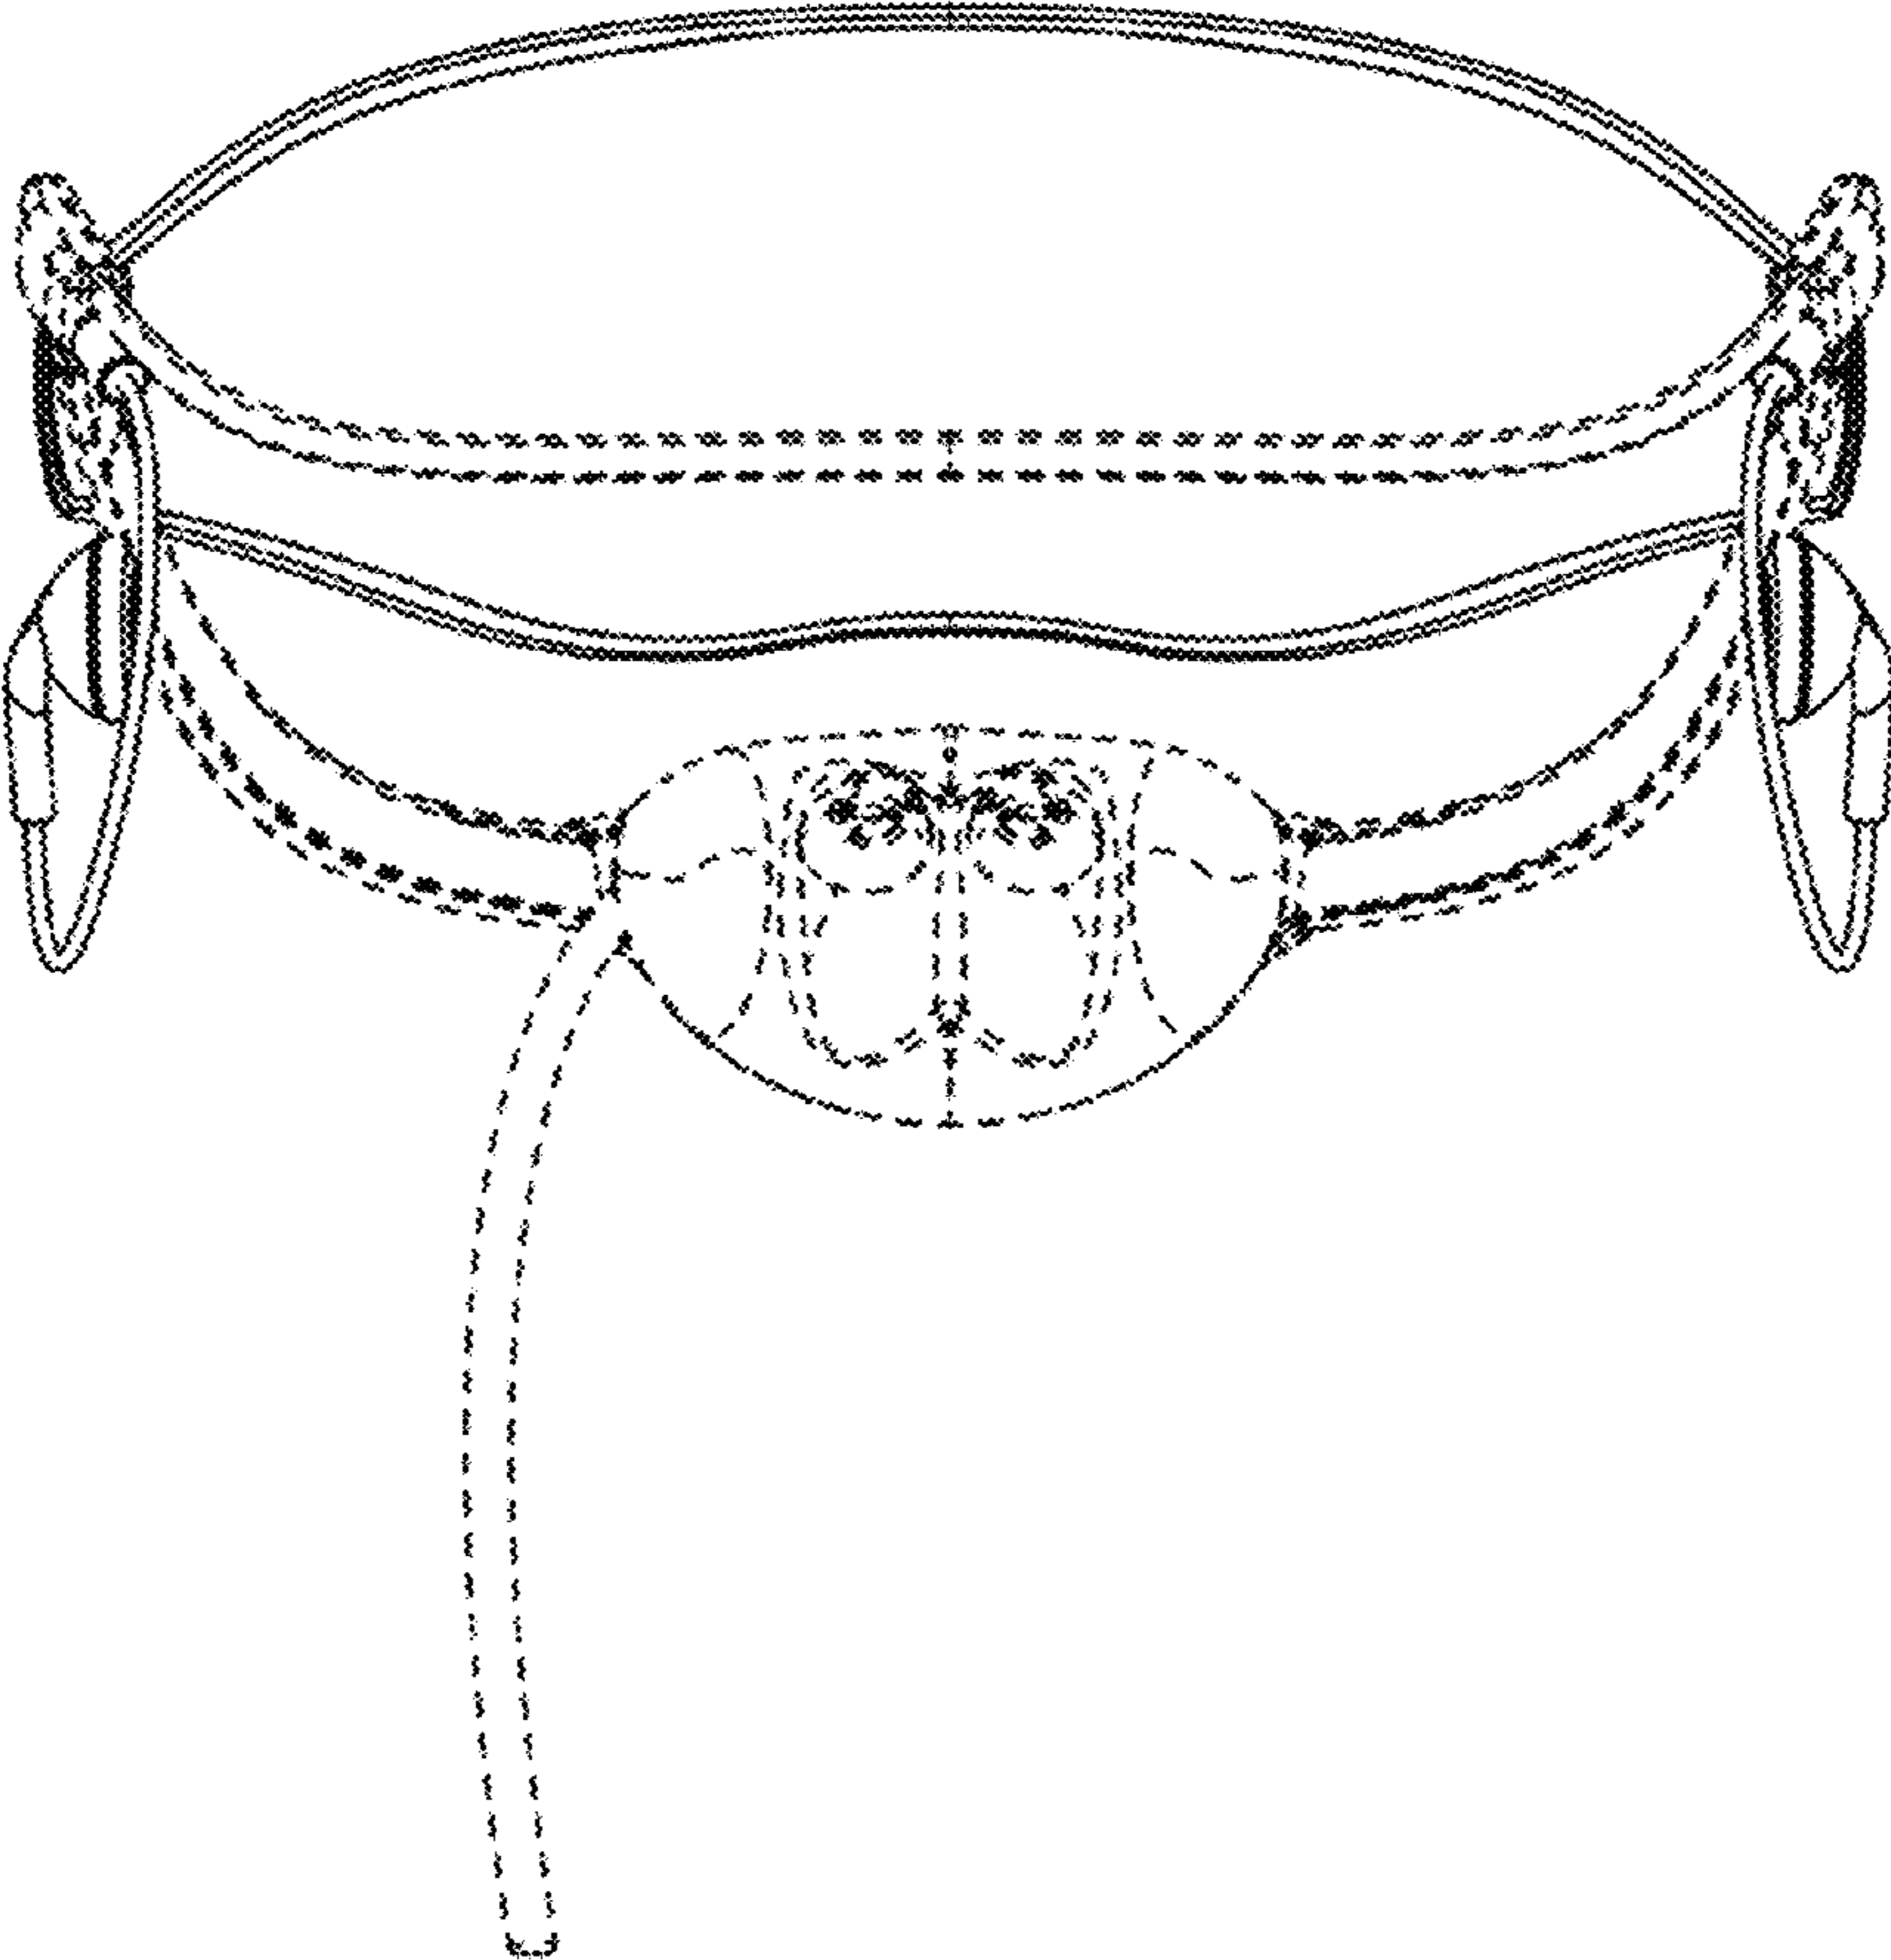


FIG. 3

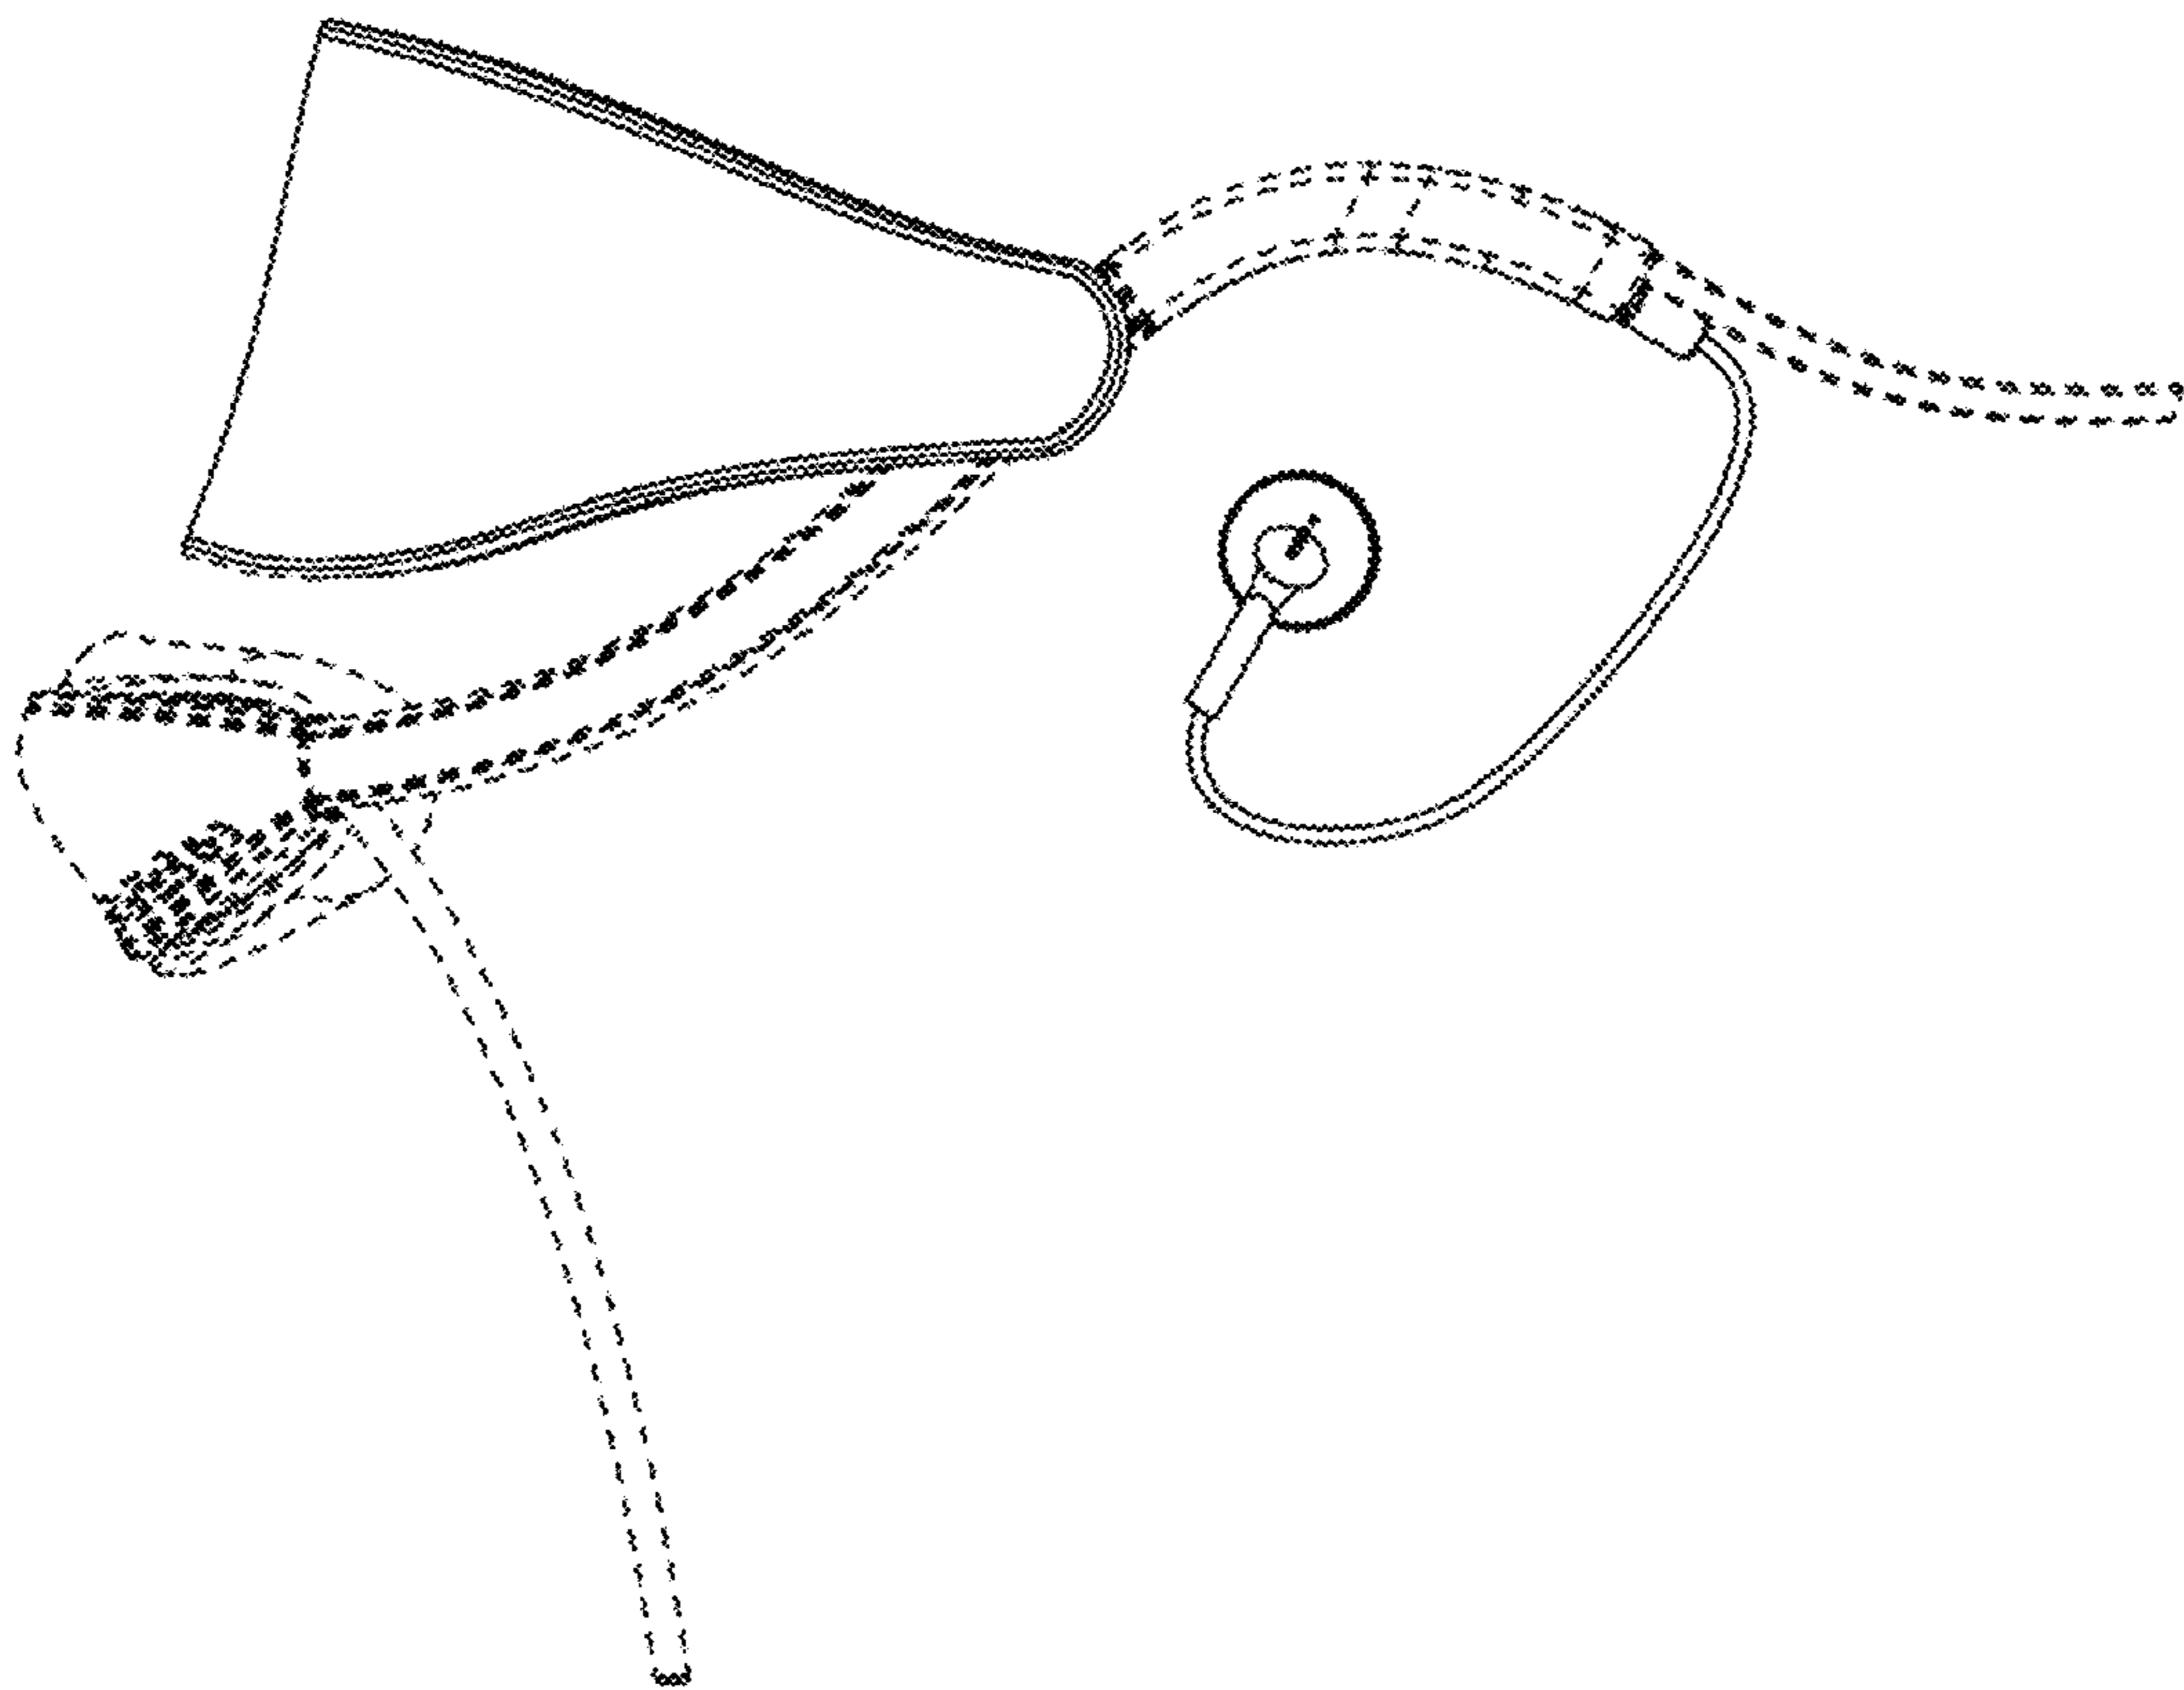


FIG. 4

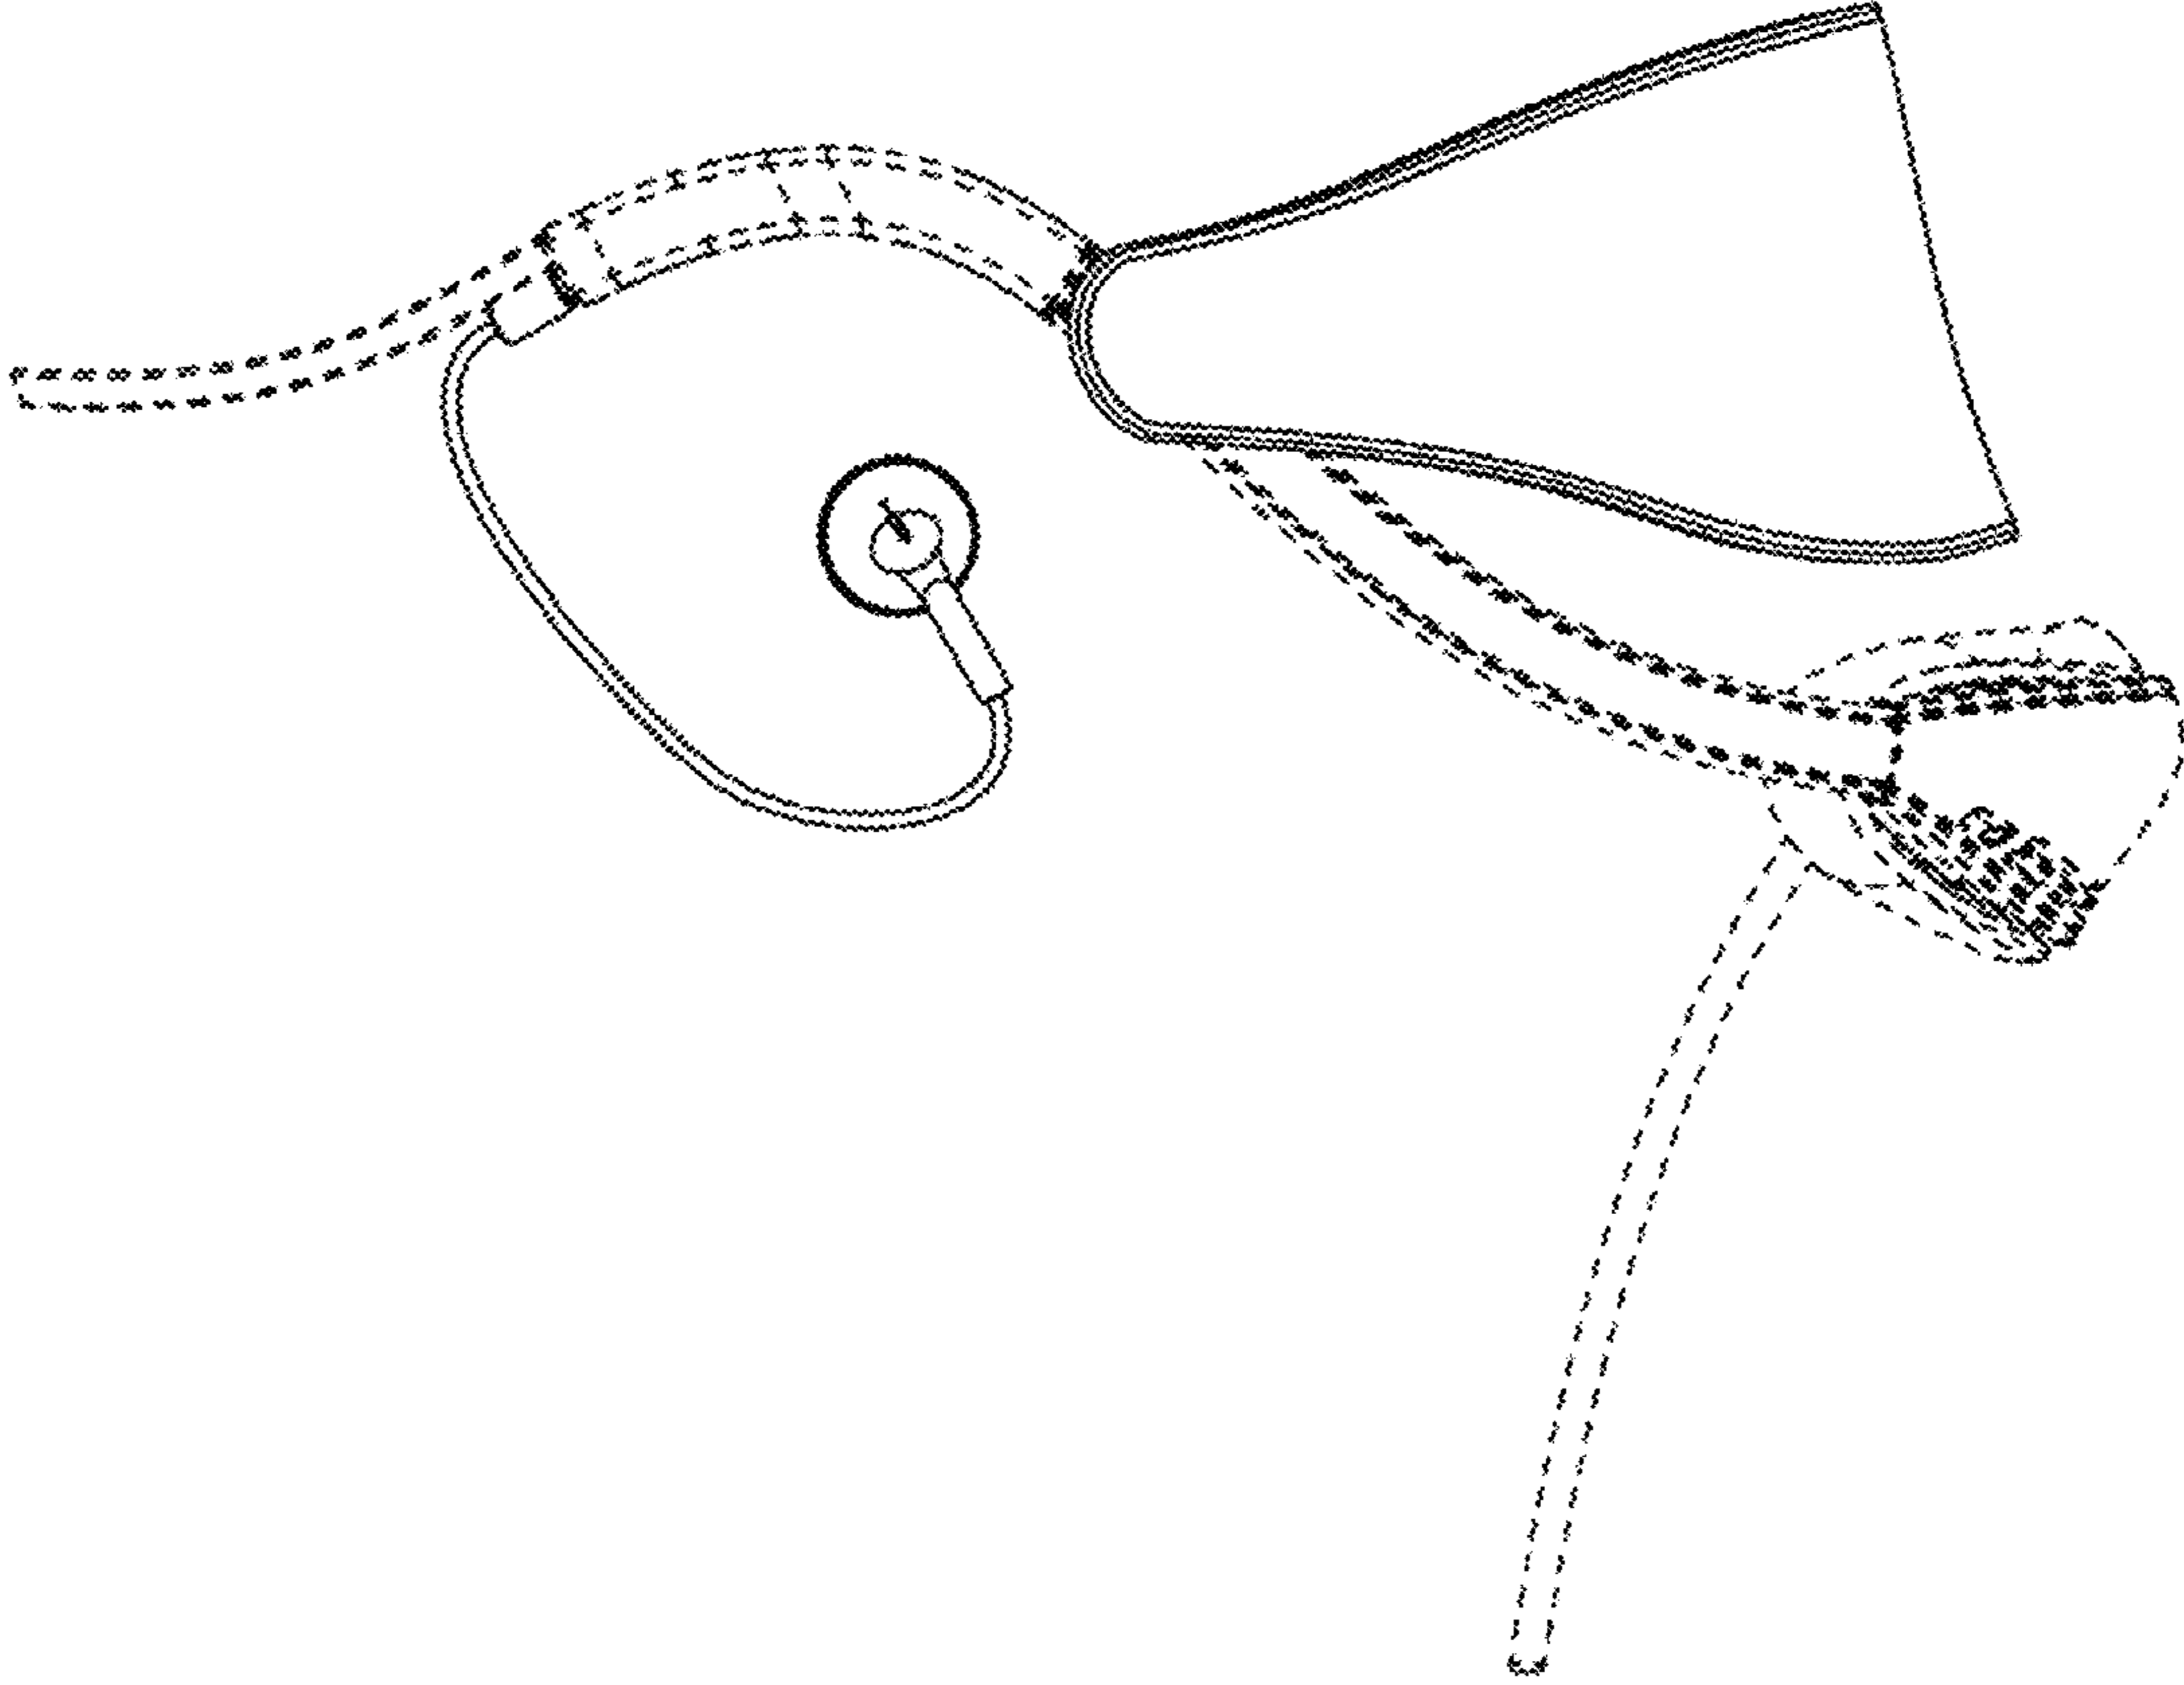


FIG. 5



FIG. 6

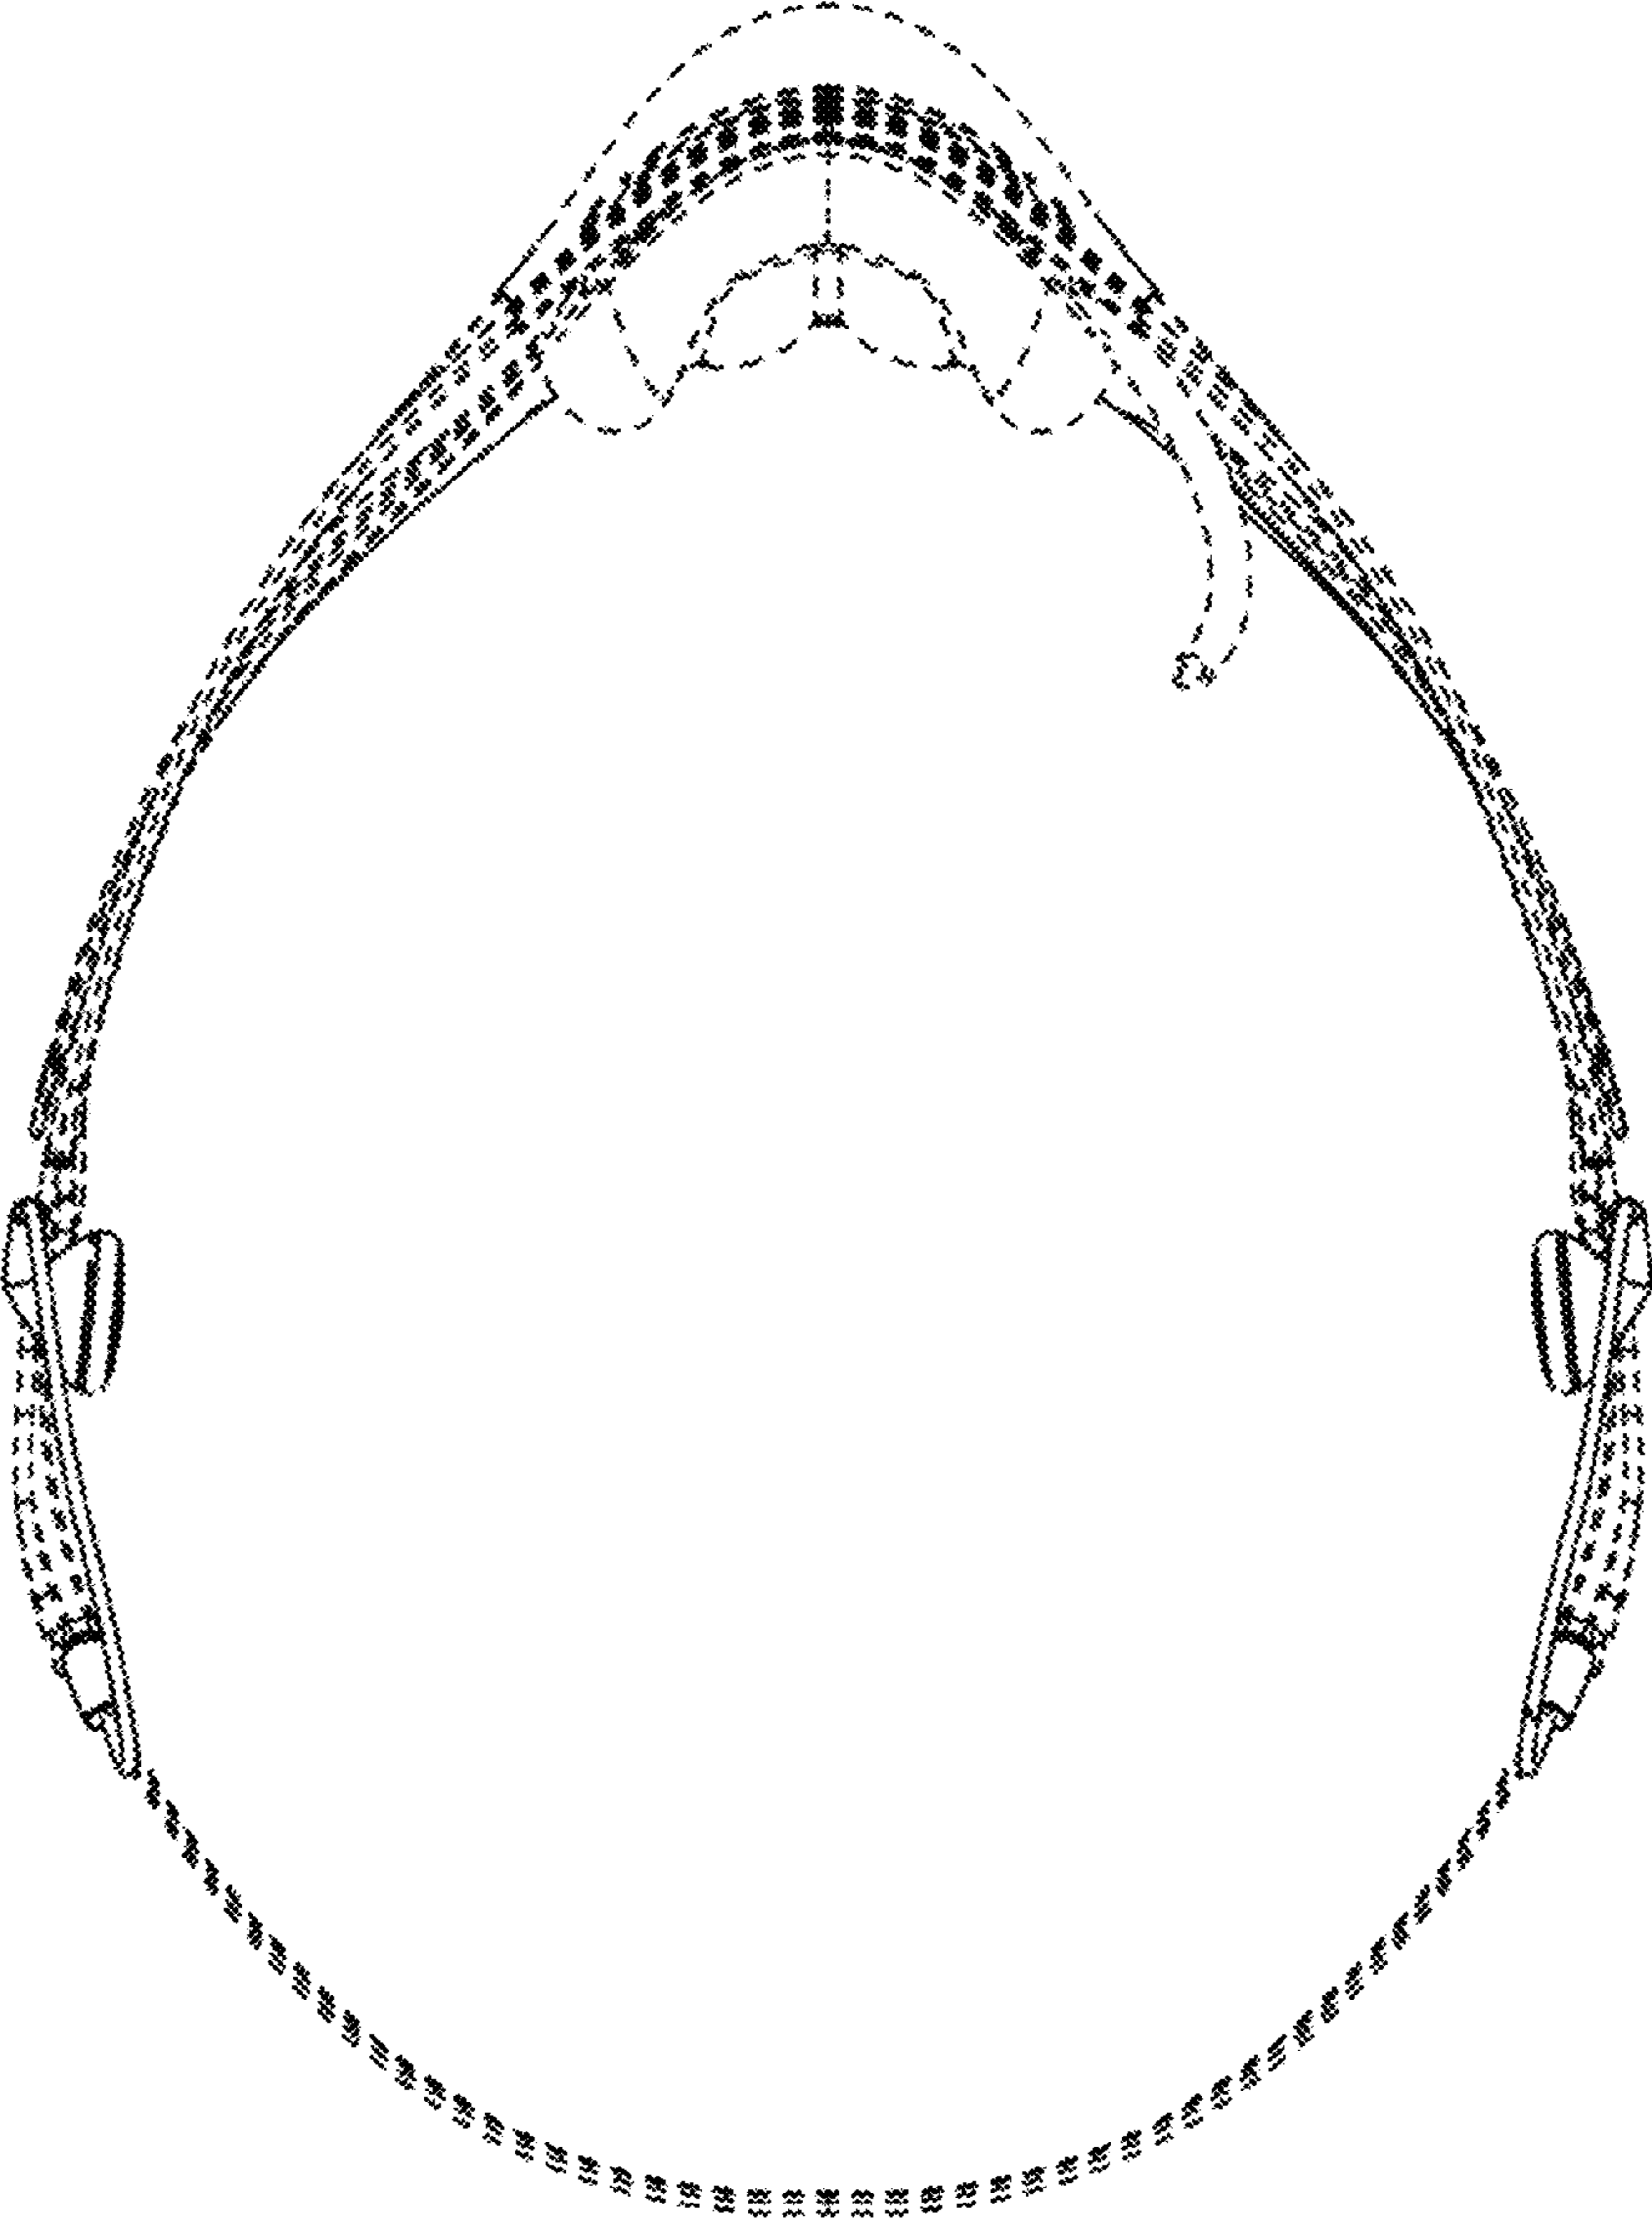


FIG. 7

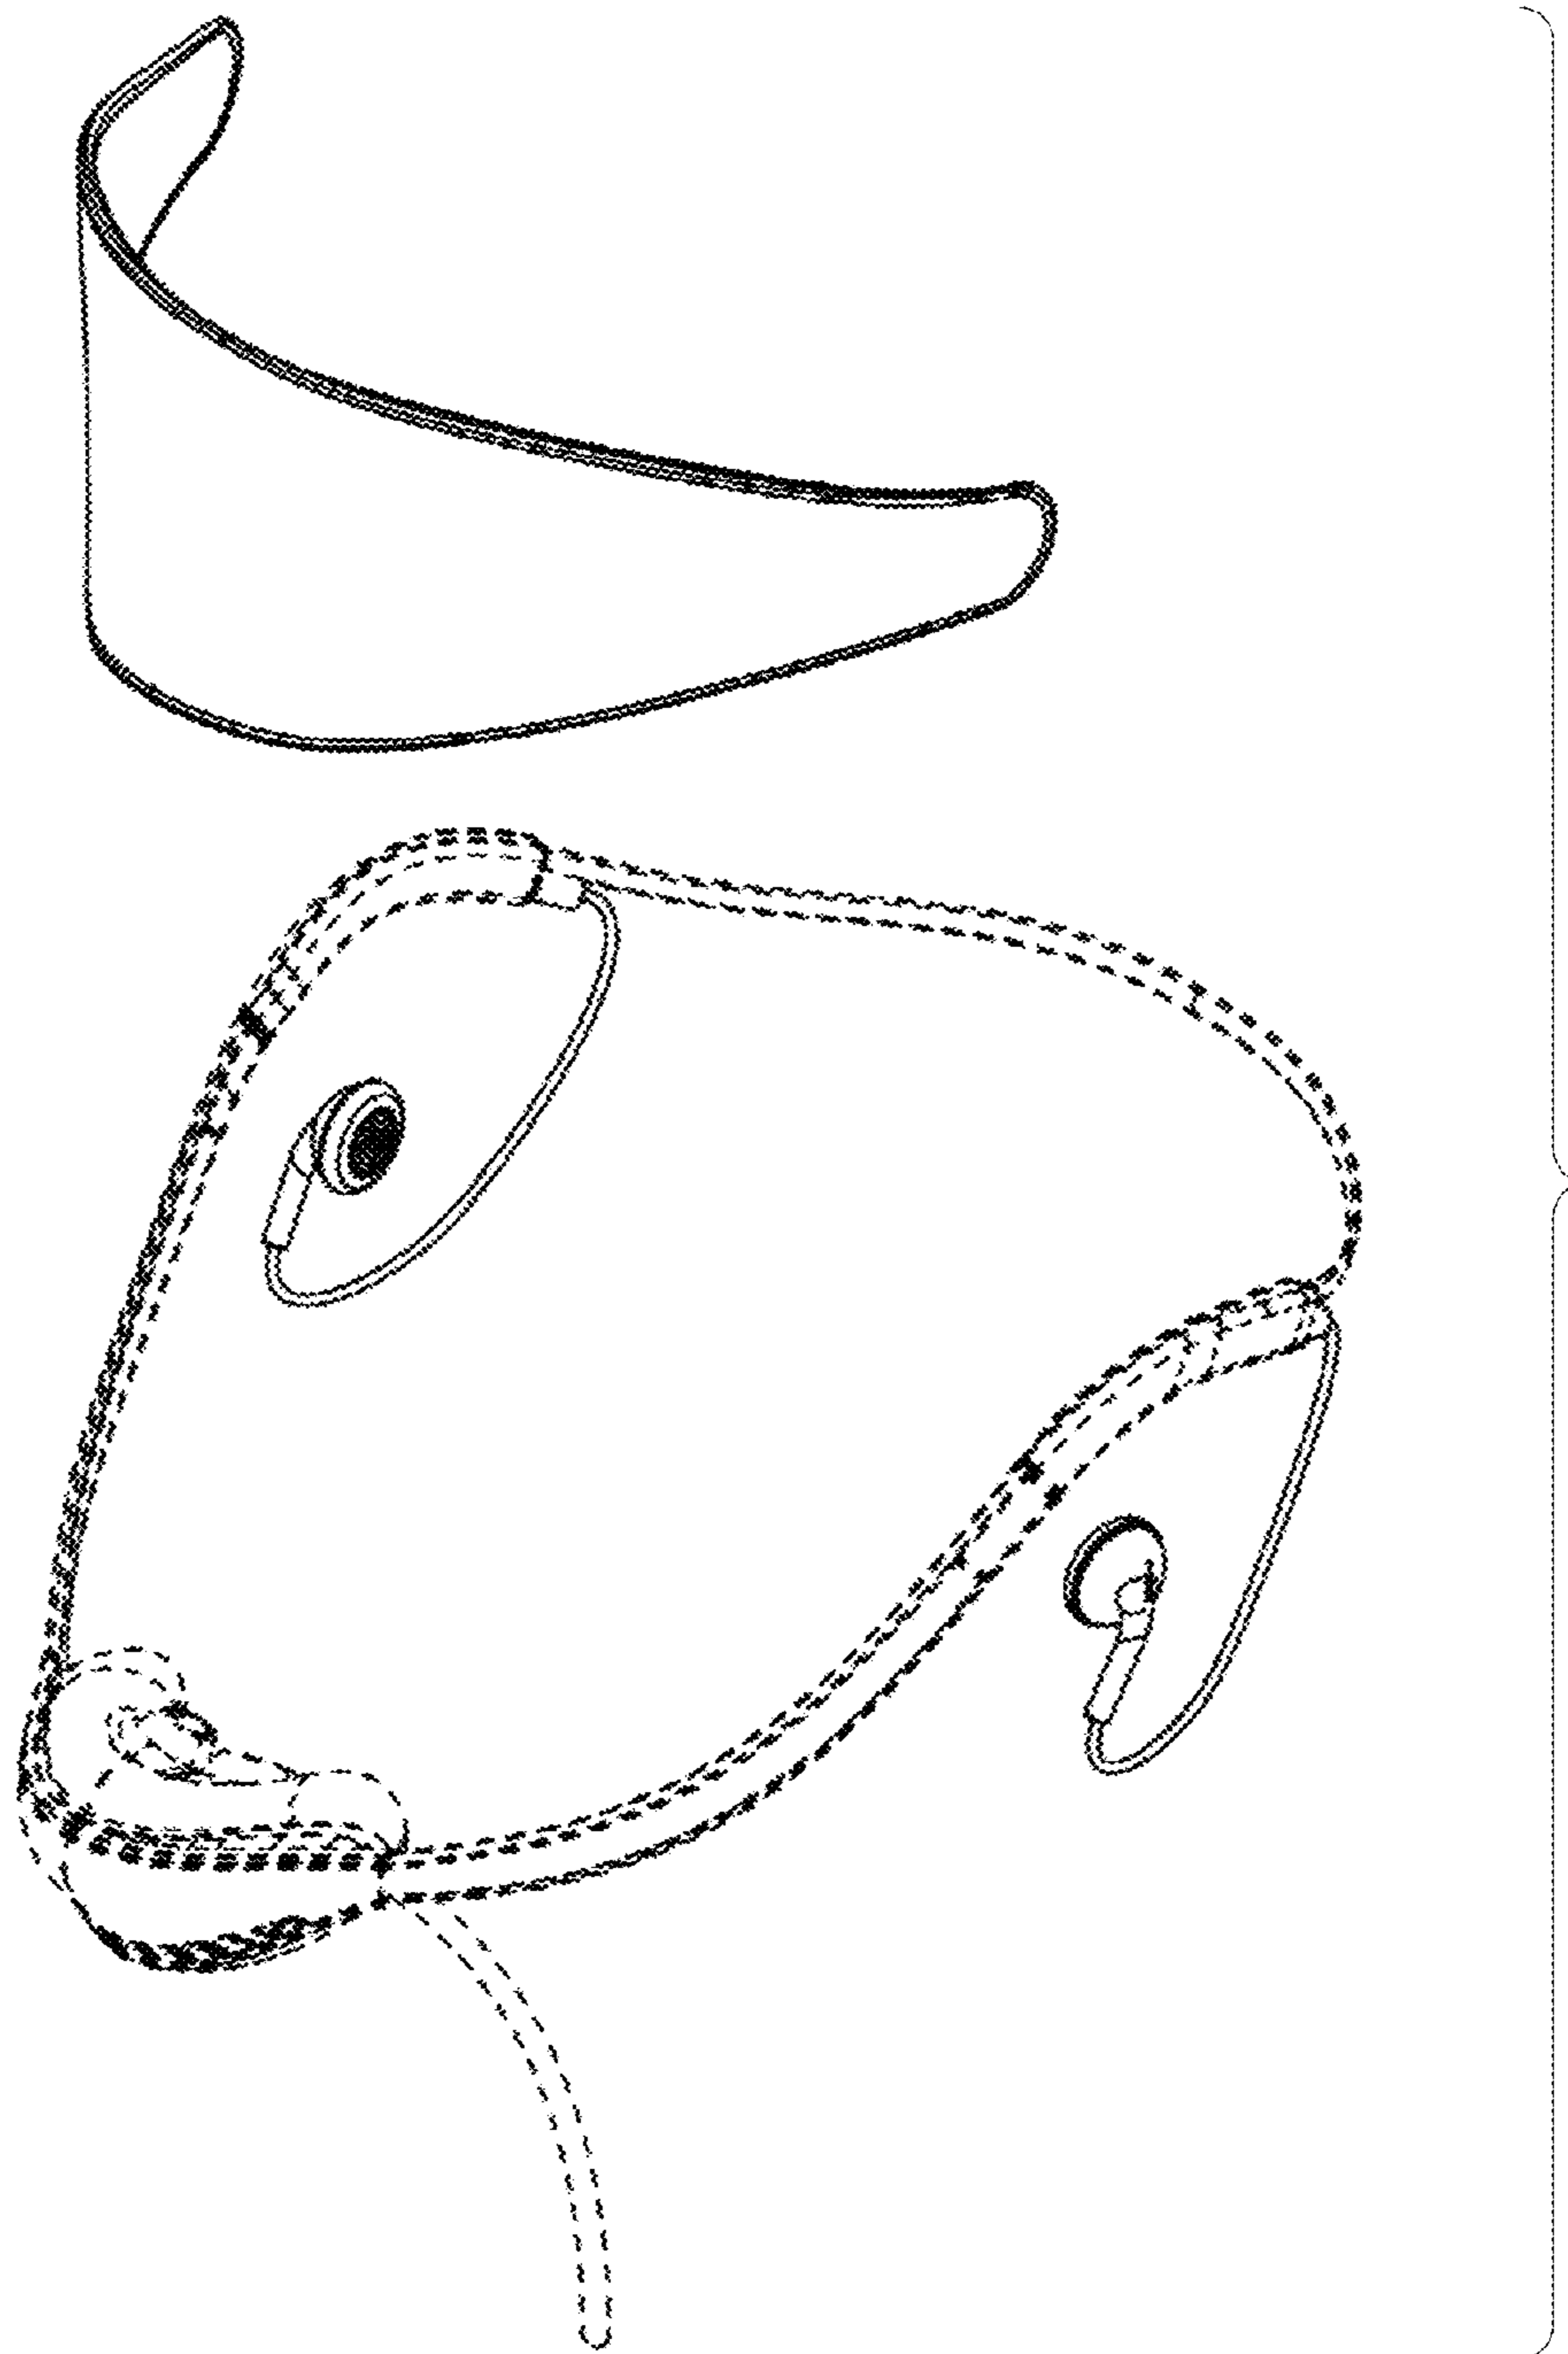


FIG. 8