



US00D741531S

(12) **United States Design Patent**
Vivenzio et al.

(10) **Patent No.:** **US D741,531 S**
(45) **Date of Patent:** **** Oct. 20, 2015**

(54) **ILLUMINATOR FOR A MEDICAL DEVICE
OR THE LIKE**

(71) Applicant: **Welch Allyn, Inc.**, Skaneateles Falls, NY
(US)

(72) Inventors: **Robert L. Vivenzio**, Skaneateles Falls,
NY (US); **Raymond A. Lia**, Skaneateles
Falls, NY (US)

(73) Assignee: **WELCH ALLYN, INC.**, Skaneateles
Falls, NY (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/434,856**

(22) Filed: **Oct. 17, 2012**

(51) **LOC (10) Cl.** **26-02**

(52) **U.S. Cl.**
USPC **D26/46; D26/38**

(58) **Field of Classification Search**
USPC D26/37, 38, 39, 45, 46, 40, 51;
362/572, 574, 575, 157, 158, 184, 186,
362/194–196, 200, 208, 253
CPC F21L 2/00; F21L 4/00; F21L 4/005;
F21L 17/00; F21L 13/08; F21Y 2101/00;
F21V 21/30; F21V 21/406; F21W 2131/406;
F21W 2131/407

See application file for complete search history.

(56) **References Cited**



U.S. PATENT DOCUMENTS

D343,453 S	1/1994	Noda	
D367,087 S *	2/1996	Mathews	D21/483
D375,372 S *	11/1996	Allen	D26/37
D425,226 S *	5/2000	Galli	D26/37
D445,928 S *	7/2001	Sharrah et al.	D26/38
D446,324 S *	8/2001	Lynch et al.	D26/37
D446,325 S *	8/2001	Guerrieri	D26/37
D457,670 S *	5/2002	Allen	D26/37
D482,469 S *	11/2003	Guerrieri	D26/37
D492,050 S *	6/2004	Chung	D26/37
D498,553 S *	11/2004	Lee	D26/37
D498,864 S *	11/2004	Lee	D26/37

D501,266 S *	1/2005	Harris et al.	D26/37
D507,368 S	7/2005	Waters	
D507,369 S *	7/2005	Waters	D26/37
D507,671 S *	7/2005	Rice	D26/37
D513,084 S	12/2005	Parker et al.	
D565,216 S *	3/2008	Markell	D26/37
D576,323 S *	9/2008	Cienfuegos	D26/37
D577,143 S *	9/2008	Lu	D26/72
D581,566 S	11/2008	Slawson et al.	
D593,693 S	6/2009	Adamany et al.	
D594,148 S *	6/2009	Heselden	D26/37
D598,593 S *	8/2009	Kingston et al.	D26/39
D627,092 S *	11/2010	Puglisi	D26/47
7,841,751 B2 *	11/2010	Mulani	362/362
7,909,759 B2	3/2011	Pecherer	
D642,310 S	7/2011	Idelson	
D656,644 S *	3/2012	Lee	D26/39
8,142,352 B2	3/2012	Vivenzio et al.	
8,157,728 B2	4/2012	Danna et al.	
D659,845 S	5/2012	Lytte	
D676,992 S *	2/2013	Trude	D26/39
8,409,082 B2 *	4/2013	Irion et al.	600/178
D683,489 S *	5/2013	Lee	D26/39
D690,043 S *	9/2013	Sun	D26/37
RE44,806 E	3/2014	Roberts et al.	
8,740,780 B2 *	6/2014	Honda et al.	600/177
D710,500 S	8/2014	Roeloffs	
8,808,175 B2	8/2014	Deitch et al.	
D712,561 S	9/2014	Hagenauer	
2008/0228038 A1	9/2008	McMahon et al.	
2009/0076334 A1	3/2009	Chen	
2009/0312610 A1	12/2009	Buchok et al.	
2012/0108907 A1	5/2012	Fitipaldi et al.	
2014/0293590 A1	10/2014	Pathy	

OTHER PUBLICATIONS

Design U.S. Appl. No. 29/434,856, filed Oct. 17, 2012; In re: Vivenzio et al., entitled *Illuminator for a Medical Device or the Like*.
Design U.S. Appl. No. 29/434,858, filed Oct. 17, 2012; In re: Vivenzio et al., entitled *Illuminator for a Medical Device or the Like*.
U.S. Appl. No. 13/839,205, filed Mar. 15, 2013; In re: Vivenzio et al., entitled *Illumination Device, System, and Method of Use*.
Disposable Vaginal Speculum With Cordless LED Source, MedGyn Products, Inc. [online] [retrieved May 1, 2014]. Retrieved from the Internet: <URL: <http://medgyn.com/?wpsc-product=disposable-speculum-cordless-led>>. (dated 2014) 2 pages.
ER-SPEC Single-use Vaginal Specula with Built-In LED-Use Light Source, OBP Medical Inc. . [online] [retrieved May 1, 2014]. Retrieved from the Internet: <URL: <https://obpmedical.com/product/er-spec/>>. (dated 2014) 3 pages.

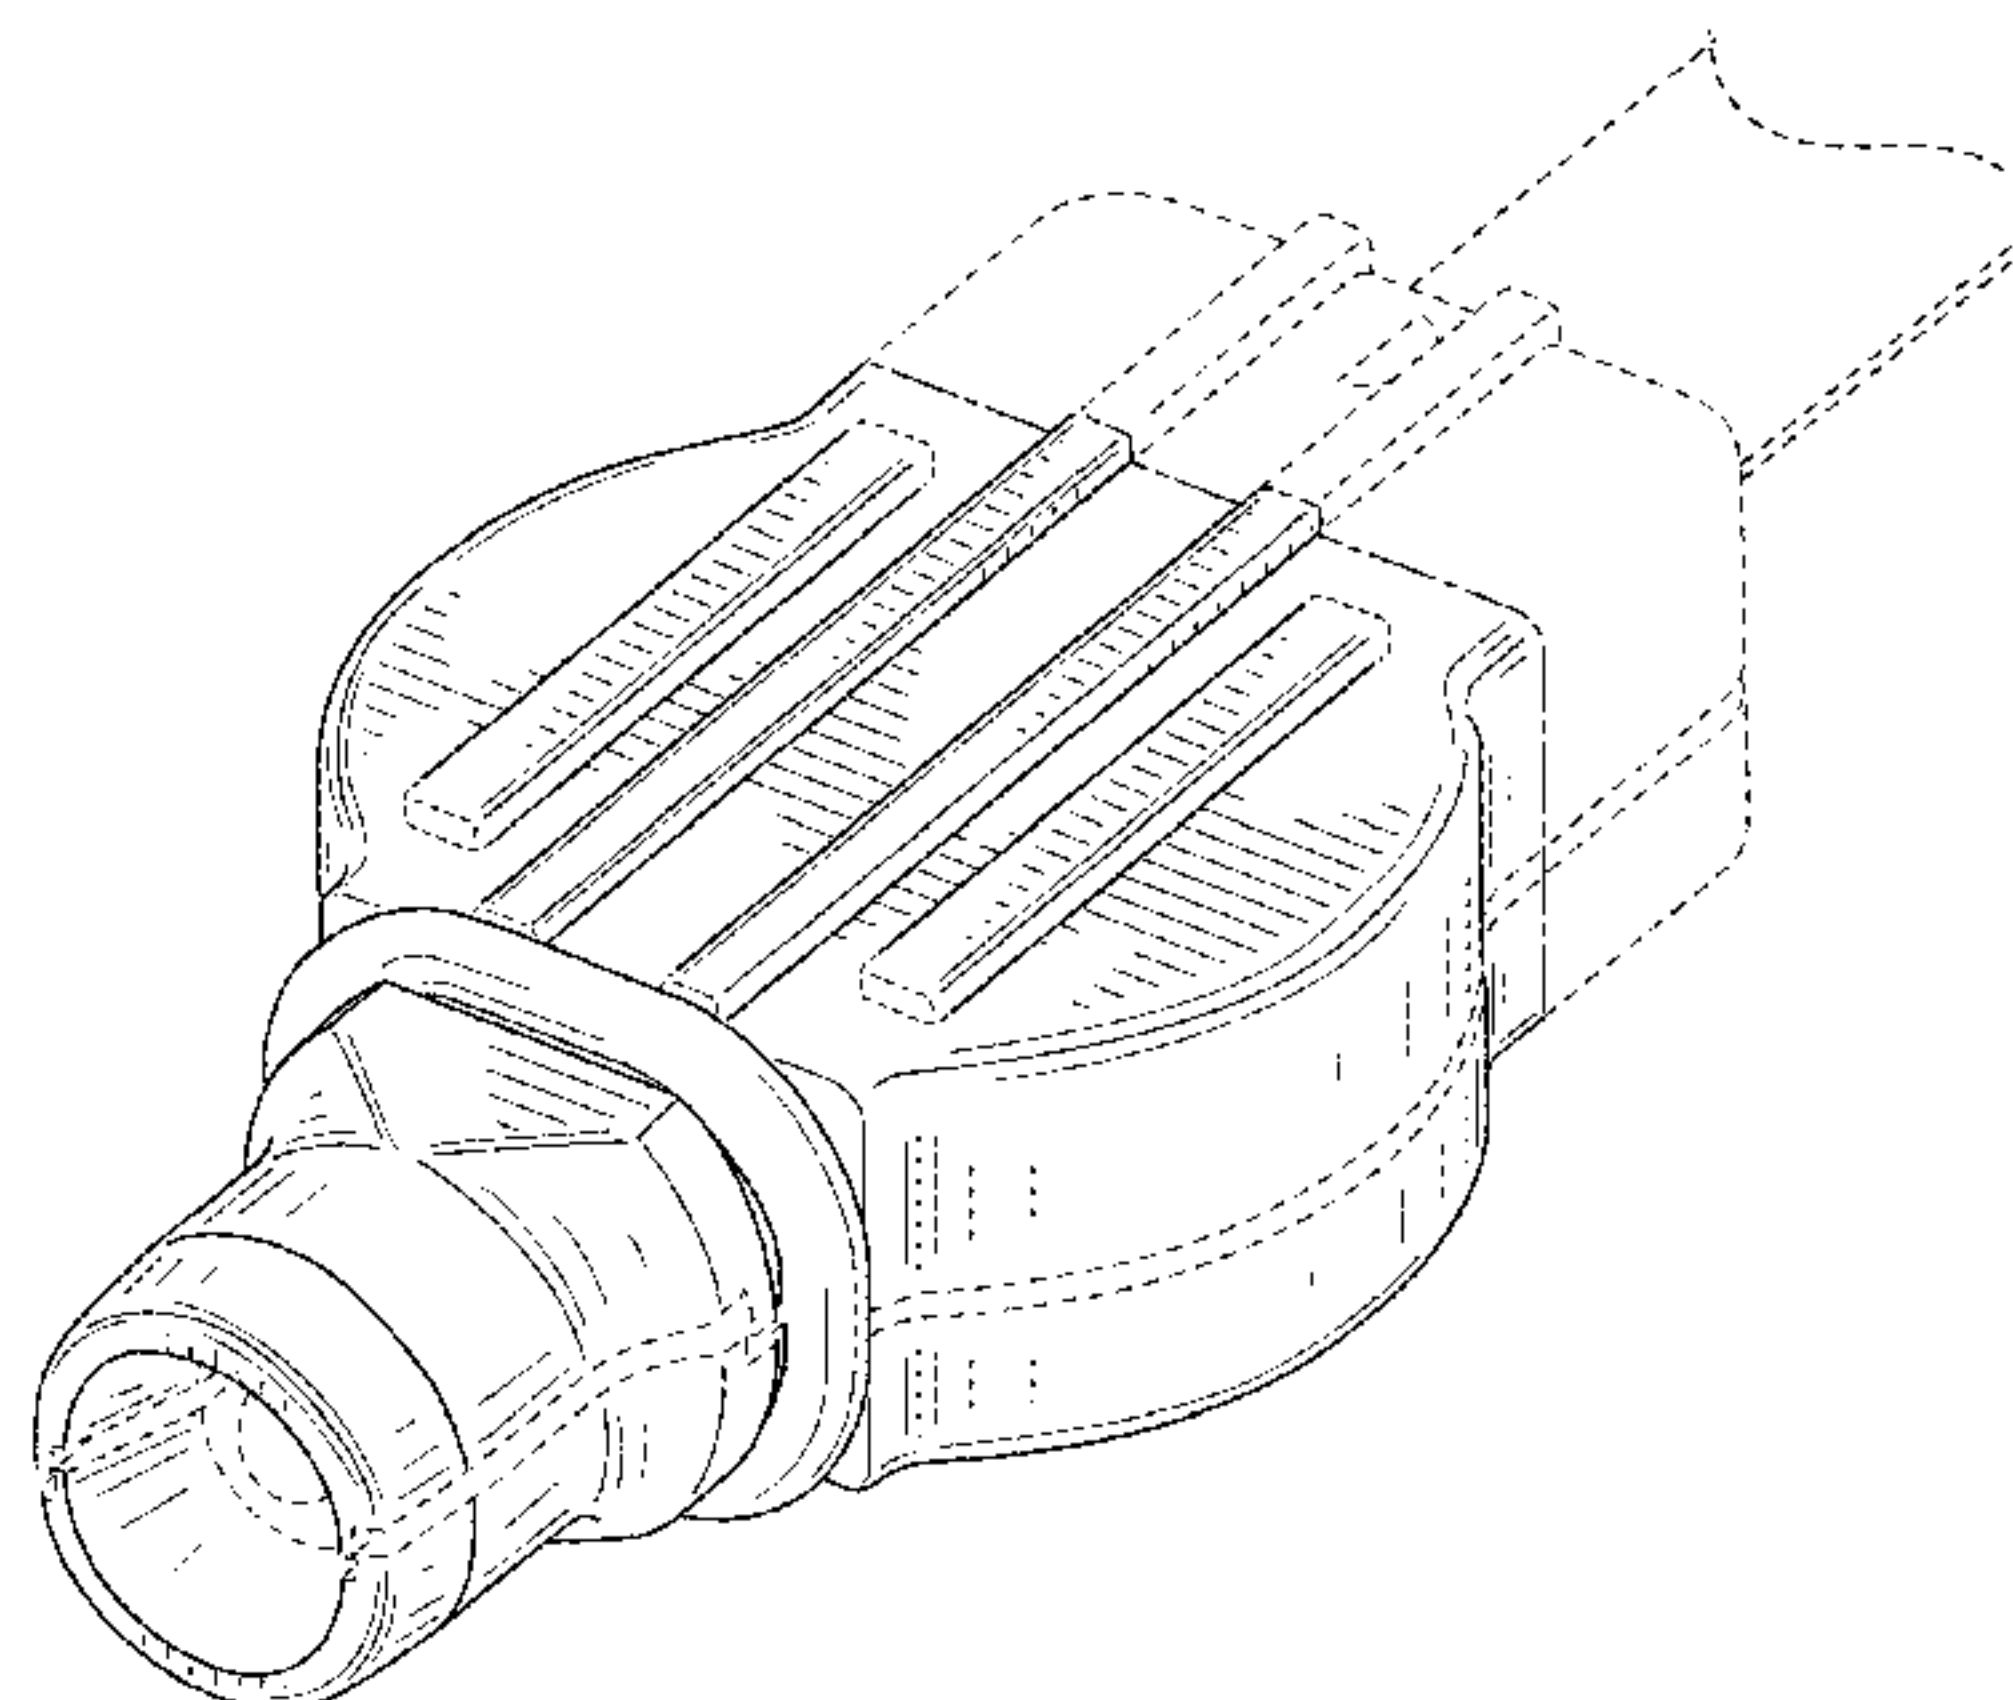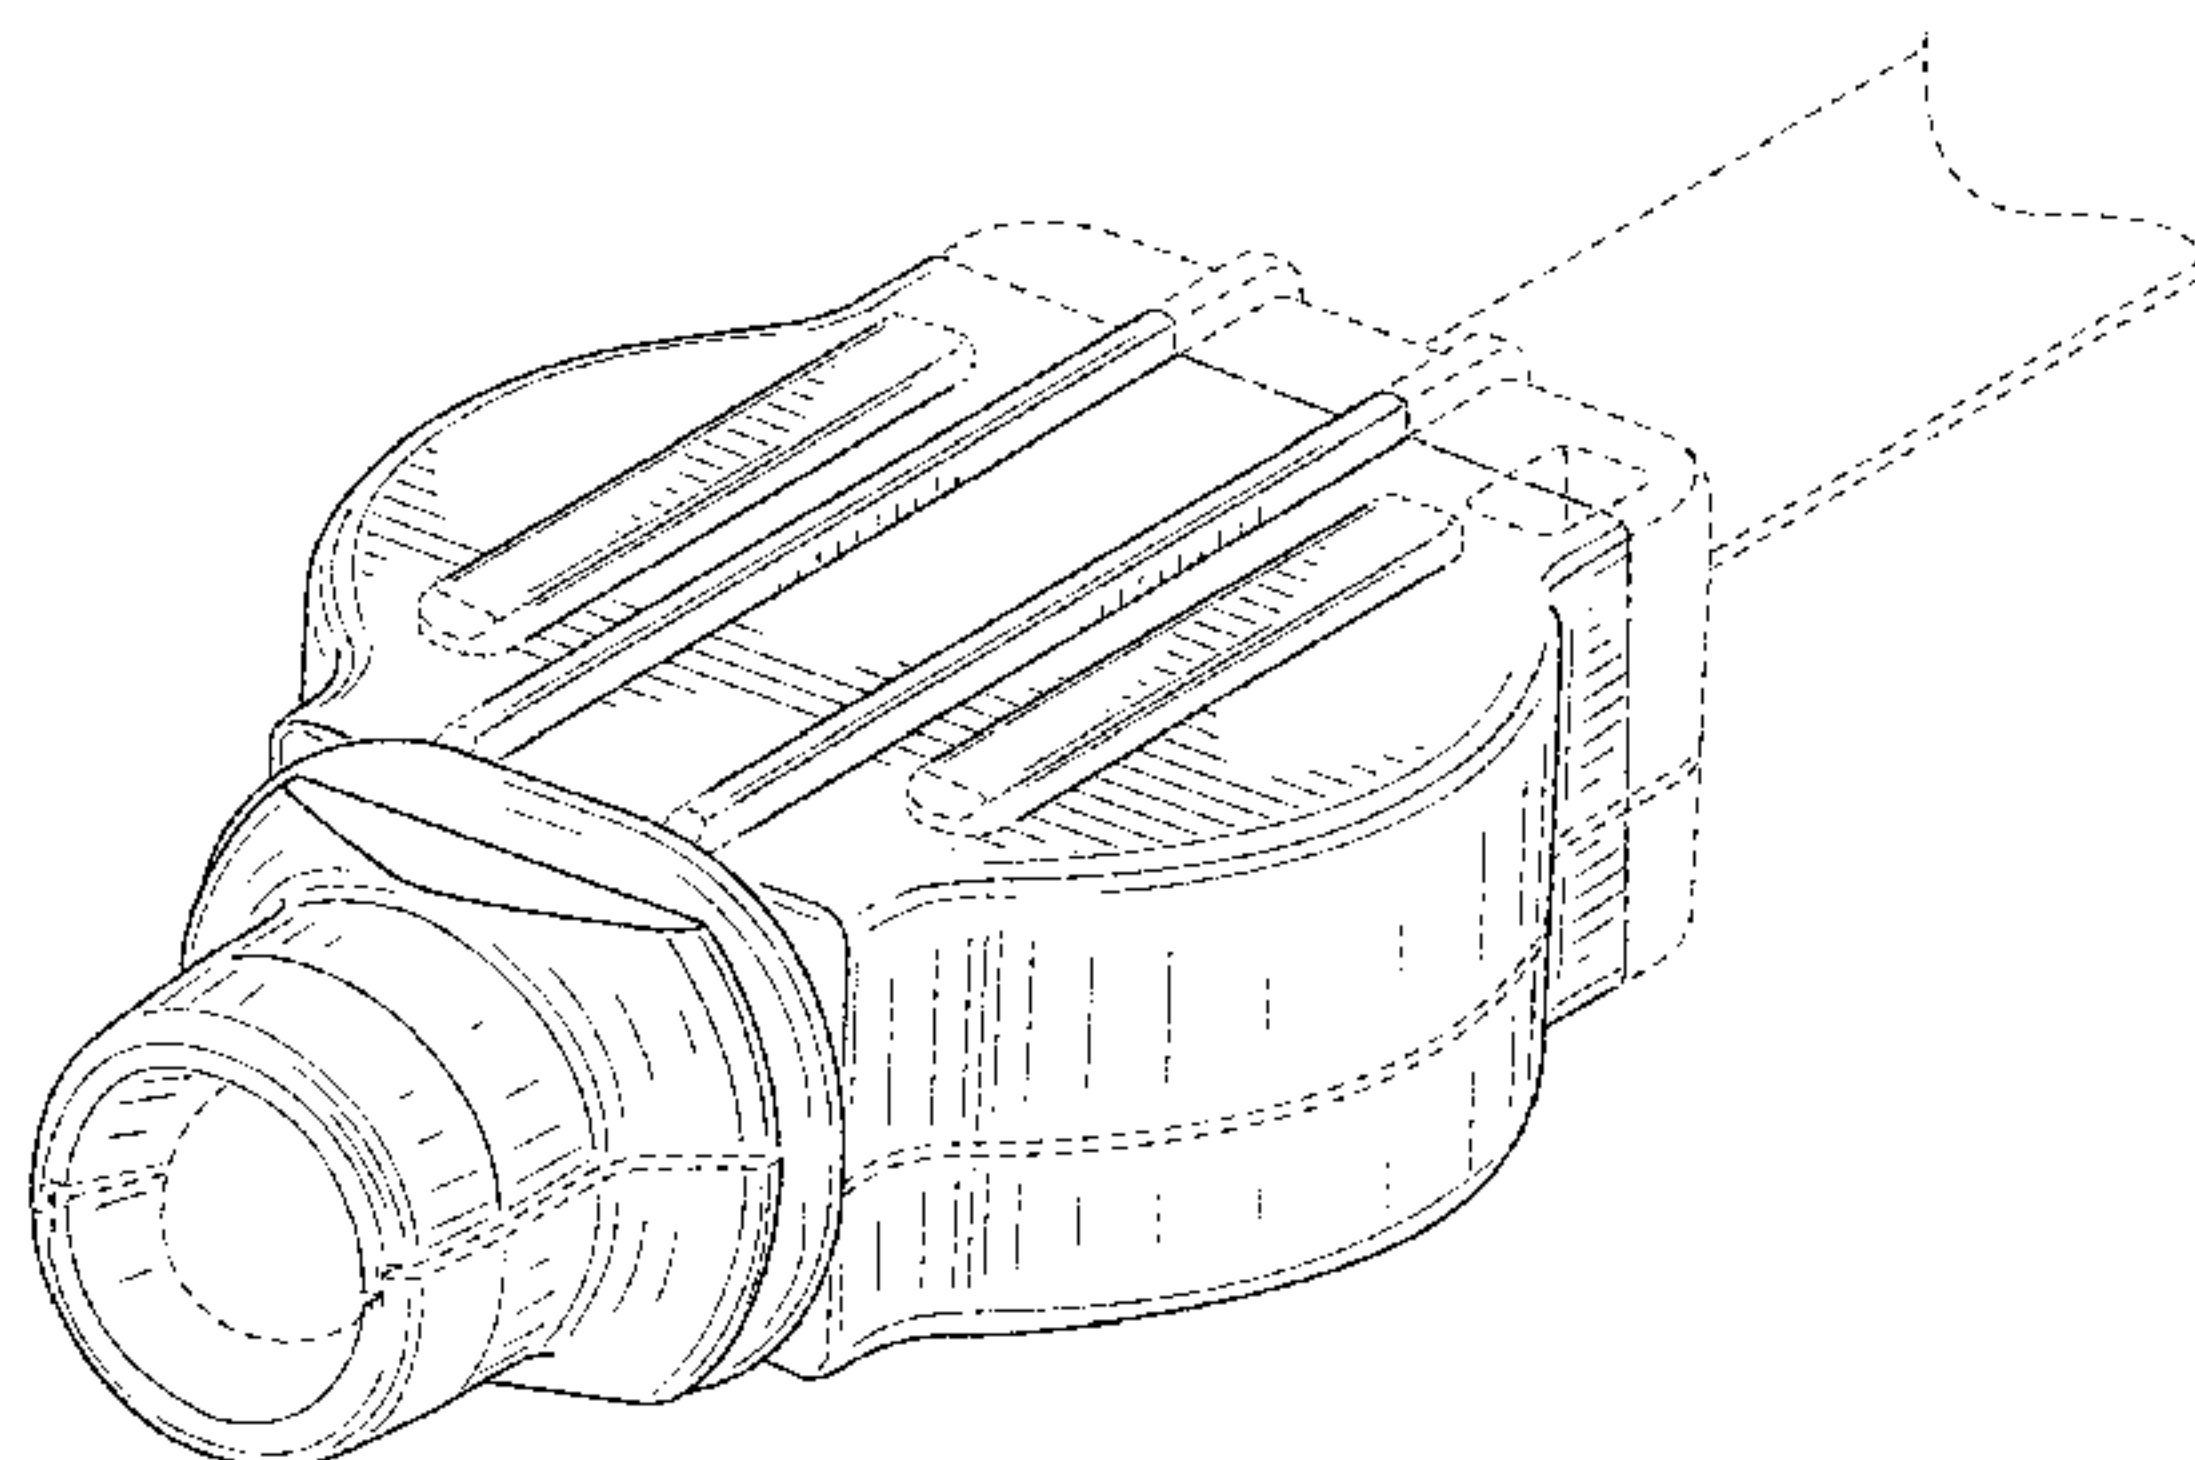

ER-SPEC® Single-Use Vaginal Speculum with Built-In Light Source, OBP Medical Inc. (brochure) (dated Apr. 16, 2014) 2 pages.
ER-SPEC, Tired of Search for a Light Source?, OBP Medical Inc. (Rep Brochure) (Feb. 2012 revision) 2 pages.
ER-SPEC Presentation, OBP Medical (dated Apr. 16, 2014), 12 pages.
ER-SPEC® User Manual, OBP Medical (dated Jun. 27, 2013), 10 pages.
Office Action from U.S. Appl. No. 13/839,205 dated Dec. 19, 2014.
Office Action from U.S. Appl. No. 29/434,858 dated Jul. 24, 2015.
Office Action from U.S. Appl. No. 13/839,205 dated Jul. 1, 2015.
Restriction Requirement from U.S. Appl. No. 29/495,181 dated Aug. 14, 2015.

* cited by examiner

Primary Examiner — Ian Simmons
Assistant Examiner — Carissa C Fitts

(57) **CLAIM**
The ornamental design for an illuminator for a medical device or the like, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an illuminator for a medical device or the like showing our new design;
FIG. 2 is another perspective view thereof;
FIG. 3 is a top plan view thereof;
FIG. 4 is a bottom plan view thereof;
FIG. 5 is a left side elevation view thereof;
FIG. 6 is a right side elevation view thereof;
FIG. 7 is a front elevation view thereof;
FIG. 8 is a rear elevation view thereof;
FIG. 9 is another perspective view thereof, shown in a position of use with a medical device;

FIG. 10 is another side view thereof, shown in a position of use with a medical device;
FIG. 11 is a perspective view of another illuminator for a medical device or the like showing our new design;
FIG. 12 is another perspective view thereof;
FIG. 13 is a top plan view thereof;
FIG. 14 is a bottom plan view thereof;
FIG. 15 is a left side elevation view thereof;
FIG. 16 is a right side elevation view thereof;
FIG. 17 is a front elevation view thereof;
FIG. 18 is a rear elevation view thereof;
FIG. 19 is another perspective view thereof, shown in a position of use with a medical device;
FIG. 20 is another side view thereof, shown in a position of use with a medical device;
FIG. 21 is a perspective view of yet another illuminator for a medical device or the like showing our new design;
FIG. 22 is another perspective view thereof;
FIG. 23 is a top plan view thereof;
FIG. 24 is a bottom plan view thereof;
FIG. 25 is a left side elevation view thereof;
FIG. 26 is a right side elevation view thereof;
FIG. 27 is a front elevation view thereof;
FIG. 28 is a rear elevation view thereof;
FIG. 29 is an exploded perspective view thereof; and,
FIG. 30 is another exploded perspective view thereof.
Broken lines immediately adjacent shaded areas represent bounds of the claimed design. Broken lines of the medical devices of FIGS. 9, 10, 19, 20, 29, and 30 are directed to environment. All other broken lines are directed to unclaimed features. The broken lines form no part of the claimed design.

1 Claim, 24 Drawing Sheets

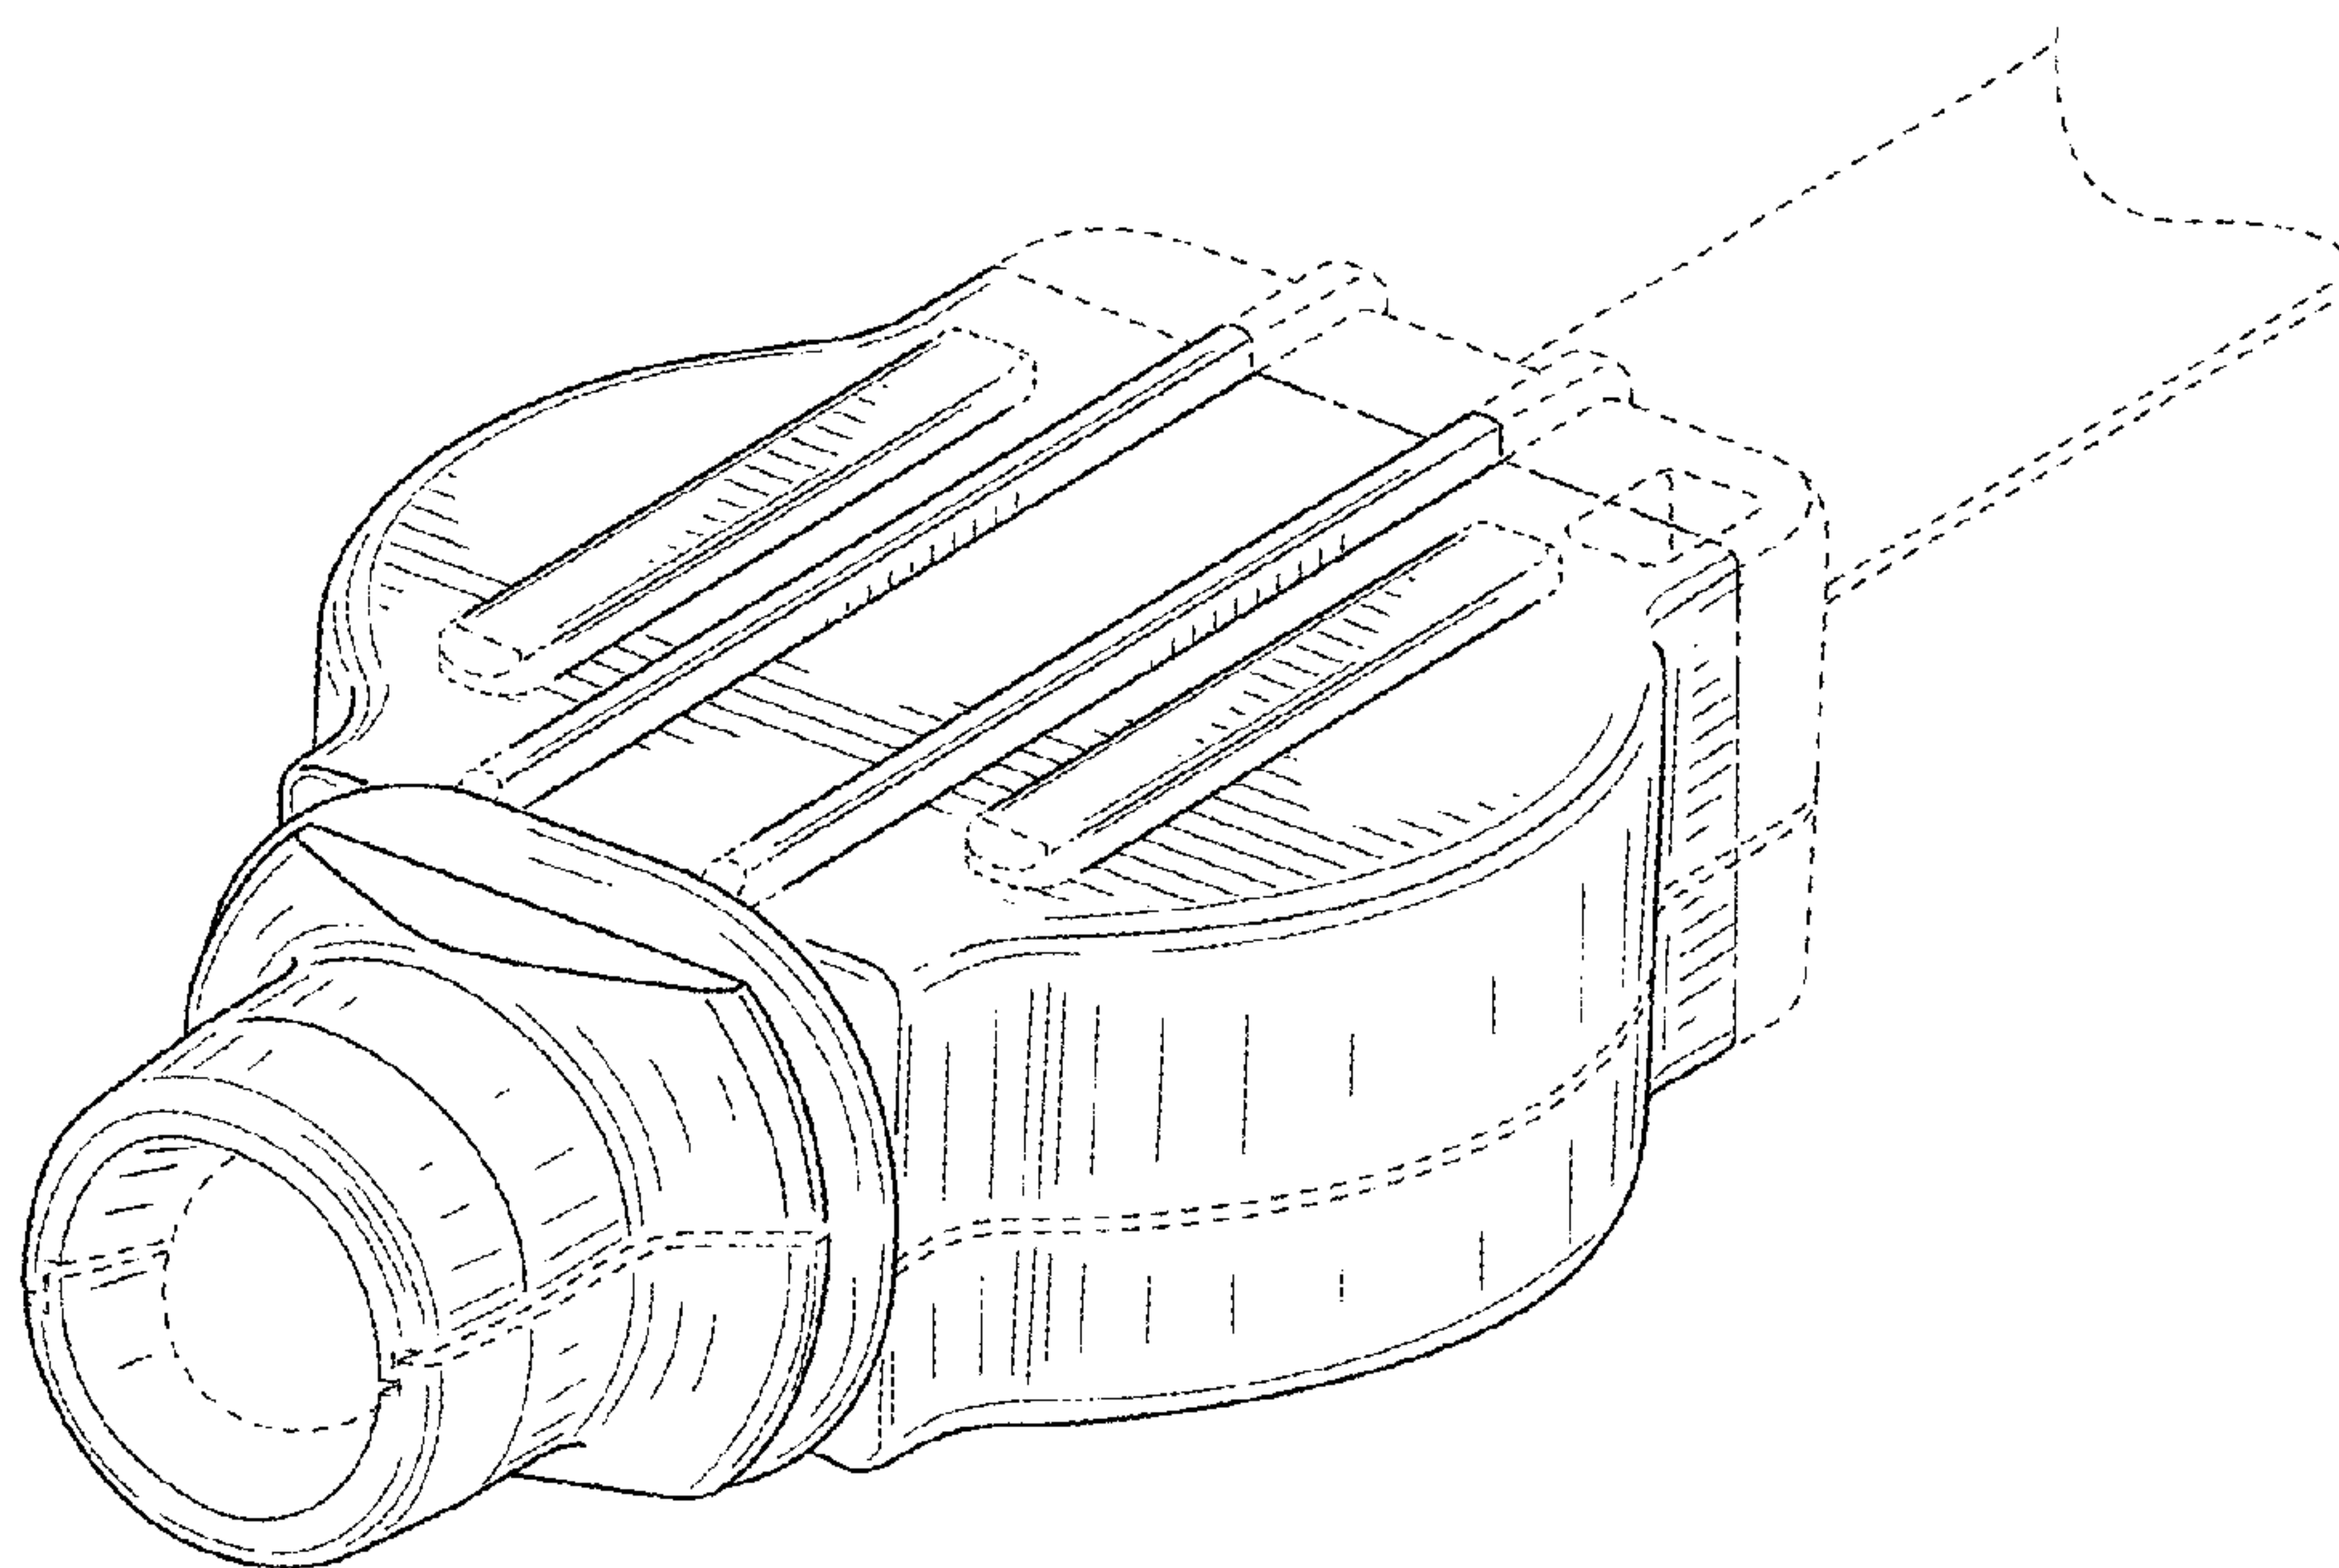


FIG. 1

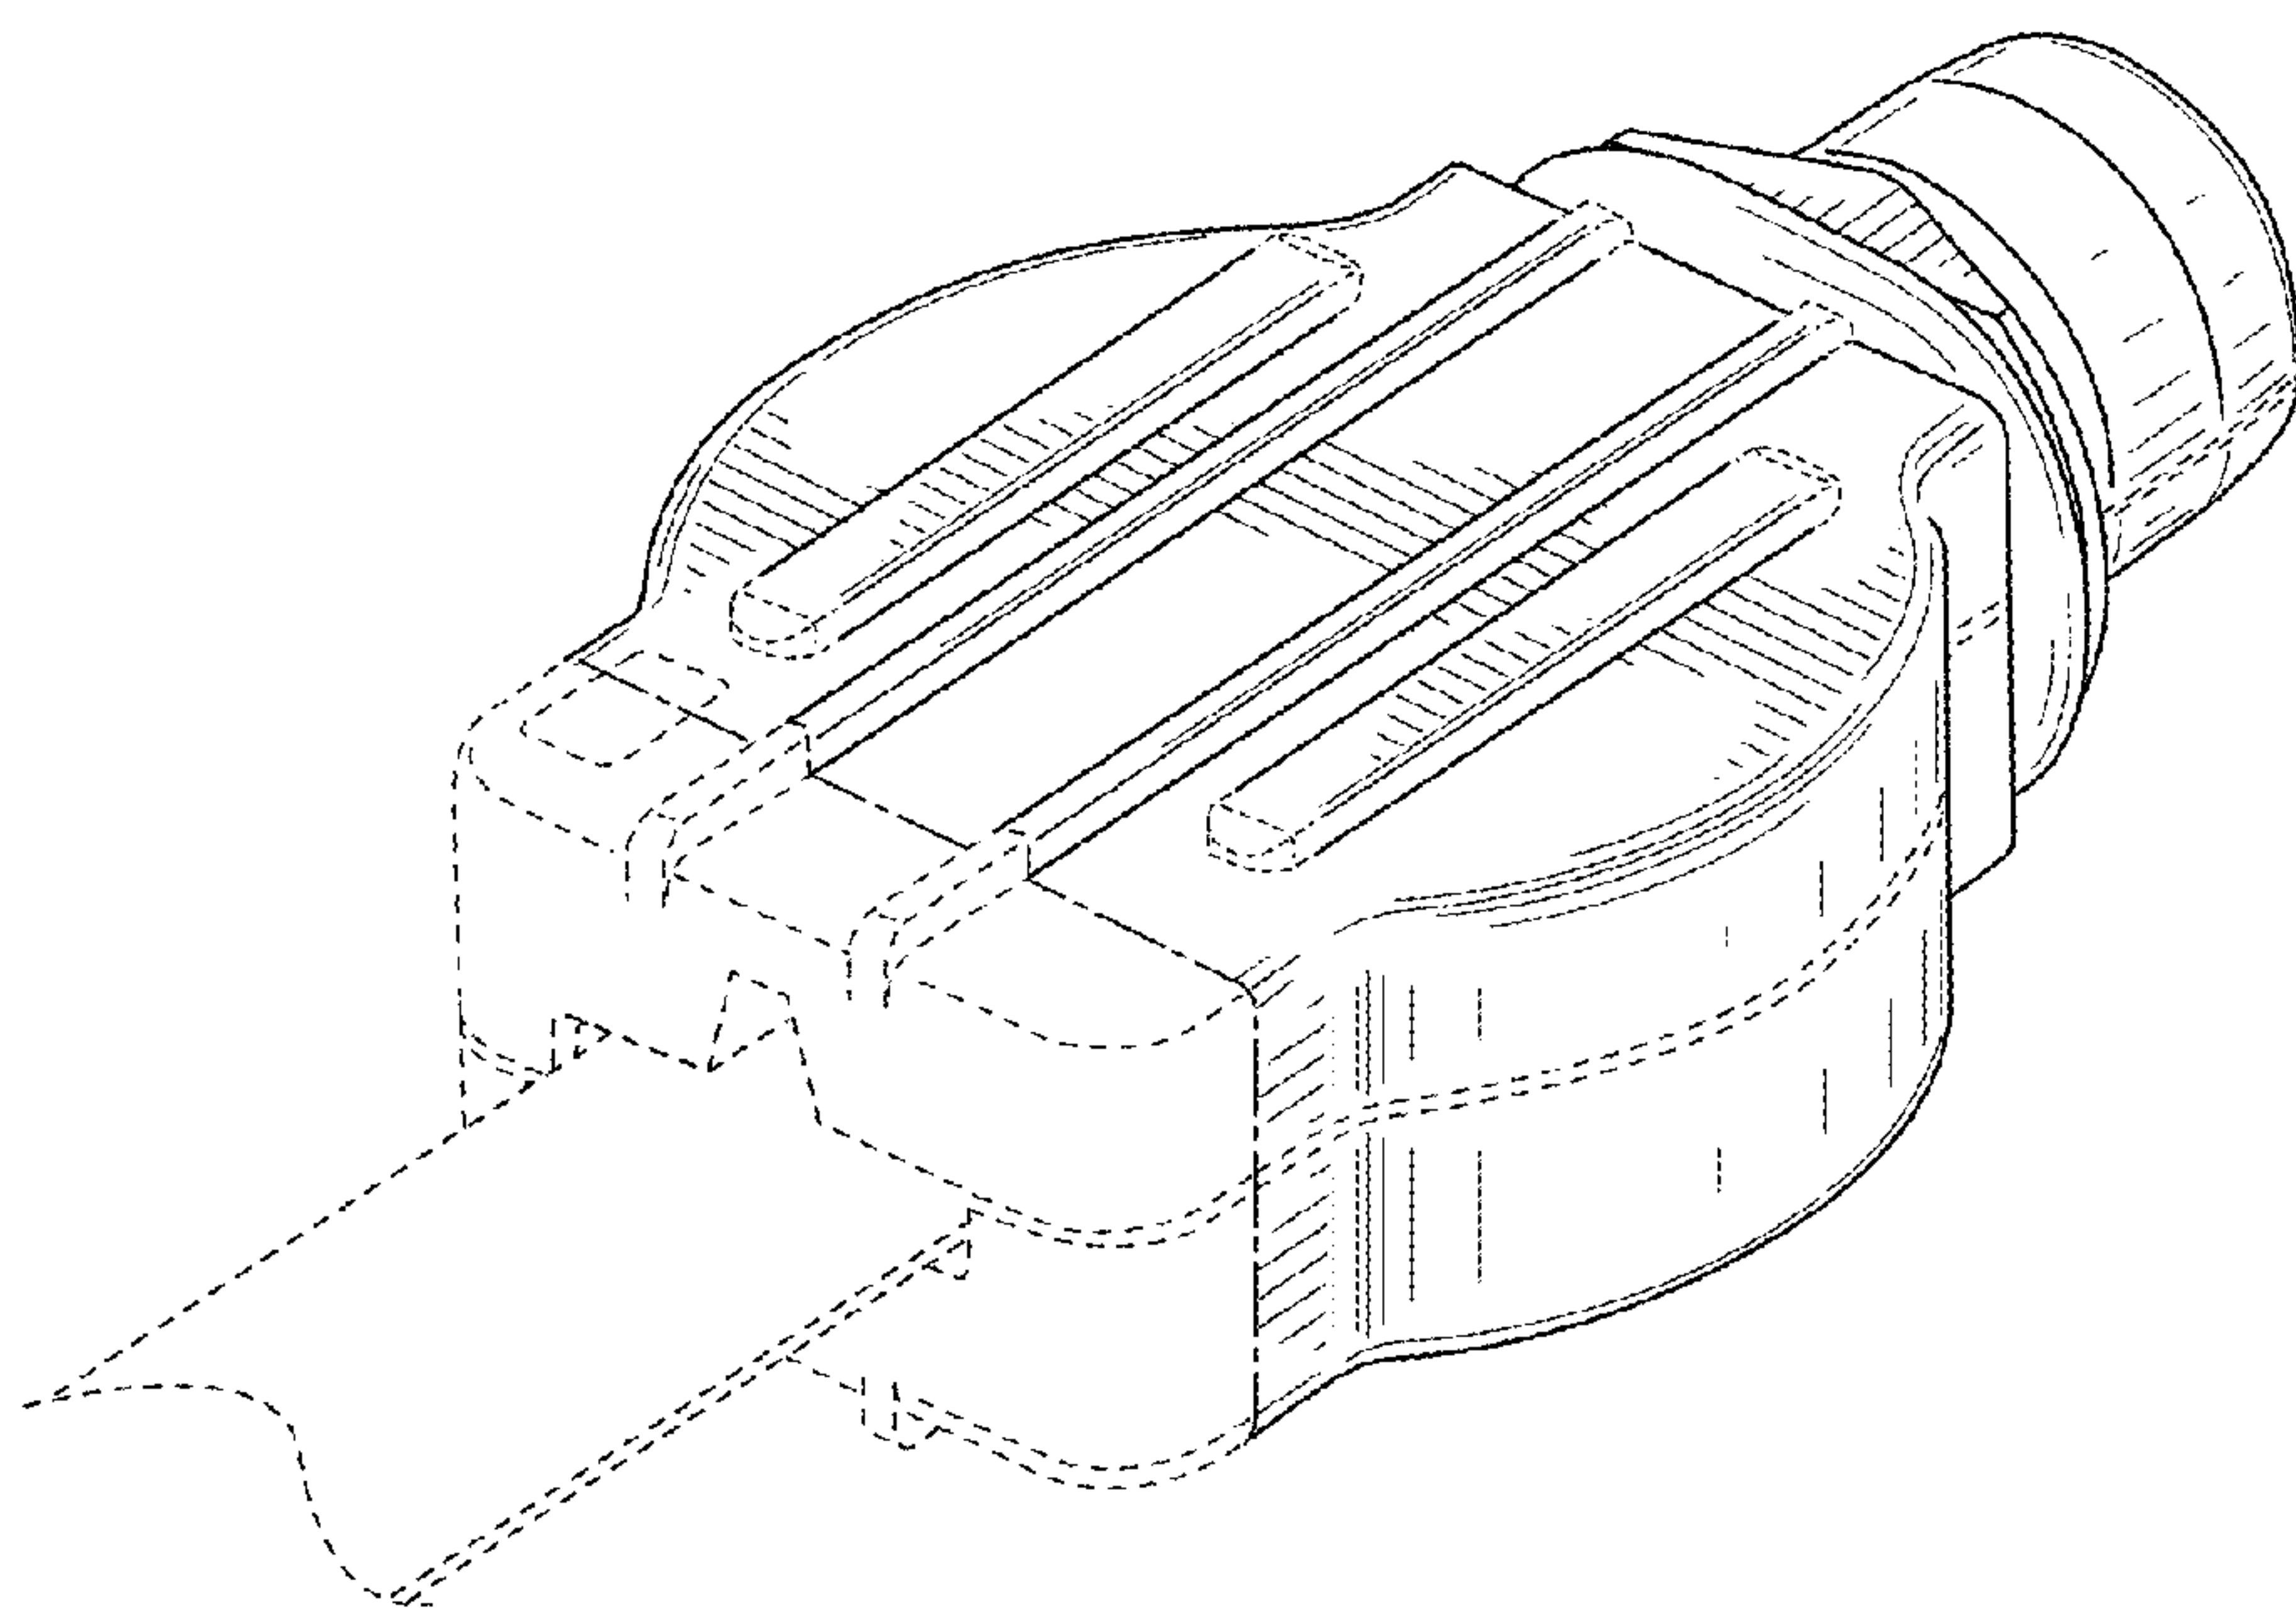


FIG. 2

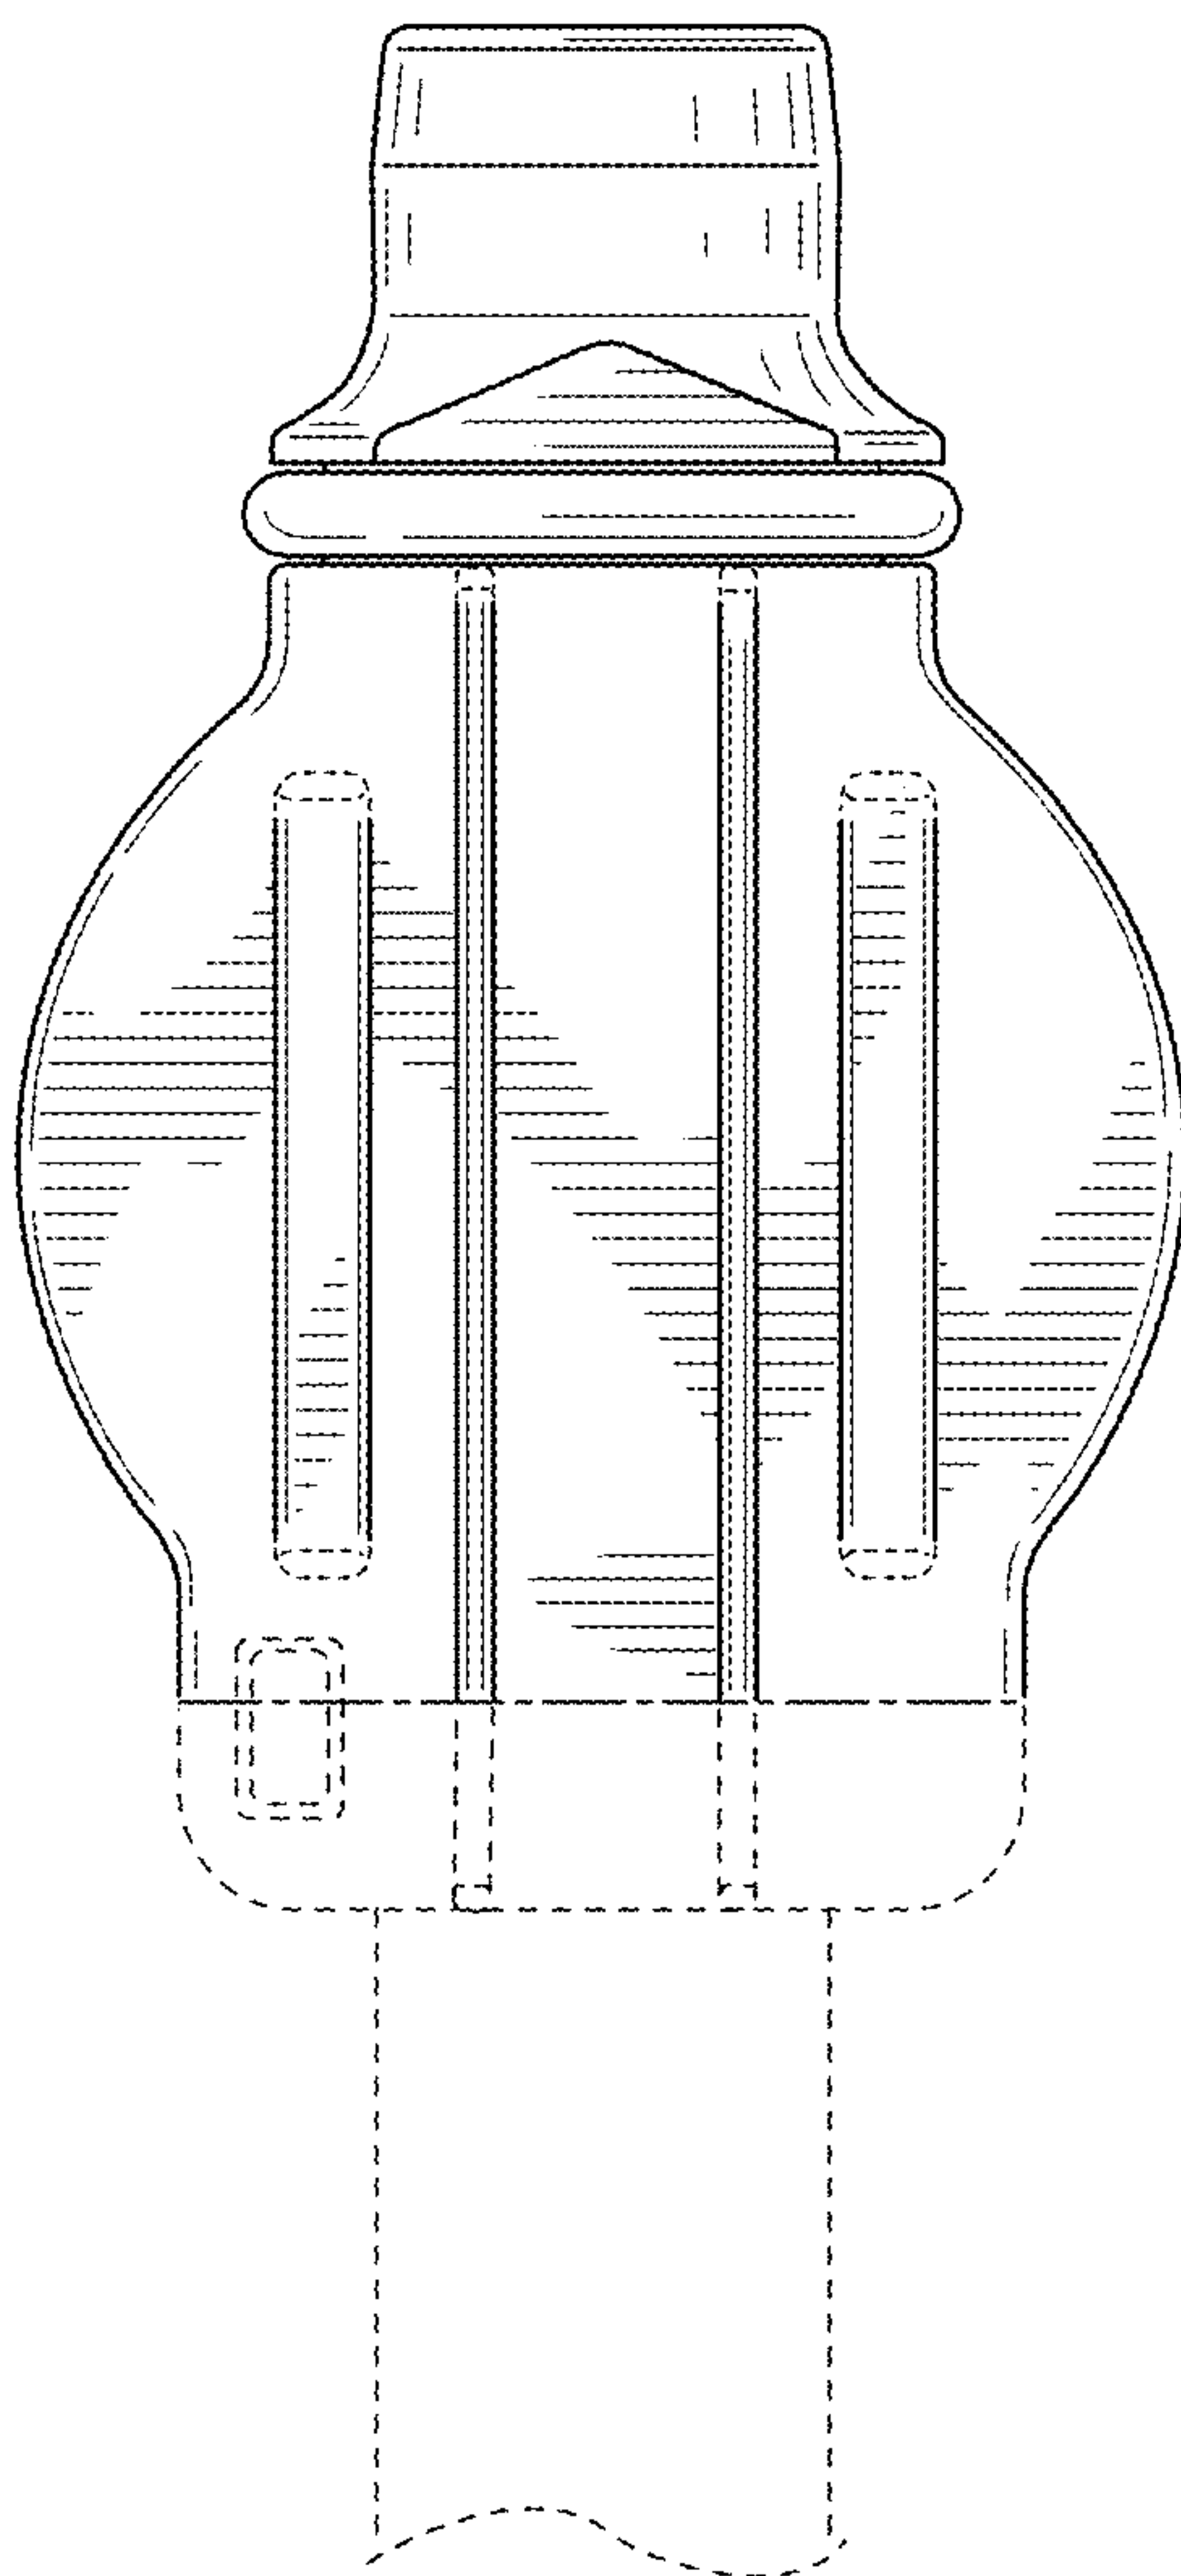


FIG. 3

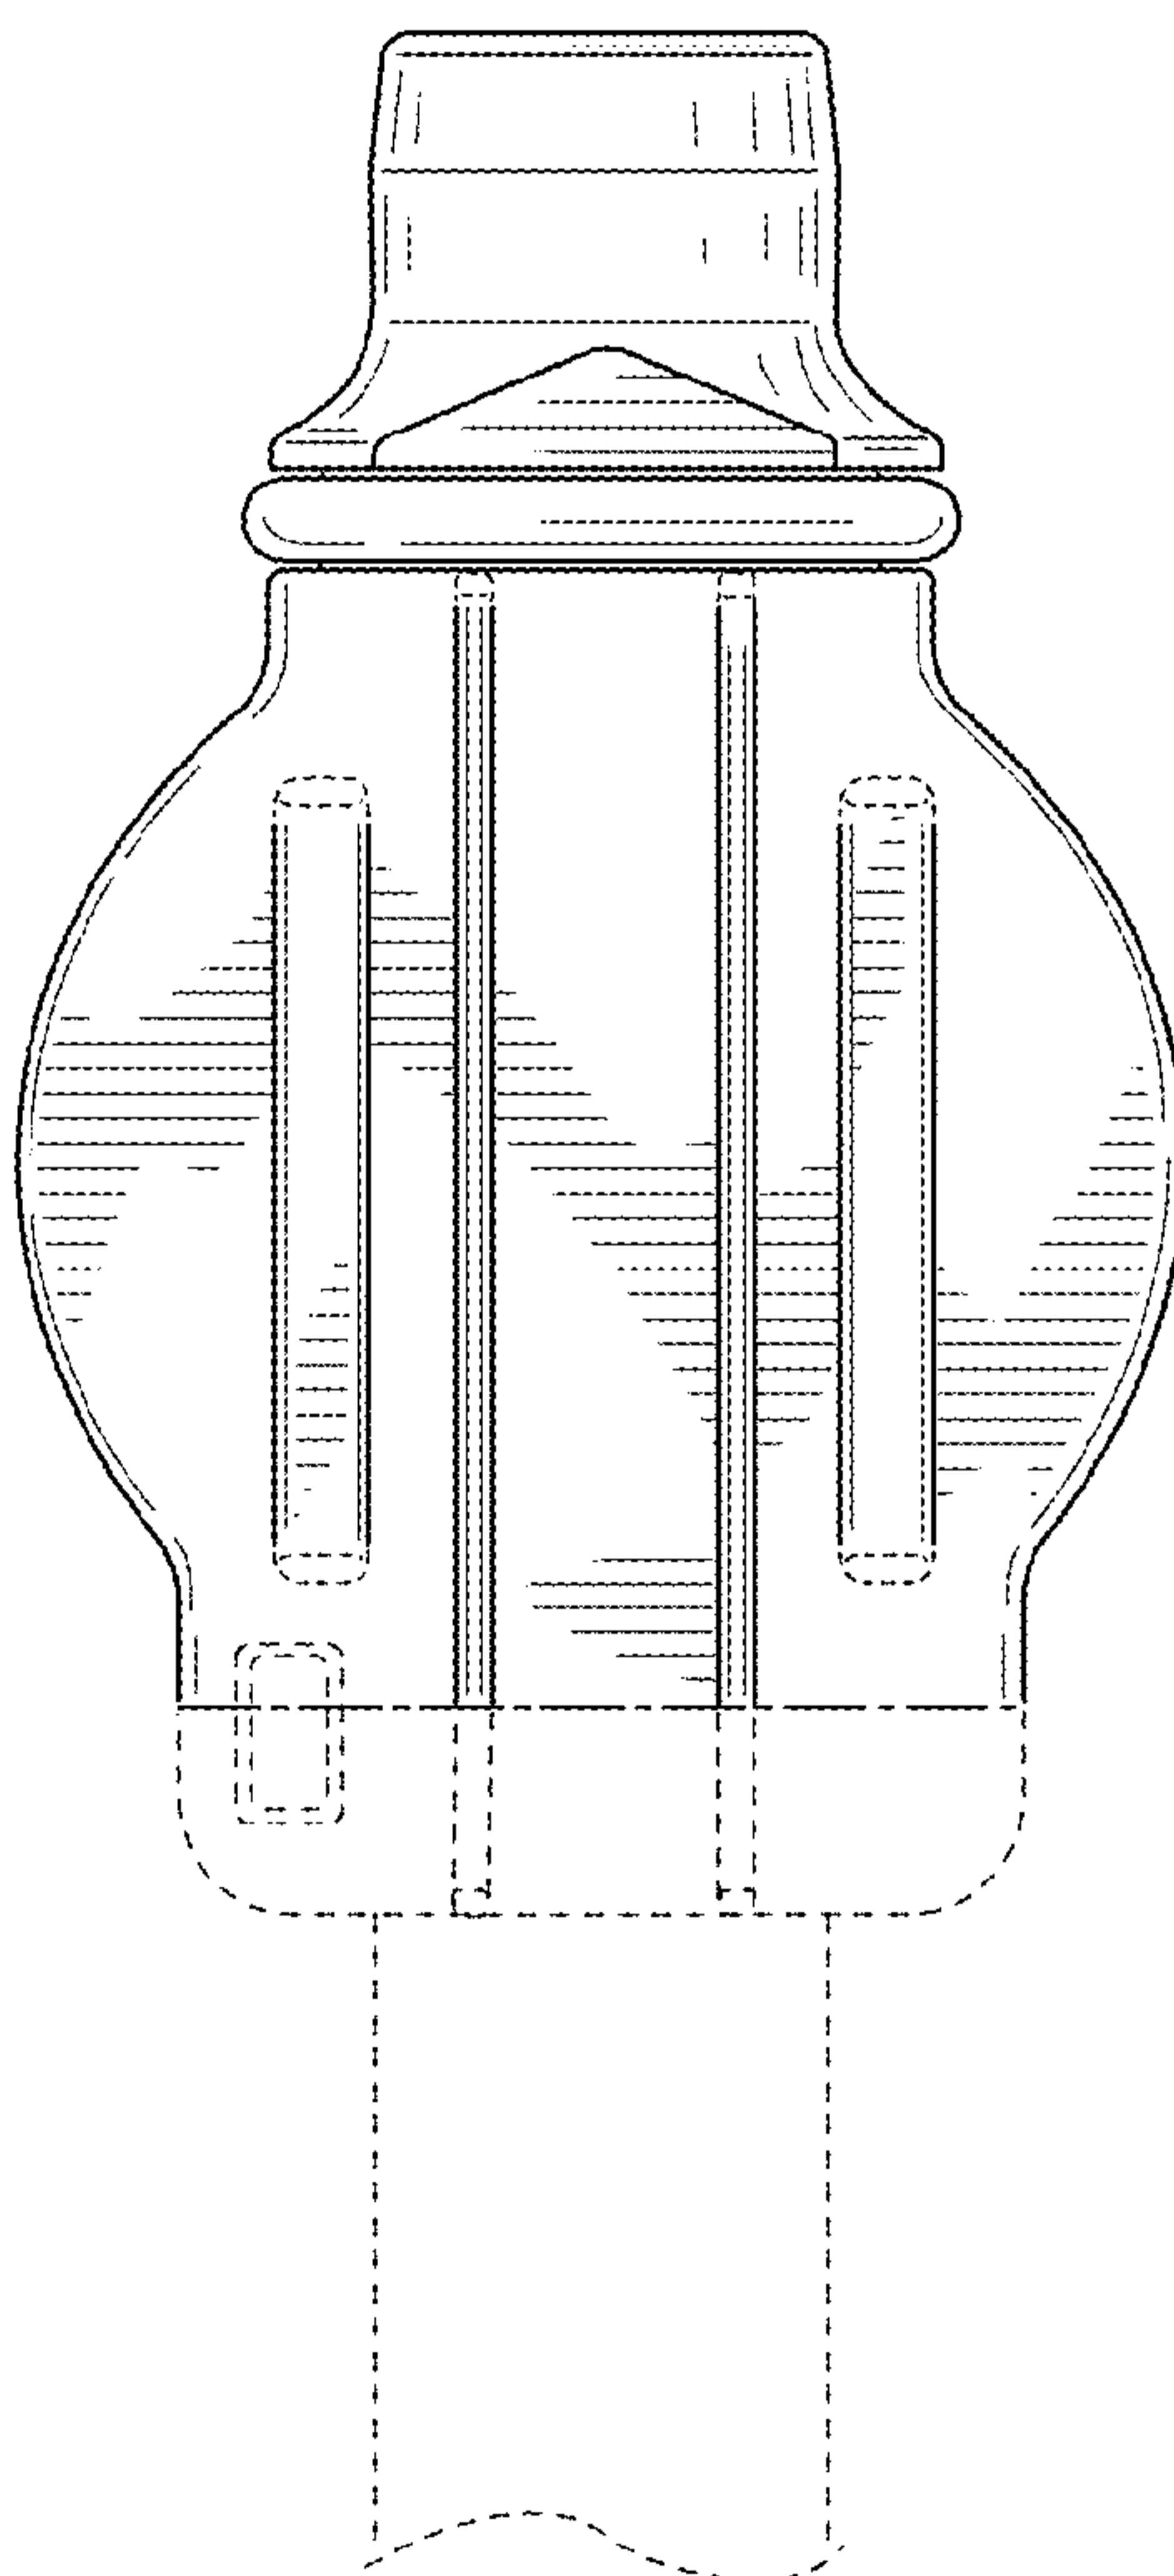


FIG. 4

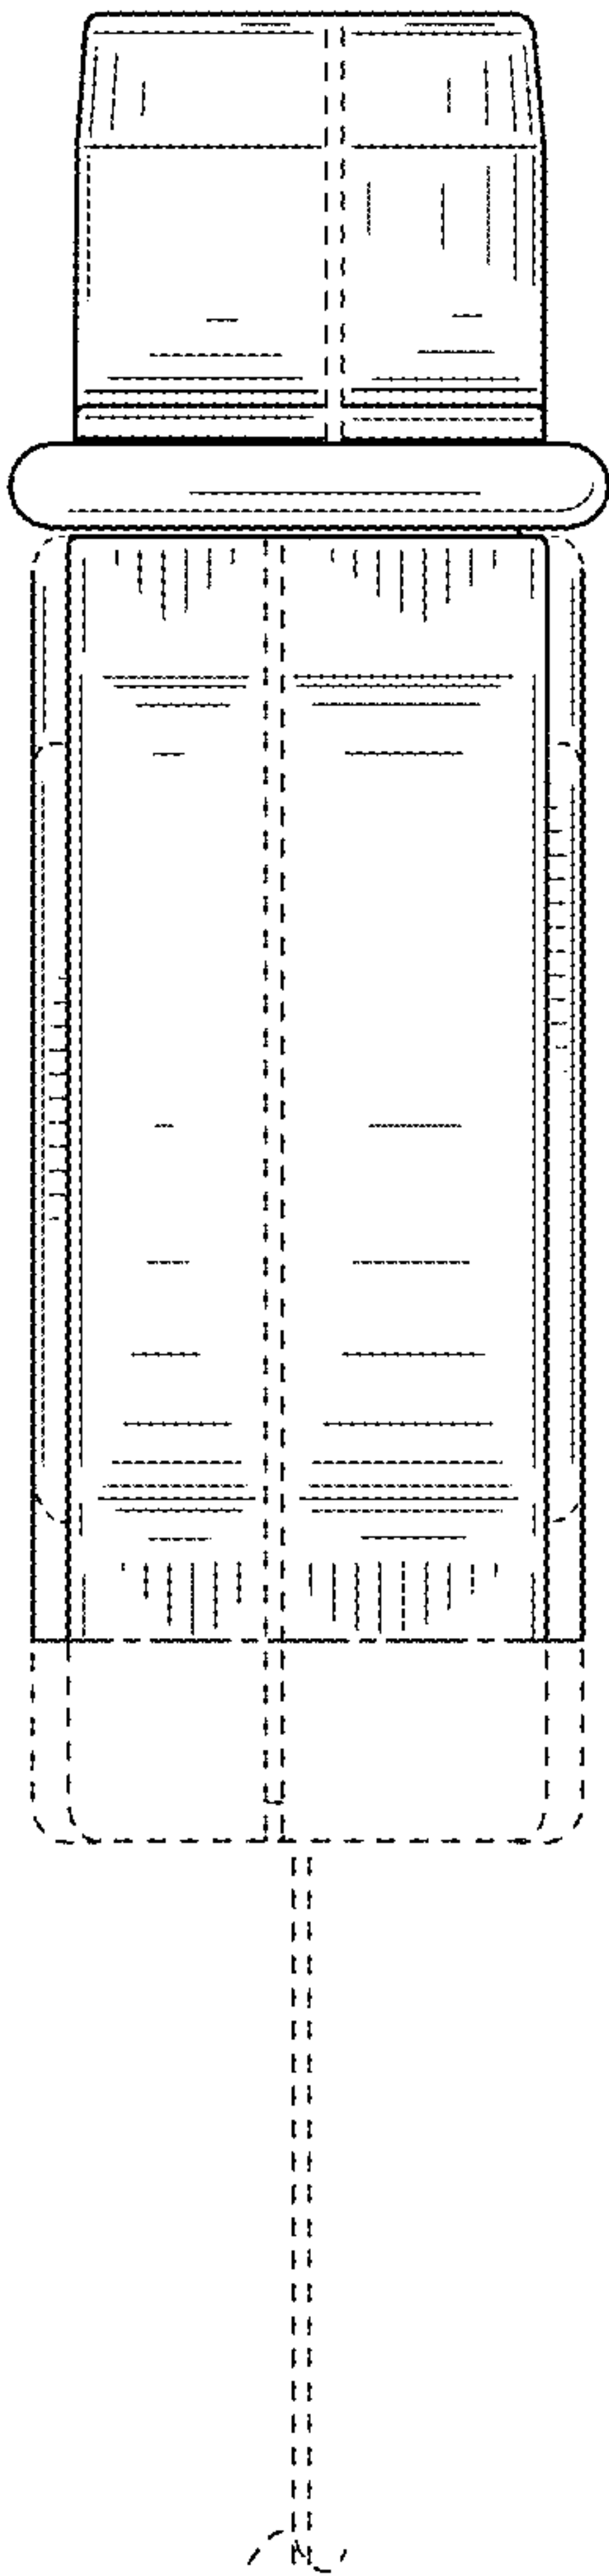


FIG. 5

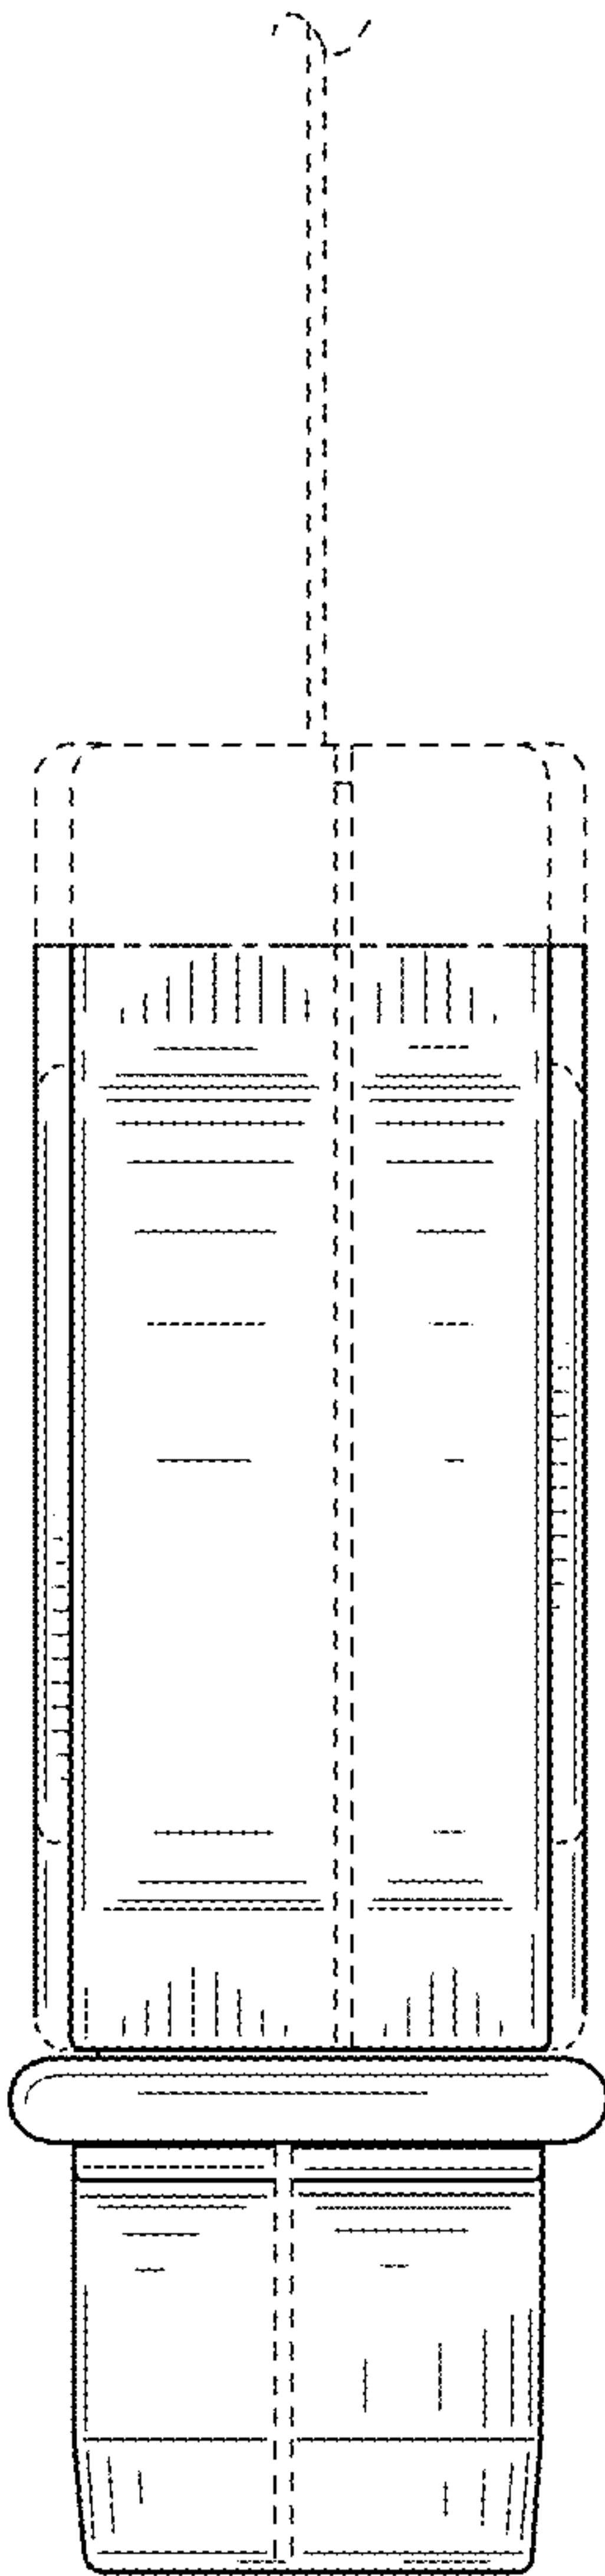


FIG. 6

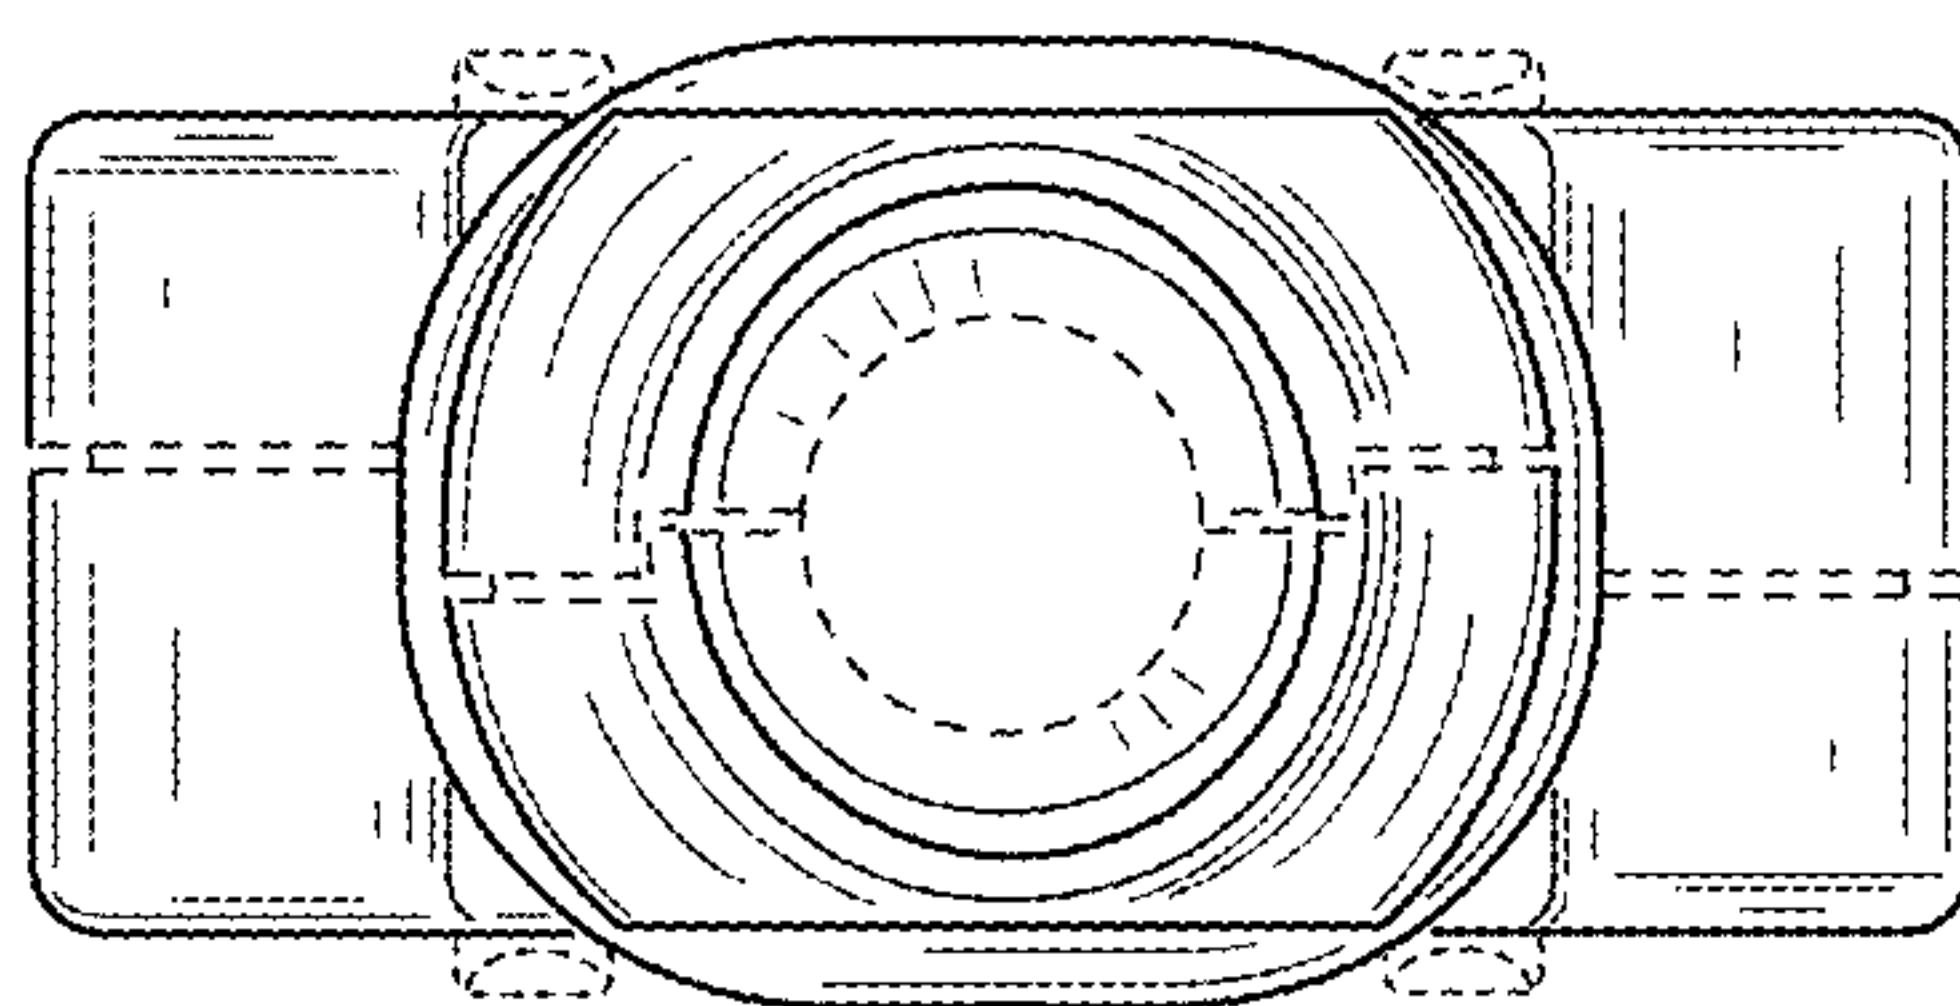


FIG. 7

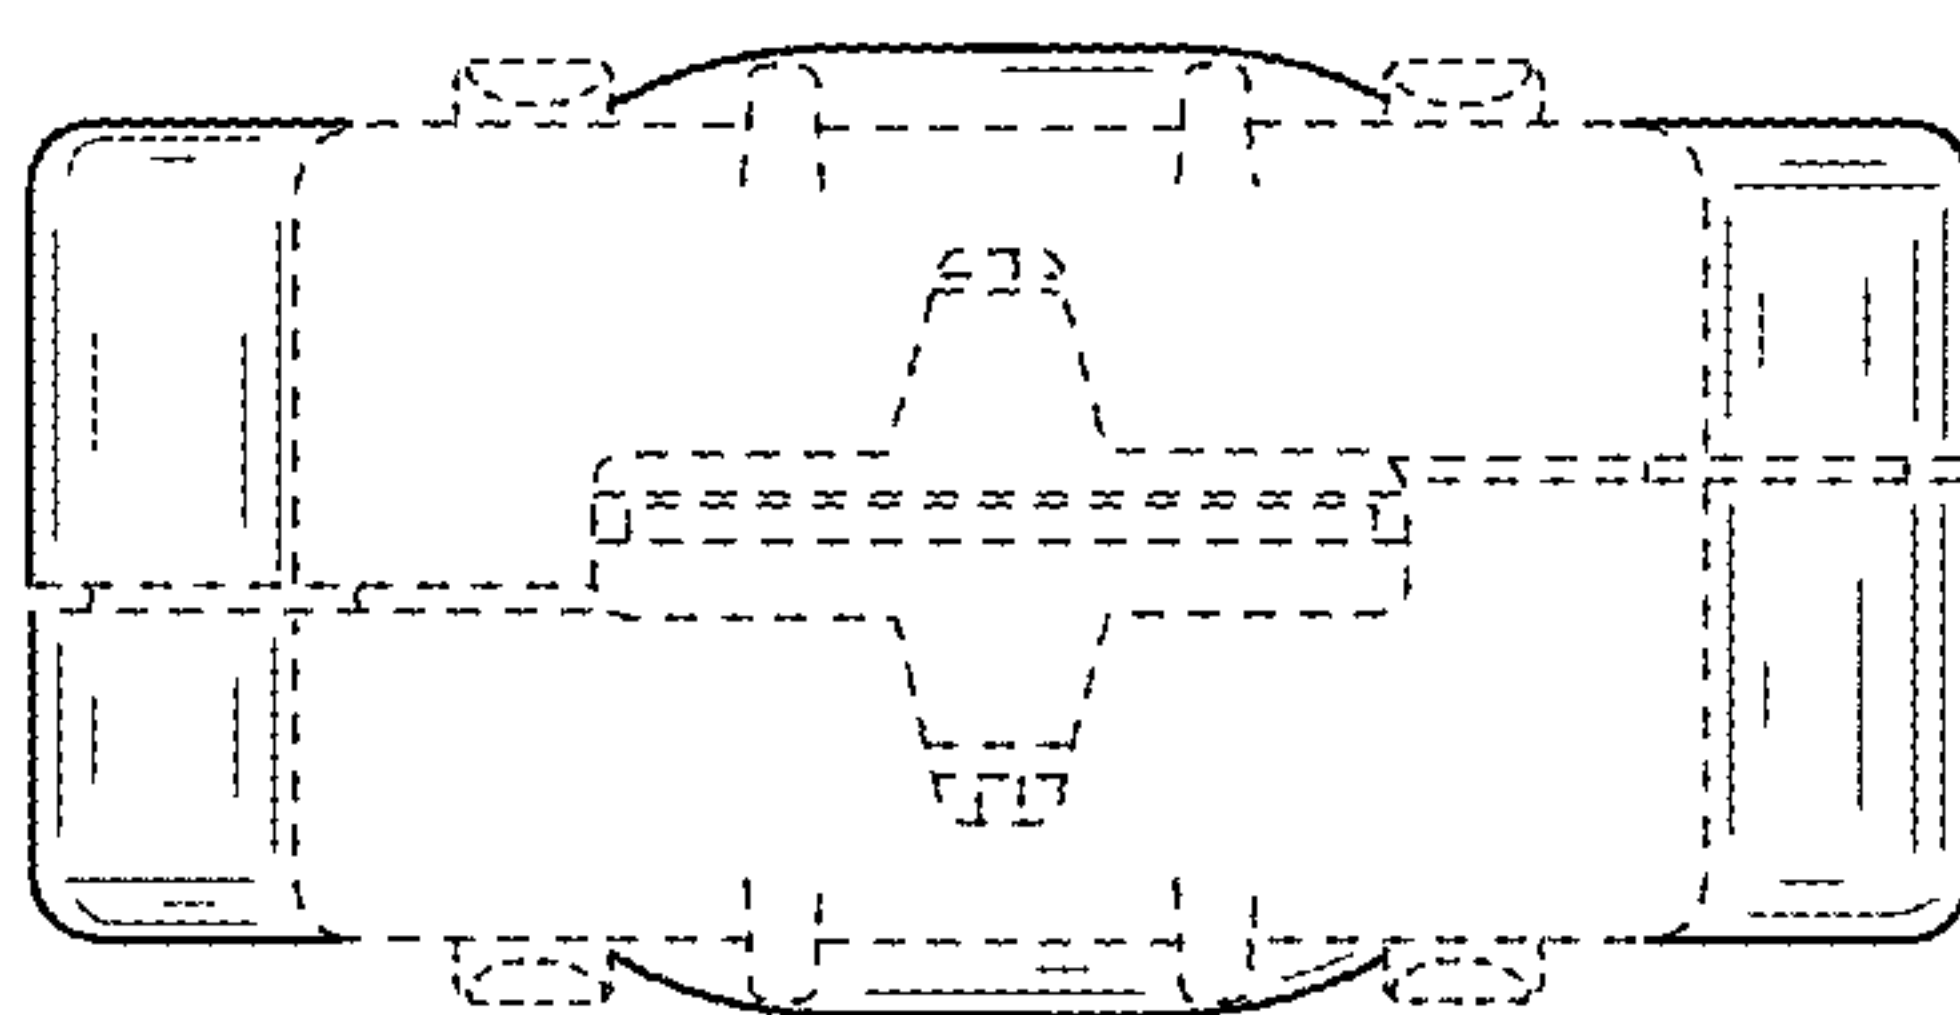


FIG. 8

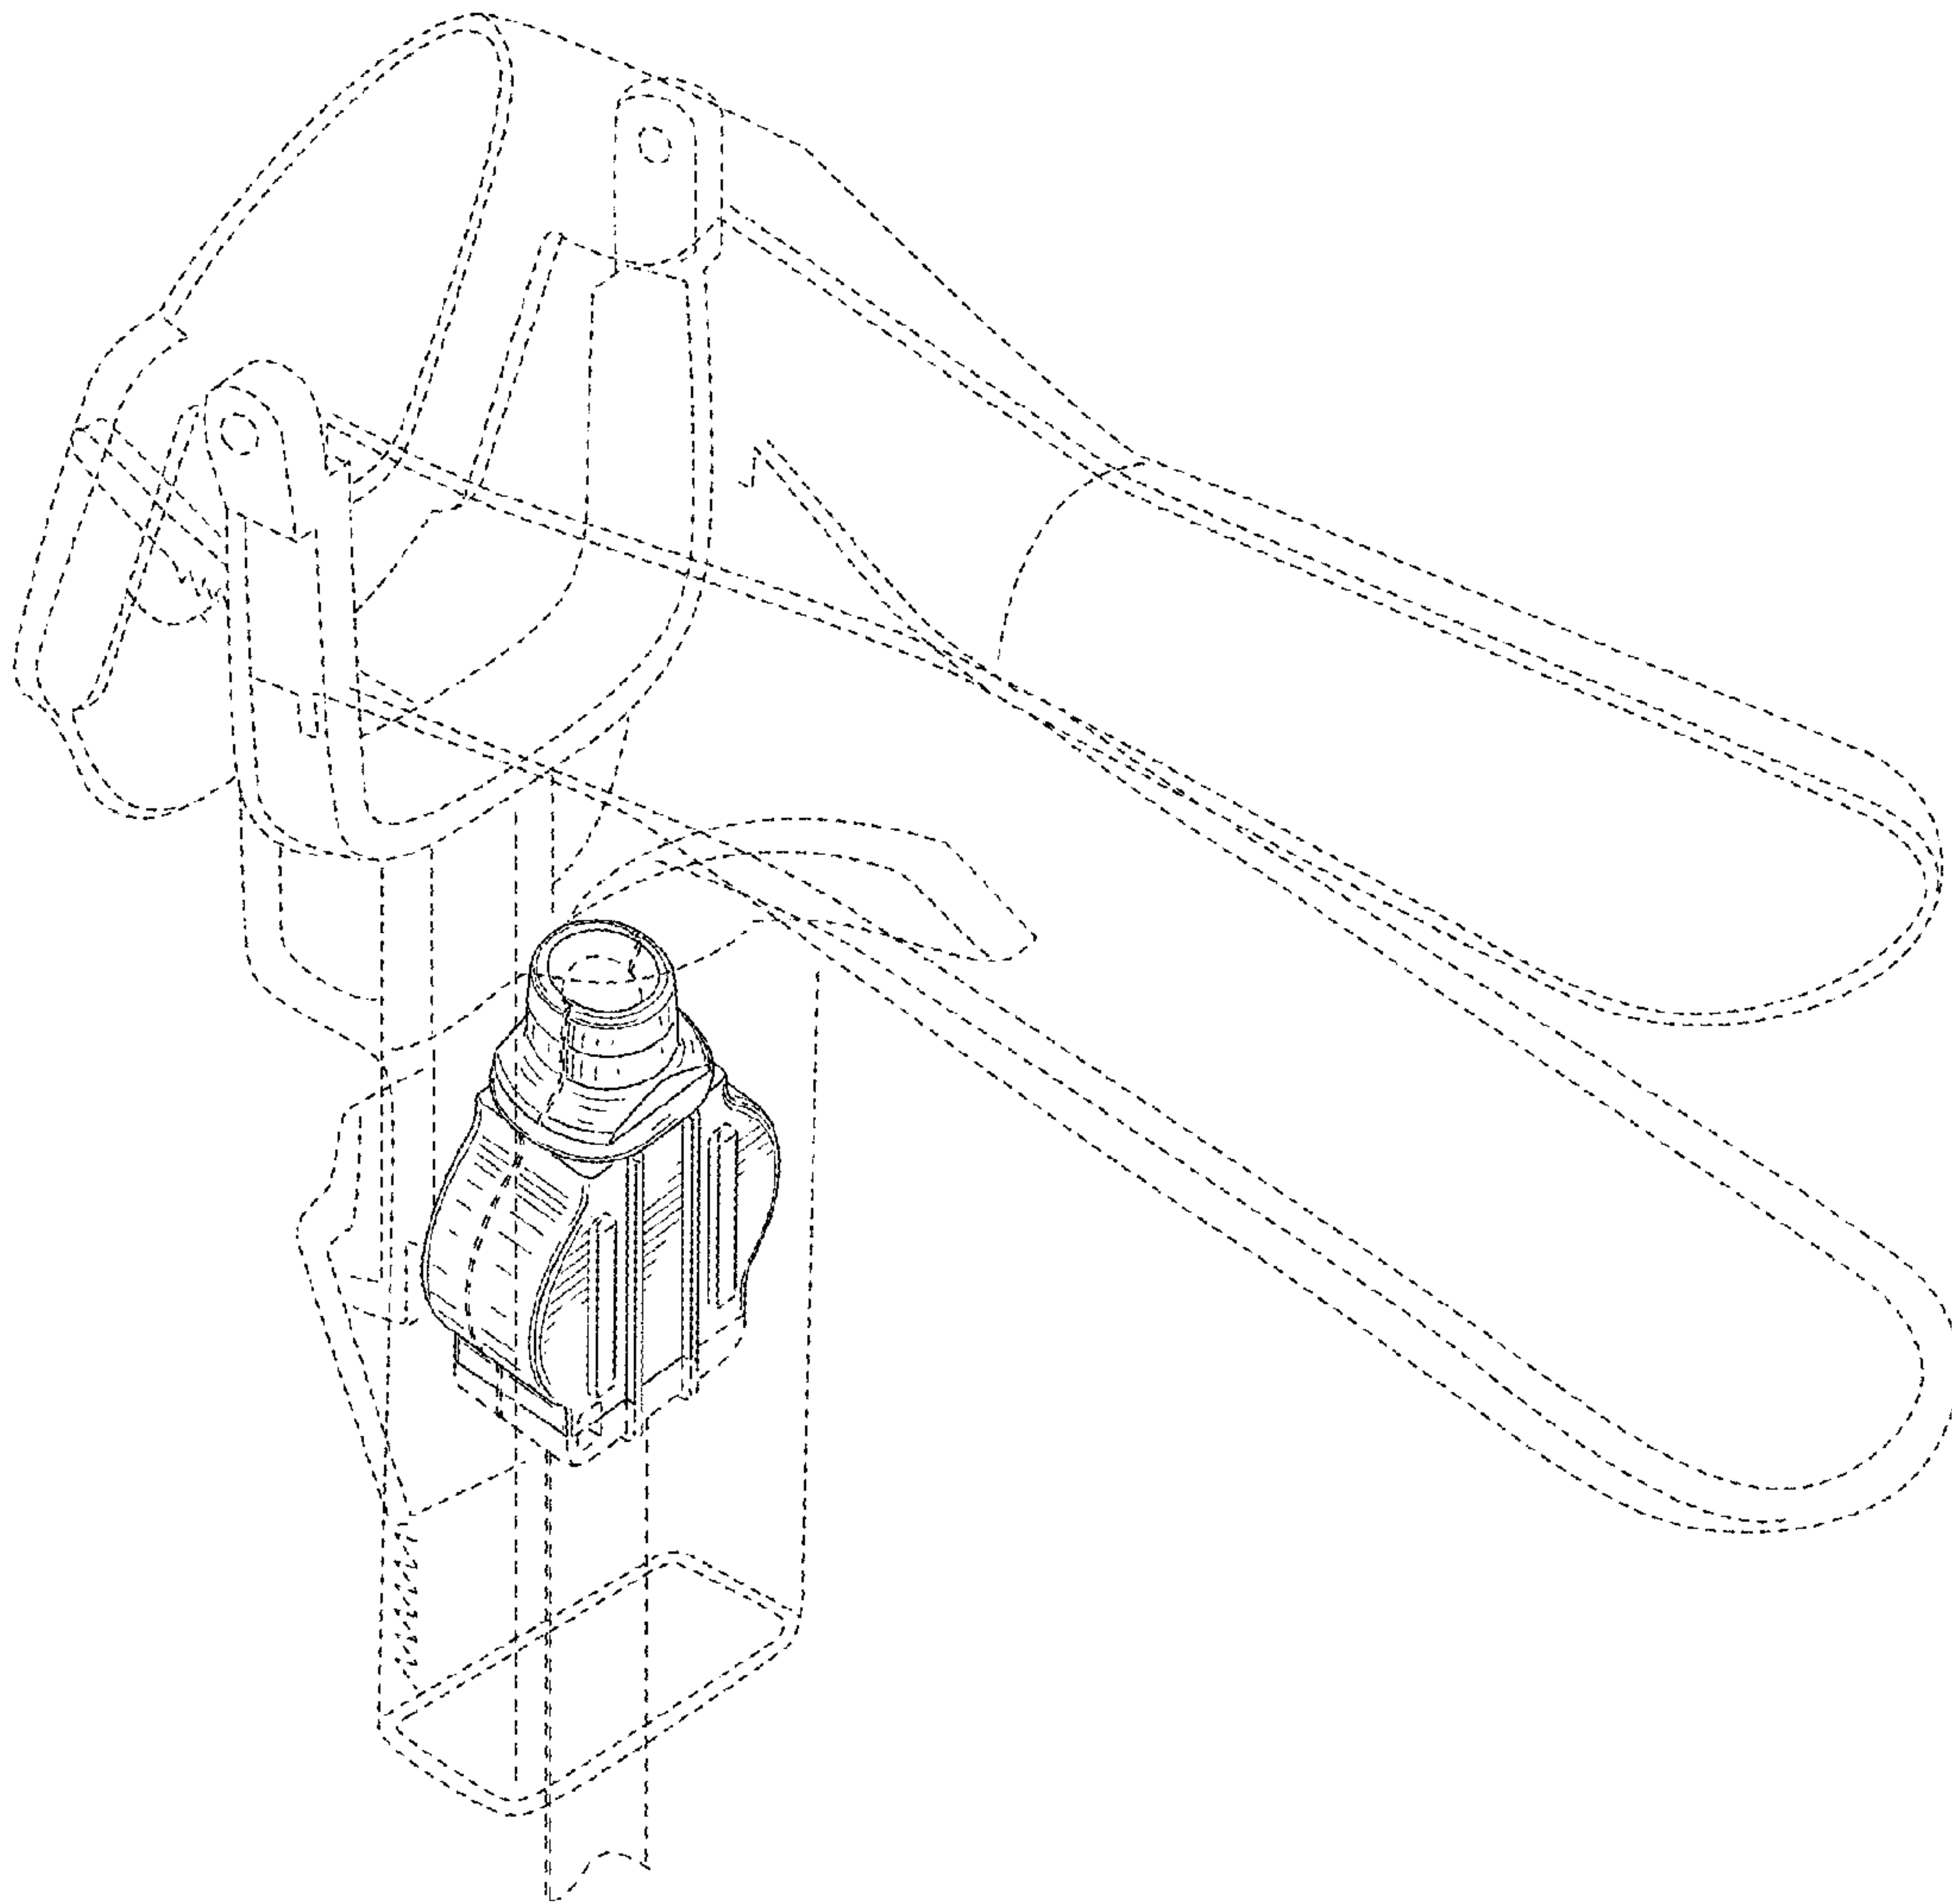


FIG. 9

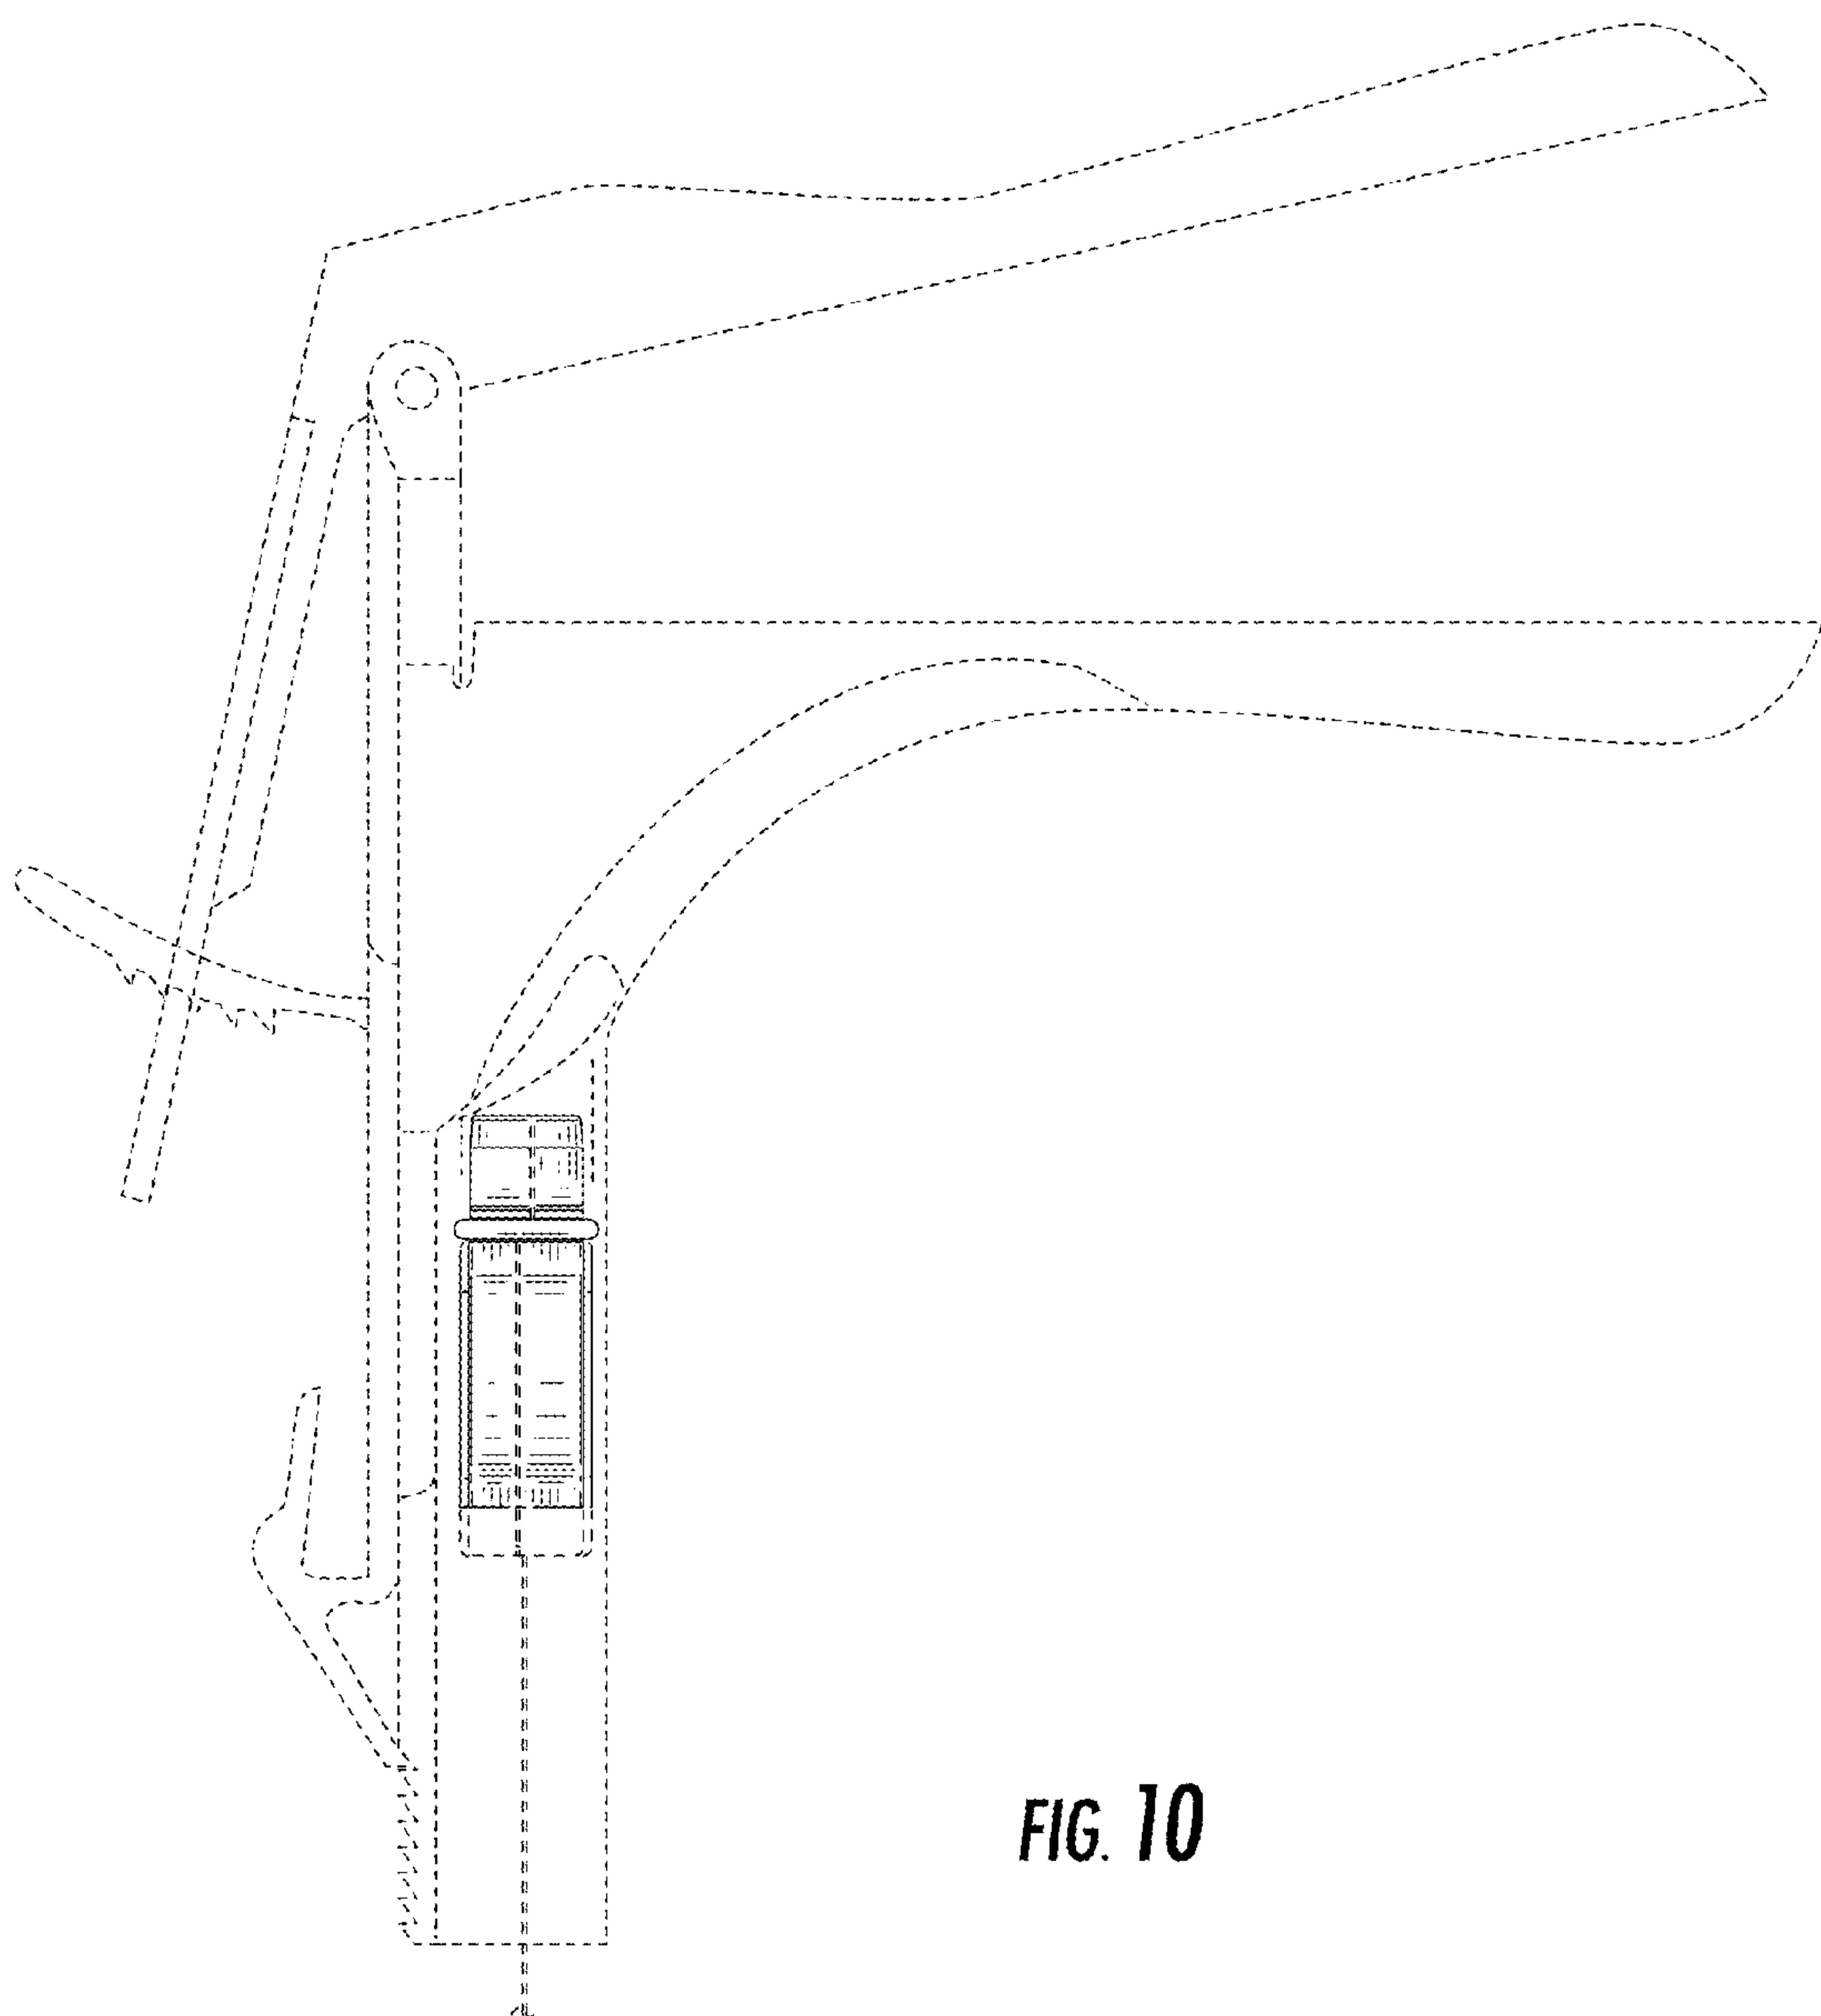


FIG. 10

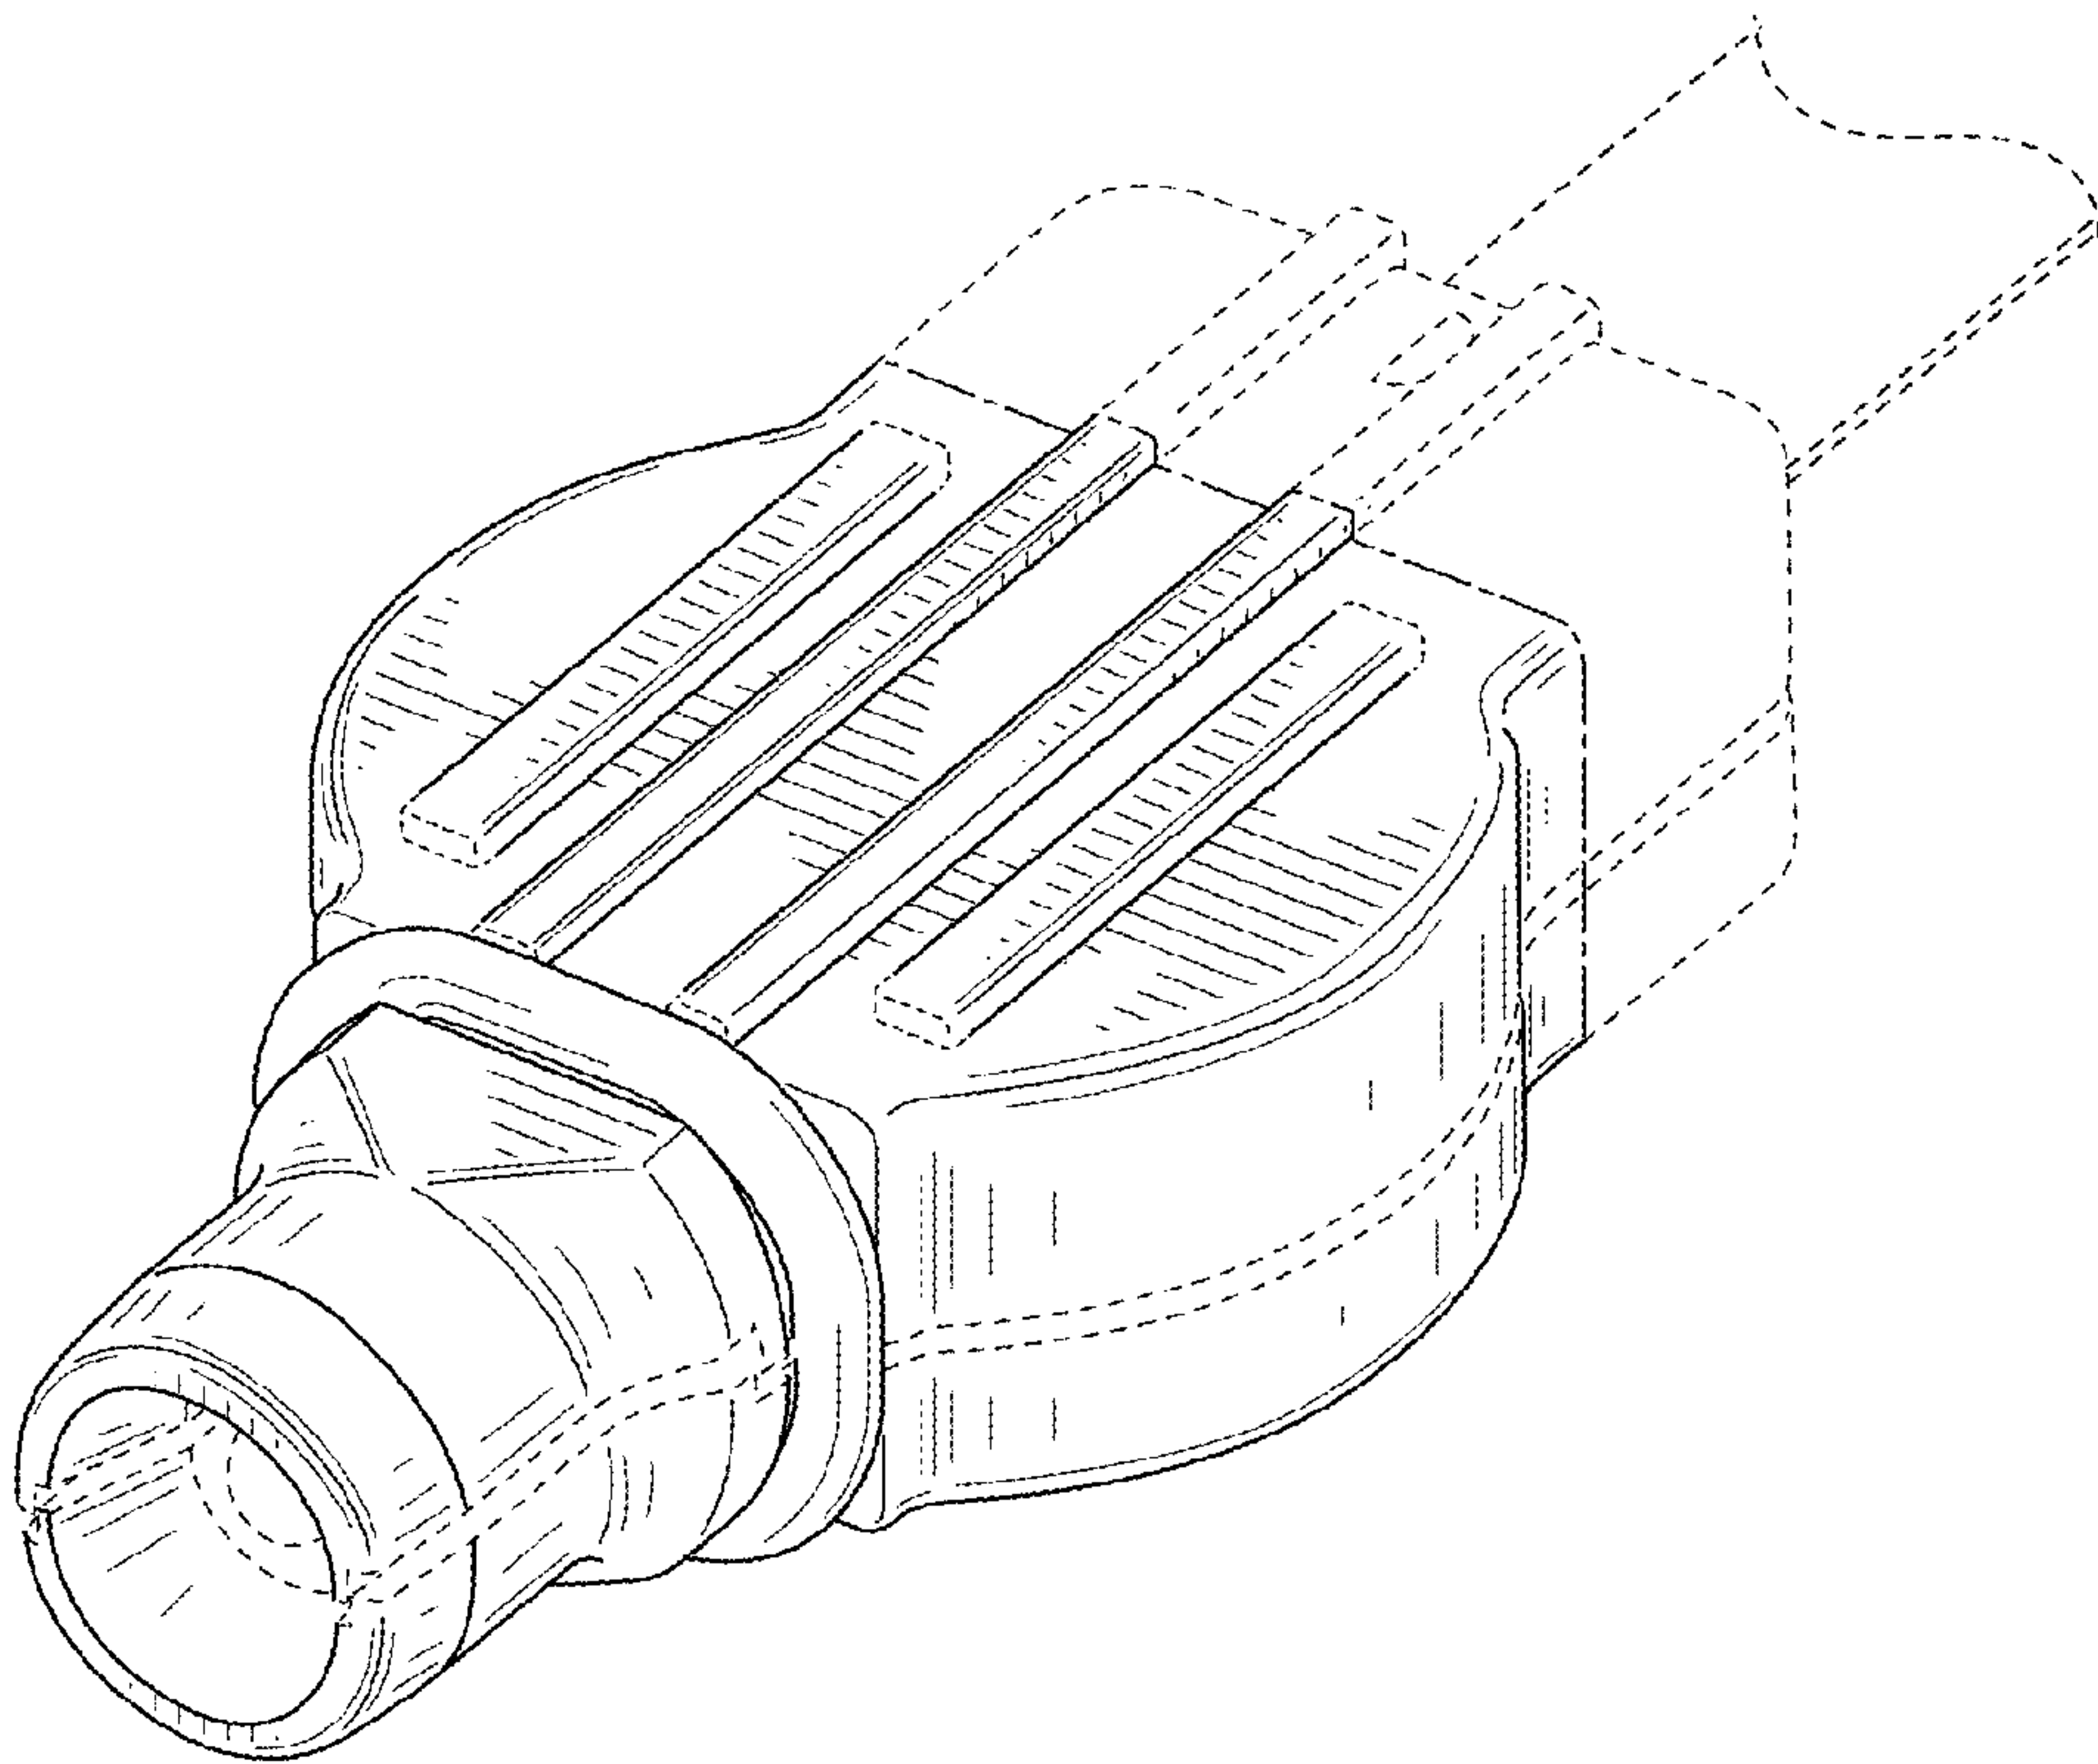


FIG. 11

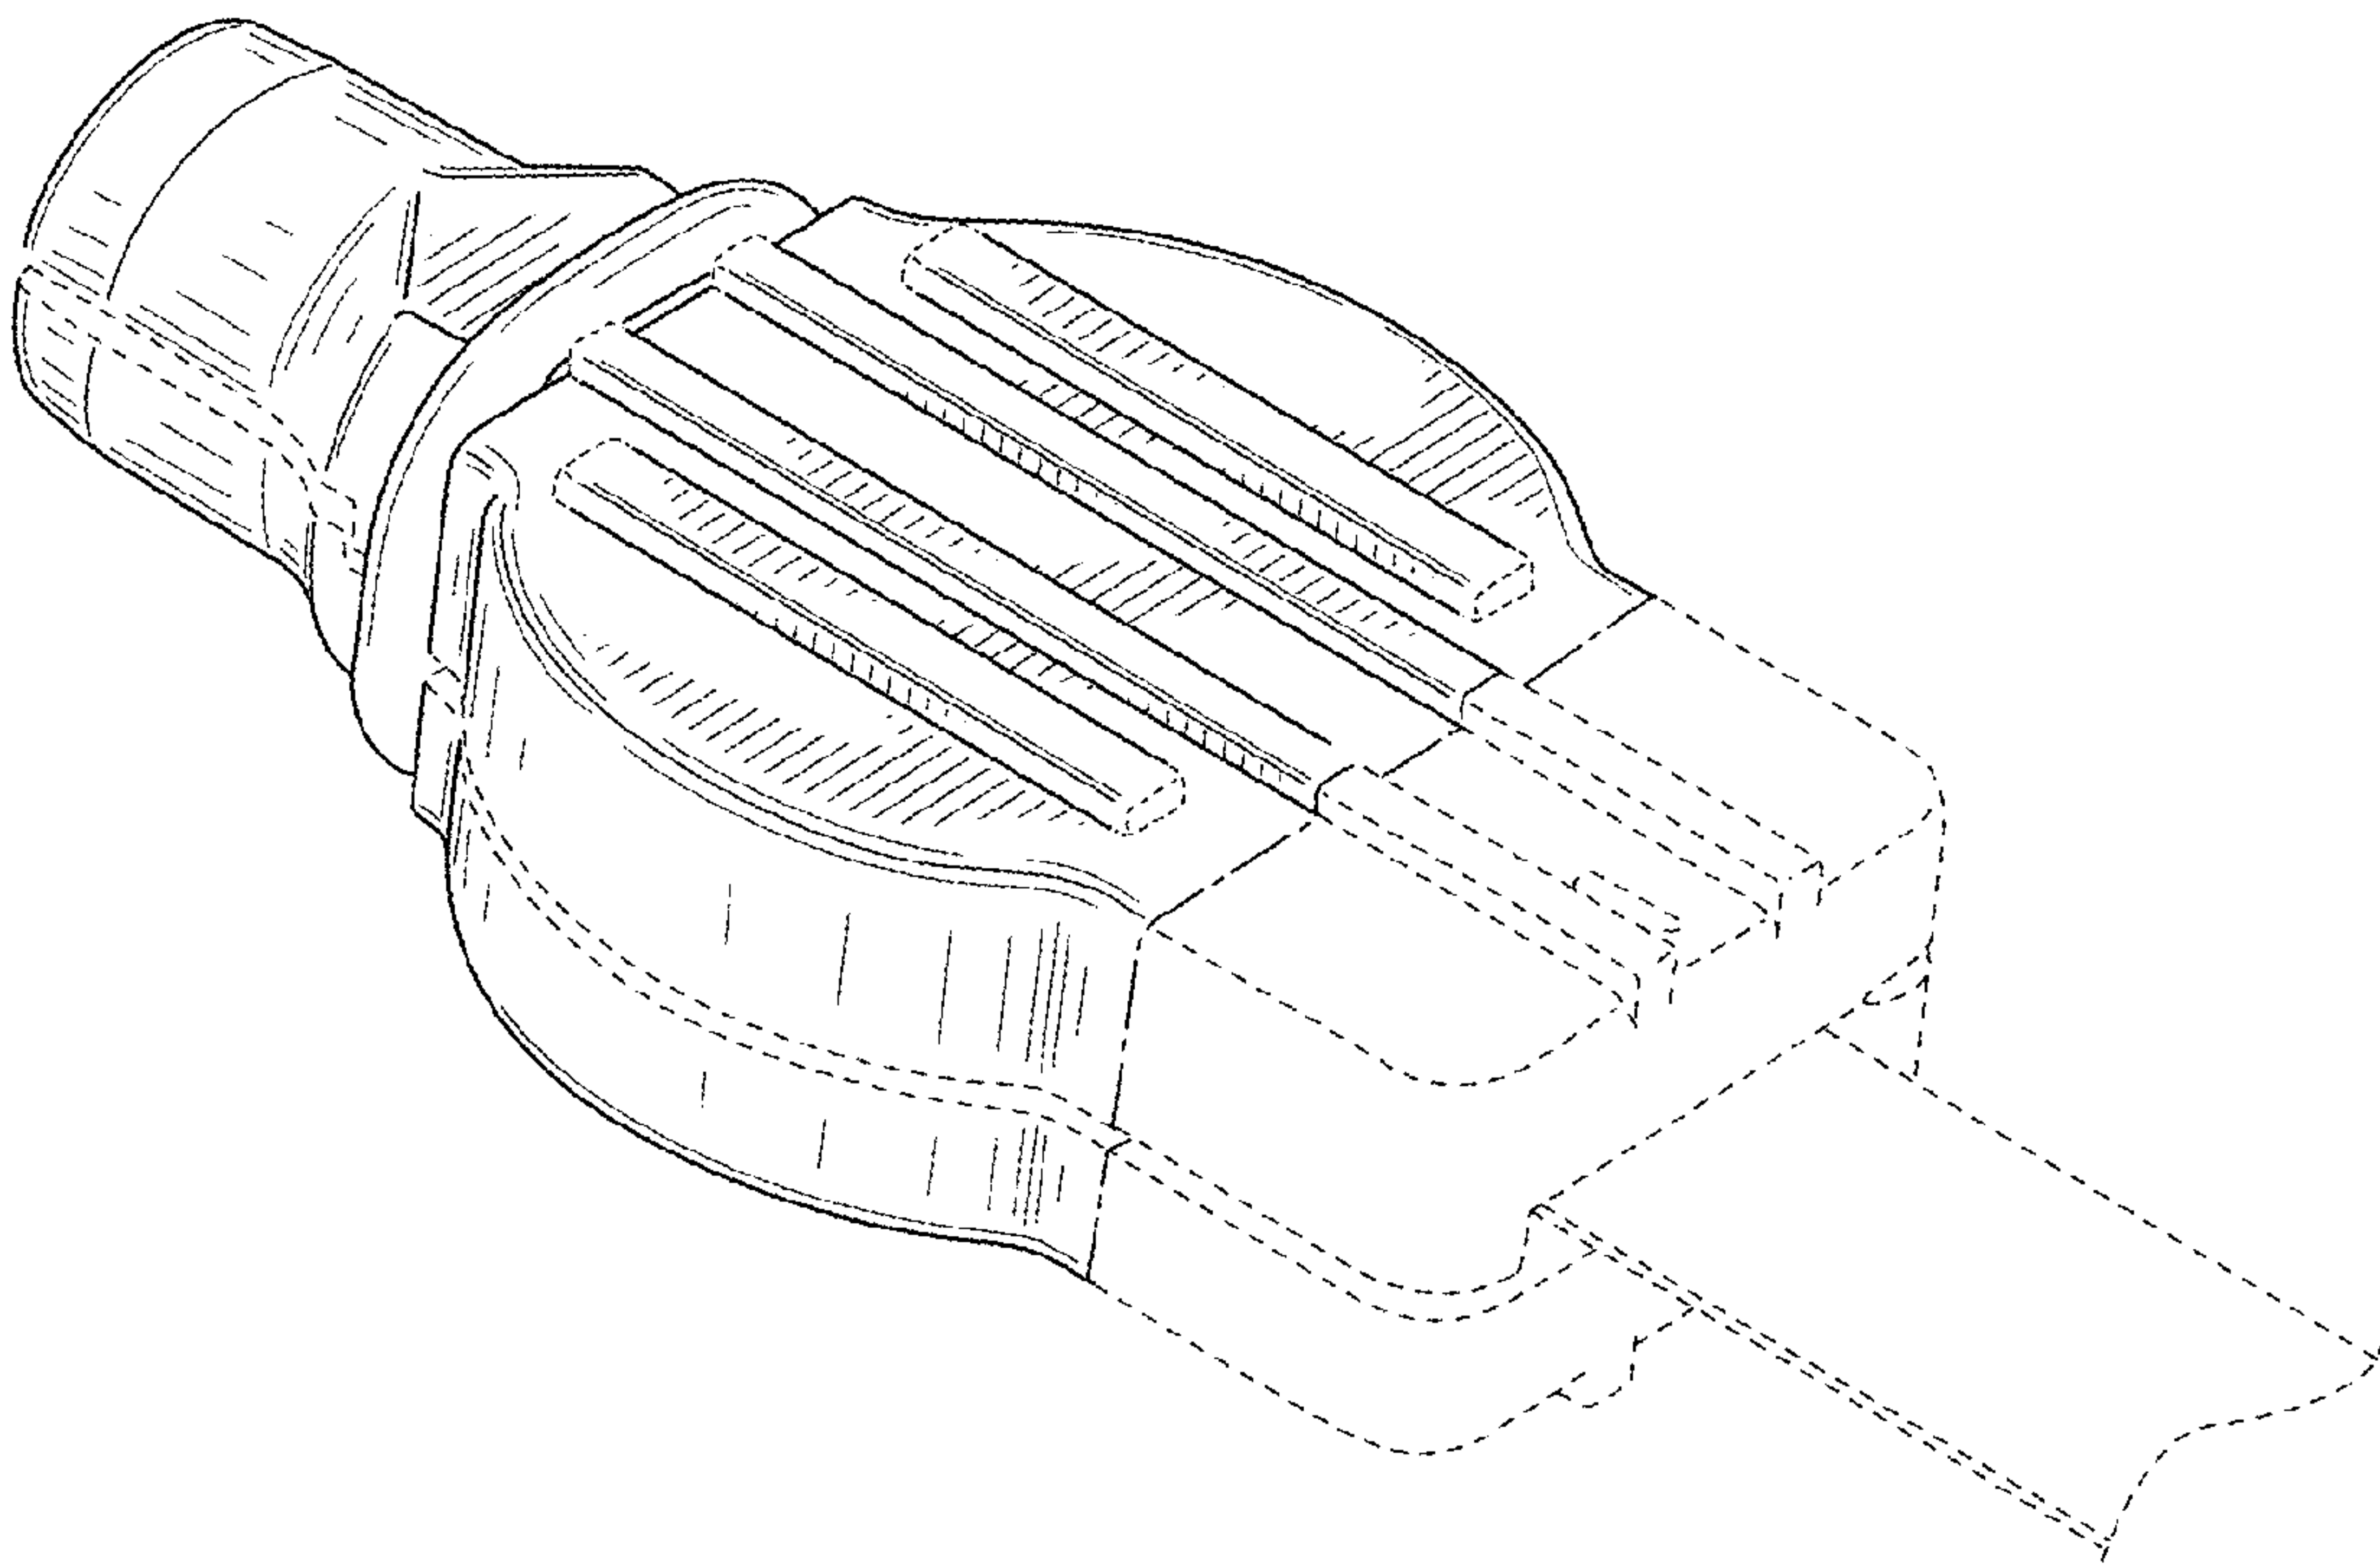


FIG. 12

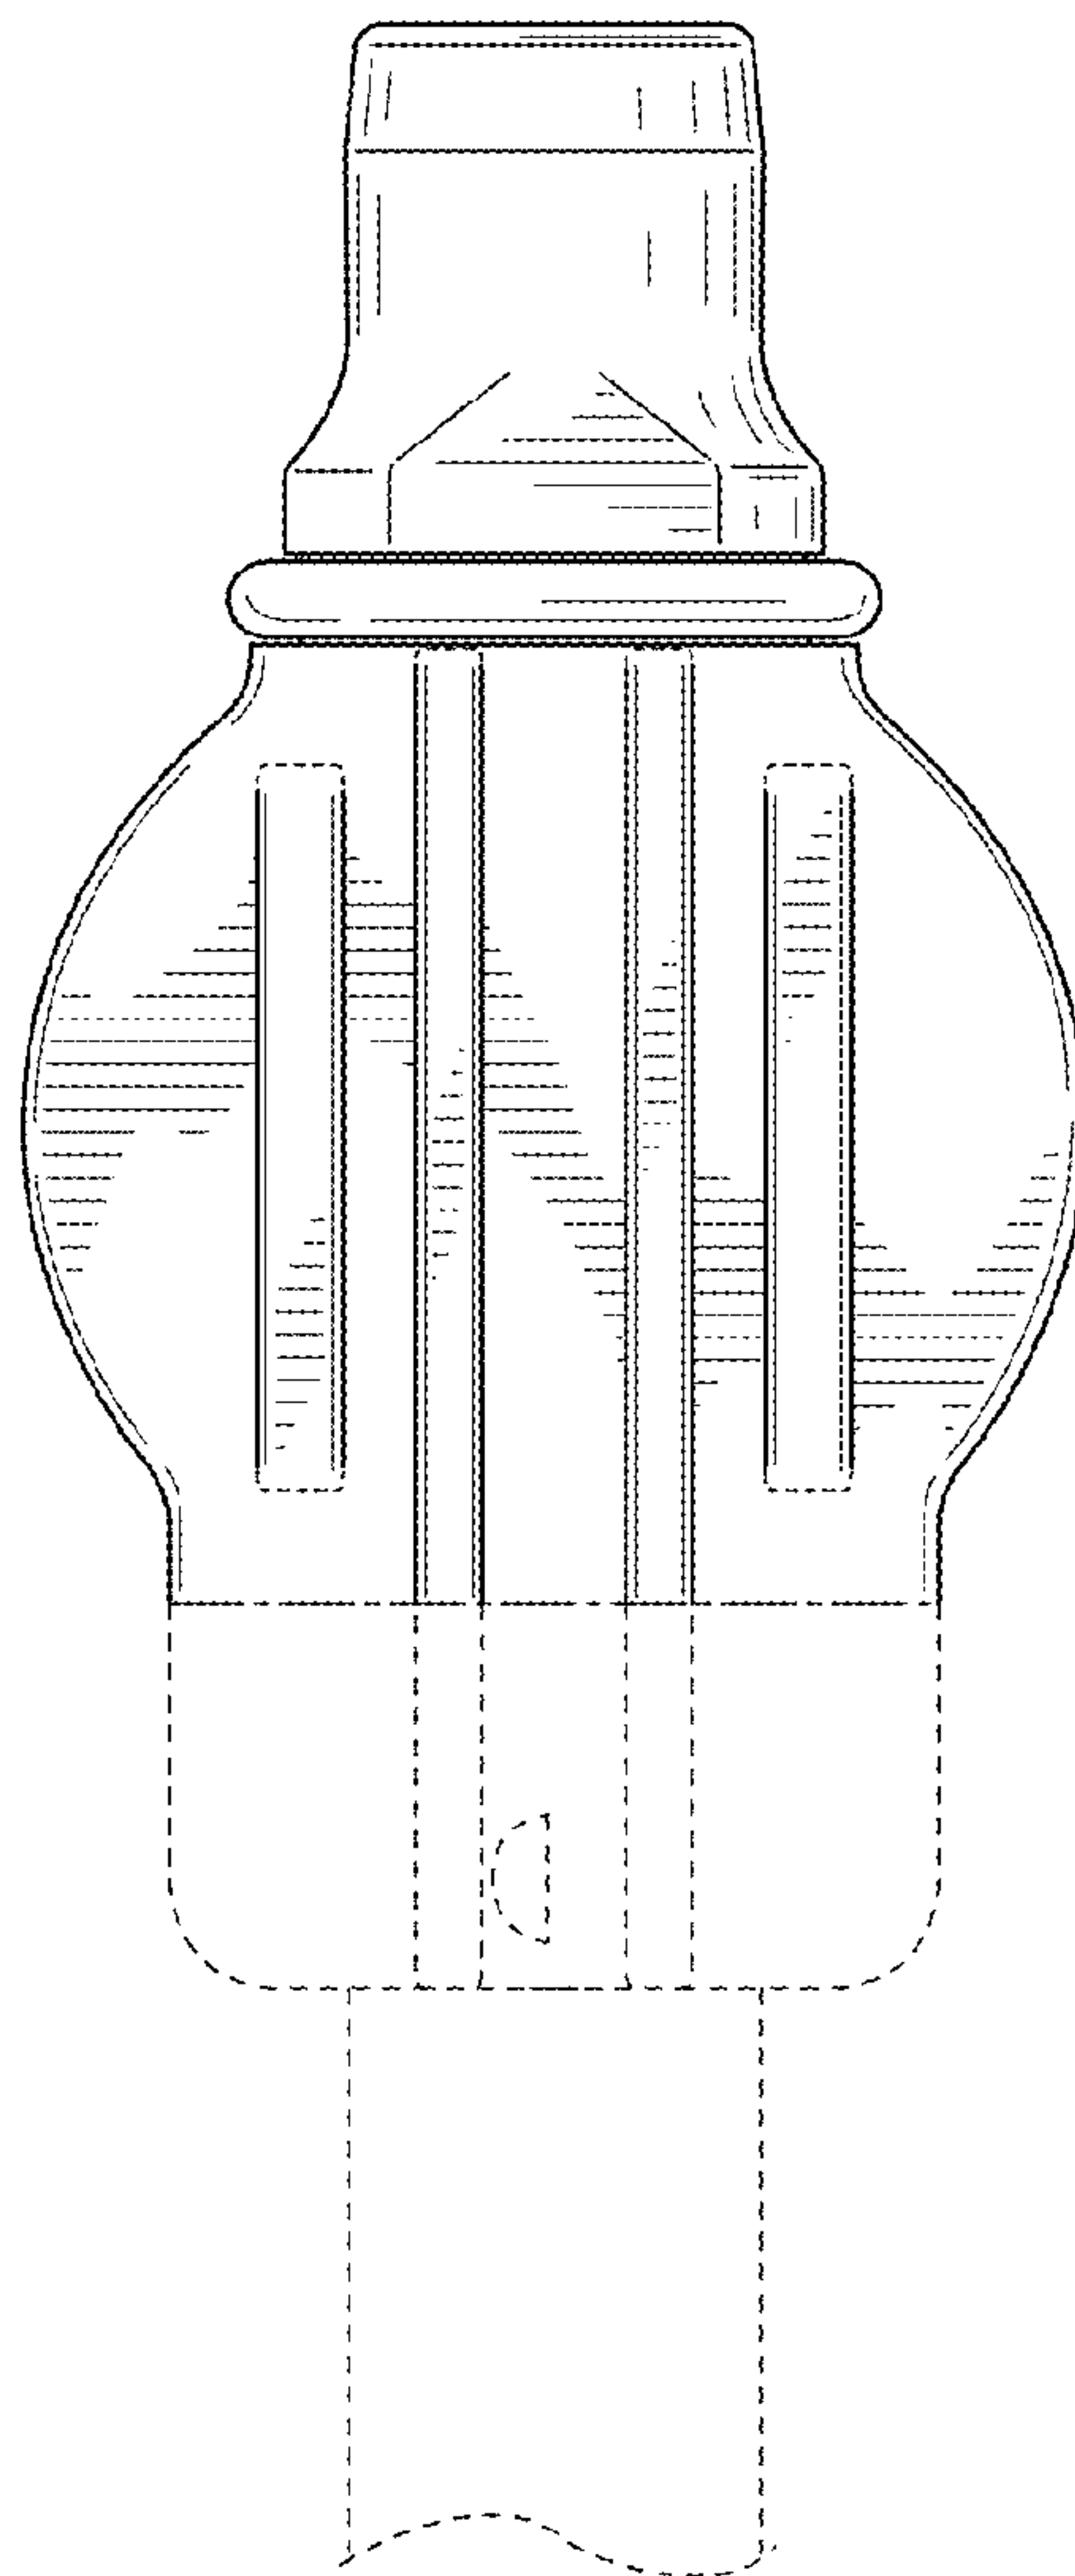


FIG. 13

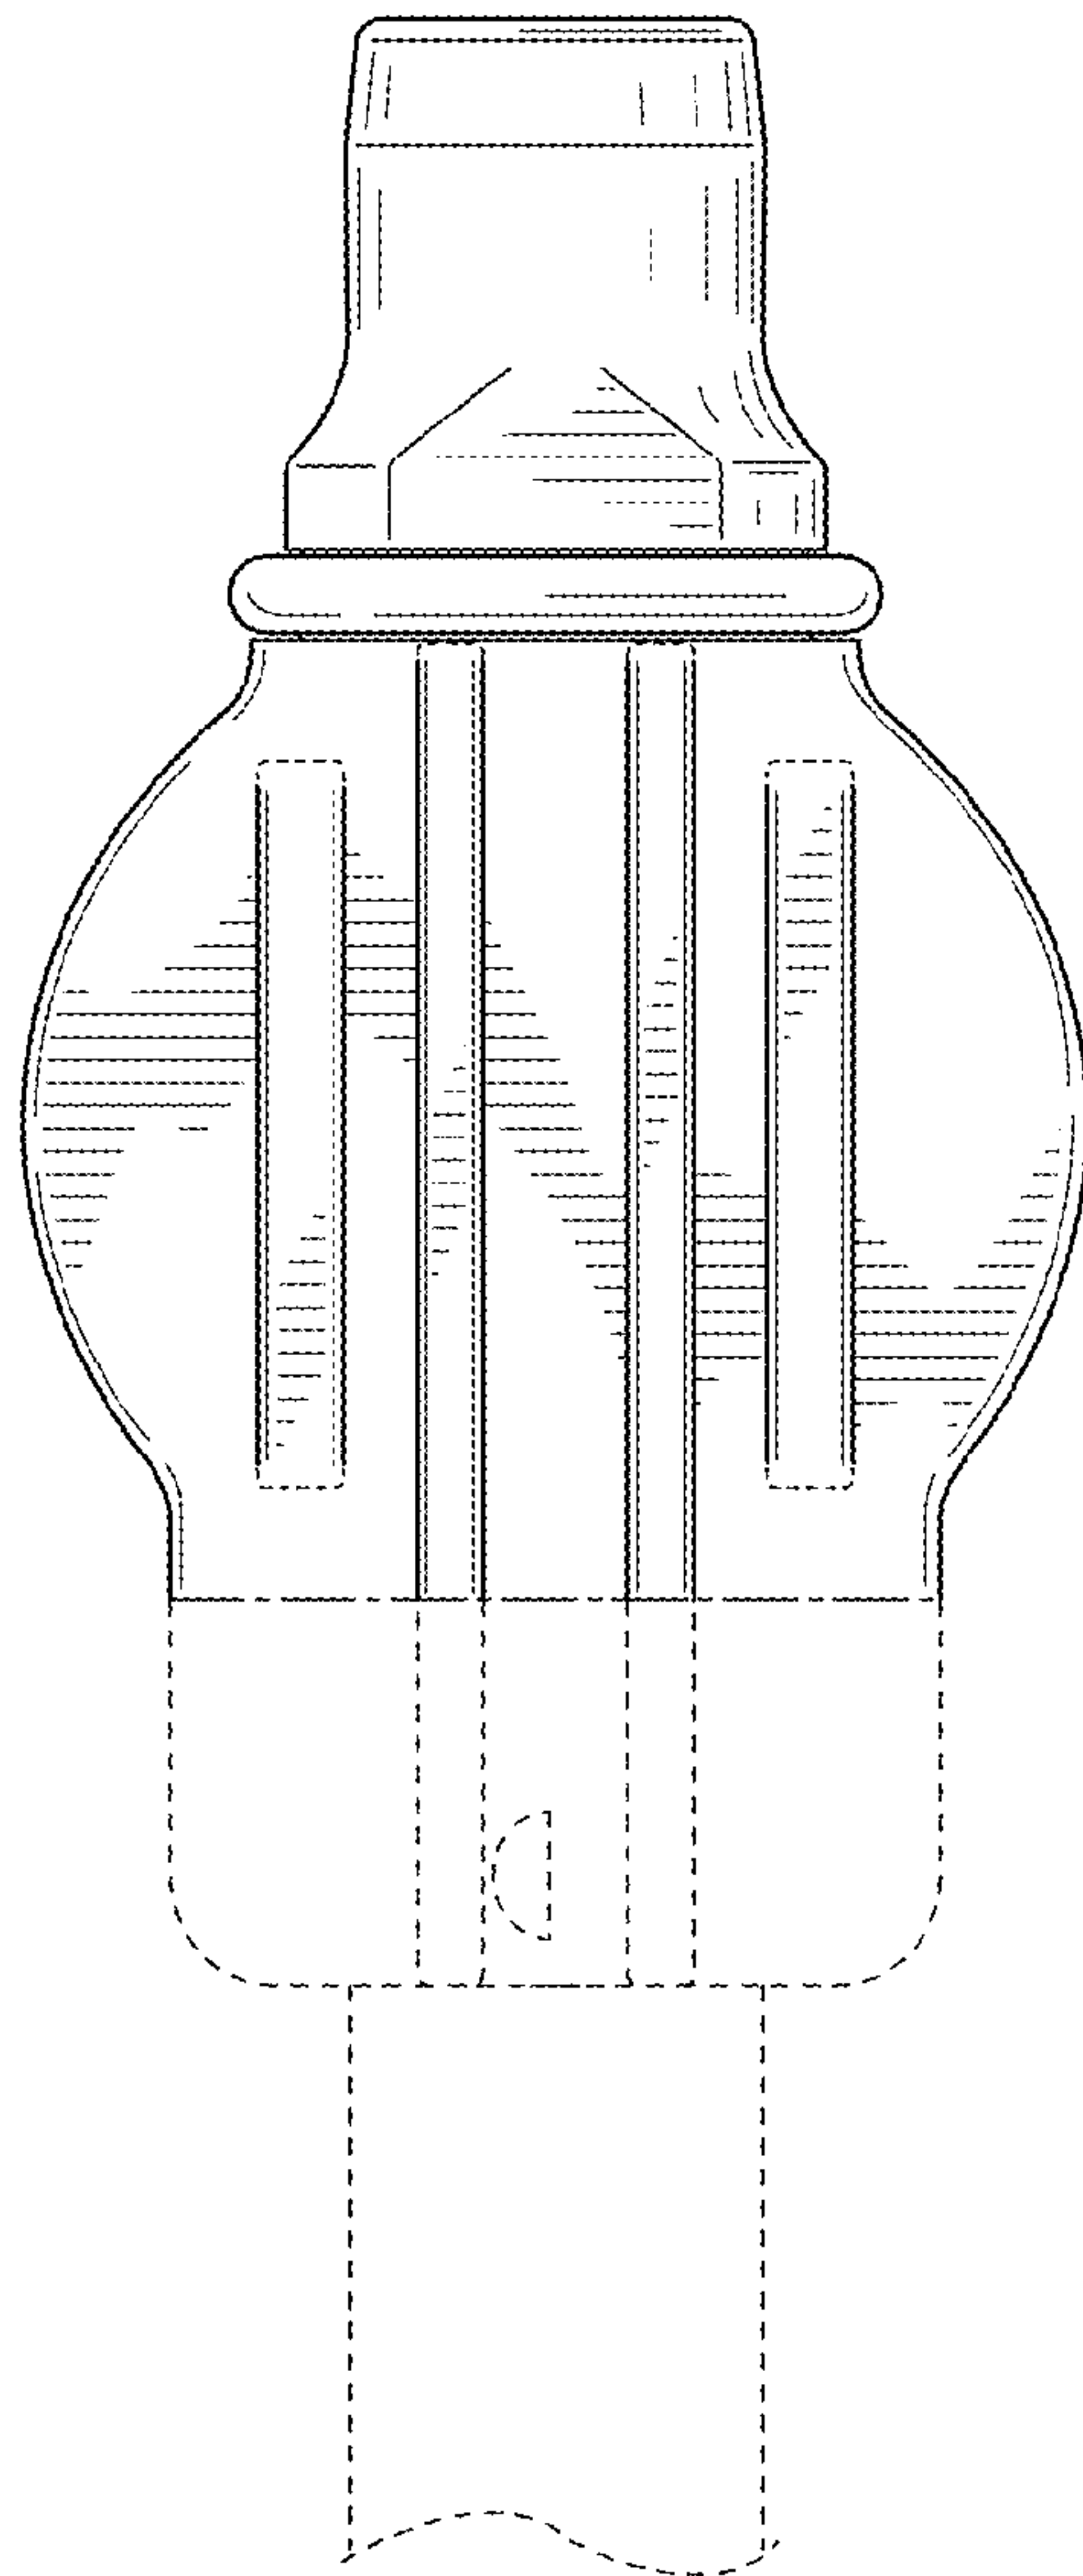


FIG. 14

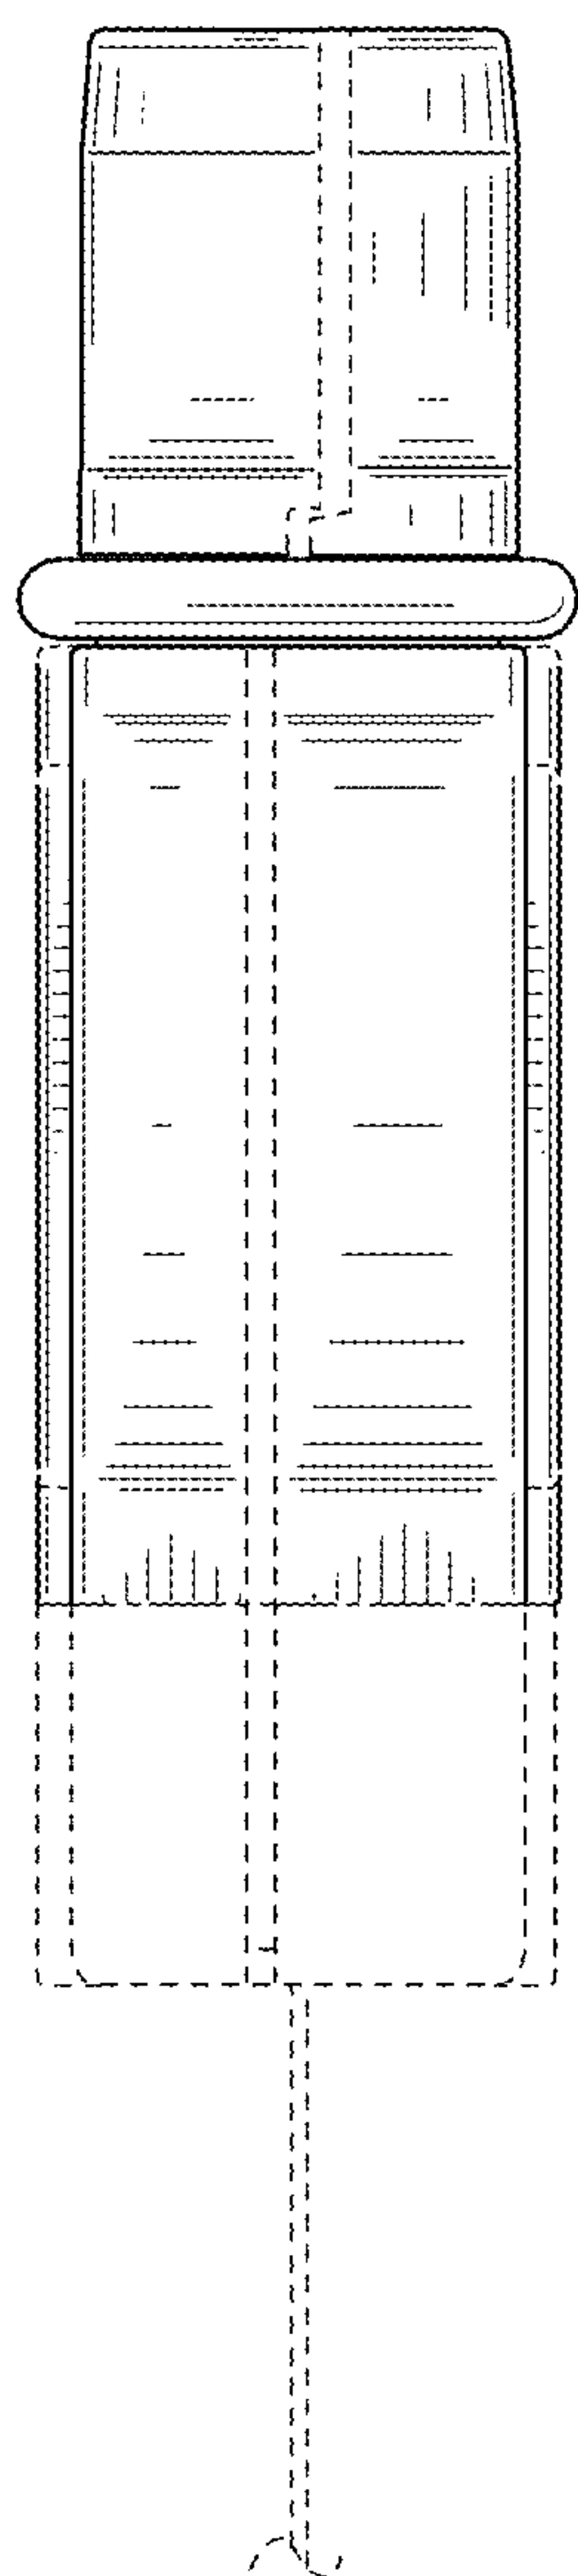


FIG. 15

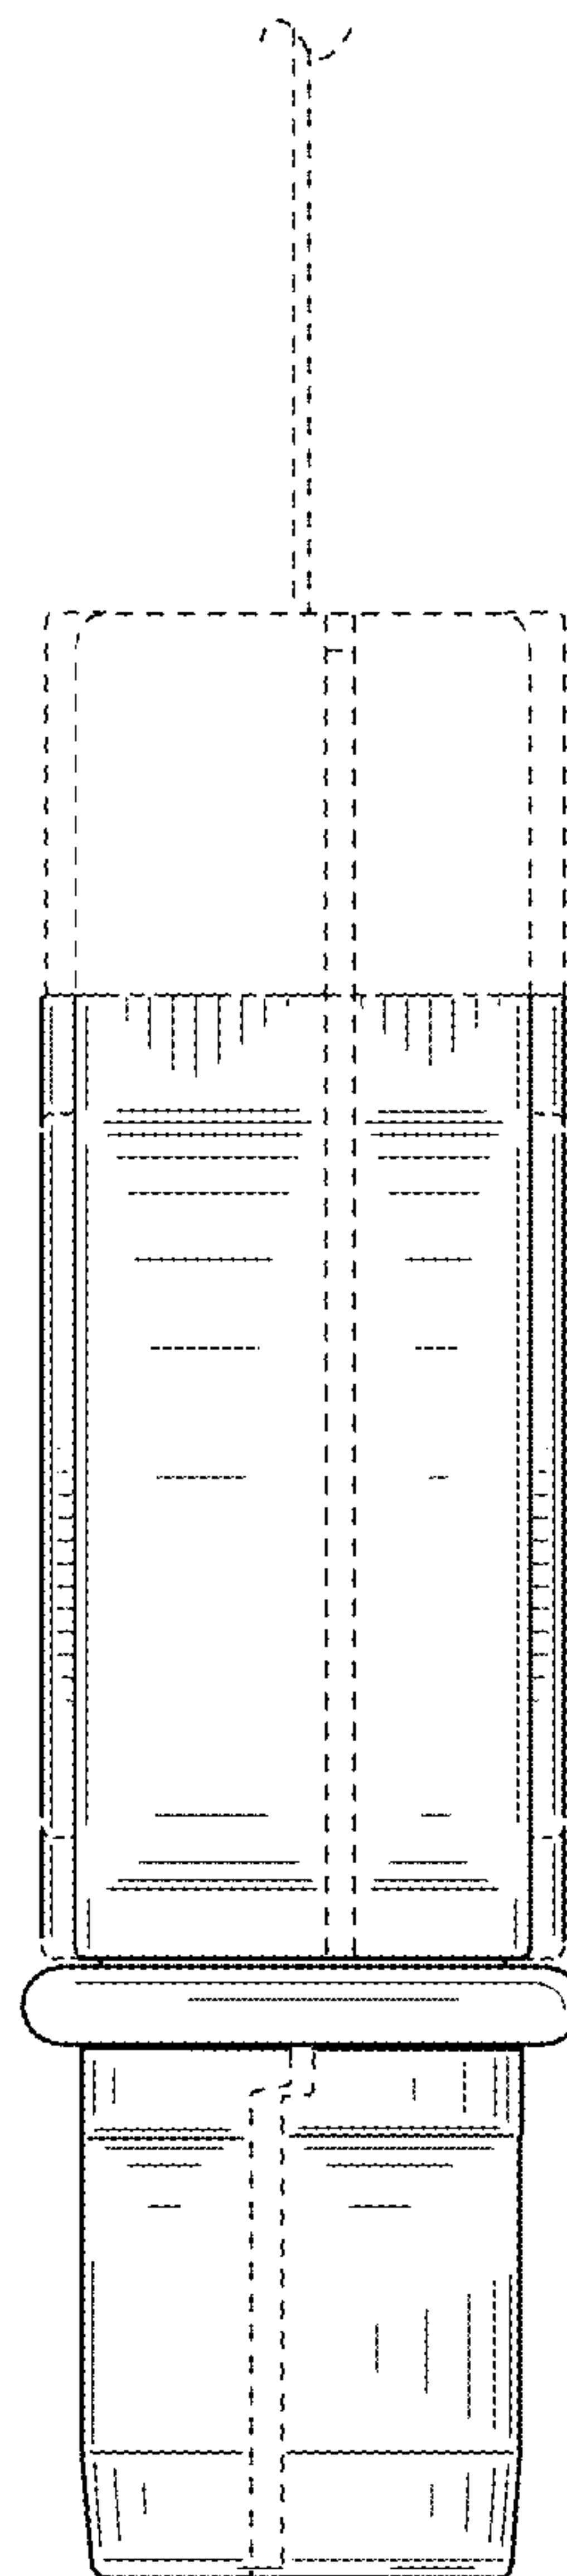


FIG. 16

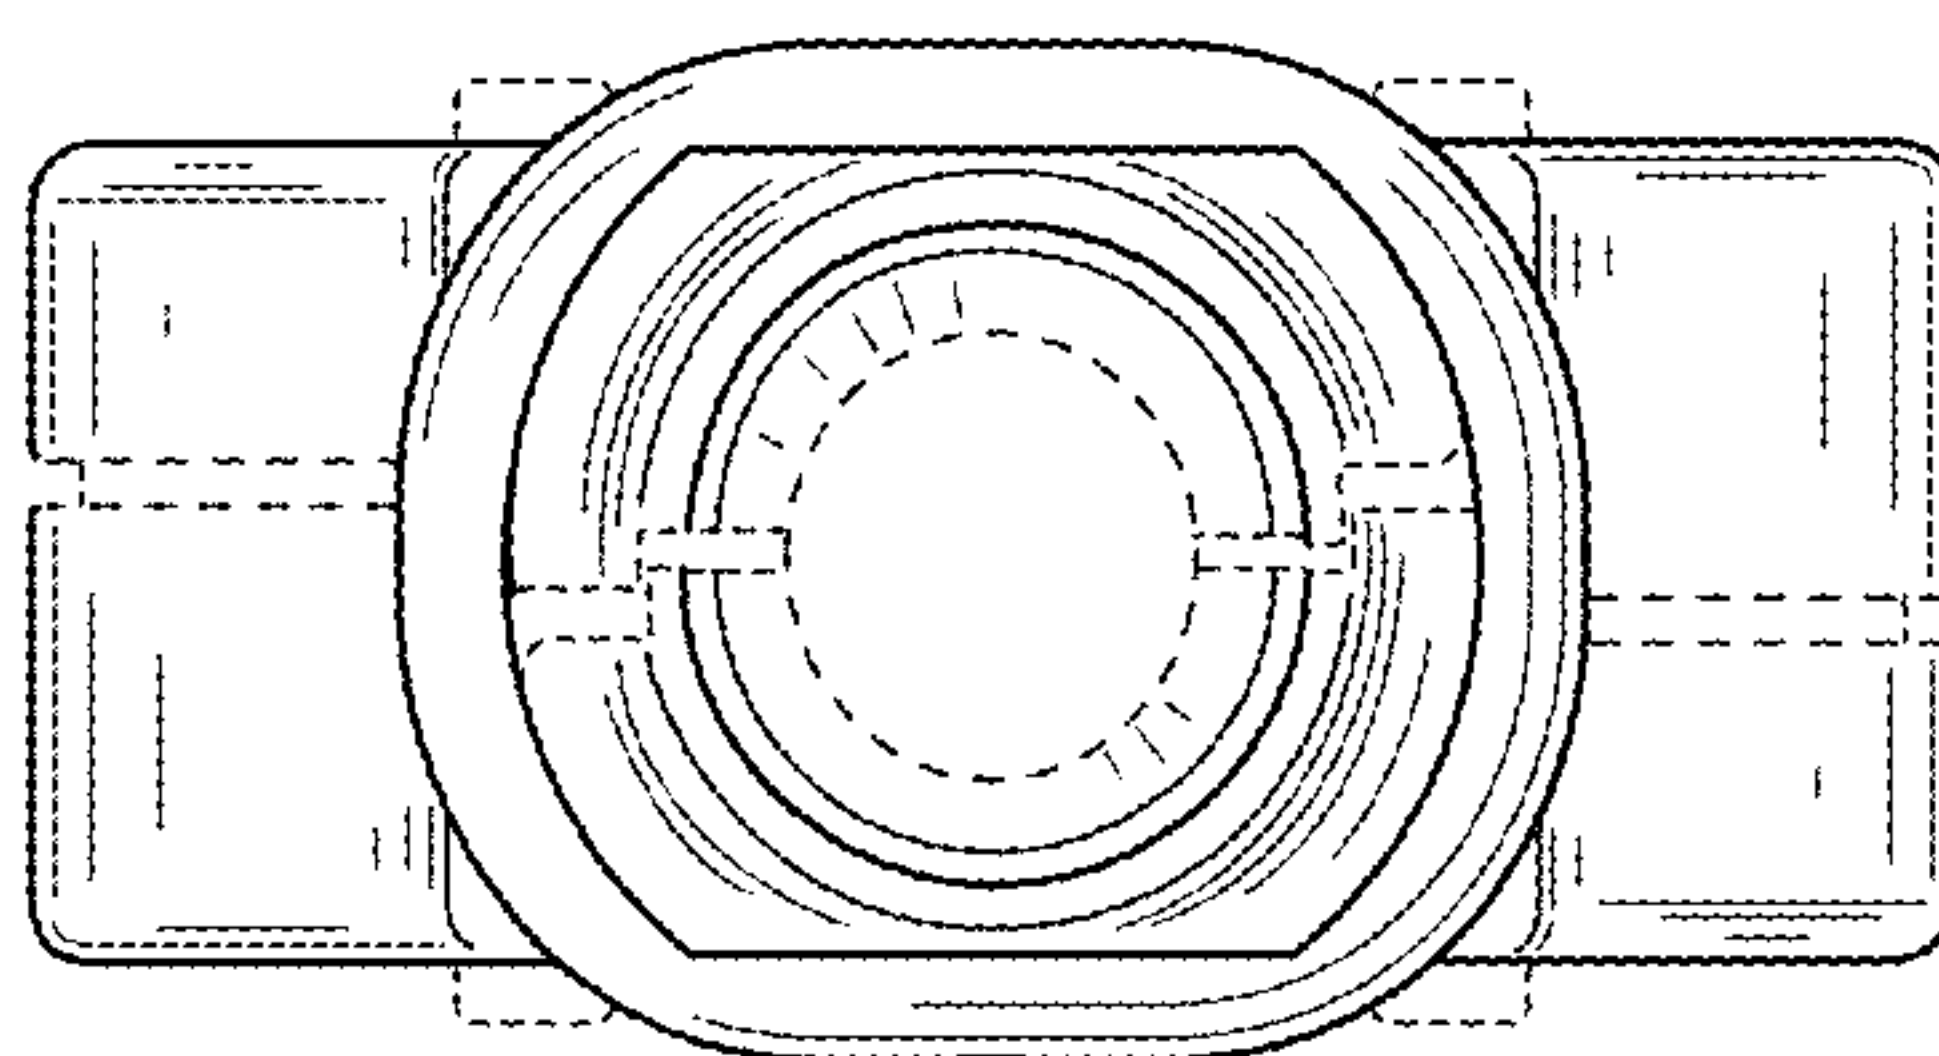


FIG. 17

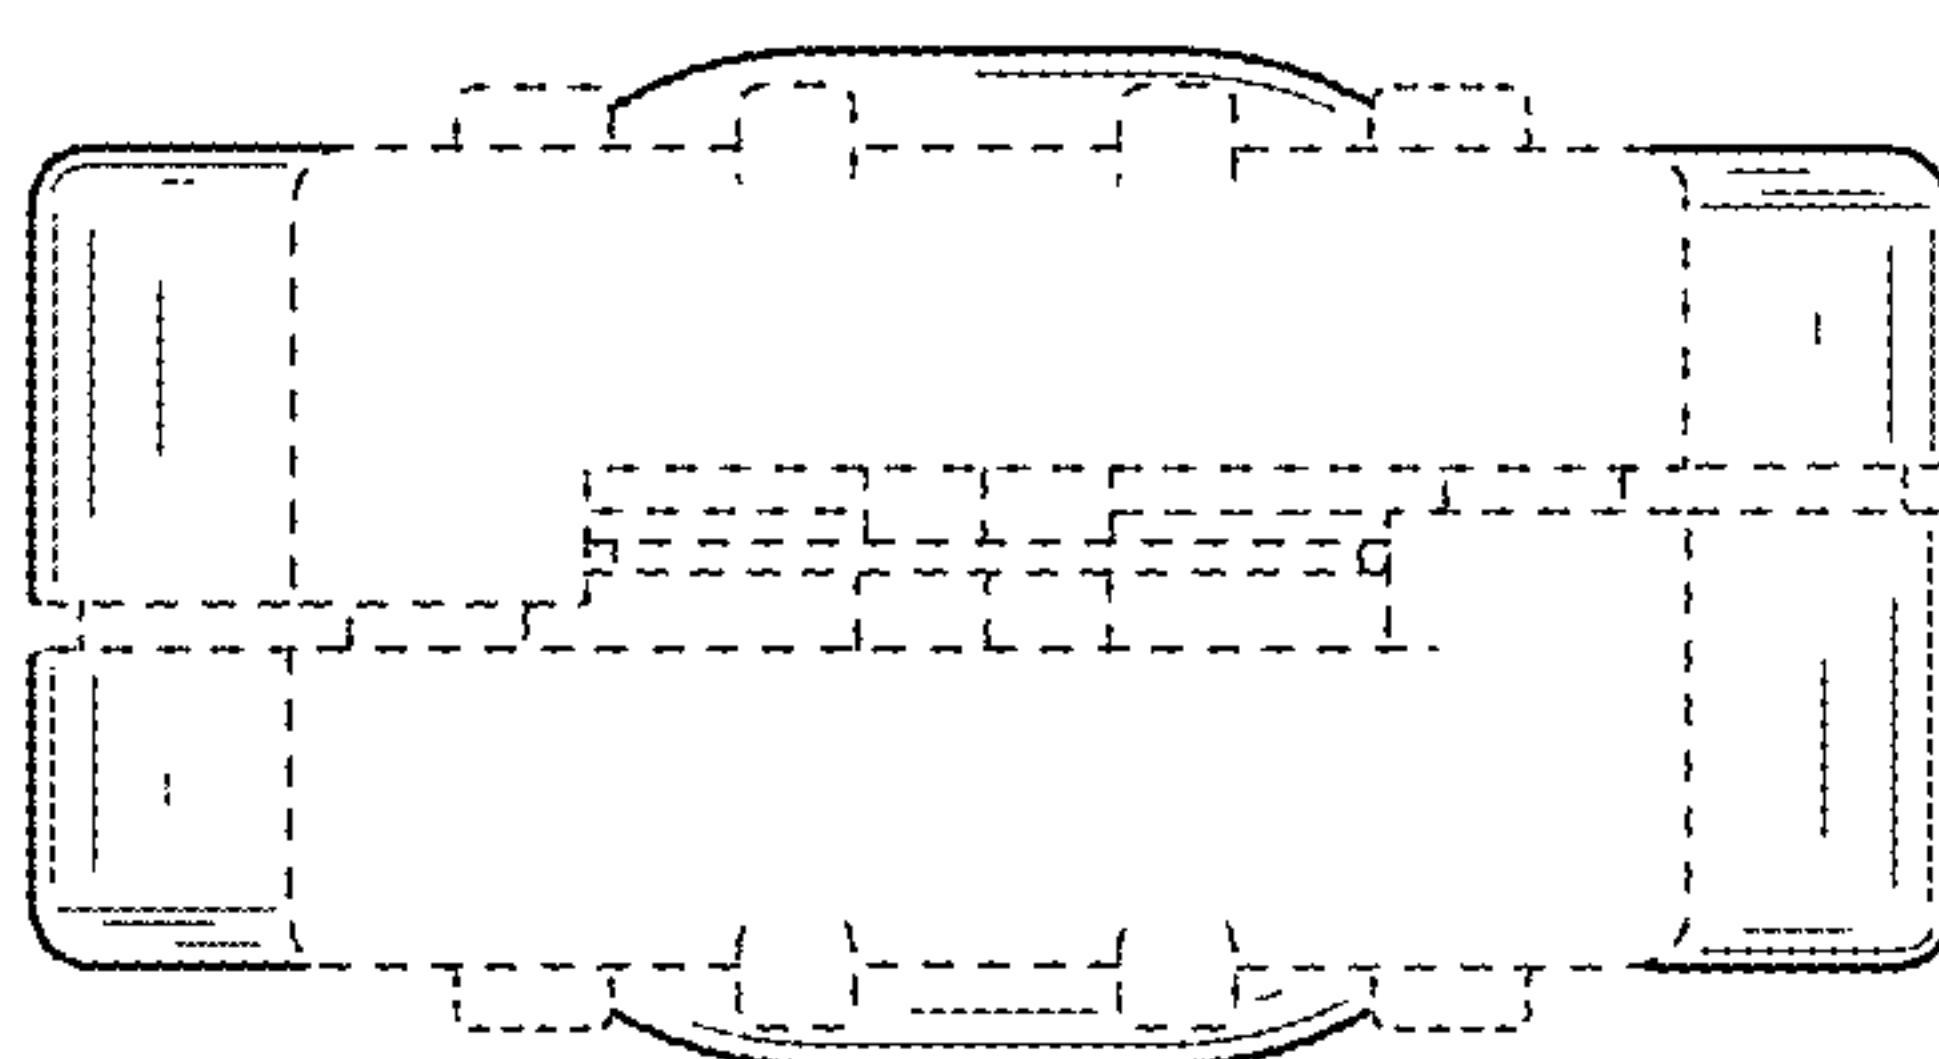
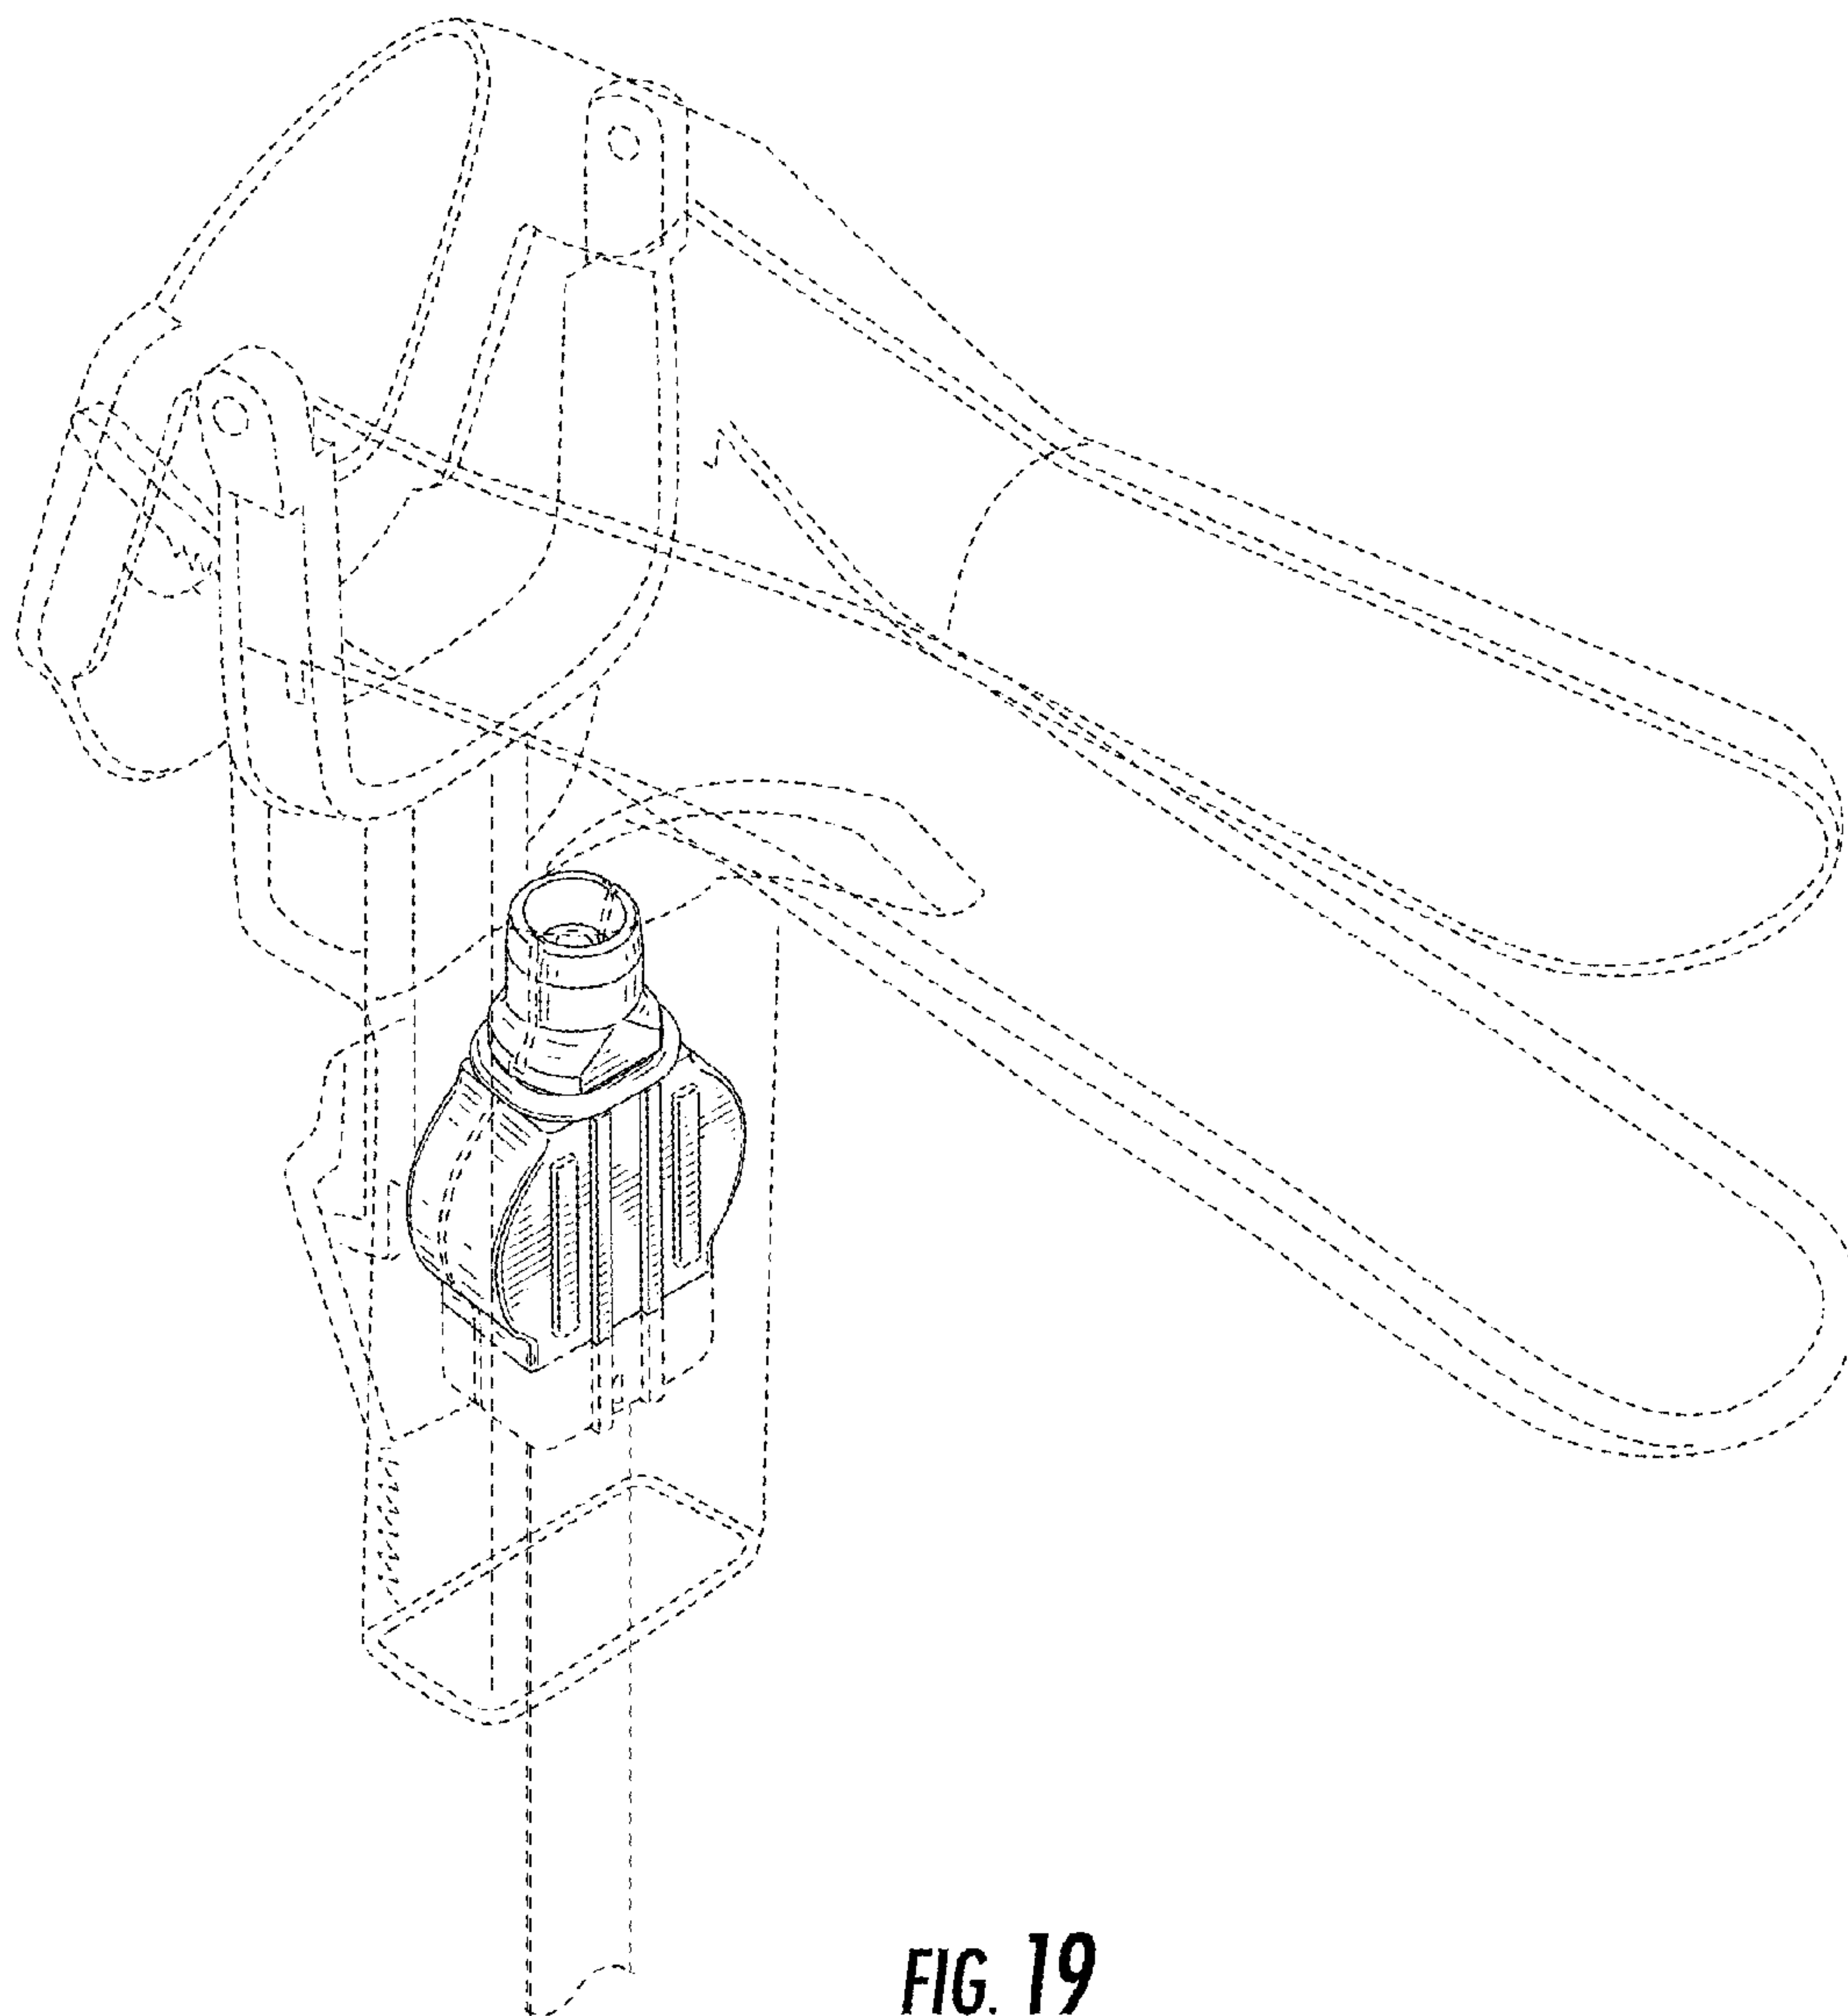


FIG. 18



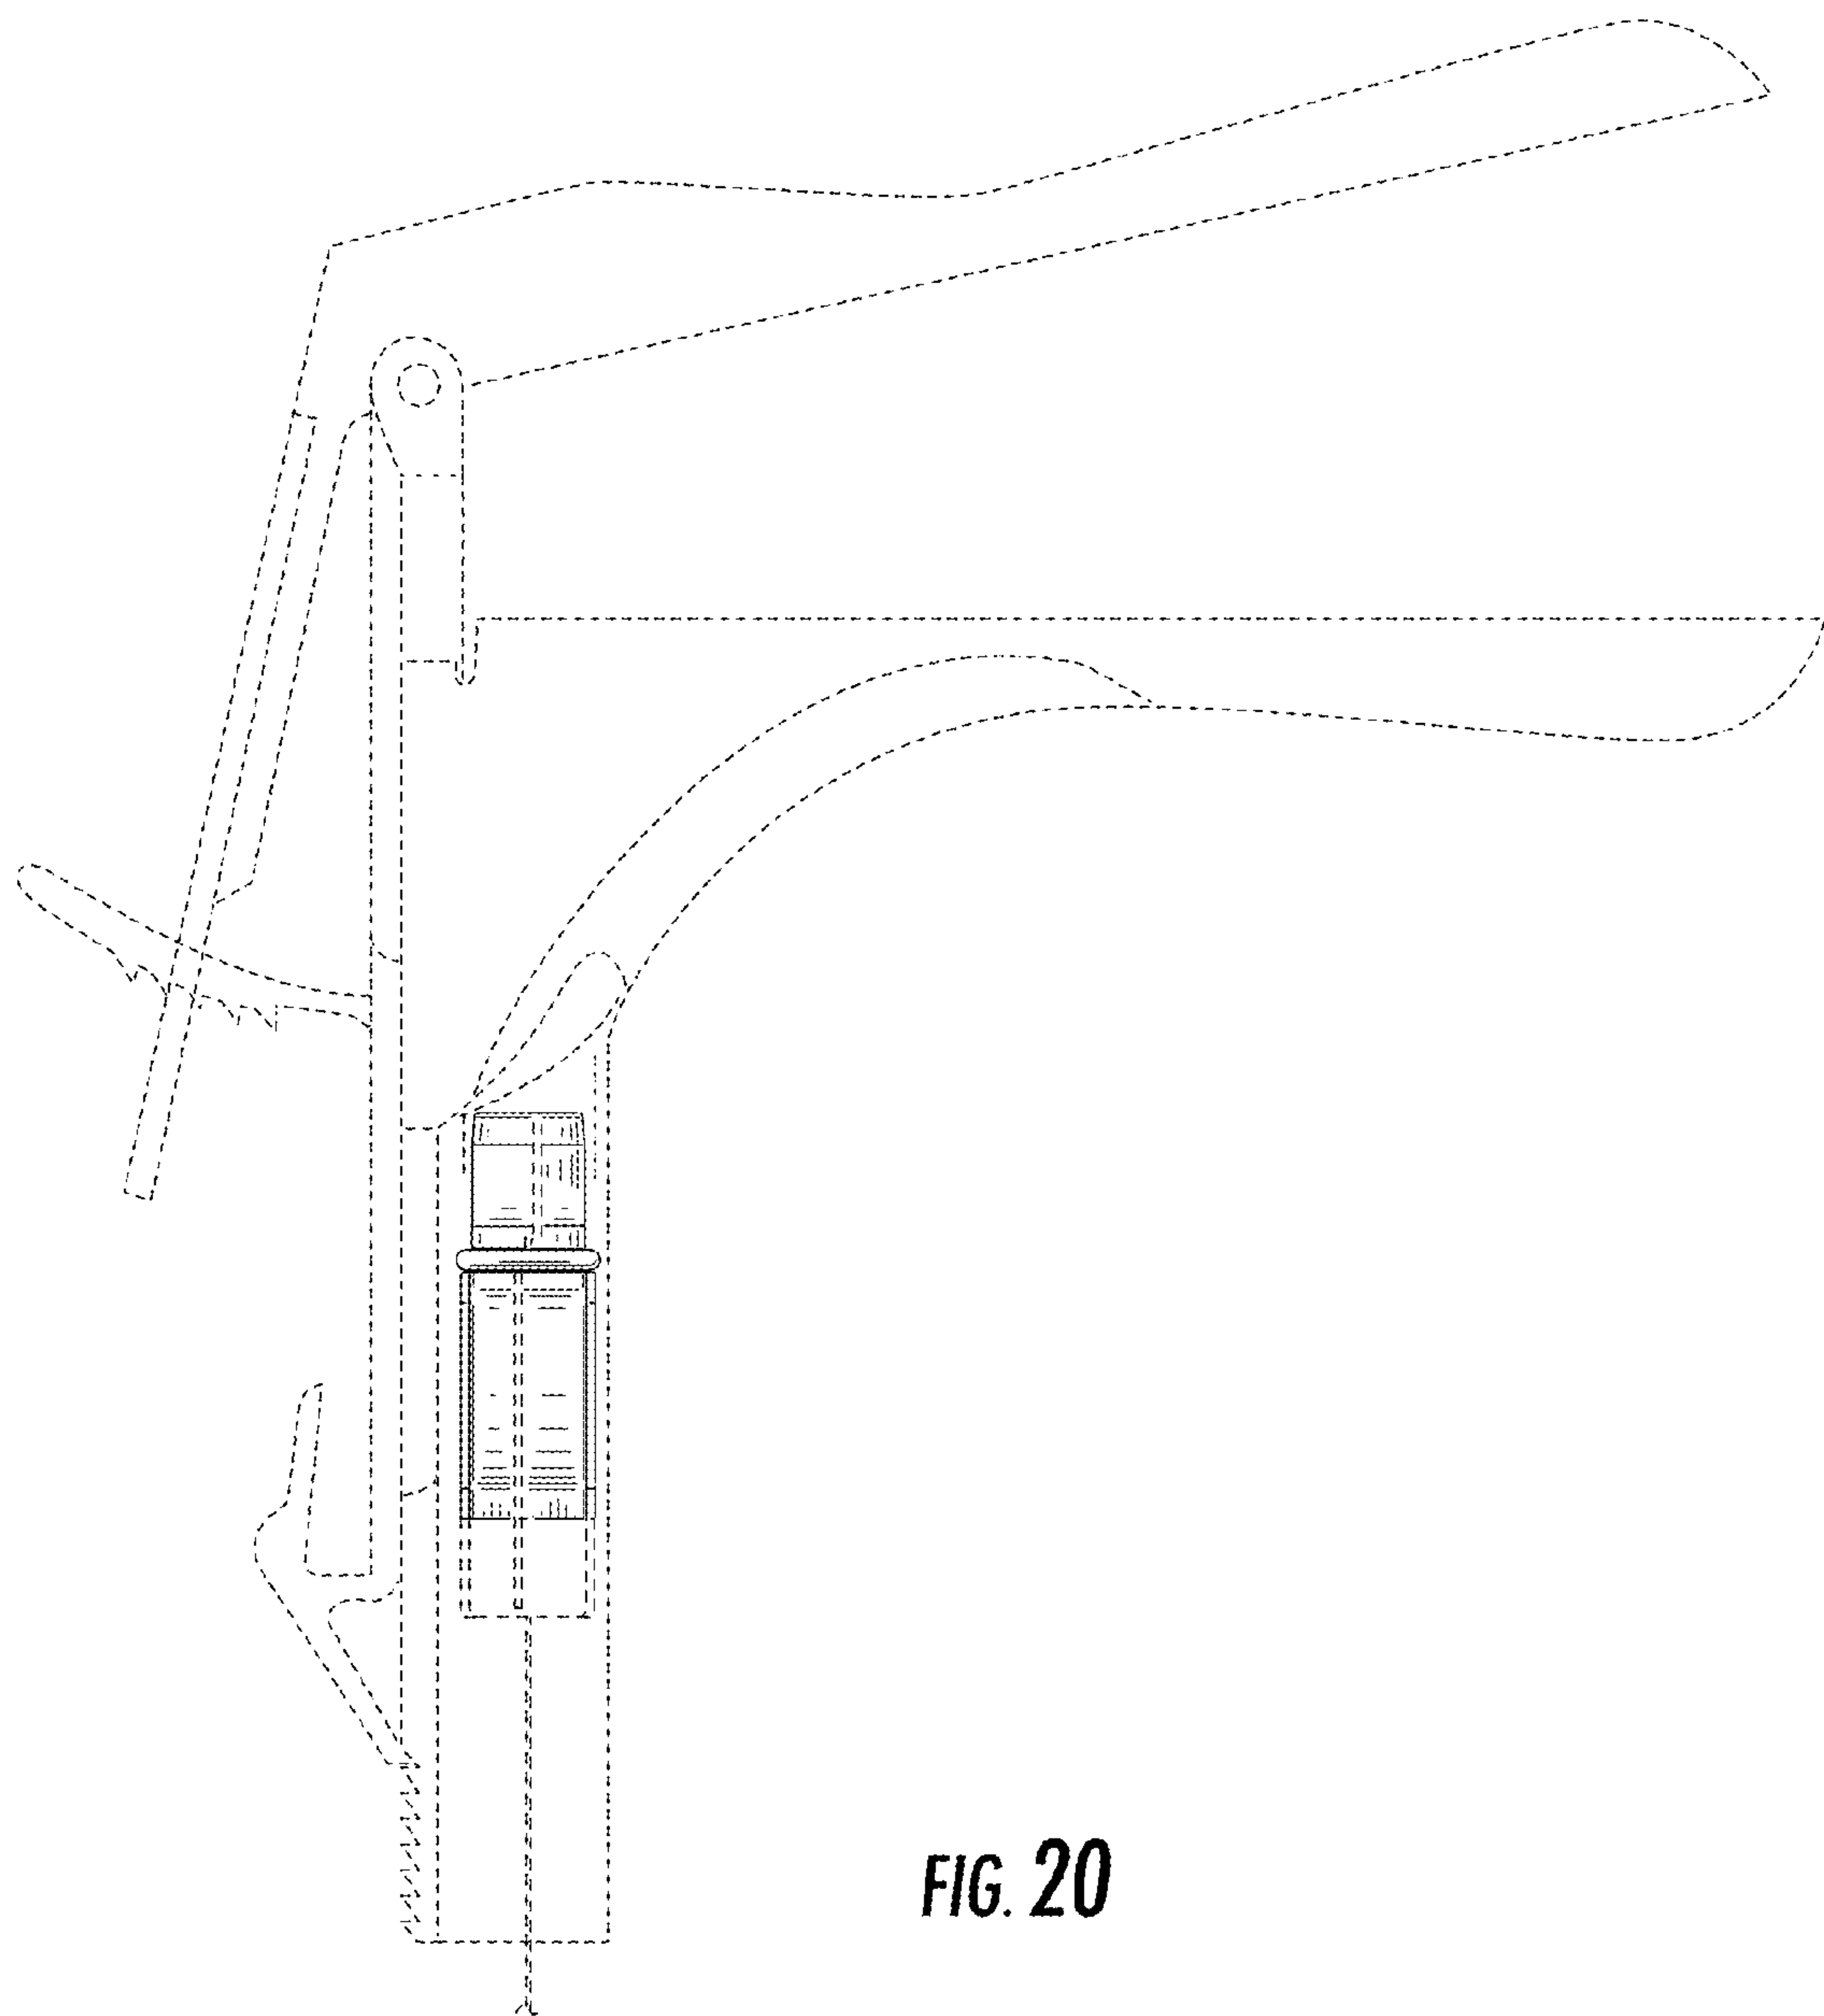


FIG. 20

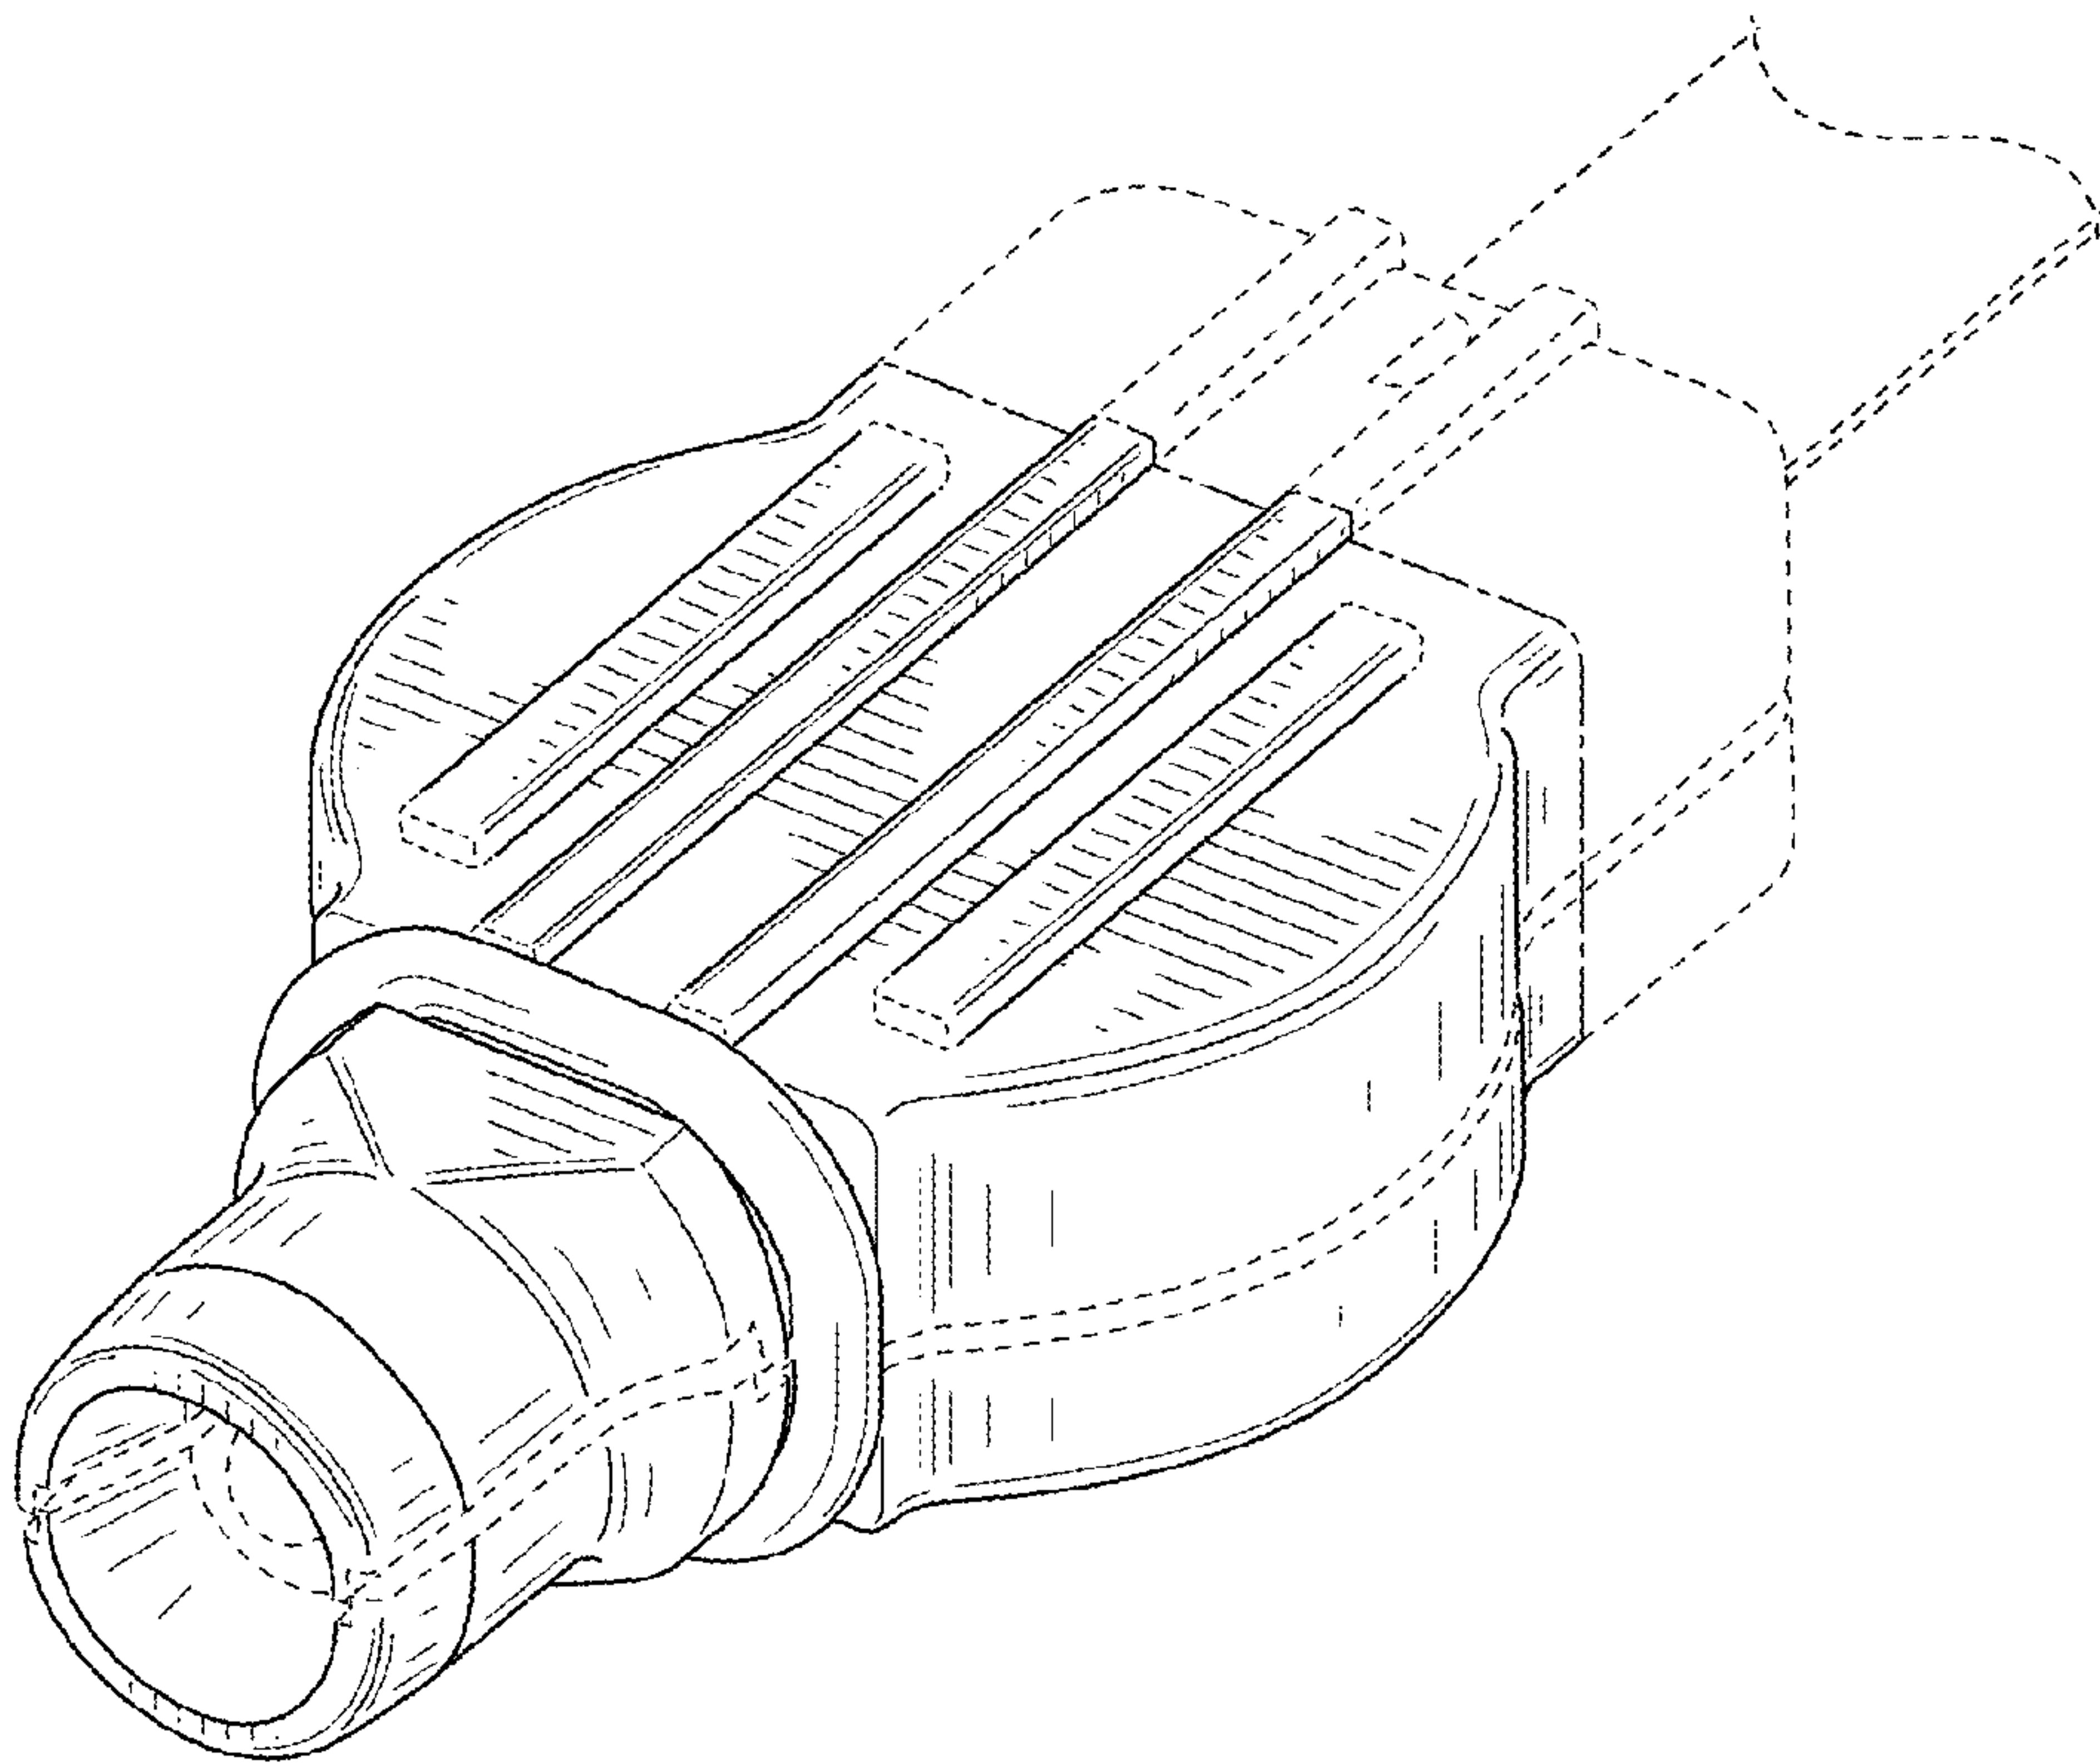


FIG. 21

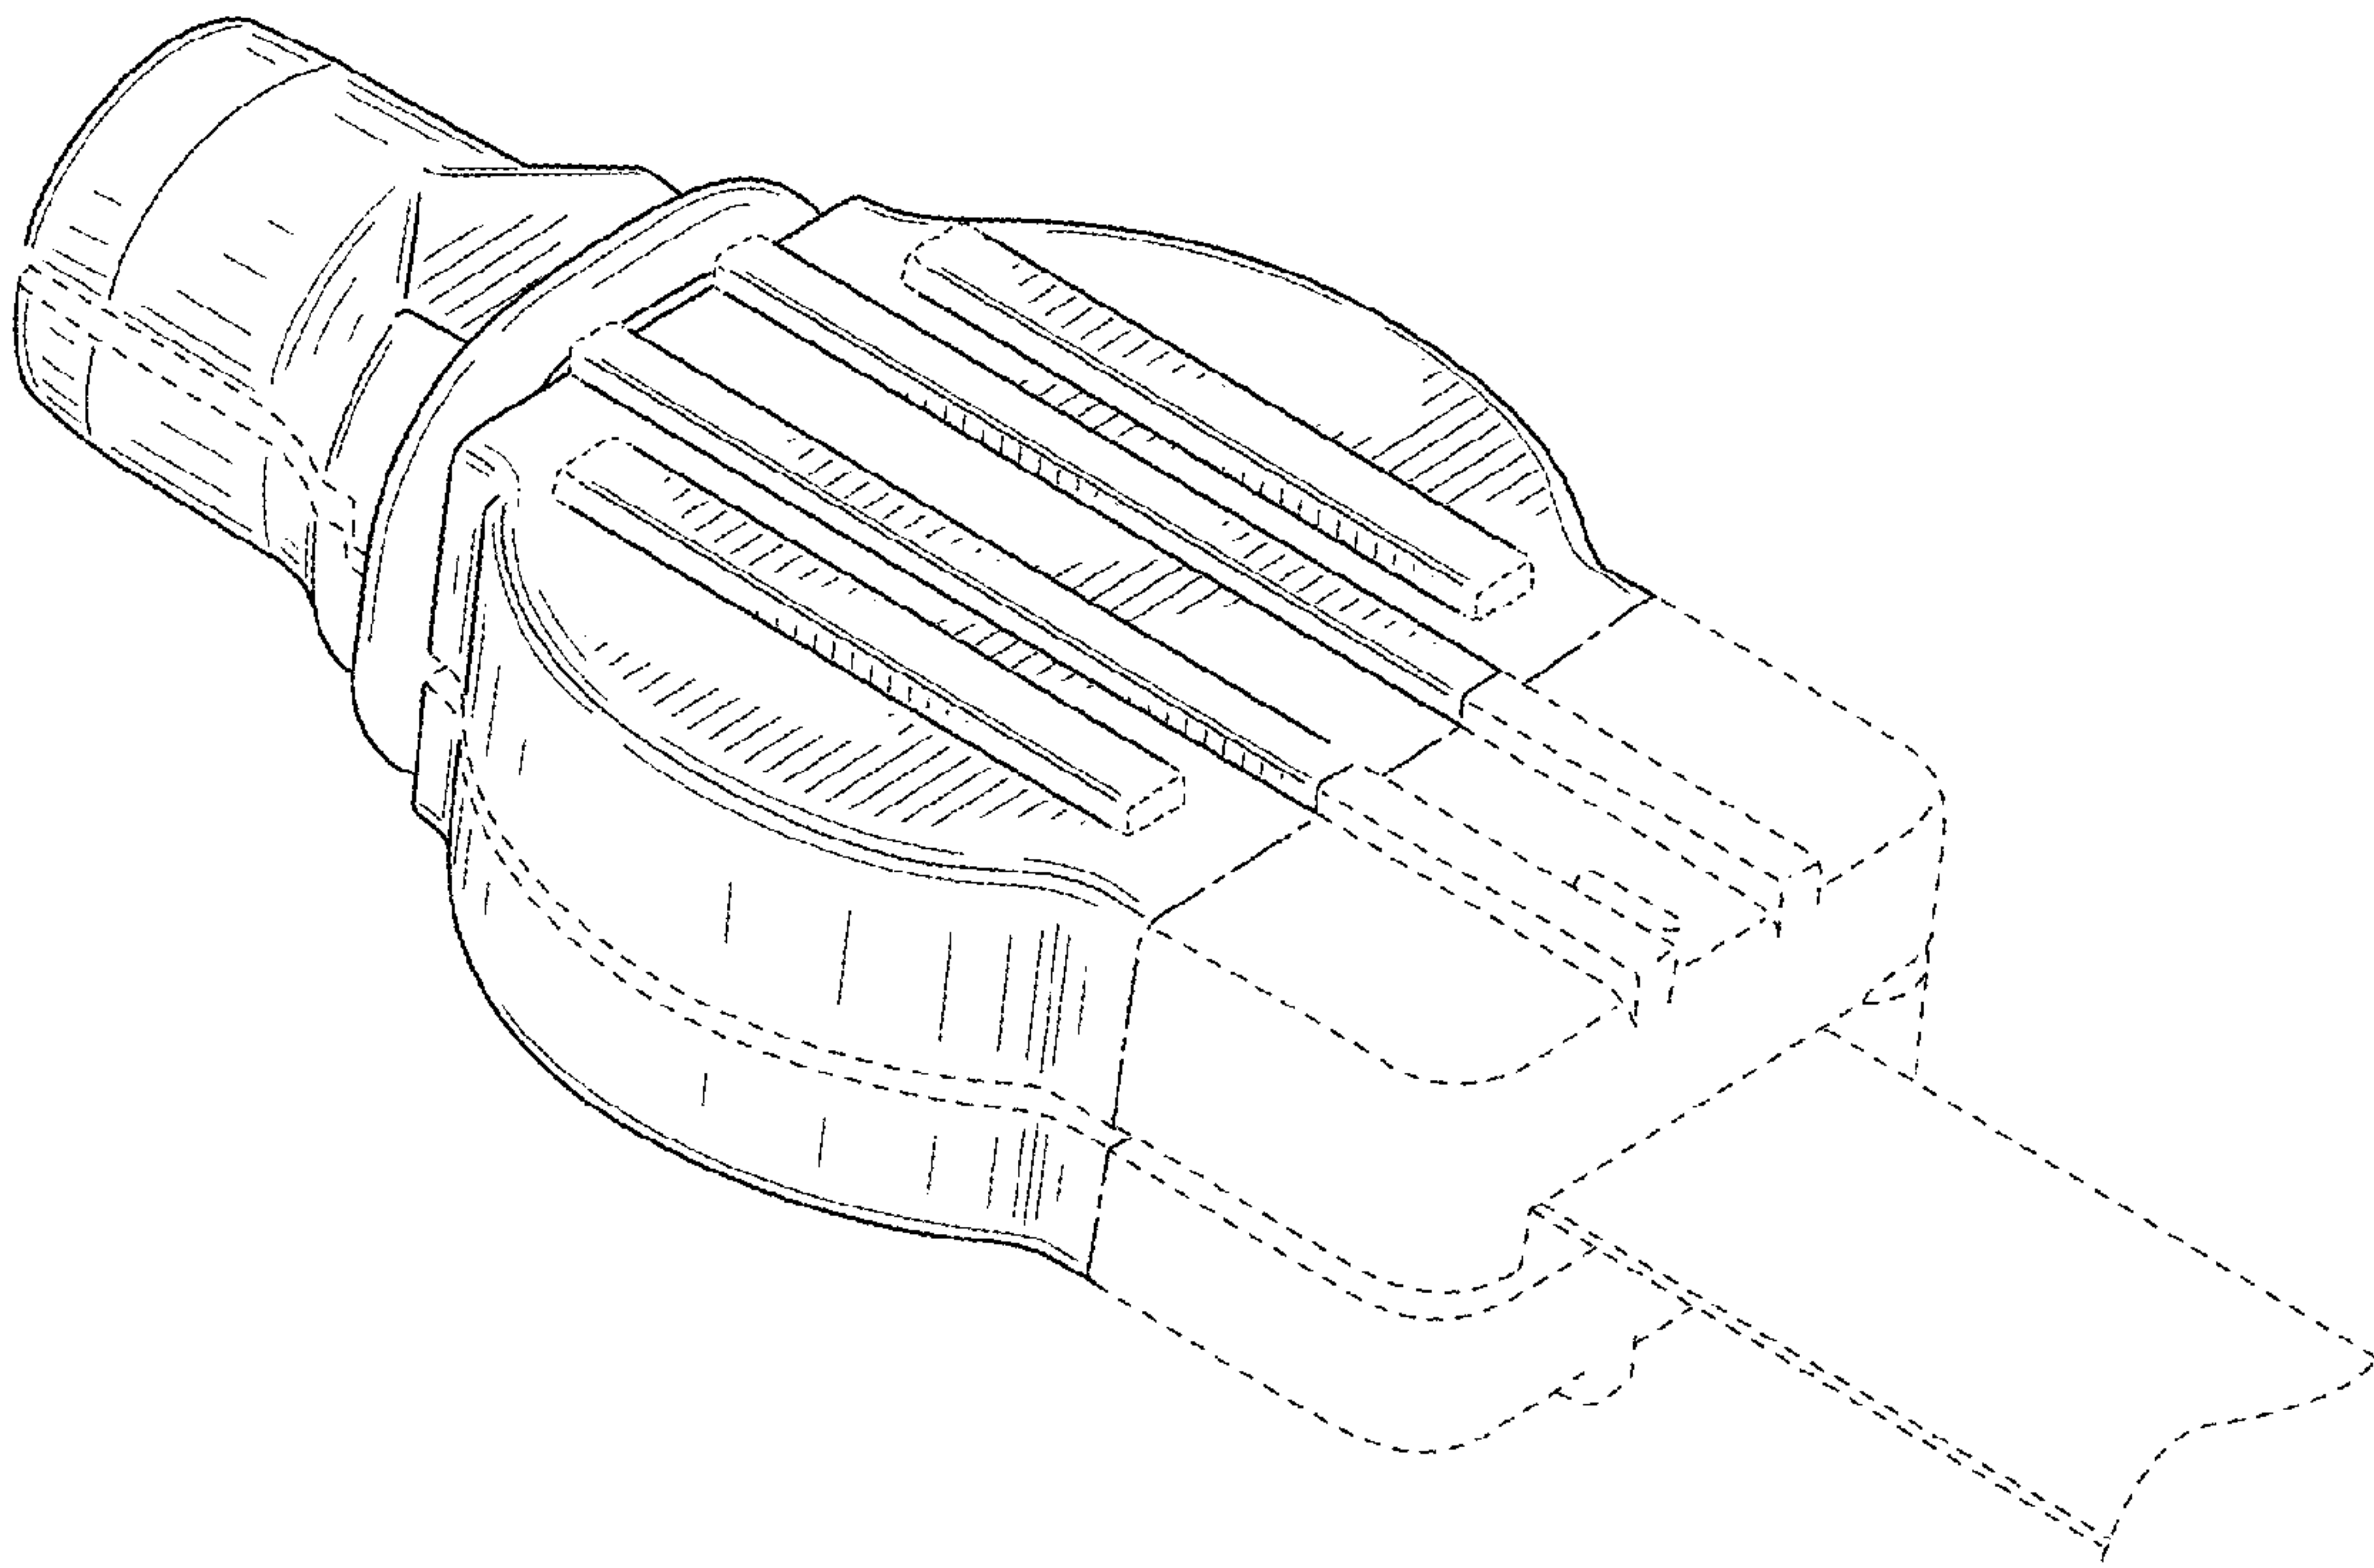


FIG. 22

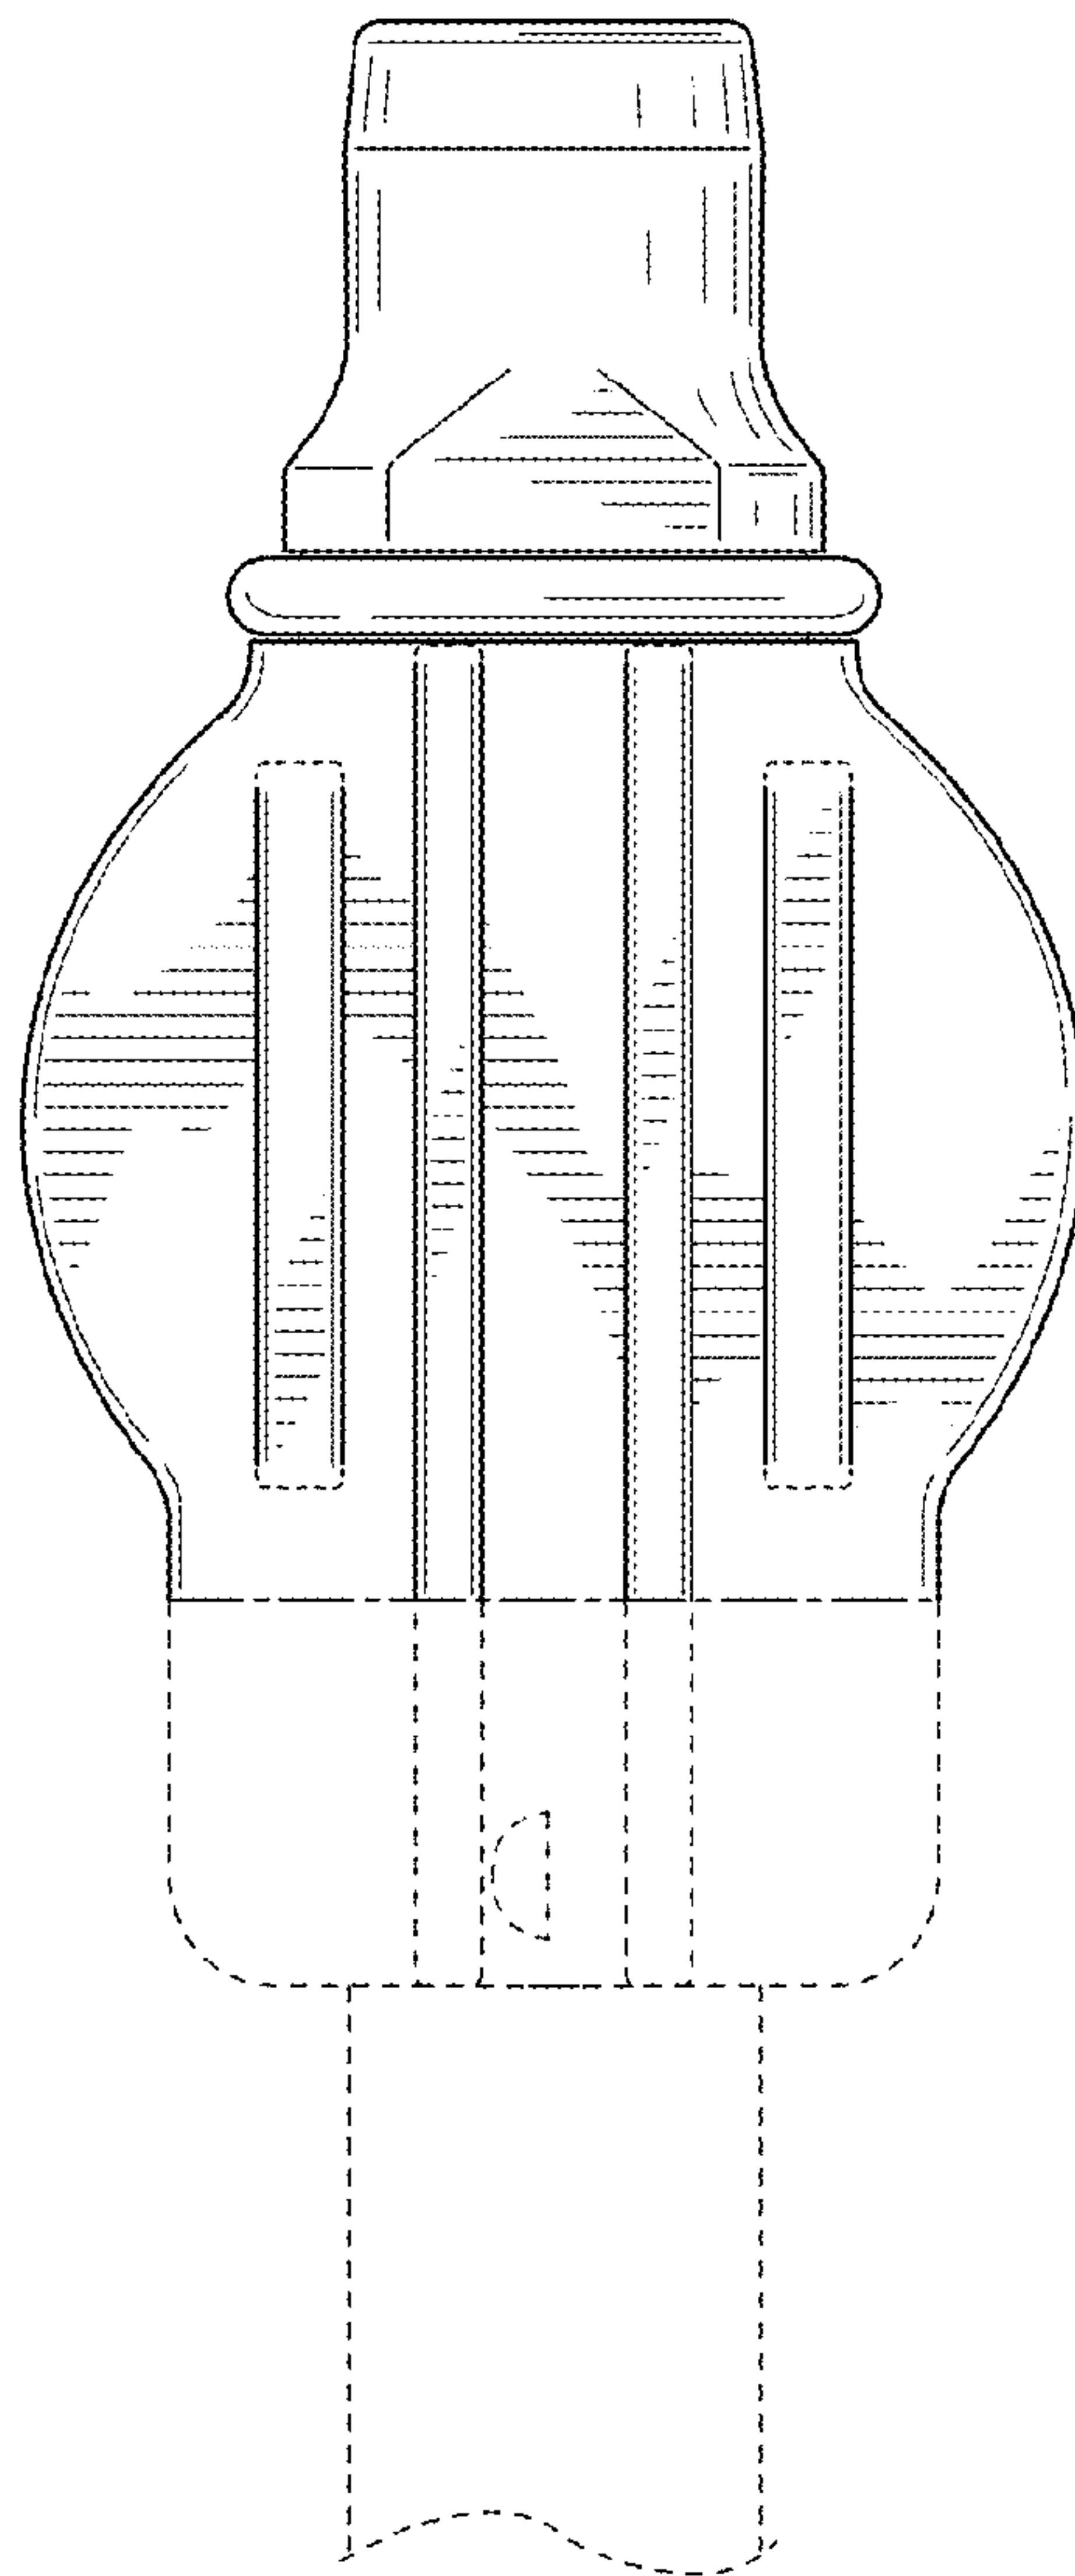


FIG. 23

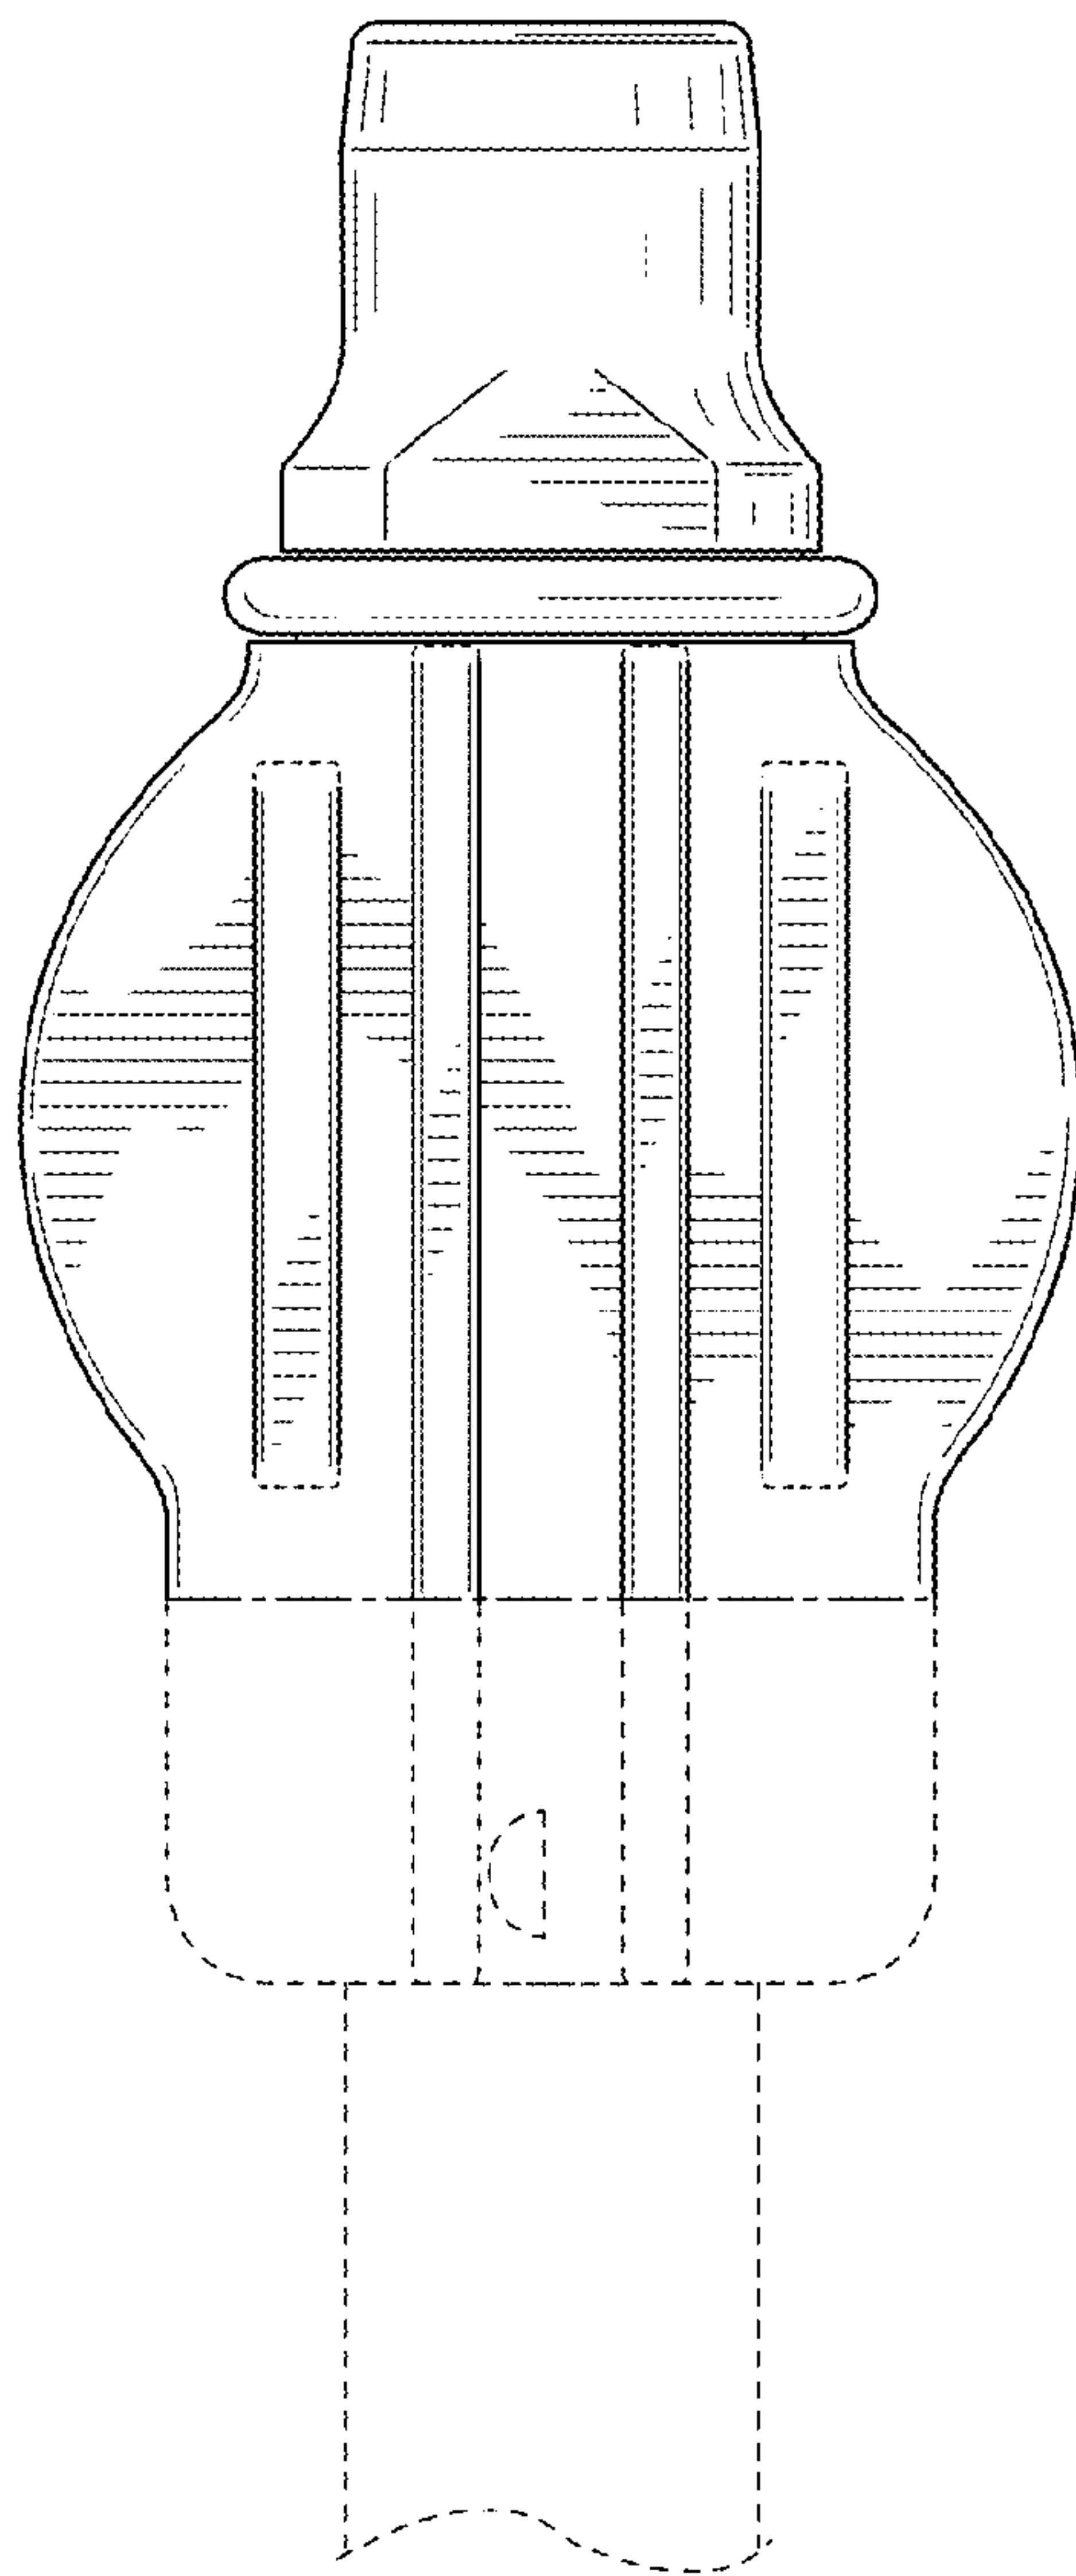


FIG. 24

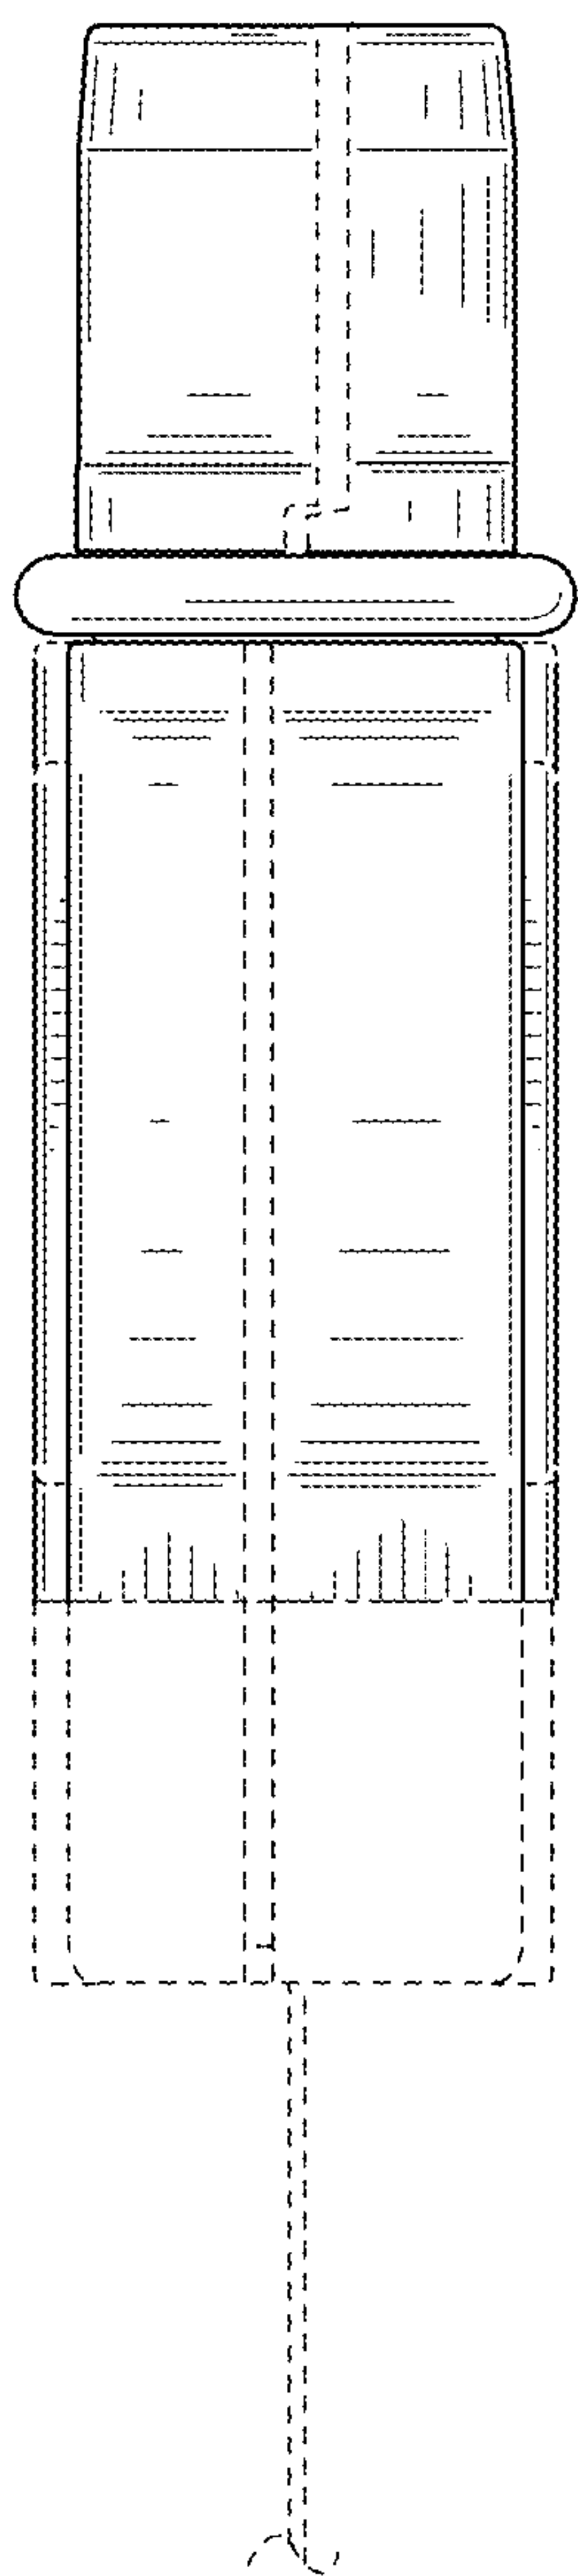


FIG. 25

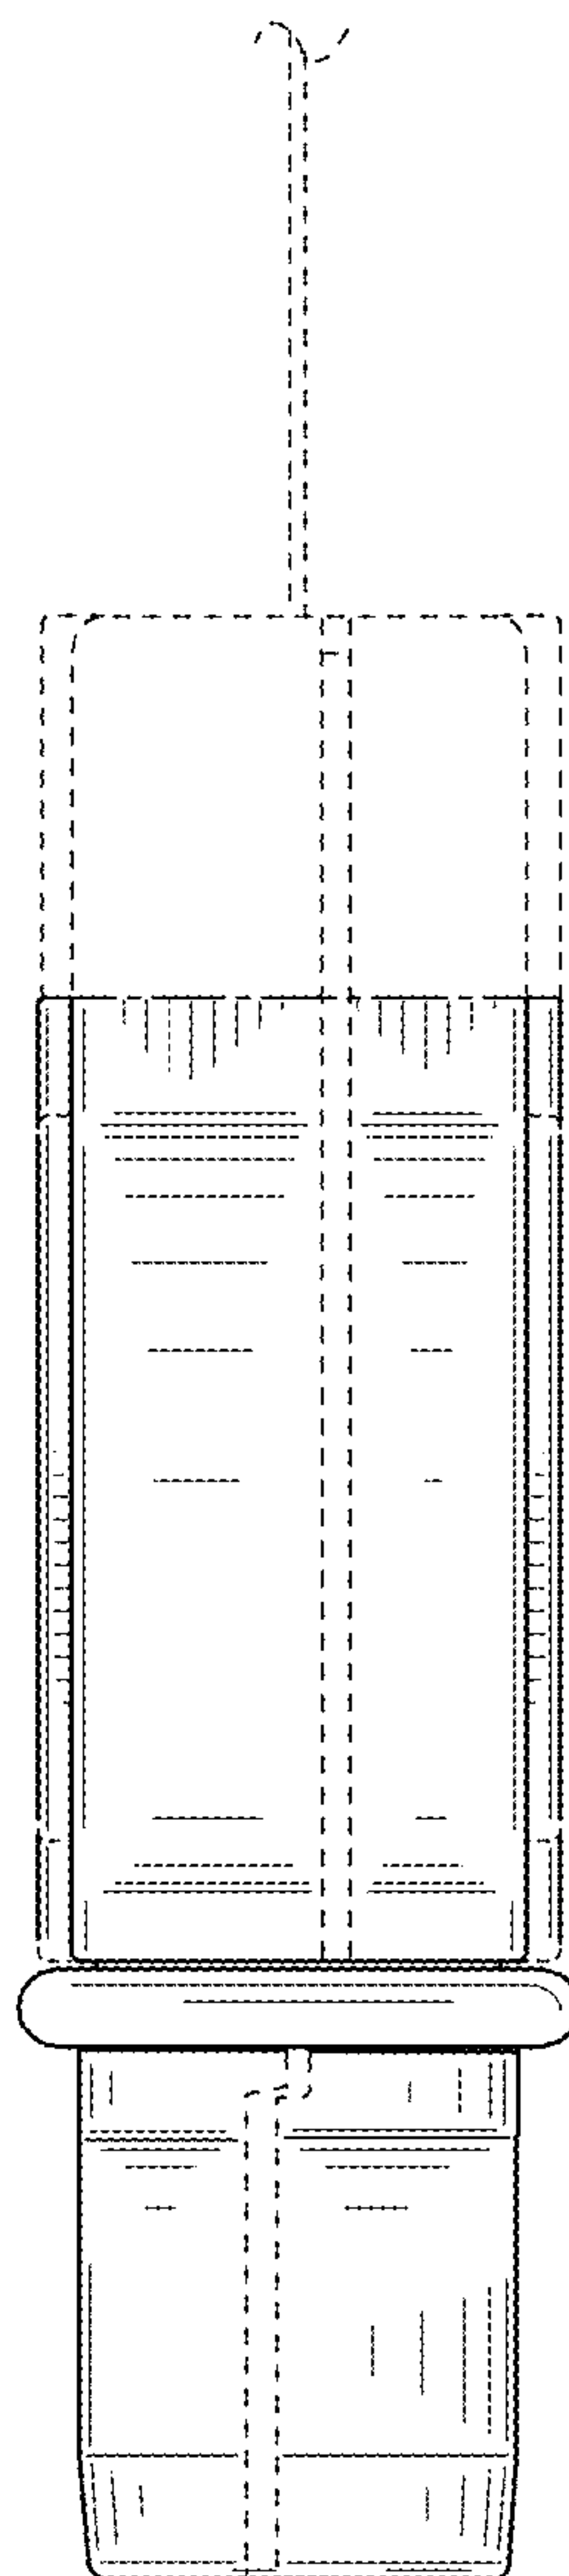


FIG. 26

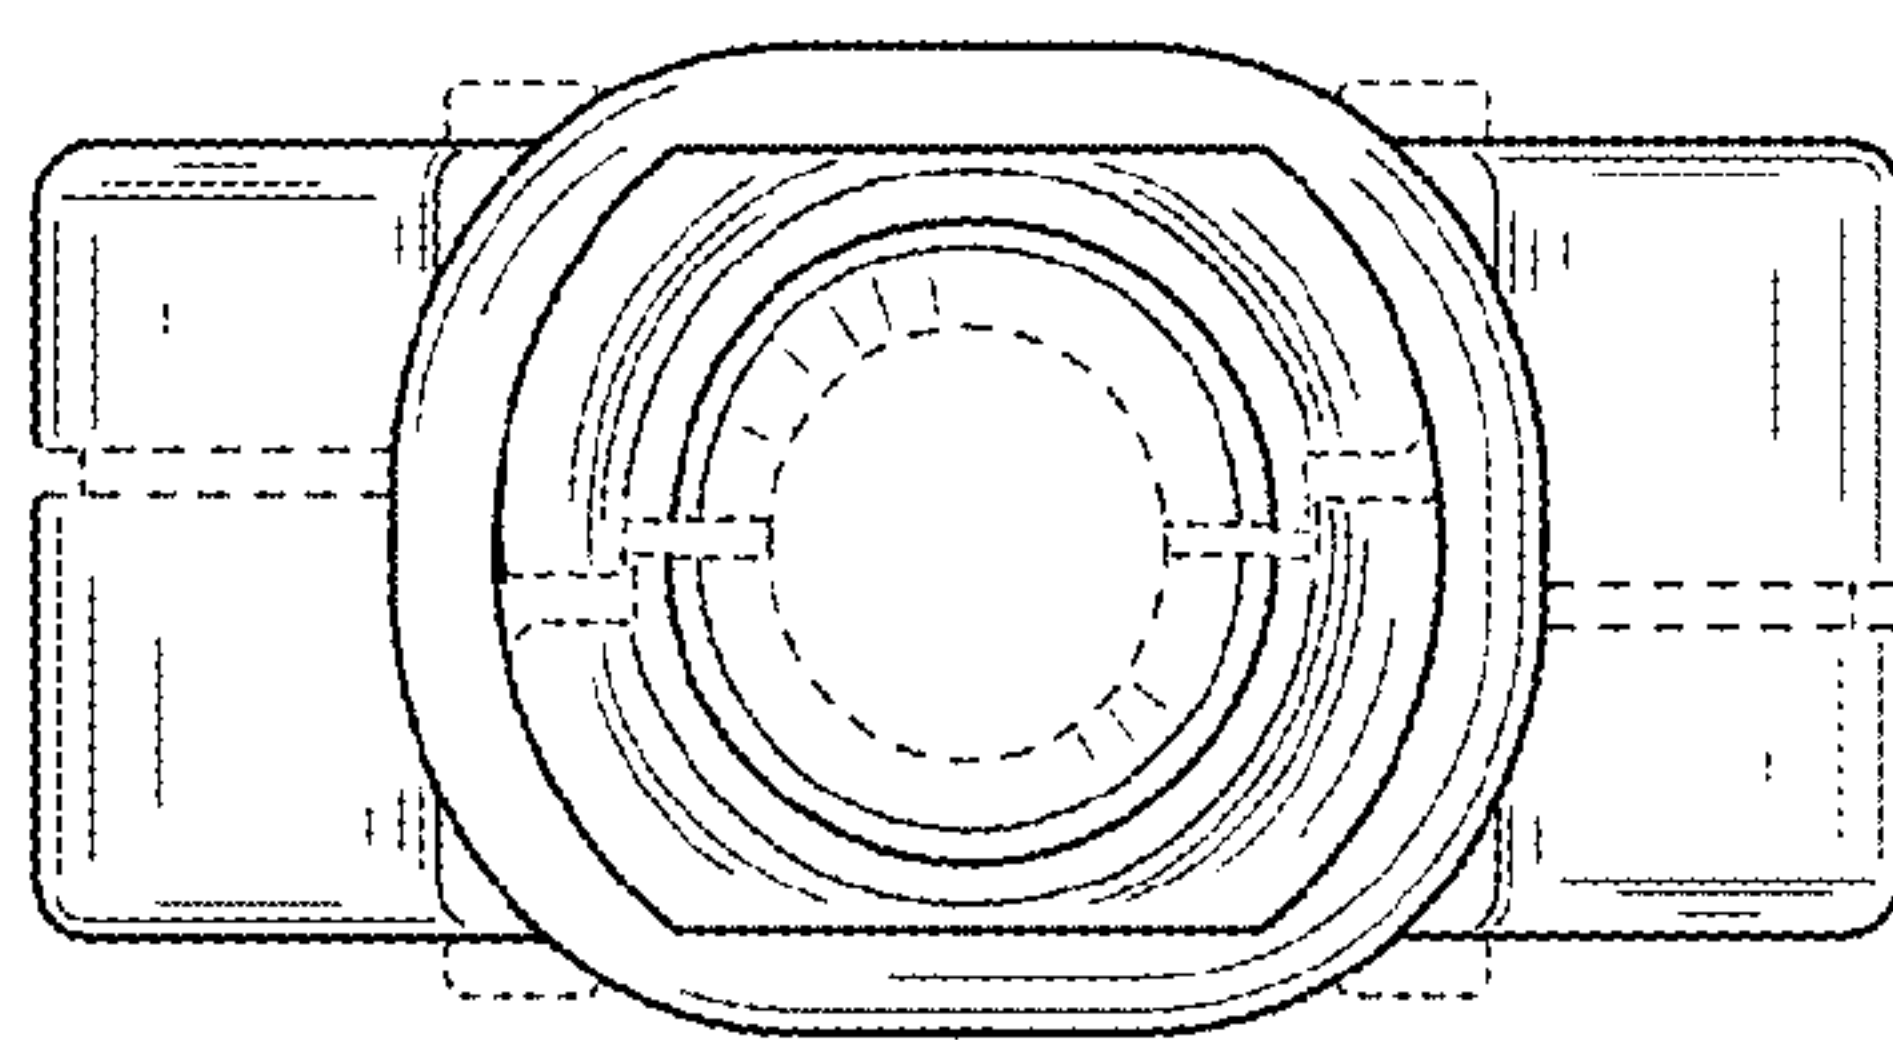


FIG. 27

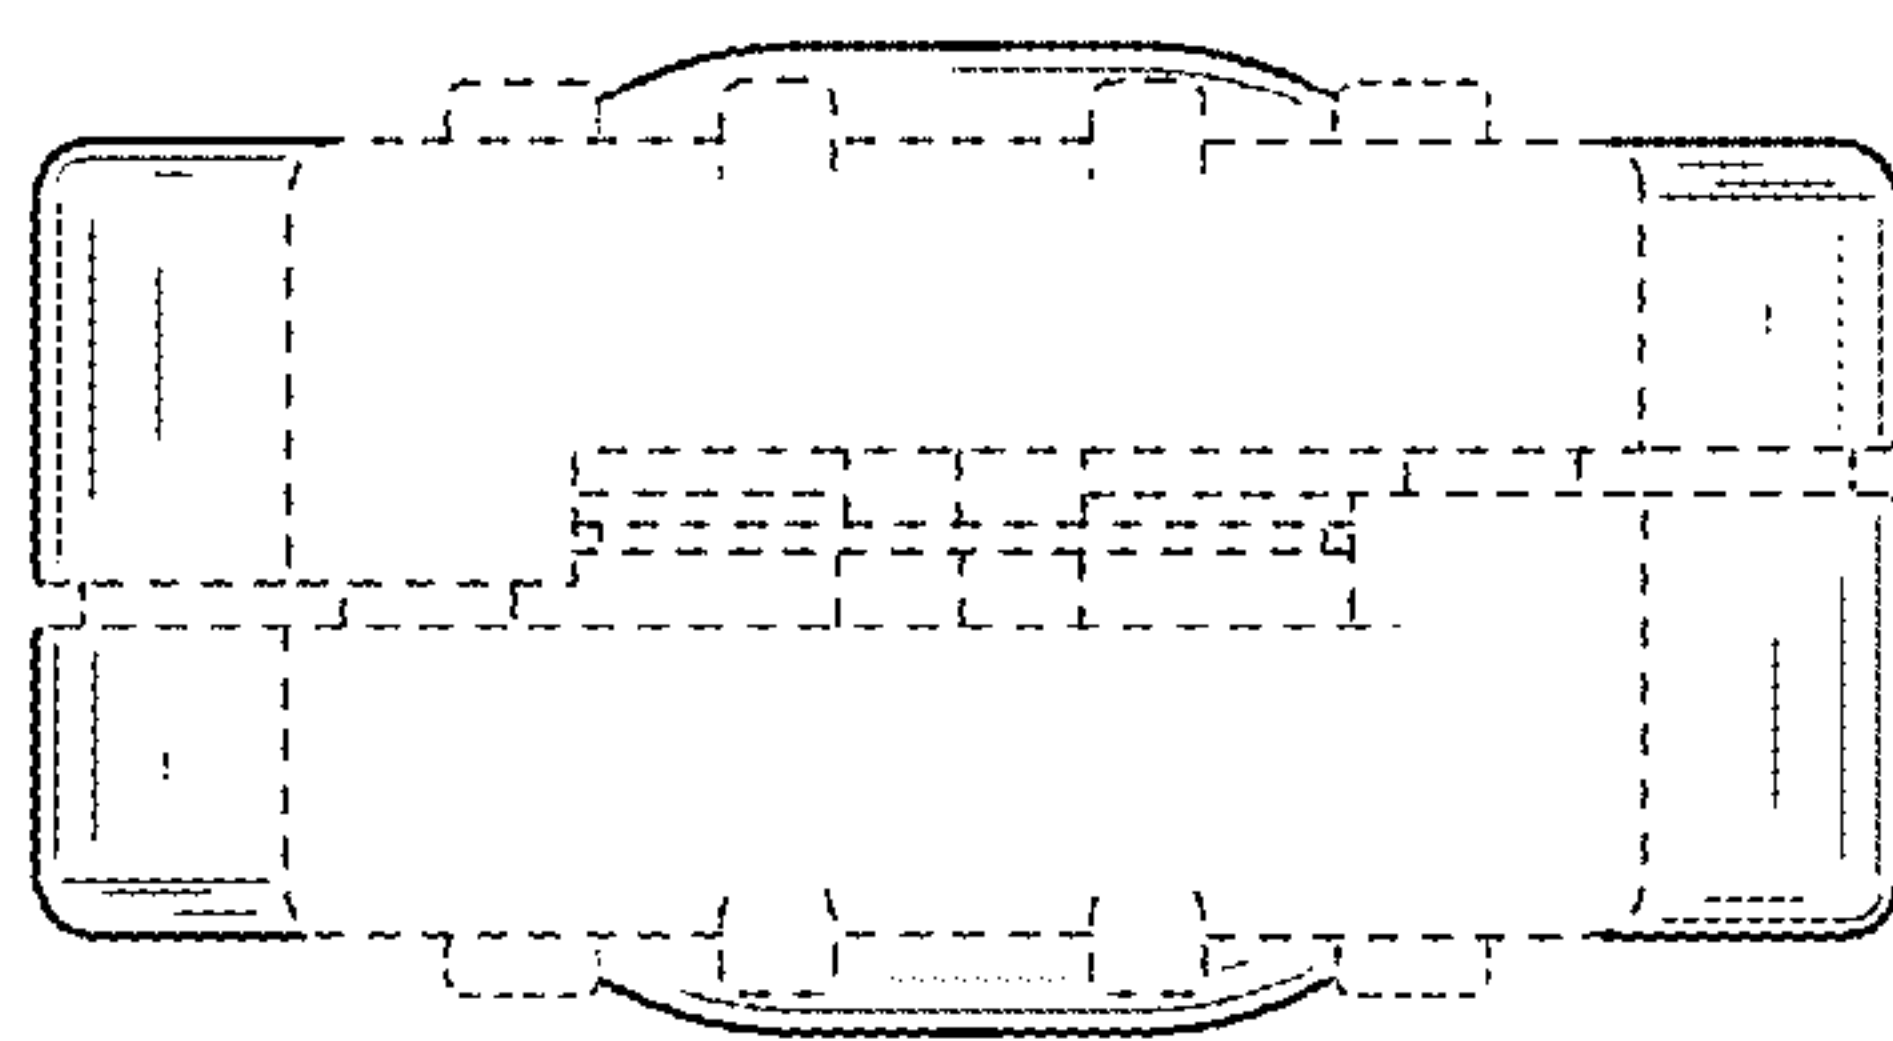


FIG. 28

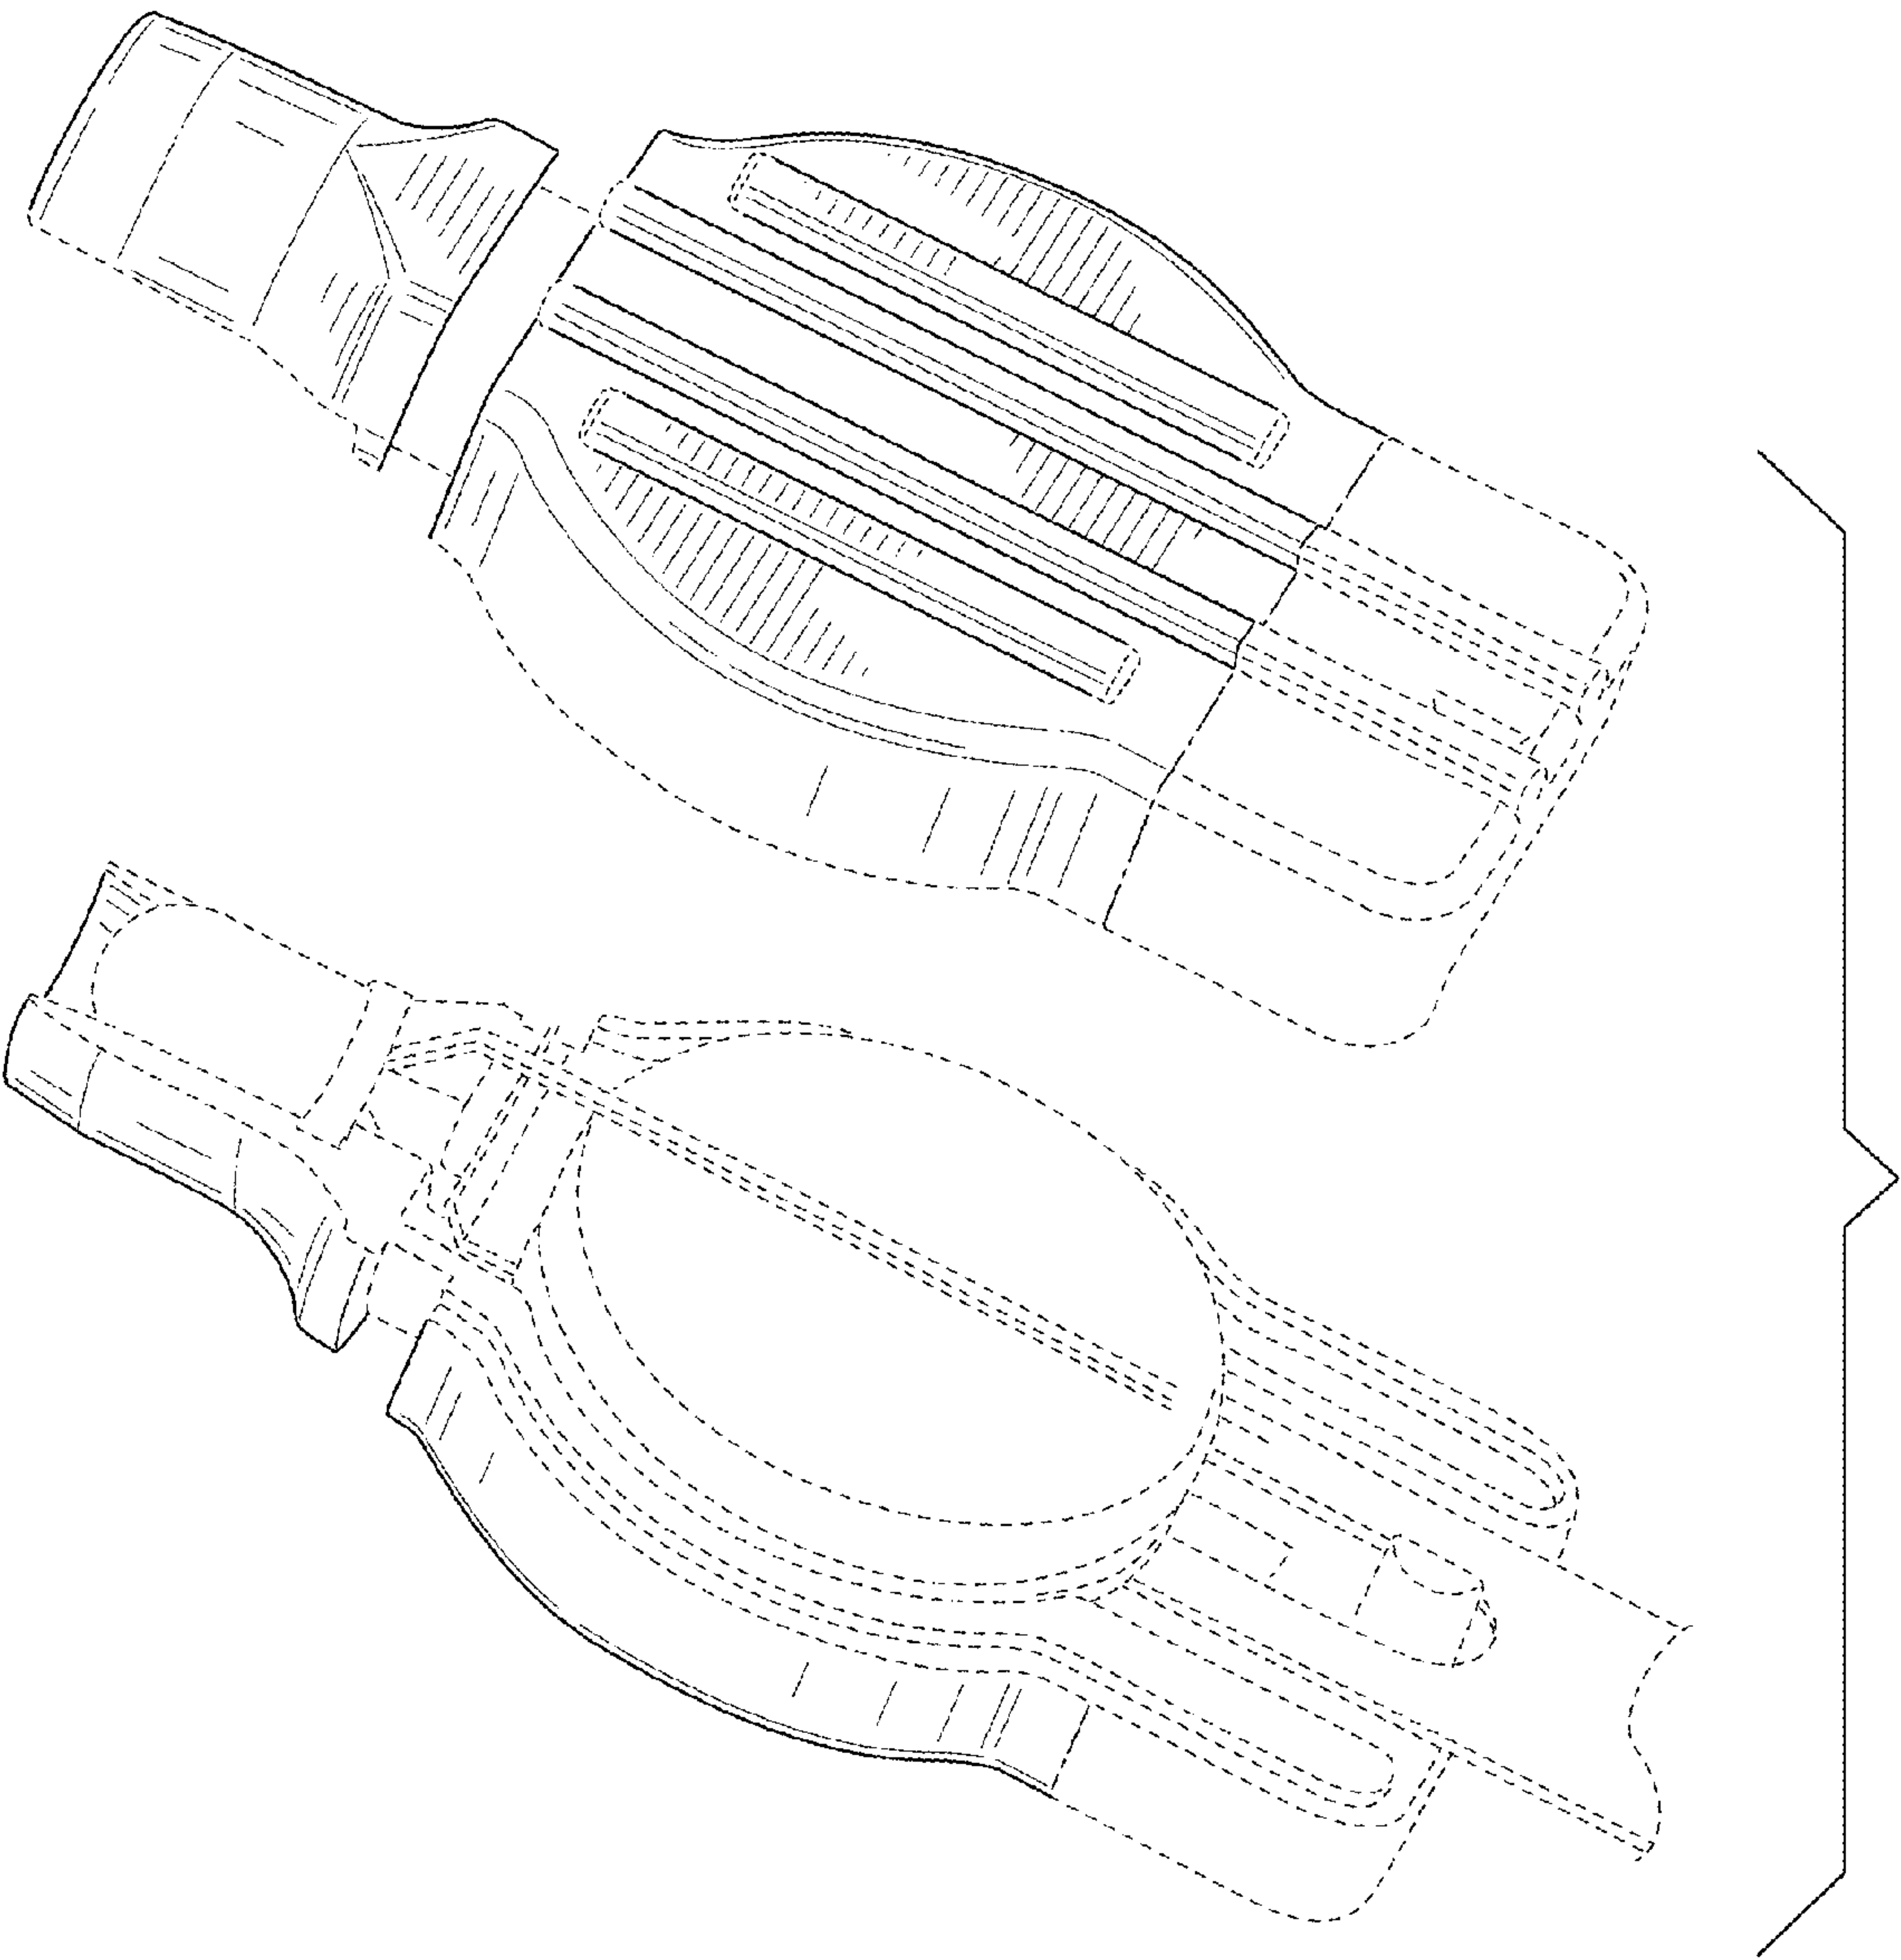


FIG. 29

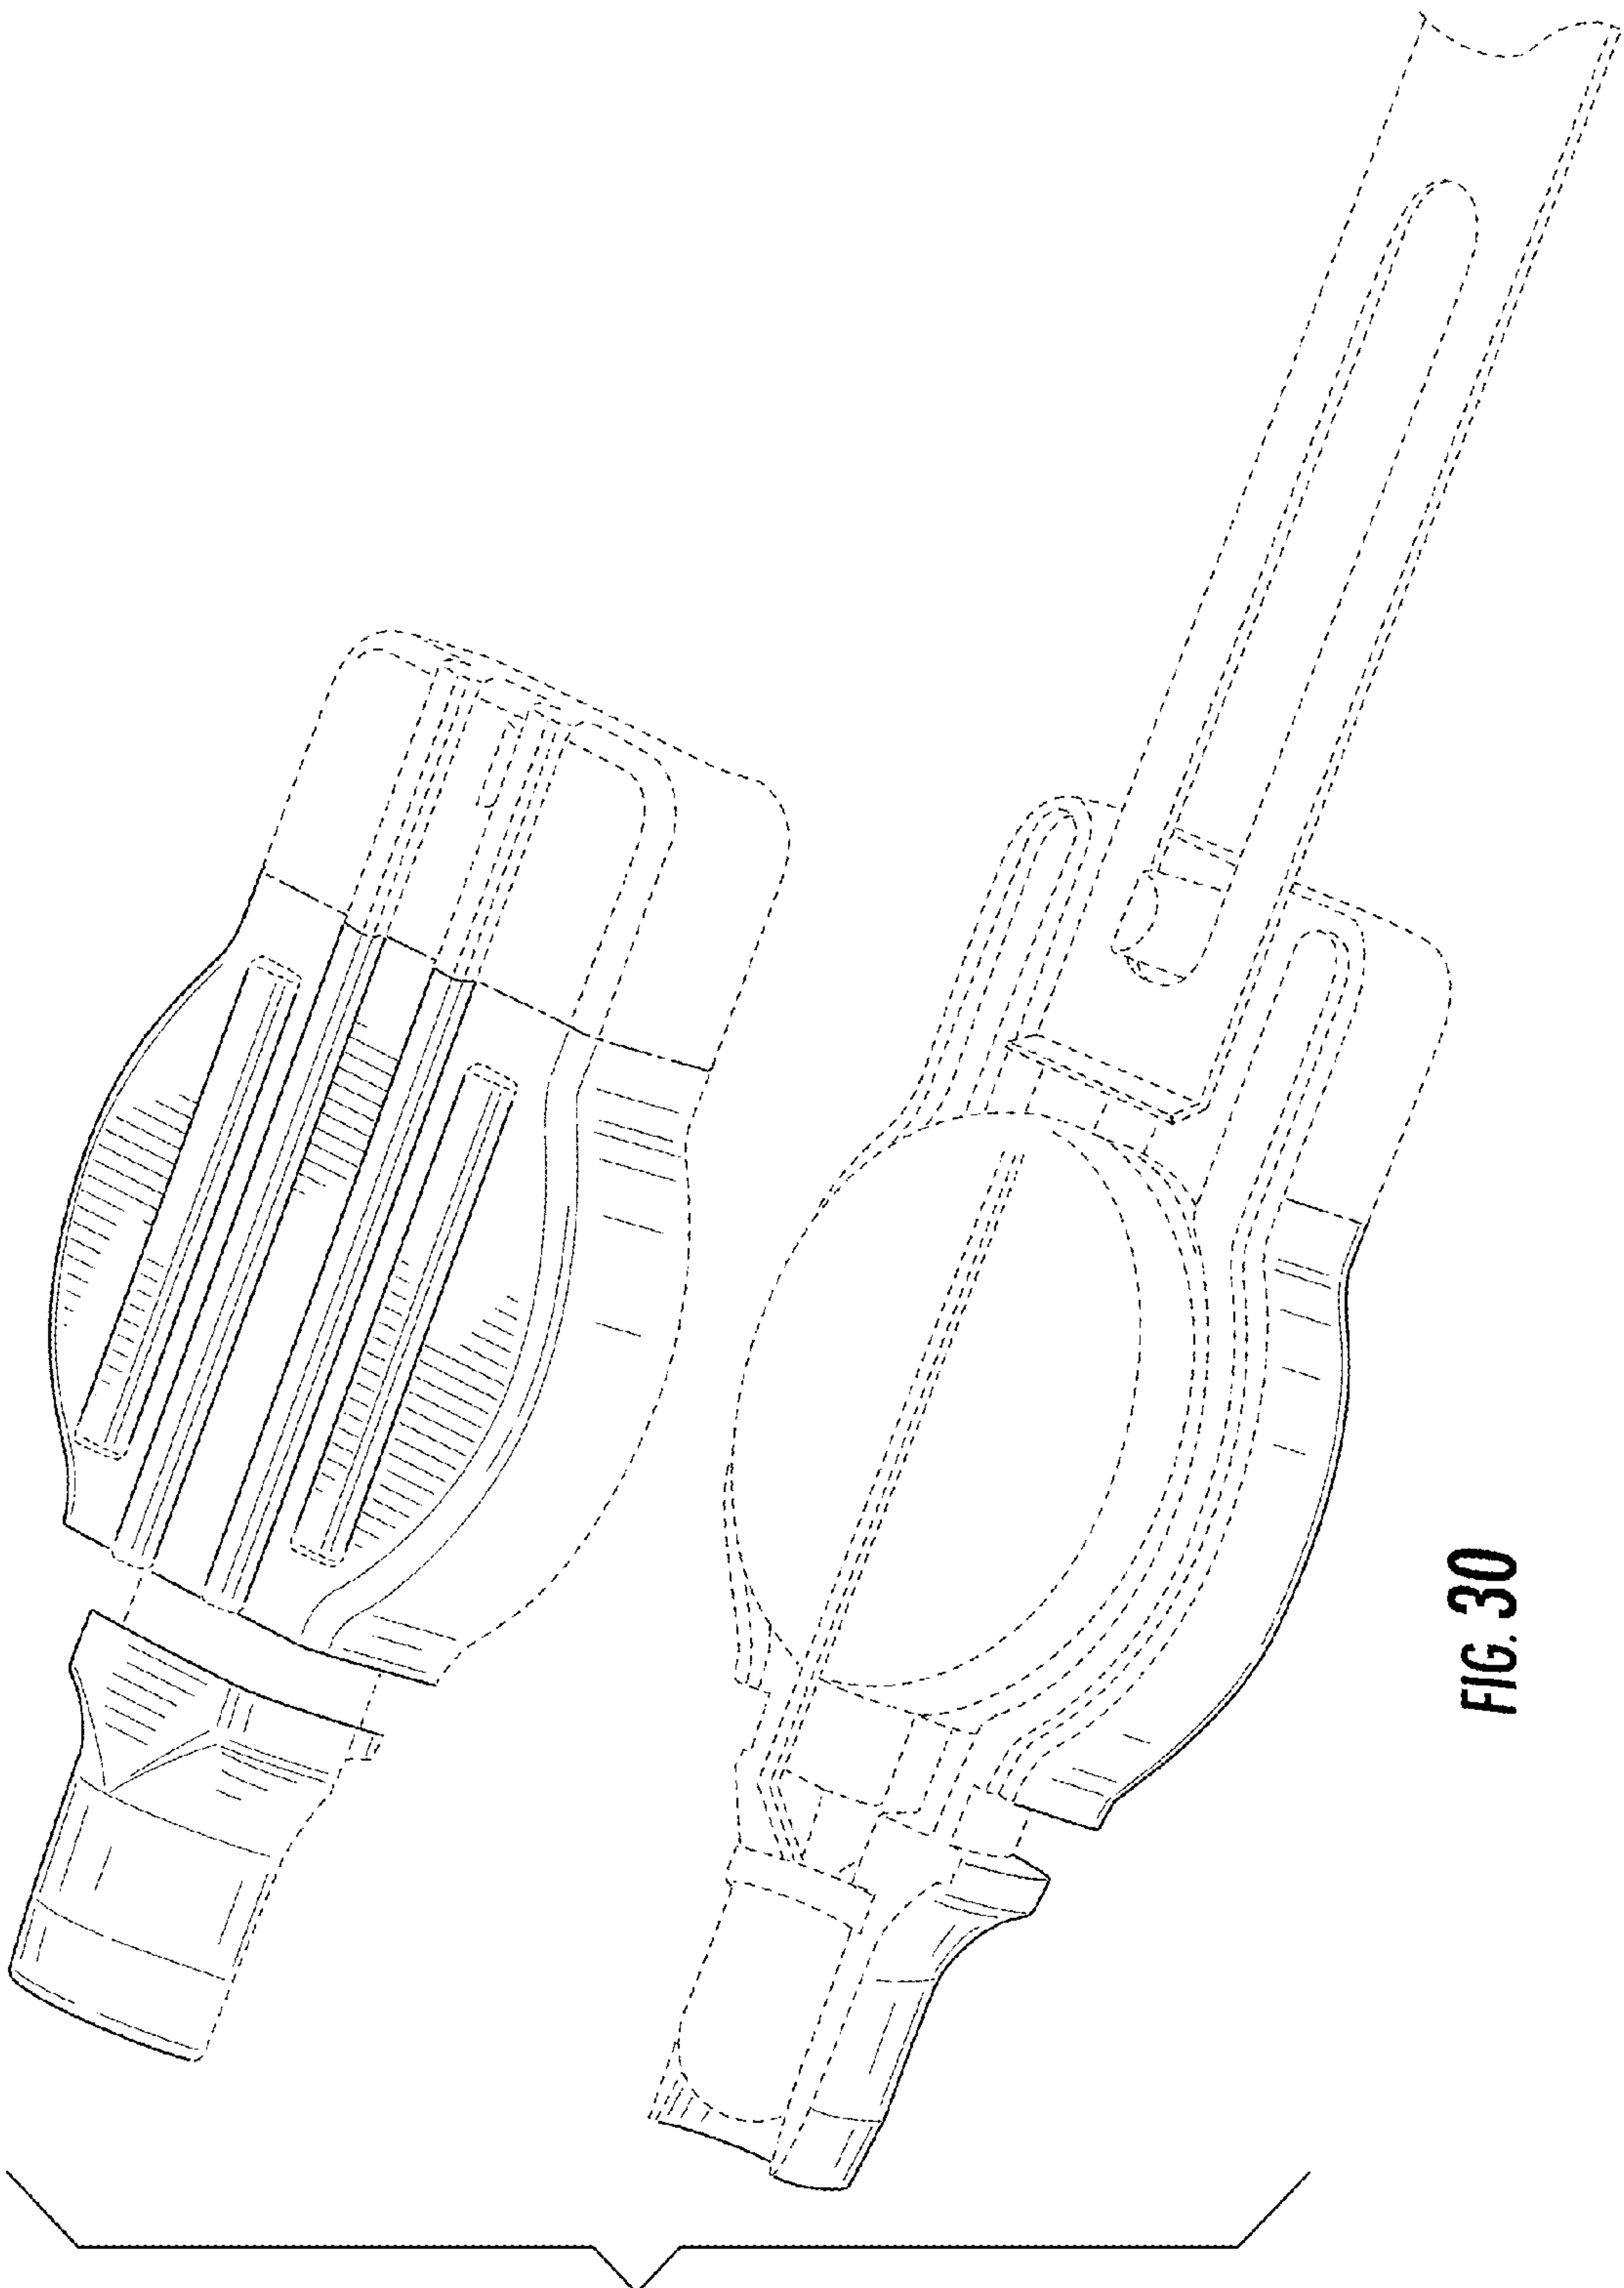


FIG. 30