



US00D742249S

(12) **United States Design Patent**  
**Farmer**

(10) **Patent No.:** **US D742,249 S**

(45) **Date of Patent:** **\*\* \*Nov. 3, 2015**

(54) **STERILIZATION WRAP MATERIAL**

(71) Applicant: **INVENIO HEALTHCARE, LLC,**  
Norcross, GA (US)

(72) Inventor: **Jeffrey James Farmer,** Roswell, GA  
(US)

(73) Assignee: **INVENIO HEALTHCARE, LLC,**  
Norcross, GA (US)

(\*) Notice: This patent is subject to a terminal disclaimer.

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/513,341**

(22) Filed: **Dec. 30, 2014**

(51) **LOC (10) Cl.** ..... **09-05**

(52) **U.S. Cl.**  
USPC ..... **D9/713**

(58) **Field of Classification Search**  
USPC ..... D9/702-714; 422/1, 28; 53/425, 570,  
53/469, 427, 433, 434; 47/72; 428/36.1,  
428/35.2, 34.2, 34.3, 192; 206/438;  
139/420 A, 426 R; 383/84;  
229/87.01-87.11

CPC ..... B65D 55/02; B65D 85/52; B65D 65/22;  
B65D 65/04

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

4,342,392 A \* 8/1982 Cox ..... 206/438  
4,874,090 A \* 10/1989 Dyke ..... 206/439  
5,441,550 A \* 8/1995 Hassenboehler et al. .... 55/486  
5,526,933 A \* 6/1996 Weder ..... 206/423

5,683,794 A \* 11/1997 Wadsworth et al. .... 442/382  
5,695,595 A \* 12/1997 Van Hout et al. .... 264/310  
6,406,764 B2 \* 6/2002 Bayer ..... 428/35.2  
6,517,916 B1 \* 2/2003 Bayer et al. .... 428/34.3  
7,361,317 B2 \* 4/2008 Bourne et al. .... 422/292  
7,560,082 B2 \* 7/2009 Stecklein et al. .... 422/294  
7,718,433 B2 \* 5/2010 Stecklein et al. .... 436/10  
7,922,983 B2 \* 4/2011 Prokash et al. .... 422/294  
8,852,502 B2 \* 10/2014 Landgrebe et al. .... 422/26

\* cited by examiner

*Primary Examiner* — Caron D Veynar

*Assistant Examiner* — Abraham Bahta

(74) *Attorney, Agent, or Firm* — Withers & Keys, LLC

(57) **CLAIM**

The ornamental design for a sterilization wrap material, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a sterilization wrap material showing my new design;

FIG. 2 is a frontal view of the sterilization wrap material shown in FIG. 1;

FIG. 3 is a rear view of the sterilization wrap material shown in FIG. 1;

FIG. 4 is a bottom view of the sterilization wrap material shown in FIG. 2;


FIG. 5 is a top view of the sterilization wrap material shown in FIG. 2;

FIG. 6 is a side view as viewed from the right-hand side of the sterilization wrap material shown in FIG. 2; and,

FIG. 7 is a side view as viewed from the left-hand side of the sterilization wrap material shown in FIG. 2.

The broken lines shown in the drawings illustrate portions of the sterilization wrap material that forms no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

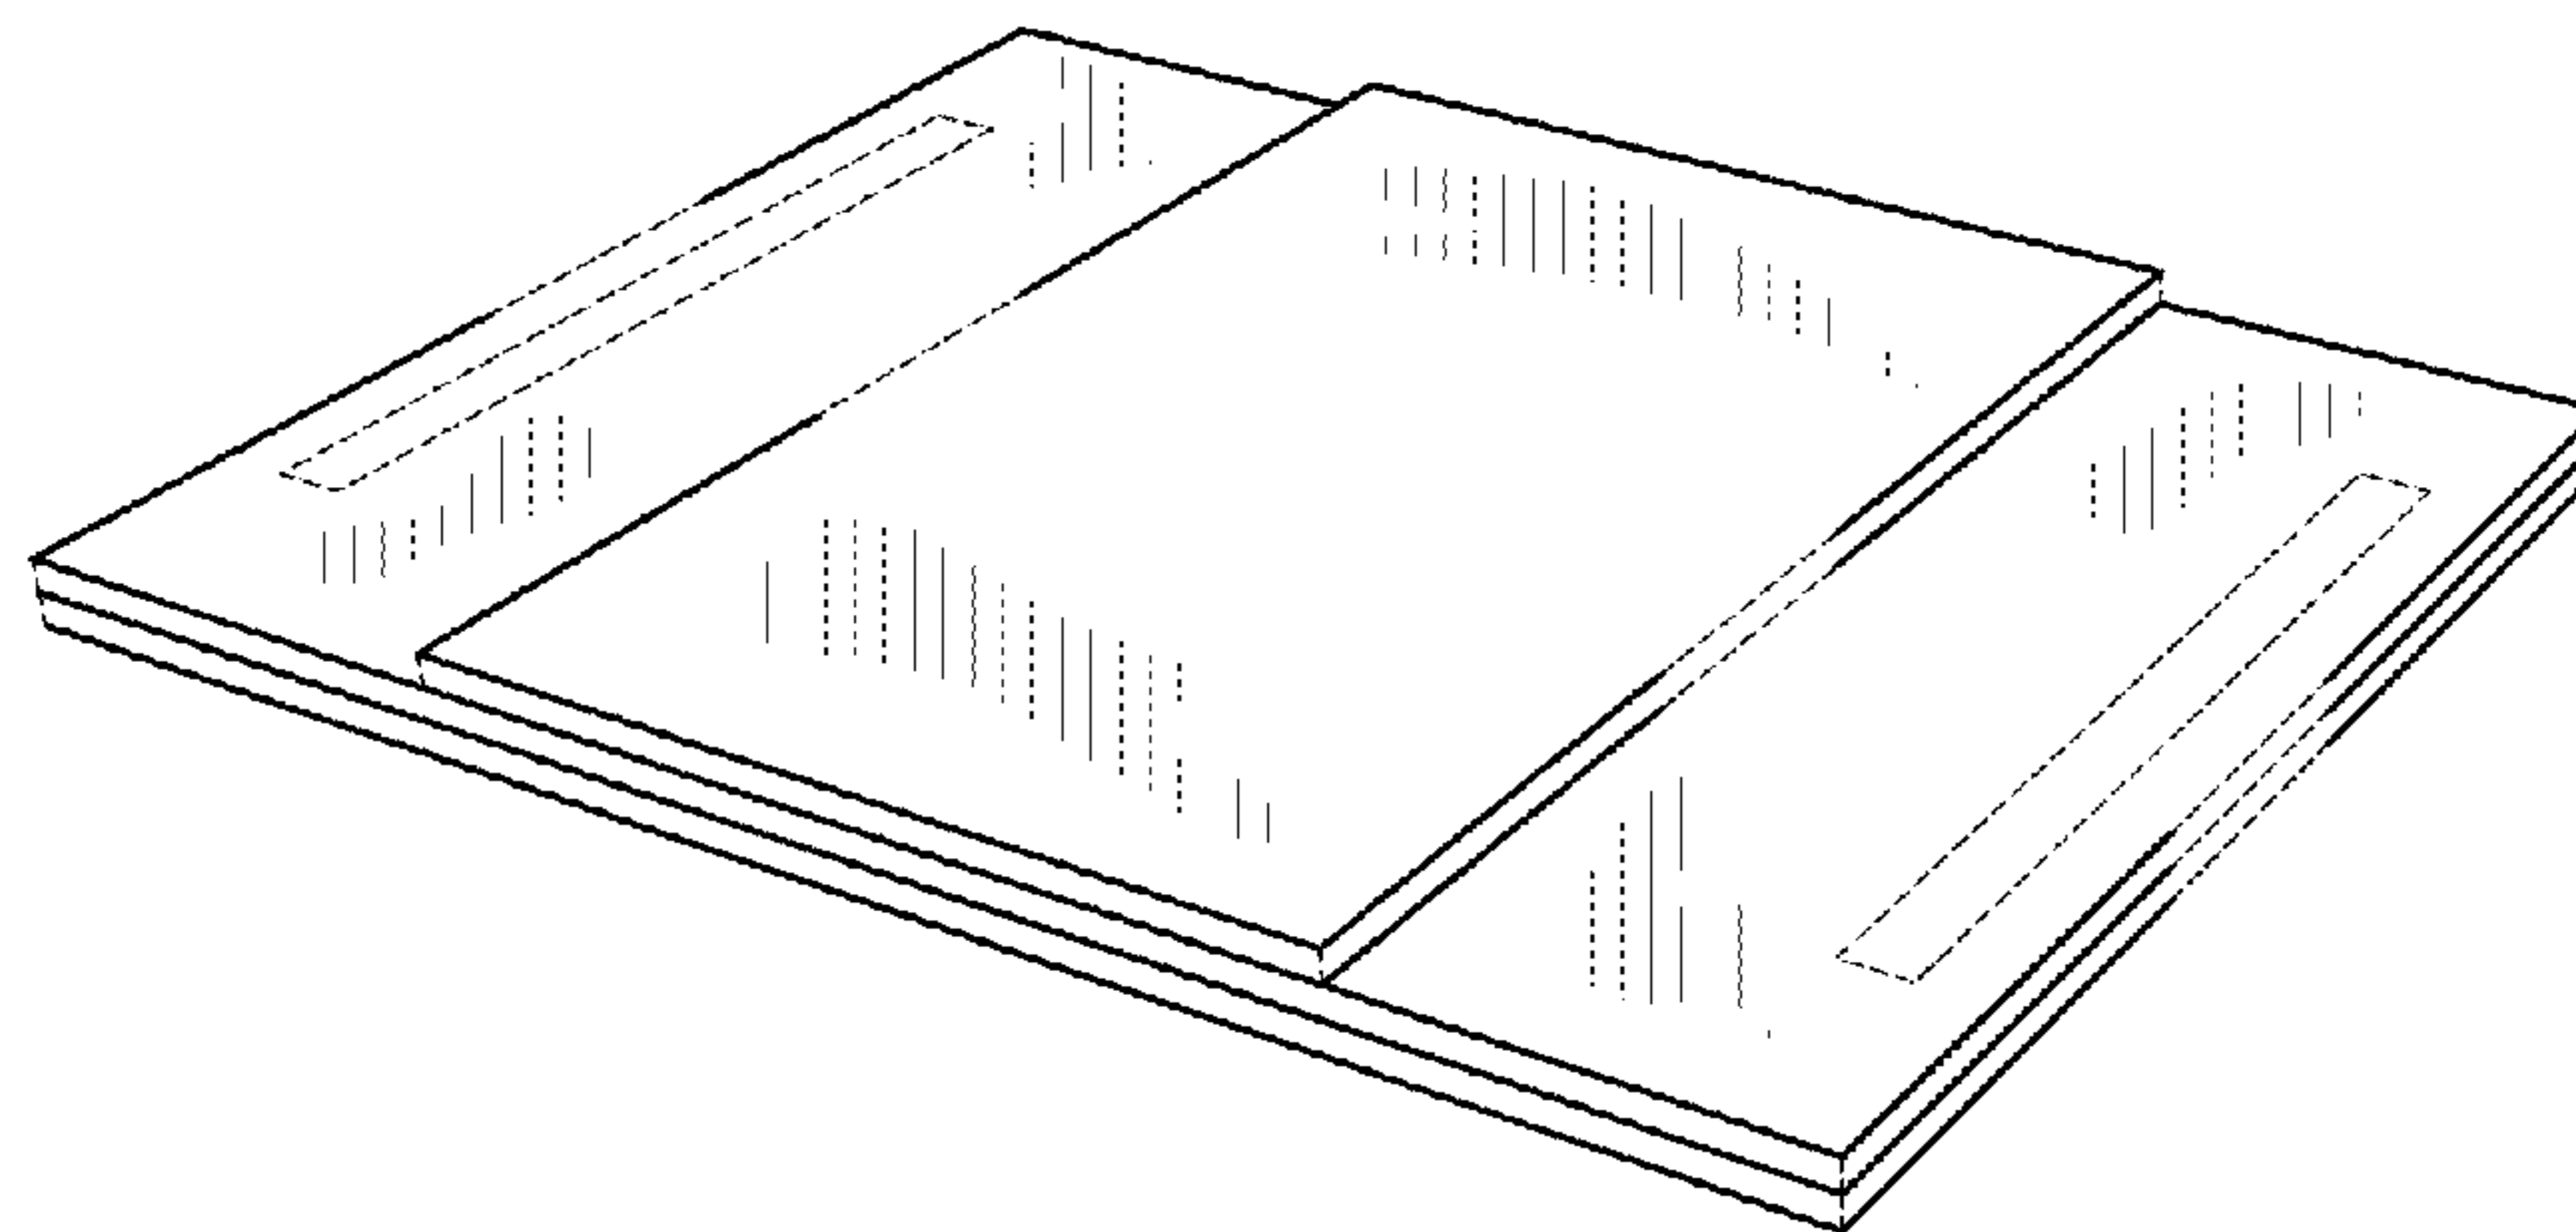

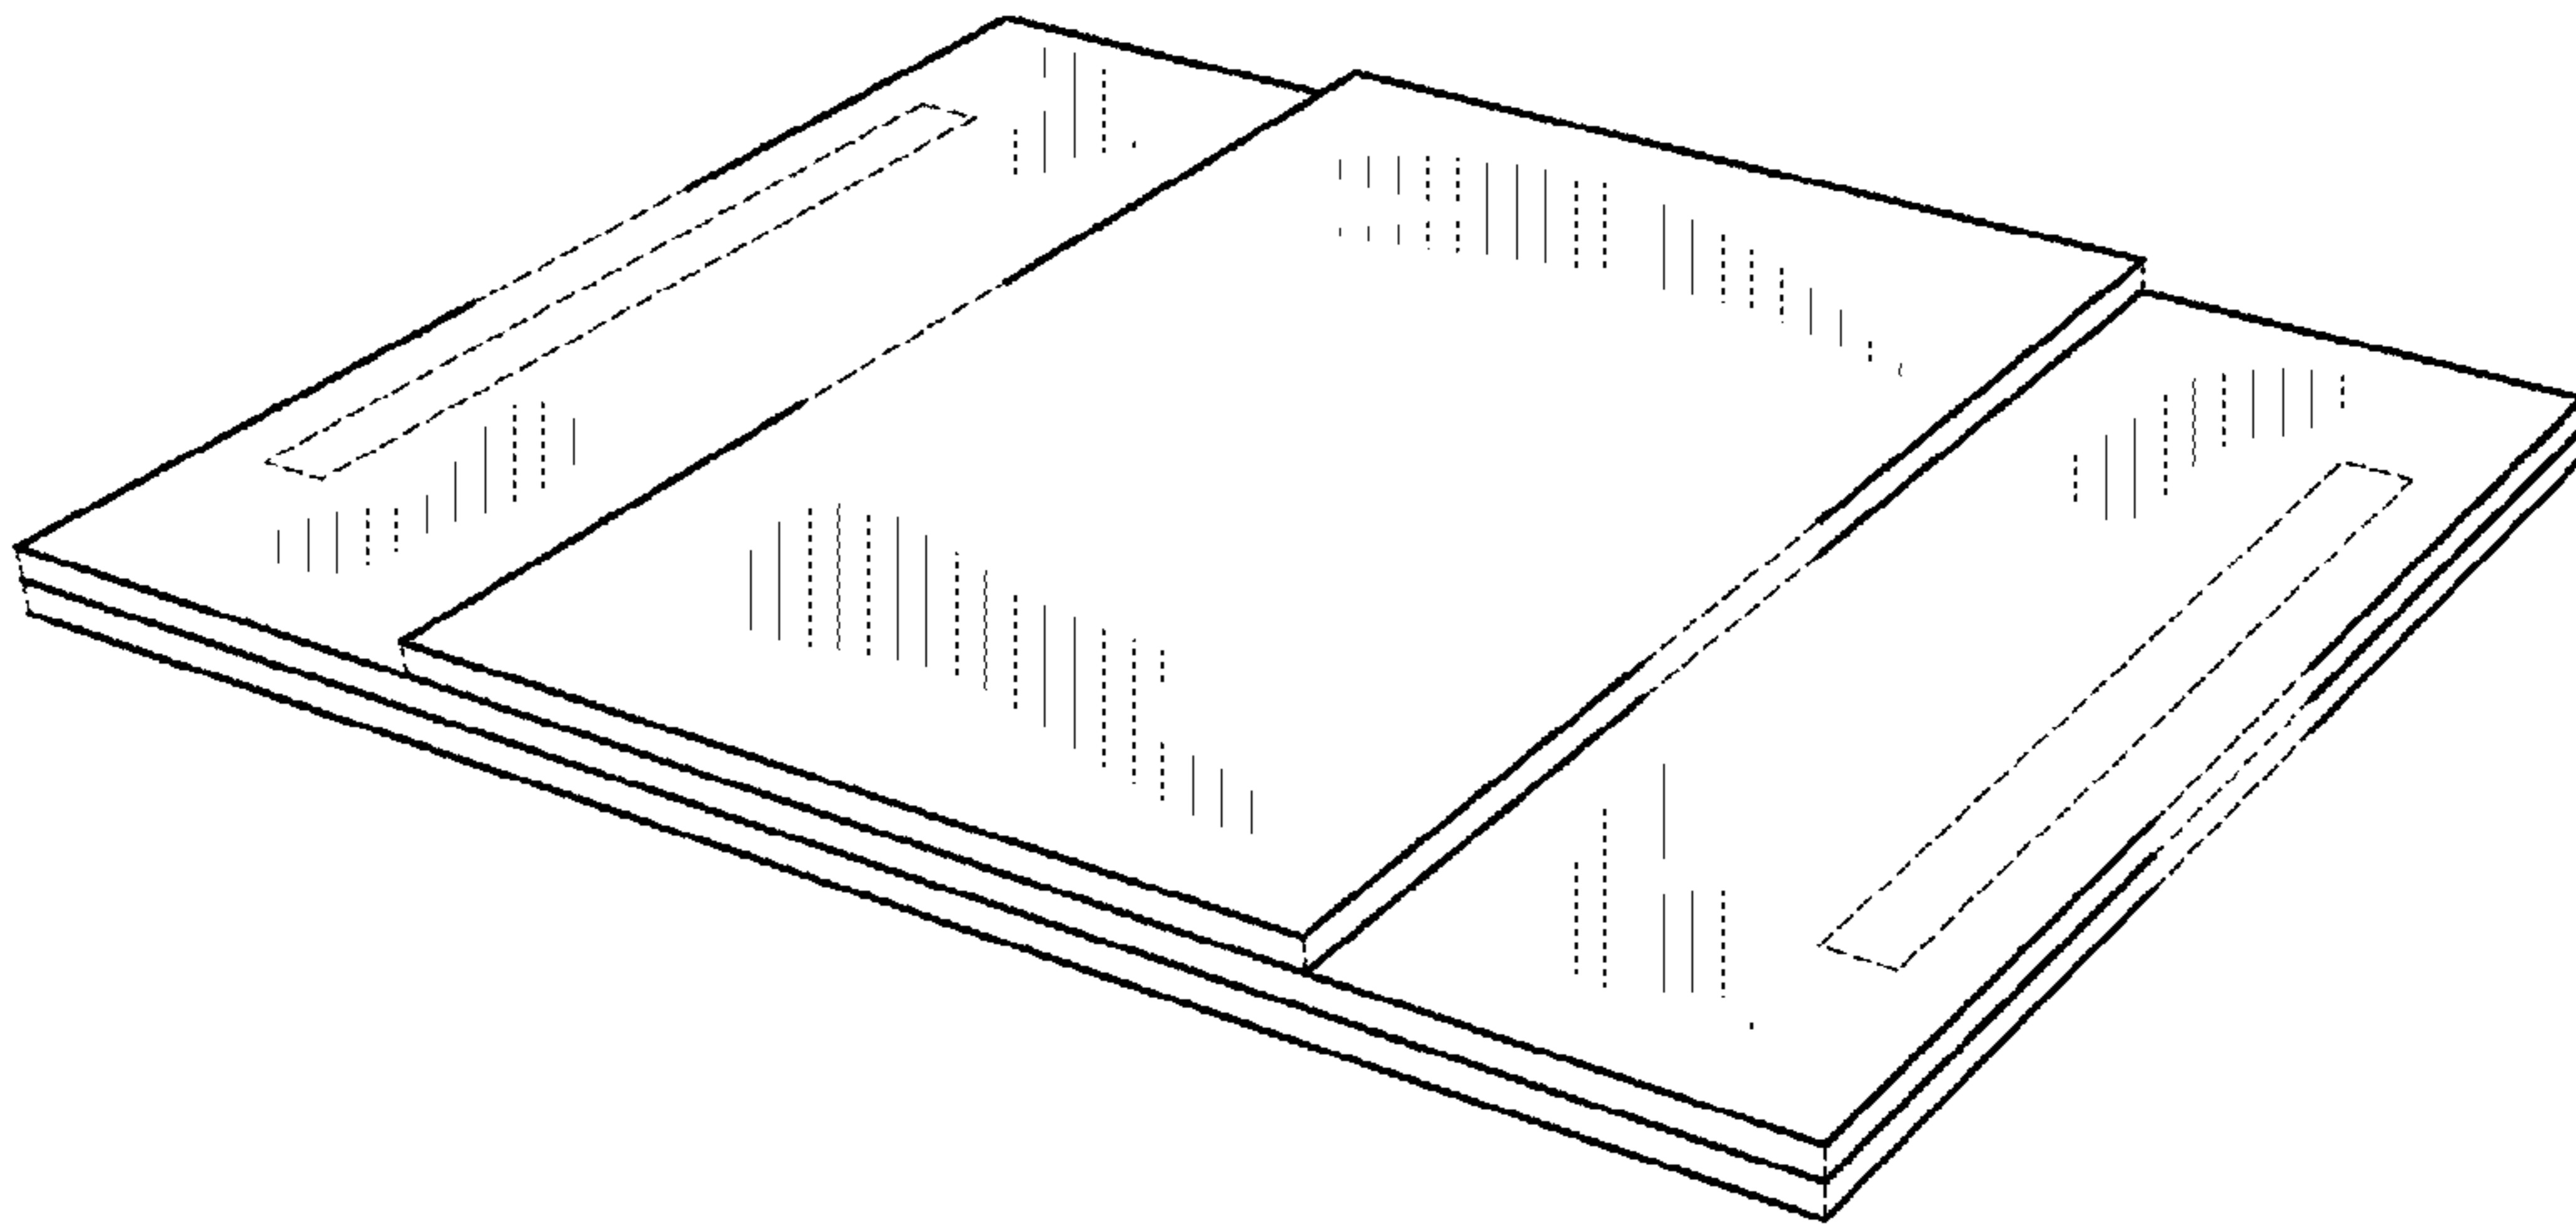


FIG. 1

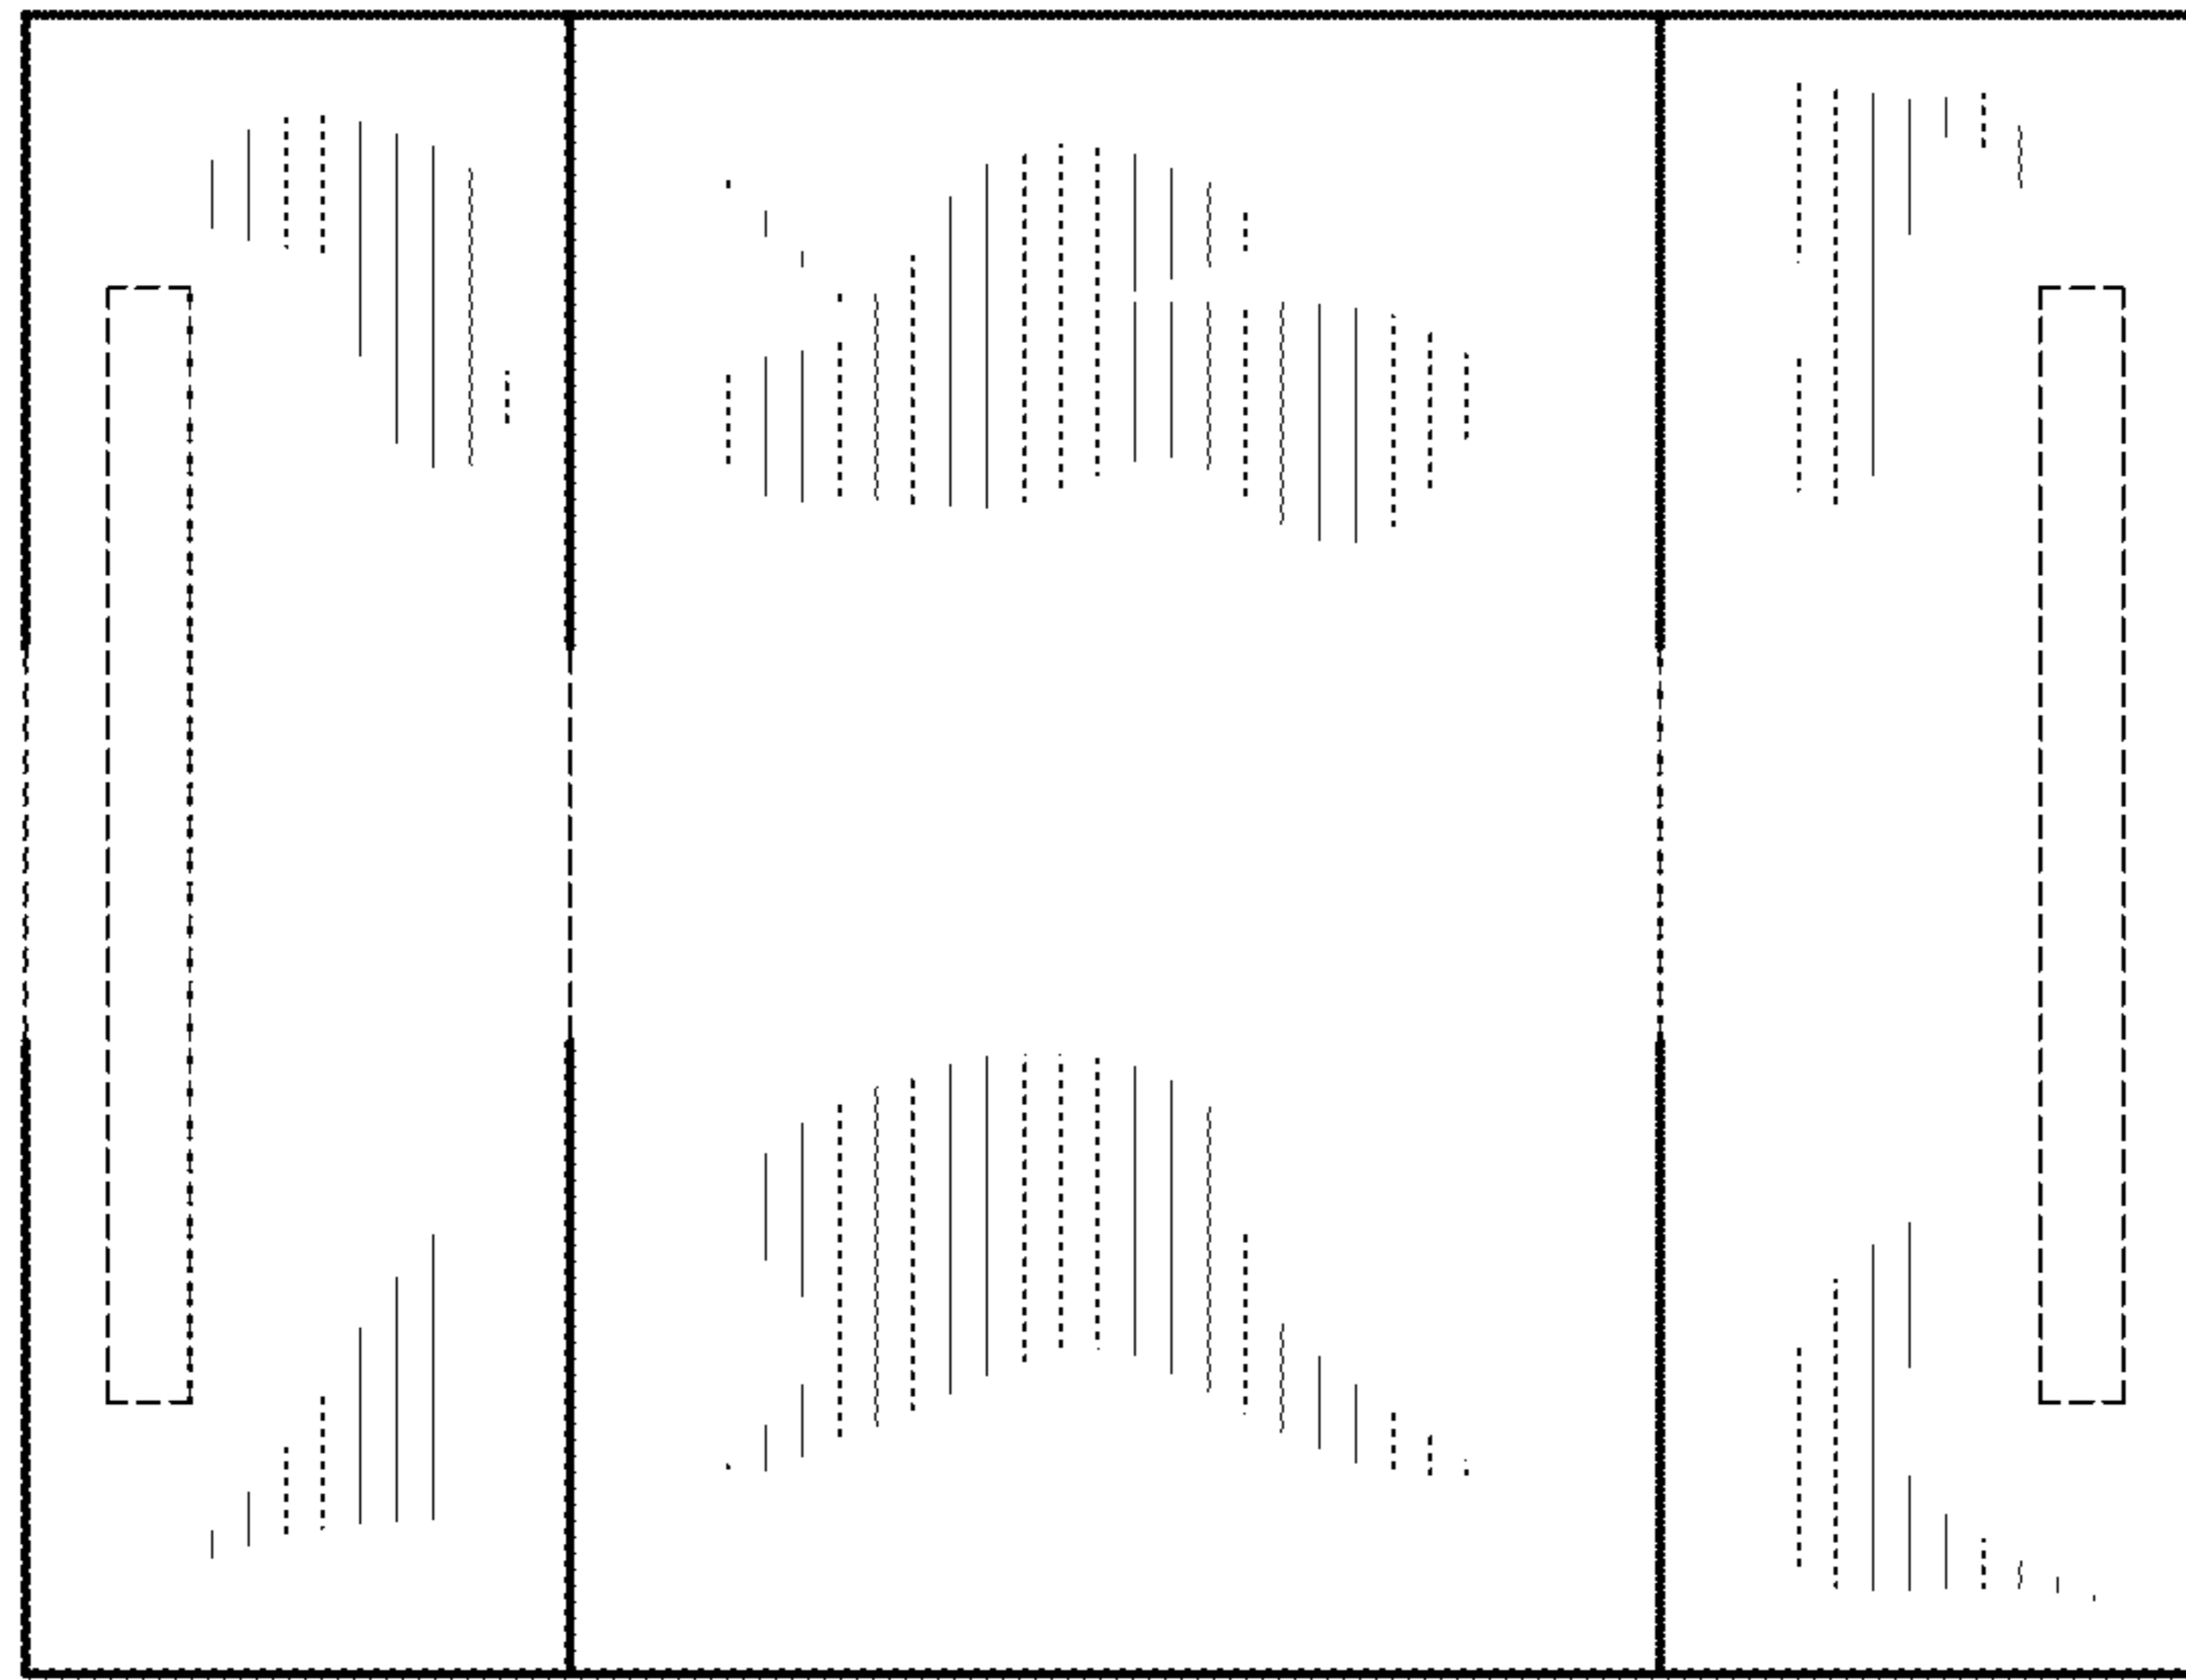


FIG. 2

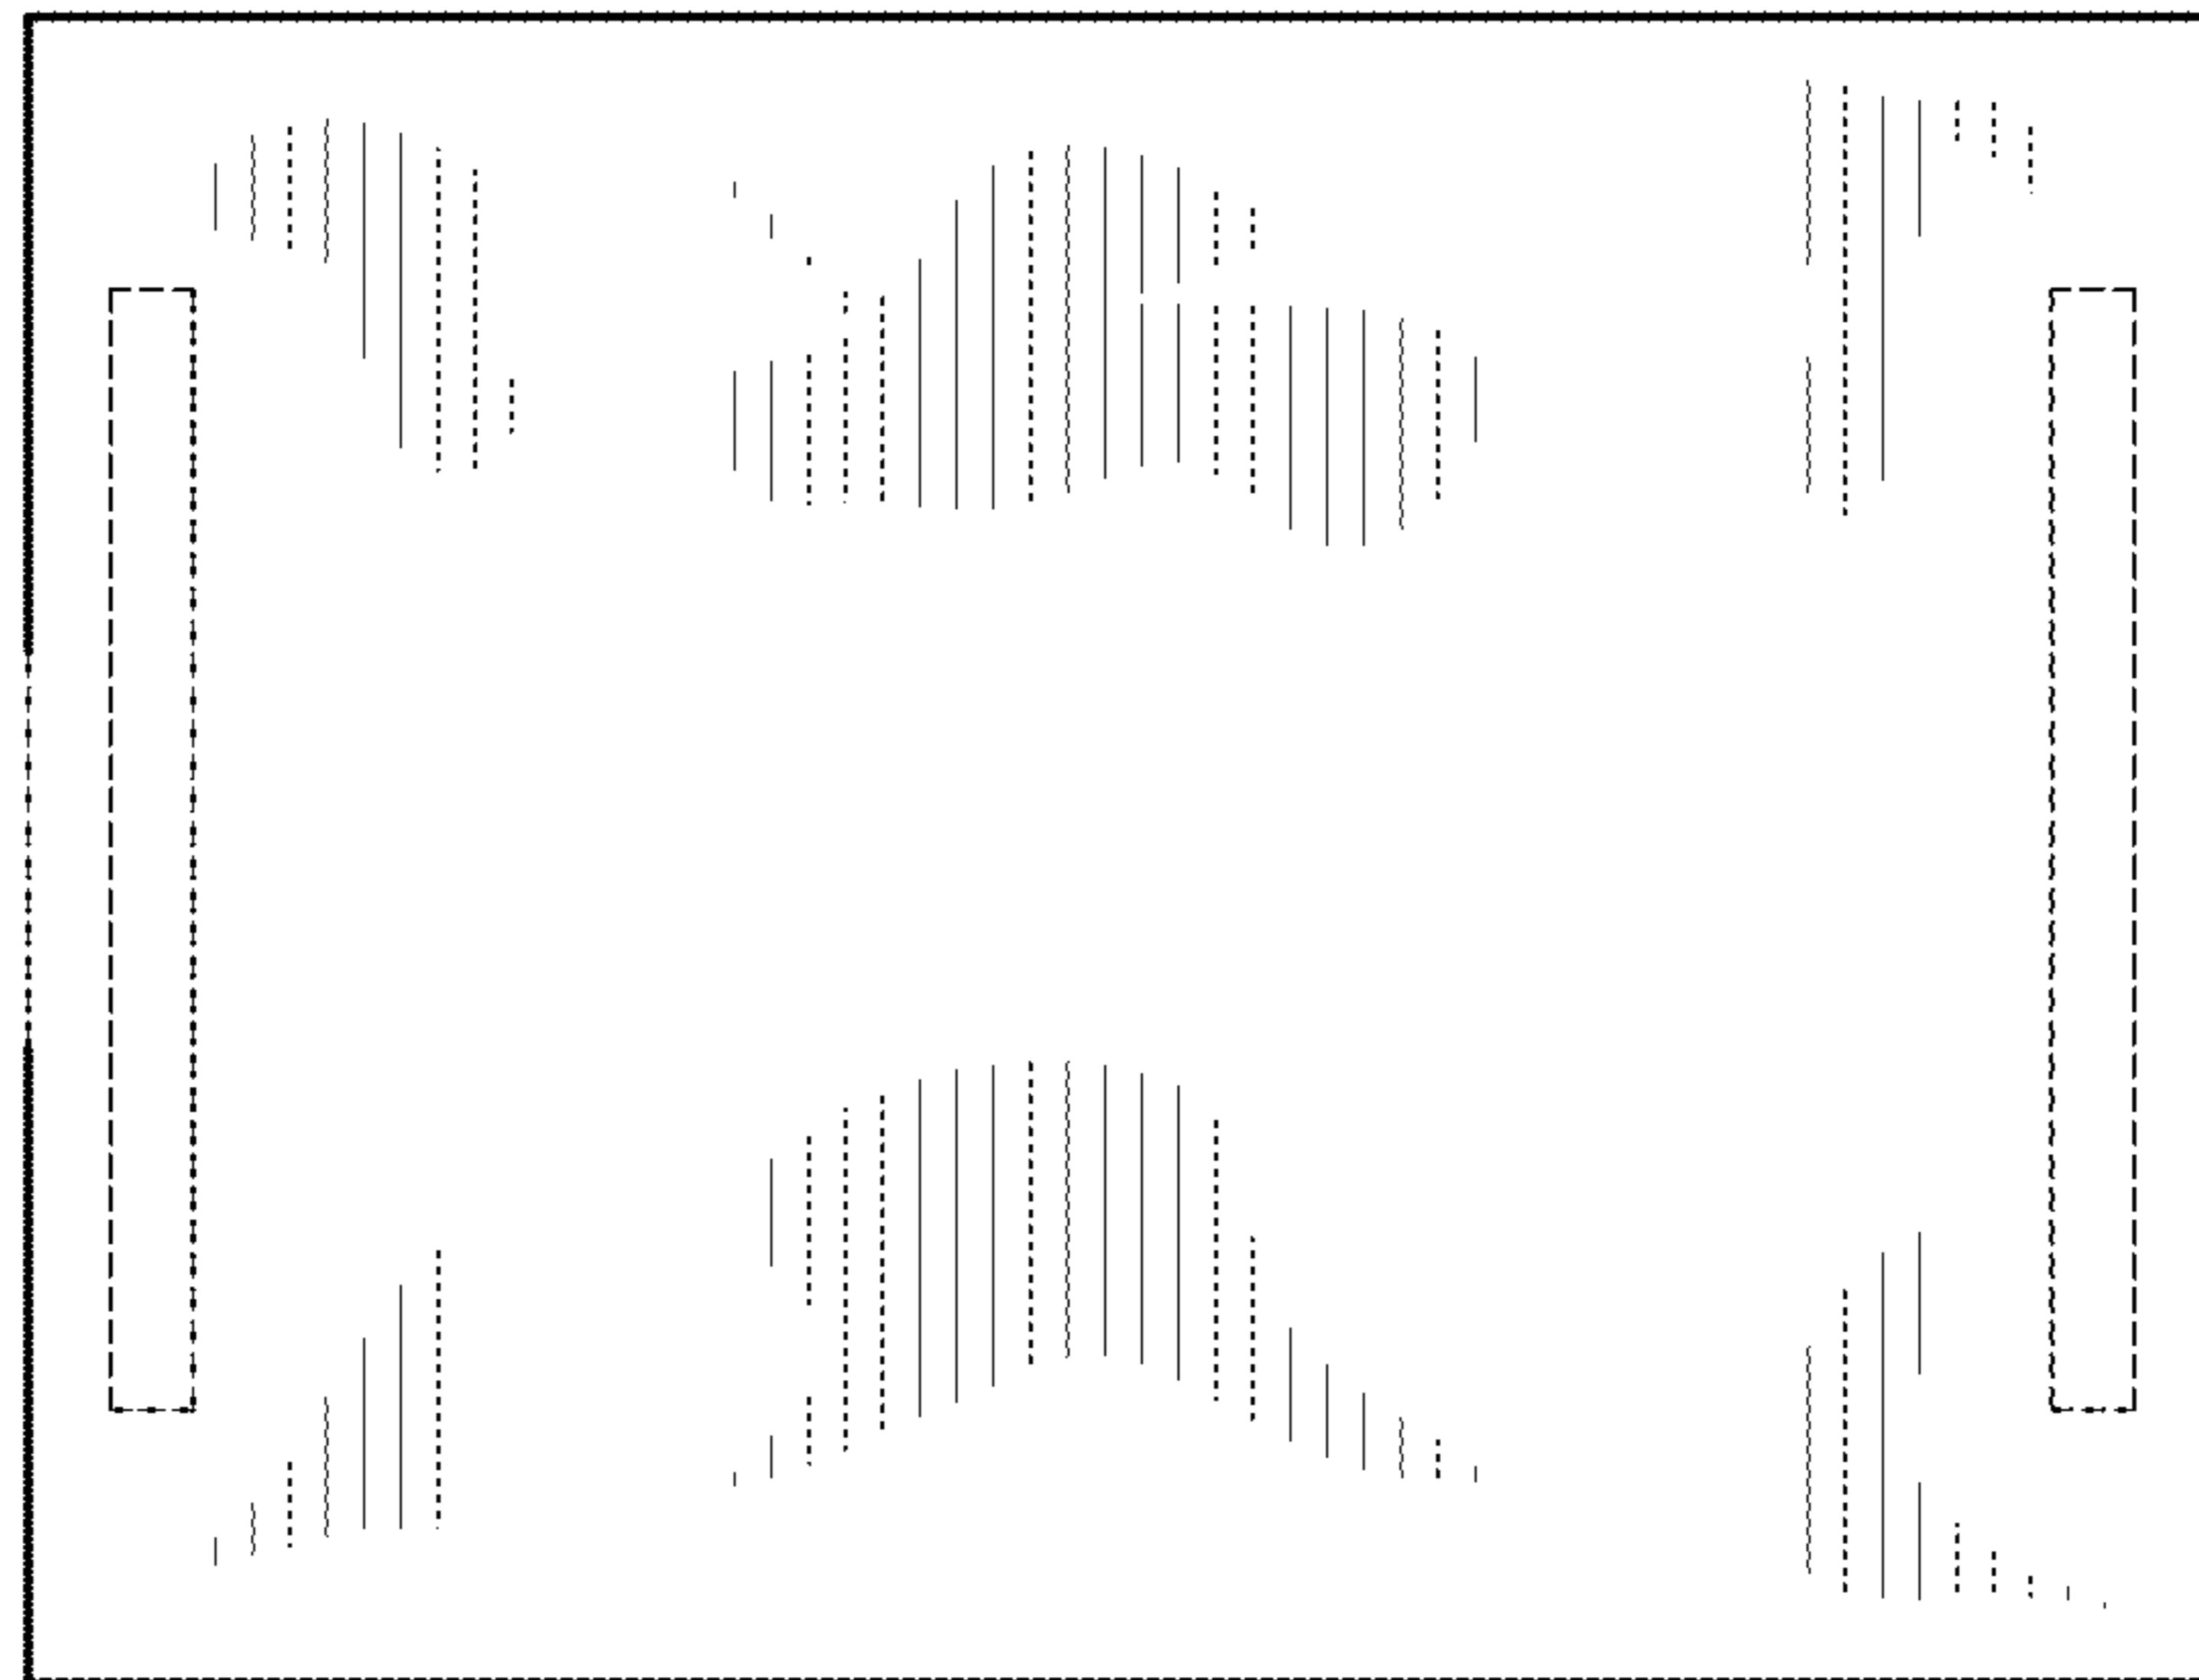


FIG. 3



FIG. 4

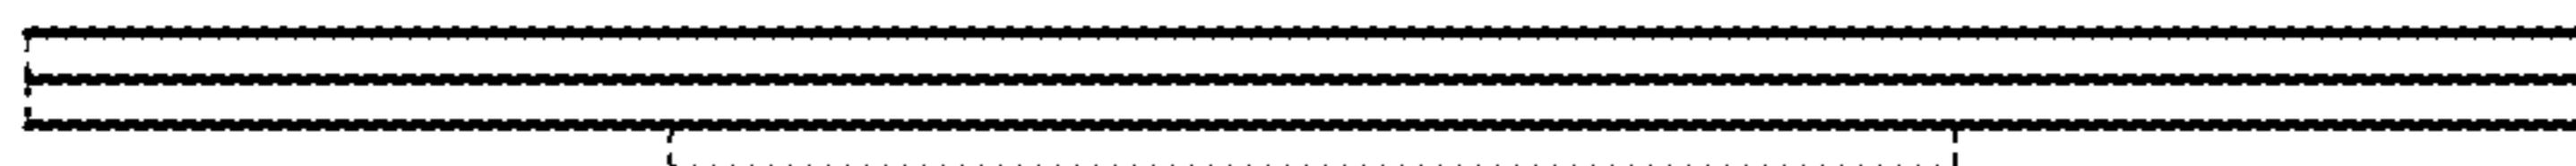


FIG. 5



FIG. 6



FIG. 7