



US00D743039S

(12) **United States Design Patent**
Hagedorn

(10) **Patent No.:** **US D743,039 S**
(45) **Date of Patent:** **** Nov. 10, 2015**

(54) **HEADGEAR FOR ELECTROPHYSIOLOGY
MEASUREMENT AND TRAINING**

(71) Applicant: **Evoke Neuroscience, Inc.**, Jacksonville,
NC (US)

(72) Inventor: **David W Hagedorn**, Jacksonville, NC
(US)

(73) Assignee: **EVOKE NEUROSCIENCE, INC.**,
Jacksonville, NC (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/499,271**

(22) Filed: **Aug. 13, 2014**

(51) **LOC (10) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/186**

(58) **Field of Classification Search**

USPC D24/165–168, 186, 187, 107, 200;
D10/70, 75, 97, 98; 600/301, 382–384,
600/386, 390, 483, 500–503, 508, 509,
600/513; 128/DIG. 15; D14/341, 344, 205
CPC A61B 5/6803; A61B 5/681; A61B 5/6824;
A61B 5/6825; A61B 5/024; A61B 5/02405;
A61B 5/02438

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,154,669 A * 11/2000 Hunter A61B 5/0478
600/383
D578,221 S * 10/2008 Sakurai D24/187
D585,557 S * 1/2009 Sakurai D24/187

8,239,030 B1 * 8/2012 Hagedorn A61B 5/0482
607/45
8,989,835 B2 * 3/2015 Badower A61B 5/00
600/383
2009/0285435 A1 * 11/2009 Nelson F16C 11/06
381/378
2014/0350431 A1 * 11/2014 Hagedorn A61B 5/0478
600/544

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Bechen PLLC

(57) **CLAIM**


The ornamental design for a headgear for electrophysiology measurement and training, as shown and described.

DESCRIPTION

FIG. 1 illustrates a perspective view of a headgear for electrophysiology measurement and training;
FIG. 2 illustrates a front view, as well as a rear view, of the headgear for electrophysiology measurement and training;
FIG. 3 illustrates a right side view, as well as a left side view, of the headgear for electrophysiology measurement and training;
FIG. 4 illustrates a top view of the headgear for electrophysiology measurement and training;
FIG. 5 illustrates a bottom view of the headgear for electrophysiology measurement and training; and,
FIG. 6 illustrates a cut-away perspective view of a top portion of the headgear for electrophysiology measurement and training.

The broken lines in the drawing views are included for the purpose of illustrating portions of the headgear for electrophysiology measurement and training that form no part of the claimed design

1 Claim, 5 Drawing Sheets

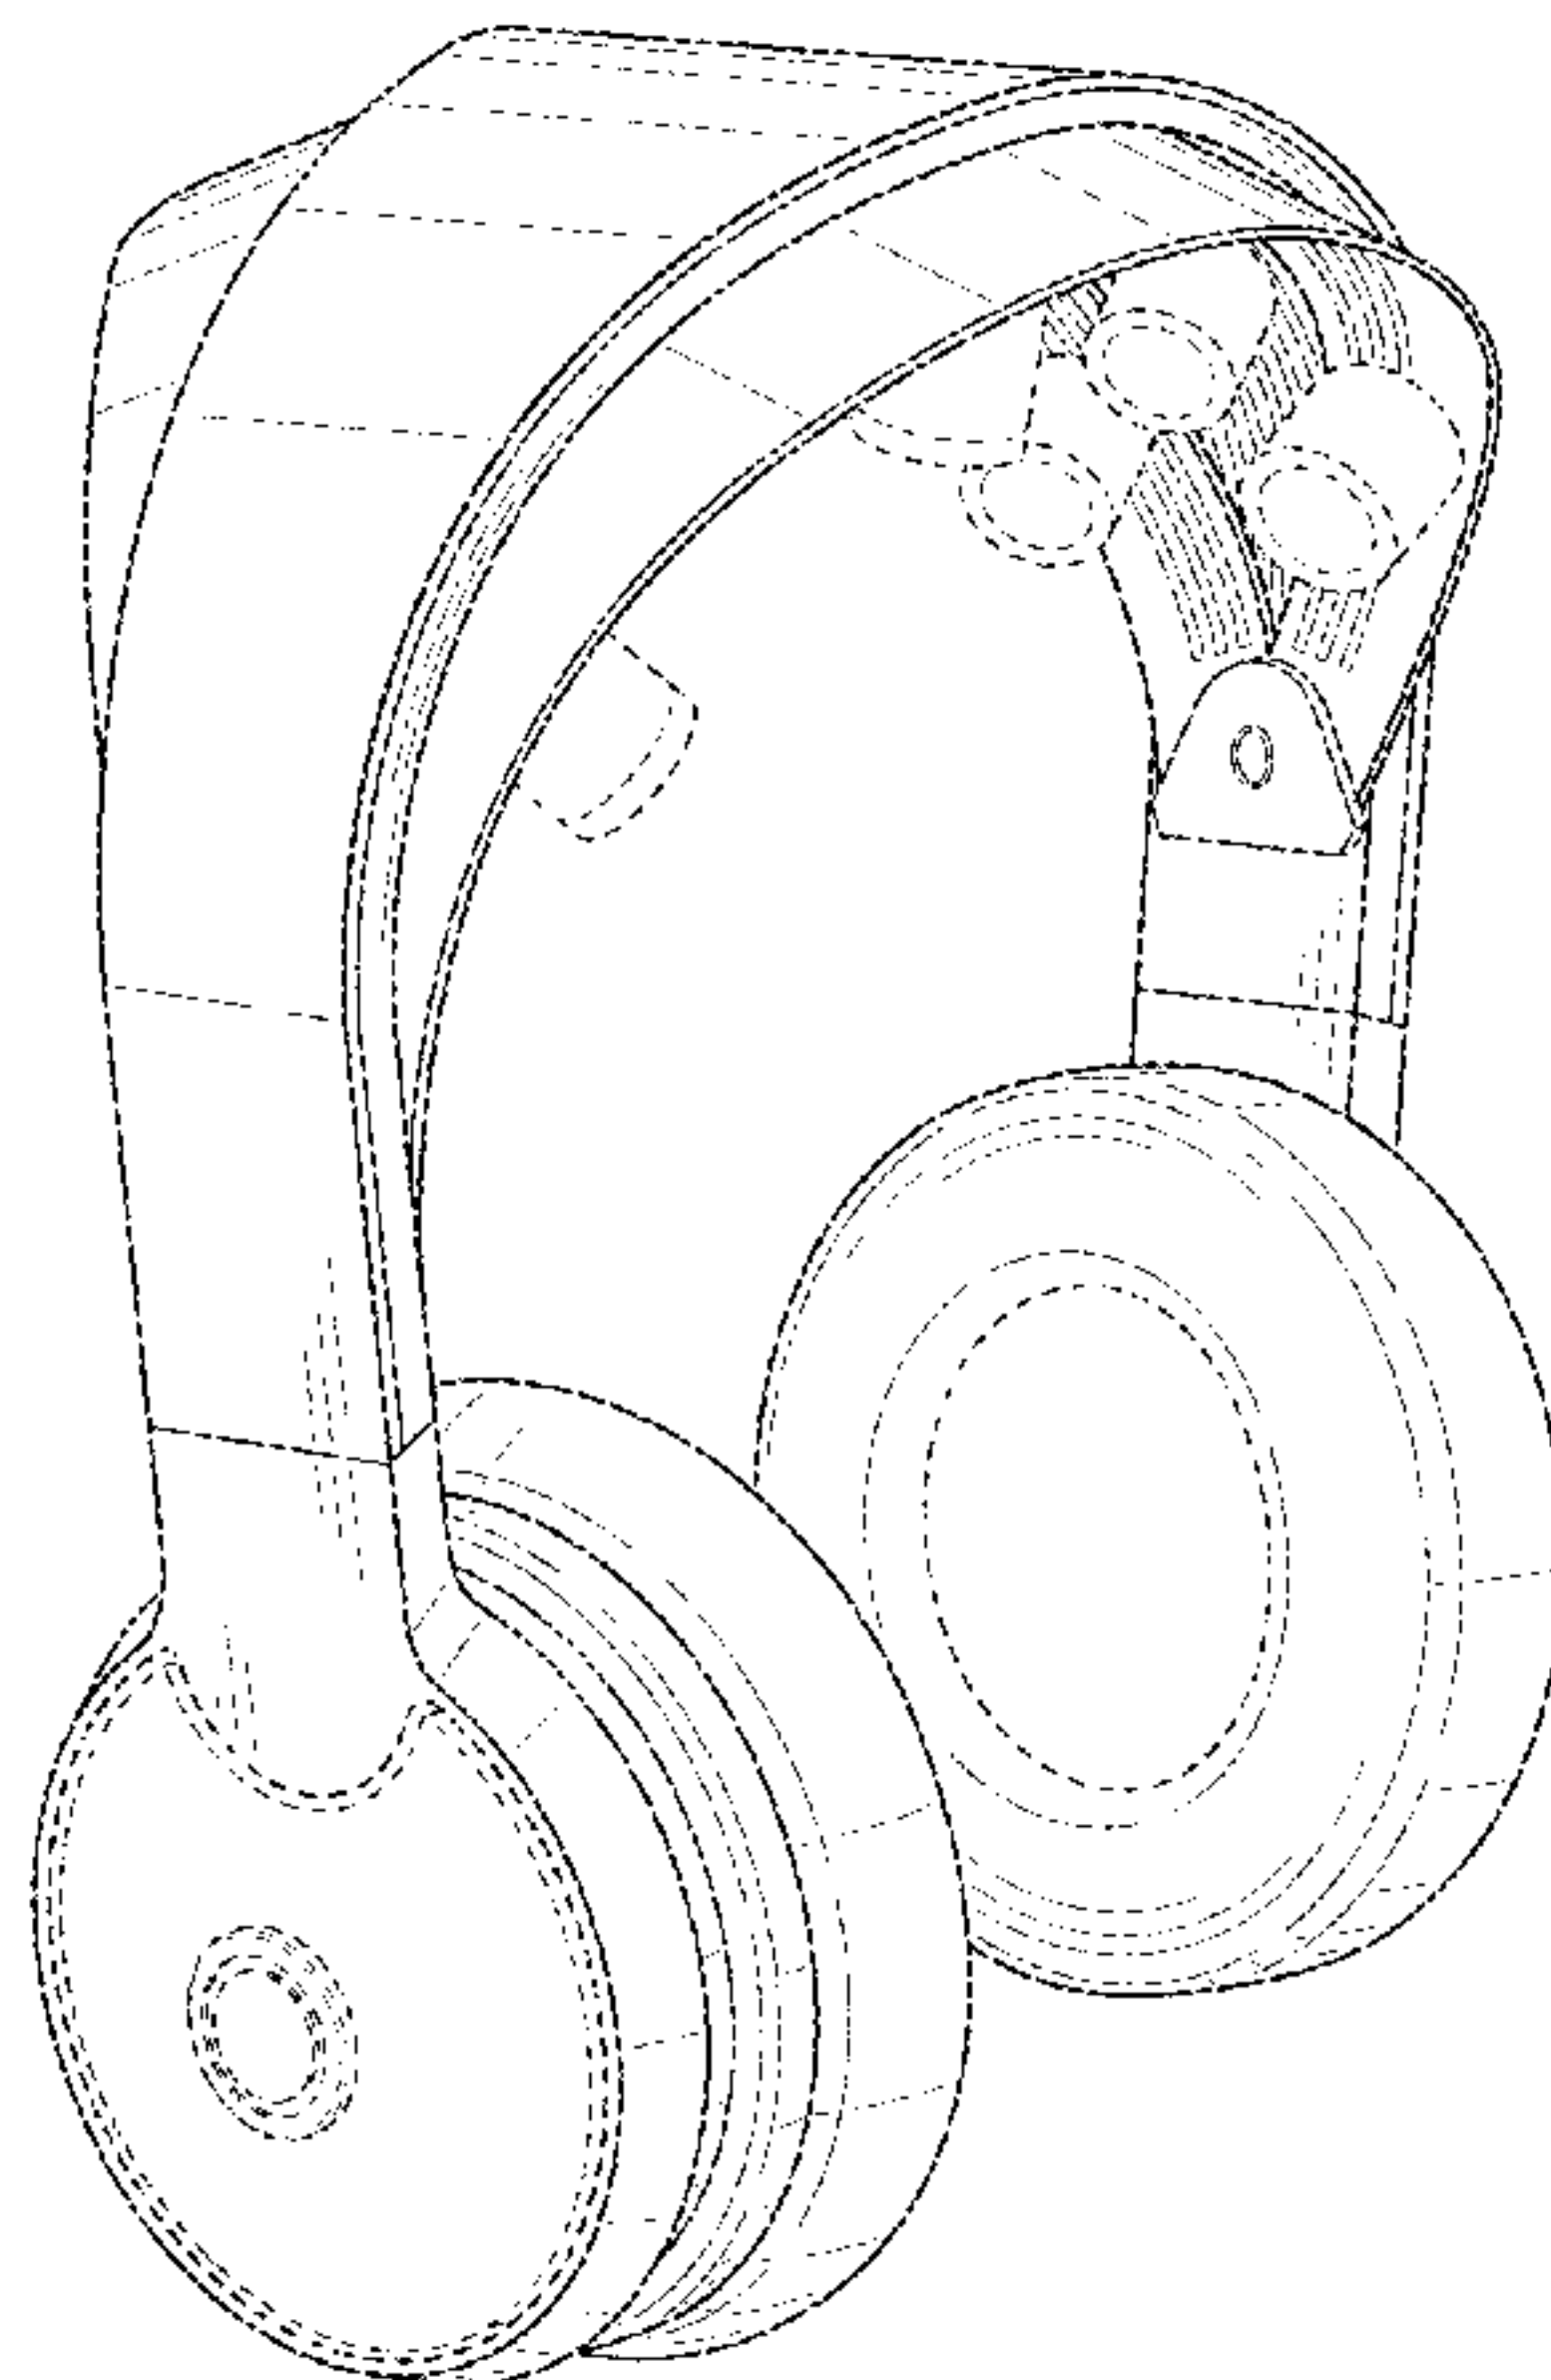

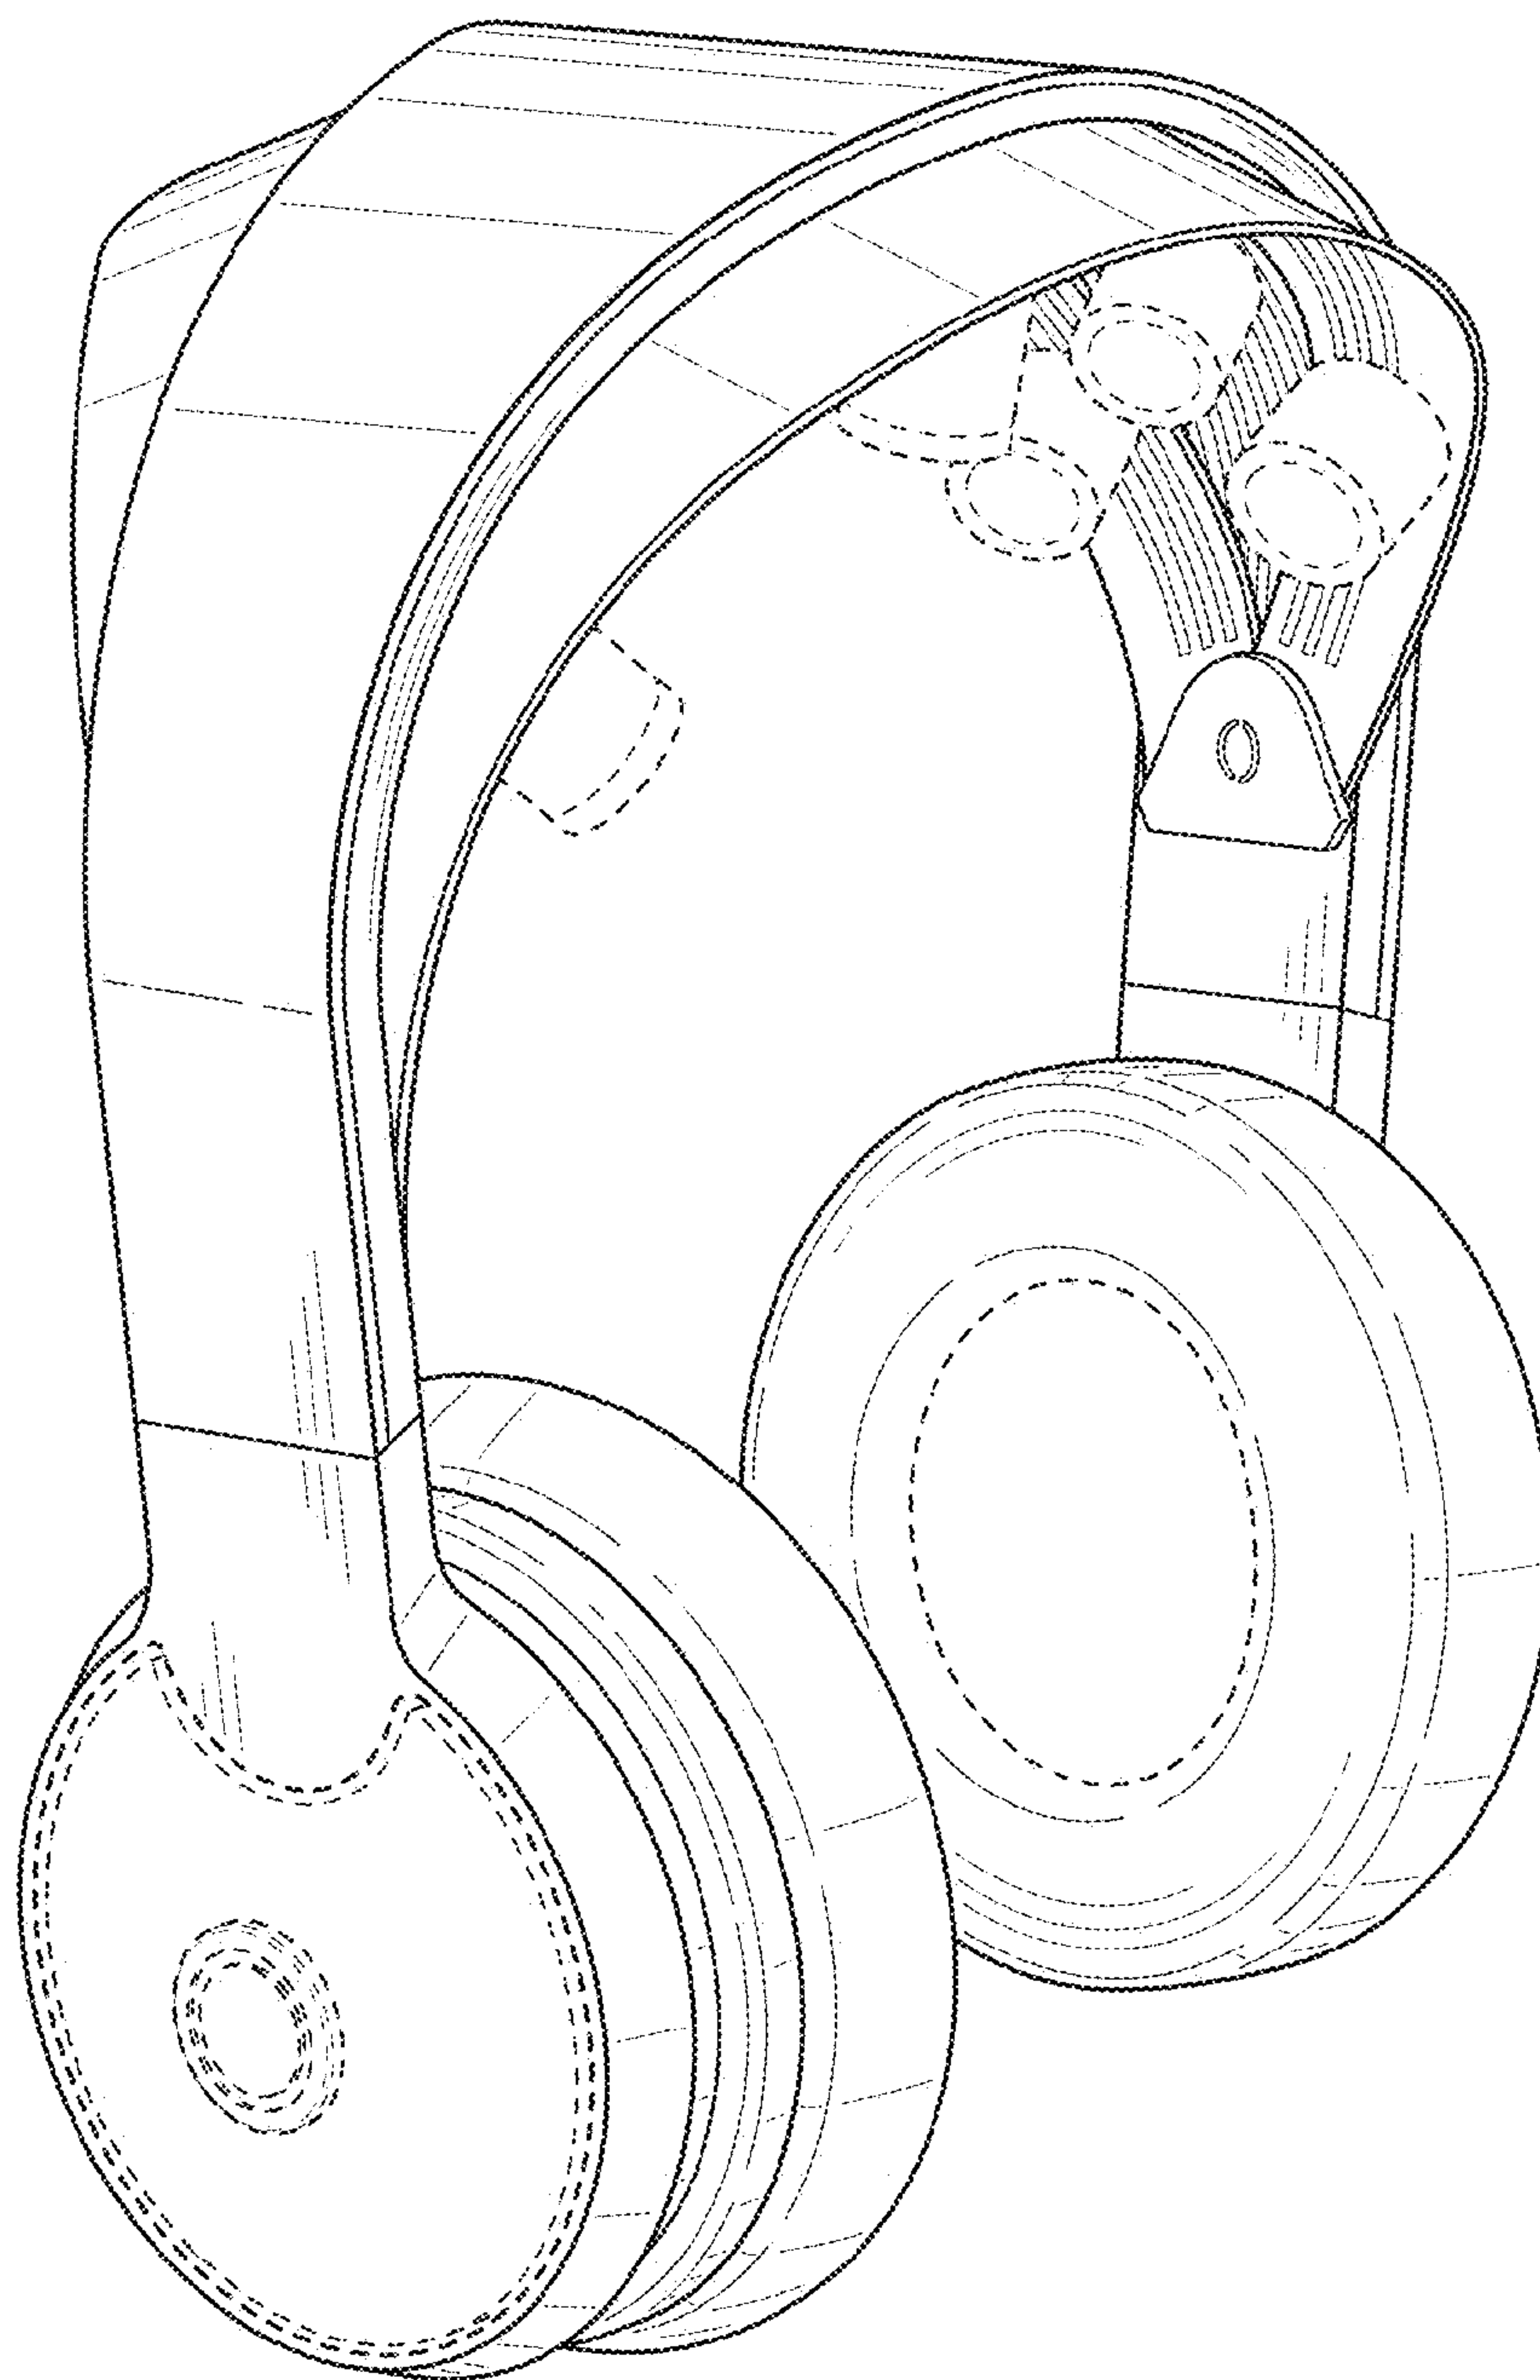


FIG. 1

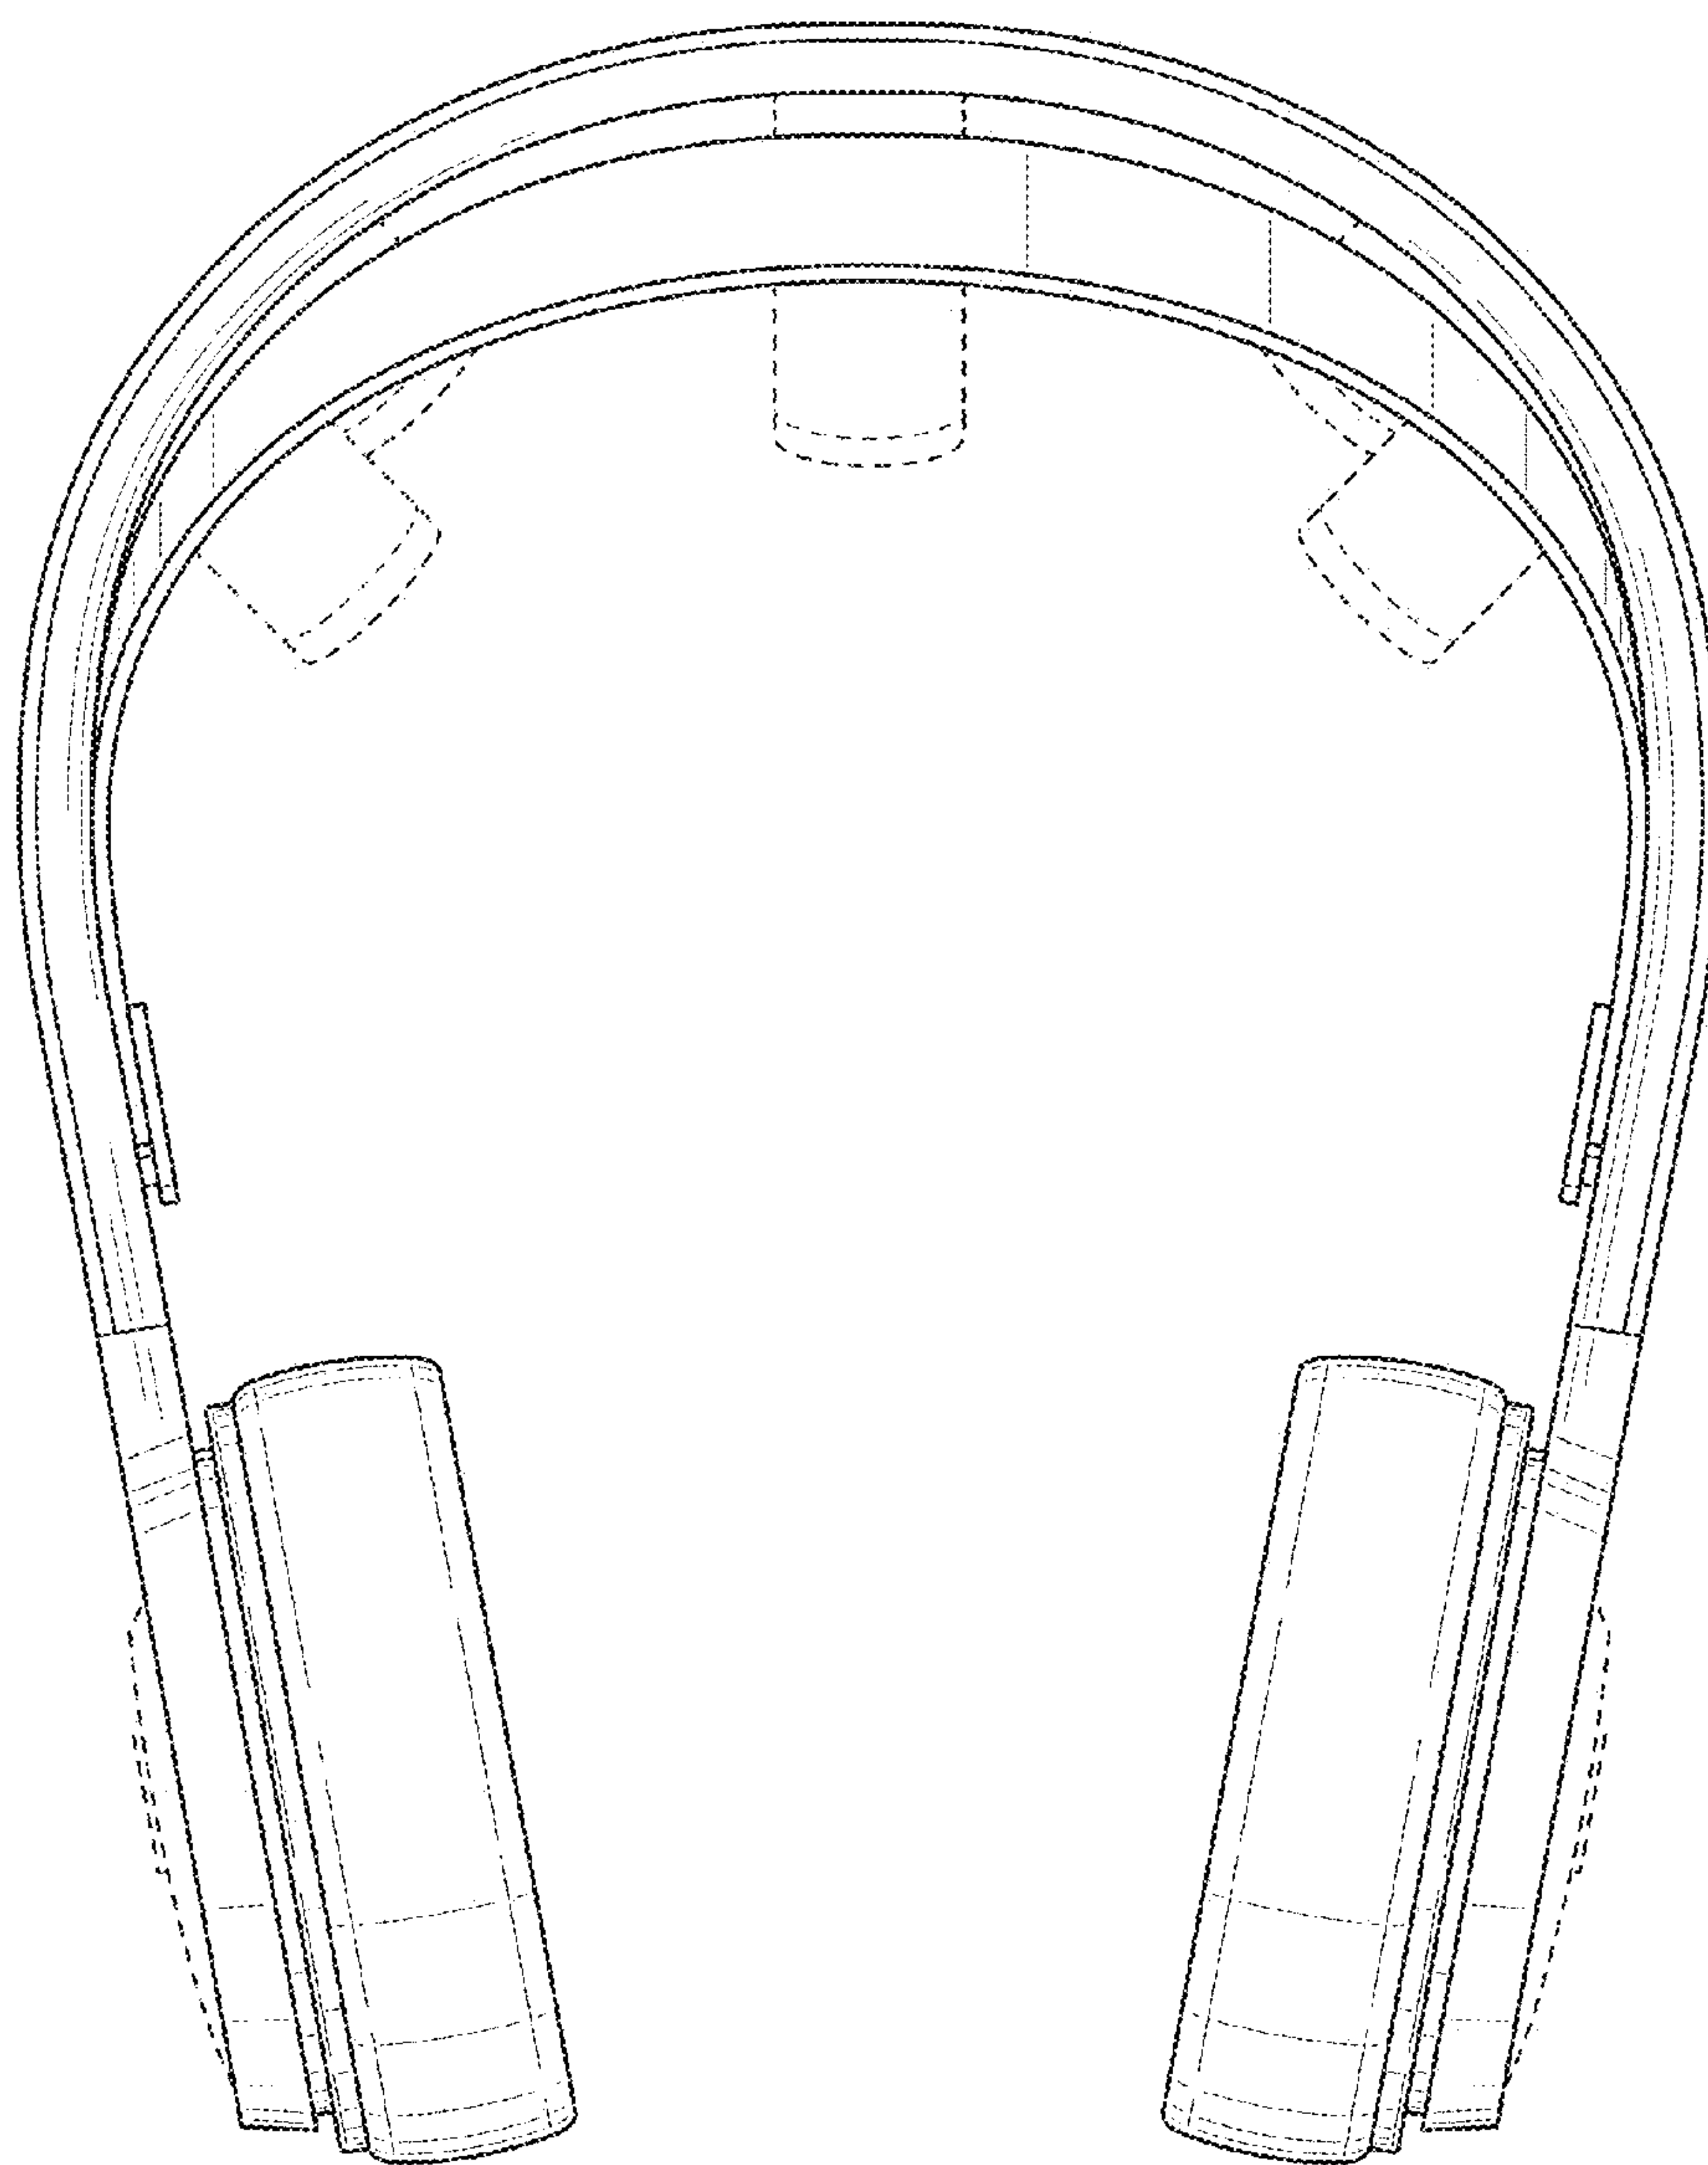


FIG. 2

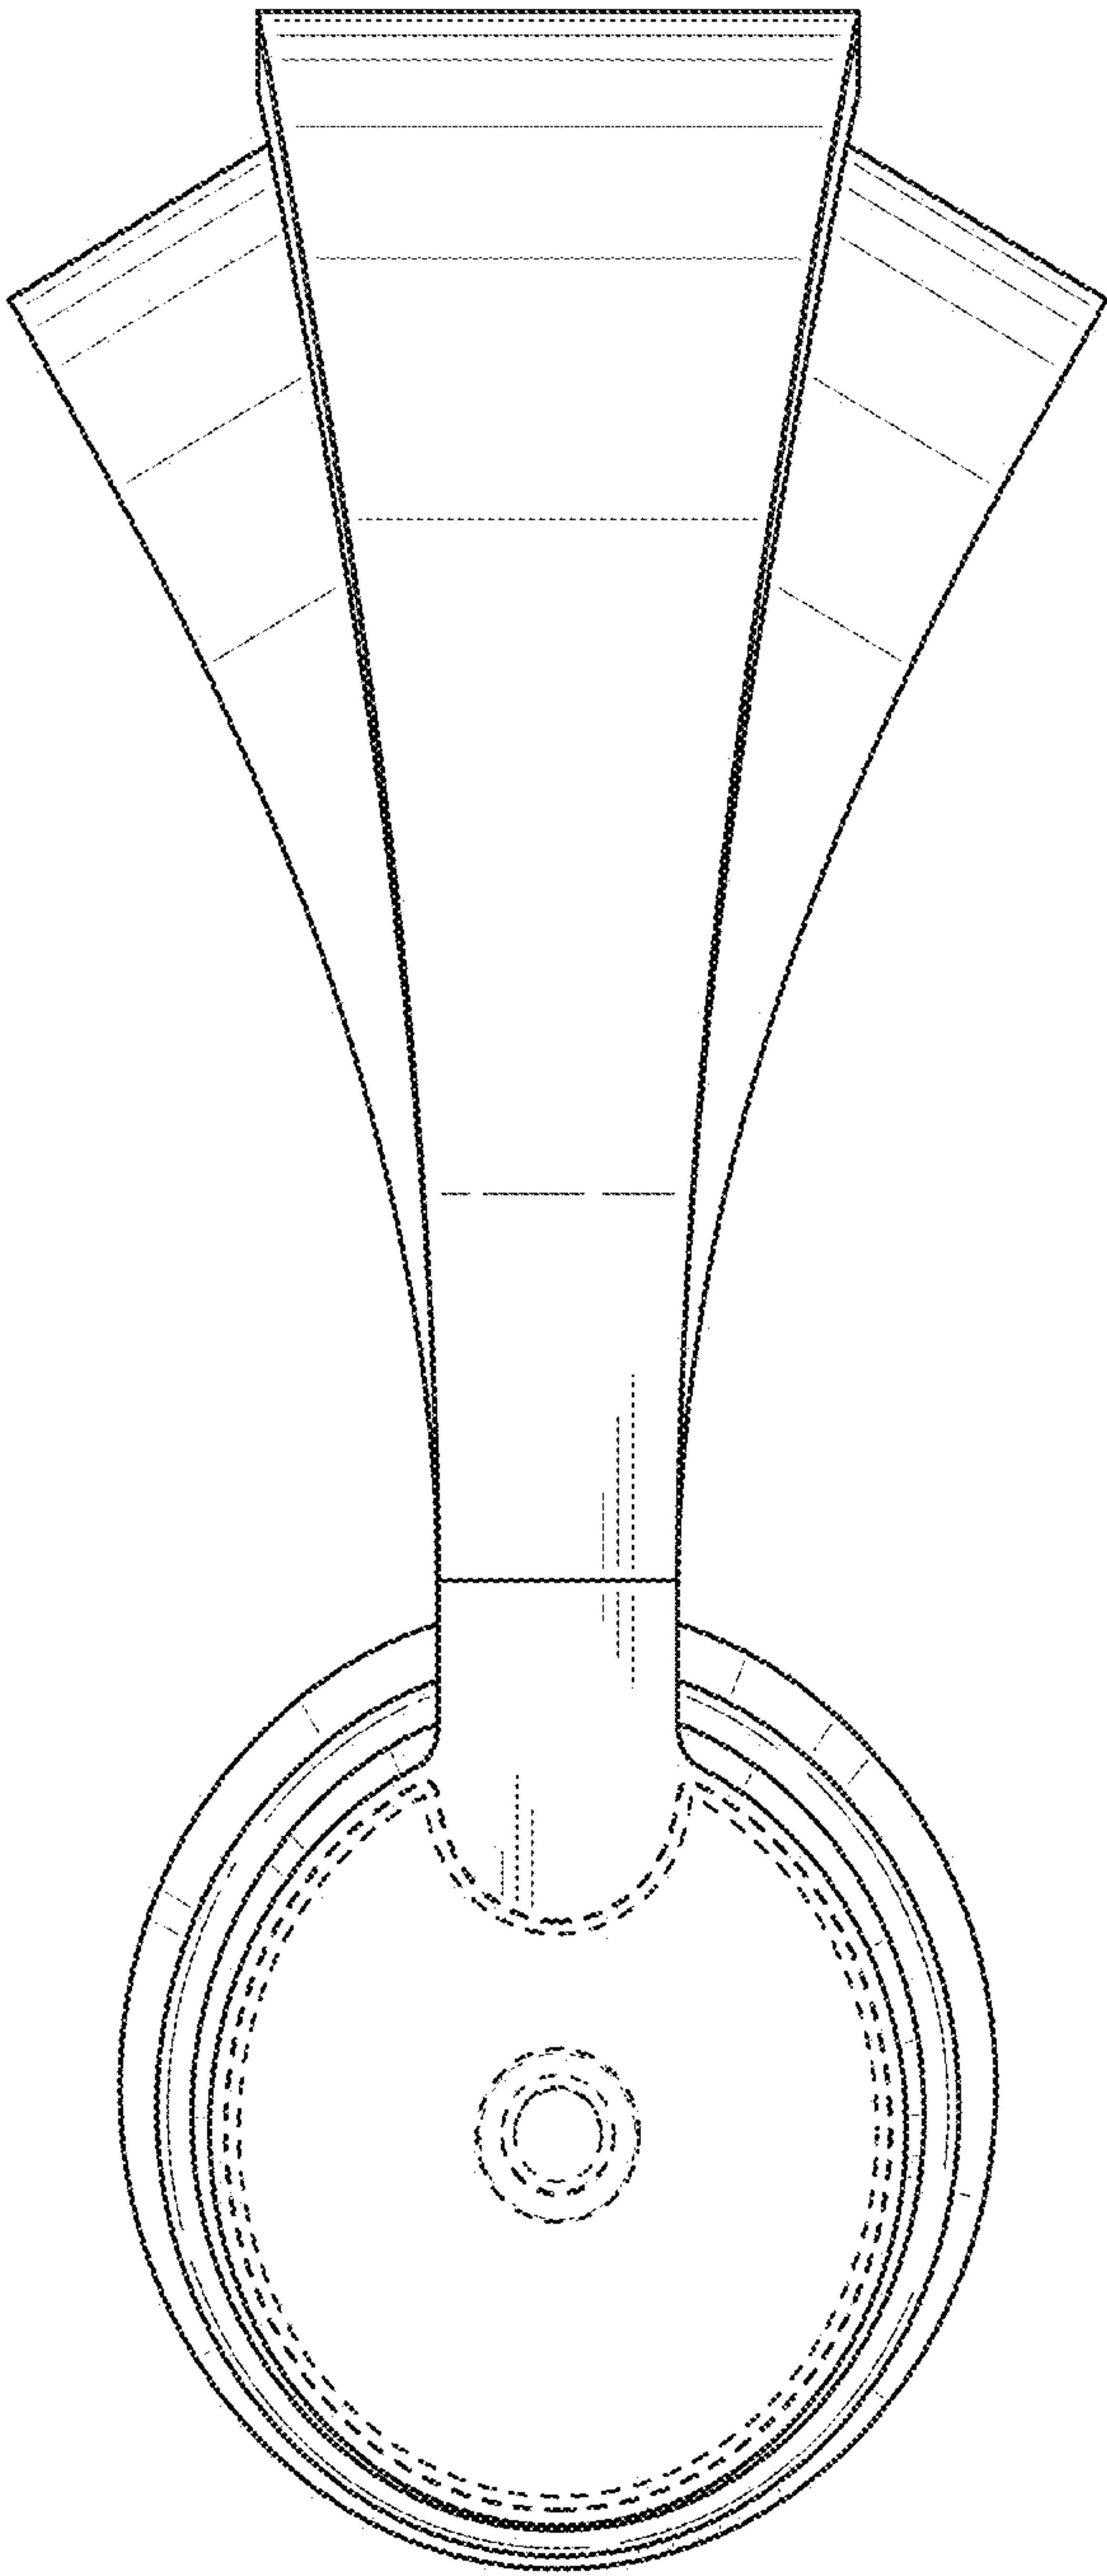


FIG. 3

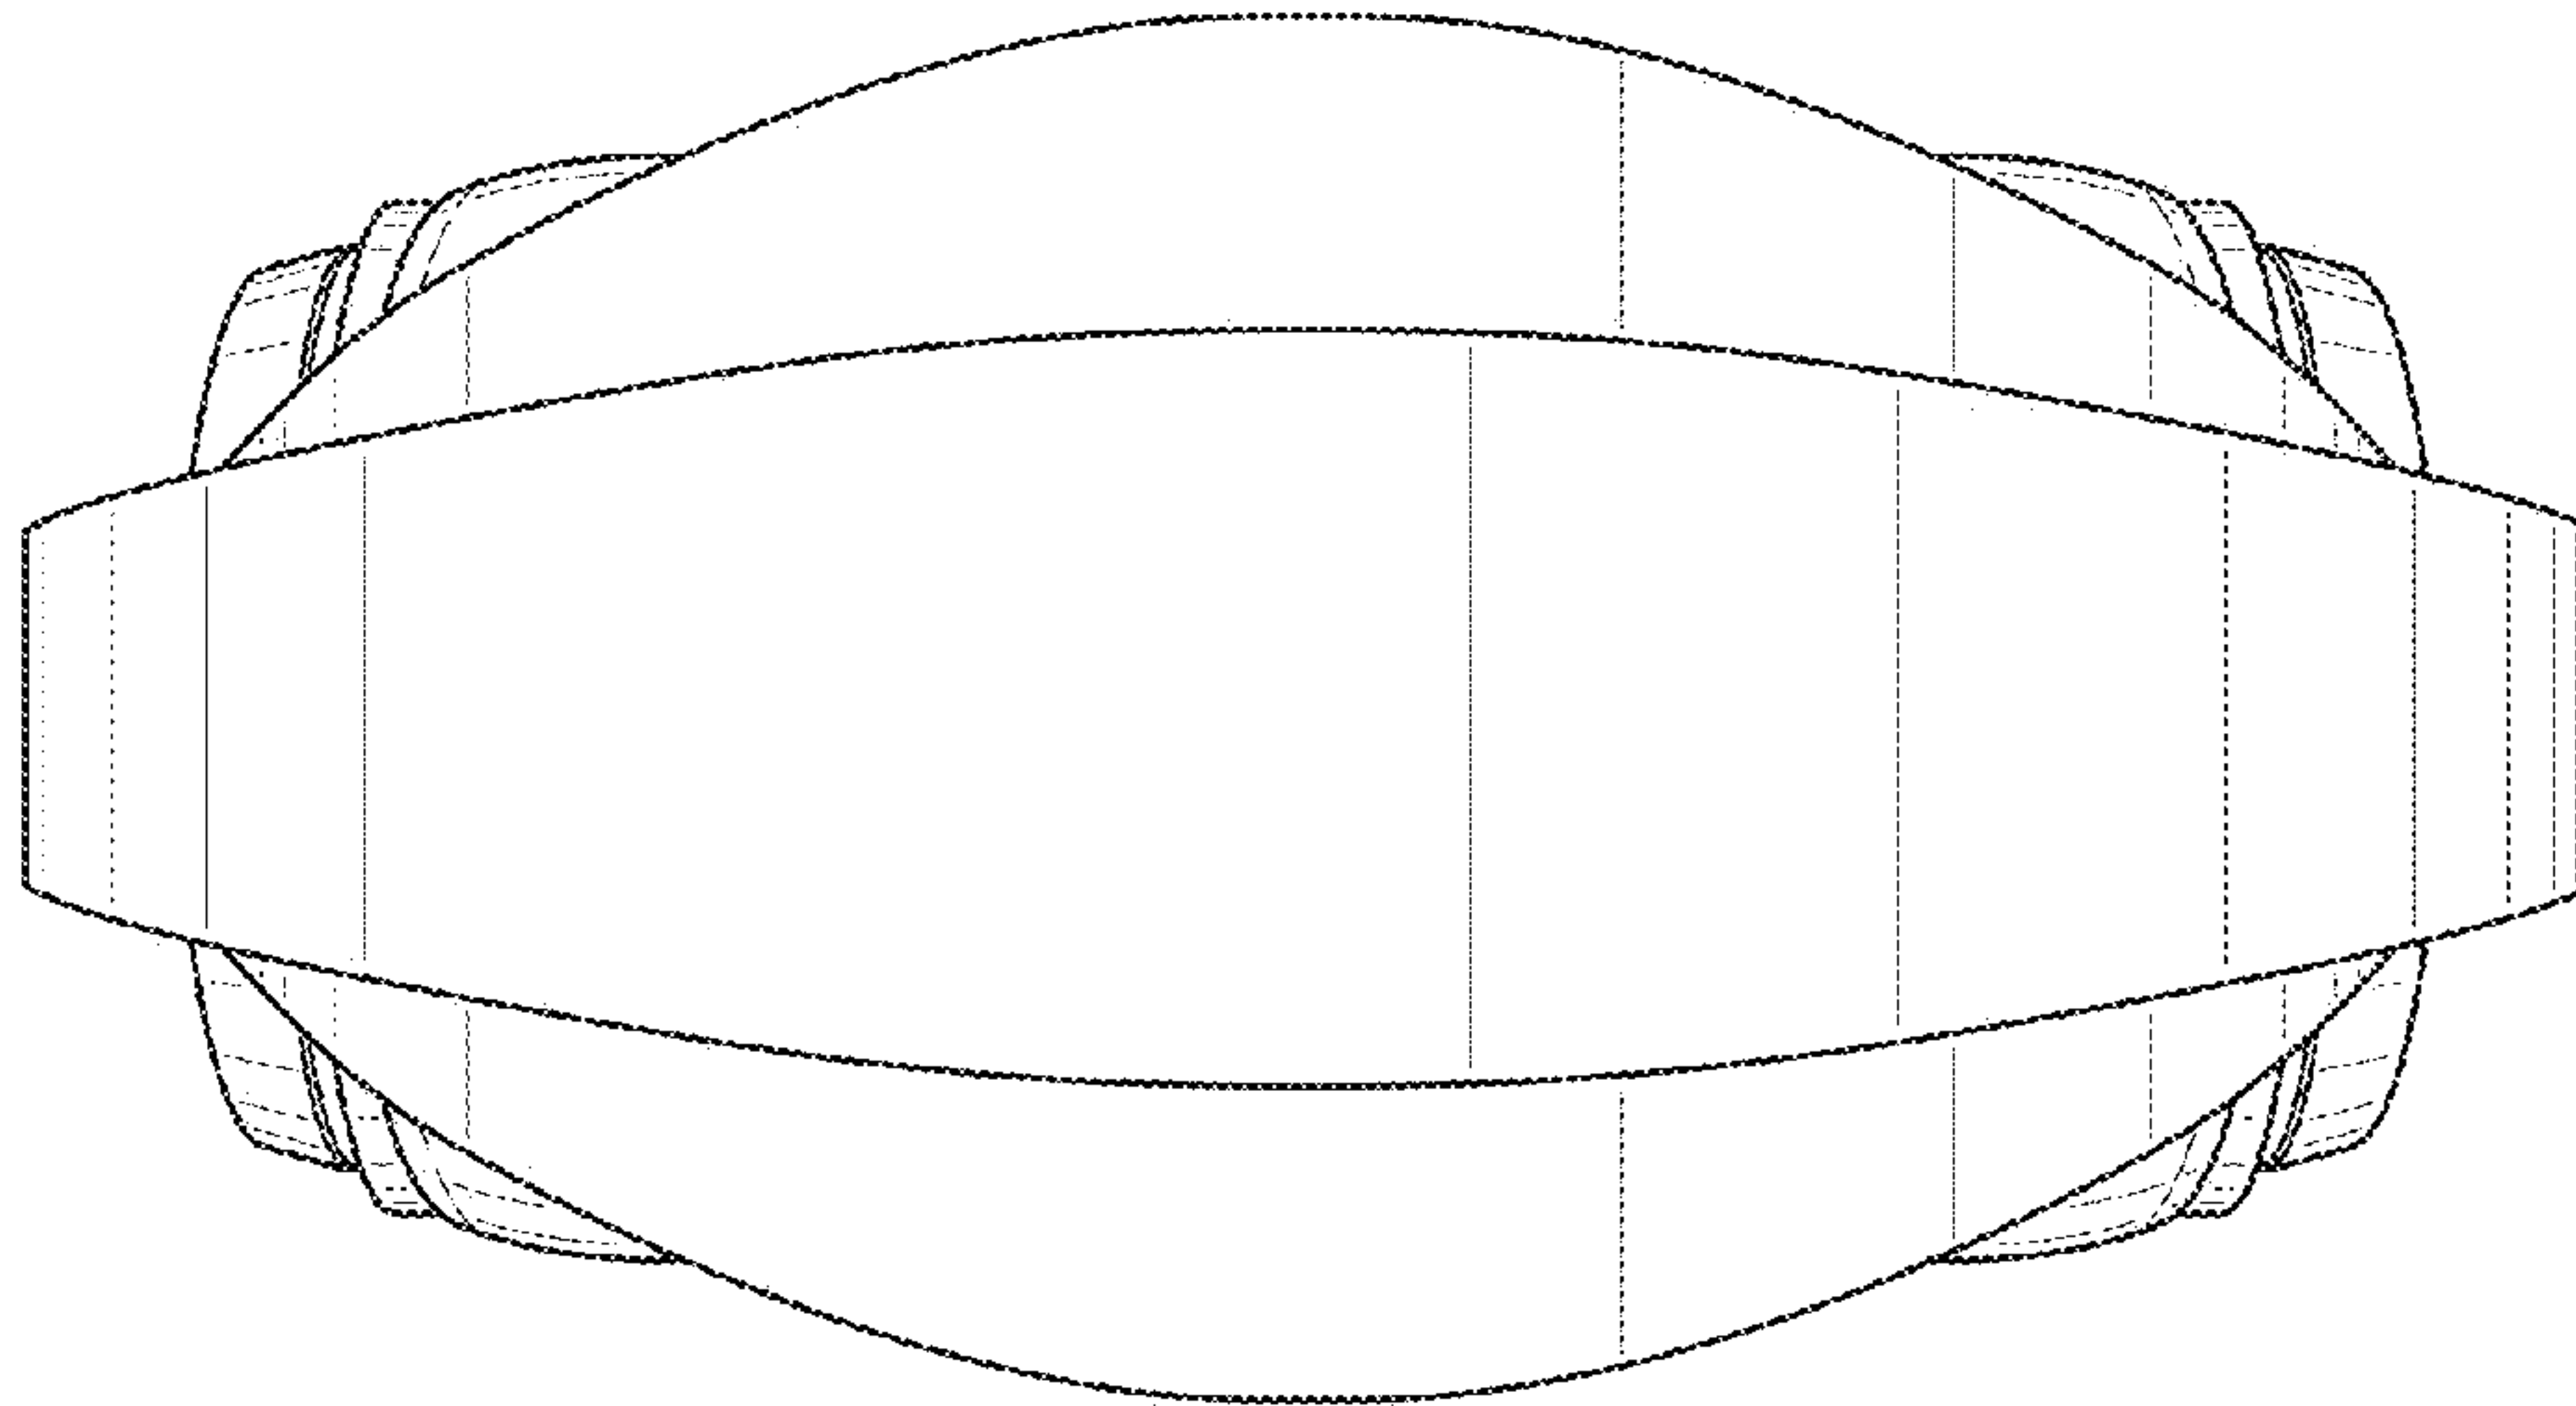


FIG. 4

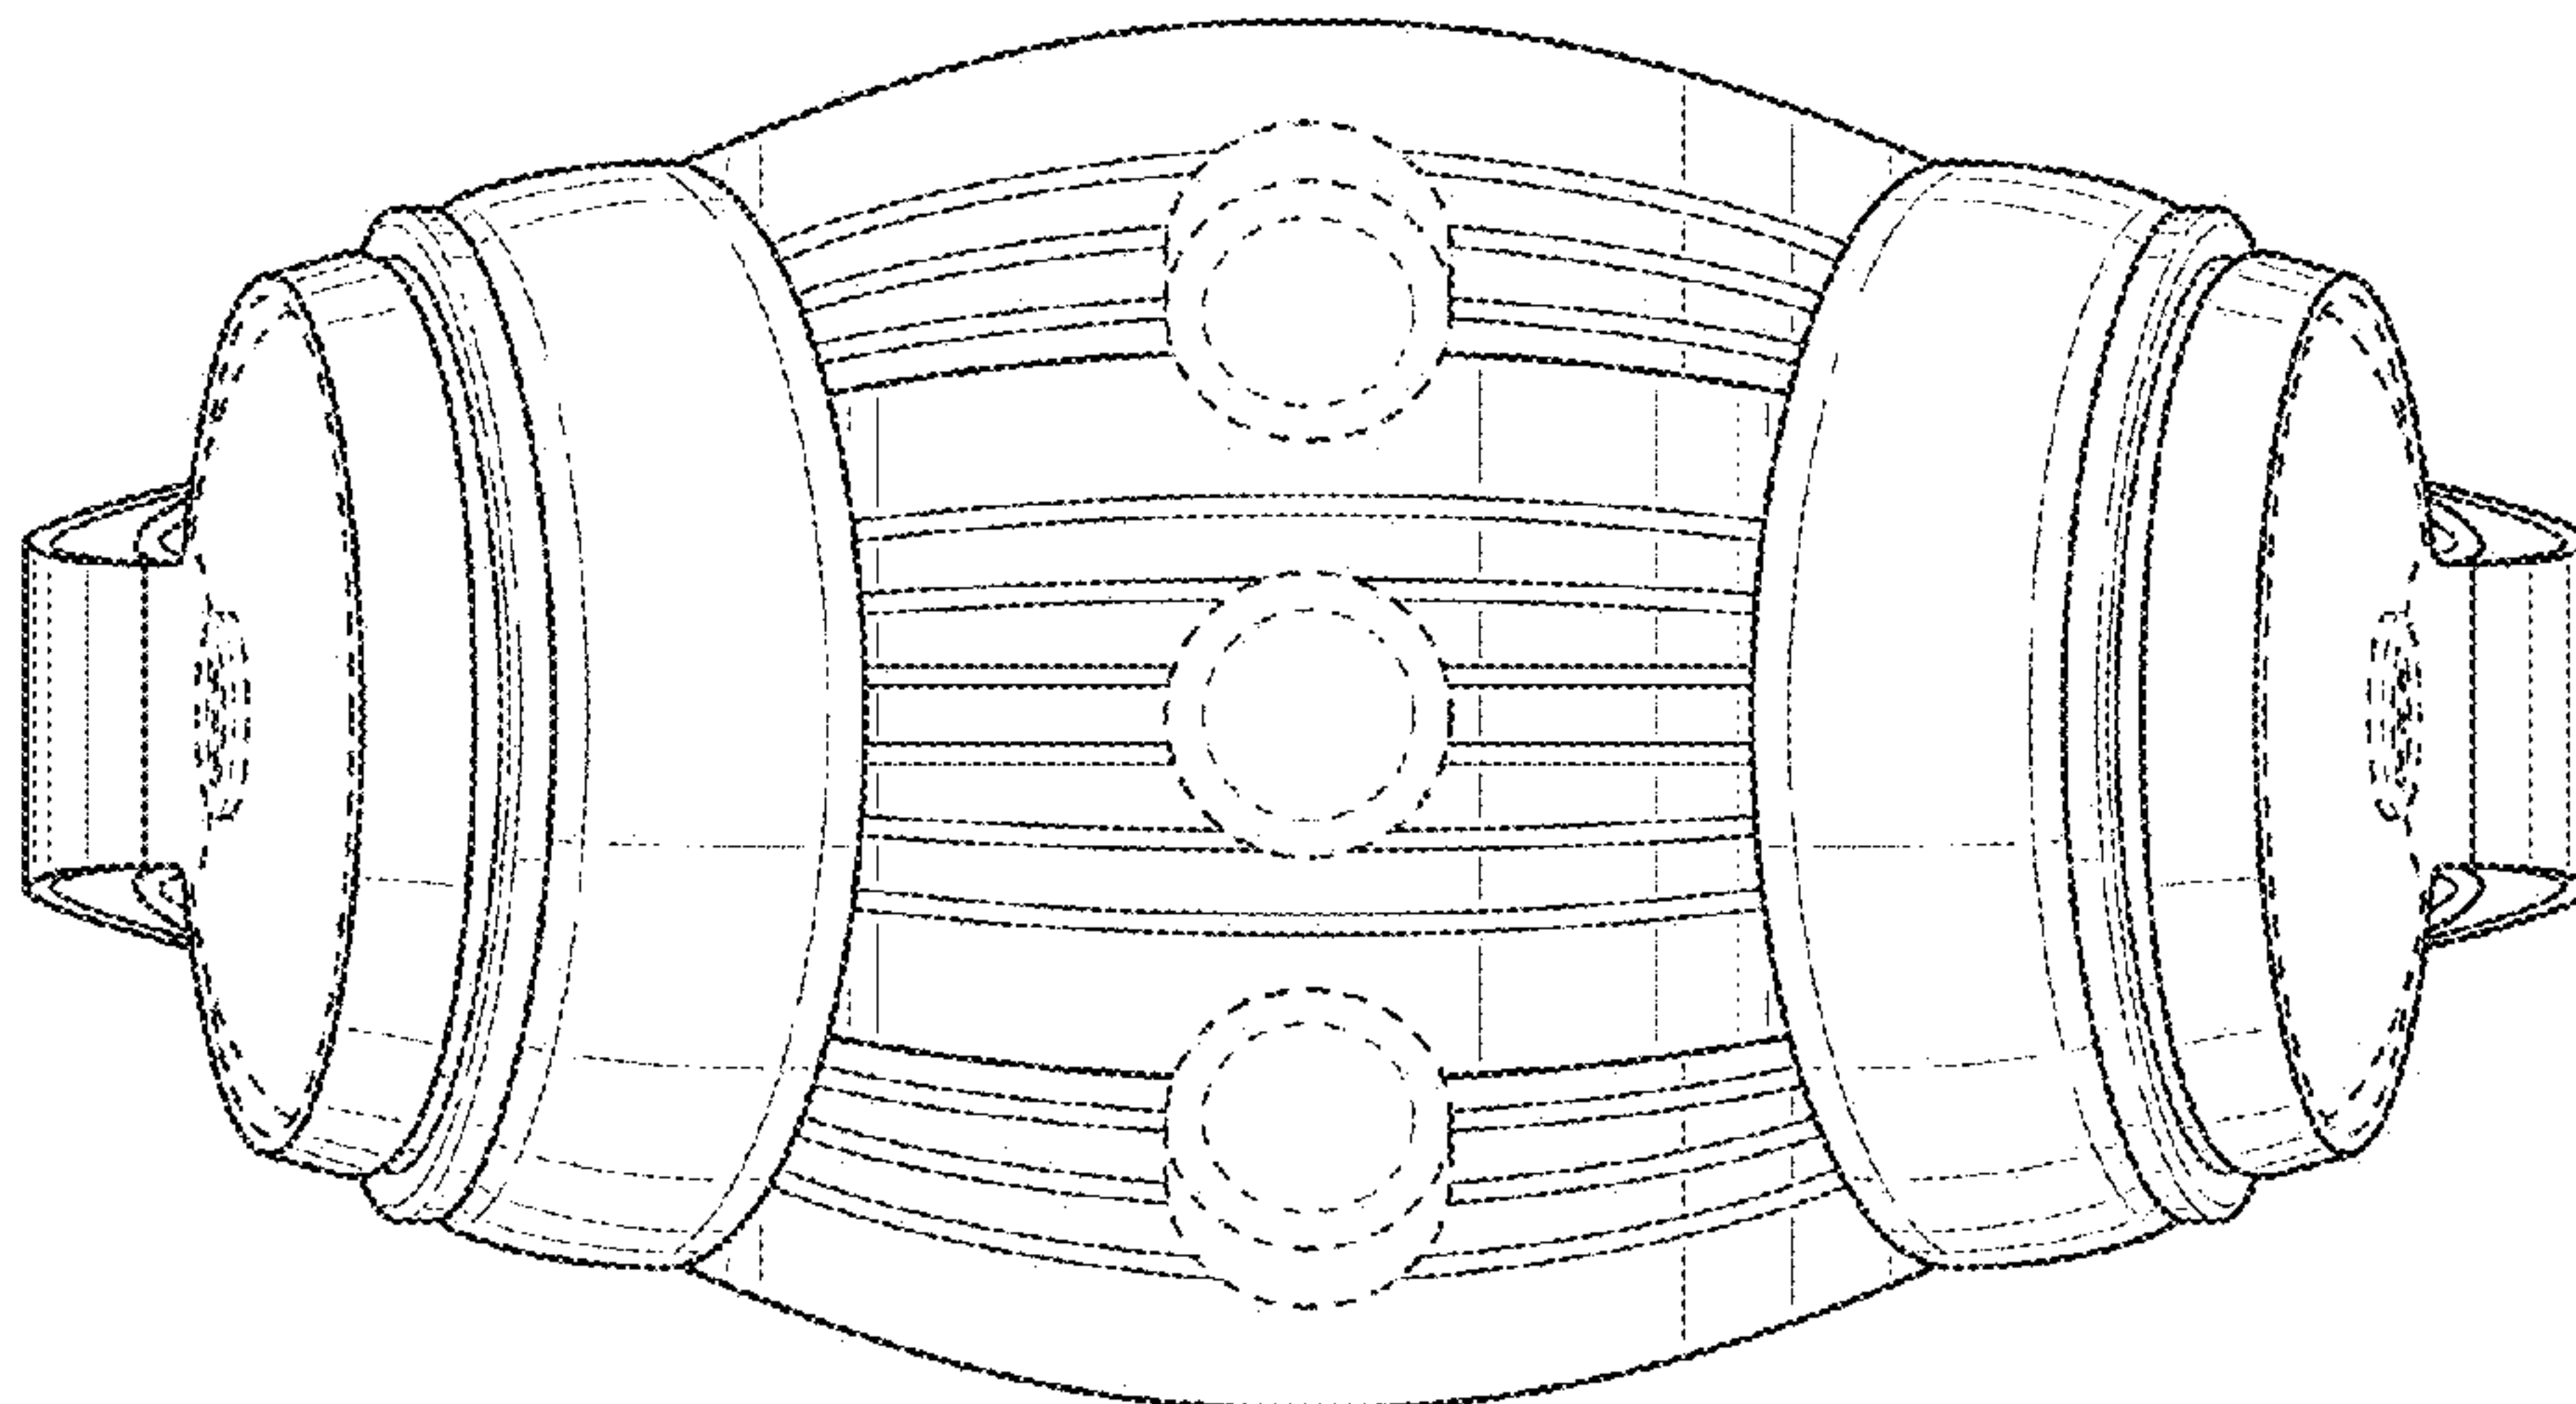


FIG. 5

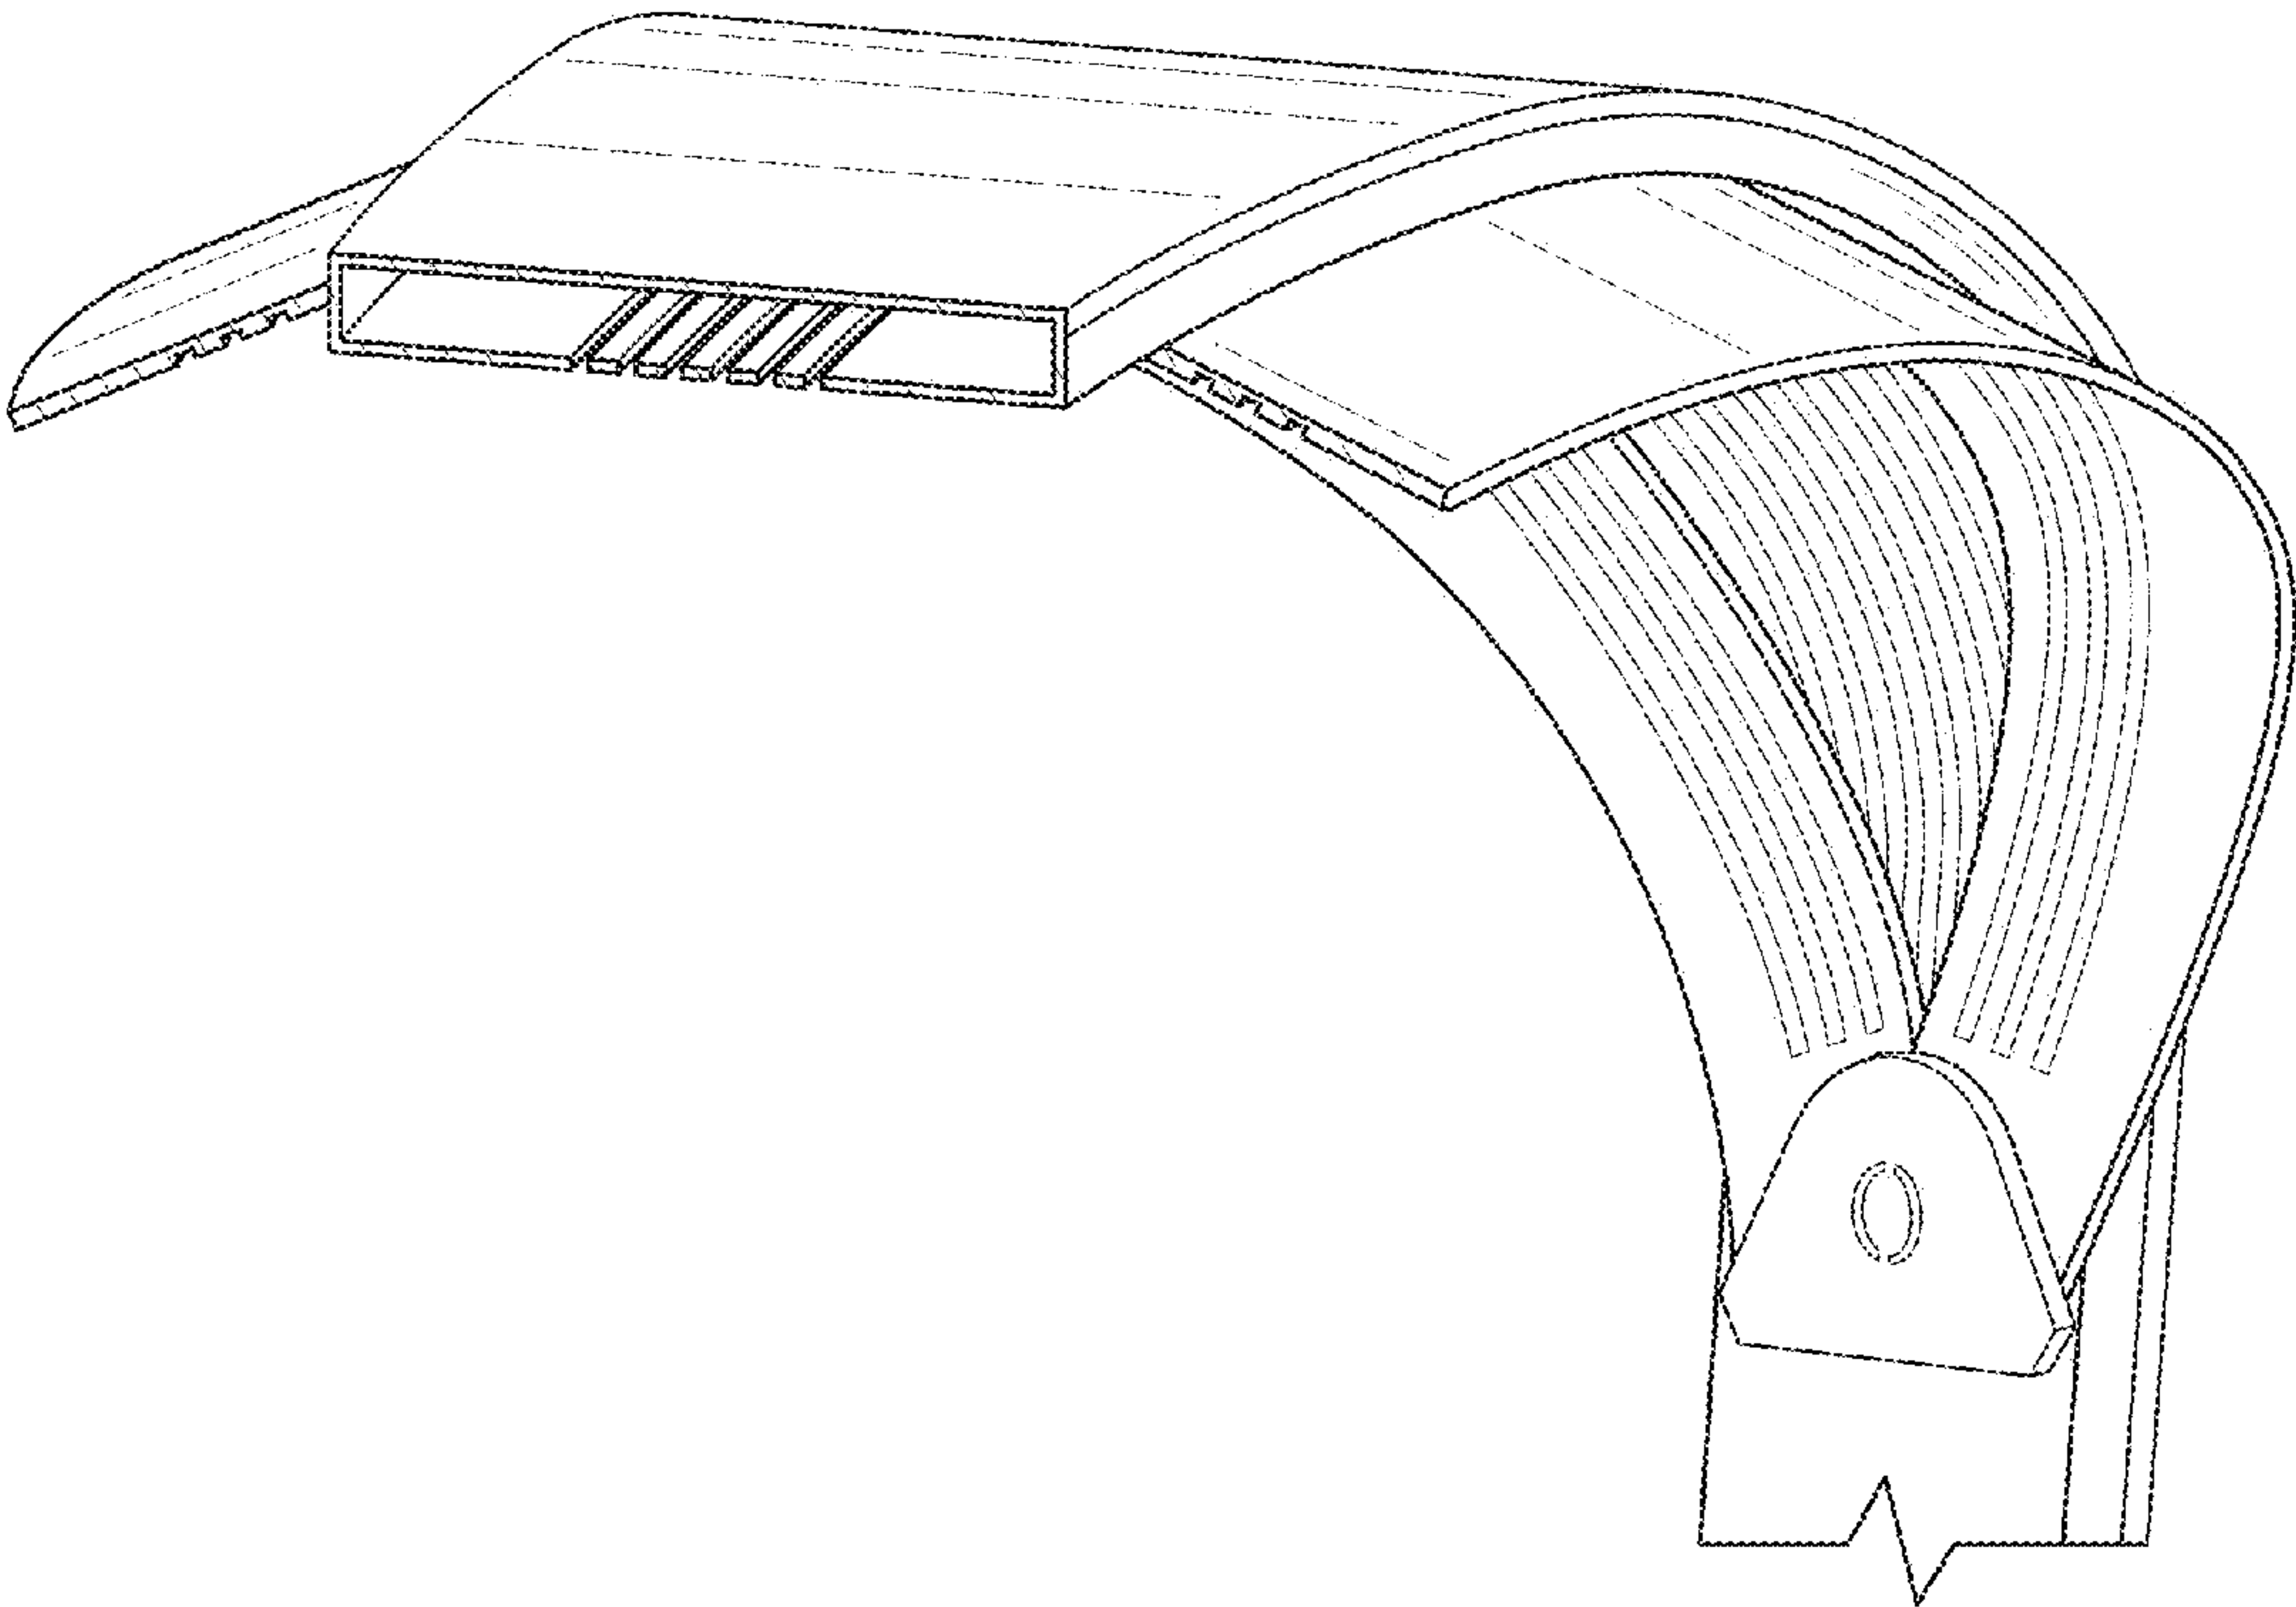


FIG. 6