

US00D744881S

(12)

United States Design Patent

Nothacker et al.

(10)

Patent No.:

US D744,881 S

(45)

Date of Patent:

\*\* Dec. 8, 2015

(54)

BREATHALYZER

(71)

Applicant:

KHN Solutions, Inc., San Francisco, CA (US)

(72)

Inventors:

Keith Harry Nothacker, San Francisco, CA (US); Imraan Aziz, Oakland, CA (US); Michael Jurgen Strasser, San Francisco, CA (US); Pauline Anne Basaran, Corte Madera, CA (US); Stacey Ilene Rettus, Greenbrae, CA (US)

(73)

Assignee:

KHN Solutions, Inc., San Francisco, CA (US)

(\*\*)

Term:

14 Years

435/4, 283.1–284.1, 286.5, 287.1, 435/287.2, 806, 13, 14, 287.4, 287.7, 435/287.94, 6.18; 436/43–54, 68, 900, 514, 436/530, 95; 600/300, 301, 309, 322, 345, 600/347, 365, 393, 578, 583, 584, 532, 600/543; 604/207, 503, 65, 66, 67, 182; 702/19, 40; 221/65, 135; 235/451, 235/422.01; 95/87; 96/101, 106; 366/286, 366/207

CPC

.....

A61B 5/083; A61B 5/087; A61B 5/0833; A61B 5/091; A61B 5/222; A61B 5/0002; A61B 5/02438; A61B 5/08; G01N 33/497; G01N 33/4972; G01N 33/483; G01N 33/98; G10L 17/00; Y10S 436/90

See application file for complete search history.

(21)

Appl. No.:

29/520,160

(22)

Filed:

Mar. 11, 2015

Related U.S. Application Data

(63)

Continuation of application No. 29/501,849, filed on Sep. 9, 2014, now Pat. No. Des. 727,764.

(51)

LOC (10) Cl.

10-04

(52)

U.S. Cl.

USPC D10/81

(58)

Field of Classification Search

USPC D10/78, 81; D24/216, 232–234; 73/1.01, 1.02–1.08, 1.16, 19.01–19.02, 73/23.2–23.27, 23.3, 23.35–24.01, 52, 73/53.01, 61.52–61.61, 864.21, 431, 73/864.73, 31.03, 31.05, 866.5, 864.84, 73/864.23, 61.55, 863.01, 866, 864.62; 204/253, 400, 403.01, 403.02, 403.04, 204/403.05, 403.1, 403.11, 403.14; 205/775, 777.5, 778, 792; 210/656–660, 198.2, 635, 101, 103; 250/252.1, 251, 25, 281–300, 305, 250/336.1, 338.1, 338.5, 339.07, 339.13, 250/343, 349, 239, 910; 356/446, 246, 356/301–337, 451, 72, 73; 422/50–53, 422/62–82, 83–98, 239.2, 400, 401, 404;

(56)

References Cited

U.S. PATENT DOCUMENTS

4,487,055 A 12/1984 Wolf

4,749,553 A 6/1988 Lopez et al.

4,996,161 A 2/1991 Conners et al.

D333,441 S 2/1993 Greene

5,216,415 A \* 6/1993 Ono et al. 345/94

5,291,898 A \* 3/1994 Wolf 600/532

D362,642 S 9/1995 Howse

D381,885 S 8/1997 Lane

6,454,723 B1 9/2002 Montagnino

6,608,399 B2 8/2003 McConnell et al.

6,824,520 B2 11/2004 Orr et al.

6,899,683 B2 5/2005 Mault et al.

D521,885 S 5/2006 Eddy et al.

D530,424 S 10/2006 Manser et al.

D539,683 S \* 4/2007 Shaw et al. D10/81

D539,684 S 4/2007 Kitamura et al.

D586,677 S \* 2/2009 Nothacker et al. D10/78

D603,281 S 11/2009 Gonzalez

D606,434 S 12/2009 Castrodale et al.

8,040,233 B2 10/2011 Adappa et al.

8,453,492 B2 6/2013 Tsuzuki et al.

8,693,597 B2 \* 4/2014 Sexton et al. 375/346

D705,100 S 5/2014 Nothacker et al.

8,808,228 B2 \* 8/2014 Brister et al. 604/66

8,814,804 B2 8/2014 Walden et al.


8,849,387 B2 \* 9/2014 Gilbert et al. 600/520

8,941,501 B1 \* 1/2015 Debijl 340/576

D724,980 S \* 3/2015 Nothacker et al. D10/81

D727,763 S \* 4/2015 Nothacker et al. D10/81

D727,764 S \* 4/2015 Nothacker et al. D10/81

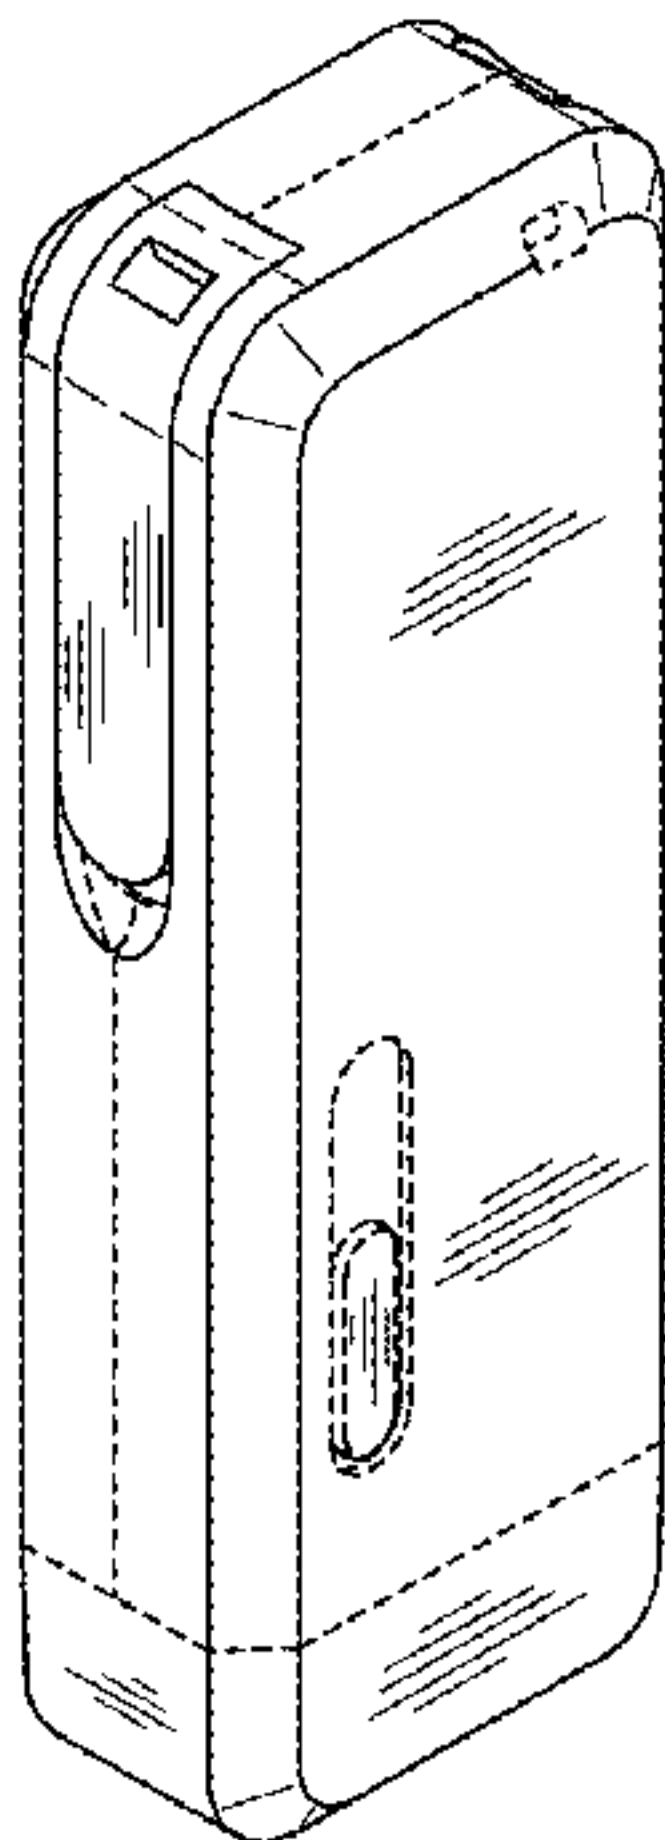



|                 |         |                  |        |
|-----------------|---------|------------------|--------|
| D731,341 S *    | 6/2015  | Kobayakawa ..... | D10/81 |
| 9,063,120 B2 *  | 6/2015  | Park .....       | 1/1    |
| 2006/0217625 A1 | 9/2006  | Forrester        |        |
| 2007/0093725 A1 | 4/2007  | Shaw             |        |
| 2007/0144812 A1 | 6/2007  | Stewart et al.   |        |
| 2010/0234064 A1 | 9/2010  | Harris           |        |
| 2011/0304465 A1 | 12/2011 | Boult et al.     |        |
| 2013/0021153 A1 | 1/2013  | Keays            |        |

\* cited by examiner

Primary Examiner — Antoine D Davis  
(74) Attorney, Agent, or Firm — Jeffrey Schox; Ivan Wong

(57) **CLAIM**  
We claim the ornamental design for a breathalyzer, as shown and described.

**DESCRIPTION**

FIG. 1 is an isometric view, from the front right, of the breathalyzer in a first configuration;  
FIG. 2 is an isometric view, from the back left, of the breathalyzer in the first configuration;  
FIG. 3 is a plan view of the top of the breathalyzer the first configuration;  
FIG. 4 is an elevation view of the right side of the breathalyzer the first configuration;

FIG. 5 is an elevation view of the back of the breathalyzer the first configuration;  
FIG. 6 is an elevation view of the left side of the breathalyzer the first configuration;  
FIG. 7 is an elevation view of the front of the breathalyzer the first configuration;  
FIG. 8 is a plan view of the bottom of the breathalyzer the first configuration;  
FIG. 9 is an isometric view, from the front right, of the breathalyzer in a second configuration;  
FIG. 10 is an isometric view, from the back left, of the breathalyzer in the second configuration;  
FIG. 11 is a plan view of the top of the breathalyzer in the second configuration;  
FIG. 12 is an elevation view of the right side of the breathalyzer in the second configuration;  
FIG. 13 is an elevation view of the back of the breathalyzer in the second configuration;  
FIG. 14 is an elevation view of the left side of the breathalyzer in the second configuration;  
FIG. 15 is an elevation view of the front of the breathalyzer in the second configuration; and,  
FIG. 16 is a plan view of the bottom of the breathalyzer in the second configuration.

**1 Claim, 6 Drawing Sheets**



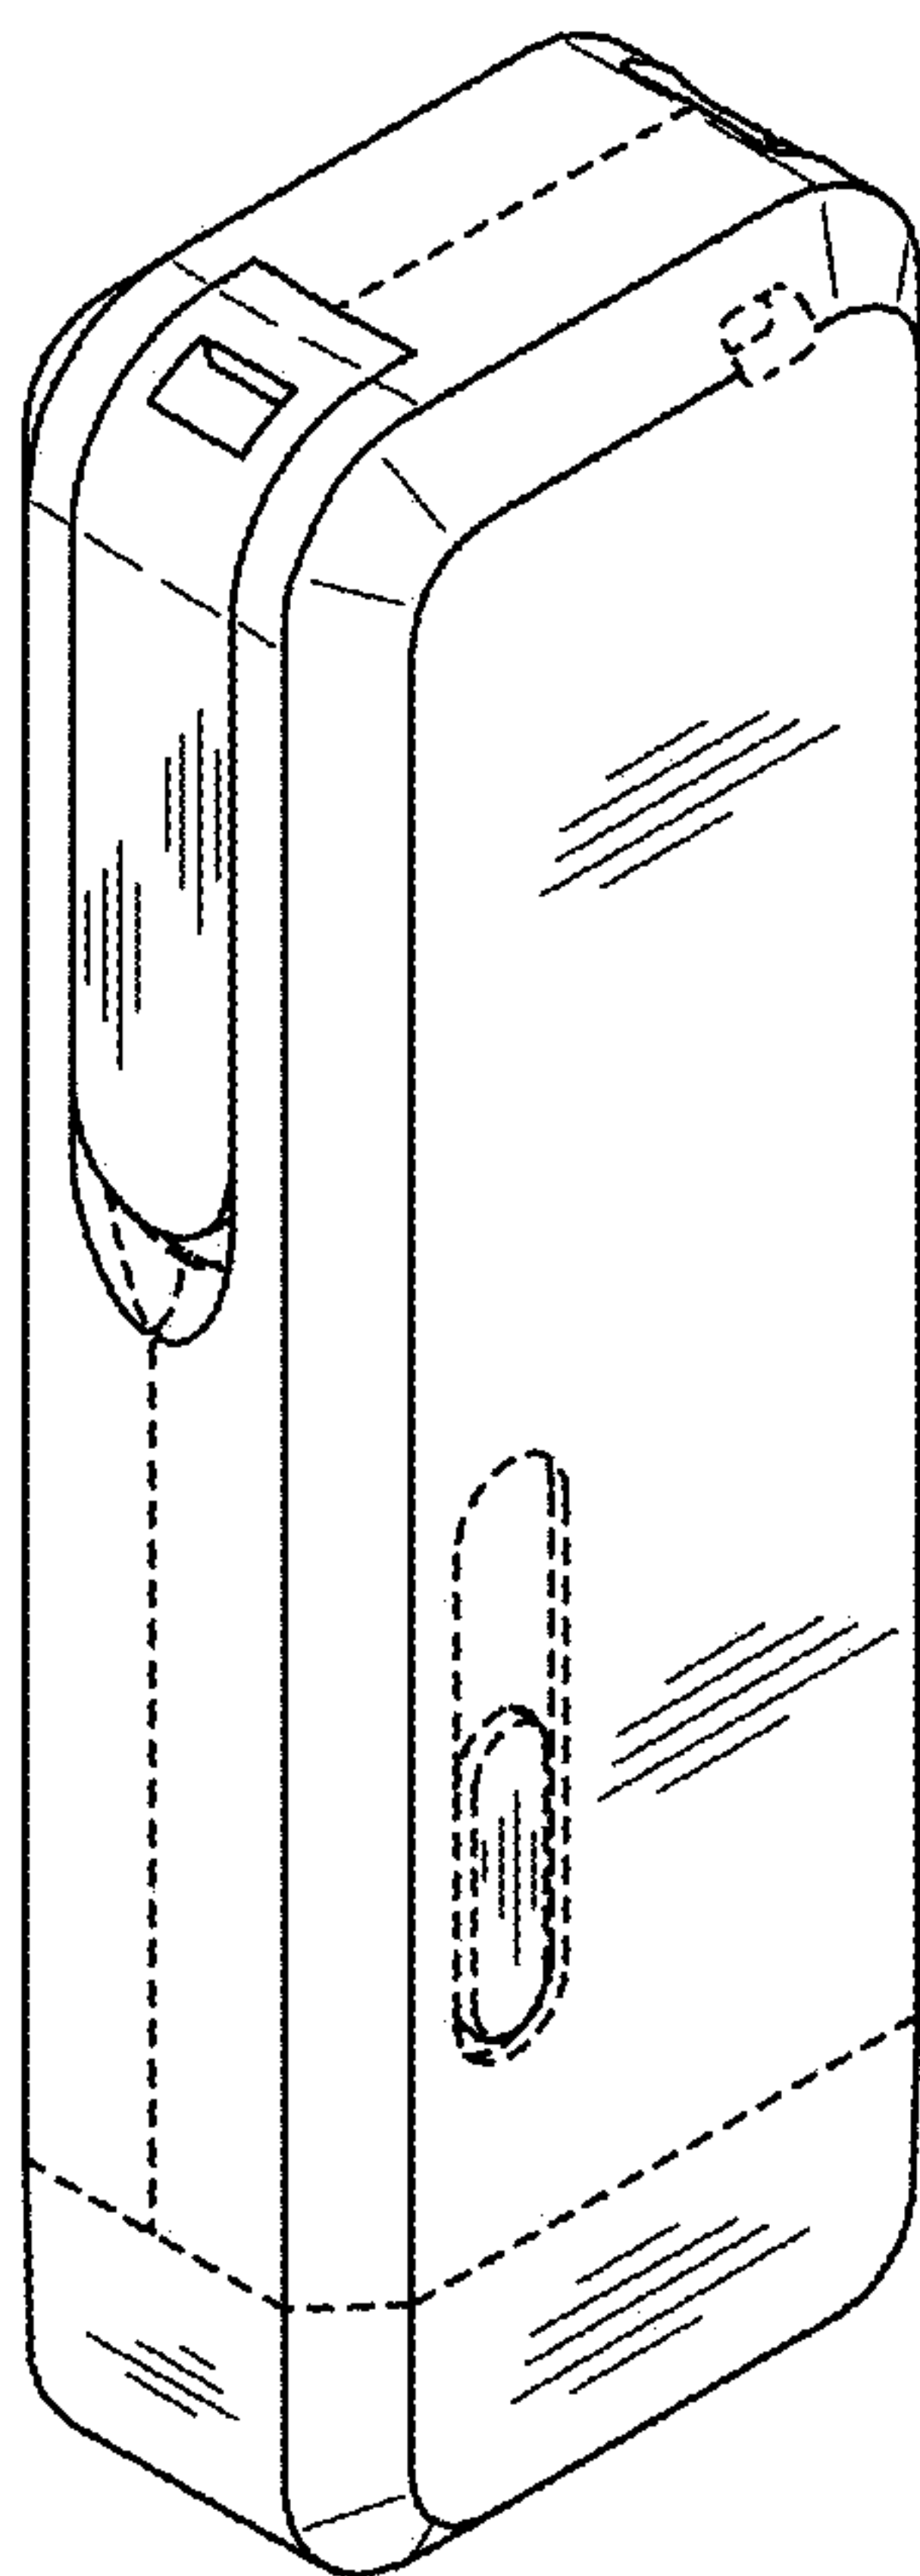


FIG. 1

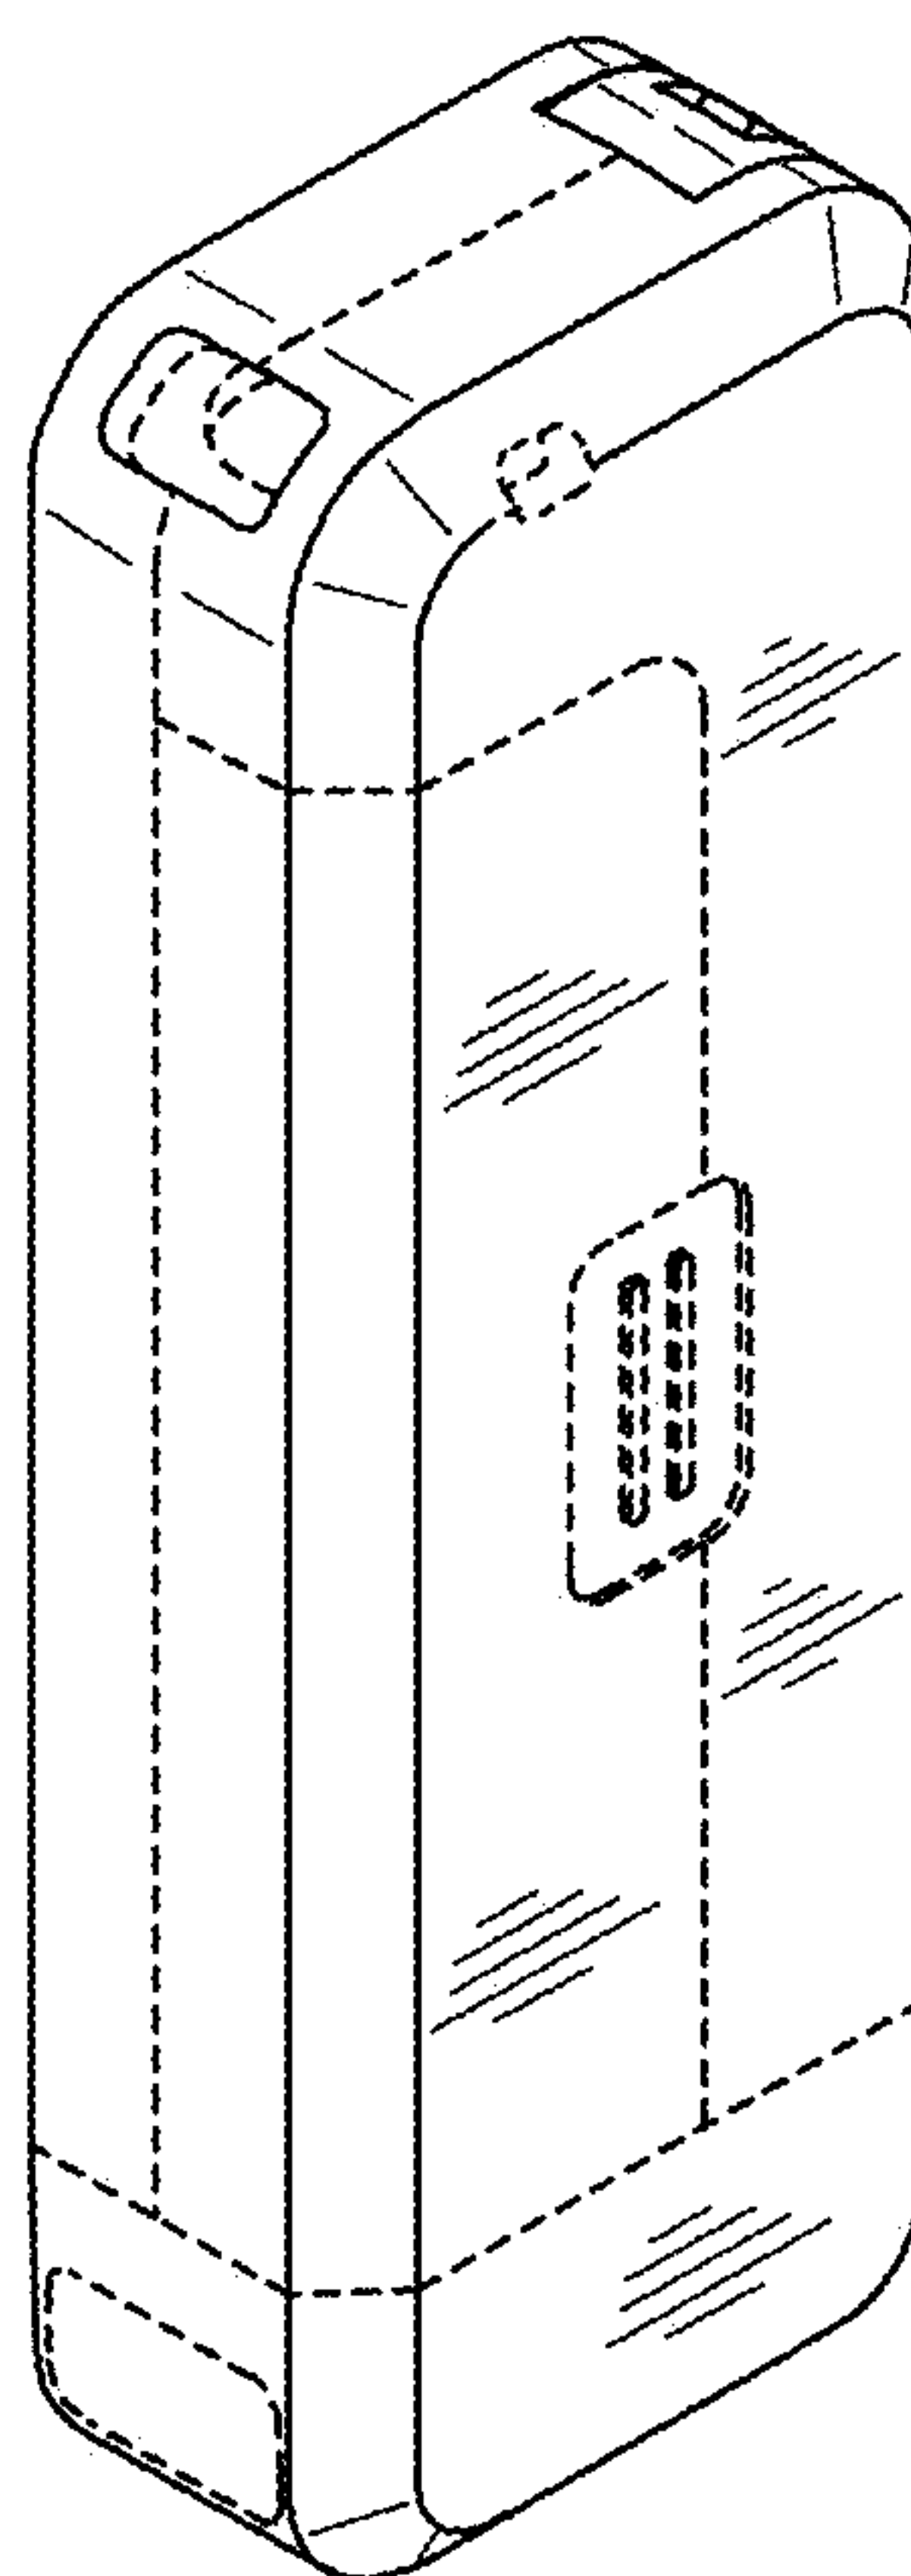


FIG. 2



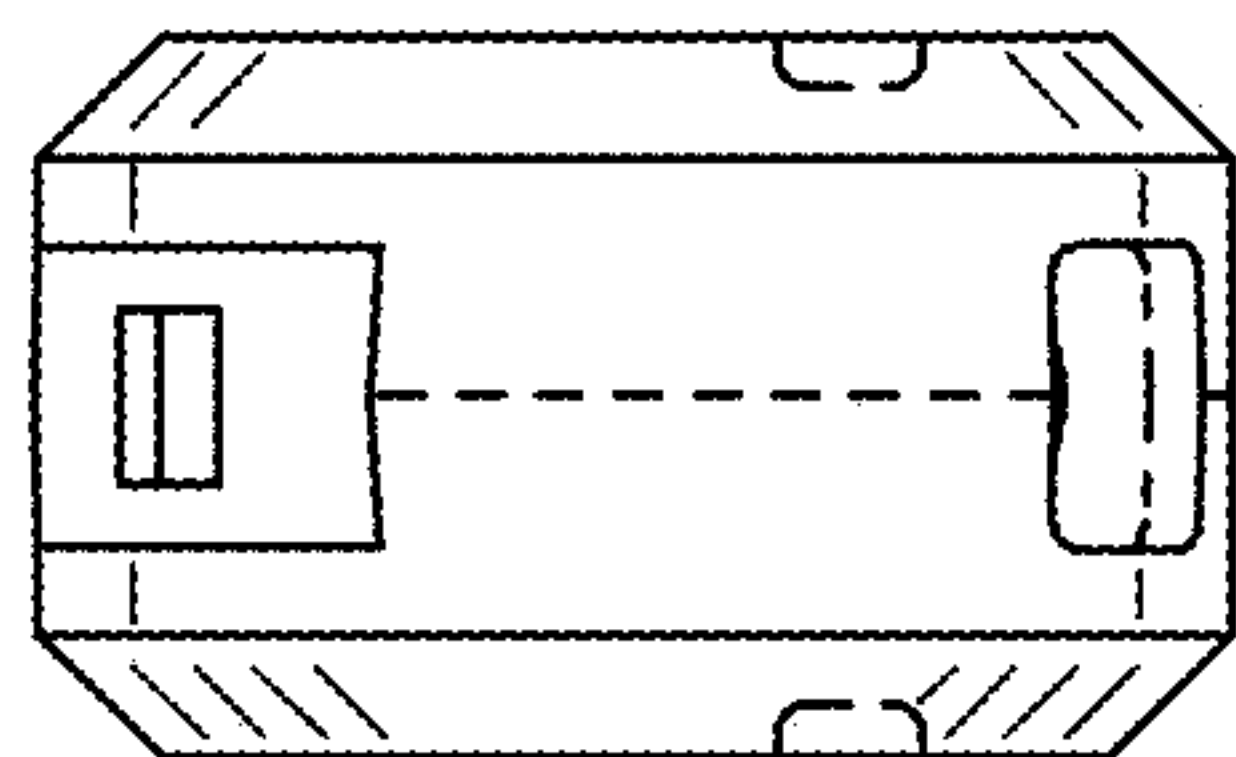


FIG. 3

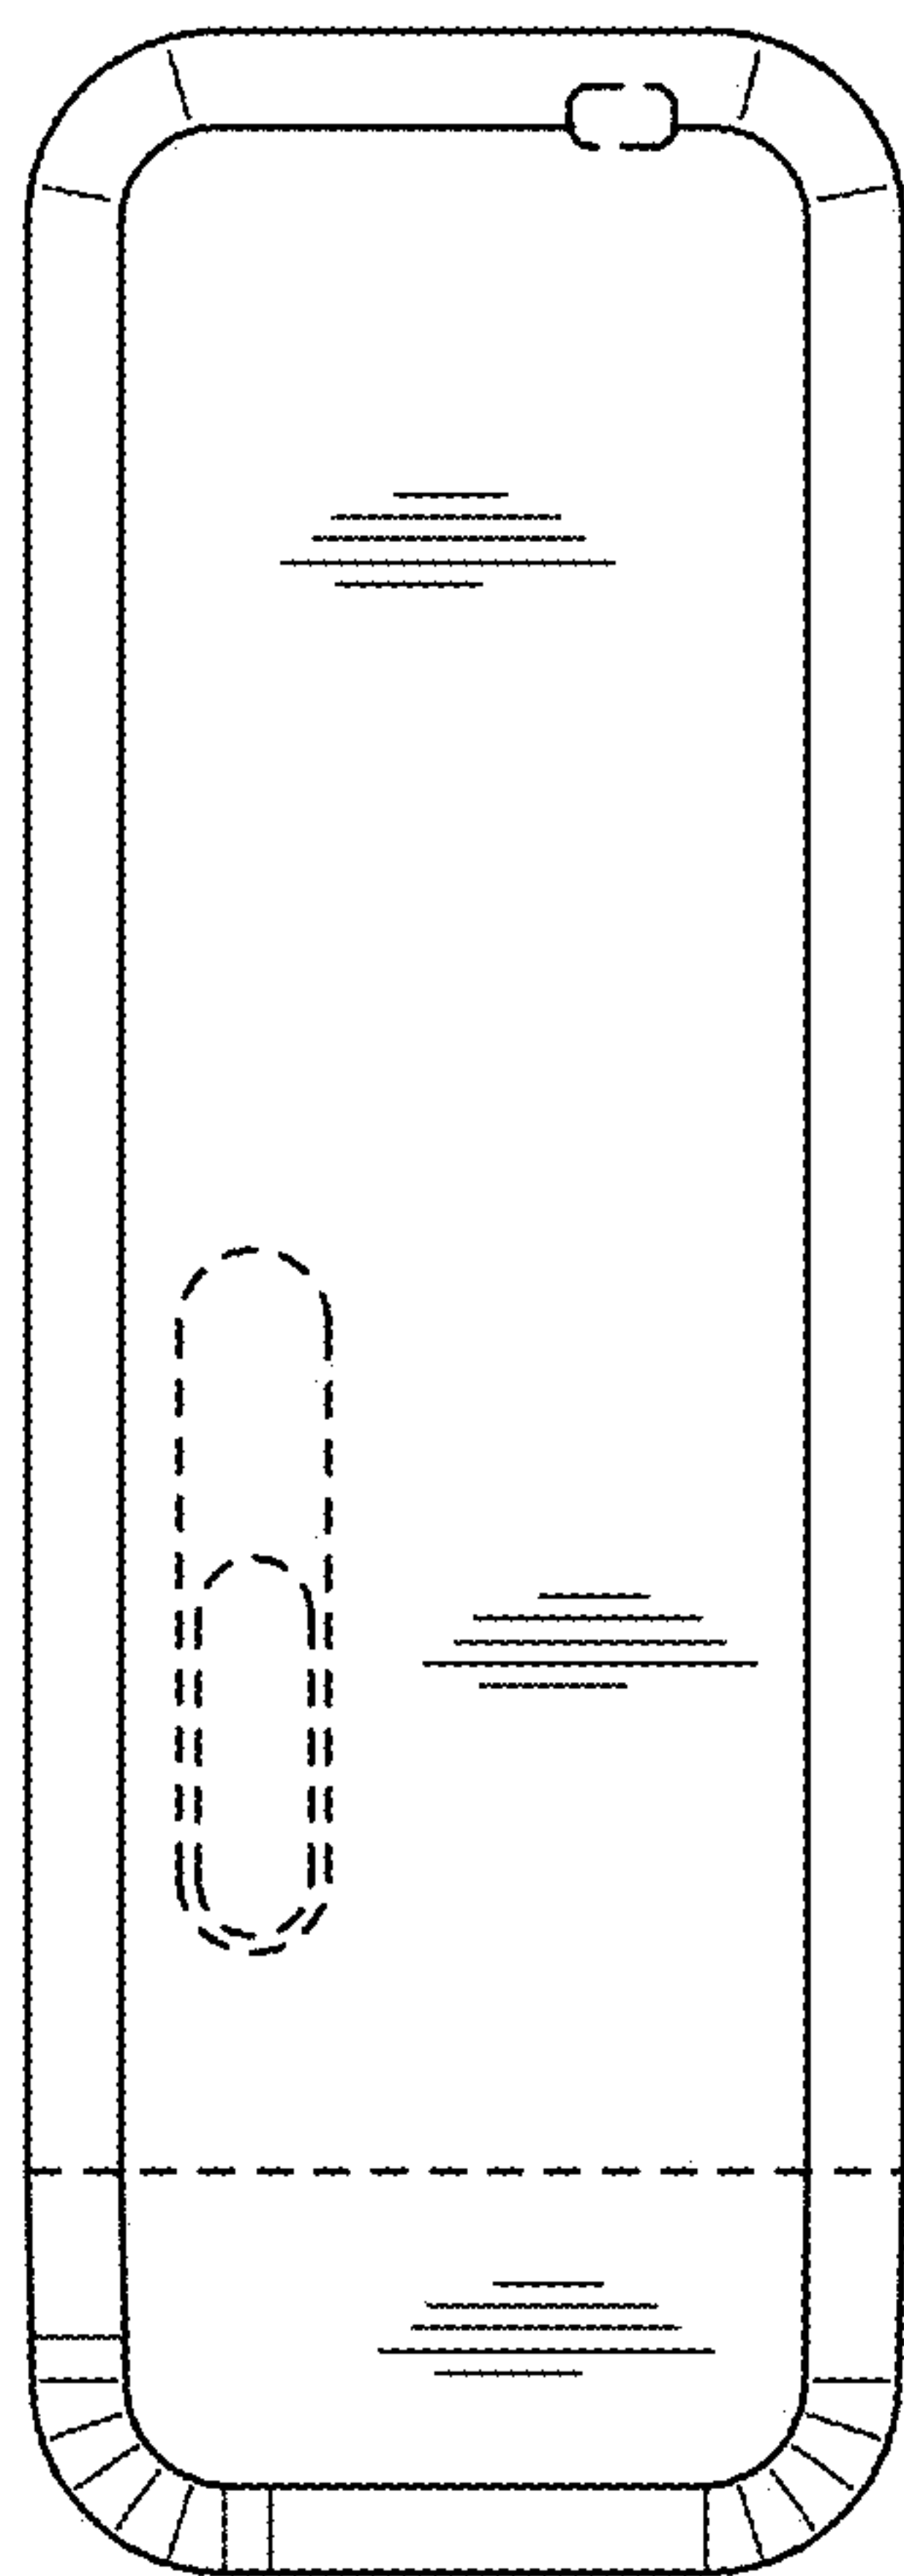


FIG. 4

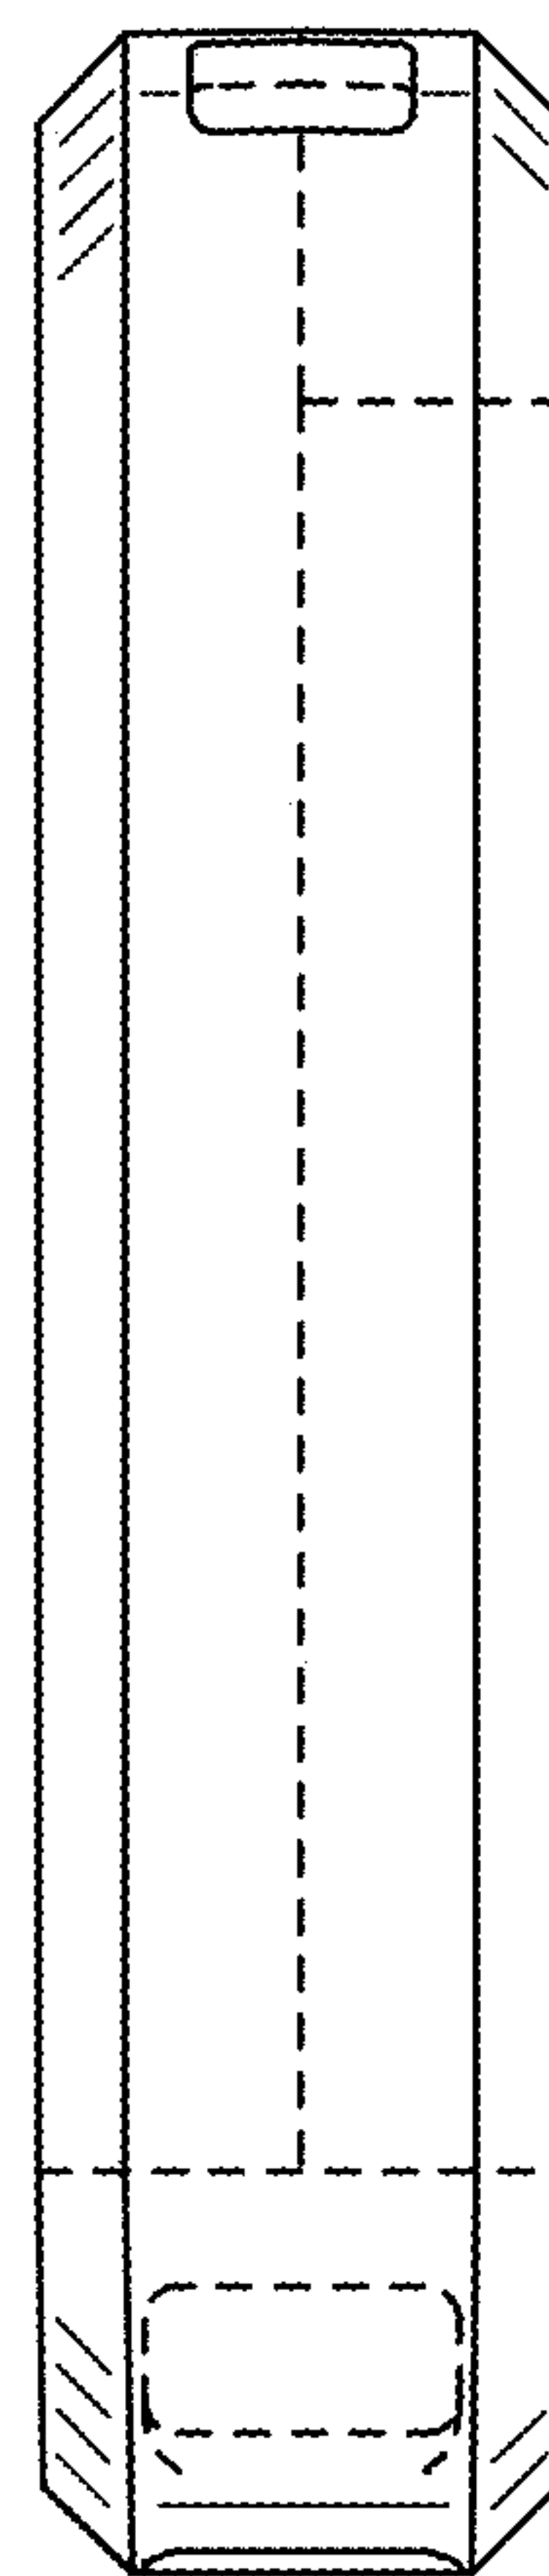


FIG. 5



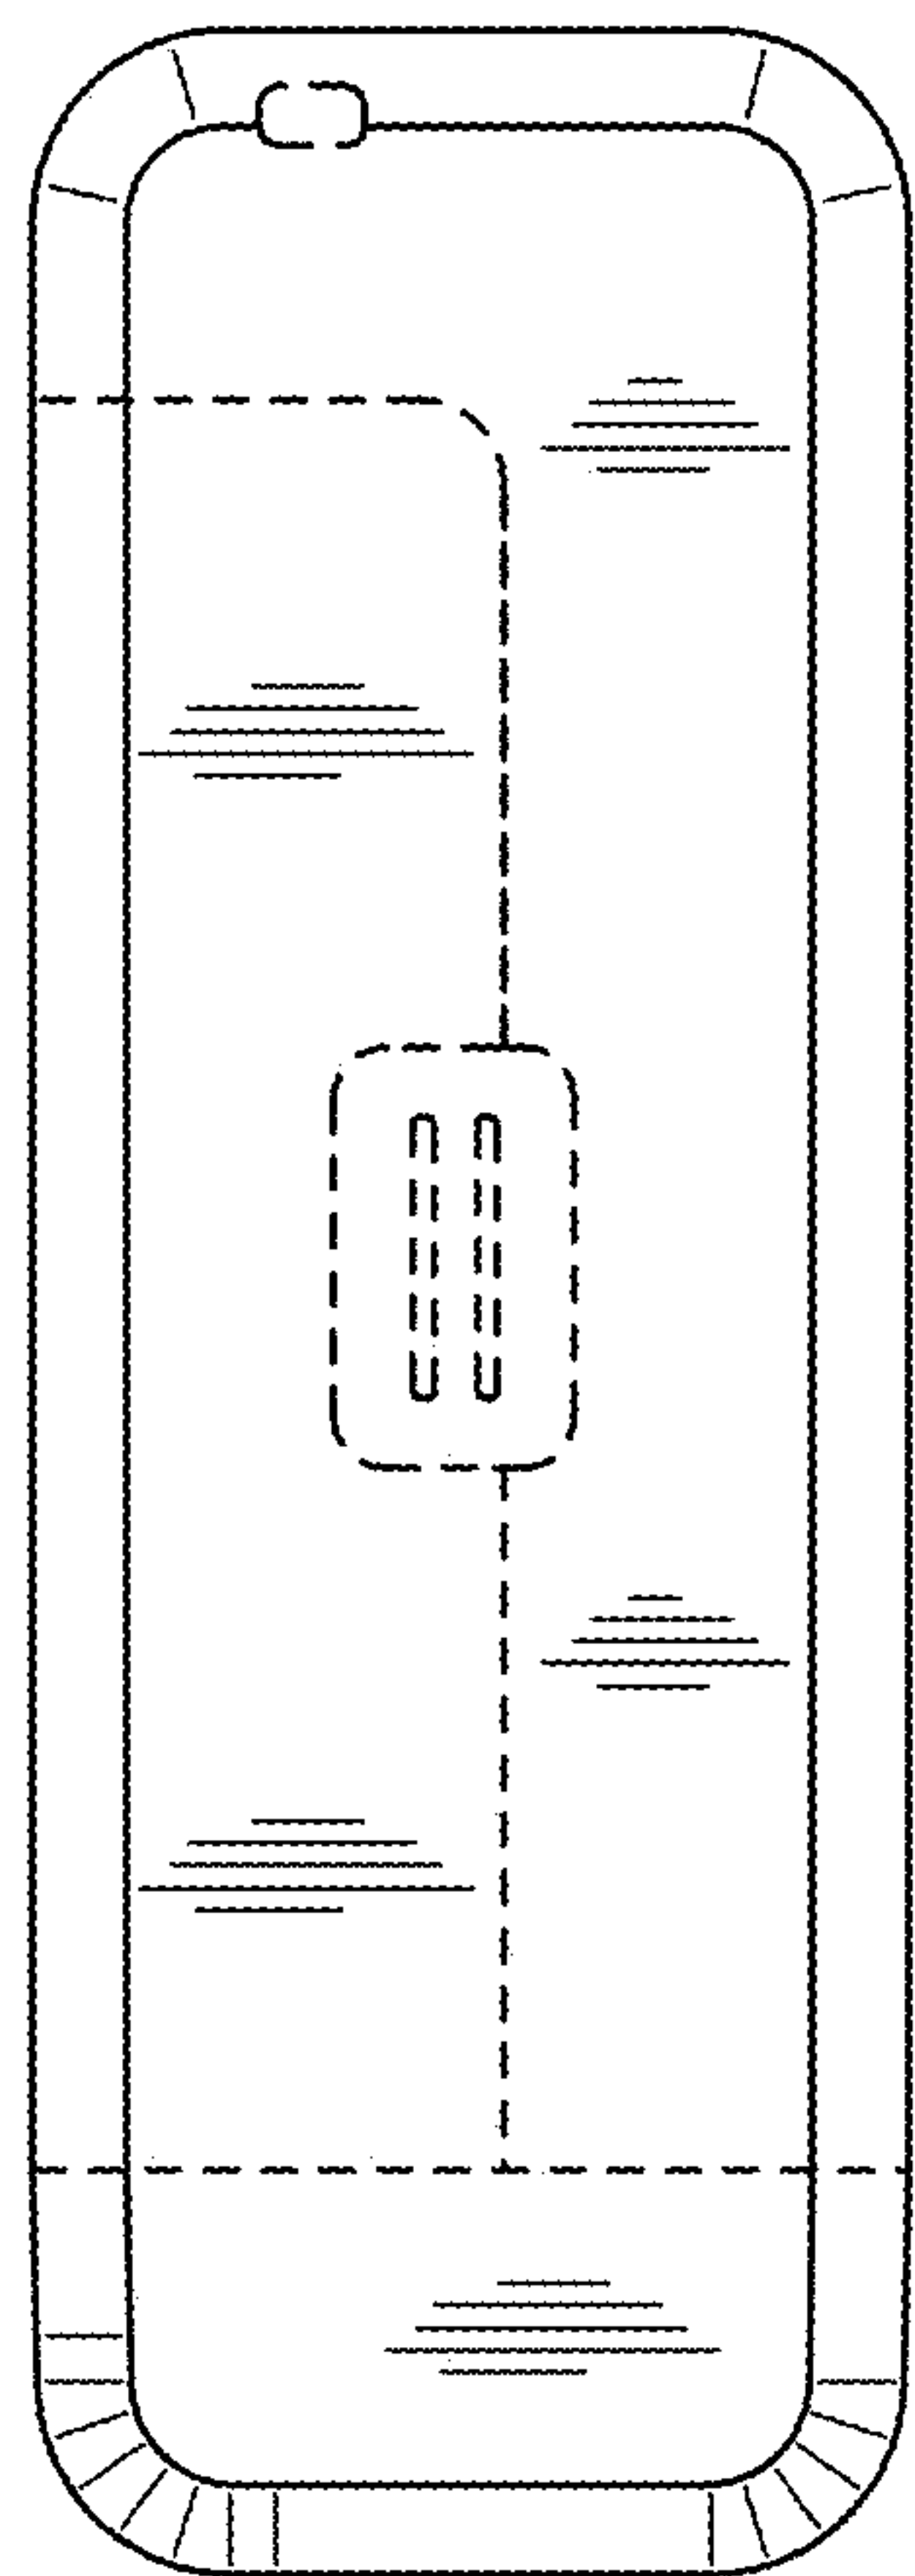


FIG. 6

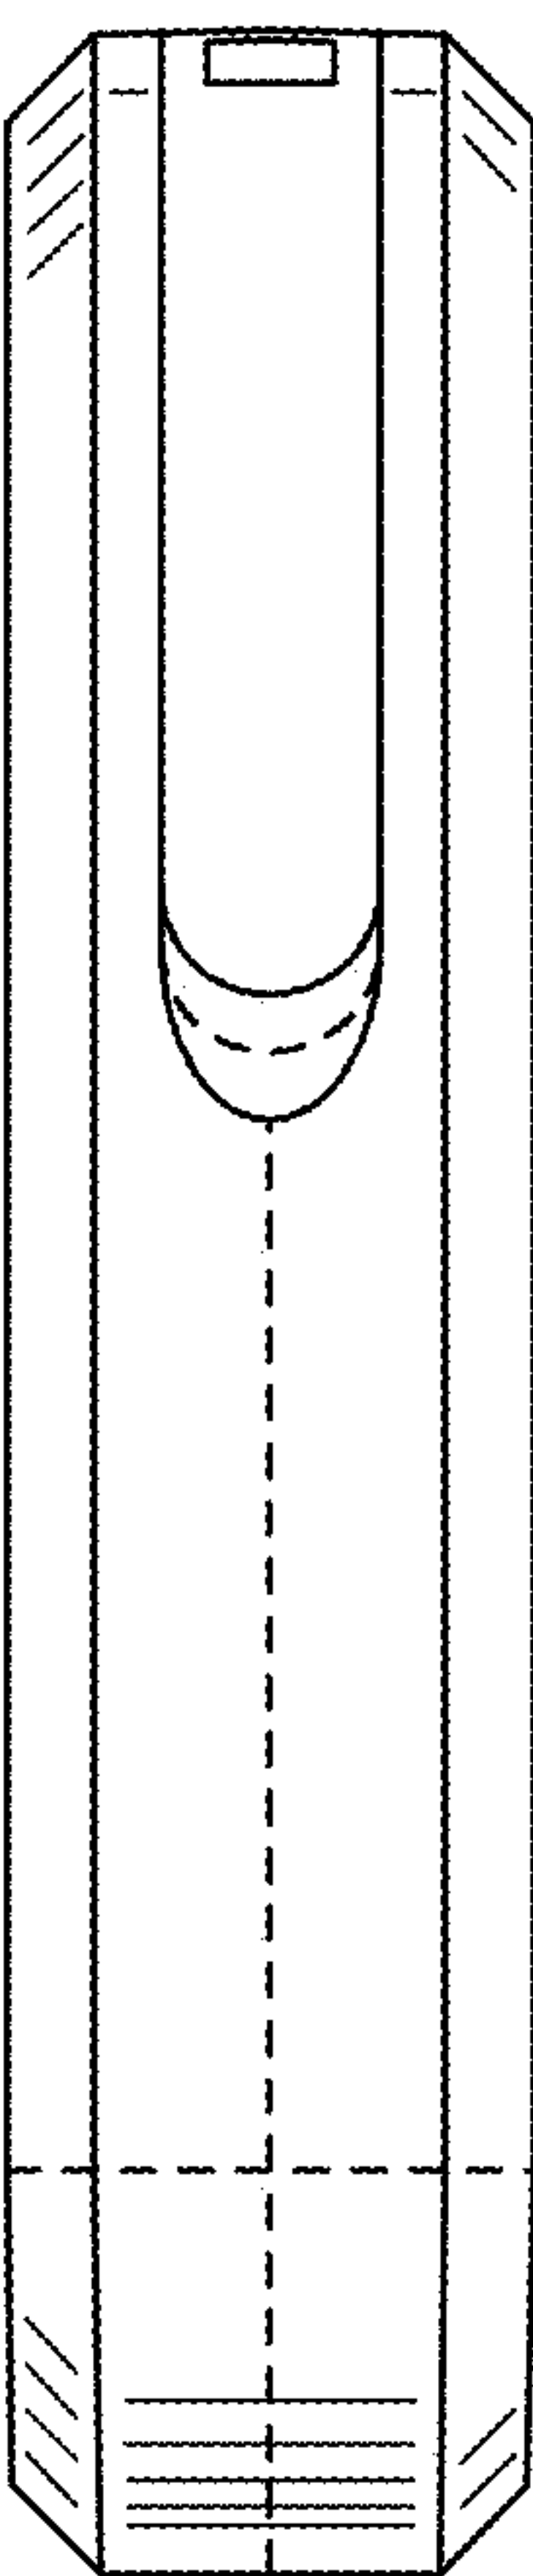


FIG. 7

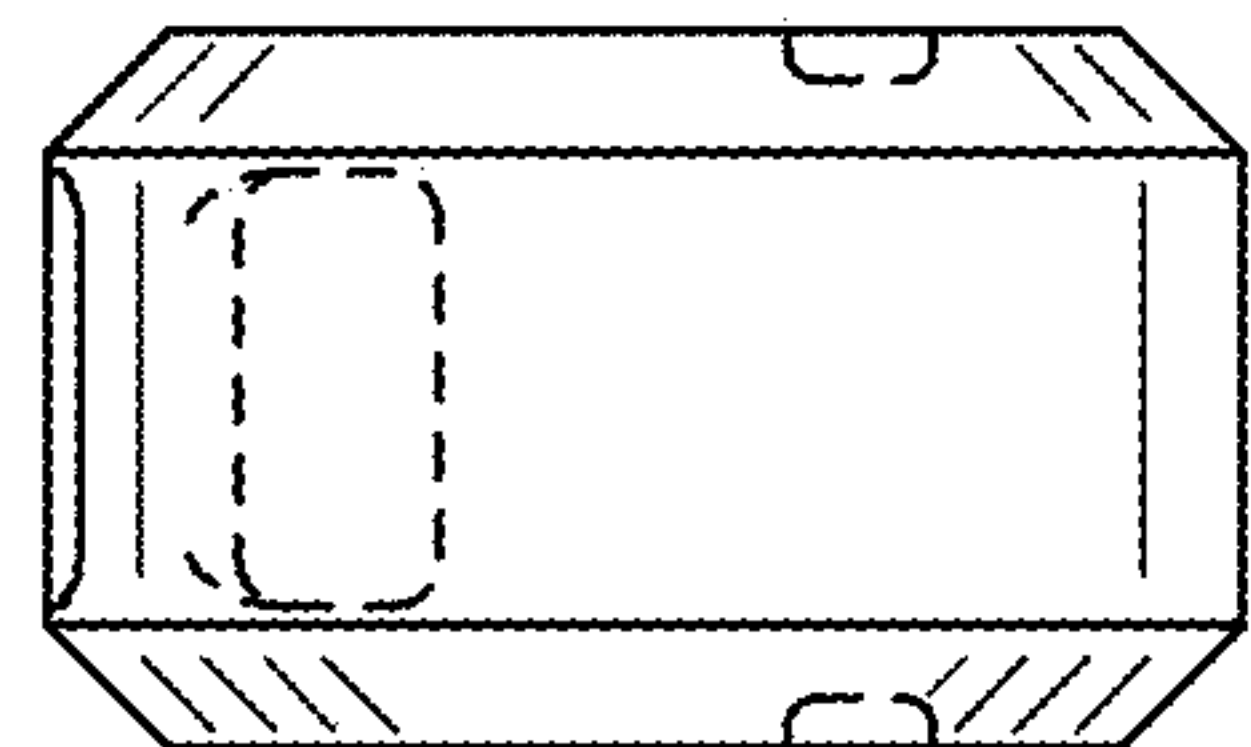


FIG. 8



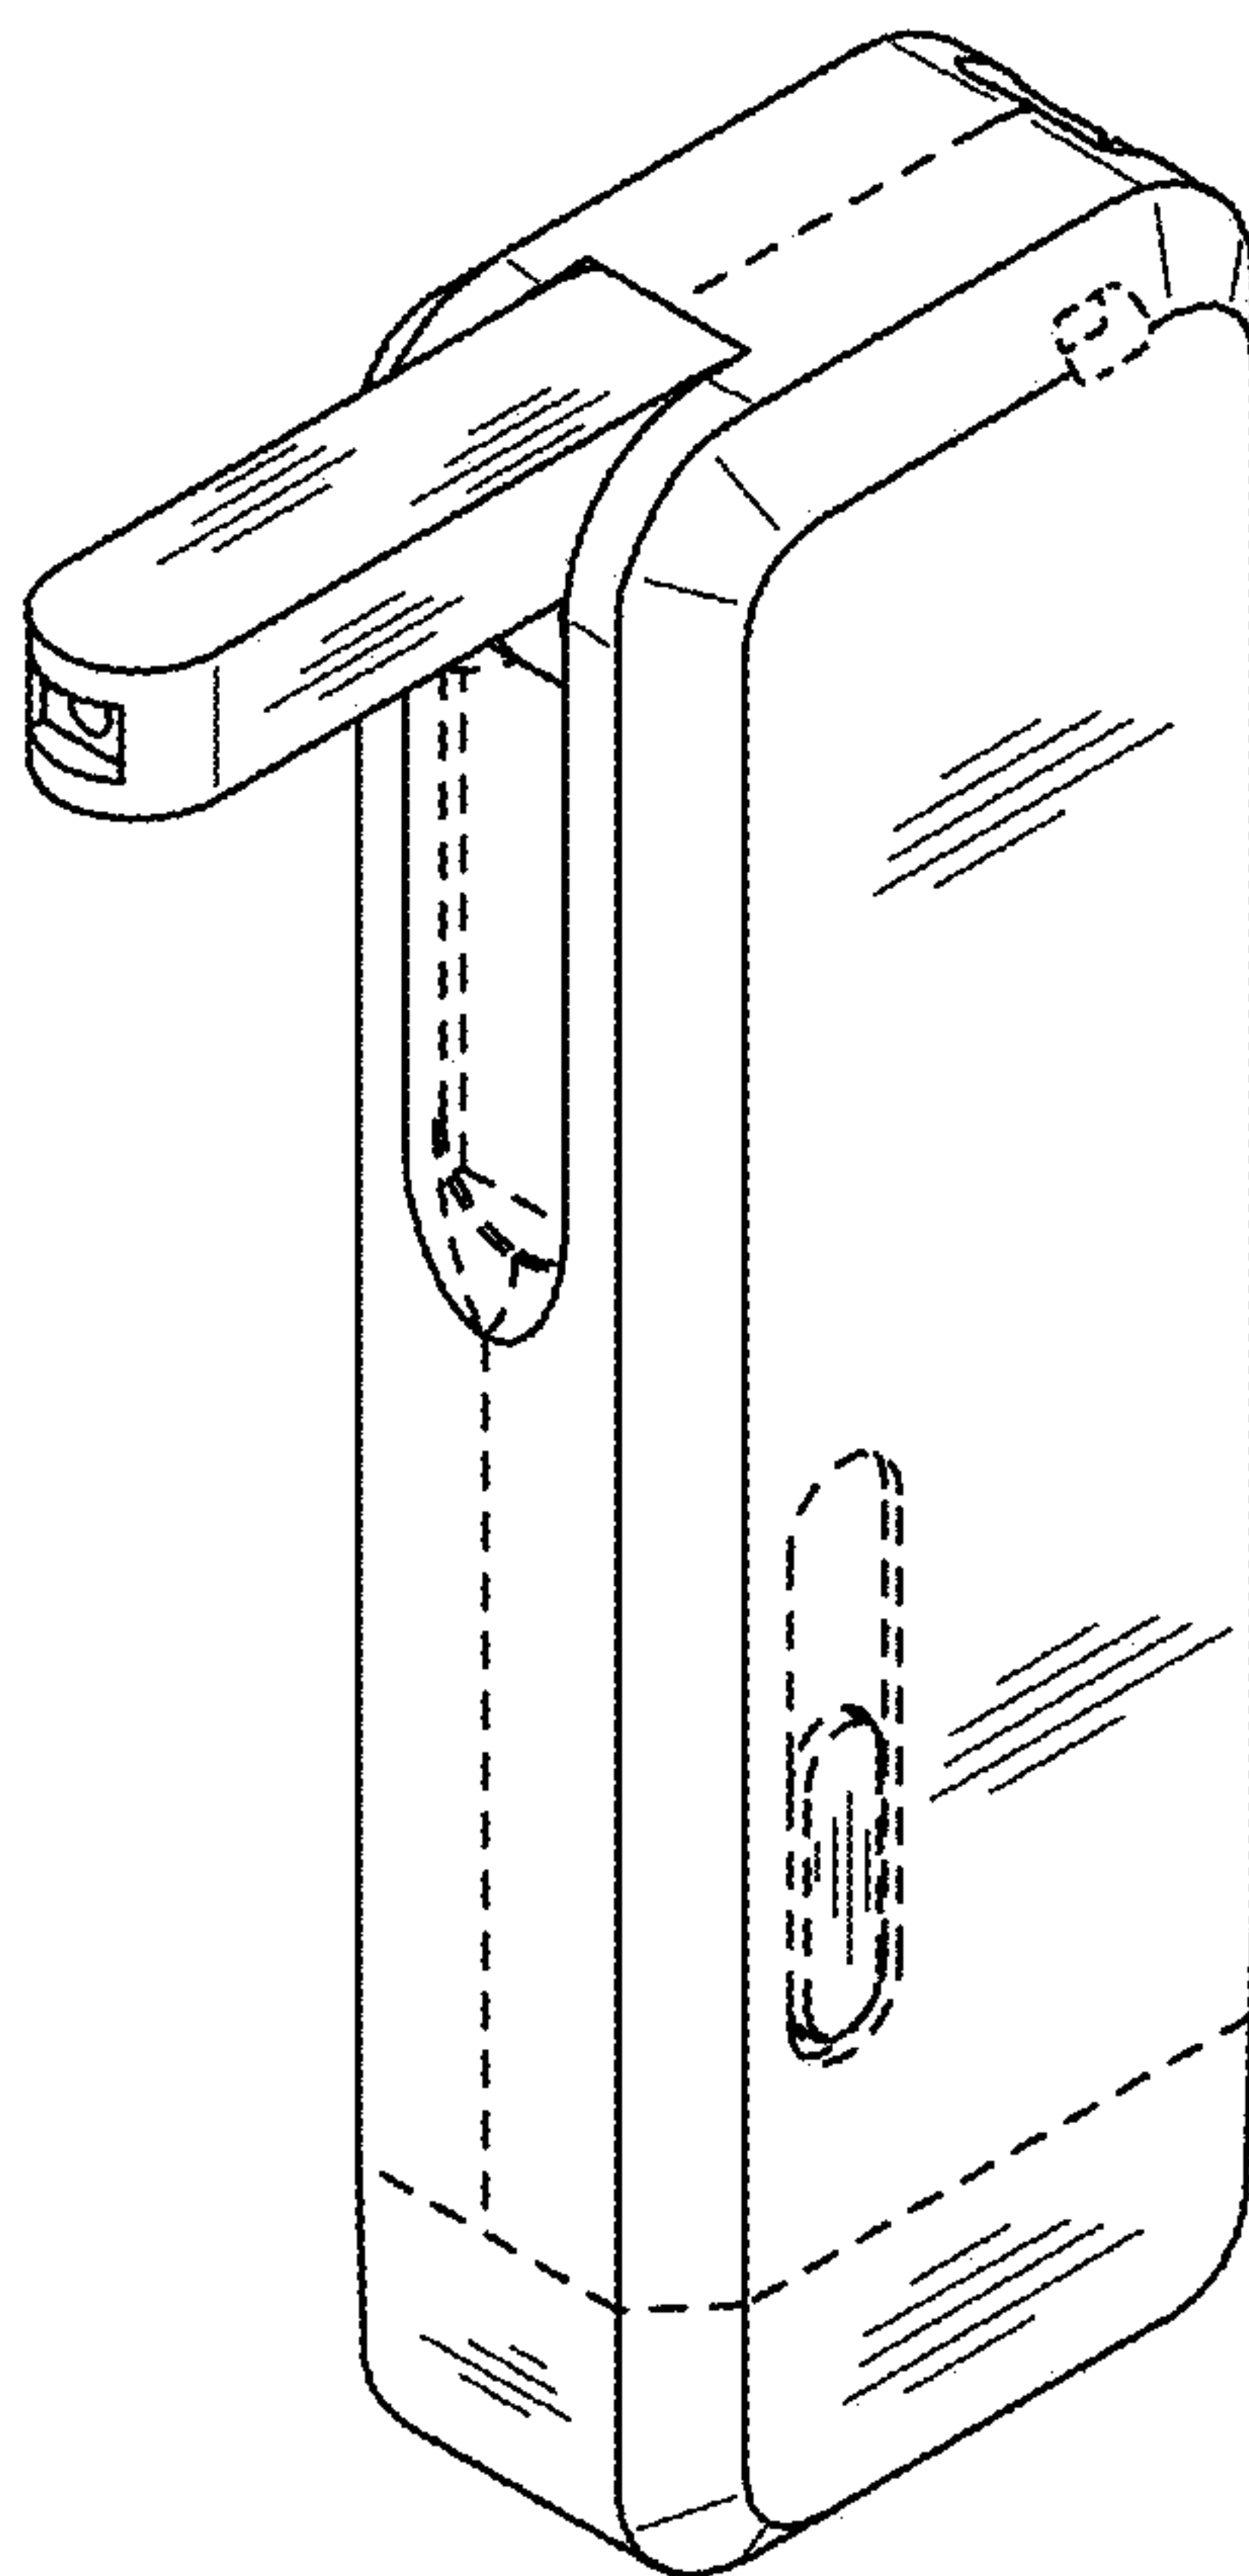


FIG. 9

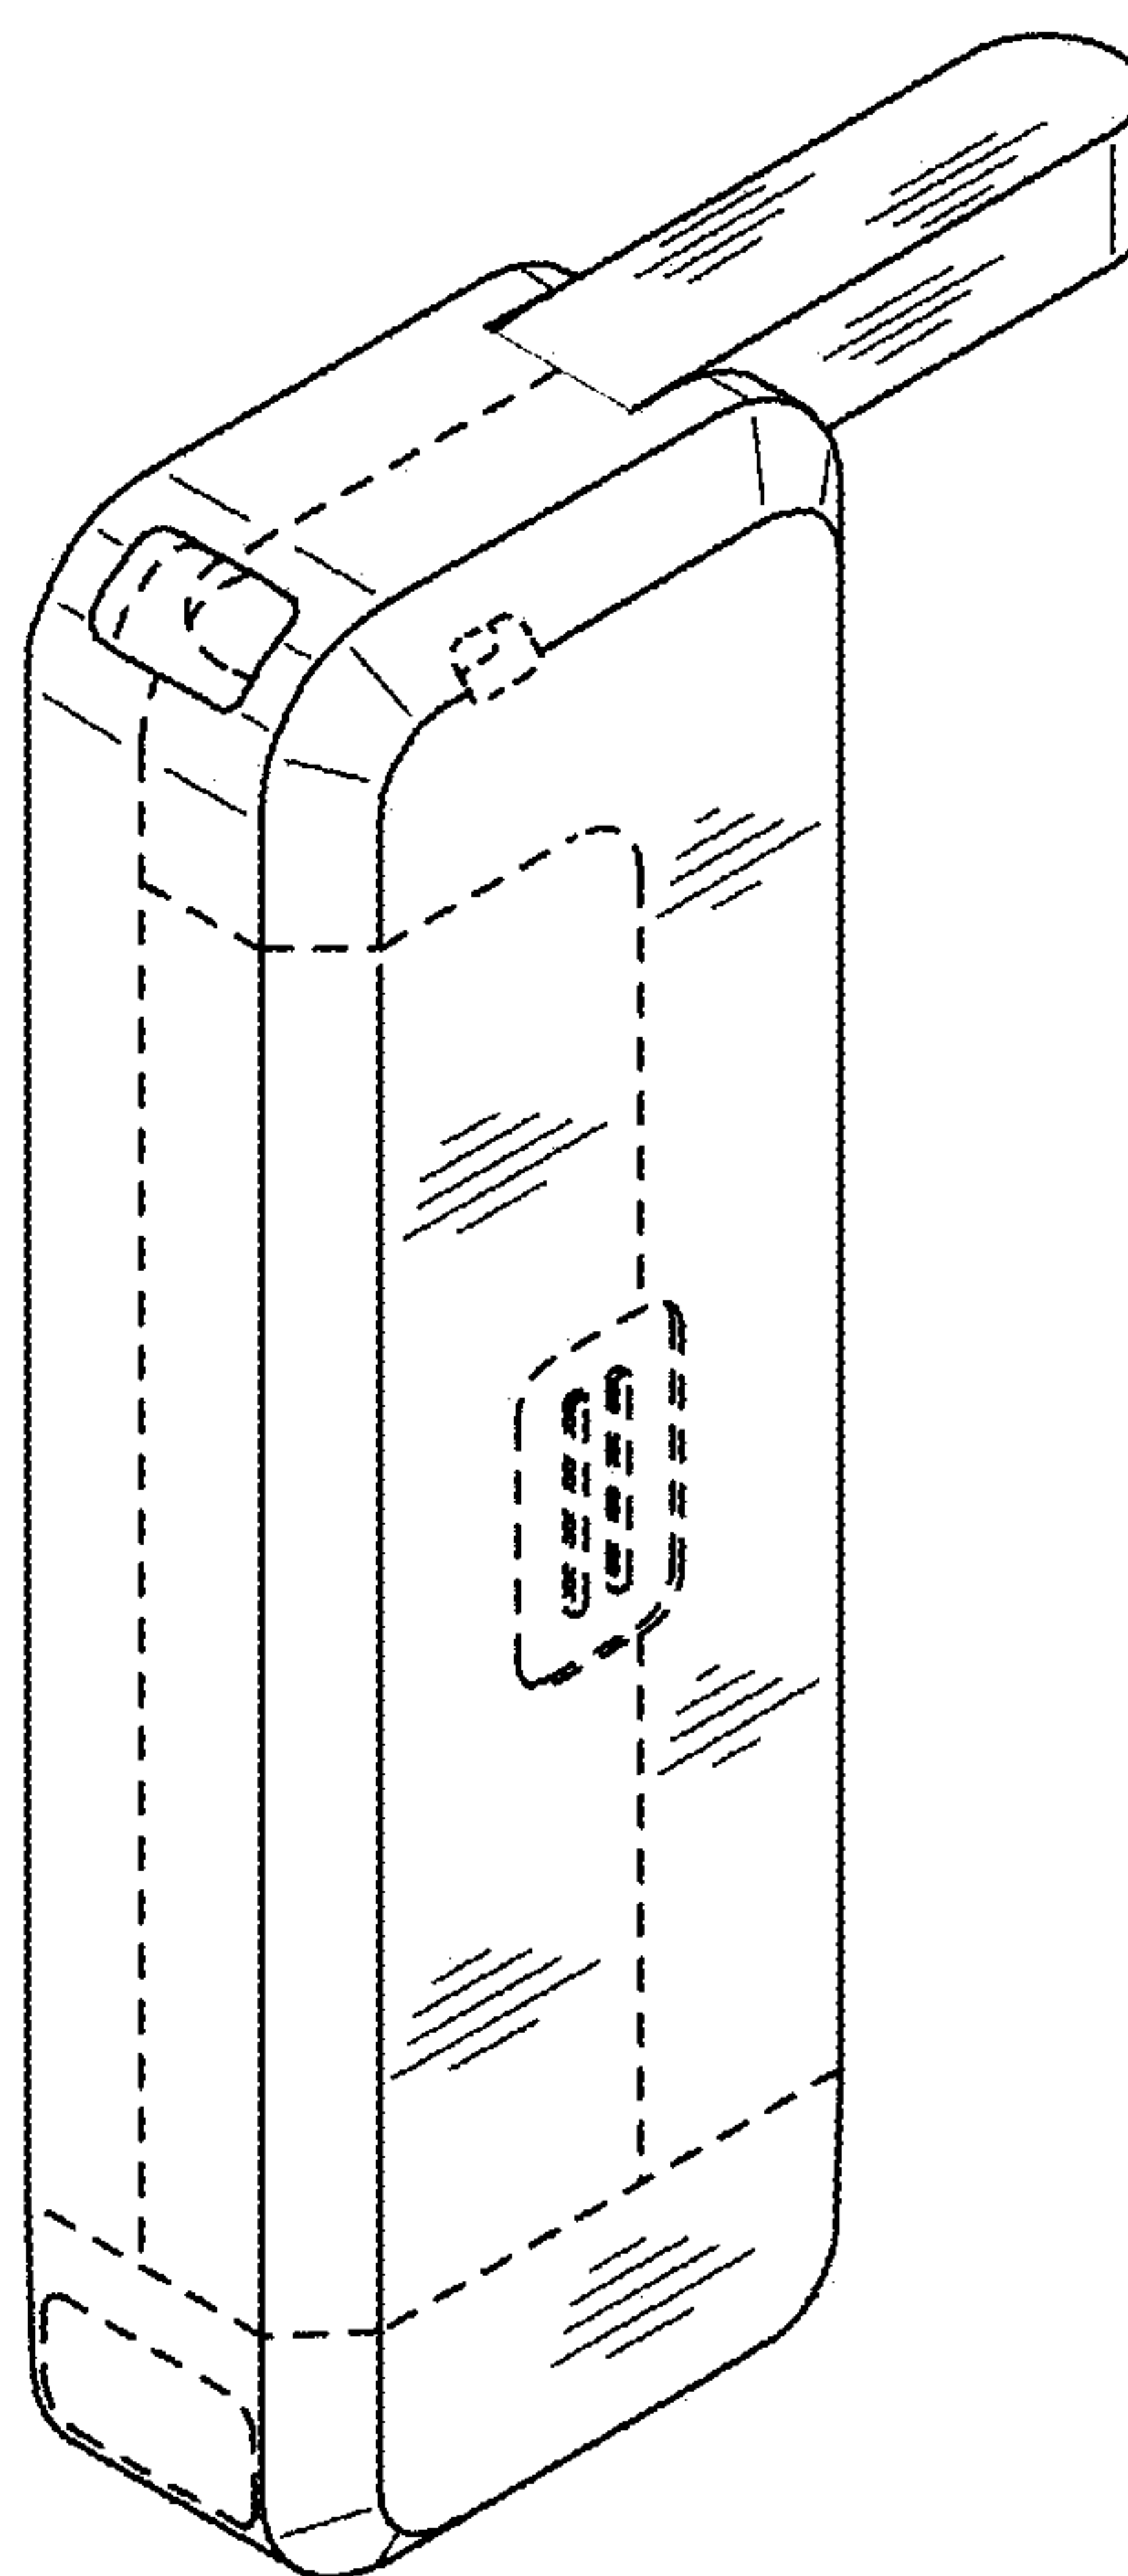


FIG. 10



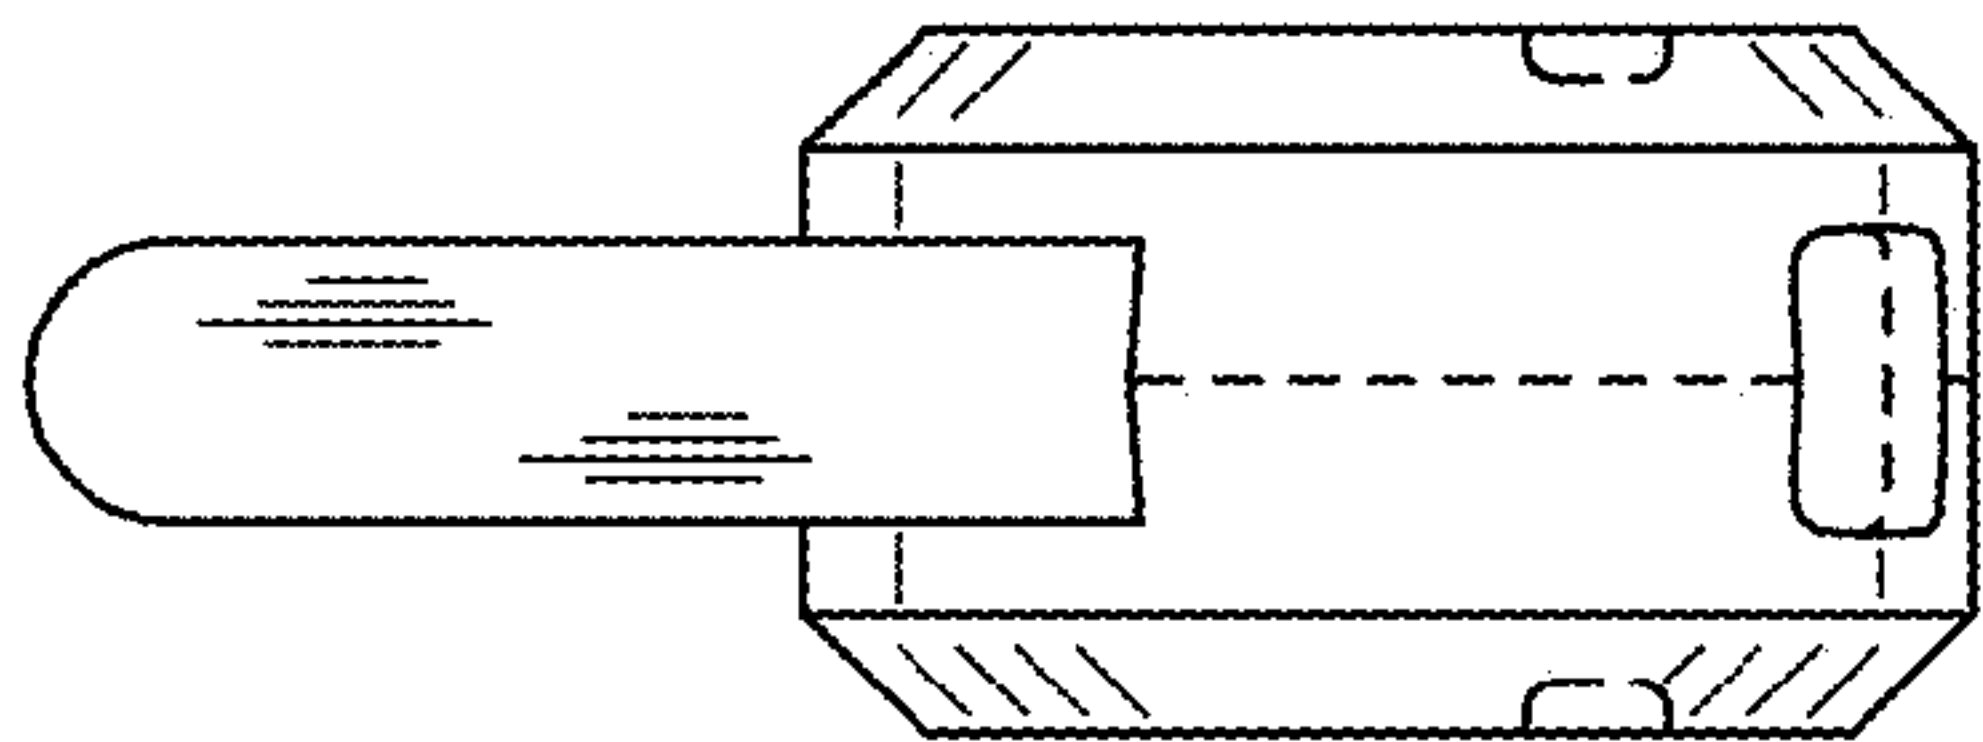


FIG. 11

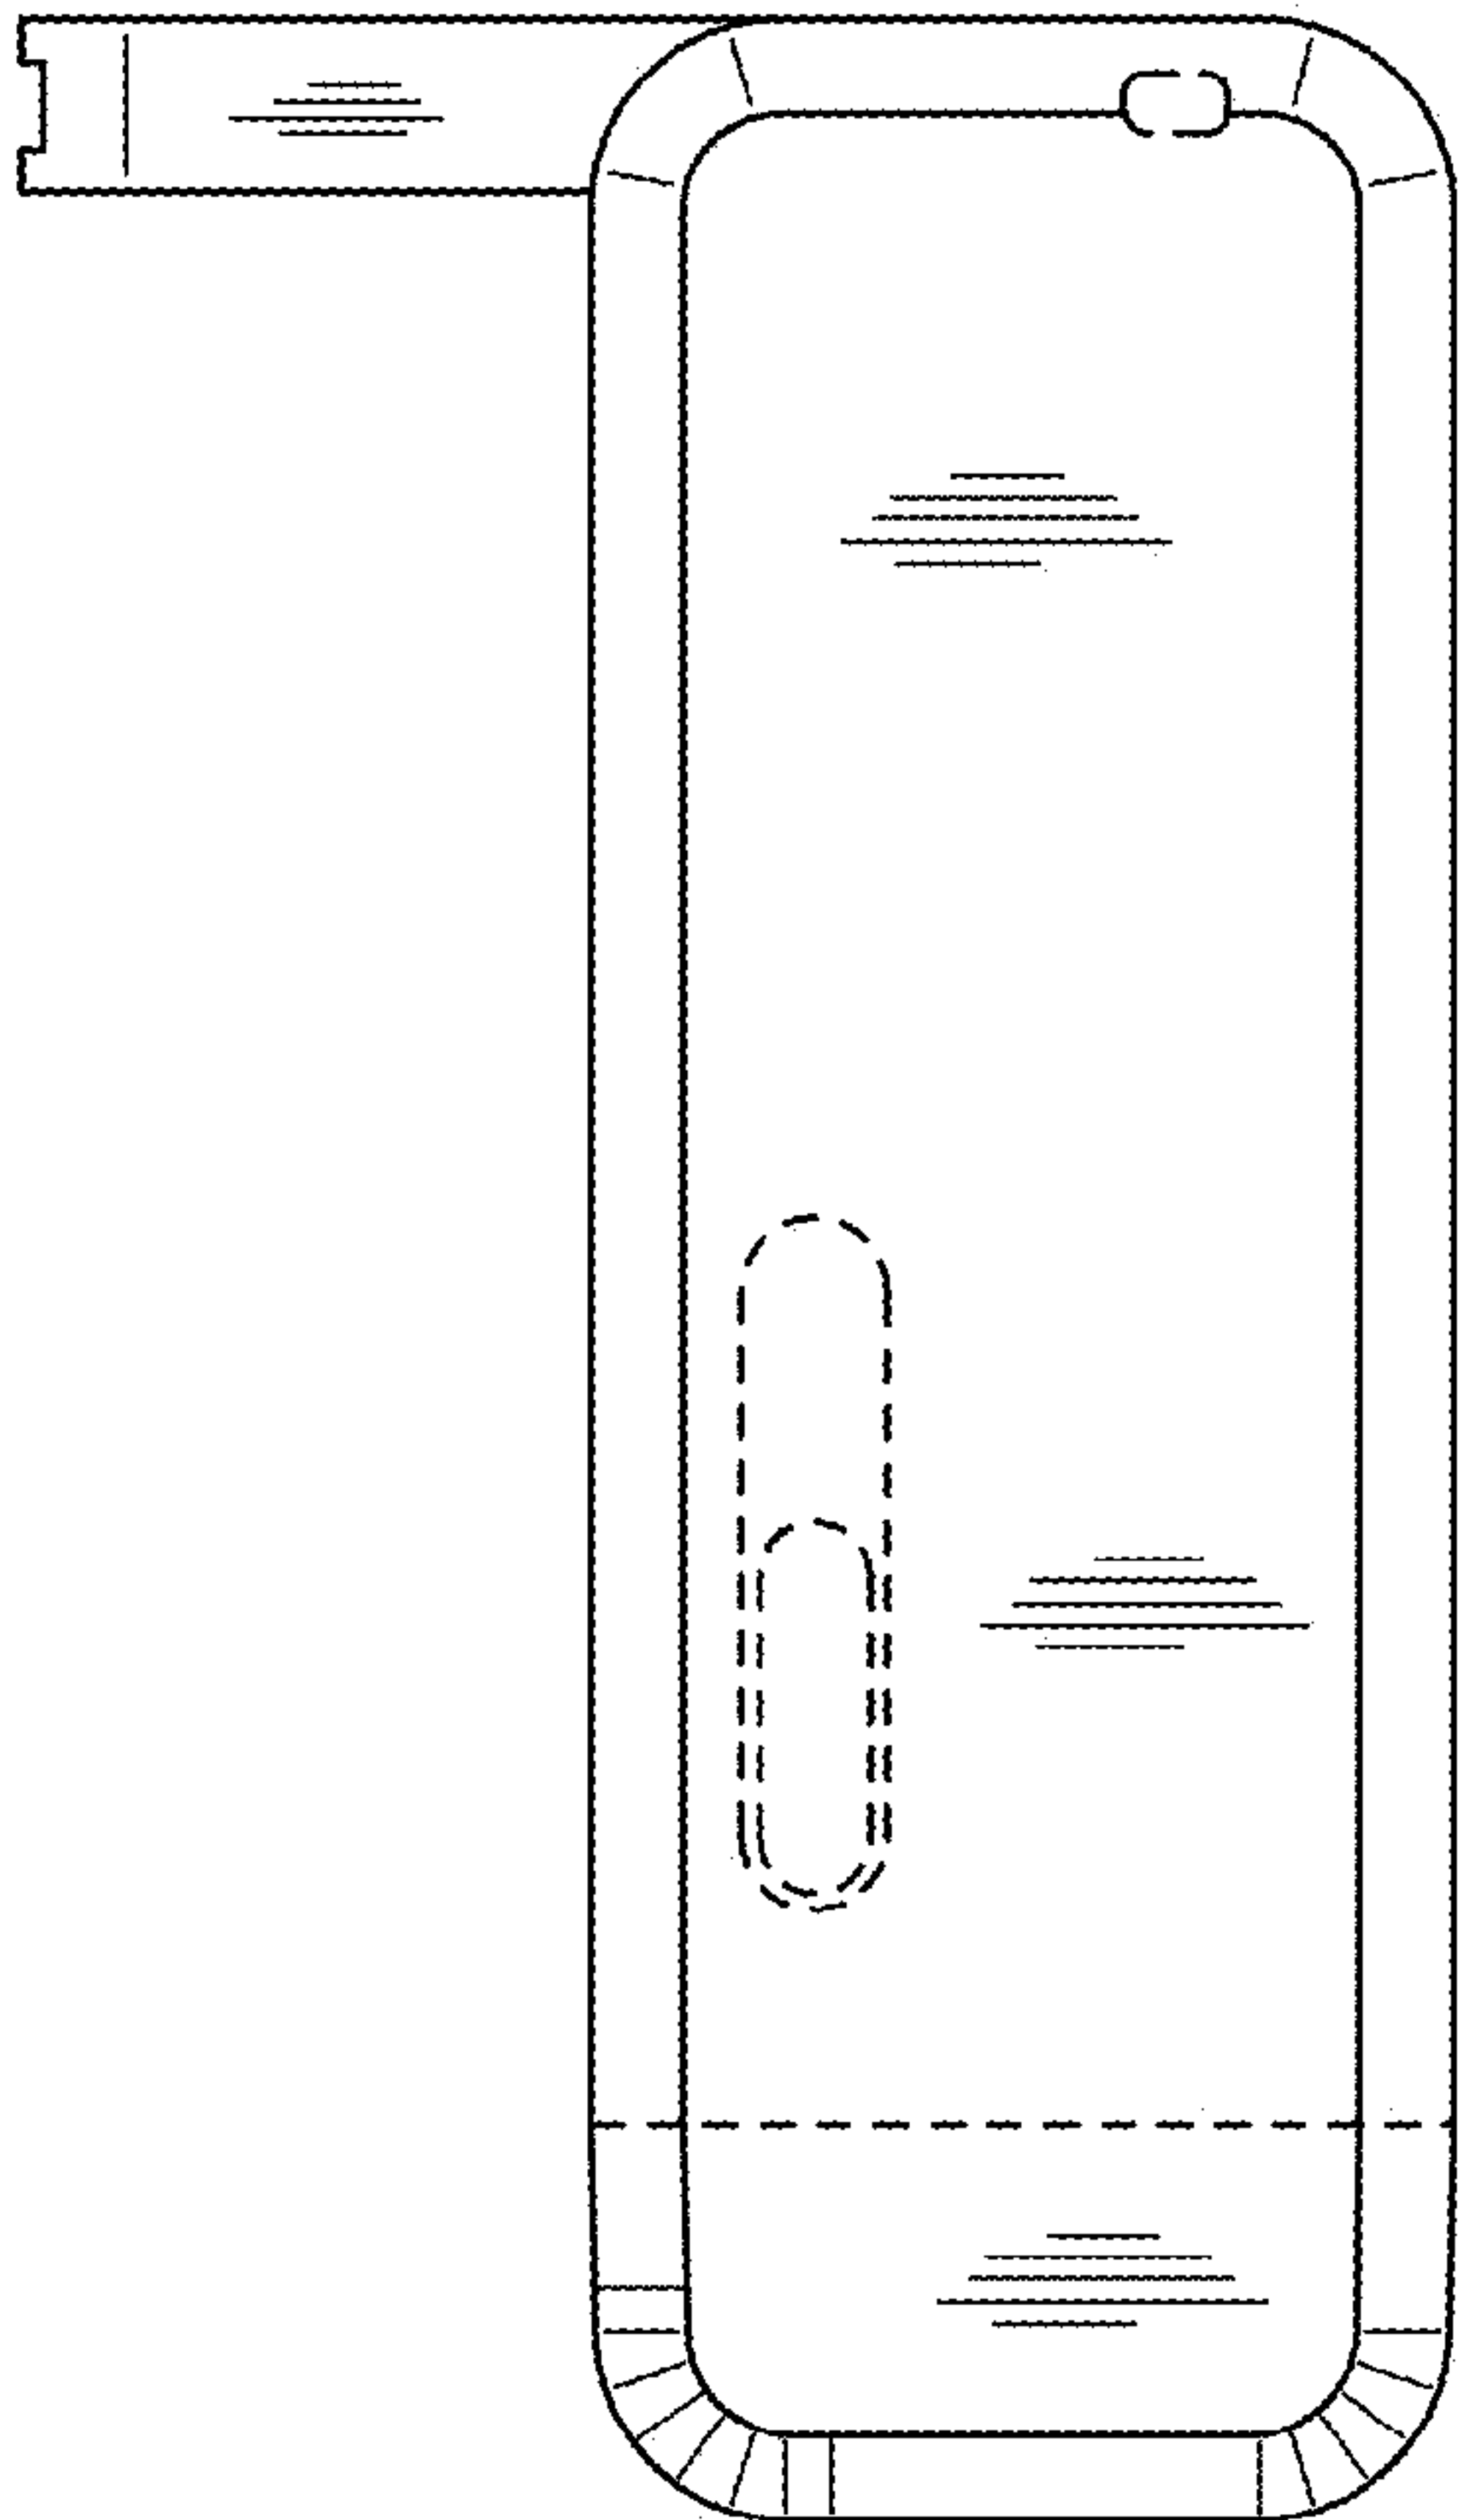


FIG. 12

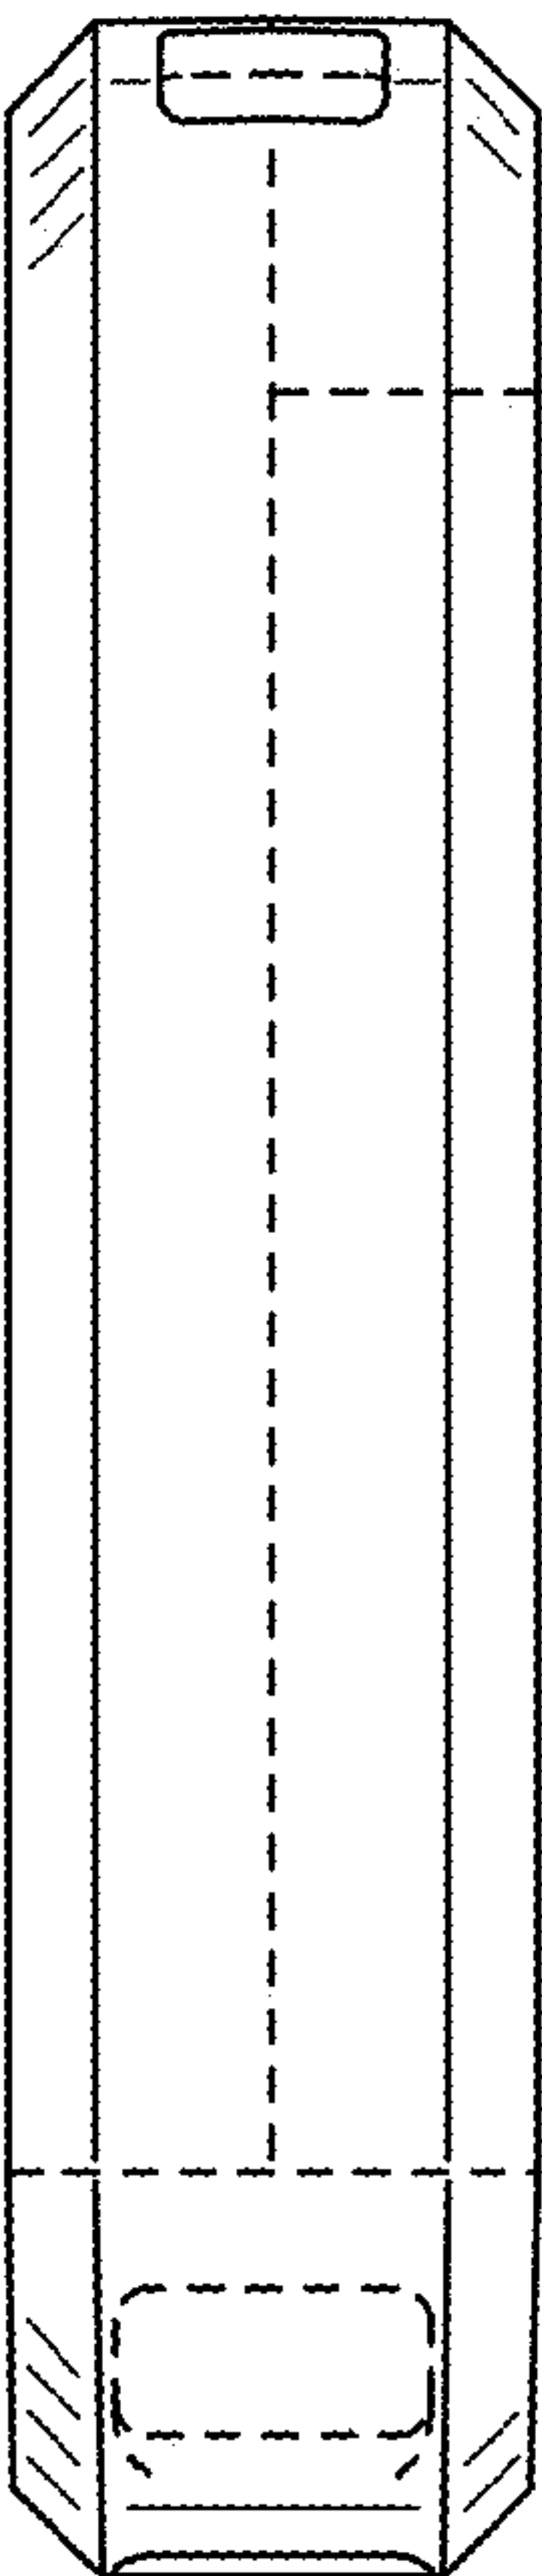


FIG. 13



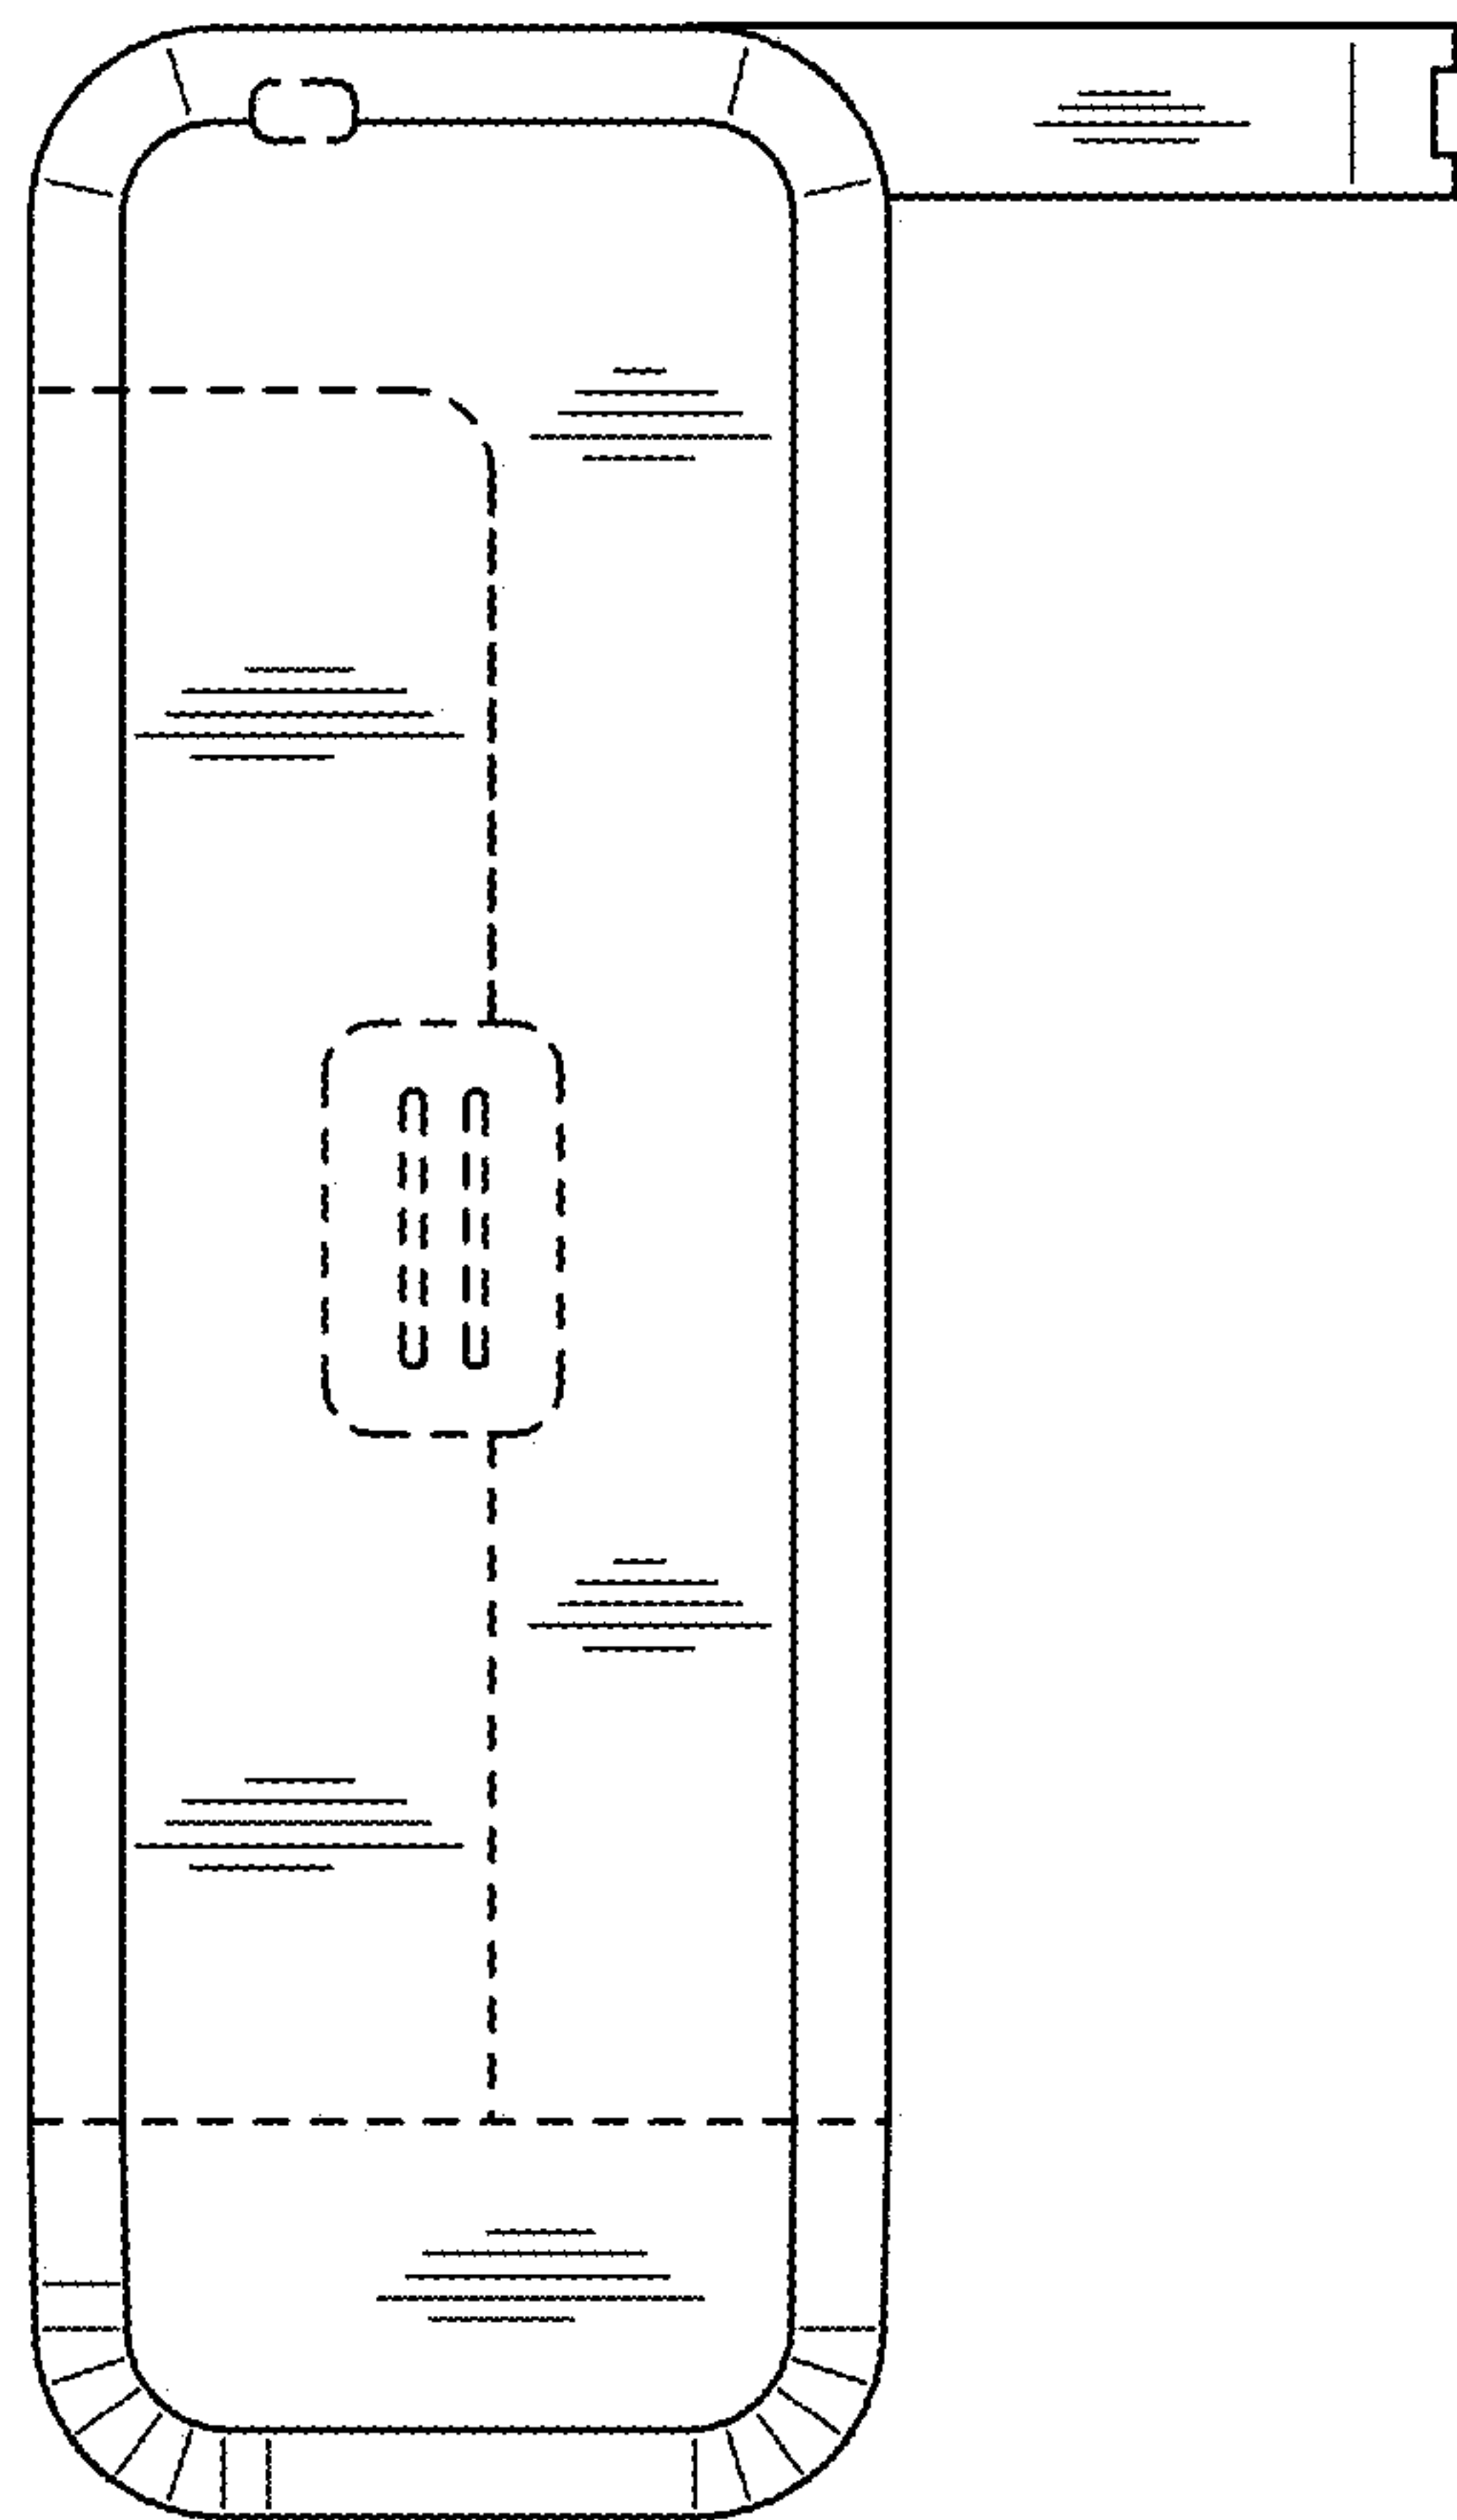


FIG. 14

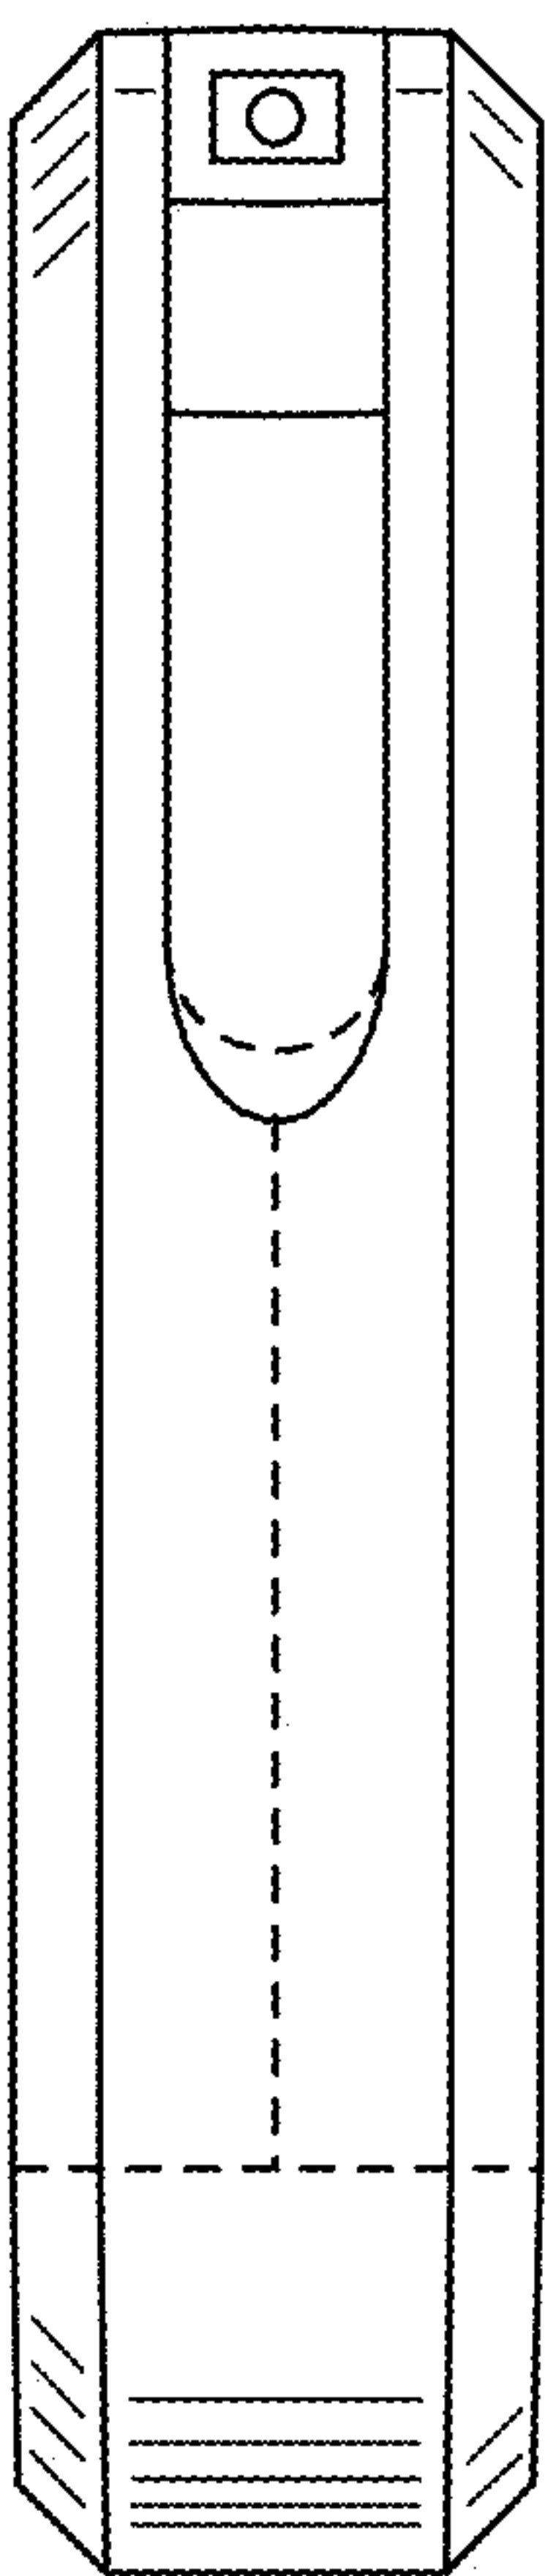


FIG. 15

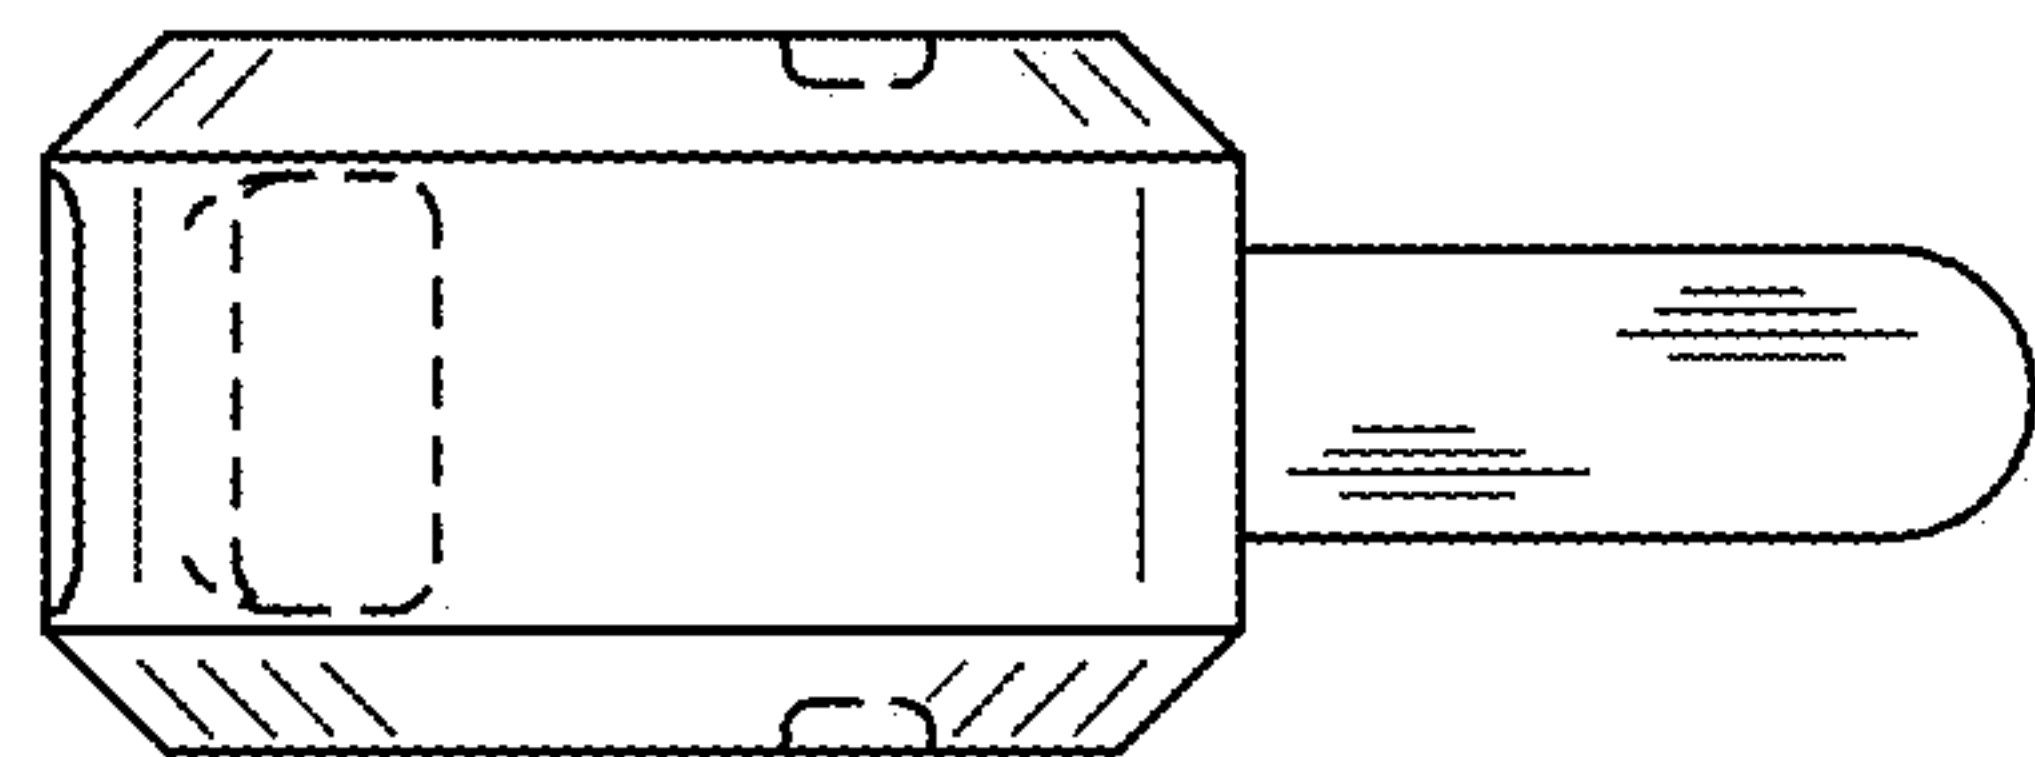


FIG. 16