



US00D745140S

(12) **United States Design Patent**  
**Wheeler et al.**(10) **Patent No.:** US D745,140 S  
(45) **Date of Patent:** \*\* Dec. 8, 2015

- (54) **CONTINUOUS POSITIVE AIRWAY PRESSURE DEVICE**
- (71) Applicant: **Engineered Medical Systems, Inc., Indianapolis, IN (US)**
- (72) Inventors: **Bradley Allen Wheeler, Greenwood Village, IN (US); Brad Quinn, Indianapolis, IN (US); Jeff Quinn, Carmel, IN (US)**
- (73) Assignee: **Engineered Medical Systems, Inc., Indianapolis, IN (US)**
- (\*\*) Term: **14 Years**
- (21) Appl. No.: **29/472,172**
- (22) Filed: **Nov. 8, 2013**
- (51) LOC (10) Cl. .... **29-02**
- (52) U.S. Cl.  
USPC ..... **D24/110**

(58) **Field of Classification Search**

USPC ..... D24/107, 110, 110.1, 110.5, 110.6, 127,  
D24/129; 128/200.11, 200.14, 200.21,  
128/200.24, 200.25, 202.27, 203.12,  
128/204.18, 205.24, 205.25, 206.12,  
128/206.15, 206.26, 207.12

See application file for complete search history.

(56) **References Cited**

## U.S. PATENT DOCUMENTS

- 4,261,355 A 4/1981 Glazener  
D305,814 S \* 1/1990 Fangrow, Jr. .... D24/110.6  
D327,338 S \* 6/1992 Wallace .... D24/110.5  
D331,281 S \* 11/1992 Levine .... D24/110  
D429,330 S \* 8/2000 Hoenig .... D24/110.6  
D441,070 S \* 4/2001 Niles et al. .... D24/110  
6,253,766 B1 7/2001 Niles  
2010/0126502 A1 \* 5/2010 Fink et al. .... 128/200.21  
2012/0272956 A1 \* 11/2012 Rusher .... 128/203.12  
2013/0228179 A1 \* 9/2013 Fischer, Jr. .... 128/204.18  
2014/0150801 A1 \* 6/2014 Rusher .... 128/207.16  
2014/0166013 A1 \* 6/2014 Stenzler et al. .... 128/204.18

## OTHER PUBLICATIONS

Exair—Amplifiers, Exair Corp.  
Infant Flow System Coanda Effect, E.M.E. Electro Medical Equipment.

Aladdin Infant Flow System, Hamilton Medical.  
C.P.A.P. "T", E. L. Glazener.  
Hillman and Huggins, (1991) Anesthesia & Intensive Care 19(2): 233-260, "Equipment A New Continuous Positive Airway Pressure (CPAP) Device".  
Shehabi, et al. (1991) Anesthesia & Intensive Care 19(2):237-243, "Tests of Six Continuous Flow CPAP Devices".  
Zamost, et al. (1980) ASA Abstracts, "Evaluation and Clinical Application of a New CPAP Device".  
Zamost, et al. (1981) Critical Care Medicine 9(2):109-113, "Description and clinical evaluation of a new continuous positive airway pressure device".

\* cited by examiner

*Primary Examiner* — Deanna L Pratt

*Assistant Examiner* — Lilyana Bekic

(74) *Attorney, Agent, or Firm* — Swanson & Bratschun, L.L.C.

(57) **CLAIM**

The ornamental design for a continuous positive airway pressure device, as shown and described.

**DESCRIPTION**

FIG. 1 is a front, top, left perspective view of a first embodiment of a continuous positive airway pressure device showing our new design;

FIG. 2 is a left side elevation view of the continuous positive airway pressure device of FIG. 1, the right side view being a mirror image thereof;

FIG. 3 is a front elevation view of the continuous positive airway pressure device of FIG. 1;

FIG. 4 is a rear elevation view of the continuous positive airway pressure device of FIG. 1;


FIG. 5 is a top plan view of the continuous positive airway pressure device of FIG. 1;

FIG. 6 is a bottom plan view of the continuous positive airway pressure device of FIG. 1; and,

FIG. 7 is a front, top, left perspective view of a second embodiment of a translucent body of the continuous positive airway pressure device of FIGS. 1-6, it being understood that all other surfaces are the same as those of the first embodiment.

The broken lines showing portions of the design in all figures are included for the purpose of illustrating environment and unclaimed features and forms not part of the claimed design.

**1 Claim, 5 Drawing Sheets**

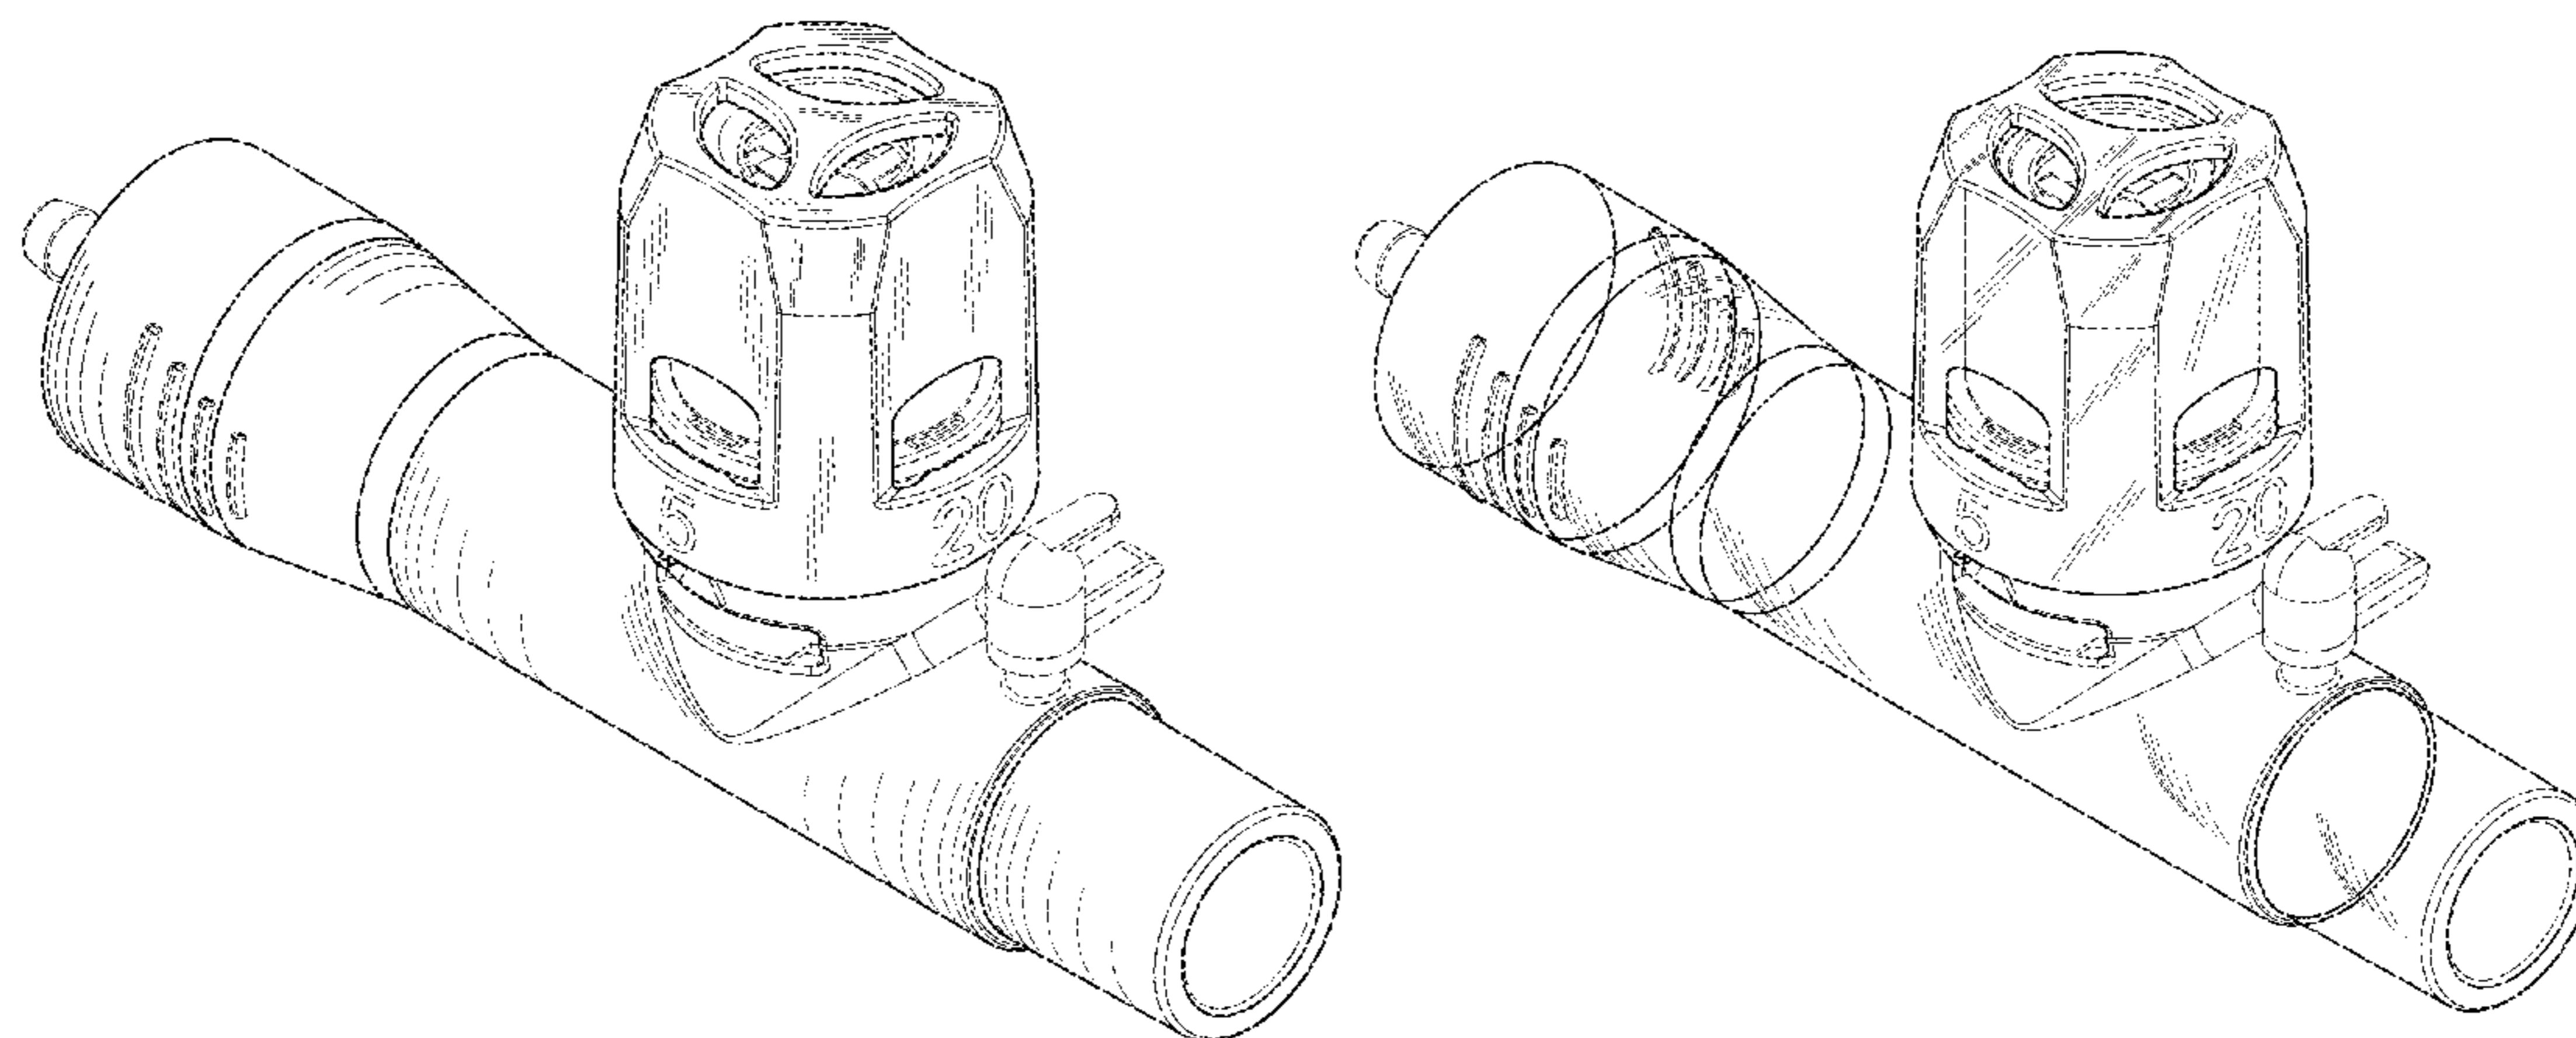

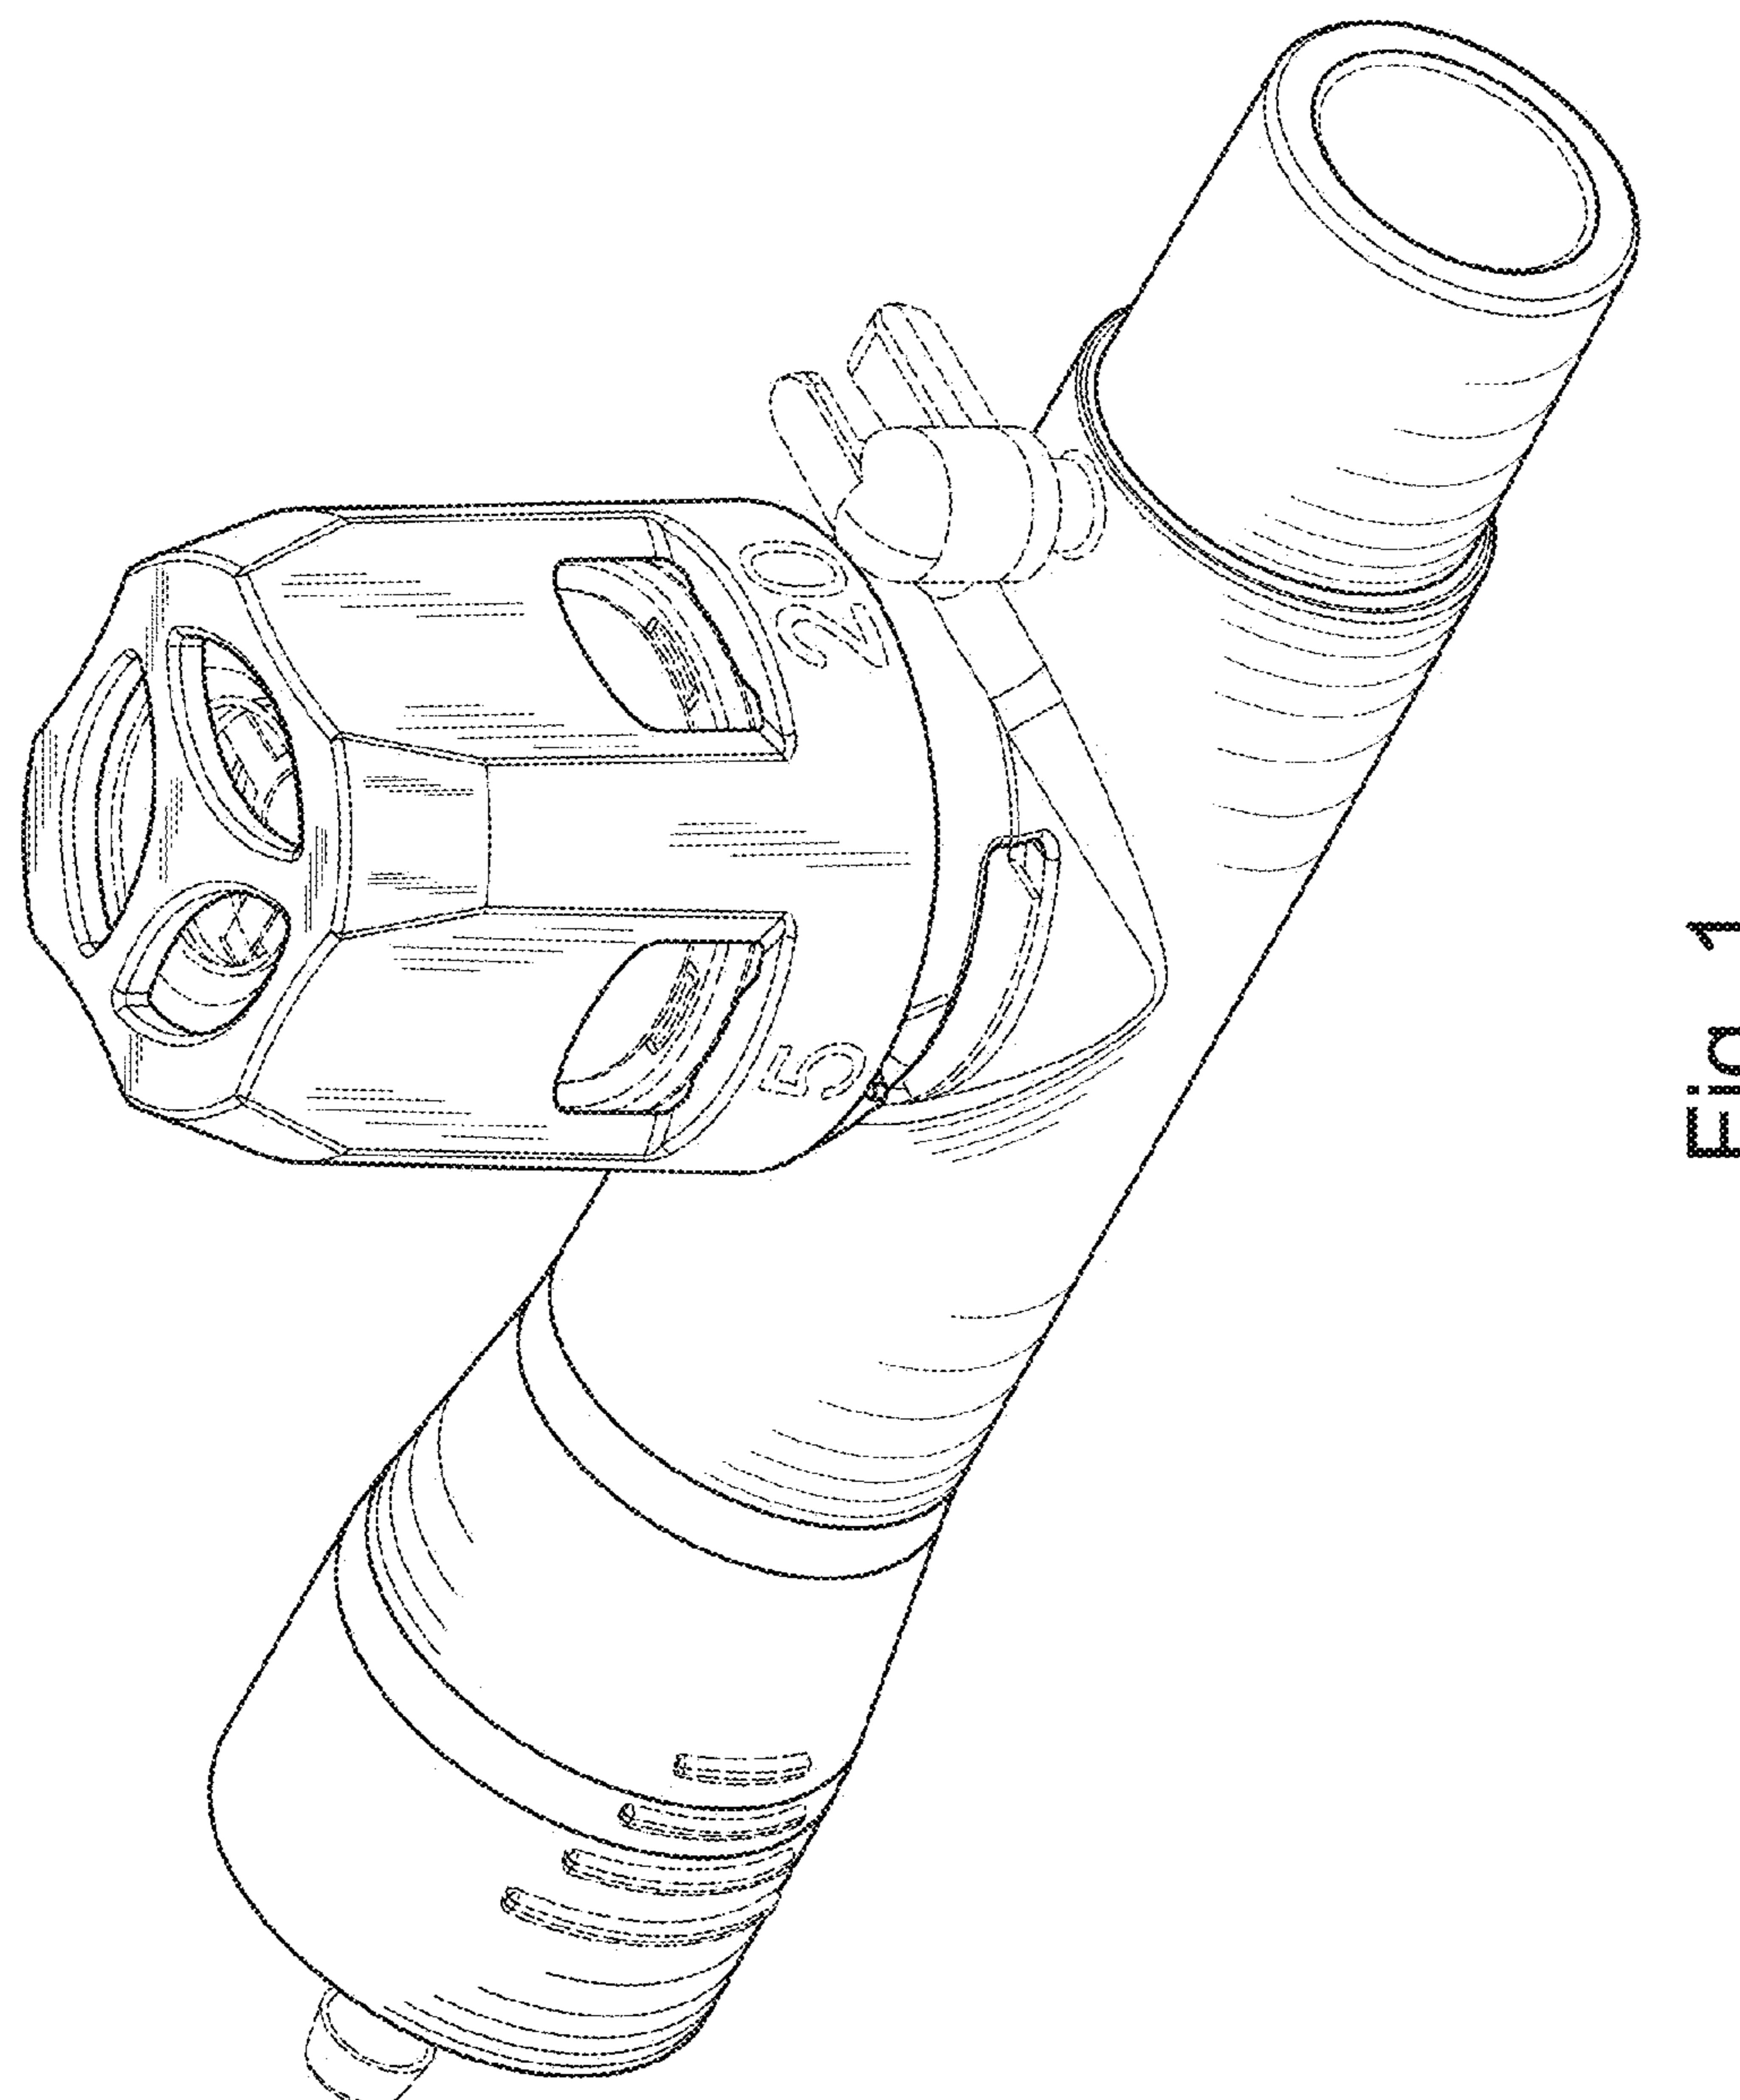


Fig. 1

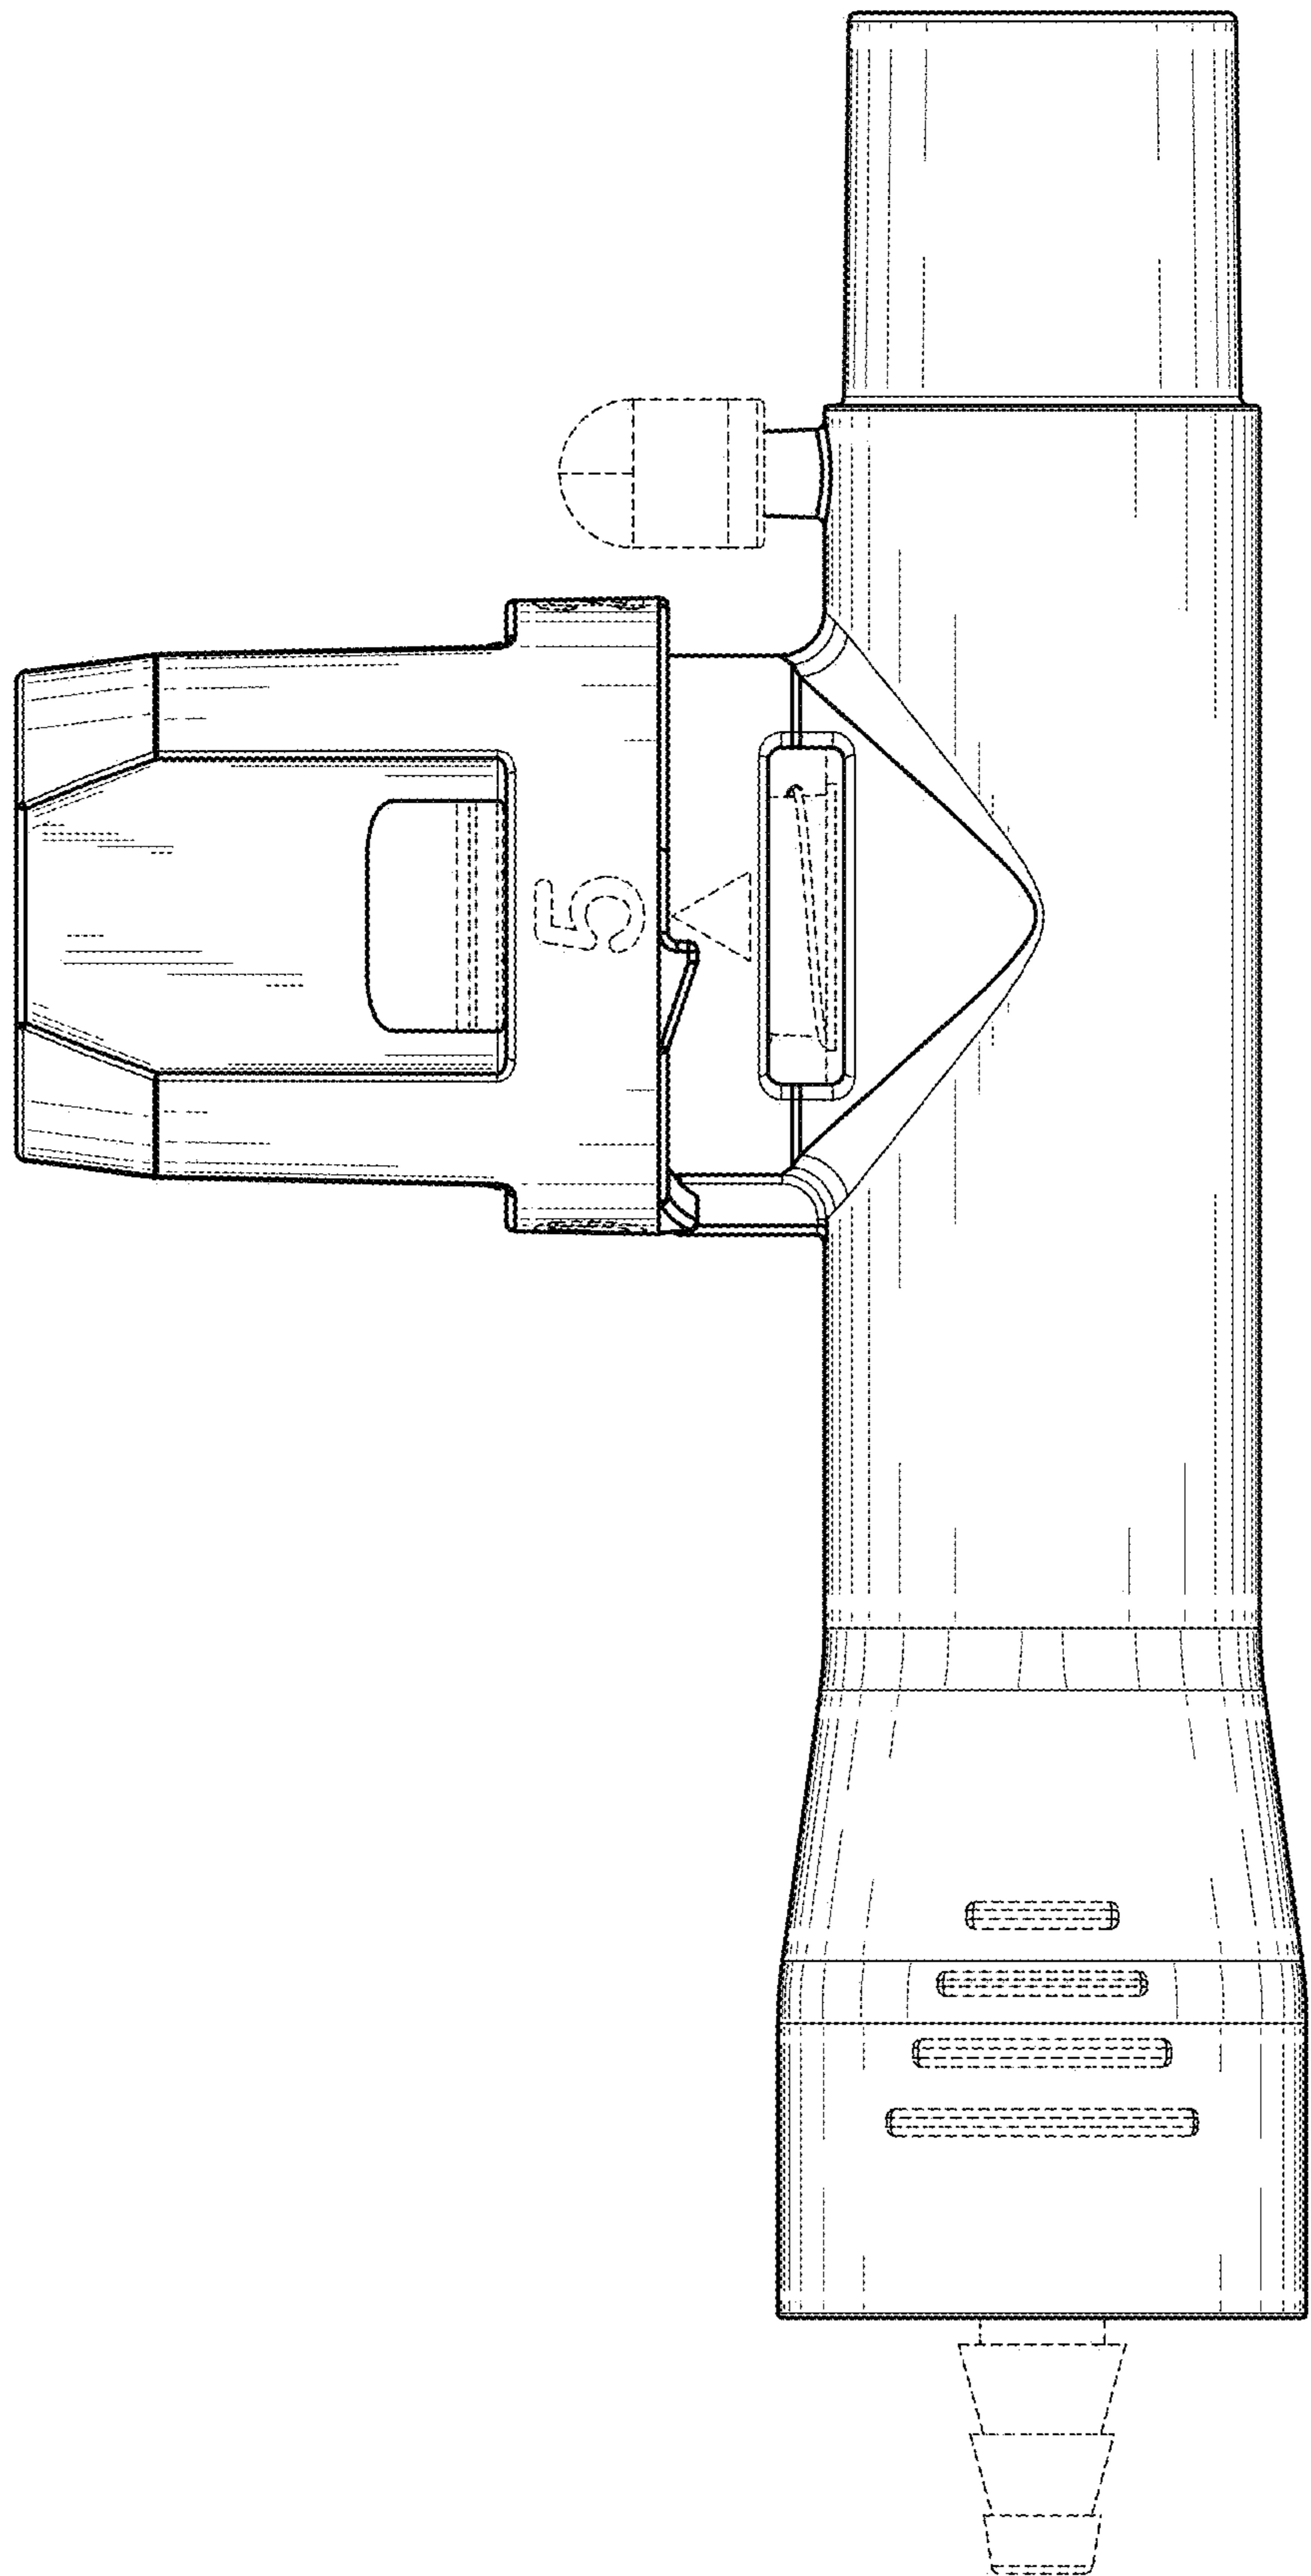


Fig. 2

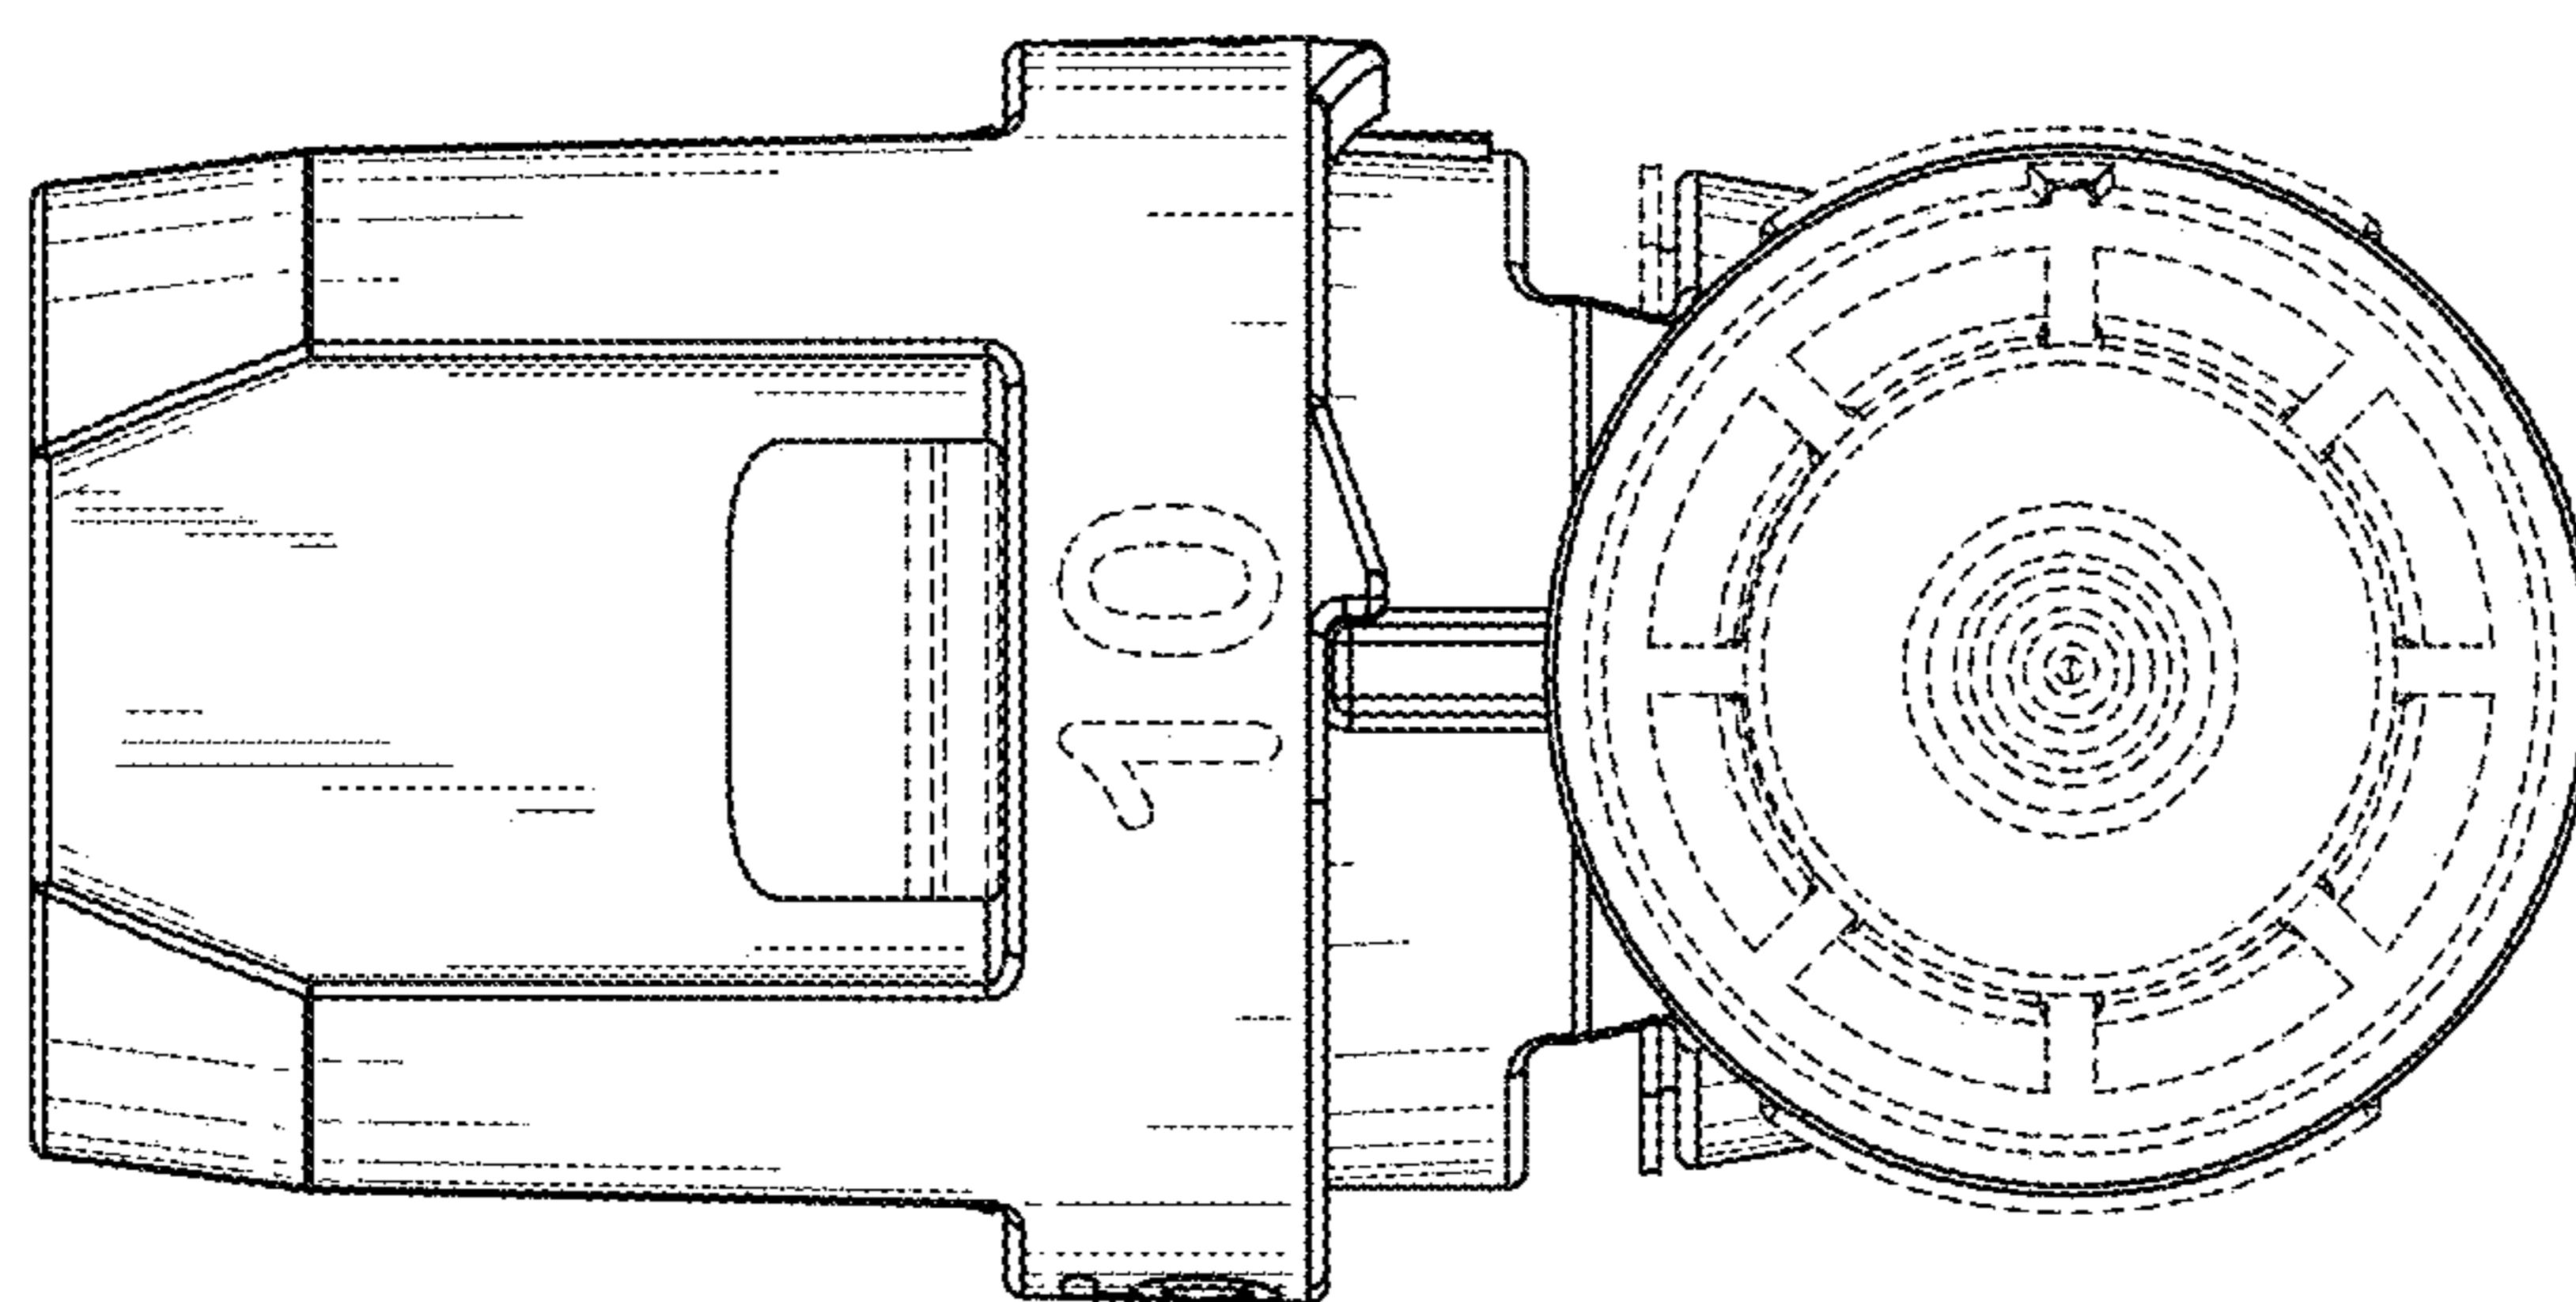


Fig. 3

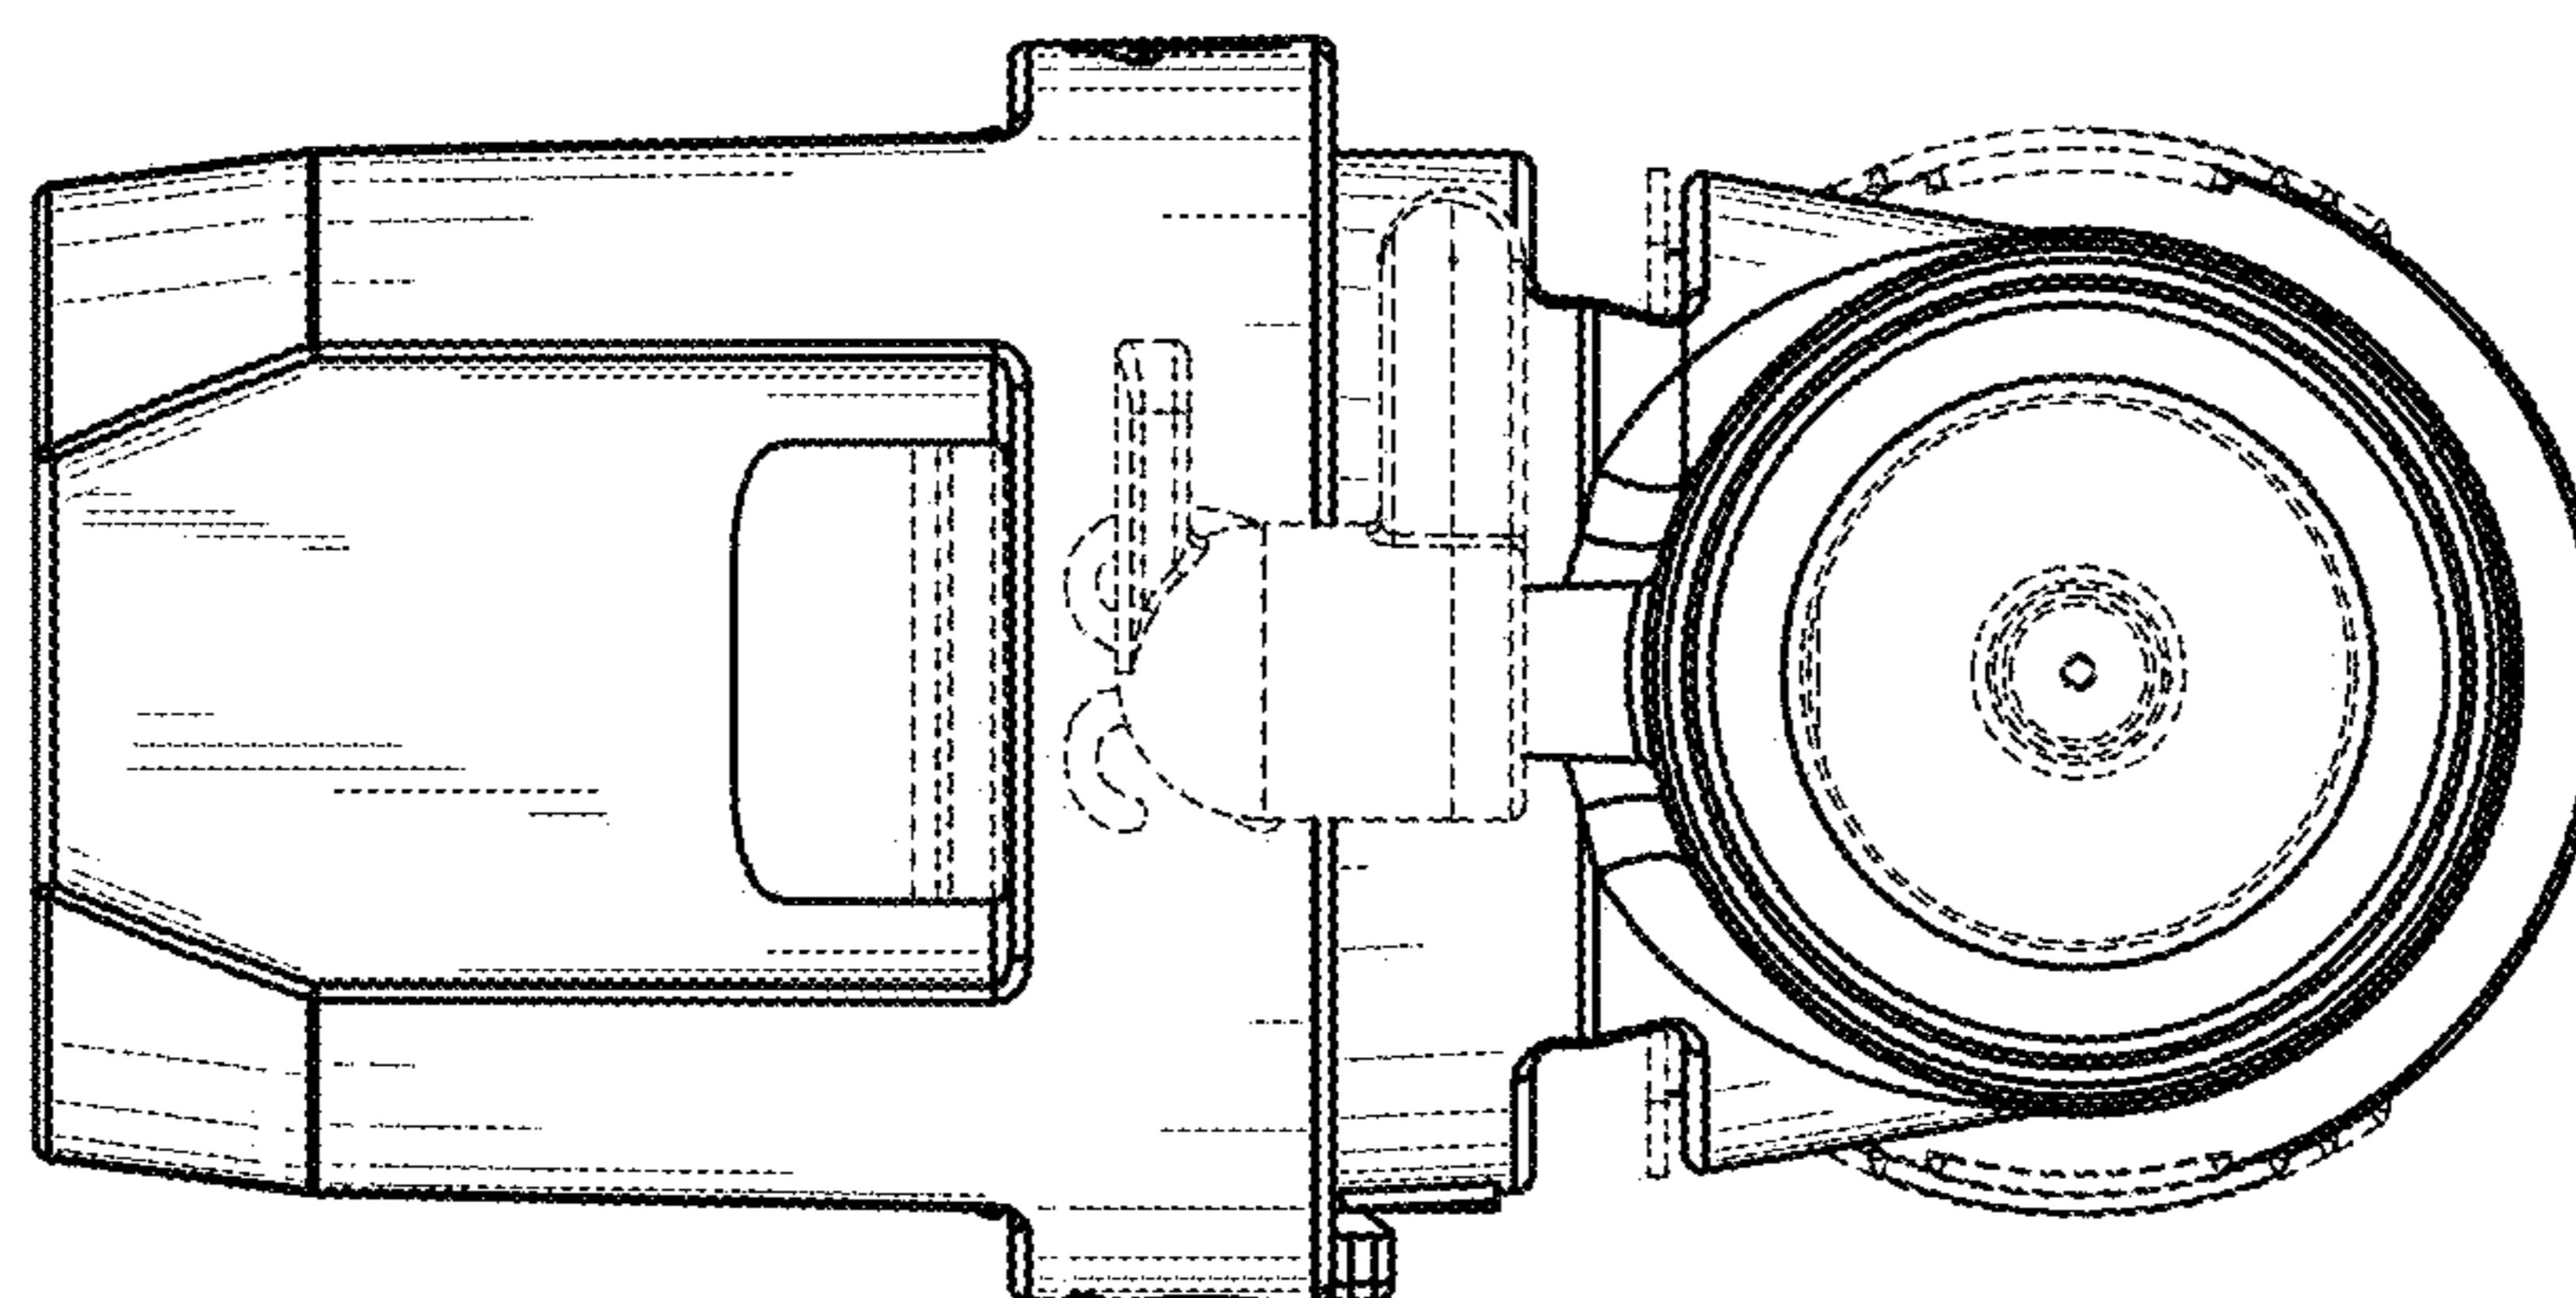


Fig. 4

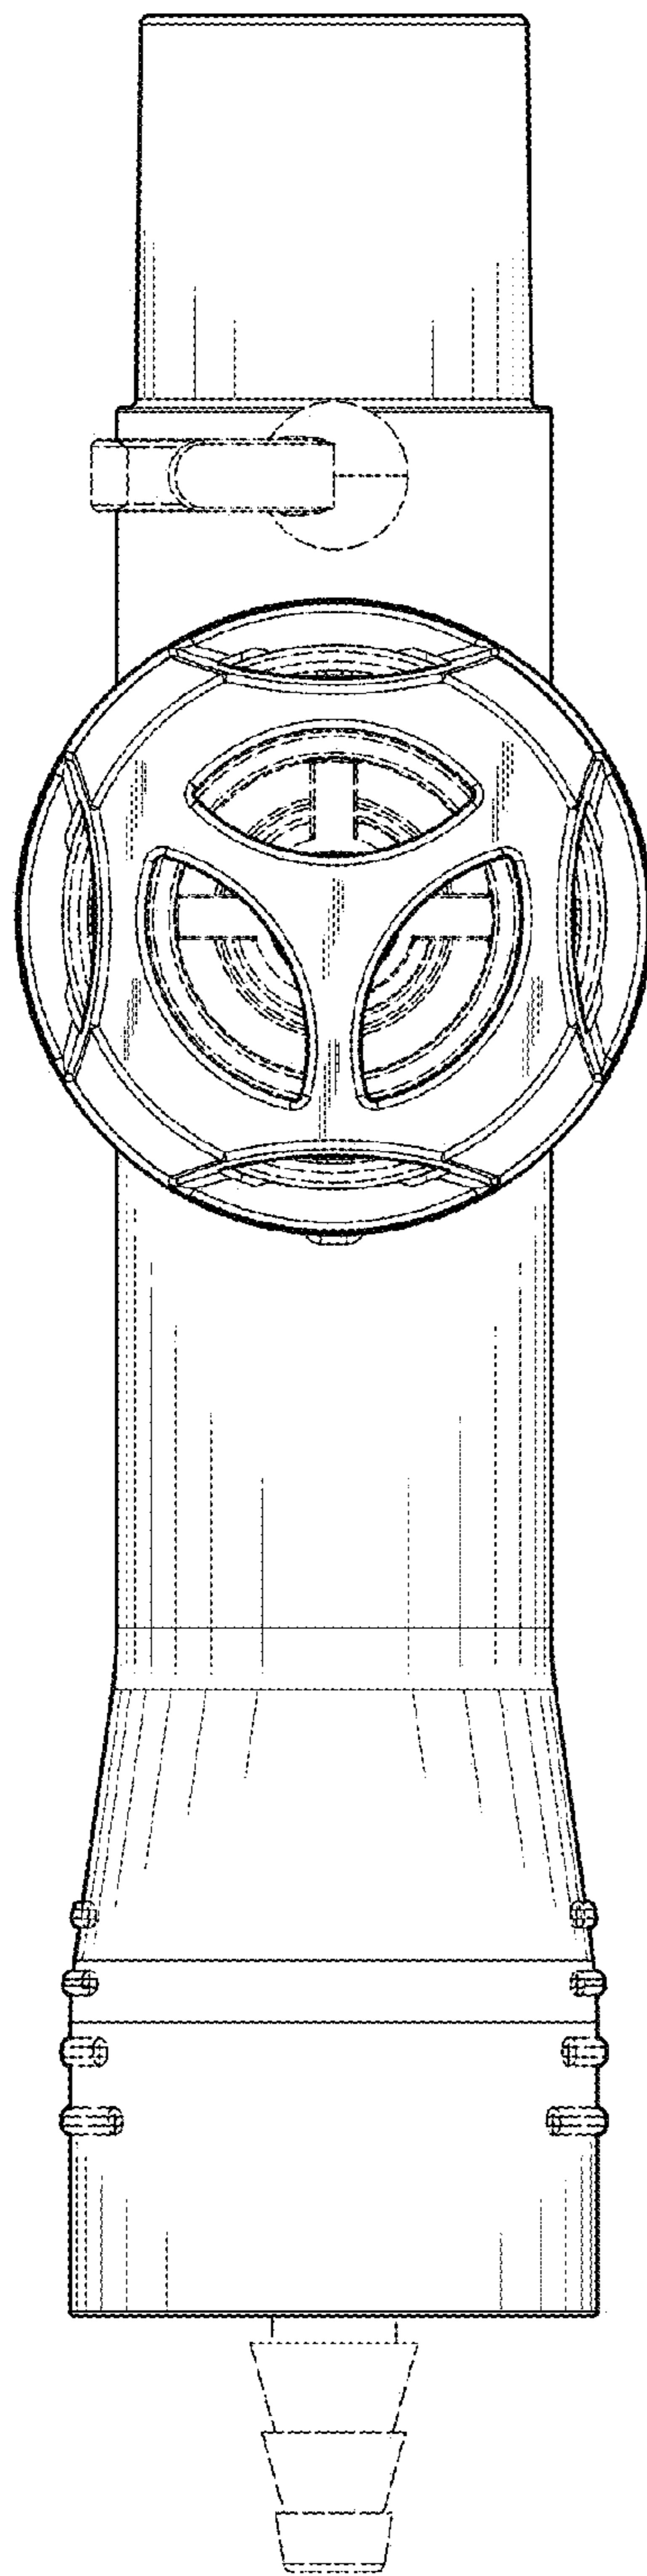


Fig. 5

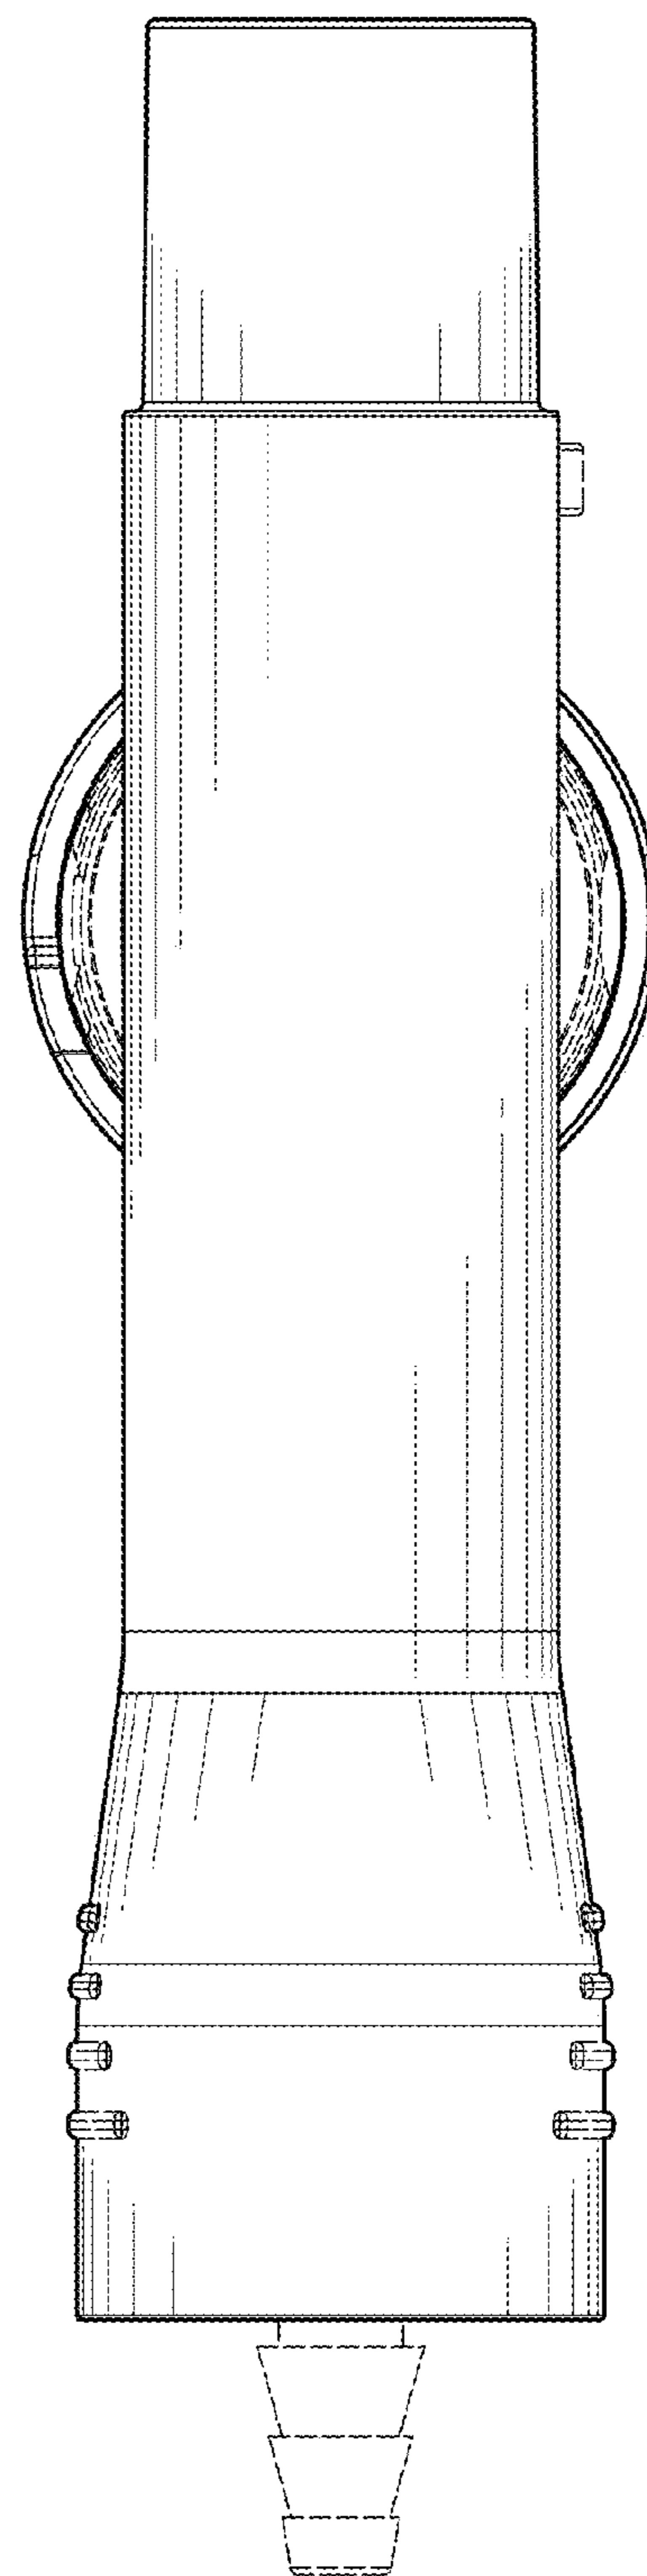


Fig. 6

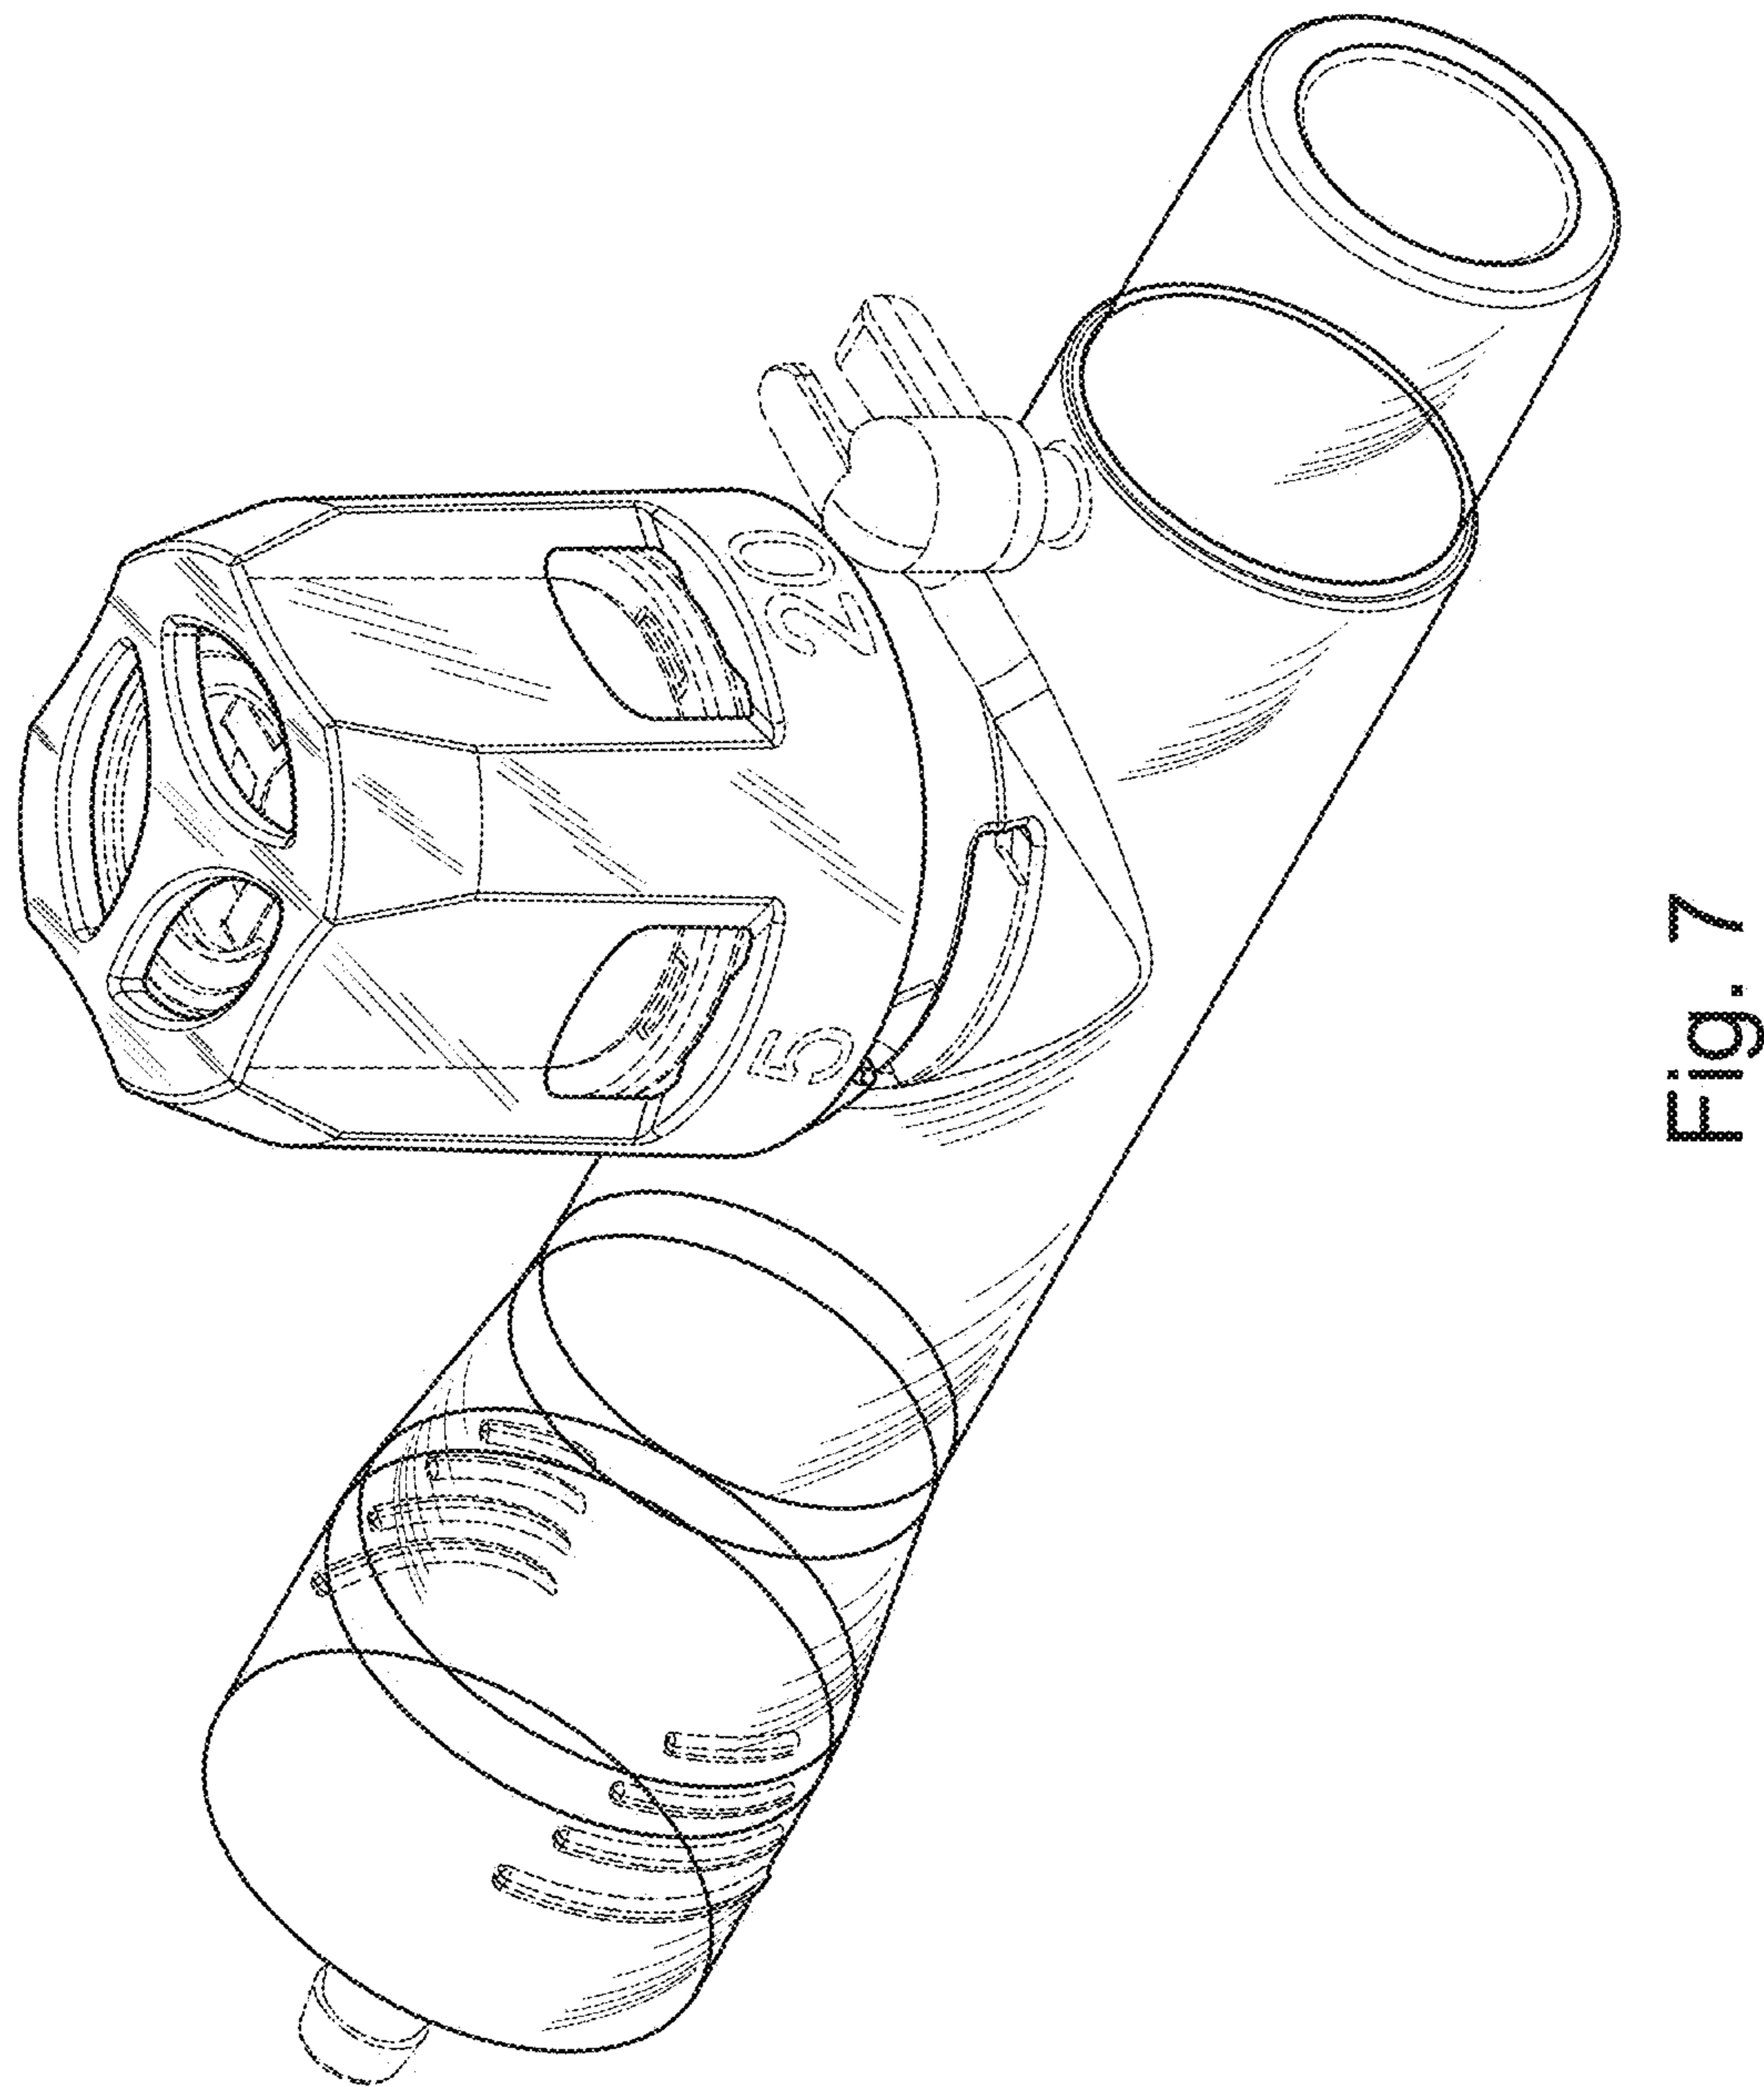


Fig. 7